

Test report

FCC 15.225 and RSS-210 A2.6 13.56 MHz 2015_291614

Date of issue: January 14, 2016

Applicant: Stryker Instruments

Product: RFID Module of Waste Management System (Surgical Medical Equipment)

Model: Manifold Receptacle
PCBA

FCC ID: Q9R-0703001820 IC Registration number: 4919A-0703001820

Specifications:

FCC 47 CFR Part 15 Subpart C, §15.225


Operation within the band 13.110-14.010 MHz.

RSS-210 Issue 8

Licence-exempt Radio Apparatus (All Frequency Bands): Category I Equipment

Test location

Company name	Nemko USA Inc.
Address	2210 Faraday Ave., Suite 150
City	Carlsbad
Province	CA
Postal code	92008-7226
Country	USA
Telephone	+1 858-755-5525
Website	www.nemko.com
Site number	FCC: US5058; IC: 2040B

Tested by	Feng You
Reviewed by	James Morris
Date	January 14, 2016
Signature	

Limits of responsibility

Note that the results contained in this report relate only to the items tested and were obtained in the period between the date of initial receipt of samples and the date of issue of the report.

This test report has been completed in accordance with the requirements of ISO/IEC 17025. All results contain in this report are within Nemko USA's ISO/IEC 17025 accreditation.

Copyright notification

Nemko USA Inc. authorizes the applicant to reproduce this report provided it is reproduced in its entirety and for use by the company's employees only. Any use which a third party makes of this report, or any reliance on or decisions to be made based on it, are the responsibility of such third parties.

Nemko USA Inc. accepts no responsibility for damages, if any, suffered by any third party as a result of decisions made or actions based on this report.

© Nemko USA Inc.

Table of contents

Table of contents	3
Section 1. Report summary	4
1.1 Applicant and manufacturer	4
1.2 Test specifications	4
1.3 Statement of compliance	4
1.4 Exclusions	4
1.5 Test report revision history	4
Section 2. Summary of test results	5
2.1 FCC Part 15 Subpart C, general requirements test results	5
2.2 FCC Part 15 Subpart C, intentional radiators test results	5
2.3 IC RSS-GEN, Issue 4, test results	5
2.4 IC RSS-210, Issue 8, test results	5
Section 3. Equipment under test (EUT) details	6
3.1 Sample information	6
3.2 EUT information	6
3.3 Technical information	6
3.4 Product description and theory of operation	6
3.5 EUT exercise details	6
3.6 EUT setup diagram	7
3.7 EUT sub assemblies	8
Section 4. Engineering considerations	9
4.1 Modifications incorporated in the EUT	9
4.2 Technical judgment	9
4.3 Deviations from laboratory tests procedures	9
Section 5. Test conditions	10
5.1 Atmospheric conditions	10
5.2 Power supply range	10
Section 6. Measurement uncertainty	11
6.1 Uncertainty of measurement	11
Section 7. Test equipment	12
7.1 Test equipment list	12
Section 8. Testing data	13
8.1 FCC 15.215(c) 20 dB bandwidth	13
8.2 RSS-Gen 6.6 Occupied bandwidth	15
8.3 FCC 15.225(a–c) and RSS-210 A2.6 (a–c) Field strength within the 13.110–14.010 MHz band	17
8.4 FCC 15.225(d) and RSS-210 A2.6(d) Field strength of emissions outside 13.110–14.010 MHz band	19
8.5 FCC 15.225(e) and RSS-210 A2.6 Frequency tolerance of the carrier signal	23
8.6 FCC 15.207(a) AC power line conducted emissions limits	24
Section 9. Block diagrams of test set-ups	27
9.1 Radiated emissions set-up	27

Section 1. Report summary

1.1 Applicant and manufacturer

Company name	Stryker Instruments
Address	4100 E. Milham Road
City	Kalamazoo
Province/State	MI
Postal/Zip code	49001
Country	U.S.A.

1.2 Test specifications

FCC 47 CFR Part 15, Subpart C, Clause 15.225	Operation in the 13.110–14.010 MHz
RSS-210 Issue 8, December 2010, Annex 2.6	Band 13.110-14.010 MHz

1.3 Statement of compliance

In the configuration tested, the EUT was found compliant.

Testing was completed against all relevant requirements of the test standard. Results obtained indicate that the product under test complies in full with the requirements tested. The test results relate only to the items tested.

See "Summary of test results" for full details.

1.4 Exclusions

None

1.5 Test report revision history

Revision #	Details of changes made to test report
1	Original report issued
2	Product Name Change
3	Updated according to review comment.
4	Updated with new test results

Section 2. Summary of test results

2.1 FCC Part 15 Subpart C, general requirements test results

Part	Test description	Verdict
§15.31(e)	Variation of power source	Pass ¹
§15.203	Antenna requirement	Pass ²
§15.207(a)	Conducted limits	Pass ³
§15.215(c)	20 dB bandwidth	Pass

Notes: ¹ Measurements of the variation of the input power or the radiated signal level of the fundamental frequency component of the emission, as appropriate, was performed with the supply voltage varied between 17VDC – 41VDC (rated by manufacturer) of the nominal rated supply voltage 36VDC. No noticeable output power variation was observed

² The Antenna is embedded on PCB.

³ Using results from Neptune 3, as tested together with host device (host device contains AC power supply).

2.2 FCC Part 15 Subpart C, intentional radiators test results

Part	Test description	Verdict
§15.225(a)	Field strength within 13.553–13.567 MHz band	Pass
§15.225(b)	Field strength within 13.410–13.553 MHz and 13.567–13.710 MHz bands	Pass
§15.225(c)	Field strength within 13.110–13.410 MHz and 13.710–14.010 MHz bands	Pass
§15.225(d)	Field strength outside 13.110–14.010 MHz band	Pass
§15.225(e)	Frequency tolerance of carrier signal ¹	Pass

Notes: ¹ Because the EUT is module for medical equipment used in operating room, the temperature range tested is according to the manufacturer declared operation range 0°C to 70°C, plus the -20°C and -10°C.

2.3 IC RSS-GEN, Issue 4, test results

Part	Test description	Verdict
6.6	Occupied bandwidth	Pass
6.11	Transmitter frequency stability	Pass ¹
7.1.2	Receiver spurious emissions limits (radiated)	Not applicable
7.1.3	Receiver spurious emissions limits (antenna conducted)	Not applicable
8.8	AC power lines conducted emission limits	Pass

Notes: ¹ Frequency stability covered in RSS-210.

2.4 IC RSS-210, Issue 8, test results

Part	Test description	Verdict
A2.6 (a)	The field strength within the band 13.553–13.567 MHz.	Pass
A2.6 (b)	The field strength within the bands 13.410–13.553 MHz and 13.567–13.710 MHz	Pass
A2.6 (c)	The field strength within the bands 13.110–13.410 MHz and 13.710–14.010 MHz.	Pass
A2.6 (d)	The field strength outside the band 13.110–14.010 MHz.	Pass
A2.6	Carrier frequency stability shall be maintained to $\pm 0.01\%$ (± 100 ppm) ¹	Pass

Section 3. Equipment under test (EUT) details

3.1 Sample information

Receipt date	July 1, 2015
Nemko sample ID number	1

3.2 EUT information

Product name	RFID Module of Waste Management System
Model	Manifold Receptacle PCBA
Serial number	00703-001-820
FCC ID	Q9R-0703001820
IC Registration Number	4919A-0703001820

3.3 Technical information

Operating band	13.553–13.567 MHz
Operating frequency	13.56 MHz
Modulation type	ASK
Occupied bandwidth (99 %)	22 kHz
Power requirements	120VAC, 60Hz
Emission designator	A1D
Antenna information	The EUT uses a unique antenna coupling/ non-detachable antenna to the intentional radiator. Embedded antenna on PCB.

3.4 Product description and theory of operation

The MR PCB is a RFID Module used in surgical equipment for suction and collect fluid waste and evacuate surgical smoke from a surgical site in an operating room. The RFID reader is to read RFID tags in manifolds.

3.5 EUT exercise details

RFID reader is set to constant transmit.

3.6 EUT setup diagram



Figure 3.6-1: Radiated Emissions Setup



Figure 3.6-2: AC Powerline Conducted Emissions Setup

3.7 EUT sub assemblies

Table 3.7-1: EUT sub assemblies

Description	Brand name	Model/Part number	Serial number
RFID Module	Stryker	MR PCB	00703-001-820
Power Supply Cable	Stryker	N/A	N/A
Neptune 3 Rover	Stryker	Neptune 3	00703-001-715
Manifold with passive RFID tag	Stryker	702-20-1	N/A
Manifold with passive RFID tag	Stryker	702-20-1	N/A

Section 4. Engineering considerations

4.1 Modifications incorporated in the EUT

None

4.2 Technical judgment

None

4.3 Deviations from laboratory tests procedures

No deviations were made from laboratory procedures.

Section 5. Test conditions

5.1 Atmospheric conditions

Temperature	15–30 °C
Relative humidity	20–75 %
Air pressure	860–1060 mbar

When it is impracticable to carry out tests under these conditions, a note to this effect stating the ambient temperature and relative humidity during the tests shall be recorded and stated.

5.2 Power supply range

The normal test voltage for equipment to be connected to the mains shall be the nominal mains voltage. For the purpose of the present document, the nominal voltage shall be the declared voltage, or any of the declared voltages $\pm 5\%$, for which the equipment was designed.
36V DC (Rated Range 17-41V DC)

Section 6. Measurement uncertainty

6.1 Uncertainty of measurement

Nemko Canada Inc. has calculated measurement uncertainty and is documented in EMC/MUC/001 "Uncertainty in EMC measurements." Measurement uncertainty was calculated using the methods described in CISPR 16-4 Specification for radio disturbance and immunity measuring apparatus and methods – Part 4: Uncertainty in EMC measurements; as well as described in UKAS LAB34: The expression of Uncertainty in EMC Testing. Measurement uncertainty calculations assume a coverage factor of $K=2$ with 95% certainty.

Frequency/Time Uncertainty $\leq 0.2\text{ms}$

Amplitude Uncertainty $\leq 1.7\text{dB}$

Section 7. Test equipment

7.1 Test equipment list

Table 7.1-1: Equipment list

Asset Tag	Description	Manufacturer	Model	Serial #	Last Cal	Next Cal
529	Antenna, DRWG	EMCO	3115	2505	08-Dec-2014	08-Dec-2016
1480	Antenna, Bilog	Schaffner-Chase	CBL6111C	2572	18-May-2015	18-May-2016
1733	Antenna, Active Loop	EMCO	6507	45939	21-Oct-2014	21-Oct-2015
E1064	Spectrum Analyzer	Agilent	E4440A	US42221762	22-Dec-2014	22-Dec-2015
E1017	9kHz to 7GHz Spectrum Analyzer	Rohde & Schwarz	FSP7	839337/0022	03-Nov-2014	03-Nov-2015
4043	True RMS Multimeter	Fluke	115	22620350	20-Jan-2015	20-Jan-2016
1839	Environmental Chamber	Tenney	T-14	14	VOU	VOU
1917	Power Supply	Xantrex	XFR-300-4	0-300V 0-4A	VOU	VOU
E1019	Two Line V-Network	Rohde & Schwarz	ENV216	101045	15-May-2015	15-May-2016
E1026	EMI Test Receiver 9kHz to 7GHz	Rohde & Schwarz	ESCI 7	100800	14-Aug-2014	14-Aug-2015

Note: NCR - no calibration required, VOU - verify on use

Section 8. Testing data

8.1 FCC 15.215(c) 20 dB bandwidth

8.1.1 Definitions and limits

Intentional radiators operating under the alternative provisions to the general emission limits, as contained in §§15.217 through 15.257 and in Subpart E of this part, must be designed to ensure that the 20 dB bandwidth of the emission, or whatever bandwidth may otherwise be specified in the specific rule section under which the equipment operates, is contained within the frequency band designated in the rule section under which the equipment is operated. The requirement to contain the designated bandwidth of the emission within the specified frequency band includes the effects from frequency sweeping, frequency hopping and other modulation techniques that may be employed as well as the frequency stability of the transmitter over expected variations in temperature and supply voltage.

8.1.2 Test summary

Test date	July 8, 2015	Temperature	24 °C
Test engineer	Feng You	Air pressure	1003 mbar
Verdict	Pass	Relative humidity	56 %

8.1.3 Observations, settings and special notes

Spectrum analyzer settings:

Detector mode	Peak
Resolution bandwidth	≥1 % of span
Video bandwidth	RBW × 3
Trace mode	Max Hold

8.1.4 Test data

Table 8.1-1: Lower 20 dBc frequency cross result


Fundamental frequency, MHz	Lower 20 dBc frequency cross, MHz	Limit, MHz	Margin, kHz
13.560	13.5538	13.553	0.8

Table 8.1-2: Upper 20 dBc frequency cross result

Fundamental frequency, MHz	Upper 20 dBc frequency cross, MHz	Limit, MHz	Margin, kHz
13.560	13.5668	13.567	0.2

8.1.4 Test data, continued

Figure 8.1-1: 20 dB bandwidth spectrum plot

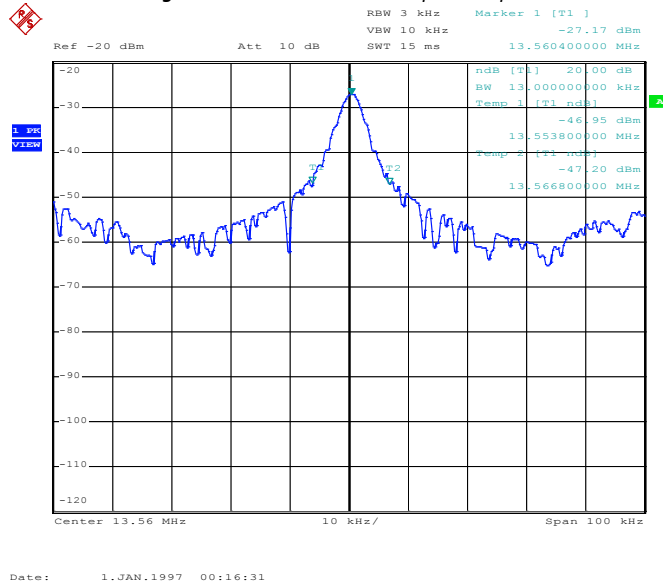

8.2 RSS-Gen 6.6 Occupied bandwidth

8.2.1 Definitions and limits

When an occupied bandwidth value is not specified in the applicable RSS, the transmitted signal bandwidth to be reported is to be its 99 percent emission bandwidth, as calculated or measured.

The transmitter shall be operated at its maximum carrier power measured under normal test conditions.

The span of the analyzer shall be set to capture all products of the modulation process, including the emission skirts. The resolution bandwidth shall be set to as close to 1 percent of the selected span as is possible without being below 1 percent. The video bandwidth shall be set to 3 times the resolution bandwidth. Video averaging is not permitted. Where practical, a sampling detector shall be used since a peak or, peak hold, may produce a wider bandwidth than actual.

The trace data points are recovered and are directly summed in linear terms. The recovered amplitude data points, beginning at the lowest frequency, are placed in a running sum until 0.5 percent of the total is reached and that frequency recorded. The process is repeated for the highest frequency data points. This frequency is recorded.

The span between the two recorded frequencies is the occupied bandwidth.

8.2.2 Test summary

Test date	July 8, 2015	Temperature	24 °C
Test engineer	Feng You	Air pressure	1003 mbar
Verdict	Pass	Relative humidity	56 %

8.2.3 Observations, settings and special notes

Spectrum analyzer settings:

Detector mode	Peak
Resolution bandwidth	≥1 % of span
Video bandwidth	RBW × 3
Trace mode	Max Hold

8.2.4 Test data

Table 8.2-1: 99 % occupied bandwidth result

Fundamental frequency, MHz	99 % occupied bandwidth, kHz
13.560	22

8.2.5 Test data, continued

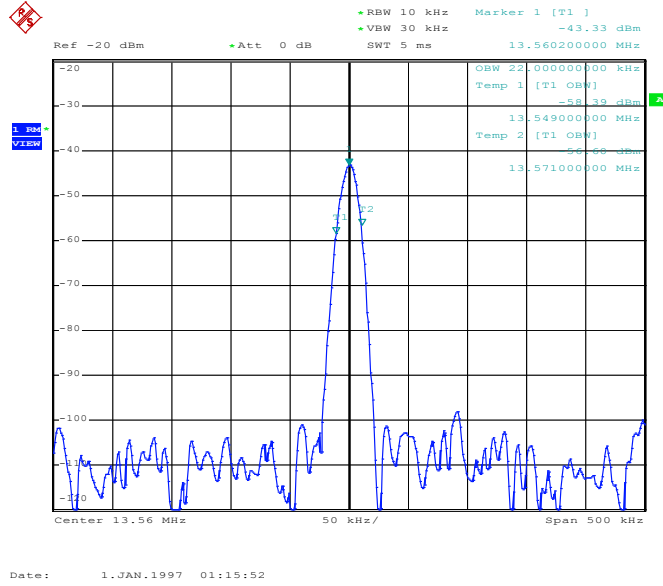


Figure 8.2-1: 99 % occupied bandwidth

8.3 FCC 15.225(a-c) and RSS-210 A2.6 (a-c) Field strength within the 13.110–14.010 MHz band

8.3.1 Definitions and limits

- a) The field strength of any emissions within the band 13.553–13.567 MHz shall not exceed 15848 $\mu\text{V/m}$ (84 dB $\mu\text{V/m}$) at 30 m.
- b) Within the bands 13.410–13.553 MHz and 13.567–13.710 MHz, the field strength of any emissions shall not exceed 334 $\mu\text{V/m}$ (50.5 dB $\mu\text{V/m}$) at 30 m.
- c) Within the bands 13.110–13.410 MHz and 13.710–14.010 MHz the field strength of any emissions shall not exceed 106 $\mu\text{V/m}$ (40.5 dB $\mu\text{V/m}$) at 30 m.

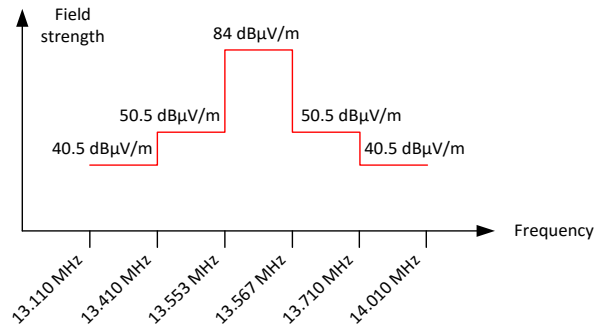


Figure 8.3-1: In-band spurious emissions limit

8.3.2 Test summary

Test date	July 1, 2015	Temperature	22 °C
Test engineer	Feng You	Air pressure	1001 mbar
Verdict	Pass	Relative humidity	55 %

8.3.3 Observations/special notes

The measurements were performed at the distance of 3 m. 40 dB distance correction factor* was applied to the measurement result in order to comply with 30 m limits.

* 30 m to 3 m distance correction factor calculation (for 13 MHz band):

$$40 \times \text{Log}_{10} (3 \text{ m}/30 \text{ m}) = 40 \times \text{Log}_{10} (0.1) = -40 \text{ dB}$$

Spectrum analyzer settings:

Detector mode	Peak
Resolution bandwidth	10 kHz
Video bandwidth	30 kHz
Trace mode	Max Hold

8.3.4 Test data

Table 8.3-1: Field strength measurements results

Frequency range, MHz	Frequency, MHz	Field strength at 3 m, dBμV/m	Calculated field strength at 30 m, dBμV/m	Limit, dBμV/m	Margin, dB
13.553–13.567	13.56025	42.0	2.0	84.00	82
13.410–13.553	13.46725	29.7	-10.3	50.50	60.8
13.567–13.710	13.622	28.9	-11.1	50.50	61.6
13.110–13.410	13.2235	29.4	-10.6	40.50	51.1
13.710–14.010	13.8995	29.8	-10.2	40.50	50.7

Note: Calculated field strength at 30 m = Measured field strength at 3 m – 40 dB

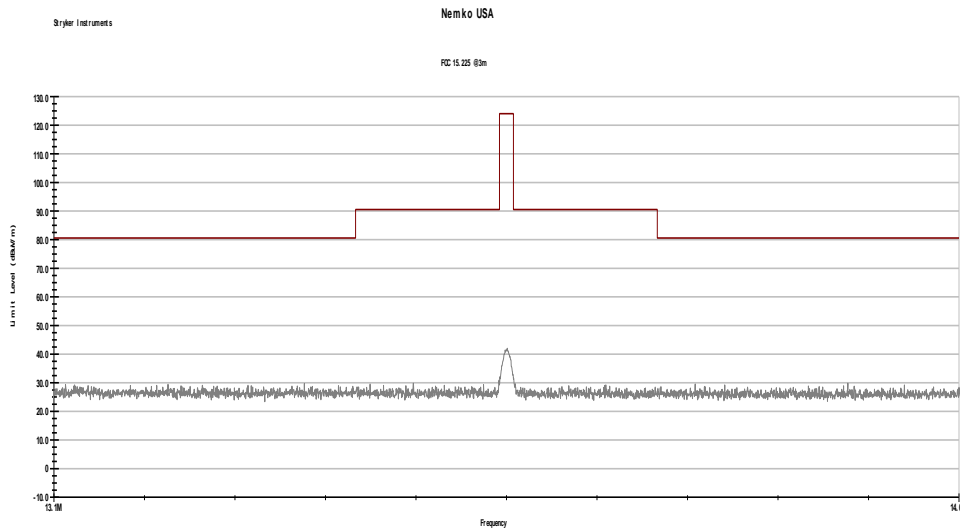


Figure 8.3-2: Field strength within 13.11–14.010 MHz band

8.4 FCC 15.225(d) and RSS-210 A2.6(d) Field strength of emissions outside 13.110–14.010 MHz band

8.4.1 Definitions and limits

FCC: The field strength of any emissions appearing outside of the 13.110–14.010 MHz band shall not exceed the general radiated emission limits in §15.209

The field strength of emissions appearing within restricted bands (as specified in §15.205) shall not exceed the limits from §15.209.

IC: The field strength of any emission outside the band 13.110–14.010 MHz shall not exceed the 30 µV/m (29.5 dBµV/m) limit.

Table 8.4-1: FCC §15.209 – Radiated emission limits

Frequency, MHz	Field strength of emissions		Measurement distance, m
	µV/m	dBµV/m	
0.009–0.490	2400/F	$67.6 - 20 \times \log_{10}(F)$	300
0.490–1.705	24000/F	$87.6 - 20 \times \log_{10}(F)$	30
1.705–30.0	30	29.5	30
30–88	100	40.0	3
88–216	150	43.5	3
216–960	200	46.0	3
above 960	500	54.0	3

Notes: In the emission table above, the tighter limit applies at the band edges. For frequencies above 1 GHz the limit on peak RF emissions is 20 dB above the maximum permitted average emission limit applicable to the equipment under test

Table 8.4-2: Restricted frequency bands

MHz	MHz	MHz	GHz
0.090–0.110	16.42–16.423	399.9–410	4.5–5.15
0.495–0.505	16.69475–16.69525	608–614	5.35–5.46
2.1735–2.1905	16.80425–16.80475	960–1240	7.25–7.75
4.125–4.128	25.5–25.67	1300–1427	8.025–8.5
4.17725–4.17775	37.5–38.25	1435–1626.5	9.0–9.2
4.20725–4.20775	73–74.6	1645.5–1646.5	9.3–9.5
6.215–6.218	74.8–75.2	1660–1710	10.6–12.7
6.26775–6.26825	108–121.94	1718.8–1722.2	13.25–13.4
6.31175–6.31225	123–138	2200–2300	14.47–14.5
8.291–8.294	149.9–150.05	2310–2390	15.35–16.2
8.362–8.366	156.52475–156.52525	2483.5–2500	17.7–21.4
8.37625–8.38675	156.7–156.9	2690–2900	22.01–23.12
8.41425–8.41475	162.0125–167.17	3260–3267	23.6–24.0
12.29–12.293	167.72–173.2	3332–3339	31.2–31.8
12.51975–12.52025	240–285	3345.8–3358	36.43–36.5
12.57675–12.57725	322–335.4	3600–4400	Above 38.6
13.36–13.41			

8.4.2 Test summary

Test date	July 1, 2015	Temperature	22 °C
Test engineer	Feng You	Air pressure	1001 mbar
Verdict	Pass	Relative humidity	55 %

8.4.3 Observations, settings and special notes

The spectrum was searched from 9 kHz to 1 GHz.
 Radiated measurements were performed at a distance of 3 m.

Spectrum analyzer settings for frequencies below 30 MHz:

Detector mode	Quasi-Peak
Resolution bandwidth	9 kHz
Video bandwidth	30 kHz
Trace mode	Max Hold
Measurement time	100 ms

Spectrum analyzer settings for frequencies above 30 MHz:

Detector mode	Peak
Resolution bandwidth	100 kHz
Video bandwidth	300 kHz
Trace mode	Max Hold
Measurement time	100 ms

8.4.4 Test data

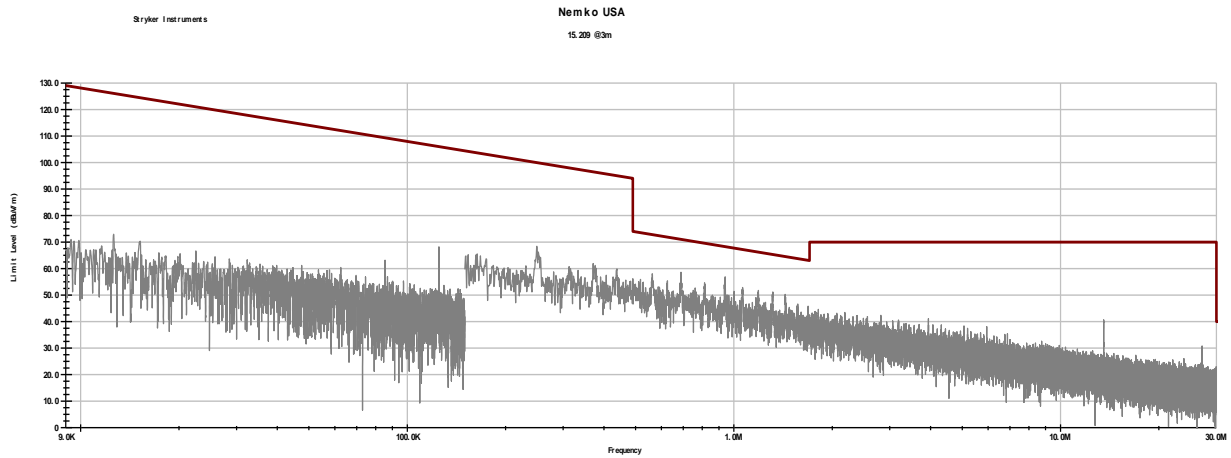


Figure 8.4-1: Field strength of spurious emissions below 30 MHz

8.4.4 Test data, continued

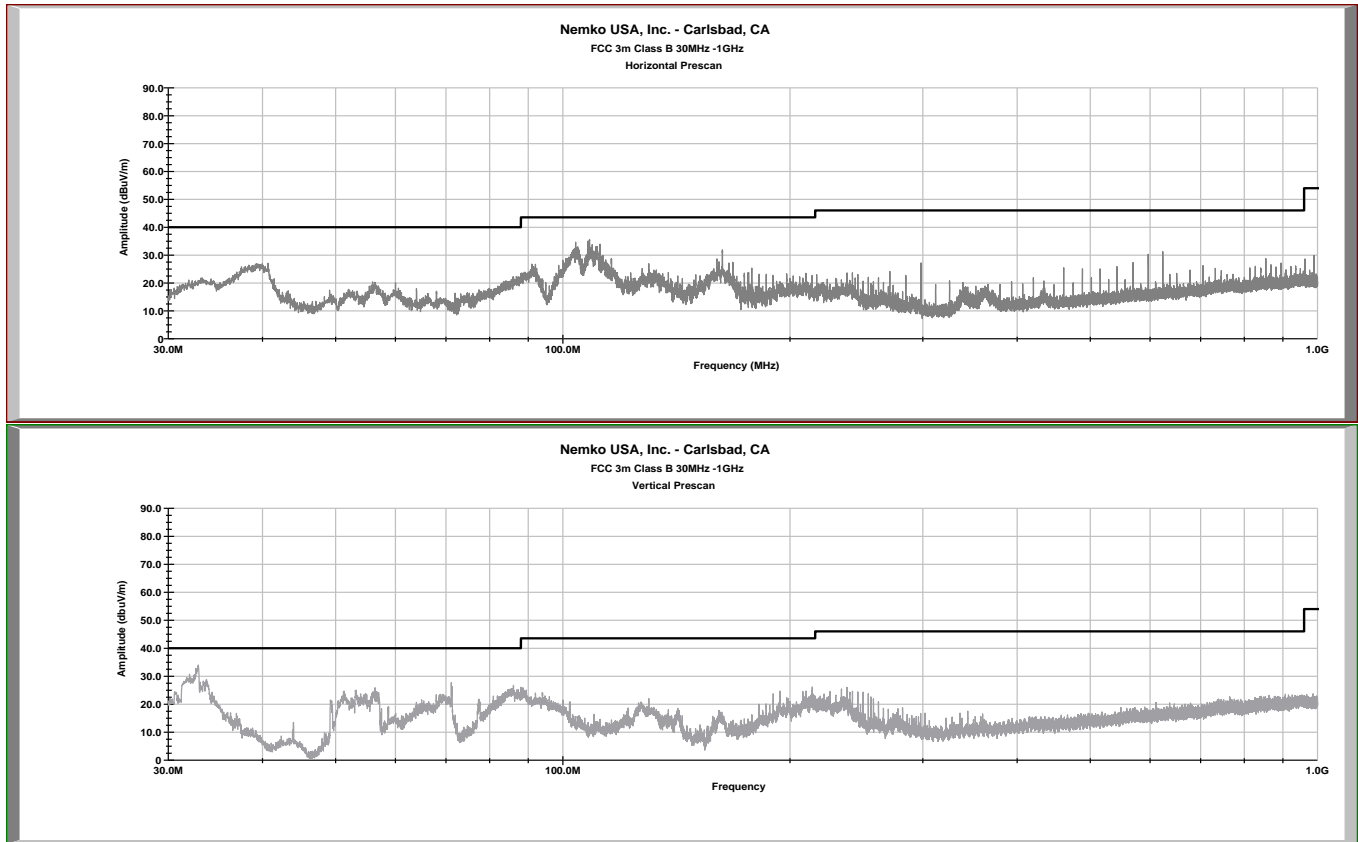


Figure 8.4-2: Field strength of spurious emissions 30-1000 MHz

Table 8.4-3: QP Measurement Results 30-1000MHz

Frequency MHz	Polarity H/V	Corrected QP dBuV/m	QP Limit dBuV/m	QP Margin dB
40.6489	H	3.99	40	36.01
104.018	H	11.1	43.5	32.42
108.49	H	4.04	43.5	39.48
162.687	H	4.29	43.5	39.23
298.318	H	6.58	46	39.44
596.629	H	13.04	46	32.98
623.761	H	13.17	46	32.85
989.901	H	17.74	54	36.24
32.884	V	14.76	40	25.24
71.144	V	15.36	40	24.64
85.998	V	19.61	40	20.39
130.02	V	15.24	43.5	28.28
214.027	V	20.24	43.5	23.28
237.995	V	21.44	46	24.58

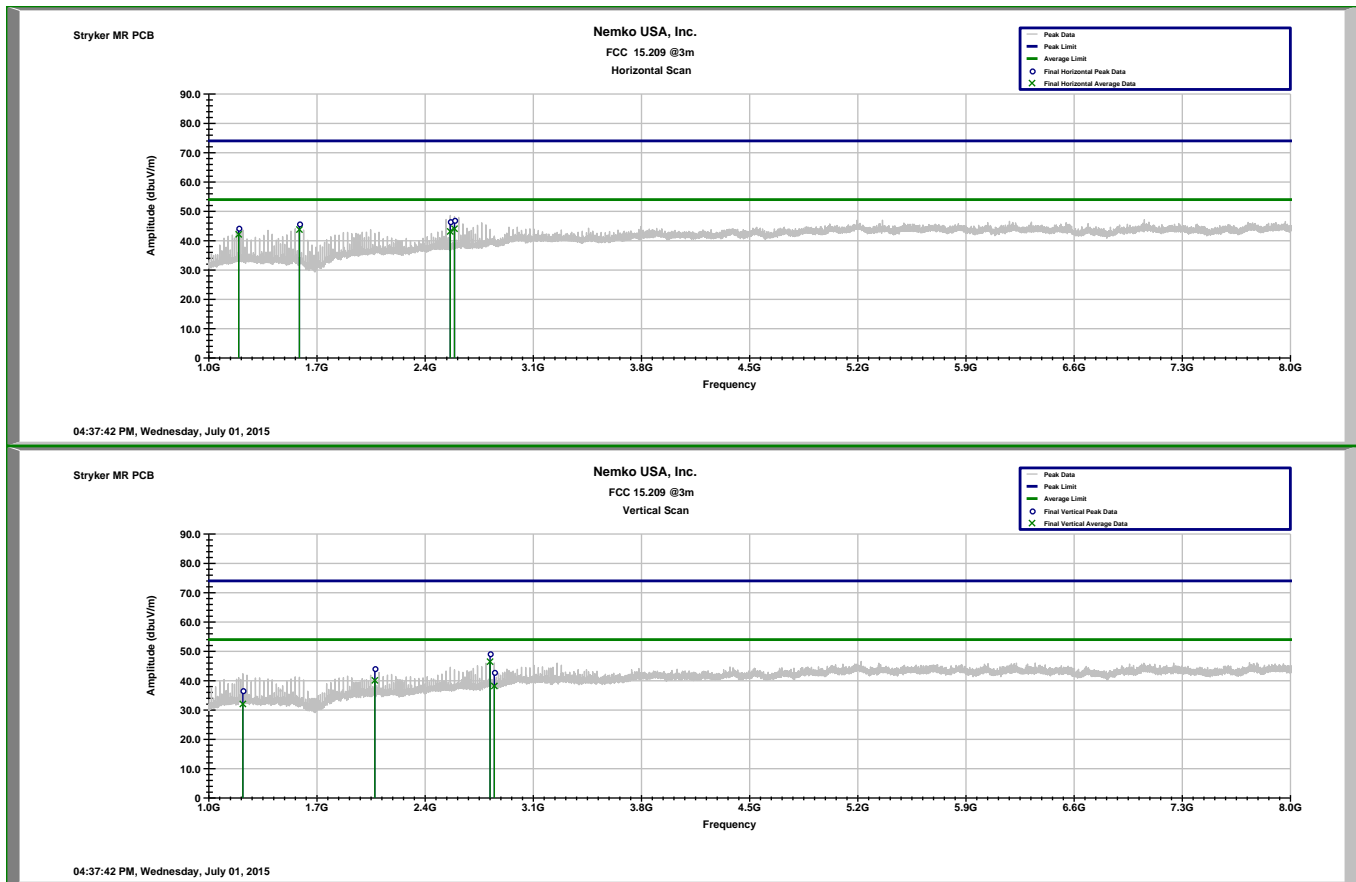


Figure 8.4-3: Field strength of spurious emissions 1-8GHz

Table 8.4-4: AVG Measurement Results 1-8GHz

Frequency MHz	Polarity H/V	AVG dBuV/m	Peak dBuV/m	AVG Limit dBuV/m	Peak Limit dBuV/m	AVG Margin dB	Peak Margin dB
1193.47	H	42.1	44.3	54	74	11.9	29.7
1586.51	H	43.8	45.7	54	74	10.2	28.3
2562.87	H	43.1	46.5	54	74	10.9	27.5
2590.01	H	44.1	47	54	74	9.9	27
1220.51	V	32.1	36.6	54	74	21.9	37.4
2074.77	V	40.1	44.1	54	74	13.9	29.9
2820.6	V	46.5	49.2	54	74	7.5	24.8
2847.71	V	38.2	42.9	54	74	15.8	31.1

8.5 FCC 15.225(e) and RSS-210 A2.6 Frequency tolerance of the carrier signal

8.5.1 Definitions and limits

The frequency tolerance of the carrier signal shall be maintained within $\pm 0.01\%$ (± 100 ppm) of the operating frequency over a temperature variation of $-20\text{ }^{\circ}\text{C}$ to $+50\text{ }^{\circ}\text{C}$ at normal supply voltage, and for a variation in the primary supply voltage from 85 % to 115 % of the rated supply voltage at a temperature of $20\text{ }^{\circ}\text{C}$. For battery operated equipment, the equipment tests shall be performed using a new battery.

8.5.2 Test summary

Test date	July 2, 2015	Temperature	22 °C
Test engineer	Feng You	Air pressure	1005 mbar
Verdict	Pass	Relative humidity	55 %

8.5.3 Observations, settings and special notes

Spectrum analyzer settings:

Detector mode	Peak
Resolution bandwidth	$\geq 1\%$ of emission bandwidth
Video bandwidth	RBW \times 3
Trace mode	Max Hold
Special Condition	Because the EUT is module for medical equipment used in operating room, the temperature range tested is extended according to the manufacturer declared operation range to $70\text{ }^{\circ}\text{C}$. The module is supplied with 36V DC nominal voltage. Declared voltage range is 17-41V DC.

8.5.4 Test data

Table 8.5-1: Frequency drift measurements results

Test conditions	Frequency, MHz	Frequency drift, \pm ppm	Limit, \pm ppm	Margin, ppm
+20 °C, Nominal 36V DC	13.56026	Reference	Reference	Reference
+20 °C, 41V DC	13.56026	0	100	100
+20 °C, 17V DC	13.56026	0	100	100
-20 °C, Nominal 36V DC	13.56024	-1.5	100	98.5
-10 °C, Nominal 36V DC	13.5603	2.9	100	97.1
0 °C, Nominal 36V DC	13.5603	2.9	100	97.1
+10 °C, Nominal 36V DC	13.5603	2.9	100	97.1
+30 °C, Nominal 36V DC	13.56024	-1.5	100	98.5
+40 °C, Nominal 36V DC	13.56024	-1.5	100	98.5
+50 °C, Nominal 36V DC	13.56024	-1.5	100	98.5
+60 °C, Nominal 36V DC	13.56022	-2.9	100	97.1
+70 °C, Nominal 36V DC	13.56034	5.9	100	94.1

Note: frequency drift was calculated as follows:

$$\text{Frequency drift (ppm)} = ((F_{\text{measured}} - F_{\text{reference}}) \div F_{\text{reference}}) \times 1 \times 10^6$$

8.6 FCC 15.207(a) AC power line conducted emissions limits

8.6.1 Definitions and limits

Except as shown in paragraphs (b) and (c) of this section, for an intentional radiator that is designed to be connected to the public utility (AC) power line, the radio frequency voltage that is conducted back onto the AC power line on any frequency or frequencies, within the band 150 kHz to 30 MHz, shall not exceed the limits in the following table, as measured using a 50 μ H/50 Ω line impedance stabilization network (LISN). Compliance with the provisions of this paragraph shall be based on the measurement of the radio frequency voltage between each power line and ground at the power terminal. The lower limit applies at the boundary between the frequency ranges.

The conducted emissions shall be measured with a 50 Ω /50 μ H line impedance stabilization network (LISN).

Table 8.6-1: Conducted emissions limit

Frequency of emission (MHz)	Conducted limit (dB μ V)	
	Quasi-peak	Average
0.15–0.5	66 to 56*	56 to 46*
0.5–5	56	46
5–30	60	50

Note: * - Decreases with the logarithm of the frequency.

8.6.2 Test summary

Test date	July 8, 2015	Temperature	24 °C
Test engineer	Feng You	Air pressure	1003 mbar
Verdict	Pass	Relative humidity	56 %

8.6.3 Observations, settings and special notes

The module is tested inside host device Stryker Neptune 3.

The EUT was set up as floor standing configuration.

The spectral scan has been corrected with transducer factors (i.e. cable loss, LISN factors, and attenuators) for determination of compliance.

A preview measurement was generated with the receiver in continuous scan mode. Emissions detected within 6 dB or above limit were re-measured with the appropriate detector against the correlating limit and recorded as the final measurement.

Test receiver settings:

Frequency span	150 kHz to 30 MHz
Detector mode	Peak and Average (preview mode); Quasi-Peak (final measurements)
Resolution bandwidth	9 kHz
Video bandwidth	30 kHz
Trace mode	Max Hold
Measurement time	1000 ms

8.6.4 Test data

Plot 8.6-1: Conducted emissions on phase line

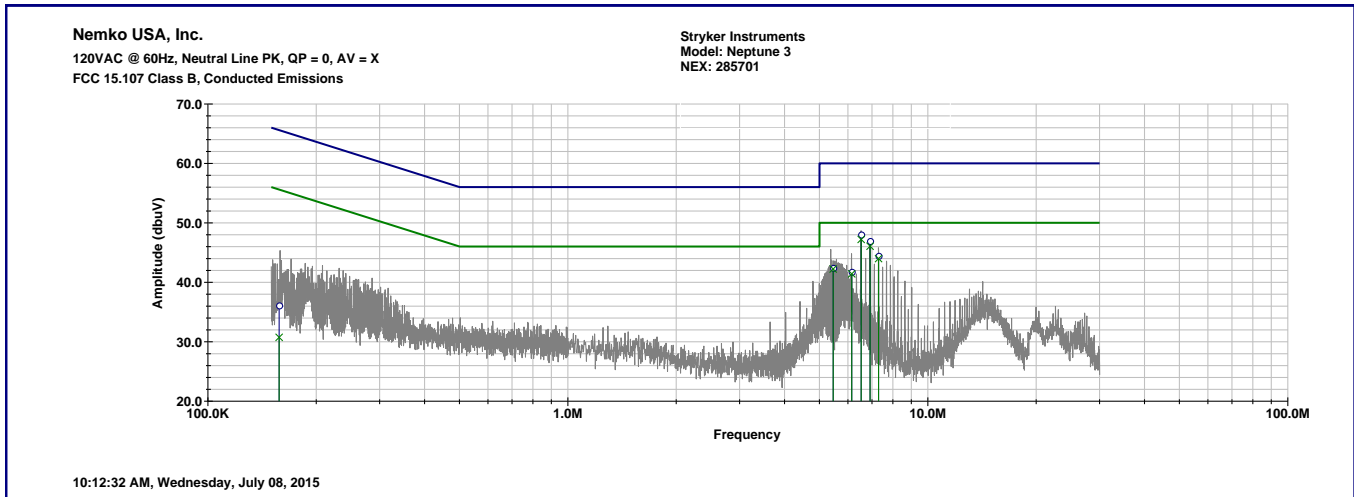


Table 8.6-2: Quasi-Peak and Average conducted emissions results on phase line

Frequency kHz	QP Rdng (dBuV)	Avg Rdng (dBuV)	QP Limit (dBuV)	Avg Limit (dBuV)	QP Margin (dB)	Avg Margin (dB)
157.786	36.1	30.7	65.6	55.6	29.5	24.9
5455.91	42.4	42.2	60	50	17.6	7.8
6141.65	41.7	41.4	60	50	18.3	8.6
6524.17	48	47.2	60	50	12	2.8
6908.83	46.9	46.1	60	50	13.1	3.9
7290.62	44.4	44	60	50	15.6	6

8.6.4 Test data, continued

Plot 8.6-2: Conducted emissions on neutral line

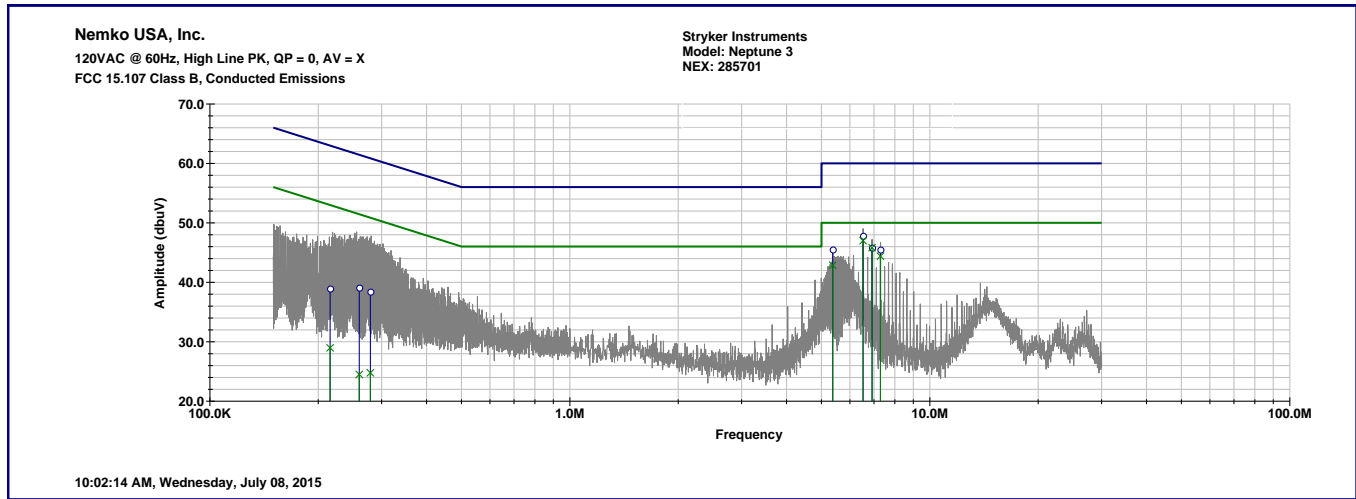


Table 8.6-3: Quasi-Peak and Average conducted emissions results on neutral line

Frequency kHz	QP Rdng (dBuV)	Avg Rdng (dBuV)	QP Limit (dBuV)	Avg Limit (dBuV)	QP Margin (dB)	Avg Margin (dB)
215.787	38.9	29	63	53	24.1	24
259.941	39.1	24.5	61.4	51.4	22.3	26.9
279.223	38.4	24.8	60.8	50.8	22.4	26
5369.5	45.5	42.9	60	50	14.5	7.1
6520.87	47.8	47	60	50	12.2	3
6906.34	45.8	45.8	60	50	14.2	4.2
7288.5	45.5	44.4	60	50	14.5	5.6

Section 9. Block diagrams of test set-ups

9.1 Radiated emissions set-up

