

Stryker Instruments 5100-050-000 11418

#### 1250 Peterson Dr., Wheeling, IL 60090

FCC Rules and Regulations / Intentional Radiators

Operational in the Band 13.553-13.567 MHz

Part 15, Subpart C, Section 15.225

#### THE FOLLOWING "MEETS" THE ABOVE TEST SPECIFICATION

Formal Name: TPS Irrigation Console w/ Stryker Electronics Control Board

- Kind of Equipment: Medical Electrical Equipment
- Test Configuration: The TPS Irrigation Console is connected to the footswitch (with a metal console and footswitch connector) and handpieces via cables plugged into its ports. Formula Shaver is run via the footswitch and an SE5 and a Saber are plugged in. (Tested at 120 vac, 60 Hz)
- Model Number(s): 5100-001-000, 5100-050-000
- Model(s) Tested: 5100-050-000
- Serial Number(s): NA
- Date of Tests: May 31, 2005
- Test Conducted For: Stryker Instruments 4100 E. Milham Ave Kalamazoo, Michigan 49001

**NOTICE**: "This report must not be used by the client to claim product endorsement by NVLAP or any agency of the U.S. Government". Please see the "Additional Description of Equipment Under Test" page listed inside of this report. This report must not be reproduced (except in full), without the approval of D.L.S. Electronic Systems.



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 60090

SIGNATURE PAGE

Report By:

Amon C Rove

Arnom C. Rowe Test Engineer EMC-001375-NE

Reviewed By:

Villiam M.S.

William Stumpf OATS Manager

Approved By:

Briand. Matts

Brian Mattson General Manager


Company Official:

Stryker Instruments



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 6009

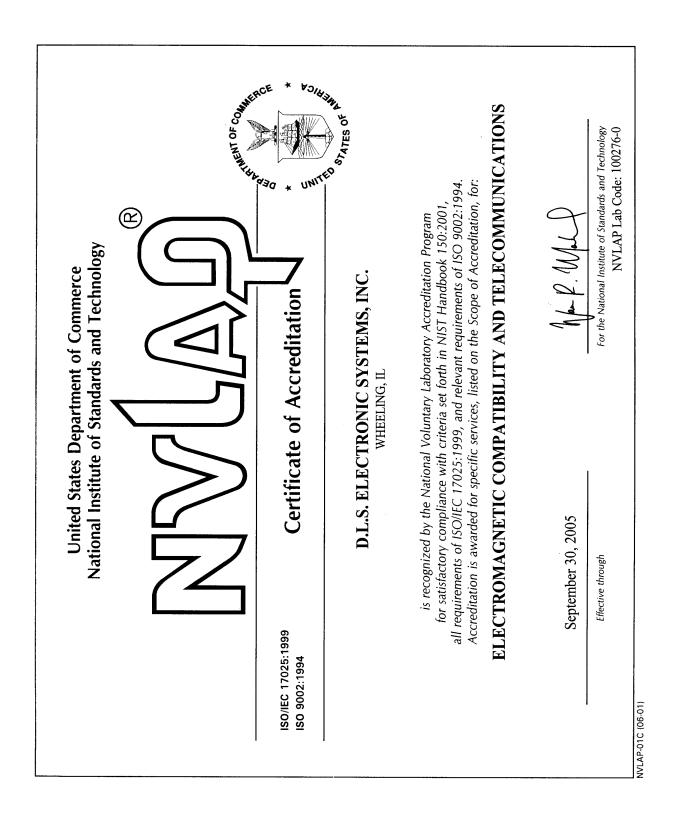



Stryker Instruments 5100-050-000 11418


## 1250 Peterson Dr., Wheeling, IL 6009

ISO/IEC 17025:19 ISO 9002:1994	<sup>39</sup> Scope of Accr	editation
	AGNETIC COMPATIBILITY OMMUNICATIONS	Page: 1 of NVLAP LAB CODE 10027
	D.L.S. ELECTRONIC S 1250 Peterson Wheeling, IL 600 Mr. Brian J. M Phone: 847-537-6400 F E-Mail: bmattson@ URL: http://www.	Drive 090-6454 Iattson ax: 847-537-6488 dlsemc.com
NVLAP Code	<b>Designation / Description</b>	
Emissions Test	Methods:	
12/160D21	RTCA/DO-160D (1997): Environmen Airborne Equipment - Section 21 - Em	
12/300220a	Matters; Short Range Devices; Radio e	romagnetic compatibility and Radio spectro equipment to be used in the 25 MHz to 1000 ls ranging up to 500 mW; Part 1: Technical
12/300386a	_	compatibility and radio spectrum matter equipment; Electromagnetic compatibility
12/C63.17	ANSI C63.17-1998: American Nationa Electromagnetic and Operational Com Communications Services (UPCS) De	1 5



Stryker Instruments 5100-050-000 11418

#### 1250 Peterson Dr., Wheeling, IL 6009

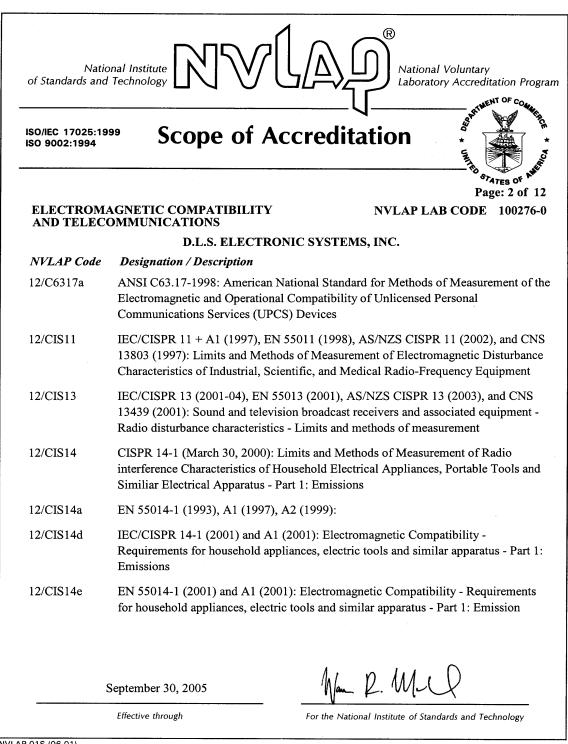


NVLAP-01S (06-01)



Stryker Instruments 5100-050-000 11418

#### 1250 Peterson Dr., Wheeling, IL 6009

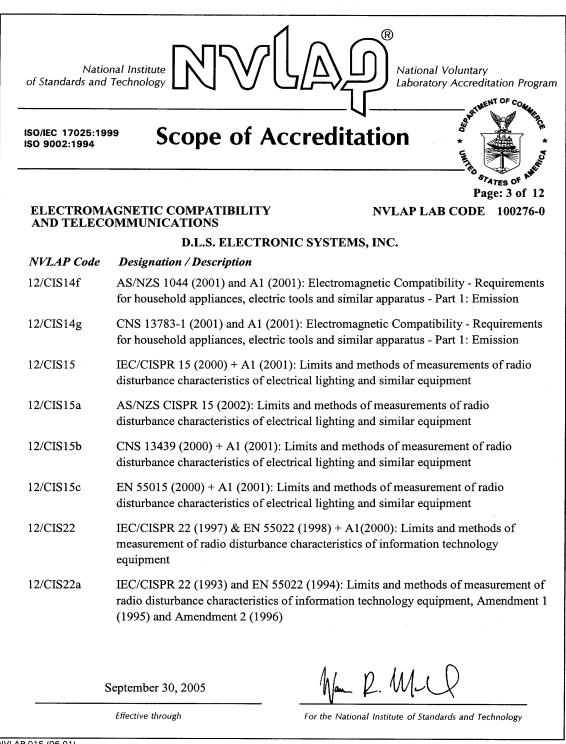


NVLAP-01S (06-01)



Stryker Instruments 5100-050-000 11418


#### 1250 Peterson Dr., Wheeling, IL 6009

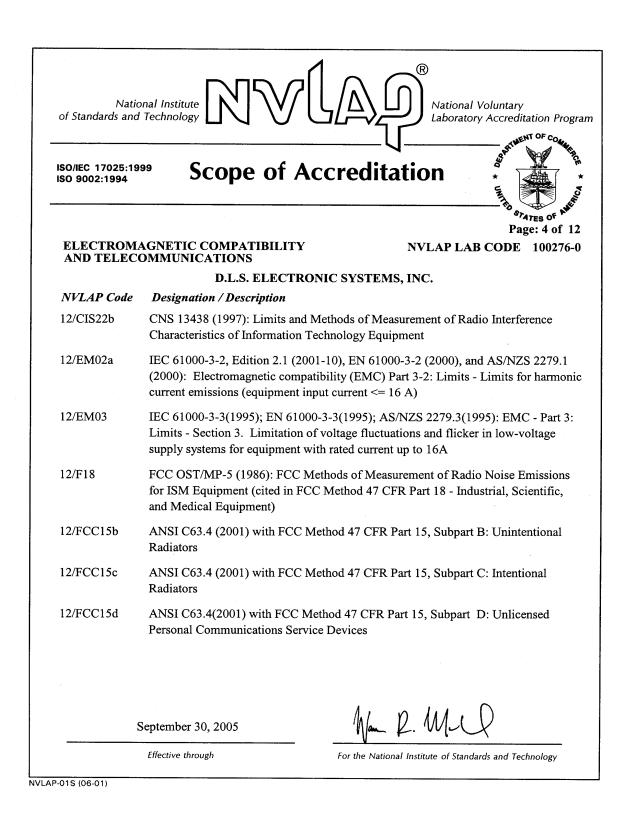



Stryker Instruments 5100-050-000 11418

#### 1250 Peterson Dr., Wheeling, IL 6009

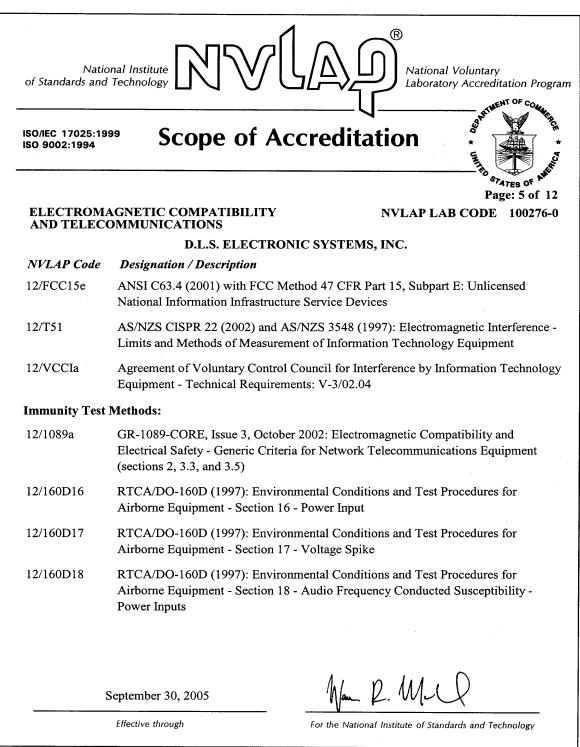


NVLAP-01S (06-01)



Stryker Instruments 5100-050-000 11418

#### 1250 Peterson Dr., Wheeling, IL 6009

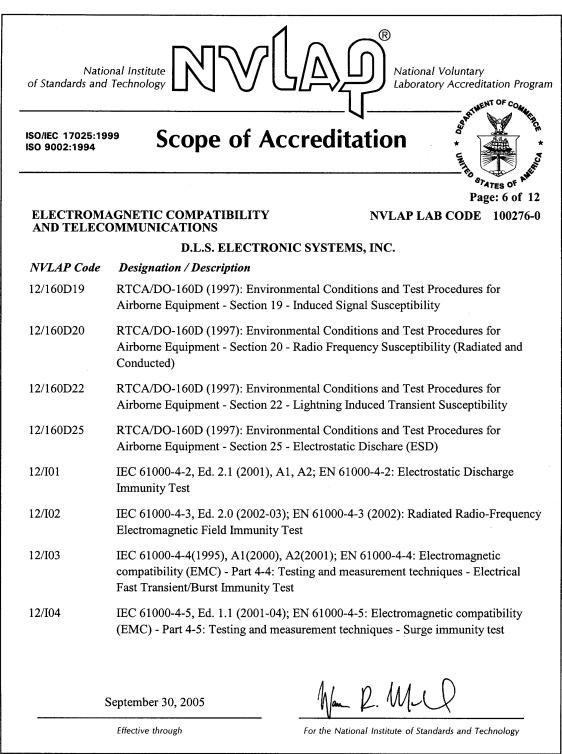


NVLAP-01S (06-01)



Stryker Instruments 5100-050-000 11418


#### 1250 Peterson Dr., Wheeling, IL 6009

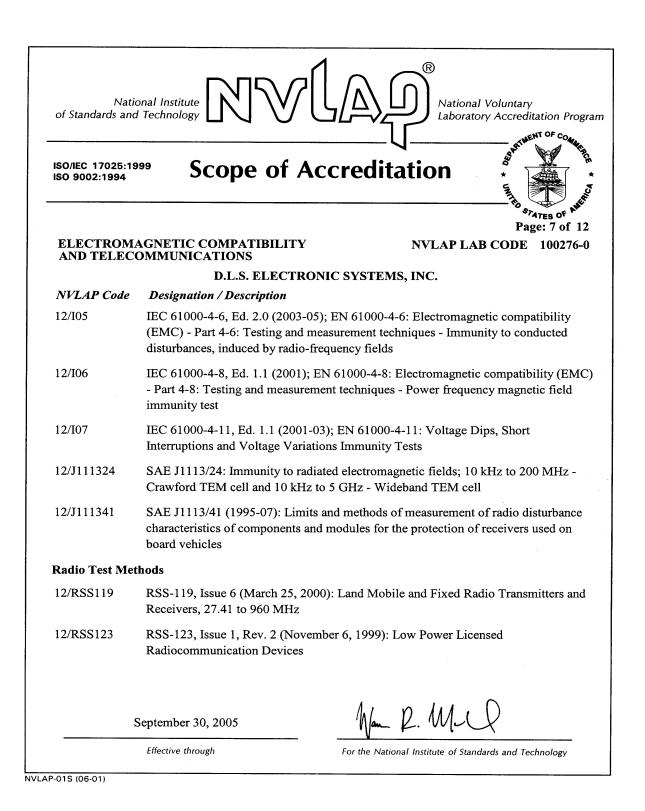



Stryker Instruments 5100-050-000 11418

#### 1250 Peterson Dr., Wheeling, IL 6009

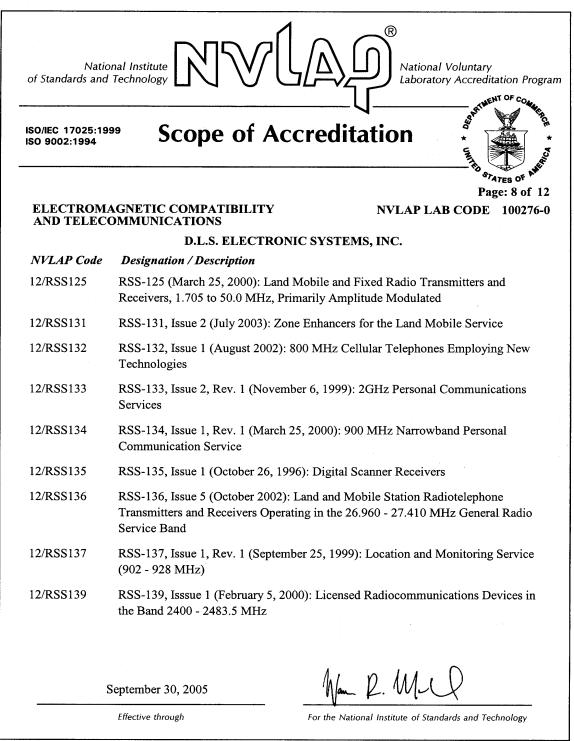


NVLAP-01S (06-01)



Stryker Instruments 5100-050-000 11418


#### 1250 Peterson Dr., Wheeling, IL 6009

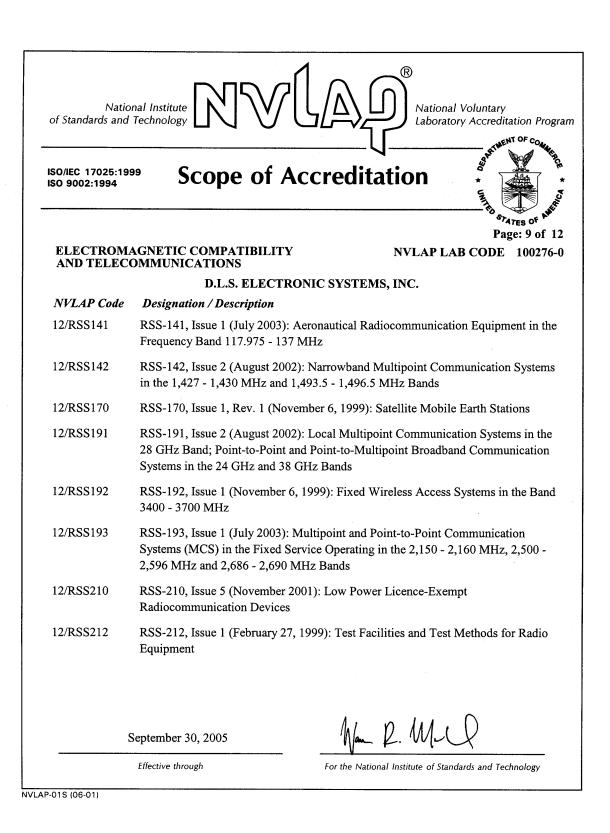



Stryker Instruments 5100-050-000 11418


#### 1250 Peterson Dr., Wheeling, IL 6009

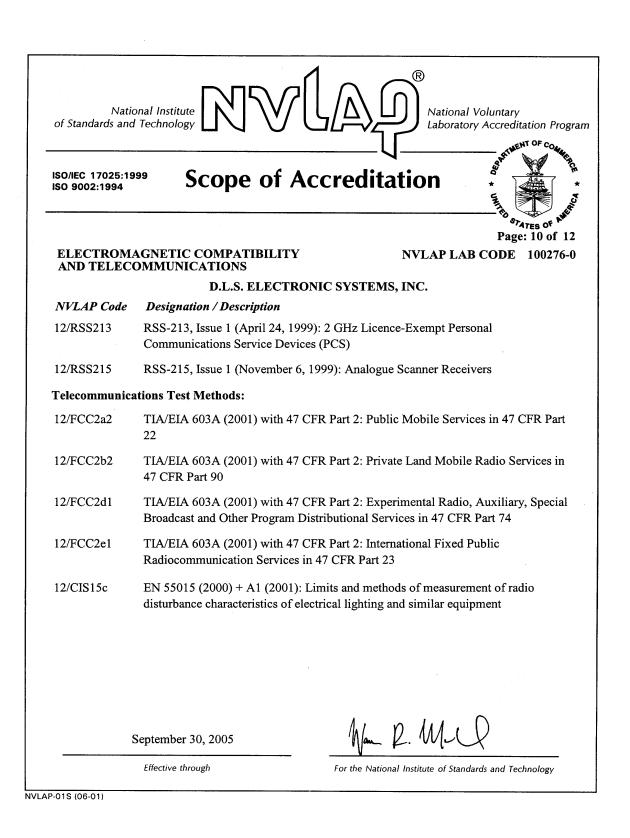



Stryker Instruments 5100-050-000 11418

#### 1250 Peterson Dr., Wheeling, IL 6009

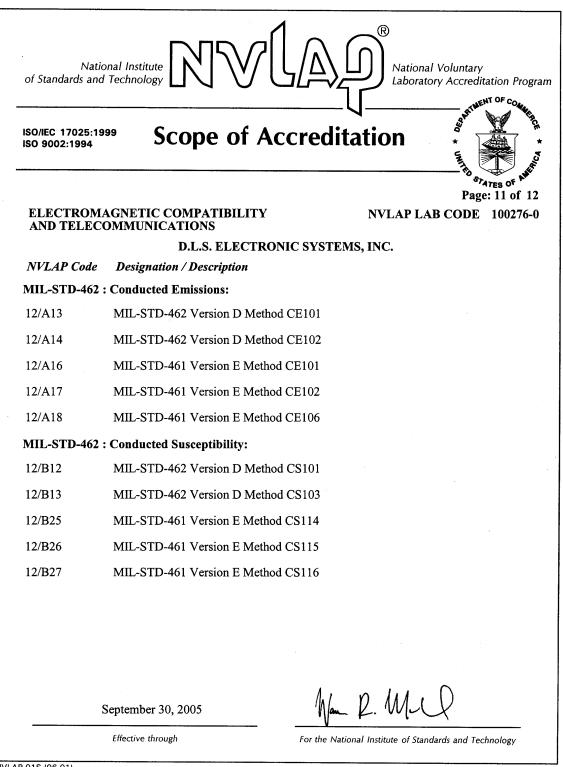

Page -14-

NVLAP-01S (06-01)



Stryker Instruments 5100-050-000 11418

#### 1250 Peterson Dr., Wheeling, IL 6009

Natio of Standards and ISO/IEC 17025:19 ISO 9002:1994		Accredit	National Voluntary Laboratory Accreditation Prog
ELECTROMA	AGNETIC COMPATIBILIT	Υ	Page: 12 of 1 NVLAP LAB CODE 100276-
AND TELECO	OMMUNICATIONS	DANIC SVETEM	
NVLAP Code	D.L.S. ELECT Designation / Description	RONIC SYSTEM	<b>1</b> 5, 111C.
	: Radiated Emissions:		
12/D04	MIL-STD-462 Version D M	ethod RE101	iy.
12/D05	MIL-STD-462 Version D M	ethod RE102	
12/D06	MIL-STD-462 Version D M	ethod RE103	
MIL-STD-462 :	: Radiated Susceptibility:		
12/E08	MIL-STD-462 Version D M	ethod RS101	
12/E09	MIL-STD-462 Version D M	ethod RS103	
S	September 30, 2005	Man	P. M.C
<u></u>	Effective through	- V	nal Institute of Standards and Technology



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 6009

## TABLE OF CONTENTS

i.	Cover Page	1
ii.	Signature Page	2
iii.	NVLAP Certificate of Accreditation	3
iv.	NVLAP Scope of Accreditation	4
v.	Table of Contents	16
1.0	Summary of Test Report	.18
2.0	Introduction	.18
3.0	Object	.18
4.0	Test Set-Up	19
5.0	Test Equipment	20
6.0	Ambient Measurements	
7.0	Description of Test Sample	22
8.0	Additional Description of Test Sample	24
9.0	Photo Information and Test Set-Up	
10.0	Radiated Photos Taken During Testing	
10.0	Conducted Photos Taken During Testing	
11.0	Results of Tests	.30
12.0	Conclusion	30
TABL	E 1 – EQUIPMENT LIST	.31



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 6009

## TABLE OF CONTENTS

33
34
35
40
41
43
44
50
57
58
59
60



Company:StrykModel Tested:5100Report Number:1141

1250 Peterson Dr., Wheeling, IL 6009

### 1.0 SUMMARY OF TEST REPORT

It was found that the TPS Irrigation Console w/ Stryker Electronics Control Board, Model Number(s) 5100-050-000, "meets" the radio interference conducted and radiated emission requirements of the FCC "Rules and Regulations", Part 15, Subpart C, Section 15.225 for operational in the 13.553-13.567 MHz Band.

This test report relates only to the items tested and contains the following number of pages.

Text: 60

#### 2.0 INTRODUCTION

On May 31, 2005, a series of radio frequency interference measurements was performed on TPS Irrigation Console w/ Stryker Electronics Control Board, Model Number(s) 5100-050-000, Serial Number: NA. The tests were performed according to the procedures of the FCC as stated in the "Methods of Measurement of Radio-Noise Emissions for Low-Voltage Electrical and Electronic Equipment in the Range of 9 kHz to 40 GHz" found in the American National Standards Institute, ANSI C63.4-2003. Tests were performed by personnel of D.L.S. Electronic Systems, Inc. who are responsible to Donald L. Sweeney, Senior EMC Engineer.

#### 3.0 OBJECT

The purpose of this series of tests was to determine if the test sample could meet the radio frequency interference emission requirements of the FCC "Rules and Regulations", Part 15, Subpart C, Sections 15.209 & 15.225 for Intentional Radiators operating in the Band 13.553-13.567 MHz.



Company:StrykeModel Tested:5100-0Report Number:11418

Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 6009

#### 4.0 TEST SET-UP

All emission tests were performed at D.L.S. Electronic Systems, Inc. and set up according to the American National Standards Institute, ANSI C63.4-2003, Section 8, (Figures 11a and 11b).

All emissions tests were performed with the test item placed on a 80 cm high rotating non-conductive table, located in the test room. Equipment normally operated on the floor was placed on a metal covered turntable which is flush with the surrounding conducting ground plane. The ground plane has an electrical isolation layer over its surface approximately 7 mm thick. The EUT is separated from the turntable ground plane by a non-conductive layer. The equipment under test was set up according to ANSI C63.4-2003, Sections 6, 7 and 8.



Company:Stryker IModel Tested:5100-05Report Number:11418

1250 Peterson Dr., Wheeling, IL 6009

### 5.0 TEST EQUIPMENT (Bandwidths and Detector Function)

All preliminary data below 1000 MHz was automatically plotted using the HP Spectrum Analyzer or ESI 26/40 Fixed Tuned Receiver. The data was taken using Peak, Quasi-Peak or the Average Detector Functions as required. This information was then used to determine the frequencies of maximum emissions. Above 1000 MHz, final data was taken using the Average Detector.

Below 1000 MHz, final data was taken using the HP Spectrum Analyzer and/or ESI 26/40 Fixed Tuned Receiver. These plots were made using the Peak or Quasi-Peak Detector functions, with manual measurements performed on the questionable frequencies using the Quasi-Peak or the Average Detector Function of the Analyzer or ESI 26/40 Fixed Tuned Receiver as required. Above 1000 MHz, final data was taken using the Average Detector on the Spectrum Analyzer.

The bandwidths shown below are specified by ANSI C63.4-2003, Section 4.2.

Frequency Range	Bandwidth (-6 dB)
10 to 150 kHz	200 Hz
150 kHz to 30 MHz	9 kHz
30 MHz to 1 GHz	120 kHz
Above 1 GHz	1 MHz

A list of the equipment used can be found in Table 1. All primary equipment was calibrated against known reference standards with a verified traceable path to NIST.



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 6009

### 6.0 AMBIENT MEASUREMENTS

For emissions measurements, broadband antennas and an EMI Test Receiver with a panoramic spectrum display are used. First the frequency range is scanned and displayed on the test receiver display. Next the scanned frequency range is divided into smaller ranges, and then it is manually tuned through to determine the emissions from the EUT. A headset or loudspeaker is connected to the test receiver's AM/FM demodulated output as an aid in detecting ambient signals and finding frequencies of significant emission from the EUT. If there is any doubt as to the source of the emission, it is further investigated by rotating the EUT, or by disconnecting the power from the EUT.

The EUT is set up in its typical configuration and operated in its various modes. For tabletop systems, cables are manipulated within the range of likely configurations. For floor-standing equipment, the cables are located in the same manner as the user would install them and no further manipulation is made. If the manner of cable installation is not known, or if it changes with each installation, cables or wires for floor-standing equipment shall be manipulated to the extent possible to produce the maximum level of emissions. For each mode of operation, the frequency spectrum is monitored. Variations in antenna height, antenna polarization, EUT azimuth, and cable or wire placement (each variable within bounds specified elsewhere) are explored to produce the emissions that have the highest amplitude relative to the limit. These methods are performed to the specifications in MP-5 or ANSI C63.4-2003, as appropriate.



Company:StryModel Tested:5100Report Number:114

Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 6009

#### 7.0 DESCRIPTION OF TEST SAMPLE: (See also Paragraph 8.0)

7.1 Description:

The TPS Irrigation Console 5100-050-000 was the unit used during testing. The standard TPS 5100-001-000, 5100-050-000 are considered to fall under this testing as they are identical to each other plus or minus the irrigation pump. The TPS system is used for drilling, cutting and shaping bone for surgical procedures. The handpieces may be controlled via a handswitch or foot operated footswitch control. The handpiece motor speeds are user selectable via a touch screen on the TPS console display and they vary from 900 rpm to 75,000 rpm. The irrigation version also incorporates an irrigation pump which operates in one of two modes. On demand when the handpiece is activated or in Flush Mode which is a continuous run operation. The TPS (Plus) system also has the capability of recognizing which cutters are placed into the handpiece via RF.

#### 7.2 PHYSICAL DIMENSIONS OF EQUIPMENT UNDER TEST

Length: 0.98 feet x Width: 0.75 feet x Height: 0.5 feet

## 7.3 LINE FILTER USED:

Corcom 6ED4C

#### 7.4 INTERNAL CLOCK FREQUENCIES:

Switching Power Supply Frequencies:

100 kHz

Clock Frequencies:

6, 12, 24, 0.285, 13.56 MHz



1250 Peterson Dr., Wheeling, IL 60090

## 7.0 DESCRIPTION OF TEST SAMPLE: (CON'T)

## 7.5 DESCRIPTION OF ALL CIRCUIT BOARDS:

- 1. TPS + Control Board AssemblyPN: 5100-002-161 Rev F2. LCD Screen Interface AssemblyPN: 5100-002-162 Rev None
- 3. TPS Irrigation Pump Board Assembly
- 4. Universal 400 Watt Power Supply

- PN: 5100-001-327 Rev C
- PN: 5100-002-345 Rev E



Company:StryModel Tested:5100Report Number:114

Stryker Instruments 5100-050-000 11418

#### 1250 Peterson Dr., Wheeling, IL 60090

# 8.0 ADDITIONAL DESCRIPTION OF TEST SAMPLE: (See also Paragraph 7.0)

1: There were no additional descriptions noted at the time of test.

I certify that the above, as described in paragraph 7.0, describes the equipment tested and will be manufactured as stated.

By:

Signature

Title

For:

Company

Date



1250 Peterson Dr., Wheeling, IL 60090

#### 9.0 PHOTO INFORMATION AND TEST SET-UP

- Item 0 TPS Irrigation Console w/ Stryker Electronics Control Board Model Number: 5100-050-000 Serial Number: NA
- Item 1 Stryker SE5/TPS Tool
- Item 2 Stryker Formula Tool
- Item 3 Stryker Saber Drill Tool
- Item 4 Stryker Foot Switch SN: 0415900853
- Item 5 Shielded AC Power Cord. 3.5m



1250 Peterson Dr., Wheeling, IL 60090


## 10.0 RADIATED PHOTOS TAKEN DURING TESTING





1250 Peterson Dr., Wheeling, IL 60090

## 10.0 RADIATED PHOTOS TAKEN DURING TESTING: (CON'T)

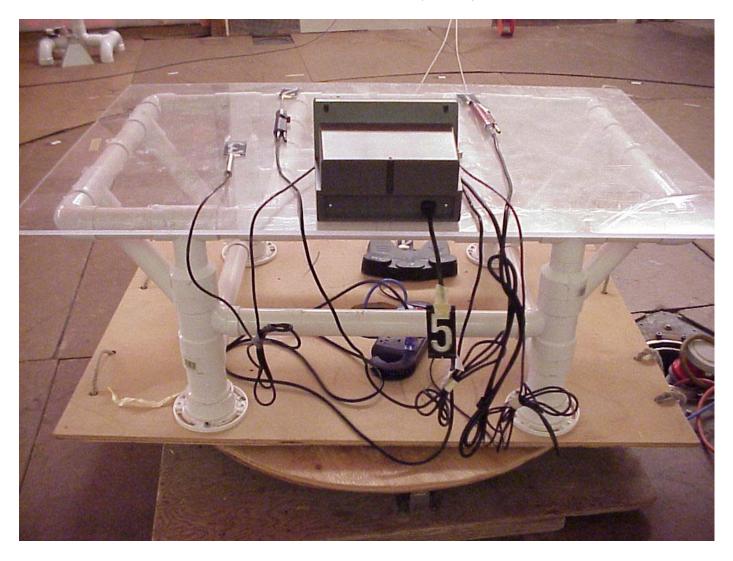



1250 Peterson Dr., Wheeling, IL 60090

## 10.0 CONDUCTED PHOTOS TAKEN DURING TESTING





1250 Peterson Dr., Wheeling, IL 60090

## 10.0 CONDUCTED PHOTOS TAKEN DURING TESTING: (CON'T)





1250 Peterson Dr., Wheeling, IL 60090

#### 11.0 RESULTS OF TESTS

The radio interference emission charts results can be seen on the pages at the end of this report. Data sheets indicating the test measurements taken during testing can also be found at the end of this report. Points on the emission charts shown with a yellow mark are background frequencies that were verified during testing.

#### 12.0 CONCLUSION

It was found that the TPS Irrigation Console w/ Stryker Electronics Control Board, Model Number(s) 5100-050-000 "**meets**" the radio interference conducted and radiated emission requirements of the FCC "Rules and Regulations", Part 15, Subpart C, Section 15.225 for operational in the 13.553-13.567 MHz Band.



1250 Peterson Dr., Wheeling, IL 60090

### TABLE 1 – EQUIPMENT LIST

Test		Model	Serial	Frequency	Cal Due
Equipment	Manufacturer	Number	Number	Range	Dates
Spectrum	Hewlett/	8566B	2240A002041	100 Hz – 22 GHz	10/05
Analyzer	Packard				
Quasi-Peak	Hewlett/	85650A	2043A00121	10 kHz – 1 GHz	10/05
Adapter	Packard				
Spectrum	Hewlett/	8566B	2421A00452	100 Hz – 22 GHz	2/06
Analyzer	Packard				
Quasi-Peak	Hewlett/	85650A	2043A00450	10 kHz – 1 GHz	2/06
Adapter	Packard				
Spectrum	Hewlett/	8591A	3009A00700	9 kHz – 1.8 GHz	3/06
Analyzer	Packard				
Receiver	Electrometrics	EMC-30	44168	10 kHz – 1 GHz	9/05
Receiver	Rohde & Schwarz	ESI 26	837491/010	20 Hz – 26 GHz	11/05
Receiver	Rohde & Schwarz	ESI 40	837808/006	20 Hz – 40 GHz	12/05
Receiver	Rohde & Schwarz	ESI 40	837808/005	20 Hz – 40 GHz	12/05
Antenna	EMCO	3104C	00054891	20 MHz – 200 MHz	2/06
Antenna	Electrometrics	LPA-25	1114	200 MHz – 1 GHz	3/06
Antenna	EMCO	3104C	00054892	20 MHz – 200 MHz	3/06

All primary equipment is calibrated against known reference standards with a verified traceable path to NIST.



1250 Peterson Dr., Wheeling, IL 60090

## TABLE 1 – EQUIPMENT LIST

Test Equipment	Manufacturer	Model Number	Serial Number	Frequency Range	Cal Due Dates
Antenna	Electrometrics	3146	1205	200 MHz – 1 GHz	3/06
Antenna	ЕМСО	3104C	97014785	20 MHz – 200 MHz	2/06
Antenna	ЕМСО	3146	97024895	200 MHz – 1 GHz	3/06
Antenna	EMCO	3115	2479	1 GHz – 18 GHz	8/05
Antenna	EMCO	3115	99035731	1 GHz – 18 GHz	4/06
Antenna	Rohde & Schwarz	HUF-Z1	829381001	20 MHz – 1 GHz	2/06
Antenna	Rohde & Schwarz	HUF-Z1	829381005	20 MHz – 1 GHz	8/05
LISN	Solar	8012-50-R- 24-BNC	8305116	10 MHz – 30 MHz	8/05
LISN	Solar	8012-50-R- 24-BNC	814548	10 MHz – 30 MHz	8/05
LISN	Solar	9252-50-R- 24-BNC	961019	10 MHz – 30 MHz	12/05
LISN	Solar	9252-50-R- 24-BNC	971612	10 MHz – 30 MHz	10/05
LISN	Solar	9252-50-R- 24-BNC	92710620	10 MHz – 30 MHz	7/05

All primary equipment is calibrated against known reference standards with a verified traceable path to NIST.



1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX A

## TEST PROCEDURE

## Part 15, Subpart C, Section 15.225a-c

## **OPERATION WITHIN THE BAND 13.553-13.567 MHz**



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 60090

#### APPENDIX A

#### 1.0 CONDUCTED EMISSION MEASUREMENTS

The conducted emissions were measured over the frequency range from 150 kHz to 30 MHz in accordance with the power line measurements, as specified in ANSI C63.4-2003. Since the device is operated from the public utility lines, the 120 Vac, 60 Hz power leads, high and low sides were measured by connecting the measuring equipment to the appropriate meter terminal of the LISN. All signals were then recorded. The allowed levels for Intentional Radiators cannot exceed 250 uV (47.96 dBuV) at any frequency between 150 kHz and 30 MHz, as stated in Section 15.207a.



Company:StrykerModel Tested:5100-0Report Number:11418

Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 60090

APPENDIX A

## CONDUCTED DATA AND GRAPHS

## TAKEN DURING TESTING

PART 15.207


#### FCC Part 15 Class B

#### Voltage Mains Test

EUT: TPS Plus new control board Manufacturer: Stryker Operating Condition: 70 deg. F, 44% R.H. Test Site: DLS O.F. Screen Room Operator: Craig Brandt Test Specification: 120 VAC; 60 Hz Comment: Line 1 Date: 05-31-2005

#### SCAN TABLE: "FCC ClassB Voltage"

Short Desc	ription:	I	FCC Class B	Voltage		
Start	Stop	Step	Detector	Meas.	IF	Transducer
Frequency	Frequency	Width		Time	Bandw.	
150.0 kHz	30.0 MHz	2.0 kHz	MaxPeak	10.0 ms	9 kHz	LISN DLS#128
			Average			

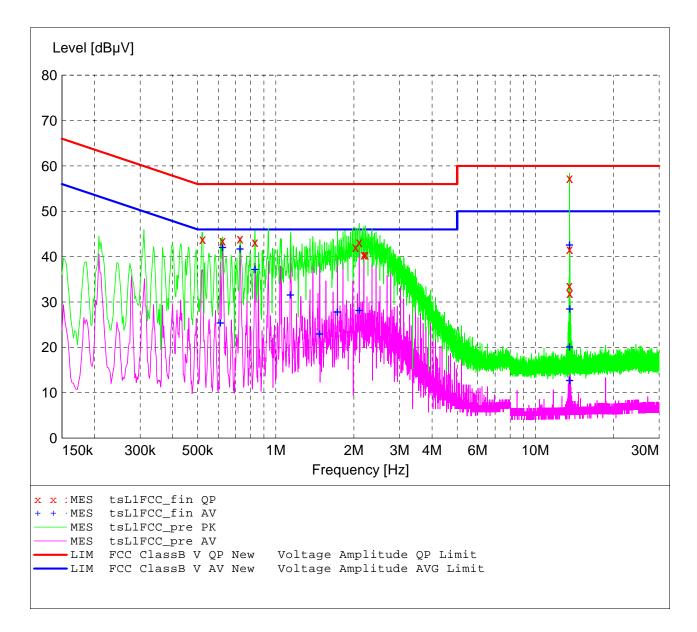

### MEASUREMENT RESULT: "tsL1FCC\_fin QP"

5/31/2005 12:0 Frequency MHz	)9PM Level dBµV	Transd dB	Limit dBµV	Margin dB	Line	PE
0.522000	43.90	10.3	56	12.1		
0.624000	43.50	10.3	56	12.5		
0.728000	44.00	10.3	56	12.0		
0.830000	43.20	10.3	56	12.8		
2.032000	42.10	10.4	56	13.9		
2.096000	43.20	10.4	56	12.8		
2.184000	40.40	10.3	56	15.6		
2.216000	40.50	10.3	56	15.5		
13.548000	33.60	10.7	60	26.4		
13.560000	57.30	10.7	60	2.7		Tx fundamental
13.568000	41.70	10.7	60	18.3		
13.576000	32.00	10.7	60	28.0		

## MEASUREMENT RESULT: "tsl1FCC\_fin AV"

5/31/2005 12 Frequency MHz	2:09PM Level dBµV	Transd dB	Limit dBµV	Margin dB	Line	PE
0.612000	25.60	10.3	46	20.4		
0.624000	42.20	10.3	46	3.8		
0.728000	41.90	10.3	46	4.1		
0.832000	37.40	10.3	46	8.6		
1.138000	31.70	10.3	46	14.3		
1.476000	23.10	10.3	46	22.9		
1.728000	28.00	10.3	46	18.0		
2.096000	28.30	10.4	46	17.7		
13.548000	20.30	10.7	50	29.7		
13.558000	42.80	10.7	50	7.2		Tx fundamental
13.568000	28.60	10.7	50	21.4		
13.578000	12.90	10.7	50	37.1		


### FCC Part 15 Class B

### Voltage Mains Test

EUT: TPS Plus new control board Manufacturer: Stryker Operating Condition: 70 deg. F, 44% R.H. Test Site: DLS O.F. Screen Room Operator: Craig Brandt Test Specification: 120 VAC; 60 Hz Comment: Line 2 Date: 05-31-2005

### SCAN TABLE: "FCC ClassB Voltage"

Short Desc	ription:	I	FCC Class B	Voltage		
Start	Stop	Step	Detector	Meas.	IF	Transducer
Frequency	Frequency	Width		Time	Bandw.	
150.0 kHz	30.0 MHz	2.0 kHz	MaxPeak	10.0 ms	9 kHz	LISN DLS#128
			Average			

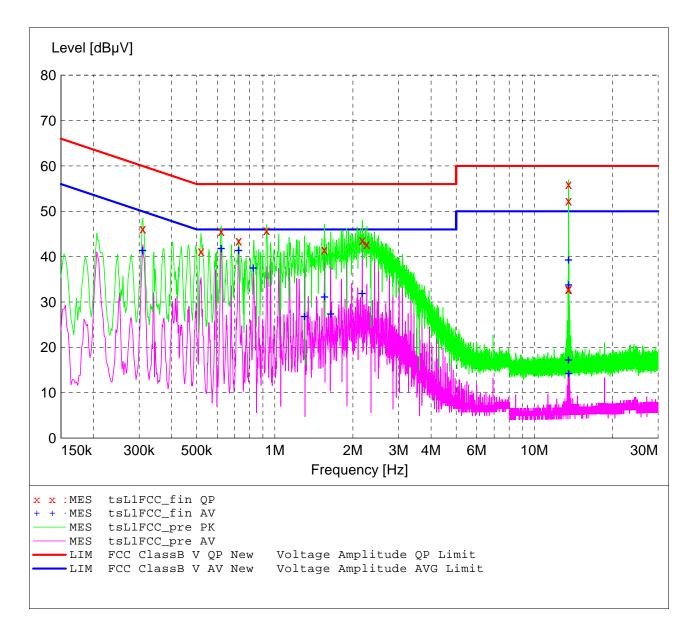

### MEASUREMENT RESULT: "tsL1FCC\_fin QP"

5/31/2005 12: Frequency MHz	16PM Level dBµV	Transd dB	Limit dBµV	Margin dB	Line	PE
0.310000	46.20	10.5	60	13.7		
0.520000	41.20	10.3	56	14.8		
0.622000	45.60	10.3	56	10.4		
0.726000	43.50	10.3	56	12.5		
0.930000	45.80	10.3	56	10.2		
1.554000	41.50	10.3	56	14.5		
2.174000	43.60	10.3	56	12.4		
2.262000	42.80	10.3	56	13.2		
13.546000	32.80	10.7	60	27.2		
13.558000	56.00	10.7	60	4.0		Tx fundamental
13.564000	52.40	10.7	60	7.6		
13.574000	33.00	10.7	60	27.0		

## MEASUREMENT RESULT: "tsl1FCC\_fin AV"

5/31/2005 Frequenc MI	12:16PM Cy Level Hz dBµV	Transd dB	Limit dBµV	Margin dB	Line	PE
0.3100	00 41.50	10.5	50	8.5		
0.62200	42.00	10.3	46	4.0		
0.72600	0 41.50	10.3	46	4.5		
0.8280	37.70	10.3	46	8.3		
1.30200	27.00	10.3	46	19.0		
1.55400	31.30	10.3	46	14.7		
1.64200	27.50	10.3	46	18.5		
2.1720	32.10	10.3	46	13.9		
13.5460	17.40	10.7	50	32.6		
13.5560	39.40	10.7	50	10.6		Tx fundamental
13.56600	33.90	10.7	50	16.1		
13.5760	14.40	10.7	50	35.6		



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX A

## 2.0 BAND EDGE AND RESTRICT BAND COMPLIANCE

The field strength of any emissions appearing outside the 13.553 to 13.567 MHz band shall not exceed the general radiated emissions limits as stated Section 15.209. The fundamental from the TPS Irrigation Console w/ Stryker Electronics Control Board transmitter shall not be inside the restrict band 13.36 to 13.41 MHz.

**NOTE:** See the following page (s) for the graph (s) made showing compliance for Band Edge and Restrict Band:



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 60090

APPENDIX A

## GRAPH (s) TAKEN SHOWING THE BAND EDGE AND RESTRICT BAND COMPLIANCE

PART 15.225 (b)




Stryker Instruments 5100-050-000 11418

### 1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX A

Test Date:	05-31-2005
Company:	Stryker
EUT:	TPS Plus New Control Board
Test:	Fundamental and Band Edges
Operator:	Craig Brandt

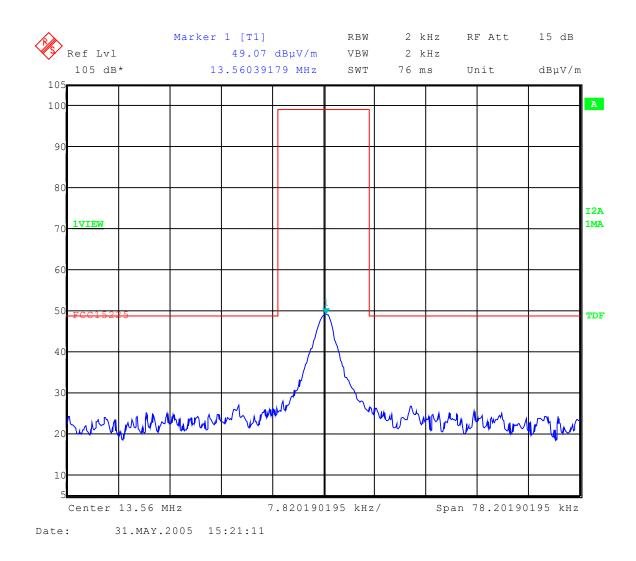



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX A

## 3.0 FIELD STRENGTH OF SPURIOUS EMISSION MEASUREMENTS (SECTION 15.225a & b)

The radiated measurements made at D.L.S. Electronic Systems, Inc., for the TPS Irrigation Console w/ Stryker Electronics Control Board, Model Number: 5100-050-000, are shown in tabulated and graph form. Preliminary radiation measurements were performed at a 3 meter test distance with the limits adjusted linearly when required. The frequency range from 9 kHz to over 960 MHz, depending upon the fundamental frequency as stated in Part 15.33a, was automatically scanned and plotted at various angles.

Measurements for the TPS Irrigation Console w/ Stryker Electronics Control Board were made up to 1000 MHz, in accordance with Section 15.33a for Intentional Radiators with a fundamental frequency of 13.56 MHz. For intentional radiators, the frequency range to be investigated is determined by the lowest radio frequency generated by the device without going below 9 kHz, up to at least the tenth harmonic of the highest fundamental frequency or 1000 MHz, whichever is lower. At those frequencies where significant signals were detected, measurements were made at an open field test site, located at Genoa City, Wisconsin, FCC file number **31040/SIT**, to determine the actual radiation levels.

All signals in the frequency range of 9 kHz to 30 MHz were measured with a low frequency Loop Antenna as a pickup device. From 30 to 200 MHz, a Biconical Antenna or tuned dipoles were used and from 200 MHz to 1000 MHz, a Log Periodic or Tuned Dipoles were used. During the test the equipment was rotated and the antenna was raised and lowered from 1 meter to 4 meters to find the maximum level. In order to find maximum emissions, the cables were moved through all the positions the equipment would be expected to experience in the field. Tests were made in the vertical polarization with the Loop Antenna, rotated 360° around its vertical axis. Tests were also made in both the horizontal and vertical planes of polarization with the Biconical and Log Periodic. In each case, the table was rotated to find the maximum emissions.

When the equipment is out of limit at 3 meters, and the signals from the equipment at 30 meters cannot be recorded due to the background, a representative sample of these frequencies were remeasured at various distances such as 4, 5, 6, 8, 15 meters and the greatest distance that can be measured to demonstrate graphically that the emissions are dropping off and will be under the limit at the specified distance. All signals were then recorded. The allowed levels for Intentional Radiators in the 13.553 MHz to 13.567 MHz band shall not exceed 10,000 uV measured at 30 meters. The field strength of any emissions appearing outside of this band shall not exceed the radiated emissions limits shown in Section 15.209.



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 60090

APPENDIX A

## RADIATED DATA AND GRAPHS TAKEN FOR

## FUNDAMENTAL FIELD STRENGTH

## SPURIOUS EMISSION MEASUREMENTS

PART 15.225

## FCC Part 15.209/225


# Spurious Radiated Emissions

EUT: TPS Plus new control board Manufacturer: Stryker Operating Condition: 75 degF; 47%R.H. Test Site: D.L.S. O.F. Site 2 Operator: Craig Brandt Test Specification: 120 VAC; 60 Hz Comment: Date: 5/31/2005

# TEXT: "Site 2 LowH 10M Act"

Short Description: Test Set-up 9kHz to 30MHz H TEST EQUIPMENT: Receiver --- Rohde&Schwarz ESI 40 SN: 837808/005 Antennas --- EMCO Active Loop Model: 6502 SN: 2038

TEST SET-UP: EuT Measured at 10 Meters with Loop Antenna

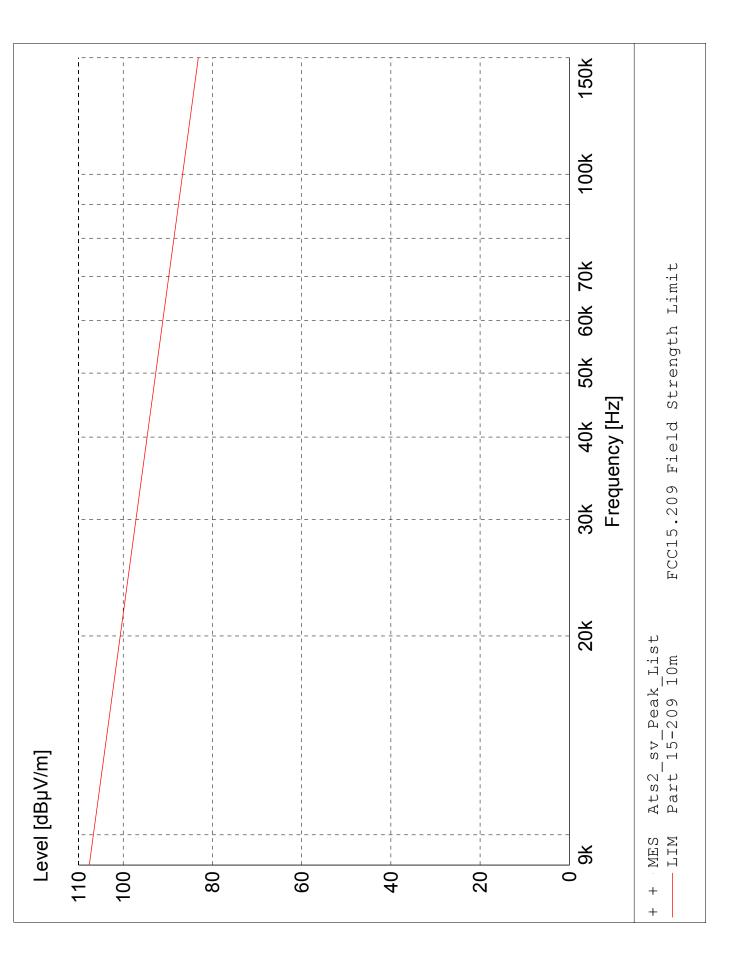

## FCC Part 15.209/225


# Spurious Radiated Emissions

EUT: TPS Plus new control board Manufacturer: Stryker Operating Condition: 75 degF; 47%R.H. Test Site: D.L.S. O.F. Site 2 Operator: Craig Brandt Test Specification: 120 VAC; 60 Hz Comment: Date: 5/31/2005

# TEXT: "Site 2 LOWH 10M Act"

Short Description: Test Set-up 9kHz to 30MHz H TEST EQUIPMENT: Receiver --- Rohde&Schwarz ESI 40 SN: 837808/005 Antennas --- EMCO Active Loop Model: 6502 SN: 2038

TEST SET-UP: EuT Measured at 10 Meters with Loop Antenna

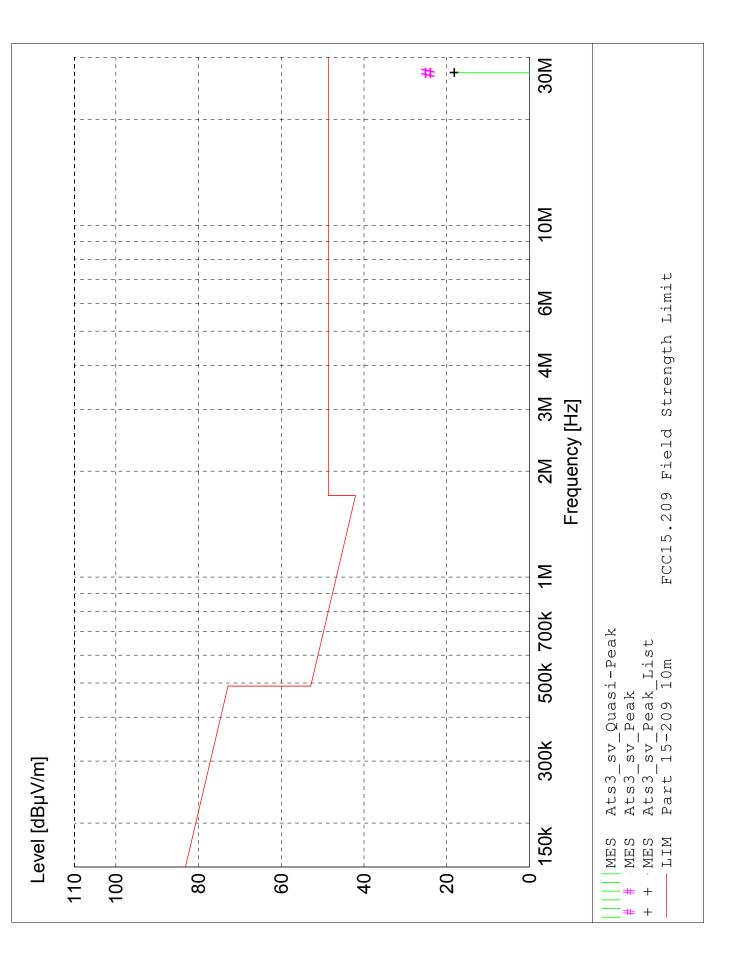

## MEASUREMENT RESULT: "Ats3\_sv\_Final"

5/31/2005 2:07PM

Frequency	Level	Antenna	System	Total	Limit	Margin	Height	EuT	Final	Comment
MHz	dBµV	Factor dBµV/m	Loss dB	Level dBµV/m		dB	Ant. m	Angle deg	Detector	
27.120000 27.120000	14.12 7.08	8.69 8.69	1.7 1.7	24.5 17.4	48.6 48.6	24.2 31.2			MAX PEAK QUASI-PEAK	None None



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 60090

APPENDIX A

## RADIATED DATA TAKEN FOR

## FIELD STRENGTH

## SPURIOUS EMISSION MEASUREMENTS

PART 15.209

## FCC Part 15

## Electric Field Strength

EUT: TPS Plus new control board Manufacturer: Stryker Operating Condition: 64 degF; 57% R.H. Test Site: DLS O.F. Site 2 Operator: Craig Brandt Test Specification: 120 VAC; 60 Hz Comment:


Date: 05/31/2005

## TEXT: "Site 2 MidV 3M"

Short Description: Test Set-up Vert30-1000MHz TEST EQUIPMENT: Receiver --- Rohde&Schwarz ESI 40 SN: 837808/005

Antennas ---Biconical -- EMCO 3104C SN: 0005-4892 Log Periodic -- Electro Metrics LPA-25 SN: 1205 Pre-Amp --- Rohde&Schwarz TS-PR10 SN: 032001/004

EuT Measured at 3 Meters with VERTICAL Antenna Polarisation TEST SET-UP:

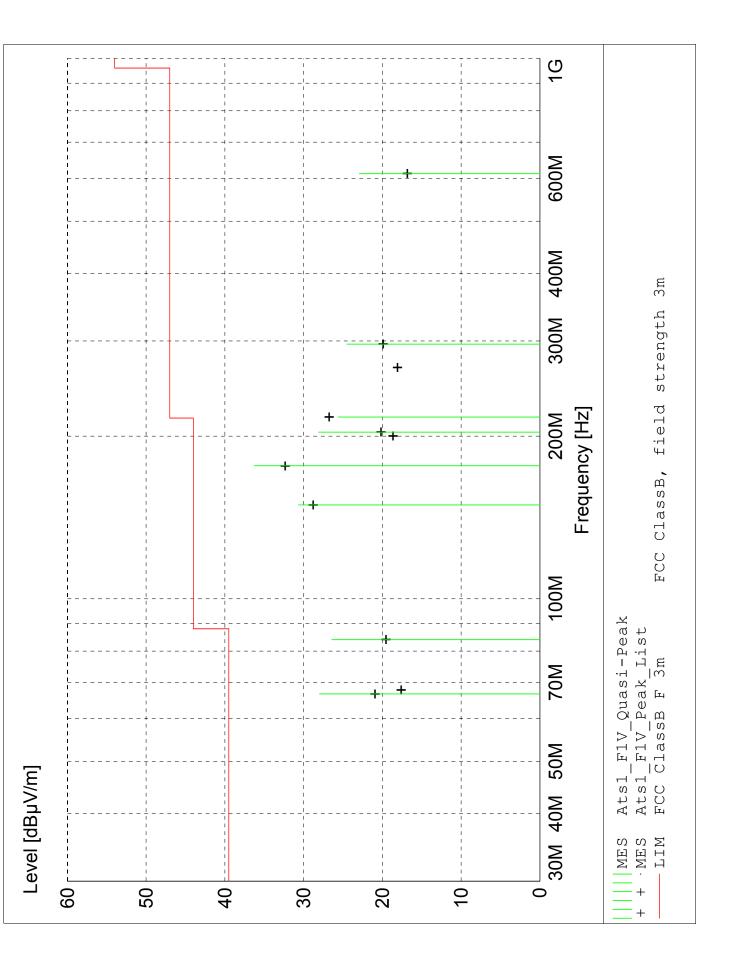

## MEASUREMENT RESULT: "Ats1\_F1V\_Final"

5/31/2005 10:48AM

Frequency	Level	Antenna	System	Total	Limit	Margin	Height	EuT	Final	Comment
MHz	dBµV	Factor dBµV/m	Loss dB	Level dBµV/m	dBµV/m	dB	Ant. m	Angle deg	Detector	
176.275400	43.09	15.81	-22.6	36.3	44.0	7.7	1.00	180	QUASI-PEAK	None
66.665000	43.89	7.79	-23.7	28.0	39.5	11.5	1.00	180	QUASI-PEAK	None
83.995000	41.96	7.83	-23.3	26.4	39.5	13.1	1.00	45	QUASI-PEAK	None
149.152900	41.41	12.19	-22.9	30.6	44.0	13.4	1.00	180	QUASI-PEAK	None
203.388000	38.99	11.55	-22.4	28.1	44.0	15.9	1.00	135	QUASI-PEAK	None
216.947000	36.67	11.36	-22.4	25.6	47.0	21.4	1.00	270	QUASI-PEAK	None
295.990000	32.23	14.32	-22.0	24.5	47.0	22.5	1.00	270	QUASI-PEAK	None
611.970000	24.02	18.98	-20.1	22.9	47.0	24.1	1.00	200	QUASI-PEAK	None

## FCC Part 15

## Electric Field Strength

EUT: TPS Plus new control board Manufacturer: Stryker Operating Condition: 64 degF; 57% R.H. Test Site: DLS O.F. Site 2 Operator: Craig Brandt Test Specification: 120 VAC; 60 Hz Comment:


Date: 05/31/2005

## TEXT: "Site 2 MidH 3M"

Short Description: Test Set-up Horz30-1000MHz TEST EQUIPMENT: Receiver --- Rohde&Schwarz ESI 40 SN: 837808/005

Antennas ---Biconical -- EMCO 3104C SN: 0005-4892 Log Periodic -- Electro Metrics LPA-25 SN: 1205 Pre-Amp --- Rohde&Schwarz TS-PR10 SN: 032001/004

EuT Measured at 3 Meters with HORIZONTAL Antenna Polarisation TEST SET-UP:

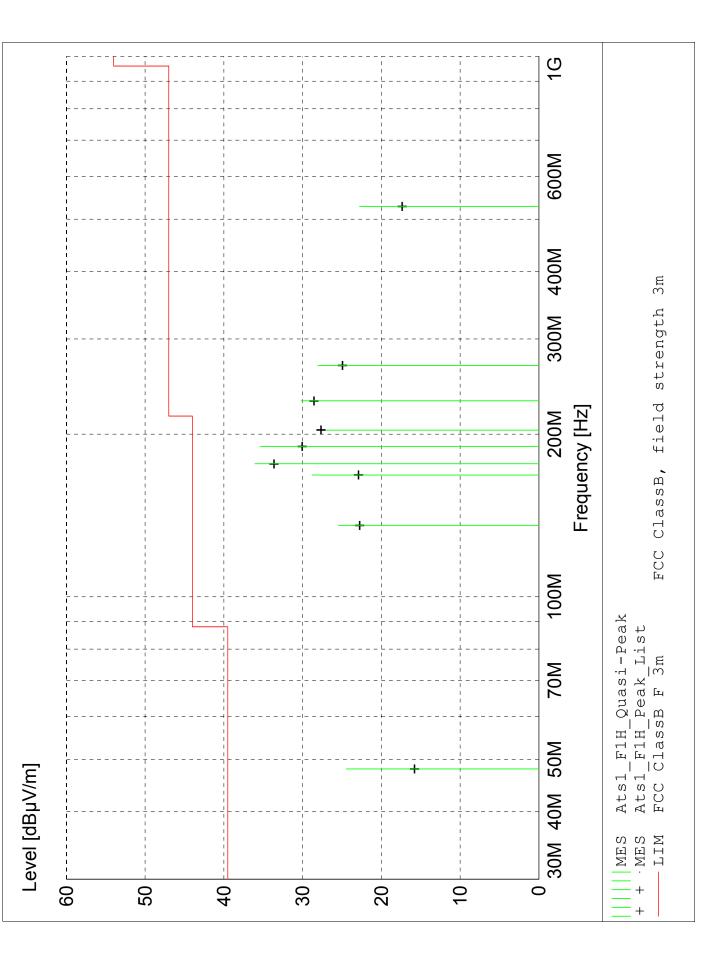

## MEASUREMENT RESULT: "Ats1\_F1H\_Final"

5/31/2005 10:41AM

Frequency	Level	Antenna Factor	System Loss	Total Level	Limit	Margin	Height Ant.	EuT Angle	Final Detector	Comment
MHz	dBµV	dBµV/m	dB	dBµV/m	dBµV/m	dB	m	deg		
176.270500	42.89	15.81	-22.6	36.1	44.0	7.9	2.00	180	QUASI-PEAK	None
189.825900	40.84	17.05	-22.5	35.4	44.0	8.6	2.00	135	QUASI-PEAK	None
47.990000	36.73	11.64	-23.9	24.5	39.5	15.0	3.00	225	QUASI-PEAK	None
167.995000	37.27	14.29	-22.8	28.8	44.0	15.2	2.00	90	QUASI-PEAK	None
230.509100	41.08	11.44	-22.3	30.2	47.0	16.8	1.00	215	QUASI-PEAK	None
203.388000	37.90	11.55	-22.4	27.0	44.0	17.0	2.00	180	QUASI-PEAK	None
135.584200	36.20	12.27	-23.0	25.5	44.0	18.5	2.50	100	QUASI-PEAK	None
267.984300	37.42	12.91	-22.3	28.1	47.0	18.9	1.00	180	QUASI-PEAK	None
527.980000	25.69	17.71	-20.6	22.8	47.0	24.2	1.00	40	QUASI-PEAK	None



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX A

## 4.0 FREQUENCY STABILITY - PART 2.1055a (Temperature)

The frequency stability was measured from  $-30^{\circ}$  to  $+50^{\circ}$  centigrade at intervals of  $10^{\circ}$  centigrade throughout the range. Prior to each frequency measurement, the equipment was left alone for a sufficient period of time (approximately 30 minutes or more) to allow the components of the TPS Irrigation Console w/ Stryker Electronics Control Board oscillator circuitry to stabilize. The following information was taken:

## FREQUENCY STABILITY FOR TEMPERATURE VARIATION IN MHz:

-20°	0
-10°	0
0°	0
+10°	0
+20°	0
+30°	0
+40°	0
+50°	0

Worst Case Variance:

0 Hz

As stated in Part 15, Section 15.225 (c), the Frequency Tolerance and Margin for this range are as follows:

Ambient Frequency: = 0.00 Hz

Frequency Tolerance: = 0

0.00 \* 0 = 0 Hz



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 60090

APPENDIX A

## **GRAPHS** TAKEN FOR FREQUENCY

## STABILITY WHEN VARYING THE

## TEMPERATURE

## PART 2.1055A



1250 Peterson Dr., Wheeling, IL 60090

## APPENDIX A

## 5.0 FREQUENCY STABILITY - PART 2.1055d (Voltage)

The frequency stability of TPS Irrigation Console w/ Stryker Electronics Control Board was measured by varying the primary supply voltage from 85% to 115% of nominal value for all equipment other than hand carried battery equipment.

## **FREQUENCY STABILITY FOR VOLTAGE VARIATION:**

85%	0
100%	0
115%	0

## The changes made to the unit do not effect the transmitter circuitry, thereby this test was not performed.

## FREQUENCY STABILITY FOR HAND HELD DEVICES:

For hand carried, battery powered equipment, the supply voltage was reduced to the battery operating end point specified by the manufacturer. Readings were taken at the reduced end point and with a fresh battery:

## Fresh Battery verses Battery end point:

Frequency #1	0 Hz
Frequency #2	0 Hz
Frequency #3	0 Hz
Frequency #4	0 Hz
Frequency #5	0 Hz
Frequency #6	0 Hz

As stated in Part 15, Section 15.225 (c), the Frequency Tolerance and Margin for this range are as follows:

**Frequency Tolerance:** 

Limit: <u>0 Hz</u>

0



Stryker Instruments 5100-050-000 11418

1250 Peterson Dr., Wheeling, IL 60090

APPENDIX A

## GRAPHS TAKEN FOR FREQUENCY

## STABILITY WHEN VARYING THE

## PRIMARY SUPPLY VOLTAGE

PART 2.1055d