


INTERNAL PHOTO OF SAMPLE-1



INTERNAL PHOTO OF SAMPLE-2

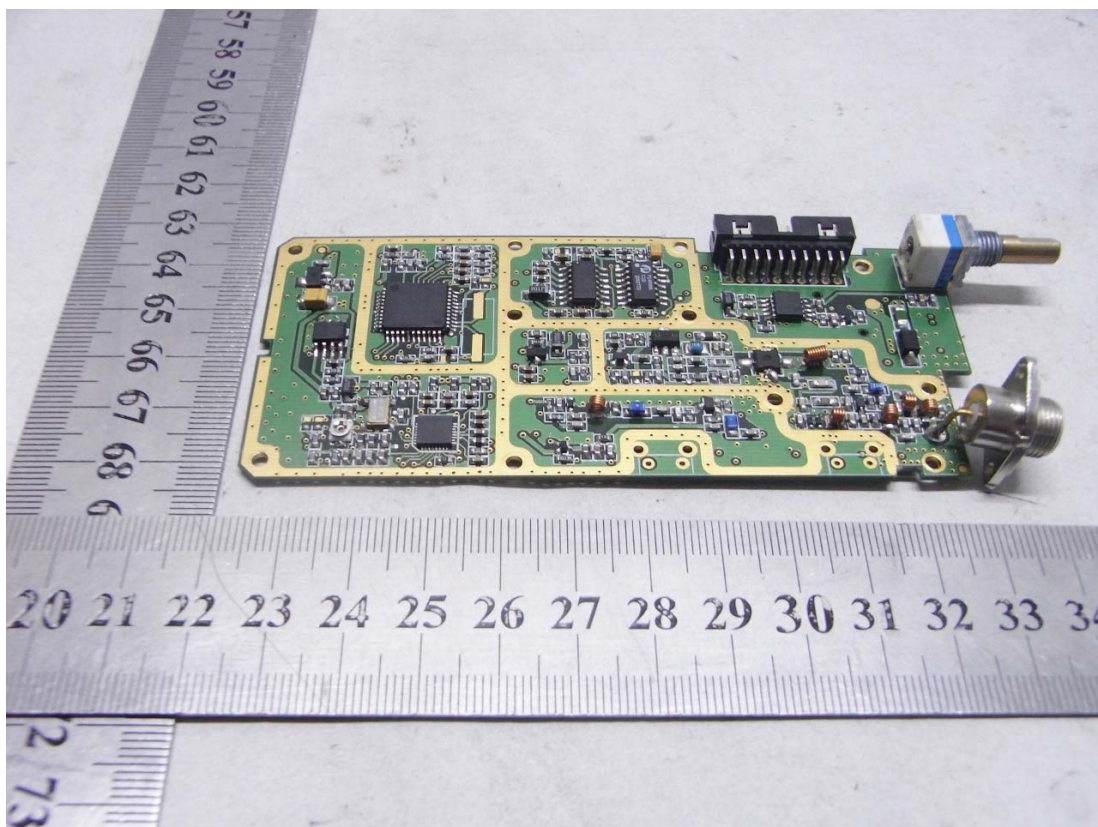