

Client **CCS, USA**

## CALIBRATION CERTIFICATE

Object(s) **ES3DV2 - SN:3021**

Calibration procedure(s) **QA CAL-01.v2  
Calibration procedure for dosimetric E-field probes**

Calibration date: **July 29, 2003**

Condition of the calibrated item **In Tolerance (according to the specific calibration document)**

This calibration statement documents traceability of M&TE used in the calibration procedures and conformity of the procedures with the ISO/IEC 17025 international standard.

All calibrations have been conducted in the closed laboratory facility: environment temperature 22 +/- 2 degrees Celsius and humidity < 75%.

Calibration Equipment used (M&TE critical for calibration)

Model Type	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
RF generator HP 8684C	US3642U01700	4-Aug-99 (SPEAG, in house check Aug-02)	In house check: Aug-05
Power sensor E4412A	MY41495277	2-Apr-03 (METAS, No 252-0250)	Apr-04
Power sensor HP 8481A	MY41092180	18-Sep-02 (Agilent, No. 20020918)	Sep-03
Power meter EPM E4419B	GB41293874	2-Apr-03 (METAS, No 252-0250)	Apr-04
Network Analyzer HP 8753E	US37390585	18-Oct-01 (Agilent, No. 24BR1033101)	In house check: Oct 03
Fluke Process Calibrator Type 702	SN: 6295803	3-Sep-01 (ELCAL, No.2360)	Sep-03

	Name	Function	Signature
Calibrated by:	Katja Pokovic	Laboratory Director	

Approved by:	Fin Bomholt	R&D Director	
--------------	-------------	--------------	---

Date issued: July 29, 2003

This calibration certificate is issued as an intermediate solution until the accreditation process (based on ISO/IEC 17025 International Standard) for Calibration Laboratory of Schmid & Partner Engineering AG is completed.

Zeughausstrasse 43, 8004 Zurich, Switzerland  
Phone +41 1 245 9700, Fax +41 1 245 9779  
info@speag.com, <http://www.speag.com>

# Probe ES3DV2

## SN:3021

Manufactured:	December 5, 2002
Last calibration:	July 29, 2003

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

## DASY - Parameters of Probe: ES3DV2 SN:3021

### Sensitivity in Free Space

NormX	<b>1.43</b> $\mu\text{V}/(\text{V}/\text{m})^2$
NormY	<b>1.20</b> $\mu\text{V}/(\text{V}/\text{m})^2$
NormZ	<b>1.29</b> $\mu\text{V}/(\text{V}/\text{m})^2$

### Diode Compression

DCP X	<b>97</b>	mV
DCP Y	<b>97</b>	mV
DCP Z	<b>97</b>	mV

### Sensitivity in Tissue Simulating Liquid

**Head**                      **900 MHz**                       $\epsilon_r = 41.5 \pm 5\%$                        $\sigma = 0.97 \pm 5\%$  mho/m

Valid for f=800-1000 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	<b>6.5</b> $\pm 9.5\%$ (k=2)	Boundary effect:
ConvF Y	<b>6.5</b> $\pm 9.5\%$ (k=2)	Alpha <b>0.93</b>
ConvF Z	<b>6.5</b> $\pm 9.5\%$ (k=2)	Depth <b>0.96</b>

**Head**                      **1800 MHz**                       $\epsilon_r = 40.0 \pm 5\%$                        $\sigma = 1.40 \pm 5\%$  mho/m

Valid for f=1710-1910 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	<b>5.1</b> $\pm 9.5\%$ (k=2)	Boundary effect:
ConvF Y	<b>5.1</b> $\pm 9.5\%$ (k=2)	Alpha <b>0.21</b>
ConvF Z	<b>5.1</b> $\pm 9.5\%$ (k=2)	Depth <b>2.73</b>

### Boundary Effect

**Head**                      **900 MHz**                      Typical SAR gradient: 5 % per mm

Probe Tip to Boundary		<b>1 mm</b>	<b>2 mm</b>
SAR <sub>be</sub> [%] Without Correction Algorithm		3.8	1.5
SAR <sub>be</sub> [%] With Correction Algorithm		0.0	0.2

**Head**                      **1800 MHz**                      Typical SAR gradient: 10 % per mm


Probe Tip to Boundary		<b>1 mm</b>	<b>2 mm</b>
SAR <sub>be</sub> [%] Without Correction Algorithm		7.1	4.6
SAR <sub>be</sub> [%] With Correction Algorithm		0.0	0.2

### Sensor Offset


Probe Tip to Sensor Center	<b>2.1</b>	mm
----------------------------	------------	----

### Receiving Pattern ( $\phi$ , $\theta = 0^\circ$ )


**f = 30 MHz, TEM cell ifi110**

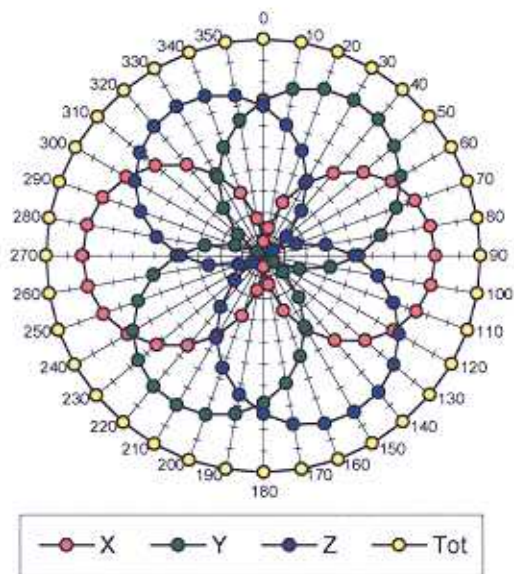


**f = 100 MHz, TEM cell ifi110**


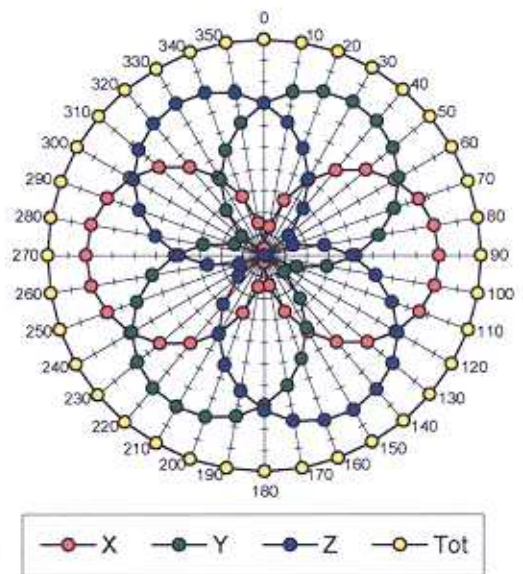


**f = 300 MHz, TEM cell ifi110**

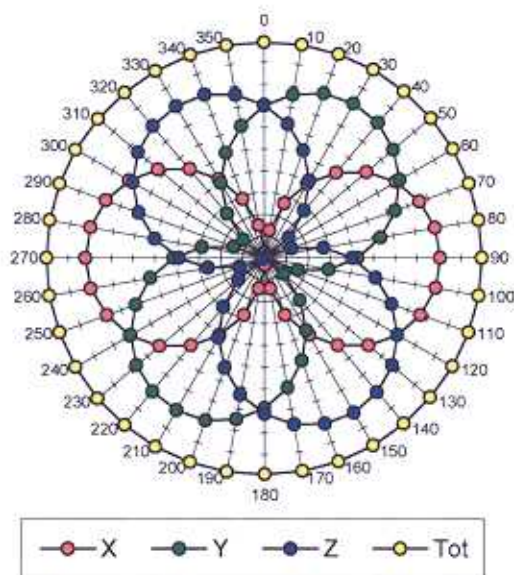


**f = 900 MHz, TEM cell ifi110**

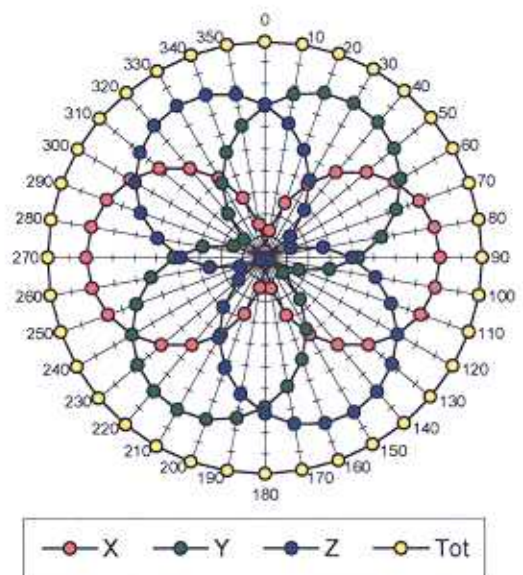

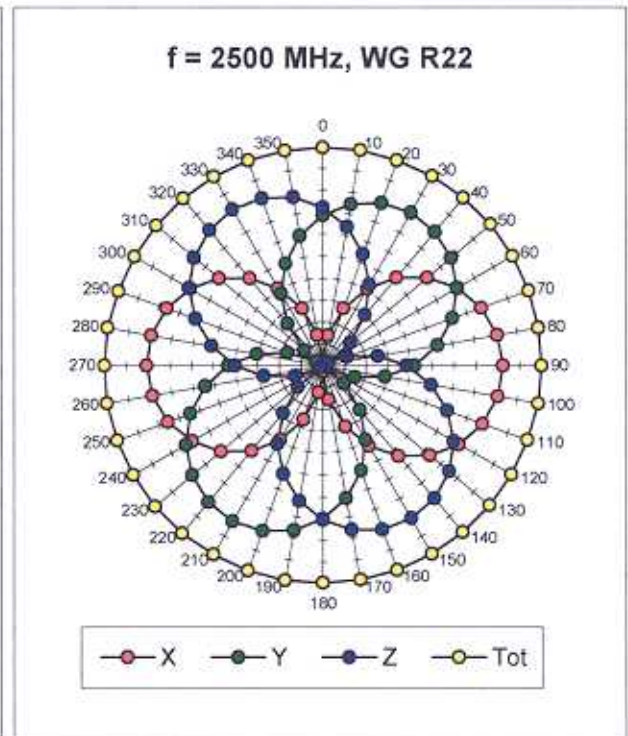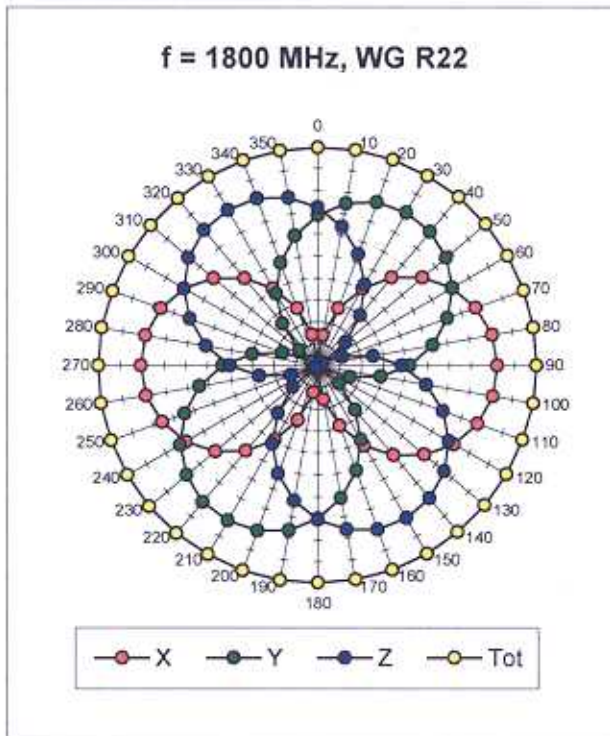


### Isotropy Error ( $\phi$ ), $\theta = 0^\circ$


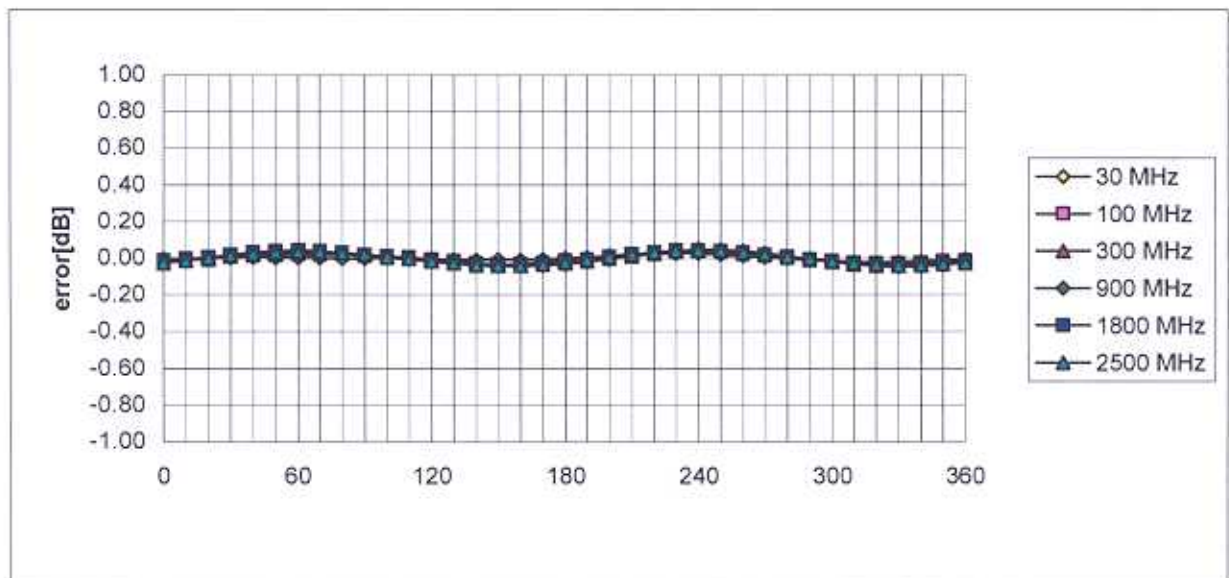


# Frequency Response of E-Field


( TEM-Cell:ifi110, Waveguide R22)

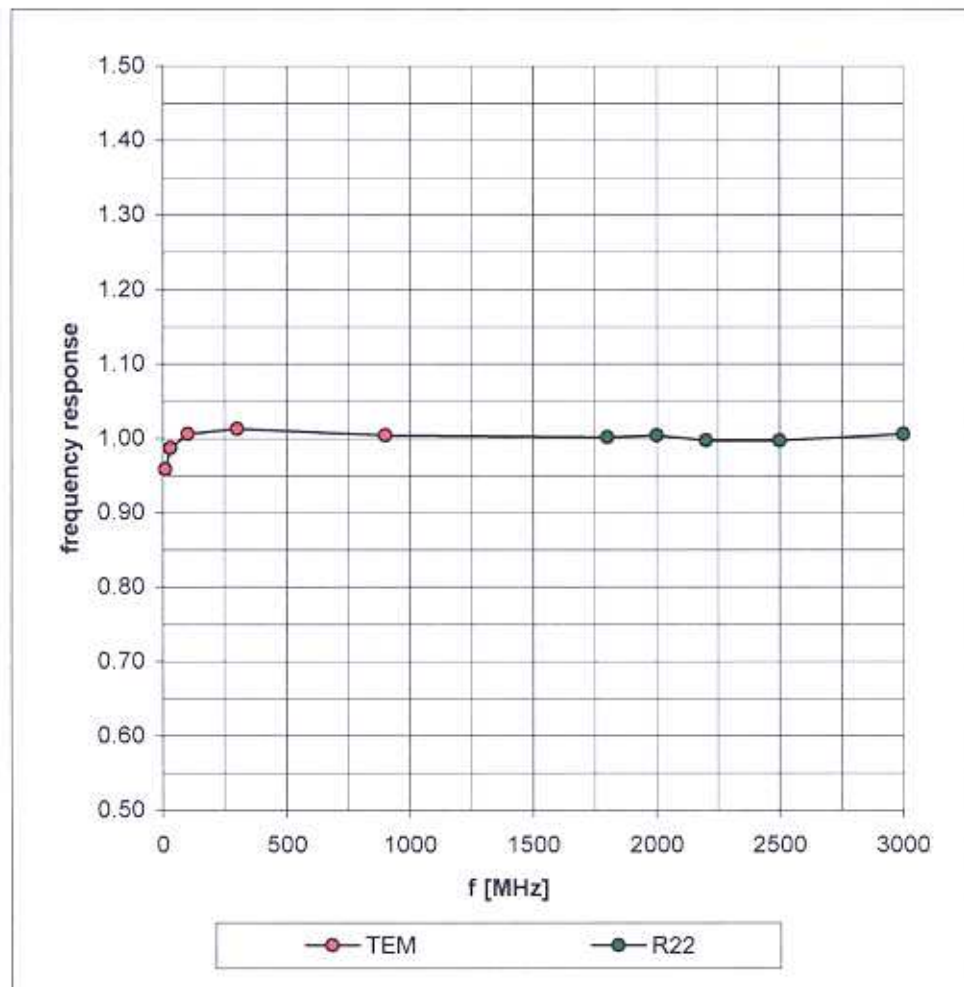

## Dynamic Range $f(\text{SAR}_{\text{brain}})$ ( Waveguide R22 )

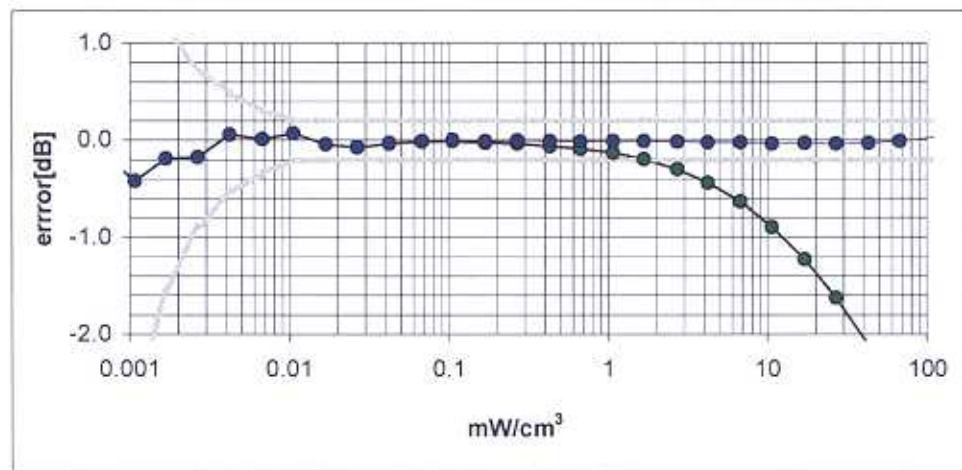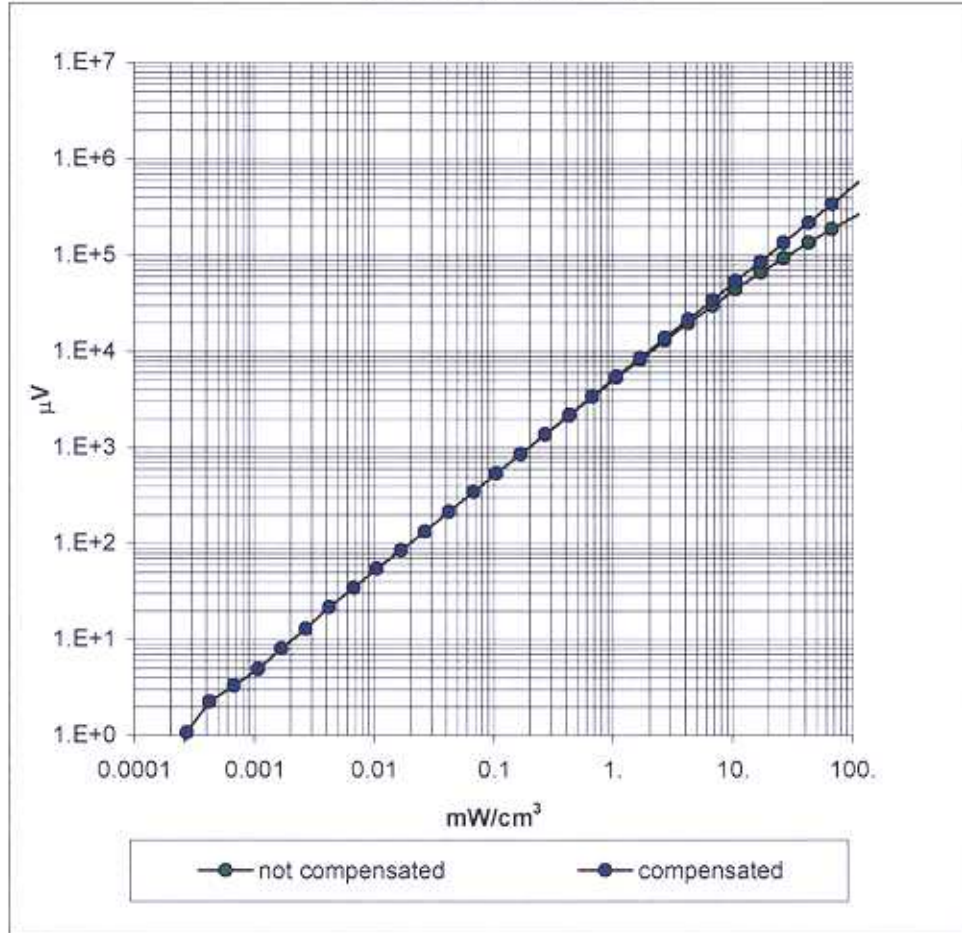

## Conversion Factor Assessment

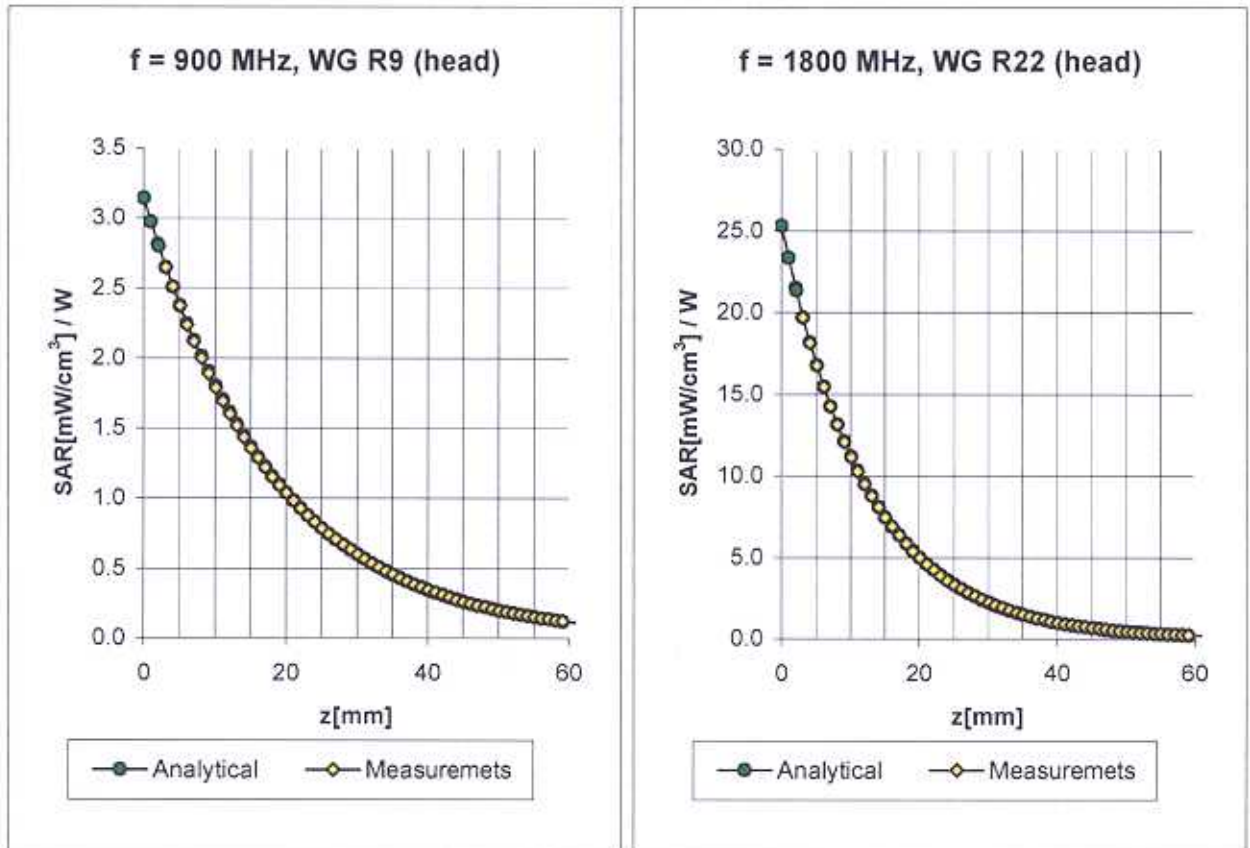

**Head                      900 MHz                       $\epsilon_r = 41.5 \pm 5\%$                        $\sigma = 0.97 \pm 5\%$  mho/m**

Valid for  $f=800-1000 \text{ MHz}$  with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	<b>6.5</b> $\pm 9.5\%$ (k=2)	Boundary effect:	
ConvF Y	<b>6.5</b> $\pm 9.5\%$ (k=2)	Alpha	<b>0.93</b>
ConvF Z	<b>6.5</b> $\pm 9.5\%$ (k=2)	Depth	<b>0.96</b>


**Head                      1800 MHz                       $\epsilon_r = 40.0 \pm 5\%$                        $\sigma = 1.40 \pm 5\%$  mho/m**

Valid for  $f=1710-1910 \text{ MHz}$  with Head Tissue Simulating Liquid according to EN 50361, P1528-200X

ConvF X	<b>5.1</b> $\pm 9.5\%$ (k=2)	Boundary effect:	
ConvF Y	<b>5.1</b> $\pm 9.5\%$ (k=2)	Alpha	<b>0.21</b>
ConvF Z	<b>5.1</b> $\pm 9.5\%$ (k=2)	Depth	<b>2.73</b>



## Conversion Factor Assessment

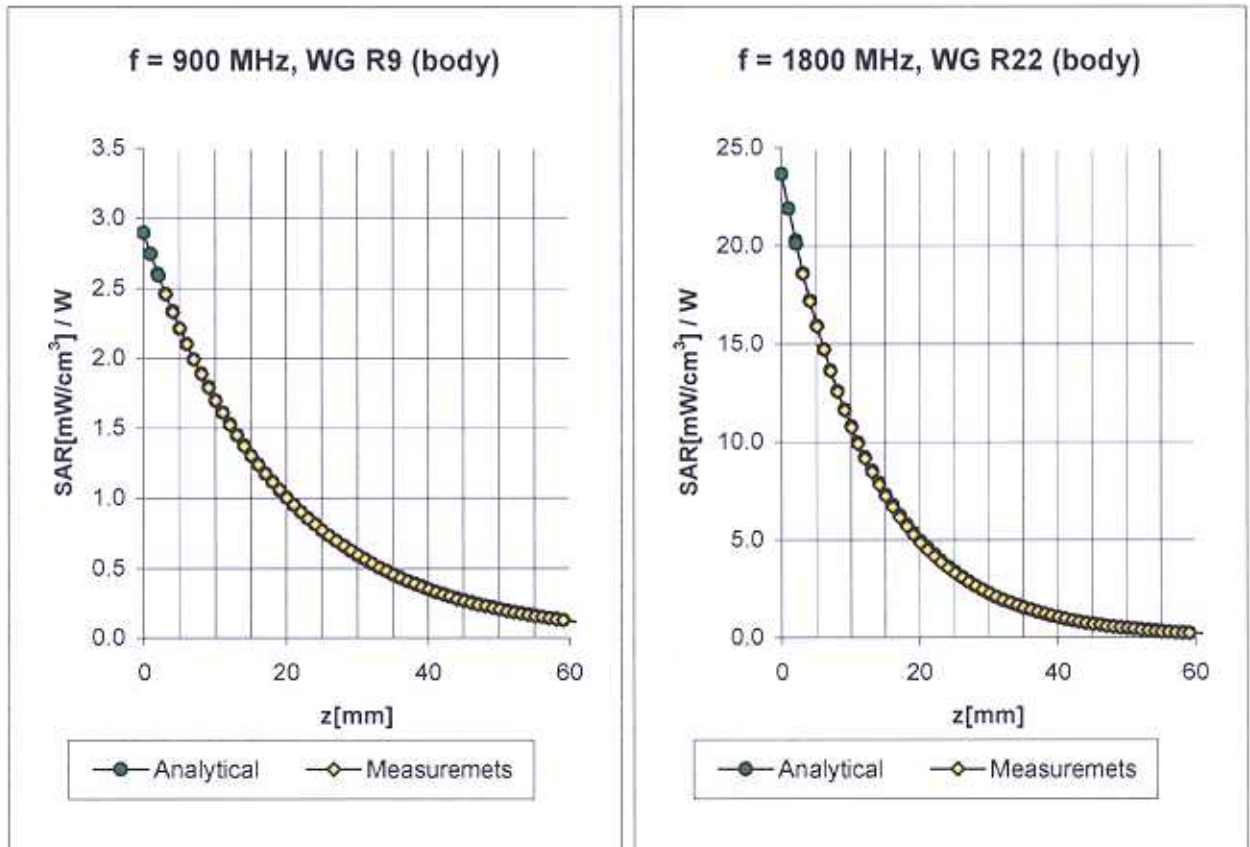

**Body**                      **900 MHz**                       $\epsilon_r = 55.0 \pm 5\%$                        $\sigma = 1.05 \pm 5\%$  mho/m

Valid for f=800-1000 MHz with Head Tissue Simulating Liquid according to OET 65 Suppl. C


ConvF X	<b>6.3</b> $\pm$ 9.5% (k=2)	Boundary effect:	
ConvF Y	<b>6.3</b> $\pm$ 9.5% (k=2)	Alpha	<b>0.58</b>
ConvF Z	<b>6.3</b> $\pm$ 9.5% (k=2)	Depth	<b>1.22</b>

**Body**                      **1800 MHz**                       $\epsilon_r = 53.3 \pm 5\%$                        $\sigma = 1.52 \pm 5\%$  mho/m

Valid for f=1710-1910 MHz with Head Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X	<b>4.8</b> $\pm$ 9.5% (k=2)	Boundary effect:	
ConvF Y	<b>4.8</b> $\pm$ 9.5% (k=2)	Alpha	<b>0.22</b>
ConvF Z	<b>4.8</b> $\pm$ 9.5% (k=2)	Depth	<b>2.90</b>

## Conversion Factor Assessment

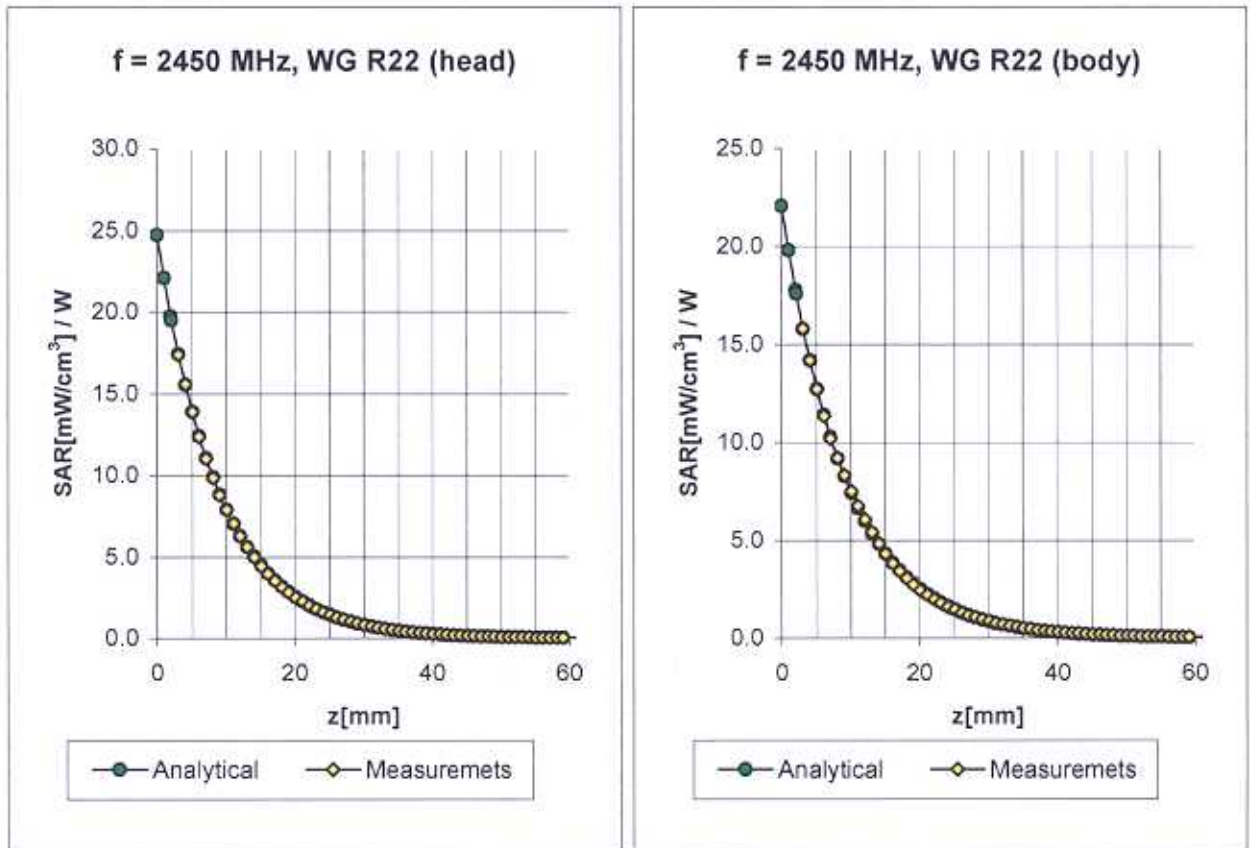

**Head**                      **2450 MHz**                       $\epsilon_r = 39.2 \pm 5\%$                        $\sigma = 1.80 \pm 5\%$  mho/m

Valid for f=2400-2500 MHz with Head Tissue Simulating Liquid according to EN 50361, P1528-200X


ConvF X	<b>4.5</b> $\pm$ 8.9% (k=2)	Boundary effect:
ConvF Y	<b>4.5</b> $\pm$ 8.9% (k=2)	Alpha <b>0.37</b>
ConvF Z	<b>4.5</b> $\pm$ 8.9% (k=2)	Depth <b>1.75</b>

**Body**                      **2450 MHz**                       $\epsilon_r = 52.7 \pm 5\%$                        $\sigma = 1.95 \pm 5\%$  mho/m

Valid for f=2400-2500 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X	<b>4.1</b> $\pm$ 8.9% (k=2)	Boundary effect:
ConvF Y	<b>4.1</b> $\pm$ 8.9% (k=2)	Alpha <b>0.27</b>
ConvF Z	<b>4.1</b> $\pm$ 8.9% (k=2)	Depth <b>2.54</b>

## Conversion Factor Assessment

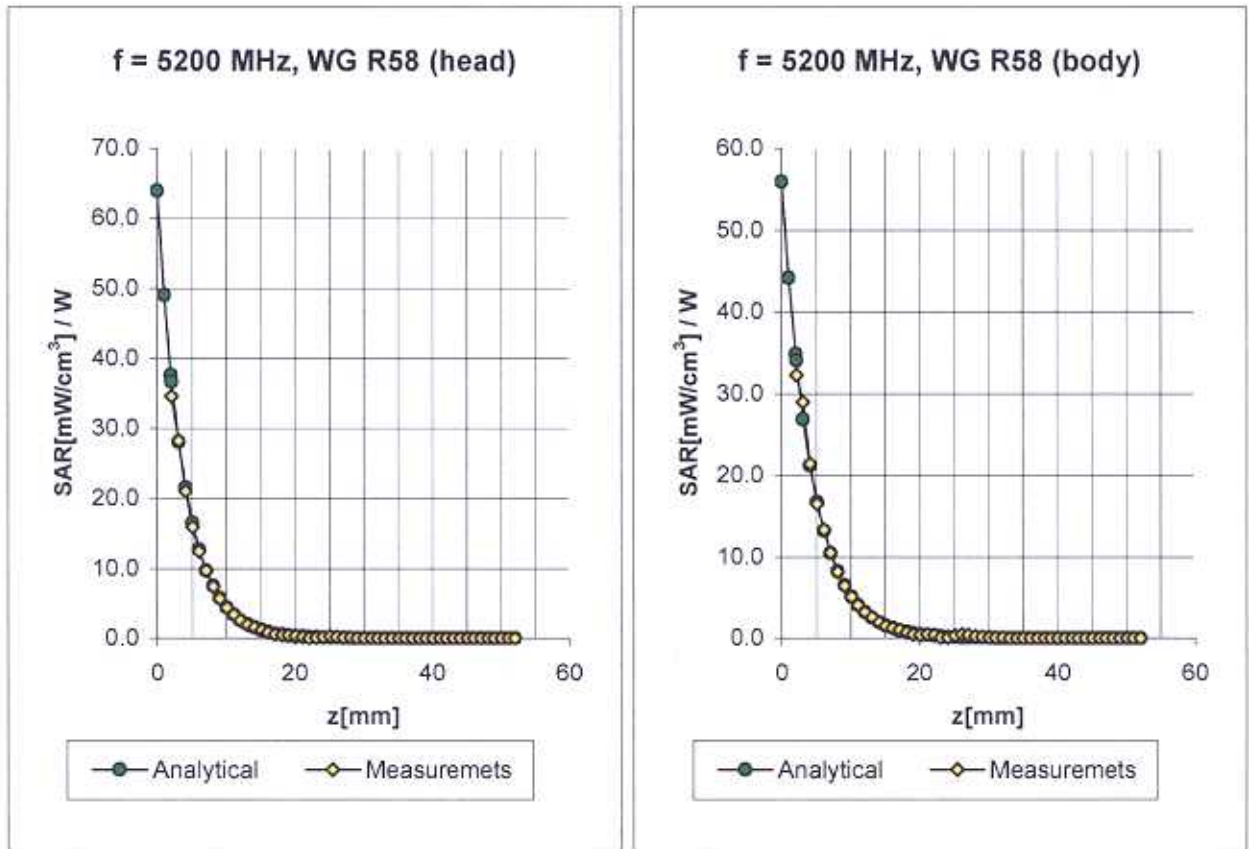

**Head**                      **5200 MHz**                       $\epsilon_r = 36.0 \pm 5\%$                        $\sigma = 4.66 \pm 5\%$  mho/m

Valid for f=4940-5460 MHz with Head Tissue Simulating Liquid according to OET 65 Suppl. C


ConvF X	2.2 ± 14.6% (k=2)	Boundary effect:
ConvF Y	2.2 ± 14.6% (k=2)	Alpha <b>0.99</b>
ConvF Z	2.2 ± 14.6% (k=2)	Depth <b>1.50</b>

**Body**                      **5200 MHz**                       $\epsilon_r = 49.0 \pm 5\%$                        $\sigma = 5.30 \pm 5\%$  mho/m

Valid for f=4940-5460 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X	1.4 ± 14.6% (k=2)	Boundary effect:
ConvF Y	1.4 ± 14.6% (k=2)	Alpha <b>1.12</b>
ConvF Z	1.4 ± 14.6% (k=2)	Depth <b>1.65</b>

## Conversion Factor Assessment

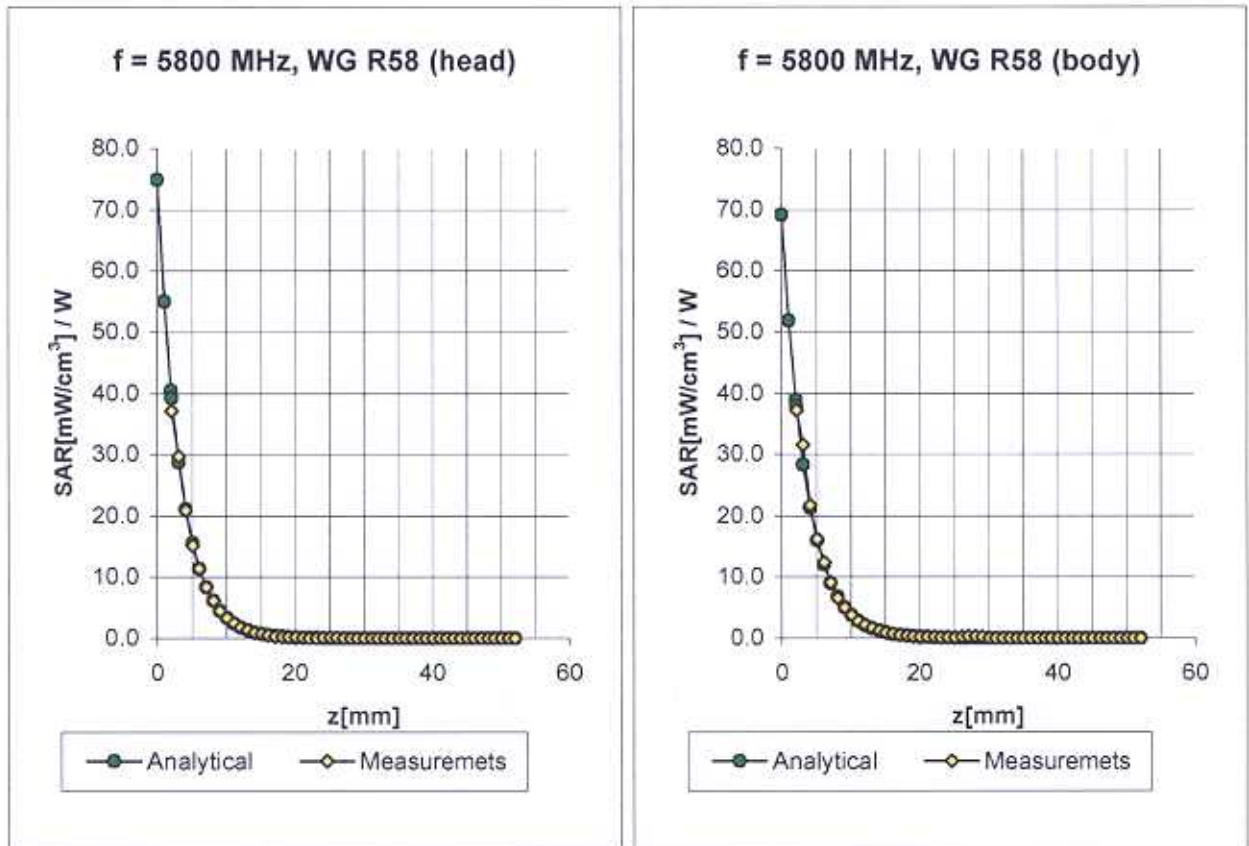

**Head**                      **5800 MHz**                       $\epsilon_r = 35.3 \pm 5\%$                        $\sigma = 5.27 \pm 5\%$  mho/m

Valid for f=5510-6090 MHz with Head Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X	1.8 ± 14.6% (k=2)	Boundary effect:
ConvF Y	1.8 ± 14.6% (k=2)	Alpha <b>1.15</b>
ConvF Z	1.8 ± 14.6% (k=2)	Depth <b>1.50</b>

**Body**                      **5800 MHz**                       $\epsilon_r = 48.2 \pm 5\%$                        $\sigma = 6.00 \pm 5\%$  mho/m

Valid for f=5510-6090 MHz with Body Tissue Simulating Liquid according to OET 65 Suppl. C

ConvF X	1.1 ± 14.6% (k=2)	Boundary effect:
ConvF Y	1.1 ± 14.6% (k=2)	Alpha <b>1.10</b>
ConvF Z	1.1 ± 14.6% (k=2)	Depth <b>1.75</b>

# Deviation from Isotropy in HSL

Error ( $\theta\phi$ ),  $f = 900$  MHz

