



Appendix A: Measurement Plots

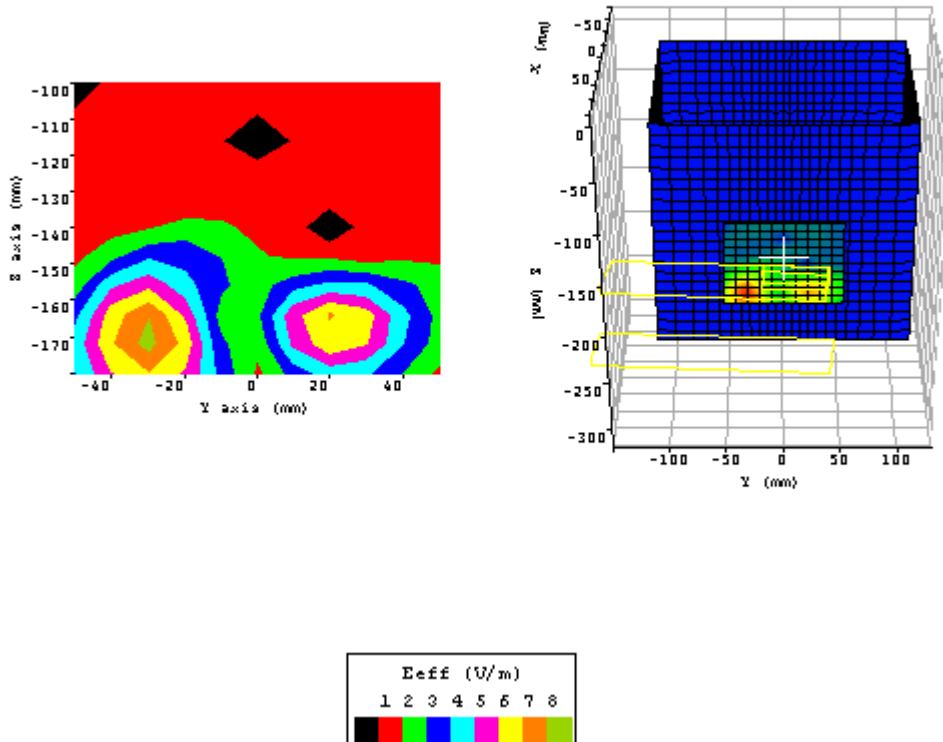

Plot 1.	
Date:	04/08/2003
Temperature Air / Liquid:	21.0°C / 21.0°C
Liquid mass density (ρ):	1
DCP ¹	20
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386
Probe S/N:0123 liquid/air conversion Factor	0.816
Simulated tissue dielectric parameters:	ϵ_r : 51.62 σ : 1.961
Transmit Antenna / Test Position	Right / bystander 5mm
Device Frequency	2437 MHz
Maximum 1 gram SAR:	0.166W/Kg
Maximum 10 gram SAR:	0.076/Kg
Power reference start:	0.032W/Kg
Power reference end	0.032W/Kg
Power reference change ²	-0.00%

¹ DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.


² The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

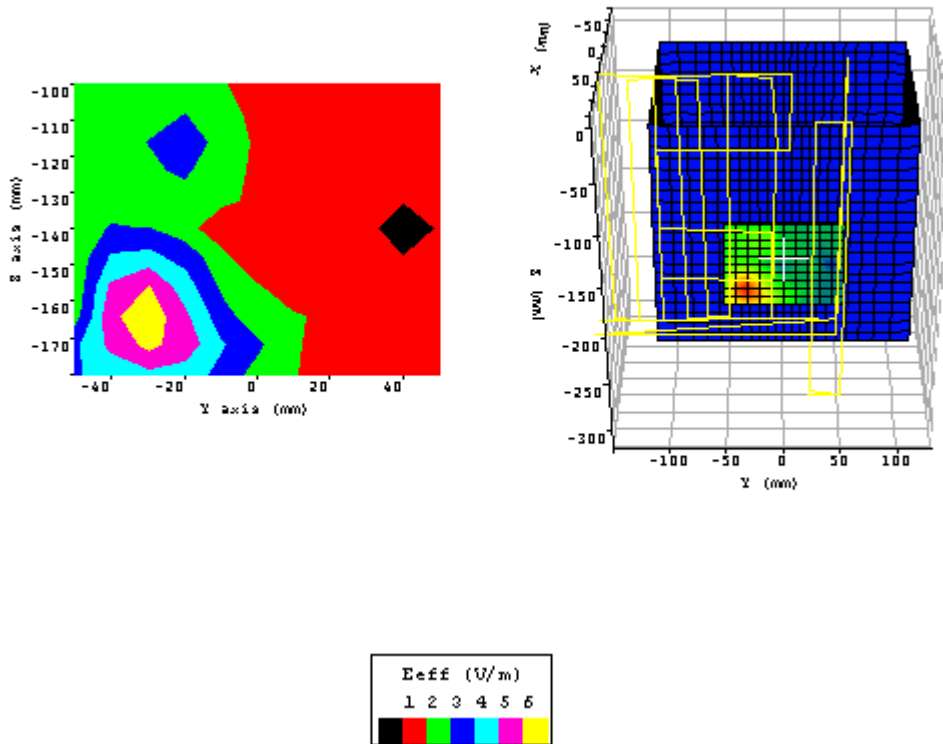

Plot 2.	
Date:	04/08/2003
Temperature Air / Liquid:	22.0°C / 21.0°C
Liquid mass density (ρ):	1
DCP ¹	20
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386
Probe S/N:0123 liquid/air conversion Factor	0.816
Simulated tissue dielectric parameters:	ϵ_r : 51.62 σ : 1.961
Transmit Antenna / Test Position	Right / lap
Device Frequency	2437 MHz
Maximum 1 gram SAR:	0.131W/Kg
Maximum 10 gram SAR:	0.063/Kg
Power reference start:	0.028W/Kg
Power reference end	0.028W/Kg
Power reference change ²	-0.00%

¹ DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.


² The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

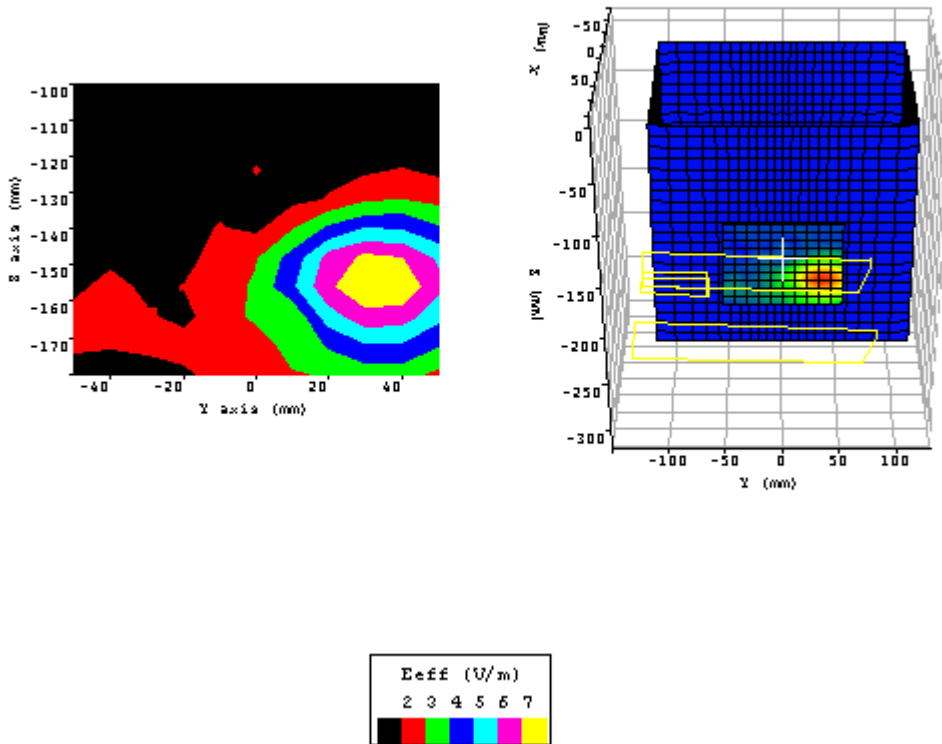

Plot 3.	
Date:	04/08/2003
Temperature Air / Liquid:	22.0°C / 22.0°C
Liquid mass density (ρ):	1
DCP ¹	20
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386
Probe S/N:0123 liquid/air conversion Factor	0.816
Simulated tissue dielectric parameters:	ϵ_r : 51.62 σ : 1.961
Transmit Antenna / Test Position	Left / bystander 5mm
Device Frequency	2437 MHz
Maximum 1 gram SAR:	0.143W/Kg
Maximum 10 gram SAR:	0.072W/Kg
Power reference start:	0.029W/Kg
Power reference end	0.029W/Kg
Power reference change ²	-0.00%

¹ DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.



² The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

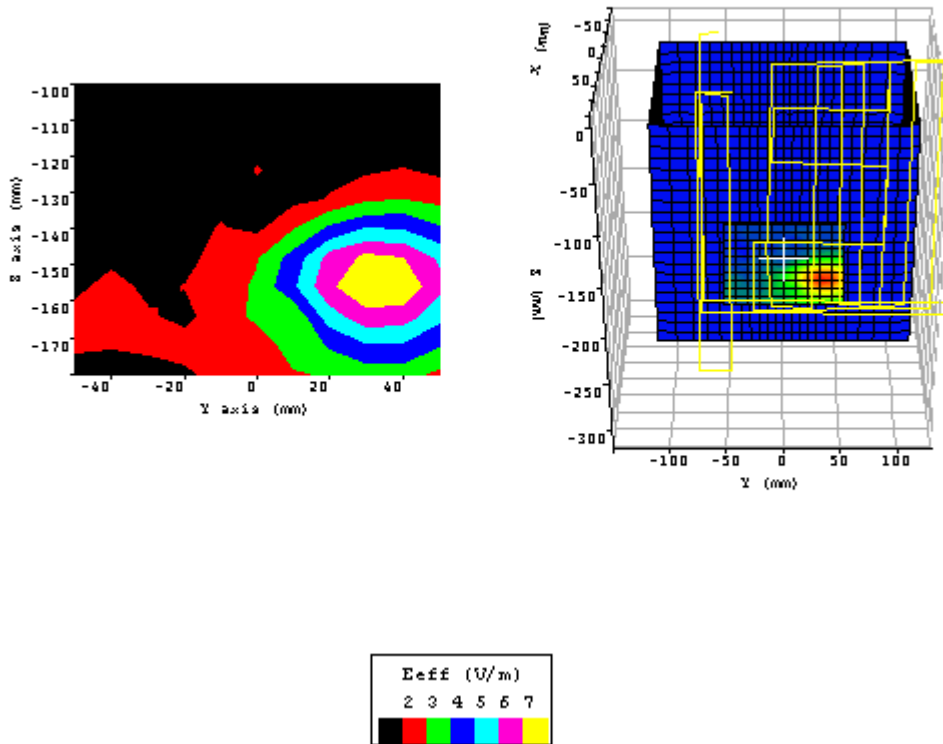

Plot 4.	
Date:	04/08/2003
Temperature Air / Liquid:	22.0°C / 22.0°C
Liquid mass density (ρ):	1
DCP ¹	20
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386
Probe S/N:0123 liquid/air conversion Factor	0.816
Simulated tissue dielectric parameters:	ϵ_r : 51.62 σ : 1.961
Transmit Antenna / Test Position	Left / lap
Device Frequency	2437 MHz
Maximum 1 gram SAR:	0.054W/Kg
Maximum 10 gram SAR:	0.030W/Kg
Power reference start:	0.010W/Kg
Power reference end	0.010W/Kg
Power reference change ²	-0.00%

¹ DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.



² The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

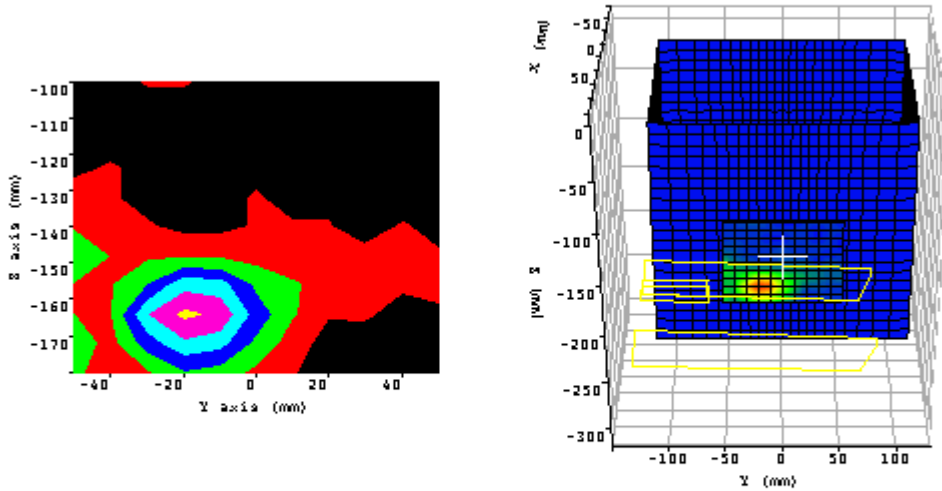

Plot 5.	
Date:	04/08/2003
Temperature Air / Liquid:	22.0°C / 21.0°C
Liquid mass density (ρ):	1
DCP ¹	20
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386
Probe S/N:0123 liquid/air conversion Factor	0.816
Simulated tissue dielectric parameters:	ϵ_r : 51.13 σ : 1.951
Transmit Antenna / Test Position	Right / bystander 5mm
Device Frequency	2412 MHz
Maximum 1 gram SAR:	0.135W/Kg
Maximum 10 gram SAR:	0.061W/Kg
Power reference start:	0.032W/Kg
Power reference end	0.032W/Kg
Power reference change ²	0.00%

¹ DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.

² The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.

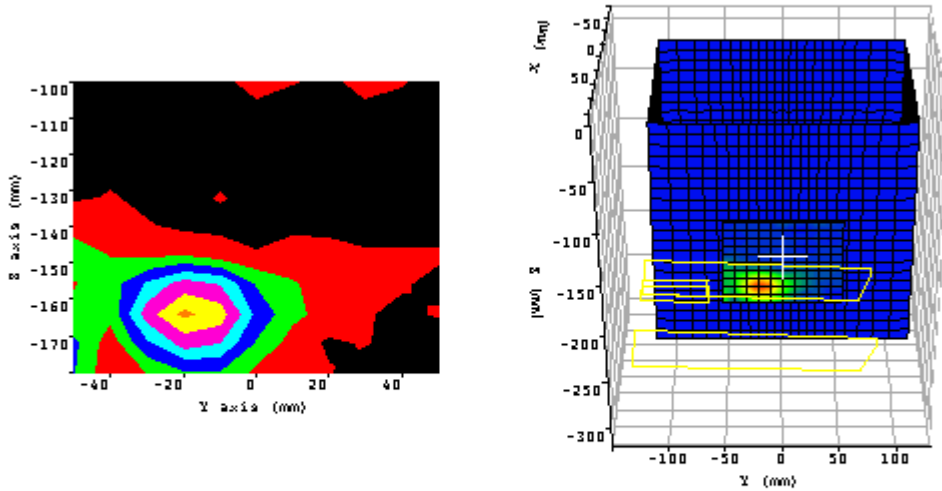

Plot 6.	
Date:	04/08/2003
Temperature Air / Liquid:	22.0°C / 21.0°C
Liquid mass density (ρ):	1
DCP ¹	20
Probe S/N:0123 Air Factor	X=346, Y=318, Z=386
Probe S/N:0123 liquid/air conversion Factor	0.816
Simulated tissue dielectric parameters:	ϵ_r : 51.15 σ : 1.961
Transmit Antenna / Test Position	Right / bystander 5mm
Device Frequency	2462 MHz
Maximum 1 gram SAR:	0.180W/Kg
Maximum 10 gram SAR:	0.078W/Kg
Power reference start:	0.036W/Kg
Power reference end	0.036W/Kg
Power reference change ²	0.00%

¹ DCP: Diode compression potential for different types of modulation is determined during the calibration of the probe. See section 6.2 of this report *Probe and Amplifier Specification*. Crest factor is not used.

² The power reference change is calculated by the test system with more digits than indicated in the power reference start and end values.