

Test Laboratory: UL CCS

System Performance Check - D2450V2

DUT: Dipole D2450V2 SN: 706; Type: D2450V2; Serial: 706

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.934$ mho/m; $\epsilon_r = 51.745$; $\rho = 1000$ kg/m³
Phantom section: Flat Section


Room Ambient Temperature: 24.0 deg. C; Liquid Temperature: 23.0 deg. C

DASY5 Configuration:

- Area Scan setting - Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Probe: EX3DV4 - SN3686; ConvF(6.86, 6.86, 6.86); Calibrated: 1/24/2011
- Sensor-Surface: 2.5mm (Mechanical Surface Detection), Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1239; Calibrated: 11/17/2010
- Phantom: ELI 4.0; Type: QDOVA001BB; Serial: 1099
- Measurement SW: DASY52, Version 52.6 (1); SEMCAD X Version 14.4.2 (2595)

Configuration/d=10mm, Pin=250mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm
Maximum value of SAR (measured) = 7.591 mW/g

Configuration/d=10mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 63.145 V/m; Power Drift = -0.03 dB
Peak SAR (extrapolated) = 11.063 W/kg
SAR(1 g) = 5.39 mW/g; SAR(10 g) = 2.48 mW/g
Maximum value of SAR (measured) = 6.204 mW/g

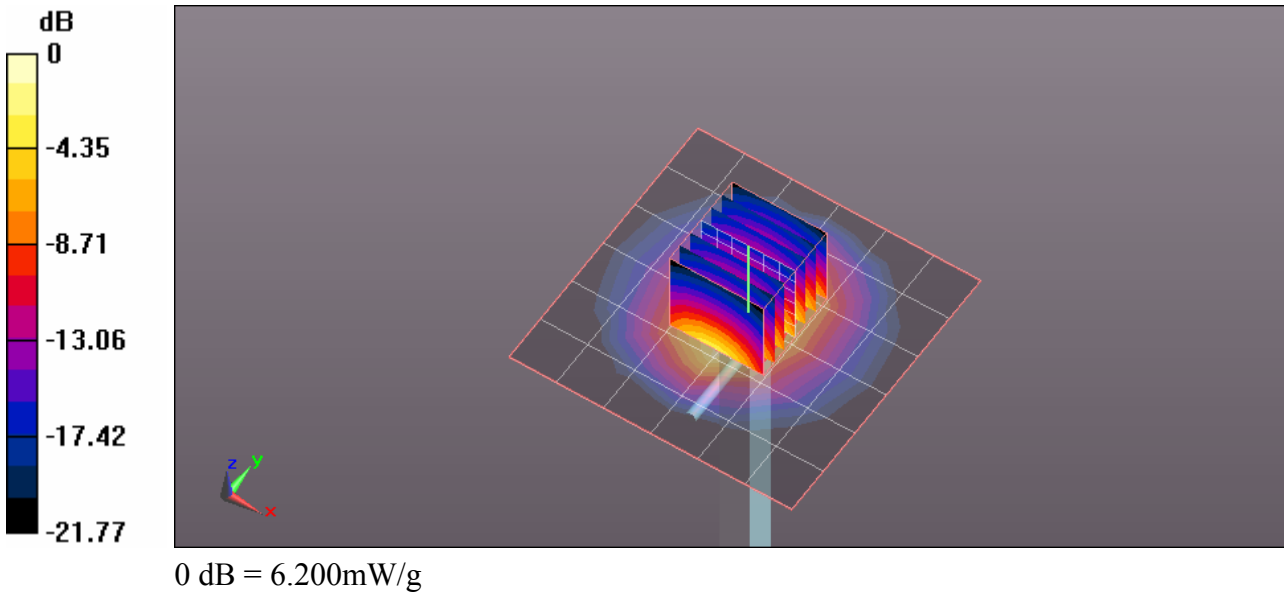

Test Laboratory: UL CCS

System Performance Check - D2450V2

DUT: Dipole D2450V2 SN: 706; Type: D2450V2; Serial: 706

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Configuration/d=10mm, Pin=250mW/Z Scan (1x1x34): Measurement grid: dx=20mm, dy=20mm, dz=3mm
Maximum value of SAR (measured) = 7.679 mW/g

