



SAR Test Report

Product Name	:	802.11bgn WLAN+BT Combo Card
Model No.	:	BCM94330UARTSDB
FCC ID	:	QDS-BRCM1065

Applicant :Broadcom CorporationAddress :190 Mathilda Place, Sunnyvale, CA 94086

Date of Receipt	:	28/06/2012
Date of Test	:	04/07/2012
Issued Date		17/07/2012
Report No.	:	126S080R-HP-US-P03V01
Report Version	:	V1.1

The test results relate only to the samples tested.

The test report shall not be reproduced except in full without the written approval of QuieTek Corporation.



Test Report Certification

Issued Date: 17/07/2012 Report No.: 126S080R-HP-US-P03V01



Product Name	:	802.11bgn WLAN+BT Combo Card
Applicant	:	Broadcom Corporation
Address	:	190 Mathilda Place, Sunnyvale, CA 94086
Manufacturer	:	Broadcom Corporation
Address	:	190 Mathilda Place Sunnyvale California United States
Model No.	:	BCM94330UARTSDB
Trade Name	:	lenovo
EUT Voltage	:	3.3V
Applicable Standard	:	FCC OET65 Supplement C June 2001
		IEEE Std. 1528-2003; 47CFR § 2.1093
Test Result	:	Max. SAR Measurement (1g)
		802.11b: 0.956W/kg
Performed Location	:	Suzhou EMC Laboratory
		No.99 Hongye Rd., Suzhou Industrial Park Loufeng Hi-Tech
		Development Zone., Suzhou, China
		TEL: +86-512-6251-5088 / FAX: +86-512-6251-5098
		FCC Registration Number: 800392
Documented By	:	Alice Ni
		(Engineering ADM: Alice Ni)
Tested By	:	Robin Wu.
		(Engineering Supervisor: Robin Wu)
Approved By	:	Marlinchen
		(Manager: Marlin Chen)

Laboratory Information

We, **QuieTek Corporation**, are an independent EMC and safety consultancy that was established the whole facility in our laboratories. The test facility has been accredited/accepted(audited or listed) by the following related bodies in compliance with ISO 17025, EN 45001 and specified testing scope:

Taiwan R.O.C.	: BSMI, NCC, TAF
Germany	: TUV Rheinland
Norway	: Nemko, DNV
USA	: FCC, NVLAP
Japan	: VCCI
China	: CNAS

The related certificate for our laboratories about the test site and management system can be downloaded from QuieTek Corporation's Web Site :<u>http://www.quietek.com/tw/ctg/cts/accreditations.htm</u> The address and introduction of QuieTek Corporation's laboratories can be founded in our Web site : <u>http://www.quietek.com/</u>

If you have any comments, Please don't hesitate to contact us. Our contact information is as below:

HsinChu Testing Laboratory :

No.75-2, 3rd Lin, Wangye Keng, Yonghxing Tsuen, Qionglin Shiang, Hsinchu County 307, Taiwan, R.O.C. TEL:+886-3-592-8858 / FAX:+886-3-592-8859 E-Mail : <u>service@quietek.com</u>

LinKou Testing Laboratory :

No.5-22, Ruishukeng, Linkou Dist., New Taipei City 24451, Taiwan, R.O.C. TEL : 886-2-8601-3788 / FAX : 886-2-8601-3789 E-Mail : <u>service@quietek.com</u>

Suzhou Testing Laboratory :

No.99 Hongye Rd., Suzhou Industrial Park Loufeng Hi-Tech Development Zone., SuZhou, China TEL : +86-512-6251-5088 / FAX : 86-512-6251-5098 E-Mail : <u>service@quietek.com</u>



TABLE OF CONTENTS

Des	scription	Page
1.	General Information	6
1	.1. EUT Description	6
1	.2. Test Environment	8
2.	SAR Measurement System	9
2	2.1. DASY5 System Description	9
	2.1.1. Applications	10
	2.1.2. Area Scans	
	2.1.3. Zoom Scan (Cube Scan Averaging)	10
	2.1.4. Uncertainty of Inter-/Extrapolation and Averaging	
2	2.2. DASY5 E-Field Probe	
	2.2.1. Isotropic E-Field Probe Specification	
	.3. Boundary Detection Unit and Probe Mounting Device	
	2.4. DATA Acquisition Electronics (DAE) and Measurement Server	
	1.5. Robot	
	2.6. Light Beam Unit	
	2.7. Device Holder	
2	2.8. SAM Twin Phantom	
3.	Tissue Simulating Liquid	15
3	1. The composition of the tissue simulating liquid	15
3	2.2. Tissue Calibration Result	15
3	3.3. Tissue Dielectric Parameters for Head and Body Phantoms	16
4.	SAR Measurement Procedure	17
4	.1. SAR System Validation	17
	4.1.1. Validation Dipoles	17
	4.1.2. Validation Result	17
4	.2. SAR Measurement Procedure	18
5.	SAR Exposure Limits	19
6.	Test Equipment List	20
7.	Measurement Uncertainty	21
8.	Conducted Power Measurement	
9.	Test Results	23

QuieTek

9.1.	SAR Test Results Summary	23
Append	lix A. SAR System Validation Data	25
Append	lix B. SAR measurement Data	26
Append	lix C. Test Setup Photographs & EUT Photographs	35
Append	lix D. Probe Calibration Data	36
Append	lix E. Dipole Calibration Data	47
Append	lix F. DAE Calibration Data	55

1. General Information

1.1. EUT Description

Product Name	802.11bgn WLAN+BT Combo Card	
Model No.	BCM94330UARTSDB	
FCC ID	QDS-BRCM1065	
Frequency Range	802.11b/g/n(20MHz): 2412 - 2462 MHz	
Channel Number	802.11b/g/n(20MHz): 11	
Type of Modulation	802.11b: DSSS	
	802.11b/n: OFDM	
Data Rate	802.11b: 1/2/5.5/11 Mbps	
	802.11g: 6/9/12/18/24/36/48/54 Mbps	
	802.11n: up to 65 Mbps	
Device Category	Mobile	
RF Exposure Environment	Uncontrolled	
Antenna Type	PIFA	
Peak Antenna Gain	Reference for list	
Max. Output Power	802.11b: 14.29dBm	
(Average)	802.11g: 9.49dBm	
	802.11n(20MHz): 9.4dBm	

Antenna List

Antenna	Manufacturer	M/N	Antenna Gain(dBi)
Main Antenna(Black)	Luxshared Corporation	L01RF018-R	4.13 for 2.4GHz
Aux Antenna(White)	Luxshared Corporation	L01RF019-R	1.79 for 2.4GHz
Main Antenna(Black)	Foxconn	WDAN-L1VN1001-DF	2.38 for 2.4GHz
Aux Antenna(White)	Foxconn	WDAN-L1VN1002-DF	1.89 for 2.4GHz

Note: "L01RF018-R" antenna was chosen to test.

Tested System Details

Product	Manufacturer	Model No.
Notebook Computer	lenovo	20187XXXX, 2696XXXX (X=0-9, A-Z or Blank)



Channel List

802.11b/g/	802.11b/g/n(20MHz) Working Frequency of Each Channel:						
Channel	Frequency	Channel	Frequency	Channel	Frequency	Channel	Frequency
01	2412 MHz	02	2417 MHz	03	2422 MHz	04	2427 MHz
05	2432 MHz	06	2437 MHz	07	2442 MHz	08	2447 MHz
09	2452 MHz	10	2457 MHz	11	2462 MHz	N/A	N/A



1.2. Test Environment


Ambient conditions in the laboratory:

ltems	Required	Actual
Temperature (°C)	18-25	21.5± 2
Humidity (%RH)	30-70	52



2. SAR Measurement System

2.1. DASY5 System Description

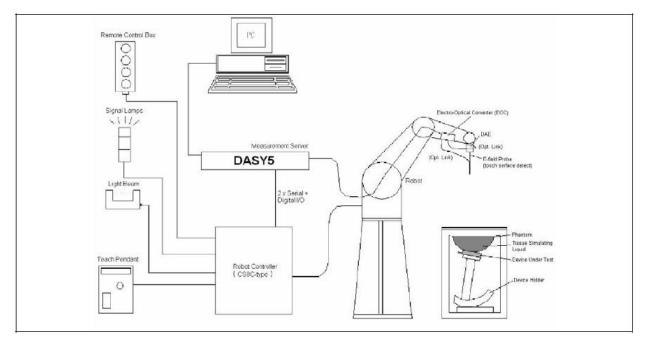

The DASY5 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot with controller, teach pendant and software.
 An arm extension for accommodating the data acquisition electronics (DAE).
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- The Electro-optical converter (EOC) performs the conversion from optical to electrical signals for the digital communication to the DAE. To use optical surface detection, a special version of the EOC is required. The EOC signal is transmitted to the measurement server.
- The Light Beam used is for probe alignment. This improves the (absolute) accuracy of the probe positioning.
- > A computer running WinXP and the DASY5 software.
- Remote control and teach pendant as well as additional circuitry for robot safety such as warning lamps, etc.
- The phantom, the device holder and other accessories according to the targeted measurement.

2.1.1. Applications

Predefined procedures and evaluations for automated compliance testing with all worldwide standards, e.g., IEEE 1528, OET 65, IEC 62209-1, IEC 62209-2, EN 50360, EN 50383 and others.

2.1.2. Area Scans

Area scans are defined prior to the measurement process being executed with a user defined variable spacing between each measurement point (integral) allowing low uncertainty measurements to be conducted. Scans defined for FCC applications utilize a 10mm² step integral, with 1mm interpolation used to locate the peak SAR area used for zoom scan assessments.

When an Area Scan has measured all reachable points, it computes the field maxima found in the scanned area, within a range of the global maximum. The range (in dB) is specified in the standards for compliance testing. For example, a 2 dB range is required in IEEE 1528-2003 and IEC 62209 standards, whereby 3 dB is a requirement when compliance is assessed in accordance with the ARIB standard (Japan).

2.1.3. Zoom Scan (Cube Scan Averaging)

Zoom Scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. A density of 1000 kg/m³ is used to represent the head and body tissue density and not the phantom liquid density, in order to be consistent with the definition of the liquid dielectric properties, i.e. the side length of the 1 g cube is 10mm, with the side length of the 10 g cube 21,5mm.

The zoom scan integer steps can be user defined so as to reduce uncertainty, but normal practice for typical test applications utilize a physical step of 7x7x7 (5mmx5mmx5mm) providing a volume of 30mm in the X & Y axis, and 30mm in the Z axis.

2.1.4. Uncertainty of Inter-/Extrapolation and Averaging

In order to evaluate the uncertainty of the interpolation, extrapolation and averaged SAR calculation algorithms of the Postprocessor, DASY5 allows the generation of measurement grids which are artificially predefined by analytically based test functions. Therefore, the grids of area scans and zoom scans can be filled with uncertainty test data, according to the SAR benchmark functions of IEEE 1528. The three analytical functions shown in equations as below are used to describe the possible range of the expected SAR distributions for the tested handsets. The field gradients are covered by the spatially flat distribution f1, the spatially steep distribution f3 and f2 accounts for H-field cancellation on the phantom/tissue surface.



$$f_1(x, y, z) = Ae^{-\frac{z}{2a}} \cos^2\left(\frac{\pi}{2}\frac{\sqrt{x'^2 + y'^2}}{5a}\right)$$
$$f_2(x, y, z) = Ae^{-\frac{z}{a}}\frac{a^2}{a^2 + x'^2} \left(3 - e^{-\frac{2z}{a}}\right)\cos^2\left(\frac{\pi}{2}\frac{y'}{3a}\right)$$
$$f_3(x, y, z) = A\frac{a^2}{\frac{a^2}{4} + x'^2 + y'^2} \left(e^{-\frac{2z}{a}} + \frac{a^2}{2(a+2z)^2}\right)$$

2.2. DASY5 E-Field Probe

The SAR measurement is conducted with the dosimetric probe manufactured by SPEAG. The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency.

SPEAG conducts the probe calibration in compliance with international and national standards (e.g. IEEE 1528, EN 62209-1, IEC 62209, etc.) under ISO 17025. The calibration data are in Appendix D.

Model	EX3DV4
Construction	Symmetrical design with triangular core Built-in shielding against staticharges PEEK enclosure material (resistant to organic solvents, e.g DGBE)
Frequency	10 MHz to 6 GHz Linearity: ± 0.2 dB (30 MHz to 6 GHz)
Directivity	± 0.3 dB in HSL (rotation around probe axis) ± 0.5 dB in tissue material (rotation normal to probe axis)
Dynamic Range	10 μW/g to 100 mW/g Linearity: ± 0.2 dB (noise: typically < 1 μW/g)
Dimensions	Overall length: 330 mm (Tip: 20 mm) Tip diameter: 2.5 mm (Body: 12 mm) Typical distance from probe tip to dipole centers: 1 mm
Application	High precision dosimetric measurements in any exposure scenari (e.g., very strong gradient fields). Only probe which enable compliance testing for frequencies up to 6 GHz with precision of bette 30%.

2.2.1. Isotropic E-Field Probe Specification

2.3. Boundary Detection Unit and Probe Mounting Device

The DASY probes use a precise connector and an additional holder for the probe, consisting of a plastic tube and a flexible silicon ring to center the probe. The connector at the DAE is flexibly mounted and held in the default position with magnets and springs. Two switching systems in the connector mount detect frontal and lateral probe collisions and trigger the necessary software response.

2.4. DATA Acquisition Electronics (DAE) and Measurement Server


The data acquisition electronics (DAE) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit.

Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.

The DASY5 measurement server is based on a PC/104 CPU board with a 400MHz intel ULV Celeron, 128MB chipdisk and 128MB RAM. The necessary circuits for communication with the DAE electronics box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY5 I/O board, which is directly connected to the PC/104 bus of the CPU board.









QuieTek

2.5. Robot

The DASY5 system uses the high precision robots TX90 XL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASY5 system, the CS8C robot controller version from Stäubli is used.

The XL robot series have many features that are important for our application:

- High precision (repeatability 0.02 mm)
- High reliability (industrial design)
- Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- 6-axis controller

2.6. Light Beam Unit

The light beam switch allows automatic "tooling" of the probe. During the process, the actual position of the probe tip with respect to the robot arm is measured, as well as the probe length and the horizontal probe offset. The software then corrects all movements, such that the robot coordinates are valid for the probe tip.

The repeatability of this process is better than 0.1 mm. If a position has been taught with an aligned probe, the same position will be reached with another aligned probe within 0.1 mm, even if the other probe has different dimensions. During probe rotations, the probe tip will keep its actual position.





QuieTek

2.7. Device Holder

The DASY5 device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation center for both scales is the ear reference point (EPR).

Thus the device needs no repositioning when changing the angles.

The DASY5 device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity $\varepsilon r = 3$ and loss tangent $\delta = 0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



2.8. SAM Twin Phantom

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- Left head
- Right head
- Flat phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

3. Tissue Simulating Liquid

3.1. The composition of the tissue simulating liquid

INGREDIENT	2450MHz
(% Weight)	Body
Water	73.2
Salt	0.04
Sugar	0.00
HEC	0.00
Preventol	0.00
DGBE	26.7
Triton X-100	0.00

3.2. Tissue Calibration Result

The dielectric parameters of the liquids were verified prior to the SAR evaluation using DASY5 Dielectric Probe Kit and Agilent Vector Network Analyzer E5071C

Body Tissue	e Simulant Measu	rement		
Frequency	Description	Dielectric Pa	arameters	Tissue Temp.
[MHz]	Description	ε _r	σ [s/m]	[°C]
	Reference result	52.7	1.95	N/A
2450MHz	± 5% window	50.07 to 55.34	1.85 to 2.05	IN/A
	04-07-2012	53.25	2.00	21.0
	·		·	



3.3. Tissue Dielectric Parameters for Head and Body Phantoms

The head tissue dielectric parameters recommended by the IEEE SCC-34/SC-2 in P1528 have been incorporated in the following table. These head parameters are derived from planar layer models simulating the highest expected SAR for the dielectric properties and tissue thickness variations in a human head. Other head and body tissue parameters that have not been specified in P1528 are derived from the tissue dielectric parameters computed from the 4-Cole-Cole equations described in Reference [12] and extrapolated according to the head parameters specified in P1528.

Target Frequency	He	ad	Bo	dy
(MHz)	٤r	σ (S/m)	٤r	σ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800 – 2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00


(ϵ_r = relative permittivity, σ = conductivity and ρ = 1000 kg/m³)



4. SAR Measurement Procedure

4.1. SAR System Validation

4.1.1. Validation Dipoles



The dipoles used is based on the IEEE-1528 standard, and is complied with mechanical and electrical specifications in line with the requirements of both IEEE and FCC Supplement C. the table below provides details for the mechanical and electrical specifications for the dipoles.

Frequency	L (mm)	h (mm)	d (mm)
2450MHz	53.5	30.4	3.6

4.1.2. Validation Result

System Perfo	rmance Check at 24	450MHz for Body		
Validation Dip	ole: D2450V2, SN:	839		
Frequency [MHz]	Description	SAR [w/kg] 1g	SAR [w/kg] 10g	Tissue Temp. [°C]
2450 MHz	Reference result ± 10% window	48.7 43.83 to 53.57	22.8 20.52 to 25.08	N/A
	04-07-2012	49.20	22.56	21.0
Note: All SAR	values are normalize	ed to 1W forward po	ower.	



Quielek

4.2. SAR Measurement Procedure

The DASY5 calculates SAR using the following equation,

$$SAR = \frac{\sigma |\mathbf{E}|^2}{\rho}$$

 σ : represents the simulated tissue conductivity ρ : represents the tissue density

The EUT is set to transmit at the required power in line with product specification, at each frequency relating to the LOW, MID, and HIGH channel settings.

Pre-scans are made on the device to establish the location for the transmitting antenna, using a large area scan in either air or tissue simulation fluid.

The EUT is placed against the Universal Phantom where the maximum area scan dimensions are larger than the physical size of the resonating antenna. When the scan size is not large enough to cover the peak SAR distribution, it is modified by either extending the area scan size in both the X and Y directions, or the device is shifted within the predefined area.

The area scan is then run to establish the peak SAR location (interpolated resolution set at 1mm²) which is then used to orient the center of the zoom scan. The zoom scan is then executed and the 1g and 10g averages are derived from the zoom scan volume (interpolated resolution set at 1mm³).

5. SAR Exposure Limits

SAR assessments have been made in line with the requirements of IEEE-1528, FCC Supplement C, and comply with ANSI/IEEE C95.1-1992 "Uncontrolled Environments" limits. These limits apply to a location which is deemed as "Uncontrolled Environment" which can be described as a situation where the general public may be exposed to an RF source with no prior knowledge or control over their exposure.

Type Exposure	Uncontrolled
	Environment Limit
Spatial Peak SAR (1g cube tissue for brain or body)	1.60 W/kg
Spatial Average SAR (whole body)	0.08 W/kg
Spatial Peak SAR (10g for hands, feet, ankles and wrist)	4.00 W/kg

Limits for General Population/Uncontrolled Exposure (W/kg)

6. Test Equipment List

Instrument	Manufacturer	Model No.	Serial No.	Cali. Due Date
Stäubli Robot TX60L	Stäubli	TX60L	F10/5C90A1/A/01	only once
Controller	Stäubli	SP1	S-0034	only once
Dipole Validation Kits	Speag	D2450V2	839	2013.02.23
SAM Twin Phantom	Speag	SAM	TP-1561/1562	N/A
Device Holder	Speag	SD 000 H01 HA	N/A	N/A
Data	Speag	DAE4	1220	2013.01.23
Acquisition Electronic				
E-Field Probe	Speag	EX3DV4	3710	2013.03.12
SAR Software	Speag	DASY5	V5.2 Build 162	N/A
Power Amplifier	Mini-Circuit	ZHL-42	D051404-28	N/A
Directional Coupler	Agilent	778D	20160	N/A
Vector Network	Agilent	E5071C	MY48367267	2013.04.10
Signal Generator	Agilent	E4438C	MY49070163	2013.04.18
Power Meter	Anritsu	ML2495A	0905006	2013.01.12
Wide Bandwidth Sensor	Anritsu	MA2411B	0846014	2013.01.12



7. Measurement Uncertainty

	DA	SY5 L	Jncer	tainty				
Measurement uncertainty for 30	00 MHz to 3	GHz avei	aged ov	er 1 gram	/ 10 grar	n.		
Error Description	Uncert.	Prob.	Div.	(Ci)	(Ci)	Std.	Std.	(Vi)
	value	Dist.		1g	10g	Unc.	Unc.	Veff
						(1g)	(10g)	
Measurement System		-			-	1		
Probe Calibration	±6.0%	Ν	1	1	1	±6.0%	±6.0%	∞
Axial Isotropy	±4.7%	R	√3	0.7	0.7	±1.9%	±1.9%	∞
Hemispherical Isotropy	±9.6%	R	√3	0.7	0.7	±3.9%	±3.9%	8
Boundary Effects	±1.0%	R	√3	1	1	±0.6%	±0.6%	8
Linearity	±4.7%	R	-√3	1	1	±2.7%	±2.7%	8
System Detection Limits	±1.0%	R	√3	1	1	±0.6%	±0.6%	8
Readout Electronics	±0.3%	Ν	1	1	1	±0.3%	±0.3%	∞
Response Time	±0.8%	R	√3	1	1	±0.5%	±0.5%	∞
Integration Time	±2.6%	R	√3	1	1	±1.5%	±1.5%	∞
RF Ambient Noise	±3.0%	R	-√3	1	1	±1.7%	±1.7%	∞
RF Ambient Reflections	±3.0%	R	-√3	1	1	±1.7%	±1.7%	∞
Probe Positioner	±0.4%	R	√3	1	1	±0.2%	±0.2%	∞
Probe Positioning	±2.9%	R	√3	1	1	±1.7%	±1.7%	∞
Max. SAR Eval.	±1.0%	R	√3	1	1	±0.6%	±0.6%	∞
Test Sample Related					•	-		•
Device Positioning	±2.9%	Ν	1	1	1	±2.9%	±2.9%	145
Device Holder	±3.6%	Ν	1	1	1	±3.6%	±3.6%	5
Power Drift	±5.0%	R	√3	1	1	±2.9%	±2.9%	∞
Phantom and Setup						·		
Phantom Uncertainty	±4.0%	R	√3	1	1	±2.3%	±2.3%	∞
Liquid Conductivity (target)	±5.0%	R	√3	0.64	0.43	±1.8%	±1.2%	∞
Liquid Conductivity (meas.)	±2.5%	Ν	1	0.64	0.43	±1.6%	±1.1%	∞
Liquid Permittivity (target)	±5.0%	R	-√3	0.6	0.49	±1.7%	±1.4%	∞
Liquid Permittivity (meas.)	±2.5%	N	1	0.6	0.49	±1.5%	±1.2%	∞
Combined Std. Uncertainty	1					±10.9%	±10.7%	387
Expanded STD Uncertainty						±21.9%	±21.4%	



8. Conducted Power Measurement

Test Mode	Data Rate	Channel No.	Frequency (MHz)	Average Power (dBm)
		01	2412	14.24
802.11b	1Mbps	06	2437	14.20
		11	2462	14.29
		01	2412	9.39
802.11g	6Mbps	06	2437	9.49
		11	2462	9.40
		01	2412	9.24
802.11n(20MHz)	6.5Mbps	06	2437	9.40
		11	2462	9.25

9. Test Results

9.1. SAR Test Results Summary

9.1.1. Test position and configuration

Body SAR was performed with the device configured in the positions according to FCC OET65. SAR test was performed with the device 0mm (touch) from the phantom for the worst case due to antenna position. Test Position: Bottom of Laptop, Bottom of Tablet, Primary Landscape of Tablet, Primary Portrait of Tablet. Please refer to the test photograph for details.

9.1.2. Co-located SAR

Bluetooth output power is less than Pref, and the distance between WiFi and BT is 116mm. Therefore, standalone SAR and simultaneous SAR for Bluetooth is not required.

9.1.3. Referenced Documents

FCC KDB 248227 D01 and KDB 447498 D01 and KDB 616217 D03

9.2. Test Results

SAR MEASUREM	IENT							
Ambient Temperatu	re (°C) : 21.	5 ±2		F	Relative	Humidity	(%): 55	
Liquid Temperature	(°C) : 21.0	±2		Γ	Depth o	f Liquid (c	:m):>15	
Product: 802.11bgn	WLAN+BT	Combo Ca	ard					
Test Mode: Laptop M	lode-802.11	b						
Test Position	Antenna	Frequ	ency		aration	Power	SAR 1g	Limit
Body	Position	Channel	MHz		tance nm)	Drift (<±0.2)	(W/kg)	(W/kg)
Bottom of PC	Fixed	1	2412		0	0.14	0.947	1.6
Bottom of PC	Fixed	6	2437		0	0.13	0.956	1.6
Bottom of PC	Fixed	11	2462		0	0.19	0.906	1.6
Test Mode: Laptop N	lode-802.11	g						
Bottom of PC	Fixed	6	2437		0	0.16	0.181	1.6
Test Mode: Laptop N	lode-802.11	n(20MHz)						
Bottom of PC	Fixed	6	2437		0	0.17	0.225	1.6
Test Mode: Tablet M	ode-802.11	b	_			_		
Bottom of Tablet	Fixed	6	2437		0	0.15	0.616	1.6
Primary Landscape	Fixed	6	2437		0	0.10	0.600	1.6
Primary Portrait	Fixed	6	2437		0	0.13	0.030	1.6

Appendix A. SAR System Validation Data

Date/Time: 04-07-2012

Test Laboratory: QuieTek Lab System Check Body 2450MHz **DUT: Dipole 2450 MHz D2450V2; Type: D2450V2** Communication System: CW; Communication System Band: D2450 (2450.0 MHz); Duty Cycle: 1:1; Frequency: 2450 MHz; Medium parameters used: f = 2450 MHz; σ = 2 mho/m; ϵ_r = 53.25; ρ = 1000 kg/m³; Phantom section: Flat Section Ambient temperature (): 21.5, Liquid temperature (): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(6.98, 6.98, 6.98); Calibrated: 12/03/2012;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 23/01/2012
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)

Configuration/System Check Body 2450MHz/Area Scan (7x11x1): Measurement grid: dx=10mm,


dy=10mm, Maximum value of SAR (measured) = 13.5 mW/g

Configuration/System Check Body 2450MHz/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm,

dy=5mm, dz=5mm, Reference Value = 81.585 V/m; Power Drift = 0.17 dB

Peak SAR (extrapolated) = 25.479 mW/g

SAR(1 g) = 12.3 mW/g; SAR(10 g) = 5.64 mW/g Maximum value of SAR (measured) = 14.1 mW/g

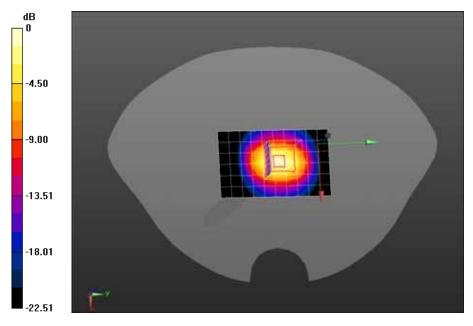

0 dB = 14.1 mW/g = 22.98 dB mW/g

Appendix B. SAR measurement Data

Date/Time: 04-07-2012

Test Laboratory: QuieTek Lab 802.11b 2412MHz-Bottom-Laptop Mode **DUT: 802.11bgn WLAN+BT Combo Card; Type: BCM94330UARTSDB** Communication System: Wi-Fi; Communication System Band: 802.11b; Duty Cycle: 1:1; Frequency: 2412 MHz; Medium parameters used: f = 2412 MHz; σ = 1.94 mho/m; ε_r = 53.49; ρ = 1000 kg/m³; Phantom section: Flat Section Ambient temperature (): 21.5, Liquid temperature (): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(6.98, 6.98, 6.98); Calibrated: 12/03/2012;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 23/01/2012
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)


Configuration/802.11b 2412MHz-Bottom/Area Scan (7x9x1): Measurement grid: dx=20mm, dy=20mm Maximum value of SAR (measured) = 1.05 mW/g

Configuration/802.11b 2412MHz-Bottom/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm,

dy=8mm, dz=5mm, Reference Value = 23.231 V/m; Power Drift = 0.14 dB

Peak SAR (extrapolated) = 2.392 mW/g

SAR(1 g) = 0.947 mW/g; SAR(10 g) = 0.391 mW/g Maximum value of SAR (measured) = 1.09 mW/g

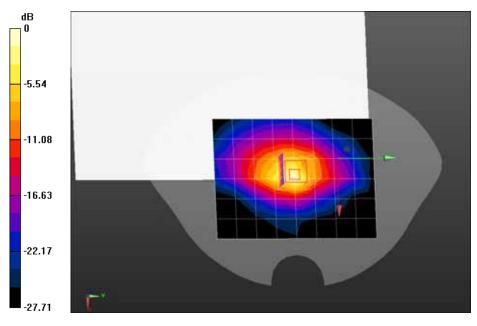

0 dB = 1.09 mW/g = 0.75 dB mW/g



Test Laboratory: QuieTek Lab 802.11b 2437MHz-Bottom-Laptop Mode

DUT: 802.11bgn WLAN+BT Combo Card; Type: BCM94330UARTSDB

Communication System: Wi-Fi; Communication System Band: 802.11b; Duty Cycle: 1:1; Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz; σ = 1.98 mho/m; ϵ_r = 53.3; ρ = 1000 kg/m³; Phantom section: Flat Section

Ambient temperature (): 21.5, Liquid temperature (): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(6.98, 6.98, 6.98); Calibrated: 12/03/2012;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 23/01/2012
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)


Configuration/802.11b 2437MHz-Bottom/Area Scan (7x9x1): Measurement grid: dx=20mm, dy=20mm Maximum value of SAR (measured) = 0.978 mW/g

Configuration/802.11b 2437MHz-Bottom/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm,

dy=8mm, dz=5mm, Reference Value = 22.210 V/m; Power Drift = 0.13 dB

Peak SAR (extrapolated) = 2.493 mW/g


SAR(1 g) = 0.956 mW/g; SAR(10 g) = 0.389 mW/g Maximum value of SAR (measured) = 1.14 mW/g

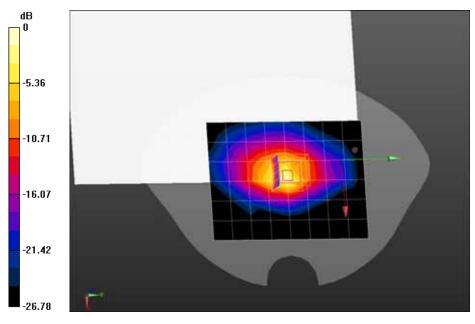

0 dB = 1.14 mW/g = 1.14 dB mW/g



Z-Axis Plot

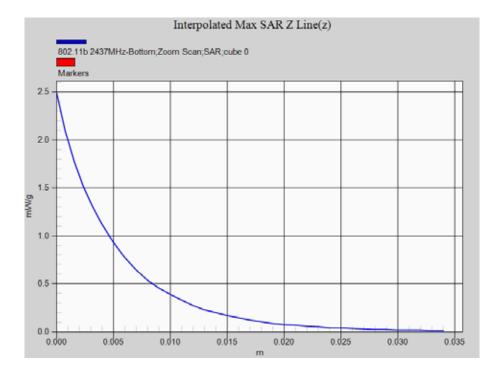



Test Laboratory: QuieTek Lab 802.11b 2462MHz-Bottom-Laptop Mode **DUT: 802.11bgn WLAN+BT Combo Card; Type: BCM94330UARTSDB** Communication System: Wi-Fi; Communication System Band: 802.11b; Duty Cycle: 1:1; Frequency: 2462 MHz; Medium parameters used: f = 2462 MHz; σ = 2.01 mho/m; ε_r = 53.21; ρ = 1000 kg/m³; Phantom section: Flat Section Ambient temperature (): 21.5, Liquid temperature (): 21.0 DASY5 Configuration:


- Probe: EX3DV4 SN3710; ConvF(6.98, 6.98, 6.98); Calibrated: 12/03/2012;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 23/01/2012
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)


Configuration/802.11b 2462MHz-Bottom/Area Scan (7x9x1): Measurement grid: dx=20mm, dy=20mm Maximum value of SAR (measured) = 1.07 mW/g

Configuration/802.11b 2462MHz-Bottom/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm,

dy=8mm, dz=5mm, Reference Value = 20.839 V/m; Power Drift = 0.19 dB

Peak SAR (extrapolated) = 2.453 mW/g



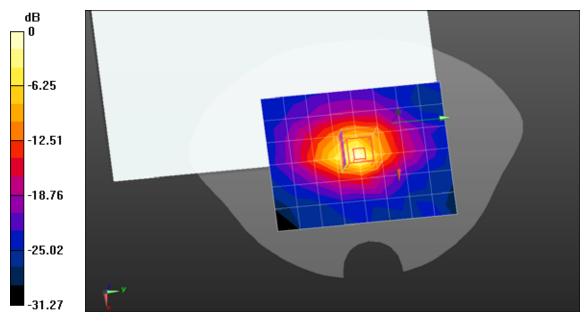

0 dB = 1.04 mW/g = 0.34 dB mW/g



Test Laboratory: QuieTek Lab 802.11g 2437MHz-Bottom-Laptop Mode

DUT: 802.11bgn WLAN+BT Combo Card; Type: BCM94330UARTSDB

Communication System: Wi-Fi; Communication System Band: 802.11g; Duty Cycle: 1:1; Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz; σ = 1.98 mho/m; ϵ_r = 53.3; ρ = 1000 kg/m³; Phantom section: Flat Section

Ambient temperature (): 21.5, Liquid temperature (): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(6.98, 6.98, 6.98); Calibrated: 12/03/2012;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 23/01/2012
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)


Configuration/802.11g 2437MHz-Bottom/Area Scan (7x9x1): Measurement grid: dx=20mm, dy=20mm Maximum value of SAR (measured) = 0.203 mW/g

Configuration/802.11g 2437MHz-Bottom/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm,

dy=8mm, dz=5mm, Reference Value = 10.061 V/m; Power Drift = 0.16 dB

Peak SAR (extrapolated) = 0.453 mW/g

SAR(1 g) = 0.181 mW/g; SAR(10 g) = 0.076 mW/g Maximum value of SAR (measured) = 0.195 mW/g

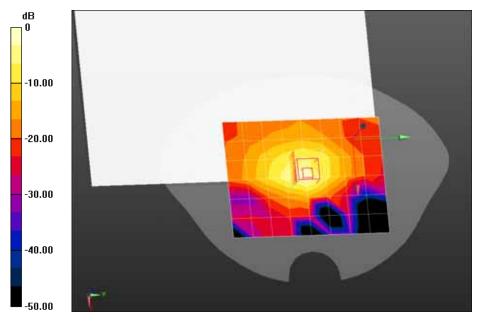

0 dB = 0.195 mW/g = -14.20 dB mW/g



Test Laboratory: QuieTek Lab

802.11n(20) 2437MHz-Bottom-Laptop Mode

DUT: 802.11bgn WLAN+BT Combo Card; Type: BCM94330UARTSDB

Communication System: Wi-Fi; Communication System Band: 802.11n(20MHz); Duty Cycle: 1:1; Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz; σ = 1.98 mho/m; ϵ_r = 53.3; ρ = 1000 kg/m³; Phantom section: Flat Section

Ambient temperature (): 21.5, Liquid temperature (): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(6.98, 6.98, 6.98); Calibrated: 12/03/2012;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 23/01/2012
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)

Configuration/802.11n(20) 2437MHz-Bottom/Area Scan (7x9x1): Measurement grid: dx=20mm,


dy=20mm, Maximum value of SAR (measured) = 0.158 mW/g

Configuration/802.11n(20) 2437MHz-Bottom/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm,

dy=8mm, dz=5mm, Reference Value = 8.878 V/m; Power Drift = 0.17 dB

Peak SAR (extrapolated) = 0.599 mW/g

SAR(1 g) = 0.225 mW/g; SAR(10 g) = 0.089 mW/g Maximum value of SAR (measured) = 0.268 mW/g

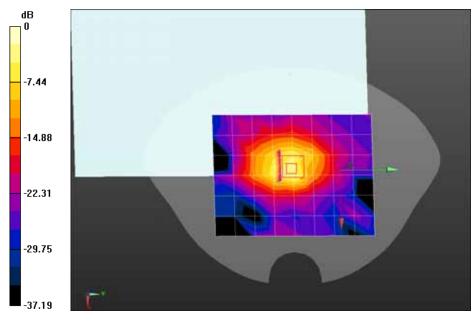

0 dB = 0.268 mW/g = -11.44 dB mW/g



Test Laboratory: QuieTek Lab 802.11b 2437MHz-Bottom-Tablet Mode

DUT: 802.11bgn WLAN+BT Combo Card; Type: BCM94330UARTSDB

Communication System: Wi-Fi; Communication System Band: 802.11b; Duty Cycle: 1:1; Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz; σ = 1.98 mho/m; ϵ_r = 53.3; ρ = 1000 kg/m³; Phantom section: Flat Section

Ambient temperature (): 21.5, Liquid temperature (): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(6.98, 6.98, 6.98); Calibrated: 12/03/2012;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 23/01/2012
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)


Configuration/802.11b 2437MHz-Bottom/Area Scan (7x9x1): Measurement grid: dx=20mm, dy=20mm Maximum value of SAR (measured) = 0.273 mW/g

Configuration/802.11b 2437MHz-Bottom/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm,

dy=8mm, dz=5mm, Reference Value = 10.722 V/m; Power Drift = 0.15 dB

Peak SAR (extrapolated) = 1.585 mW/g

SAR(1 g) = 0.616 mW/g; SAR(10 g) = 0.245 mW/g Maximum value of SAR (measured) = 0.750 mW/g

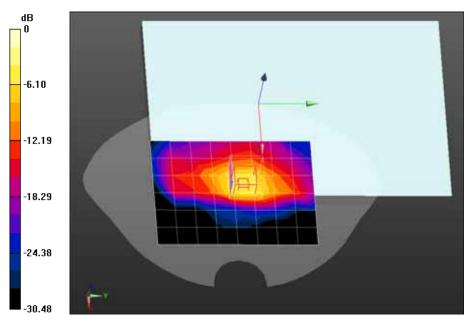

0 dB = 0.750 mW/g = -2.50 dB mW/g



Test Laboratory: QuieTek Lab

802.11b 2437MHz-Primary landscape-Tablet Mode

DUT: 802.11bgn WLAN+BT Combo Card; Type: BCM94330UARTSDB

Communication System: Wi-Fi; Communication System Band: 802.11b; Duty Cycle: 1:1; Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz; σ = 1.98 mho/m; ϵ_r = 53.3; ρ = 1000 kg/m³; Phantom section: Flat Section

Ambient temperature (): 21.5, Liquid temperature (): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(6.98, 6.98, 6.98); Calibrated: 12/03/2012;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 23/01/2012
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)


Configuration/802.11b 2437MHz-Primary landscape/Area Scan (7x9x1): Measurement grid: dx=20mm, dy=20mm, Maximum value of SAR (measured) = 0.303 mW/g

Configuration/802.11b 2437MHz-Primary landscape/Zoom Scan (5x5x7)/Cube 0: Measurement grid:

dx=8mm, dy=8mm, dz=5mm, Reference Value = 9.716 V/m; Power Drift = 0.10 dB

Peak SAR (extrapolated) = 1.529 mW/g

SAR(1 g) = 0.600 mW/g; SAR(10 g) = 0.229 mW/g Maximum value of SAR (measured) = 0.696 mW/g

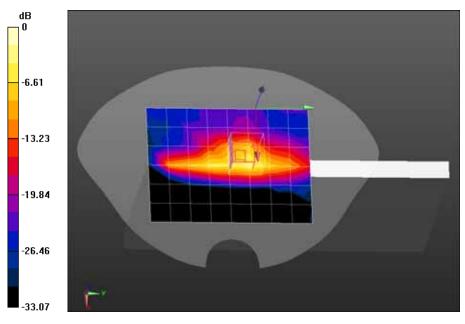

0 dB = 0.696 mW/g = -3.15 dB mW/g



Test Laboratory: QuieTek Lab

802.11b 2437MHz-Primary Portrait-Tablet Mode

DUT: 802.11bgn WLAN+BT Combo Card; Type: BCM94330UARTSDB

Communication System: Wi-Fi; Communication System Band: 802.11b; Duty Cycle: 1:1; Frequency: 2437 MHz; Medium parameters used: f = 2437 MHz; σ = 1.98 mho/m; ϵ_r = 53.3; ρ = 1000 kg/m³; Phantom section: Flat Section

Ambient temperature (): 21.5, Liquid temperature (): 21.0 DASY5 Configuration:

- Probe: EX3DV4 SN3710; ConvF(6.98, 6.98, 6.98); Calibrated: 12/03/2012;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1220; Calibrated: 23/01/2012
- Phantom: SAM1; Type: SAM; Serial: TP1561
- Measurement SW: DASY52, Version 52.8 (1); SEMCAD X Version 14.6.5 (6469)


Configuration/802.11b 2437MHz-Primary portrait/Area Scan (7x9x1): Measurement grid: dx=20mm, dy=20mm, Maximum value of SAR (measured) = 0.0302 mW/g

Configuration/802.11b 2437MHz-Primary portrait/Zoom Scan (5x5x7)/Cube 0: Measurement grid:

dx=8mm, dy=8mm, dz=5mm, Reference Value = 4.014 V/m; Power Drift = 0.13 dB

Peak SAR (extrapolated) = 0.061 mW/g


SAR(1 g) = 0.030 mW/g; SAR(10 g) = 0.013 mW/g Maximum value of SAR (measured) = 0.0358 mW/g

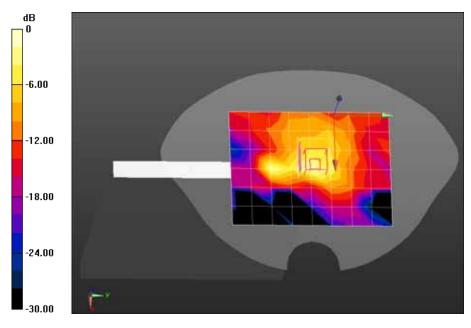

0 dB = 0.0358 mW/g = -28.92 dB mW/g

Appendix C. Test Setup Photographs & EUT Photographs

Antenna to User Separation Distances Bottom of the Tablet

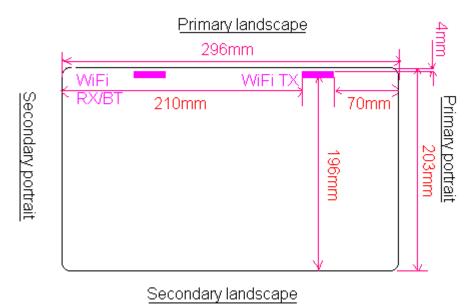

Antenna-to-user separation distances:	WiFi Antenna
	Tablet-Bottom face: 4mm from WiFi Antenna-to-user
	Tablet-Edges with the following configurations
	Primary landscape: 4mm from WiFi Antenna-to-user
	Secondary landscape: 196mm from WiFi Antenna-to-user
	Primary portrait: 70mm from WiFi Antenna-to-user
	Secondary portrait: 210mm from WiFi Antenna-to-user

Appendix D. Probe Calibration Data

	ch, Switzerland	and the second second	Swiss Calibration Service
ccredited by the Swiss Accredit he Swiss Accreditation Servic ultilateral Agreement for the r	e is one of the signatories	to the EA	lo.: SCS 108
lient Quietek-CN (A	uden)	Certificate No:	EX3-3710_Mar12
CALIBRATION	CERTIFICATE		
Dbject	EX3DV4 - SN:37	10	
Calibration procedure(s)	QA CAL-25.v4	A CAL-12.v7, QA CAL-14.v3, QA dure for dosimetric E-field probes	CAL-23.v4,
Calibration date:	March 12, 2012		
All calibrations have been condu	ucted in the closed laborator	obability are given on the following pages and a y facility: environment temperature (22 ± 3) °C a	
All calibrations have been condu	ucted in the closed laborator		
All calibrations have been condu Calibration Equipment used (M&	ucted in the closed laborator		
Il calibrations have been condu Calibration Equipment used (M& Primary Standards Power mater E4419B	Incled in the closed laborator INTE critical for calibration)	y facility: environment temperature (22 ± 3)"C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372)	and humidity < 70%. Scheduled Calibration Apr-12
All calibrations have been conducted in the conducted of	ucted in the closed laborator	y facility: environment temperature (22 ± 3)"C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372)	Apr-12 Apr-12
All calibrations have been conducted Calibration Equipment used (M& Primary Standards Power mater E4419B Power sensor E4412A Reference 3 dB Attenuator	ID GB41293874 MY41498087 SN: S5054 (3c)	y facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369)	Apr-12 Apr-12 Apr-12
All calibrations have been conducted Calibration Equipment used (M& Primary Standards Power mater E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator	ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5086 (20b)	y facility: environment temperature (22 ± 3)*C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12
All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator	ID GB41293874 MY41499087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b)	y facility: environment temperature (22 ± 3)*C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01370)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12
All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power sensor E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013	y facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01370) 29-Dec-11 (No. ES3-3013_Dec11)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-12
All calibrations have been conductive Calibration Equipment used (M& Primary Standards Power sensor E4419B Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2	ID GB41293874 MY41499087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b)	y facility: environment temperature (22 ± 3)*C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01370)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12
All calibrations have been conduct Calibration Equipment used (M& Primary Standards Power mater E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	LTE critical for calibration) ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 854	y facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Dec-11 (No. ES3-3013_Dec11) 3-May-11 (No. DAE4-654_May11)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-12 May-12
All calibrations have been conduct Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 3 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards	ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013	y facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367) 29-Dec-11 (No. ES3-3013_Dec11) 3-May-11 (No. DAE4-654_May11) Check Date (in house)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-12
All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 30 dB Attenuator Reference Probe ES3DV2 DAE4	ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 654	y facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Dec-11 (No. ES3-3013_Dec11) 3-May-11 (No. DAE4-654_May11)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-12 May-12 Scheduled Check
All calibrations have been conduct Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID US3642U01700	y facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. ES3-3013_Dec11) 3-May-11 (No. DAE4-654_May11) Check Date (in house) 4-Aug-99 (in house check Apr-11)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-12 May-12 Scheduled Check In house check: Apr-13 In house check: Oct-12
All calibrations have been conduct Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 20 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C	ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5054 (3c) SN: S5086 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID US3642U01700 US37390585	y facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367) 29-Dec-11 (No. ES3-3013_Dec11) 3-May-11 (No. DAE4-654_May11) Check Date (in house) 4-Aug-99 (in house check Apr-11) 18-Oct-01 (in house check Oct-11)	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-12 May-12 Scheduled Check In house check: Apr-13
All calibrations have been condu Calibration Equipment used (M8 Primary Standards Power meter E44198 Power sensor E4412A Reference 3 dB Attenuator Reference 30 dB Attenuator Reference 20 dB Attenuator Reference Probe ES3DV2 DAE4 Secondary Standards RF generator HP 8648C Network Analyzer HP 8753E	ATE critical for calibration) ID GB41293874 MY41498087 SN: S5054 (3c) SN: S5056 (20b) SN: S5129 (30b) SN: 3013 SN: 654 ID US3642U01700 US37390585 Name	y facility: environment temperature (22 ± 3)°C a Cal Date (Certificate No.) 31-Mar-11 (No. 217-01372) 31-Mar-11 (No. 217-01372) 29-Mar-11 (No. 217-01369) 29-Mar-11 (No. 217-01367) 29-Mar-11 (No. 217-01367) 29-Dec-11 (No. ES3-3013_Dec11) 3-May-11 (No. DAE4-654_May11) Check Date (in house) 4-Aug-99 (in house check Apr-11) 18-Oct-01 (in house check Oct-11) Function	Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Apr-12 Dec-12 May-12 Scheduled Check In house check: Apr-13 In house check: Oct-12

Certificate No: EX3-3710_Mar12

Page 1 of 11



Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage

C Service suisse d'étalonnage Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
NORMx,y,z	sensitivity in free space
ConvF	sensitivity in TSL / NORMx,y,z
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization 9	9 rotation around an axis that is in the plane normal to probe axis (at measurement center),
	i.e., 9 = 0 is normal to probe axis

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below *ConvF*).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax.y.z; Bx,y.z; Cx,y.z, VRx,y.z: A, B, C are numerical linearization parameters assessed based on the data of
 power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the
 maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom
 exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

Certificate No: EX3-3710_Mar12

Page 2 of 11



March 12, 2012

Probe EX3DV4

SN:3710

Manufactured: Repaired: Calibrated:

July 21, 2009 February 21, 2012 March 12, 2012

Calibrated for DASY/EASY Systems (Note: non-compatible with DASY2 system!)

Certificate No: EX3-3710_Mar12

Page 3 of 11



March 12, 2012

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3710

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^A$	0.51	0.56	0.44	± 10.1 %
DCP (mV) ^B	101.3	98.9	100.9	

Modulation Calibration Parameters

UID	Communication System Name	PAR		A dB	B dB	C dB	VR mV	Unc ^E (k=2)
10000	CW	0.00	X	0.00	0.00	1.00	114.4	±2.2 %
			Y	0.00	0.00	1.00	94.4	
			Z	0.00	0.00	1.00	114.2	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

 ^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).
 ^B Numerical linearization parameter: uncertainty not required.
 ^E Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the distribution. field value.

Certificate No: EX3-3710_Mar12

Page 4 of 11



March 12, 2012

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3710

f (MHz) ^c	Relative Permittivity ^F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
450	43.5	0.87	9.61	9.61	9.61	0.12	1.00	± 13.4 %
750	41.9	0.89	9.51	9.51	9.51	0.24	1.16	± 12.0 %
835	41.5	0.90	9.18	9.18	9.18	0.22	1.15	± 12.0 %
900	41.5	0.97	8.97	8.97	8.97	0.19	1.35	± 12.0 %
1810	40.0	1.40	8.32	8.32	8.32	0.79	0.60	± 12.0 %
1900	40.0	1.40	8.16	8.16	8.16	0.72	0.66	± 12.0 %
2450	39.2	1.80	7.25	7.25	7.25	0.36	0.91	± 12.0 %
2600	39.0	1.96	6.96	6.96	6.96	0.39	0.95	± 12.0 %
3500	37.9	2.91	6.80	6.80	6.80	0.33	1.09	± 13.1 %
5200	36.0	4.66	5.21	5.21	5.21	0.35	1.80	± 13.1 %
5500	35.6	4.96	4.9.5	4.9.5	4.9.5	0.35	1.80	± 13.1 %
5800	35.3	5.27	4.56	4.56	4.56	0.45	1.80	± 13.1 %

Calibration Parameter Determined in Head Tissue Simulating Media

^C Frequency validity of ± 100 MI tz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. ^F At frequencies below 3 GHz, the validity of tissue parameters (c and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (c and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for the indicated frequency (c and σ) is restricted to ± 5%. the ConvF uncertainty for indicated target tissue parameters.

Certificate No: EX3-3710_Mar12

Page 5 of 11



March 12, 2012

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3710

alibration	Parameter De	etermined in	Body 11s	sue Simi	ulating Me	edia		
f (MHz) ^c	Relative Permittivity ^F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
450	56.7	0.94	10.69	10.69	10.69	0.06	1.00	± 13.4 %
750	55.5	0.96	9.33	9.33	9.33	0.43	0.86	± 12.0 %
835	55.2	0.97	9.13	9.13	9.13	0.63	0.70	± 12.0 %
900	55.0	1.05	9.04	9.04	9.04	0.39	0.88	± 12.0 %
1810	53.3	1.52	7.73	7.73	7.73	0.33	1.10	± 12.0 %
1900	53.3	1.52	7.43	7.43	7.43	0.42	0.90	± 12.0 %
2450	52.7	1.95	6.98	6.98	6.98	0.79	0.59	± 12.0 %
2600	52.5	2.16	6.68	6.68	6.68	0.79	0.52	± 12.0 %
3500	51.3	3.31	6.23	6.23	6.23	0.36	1.13	± 13.1 %
5200	49.0	5.30	4.20	4.20	4.20	0.50	1.90	± 13.1 %
5500	48.6	5.65	3.82	3.82	3.82	0.50	1.90	± 13.1 %
5800	48.2	6.00	3.89	3.89	3.89	0.60	1.90	± 13.1 %

Calibration Parameter Determined in Body Tissue Simulating Media

ⁿ Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.
^F At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.


Certificate No: EX3-3710_Mar12

Page 6 of 11



March 12, 2012

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

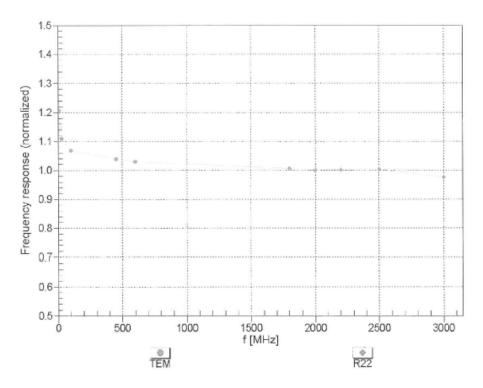


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: EX3-3710_Mar12

Page 7 of 11



March 12, 2012

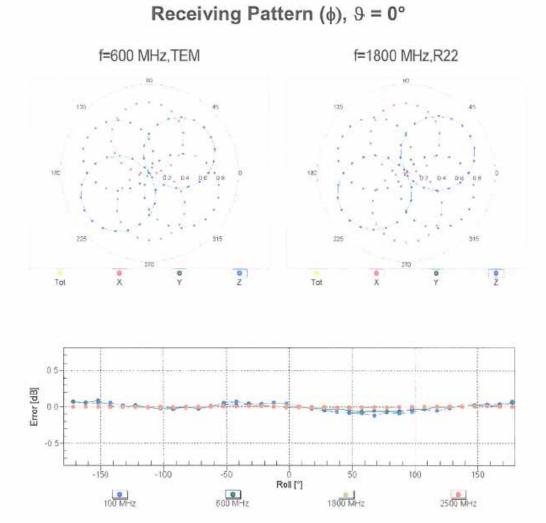


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

Certificate No: EX3-3710_Mar12

Page 8 of 11



March 12, 2012

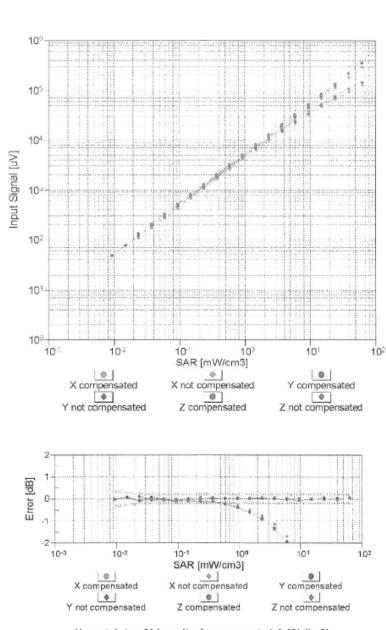


Dynamic Range f(SAR_{head}) (TEM cell , f = 900 MHz)

Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Certificate No: EX3-3710_Mar12

Page 9 of 11



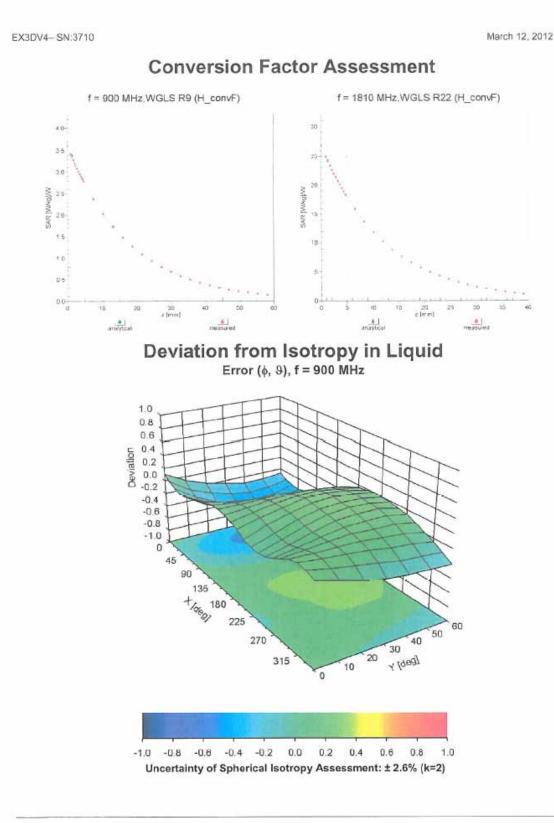

Certificate No: EX3-3710_Mar12

Page 10 of 11



March 12, 2012

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3710

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	Not applicable
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

Certificate No: EX3-3710_Mar12

Page 11 of 11

Appendix E. Dipole Calibration Data

Schmid & Partner Engineering AG eughausstrasse 43, 8004 Zuricl	y Of h, Switzerland	Hac MRA (c U z	 Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service
Accredited by the Swiss Accredita The Swiss Accreditation Service Aultilateral Agreement for the re	a is one of the signatories	s to the EA	ion No.: SCS 108
Client Quietek-CN (All			No: D2450V2-839_Feb12
	D2450V2 - SN: 8		
Object	D2450V2 - 5IN. 6	39	
Calibration procedure(s)	QA CAL-05.v8 Calibration proce	dure for dipole validation kits a	bove 700 MHz
Calibration date:	February 23, 201	2	
The measurements and the unce	rtainties with confidence p	onal standards, which realize the physica robability are given on the following pages ry facility: environment temperature (22 ±	and are part of the certificate.
The measurements and the unce All calibrations have been condu Calibration Equipment used (M&	ertainties with confidence p cted in the closed laborato TE critical for calibration)	robability are given on the following paget ry facility: environment temperature (22 ±	s and are part of the certificate. 3)°C and humidity < 70%.
The measurements and the unce All calibrations have been condu	ertainties with confidence p oted in the closed laborato	robability are given on the following page:	and are part of the certificate.
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards	ertainties with confidence p cted in the closed laborato TE critical for calibration)	robability are given on the following pages ry facility: environment temperature (22 ± Cal Date (Certificate No.)	and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A	ertainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704	robability are given on the following pages ry facility: environment temperature (22 ± Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451)	and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Oct-12
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type N mismatch combination	ertainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Mar-11 (No. 217-01368) 29-Mar-11 (No. 217-01371)	s and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Apr-12 Apr-12
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	ertainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g)	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Mar-11 (No. 217-01368)	s and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Apr-12
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type N mismatoh combination Reference Probe ES3DV3	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Mar-11 (No. 217-01368) 29-Mar-11 (No. 217-01371) 30-Dec-11 (No. ES3-3205_Dec11)	s and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Apr-12 Apr-12 Dec-12
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type N mismatch combination Reference Probe ES3DV3 DAE4	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205 SN: 601	robability are given on the following pages ry facility: environment temperature (22 ± <u>Cal Date (Certificate No.)</u> 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Mar-11 (No. 217-01368) 29-Mar-11 (No. 217-01371) 30-Dec-11 (No. ES3-3205_Dec11) 04-Jul-11 (No. DAE4-601_Jul11)	s and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Apr-12 Apr-12 Dec-12 Jul-12
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Mar-11 (No. 217-01368) 29-Mar-11 (No. 217-01371) 30-Dec-11 (No. ES3-3205_Dec11) 04-Jul-11 (No. DAE4-601_Jul11) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11)	s and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Apr-12 Apr-12 Dec-12 Jul-12 Scheduled Check
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type N miematch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A	ertainties with confidence p cted in the closed laborato TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205 SN: 601 ID # MY41092317	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Mar-11 (No. 217-01368) 29-Mar-11 (No. 217-01371) 30-Dec-11 (No. ES3-3205_Dec11) 04-Jul-11 (No. DAE4-601_Jul11) Check Date (in house) 18-Oct-02 (in house check Oct-11)	s and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Apr-12 Apr-12 Dec-12 Jul-12 Scheduled Check In house check: Oct-13
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5047.2 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005	Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Mar-11 (No. 217-01368) 29-Mar-11 (No. 217-01371) 30-Dec-11 (No. ES3-3205_Dec11) 04-Jul-11 (No. DAE4-601_Jul11) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11)	s and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Apr-12 Apr-12 Dec-12 Jul-12 Scheduled Check In house check: Oct-13 In house check: Oct-13
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06	ertainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5017.2 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005 US37390585 S4206	robability are given on the following pages ry facility: environment temperature (22 ± Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Mar-11 (No. 217-01368) 29-Mar-11 (No. 217-01371) 30-Dec-11 (No. ES3-3205_Dec11) 04-Jul-11 (No. DAE4-601_Jul11) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11) 18-Oct-01 (in house check Oct-11)	s and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Oct-12 Apr-12 Apr-12 Dec-12 Jul-12 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-12 Signature
The measurements and the unce All calibrations have been conduc Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type N miematch combination Reference Probe ES3DV3 DAE4 Secondary Standards Power sensor HP 8481A RF generator R&S SMT-06 Network Analyzer HP 8753E	artainties with confidence p cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 SN: 5086 (20g) SN: 5086 (20g) SN: 5017.2 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name	robability are given on the following pages ry facility: environment temperature (22 ± Cal Date (Certificate No.) 05-Oct-11 (No. 217-01451) 05-Oct-11 (No. 217-01451) 29-Mar-11 (No. 217-01368) 29-Mar-11 (No. 217-01368) 29-Mar-11 (No. 237-01371) 30-Dec-11 (No. ES3-3205_Dec11) 04-Jul-11 (No. DAE4-601_Jul11) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11) 18-Oct-01 (in house check Oct-11) 18-Oct-01 (in house check Oct-11)	s and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Oct-12 Oct-12 Oct-12 Apr-12 Apr-12 Dec-12 Jul-12 Scheduled Check In house check: Oct-13 In house check: Oct-13 In house check: Oct-12

Certificate No: D2450V2-839_Feb12

Page 1 of 8



Calibration Laboratory of Schmid & Partner







Schweizerischer Kalibrierdienst

S Service suisse d'étalonnage

- С Servizio svizzero di taratura
- S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- · Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

Certificate No: D2450V2-839_Feb12

Page 2 of 8

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.0
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.9 ± 6 %	1.86 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.2 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	51.9 mW /g ± 17.0 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR averaged over 10 cm ³ (10 g) of Head TSL SAR measured	condition 250 mW input power	6.09 mW / g

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.3 ± 6 %	2.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition		
SAR measured	250 mW input power	12.4 mW / g	
SAR for nominal Body TSL parameters	normalized to 1W	48.7 mW / g ± 17.0 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Body TSL	condition		
SAR averaged over 10 cm ³ (10 g) of Body TSL SAR measured	condition 250 mW input power	5.76 mW / g	

Certificate No: D2450V2-839_Feb12



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	55.7 Ω - 1.0 jΩ
Return Loss	- 25.2 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	52.1 Ω + 1.0 jΩ
Return Loss	- 32.9 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.160 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	July 20, 2009	

Certificate No: D2450V2-839_Feb12

Page 4 of 8

QuieTek

DASY5 Validation Report for Head TSL

Date: 23.02.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 839


Communication System: CW: Frequency: 2450 MHz Medium parameters used: f = 2450 MHz; $\sigma = 1.86$ mho/m; $\epsilon_r = 38.9$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANS1 C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.45, 4.45, 4.45); Calibrated: 30.12.2011
- · Sensor-Surface: 3mm (Mechanical Surface Detection)
- · Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- · Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.0(692); SEMCAD X 14.6.4(4989)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 98.155 V/m; Power Drift = 0.08 dB Peak SAR (extrapolated) = 27.8700 SAR(1 g) = 13.2 mW/g; SAR(10 g) = 6.09 mW/g Maximum value of SAR (measured) = 16.839 mW/g

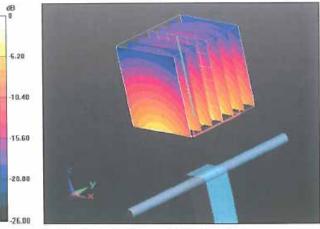


0 dB = 16.840 mW/g = 24.53 dB mW/g

Certificate No: D2450V2-839_Feb12

Page 5 of 8



Impedance Measurement Plot for Head TSL

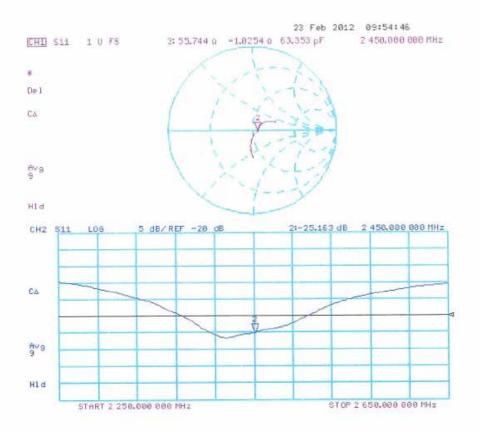

Certificate No: D2450V2-839_Feb12

Page 6 of 8

QuieTek

DASY5 Validation Report for Body TSL

Date: 23.02.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 839


Communication System: CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz; $\sigma = 2.02$ mho/m; $\varepsilon_r = 52.3$; $\rho = 1000$ kg/m³ Phantom section: Flat Section Measurement Standard; DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.26, 4.26, 4.26); Calibrated: 30.12.2011
- · Sensor-Surface: 3mm (Mechanical Surface Detection)
- · Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.0(692); SEMCAD X 14.6.4(4989)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 93.056 V/m; Power Drift = 0.0053 dB Peak SAR (extrapolated) = 25.2250 SAR(1 g) = 12.4 mW/g; SAR(10 g) = 5.76 mW/g Maximum value of SAR (measured) - 16.258 mW/g

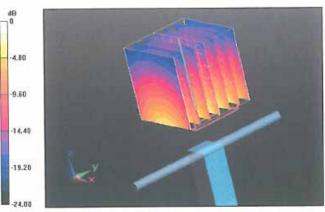

0 dB = 16.260mW/g = 24.22 dB mW/g


Certificate No: D2450V2-839_Feb12

Page 7 of 8



QuieTek

Impedance Measurement Plot for Body TSL

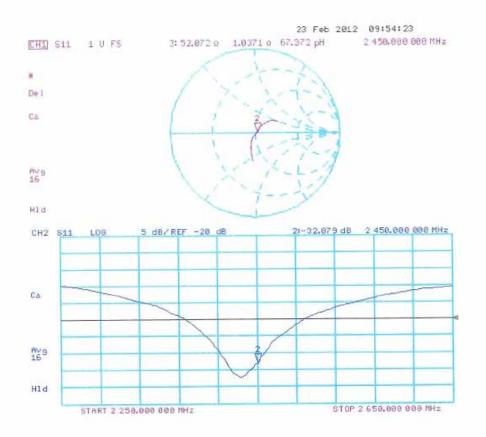

Certificate No: D2450V2-839_Feb12

Page 8 of 8



Appendix F. DAE Calibration Data

accredited by the Swiss Accredit he Swiss Accreditation Servic fultilateral Agreement for the r	e is one of the signatories	to the EA	tion No.: SCS 108
Client Quietek-CN (A	uden)	Certificate	e No: DAE4-1220_Jan12
CALIBRATION (CERTIFICATE		
Object	DAE4 - SD 000 D	04 BJ - SN: 1220	
Calibration procedure(s)	QA CAL-06.v24 Calibration proceed	dure for the data acquisition e	electronics (DAE)
Calibration date:	January 23, 2012		
The measurements and the uno All calibrations have been condu	ertainties with confidence pro	nal standards, which realize the physics obability are given on the following page / facility: environment temperature (22 ±	s and are part of the certificate.
The measurements and the unco All calibrations have been condu Calibration Equipment used (M& Primary Standards	ertainties with confidence pro- ucted in the closed laboratory NTE critical for calibration)	coability are given on the following page (facility: environment temperature (22 ± Cal Date (Certificate No.)	and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration
The measurements and the unco All calibrations have been condu Calibration Equipment used (M& Primary Standards	ertainties with confidence pro ucted in the closed laboratory NTE critical for calibration)	obability are given on the following page r facility: environment temperature (22 ±	s and are part of the certificate.
The measurements and the unc	ertainties with confidence pro ucted in the closed laboratory ITE critical for calibration) ID # SN: 0810278 ID #	coability are given on the following page (facility: environment temperature (22 ± Cal Date (Certificate No.)	and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration
The measurements and the unc All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards	ertainties with confidence pro ucted in the closed laboratory ITE critical for calibration) ID # SN: 0810278 ID #	chability are given on the following page (facility: environment temperature (22 ± Cal Date (Certificate No.) 28-Sep-11 (No:11450) Check Date (in house)	and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Sep-12 Scheduled Check
The measurements and the unc All calibrations have been condu Calibration Equipment used (M& Primary Standards Keithley Multimeter Type 2001 Secondary Standards	ertainties with confidence pro ucted in the closed laboratory ITE critical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001	coability are given on the following page (facility: environment temperature (22 ± <u>Cal Date (Certificate No.)</u> 28-Sep-11 (No:11450) <u>Check Date (in house)</u> 05-Jan-12 (in house check) Function Technician	a and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Sep-12 Scheduled Check In house check: Jan-13 Signature
The measurements and the unc All calibrations have been condu Calibration Equipment used (M8 Primary Standards Keithley Multimeter Type 2001 Secondary Standards Calibrator Box V2.1	ertainties with confidence pro ucted in the closed laboratory ITE critical for calibration) ID # SN: 0810278 ID # SE UWS 053 AA 1001	coability are given on the following page (facility: environment temperature (22 ± <u>Cal Date (Certificate No.)</u> 28-Sep-11 (No:11450) <u>Check Date (in house)</u> 05-Jan-12 (in house check) Function Technician	a and are part of the certificate. 3)°C and humidity < 70%. Scheduled Calibration Sep-12 Scheduled Check In house check: Jan-13



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst

- C Service suisse d'étalonnage
- Servizio svizzero di taratura Servizio Calibration Service
- Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service Is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE Connector angle data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a
 result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - *Power consumption:* Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-1220_Jan12

Page 2 of 5



DC Voltage Measurement

-			
A/D - Converter	Resolution	nominal	

High Range:	1LSB =	6.1µV,	full range =	-100+300 mV
Low Range:	1LSB =	61nV ,	full range =	-1+3mV
DASY measurement	parameters: Aut	to Zero Time: 3	sec; Measuring	time: 3 sec

Calibration Factors	x	Y	Z
High Range	405.267 ± 0.1% (k=2)	404.990 ± 0.1% (k=2)	404.221 ± 0.1% (k=2)
Low Range	3.97762 ± 0.7% (k=2)	3.99629 ± 0.7% (k=2)	3.98707 ± 0.7% (k=2)

Connector Angle

	T
Connector Angle to be used in DASY system	176.5 ° ± 1 °

Certificate No: DAE4-1220_Jan12

Page 3 of 5

QuieTek

Appendix

1. DC Voltage Linearity

High Range		Reading (µV)	Difference (µV)	Error (%)
Channel X	+ Input	199991.77	-2.52	-0.00
Channel X	+ Input	20001.19	1.01	0.01
Channel X	- Input	-19996.52	3.93	-0.02
Channel Y	+ Input	199992.70	-2.15	-0.00
Channel Y	+ Input	19999.00	-1.14	-0.01
Channel Y	- Input	-19999.75	0.71	-0.00
Channel Z	+ Input	199991.55	-3.11	-0.00
Channel Z	+ Input	19999.33	-0.76	-0.00
Channel Z	- Input	-20001.23	-0.67	0.00

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	1999.14	-1.60	-0.08
Channel X + Input	201.79	0.59	0.29
Channel X - Input	-198.19	0.48	-0.24
Channel Y + Input	1999.56	-0.99	-0.05
Channel Y + Input	200.20	-0.96	-0.48
Channel Y - Input	-199.38	-0.54	0.27
Channel Z + Input	2000.07	-0.52	-0.03
Channel Z + Input	200.32	-0.83	-0.41
Channel Z - Input	-199.60	-0.78	0.39

2. Common mode sensitivity DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (µV)
Channel X	200	10.22	8.65
	- 200	-6.99	-8.91
Channel Y	200	-10.43	-11.02
	- 200	7.95	9.22
Channel Z	200	14.25	13.66
	- 200	-15.77	-14.99

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (μV)
Channel X	200		-1.62	-2.79
Channel Y	200	8.07		-2.95
Channel Z	200	7.90	6.93	

Certificate No: DAE4-1220_Jan12

Page 4 of 5

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15896	16218
Channel Y	16012	15924
Channel Z	15702	15710

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input 10M Ω

	Average (µV)	min. Offset (µV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	0.67	-0.77	1.84	0.43
Channel Y	-1.44	-2.35	-0.02	0.39
Channel Z	-0.81	-1.60	0.01	0.37

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-1220_Jan12

Page 5 of 5