

APPENDIX

10. Photographs of Test Setup

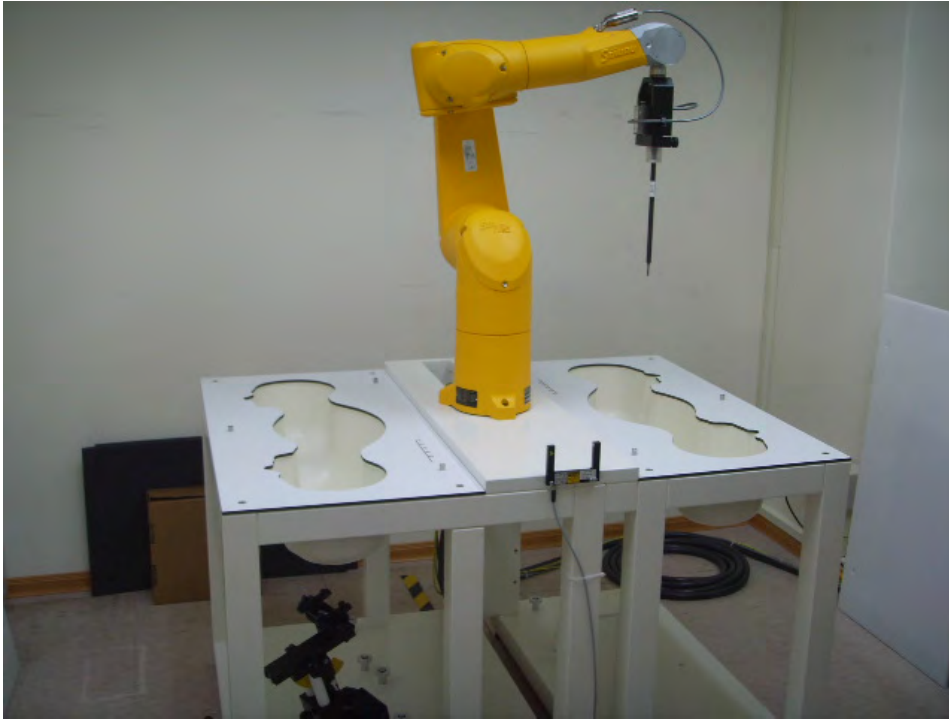


Fig.1 Photograph of the SAR measurement system

Photograph of the Tissue Simulant Fluid Liquid Depth (Body)

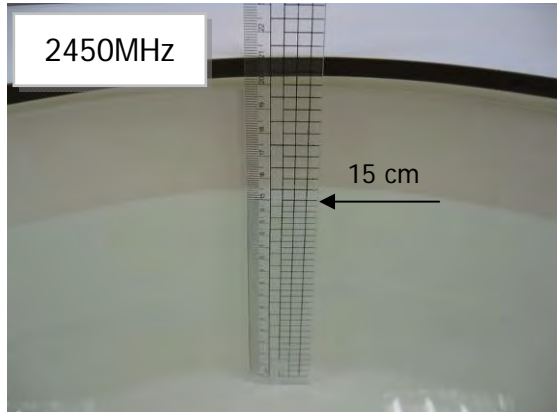


Fig.2.1

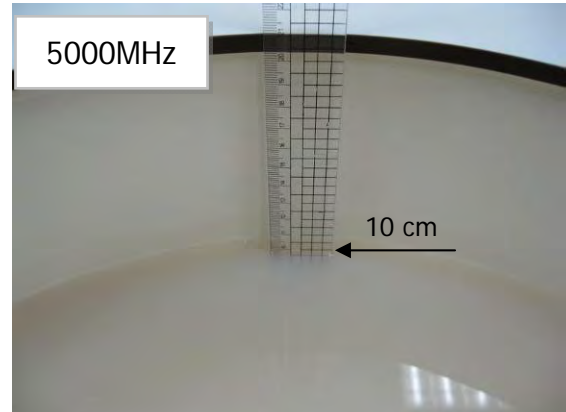


Fig.2.2

Body worn - distance between flat phantom and EUT is 0 mm

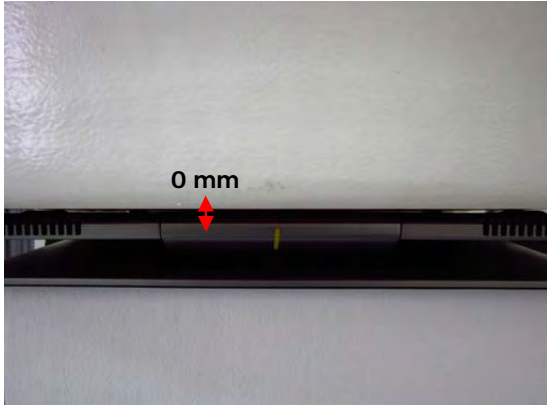


Fig.3 EUT Lap-held mode to flat phantom

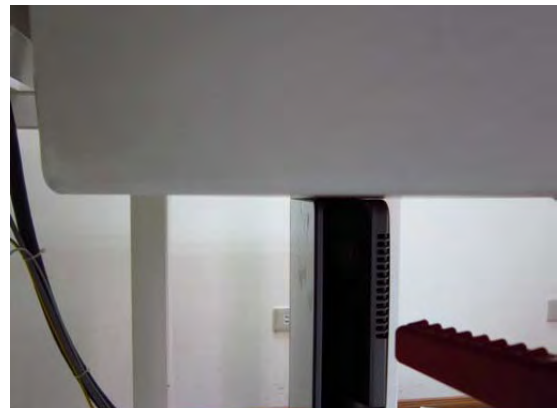
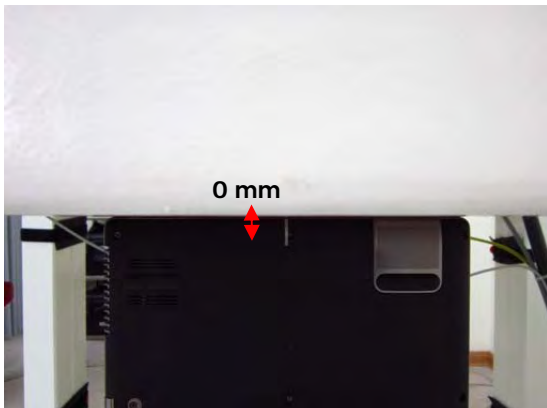


Fig.4 EUT Left to flat phantom

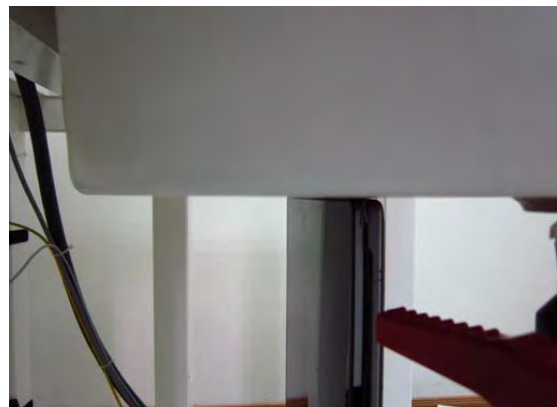
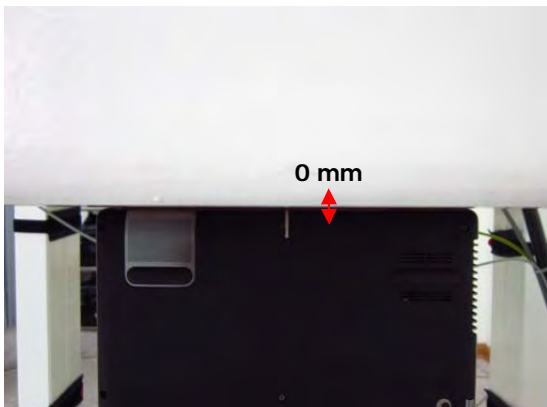


Fig.5 EUT Right to flat phantom