


Label Photo_1717WCE

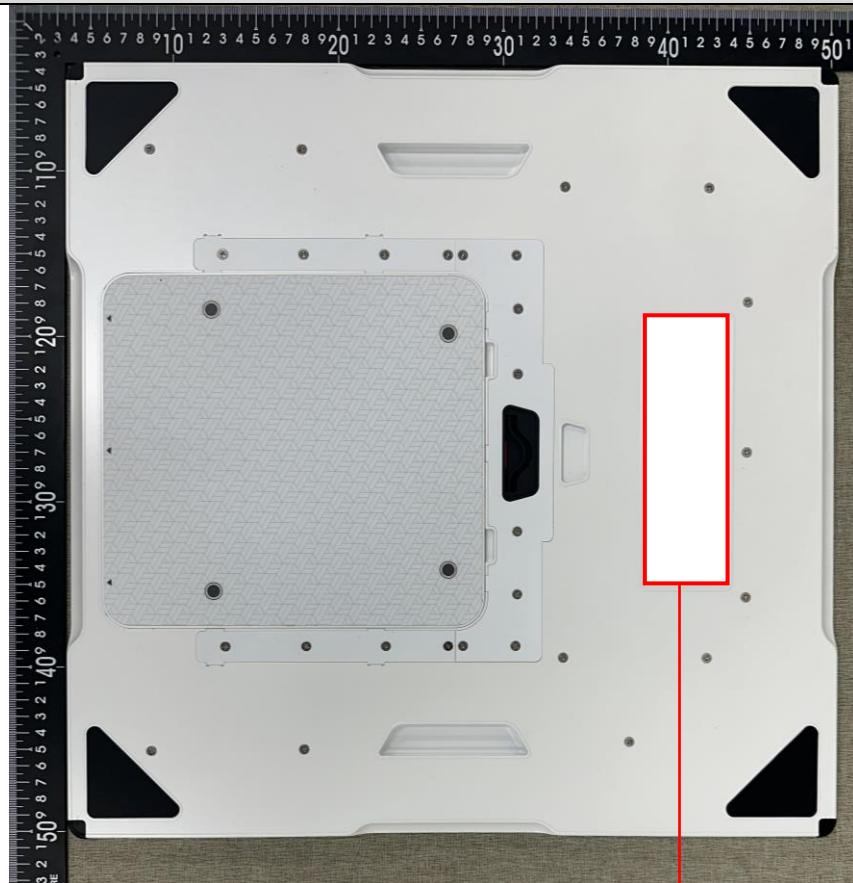

Rayence Co.,Ltd.

14, Samsung 1-ro 1-gil, Hwaseong-si, Gyeonggi-do, Korea / www.rayence.com

Model : 1717WCE (Medical Image Processing Unit)

Rating : 24V 1.7A

**CAUTION : Use Only with RB37BLA
(Li-Ion Battery) or RP003A
(Power supply)**

**Prudence : N'utilisez qu'avec
RB37BLA (batterie) ou RP003A
(Circuit d'alimentation)**



Date of Manufacture



Serial Number

Contains FCC ID : QIIRYRWM001A

This device complies with part 15 of the FCC Rules.

Operation is subject to the following two conditions:

1. This device may not cause harmful interference, and
2. This device must accept any interference received, including interference that may cause undesired operation.

Contains IC ID : 10742A-RWM001A

This Class A digital apparatus complies with Canadian ICES-0033.
5150-5250MHz is indoor use only.

rayence



R-R-RDF-1717WCE




E471661



Made in Korea

Rev.0

Label Photo_1717WCE-HS

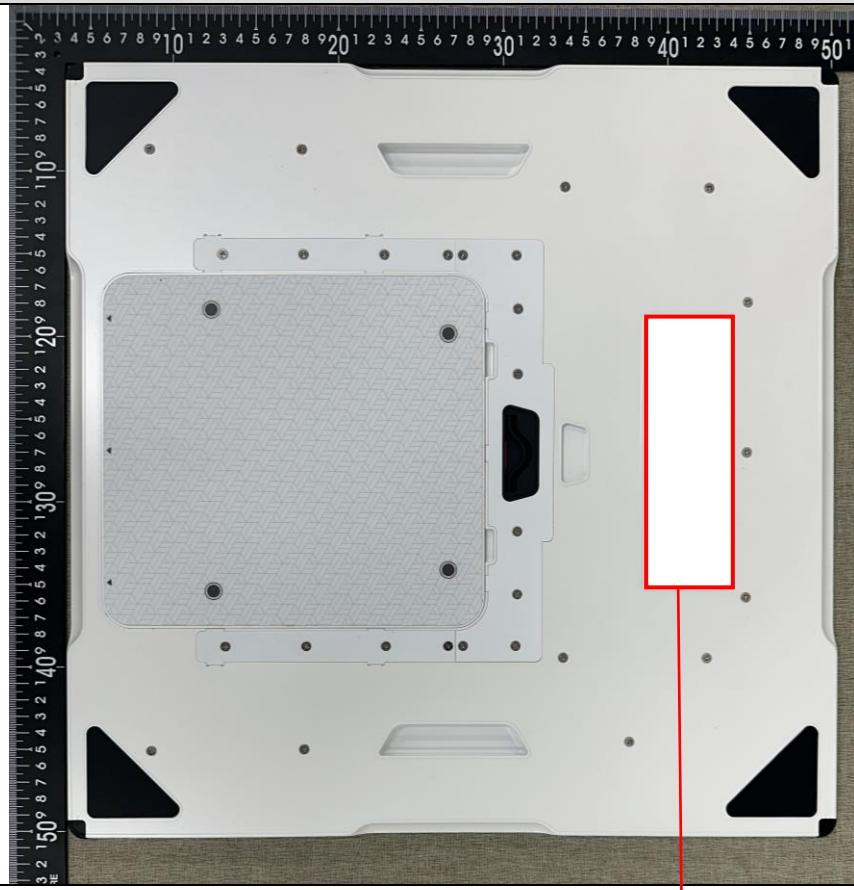

Rayence Co.,Ltd.
14, Samsung 1-ro 1-gil, Hwaseong-si, Gyeonggi-do, Korea / www.rayence.com

Model : 1717WCE-HS (Medical Image Processing Unit)

Rating : 24V 1.7A

CAUTION : Use Only with RB37BLA
(Li-ion Battery) or RP003A
(Power supply)

Prudence : N'utilisez qu'avec
RB37BLA (batterie) ou RP003A
(Circuit d'alimentation)



Date of Manufacture



Serial Number

Contains FCC ID : QIIRYRWM001A

This device complies with part 15 of the FCC Rules.

Operation is subject to the following two conditions:

1. This device may not cause harmful interference, and
2. This device must accept any interference received, including interference that may cause undesired operation.

Contains IC ID : 10742A-RWM001A

This Class A digital apparatus complies with Canadian ICES-0033.
5150-5250MHz is indoor use only.

rayence

 R-R-RDF-1717WCE




IP67  E471661



Made in Korea

Rev.0

Label Photo_1717WCE-HR

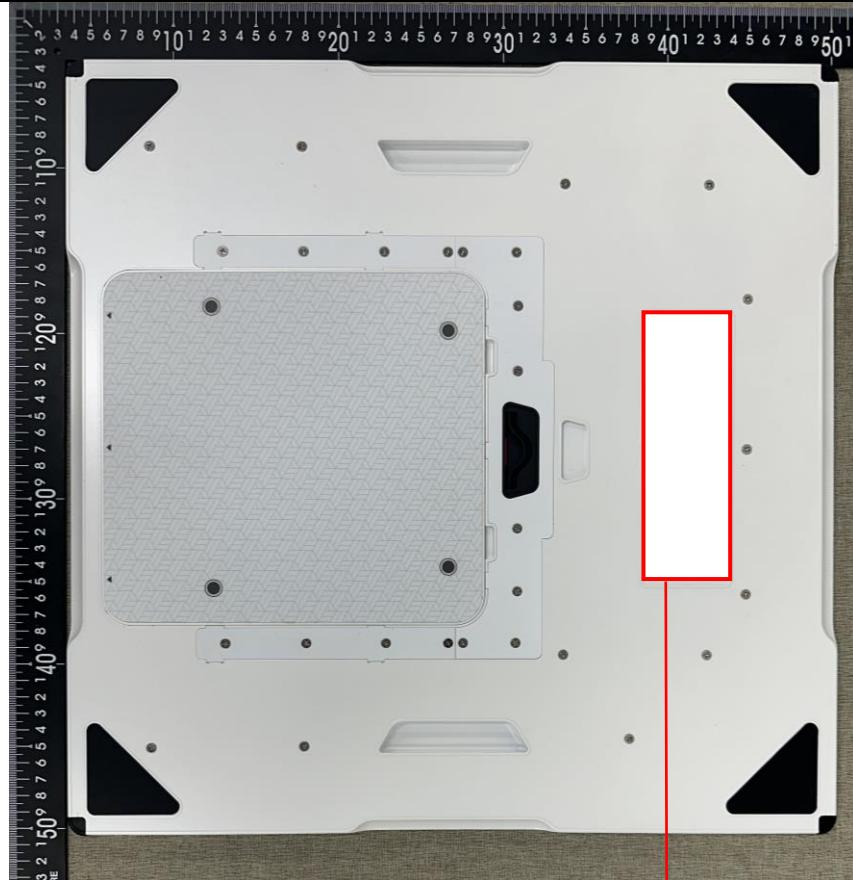

Rayence Co.,Ltd.
14, Samsung 1-ro 1-gil, Hwaseong-si, Gyeonggi-do, Korea / www.rayence.com

Model : 1717WCE-HR(Medical Image Processing Unit)

Rating : 24V 1.7A

CAUTION : Use Only with RB37BLA
(Li-ion Battery) or RP003A
(Power supply)

Prudence : N'utilisez qu'avec
RB37BLA (batterie) ou RP003A
(Circuit d'alimentation)



Date of Manufacture



Serial Number

Contains FCC ID : QIIRYRWM001A

This device complies with part 15 of the FCC Rules.

Operation is subject to the following two conditions:

1. This device may not cause harmful interference;
2. This device must accept any interference received,

including interference that may cause undesired operation.

Contains IC ID : 10742A-RWM001A

This Class A digital apparatus complies with Canadian ICES-003.

S150-S250MHz is indoor use only.

rayence

IC R-R-RDF-1717WCE


IP67 



Made in Korea

Rev.0

Label Photo_1717WCE-GF

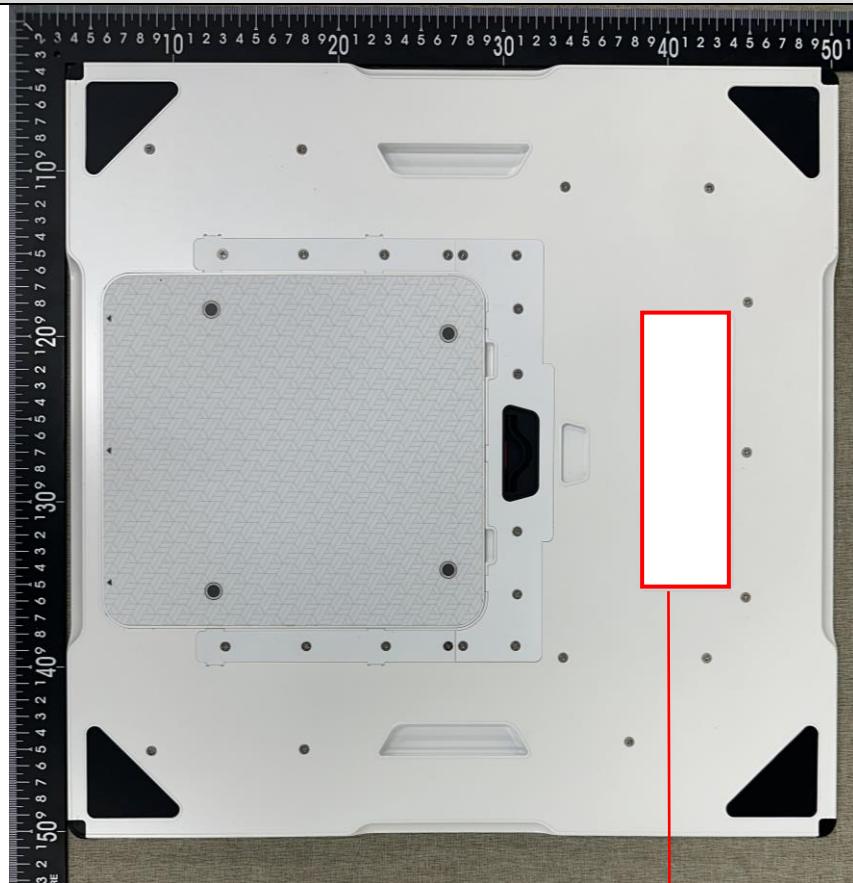

Rayence Co.,Ltd.
14, Samsung 1-ro 1-gil, Hwaseong-si, Gyeonggi-do, Korea / www.rayence.com

Model : 1717WCE-GF(Medical Image Processing Unit)

Rating : 24V == 1.7A

**CAUTION : Use Only with RB37BLA
(Li-ion Battery) or RP003A
(Power supply)**

**Prudence : N'utilisez qu'avec
RB37BLA (batterie) ou RP003A
(Circuit d'alimentation)**



Date of Manufacture



Serial Number

Contains FCC ID : QIIRYRWM001A

This device complies with part 15 of the FCC Rules.

Operation is subject to the following two conditions:

1. This device may not cause harmful interference, and
2. This device must accept any interference received, including interference that may cause undesired operation.

Contains IC ID : 10742A-RWM001A

This Class A digital apparatus complies with Canadian ICES-003.

5150-5250MHz is indoor use only.

rayence

 R-R-RDF-1717WCE 

IP67   E471661



Made in Korea

Rev.0