


Client	Rehabtronics Inc.	
Product	Hand Stimulator with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	

EUT INTERNAL PHOTOS – HSST1



Hand Stimulator – Photo 1

Client	Rehabtronics Inc.	
Product	Hand Stimulator with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	

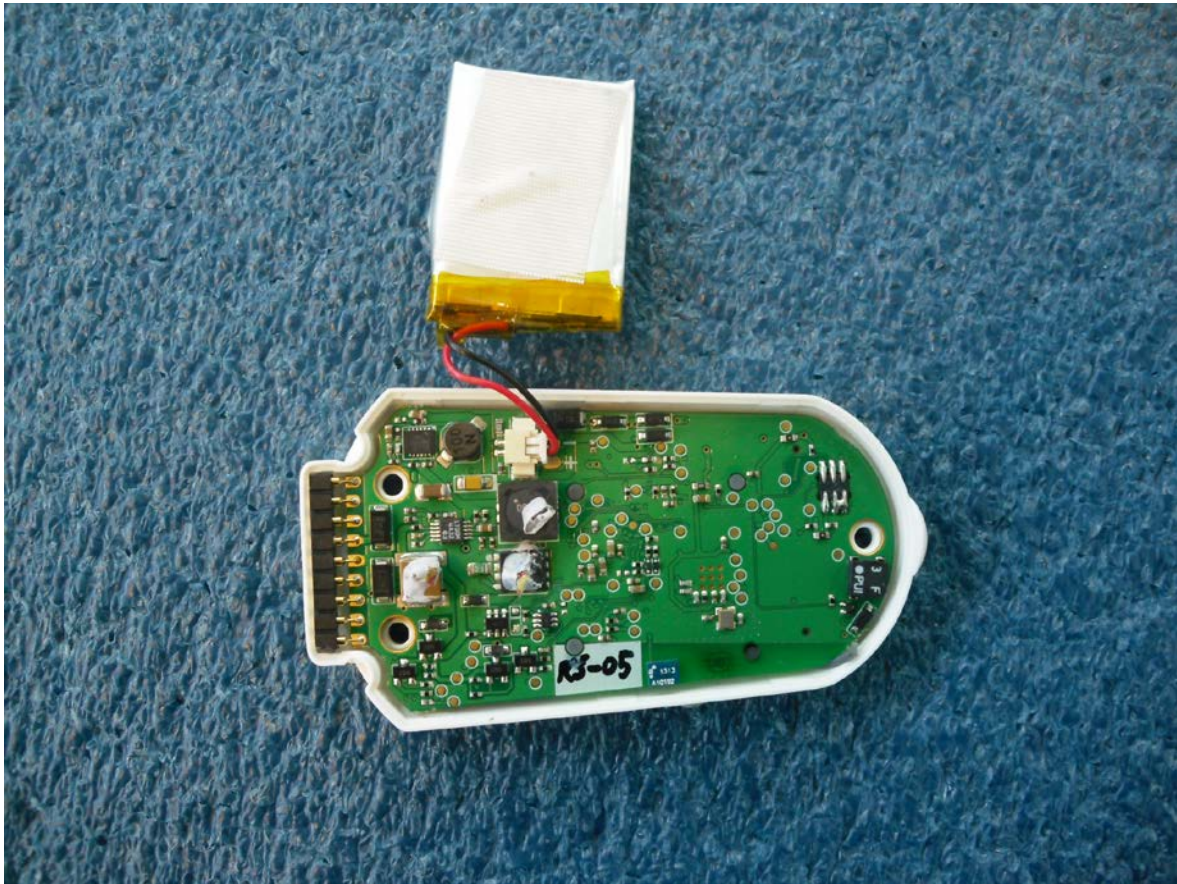


Hand Stimulator – Photo 2

Client	Rehabtronics Inc.	
Product	Hand Stimulator with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	




Hand Stimulator – Photo 3

Client	Rehabtronics Inc.	
Product	Hand Stimulator with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	

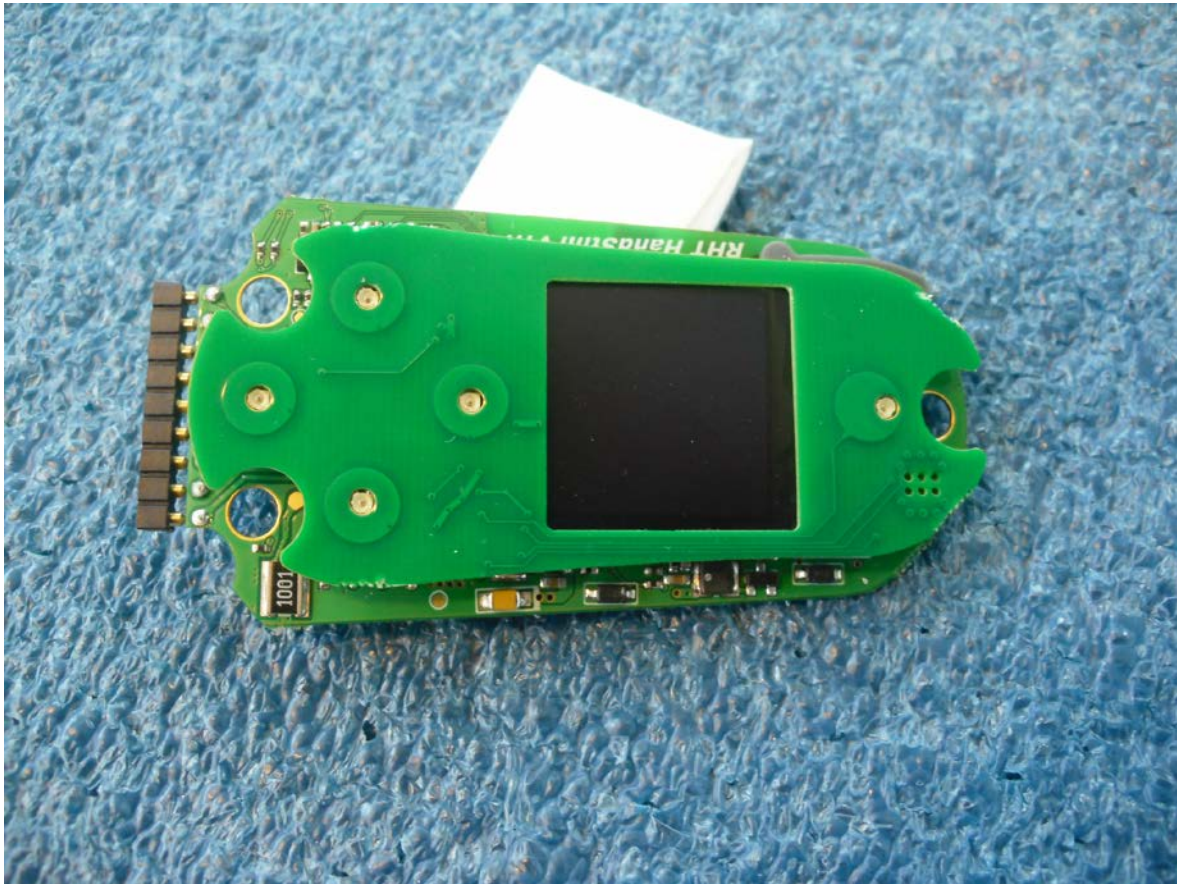


Hand Stimulator – Photo 4

Client	Rehabtronics Inc.	
Product	Hand Stimulator with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	

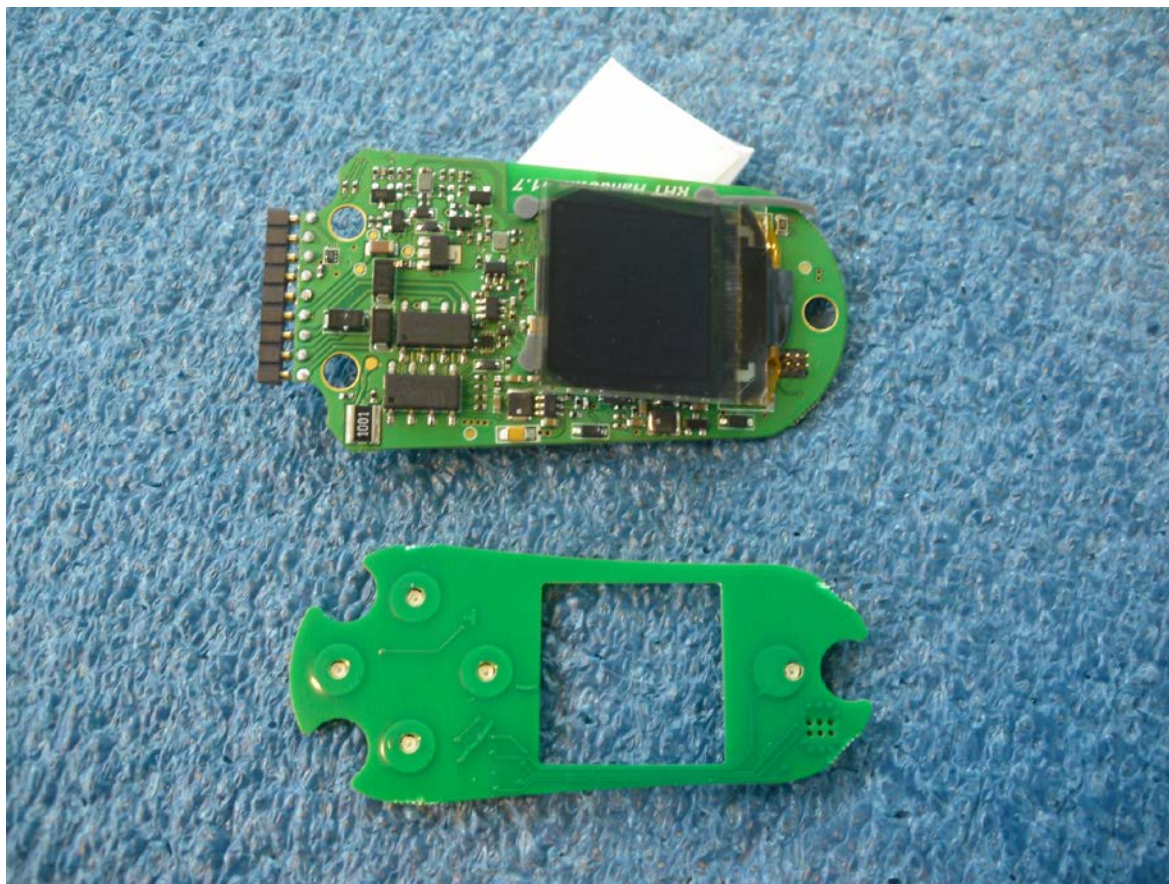


Hand Stimulator – Photo 5

Client	Rehabtronics Inc.	
Product	Hand Stimulator with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	

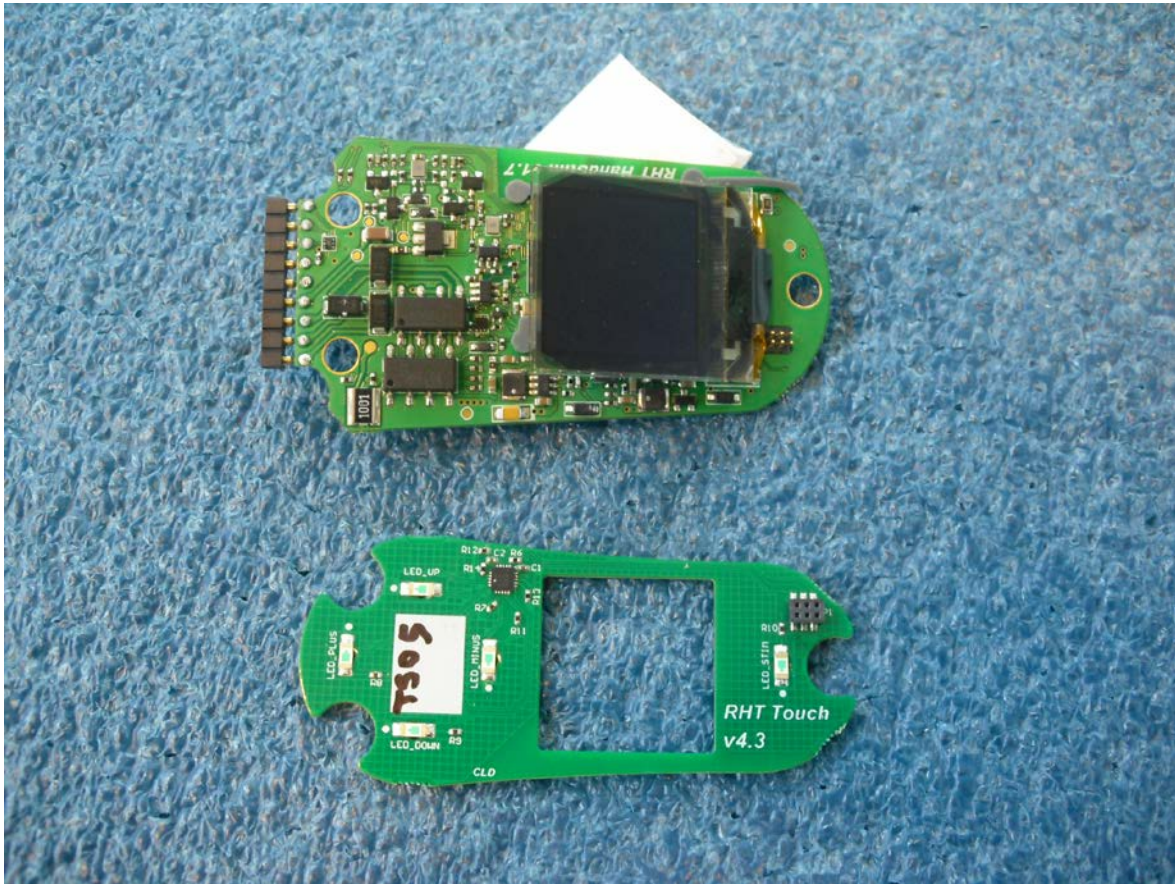


Hand Stimulator – Photo 6

Client	Rehabtronics Inc.	
Product	Hand Stimulator with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	

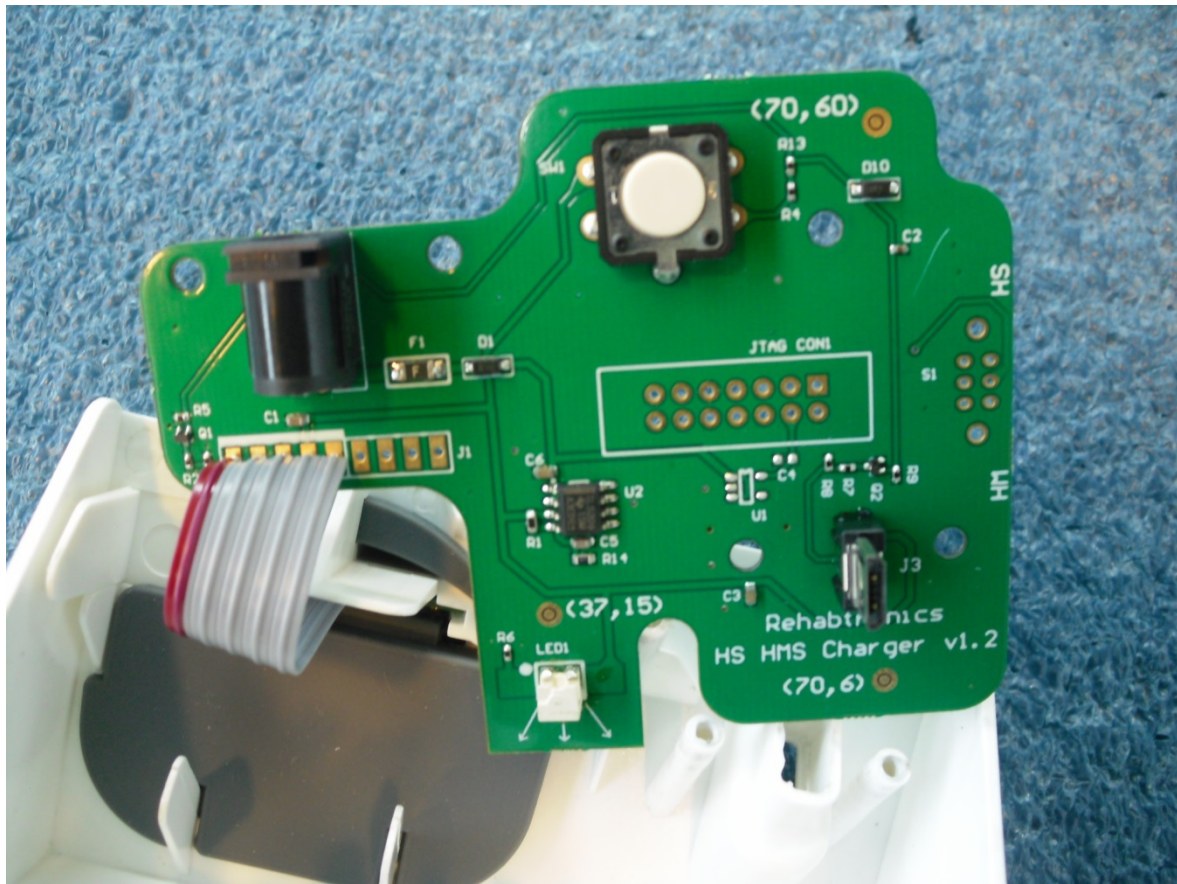

Charge Dock – Photo 1

Client	Rehabtronics Inc.	
Product	Hand Stimulator with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	

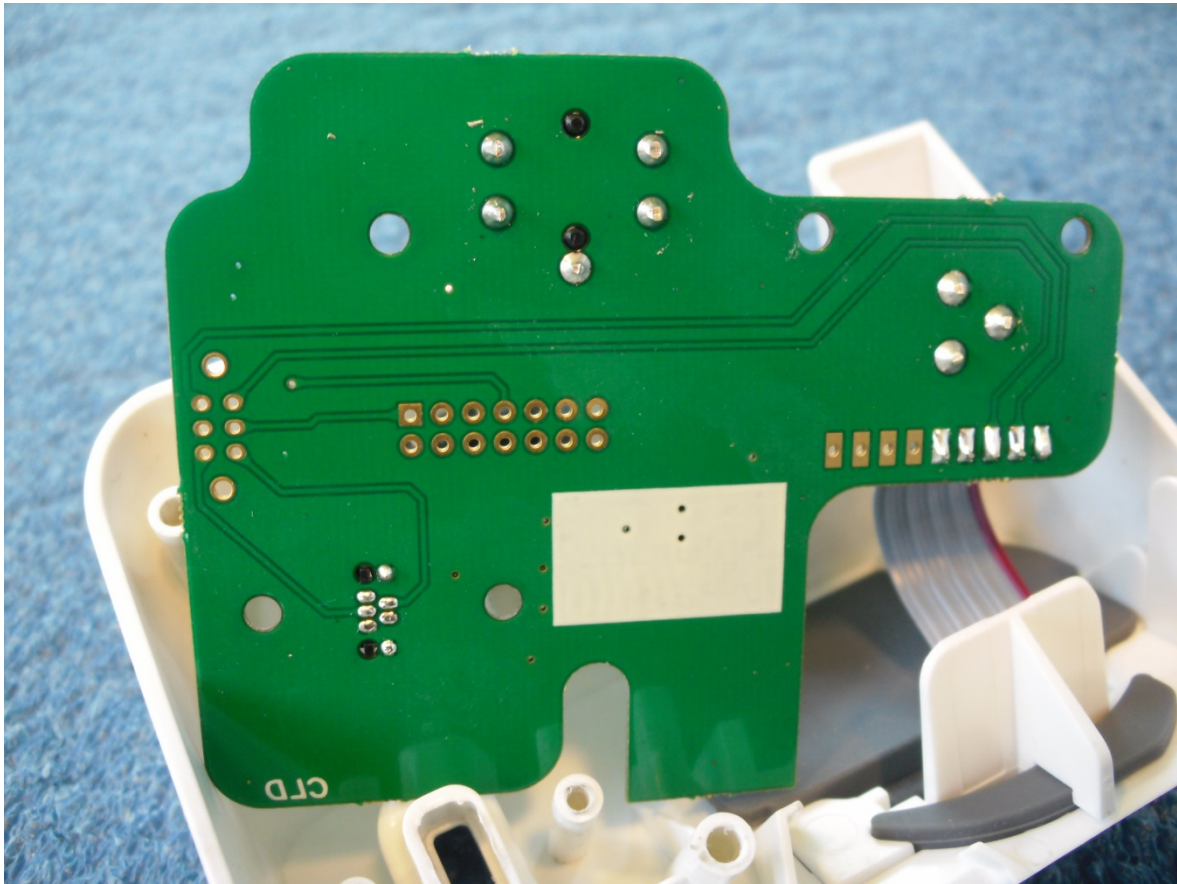

Charge Dock – Photo 2