



Client	Rehabtronics Inc.	
Product	Head Motion Sensor with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	

EUT EXTERNAL PHOTOS – HSHM1




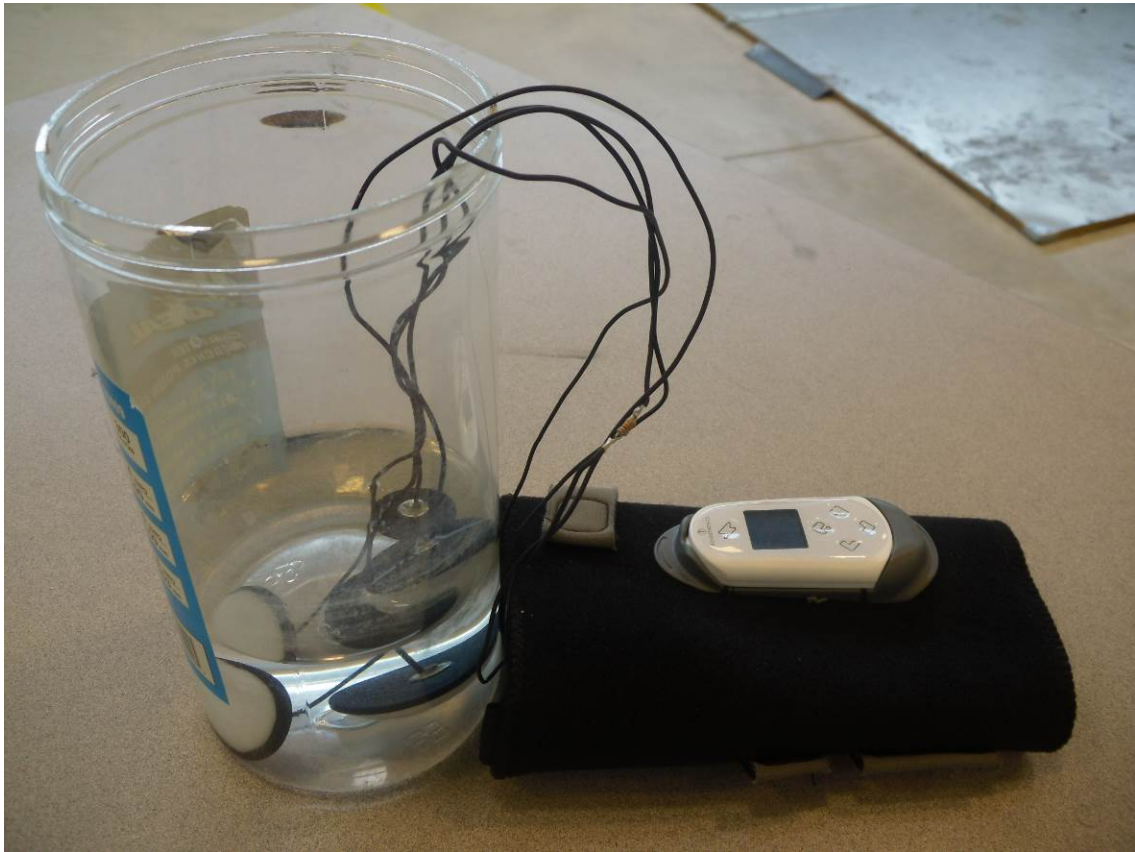
Head Motion Sensor with AC/DC Power supply adaptor and Charge Dock

Client	Rehabtronics Inc.	
Product	Head Motion Sensor with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	




Head Motion Sensor with AC/DC Power supply adaptor, Charge Dock and Hand Stimulator

Client	Rehabtronics Inc.	
Product	Head Motion Sensor with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	




HS unit with Garment and Electrodes in Saline solution

Client	Rehabtronics Inc.	
Product	Head Motion Sensor with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	




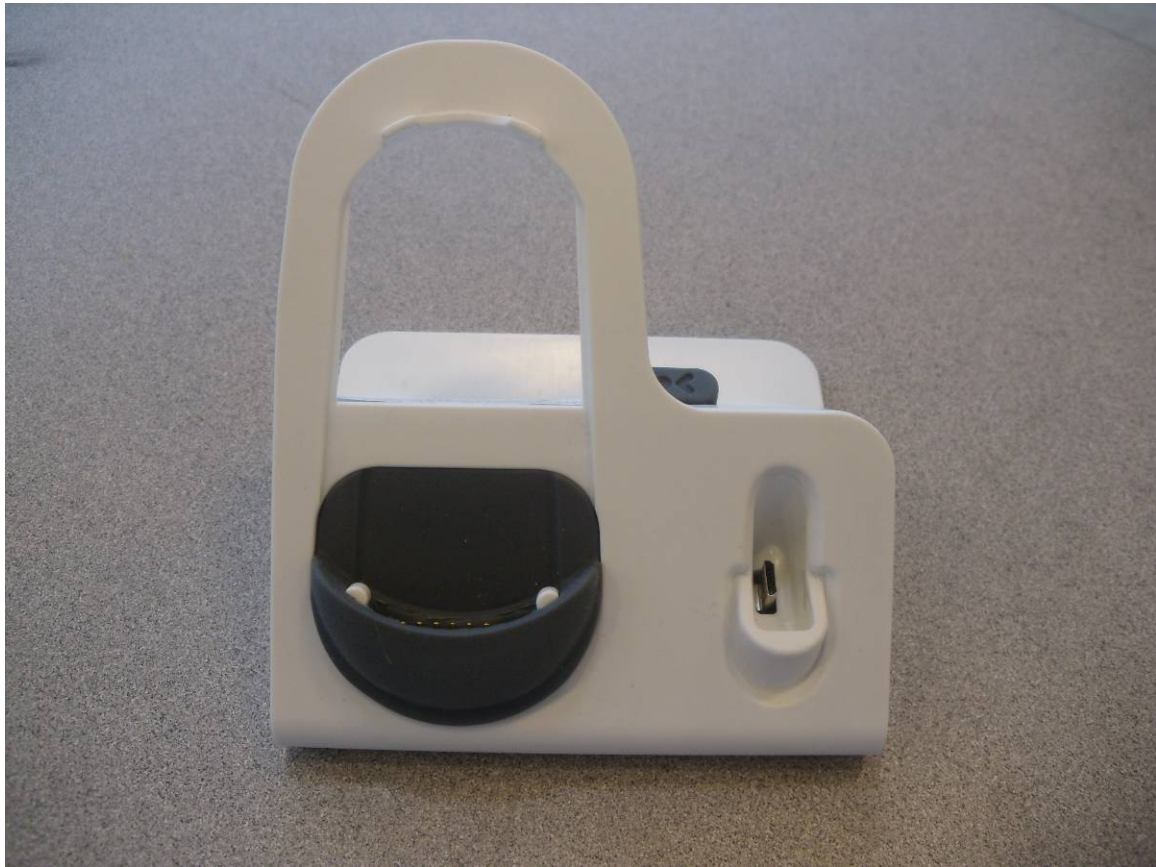
Head Motion Sensor – Photo 1

Client	Rehabtronics Inc.	
Product	Head Motion Sensor with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	




Head Motion Sensor – Photo 2

Client	Rehabtronics Inc.	
Product	Head Motion Sensor with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	




Charge Dock – Photo 1

Client	Rehabtronics Inc.	
Product	Head Motion Sensor with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	



Charge Dock – Photo 2

Client	Rehabtronics Inc.	
Product	Head Motion Sensor with Charge Dock	
Standard(s)	RSS 210 Issue 8:2010 / FCC Part 15 Subpart C:2015	



AC/DC Power Supply Adaptor