



Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

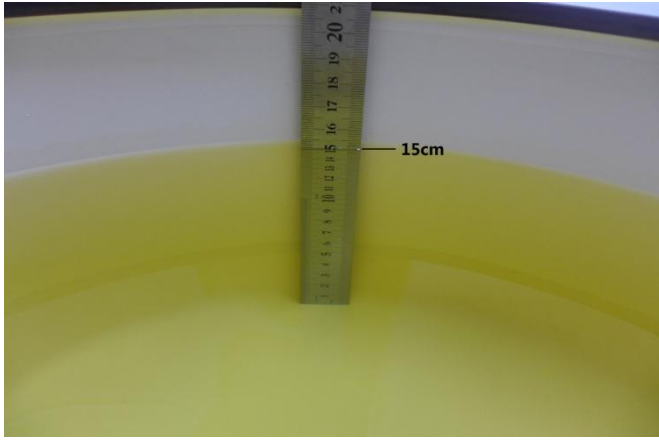
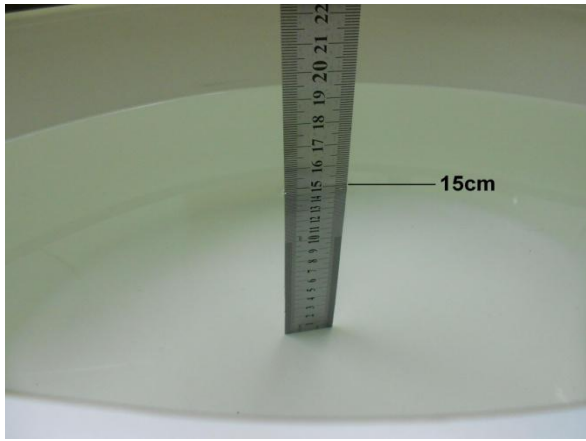
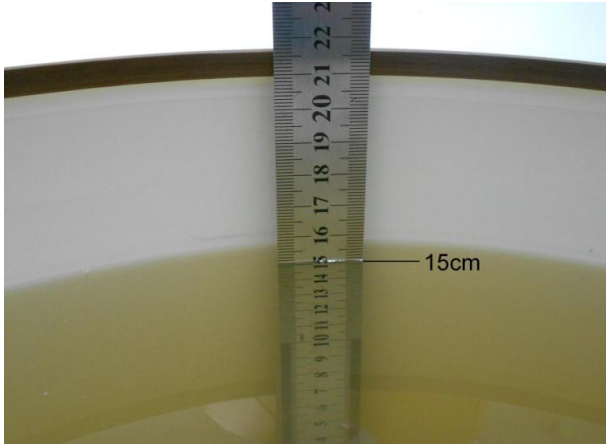
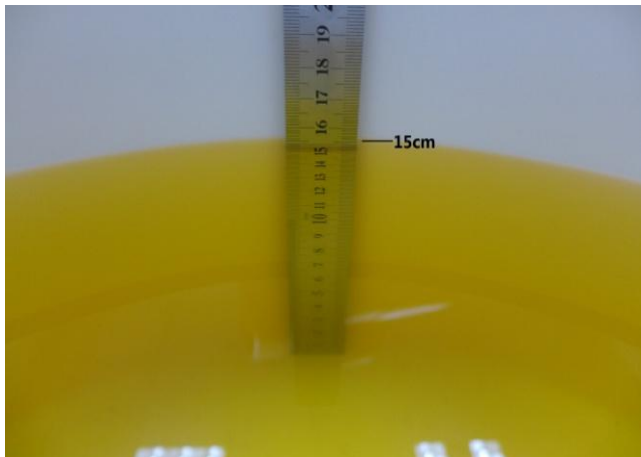
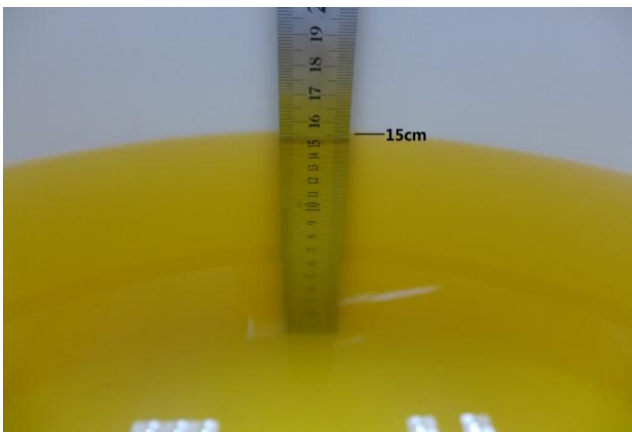
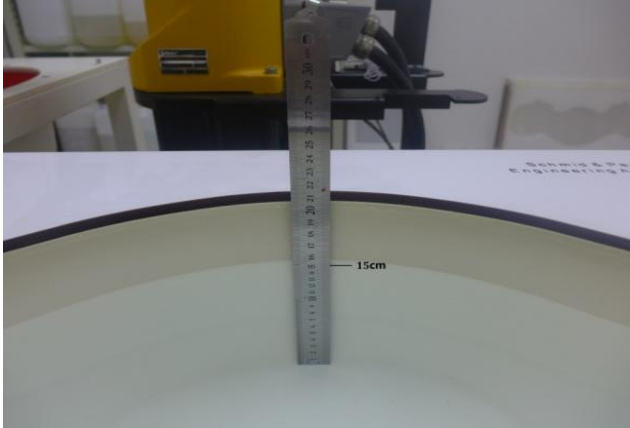
Photo 1: Tissue Simulant Liquid for Body 750	Photo 2: Tissue Simulant Liquid for Body 835
	
Photo 3: Tissue Simulant Liquid for Body 1750	Photo 4: Tissue Simulant Liquid for Body 1900
	
Photo 5: Tissue Simulant Liquid for Body 2450	Photo 6: Tissue Simulant Liquid for Body 2600
	



Photo 7: Tissue Simulant Liquid for Body 5G	NA
	NA

3. Photographs of EUT test position

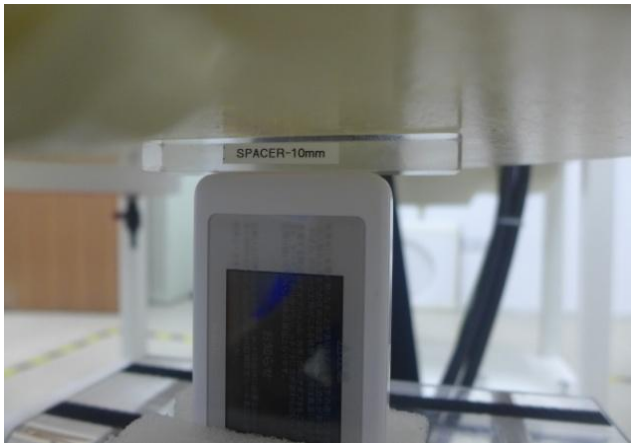
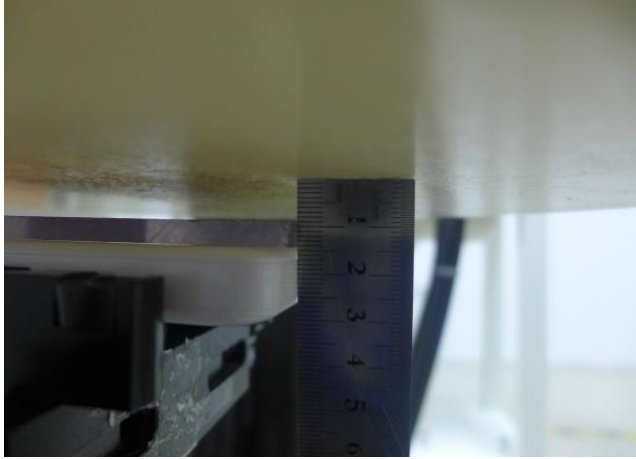
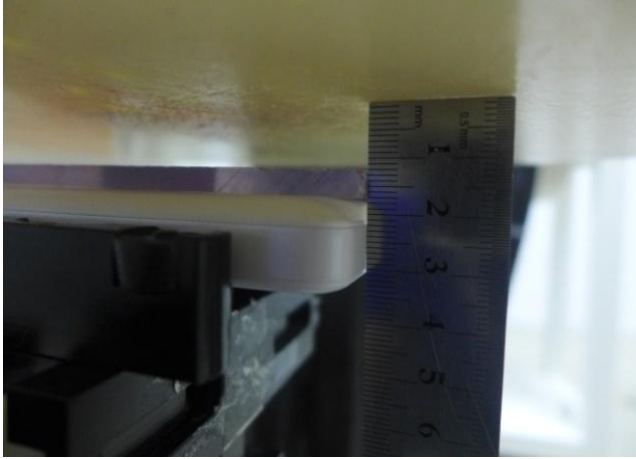
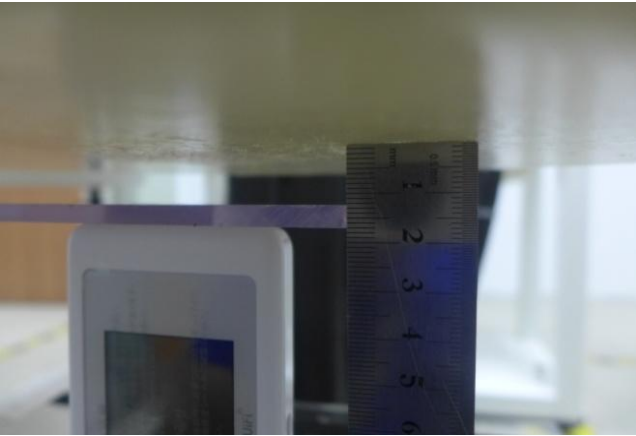
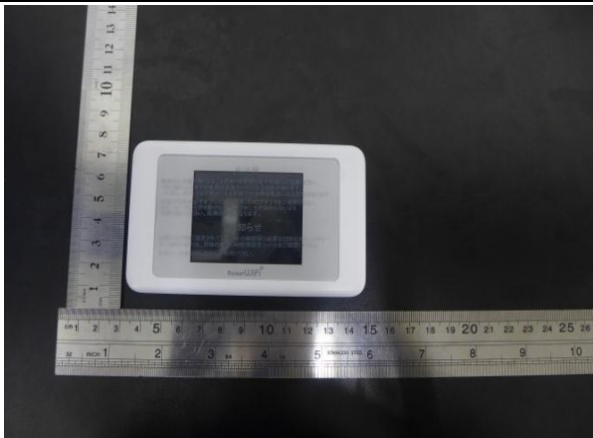
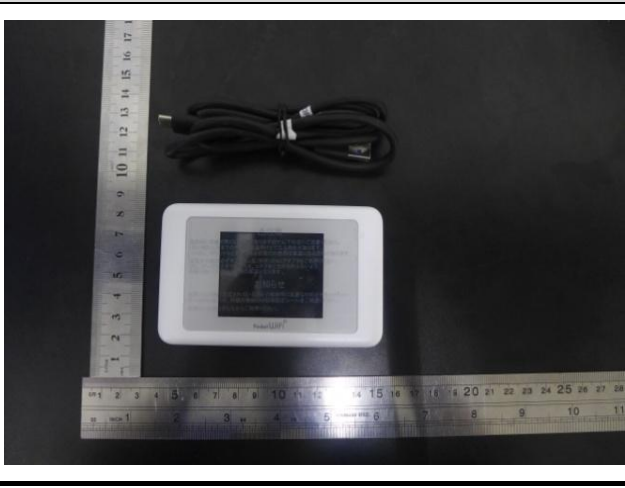
Photo 8: Front side 10mm	Photo 9: Back side 10mm
	
Photo 10: Left side 10mm	Photo 11: Right side 10mm
	
Photo 12: Top side 10mm	Photo 13: Bottom side 10mm
	

Photo 14: Front side 14mm	Photo 15: Back side 17mm
	
Photo 16: Right side 17mm	N/A
	N/A

4. EUT Constructional Details

Photo 17: Front View	Photo 18: Back View
	
Photo 19: Accessory	N/A
	N/A