




# **Appendix D**






## **Photographs**

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

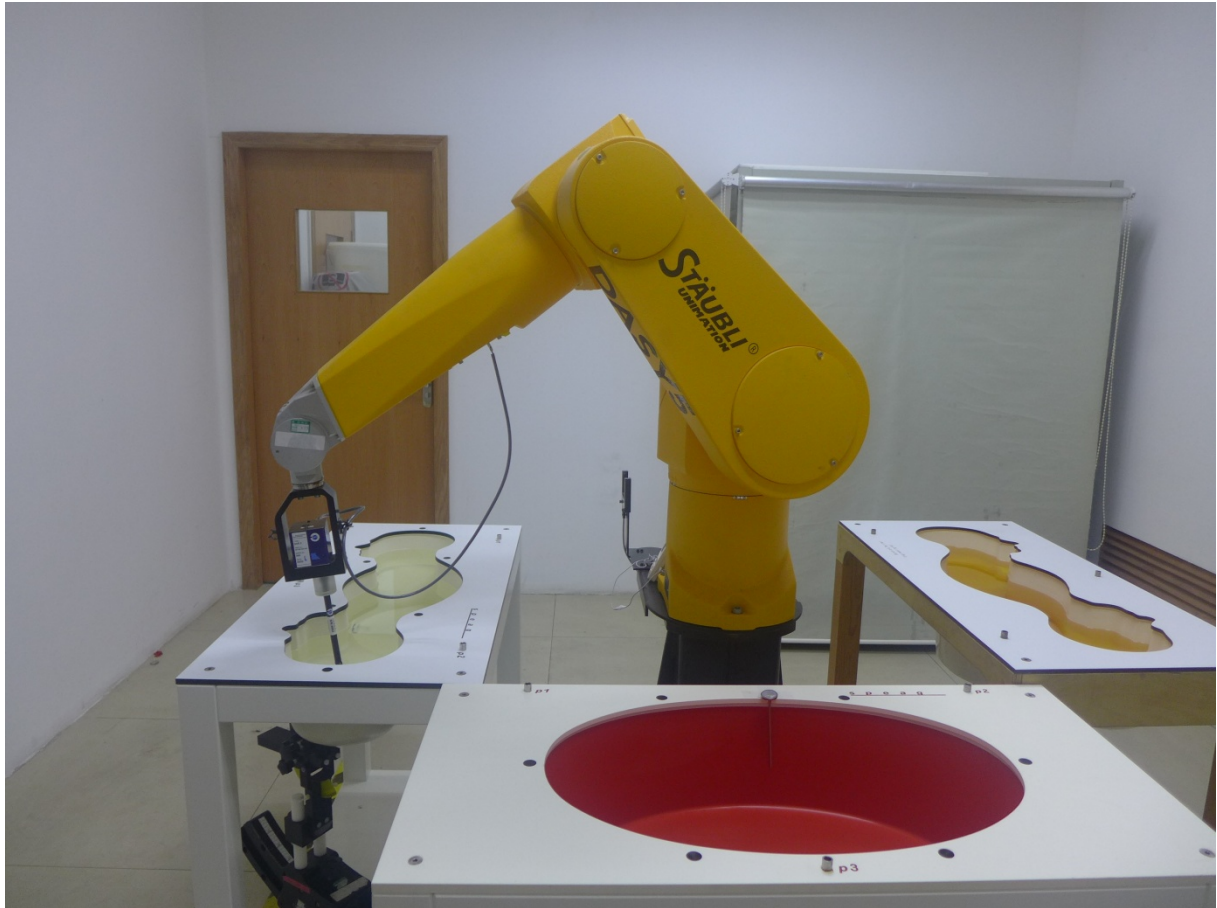



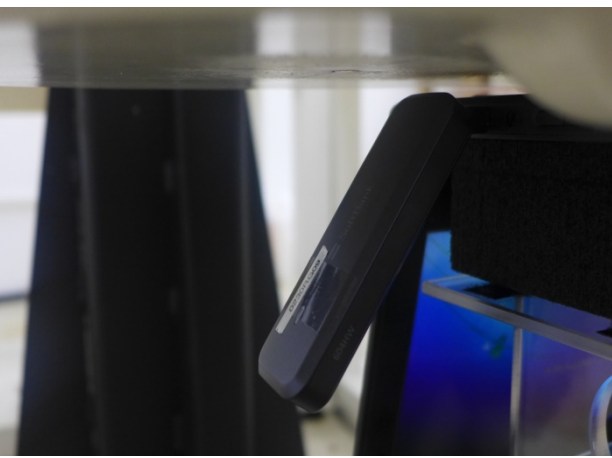
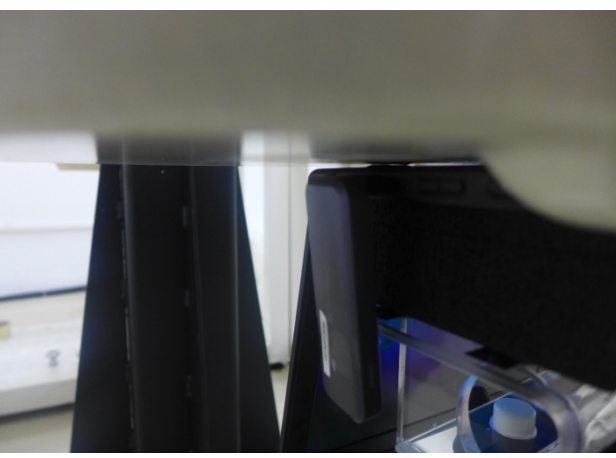
## 1. SAR measurement System

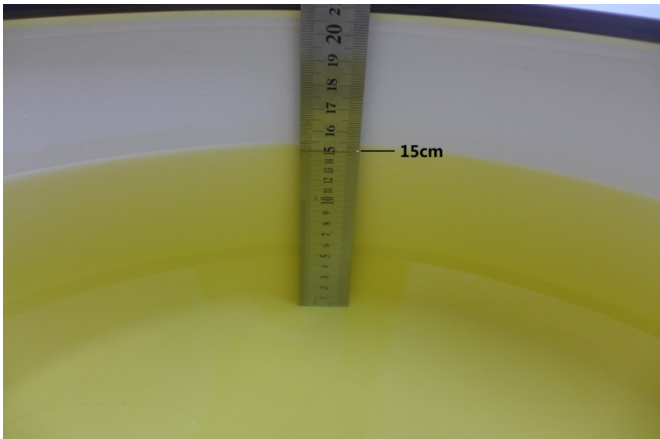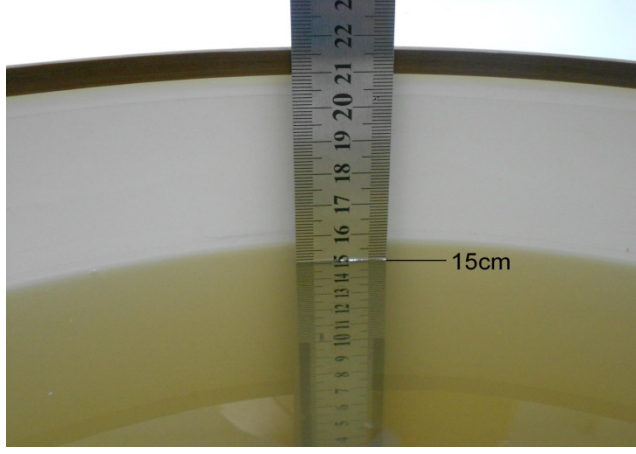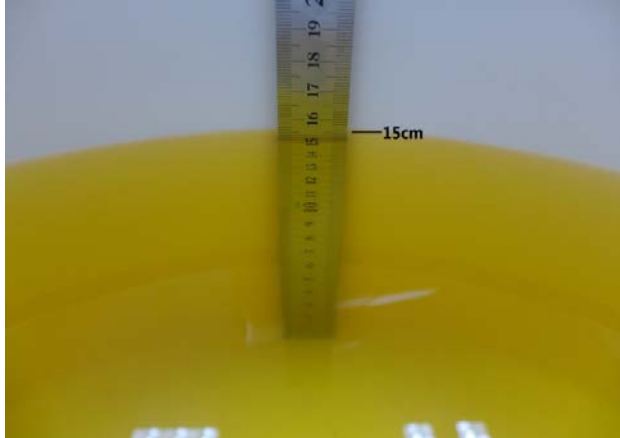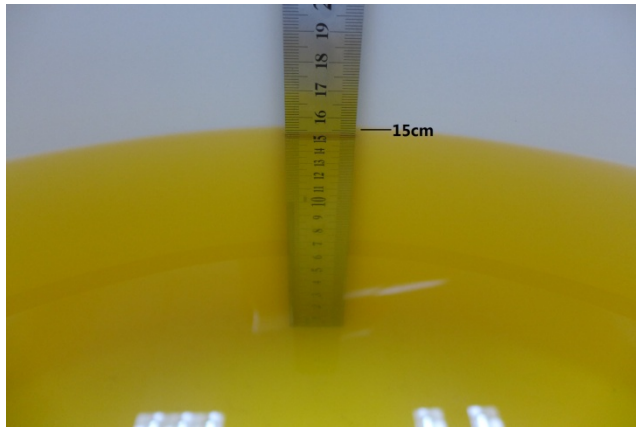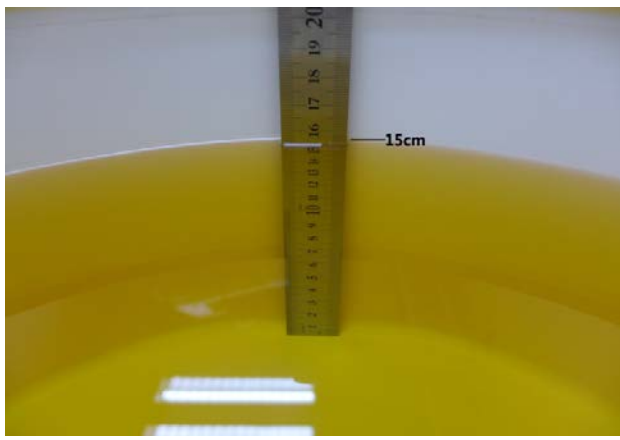

## 2. Photographs of Tissue Simulate Liquid

<p><b>Photo 1: Tissue Simulant Liquid for Body 750</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Body 835</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Body 1750</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Body 1900</b></p>
	
<p><b>Photo 5: Tissue Simulant Liquid for Body 2600</b></p>	<p>N/A</p>
	<p>N/A</p>
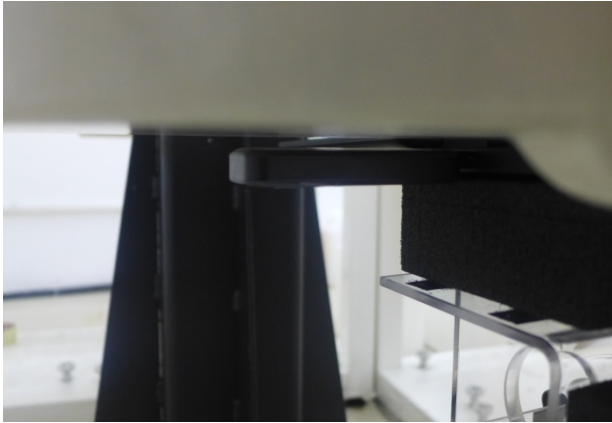
### 3. Photographs of EUT test position

<p><b>Photo 6: Front side 5mm</b></p>	<p><b>Photo 7: Back side 5mm</b></p>
	
<p><b>Photo 8: Left side 5mm</b></p>	<p><b>Photo 9: Right side 5mm</b></p>
	
<p><b>Photo 10: Back side positioned at 45° 5mm</b></p>	<p><b>Photo 11: Back side positioned at 90° 5mm</b></p>
	

#### 4. EUT Constructional Details

