
Appendix D

Photographs

- 1. SAR measurement System
- 2. Photographs of Tissue Simulate Liquid
- 3. Photographs of EUT test position
- 4. EUT Constructional Details

1. SAR measurement System

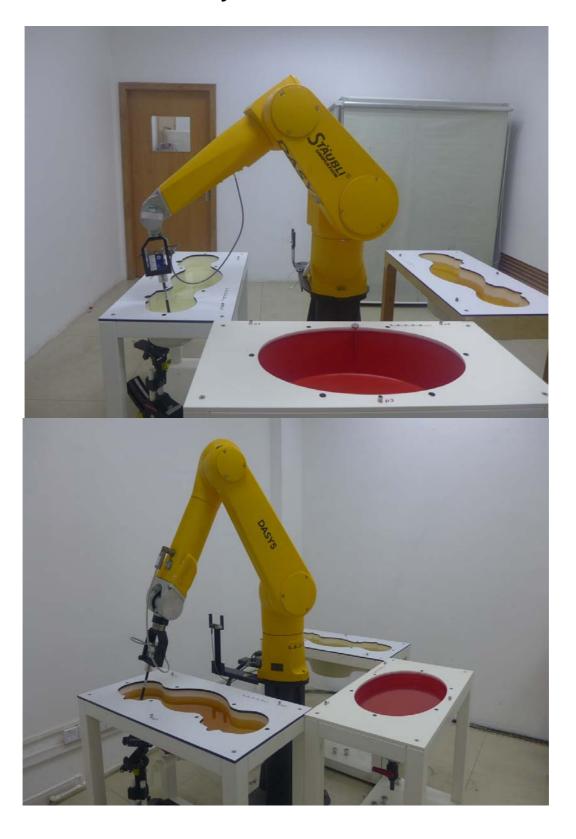

2. Photographs of Tissue Simulate Liquid

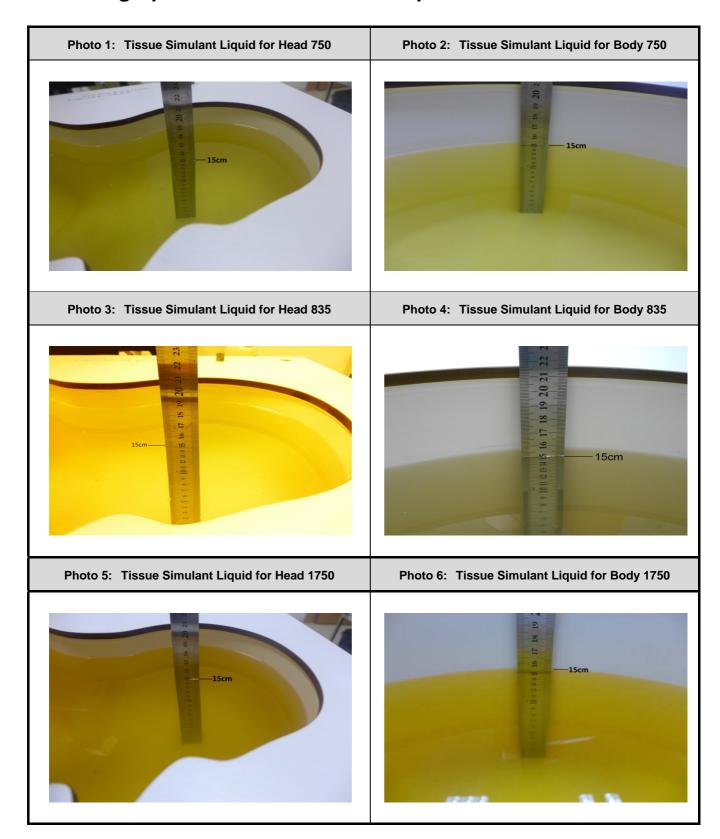


Photo 7: Tissue Simulant Liquid for Head 1900 Photo 8: Tissue Simulant Liquid for Body 1900 Photo 9: Tissue Simulant Liquid for Head 2450 Photo 10: Tissue Simulant Liquid for Body 2450 Photo 11: Tissue Simulant Liquid for Head 2600 Photo 12: Tissue Simulant Liquid for Body 2600

Photo 13: Tissue Simulant Liquid for Head 5G

Photo 14: Tissue Simulant Liquid for Body 5G

3. Photographs of EUT test position Photo 15: Left touch cheek Photo 16: Left tilted 15 degree Photo 17: Right touch cheek Photo 18: Right tilted 15 degree Photo 19: Front side 15mm Photo 20: Back side 15mm


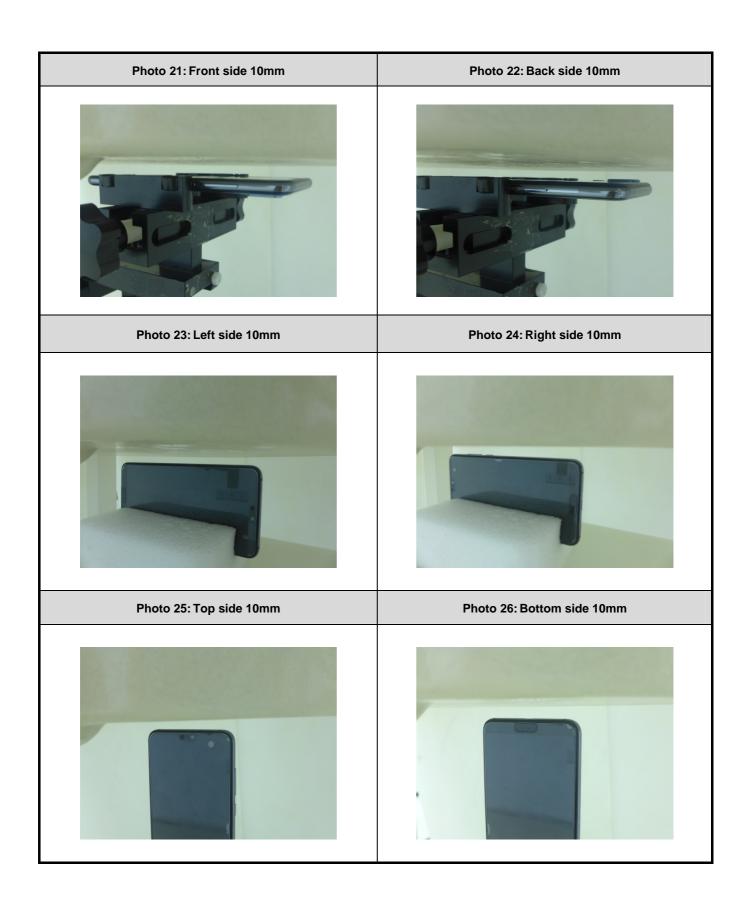


Photo 27: Front side 0mm Photo 28: Back side 0mm Photo 30: Right side 0mm Photo 29: Left side 0mm Photo 31: Top side 0mm Photo 32: Bottom side 0mm



4. EUT Constructional Details

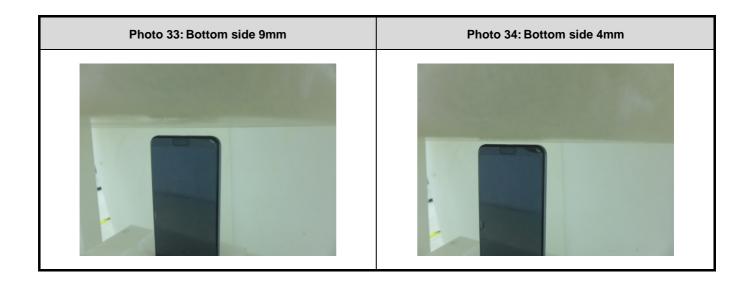