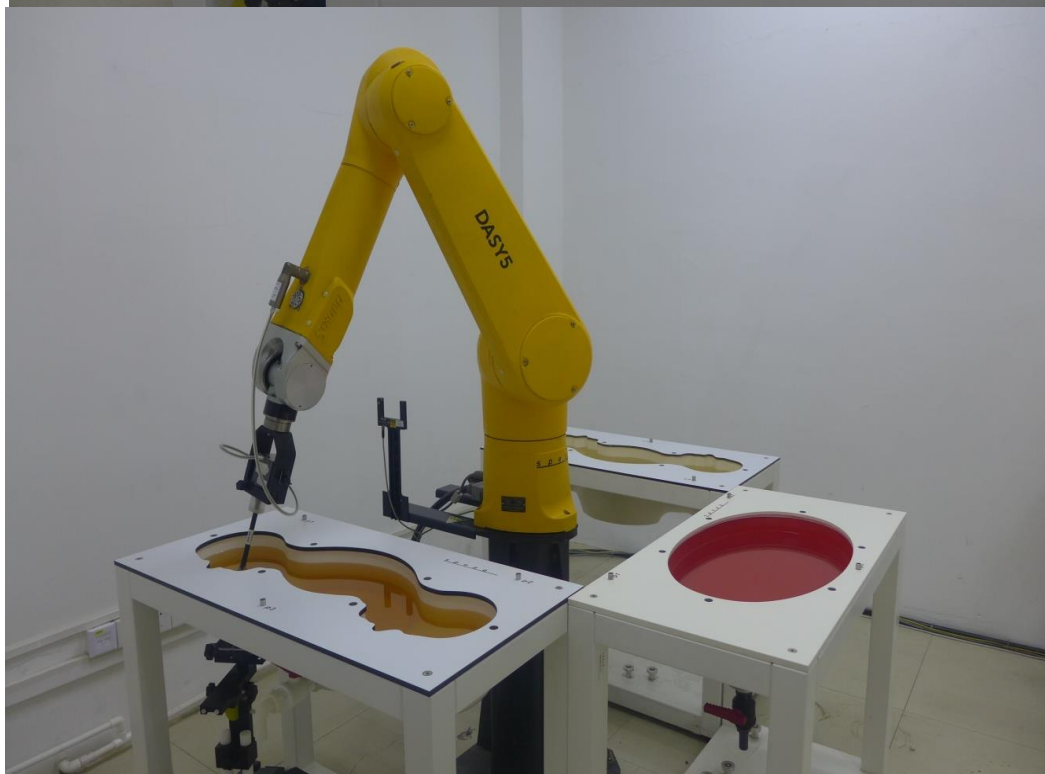


Appendix D

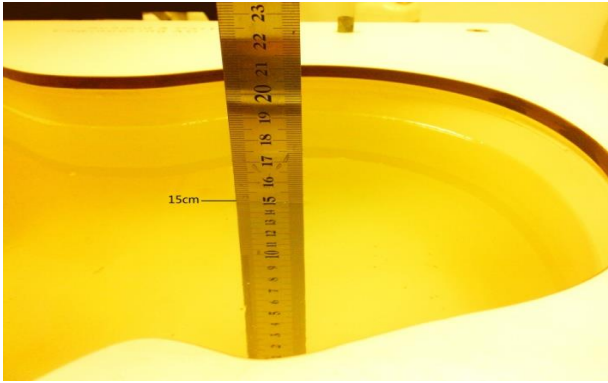
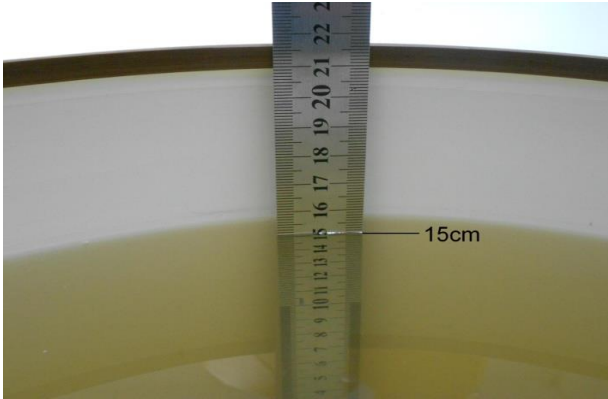
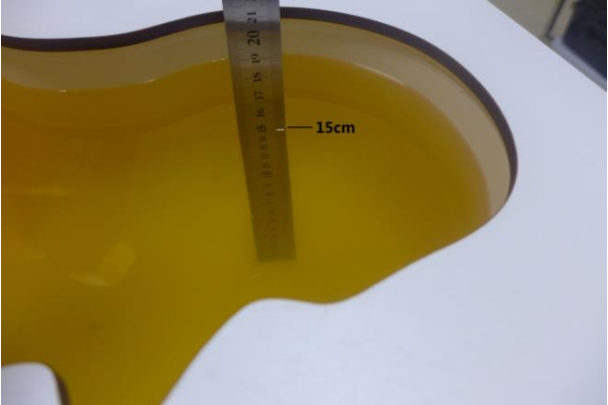
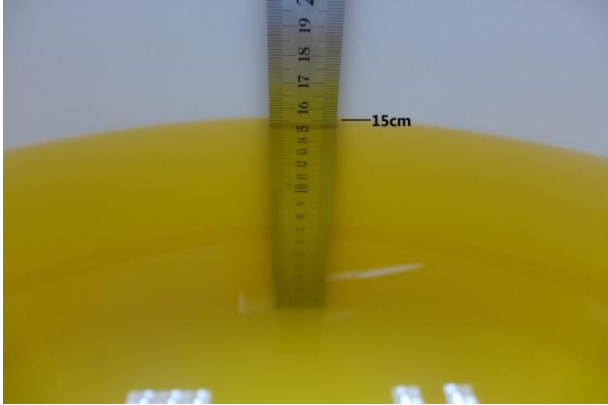
Photographs

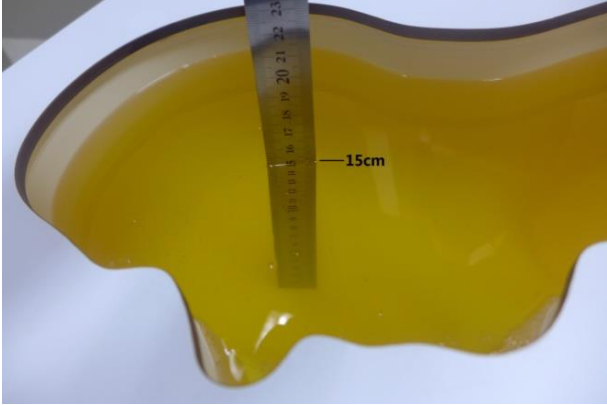
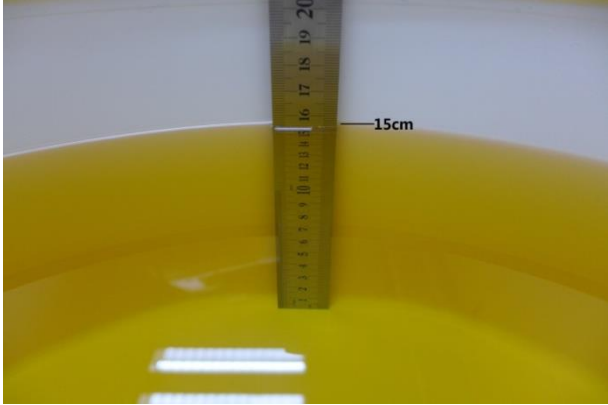
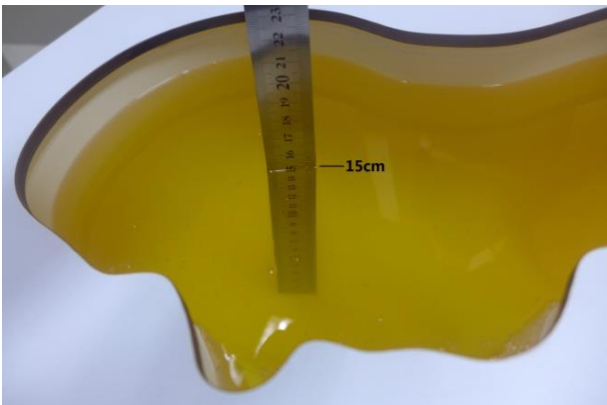
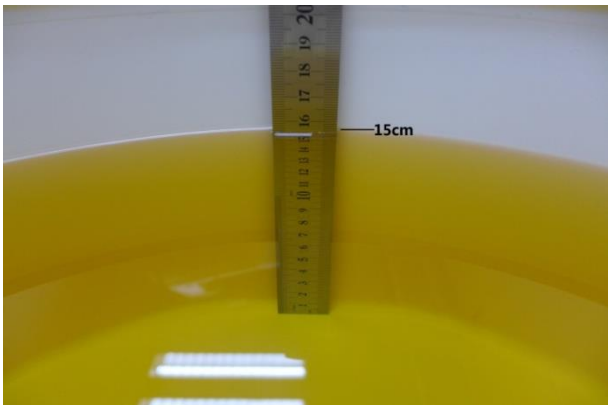
1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details
5. Serial Number of EUT

1. SAR measurement System

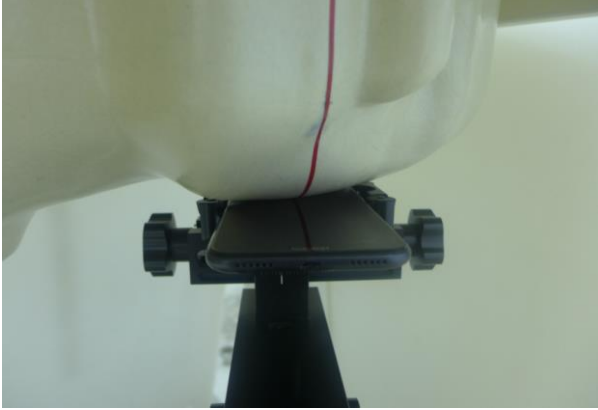

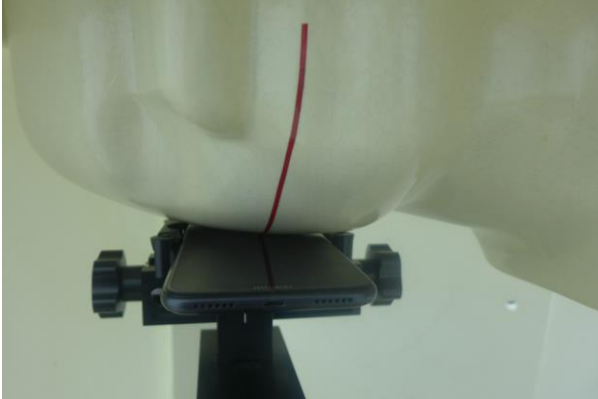

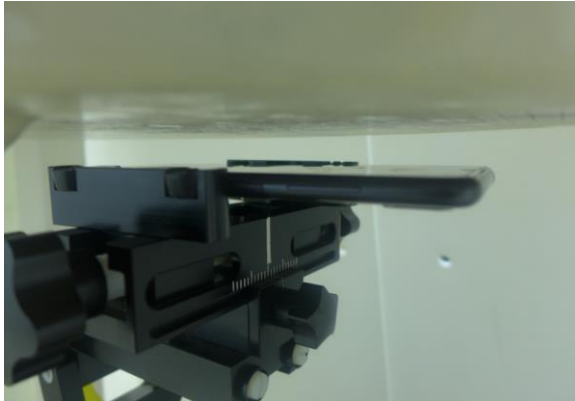



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 835</p>	<p>Photo 2: Tissue Simulant Liquid for Body 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 1900</p>	<p>Photo 4: Tissue Simulant Liquid for Body 1900</p>
	

<p>Photo 5: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 6: Tissue Simulant Liquid for Body 2450</p>
	
<p>Photo 7: Tissue Simulant Liquid for Head 2600</p>	<p>Photo 8: Tissue Simulant Liquid for Body 2600</p>
	

3. Photographs of EUT test position

<p>Photo 9: Left cheek</p>	<p>Photo 10: Left tilted</p>
	
<p>Photo 11: Right cheek</p>	<p>Photo 12: Right tilted</p>
	
<p>Photo 13: Front side 15mm</p>	<p>Photo 14: Back side 15mm</p>
	

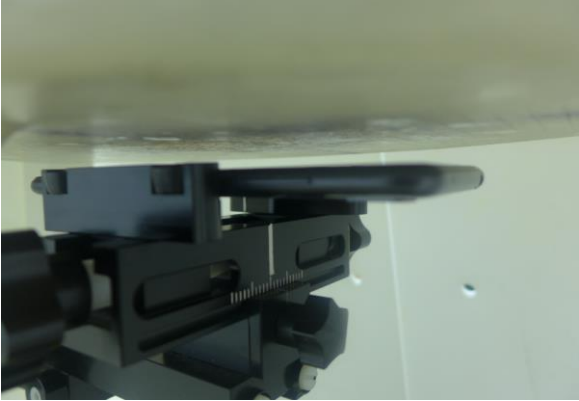
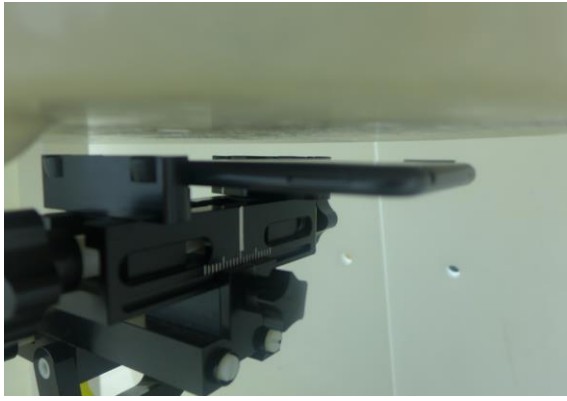




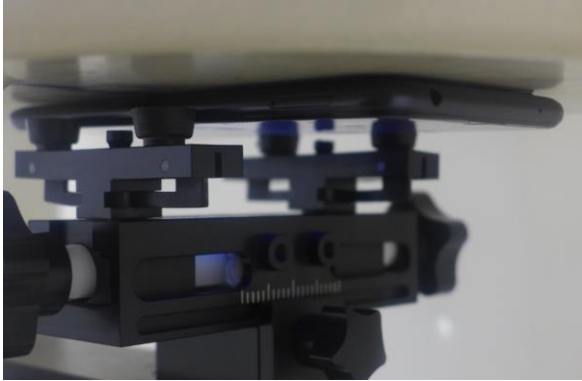


<p>Photo 15: Front side 10mm</p>	<p>Photo 16: Back side 10mm</p>
	
<p>Photo 17: Left side 10mm</p>	<p>Photo 18: Right side 10mm</p>
	
<p>Photo 19: Top side 10mm</p>	<p>Photo 20: Bottom side 10mm</p>
	

Photo 21: Back side 0mm	Photo 22: Bottom side 0mm
	
Photo 23: Bottom side 15mm	N/A
	N/A

4. EUT Constructional Details

Photo 24: Front View	Photo 25: Back View
