

**Appendix C. Calibration Certificate**

<b>Table of contents</b>
<b>DAE3-393</b>
<b>DAE4-916</b>
<b>DAE4-1235</b>
<b>DAE4-1492</b>
<b>DAE4-851</b>
<b>DAE4-1236</b>
<b>Probe ES3DV3-3168</b>
<b>Probe EX3DV4-3743</b>
<b>Probe EX3DV4-3744</b>
<b>Probe EX3DV4-7381</b>
<b>Probe EX3DV4-7489</b>
<b>Dipole D750V3-1044</b>
<b>Dipole D835V2-4d059</b>
<b>Dipole D835V2-4d126</b>
<b>Dipole D1750V2-1145</b>
<b>Dipole D1900V2-5d091</b>
<b>Dipole D1900V2-5d143</b>
<b>Dipole D2450V2-860</b>
<b>Dipole D2600V2-1021</b>
<b>Dipole D2600V2-1032</b>
<b>Dipole D5GHzV2-1155</b>
<b>Justification of the extended calibration of Dipole D835V2-4d059</b>
<b>Justification of the extended calibration of Dipole D1900V2-5d143</b>



In Collaboration with  
**s p e a g**  
**CALIBRATION LABORATORY**



中国认可  
国际互认  
校准  
CALIBRATION  
CNAS L0570

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com [Http://www.chinattl.cn](http://www.chinattl.cn)

Client : **Auden**

Certificate No: **Z18-60290**

## CALIBRATION CERTIFICATE

Object: **DAE3 - SN: 393**

Calibration Procedure(s): **FF-Z11-002-01**  
**Calibration Procedure for the Data Acquisition Electronics (DAEx)**

Calibration date: **August 14, 2018**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements(SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature(22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Process Calibrator 753	1971018	20-Jun-18 (CTTL, No.J18X05034)	June-19

	Name	Function	Signature
Calibrated by:	Yu Zongying	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyuan	SAR Project Leader	

Issued: August 15, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



In Collaboration with

**s p e a g**

**CALIBRATION LABORATORY**

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62304633-2512

Fax: +86-10-62304633-2504

E-mail: [ctl@chinattl.com](mailto:ctl@chinattl.com)

[Http://www.chinattl.cn](http://www.chinattl.cn)

### **Glossary:**

DAE                                    data acquisition electronics  
Connector angle                information used in DASY system to align probe sensor X  
to the robot coordinate system.

### **Methods Applied and Interpretation of Parameters:**

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China  
Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504  
E-mail: cttl@chinattl.com Http://www.chinattl.cn

### DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 $\mu$ V, full range = -100...+300 mV  
Low Range: 1LSB = 61nV, full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	403.890 $\pm$ 0.15% (k=2)	404.114 $\pm$ 0.15% (k=2)	403.987 $\pm$ 0.15% (k=2)
Low Range	3.96967 $\pm$ 0.7% (k=2)	3.96032 $\pm$ 0.7% (k=2)	3.95474 $\pm$ 0.7% (k=2)

### Connector Angle

Connector Angle to be used in DASY system	104.5 $^{\circ}$ $\pm$ 1 $^{\circ}$
---	-------------------------------------



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Auden**

Certificate No: **DAE4-916\_Dec18**

## CALIBRATION CERTIFICATE

Object **DAE4 - SD 000 D04 BK - SN: 916**

Calibration procedure(s) **QA CAL-06.v29  
Calibration procedure for the data acquisition electronics (DAE)**

Calibration date: **December 12, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	03-Sep-18 (No:23488)	Sep-19
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	04-Jan-18 (in house check)	In house check: Jan-19
Calibrator Box V2.1	SE UMS 006 AA 1002	04-Jan-18 (in house check)	In house check: Jan-19

Calibrated by:	Name <b>Adrian Gehring</b>	Function Laboratory Technician	Signature 
----------------	-------------------------------	-----------------------------------	---------------

Approved by:	Name <b>Sven Kühn</b>	Deputy Manager	
--------------	--------------------------	----------------	--

Issued: December 12, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

## Glossary

DAE	data acquisition electronics
Connector angle	information used in DASY system to align probe sensor X to the robot coordinate system.

## Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - *DC Voltage Measurement Linearity:* Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
  - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
  - *AD Converter Values with inputs shorted:* Values on the internal AD converter corresponding to zero input voltage
  - *Input Offset Measurement:* Output voltage and statistical results over a large number of zero voltage measurements.
  - *Input Offset Current:* Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - *Input resistance:* Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - *Low Battery Alarm Voltage:* Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption:* Typical value for information. Supply currents in various operating modes.

## DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 $\mu$ V, full range = -100...+300 mV

Low Range: 1LSB = 61nV, full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	403.888 $\pm$ 0.02% (k=2)	403.673 $\pm$ 0.02% (k=2)	403.805 $\pm$ 0.02% (k=2)
Low Range	3.97348 $\pm$ 1.50% (k=2)	3.98716 $\pm$ 1.50% (k=2)	3.98005 $\pm$ 1.50% (k=2)

## Connector Angle

Connector Angle to be used in DASY system	238.0 $^{\circ}$ $\pm$ 1 $^{\circ}$
---	-------------------------------------

## Appendix (Additional assessments outside the scope of SCS0108)

### 1. DC Voltage Linearity

High Range	Reading ( $\mu\text{V}$ )	Difference ( $\mu\text{V}$ )	Error (%)
Channel X + Input	199992.11	-2.78	-0.00
Channel X + Input	20005.08	3.66	0.02
Channel X - Input	-19997.19	4.29	-0.02
Channel Y + Input	199992.36	-2.61	-0.00
Channel Y + Input	20003.73	2.27	0.01
Channel Y - Input	-19999.71	1.73	-0.01
Channel Z + Input	199995.79	0.56	0.00
Channel Z + Input	20002.74	1.40	0.01
Channel Z - Input	-20000.30	1.28	-0.01

Low Range	Reading ( $\mu\text{V}$ )	Difference ( $\mu\text{V}$ )	Error (%)
Channel X + Input	2001.22	0.29	0.01
Channel X + Input	201.35	-0.00	-0.00
Channel X - Input	-198.82	-0.27	0.14
Channel Y + Input	2000.96	0.06	0.00
Channel Y + Input	200.69	-0.57	-0.29
Channel Y - Input	-199.49	-0.85	0.43
Channel Z + Input	2001.26	0.44	0.02
Channel Z + Input	200.34	-0.82	-0.41
Channel Z - Input	-199.73	-1.01	0.51

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading ( $\mu\text{V}$ )	Low Range Average Reading ( $\mu\text{V}$ )
Channel X	200	3.88	2.12
	- 200	-1.99	-3.85
Channel Y	200	-16.05	-16.55
	- 200	15.89	15.30
Channel Z	200	-22.49	-22.84
	- 200	20.68	21.11

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X ( $\mu\text{V}$ )	Channel Y ( $\mu\text{V}$ )	Channel Z ( $\mu\text{V}$ )
Channel X	200	-	-1.48	-2.74
Channel Y	200	4.93	-	1.01
Channel Z	200	8.06	3.05	-



#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15875	14101
Channel Y	16117	17519
Channel Z	15956	14920

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

	Average ( $\mu$ V)	min. Offset ( $\mu$ V)	max. Offset ( $\mu$ V)	Std. Deviation ( $\mu$ V)
Channel X	0.29	-1.07	2.33	0.51
Channel Y	-0.30	-1.32	1.31	0.42
Channel Z	-0.23	-1.29	1.28	0.51

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

#### 8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

#### 9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

## IMPORTANT NOTICE

### USAGE OF THE DAE 4

The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:

**Battery Exchange:** The battery cover of the DAE4 unit is closed using a screw, over tightening the screw may cause the threads inside the DAE to wear out.

**Shipping of the DAE:** Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an antistatic bag. This antistatic bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.

**E-Stop Failures:** Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.

**Repair:** Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect.

**DASY Configuration Files:** Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file.

**Important Note:**

**Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer.**

**Important Note:**

**Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure.**

**Important Note:**

**To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.**



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Huawei-SZ (Auden)**

Certificate No: **DAE4-1235\_Nov18**

## CALIBRATION CERTIFICATE

Object **DAE4 - SD 000 D04 BM - SN: 1235**

Calibration procedure(s) **QA CAL-06.v29  
Calibration procedure for the data acquisition electronics (DAE)**

Calibration date: **November 14, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	03-Sep-18 (No:23488)	Sep-19
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	04-Jan-18 (in house check)	In house check: Jan-19
Calibrator Box V2.1	SE UMS 006 AA 1002	04-Jan-18 (in house check)	In house check: Jan-19

Calibrated by:	Name <b>Adrian Gehring</b>	Function Laboratory Technician	Signature 
Approved by:	Name <b>Sven Kühn</b>	Function Deputy Manager	

Issued: November 14, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

## Glossary

DAE data acquisition electronics  
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

## Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement*: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle*: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - *DC Voltage Measurement Linearity*: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - *Common mode sensitivity*: Influence of a positive or negative common mode voltage on the differential measurement.
  - *Channel separation*: Influence of a voltage on the neighbor channels not subject to an input voltage.
  - *AD Converter Values with inputs shorted*: Values on the internal AD converter corresponding to zero input voltage
  - *Input Offset Measurement*: Output voltage and statistical results over a large number of zero voltage measurements.
  - *Input Offset Current*: Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - *Input resistance*: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - *Low Battery Alarm Voltage*: Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption*: Typical value for information. Supply currents in various operating modes.

## DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 $\mu$ V, full range = -100...+300 mV  
Low Range: 1LSB = 61nV, full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	405.073 $\pm$ 0.02% (k=2)	403.827 $\pm$ 0.02% (k=2)	404.513 $\pm$ 0.02% (k=2)
Low Range	3.98278 $\pm$ 1.50% (k=2)	3.98936 $\pm$ 1.50% (k=2)	4.00181 $\pm$ 1.50% (k=2)

## Connector Angle

Connector Angle to be used in DASY system	206.0 $^{\circ}$ $\pm$ 1 $^{\circ}$
---	-------------------------------------

## Appendix (Additional assessments outside the scope of SCS0108)

### 1. DC Voltage Linearity

High Range	Reading ( $\mu\text{V}$ )	Difference ( $\mu\text{V}$ )	Error (%)
Channel X + Input	200029.91	-4.89	-0.00
Channel X + Input	20006.05	0.78	0.00
Channel X - Input	-20004.15	1.48	-0.01
Channel Y + Input	200032.57	-7.84	-0.00
Channel Y + Input	20004.20	-0.90	-0.00
Channel Y - Input	-20006.58	-0.94	0.00
Channel Z + Input	200031.79	-2.43	-0.00
Channel Z + Input	20004.21	-0.87	-0.00
Channel Z - Input	-20007.93	-2.15	0.01

Low Range	Reading ( $\mu\text{V}$ )	Difference ( $\mu\text{V}$ )	Error (%)
Channel X + Input	2001.15	0.13	0.01
Channel X + Input	200.99	-0.09	-0.05
Channel X - Input	-198.60	0.25	-0.13
Channel Y + Input	2000.45	-0.58	-0.03
Channel Y + Input	200.51	-0.57	-0.28
Channel Y - Input	-199.76	-0.82	0.41
Channel Z + Input	2001.01	0.11	0.01
Channel Z + Input	199.82	-1.19	-0.59
Channel Z - Input	-200.00	-0.96	0.48

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading ( $\mu\text{V}$ )	Low Range Average Reading ( $\mu\text{V}$ )
Channel X	200	6.42	4.23
	- 200	-3.58	-5.54
Channel Y	200	-23.72	-24.15
	- 200	23.73	23.09
Channel Z	200	6.70	6.61
	- 200	-9.31	-9.70

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X ( $\mu\text{V}$ )	Channel Y ( $\mu\text{V}$ )	Channel Z ( $\mu\text{V}$ )
Channel X	200	-	1.53	-4.09
Channel Y	200	8.21	-	2.79
Channel Z	200	10.00	5.95	-

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16148	13320
Channel Y	16262	15806
Channel Z	15844	15684

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

	Average ( $\mu$ V)	min. Offset ( $\mu$ V)	max. Offset ( $\mu$ V)	Std. Deviation ( $\mu$ V)
Channel X	0.50	-0.46	1.23	0.34
Channel Y	0.04	-1.39	2.11	0.53
Channel Z	-0.31	-1.44	0.72	0.45

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

#### 8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

#### 9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

## **IMPORTANT NOTICE**

### **USAGE OF THE DAE 4**

The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:

**Battery Exchange:** The battery cover of the DAE4 unit is closed using a screw, over tightening the screw may cause the threads inside the DAE to wear out.

**Shipping of the DAE:** Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an antistatic bag. This antistatic bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.

**E-Stop Failures:** Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and dirt accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements.

**Repair:** Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect.

**DASY Configuration Files:** Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MOhm is given in the corresponding configuration file.

**Important Note:**

**Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer.**

**Important Note:**

**Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure.**

**Important Note:**

**To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE.**





Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Huawei (Auden)**

Certificate No: **DAE4-1492\_Nov18**

## CALIBRATION CERTIFICATE

Object **DAE4 - SD 000 D04 BM - SN: 1492**

Calibration procedure(s) **QA CAL-06.v29  
Calibration procedure for the data acquisition electronics (DAE)**

Calibration date: **November 14, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	03-Sep-18 (No:23488)	Sep-19
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	04-Jan-18 (in house check)	In house check: Jan-19
Calibrator Box V2.1	SE UMS 006 AA 1002	04-Jan-18 (in house check)	In house check: Jan-19

Calibrated by:	Name <b>Adrian Gehring</b>	Function <b>Laboratory Technician</b>	Signature 
Approved by:	Name <b>Sven Kühn</b>	Function <b>Deputy Manager</b>	Signature 

Issued: November 14, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

## Glossary

DAE	data acquisition electronics
Connector angle	information used in DASY system to align probe sensor X to the robot coordinate system.

## Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - *DC Voltage Measurement Linearity:* Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
  - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
  - *AD Converter Values with inputs shorted:* Values on the internal AD converter corresponding to zero input voltage
  - *Input Offset Measurement:* Output voltage and statistical results over a large number of zero voltage measurements.
  - *Input Offset Current:* Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - *Input resistance:* Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - *Low Battery Alarm Voltage:* Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption:* Typical value for information. Supply currents in various operating modes.

## DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1  $\mu$ V , full range = -100...+300 mV  
Low Range: 1LSB = 61nV , full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	403.956 $\pm$ 0.02% (k=2)	403.858 $\pm$ 0.02% (k=2)	404.094 $\pm$ 0.02% (k=2)
Low Range	3.94639 $\pm$ 1.50% (k=2)	3.96785 $\pm$ 1.50% (k=2)	3.98626 $\pm$ 1.50% (k=2)

## Connector Angle

Connector Angle to be used in DASY system	358.0 $^{\circ}$ $\pm$ 1 $^{\circ}$
---	-------------------------------------

## Appendix (Additional assessments outside the scope of SCS0108)

### 1. DC Voltage Linearity

High Range	Reading ( $\mu\text{V}$ )	Difference ( $\mu\text{V}$ )	Error (%)
Channel X + Input	200037.21	-2.75	-0.00
Channel X + Input	20003.40	-2.08	-0.01
Channel X - Input	-20003.99	1.92	-0.01
Channel Y + Input	200036.03	-1.70	-0.00
Channel Y + Input	20004.14	-1.25	-0.01
Channel Y - Input	-20001.98	4.09	-0.02
Channel Z + Input	200036.83	-0.22	-0.00
Channel Z + Input	20002.21	-3.15	-0.02
Channel Z - Input	-20006.69	-0.42	0.00

Low Range	Reading ( $\mu\text{V}$ )	Difference ( $\mu\text{V}$ )	Error (%)
Channel X + Input	2000.89	-0.19	-0.01
Channel X + Input	203.45	2.41	1.20
Channel X - Input	-199.24	-0.24	0.12
Channel Y + Input	2002.17	1.14	0.06
Channel Y + Input	200.17	-0.74	-0.37
Channel Y - Input	-199.93	-0.92	0.46
Channel Z + Input	2001.39	0.42	0.02
Channel Z + Input	199.25	-1.62	-0.81
Channel Z - Input	-200.04	-0.96	0.48

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading ( $\mu\text{V}$ )	Low Range Average Reading ( $\mu\text{V}$ )
Channel X	200	25.15	23.13
	-200	-22.21	-23.74
Channel Y	200	0.74	0.62
	-200	-2.03	-2.23
Channel Z	200	6.05	5.36
	-200	-8.35	-8.14

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X ( $\mu\text{V}$ )	Channel Y ( $\mu\text{V}$ )	Channel Z ( $\mu\text{V}$ )
Channel X	200	-	-2.22	-2.97
Channel Y	200	5.99	-	-0.76
Channel Z	200	10.67	3.33	-

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16353	16223
Channel Y	16523	15858
Channel Z	15888	15528

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

	Average ( $\mu$ V)	min. Offset ( $\mu$ V)	max. Offset ( $\mu$ V)	Std. Deviation ( $\mu$ V)
Channel X	0.70	-0.60	2.12	0.51
Channel Y	0.39	-0.98	2.15	0.67
Channel Z	-0.32	-1.56	1.30	0.51

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

#### 8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

#### 9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0106

Client: Huawei-SZ (Aachen)

Certificate No.: DAE4-851\_Jul18

## CALIBRATION CERTIFICATE

Object: DAE4; SD 000-D04 BM; SN: 851

Calibration procedure(s): DA-CAL-06-v29  
Calibration procedure for the data acquisition electronics (DAE)

Calibration date: July 18, 2018

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $< 70\%$ .

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Kaithley Multimeter Type 2001	SN: 0810278	31-Aug-17 (No:21092)	Aug-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	04-Jan-18 (in house check)	In house check: Jan-19
Calibrator Box V2.1	SE UMS 006 AA 1002	04-Jan-18 (in house check)	In house check: Jan-19

	Name	Function	Signature
Calibrated by:	Dominique Steffen	Laboratory Technician	
Approved by:	Sven Kuhn	Deputy Manager	

Issued: July 18, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

## Glossary

DAE	data acquisition electronics
Connector angle	information used in DASY system to align probe sensor X to the robot coordinate system.

## Methods Applied and Interpretation of Parameters

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - **DC Voltage Measurement Linearity:** Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - **Common mode sensitivity:** Influence of a positive or negative common mode voltage on the differential measurement.
  - **Channel separation:** Influence of a voltage on the neighbor channels not subject to an input voltage.
  - **AD Converter Values with inputs shorted:** Values on the internal AD converter corresponding to zero input voltage
  - **Input Offset Measurement:** Output voltage and statistical results over a large number of zero voltage measurements.
  - **Input Offset Current:** Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - **Input resistance:** Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - **Low Battery Alarm Voltage:** Typical value for information. Below this voltage, a battery alarm signal is generated.
  - **Power consumption:** Typical value for information. Supply currents in various operating modes.

## DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 $\mu$ V, full range = 100...+300 mV

Low Range: 1LSB = 61nV, full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	405.371 $\pm$ 0.02% (k=2)	405.337 $\pm$ 0.02% (k=2)	404.889 $\pm$ 0.02% (k=2)
Low Range	3.95523 $\pm$ 1.50% (k=2)	3.99271 $\pm$ 1.50% (k=2)	3.99022 $\pm$ 1.50% (k=2)

## Connector Angle

Connector Angle to be used in DASY system	217.0 $^{\circ}$ + 1 $^{\circ}$
---	---------------------------------



Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range		Reading ( $\mu\text{V}$ )	Difference ( $\mu\text{V}$ )	Error (%)
Channel X	+ Input	200028.22	-7.10	-0.00
Channel X	+ Input	20007.49	1.61	0.01
Channel X	- Input	-20002.47	2.43	-0.01
Channel Y	+ Input	200033.85	-1.76	-0.00
Channel Y	+ Input	20004.43	-1.33	-0.01
Channel Y	- Input	-20005.79	-0.63	0.00
Channel Z	+ Input	200030.90	-4.66	-0.00
Channel Z	+ Input	20003.09	-2.50	-0.01
Channel Z	- Input	-20006.86	-1.72	0.01

Low Range		Reading ( $\mu\text{V}$ )	Difference ( $\mu\text{V}$ )	Error (%)
Channel X	+ Input	2001.99	0.24	0.01
Channel X	+ Input	202.61	0.78	0.39
Channel X	- Input	-197.28	0.38	-0.49
Channel Y	+ Input	2002.02	0.19	0.01
Channel Y	+ Input	201.33	-0.38	-0.19
Channel Y	- Input	-199.63	-1.39	0.70
Channel Z	+ Input	2002.13	0.39	0.02
Channel Z	+ Input	200.45	-1.13	-0.56
Channel Z	- Input	-200.04	-1.64	0.83

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading ( $\mu\text{V}$ )	Low Range Average Reading ( $\mu\text{V}$ )
Channel X	200	9.51	8.58
	-200	-7.05	-8.85
Channel Y	200	-5.19	-5.73
	-200	3.60	3.82
Channel Z	200	12.37	12.47
	-200	-14.28	-14.14

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X ( $\mu\text{V}$ )	Channel Y ( $\mu\text{V}$ )	Channel Z ( $\mu\text{V}$ )
Channel X	200	-	1.09	-4.95
Channel Y	200	7.43	-	0.76
Channel Z	200	10.18	5.64	-

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15355	15492
Channel Y	16033	15978
Channel Z	15781	15991

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

	Average ( $\mu$ V)	min. Offset ( $\mu$ V)	max. Offset ( $\mu$ V)	Std. Deviation ( $\mu$ V)
Channel X	0.24	-1.24	2.54	0.78
Channel Y	0.94	-0.53	2.89	0.74
Channel Z	0.84	-0.51	2.49	0.67

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

#### 8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

#### 9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+11
Supply (- Vcc)	-0.01	-8	-9



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: SCS 0108

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Client: **Huawei SZ (Auder)**

Certificate No.: **DAE4-1236-Jul18**

## CALIBRATION CERTIFICATE

Object: **DAE4 SD 000 D04 BM SN 1236**

Calibration procedure(s): **QA CAL 06 v29  
Calibration procedure for the data acquisition electronics (DAE)**

Calibration date: **July 18, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature  $(22 \pm 3)^\circ\text{C}$  and humidity  $\leq 70\%$ .

Calibration Equipment used (M&TC critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	31-Aug-17 (No:21092)	Aug-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	04-Jan-18 (in house check)	In house check: Jan-18
Calibrator Box V2.1	SE UMS 006 AA 1002	04-Jan-18 (in house check)	In house check: Jan-18

Calibrated by: **Dominique Steffen** (Name) / **Laboratory Technician** (Function) / **[Signature]** (Signature)

Approved by: **Sven Kuhn** (Name) / **Deputy Manager** (Function) / **[Signature]** (Signature)

Issued: July 18, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

## Glossary

DAE	data acquisition electronics
Connector angle	information used in DASY system to align probe sensor X to the robot coordinate system.

## Methods Applied and Interpretation of Parameters

- *DC Voltage Measurement:* Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- *Connector angle:* The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
  - *DC Voltage Measurement Linearity:* Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
  - *Common mode sensitivity:* Influence of a positive or negative common mode voltage on the differential measurement.
  - *Channel separation:* Influence of a voltage on the neighbor channels not subject to an input voltage.
  - *AD Converter Values with inputs shorted:* Values on the internal AD converter corresponding to zero input voltage
  - *Input Offset Measurement:* Output voltage and statistical results over a large number of zero voltage measurements.
  - *Input Offset Current:* Typical value for information; Maximum channel input offset current, not considering the input resistance.
  - *Input resistance:* Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
  - *Low Battery Alarm Voltage:* Typical value for information. Below this voltage, a battery alarm signal is generated.
  - *Power consumption:* Typical value for information. Supply currents in various operating modes.

## DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 $\mu$ V, full range = -100...+300 mV

Low Range: 1LSB = 61nV, full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	404.914 $\pm$ 0.02% (k=2)	404.828 $\pm$ 0.02% (k=2)	405.811 $\pm$ 0.02% (k=2)
Low Range	3.99625 $\pm$ 1.50% (k=2)	3.96391 $\pm$ 1.50% (k=2)	3.99611 $\pm$ 1.50% (k=2)

## Connector Angle

Connector Angle to be used in DASY system	45.5 $^{\circ}$ $\pm$ 1 $^{\circ}$
---	------------------------------------

## Appendix (Additional assessments outside the scope of SCS0108)

### 1. DC Voltage Linearity

High Range		Reading ( $\mu\text{V}$ )	Difference ( $\mu\text{V}$ )	Error (%)
Channel X	+ Input	199996.45	0.25	0.00
Channel X	+ Input	20001.70	-0.30	-0.00
Channel X	- Input	-19998.70	2.36	-0.01
Channel Y	+ Input	199995.67	-0.95	-0.00
Channel Y	+ Input	20001.49	-0.43	-0.00
Channel Y	- Input	-20002.28	-1.16	0.01
Channel Z	+ Input	199993.44	3.24	-0.00
Channel Z	+ Input	19998.00	-3.84	-0.02
Channel Z	- Input	-20001.60	-0.42	0.00

Low Range		Reading ( $\mu\text{V}$ )	Difference ( $\mu\text{V}$ )	Error (%)
Channel X	+ Input	2001.23	-0.07	-0.00
Channel X	+ Input	201.94	0.22	0.11
Channel X	- Input	-197.23	0.90	-0.45
Channel Y	+ Input	2002.45	1.14	0.06
Channel Y	+ Input	200.73	-0.94	-0.46
Channel Y	- Input	-199.20	-0.99	0.50
Channel Z	+ input	2000.56	-0.57	-0.03
Channel Z	+ Input	201.26	-0.26	-0.13
Channel Z	- Input	-199.66	-1.36	0.68

### 2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading ( $\mu\text{V}$ )	Low Range Average Reading ( $\mu\text{V}$ )
Channel X	200	16.66	14.50
	-200	-15.19	-16.53
Channel Y	200	-15.44	-15.62
	-200	14.55	14.28
Channel Z	200	-12.69	-13.20
	-200	11.49	11.23

### 3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X ( $\mu\text{V}$ )	Channel Y ( $\mu\text{V}$ )	Channel Z ( $\mu\text{V}$ )
Channel X	200	-	3.82	-3.41
Channel Y	200	8.64	-	5.14
Channel Z	200	9.45	6.60	-

#### 4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	15768	16195
Channel Y	16027	16704
Channel Z	16313	16381

#### 5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M $\Omega$

	Average ( $\mu$ V)	min. Offset ( $\mu$ V)	max. Offset ( $\mu$ V)	Std. Deviation ( $\mu$ V)
Channel X	0.11	-1.54	1.92	0.70
Channel Y	-0.13	-1.45	1.36	0.65
Channel Z	0.44	-1.71	2.34	0.52

#### 6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

#### 7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

#### 8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

#### 9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+8	+14
Supply (- Vcc)	-0.01	-8	-9



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Huawei-SZ (Auden)**

Certificate No: **ES3-3168\_Sep18**

## CALIBRATION CERTIFICATE

Object **ES3DV3 - SN:3168**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-23.v5, QA CAL-25.v6  
Calibration procedure for dosimetric E-field probes**

Calibration date: **September 27, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-18 (No. 217-02682)	Apr-19
Reference Probe ES3DV2	SN: 3013	30-Dec-17 (No. ES3-3013_Dec17)	Dec-18
DAE4	SN: 660	21-Dec-17 (No. DAE4-660_Dec17)	Dec-18
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-17)	In house check: Oct-18

Calibrated by:	Name <b>Jeton Kastrati</b>	Function <b>Laboratory Technician</b>	Signature 
Approved by:	Name <b>Katja Pokovic</b>	Function <b>Technical Manager</b>	
			Issued: September 29, 2018
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			





Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

**Glossary:**

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\varphi$	$\varphi$ rotation around probe axis
Polarization $\vartheta$	$\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Methods Applied and Interpretation of Parameters:**

- *NORM<sub>x,y,z</sub>*: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). *NORM<sub>x,y,z</sub>* are only intermediate values, i.e., the uncertainties of *NORM<sub>x,y,z</sub>* does not affect the  $E^2$ -field uncertainty inside TSL (see below *ConvF*).
- *NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- *DCP<sub>x,y,z</sub>*: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- *PAR*: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- *A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>; A, B, C, D* are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. *VR* is the maximum calibration range expressed in RMS voltage across the diode.
- *ConvF and Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to *NORM<sub>x,y,z</sub> \* ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- *Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- *Connector Angle*: The angle is assessed using the information gained by determining the *NORM<sub>x</sub>* (no uncertainty required).

# Probe ES3DV3

## SN:3168

Manufactured: October 8, 2008  
Calibrated: September 27, 2018

**Calibrated for DASY/EASY Systems**  
(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3168

### Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup>	1.12	1.05	1.00	$\pm 10.1\%$
DCP (mV) <sup>B</sup>	102.0	94.2	96.1	

### Modulation Calibration Parameters

UID	Communication System Name	A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc <sup>F</sup> (k=2)
0	CW	0.0	0.0	1.0	0.00	199.6	$\pm 3.5\%$
	X	0.0	0.0	1.0		183.0	
	Y	0.0	0.0	1.0		183.9	
	Z	0.0	0.0	1.0			

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X,Y Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>F</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3168

### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	41.9	0.89	6.60	6.60	6.60	0.64	1.36	± 12.0 %
850	41.5	0.92	6.35	6.35	6.35	0.67	1.30	± 12.0 %
1750	40.1	1.37	5.43	5.43	5.43	0.40	1.69	± 12.0 %
1900	40.0	1.40	5.20	5.20	5.20	0.69	1.32	± 12.0 %
2000	40.0	1.40	5.17	5.17	5.17	0.46	1.51	± 12.0 %
2300	39.5	1.67	5.05	5.05	5.05	0.69	1.23	± 12.0 %
2450	39.2	1.80	4.70	4.70	4.70	0.80	1.20	± 12.0 %
2600	39.0	1.96	4.57	4.57	4.57	0.80	1.23	± 12.0 %

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3168

### Calibration Parameter Determined in Body Tissue Simulating Media


f (MHz) <sup>c</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth <sup>g</sup> (mm)	Unc (k=2)
750	55.5	0.96	6.24	6.24	6.24	0.54	1.47	± 12.0 %
850	55.2	0.99	6.15	6.15	6.15	0.69	1.23	± 12.0 %
1750	53.4	1.49	5.02	5.02	5.02	0.31	2.48	± 12.0 %
1900	53.3	1.52	4.77	4.77	4.77	0.32	2.47	± 12.0 %
2300	52.9	1.81	4.71	4.71	4.71	0.68	1.30	± 12.0 %
2450	52.7	1.95	4.52	4.52	4.52	0.80	1.10	± 12.0 %
2600	52.5	2.16	4.36	4.36	4.36	0.55	1.20	± 12.0 %

<sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 7), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 78, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters  $\epsilon_r$  and  $\sigma$  can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon_r$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>g</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


### Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

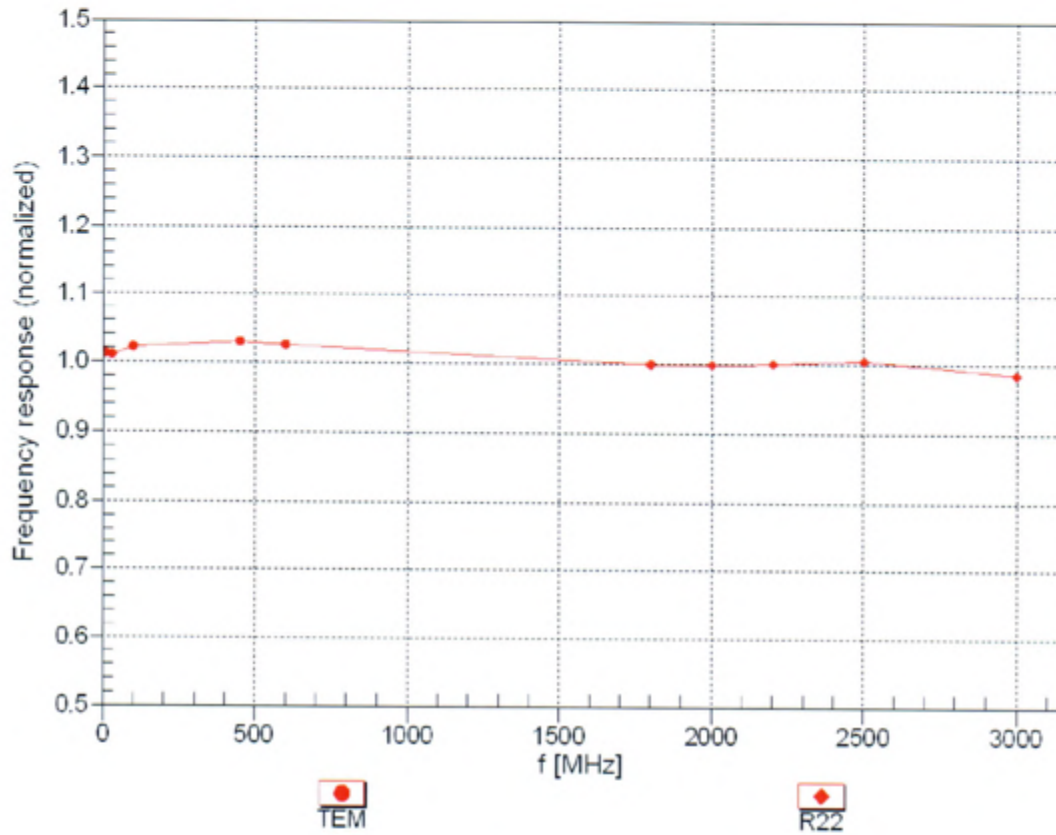



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)

### Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

f=600 MHz,TEM


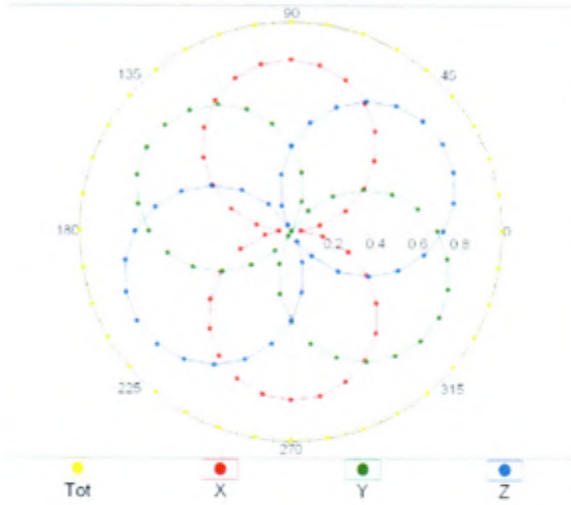


f=1800 MHz,R22

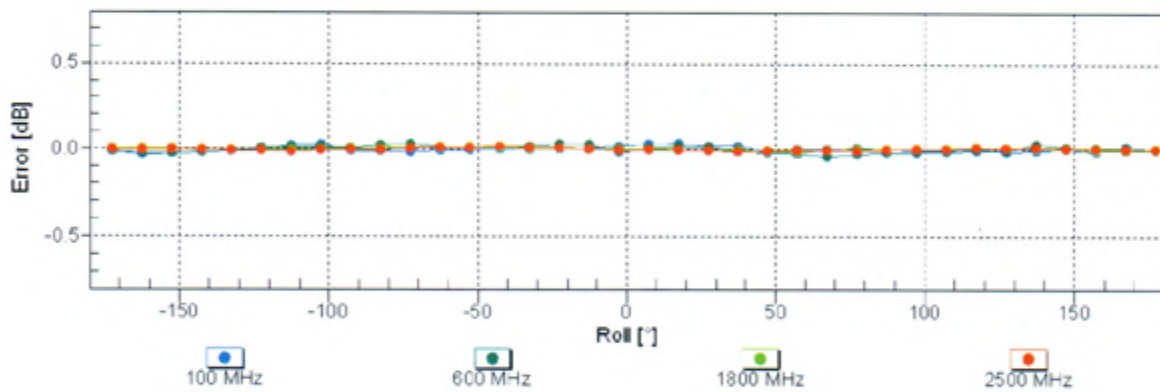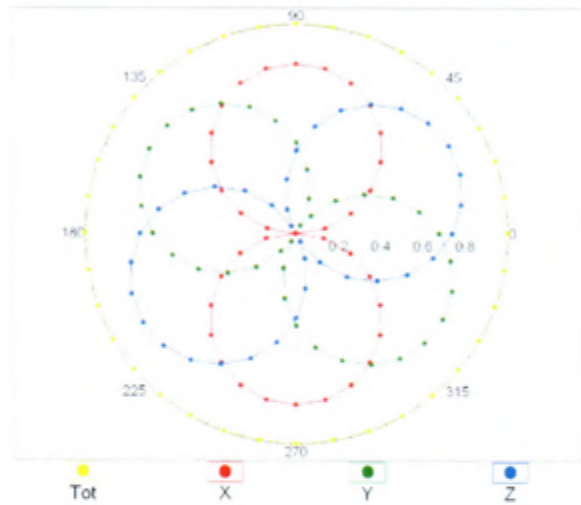

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  ( $k=2$ )


### Dynamic Range $f(SAR_{head})$ (TEM cell , $f_{eval} = 1900$ MHz)

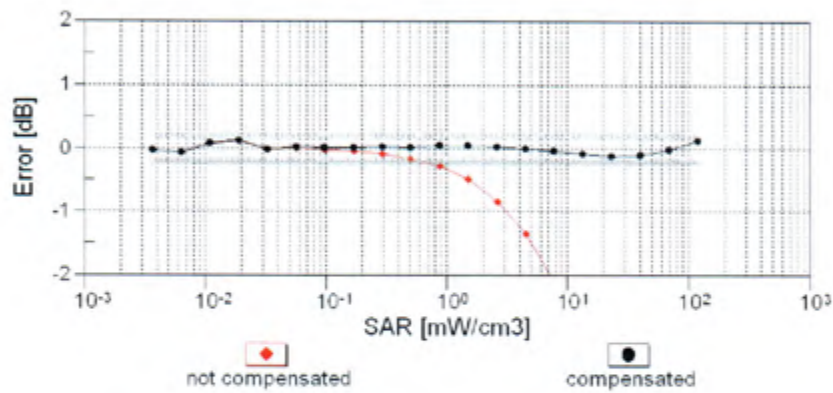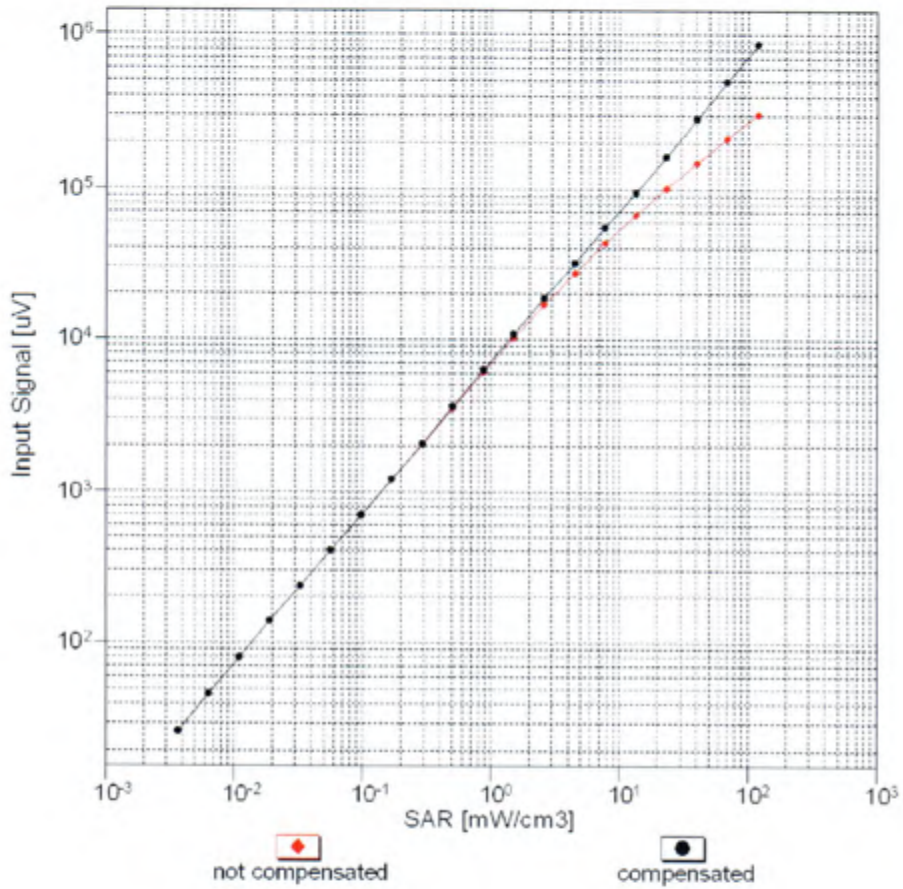


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  (k=2)



# Conversion Factor Assessment

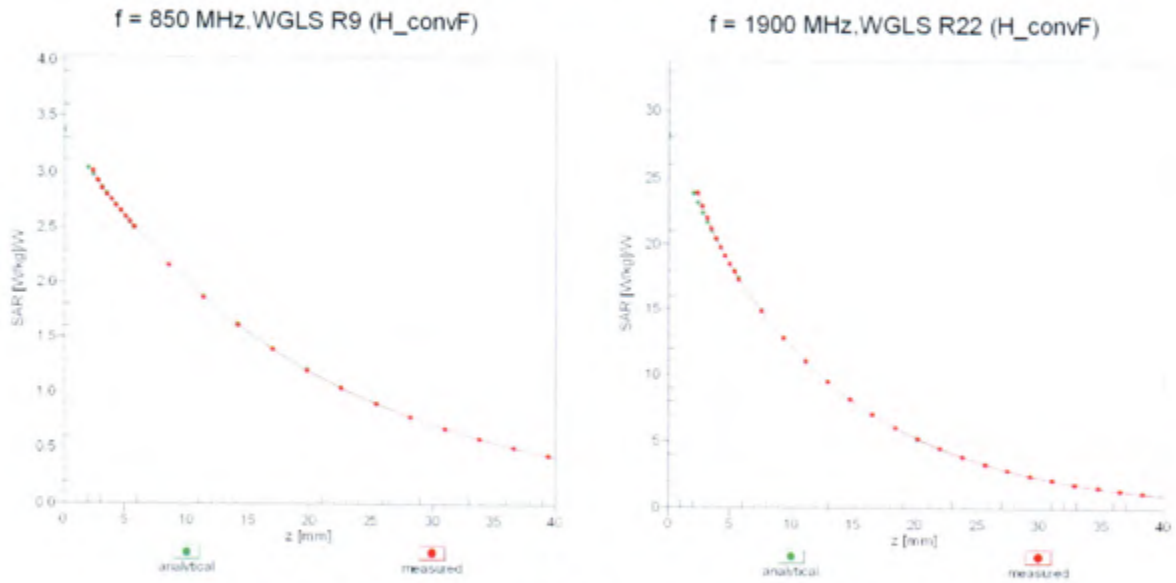

## Deviation from Isotropy in Liquid Error ( $\phi, \theta$ ), f = 900 MHz

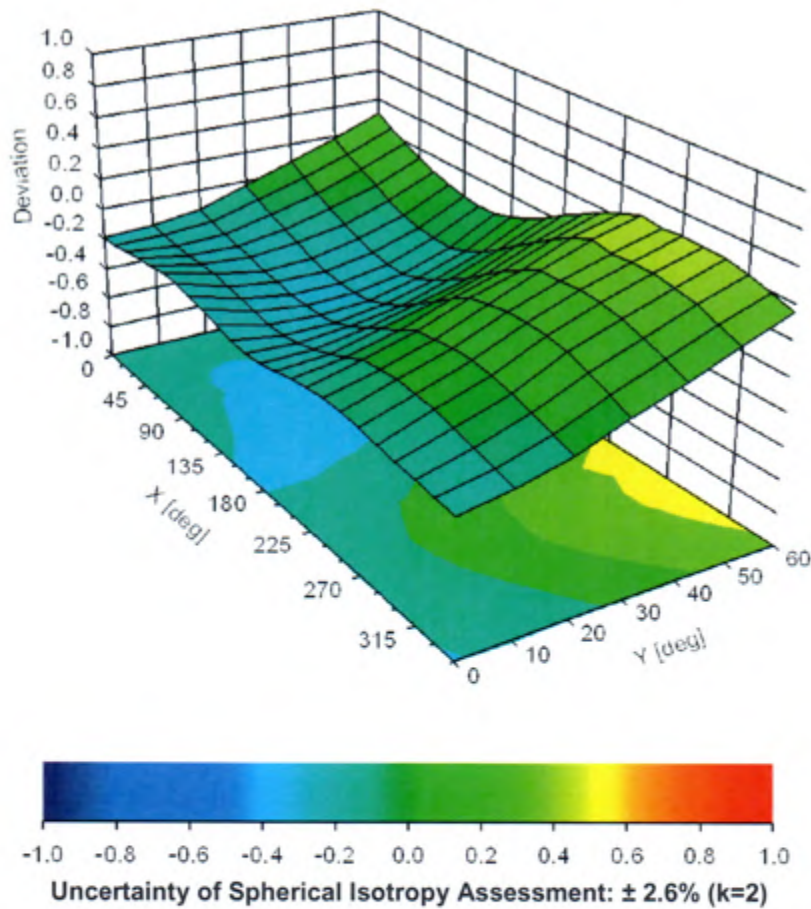

## DASY/EASY - Parameters of Probe: ES3DV3 - SN:3168

### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-42.6
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Huawei-SZ (Auden)**

Certificate No: **EX3-3743\_Nov18**

## CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3743**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-23.v5, QA CAL-25.v6  
Calibration procedure for dosimetric E-field probes**

Calibration date: **November 19, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-18 (No. 217-02682)	Apr-19
Reference Probe ES3DV2	SN: 3013	30-Dec-17 (No. ES3-3013_Dec17)	Dec-18
DAE4	SN: 660	21-Dec-17 (No. DAE4-660_Dec17)	Dec-18
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: November 22, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

### Glossary:

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\varphi$	$\varphi$ rotation around probe axis
Polarization $\vartheta$	$\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

### Methods Applied and Interpretation of Parameters:

- NORM<sub>x,y,z</sub>**: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). NORM<sub>x,y,z</sub> are only intermediate values, i.e., the uncertainties of NORM<sub>x,y,z</sub> does not affect the E<sup>2</sup>-field uncertainty inside TSL (see below ConvF).
- NORM(f)<sub>x,y,z</sub> = NORM<sub>x,y,z</sub> \* frequency\_response** (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP<sub>x,y,z</sub>**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A<sub>x,y,z</sub>; B<sub>x,y,z</sub>; C<sub>x,y,z</sub>; D<sub>x,y,z</sub>; VR<sub>x,y,z</sub>; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM<sub>x,y,z</sub> \* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM<sub>x</sub> (no uncertainty required).

# Probe EX3DV4

## SN:3743

Manufactured: March 26, 2010  
Calibrated: November 19, 2018

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3743

### Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup>	0.44	0.47	0.51	$\pm 10.1\%$
DCP (mV) <sup>B</sup>	105.7	102.0	96.4	

### Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc <sup>E</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	146.6	$\pm 2.7\%$
		Y	0.0	0.0	1.0		137.1	
		Z	0.0	0.0	1.0		143.4	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter; uncertainty not required

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3743

### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	41.9	0.89	9.77	9.77	9.77	0.49	0.80	± 12.0 %
850	41.5	0.92	9.41	9.41	9.41	0.34	1.01	± 12.0 %
1750	40.1	1.37	8.36	8.36	8.36	0.28	0.90	± 12.0 %
1900	40.0	1.40	7.87	7.87	7.87	0.29	0.88	± 12.0 %
2000	40.0	1.40	7.85	7.85	7.85	0.30	0.87	± 12.0 %
2300	39.5	1.67	7.50	7.50	7.50	0.28	0.90	± 12.0 %
2450	39.2	1.80	7.13	7.13	7.13	0.35	0.90	± 12.0 %
2600	39.0	1.96	6.96	6.96	6.96	0.38	0.90	± 12.0 %

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3743

### Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	55.5	0.96	9.65	9.65	9.85	0.39	1.00	± 12.0 %
850	55.2	0.99	9.45	9.45	9.45	0.42	0.92	± 12.0 %
1750	53.4	1.49	7.85	7.85	7.85	0.40	0.83	± 12.0 %
1900	53.3	1.52	7.52	7.52	7.52	0.36	0.95	± 12.0 %
2300	52.9	1.81	7.44	7.44	7.44	0.43	0.89	± 12.0 %
2450	52.7	1.95	7.33	7.33	7.33	0.41	0.93	± 12.0 %
2600	52.5	2.16	6.90	6.90	6.90	0.33	0.95	± 12.0 %


<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to + 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below + 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.




### Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

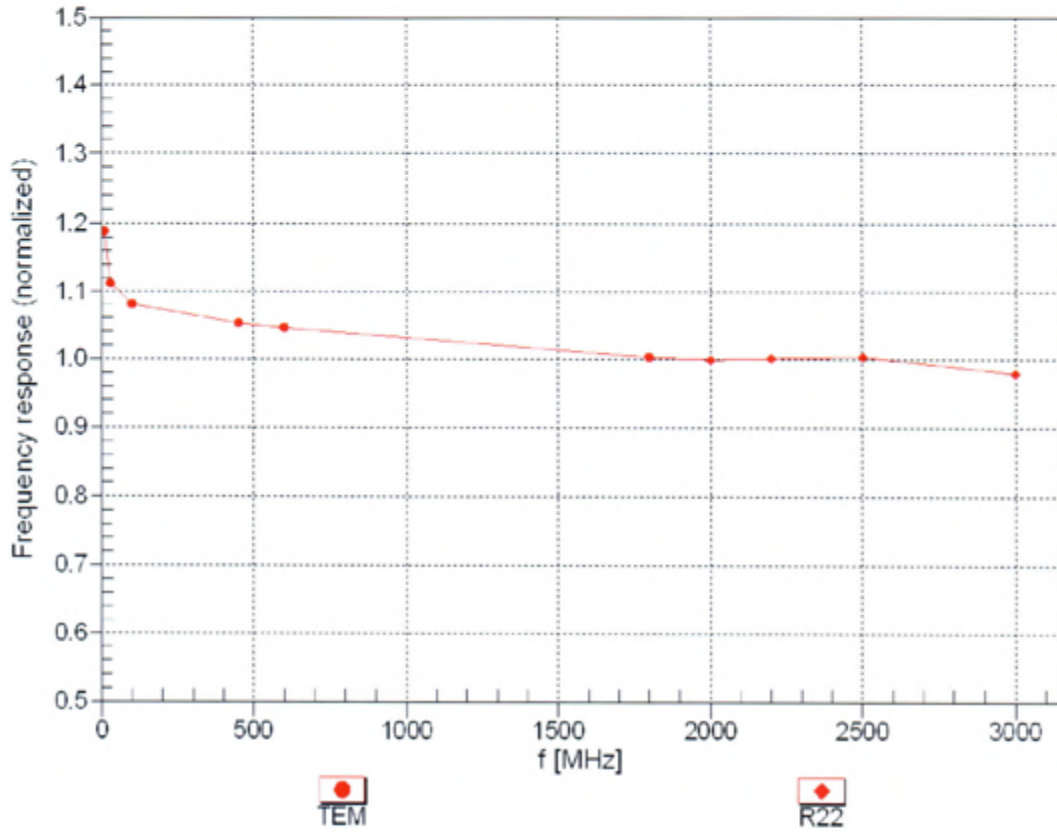



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)

### Receiving Pattern ( $\phi$ ), $\vartheta = 0^\circ$

f=600 MHz,TEM


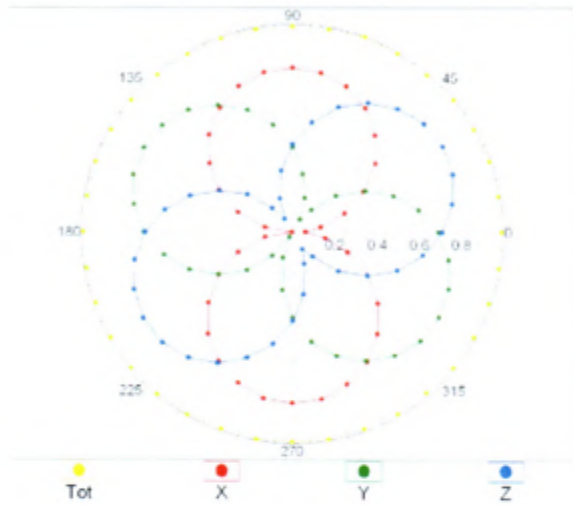


f=1800 MHz,R22

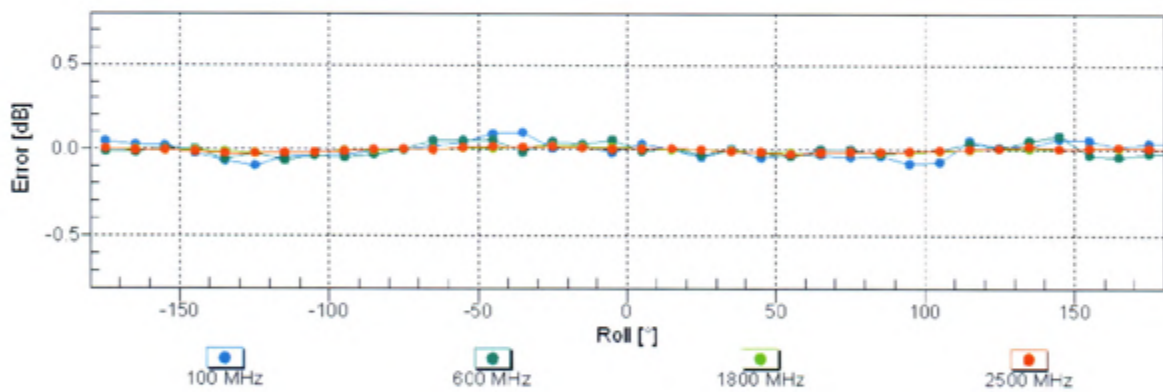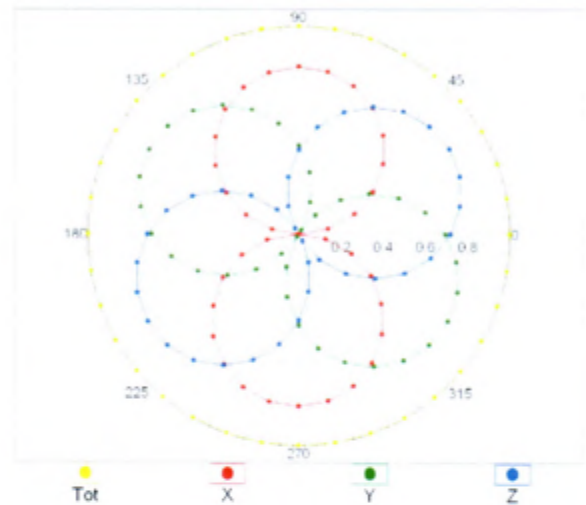


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)

### Dynamic Range $f(SAR_{head})$ (TEM cell , $f_{eval}= 1900$ MHz)

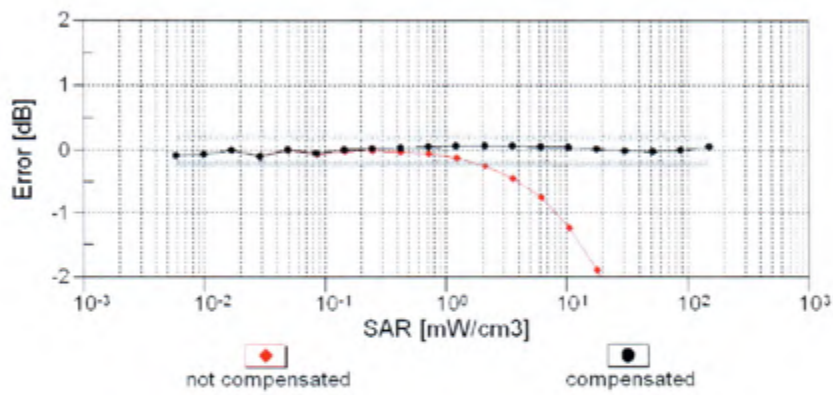
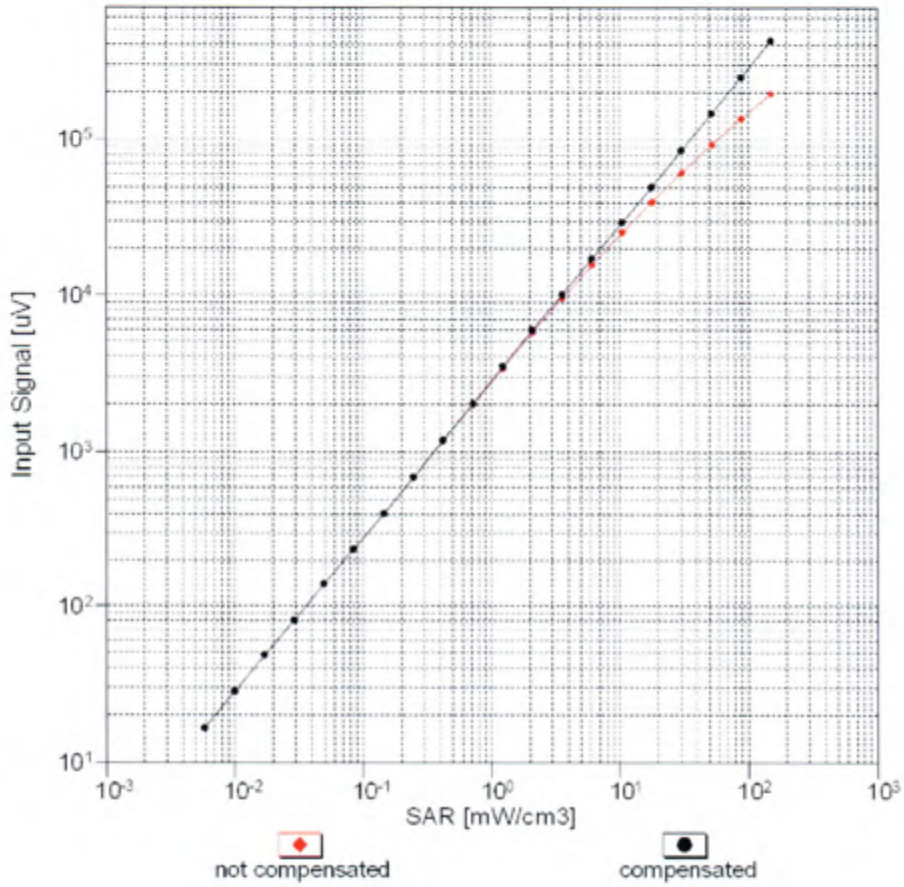


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  (k=2)

## Conversion Factor Assessment

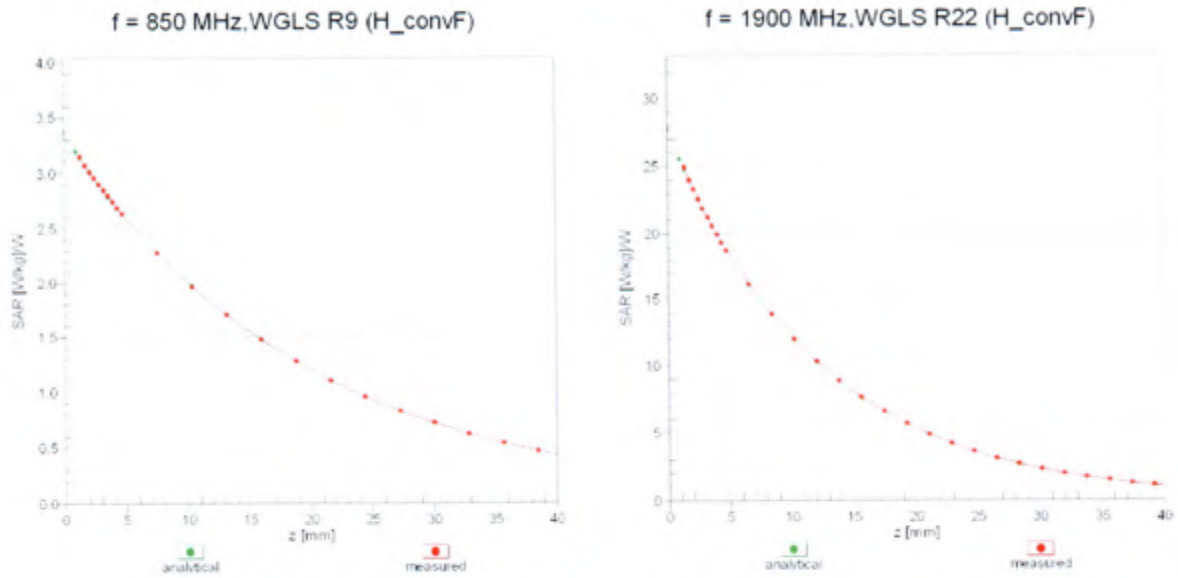

### Deviation from Isotropy in Liquid Error ( $\phi, \theta$ ), f = 900 MHz

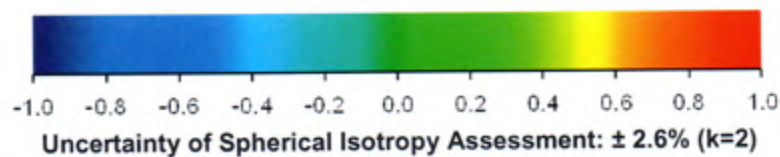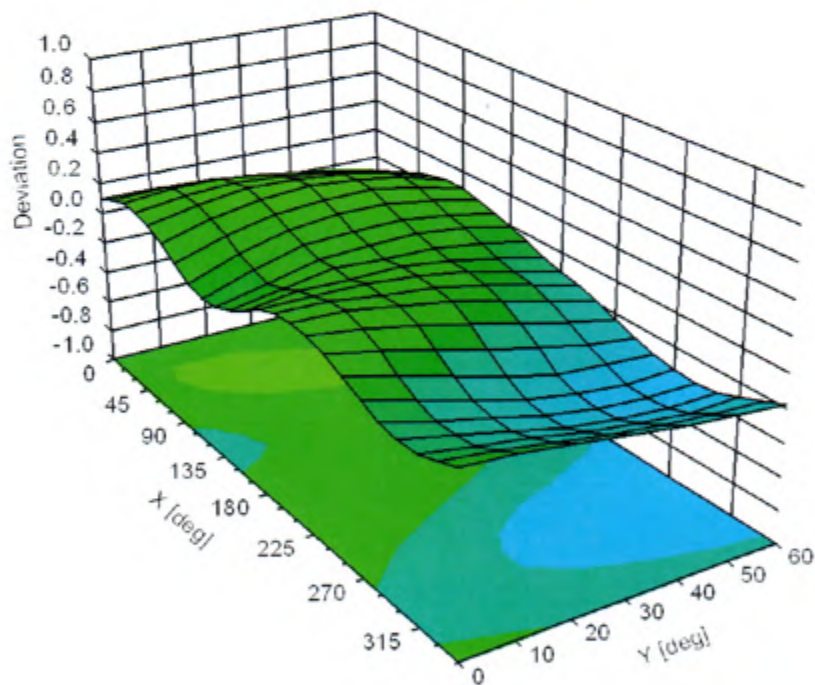

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3743

### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	75
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client: **Hisawal SZ (Aubien)**

Certificate No.: **EX3-3744 Jul18**

## CALIBRATION CERTIFICATE

Object: **EX3DV4 SSN:3744**

Calibration procedure(s): **QA CAL-01 v9, QA CAL-23 v5, QA CAL-25 v6**  
**Calibration procedure for dosimetric E-field probes**

Calibration date: **July 25, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration):

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-ZR1	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-ZR1	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-18 (No. 217-02682)	Apr-19
Reference Probe ESSDV2	SN: 3013	30-Dec-17 (No. ESS3-3013 Dec17)	Dec-18
DAF4	SN: 660	21-Dec-17 (No. DAF4-660 Dec17)	Dec-18
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter F4419B	SN: GB41295874	03-Apr-16 (in house check Jun-18)	In house check Jun-20
Power sensor F4412A	SN: MY41488367	03-Apr-16 (in house check Jun-18)	In house check Jun-20
Power sensor F4412A	SN: 000110210	03-Apr-16 (in house check Jun-18)	In house check Jun-20
RF generator HP 8048C	SN: US3842U01700	04-Aug-99 (in house check Jun-18)	In house check Jun-20
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-17)	In house check Oct-18

	Name	Function	Signature
Calibrated by:	Stefano Leudler	Laboratory Technician	
Approved by:	Karin P. Kohn	Technical Manager	

Issued: July 28, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: SCS 0108

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

### Glossary:

TSL	tissue simulating liquid
$NORM_{x,y,z}$	sensitivity in free space
$ConvF$	sensitivity in TSL / $NORM_{x,y,z}$
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\phi$	$\phi$ rotation around probe axis
Polarization $\theta$	$\theta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

### Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 5 GHz"

### Methods Applied and Interpretation of Parameters:

- $NORM_{x,y,z}$ : Assessed for E-field polarization  $\theta = 0$  ( $f \leq 800$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide).  $NORM_{x,y,z}$  are only intermediate values, i.e., the uncertainties of  $NORM_{x,y,z}$  does not affect the  $E^2$ -field uncertainty inside TSL (see below  $ConvF$ ).
- $NORM(f)_{x,y,z} = NORM_{x,y,z} \cdot frequency\_response$  (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of  $ConvF$ .
- $DCP_{x,y,z}$ : DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- $A_{x,y,z}$ ;  $B_{x,y,z}$ ;  $C_{x,y,z}$ ;  $D_{x,y,z}$ ;  $VR_{x,y,z}$ ; A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- $ConvF$  and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to  $NORM_{x,y,z} \cdot ConvF$  whereby the uncertainty corresponds to that given for  $ConvF$ . A frequency dependent  $ConvF$  is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the  $NORM_{x,y,z}$  (no uncertainty required).

# Probe EX3DV4

## SN:3744

Manufactured: March 26, 2010  
Calibrated: July 25, 2018

Calibrated for DASY/EASY Systems  
(Note: non-compatible with DASY2 system!)



## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3744

### Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>4</sup>	0.47	0.48	0.40	$\pm 10.1 \%$
DCP ( $\text{mV}$ ) <sup>5</sup>	97.6	99.6	113.8	

### Modulation Calibration Parameters

UID	Communication System Name		A	B	C	D	VR	Unc (k=2)
			dB	dB $\sqrt{\mu\text{V}}$		dB	mV	
0	CW	X	0.0	0.0	1.0	0.00	156.2	$\pm 3.0 \%$
		Y	0.0	0.0	1.0		156.0	
		Z	0.0	0.0	1.0		170.2	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>4</sup> The uncertainties of Norm X,Y,Z do not affect the E<sup>2</sup>-field uncertainty inside TSL (see Pages 5 and 6).

<sup>1</sup> Numerical linearization parameter; uncertainty not required.

<sup>5</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3744

### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>G</sup> (mm)	Unc (k=2)
750	41.8	0.89	9.40	9.40	9.40	0.54	0.80	± 12.0 %
850	41.5	0.92	8.96	8.96	8.96	0.49	0.84	± 12.0 %
1750	40.1	1.37	8.27	8.27	8.27	0.10	1.12	± 12.0 %
1900	40.0	1.40	7.99	7.99	7.99	0.10	0.83	± 12.0 %
2000	40.0	1.40	7.78	7.78	7.78	0.10	0.80	± 12.0 %
2300	39.5	1.57	7.74	7.74	7.74	0.30	0.90	± 12.0 %
2450	39.2	1.60	7.24	7.24	7.24	0.30	0.95	± 12.0 %
2600	39.0	1.96	6.90	6.90	6.90	0.30	0.95	± 12.0 %

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 50, 64, 128, 160 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 100 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon'$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon'$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPLAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:3744

### Calibration Parameter Determined in Body Tissue Simulating Media


f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>E</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth <sup>H</sup> (mm)	Unc (k=2)
750	55.5	0.95	9.54	9.54	9.54	0.49	0.80	± 12.0 %
850	55.2	0.99	9.12	9.12	9.12	0.53	0.80	± 12.0 %
1750	53.4	1.40	7.74	7.74	7.74	0.45	0.80	± 12.0 %
1900	53.3	1.52	7.60	7.60	7.60	0.40	0.84	± 12.0 %
2300	52.9	1.81	7.56	7.56	7.56	0.45	0.85	± 12.0 %
2450	52.7	1.95	7.39	7.39	7.39	0.35	0.85	± 12.0 %
2600	52.5	2.16	7.35	7.35	7.35	0.30	0.99	± 12.0 %

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), so it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 100 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>H</sup> Alpha/Depth are determined during calibration. SPFAC warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


## Frequency Response of E-Field (TEM-Cell: ifi110 EXX, Waveguide: R22)

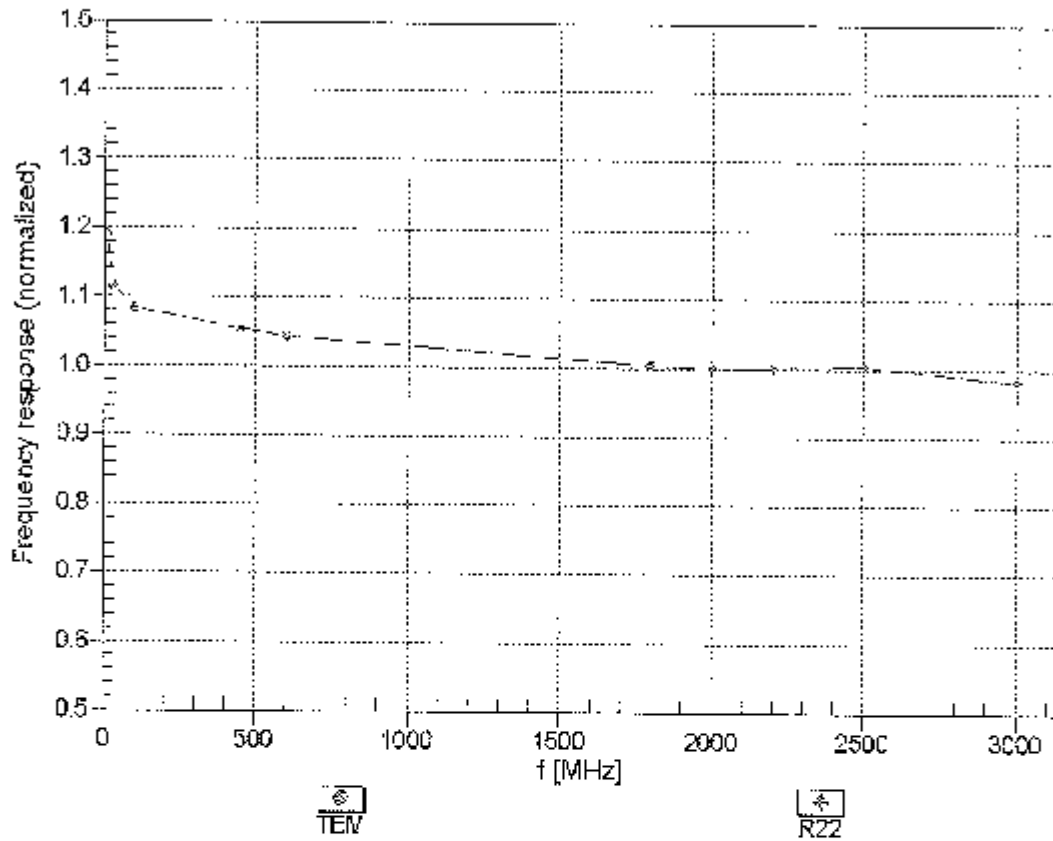



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  ( $k=2$ )

### Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

f=600 MHz,TEM


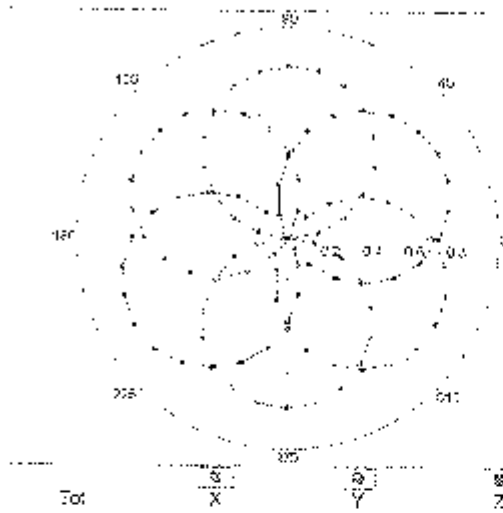


f=1800 MHz,R22

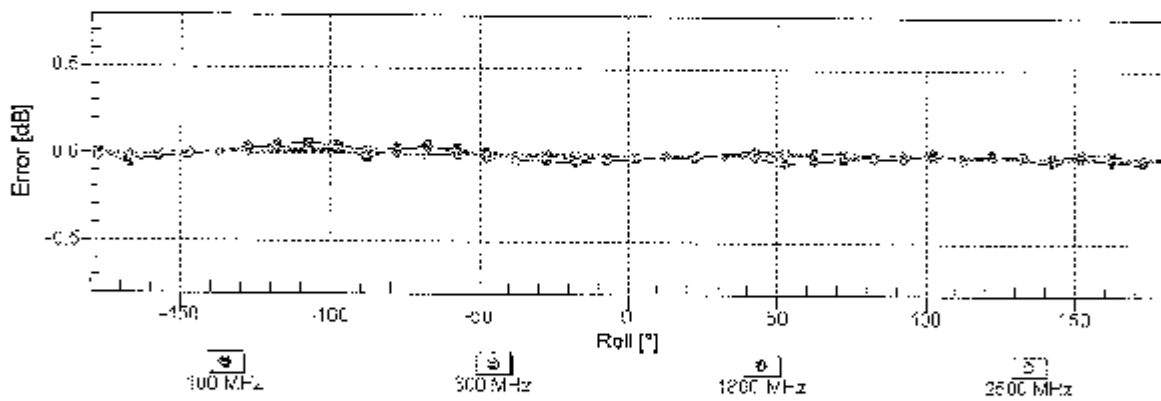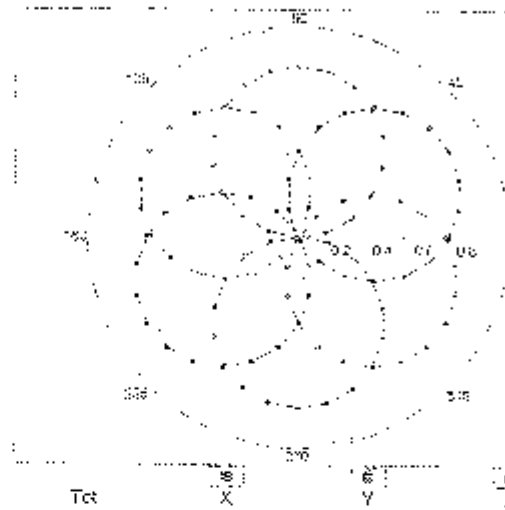


Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)

### Dynamic Range $f(SAR_{head})$ (TEM cell, $f_{eval} = 1900$ MHz)

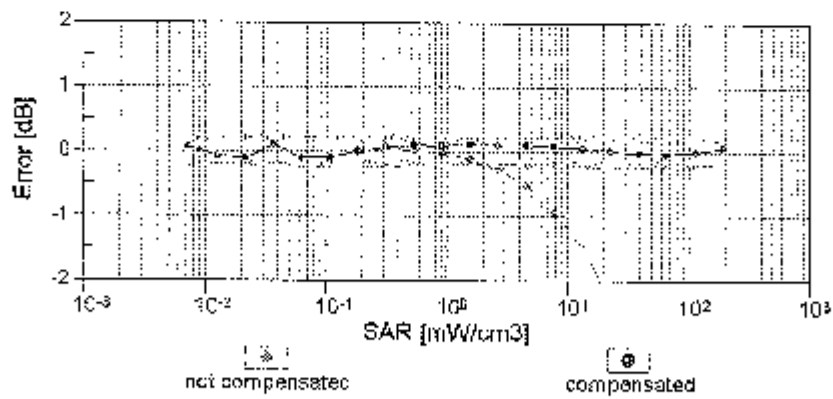
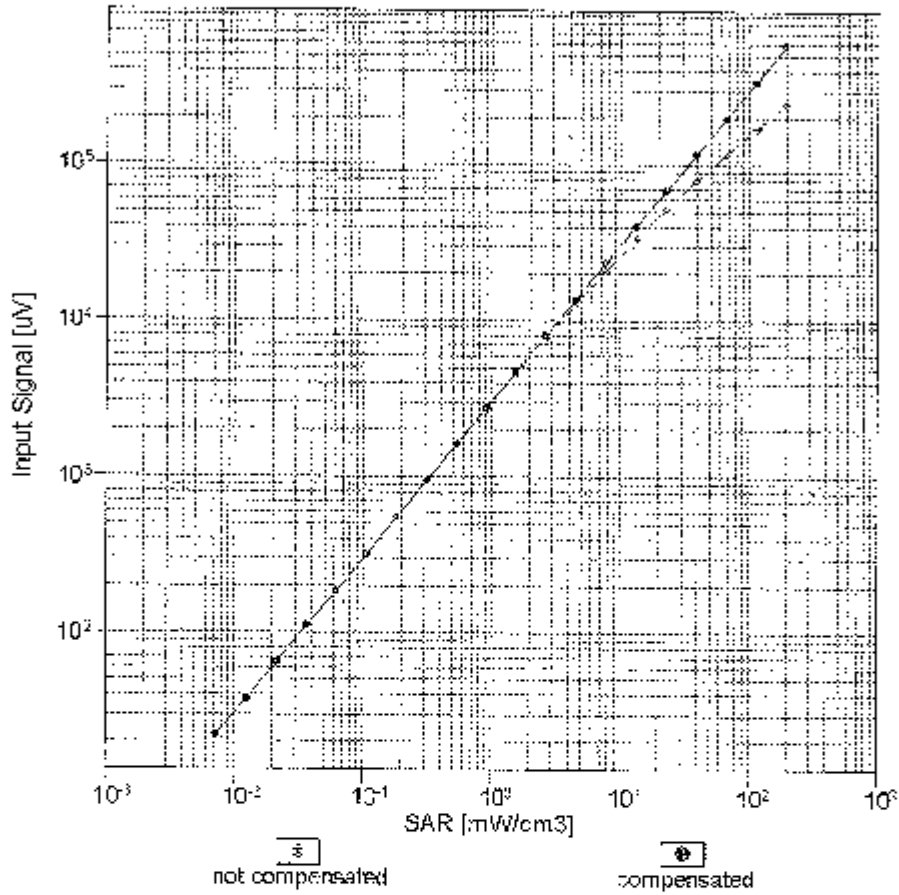


Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )

### Conversion Factor Assessment

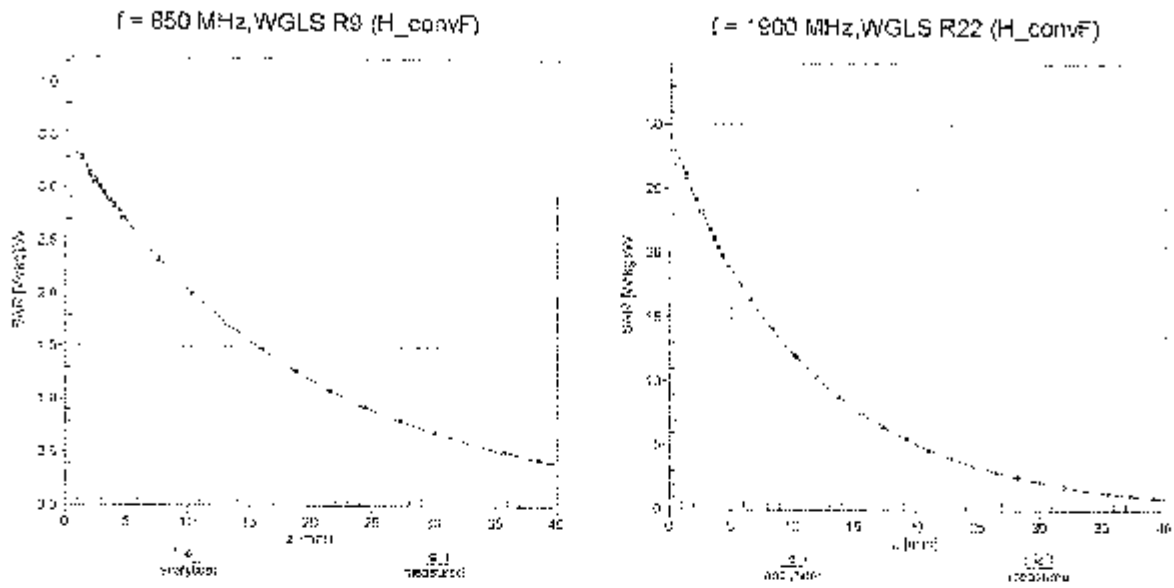

### Deviation from Isotropy in Liquid Error ( $\phi, \theta$ ), f = 900 MHz

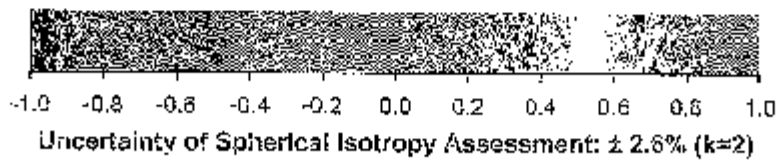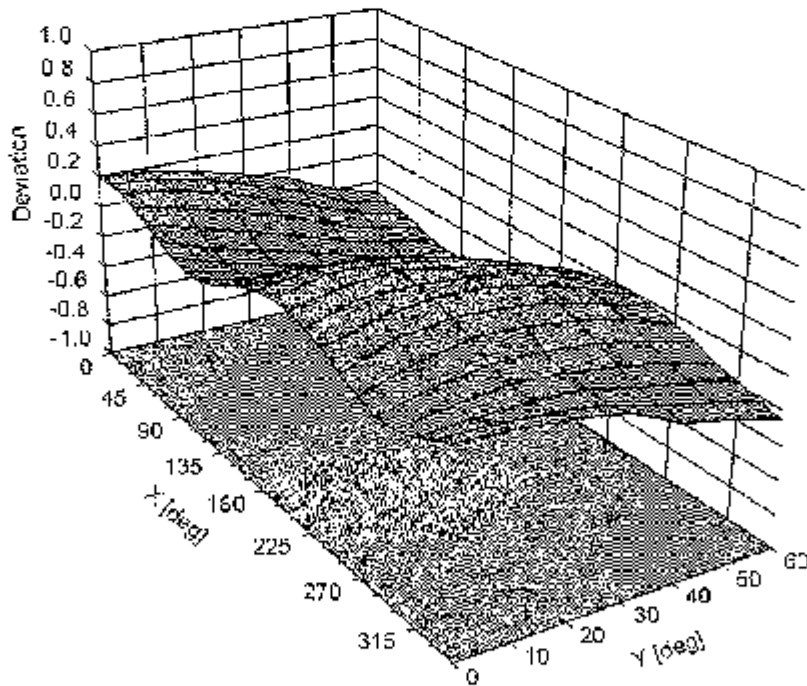

**DASY/EASY - Parameters of Probe: EX3DV4 - SN:3744****Other Probe Parameters**

Sensor Arrangement	Triangular
Connector Angle (°)	72.5
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm





Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Client **Huawei-SZ (Auden)**

Certificate No: **EX3-7381\_Sep18**

## CALIBRATION CERTIFICATE

Object: **EX3DV4 - SN:7381**

Calibration procedure(s): **QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6  
Calibration procedure for dosimetric E-field probes**

Calibration date: **September 28, 2018**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: S5277 (20x)	04-Apr-18 (No. 217-02682)	Apr-19
Reference Probe ES3DV2	SN: 3013	30-Dec-17 (No. ES3-3013_Dec17)	Dec-18
DAE4	SN: 660	21-Dec-17 (No. DAE4-660_Dec17)	Dec-18
Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41293874	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: MY41498087	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
Power sensor E4412A	SN: 000110210	06-Apr-16 (in house check Jun-18)	In house check: Jun-20
RF generator HP 8648C	SN: US3642U01700	04-Aug-99 (in house check Jun-18)	In house check: Jun-20
Network Analyzer E8358A	SN: US41080477	31-Mar-14 (in house check Oct-17)	In house check: Oct-18

Calibrated by:	Name <b>Michael Weber</b>	Function <b>Laboratory Technician</b>	Signature 
Approved by:	Name <b>Katja Pokovic</b>	Function <b>Technical Manager</b>	Signature 
			Issued: September 29, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

**Glossary:**

TSL	tissue simulating liquid
NORM <sub>x,y,z</sub>	sensitivity in free space
ConvF	sensitivity in TSL / NORM <sub>x,y,z</sub>
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization $\varphi$	$\varphi$ rotation around probe axis
Polarization $\vartheta$	$\vartheta$ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Methods Applied and Interpretation of Parameters:**

- *NORM<sub>x,y,z</sub>*: Assessed for E-field polarization  $\vartheta = 0$  ( $f \leq 900$  MHz in TEM-cell;  $f > 1800$  MHz: R22 waveguide). *NORM<sub>x,y,z</sub>* are only intermediate values, i.e., the uncertainties of *NORM<sub>x,y,z</sub>* does not affect the  $E^2$ -field uncertainty inside TSL (see below *ConvF*).
- *NORM(f)<sub>x,y,z</sub>* = *NORM<sub>x,y,z</sub>* \* *frequency\_response* (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of *ConvF*.
- *DCP<sub>x,y,z</sub>*: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- *PAR*: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- *A<sub>x,y,z</sub>*; *B<sub>x,y,z</sub>*; *C<sub>x,y,z</sub>*; *D<sub>x,y,z</sub>*; *VR<sub>x,y,z</sub>*; *A, B, C, D* are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. *VR* is the maximum calibration range expressed in RMS voltage across the diode.
- *ConvF* and *Boundary Effect Parameters*: Assessed in flat phantom using E-field (or Temperature Transfer Standard for  $f \leq 800$  MHz) and inside waveguide using analytical field distributions based on power measurements for  $f > 800$  MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to *NORM<sub>x,y,z</sub>* \* *ConvF* whereby the uncertainty corresponds to that given for *ConvF*. A frequency dependent *ConvF* is used in DASY version 4.4 and higher which allows extending the validity from  $\pm 50$  MHz to  $\pm 100$  MHz.
- *Spherical isotropy (3D deviation from isotropy)*: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- *Sensor Offset*: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- *Connector Angle*: The angle is assessed using the information gained by determining the *NORM<sub>x</sub>* (no uncertainty required).

# Probe EX3DV4

## SN:7381

Manufactured:	April 13, 2015
Repaired:	September 20, 2018
Calibrated:	September 28, 2018

**Calibrated for DASY/EASY Systems**  
(Note: non-compatible with DASY2 system!)

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:7381

### Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) <sup>A</sup>	0.64	0.53	0.36	$\pm 10.1\%$
DCP (mV) <sup>B</sup>	95.1	93.1	95.0	

### Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc <sup>C</sup> (k=2)
0	CW	X	0.0	0.0	1.0	0.00	182.9	$\pm 3.0\%$
		Y	0.0	0.0	1.0		190.3	
		Z	0.0	0.0	1.0		178.1	

Note: For details on UID parameters see Appendix.

### Sensor Model Parameters

	C1 fF	C2 fF	$\alpha$ V <sup>-1</sup>	T1 ms.V <sup>-2</sup>	T2 ms.V <sup>-1</sup>	T3 ms	T4 V <sup>-2</sup>	T5 V <sup>-1</sup>	T6
X	35.70	266.3	35.57	9.330	0.900	5.00	0.100	0.005	1.020
Y	40.50	334.6	44.32	5.164	0.417	5.10	0.100	0.600	1.014
Z	52.87	417.1	39.84	7.817	0.237	5.10	0.291	0.427	1.011

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>A</sup> The uncertainties of Norm X,Y,Z do not affect the  $E^2$ -field uncertainty inside TSL (see Pages 5 and 6).

<sup>B</sup> Numerical linearization parameter: uncertainty not required.

<sup>C</sup> Uncertainty is determined using the maximum deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:7381

### Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) <sup>c</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>g</sup>	Depth (mm) <sup>g</sup>	Unc (k=2)
750	41.9	0.89	10.66	10.66	10.66	0.40	0.92	± 12.0 %
850	41.5	0.92	10.30	10.30	10.30	0.34	0.98	± 12.0 %
1750	40.1	1.37	8.79	8.79	8.79	0.38	0.84	± 12.0 %
1900	40.0	1.40	8.32	8.32	8.32	0.34	0.87	± 12.0 %
2000	40.0	1.40	8.15	8.15	8.15	0.34	0.85	± 12.0 %
2300	39.5	1.67	7.95	7.95	7.95	0.35	0.90	± 12.0 %
2450	39.2	1.80	7.61	7.61	7.61	0.25	1.18	± 12.0 %
2600	39.0	1.96	7.35	7.35	7.35	0.29	1.15	± 12.0 %
5250	35.9	4.71	5.67	5.67	5.67	0.40	1.80	± 13.1 %
5600	35.6	5.07	5.04	5.04	5.04	0.40	1.80	± 13.1 %
5800	35.3	5.27	5.23	5.23	5.23	0.40	1.80	± 13.1 %

<sup>c</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>g</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:7381

### Calibration Parameter Determined in Body Tissue Simulating Media


f (MHz) <sup>C</sup>	Relative Permittivity <sup>F</sup>	Conductivity (S/m) <sup>F</sup>	ConvF X	ConvF Y	ConvF Z	Alpha <sup>G</sup>	Depth (mm) <sup>G</sup>	Unc (k=2)
750	55.5	0.96	10.74	10.74	10.74	0.24	1.24	± 12.0 %
850	55.2	0.99	10.46	10.46	10.46	0.25	1.17	± 12.0 %
1750	53.4	1.49	8.61	8.61	8.61	0.27	1.03	± 12.0 %
1900	53.3	1.52	8.22	8.22	8.22	0.31	0.95	± 12.0 %
2300	52.9	1.81	8.03	8.03	8.03	0.36	0.93	± 12.0 %
2450	52.7	1.95	7.76	7.76	7.76	0.41	0.90	± 12.0 %
2600	52.5	2.16	7.53	7.53	7.53	0.42	0.88	± 12.0 %
5250	48.9	5.36	4.75	4.75	4.75	0.50	1.90	± 13.1 %
5600	48.5	5.77	4.26	4.26	4.26	0.50	1.90	± 13.1 %
5750	48.3	5.94	4.37	4.37	4.37	0.50	1.90	± 13.1 %

<sup>C</sup> Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), also it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

<sup>F</sup> At frequencies below 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters ( $\epsilon$  and  $\sigma$ ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

<sup>G</sup> Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


### Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

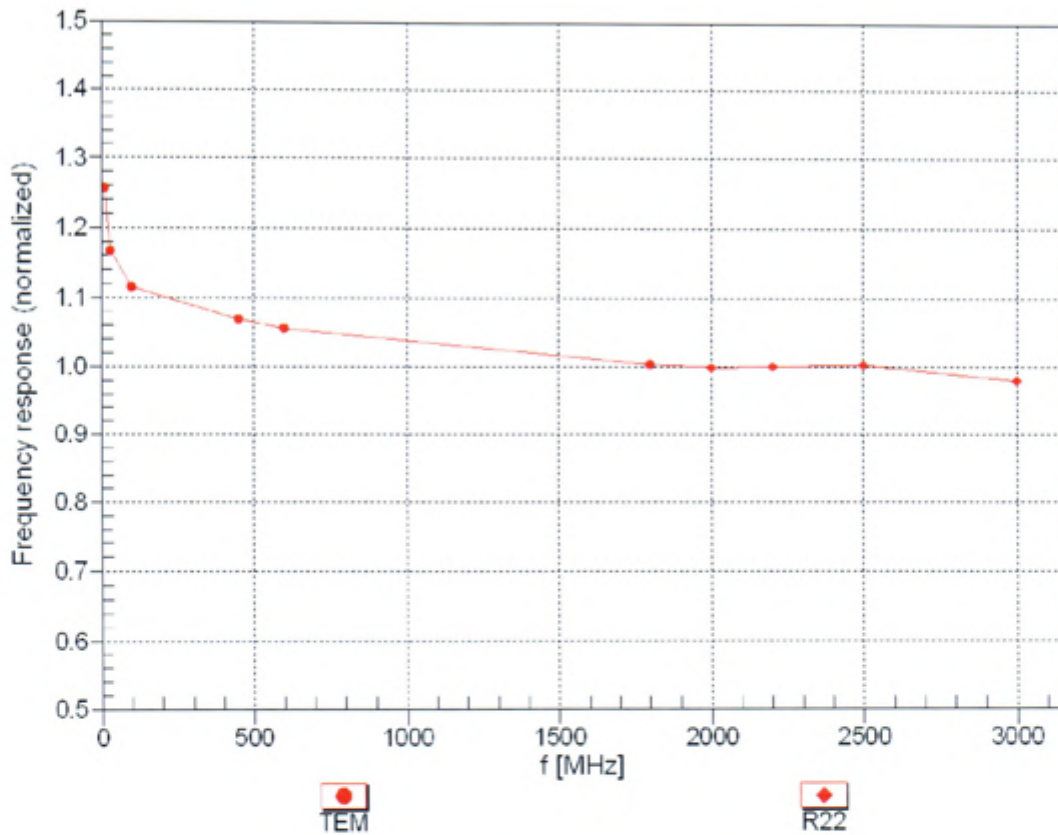



Uncertainty of Frequency Response of E-field:  $\pm 6.3\%$  (k=2)

### Receiving Pattern ( $\phi$ ), $\theta = 0^\circ$

f=600 MHz,TEM

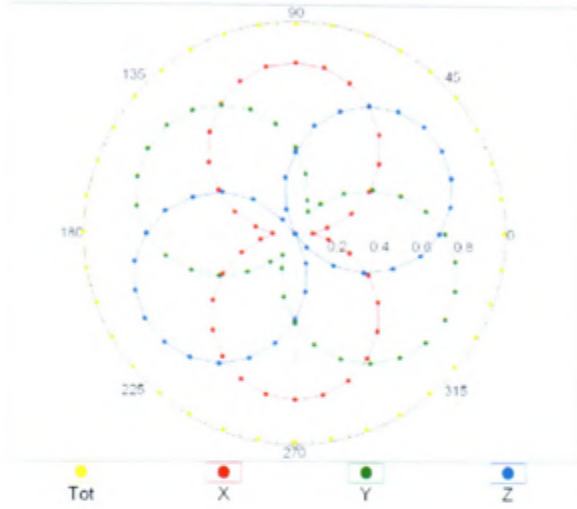



f=1800 MHz,R22

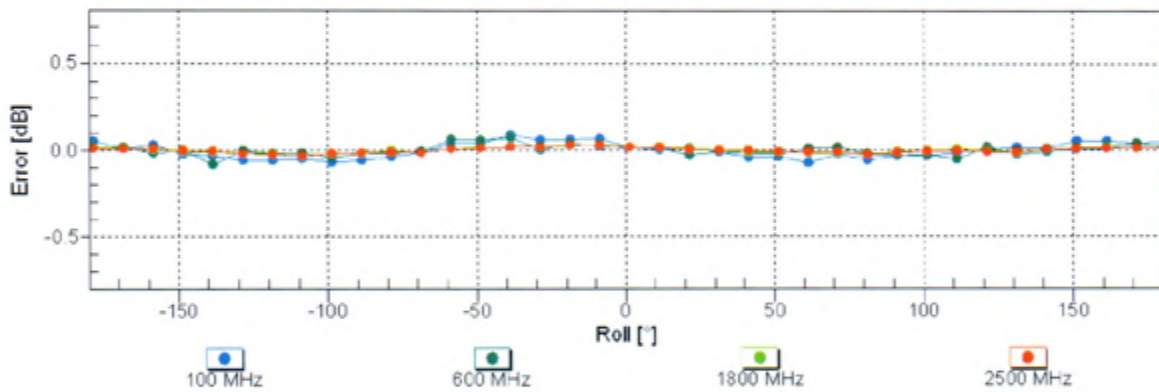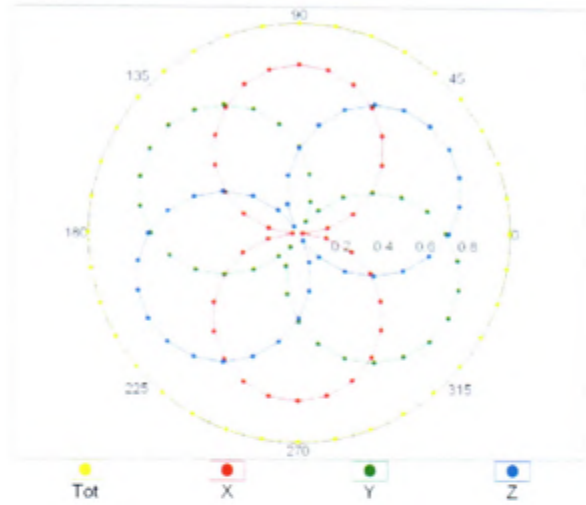

Uncertainty of Axial Isotropy Assessment:  $\pm 0.5\%$  (k=2)




## Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell , $f_{\text{eval}} = 1900 \text{ MHz}$ )

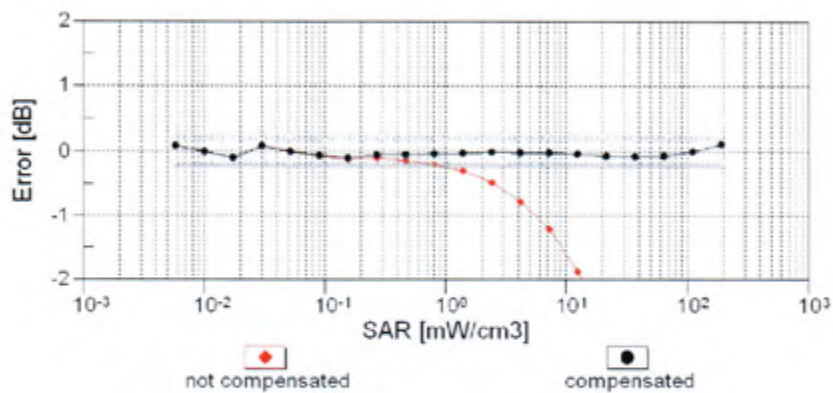
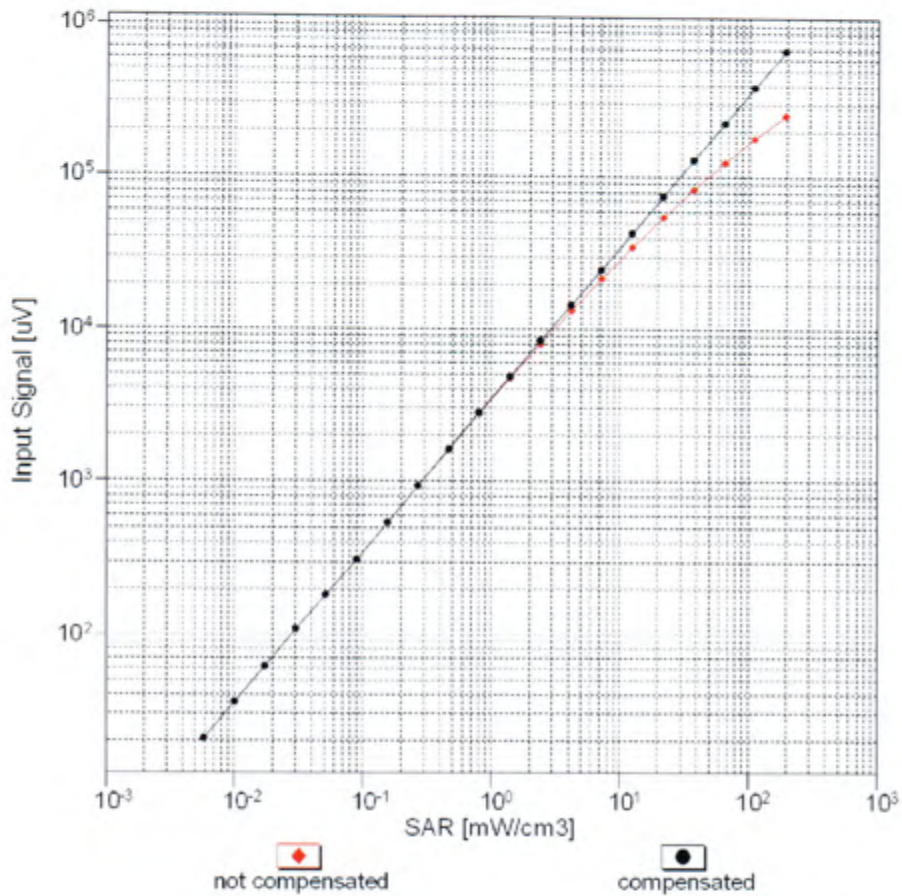


**Uncertainty of Linearity Assessment:  $\pm 0.6\%$  ( $k=2$ )**

# Conversion Factor Assessment

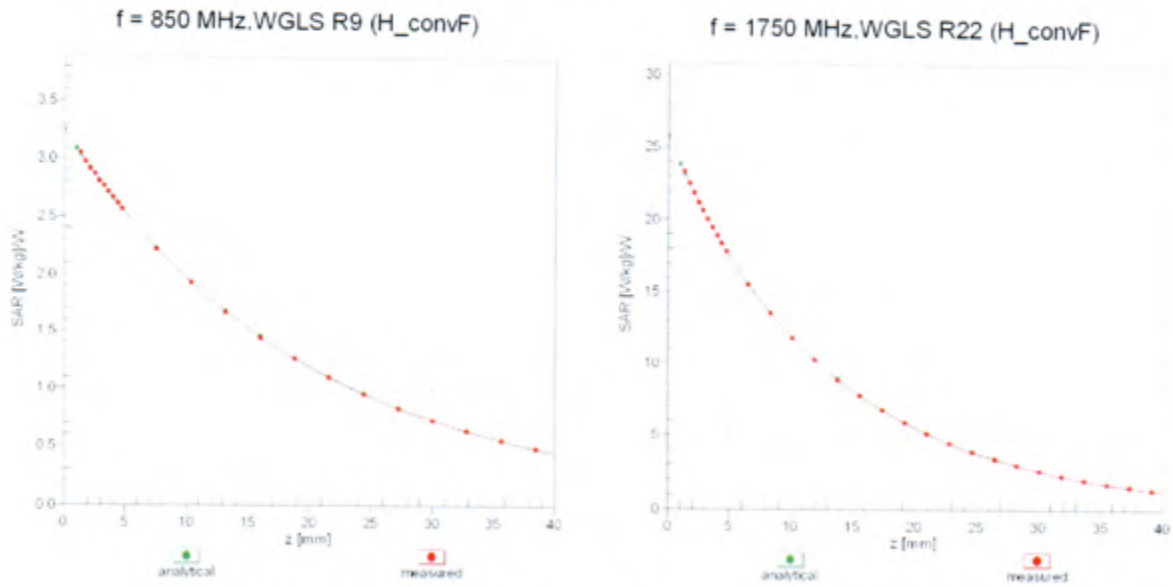

## Deviation from Isotropy in Liquid Error ( $\phi, \theta$ ), f = 900 MHz

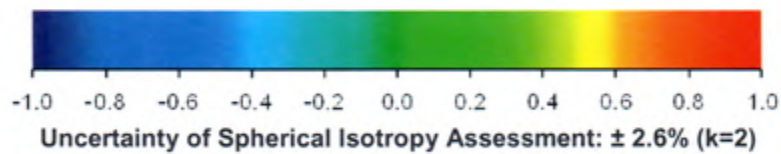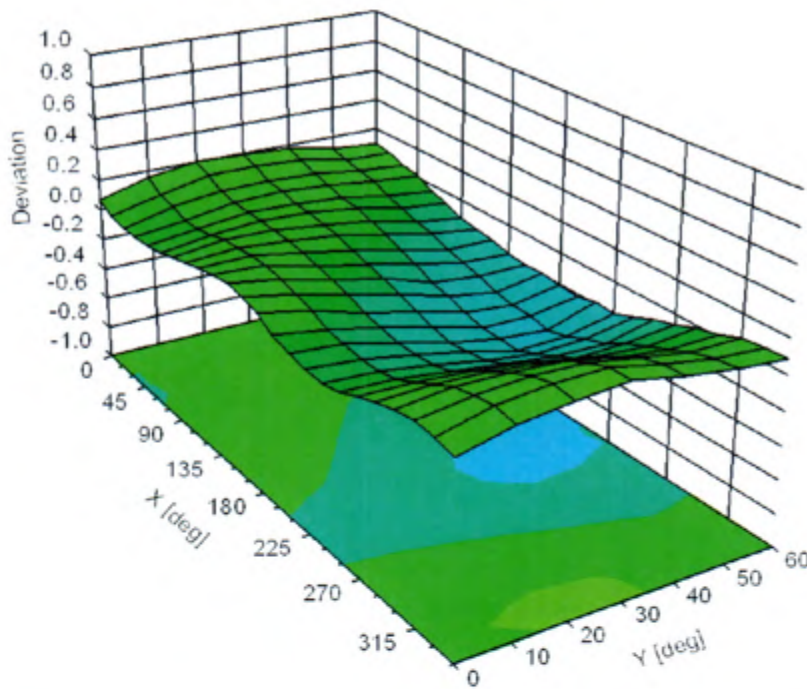

## DASY/EASY - Parameters of Probe: EX3DV4 - SN:7381

### Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	131.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

**Appendix: Modulation Calibration Parameters**

UID	Communication System Name		A dB	B dB $\sqrt{\mu}$ V	C	D dB	VR mV	Max Unc <sup>E</sup> (k=2)
0	CW	X	0.00	0.00	1.00	0.00	182.9	$\pm 3.0\%$
		Y	0.00	0.00	1.00		190.3	
		Z	0.00	0.00	1.00		176.1	
10010- CAA	SAR Validation (Square, 100ms, 10ms)	X	11.00	70.00	30.00	10.00	20.0	$\pm 9.6\%$
		Y	1.35	61.38	6.83		20.0	
		Z	1.92	65.21	9.46		20.0	
10011- CAB	UMTS-FDD (WCDMA)	X	1.15	67.14	15.68	0.00	150.0	$\pm 9.6\%$
		Y	100.00	216.99	69.51		150.0	
		Z	13.47	117.54	34.62		150.0	
10012- CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	X	1.32	63.81	15.29	0.41	150.0	$\pm 9.6\%$
		Y	8.14	128.56	47.42		150.0	
		Z	1.30	68.66	19.76		150.0	
10013- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps)	X	4.87	66.86	17.13	1.46	150.0	$\pm 9.6\%$
		Y	5.04	69.28	20.04		150.0	
		Z	4.98	67.22	18.07		150.0	
10021- DAC	GSM-FDD (TDMA, GMSK)	X	100.00	118.25	30.34	9.39	50.0	$\pm 9.6\%$
		Y	100.00	110.03	24.78		50.0	
		Z	100.00	115.56	27.47		50.0	
10023- DAC	GPRS-FDD (TDMA, GMSK, TN 0)	X	100.00	117.75	30.17	9.57	50.0	$\pm 9.6\%$
		Y	100.00	109.01	24.39		50.0	
		Z	100.00	114.64	27.11		50.0	
10024- DAC	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	100.00	120.69	30.13	6.56	60.0	$\pm 9.6\%$
		Y	100.00	126.91	30.65		60.0	
		Z	100.00	125.28	30.48		60.0	
10025- DAC	EDGE-FDD (TDMA, 8PSK, TN 0)	X	24.11	122.63	48.01	12.57	50.0	$\pm 9.6\%$
		Y	4.60	78.41	33.03		50.0	
		Z	4.28	74.19	30.01		50.0	
10026- DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1)	X	9.91	93.59	33.79	9.56	60.0	$\pm 9.6\%$
		Y	18.52	123.39	47.38		60.0	
		Z	9.47	98.14	37.01		60.0	
10027- DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	X	100.00	125.06	31.17	4.80	80.0	$\pm 9.6\%$
		Y	100.00	479.59	170.55		80.0	
		Z	100.00	147.30	38.75		80.0	
10028- DAC	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	X	100.00	130.95	32.97	3.55	100.0	$\pm 9.6\%$
		Y	0.12	60.00	30.00		100.0	
		Z	100.00	195.98	57.32		100.0	
10029- DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2)	X	5.53	79.72	27.05	7.80	80.0	$\pm 9.6\%$
		Y	6.59	94.20	36.35		80.0	
		Z	5.37	83.49	30.07		80.0	
10030- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH1)	X	100.00	120.91	29.62	5.30	70.0	$\pm 9.6\%$
		Y	100.00	196.62	58.60		70.0	
		Z	100.00	130.24	32.03		70.0	
10031- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH3)	X	100.00	139.36	35.10	1.88	100.0	$\pm 9.6\%$
		Y	0.07	60.00	30.00		100.0	
		Z	99.99	150.00	30.00		100.0	

10032-CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	X	97.94	152.13	39.63	1.17	100.0	± 9.6 %
		Y	0.06	60.00	30.00		100.0	
		Z	0.05	60.00	30.00		100.0	
10033-CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH1)	X	7.66	86.59	22.86	5.30	70.0	± 9.6 %
		Y	100.00	149.72	43.17		70.0	
		Z	100.00	144.67	41.53		70.0	
10034-CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH3)	X	2.79	75.44	17.50	1.88	100.0	± 9.6 %
		Y	100.00	170.78	50.20		100.0	
		Z	100.00	143.95	39.60		100.0	
10035-CAA	IEEE 802.15.1 Bluetooth (PI/4-DQPSK, DH5)	X	2.09	72.81	16.27	1.17	100.0	± 9.6 %
		Y	100.00	180.10	53.53		100.0	
		Z	100.00	143.34	38.92		100.0	
10036-CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH1)	X	9.07	89.46	23.88	5.30	70.0	± 9.6 %
		Y	100.00	150.95	43.71		70.0	
		Z	100.00	145.42	41.88		70.0	
10037-CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH3)	X	2.56	74.36	17.07	1.88	100.0	± 9.6 %
		Y	100.00	172.04	50.66		100.0	
		Z	100.00	144.18	39.64		100.0	
10038-CAA	IEEE 802.15.1 Bluetooth (8-DPSK, DH5)	X	2.07	72.81	16.39	1.17	100.0	± 9.6 %
		Y	100.00	183.38	54.93		100.0	
		Z	100.00	144.60	39.47		100.0	
10039-CAB	CDMA2000 (1xRTT, RC1)	X	1.85	72.59	15.95	0.00	150.0	± 9.6 %
		Y	100.00	175.27	51.06		150.0	
		Z	100.00	134.81	35.14		150.0	
10042-CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Halfrate)	X	100.00	117.39	29.00	7.78	50.0	± 9.6 %
		Y	100.00	104.70	21.46		50.0	
		Z	100.00	112.98	25.44		50.0	
10044-CAA	IS-91/EIA/TIA-553 FDD (FDMA, FM)	X	0.13	60.00	15.99	0.00	150.0	± 9.6 %
		Y	0.00	60.00	0.00		150.0	
		Z	0.00	128.20	45.27		150.0	
10048-CAA	DECT (TDD, TDMA/FDM, GFSK, Full Slot, 24)	X	28.69	95.37	25.31	13.80	25.0	± 9.6 %
		Y	100.00	103.96	23.93		25.0	
		Z	100.00	108.81	26.14		25.0	
10049-CAA	DECT (TDD, TDMA/FDM, GFSK, Double Slot, 12)	X	67.71	110.77	28.63	10.79	40.0	± 9.6 %
		Y	100.00	106.44	23.68		40.0	
		Z	260.43	123.05	28.63		40.0	
10056-CAA	UMTS-TDD (TD-SCDMA, 1.28 Mcps)	X	23.23	98.98	27.11	9.03	50.0	± 9.6 %
		Y	100.00	126.19	33.96		50.0	
		Z	100.00	130.47	36.35		50.0	
10058-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-1-2-3)	X	4.23	74.26	23.86	6.55	100.0	± 9.6 %
		Y	4.66	85.66	32.29		100.0	
		Z	4.14	77.76	26.79		100.0	
10059-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps)	X	1.34	64.54	15.70	0.61	110.0	± 9.6 %
		Y	100.00	203.81	66.88		110.0	
		Z	1.40	71.11	21.17		110.0	
10060-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps)	X	2.40	81.52	22.07	1.30	110.0	± 9.6 %
		Y	100.00	335.12	116.68		110.0	
		Z	100.00	175.52	51.30		110.0	

10061-CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps)	X	2.14	73.59	19.82	2.04	110.0	± 9.6 %
		Y	100.00	209.14	68.58		110.0	
		Z	100.00	164.99	49.53		110.0	
10062-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps)	X	4.67	66.83	16.58	0.49	100.0	± 9.6 %
		Y	4.94	69.77	19.74		100.0	
		Z	4.83	67.37	17.56		100.0	
10063-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps)	X	4.68	66.91	16.66	0.72	100.0	± 9.6 %
		Y	4.97	69.94	19.88		100.0	
		Z	4.84	67.48	17.68		100.0	
10064-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps)	X	4.92	67.11	16.86	0.86	100.0	± 9.6 %
		Y	5.20	69.91	19.90		100.0	
		Z	5.15	67.73	17.88		100.0	
10065-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps)	X	4.80	66.96	16.93	1.21	100.0	± 9.6 %
		Y	5.05	69.80	20.06		100.0	
		Z	5.00	67.63	18.00		100.0	
10066-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps)	X	4.81	66.96	17.07	1.46	100.0	± 9.6 %
		Y	5.03	69.72	20.18		100.0	
		Z	5.01	67.62	18.17		100.0	
10067-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps)	X	5.11	67.25	17.56	2.04	100.0	± 9.6 %
		Y	5.28	69.64	20.42		100.0	
		Z	5.27	67.63	18.52		100.0	
10068-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps)	X	5.15	67.19	17.73	2.55	100.0	± 9.6 %
		Y	5.27	69.40	20.50		100.0	
		Z	5.32	67.71	18.76		100.0	
10069-CAC	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps)	X	5.22	67.25	17.93	2.67	100.0	± 9.6 %
		Y	5.32	69.35	20.65		100.0	
		Z	5.39	67.63	18.91		100.0	
10071-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 9 Mbps)	X	4.97	66.94	17.42	1.99	100.0	± 9.6 %
		Y	5.09	69.17	20.23		100.0	
		Z	5.06	67.25	18.35		100.0	
10072-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 12 Mbps)	X	4.93	67.18	17.61	2.30	100.0	± 9.6 %
		Y	5.09	69.69	20.59		100.0	
		Z	5.05	67.65	18.62		100.0	
10073-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 18 Mbps)	X	5.01	67.39	17.95	2.83	100.0	± 9.6 %
		Y	5.13	69.81	20.90		100.0	
		Z	5.08	67.74	18.93		100.0	
10074-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 24 Mbps)	X	5.03	67.37	18.12	3.30	100.0	± 9.6 %
		Y	5.08	69.54	20.94		100.0	
		Z	5.03	67.52	19.03		100.0	
10075-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 36 Mbps)	X	5.07	67.44	18.41	3.82	90.0	± 9.6 %
		Y	5.07	69.45	21.15		90.0	
		Z	5.05	67.62	19.36		90.0	
10076-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 48 Mbps)	X	5.12	67.36	18.60	4.15	90.0	± 9.6 %
		Y	5.05	69.03	21.16		90.0	
		Z	5.02	67.23	19.38		90.0	
10077-CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS/OFDM, 54 Mbps)	X	5.15	67.48	18.73	4.30	90.0	± 9.6 %
		Y	5.08	69.11	21.25		90.0	
		Z	5.04	67.26	19.46		90.0	

10081-CAB	CDMA2000 (1xRTT, RC3)	X	0.98	67.39	13.56	0.00	150.0	± 9.6 %
		Y	100.00	268.60	86.44		150.0	
		Z	100.00	140.60	36.25		150.0	
10082-CAB	IS-54 / IS-136 FDD (TDMA/FDM, PI/4-DQPSK, Fullrate)	X	0.96	61.09	6.58	4.77	80.0	± 9.6 %
		Y	0.08	145.72	12.60		80.0	
		Z	2.70	64.54	4.89		80.0	
10090-DAC	GPRS-FDD (TDMA, GMSK, TN 0-4)	X	100.00	120.61	30.11	6.56	60.0	± 9.6 %
		Y	100.00	127.43	30.91		60.0	
		Z	100.00	125.37	30.55		60.0	
10097-CAB	UMTS-FDD (HSDPA)	X	1.96	68.20	16.00	0.00	150.0	± 9.6 %
		Y	100.00	158.98	47.61		150.0	
		Z	2.97	77.93	21.56		150.0	
10098-CAB	UMTS-FDD (HSUPA, Subtest 2)	X	1.93	68.14	15.98	0.00	150.0	± 9.6 %
		Y	100.00	160.08	48.01		150.0	
		Z	2.95	78.23	21.69		150.0	
10099-DAC	EDGE-FDD (TDMA, 8PSK, TN 0-4)	X	9.97	93.70	33.82	9.56	60.0	± 9.6 %
		Y	18.92	123.97	47.55		60.0	
		Z	9.57	98.41	37.10		60.0	
10100-CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	3.10	69.89	16.90	0.00	150.0	± 9.6 %
		Y	100.00	142.36	42.01		150.0	
		Z	4.57	77.73	20.76		150.0	
10101-CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X	3.27	67.42	16.09	0.00	150.0	± 9.6 %
		Y	5.41	81.04	24.37		150.0	
		Z	3.67	70.29	18.08		150.0	
10102-CAE	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	X	3.37	67.42	16.17	0.00	150.0	± 9.6 %
		Y	5.17	79.39	23.76		150.0	
		Z	3.74	70.00	18.04		150.0	
10103-CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.34	75.72	20.70	3.98	65.0	± 9.6 %
		Y	11.34	93.43	29.74		65.0	
		Z	6.86	79.59	23.23		65.0	
10104-CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM)	X	6.17	73.27	20.31	3.98	65.0	± 9.6 %
		Y	6.54	79.22	25.10		65.0	
		Z	5.98	74.59	21.93		65.0	
10105-CAG	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM)	X	6.14	73.03	20.50	3.98	65.0	± 9.6 %
		Y	6.17	77.48	24.57		65.0	
		Z	5.62	73.01	21.49		65.0	
10108-CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	2.70	69.19	16.71	0.00	150.0	± 9.6 %
		Y	100.00	147.33	43.88		150.0	
		Z	4.03	77.32	20.88		150.0	
10109-CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	2.91	67.36	15.96	0.00	150.0	± 9.6 %
		Y	7.00	89.30	27.63		150.0	
		Z	3.38	70.77	18.36		150.0	
10110-CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	2.20	68.47	16.29	0.00	150.0	± 9.6 %
		Y	100.00	154.17	46.09		150.0	
		Z	3.51	77.96	21.32		150.0	
10111-CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	2.63	68.40	16.20	0.00	150.0	± 9.6 %
		Y	100.00	146.51	43.54		150.0	
		Z	3.37	73.66	19.68		150.0	

10112-CAG	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	X	3.04	67.42	16.03	0.00	150.0	± 9.6 %
		Y	6.33	86.22	26.47		150.0	
		Z	3.47	70.42	18.24		150.0	
10113-CAG	LTE-FDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	X	2.77	68.55	16.31	0.00	150.0	± 9.6 %
		Y	100.00	145.16	43.16		150.0	
		Z	3.48	73.29	19.55		150.0	
10114-CAC	IEEE 802.11n (HT Greenfield, 13.5 Mbps, BPSK)	X	5.13	67.26	16.58	0.00	150.0	± 9.6 %
		Y	5.49	70.06	19.49		150.0	
		Z	5.32	67.96	17.43		150.0	
10115-CAC	IEEE 802.11n (HT Greenfield, 81 Mbps, 16-QAM)	X	5.38	67.34	16.61	0.00	150.0	± 9.6 %
		Y	5.80	70.16	19.48		150.0	
		Z	5.63	68.08	17.48		150.0	
10116-CAC	IEEE 802.11n (HT Greenfield, 135 Mbps, 64-QAM)	X	5.21	67.45	16.60	0.00	150.0	± 9.6 %
		Y	5.64	70.43	19.57		150.0	
		Z	5.45	68.24	17.49		150.0	
10117-CAC	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	5.12	67.21	16.57	0.00	150.0	± 9.6 %
		Y	5.47	69.94	19.45		150.0	
		Z	5.28	67.79	17.36		150.0	
10118-CAC	IEEE 802.11n (HT Mixed, 81 Mbps, 16-QAM)	X	5.45	67.52	16.71	0.00	150.0	± 9.6 %
		Y	6.03	70.88	19.83		150.0	
		Z	5.79	68.53	17.71		150.0	
10119-CAC	IEEE 802.11n (HT Mixed, 135 Mbps, 64-QAM)	X	5.21	67.44	16.61	0.00	150.0	± 9.6 %
		Y	5.72	70.73	19.73		150.0	
		Z	5.43	68.21	17.49		150.0	
10140-CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	3.39	67.46	16.10	0.00	150.0	± 9.6 %
		Y	5.27	79.54	23.68		150.0	
		Z	3.78	69.96	17.93		150.0	
10141-CAE	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	X	3.52	67.59	16.26	0.00	150.0	± 9.6 %
		Y	5.20	78.65	23.40		150.0	
		Z	3.88	69.88	18.01		150.0	
10142-CAE	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X	1.98	68.60	15.86	0.00	150.0	± 9.6 %
		Y	100.00	156.00	46.00		150.0	
		Z	3.90	81.59	22.46		150.0	
10143-CAE	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	2.47	69.21	15.74	0.00	150.0	± 9.6 %
		Y	100.00	143.49	41.14		150.0	
		Z	3.95	77.99	20.86		150.0	
10144-CAE	LTE-FDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	X	2.20	66.71	13.99	0.00	150.0	± 9.6 %
		Y	100.00	137.29	38.21		150.0	
		Z	3.05	72.40	17.90		150.0	
10145-CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	1.17	64.72	11.17	0.00	150.0	± 9.6 %
		Y	100.00	137.82	35.15		150.0	
		Z	14.17	100.72	25.63		150.0	
10146-CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	9.35	88.35	20.34	0.00	150.0	± 9.6 %
		Y	100.00	121.34	29.35		150.0	
		Z	100.00	120.70	29.90		150.0	
10147-CAF	LTE-FDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	X	100.00	118.16	28.11	0.00	150.0	± 9.6 %
		Y	100.00	123.93	30.58		150.0	
		Z	100.00	122.09	30.61		150.0	



10149-CAE	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	2.92	67.41	16.01	0.00	150.0	± 9.6 %
		Y	7.11	89.66	27.79		150.0	
		Z	3.39	70.87	18.42		150.0	
10150-CAE	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	X	3.04	67.47	16.07	0.00	150.0	± 9.6 %
		Y	6.40	86.49	26.60		150.0	
		Z	3.48	70.50	18.29		150.0	
10151-CAG	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	6.38	77.45	21.42	3.98	65.0	± 9.6 %
		Y	30.78	118.12	37.83		65.0	
		Z	7.72	84.02	25.22		65.0	
10152-CAG	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM)	X	5.68	73.18	19.88	3.98	65.0	± 9.6 %
		Y	6.90	82.70	26.24		65.0	
		Z	5.64	75.17	21.99		65.0	
10153-CAG	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM)	X	6.05	74.13	20.62	3.98	65.0	± 9.6 %
		Y	7.36	83.86	27.11		65.0	
		Z	5.95	75.97	22.70		65.0	
10154-CAG	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	2.23	68.75	16.47	0.00	150.0	± 9.6 %
		Y	100.00	154.70	46.35		150.0	
		Z	3.72	79.10	21.86		150.0	
10155-CAG	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	X	2.64	68.43	16.23	0.00	150.0	± 9.6 %
		Y	100.00	146.60	43.58		150.0	
		Z	3.37	73.67	19.69		150.0	
10156-CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	1.81	68.60	15.53	0.00	150.0	± 9.6 %
		Y	100.00	158.65	46.50		150.0	
		Z	4.86	86.74	24.11		150.0	
10157-CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	2.04	67.24	13.96	0.00	150.0	± 9.6 %
		Y	100.00	138.28	38.00		150.0	
		Z	3.49	76.44	19.40		150.0	
10158-CAG	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	X	2.78	68.62	16.36	0.00	150.0	± 9.6 %
		Y	100.00	145.31	43.23		150.0	
		Z	3.50	73.41	19.62		150.0	
10159-CAG	LTE-FDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	X	2.12	67.57	14.15	0.00	150.0	± 9.6 %
		Y	100.00	138.27	38.10		150.0	
		Z	3.75	77.32	19.82		150.0	
10160-CAE	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	2.75	68.61	16.52	0.00	150.0	± 9.6 %
		Y	100.00	145.25	43.24		150.0	
		Z	3.71	74.81	20.04		150.0	
10161-CAE	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	X	2.93	67.45	15.96	0.00	150.0	± 9.6 %
		Y	7.41	90.31	27.93		150.0	
		Z	3.39	70.63	18.34		150.0	
10162-CAE	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	X	3.04	67.65	16.09	0.00	150.0	± 9.6 %
		Y	7.27	89.25	27.52		150.0	
		Z	3.49	70.61	18.35		150.0	
10166-CAF	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	X	3.25	68.78	19.90	3.01	150.0	± 9.6 %
		Y	5.76	85.66	29.21		150.0	
		Z	3.95	72.47	21.60		150.0	
10167-CAF	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	3.43	70.84	20.33	3.01	150.0	± 9.6 %
		Y	13.83	102.81	33.84		150.0	
		Z	5.17	76.77	22.54		150.0	

10168-CAF	LTE-FDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM)	X	3.73	72.85	21.65	3.01	150.0	± 9.6 %
		Y	29.00	120.66	39.75		150.0	
		Z	6.02	80.26	24.36		150.0	
10169-CAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	2.39	65.72	18.67	3.01	150.0	± 9.6 %
		Y	4.79	85.18	29.52		150.0	
		Z	3.29	72.66	21.97		150.0	
10170-CAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	2.43	68.34	20.24	3.01	150.0	± 9.6 %
		Y	31.37	128.86	43.10		150.0	
		Z	5.45	83.37	26.16		150.0	
10171-AAE	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	X	2.19	66.35	18.30	3.01	150.0	± 9.6 %
		Y	11.64	103.05	34.00		150.0	
		Z	4.06	76.52	22.29		150.0	
10172-CAG	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	4.72	83.25	27.75	6.02	65.0	± 9.6 %
		Y	100.00	168.92	55.74		65.0	
		Z	20.60	118.40	39.79		65.0	
10173-CAG	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM)	X	6.53	90.17	28.92	6.02	65.0	± 9.6 %
		Y	100.00	154.09	48.32		65.0	
		Z	100.00	143.61	43.42		65.0	
10174-CAG	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM)	X	6.38	89.02	27.96	6.02	65.0	± 9.6 %
		Y	100.00	150.07	46.22		65.0	
		Z	100.00	140.29	41.73		65.0	
10175-CAG	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	2.38	65.57	18.50	3.01	150.0	± 9.6 %
		Y	4.68	84.38	29.06		150.0	
		Z	3.23	72.21	21.65		150.0	
10176-CAG	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	2.43	68.36	20.25	3.01	150.0	± 9.6 %
		Y	31.64	129.04	43.15		150.0	
		Z	5.46	83.41	26.18		150.0	
10177-CAI	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	2.39	65.66	18.56	3.01	150.0	± 9.6 %
		Y	4.73	84.67	29.20		150.0	
		Z	3.27	72.44	21.78		150.0	
10178-CAG	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	2.42	68.28	20.19	3.01	150.0	± 9.6 %
		Y	29.59	127.38	42.66		150.0	
		Z	5.36	82.95	25.97		150.0	
10179-CAG	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	X	2.30	67.45	19.26	3.01	150.0	± 9.6 %
		Y	20.22	116.68	38.77		150.0	
		Z	4.72	79.90	24.13		150.0	
10180-CAG	LTE-FDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	X	2.19	66.34	18.28	3.01	150.0	± 9.6 %
		Y	11.48	102.68	33.86		150.0	
		Z	4.04	76.38	22.21		150.0	
10181-CAE	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	2.39	65.64	18.56	3.01	150.0	± 9.6 %
		Y	4.72	84.64	29.19		150.0	
		Z	3.26	72.41	21.77		150.0	
10182-CAE	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	2.42	68.26	20.18	3.01	150.0	± 9.6 %
		Y	29.40	127.23	42.62		150.0	
		Z	5.34	82.91	25.95		150.0	
10183-AAD	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	X	2.19	66.32	18.27	3.01	150.0	± 9.6 %
		Y	11.41	102.56	33.82		150.0	
		Z	4.03	76.34	22.20		150.0	

10184-CAE	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	2.39	65.67	18.57	3.01	150.0	± 9.6 %
		Y	4.75	84.73	29.22		150.0	
		Z	3.28	72.47	21.80		150.0	
10185-CAE	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	2.43	68.31	20.21	3.01	150.0	± 9.6 %
		Y	29.95	127.65	42.74		150.0	
		Z	5.38	83.03	26.00		150.0	
10186-AAE	LTE-FDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	X	2.19	66.37	18.30	3.01	150.0	± 9.6 %
		Y	11.59	102.87	33.93		150.0	
		Z	4.06	76.45	22.25		150.0	
10187-CAF	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	2.40	65.71	18.63	3.01	150.0	± 9.6 %
		Y	4.77	84.88	29.34		150.0	
		Z	3.28	72.52	21.86		150.0	
10188-CAF	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	2.46	68.61	20.45	3.01	150.0	± 9.6 %
		Y	36.87	132.92	44.31		150.0	
		Z	5.68	84.25	26.59		150.0	
10189-AAF	LTE-FDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	X	2.22	66.60	18.50	3.01	150.0	± 9.6 %
		Y	12.77	105.22	34.79		150.0	
		Z	4.20	77.17	22.65		150.0	
10193-CAC	IEEE 802.11n (HT Greenfield, 6.5 Mbps, BPSK)	X	4.54	66.91	16.29	0.00	150.0	± 9.6 %
		Y	4.88	70.16	19.56		150.0	
		Z	4.69	67.38	17.19		150.0	
10194-CAC	IEEE 802.11n (HT Greenfield, 39 Mbps, 16-QAM)	X	4.68	67.14	16.42	0.00	150.0	± 9.6 %
		Y	5.05	70.39	19.65		150.0	
		Z	4.88	67.73	17.31		150.0	
10195-CAC	IEEE 802.11n (HT Greenfield, 65 Mbps, 64-QAM)	X	4.71	67.16	16.43	0.00	150.0	± 9.6 %
		Y	5.08	70.37	19.63		150.0	
		Z	4.92	67.74	17.32		150.0	
10196-CAC	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	4.52	66.90	16.28	0.00	150.0	± 9.6 %
		Y	4.88	70.24	19.59		150.0	
		Z	4.70	67.48	17.23		150.0	
10197-CAC	IEEE 802.11n (HT Mixed, 39 Mbps, 16-QAM)	X	4.69	67.15	16.43	0.00	150.0	± 9.6 %
		Y	5.06	70.40	19.65		150.0	
		Z	4.89	67.75	17.33		150.0	
10198-CAC	IEEE 802.11n (HT Mixed, 65 Mbps, 64-QAM)	X	4.71	67.16	16.44	0.00	150.0	± 9.6 %
		Y	5.08	70.40	19.65		150.0	
		Z	4.92	67.77	17.33		150.0	
10219-CAC	IEEE 802.11n (HT Mixed, 7.2 Mbps, BPSK)	X	4.48	66.94	16.25	0.00	150.0	± 9.6 %
		Y	4.87	70.47	19.67		150.0	
		Z	4.66	67.53	17.22		150.0	
10220-CAC	IEEE 802.11n (HT Mixed, 43.3 Mbps, 16-QAM)	X	4.68	67.11	16.41	0.00	150.0	± 9.6 %
		Y	5.04	70.33	19.63		150.0	
		Z	4.89	67.72	17.32		150.0	
10221-CAC	IEEE 802.11n (HT Mixed, 72.2 Mbps, 64-QAM)	X	4.72	67.10	16.42	0.00	150.0	± 9.6 %
		Y	5.07	70.22	19.58		150.0	
		Z	4.93	67.67	17.31		150.0	
10222-CAC	IEEE 802.11n (HT Mixed, 15 Mbps, BPSK)	X	5.09	67.19	16.55	0.00	150.0	± 9.6 %
		Y	5.44	69.94	19.44		150.0	
		Z	5.25	67.80	17.36		150.0	

10223-CAC	IEEE 802.11n (HT Mixed, 90 Mbps, 16-QAM)	X	5.36	67.39	16.66	0.00	150.0	± 9.6 %
		Y	5.79	70.24	19.55		150.0	
		Z	5.58	68.01	17.47		150.0	
10224-CAC	IEEE 802.11n (HT Mixed, 150 Mbps, 64-QAM)	X	5.13	67.31	16.54	0.00	150.0	± 9.6 %
		Y	5.50	70.13	19.45		150.0	
		Z	5.31	67.93	17.35		150.0	
10225-CAB	UMTS-FDD (HSPA+)	X	2.82	66.39	15.24	0.00	150.0	± 9.6 %
		Y	5.39	83.22	25.04		150.0	
		Z	3.10	68.52	17.43		150.0	
10226-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM)	X	6.82	91.13	29.34	6.02	65.0	± 9.6 %
		Y	100.00	154.35	48.49		65.0	
		Z	100.00	143.89	43.61		65.0	
10227-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM)	X	7.64	92.49	29.17	6.02	65.0	± 9.6 %
		Y	100.00	150.17	46.35		65.0	
		Z	100.00	140.23	41.76		65.0	
10228-CAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK)	X	5.03	84.39	28.13	6.02	65.0	± 9.6 %
		Y	100.00	171.17	56.77		65.0	
		Z	36.11	132.10	43.75		65.0	
10229-CAC	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM)	X	6.57	90.27	28.96	6.02	65.0	± 9.6 %
		Y	100.00	154.02	48.30		65.0	
		Z	100.00	143.56	43.42		65.0	
10230-CAC	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM)	X	7.22	91.34	28.71	6.02	65.0	± 9.6 %
		Y	100.00	150.07	46.27		65.0	
		Z	100.00	140.03	41.62		65.0	
10231-CAC	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK)	X	4.90	83.79	27.84	6.02	65.0	± 9.6 %
		Y	100.00	170.98	56.64		65.0	
		Z	31.84	129.00	42.83		65.0	
10232-CAF	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM)	X	6.56	90.24	28.95	6.02	65.0	± 9.6 %
		Y	100.00	154.06	48.32		65.0	
		Z	100.00	143.59	43.42		65.0	
10233-CAF	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM)	X	7.19	91.28	28.70	6.02	65.0	± 9.6 %
		Y	100.00	150.12	46.29		65.0	
		Z	100.00	140.06	41.63		65.0	
10234-CAF	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK)	X	4.81	83.37	27.58	6.02	65.0	± 9.6 %
		Y	100.00	170.48	56.34		65.0	
		Z	29.21	126.68	42.05		65.0	
10235-CAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM)	X	6.56	90.26	28.96	6.02	65.0	± 9.6 %
		Y	100.00	154.09	48.33		65.0	
		Z	100.00	143.62	43.44		65.0	
10236-CAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM)	X	7.30	91.54	28.78	6.02	65.0	± 9.6 %
		Y	100.00	149.96	46.22		65.0	
		Z	100.00	139.96	41.59		65.0	
10237-CAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	4.89	83.82	27.85	6.02	65.0	± 9.6 %
		Y	100.00	171.08	56.68		65.0	
		Z	32.39	129.46	42.96		65.0	
10238-CAF	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM)	X	6.54	90.21	28.94	6.02	65.0	± 9.6 %
		Y	100.00	154.11	48.34		65.0	
		Z	100.00	143.62	43.44		65.0	

10239-CAF	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM)	X	7.16	91.22	28.68	6.02	65.0	± 9.6 %
		Y	100.00	150.18	46.31		65.0	
		Z	100.00	140.11	41.65		65.0	
10240-CAF	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	4.89	83.79	27.85	6.02	65.0	± 9.6 %
		Y	100.00	171.14	56.70		65.0	
		Z	32.07	129.26	42.91		65.0	
10241-CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM)	X	6.89	80.86	26.48	6.98	65.0	± 9.6 %
		Y	15.14	102.74	36.01		65.0	
		Z	7.96	83.07	27.57		65.0	
10242-CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM)	X	6.80	80.72	26.37	6.98	65.0	± 9.6 %
		Y	14.33	101.02	35.18		65.0	
		Z	7.38	81.22	26.68		65.0	
10243-CAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK)	X	5.93	77.53	25.75	6.98	65.0	± 9.6 %
		Y	7.95	88.70	32.02		65.0	
		Z	5.71	76.44	25.56		65.0	
10244-CAC	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	6.09	77.33	19.18	3.98	65.0	± 9.6 %
		Y	100.00	128.91	35.76		65.0	
		Z	12.63	92.71	26.45		65.0	
10245-CAC	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	X	5.77	76.20	18.64	3.98	65.0	± 9.6 %
		Y	100.00	128.15	35.42		65.0	
		Z	11.34	90.40	25.59		65.0	
10246-CAC	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	4.45	74.40	17.70	3.98	65.0	± 9.6 %
		Y	100.00	136.14	38.09		65.0	
		Z	22.41	107.23	31.00		65.0	
10247-CAF	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM)	X	4.56	71.86	17.13	3.98	65.0	± 9.6 %
		Y	73.33	128.51	37.19		65.0	
		Z	5.99	80.00	22.59		65.0	
10248-CAF	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM)	X	4.51	71.27	16.84	3.98	65.0	± 9.6 %
		Y	26.38	109.01	31.99		65.0	
		Z	5.74	78.49	21.91		65.0	
10249-CAF	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK)	X	5.66	78.41	20.44	3.98	65.0	± 9.6 %
		Y	100.00	142.87	42.05		65.0	
		Z	18.21	104.78	31.43		65.0	
10250-CAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM)	X	5.61	74.95	20.41	3.98	65.0	± 9.6 %
		Y	13.54	100.79	32.79		65.0	
		Z	6.07	79.55	24.03		65.0	
10251-CAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM)	X	5.38	73.15	19.26	3.98	65.0	± 9.6 %
		Y	8.77	89.12	28.04		65.0	
		Z	5.62	76.39	22.24		65.0	
10252-CAF	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	6.27	79.36	22.01	3.98	65.0	± 9.6 %
		Y	100.00	147.00	45.24		65.0	
		Z	9.92	92.18	28.37		65.0	
10253-CAF	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM)	X	5.61	72.83	19.63	3.98	65.0	± 9.6 %
		Y	6.66	81.73	25.73		65.0	
		Z	5.44	74.31	21.61		65.0	
10254-CAF	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM)	X	5.93	73.65	20.27	3.98	65.0	± 9.6 %
		Y	7.09	82.86	26.51		65.0	
		Z	5.76	75.13	22.28		65.0	

10255-CAF	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.13	76.89	21.33	3.98	65.0	± 9.6 %
		Y	22.24	111.88	36.31		65.0	
		Z	6.94	82.22	24.80		65.0	
10256-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM)	X	4.46	72.23	15.83	3.98	65.0	± 9.6 %
		Y	100.00	121.25	31.39		65.0	
		Z	11.37	89.76	24.19		65.0	
10257-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM)	X	4.16	70.86	15.07	3.98	65.0	± 9.6 %
		Y	100.00	119.86	30.76		65.0	
		Z	9.33	85.94	22.74		65.0	
10258-CAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK)	X	3.29	69.56	14.55	3.98	65.0	± 9.6 %
		Y	100.00	127.44	33.46		65.0	
		Z	15.22	98.84	27.43		65.0	
10259-CAC	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM)	X	4.98	73.11	18.35	3.98	65.0	± 9.6 %
		Y	30.79	114.92	34.97		65.0	
		Z	6.02	79.75	23.07		65.0	
10260-CAC	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM)	X	5.00	72.84	18.22	3.98	65.0	± 9.6 %
		Y	21.82	107.57	32.81		65.0	
		Z	5.94	79.01	22.75		65.0	
10261-CAC	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK)	X	5.70	78.16	20.80	3.98	65.0	± 9.6 %
		Y	100.00	144.55	43.34		65.0	
		Z	11.30	95.48	28.98		65.0	
10262-CAF	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM)	X	5.59	74.89	20.36	3.98	65.0	± 9.6 %
		Y	13.45	100.60	32.69		65.0	
		Z	6.07	79.51	23.99		65.0	
10263-CAF	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM)	X	5.37	73.13	19.26	3.98	65.0	± 9.6 %
		Y	8.73	89.04	28.02		65.0	
		Z	5.61	76.36	22.23		65.0	
10264-CAF	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK)	X	6.22	79.19	21.93	3.98	65.0	± 9.6 %
		Y	100.00	146.87	45.17		65.0	
		Z	9.77	91.84	28.22		65.0	
10265-CAF	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM)	X	5.68	73.18	19.88	3.98	65.0	± 9.6 %
		Y	6.90	82.70	26.25		65.0	
		Z	5.63	75.17	21.99		65.0	
10266-CAF	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM)	X	6.04	74.11	20.62	3.98	65.0	± 9.6 %
		Y	7.35	83.84	27.09		65.0	
		Z	5.95	75.95	22.69		65.0	
10267-CAF	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	6.37	77.41	21.40	3.98	65.0	± 9.6 %
		Y	30.19	117.69	37.71		65.0	
		Z	7.69	83.94	25.19		65.0	
10268-CAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM)	X	6.34	73.27	20.38	3.98	65.0	± 9.6 %
		Y	6.53	78.38	24.77		65.0	
		Z	6.07	74.12	21.80		65.0	
10269-CAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM)	X	6.35	72.95	20.28	3.98	65.0	± 9.6 %
		Y	6.35	77.23	24.28		65.0	
		Z	6.00	73.46	21.55		65.0	
10270-CAF	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	6.38	75.20	20.64	3.98	65.0	± 9.6 %
		Y	9.50	89.19	28.55		65.0	
		Z	6.59	78.01	22.84		65.0	

10274-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.10)	X	2.67	67.00	15.36	0.00	150.0	± 9.6 %
		Y	10.84	98.97	30.38		150.0	
		Z	2.98	69.70	17.77		150.0	
10275-CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	X	1.70	67.97	15.87	0.00	150.0	± 9.6 %
		Y	100.00	167.59	50.63		150.0	
		Z	3.57	83.80	23.61		150.0	
10277-CAA	PHS (QPSK)	X	2.97	63.64	8.94	9.03	50.0	± 9.6 %
		Y	1.46	59.37	4.79		50.0	
		Z	1.77	61.03	6.66		50.0	
10278-CAA	PHS (QPSK, BW 884MHz, Rolloff 0.5)	X	5.12	71.66	15.18	9.03	50.0	± 9.6 %
		Y	4.05	70.90	13.69		50.0	
		Z	39.09	105.24	26.82		50.0	
10279-CAA	PHS (QPSK, BW 884MHz, Rolloff 0.38)	X	5.19	71.80	15.29	9.03	50.0	± 9.6 %
		Y	4.36	71.78	14.15		50.0	
		Z	38.18	104.98	26.85		50.0	
10290-AAB	CDMA2000, RC1, SO55, Full Rate	X	1.44	69.04	14.10	0.00	150.0	± 9.6 %
		Y	100.00	167.69	47.65		150.0	
		Z	100.00	132.24	33.89		150.0	
10291-AAB	CDMA2000, RC3, SO55, Full Rate	X	0.96	67.16	13.43	0.00	150.0	± 9.6 %
		Y	100.00	268.49	86.34		150.0	
		Z	100.00	140.46	36.17		150.0	
10292-AAB	CDMA2000, RC3, SO32, Full Rate	X	1.30	72.32	16.26	0.00	150.0	± 9.6 %
		Y	100.00	339.47	114.76		150.0	
		Z	100.00	148.22	39.44		150.0	
10293-AAB	CDMA2000, RC3, SO3, Full Rate	X	2.11	79.54	19.56	0.00	150.0	± 9.6 %
		Y	100.00	339.44	115.72		150.0	
		Z	100.00	153.47	41.91		150.0	
10295-AAB	CDMA2000, RC1, SO3, 1/8th Rate 25 fr.	X	16.12	91.99	25.52	9.03	50.0	± 9.6 %
		Y	100.00	122.32	33.26		50.0	
		Z	39.98	116.52	34.87		50.0	
10297-AAD	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	2.71	69.27	16.77	0.00	150.0	± 9.6 %
		Y	100.00	147.50	43.97		150.0	
		Z	4.07	77.55	20.99		150.0	
10298-AAD	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, QPSK)	X	1.50	67.28	13.70	0.00	150.0	± 9.6 %
		Y	100.00	153.53	42.95		150.0	
		Z	9.87	97.83	26.35		150.0	
10299-AAD	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM)	X	7.67	88.02	21.99	0.00	150.0	± 9.6 %
		Y	100.00	132.38	35.14		150.0	
		Z	70.95	120.54	31.58		150.0	
10300-AAD	LTE-FDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM)	X	2.22	69.32	13.93	0.00	150.0	± 9.6 %
		Y	100.00	121.47	29.95		150.0	
		Z	4.30	76.94	17.78		150.0	
10301-AAA	IEEE 802.16e WiMAX (29:18, 5ms, 10MHz, QPSK, PUSC)	X	4.70	65.88	17.62	4.17	50.0	± 9.6 %
		Y	5.31	70.07	20.92		50.0	
		Z	5.01	66.67	18.68		50.0	
10302-AAA	IEEE 802.16e WiMAX (29:18, 5ms, 10MHz, QPSK, PUSC, 3 CTRL symbols)	X	5.22	66.65	18.43	4.96	50.0	± 9.6 %
		Y	5.51	69.33	20.92		50.0	
		Z	5.36	66.61	19.00		50.0	

10303-AAA	IEEE 802.16e WiMAX (31:15, 5ms, 10MHz, 64QAM, PUSC)	X	4.99	66.34	18.26	4.96	50.0	± 9.6 %
		Y	5.24	69.04	20.80		50.0	
		Z	5.09	66.24	18.85		50.0	
10304-AAA	IEEE 802.16e WiMAX (29:18, 5ms, 10MHz, 64QAM, PUSC)	X	4.78	66.12	17.70	4.17	50.0	± 9.6 %
		Y	5.17	69.49	20.64		50.0	
		Z	4.92	66.22	18.41		50.0	
10305-AAA	IEEE 802.16e WiMAX (31:15, 10ms, 10MHz, 64QAM, PUSC, 15 symbols)	X	4.77	69.59	20.25	6.02	35.0	± 9.6 %
		Y	5.41	75.27	24.15		35.0	
		Z	4.44	68.01	20.57		35.0	
10306-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, 64QAM, PUSC, 18 symbols)	X	4.91	67.94	19.68	6.02	35.0	± 9.6 %
		Y	5.18	71.41	22.58		35.0	
		Z	4.78	66.92	20.02		35.0	
10307-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, QPSK, PUSC, 18 symbols)	X	4.82	68.09	19.65	6.02	35.0	± 9.6 %
		Y	5.14	71.94	22.72		35.0	
		Z	4.68	67.17	20.04		35.0	
10308-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, 16QAM, PUSC)	X	4.82	68.38	19.84	6.02	35.0	± 9.6 %
		Y	5.19	72.52	23.06		35.0	
		Z	4.65	67.35	20.17		35.0	
10309-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, 16QAM, AMC 2x3, 18 symbols)	X	4.93	68.02	19.77	6.02	35.0	± 9.6 %
		Y	5.24	71.67	22.76		35.0	
		Z	4.85	67.23	20.21		35.0	
10310-AAA	IEEE 802.16e WiMAX (29:18, 10ms, 10MHz, QPSK, AMC 2x3, 18 symbols)	X	4.88	68.05	19.70	6.02	35.0	± 9.6 %
		Y	5.17	71.72	22.69		35.0	
		Z	4.72	66.99	20.00		35.0	
10311-AAD	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	3.07	68.61	16.42	0.00	150.0	± 9.6 %
		Y	79.81	135.69	40.32		150.0	
		Z	4.40	75.62	20.03		150.0	
10313-AAA	iDEN 1:3	X	4.61	77.72	19.35	6.99	70.0	± 9.6 %
		Y	100.00	134.35	35.76		70.0	
		Z	100.00	127.14	32.92		70.0	
10314-AAA	iDEN 1:6	X	6.77	85.06	24.68	10.00	30.0	± 9.6 %
		Y	100.00	145.94	42.34		30.0	
		Z	100.00	139.62	39.85		30.0	
10315-AAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 96pc duty cycle)	X	1.23	63.78	15.26	0.17	150.0	± 9.6 %
		Y	48.91	185.97	63.30		150.0	
		Z	1.24	69.36	20.19		150.0	
10316-AAB	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 96pc duty cycle)	X	4.57	66.83	16.36	0.17	150.0	± 9.6 %
		Y	4.90	70.05	19.66		150.0	
		Z	4.74	67.44	17.35		150.0	
10317-AAC	IEEE 802.11a WiFi 5 GHz (OFDM, 6 Mbps, 96pc duty cycle)	X	4.57	66.83	16.36	0.17	150.0	± 9.6 %
		Y	4.90	70.05	19.66		150.0	
		Z	4.74	67.44	17.35		150.0	
10400-AAD	IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)	X	4.64	67.16	16.41	0.00	150.0	± 9.6 %
		Y	5.05	70.58	19.72		150.0	
		Z	4.88	67.82	17.32		150.0	
10401-AAD	IEEE 802.11ac WiFi (40MHz, 64-QAM, 99pc duty cycle)	X	5.31	67.01	16.43	0.00	150.0	± 9.6 %
		Y	5.74	69.83	19.29		150.0	
		Z	5.60	67.93	17.40		150.0	



10402-AAD	IEEE 802.11ac WiFi (80MHz, 64-QAM, 99pc duty cycle)	X	5.65	67.55	16.59	0.00	150.0	± 9.6 %
		Y	5.92	69.59	19.00		150.0	
		Z	5.83	68.10	17.32		150.0	
10403-AAB	CDMA2000 (1xEV-DO, Rev. 0)	X	1.44	69.04	14.10	0.00	115.0	± 9.6 %
		Y	100.00	167.69	47.65		115.0	
		Z	100.00	132.24	33.89		115.0	
10404-AAB	CDMA2000 (1xEV-DO, Rev. A)	X	1.44	69.04	14.10	0.00	115.0	± 9.6 %
		Y	100.00	167.69	47.65		115.0	
		Z	100.00	132.24	33.89		115.0	
10406-AAB	CDMA2000, RC3, SO32, SCH0, Full Rate	X	100.00	157.31	45.09	0.00	100.0	± 9.6 %
		Y	100.00	156.13	45.96		100.0	
		Z	100.00	136.83	37.30		100.0	
10410-AAF	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9, Subframe Conf=4)	X	100.00	147.71	41.95	3.23	80.0	± 9.6 %
		Y	100.00	182.38	56.63		80.0	
		Z	100.00	142.83	39.60		80.0	
10415-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	1.17	63.30	14.91	0.00	150.0	± 9.6 %
		Y	24.98	166.87	58.63		150.0	
		Z	1.16	68.25	19.44		150.0	
10416-AAA	IEEE 802.11g WiFi 2.4 GHz (ERP-OFDM, 6 Mbps, 99pc duty cycle)	X	4.53	66.89	16.35	0.00	150.0	± 9.6 %
		Y	4.87	70.15	19.64		150.0	
		Z	4.69	67.43	17.26		150.0	
10417-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 99pc duty cycle)	X	4.53	66.89	16.35	0.00	150.0	± 9.6 %
		Y	4.87	70.15	19.64		150.0	
		Z	4.69	67.43	17.26		150.0	
10418-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Long preamble)	X	4.53	67.09	16.41	0.00	150.0	± 9.6 %
		Y	4.92	70.65	19.84		150.0	
		Z	4.69	67.64	17.31		150.0	
10419-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 99pc duty cycle, Short preamble)	X	4.54	67.02	16.40	0.00	150.0	± 9.6 %
		Y	4.91	70.44	19.75		150.0	
		Z	4.71	67.57	17.30		150.0	
10422-AAB	IEEE 802.11n (HT Greenfield, 7.2 Mbps, BPSK)	X	4.65	67.01	16.41	0.00	150.0	± 9.6 %
		Y	4.98	70.13	19.59		150.0	
		Z	4.82	67.51	17.27		150.0	
10423-AAB	IEEE 802.11n (HT Greenfield, 43.3 Mbps, 16-QAM)	X	4.78	67.26	16.49	0.00	150.0	± 9.6 %
		Y	5.15	70.46	19.68		150.0	
		Z	5.01	67.86	17.39		150.0	
10424-AAB	IEEE 802.11n (HT Greenfield, 72.2 Mbps, 64-QAM)	X	4.71	67.21	16.47	0.00	150.0	± 9.6 %
		Y	5.09	70.51	19.72		150.0	
		Z	4.93	67.83	17.38		150.0	
10425-AAB	IEEE 802.11n (HT Greenfield, 15 Mbps, BPSK)	X	5.33	67.41	16.65	0.00	150.0	± 9.6 %
		Y	5.75	70.27	19.54		150.0	
		Z	5.57	68.18	17.53		150.0	
10426-AAB	IEEE 802.11n (HT Greenfield, 90 Mbps, 16-QAM)	X	5.35	67.50	16.69	0.00	150.0	± 9.6 %
		Y	5.96	71.01	19.90		150.0	
		Z	5.59	68.24	17.56		150.0	

10427-AAB	IEEE 802.11n (HT Greenfield, 150 Mbps, 64-QAM)	X	5.31	67.29	16.58	0.00	150.0	± 9.6 %
		Y	5.73	70.13	19.47		150.0	
		Z	5.58	68.13	17.50		150.0	
10430-AAD	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1)	X	4.19	71.23	18.04	0.00	150.0	± 9.6 %
		Y	16.02	102.21	31.95		150.0	
		Z	4.91	74.11	20.54		150.0	
10431-AAD	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1)	X	4.14	67.45	16.25	0.00	150.0	± 9.6 %
		Y	4.98	73.42	20.89		150.0	
		Z	4.46	68.44	17.52		150.0	
10432-AAC	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1)	X	4.47	67.30	16.40	0.00	150.0	± 9.6 %
		Y	4.99	71.46	20.12		150.0	
		Z	4.72	68.03	17.43		150.0	
10433-AAC	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1)	X	4.72	67.24	16.49	0.00	150.0	± 9.6 %
		Y	5.11	70.54	19.74		150.0	
		Z	4.94	67.87	17.40		150.0	
10434-AAA	W-CDMA (BS Test Model 1, 64 DPCH)	X	4.26	72.03	17.88	0.00	150.0	± 9.6 %
		Y	86.61	134.15	39.78		150.0	
		Z	5.32	75.97	20.91		150.0	
10435-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	147.37	41.79	3.23	80.0	± 9.6 %
		Y	100.00	182.03	56.46		80.0	
		Z	100.00	142.57	39.48		80.0	
10447-AAD	LTE-FDD (OFDMA, 5 MHz, E-TM 3.1, Clipping 44%)	X	3.39	67.36	15.28	0.00	150.0	± 9.6 %
		Y	6.31	81.96	23.56		150.0	
		Z	3.88	69.36	17.36		150.0	
10448-AAD	LTE-FDD (OFDMA, 10 MHz, E-TM 3.1, Clipping 44%)	X	4.01	67.25	16.13	0.00	150.0	± 9.6 %
		Y	4.84	73.40	20.90		150.0	
		Z	4.29	68.25	17.41		150.0	
10449-AAC	LTE-FDD (OFDMA, 15 MHz, E-TM 3.1, Clipping 44%)	X	4.31	67.12	16.30	0.00	150.0	± 9.6 %
		Y	4.84	71.52	20.19		150.0	
		Z	4.52	67.91	17.37		150.0	
10450-AAC	LTE-FDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)	X	4.52	67.03	16.35	0.00	150.0	± 9.6 %
		Y	4.91	70.51	19.74		150.0	
		Z	4.70	67.68	17.30		150.0	
10451-AAA	W-CDMA (BS Test Model 1, 64 DPCH, Clipping 44%)	X	3.21	67.28	14.69	0.00	150.0	± 9.6 %
		Y	9.18	88.88	25.28		150.0	
		Z	3.88	70.03	17.20		150.0	
10456-AAB	IEEE 802.11ac WiFi (160MHz, 64-QAM, 99pc duty cycle)	X	6.25	67.96	16.82	0.00	150.0	± 9.6 %
		Y	6.79	70.57	19.43		150.0	
		Z	6.43	68.52	17.53		150.0	
10457-AAA	UMTS-FDD (DC-HSDPA)	X	3.89	65.65	16.07	0.00	150.0	± 9.6 %
		Y	4.04	68.61	19.47		150.0	
		Z	3.89	66.00	17.02		150.0	
10458-AAA	CDMA2000 (1xEV-DO, Rev. B, 2 carriers)	X	3.78	70.72	16.79	0.00	150.0	± 9.6 %
		Y	100.00	135.03	39.05		150.0	
		Z	4.92	75.32	20.38		150.0	
10459-AAA	CDMA2000 (1xEV-DO, Rev. B, 3 carriers)	X	4.84	68.36	17.55	0.00	150.0	± 9.6 %
		Y	6.74	77.14	23.30		150.0	
		Z	5.46	69.90	19.56		150.0	

10460-AAA	UMTS-FDD (WCDMA, AMR)	X	1.02	67.53	16.31	0.00	150.0	± 9.6 %
		Y	100.00	268.38	89.96		150.0	
		Z	100.00	165.50	47.42		150.0	
10461-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	30.29	128.32	38.39	3.29	80.0	± 9.6 %
		Y	100.00	227.54	75.96		80.0	
		Z	100.00	156.67	45.76		80.0	
10462-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	132.43	34.11	3.23	80.0	± 9.6 %
		Y	100.00	189.47	58.20		80.0	
		Z	100.00	128.13	32.45		80.0	
10463-AAA	LTE-TDD (SC-FDMA, 1 RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	125.96	31.09	3.23	80.0	± 9.6 %
		Y	100.00	181.08	54.22		80.0	
		Z	100.00	120.08	28.81		80.0	
10464-AAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	86.49	146.66	42.03	3.23	80.0	± 9.6 %
		Y	100.00	235.38	78.70		80.0	
		Z	100.00	155.27	44.82		80.0	
10465-AAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	131.34	33.60	3.23	80.0	± 9.6 %
		Y	100.00	186.94	57.07		80.0	
		Z	100.00	126.73	31.81		80.0	
10466-AAB	LTE-TDD (SC-FDMA, 1 RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	124.72	30.55	3.23	80.0	± 9.6 %
		Y	100.00	176.97	52.47		80.0	
		Z	100.00	118.66	28.18		80.0	
10467-AAE	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	149.70	42.78	3.23	80.0	± 9.6 %
		Y	100.00	236.58	79.22		80.0	
		Z	100.00	155.78	45.04		80.0	
10468-AAE	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	131.79	33.80	3.23	80.0	± 9.6 %
		Y	100.00	188.21	57.62		80.0	
		Z	100.00	127.23	32.03		80.0	
10469-AAE	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	124.92	30.63	3.23	80.0	± 9.6 %
		Y	100.00	177.66	52.75		80.0	
		Z	100.00	118.74	28.21		80.0	
10470-AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	149.81	42.82	3.23	80.0	± 9.6 %
		Y	100.00	237.48	79.57		80.0	
		Z	100.00	155.98	45.11		80.0	
10471-AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	131.76	33.78	3.23	80.0	± 9.6 %
		Y	100.00	188.41	57.69		80.0	
		Z	100.00	127.14	31.98		80.0	
10472-AAE	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	124.86	30.60	3.23	80.0	± 9.6 %
		Y	100.00	177.88	52.83		80.0	
		Z	100.00	118.64	28.16		80.0	
10473-AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	100.00	149.79	42.80	3.23	80.0	± 9.6 %
		Y	100.00	237.45	79.56		80.0	
		Z	100.00	155.92	45.09		80.0	
10474-AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	131.79	33.79	3.23	80.0	± 9.6 %
		Y	100.00	188.70	57.80		80.0	
		Z	100.00	127.19	32.00		80.0	
10475-AAE	LTE-TDD (SC-FDMA, 1 RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	124.90	30.61	3.23	80.0	± 9.6 %
		Y	100.00	178.11	52.92		80.0	
		Z	100.00	118.68	28.17		80.0	

10477-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	131.48	33.65	3.23	80.0	± 9.6 %
		Y	100.00	188.07	57.51		80.0	
		Z	100.00	126.79	31.81		80.0	
10478-AAF	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	124.73	30.54	3.23	80.0	± 9.6 %
		Y	100.00	177.85	52.80		80.0	
		Z	100.00	118.54	28.11		80.0	
10479-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	21.69	110.19	32.27	3.23	80.0	± 9.6 %
		Y	100.00	165.12	51.20		80.0	
		Z	100.00	139.63	40.30		80.0	
10480-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	125.84	33.24	3.23	80.0	± 9.6 %
		Y	100.00	141.46	40.32		80.0	
		Z	100.00	126.11	33.98		80.0	
10481-AAA	LTE-TDD (SC-FDMA, 50% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	100.00	123.10	31.88	3.23	80.0	± 9.6 %
		Y	100.00	137.55	38.41		80.0	
		Z	100.00	123.64	32.75		80.0	
10482-AAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	2.17	67.58	14.46	2.23	80.0	± 9.6 %
		Y	100.00	149.15	42.74		80.0	
		Z	100.00	131.37	35.78		80.0	
10483-AAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	10.85	87.56	21.98	2.23	80.0	± 9.6 %
		Y	100.00	133.92	37.04		80.0	
		Z	100.00	125.29	33.83		80.0	
10484-AAB	LTE-TDD (SC-FDMA, 50% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	8.19	83.39	20.60	2.23	80.0	± 9.6 %
		Y	100.00	132.37	36.40		80.0	
		Z	100.00	124.74	33.65		80.0	
10485-AAE	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	2.64	69.84	16.61	2.23	80.0	± 9.6 %
		Y	100.00	154.16	46.03		80.0	
		Z	38.17	118.90	34.32		80.0	
10486-AAE	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	2.67	66.93	14.51	2.23	80.0	± 9.6 %
		Y	100.00	135.10	38.01		80.0	
		Z	7.94	86.47	24.06		80.0	
10487-AAE	LTE-TDD (SC-FDMA, 50% RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	2.67	66.60	14.31	2.23	80.0	± 9.6 %
		Y	100.00	133.67	37.44		80.0	
		Z	7.07	84.08	23.21		80.0	
10488-AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.05	69.91	17.60	2.23	80.0	± 9.6 %
		Y	100.00	150.55	45.87		80.0	
		Z	8.12	89.97	26.75		80.0	
10489-AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.21	67.77	16.46	2.23	80.0	± 9.6 %
		Y	100.00	141.09	42.34		80.0	
		Z	4.54	75.71	21.43		80.0	
10490-AAE	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.29	67.69	16.41	2.23	80.0	± 9.6 %
		Y	100.00	139.78	41.89		80.0	
		Z	4.51	74.82	21.04		80.0	
10491-AAE	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.40	69.16	17.47	2.23	80.0	± 9.6 %
		Y	100.00	144.25	43.91		80.0	
		Z	5.70	80.39	23.33		80.0	
10492-AAE	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.60	67.37	16.69	2.23	80.0	± 9.6 %
		Y	11.08	94.67	30.08		80.0	
		Z	4.34	72.10	20.09		80.0	

10493-AAE	LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.66	67.29	16.65	2.23	80.0	± 9.6 %
		Y	9.83	91.62	28.99		80.0	
		Z	4.36	71.66	19.89		80.0	
10494-AAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.57	70.14	17.82	2.23	80.0	± 9.6 %
		Y	100.00	143.73	43.57		80.0	
		Z	7.48	85.35	24.92		80.0	
10495-AAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.62	67.57	16.87	2.23	80.0	± 9.6 %
		Y	11.53	95.88	30.63		80.0	
		Z	4.46	72.87	20.46		80.0	
10496-AAF	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.71	67.43	16.84	2.23	80.0	± 9.6 %
		Y	9.36	90.73	28.85		80.0	
		Z	4.43	72.03	20.10		80.0	
10497-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	1.56	63.60	11.39	2.23	80.0	± 9.6 %
		Y	100.00	137.64	36.75		80.0	
		Z	100.00	126.22	32.89		80.0	
10498-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	1.30	60.00	8.26	2.23	80.0	± 9.6 %
		Y	100.00	105.27	22.62		80.0	
		Z	8.37	83.55	19.67		80.0	
10499-AAA	LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	1.32	60.00	8.09	2.23	80.0	± 9.6 %
		Y	100.00	102.17	21.24		80.0	
		Z	5.44	77.62	17.52		80.0	
10500-AAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	2.80	69.82	16.99	2.23	80.0	± 9.6 %
		Y	100.00	151.96	45.66		80.0	
		Z	13.13	99.69	29.44		80.0	
10501-AAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	2.93	67.50	15.34	2.23	80.0	± 9.6 %
		Y	100.00	136.97	39.47		80.0	
		Z	5.76	80.70	22.57		80.0	
10502-AAB	LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	2.97	67.38	15.21	2.23	80.0	± 9.6 %
		Y	100.00	135.40	38.81		80.0	
		Z	5.69	79.92	22.18		80.0	
10503-AAE	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.03	69.77	17.53	2.23	80.0	± 9.6 %
		Y	100.00	150.48	45.82		80.0	
		Z	7.88	89.44	26.56		80.0	
10504-AAE	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.20	67.70	16.40	2.23	80.0	± 9.6 %
		Y	100.00	140.97	42.28		80.0	
		Z	4.51	75.56	21.35		80.0	
10505-AAE	LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.28	67.62	16.36	2.23	80.0	± 9.6 %
		Y	100.00	139.68	41.83		80.0	
		Z	4.47	74.67	20.96		80.0	
10506-AAE	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	3.55	70.05	17.76	2.23	80.0	± 9.6 %
		Y	100.00	143.63	43.52		80.0	
		Z	7.35	85.02	24.79		80.0	
10507-AAE	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.60	67.52	16.84	2.23	80.0	± 9.6 %
		Y	11.40	95.64	30.54		80.0	
		Z	4.44	72.79	20.41		80.0	

10508-AAE	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	3.70	67.38	16.80	2.23	80.0	± 9.6 %
		Y	9.23	90.42	28.73		80.0	
		Z	4.41	71.94	20.05		80.0	
10509-AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	4.01	69.47	17.53	2.23	80.0	± 9.6 %
		Y	53.57	125.53	38.61		80.0	
		Z	6.08	78.49	22.24		80.0	
10510-AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	4.10	67.43	16.97	2.23	80.0	± 9.6 %
		Y	6.91	81.81	25.51		80.0	
		Z	4.71	71.13	19.66		80.0	
10511-AAE	LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	4.18	67.30	16.94	2.23	80.0	± 9.6 %
		Y	6.46	79.80	24.71		80.0	
		Z	4.68	70.51	19.41		80.0	
10512-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9)	X	4.04	70.41	17.82	2.23	80.0	± 9.6 %
		Y	100.00	138.39	41.56		80.0	
		Z	7.77	83.71	24.02		80.0	
10513-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9)	X	3.98	67.51	17.01	2.23	80.0	± 9.6 %
		Y	7.39	84.17	26.51		80.0	
		Z	4.68	71.90	20.02		80.0	
10514-AAF	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9)	X	4.03	67.25	16.94	2.23	80.0	± 9.6 %
		Y	6.57	81.06	25.32		80.0	
		Z	4.59	70.95	19.65		80.0	
10515-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle)	X	1.13	63.45	14.97	0.00	150.0	± 9.6 %
		Y	100.00	212.37	69.78		150.0	
		Z	1.15	69.27	20.00		150.0	
10516-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 99pc duty cycle)	X	0.71	67.89	16.98	0.00	150.0	± 9.6 %
		Y	99.96	250.00	60.00		150.0	
		Z	100.00	203.45	60.50		150.0	
10517-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 99pc duty cycle)	X	0.97	64.91	15.54	0.00	150.0	± 9.6 %
		Y	100.00	250.98	84.10		150.0	
		Z	1.77	85.15	26.99		150.0	
10518-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 99pc duty cycle)	X	4.52	66.99	16.35	0.00	150.0	± 9.6 %
		Y	4.90	70.44	19.72		150.0	
		Z	4.69	67.55	17.26		150.0	
10519-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 99pc duty cycle)	X	4.67	67.16	16.43	0.00	150.0	± 9.6 %
		Y	5.05	70.50	19.72		150.0	
		Z	4.89	67.78	17.36		150.0	
10520-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 99pc duty cycle)	X	4.52	67.09	16.35	0.00	150.0	± 9.6 %
		Y	4.95	70.74	19.82		150.0	
		Z	4.75	67.81	17.33		150.0	
10521-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 99pc duty cycle)	X	4.46	67.05	16.33	0.00	150.0	± 9.6 %
		Y	4.89	70.83	19.88		150.0	
		Z	4.69	67.84	17.34		150.0	
10522-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 99pc duty cycle)	X	4.51	67.16	16.42	0.00	150.0	± 9.6 %
		Y	4.97	71.03	20.00		150.0	
		Z	4.74	67.90	17.41		150.0	

10523-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 99pc duty cycle)	X	4.44	67.18	16.36	0.00	150.0	± 9.6 %
		Y	4.91	71.14	19.99		150.0	
		Z	4.62	67.80	17.28		150.0	
10524-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 99pc duty cycle)	X	4.46	67.13	16.42	0.00	150.0	± 9.6 %
		Y	4.91	71.02	20.02		150.0	
		Z	4.69	67.84	17.39		150.0	
10525-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 99pc duty cycle)	X	4.49	66.26	16.03	0.00	150.0	± 9.6 %
		Y	4.95	69.92	19.51		150.0	
		Z	4.68	66.85	16.96		150.0	
10526-AAB	IEEE 802.11ac WiFi (20MHz, MCS1, 99pc duty cycle)	X	4.61	66.52	16.15	0.00	150.0	± 9.6 %
		Y	5.13	70.34	19.66		150.0	
		Z	4.87	67.27	17.11		150.0	
10527-AAB	IEEE 802.11ac WiFi (20MHz, MCS2, 99pc duty cycle)	X	4.54	66.49	16.09	0.00	150.0	± 9.6 %
		Y	5.09	70.47	19.70		150.0	
		Z	4.79	67.26	17.08		150.0	
10528-AAB	IEEE 802.11ac WiFi (20MHz, MCS3, 99pc duty cycle)	X	4.56	66.51	16.12	0.00	150.0	± 9.6 %
		Y	5.09	70.44	19.71		150.0	
		Z	4.81	67.28	17.11		150.0	
10529-AAB	IEEE 802.11ac WiFi (20MHz, MCS4, 99pc duty cycle)	X	4.56	66.51	16.12	0.00	150.0	± 9.6 %
		Y	5.09	70.44	19.71		150.0	
		Z	4.81	67.28	17.11		150.0	
10531-AAB	IEEE 802.11ac WiFi (20MHz, MCS6, 99pc duty cycle)	X	4.52	66.52	16.10	0.00	150.0	± 9.6 %
		Y	5.10	70.68	19.80		150.0	
		Z	4.81	67.45	17.16		150.0	
10532-AAB	IEEE 802.11ac WiFi (20MHz, MCS7, 99pc duty cycle)	X	4.40	66.39	16.03	0.00	150.0	± 9.6 %
		Y	4.98	70.66	19.82		150.0	
		Z	4.67	67.33	17.11		150.0	
10533-AAB	IEEE 802.11ac WiFi (20MHz, MCS8, 99pc duty cycle)	X	4.56	66.59	16.13	0.00	150.0	± 9.6 %
		Y	5.13	70.66	19.77		150.0	
		Z	4.82	67.33	17.10		150.0	
10534-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 99pc duty cycle)	X	5.12	66.52	16.18	0.00	150.0	± 9.6 %
		Y	5.53	69.34	19.09		150.0	
		Z	5.33	67.19	17.03		150.0	
10535-AAB	IEEE 802.11ac WiFi (40MHz, MCS1, 99pc duty cycle)	X	5.16	66.64	16.24	0.00	150.0	± 9.6 %
		Y	5.65	69.76	19.28		150.0	
		Z	5.42	67.43	17.13		150.0	
10536-AAB	IEEE 802.11ac WiFi (40MHz, MCS2, 99pc duty cycle)	X	5.05	66.64	16.22	0.00	150.0	± 9.6 %
		Y	5.54	69.84	19.32		150.0	
		Z	5.28	67.38	17.10		150.0	
10537-AAB	IEEE 802.11ac WiFi (40MHz, MCS3, 99pc duty cycle)	X	5.11	66.64	16.22	0.00	150.0	± 9.6 %
		Y	5.61	69.80	19.29		150.0	
		Z	5.34	67.34	17.08		150.0	
10538-AAB	IEEE 802.11ac WiFi (40MHz, MCS4, 99pc duty cycle)	X	5.18	66.60	16.24	0.00	150.0	± 9.6 %
		Y	5.64	69.56	19.20		150.0	
		Z	5.42	67.32	17.10		150.0	
10540-AAB	IEEE 802.11ac WiFi (40MHz, MCS6, 99pc duty cycle)	X	5.11	66.56	16.24	0.00	150.0	± 9.6 %
		Y	5.52	69.41	19.17		150.0	
		Z	5.36	67.39	17.16		150.0	

10541-AAB	IEEE 802.11ac WiFi (40MHz, MCS7, 99pc duty cycle)	X	5.10	66.48	16.18	0.00	150.0	± 9.6 %
		Y	5.45	69.13	19.01		150.0	
		Z	5.31	67.18	17.05		150.0	
10542-AAB	IEEE 802.11ac WiFi (40MHz, MCS8, 99pc duty cycle)	X	5.25	66.58	16.25	0.00	150.0	± 9.6 %
		Y	5.63	69.21	19.03		150.0	
		Z	5.47	67.22	17.07		150.0	
10543-AAB	IEEE 802.11ac WiFi (40MHz, MCS9, 99pc duty cycle)	X	5.32	66.66	16.31	0.00	150.0	± 9.6 %
		Y	5.73	69.34	19.11		150.0	
		Z	5.56	67.29	17.12		150.0	
10544-AAB	IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle)	X	5.47	66.61	16.18	0.00	150.0	± 9.6 %
		Y	5.78	68.80	18.70		150.0	
		Z	5.62	67.17	16.94		150.0	
10545-AAB	IEEE 802.11ac WiFi (80MHz, MCS1, 99pc duty cycle)	X	5.64	67.03	16.35	0.00	150.0	± 9.6 %
		Y	6.22	70.04	19.24		150.0	
		Z	5.88	67.78	17.18		150.0	
10546-AAB	IEEE 802.11ac WiFi (80MHz, MCS2, 99pc duty cycle)	X	5.50	66.73	16.21	0.00	150.0	± 9.6 %
		Y	5.87	69.11	18.81		150.0	
		Z	5.72	67.47	17.05		150.0	
10547-AAB	IEEE 802.11ac WiFi (80MHz, MCS3, 99pc duty cycle)	X	5.58	66.84	16.26	0.00	150.0	± 9.6 %
		Y	6.07	69.60	19.03		150.0	
		Z	5.80	67.54	17.07		150.0	
10548-AAB	IEEE 802.11ac WiFi (80MHz, MCS4, 99pc duty cycle)	X	5.71	67.41	16.53	0.00	150.0	± 9.6 %
		Y	6.85	72.09	20.16		150.0	
		Z	6.31	69.26	17.88		150.0	
10550-AAB	IEEE 802.11ac WiFi (80MHz, MCS6, 99pc duty cycle)	X	5.56	66.91	16.32	0.00	150.0	± 9.6 %
		Y	6.17	70.09	19.30		150.0	
		Z	5.75	67.51	17.07		150.0	
10551-AAB	IEEE 802.11ac WiFi (80MHz, MCS7, 99pc duty cycle)	X	5.49	66.70	16.17	0.00	150.0	± 9.6 %
		Y	5.87	69.09	18.78		150.0	
		Z	5.73	67.47	17.01		150.0	
10552-AAB	IEEE 802.11ac WiFi (80MHz, MCS8, 99pc duty cycle)	X	5.48	66.73	16.19	0.00	150.0	± 9.6 %
		Y	5.80	68.94	18.71		150.0	
		Z	5.63	67.23	16.91		150.0	
10553-AAB	IEEE 802.11ac WiFi (80MHz, MCS9, 99pc duty cycle)	X	5.53	66.68	16.19	0.00	150.0	± 9.6 %
		Y	5.82	68.77	18.64		150.0	
		Z	5.71	67.24	16.94		150.0	
10554-AAC	IEEE 802.11ac WiFi (160MHz, MCS0, 99pc duty cycle)	X	5.89	66.95	16.26	0.00	150.0	± 9.6 %
		Y	6.24	68.99	18.62		150.0	
		Z	6.04	67.51	16.99		150.0	
10555-AAC	IEEE 802.11ac WiFi (160MHz, MCS1, 99pc duty cycle)	X	5.98	67.17	16.36	0.00	150.0	± 9.6 %
		Y	6.47	69.63	18.91		150.0	
		Z	6.21	67.92	17.16		150.0	
10556-AAC	IEEE 802.11ac WiFi (160MHz, MCS2, 99pc duty cycle)	X	6.02	67.28	16.41	0.00	150.0	± 9.6 %
		Y	6.51	69.75	18.95		150.0	
		Z	6.22	67.93	17.16		150.0	
10557-AAC	IEEE 802.11ac WiFi (160MHz, MCS3, 99pc duty cycle)	X	5.97	67.15	16.36	0.00	150.0	± 9.6 %
		Y	6.36	69.28	18.75		150.0	
		Z	6.18	67.81	17.12		150.0	



10558-AAC	IEEE 802.11ac WiFi (160MHz, MCS4, 99pc duty cycle)	X	5.98	67.21	16.40	0.00	150.0	± 9.6 %
		Y	6.39	69.41	18.83		150.0	
		Z	6.24	68.02	17.24		150.0	
10560-AAC	IEEE 802.11ac WiFi (160MHz, MCS6, 99pc duty cycle)	X	6.00	67.14	16.40	0.00	150.0	± 9.6 %
		Y	6.37	69.22	18.77		150.0	
		Z	6.21	67.77	17.16		150.0	
10561-AAC	IEEE 802.11ac WiFi (160MHz, MCS7, 99pc duty cycle)	X	5.94	67.12	16.43	0.00	150.0	± 9.6 %
		Y	6.34	69.36	18.89		150.0	
		Z	6.14	67.80	17.21		150.0	
10562-AAC	IEEE 802.11ac WiFi (160MHz, MCS8, 99pc duty cycle)	X	5.98	67.28	16.51	0.00	150.0	± 9.6 %
		Y	6.39	69.51	18.95		150.0	
		Z	6.32	68.34	17.48		150.0	
10563-AAC	IEEE 802.11ac WiFi (160MHz, MCS9, 99pc duty cycle)	X	6.09	67.26	16.46	0.00	150.0	± 9.6 %
		Y	7.38	71.96	20.06		150.0	
		Z	6.72	69.10	17.80		150.0	
10564-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 99pc duty cycle)	X	4.84	67.04	16.50	0.46	150.0	± 9.6 %
		Y	5.12	69.74	19.39		150.0	
		Z	5.00	67.48	17.32		150.0	
10565-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 99pc duty cycle)	X	5.03	67.42	16.79	0.46	150.0	± 9.6 %
		Y	5.34	70.19	19.69		150.0	
		Z	5.25	67.95	17.64		150.0	
10566-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 99pc duty cycle)	X	4.87	67.24	16.60	0.46	150.0	± 9.6 %
		Y	5.20	70.18	19.61		150.0	
		Z	5.09	67.84	17.49		150.0	
10567-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 99pc duty cycle)	X	4.90	67.58	16.94	0.46	150.0	± 9.6 %
		Y	5.28	70.87	20.16		150.0	
		Z	5.13	68.31	17.89		150.0	
10568-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 99pc duty cycle)	X	4.77	67.00	16.37	0.46	150.0	± 9.6 %
		Y	5.10	69.94	19.37		150.0	
		Z	4.99	67.60	17.25		150.0	
10569-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 99pc duty cycle)	X	4.88	67.78	17.05	0.46	150.0	± 9.6 %
		Y	5.31	71.34	20.44		150.0	
		Z	5.08	68.42	17.97		150.0	
10570-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 99pc duty cycle)	X	4.89	67.60	16.97	0.46	150.0	± 9.6 %
		Y	5.28	70.91	20.21		150.0	
		Z	5.11	68.22	17.87		150.0	
10571-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	1.29	64.06	15.41	0.46	130.0	± 9.6 %
		Y	39.01	176.86	60.78		130.0	
		Z	1.31	69.79	20.44		130.0	
10572-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	1.30	64.47	15.68	0.46	130.0	± 9.6 %
		Y	100.00	206.48	67.90		130.0	
		Z	1.37	71.27	21.27		130.0	
10573-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 90pc duty cycle)	X	1.13	72.95	19.31	0.46	130.0	± 9.6 %
		Y	100.00	531.14	193.89		130.0	
		Z	100.00	192.03	57.17		130.0	
10574-AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 90pc duty cycle)	X	1.29	68.03	17.69	0.46	130.0	± 9.6 %
		Y	100.00	237.32	79.79		130.0	
		Z	4.23	102.32	34.00		130.0	

10575-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle)	X	4.61	66.75	16.46	0.46	130.0	± 9.6 %
		Y	4.89	69.69	19.60		130.0	
		Z	4.78	67.29	17.42		130.0	
10576-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle)	X	4.64	66.95	16.54	0.46	130.0	± 9.6 %
		Y	4.95	70.06	19.77		130.0	
		Z	4.81	67.49	17.50		130.0	
10577-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 90pc duty cycle)	X	4.80	67.16	16.68	0.46	130.0	± 9.6 %
		Y	5.13	70.24	19.85		130.0	
		Z	5.03	67.79	17.66		130.0	
10578-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 90pc duty cycle)	X	4.70	67.28	16.77	0.46	130.0	± 9.6 %
		Y	5.09	70.76	20.18		130.0	
		Z	4.93	68.04	17.82		130.0	
10579-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 90pc duty cycle)	X	4.47	66.55	16.09	0.46	130.0	± 9.6 %
		Y	4.78	69.67	19.29		130.0	
		Z	4.68	67.27	17.10		130.0	
10580-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 90pc duty cycle)	X	4.50	66.61	16.11	0.46	130.0	± 9.6 %
		Y	4.83	69.78	19.33		130.0	
		Z	4.73	67.29	17.11		130.0	
10581-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 90pc duty cycle)	X	4.62	67.36	16.75	0.46	130.0	± 9.6 %
		Y	5.05	71.16	20.34		130.0	
		Z	4.84	68.14	17.81		130.0	
10582-AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 90pc duty cycle)	X	4.40	66.35	15.90	0.46	130.0	± 9.6 %
		Y	4.70	69.39	19.04		130.0	
		Z	4.63	67.01	16.87		130.0	
10583-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle)	X	4.61	66.75	16.46	0.46	130.0	± 9.6 %
		Y	4.89	69.69	19.60		130.0	
		Z	4.78	67.29	17.42		130.0	
10584-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 90pc duty cycle)	X	4.64	66.95	16.54	0.46	130.0	± 9.6 %
		Y	4.95	70.06	19.77		130.0	
		Z	4.81	67.49	17.50		130.0	
10585-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 90pc duty cycle)	X	4.80	67.16	16.68	0.46	130.0	± 9.6 %
		Y	5.13	70.24	19.85		130.0	
		Z	5.03	67.79	17.66		130.0	
10586-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 90pc duty cycle)	X	4.70	67.28	16.77	0.46	130.0	± 9.6 %
		Y	5.09	70.76	20.18		130.0	
		Z	4.93	68.04	17.82		130.0	
10587-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 90pc duty cycle)	X	4.47	66.55	16.09	0.46	130.0	± 9.6 %
		Y	4.78	69.67	19.29		130.0	
		Z	4.68	67.27	17.10		130.0	
10588-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 90pc duty cycle)	X	4.50	66.61	16.11	0.46	130.0	± 9.6 %
		Y	4.83	69.78	19.33		130.0	
		Z	4.73	67.29	17.11		130.0	
10589-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 90pc duty cycle)	X	4.62	67.36	16.75	0.46	130.0	± 9.6 %
		Y	5.05	71.16	20.34		130.0	
		Z	4.84	68.14	17.81		130.0	
10590-AAB	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 90pc duty cycle)	X	4.40	66.35	15.90	0.46	130.0	± 9.6 %
		Y	4.70	69.39	19.04		130.0	
		Z	4.63	67.01	16.87		130.0	

10591-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	X	4.77	66.84	16.58	0.46	130.0	± 9.6 %
		Y	5.01	69.51	19.56		130.0	
		Z	4.92	67.30	17.48		130.0	
10592-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle)	X	4.89	67.12	16.70	0.46	130.0	± 9.6 %
		Y	5.17	69.92	19.71		130.0	
		Z	5.09	67.67	17.62		130.0	
10593-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS2, 90pc duty cycle)	X	4.81	67.00	16.57	0.46	130.0	± 9.6 %
		Y	5.10	69.86	19.61		130.0	
		Z	5.02	67.60	17.51		130.0	
10594-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS3, 90pc duty cycle)	X	4.86	67.16	16.72	0.46	130.0	± 9.6 %
		Y	5.16	70.08	19.80		130.0	
		Z	5.07	67.77	17.67		130.0	
10595-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS4, 90pc duty cycle)	X	4.83	67.15	16.64	0.46	130.0	± 9.6 %
		Y	5.15	70.14	19.75		130.0	
		Z	5.04	67.74	17.58		130.0	
10596-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS5, 90pc duty cycle)	X	4.76	67.11	16.63	0.46	130.0	± 9.6 %
		Y	5.09	70.21	19.81		130.0	
		Z	4.98	67.77	17.60		130.0	
10597-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS6, 90pc duty cycle)	X	4.71	66.99	16.49	0.46	130.0	± 9.6 %
		Y	5.04	70.07	19.66		130.0	
		Z	4.93	67.68	17.49		130.0	
10598-AAB	IEEE 802.11n (HT Mixed, 20MHz, MCS7, 90pc duty cycle)	X	4.70	67.18	16.73	0.46	130.0	± 9.6 %
		Y	5.05	70.51	20.07		130.0	
		Z	4.92	67.97	17.79		130.0	
10599-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	5.45	67.31	16.83	0.46	130.0	± 9.6 %
		Y	5.92	70.28	19.80		130.0	
		Z	5.63	67.84	17.64		130.0	
10600-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS1, 90pc duty cycle)	X	5.54	67.64	16.98	0.46	130.0	± 9.6 %
		Y	6.41	71.93	20.55		130.0	
		Z	5.89	68.70	18.04		130.0	
10601-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS2, 90pc duty cycle)	X	5.45	67.44	16.89	0.46	130.0	± 9.6 %
		Y	5.92	70.44	19.87		130.0	
		Z	5.71	68.21	17.81		130.0	
10602-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS3, 90pc duty cycle)	X	5.54	67.48	16.83	0.46	130.0	± 9.6 %
		Y	6.08	70.62	19.84		130.0	
		Z	5.80	68.19	17.71		130.0	
10603-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS4, 90pc duty cycle)	X	5.61	67.75	17.10	0.46	130.0	± 9.6 %
		Y	6.25	71.29	20.32		130.0	
		Z	5.86	68.45	17.97		130.0	
10604-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS5, 90pc duty cycle)	X	5.49	67.39	16.90	0.46	130.0	± 9.6 %
		Y	6.11	70.89	20.12		130.0	
		Z	5.62	67.77	17.62		130.0	
10605-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS6, 90pc duty cycle)	X	5.54	67.52	16.97	0.46	130.0	± 9.6 %
		Y	6.18	71.09	20.21		130.0	
		Z	5.81	68.36	17.92		130.0	
10606-AAB	IEEE 802.11n (HT Mixed, 40MHz, MCS7, 90pc duty cycle)	X	5.33	67.01	16.57	0.46	130.0	± 9.6 %
		Y	5.76	69.87	19.47		130.0	
		Z	5.50	67.51	17.36		130.0	

10607-AAB	IEEE 802.11ac WiFi (20MHz, MCS0, 90pc duty cycle)	X	4.61	66.18	16.22	0.46	130.0	± 9.6 %
		Y	4.99	69.45	19.52		130.0	
		Z	4.80	66.76	17.19		130.0	
10608-AAB	IEEE 802.11ac WiFi (20MHz, MCS1, 90pc duty cycle)	X	4.75	66.49	16.35	0.46	130.0	± 9.6 %
		Y	5.19	69.93	19.71		130.0	
		Z	5.00	67.21	17.36		130.0	
10609-AAB	IEEE 802.11ac WiFi (20MHz, MCS2, 90pc duty cycle)	X	4.65	66.34	16.19	0.46	130.0	± 9.6 %
		Y	5.10	69.85	19.59		130.0	
		Z	4.89	67.08	17.22		130.0	
10610-AAB	IEEE 802.11ac WiFi (20MHz, MCS3, 90pc duty cycle)	X	4.69	66.48	16.34	0.46	130.0	± 9.6 %
		Y	5.16	70.05	19.78		130.0	
		Z	4.95	67.26	17.39		130.0	
10611-AAB	IEEE 802.11ac WiFi (20MHz, MCS4, 90pc duty cycle)	X	4.61	66.29	16.20	0.46	130.0	± 9.6 %
		Y	5.06	69.84	19.63		130.0	
		Z	4.86	67.06	17.24		130.0	
10612-AAB	IEEE 802.11ac WiFi (20MHz, MCS5, 90pc duty cycle)	X	4.60	66.41	16.24	0.46	130.0	± 9.6 %
		Y	5.10	70.22	19.79		130.0	
		Z	4.88	67.27	17.31		130.0	
10613-AAB	IEEE 802.11ac WiFi (20MHz, MCS6, 90pc duty cycle)	X	4.60	66.25	16.09	0.46	130.0	± 9.6 %
		Y	5.06	69.85	19.53		130.0	
		Z	4.88	67.13	17.18		130.0	
10614-AAB	IEEE 802.11ac WiFi (20MHz, MCS7, 90pc duty cycle)	X	4.56	66.43	16.31	0.46	130.0	± 9.6 %
		Y	5.06	70.34	19.95		130.0	
		Z	4.83	67.37	17.45		130.0	
10615-AAB	IEEE 802.11ac WiFi (20MHz, MCS8, 90pc duty cycle)	X	4.61	66.17	15.99	0.46	130.0	± 9.6 %
		Y	5.04	69.57	19.32		130.0	
		Z	4.86	66.85	16.99		130.0	
10616-AAB	IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle)	X	5.25	66.49	16.40	0.46	130.0	± 9.6 %
		Y	5.64	69.19	19.26		130.0	
		Z	5.47	67.18	17.30		130.0	
10617-AAB	IEEE 802.11ac WiFi (40MHz, MCS1, 90pc duty cycle)	X	5.29	66.60	16.44	0.46	130.0	± 9.6 %
		Y	5.83	69.82	19.54		130.0	
		Z	5.57	67.45	17.40		130.0	
10618-AAB	IEEE 802.11ac WiFi (40MHz, MCS2, 90pc duty cycle)	X	5.20	66.66	16.48	0.46	130.0	± 9.6 %
		Y	5.70	69.84	19.59		130.0	
		Z	5.44	67.45	17.43		130.0	
10619-AAB	IEEE 802.11ac WiFi (40MHz, MCS3, 90pc duty cycle)	X	5.23	66.52	16.34	0.46	130.0	± 9.6 %
		Y	5.73	69.64	19.40		130.0	
		Z	5.46	67.24	17.25		130.0	
10620-AAB	IEEE 802.11ac WiFi (40MHz, MCS4, 90pc duty cycle)	X	5.29	66.51	16.38	0.46	130.0	± 9.6 %
		Y	5.75	69.42	19.33		130.0	
		Z	5.55	67.25	17.30		130.0	
10621-AAB	IEEE 802.11ac WiFi (40MHz, MCS5, 90pc duty cycle)	X	5.30	66.59	16.54	0.46	130.0	± 9.6 %
		Y	5.69	69.32	19.43		130.0	
		Z	5.53	67.33	17.46		130.0	
10622-AAB	IEEE 802.11ac WiFi (40MHz, MCS6, 90pc duty cycle)	X	5.29	66.68	16.58	0.46	130.0	± 9.6 %
		Y	5.69	69.47	19.50		130.0	
		Z	5.59	67.66	17.62		130.0	