

Appendix D

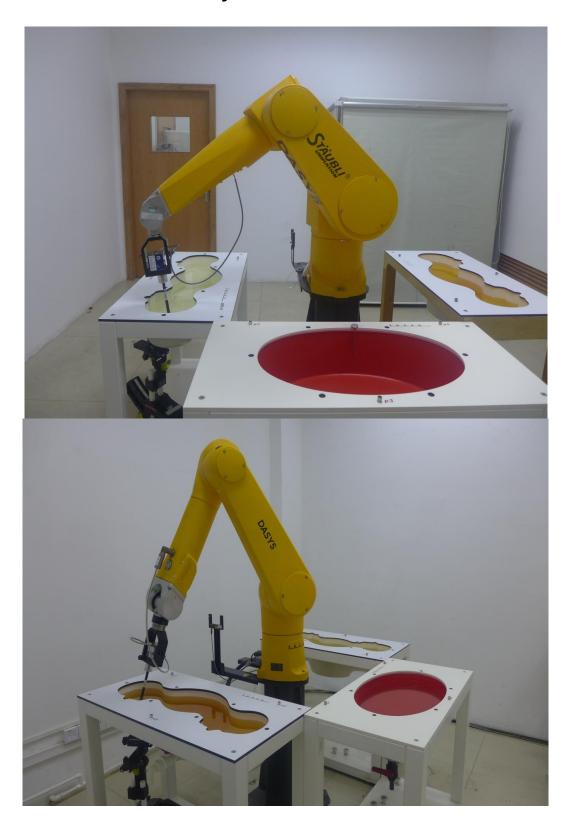
Photographs

- 1. SAR measurement System
- 2. Photographs of Tissue Simulate Liquid
- 3. Photographs of EUT test position
- 4. EUT Constructional Details
- 5. Serial Number of EUT

Report No.: E5/2018/80016




1. SAR measurement System




Report No.: E5/2018/80016



2. Photographs of Tissue Simulate Liquid

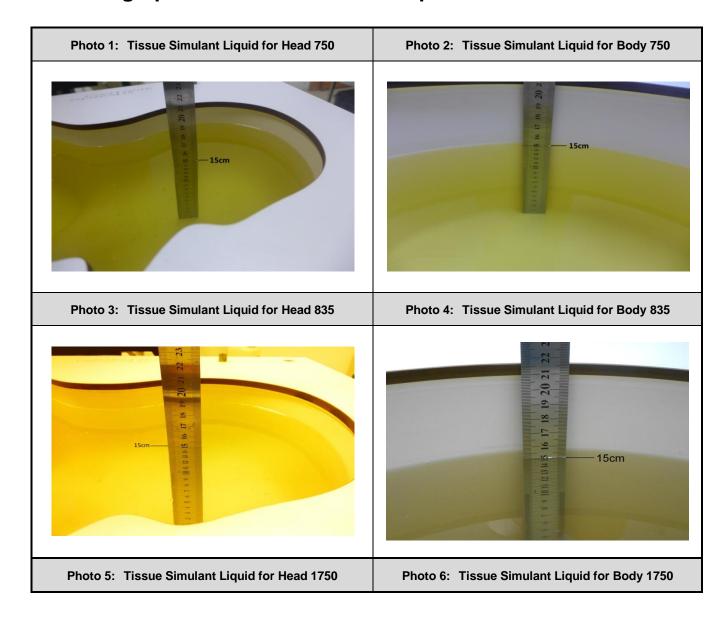




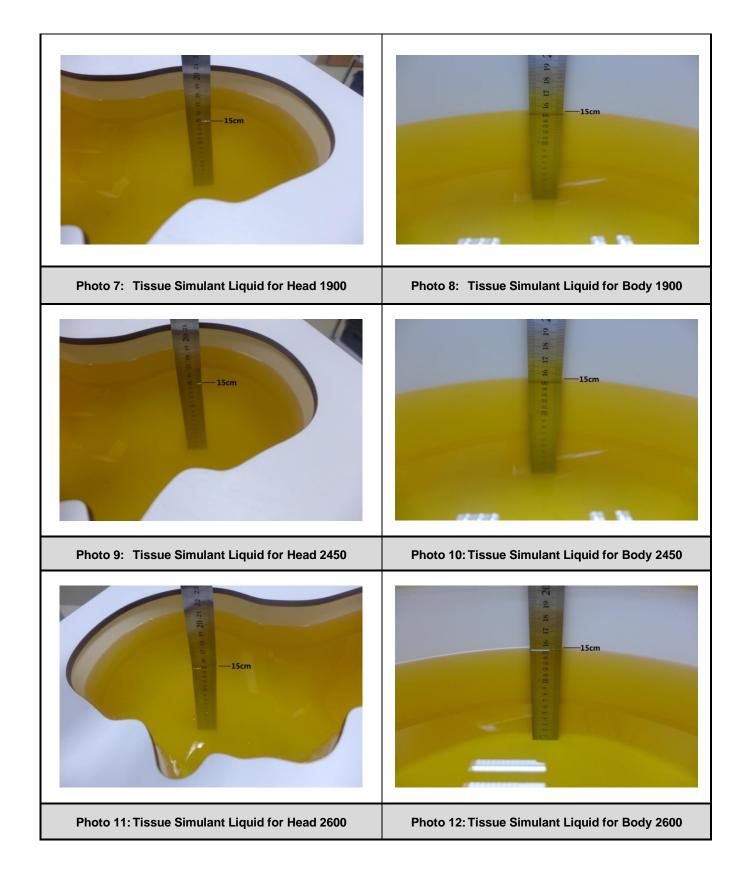





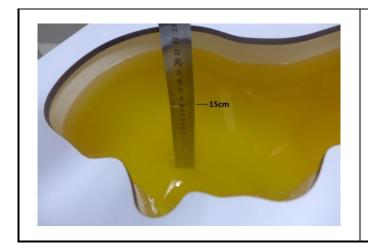








Photo 13: Tissue Simulant Liquid for Head 5G

Photo 14: Tissue Simulant Liquid for Body 5G





3. Photographs of EUT test position

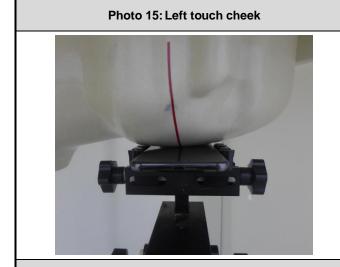


Photo 17: Right touch cheek




Photo 19: Front side 15mm



Photo 16: Left tilted 15 degree




Photo 18: Right tilted 15 degree




Photo 20: Back side 15mm








Photo 21: Front side 10mm

Photo 22: Back side 10mm

Photo 23: Left side 10mm

Photo 23: Left side 10mm






Photo 25: Top side 10mm



Photo 26: Bottom side 10mm





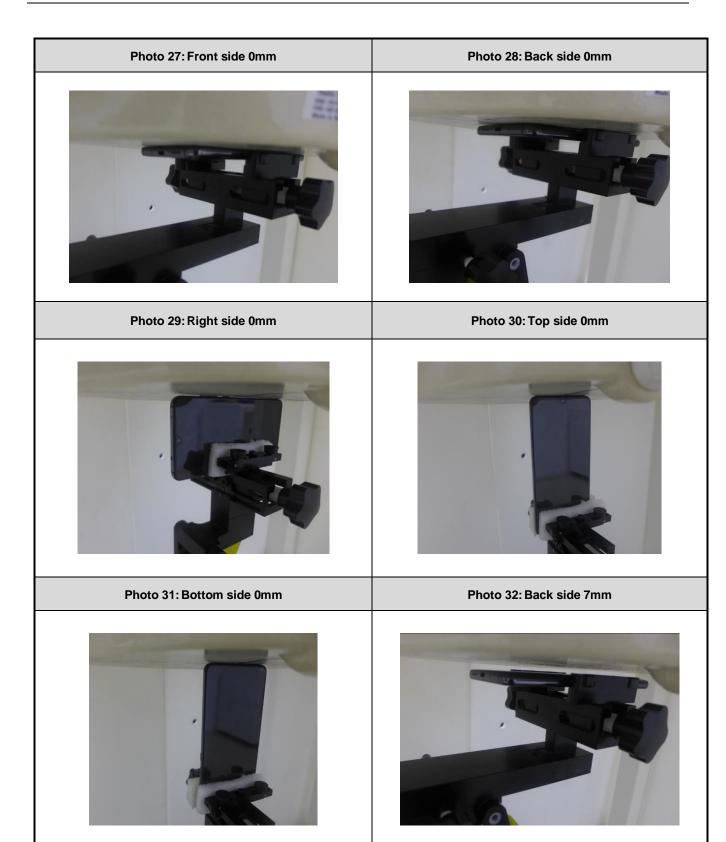







Photo 33: Bottom side 9mm

Photo 34: Back side with protected cove 15mm

Photo 35: Bottom side with protected cove 10mm

Photo 36: Back side with protected cove 0mm





4. EUT Constructional Details

Photo 37: Front View	Photo 38: Back View
Photo 39: Accessory	NA
## ## ## ## ## ## ## ## ## ## ## ## ##	NA