


SAR Dipole


Performance Measurement Report


ISSUED BY
Shenzhen BALUN Technology Co., Ltd.



FOR
Validation Dipoles

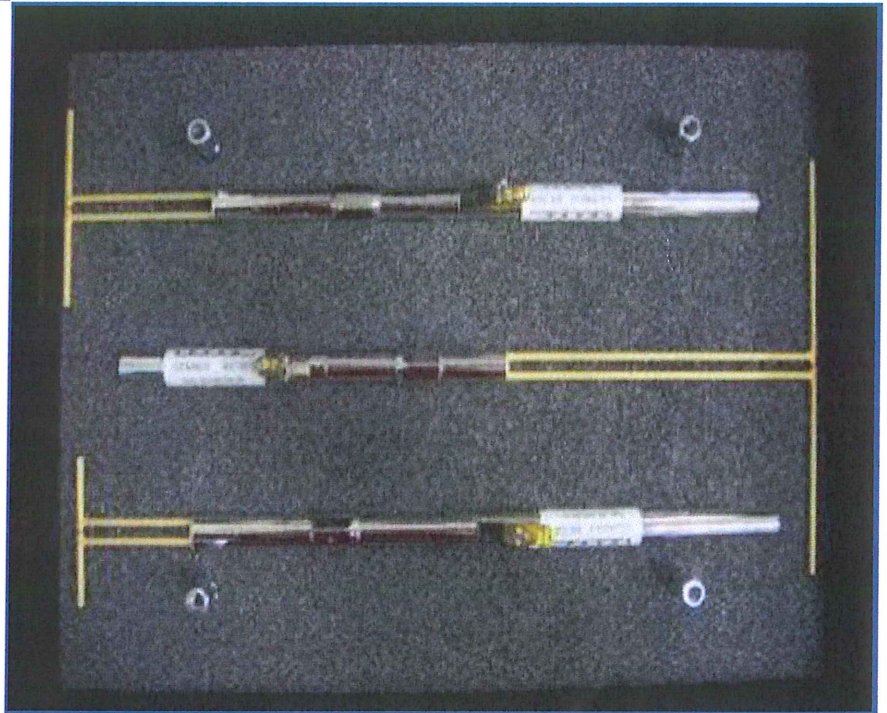

Tested by: 
Zong Liyao
(Engineer)

Approved by: 
Liao Jianming
(Technical Director)

Report No.: LW-SZ1860070-701
EUT Type: SAR Validation Dipole
Model Name: D750V3, D835V2, D1750V2
D1900V2, D2450V2
D2600V2, D5GHzV2
Brand Name: Speag

Test Conclusion: Pass
Test Date: Mar. 16, 2018 ~ Jul. 05, 2018
Date of Issue: Jul. 08, 2018

NOTE: This test report can be duplicated completely for the legal use with the approval of the applicant; it shall not be reproduced except in full, without the written approval of Shenzhen BALUN Technology Co., Ltd. BALUN Laboratory. Any objections should be raised within thirty days from the date of issue. To validate the report, please contact us.



1 GENERAL INFORMATION

1.1 Introduction

This document contains a summary of the requirements set forth by the IEEE 1528, FCC KDB 865664 D01 for reference dipoles used for SAR measurement system validations. Instead of the typical annual calibration recommended by measurement standards, the reference dipoles were demonstrated that the SAR target, impedance and return loss have remain stable, so the longer calibration interval is acceptable.

1.2 General Description for Equipment under Test (EUT)

| | |
|--------------|--------------------------|
| EUT Type | DASY 5 Reference Dipoles |
| Manufacturer | Speag |

| Parameter | EUT 1 | EUT 2 | EUT 3 | EUT 4 | EUT 5 | EUT 6 | EUT 7 |
|-------------------------------|-----------|-----------|-----------|-----------|-----------|-----------|-----------|
| Model | D750V3 | D835V2 | D1750V2 | D1900V2 | D2450V2 | D2600V2 | D5GHzV2 |
| Frequency | 750 MHz | 835 MHz | 1750 MHz | 1900 MHz | 2450 MHz | 2600 MHz | 5GHz-6GHz |
| Serial Number | SN 1055 | SN 4d187 | SN 1130 | SN 5d193 | SN 952 | SN 1095 | SN 1200 |
| Product Condition (New/ Used) | Used | Used | Used | Used | Used | Used | Used |
| Last Cal. Date | 2017/6/26 | 2017/6/26 | 2017/7/1 | 2017/6/30 | 2017/3/21 | 2017/7/10 | 2017/6/29 |
| Current meas. Date | 2018/6/24 | 2018/6/24 | 2018/6/26 | 2018/6/26 | 2018/3/16 | 2018/7/5 | 2018/6/25 |



1.3 Test Equipment List

| Description | Manufacturer | Model | Serial No. | Cal. Date | Cal. Due |
|------------------------------|--------------|-----------|-----------------|------------|------------|
| PC | Dell | N/A | N/A | N/A | N/A |
| E-Field Probe | Speag | EX3DV4 | SN: 7340 | 2018/01/11 | 2019/01/10 |
| E-Field Probe | Speag | ES3DV3 | SN: 3110 | 2017/08/02 | 2018/08/01 |
| Data Acquisition Electronics | Speag | DAE4 | SN: 1454 | 2018/01/11 | 2019/01/11 |
| Signal Generator | R&S | SMBV100A | 260592 | 2018/06/15 | 2019/06/14 |
| Power Meter | Agilent | E4419B | GB40201833 | 2017/11/02 | 2018/11/01 |
| Power Sensor | Agilent | E9300A | MY41498012 | 2017/11/02 | 2018/11/01 |
| Power Sensor | Agilent | E9300A | MY41499891 | 2017/11/02 | 2018/11/01 |
| Network Analyzer | Agilent | 5071C | MY46103472 | 2018/03/14 | 2019/03/13 |
| Thermometer | Elitech | RC-4HC | N/A | 2017/11/13 | 2018/11/12 |
| Dielectric Probe Kit | SATIMO | SCLMP | SN 25/13 OCPG56 | N/A | N/A |
| Phantom1 | Speag | SAM | SN: 1859 | N/A | N/A |
| Phantom2 | Speag | SAM | SN: 1857 | N/A | N/A |
| Power Amplifier | SATIMO | 6552B | 22374 | N/A | N/A |
| Attenuator | COM-MW | ZA-S1-31 | 1305003187 | N/A | N/A |
| Directional coupler | AA-MCS | AAMCS-UDC | 000272 | N/A | N/A |

1.4 EUT Photos

D750V3



D835V2



D1750V2



D1900V2



D2450V2



D2600V2



D5GHzV2





2 SIMULATING LIQUID VERIFICATION

| Liquid Type | Fre. (MHz) | Meas. Conductivity (σ) (S/m) | Meas. Permittivity (ϵ) | Target Conductivity (σ) (S/m) | Target Permittivity (ϵ) | Conductivity Tolerance (%) | Permittivity Tolerance (%) |
|-------------|------------|---------------------------------------|-----------------------------------|--|------------------------------------|----------------------------|----------------------------|
| Head | 750 | 0.91 | 40.53 | 0.893 | 41.94 | 1.90 | -3.36 |
| Body | 750 | 0.99 | 54.68 | 0.963 | 55.53 | 2.80 | -1.53 |
| Head | 835 | 0.89 | 40.78 | 0.90 | 41.50 | -1.11 | -1.73 |
| Body | 835 | 0.98 | 53.86 | 0.97 | 55.20 | 1.03 | -2.43 |
| Head | 1750 | 1.38 | 39.96 | 1.371 | 40.08 | 0.66 | -0.30 |
| Body | 1750 | 1.45 | 52.56 | 1.488 | 53.43 | -2.55 | -1.63 |
| Head | 1900 | 1.43 | 39.71 | 1.40 | 40.00 | 2.14 | -0.72 |
| Body | 1900 | 1.55 | 51.58 | 1.52 | 53.30 | 1.97 | -3.23 |
| Head | 2450 | 1.84 | 38.94 | 1.80 | 39.20 | 2.22 | -0.66 |
| Body | 2450 | 1.93 | 50.88 | 1.95 | 52.70 | -1.03 | -3.45 |
| Head | 2600 | 1.99 | 39.03 | 1.964 | 39.01 | 1.32 | 0.05 |
| Body | 2600 | 2.21 | 50.89 | 2.163 | 52.51 | 2.17 | -3.09 |
| Head | 5250 | 4.63 | 36.06 | 4.706 | 35.93 | -1.61 | 0.36 |
| Body | 5250 | 5.34 | 47.48 | 5.358 | 48.95 | -0.34 | -3.00 |
| Head | 5600 | 5.07 | 35.83 | 5.065 | 35.53 | 0.10 | 0.84 |
| Body | 5600 | 5.65 | 46.63 | 5.766 | 48.47 | -2.01 | -3.80 |
| Head | 5750 | 5.17 | 35.41 | 5.219 | 35.36 | -0.94 | 0.14 |
| Body | 5750 | 5.87 | 46.28 | 5.942 | 48.27 | -1.21 | -4.12 |



3 DIPOLE IMPEDANCE AND RETURN LOSS

The dipoles are designed to have low return loss when presented against a flat phantom at the specified distance. A Vector Network Analyser was used to perform a return loss measurement on the specific dipole when in the measurement location against the phantom and the distance was specified by the manufacturer with a special, low loss and low relative permittivity spacer.

The impedance was measured at the SMA-connector with the network analyser.

The measurement of verification with return loss should not deviate by more than 20% and minimum of 20 dB of the return loss, and the impedance (real or imaginary parts) should not deviate by more than 5 Ohms from the previous measurement using network analyzer.

Note:

The "Previous Meas." in the following table refer to dipoles or other equivalent RF sources calibration reports.




3.1 D750V3


RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|-----------------|-----------------------------------|-----------------------------------|-------------------------------|
| Return Loss(dB) | -30.728 | -29.563 | 3.7% |
| Impedance | 52.793 Ω - 3.016 $j\Omega$ | 51.740 Ω - 2.903 $j\Omega$ | 1.053 Ω (Real part) |

Return Loss

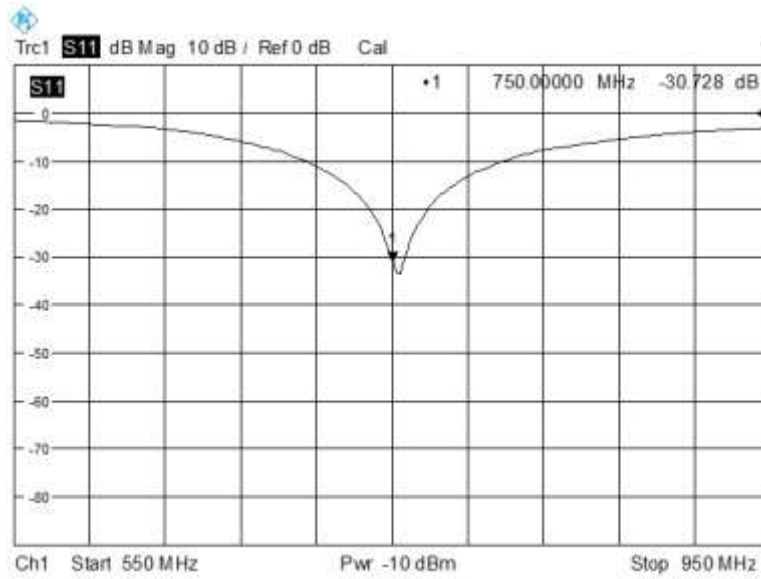


Impedance

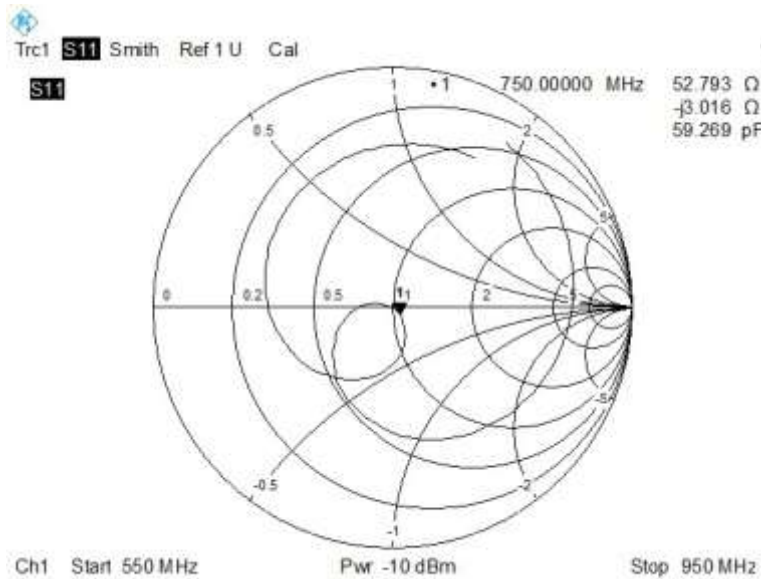


RETURN LOSS AND IMPEDANCE IN BODY LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|-----------------|-----------------------------------|-----------------------------------|-------------------------------|
| Return Loss(dB) | -30.881 | -29.870 | 3.4% |
| Impedance | 51.921 Ω - 3.131 $j\Omega$ | 49.994 Ω - 3.211 $j\Omega$ | 1.927 Ω (Real part) |

Return Loss

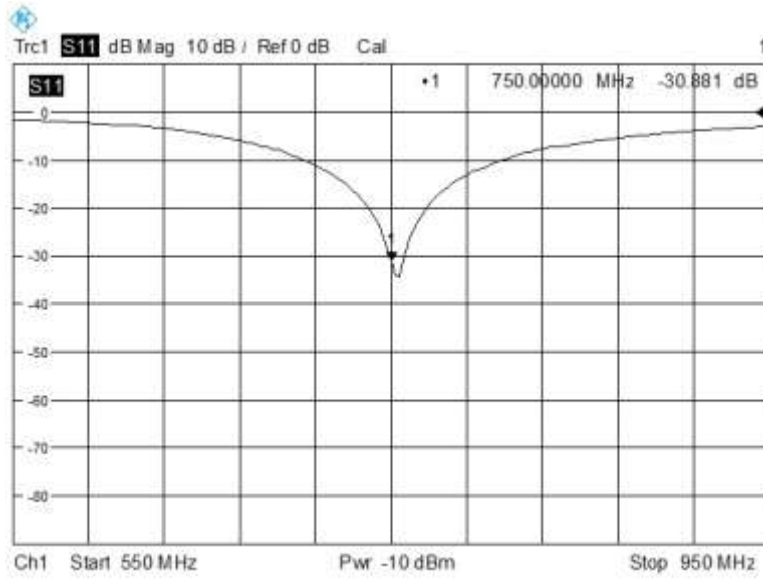

Impedance

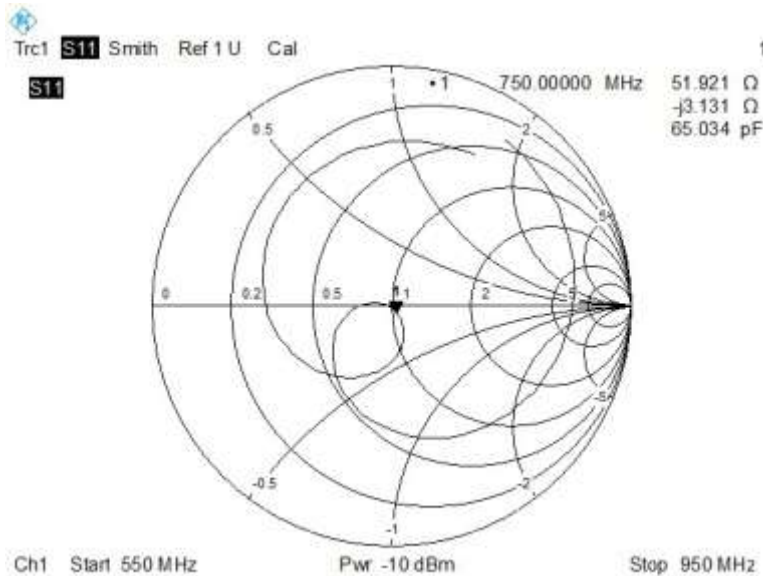




3.2 D835V2


RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|-----------------|---------------------------------------|---------------------------------------|------------------------------------|
| Return Loss(dB) | -29.391 | -30.413 | -3.4% |
| Impedance | 48.614 Ω - 2.557 j Ω | 48.617 Ω - 2.634 j Ω | 0.077 Ω (Imaginary part) |

Return Loss

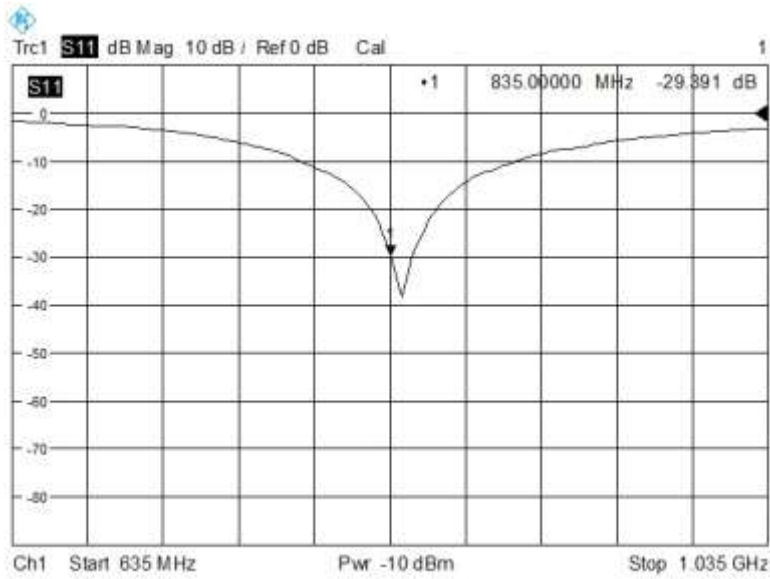

Impedance

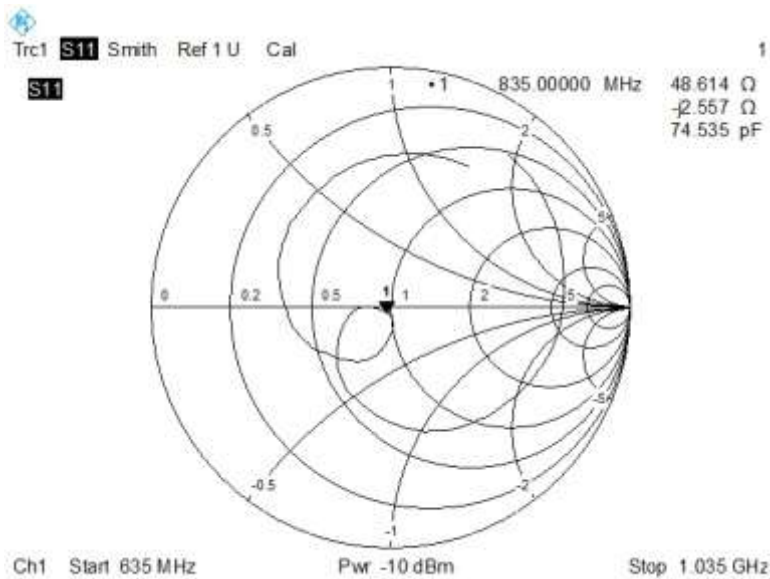





RETURN LOSS AND IMPEDANCE IN BODY LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|-----------------|-----------------------------------|-----------------------------------|--------------------------------|
| Return Loss(dB) | -25.430 | -24.862 | 2.3% |
| Impedance | 46.544 Ω - 3.507 $j\Omega$ | 45.749 Ω - 3.449 $j\Omega$ | -0.795 Ω (Real part) |

Return Loss

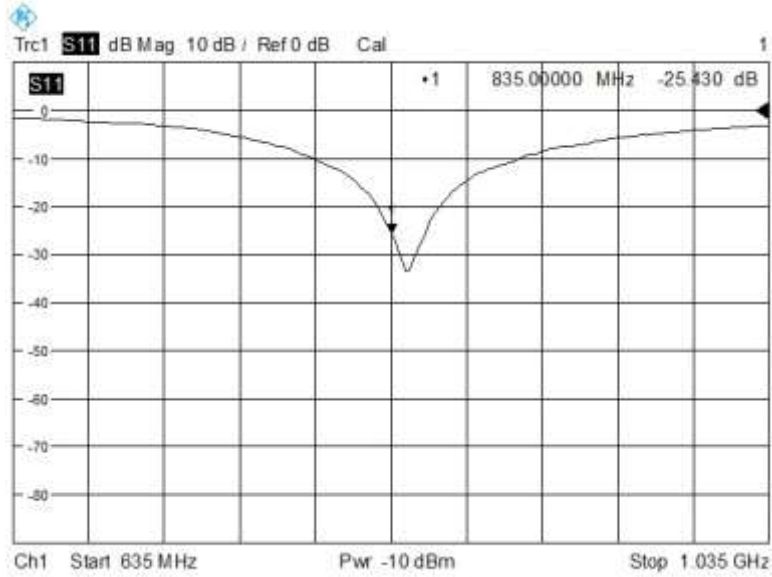

Impedance

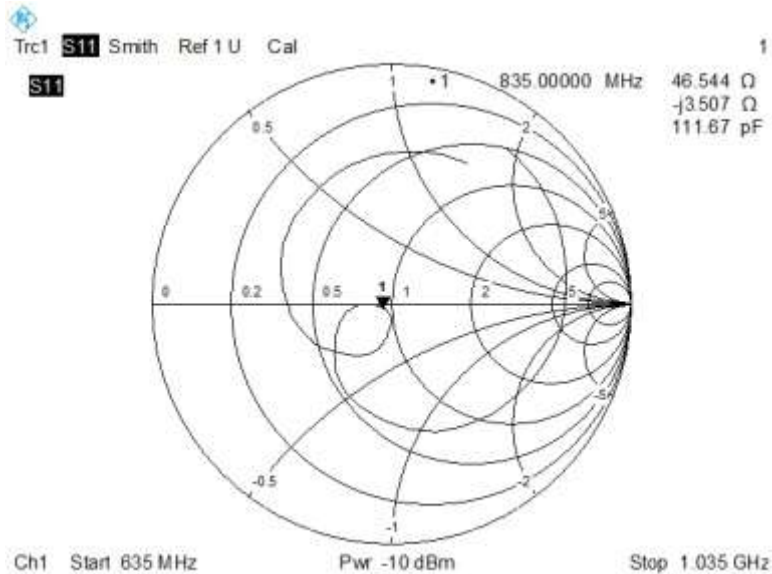


3.3 D1750V2


RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|-----------------|-----------------------------------|-----------------------------------|-------------------------------|
| Return Loss(dB) | -34.478 | -33.945 | 1.6% |
| Impedance | 48.643 Ω - 1.407 $j\Omega$ | 48.596 Ω - 1.396 $j\Omega$ | 0.047 Ω (Real part) |

Return Loss

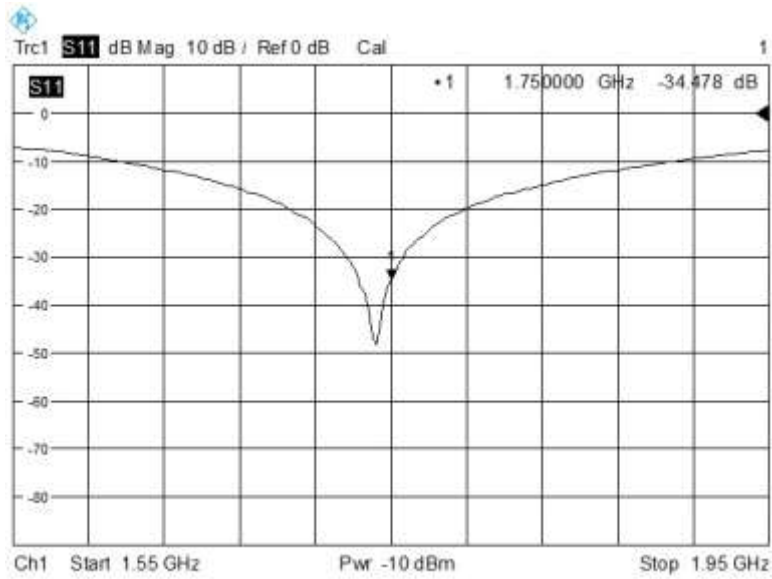


Impedance

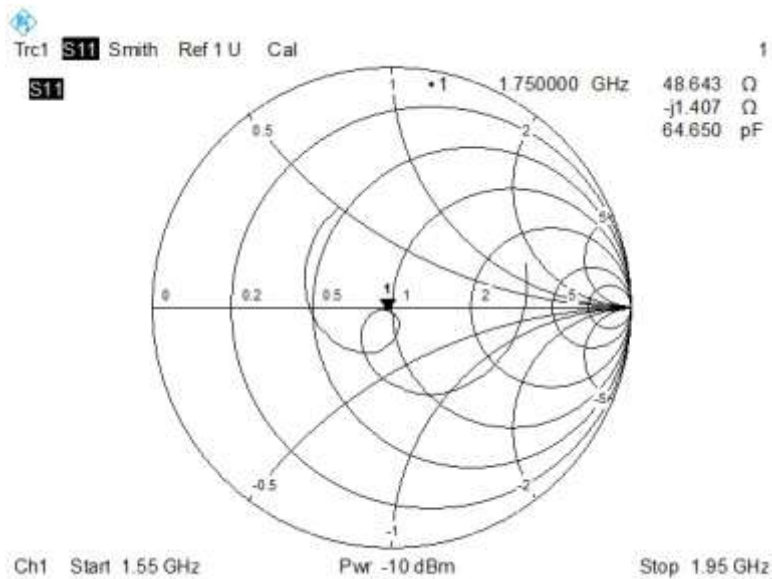


RETURN LOSS AND IMPEDANCE IN BODY LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|-----------------|---------------------------------------|---------------------------------------|-------------------------------|
| Return Loss(dB) | -27.872 | -27.463 | 1.5% |
| Impedance | 46.763 Ω + 0.612 j Ω | 45.981 Ω + 0.606 j Ω | 0.782 Ω (Real part) |

Return Loss

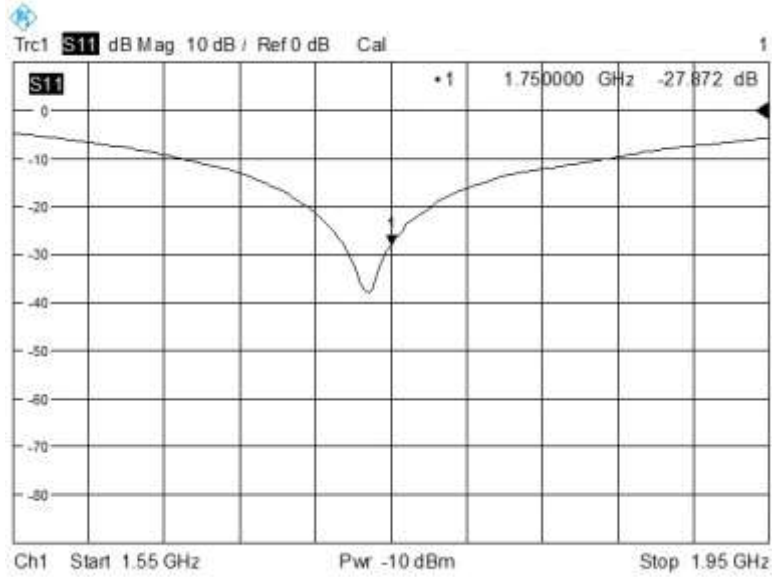

Impedance

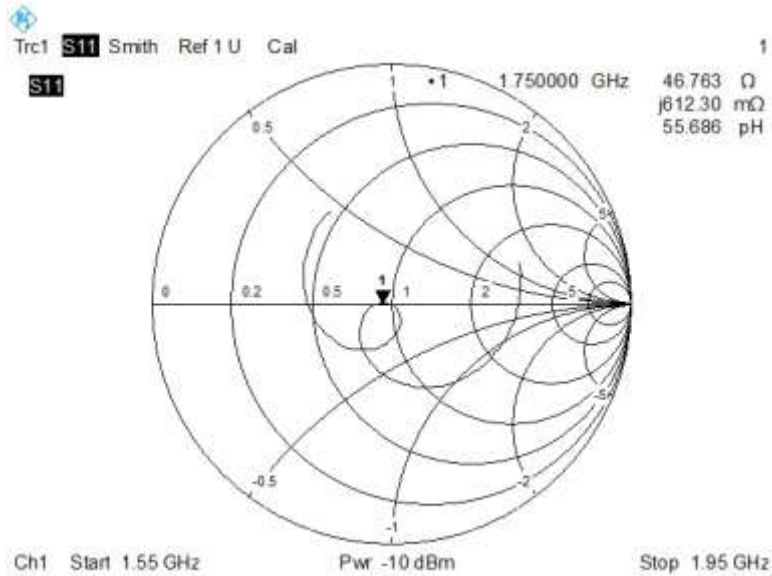




3.4 D1900V2


RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|-----------------|---------------------------------------|---------------------------------------|--------------------------------|
| Return Loss(dB) | -25.822 | -25.408 | 1.6% |
| Impedance | 48.893 Ω + 5.253 j Ω | 49.192 Ω + 5.268 j Ω | -0.299 Ω (Real part) |

Return Loss

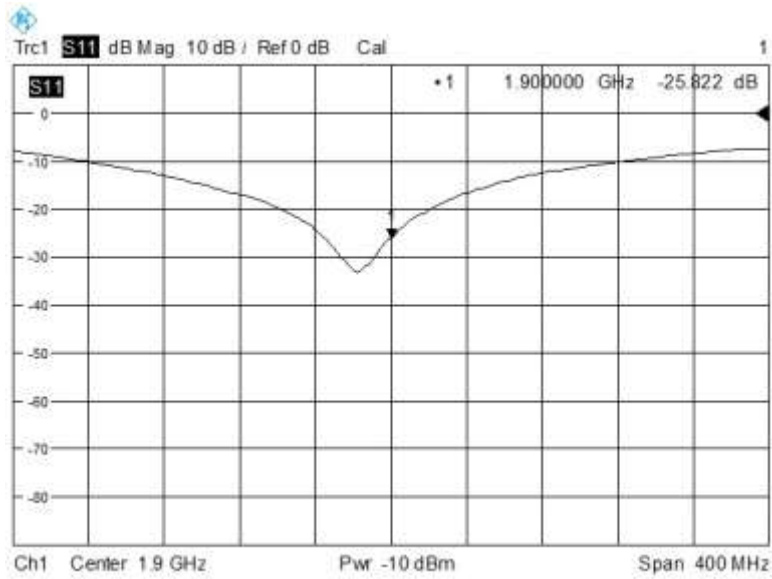


Impedance

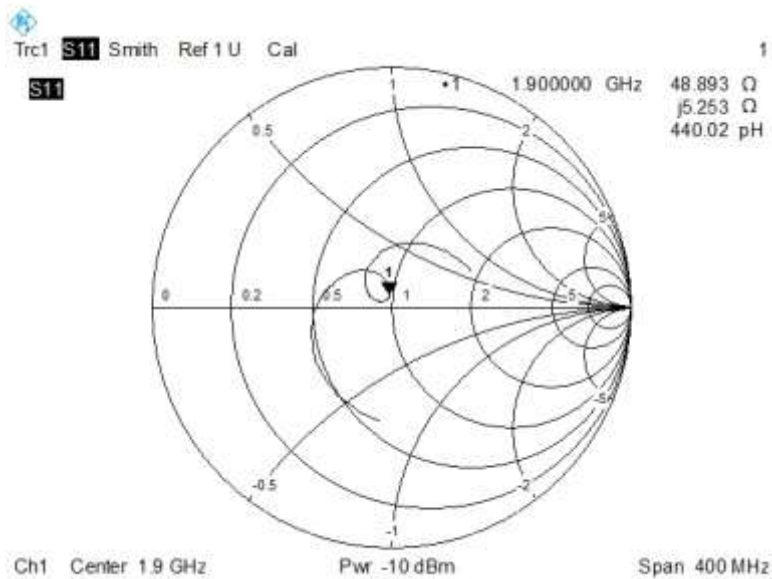


RETURN LOSS AND IMPEDANCE IN BODY LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|-----------------|---------------------------------------|---------------------------------------|-------------------------------|
| Return Loss(dB) | -24.513 | -24.883 | -1.5% |
| Impedance | 46.749 Ω + 4.221 j Ω | 46.585 Ω + 4.324 j Ω | 0.164 Ω (Real part) |

Return Loss

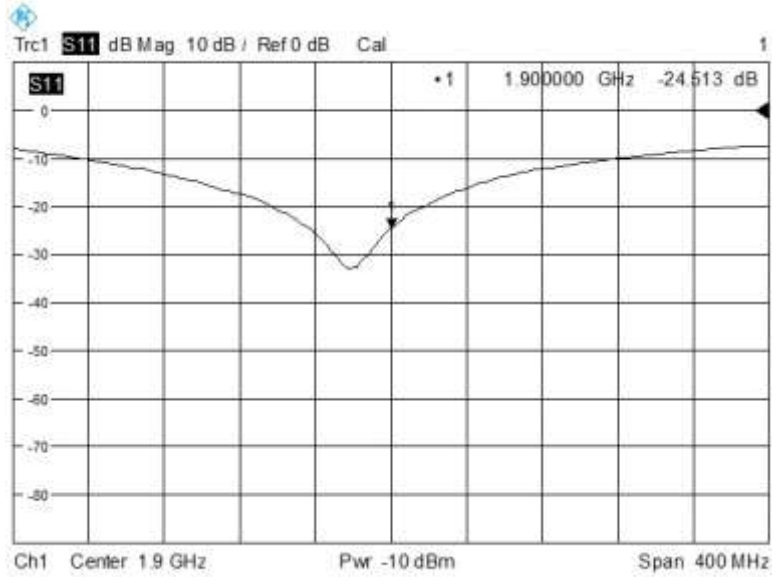

Impedance

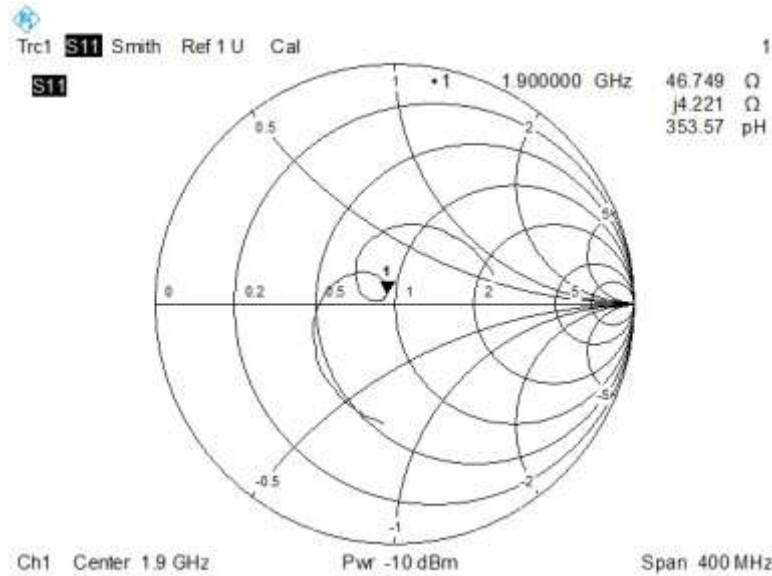




3.5 D2450V2


RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|------------------|----------------------------------|----------------------------------|------------------------------------|
| Return Loss (dB) | -28.271 | -24.261 | 16.5% |
| Impedance | 49.7 Ω + 1.669 j Ω | 52.0 Ω + 5.937 j Ω | 4.268 Ω (Imaginary part) |

Return Loss

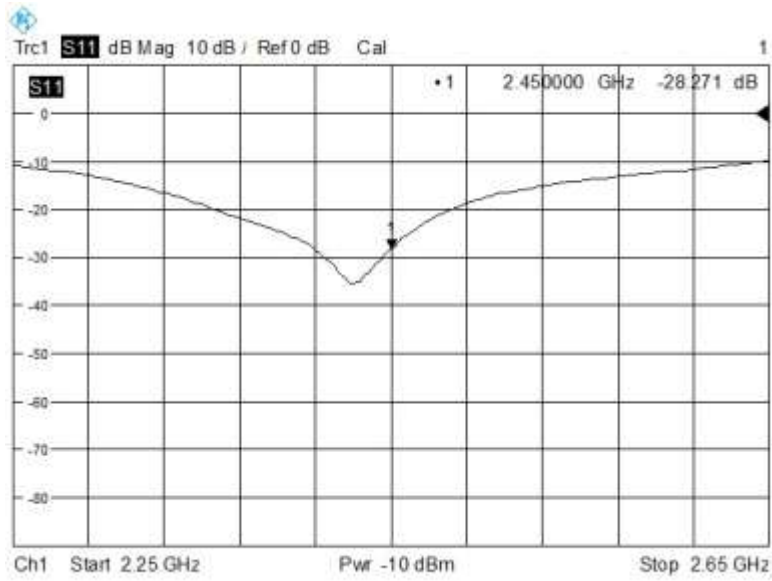


Impedance

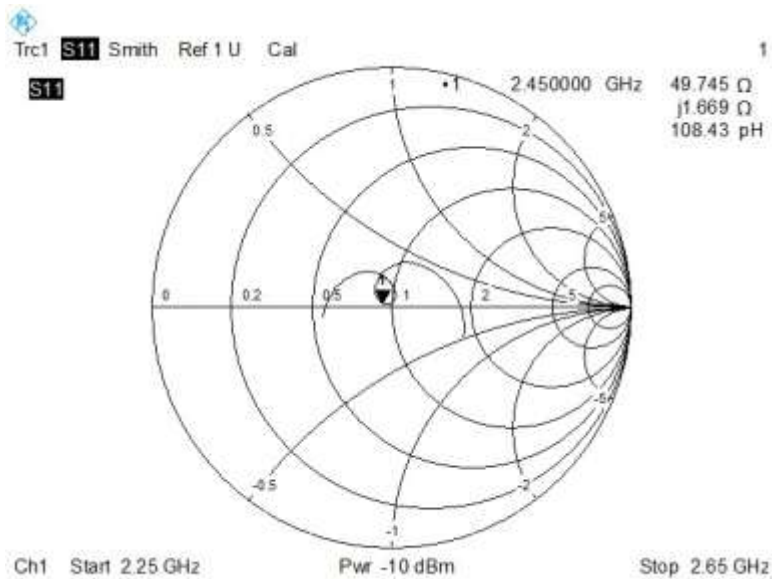


RETURN LOSS AND IMPEDANCE IN BODY LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|------------------|-------------------|-------------------|----------------------------|
| Return Loss (dB) | -27.205 | -23.809 | 14.3% |
| Impedance | 46.8 Ω + 1.658 jΩ | 48.7 Ω + 6.254 jΩ | 4.596Ω (Imaginary part) |

Return Loss

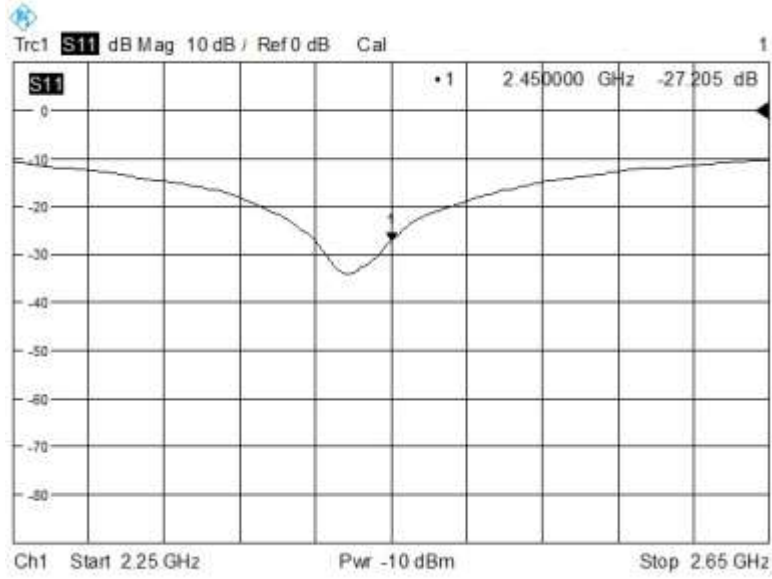

+Impedance

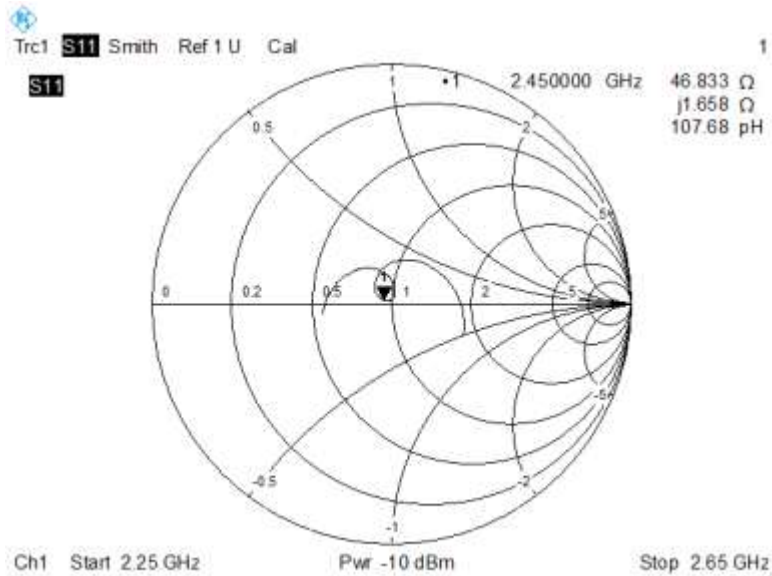


3.6 D2600V2


RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|-----------------|--------------------------------------|--------------------------------------|--------------------------------|
| Return Loss(dB) | -22.192 | -21.851 | 1.6% |
| Impedance | 46.754 Ω -7.288 j Ω | 47.178 Ω -7.354 j Ω | -0.424 Ω (Real part) |

Return Loss

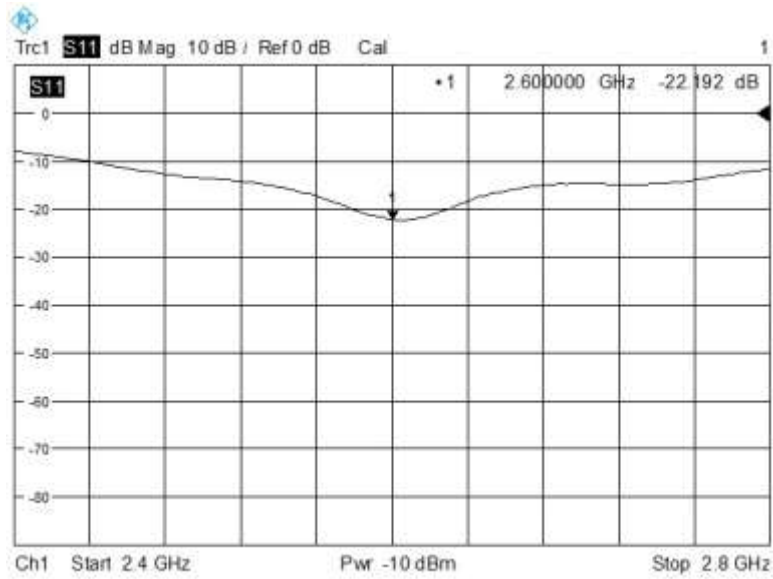

Impedance

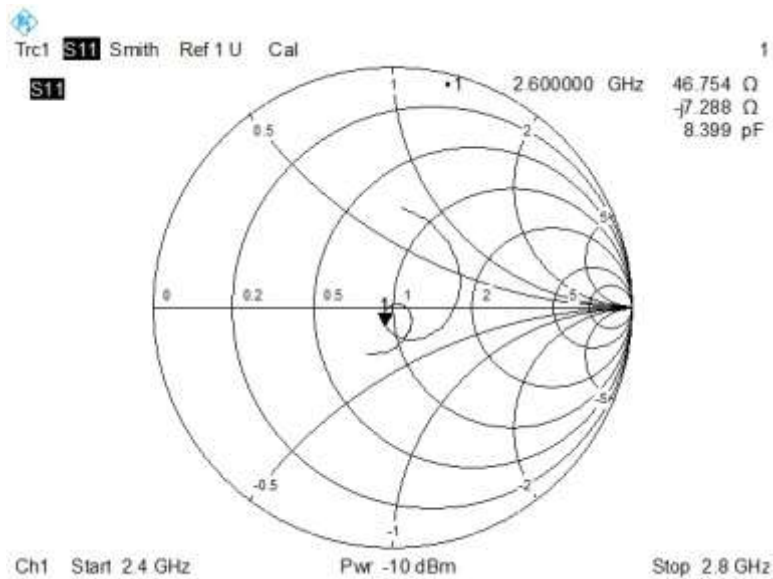





RETURN LOSS AND IMPEDANCE IN BODY LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|-----------------|----------------------------------|----------------------------------|-------------------------------|
| Return Loss(dB) | -21.794 | -21.481 | 1.5% |
| Impedance | 46.334 Ω -5.883 $j\Omega$ | 44.590 Ω -5.879 $j\Omega$ | 1.744 Ω (Real part) |

Return Loss

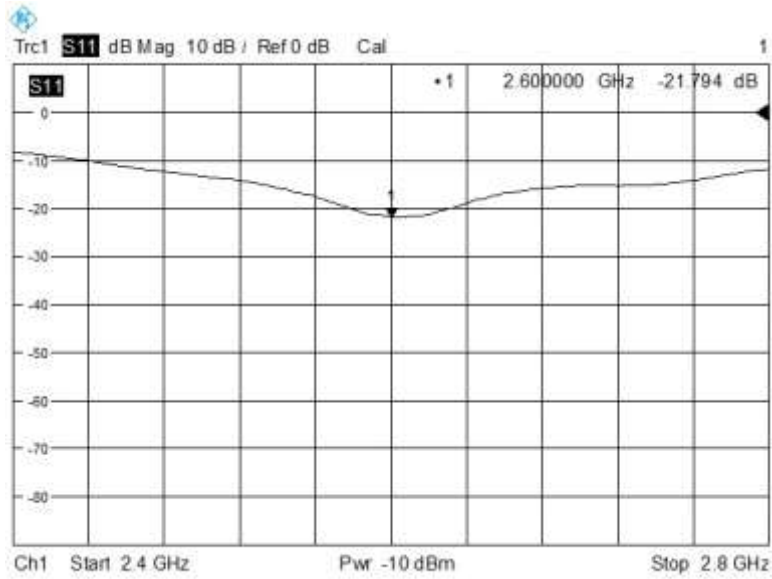

Impedance

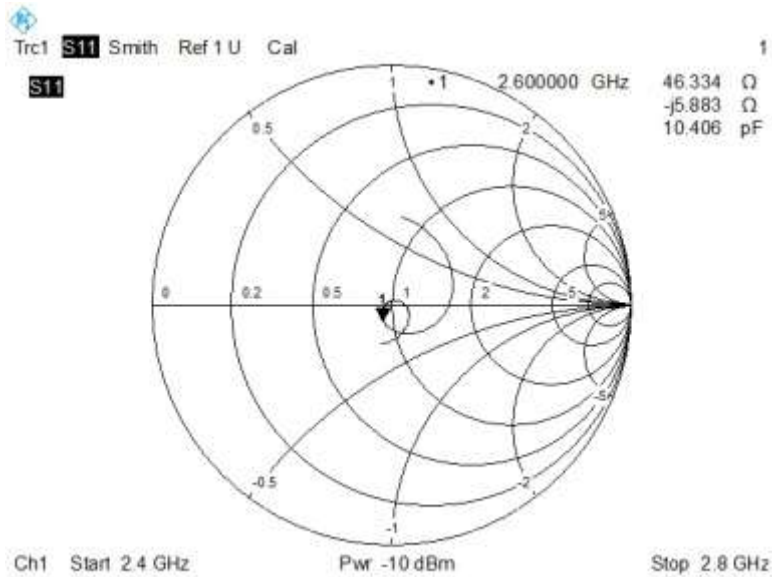




3.7 D5GHzV2

RETURN LOSS AND IMPEDANCE IN HEAD LIQUID


| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation | | | | | | | | | | | | |
|---|--------------------|--------------------|--------------------|-------|-----------------|------------------|---|----------|---------|---|----------|---------|---|----------|---------|
| 5250 MHz | | | | | | | | | | | | | | | |
| Return Loss(dB) | -25.052 | -26.013 | -3.7% | | | | | | | | | | | | |
| Impedance | 47.735 Ω -4.621 jΩ | 48.180 Ω -4.570 jΩ | 0.445Ω (Real part) | | | | | | | | | | | | |
| 5600 MHz | | | | | | | | | | | | | | | |
| Return Loss(dB) | -26.377 | -25.418 | 3.8% | | | | | | | | | | | | |
| Impedance | 54.525 Ω +2.142 jΩ | 55.218 Ω +2.140 jΩ | 0.693Ω (Real part) | | | | | | | | | | | | |
| 5750 MHz | | | | | | | | | | | | | | | |
| Return Loss(dB) | -29.503 | -29.687 | -0.6% | | | | | | | | | | | | |
| Impedance | 51.171 Ω -3.278 jΩ | 50.573 Ω -3.249 jΩ | 0.598Ω (Real part) | | | | | | | | | | | | |
| Return Loss | | | | | | | | | | | | | | | |
| <p>Trc1 S11 dB Mag 10 dB / Ref 0 dB Cal 1</p> <table border="1"> <thead> <tr> <th>Point</th> <th>Frequency (GHz)</th> <th>Return Loss (dB)</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>5.250000</td> <td>-25.052</td> </tr> <tr> <td>2</td> <td>5.600000</td> <td>-26.377</td> </tr> <tr> <td>3</td> <td>5.750000</td> <td>-29.503</td> </tr> </tbody> </table> <p>Ch1 Start 5 GHz Pwr -10 dBm Stop 6 GHz</p> | | | | Point | Frequency (GHz) | Return Loss (dB) | 1 | 5.250000 | -25.052 | 2 | 5.600000 | -26.377 | 3 | 5.750000 | -29.503 |
| Point | Frequency (GHz) | Return Loss (dB) | | | | | | | | | | | | | |
| 1 | 5.250000 | -25.052 | | | | | | | | | | | | | |
| 2 | 5.600000 | -26.377 | | | | | | | | | | | | | |
| 3 | 5.750000 | -29.503 | | | | | | | | | | | | | |
| Impedance | | | | | | | | | | | | | | | |

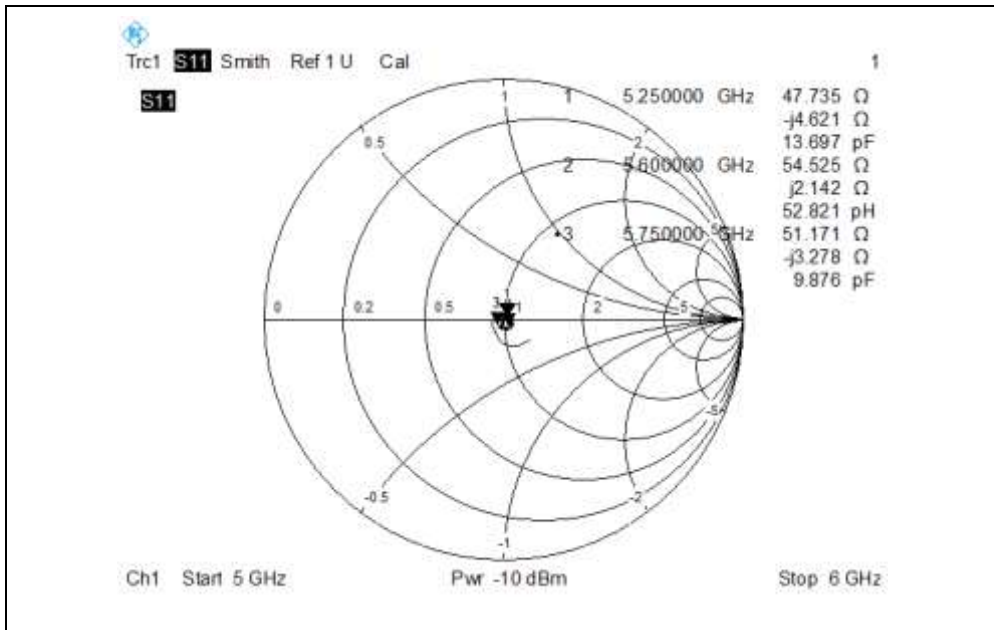




RETURN LOSS AND IMPEDANCE IN BODY LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation | | | | | | | | | | | | |
|---|---------------------------------------|---------------------------------------|-------------------------------|-------|-----------------|------------------|---|----------|---------|---|----------|---------|---|----------|---------|
| 5250 MHz | | | | | | | | | | | | | | | |
| Return Loss(dB) | -30.483 | -28.952 | 5.3% | | | | | | | | | | | | |
| Impedance | 47.975 Ω -2.840 j Ω | 47.902 Ω -2.794 j Ω | 0.073 Ω (Real part) | | | | | | | | | | | | |
| 5600 MHz | | | | | | | | | | | | | | | |
| Return Loss(dB) | -24.636 | -24.095 | 2.2% | | | | | | | | | | | | |
| Impedance | 54.321 Ω + 3.910 j Ω | 55.313 Ω + 3.876 j Ω | 0.992 Ω (Real part) | | | | | | | | | | | | |
| 5750 MHz | | | | | | | | | | | | | | | |
| Return Loss(dB) | -29.774 | -30.925 | -3.7% | | | | | | | | | | | | |
| Impedance | 51.737 Ω -2.126 j Ω | 51.882 Ω -2.203 j Ω | 0.145 Ω (Real part) | | | | | | | | | | | | |
| Return Loss | | | | | | | | | | | | | | | |
| <p>Trc1 S11 dB Mag 10 dB / Ref 0 dB Cal 1</p> <table border="1"> <thead> <tr> <th>Point</th> <th>Frequency (GHz)</th> <th>Return Loss (dB)</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>5.250000</td> <td>-30.483</td> </tr> <tr> <td>2</td> <td>5.600000</td> <td>-24.636</td> </tr> <tr> <td>3</td> <td>5.750000</td> <td>-29.774</td> </tr> </tbody> </table> <p>Ch1 Start 5 GHz Pwr -10 dBm Stop 6 GHz</p> | | | | Point | Frequency (GHz) | Return Loss (dB) | 1 | 5.250000 | -30.483 | 2 | 5.600000 | -24.636 | 3 | 5.750000 | -29.774 |
| Point | Frequency (GHz) | Return Loss (dB) | | | | | | | | | | | | | |
| 1 | 5.250000 | -30.483 | | | | | | | | | | | | | |
| 2 | 5.600000 | -24.636 | | | | | | | | | | | | | |
| 3 | 5.750000 | -29.774 | | | | | | | | | | | | | |
| Impedance | | | | | | | | | | | | | | | |

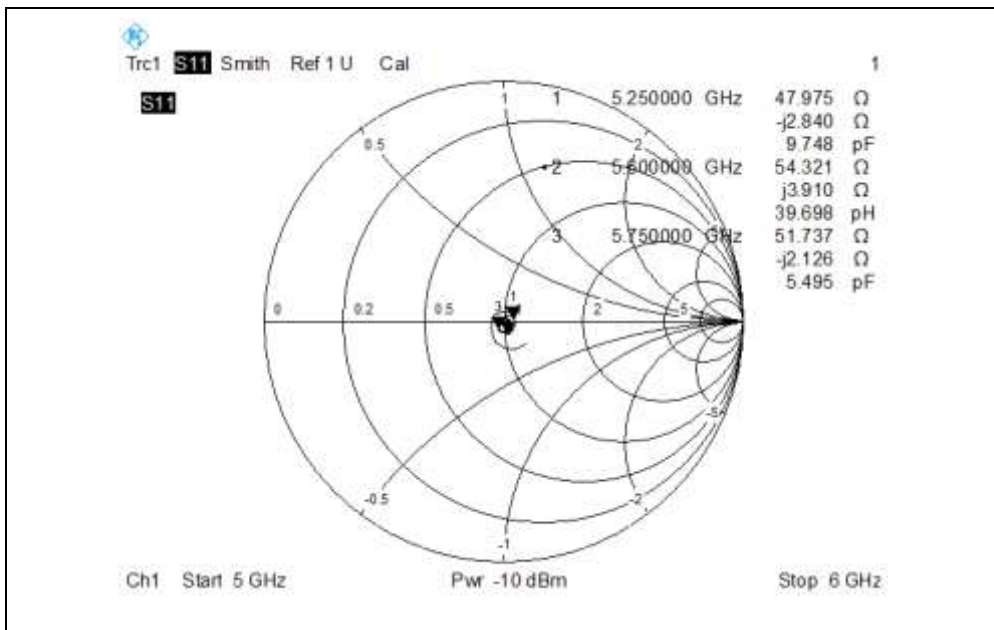

4 VALIDATION MEASUREMENT

The IEEE Std. 1528, FCC KDBs and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

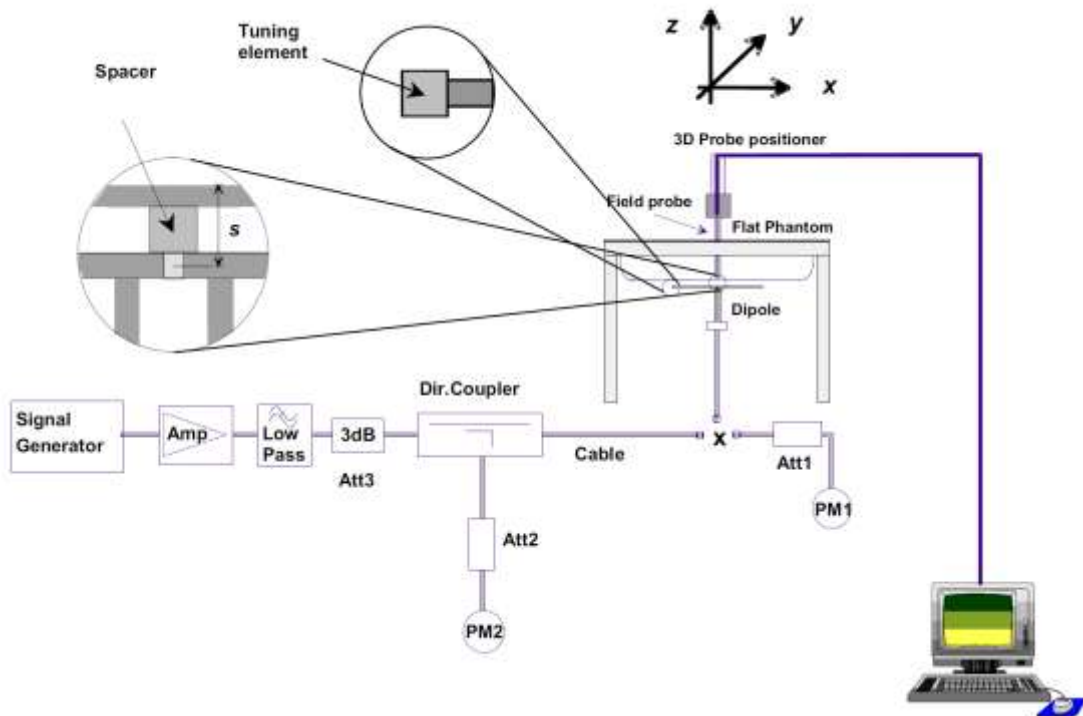



4.1 Dipole SAR Validation Measurement Result

| Freq. (MHz) | Liquid Type | Power (mW) | 1 g Measured SAR (W/kg) | Normalized SAR (W/kg) | 10 g Measured SAR (W/kg) | Normalized SAR (W/kg) | 1 g Targeted SAR (W/kg) | Tolerance (%) | 10 g Targeted SAR (W/kg) | Tolerance (%) |
|-------------|-------------|------------|-------------------------|-----------------------|--------------------------|-----------------------|-------------------------|---------------|--------------------------|---------------|
| 750 | Head | 100 | 0.815 | 8.15 | 0.548 | 5.48 | 8.49 | -4.00 | 5.55 | -1.26 |
| | Body | 100 | 0.823 | 8.23 | 0.552 | 5.52 | 8.49 | -3.06 | 5.55 | -0.54 |
| 835 | Head | 100 | 0.996 | 9.96 | 0.641 | 6.41 | 9.56 | 4.18 | 6.22 | 3.05 |
| | Body | 100 | 0.963 | 9.63 | 0.636 | 6.36 | 9.56 | 0.73 | 6.22 | 2.25 |
| 1750 | Head | 100 | 3.590 | 35.90 | 1.870 | 18.70 | 36.40 | -1.37 | 19.30 | -3.11 |
| | Body | 100 | 3.810 | 38.10 | 1.990 | 19.90 | 36.40 | 4.67 | 19.30 | 3.11 |
| 1900 | Head | 100 | 4.030 | 40.30 | 2.090 | 20.90 | 39.70 | 1.51 | 20.50 | 1.95 |
| | Body | 100 | 3.840 | 38.40 | 1.970 | 19.70 | 39.70 | -3.27 | 20.50 | -3.90 |
| 2450 | Head | 100 | 5.390 | 53.90 | 2.380 | 23.80 | 52.40 | 2.86 | 24.00 | -0.83 |
| | Body | 100 | 5.310 | 53.10 | 2.290 | 22.90 | 52.40 | 1.34 | 24.00 | -4.58 |
| 2600 | Head | 100 | 5.840 | 58.40 | 2.490 | 24.90 | 55.30 | 5.61 | 24.60 | 1.22 |
| | Body | 100 | 5.830 | 58.30 | 2.510 | 25.10 | 55.30 | 5.42 | 24.60 | 2.03 |
| 5200 | Head | 100 | 7.980 | 79.80 | 2.130 | 21.30 | 76.50 | 4.31 | 21.60 | -1.39 |
| | Body | 100 | 7.320 | 73.20 | 2.050 | 20.50 | 76.50 | -4.31 | 21.60 | -5.09 |
| 5600 | Head | 100 | 8.270 | 82.70 | 2.220 | 22.20 | 83.30 | -0.72 | 23.40 | -5.13 |
| | Body | 100 | 8.270 | 82.70 | 2.310 | 23.10 | 83.30 | -0.72 | 23.40 | -1.28 |
| 5800 | Head | 100 | 8.030 | 80.30 | 2.140 | 21.40 | 78.00 | 2.95 | 21.90 | -2.28 |
| | Body | 100 | 7.730 | 77.30 | 2.120 | 21.20 | 78.00 | -0.90 | 21.90 | -3.20 |



4.2D750V3

4.2.1 Dipole 750 MHz Validation Measurement for Head Tissue

Dipole 750 MHz; Type: D750V3; Serial: D750V3-SN:1055

Date/Time: 6/24/2018

Communication System Band: D750 (750.0 MHz); Frequency: 750 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 750$ MHz; $\sigma = 0.91$ S/m; $\epsilon_r = 40.53$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.2 Liquid Temperature: 21.1

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(6.16, 6.16, 6.16);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 Right 1859; Type: QD000P40CD; Serial: TP1859
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)


Dipolevalidation measurement for Head Tissue/Pin= 100mW ,d=15mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 29.34 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 1.19 W/kg

SAR(1 g) = 0.815 W/kg; SAR(10 g) = 0.548 W/kg

Maximum value of SAR (measured) = 0.878 W/kg

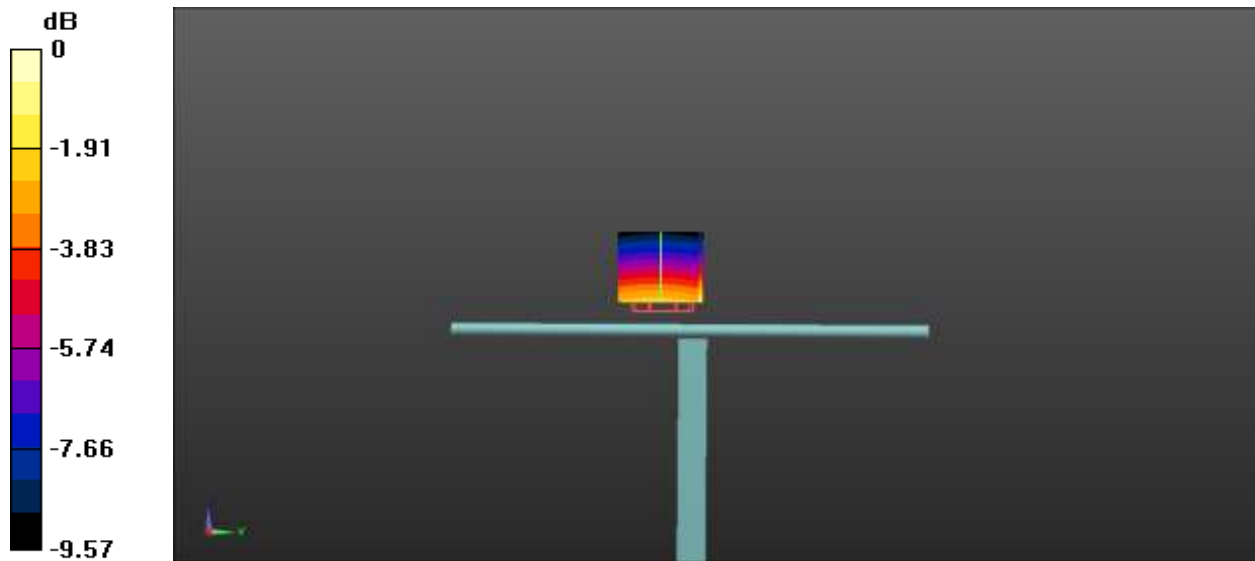

0 dB = 0.878 W/kg = -0.57 dBW/kg



4.2.2 Dipole 750 MHz Validation Measurement for Body Tissue

Dipole 750 MHz; Type: D750V3; Serial: D750V3-SN:1055

Date/Time: 6/24/2018

Communication System Band: D750 (750.0 MHz); Frequency: 750 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 750$ MHz; $\sigma = 0.99$ S/m; $\epsilon_r = 54.68$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.2 Liquid Temperature: 21.1

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(6.15, 6.15, 6.15);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 on Right 1857; Type: QD000P40CD; Serial: TP1857
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole validation measurement for Body Tissue/ Pin= 100mW ,d=15mm /Zoom


Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 30.58 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 1.21 W/kg

SAR(1 g) = 0.823 W/kg; SAR(10 g) = 0.552 W/kg

Maximum value of SAR (measured) = 0.885 W/kg

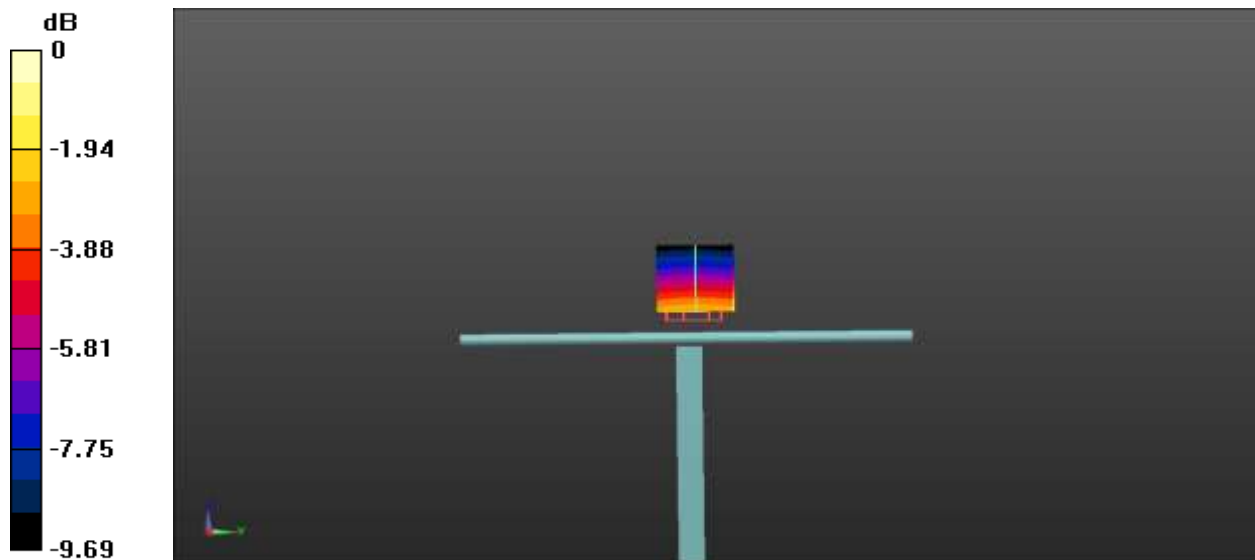

0 dB = 0.885 W/kg = -0.53 dBW/kg



4.3 D835V2

4.3.1 Dipole 835 MHz Validation Measurement for Head Tissue

Dipole 835 MHz; Type: D835V2; Serial: D835V2-SN:4d187

Date/Time: 6/24/2018

Communication System Band: D835 (835.0 MHz); Frequency: 835 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 835$ MHz; $\sigma = 0.89$ S/m; $\epsilon_r = 40.78$ $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.2 Liquid Temperature: 21.1

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(6.1, 6.1, 6.1);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 on Right 1857; Type: QD000P40CD; Serial: TP1857
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)



Dipole validation measurement for Head Tissue/Pin= 100mW , d=15mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 33.47 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 1.48 W/kg

SAR(1 g) = 0.996 W/kg; SAR(10 g) = 0.641 W/kg

Maximum value of SAR (measured) = 1.06 W/kg

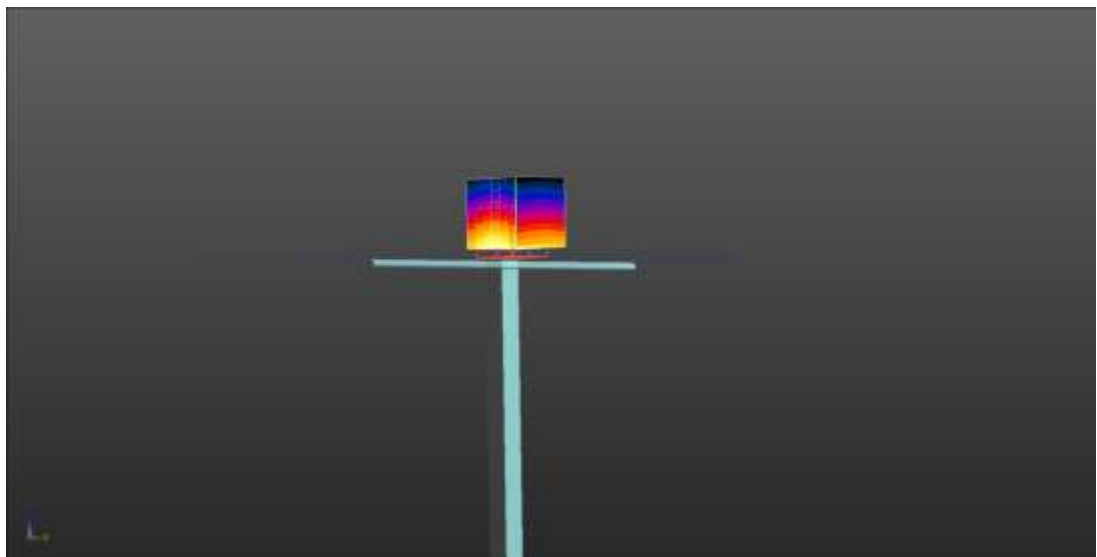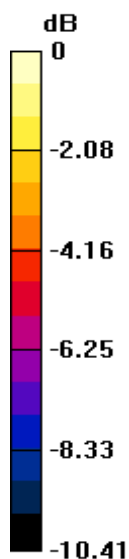

0 dB = 1.06 W/kg = 0.25 dBW/kg



4.3.2 Dipole 835 MHz Validation Measurement for Body Tissue

Dipole 835 MHz; Type: D835V2; Serial: D835V2-SN:4d187

Date/Time: 6/24/2018

Communication System Band: D835 (835.0 MHz); Frequency: 835 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 835$ MHz; $\sigma = 0.98$ S/m; $\epsilon_r = 53.86$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.2 Liquid Temperature: 21.1

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(6.1, 6.1, 6.1);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 on Right 1857; Type: QD000P40CD; Serial: TP1857
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole validation measurement for Body Tissue/Pin= 100mW , d=15mm /Zoom


Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 31.61 V/m; Power Drift = -0.11 dB

Peak SAR (extrapolated) = 1.41 W/kg

SAR(1 g) = 0.963 W/kg; SAR(10 g) = 0.636 W/kg

Maximum value of SAR (measured) = 1.04 W/kg

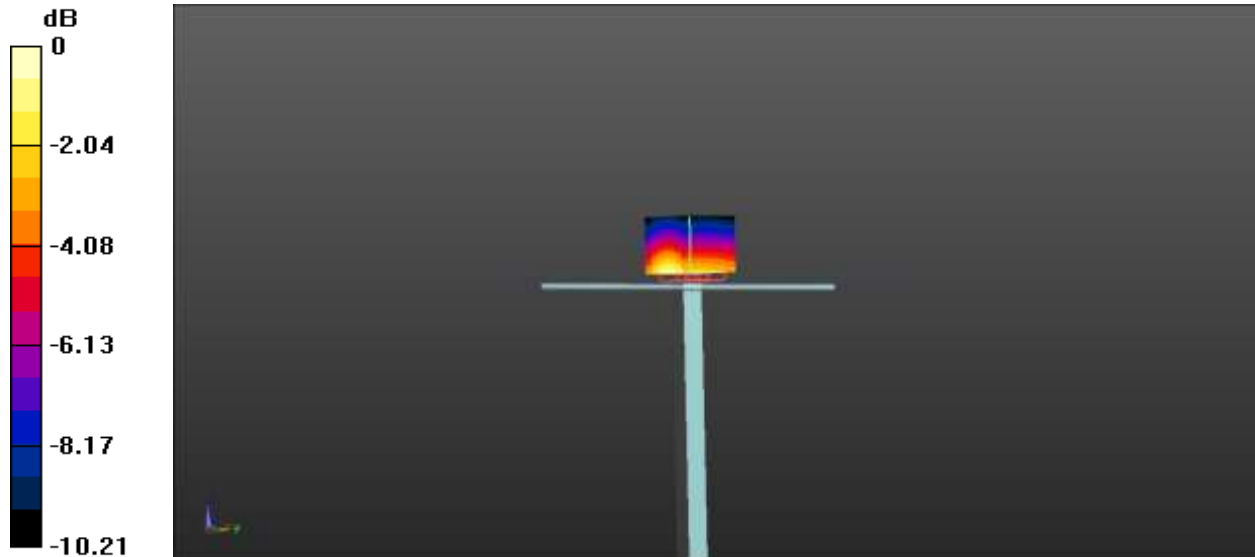

0 dB = 1.04 W/kg = 0.17 dBW/kg



4.4 D1750V2

4.4.1 Dipole 1750 MHz Validation Measurement for Head Tissue

Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2-SN: 1130

Date/Time: 6/26/2018

Communication System Band: D1750 (1750.0 MHz); Frequency: 1750 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 39.96$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.4 Liquid Temperature: 21.3

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(5.17, 5.17, 5.17);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 on Left 1859; Type: QD000P40CD; Serial: TP1859
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)



Dipole validation measurement for Head Tissue/Pin= 100mW ,d=10mm /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 50.02 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 6.67 W/kg

SAR(1 g) = 3.59W/kg; SAR(10 g) = 1.87 W/kg

Maximum value of SAR (measured) = 3.98 W/kg

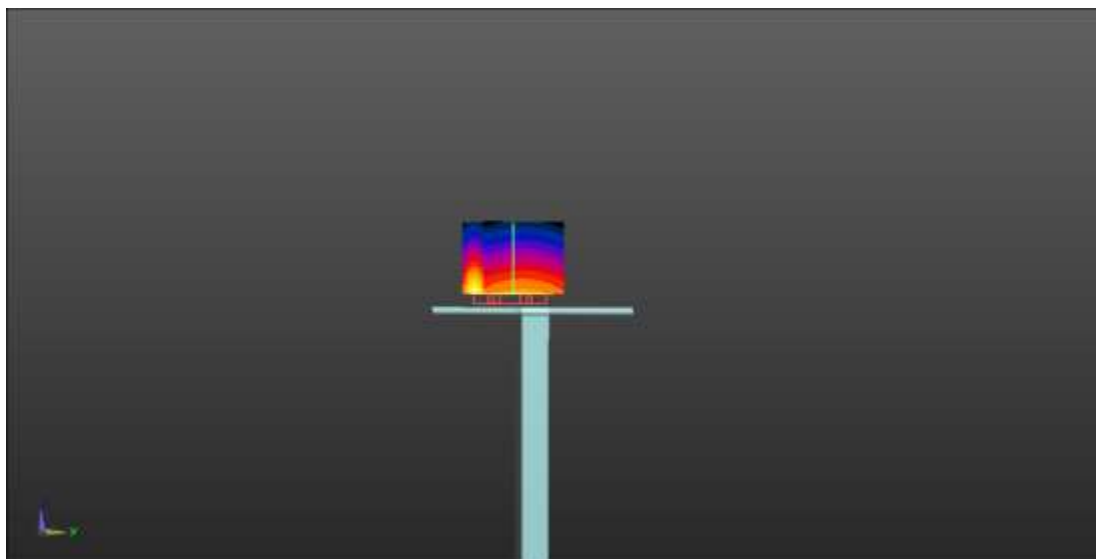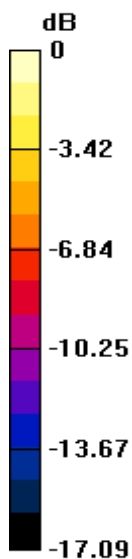

0 dB = 3.98 W/kg = 5.80 dBW/kg



4.4.2 Dipole 1750 MHz Validation Measurement for Body Tissue

Dipole 1750 MHz; Type: D1750V2; Serial: D1750V2-SN:1130

Date/Time: 6/26/2018

Communication System Band: D1750 (1750.0 MHz); Frequency: 1750 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 1750$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 52.56$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.4 Liquid Temperature: 21.3

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(4.87, 4.87, 4.87);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 on Left 1859; Type: QD000P40CD; Serial: TP1859
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole validation measurement for Body Tissue/Pin= 100mW ,d=10mm /Zoom


Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 54.61 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 6.98 W/kg

SAR(1 g) = 3.81 W/kg; SAR(10 g) = 1.99 W/kg

Maximum value of SAR (measured) = 4.26 W/kg

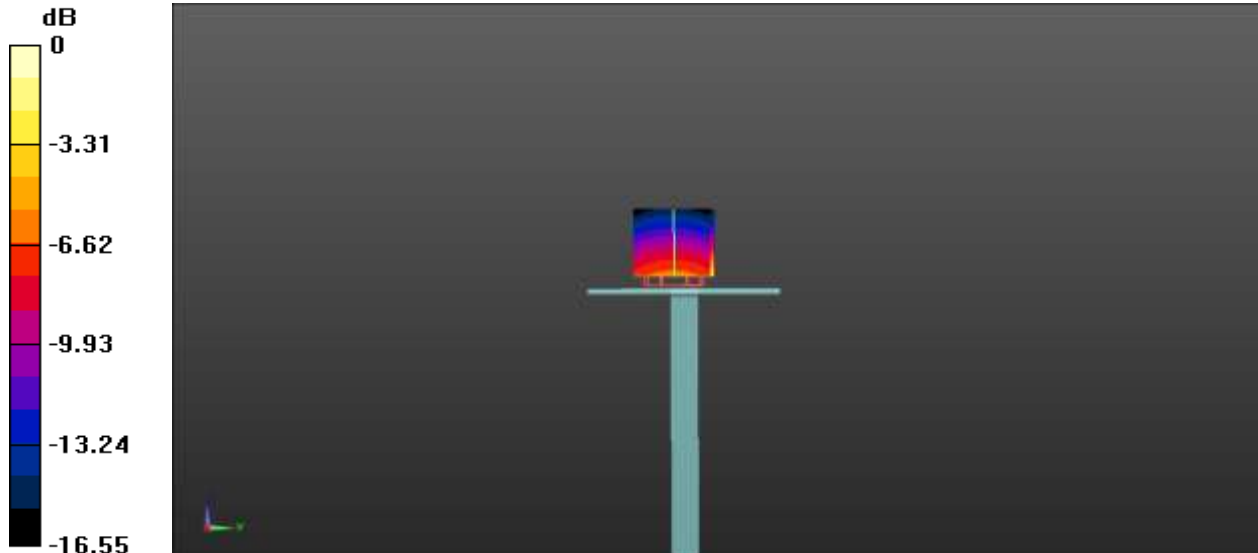

0 dB = 4.26 W/kg = 6.29 dBW/kg



4.5D1900V2

4.5.1 Dipole 1900 MHz Validation Measurement for Head Tissue

Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2-SN:5d193

Date/Time: 6/26/2018

Communication System Band: D1900 (1900.0 MHz); Frequency: 1900 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.43$ S/m; $\epsilon_r = 39.71$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.4 Liquid Temperature: 21.3

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(4.87, 4.87, 4.87);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 on Left 1859; Type: QD000P40CD; Serial: TP1859
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)


Dipole validation measurement for Head Tissue/Pin= 100mW ,d=10mm /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 53.57 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 7.42 W/kg

SAR(1 g) = 4.03 W/kg; SAR(10 g) = 2.09 W/kg

Maximum value of SAR (measured) = 4.55 W/kg

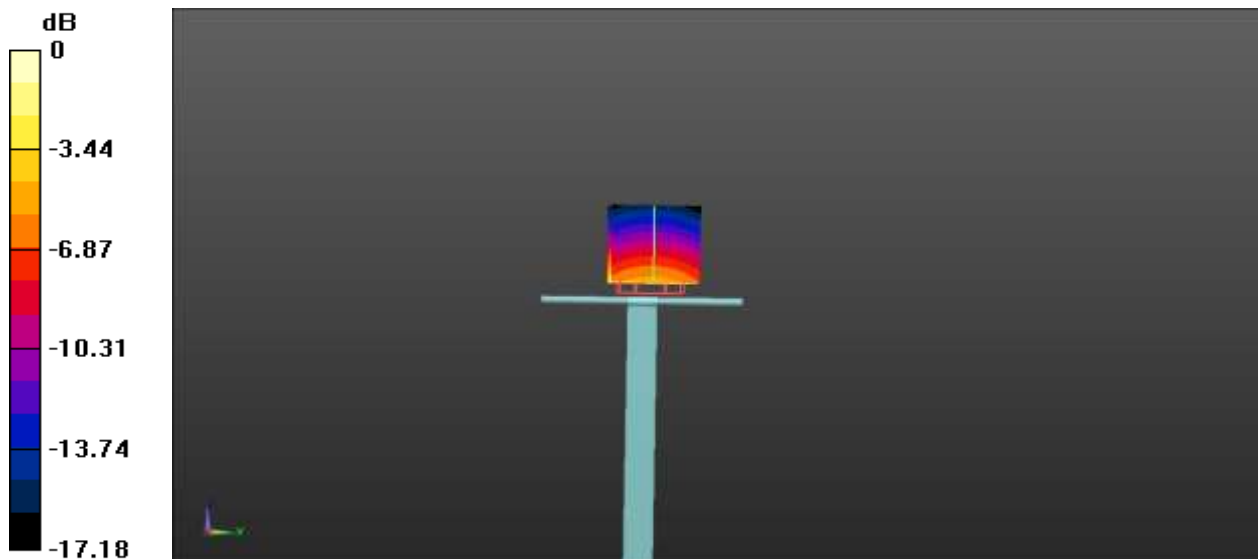

0 dB = 4.55 W/kg = 6.58 dBW/kg



4.5.2 Dipole 1900 MHz Validation Measurement for Body Tissue

Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2-SN:5d193

Date/Time: 6/26/2018

Communication System Band: D1900 (1900.0 MHz); Frequency: 1900 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.55$ S/m; $\epsilon_r = 51.58$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.4 Liquid Temperature: 21.3

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(4.61, 4.61, 4.61);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 on Right 1857; Type: QD000P40CD; Serial: TP1857
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole validation measurement for Body Tissue/Pin= 100mW ,d=10mm /Zoom


Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 52.57 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 7.15 W/kg

SAR(1 g) = 3.84 W/kg; SAR(10 g) = 1.97 W/kg

Maximum value of SAR (measured) = 4.28 W/kg

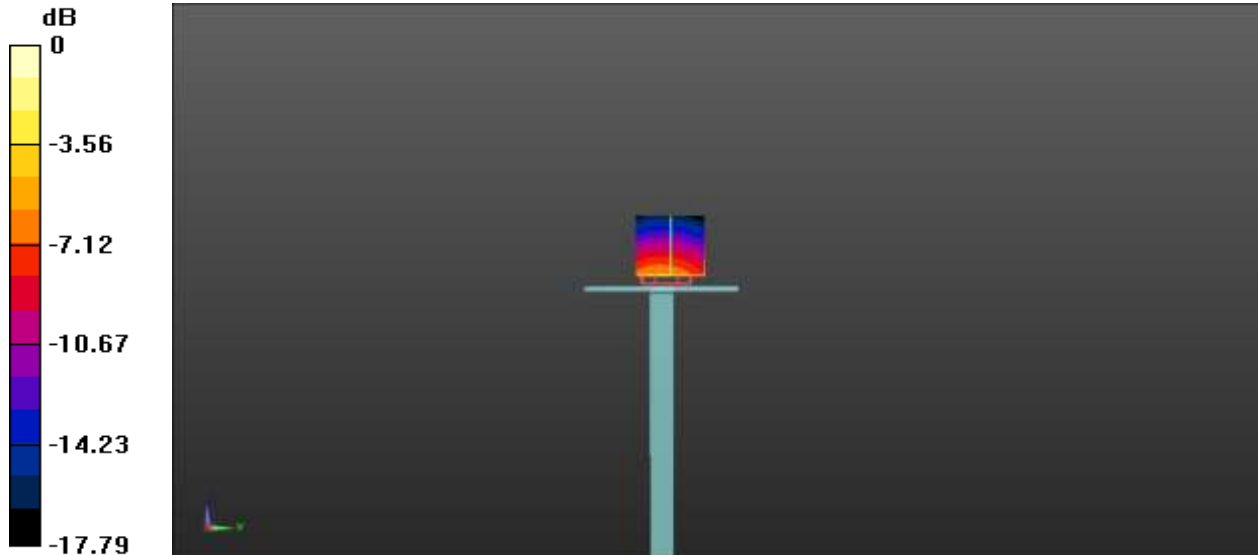

0 dB = 4.28 W/kg = 6.31 dBW/kg



4.6 D2450V2

4.6.1 Dipole 2450 MHz Validation Measurement for Head Tissue

Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2-SN:952

Date/Time: 3/16/2018

Communication System Band: CD2450 (2450.0 MHz); Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.84$ S/m; $\epsilon_r = 38.94$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.5 Liquid Temperature: 21.3

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(4.4, 4.4, 4.4);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 Right 1857; Type: QD000P40CD; Serial: TP1857
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)


Dipole validation measurement for Head Tissue/Pin= 100mW ,d=10mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 54.28 V/m; Power Drift = 0.07 dB

Peak SAR (extrapolated) = 11.8 W/kg

SAR(1 g) = 5.39 W/kg; SAR(10 g) = 2.38 W/kg

Maximum value of SAR (measured) = 6.21 W/kg

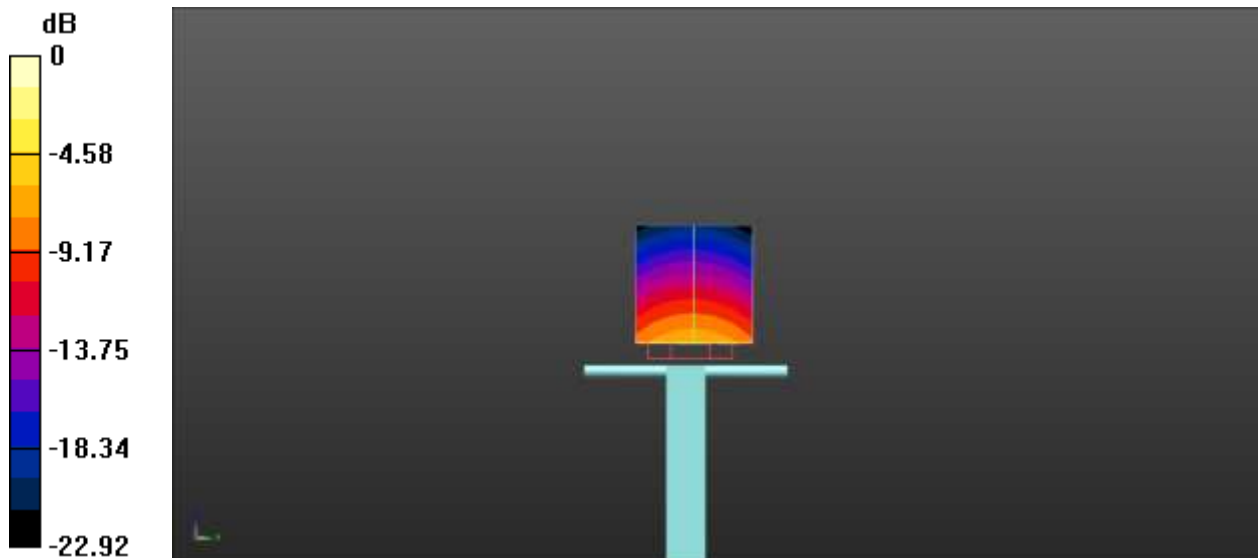

0 dB = 6.21 W/kg = 7.93 dBW/kg



4.6.2 Dipole 2450 MHz Validation Measurement for Body Tissue

Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2-SN:952

Date/Time: 3/16/2018

Communication System Band: D2450 (2450.0 MHz); Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.93$ S/m; $\epsilon_r = 50.88$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.5 Liquid Temperature: 21.3

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(4.23, 4.23, 4.23);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 left 1859; Type: QD000P40CD; Serial: TP1859
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole validation measurement for Body Tissue/Pin= 100mW ,d=10mm /Zoom


Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 49.11 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 10.9 W/kg

SAR(1 g) = 5.31 W/kg; SAR(10 g) = 2.29 W/kg

Maximum value of SAR (measured) = 5.92 W/kg

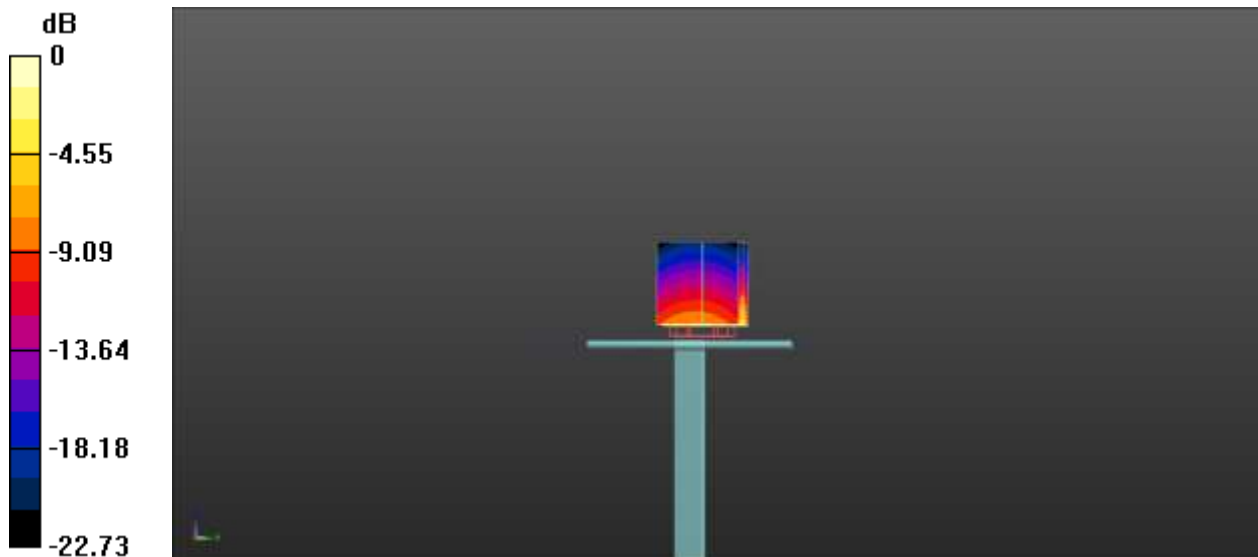

0 dB = 5.92 W/kg = 7.72 dBW/kg



4.7 D2600V2

4.7.1 Dipole 2600 MHz Validation Measurement for Head Tissue

Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2-SN: 1095

Date/Time: 7/5/2018

Communication System Band: D2600 (2600.0 MHz); Frequency: 2600 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 2600$ MHz; $\sigma = 1.99$ S/m; $\epsilon_r = 39.03$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.3 Liquid Temperature: 21.1

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(4.25, 4.25, 4.25);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 Right 1857; Type: QD000P40CD; Serial: TP1857
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)


Dipole validation measurement for Head Tissue/Pin= 100mW ,d=10mm /Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 32.49 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 11.17 W/kg

SAR(1 g) = 5.84 W/kg; SAR(10 g) = 2.49 W/kg

Maximum value of SAR (measured) = 6.38 W/kg

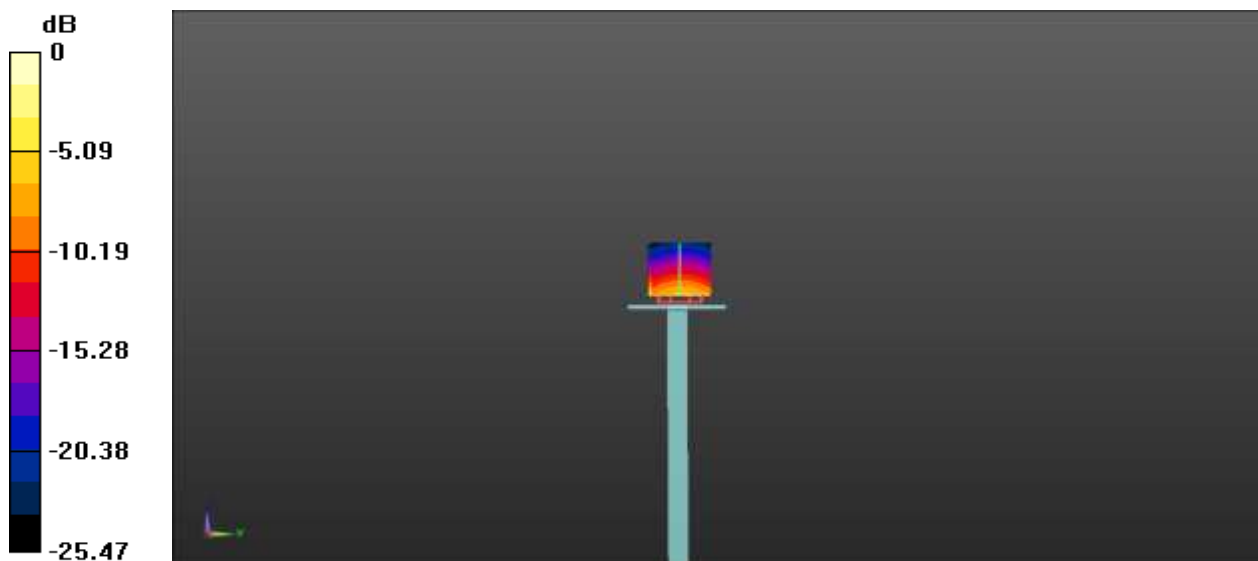

0 dB = 6.38 W/kg = 8.05 dBW/kg



4.7.2 Dipole 2600 MHz Validation Measurement for Body Tissue

Dipole 2600 MHz; Type: D2600V2; Serial: D835V2-SN: 1095

Date/Time: 7/5/2018

Communication System Band: D2600 (2600.0 MHz); Frequency: 2600 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 2600$ MHz; $\sigma = 2.21$ S/m; $\epsilon_r = 50.89$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.3 Liquid Temperature: 21.1

DASY5 Configuration:

- Probe: ES3DV3 - SN3110; ConvF(4.12, 4.12, 4.12);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454
- Phantom: SAM (30deg probe tilt) with CRP v5.0 Right 1857; Type: QD000P40CD; Serial: TP1857
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole validation measurement for Body Tissue/Pin= 100mW ,d=10mm /Zoom


Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 37.27 V/m; Power Drift = 0.12 dB

Peak SAR (extrapolated) = 12.5 W/kg

SAR(1 g) = 5.83 W/kg; SAR(10 g) = 2.51 W/kg

Maximum value of SAR (measured) = 6.67 W/kg

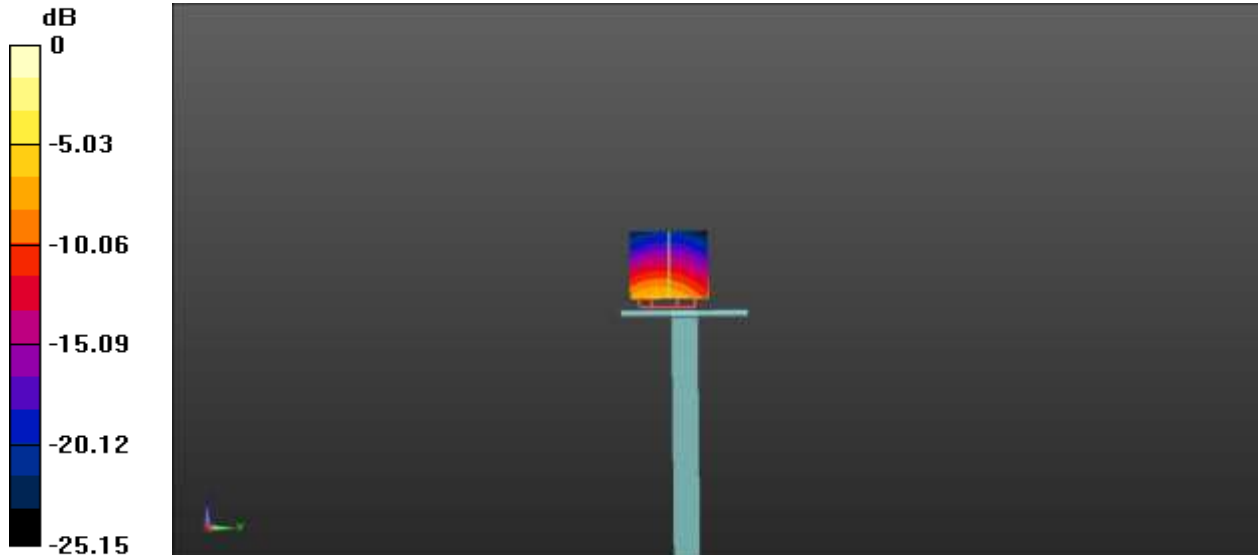

0 dB = 6.67 W/kg = 8.24 dBW/kg



4.8D5GHzV2

4.8.1 Dipole 5 GHz Validation Measurement for Head Tissue

Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2-SN:1200

Date/Time: 6/25/2018

Communication System Band: D5GHz (5000.0 - 6000.0 MHz);

Frequency: 5250 MHz,

Frequency: 5600 MHz,

Frequency: 5750 MHz;

Duty Cycle: 1:1

Medium parameters used: $f = 5250$ MHz; $\sigma = 4.63$ S/m; $\epsilon_r = 36.06$; $\rho = 1000$ kg/m³ , Medium

parameters used: $f = 5600$ MHz; $\sigma = 5.07$ S/m; $\epsilon_r = 35.83$; $\rho = 1000$ kg/m³ , Medium parameters

used: $f = 5750$ MHz; $\sigma = 5.17$ S/m; $\epsilon_r = 35.41$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature:22.3 Liquid Temperature:21.2

DASY5 Configuration:

- Probe: EX3DV4 - SN7340; ConvF(5.65, 5.65, 5.65); ConvF(4.87, 4.87, 4.87); ConvF(4.95, 4.95, 4.95);
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454;
- Phantom: SAM (30deg probe tilt) with CRP v5.0 on left 1859; Type: QD000P40CD; Serial: TP:1859
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole validation measurement for Head Tissue/Pin= 100mW ,dist=10mm,f=5250


MHz /Zoom Scan (7x7x21)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 37.41 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 33.6 W/kg

SAR(1 g) = 7.98 W/kg; SAR(10 g) = 2.13 W/kg

Maximum value of SAR (measured) = 19.79 W/kg

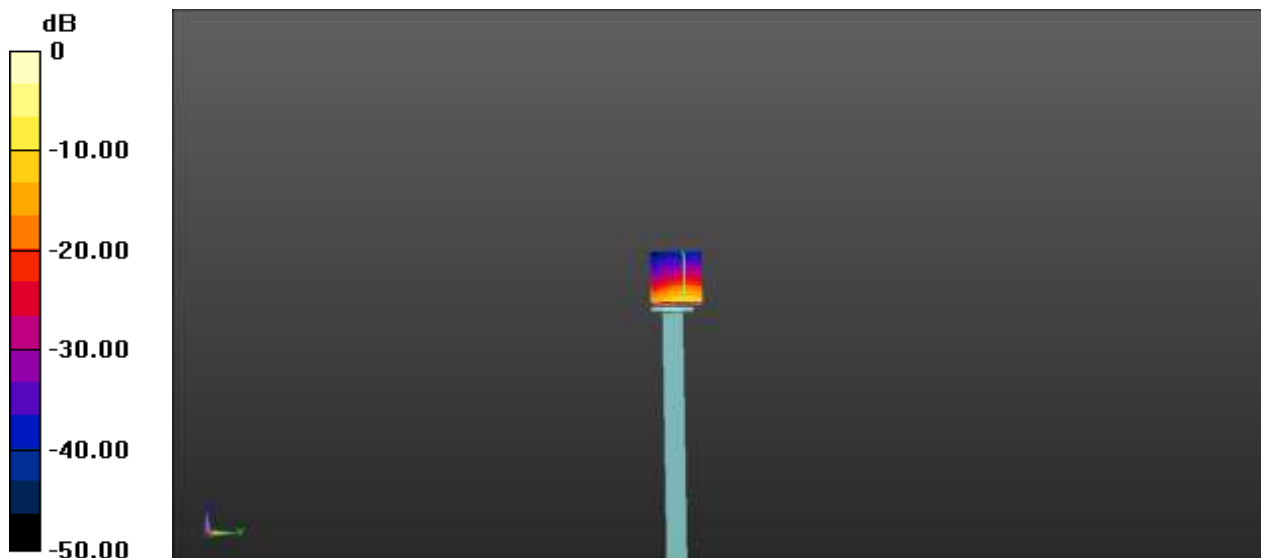

0 dB = 19.79 W/kg = 12.96 dBW/kg


Dipole validation measurement for Head Tissue/Pin= 100mW ,dist=10mm,f=5600 MHz /Zoom Scan (7x7x21)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 28.37 V/m; Power Drift = 0.12 dB

Peak SAR (extrapolated) = 37.5 W/kg

SAR(1 g) = 8.27 W/kg; SAR(10 g) = 2.22 W/kg

Maximum value of SAR (measured) = 20.51 W/kg

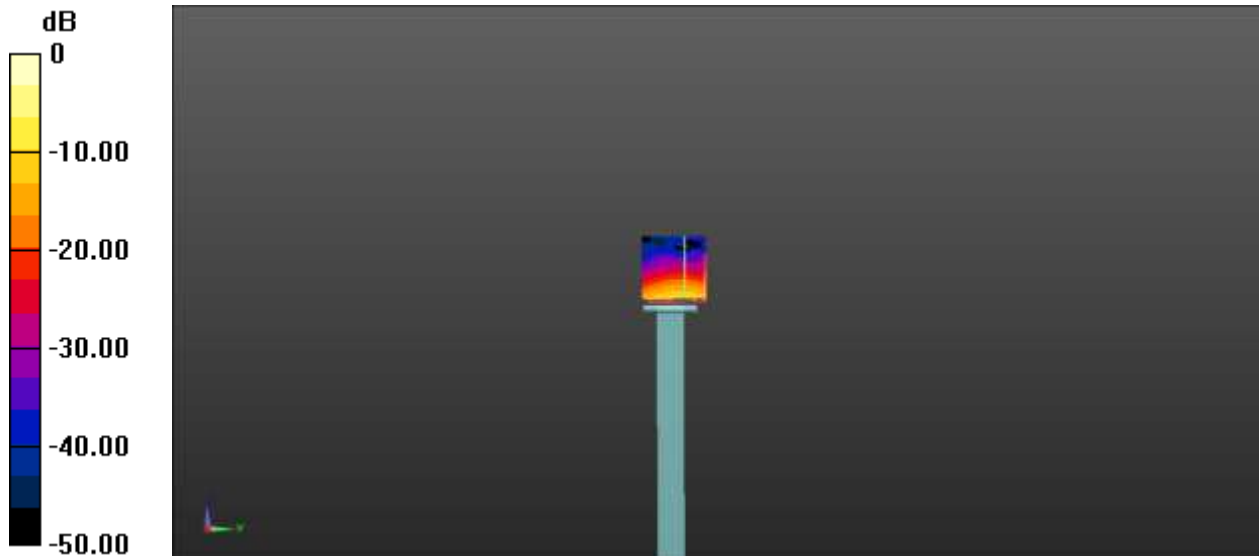

0 dB = 20.51 W/kg = 13.12 dBW/kg


Dipole Calibration for Head Tissue/Pin= 100mW ,dist=10mm,f=5750 MHz /Zoom Scan (7x7x21)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 33.52 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 40.42 W/kg

SAR(1 g) = 8.03 W/kg; SAR(10 g) = 2.14 W/kg

Maximum value of SAR (measured) = 17.29 W/kg

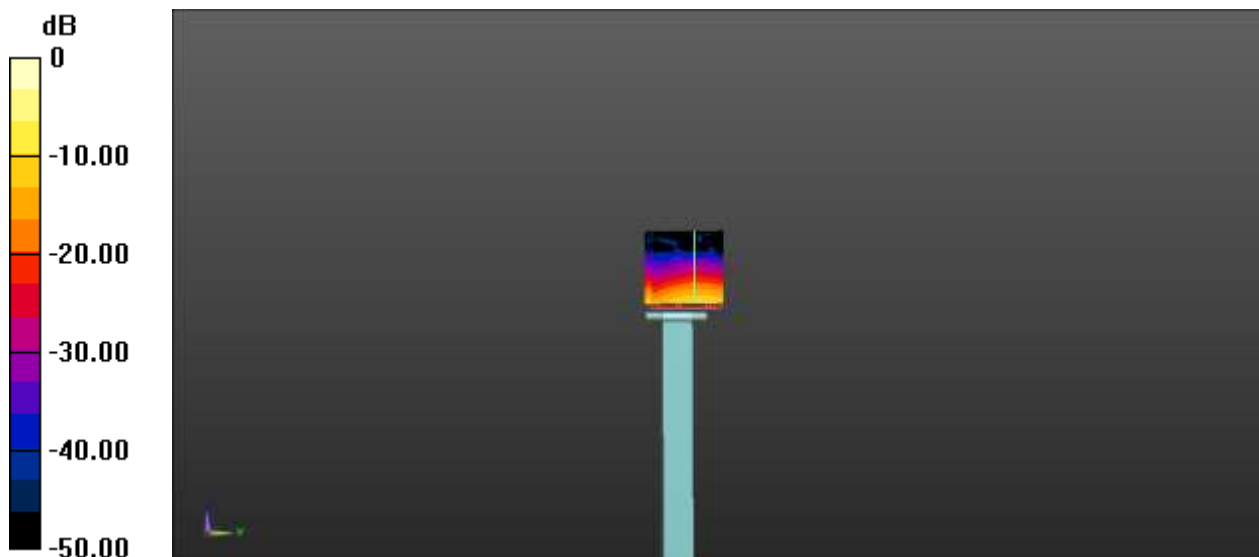

0 dB = 17.29 W/kg = 12.38 dBW/kg



4.8.2 Dipole 5 GHz Validation Measurement for Body Tissue

Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2-SN:1200

Date/Time: 6/25/2018

Communication System Band: D5GHz (5000.0 - 6000.0 MHz); Frequency: 5250 MHz; Frequency: 5600 MHz; Frequency: 5750 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 5250$ MHz; $\sigma = 5.34$ S/m; $\epsilon_r = 47.48$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5600$ MHz; $\sigma = 5.65$ S/m; $\epsilon_r = 46.63$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5750$ MHz; $\sigma = 5.87$ S/m; $\epsilon_r = 46.28$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature:22.3 Liquid Temperature:21.2

DASY5 Configuration:

- Probe: EX3DV4 - SN7340; ConvF(5.16, 5.16, 5.16);ConvF(4.35, 4.35, 4.35); ConvF(4.58, 4.58, 4.58);
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1454;
- Phantom: SAM (30deg probe tilt) with CRP v5.0 on left 1859; Type: QD000P40CD; Serial: TP:1859
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)


Dipolevalidation measurement for Body Tissue/Pin= 100mW ,dist=10mm,f=5250 MHz /Zoom Scan (7x7x21)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 36.65 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 27.1 W/kg

SAR(1 g) = 7.32 W/kg; SAR(10 g) = 2.05 W/kg

Maximum value of SAR (measured) = 14.41 W/kg

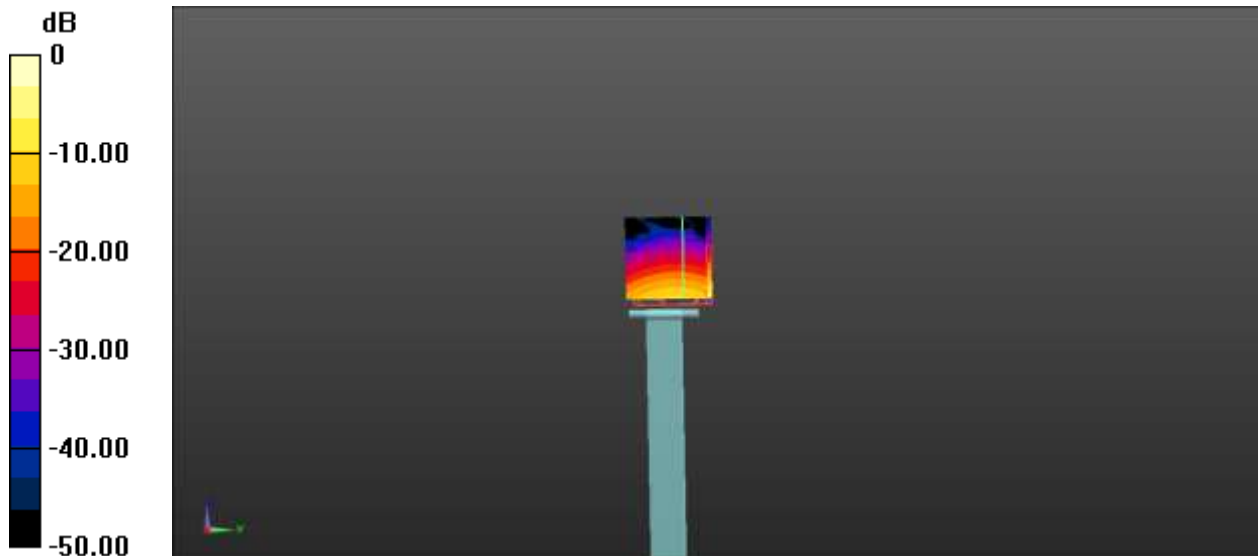

0 dB = 14.41 W/kg = 11.59 dBW/kg

Dipole validation measurement for Body Tissue/Pin= 100mW , dist=10mm,f=5600 MHz /Zoom Scan (7x7x21)/Cube 0:


Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 40.17 V/m; Power Drift = 0.09 dB

Peak SAR (extrapolated) = 35.4 W/kg

SAR(1 g) = 8.27 W/kg; SAR(10 g) = 2.31 W/kg

Maximum value of SAR (measured) = 20.28 W/kg

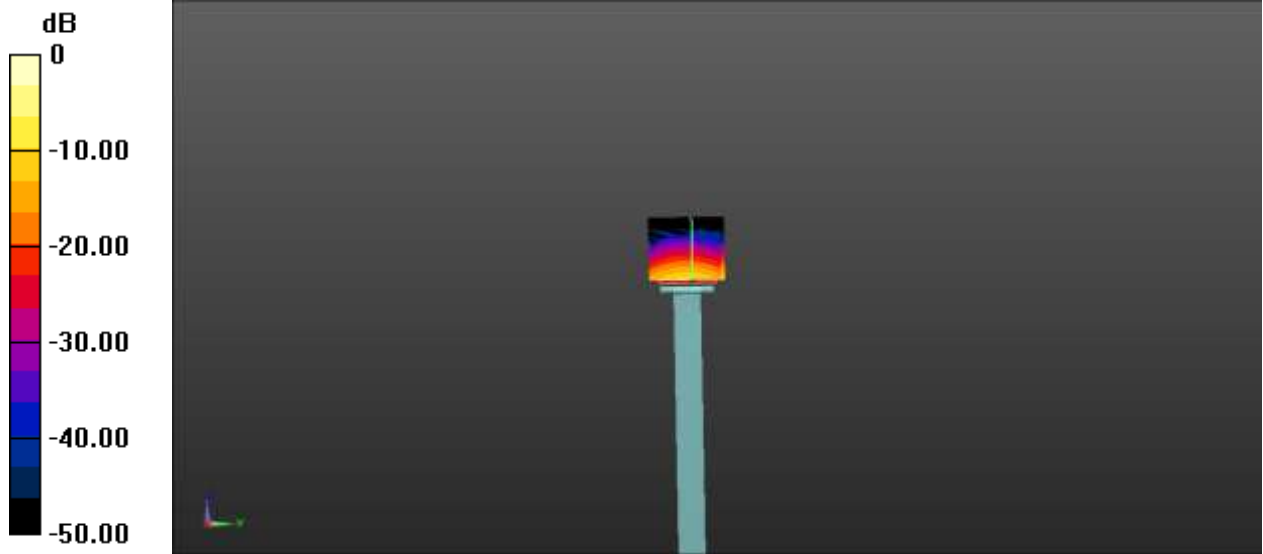

0 dB = 20.28 W/kg = 13.07 dBW/kg

Dipole validation measurement for Body Tissue/Pin= 100mW , dist=10mm,f=5750 MHz /Zoom Scan (7x7x21)/Cube 0:


Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 36.43 V/m; Power Drift = 0.13 dB

Peak SAR (extrapolated) = 35.6 W/kg

SAR(1 g) = 7.73 W/kg; SAR(10 g) = 2.12 W/kg

Maximum value of SAR (measured) = 19.33 W/kg

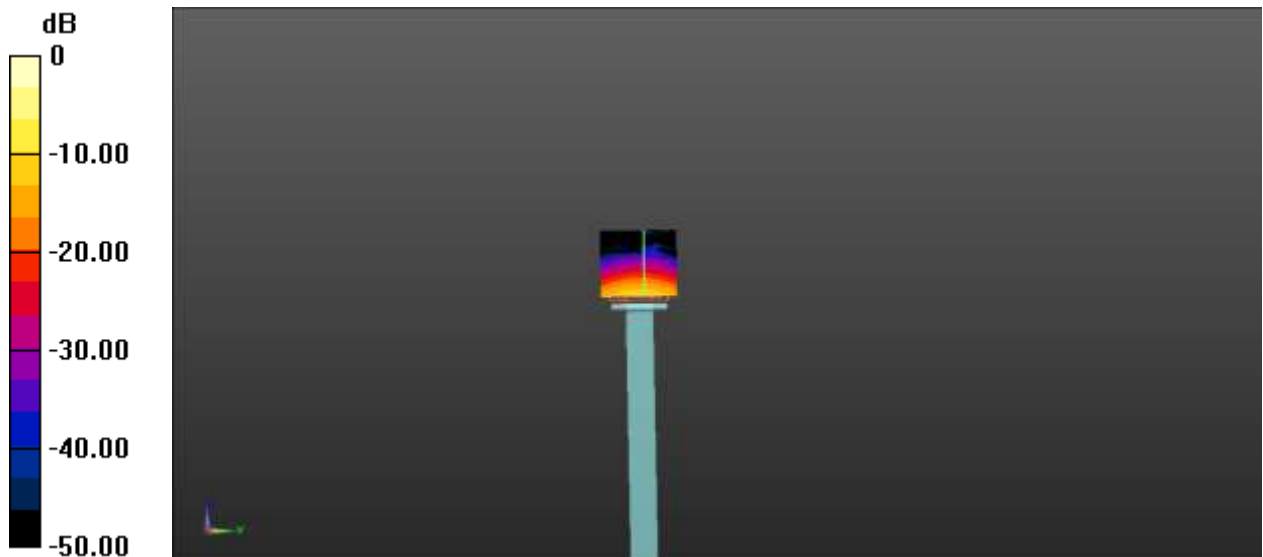

0 dB = 19.33 W/kg = 12.86 dBW/kg

--END OF REPORT--


SAR Dipole

ISSUED BY
Shenzhen BALUN Technology Co., Ltd.



Performance Measurement Report

FOR
Validation Dipoles

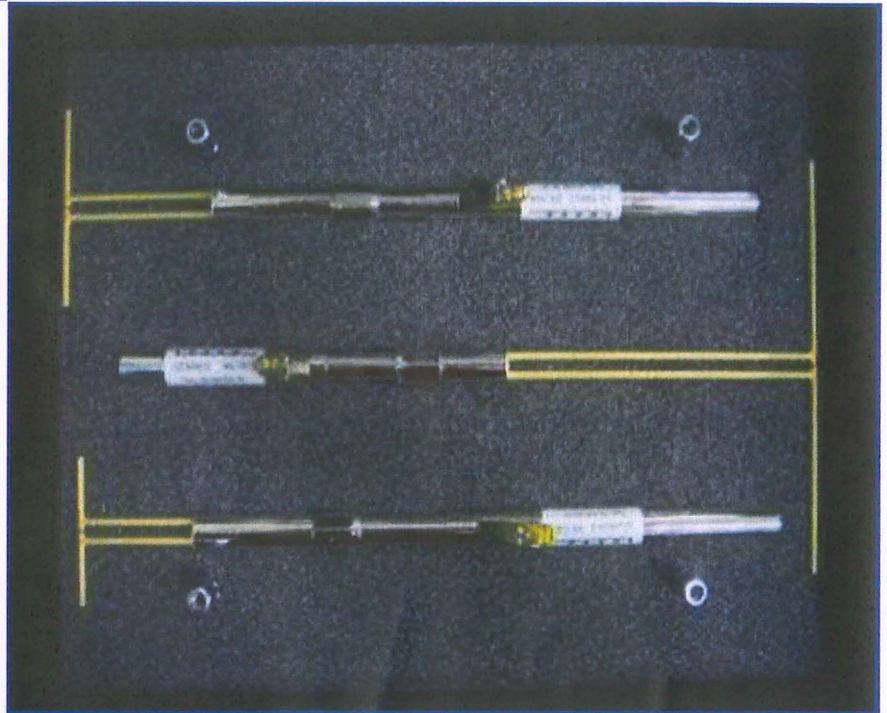

Tested by:

Zong Liyao
Zong Liyao
(Engineer)

Approved by:

Liao Jianming
Liao Jianming
(Technical Director)



Report No.: LW-SZ1930991-701

EUT Type: SAR Validation Dipole

Model Name: D2450V2

Brand Name: Speag

Test Conclusion: Pass

Test Date: Mar. 12, 2019

Date of Issue: Mar. 13, 2019

NOTE: This test report can be duplicated completely for the legal use with the approval of the applicant; it shall not be reproduced except in full, without the written approval of Shenzhen BALUN Technology Co., Ltd. BALUN Laboratory. Any objections should be raised within thirty days from the date of issue. To validate the report, please contact us.



1 GENERAL INFORMATION

1.1 Introduction

This document contains a summary of the requirements set forth by the IEEE 1528, FCC KDB 865664 D01 for reference dipoles used for SAR measurement system validations. Instead of the typical annual calibration recommended by measurement standards, the reference dipoles were demonstrated that the SAR target, impedance and return loss have remain stable, so the longer calibration interval is acceptable.

1.2 General Description for Equipment under Test (EUT)

| | |
|--------------|--------------------------|
| EUT Type | DASY 5 Reference Dipoles |
| Manufacturer | Speag |

| Parameter | EUT 1 |
|-------------------------------|-----------|
| Model | D2450V2 |
| Frequency | 2450 MHz |
| Serial Number | SN 952 |
| Product Condition (New/ Used) | Used |
| Last Cal. Date | 2017/3/21 |
| Current meas. Date | 2019/3/12 |



1.3 Test Equipment List

| Description | Manufacturer | Model | Serial No. | Cal. Date | Cal. Due |
|------------------------------|--------------|-----------|-----------------|------------|------------|
| PC | Dell | N/A | N/A | N/A | N/A |
| E-Field Probe | Speag | EX3DV4 | SN: 7510 | 2018/07/14 | 2019/07/13 |
| Data Acquisition Electronics | Speag | DAE4 | SN: 685 | 2018/07/14 | 2019/07/13 |
| Signal Generator | R&S | SMBV100A | 260592 | 2018/06/15 | 2019/06/14 |
| Power Meter | Agilent | E4419B | GB40201833 | 2018/06/02 | 2019/06/01 |
| Power Sensor | Agilent | E9300A | MY41498012 | 2018/07/02 | 2019/07/01 |
| Power Sensor | Agilent | E9300A | MY41499891 | 2018/07/02 | 2019/07/01 |
| Network Analyzer | Agilent | 5071C | MY46103472 | 2018/03/14 | 2019/03/13 |
| Thermometer | Elitech | RC-4HC | N/A | 2018/11/05 | 2019/11/04 |
| Dielectric Probe Kit | SATIMO | SCLMP | SN 25/13 OCPG56 | N/A | N/A |
| Phantom1 | Speag | SAM | SN: 1859 | N/A | N/A |
| Phantom2 | Speag | SAM | SN: 1857 | N/A | N/A |
| Power Amplifier | SATIMO | 6552B | 22374 | N/A | N/A |
| Attenuator | COM-MW | ZA-S1-31 | 1305003187 | N/A | N/A |
| Directional coupler | AA-MCS | AAMCS-UDC | 000272 | N/A | N/A |

1.4 EUT Photos





2 SIMULATING LIQUID VERIFICATION

| Liquid Type | Fre. (MHz) | Meas. Conductivity (σ) (S/m) | Meas. Permittivity (ϵ) | Target Conductivity (σ) (S/m) | Target Permittivity (ϵ) | Conductivity Tolerance (%) | Permittivity Tolerance (%) |
|-------------|------------|---------------------------------------|-----------------------------------|--|------------------------------------|----------------------------|----------------------------|
| Head | 2450 | 1.85 | 39.67 | 1.80 | 39.20 | 2.67 | 1.20 |
| Body | 2450 | 1.93 | 53.66 | 1.95 | 52.70 | -1.03 | 1.82 |



3 DIPOLE IMPEDANCE AND RETURN LOSS

The dipoles are designed to have low return loss when presented against a flat phantom at the specified distance. A Vector Network Analyser was used to perform a return loss measurement on the specific dipole when in the measurement location against the phantom and the distance was specified by the manufacturer with a special, low loss and low relative permittivity spacer.

The impedance was measured at the SMA-connector with the network analyser.

The measurement of verification with return loss should not deviate by more than 20% and minimum of 20 dB of the return loss, and the impedance (real or imaginary parts) should not deviate by more than 5 Ohms from the previous measurement using network analyzer.

Note:

The "Previous Meas." in the following table refer to dipoles or other equivalent RF sources calibration reports.




3.1 D2450V2


RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|-----------------|----------------------------------|----------------------------------|-------------------------------|
| Return Loss(dB) | -26.350 | -28.271 | -6.8% |
| Impedance | 46.7 Ω + 1.584 j Ω | 49.7 Ω + 1.669 j Ω | 3.011 Ω (Real part) |

Return Loss

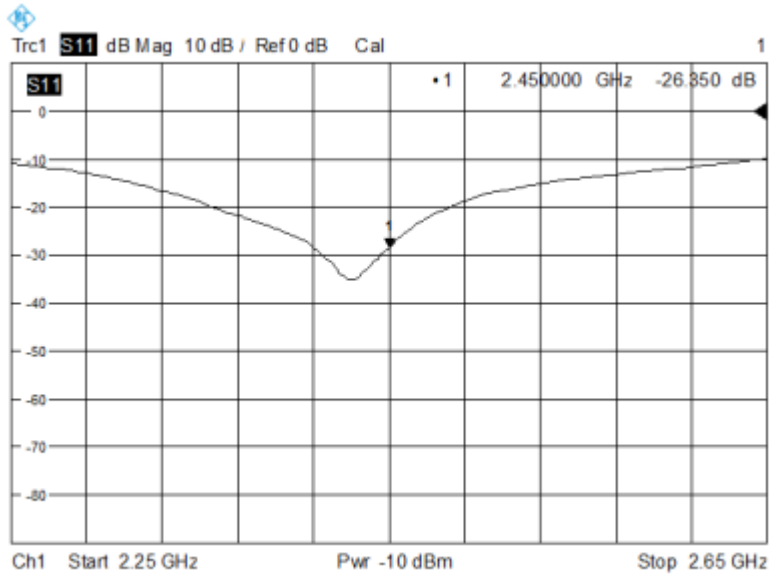

Impedance

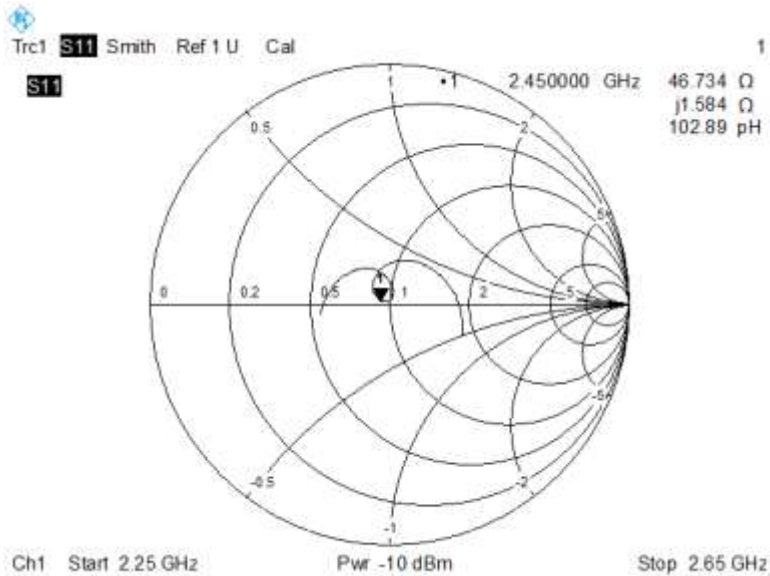





RETURN LOSS AND IMPEDANCE IN BODY LIQUID

| Meas. Results | Current Meas. | Previous Meas. | Max. Deviation |
|------------------|-------------------|-------------------|----------------------------|
| Return Loss (dB) | -27.330 | -27.205 | -0.5% |
| Impedance | 46.3 Ω + 0.422 jΩ | 46.8 Ω + 1.658 jΩ | 1.236Ω (Imaginary part) |

Return Loss

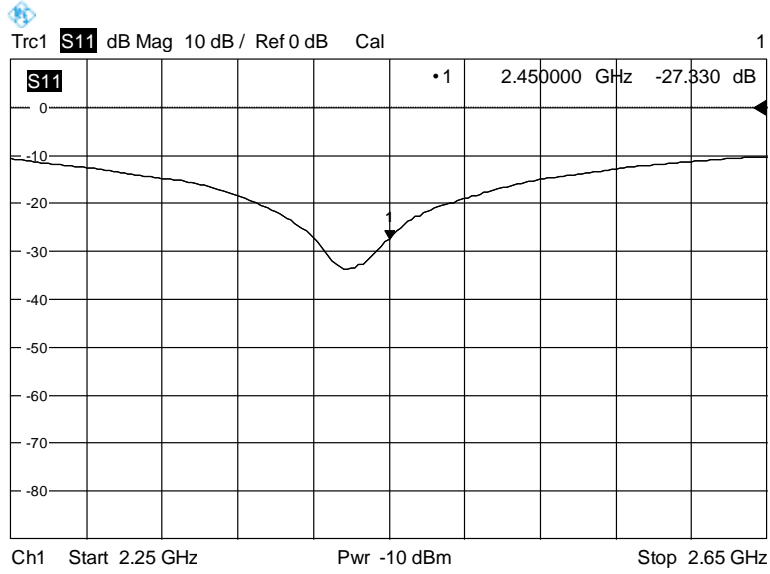


+Impedance

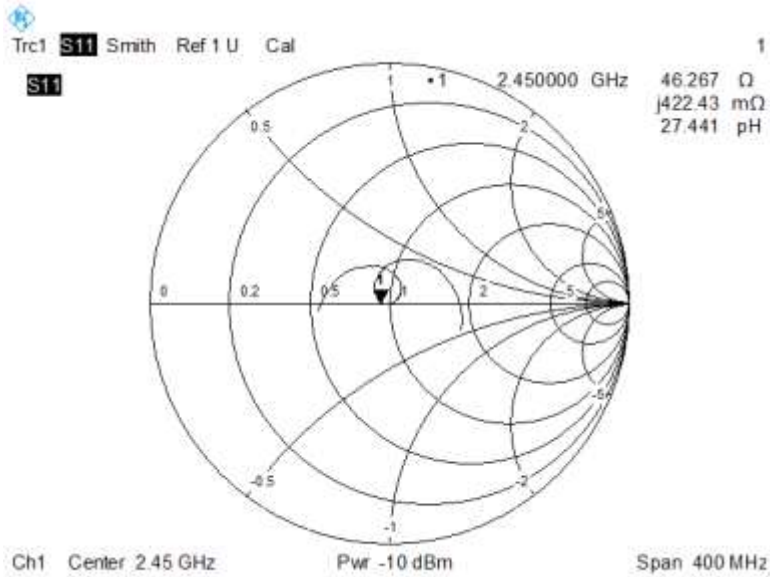

4 VALIDATION MEASUREMENT

The IEEE Std. 1528, FCC KDBs and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

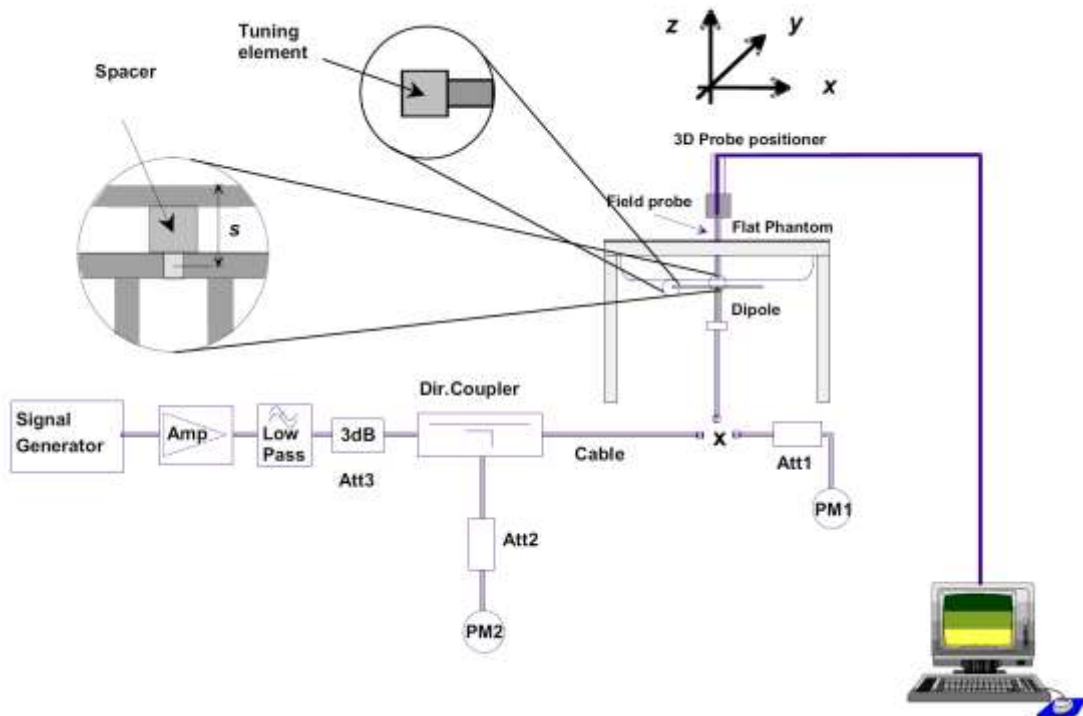



4.1 Dipole SAR Validation Measurement Result

| Freq. (MHz) | Liquid Type | Power (mW) | 1 g Measured SAR (W/kg) | Normalized SAR (W/kg) | 10 g Measured SAR (W/kg) | Normalized SAR (W/kg) | 1 g Targeted SAR (W/kg) | Tolerance (%) | 10 g Targeted SAR (W/kg) | Tolerance (%) |
|-------------|-------------|------------|-------------------------|-----------------------|--------------------------|-----------------------|-------------------------|---------------|--------------------------|---------------|
| 2450 | Head | 100 | 5.12 | 51.2 | 2.39 | 23.9 | 52.40 | -2.29 | 24.00 | -0.42 |
| | Body | 100 | 5.33 | 53.3 | 2.46 | 24.6 | 52.40 | 1.72 | 24.00 | 2.50 |



4.2 D2450V2

4.2.1 Dipole 2450 MHz Validation Measurement for Head Tissue

Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2-SN:952

Date/Time: 3/12/2019

Communication System Band: CD2450 (2450.0 MHz); Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.85$ S/m; $\epsilon_r = 39.67$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.7 Liquid Temperature: 21.2

DASY5 Configuration:

- Probe: EX3DV4 – SN7510; ConvF(7.88, 7.88, 7.88);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn685;
- Phantom: SAM (30deg probe tilt) with CRP v5.0 Right 1857; Type: QD000P40CD; Serial: TP1857
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)


Dipole validation measurement for Head Tissue/Pin= 100mW ,d=10mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 51.57 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 11.3 W/kg

SAR(1 g) = 5.12 W/kg; SAR(10 g) = 2.39 W/kg

Maximum value of SAR (measured) = 6.18 W/kg

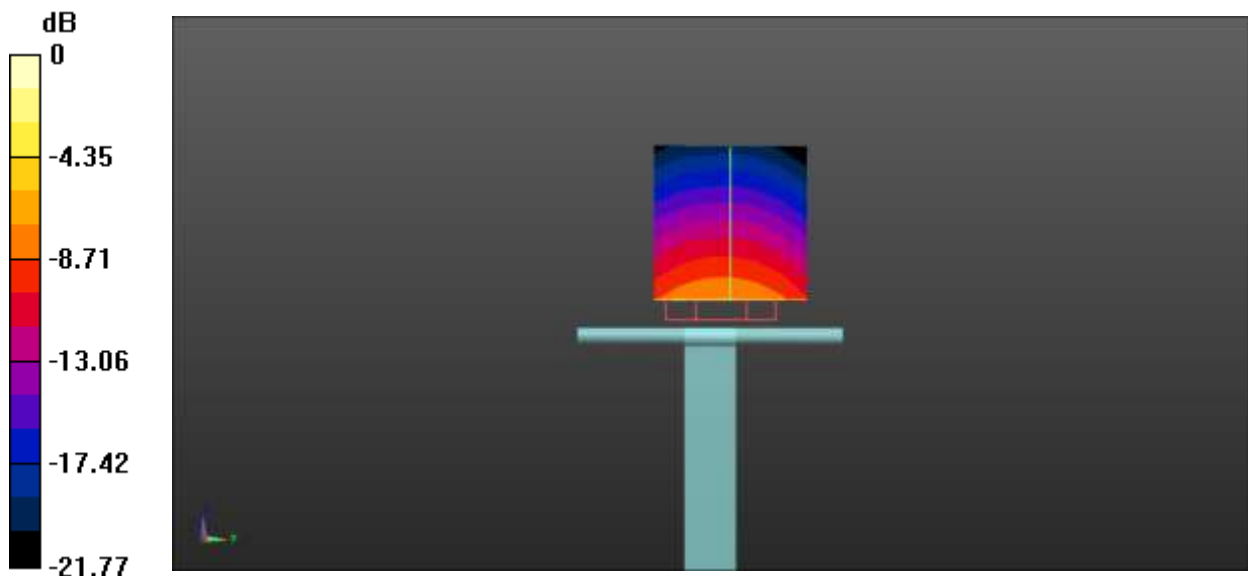

0 dB = 6.18 W/kg



4.2.2 Dipole 2450 MHz Validation Measurement for Body Tissue

Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2-SN:952

Date/Time: 3/12/2019

Communication System Band: D2450 (2450.0 MHz); Frequency: 2450 MHz; Duty Cycle: 1:1

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.93$ S/m; $\epsilon_r = 53.66$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Ambient Temperature: 22.7 Liquid Temperature: 21.4

DASY5 Configuration:

- Probe: EX3DV4 – SN7510; ConvF(7.8, 7.8, 7.8);
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn685;
- Phantom: SAM (30deg probe tilt) with CRP v5.0 left 1859; Type: QD000P40CD; Serial: TP1859
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole validation measurement for Body Tissue/Pin= 100mW ,d=10mm /Zoom


Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 48.66 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 11.4 W/kg

SAR(1 g) = 5.33 W/kg; SAR(10 g) = 2.46 W/kg

Maximum value of SAR (measured) = 5.97 W/kg

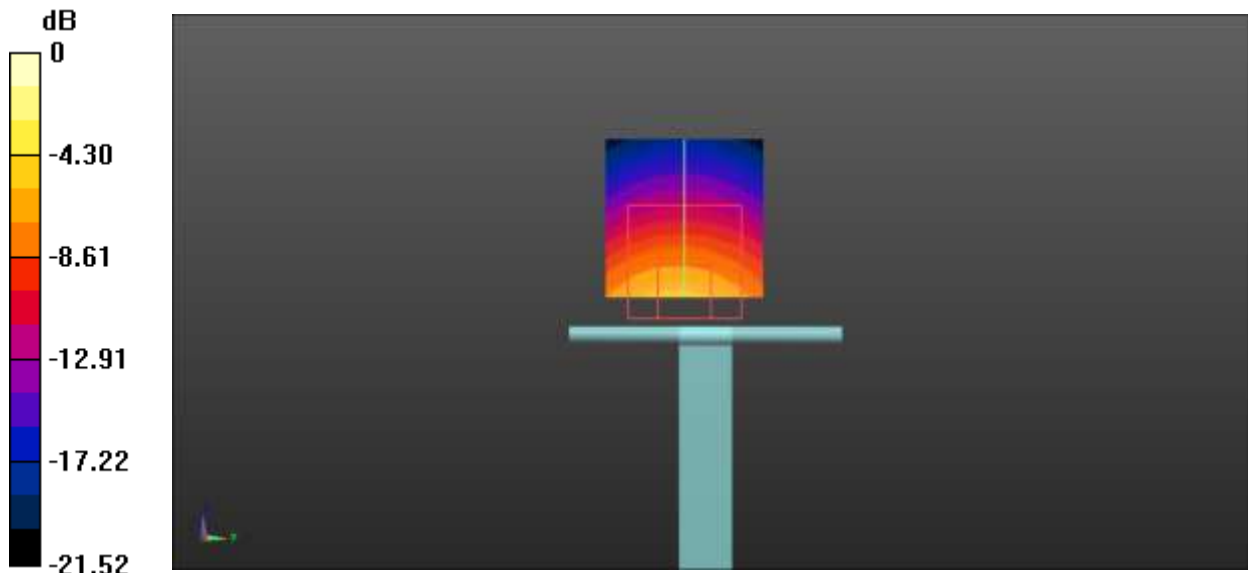

0 dB = 5.97 W/kg

--END OF REPORT--