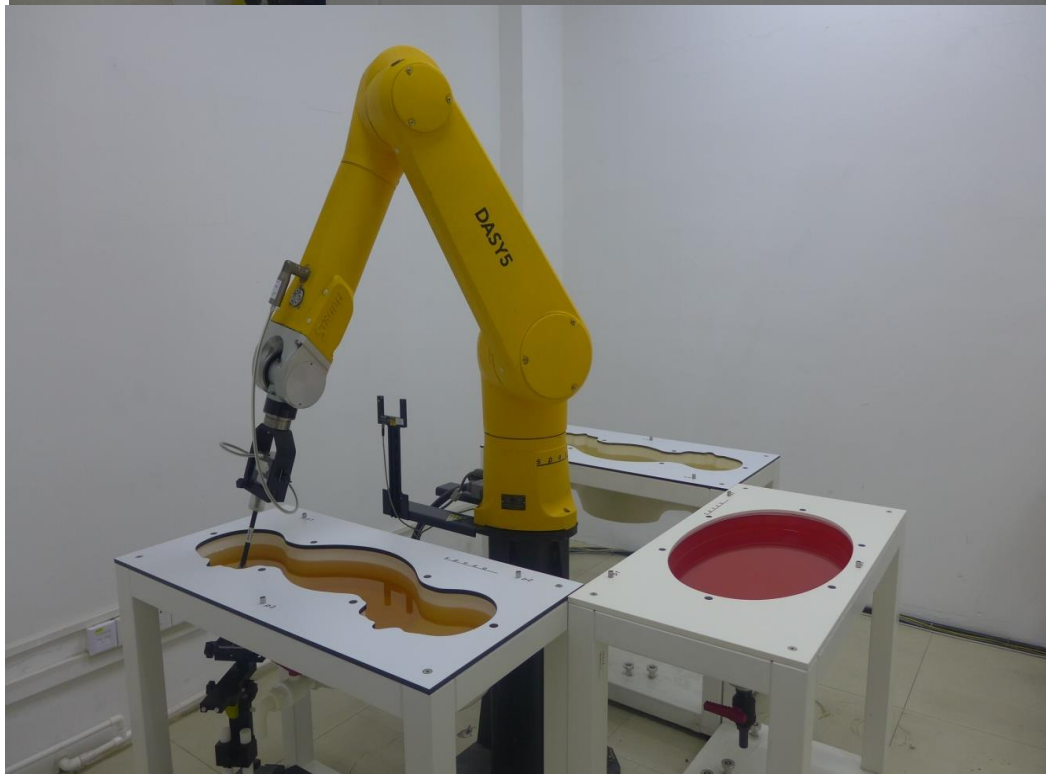

Appendix D

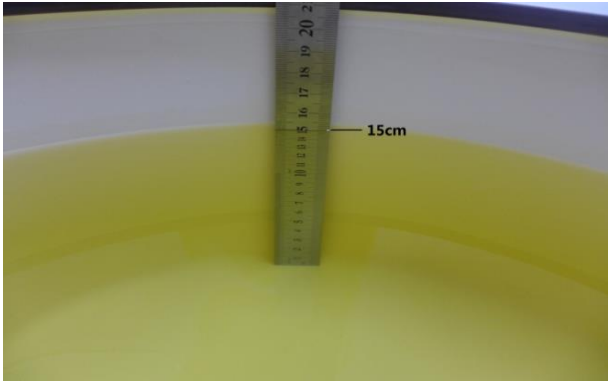
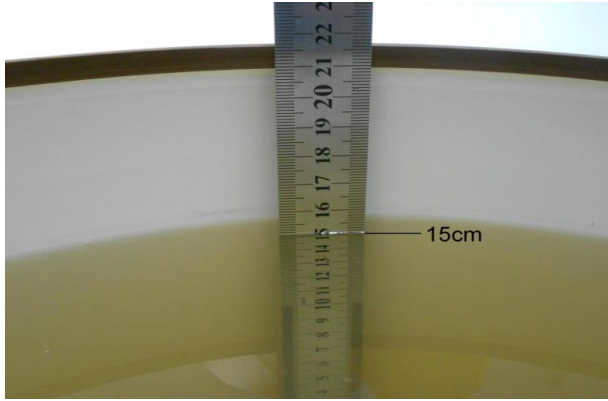
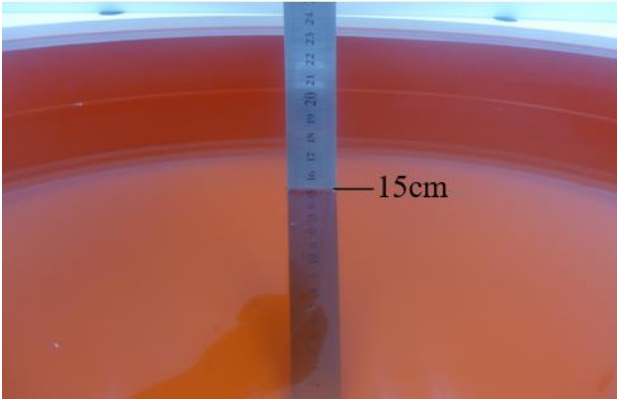
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details
5. Serial Number of EUT

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Body 750</p>	<p>Photo 2: Tissue Simulant Liquid for Body 835</p>
	
<p>Photo 3: Tissue Simulant Liquid for Body 2450</p>	<p>N/A</p>
	<p>N/A</p>

3. Photographs of EUT test position




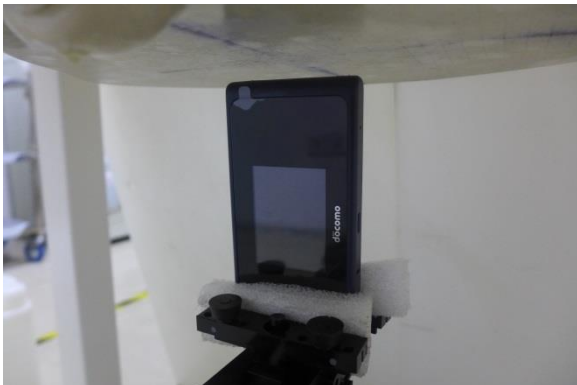
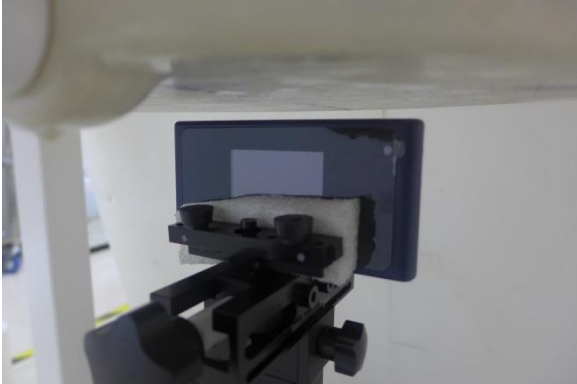






Photo 4: Front side 10mm	Photo 5: Back side 10mm
	
Photo 6: Left side 10mm	Photo 7: Right side 10mm
	
Photo 8: Top side 10mm	Photo 9: Bottom side 10mm
	

Photo 10: Front side 13mm	Photo 11: Back side 13mm
	
Photo 12: Right side 13mm	N/A
	N/A

4. EUT Constructional Details

Photo 13: Front View	Photo 14: Back View
 <p>A photograph showing the front view of a blue mobile phone. The phone has a black screen and the 'docomo' logo is visible at the bottom. Two rulers are placed around the phone for scale: one vertically on the left and one horizontally at the bottom. The background is a blue surface.</p>	 <p>A photograph showing the back view of the same blue mobile phone. The back cover is a solid blue color. A ruler is placed horizontally below the phone for scale. The background is a blue surface.</p>