

| | | | | | | | | |
|-----------|--|---|---------|--------|-------|------|------|---------|
| 10493-AAB | LTE-TDD (SC-FDMA, 50% RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.70 | 66.64 | 16.00 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 3.93 | 68.31 | 17.13 | | 80.0 | |
| | | Z | 100.00 | 141.88 | 44.26 | | 80.0 | |
| 10494-AAB | LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9) | X | 3.54 | 69.01 | 16.57 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 4.18 | 72.54 | 18.61 | | 80.0 | |
| | | Z | 100.00 | 149.55 | 46.93 | | 80.0 | |
| 10495-AAB | LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.64 | 66.96 | 16.14 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 3.90 | 68.77 | 17.37 | | 80.0 | |
| | | Z | 100.00 | 143.61 | 45.02 | | 80.0 | |
| 10496-AAB | LTE-TDD (SC-FDMA, 50% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.74 | 66.85 | 16.14 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 3.97 | 68.52 | 17.30 | | 80.0 | |
| | | Z | 100.00 | 142.51 | 44.66 | | 80.0 | |
| 10497-AAA | LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, QPSK, UL Subframe=2,3,4,7,8,9) | X | 1.56 | 62.59 | 10.95 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 1.91 | 65.75 | 12.62 | | 80.0 | |
| | | Z | 100.00 | 167.80 | 50.85 | | 80.0 | |
| 10498-AAA | LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9) | X | 1.46 | 60.03 | 8.70 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 1.45 | 60.57 | 8.96 | | 80.0 | |
| | | Z | 7420.13 | 188.24 | 44.06 | | 80.0 | |
| 10499-AAA | LTE-TDD (SC-FDMA, 100% RB, 1.4 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9) | X | 1.48 | 60.00 | 8.56 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 1.41 | 60.09 | 8.55 | | 80.0 | |
| | | Z | 2476.53 | 164.73 | 38.68 | | 80.0 | |
| 10500-AAA | LTE-TDD (SC-FDMA, 100% RB, 3 MHz, QPSK, UL Subframe=2,3,4,7,8,9) | X | 2.66 | 67.85 | 15.57 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 3.46 | 72.87 | 18.21 | | 80.0 | |
| | | Z | 100.00 | 162.25 | 51.13 | | 80.0 | |
| 10501-AAA | LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9) | X | 2.89 | 66.22 | 14.61 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 3.34 | 69.22 | 16.27 | | 80.0 | |
| | | Z | 100.00 | 144.43 | 43.48 | | 80.0 | |
| 10502-AAA | LTE-TDD (SC-FDMA, 100% RB, 3 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9) | X | 2.95 | 66.17 | 14.55 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 3.39 | 69.04 | 16.13 | | 80.0 | |
| | | Z | 100.00 | 142.63 | 42.69 | | 80.0 | |
| 10503-AAB | LTE-TDD (SC-FDMA, 100% RB, 5 MHz, QPSK, UL Subframe=2,3,4,7,8,9) | X | 2.96 | 68.30 | 16.19 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 3.62 | 72.48 | 18.53 | | 80.0 | |
| | | Z | 100.00 | 158.22 | 50.12 | | 80.0 | |
| 10504-AAB | LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.17 | 66.64 | 15.58 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 3.51 | 69.08 | 17.07 | | 80.0 | |
| | | Z | 100.00 | 146.21 | 45.28 | | 80.0 | |
| 10505-AAB | LTE-TDD (SC-FDMA, 100% RB, 5 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.27 | 66.63 | 15.60 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 3.60 | 68.91 | 17.01 | | 80.0 | |
| | | Z | 100.00 | 144.59 | 44.65 | | 80.0 | |
| 10506-AAB | LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK, UL Subframe=2,3,4,7,8,9) | X | 3.51 | 68.90 | 16.51 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 4.14 | 72.40 | 18.54 | | 80.0 | |
| | | Z | 100.00 | 149.45 | 46.87 | | 80.0 | |
| 10507-AAB | LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.63 | 66.90 | 16.10 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 3.88 | 68.71 | 17.34 | | 80.0 | |
| | | Z | 100.00 | 143.58 | 45.00 | | 80.0 | |

| | | | | | | | | |
|-----------|---|---|--------|--------|-----------|------|-------|---------|
| 10508-AAB | LTE-TDD (SC-FDMA, 100% RB, 10 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9) | X | 3.73 | 66.79 | 16.10 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 3.96 | 68.45 | 17.26 | | 80.0 | |
| | | Z | 100.00 | 142.43 | 44.62 | | 80.0 | |
| 10509-AAB | LTE-TDD (SC-FDMA, 100% RB, 15 MHz, QPSK, UL Subframe=2,3,4,7,8,9) | X | 3.99 | 68.59 | 16.47 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 4.46 | 71.13 | 18.04 | | 80.0 | |
| | | Z | 100.00 | 142.11 | 44.18 | | 80.0 | |
| 10510-AAB | LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9) | X | 4.16 | 67.04 | 16.33 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 4.36 | 68.42 | 17.34 | | 80.0 | |
| | | Z | 50.98 | 125.20 | 40.21 | | 80.0 | |
| 10511-AAB | LTE-TDD (SC-FDMA, 100% RB, 15 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9) | X | 4.23 | 66.91 | 16.33 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 4.42 | 68.19 | 17.28 | | 80.0 | |
| | | Z | 30.77 | 113.70 | 37.01 | | 80.0 | |
| 10512-AAB | LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK, UL Subframe=2,3,4,7,8,9) | X | 4.00 | 69.40 | 16.64 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 4.65 | 72.58 | 18.49 | | 80.0 | |
| | | Z | 100.00 | 143.21 | 44.41 | | 80.0 | |
| 10513-AAB | LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 16-QAM, UL Subframe=2,3,4,7,8,9) | X | 4.02 | 67.16 | 16.35 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 4.25 | 68.65 | 17.43 | | 80.0 | |
| | | Z | 100.00 | 140.91 | 44.33 | | 80.0 | |
| 10514-AAB | LTE-TDD (SC-FDMA, 100% RB, 20 MHz, 64-QAM, UL Subframe=2,3,4,7,8,9) | X | 4.08 | 66.91 | 16.31 | 2.23 | 80.0 | ± 9.6 % |
| | | Y | 4.27 | 68.26 | 17.32 | | 80.0 | |
| | | Z | 41.23 | 121.15 | 39.27 | | 80.0 | |
| 10515-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 99pc duty cycle) | X | 0.96 | 62.66 | 14.25 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 1.02 | 63.95 | 15.44 | | 150.0 | |
| | | Z | 100.00 | 263.21 | 93.12 | | 150.0 | |
| 10516-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 99pc duty cycle) | X | 0.52 | 66.95 | 15.36 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 0.81 | 75.72 | 20.49 | | 150.0 | |
| | | Z | 0.24 | 60.00 | 15168.414 | | 150.0 | |
| 10517-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 99pc duty cycle) | X | 0.80 | 64.07 | 14.59 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 0.89 | 66.47 | 16.48 | | 150.0 | |
| | | Z | 100.00 | 354.05 | 129.74 | | 150.0 | |
| 10518-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 99pc duty cycle) | X | 4.51 | 66.62 | 16.09 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.52 | 66.96 | 16.40 | | 150.0 | |
| | | Z | 5.77 | 75.40 | 23.05 | | 150.0 | |
| 10519-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 99pc duty cycle) | X | 4.69 | 66.84 | 16.21 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.69 | 67.16 | 16.50 | | 150.0 | |
| | | Z | 5.89 | 75.21 | 22.89 | | 150.0 | |
| 10520-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 99pc duty cycle) | X | 4.54 | 66.79 | 16.13 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.54 | 67.12 | 16.42 | | 150.0 | |
| | | Z | 5.89 | 75.94 | 23.25 | | 150.0 | |
| 10521-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 99pc duty cycle) | X | 4.47 | 66.78 | 16.11 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.48 | 67.11 | 16.41 | | 150.0 | |
| | | Z | 5.86 | 76.21 | 23.41 | | 150.0 | |
| 10522-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 99pc duty cycle) | X | 4.53 | 66.88 | 16.20 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.54 | 67.24 | 16.51 | | 150.0 | |

| | | | | | | | | |
|-----------|--|---|------|-------|-------|------|-------|---------|
| | | Z | 5.94 | 76.40 | 23.51 | | 150.0 | |
| 10523-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 99pc duty cycle) | X | 4.42 | 66.76 | 16.05 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.43 | 67.14 | 16.38 | | 150.0 | |
| | | Z | 6.01 | 77.05 | 23.77 | | 150.0 | |
| 10524-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 99pc duty cycle) | X | 4.48 | 66.80 | 16.16 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.48 | 67.15 | 16.48 | | 150.0 | |
| | | Z | 5.91 | 76.54 | 23.62 | | 150.0 | |
| 10525-AAA | IEEE 802.11ac WiFi (20MHz, MCS0, 99pc duty cycle) | X | 4.47 | 65.86 | 15.76 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.49 | 66.23 | 16.08 | | 150.0 | |
| | | Z | 5.96 | 75.26 | 22.99 | | 150.0 | |
| 10526-AAA | IEEE 802.11ac WiFi (20MHz, MCS1, 99pc duty cycle) | X | 4.63 | 66.21 | 15.90 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.64 | 66.57 | 16.22 | | 150.0 | |
| | | Z | 6.19 | 75.75 | 23.13 | | 150.0 | |
| 10527-AAA | IEEE 802.11ac WiFi (20MHz, MCS2, 99pc duty cycle) | X | 4.55 | 66.17 | 15.84 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.56 | 66.53 | 16.16 | | 150.0 | |
| | | Z | 6.23 | 76.22 | 23.33 | | 150.0 | |
| 10528-AAA | IEEE 802.11ac WiFi (20MHz, MCS3, 99pc duty cycle) | X | 4.57 | 66.18 | 15.87 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.58 | 66.55 | 16.19 | | 150.0 | |
| | | Z | 6.21 | 76.10 | 23.30 | | 150.0 | |
| 10529-AAA | IEEE 802.11ac WiFi (20MHz, MCS4, 99pc duty cycle) | X | 4.57 | 66.18 | 15.87 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.58 | 66.55 | 16.19 | | 150.0 | |
| | | Z | 6.21 | 76.10 | 23.30 | | 150.0 | |
| 10531-AAA | IEEE 802.11ac WiFi (20MHz, MCS6, 99pc duty cycle) | X | 4.55 | 66.27 | 15.88 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.56 | 66.63 | 16.20 | | 150.0 | |
| | | Z | 6.29 | 76.60 | 23.51 | | 150.0 | |
| 10532-AAA | IEEE 802.11ac WiFi (20MHz, MCS7, 99pc duty cycle) | X | 4.42 | 66.12 | 15.81 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.43 | 66.49 | 16.13 | | 150.0 | |
| | | Z | 6.20 | 76.82 | 23.66 | | 150.0 | |
| 10533-AAA | IEEE 802.11ac WiFi (20MHz, MCS8, 99pc duty cycle) | X | 4.58 | 66.23 | 15.87 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 4.59 | 66.62 | 16.19 | | 150.0 | |
| | | Z | 6.34 | 76.60 | 23.48 | | 150.0 | |
| 10534-AAA | IEEE 802.11ac WiFi (40MHz, MCS0, 99pc duty cycle) | X | 5.11 | 66.30 | 15.95 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.12 | 66.57 | 16.22 | | 150.0 | |
| | | Z | 6.21 | 72.90 | 21.62 | | 150.0 | |
| 10535-AAA | IEEE 802.11ac WiFi (40MHz, MCS1, 99pc duty cycle) | X | 5.17 | 66.48 | 16.03 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.18 | 66.75 | 16.31 | | 150.0 | |
| | | Z | 6.34 | 73.31 | 21.81 | | 150.0 | |
| 10536-AAA | IEEE 802.11ac WiFi (40MHz, MCS2, 99pc duty cycle) | X | 5.04 | 66.43 | 15.98 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.06 | 66.72 | 16.27 | | 150.0 | |
| | | Z | 6.28 | 73.63 | 21.98 | | 150.0 | |
| 10537-AAA | IEEE 802.11ac WiFi (40MHz, MCS3, 99pc duty cycle) | X | 5.10 | 66.40 | 15.97 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.11 | 66.67 | 16.25 | | 150.0 | |
| | | Z | 6.39 | 73.67 | 21.97 | | 150.0 | |
| 10538-AAA | IEEE 802.11ac WiFi (40MHz, MCS4, 99pc duty cycle) | X | 5.19 | 66.41 | 16.02 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.19 | 66.67 | 16.28 | | 150.0 | |
| | | Z | 6.31 | 73.05 | 21.69 | | 150.0 | |
| 10540-AAA | IEEE 802.11ac WiFi (40MHz, MCS6, 99pc duty cycle) | X | 5.12 | 66.42 | 16.04 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.12 | 66.66 | 16.30 | | 150.0 | |
| | | Z | 6.18 | 72.92 | 21.68 | | 150.0 | |

| | | | | | | | | |
|-----------|---|---|------|-------|-------|------|-------|---------|
| 10541-AAA | IEEE 802.11ac WiFi (40MHz, MCS7, 99pc duty cycle) | X | 5.09 | 66.30 | 15.97 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.10 | 66.56 | 16.23 | | 150.0 | |
| | | Z | 6.12 | 72.66 | 21.54 | | 150.0 | |
| 10542-AAA | IEEE 802.11ac WiFi (40MHz, MCS8, 99pc duty cycle) | X | 5.25 | 66.38 | 16.02 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.26 | 66.63 | 16.29 | | 150.0 | |
| | | Z | 6.26 | 72.49 | 21.41 | | 150.0 | |
| 10543-AAA | IEEE 802.11ac WiFi (40MHz, MCS9, 99pc duty cycle) | X | 5.32 | 66.41 | 16.06 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.32 | 66.64 | 16.31 | | 150.0 | |
| | | Z | 6.40 | 72.71 | 21.52 | | 150.0 | |
| 10544-AAA | IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle) | X | 5.42 | 66.43 | 15.96 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.44 | 66.66 | 16.20 | | 150.0 | |
| | | Z | 6.33 | 71.61 | 20.82 | | 150.0 | |
| 10545-AAA | IEEE 802.11ac WiFi (80MHz, MCS1, 99pc duty cycle) | X | 5.61 | 66.83 | 16.10 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.63 | 67.09 | 16.37 | | 150.0 | |
| | | Z | 6.89 | 73.16 | 21.47 | | 150.0 | |
| 10546-AAA | IEEE 802.11ac WiFi (80MHz, MCS2, 99pc duty cycle) | X | 5.48 | 66.62 | 16.02 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.49 | 66.83 | 16.26 | | 150.0 | |
| | | Z | 6.44 | 71.99 | 20.97 | | 150.0 | |
| 10547-AAA | IEEE 802.11ac WiFi (80MHz, MCS3, 99pc duty cycle) | X | 5.55 | 66.66 | 16.03 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.56 | 66.89 | 16.28 | | 150.0 | |
| | | Z | 6.75 | 72.76 | 21.30 | | 150.0 | |
| 10548-AAA | IEEE 802.11ac WiFi (80MHz, MCS4, 99pc duty cycle) | X | 5.77 | 67.48 | 16.41 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.77 | 67.70 | 16.66 | | 150.0 | |
| | | Z | 7.54 | 75.19 | 22.36 | | 150.0 | |
| 10550-AAA | IEEE 802.11ac WiFi (80MHz, MCS6, 99pc duty cycle) | X | 5.51 | 66.65 | 16.04 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.53 | 66.91 | 16.31 | | 150.0 | |
| | | Z | 6.90 | 73.42 | 21.63 | | 150.0 | |
| 10551-AAA | IEEE 802.11ac WiFi (80MHz, MCS7, 99pc duty cycle) | X | 5.52 | 66.69 | 16.02 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.52 | 66.89 | 16.26 | | 150.0 | |
| | | Z | 6.37 | 71.77 | 20.84 | | 150.0 | |
| 10552-AAA | IEEE 802.11ac WiFi (80MHz, MCS8, 99pc duty cycle) | X | 5.43 | 66.50 | 15.94 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.45 | 66.75 | 16.19 | | 150.0 | |
| | | Z | 6.39 | 71.92 | 20.92 | | 150.0 | |
| 10553-AAA | IEEE 802.11ac WiFi (80MHz, MCS9, 99pc duty cycle) | X | 5.51 | 66.53 | 15.98 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.52 | 66.74 | 16.22 | | 150.0 | |
| | | Z | 6.37 | 71.55 | 20.75 | | 150.0 | |
| 10554-AAA | IEEE 1602.11ac WiFi (160MHz, MCS0, 99pc duty cycle) | X | 5.83 | 66.80 | 16.05 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.86 | 67.01 | 16.28 | | 150.0 | |
| | | Z | 6.75 | 71.45 | 20.51 | | 150.0 | |
| 10555-AAA | IEEE 1602.11ac WiFi (160MHz, MCS1, 99pc duty cycle) | X | 5.95 | 67.08 | 16.17 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.97 | 67.29 | 16.40 | | 150.0 | |
| | | Z | 7.01 | 72.16 | 20.82 | | 150.0 | |
| 10556-AAA | IEEE 1602.11ac WiFi (160MHz, MCS2, 99pc duty cycle) | X | 5.97 | 67.13 | 16.18 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 6.00 | 67.35 | 16.43 | | 150.0 | |
| | | Z | 7.09 | 72.36 | 20.90 | | 150.0 | |
| 10557-AAA | IEEE 1602.11ac WiFi (160MHz, MCS3, 99pc duty cycle) | X | 5.94 | 67.03 | 16.16 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.96 | 67.23 | 16.39 | | 150.0 | |
| | | Z | 6.88 | 71.76 | 20.64 | | 150.0 | |

| | | | | | | | | |
|-----------|---|---|--------|--------|--------|------|-------|---------|
| 10558-AAA | IEEE 1602.11ac WiFi (160MHz, MCS4, 99pc duty cycle) | X | 5.98 | 67.18 | 16.25 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 6.00 | 67.39 | 16.48 | | 150.0 | |
| | | Z | 6.87 | 71.79 | 20.68 | | 150.0 | |
| 10560-AAA | IEEE 1602.11ac WiFi (160MHz, MCS6, 99pc duty cycle) | X | 5.98 | 67.04 | 16.22 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.99 | 67.24 | 16.44 | | 150.0 | |
| | | Z | 6.85 | 71.56 | 20.59 | | 150.0 | |
| 10561-AAA | IEEE 1602.11ac WiFi (160MHz, MCS7, 99pc duty cycle) | X | 5.90 | 67.01 | 16.23 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 5.92 | 67.22 | 16.47 | | 150.0 | |
| | | Z | 6.83 | 71.76 | 20.74 | | 150.0 | |
| 10562-AAA | IEEE 1602.11ac WiFi (160MHz, MCS8, 99pc duty cycle) | X | 6.01 | 67.35 | 16.40 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 6.02 | 67.51 | 16.62 | | 150.0 | |
| | | Z | 6.88 | 71.91 | 20.81 | | 150.0 | |
| 10563-AAA | IEEE 1602.11ac WiFi (160MHz, MCS9, 99pc duty cycle) | X | 6.18 | 67.47 | 16.42 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 6.11 | 67.42 | 16.53 | | 150.0 | |
| | | Z | 7.95 | 74.44 | 21.89 | | 150.0 | |
| 10564-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 99pc duty cycle) | X | 4.83 | 66.66 | 16.22 | 0.46 | 150.0 | ± 9.6 % |
| | | Y | 4.84 | 66.98 | 16.52 | | 150.0 | |
| | | Z | 5.76 | 73.50 | 22.07 | | 150.0 | |
| 10565-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 99pc duty cycle) | X | 5.06 | 67.12 | 16.56 | 0.46 | 150.0 | ± 9.6 % |
| | | Y | 5.05 | 67.41 | 16.83 | | 150.0 | |
| | | Z | 6.00 | 73.94 | 22.35 | | 150.0 | |
| 10566-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 99pc duty cycle) | X | 4.89 | 66.95 | 16.36 | 0.46 | 150.0 | ± 9.6 % |
| | | Y | 4.89 | 67.24 | 16.64 | | 150.0 | |
| | | Z | 5.90 | 74.17 | 22.41 | | 150.0 | |
| 10567-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 99pc duty cycle) | X | 4.92 | 67.36 | 16.73 | 0.46 | 150.0 | ± 9.6 % |
| | | Y | 4.92 | 67.65 | 17.01 | | 150.0 | |
| | | Z | 6.08 | 75.25 | 23.16 | | 150.0 | |
| 10568-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 99pc duty cycle) | X | 4.79 | 66.68 | 16.09 | 0.46 | 150.0 | ± 9.6 % |
| | | Y | 4.80 | 67.03 | 16.41 | | 150.0 | |
| | | Z | 5.78 | 73.87 | 22.13 | | 150.0 | |
| 10569-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 99pc duty cycle) | X | 4.88 | 67.46 | 16.79 | 0.46 | 150.0 | ± 9.6 % |
| | | Y | 4.89 | 67.80 | 17.10 | | 150.0 | |
| | | Z | 6.24 | 76.25 | 23.68 | | 150.0 | |
| 10570-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 99pc duty cycle) | X | 4.91 | 67.31 | 16.73 | 0.46 | 150.0 | ± 9.6 % |
| | | Y | 4.91 | 67.62 | 17.02 | | 150.0 | |
| | | Z | 6.08 | 75.36 | 23.23 | | 150.0 | |
| 10571-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle) | X | 1.15 | 63.63 | 14.73 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 1.22 | 65.05 | 16.04 | | 130.0 | |
| | | Z | 100.00 | 235.22 | 81.84 | | 130.0 | |
| 10572-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle) | X | 1.16 | 64.10 | 15.02 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 1.24 | 65.67 | 16.42 | | 130.0 | |
| | | Z | 100.00 | 238.71 | 83.30 | | 130.0 | |
| 10573-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 90pc duty cycle) | X | 1.10 | 73.74 | 17.96 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 3.08 | 92.78 | 26.10 | | 130.0 | |
| | | Z | 100.00 | 802.14 | 312.80 | | 130.0 | |
| 10574-AAA | IEEE 802.11b WiFi 2.4 GHz (DSSS, 11 Mbps, 90pc duty cycle) | X | 1.20 | 68.46 | 17.25 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 1.41 | 72.12 | 19.70 | | 130.0 | |
| | | Z | 100.00 | 289.47 | 104.04 | | 130.0 | |

| | | | | | | | | |
|-----------|---|---|------|-------|-------|------|-------|---------|
| 10575-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 6 Mbps, 90pc duty cycle) | X | 4.60 | 66.36 | 16.16 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.61 | 66.73 | 16.51 | | 130.0 | |
| | | Z | 5.57 | 73.76 | 22.47 | | 130.0 | |
| 10576-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 9 Mbps, 90pc duty cycle) | X | 4.62 | 66.53 | 16.24 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.64 | 66.91 | 16.59 | | 130.0 | |
| | | Z | 5.72 | 74.44 | 22.79 | | 130.0 | |
| 10577-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 12 Mbps, 90pc duty cycle) | X | 4.82 | 66.82 | 16.41 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.83 | 67.18 | 16.75 | | 130.0 | |
| | | Z | 5.87 | 74.42 | 22.74 | | 130.0 | |
| 10578-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 18 Mbps, 90pc duty cycle) | X | 4.72 | 66.98 | 16.52 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.73 | 67.33 | 16.85 | | 130.0 | |
| | | Z | 5.95 | 75.50 | 23.37 | | 130.0 | |
| 10579-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 24 Mbps, 90pc duty cycle) | X | 4.47 | 66.19 | 15.77 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.49 | 66.58 | 16.14 | | 130.0 | |
| | | Z | 5.53 | 74.04 | 22.32 | | 130.0 | |
| 10580-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 36 Mbps, 90pc duty cycle) | X | 4.52 | 66.23 | 15.79 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.53 | 66.64 | 16.17 | | 130.0 | |
| | | Z | 5.57 | 74.07 | 22.30 | | 130.0 | |
| 10581-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 48 Mbps, 90pc duty cycle) | X | 4.61 | 66.99 | 16.44 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.63 | 67.38 | 16.80 | | 130.0 | |
| | | Z | 6.06 | 76.54 | 23.83 | | 130.0 | |
| 10582-AAA | IEEE 802.11g WiFi 2.4 GHz (DSSS-OFDM, 54 Mbps, 90pc duty cycle) | X | 4.42 | 65.94 | 15.55 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.42 | 66.35 | 15.93 | | 130.0 | |
| | | Z | 5.41 | 73.63 | 22.00 | | 130.0 | |
| 10583-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle) | X | 4.60 | 66.36 | 16.16 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.61 | 66.73 | 16.51 | | 130.0 | |
| | | Z | 5.57 | 73.76 | 22.47 | | 130.0 | |
| 10584-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 90pc duty cycle) | X | 4.62 | 66.53 | 16.24 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.64 | 66.91 | 16.59 | | 130.0 | |
| | | Z | 5.72 | 74.44 | 22.79 | | 130.0 | |
| 10585-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 90pc duty cycle) | X | 4.82 | 66.82 | 16.41 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.83 | 67.18 | 16.75 | | 130.0 | |
| | | Z | 5.87 | 74.42 | 22.74 | | 130.0 | |
| 10586-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 90pc duty cycle) | X | 4.72 | 66.98 | 16.52 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.73 | 67.33 | 16.85 | | 130.0 | |
| | | Z | 5.95 | 75.50 | 23.37 | | 130.0 | |
| 10587-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 90pc duty cycle) | X | 4.47 | 66.19 | 15.77 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.49 | 66.58 | 16.14 | | 130.0 | |
| | | Z | 5.53 | 74.04 | 22.32 | | 130.0 | |
| 10588-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 90pc duty cycle) | X | 4.52 | 66.23 | 15.79 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.53 | 66.64 | 16.17 | | 130.0 | |
| | | Z | 5.57 | 74.07 | 22.30 | | 130.0 | |
| 10589-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 90pc duty cycle) | X | 4.61 | 66.99 | 16.44 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.63 | 67.38 | 16.80 | | 130.0 | |
| | | Z | 6.06 | 76.54 | 23.83 | | 130.0 | |
| 10590-AAA | IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 90pc duty cycle) | X | 4.42 | 65.94 | 15.55 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.42 | 66.35 | 15.93 | | 130.0 | |
| | | Z | 5.41 | 73.63 | 22.00 | | 130.0 | |

| | | | | | | | | |
|-----------|---|---|------|-------|-------|------|-------|---------|
| 10591-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle) | X | 4.75 | 66.45 | 16.29 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.77 | 66.79 | 16.61 | | 130.0 | |
| | | Z | 5.63 | 73.21 | 22.23 | | 130.0 | |
| 10592-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle) | X | 4.90 | 66.77 | 16.42 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.90 | 67.11 | 16.74 | | 130.0 | |
| | | Z | 5.83 | 73.70 | 22.41 | | 130.0 | |
| 10593-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS2, 90pc duty cycle) | X | 4.82 | 66.66 | 16.28 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.82 | 67.01 | 16.61 | | 130.0 | |
| | | Z | 5.77 | 73.76 | 22.37 | | 130.0 | |
| 10594-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS3, 90pc duty cycle) | X | 4.87 | 66.84 | 16.45 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.88 | 67.18 | 16.77 | | 130.0 | |
| | | Z | 5.85 | 74.01 | 22.57 | | 130.0 | |
| 10595-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS4, 90pc duty cycle) | X | 4.84 | 66.78 | 16.33 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.85 | 67.14 | 16.68 | | 130.0 | |
| | | Z | 5.87 | 74.24 | 22.60 | | 130.0 | |
| 10596-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS5, 90pc duty cycle) | X | 4.77 | 66.76 | 16.33 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.78 | 67.13 | 16.68 | | 130.0 | |
| | | Z | 5.82 | 74.40 | 22.72 | | 130.0 | |
| 10597-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS6, 90pc duty cycle) | X | 4.72 | 66.66 | 16.20 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.73 | 67.02 | 16.55 | | 130.0 | |
| | | Z | 5.77 | 74.27 | 22.58 | | 130.0 | |
| 10598-AAA | IEEE 802.11n (HT Mixed, 20MHz, MCS7, 90pc duty cycle) | X | 4.71 | 66.91 | 16.48 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.72 | 67.25 | 16.81 | | 130.0 | |
| | | Z | 5.86 | 75.02 | 23.15 | | 130.0 | |
| 10599-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle) | X | 5.42 | 67.00 | 16.52 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.43 | 67.25 | 16.81 | | 130.0 | |
| | | Z | 6.42 | 73.01 | 21.87 | | 130.0 | |
| 10600-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS1, 90pc duty cycle) | X | 5.54 | 67.36 | 16.67 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.55 | 67.65 | 16.98 | | 130.0 | |
| | | Z | 7.04 | 75.03 | 22.76 | | 130.0 | |
| 10601-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS2, 90pc duty cycle) | X | 5.43 | 67.13 | 16.57 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.44 | 67.42 | 16.88 | | 130.0 | |
| | | Z | 6.46 | 73.32 | 22.01 | | 130.0 | |
| 10602-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS3, 90pc duty cycle) | X | 5.53 | 67.17 | 16.51 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.57 | 67.56 | 16.87 | | 130.0 | |
| | | Z | 6.58 | 73.31 | 21.88 | | 130.0 | |
| 10603-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS4, 90pc duty cycle) | X | 5.61 | 67.47 | 16.79 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.63 | 67.80 | 17.12 | | 130.0 | |
| | | Z | 6.77 | 74.07 | 22.40 | | 130.0 | |
| 10604-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS5, 90pc duty cycle) | X | 5.44 | 67.02 | 16.55 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.50 | 67.45 | 16.93 | | 130.0 | |
| | | Z | 6.76 | 74.06 | 22.38 | | 130.0 | |
| 10605-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS6, 90pc duty cycle) | X | 5.53 | 67.26 | 16.67 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.55 | 67.59 | 17.00 | | 130.0 | |
| | | Z | 6.67 | 73.74 | 22.21 | | 130.0 | |
| 10606-AAA | IEEE 802.11n (HT Mixed, 40MHz, MCS7, 90pc duty cycle) | X | 5.27 | 66.59 | 16.19 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.28 | 66.87 | 16.50 | | 130.0 | |
| | | Z | 6.26 | 72.60 | 21.54 | | 130.0 | |

| | | | | | | | | |
|-----------|---|---|------|-------|-------|------|-------|---------|
| 10607-AAA | IEEE 802.11ac WiFi (20MHz, MCS0, 90pc duty cycle) | X | 4.58 | 65.73 | 15.89 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.61 | 66.14 | 16.26 | | 130.0 | |
| | | Z | 5.83 | 74.03 | 22.61 | | 130.0 | |
| 10608-AAA | IEEE 802.11ac WiFi (20MHz, MCS1, 90pc duty cycle) | X | 4.76 | 66.12 | 16.05 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.78 | 66.51 | 16.41 | | 130.0 | |
| | | Z | 6.08 | 74.58 | 22.80 | | 130.0 | |
| 10609-AAA | IEEE 802.11ac WiFi (20MHz, MCS2, 90pc duty cycle) | X | 4.65 | 65.94 | 15.88 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.67 | 66.36 | 16.25 | | 130.0 | |
| | | Z | 6.02 | 74.70 | 22.78 | | 130.0 | |
| 10610-AAA | IEEE 802.11ac WiFi (20MHz, MCS3, 90pc duty cycle) | X | 4.70 | 66.11 | 16.05 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.72 | 66.52 | 16.41 | | 130.0 | |
| | | Z | 6.09 | 74.94 | 22.99 | | 130.0 | |
| 10611-AAA | IEEE 802.11ac WiFi (20MHz, MCS4, 90pc duty cycle) | X | 4.61 | 65.91 | 15.88 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.63 | 66.32 | 16.26 | | 130.0 | |
| | | Z | 5.98 | 74.73 | 22.85 | | 130.0 | |
| 10612-AAA | IEEE 802.11ac WiFi (20MHz, MCS5, 90pc duty cycle) | X | 4.61 | 66.03 | 15.91 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.64 | 66.47 | 16.30 | | 130.0 | |
| | | Z | 6.10 | 75.37 | 23.13 | | 130.0 | |
| 10613-AAA | IEEE 802.11ac WiFi (20MHz, MCS6, 90pc duty cycle) | X | 4.62 | 65.91 | 15.79 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.64 | 66.32 | 16.17 | | 130.0 | |
| | | Z | 5.99 | 74.74 | 22.74 | | 130.0 | |
| 10614-AAA | IEEE 802.11ac WiFi (20MHz, MCS7, 90pc duty cycle) | X | 4.57 | 66.13 | 16.05 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.59 | 66.53 | 16.41 | | 130.0 | |
| | | Z | 6.09 | 75.68 | 23.40 | | 130.0 | |
| 10615-AAA | IEEE 802.11ac WiFi (20MHz, MCS8, 90pc duty cycle) | X | 4.61 | 65.72 | 15.64 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 4.63 | 66.15 | 16.03 | | 130.0 | |
| | | Z | 5.94 | 74.33 | 22.47 | | 130.0 | |
| 10616-AAA | IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle) | X | 5.23 | 66.22 | 16.11 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.25 | 66.52 | 16.43 | | 130.0 | |
| | | Z | 6.24 | 72.33 | 21.56 | | 130.0 | |
| 10617-AAA | IEEE 802.11ac WiFi (40MHz, MCS1, 90pc duty cycle) | X | 5.30 | 66.39 | 16.17 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.32 | 66.72 | 16.50 | | 130.0 | |
| | | Z | 6.42 | 72.91 | 21.80 | | 130.0 | |
| 10618-AAA | IEEE 802.11ac WiFi (40MHz, MCS2, 90pc duty cycle) | X | 5.18 | 66.39 | 16.19 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.21 | 66.74 | 16.53 | | 130.0 | |
| | | Z | 6.34 | 73.19 | 22.00 | | 130.0 | |
| 10619-AAA | IEEE 802.11ac WiFi (40MHz, MCS3, 90pc duty cycle) | X | 5.19 | 66.19 | 16.02 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.22 | 66.52 | 16.35 | | 130.0 | |
| | | Z | 6.39 | 72.99 | 21.80 | | 130.0 | |
| 10620-AAA | IEEE 802.11ac WiFi (40MHz, MCS4, 90pc duty cycle) | X | 5.28 | 66.23 | 16.09 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.30 | 66.54 | 16.41 | | 130.0 | |
| | | Z | 6.33 | 72.47 | 21.57 | | 130.0 | |
| 10621-AAA | IEEE 802.11ac WiFi (40MHz, MCS5, 90pc duty cycle) | X | 5.29 | 66.40 | 16.30 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.31 | 66.69 | 16.60 | | 130.0 | |
| | | Z | 6.23 | 72.27 | 21.64 | | 130.0 | |
| 10622-AAA | IEEE 802.11ac WiFi (40MHz, MCS6, 90pc duty cycle) | X | 5.30 | 66.54 | 16.36 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.33 | 66.87 | 16.69 | | 130.0 | |
| | | Z | 6.28 | 72.61 | 21.81 | | 130.0 | |

| | | | | | | | | |
|-----------|---|---|------|-------|-------|------|-------|---------|
| 10623-AAA | IEEE 802.11ac WiFi (40MHz, MCS7, 90pc duty cycle) | X | 5.18 | 66.06 | 15.98 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.20 | 66.36 | 16.30 | | 130.0 | |
| | | Z | 6.06 | 71.77 | 21.25 | | 130.0 | |
| 10624-AAA | IEEE 802.11ac WiFi (40MHz, MCS8, 90pc duty cycle) | X | 5.37 | 66.27 | 16.16 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.39 | 66.57 | 16.47 | | 130.0 | |
| | | Z | 6.30 | 71.98 | 21.36 | | 130.0 | |
| 10625-AAA | IEEE 802.11ac WiFi (40MHz, MCS9, 90pc duty cycle) | X | 5.70 | 67.13 | 16.64 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.65 | 67.24 | 16.86 | | 130.0 | |
| | | Z | 6.41 | 72.14 | 21.49 | | 130.0 | |
| 10626-AAA | IEEE 802.11ac WiFi (80MHz, MCS0, 90pc duty cycle) | X | 5.53 | 66.30 | 16.09 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.56 | 66.57 | 16.38 | | 130.0 | |
| | | Z | 6.36 | 71.13 | 20.79 | | 130.0 | |
| 10627-AAA | IEEE 802.11ac WiFi (80MHz, MCS1, 90pc duty cycle) | X | 5.76 | 66.83 | 16.31 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.79 | 67.15 | 16.63 | | 130.0 | |
| | | Z | 7.11 | 73.26 | 21.73 | | 130.0 | |
| 10628-AAA | IEEE 802.11ac WiFi (80MHz, MCS2, 90pc duty cycle) | X | 5.55 | 66.35 | 16.00 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.58 | 66.61 | 16.30 | | 130.0 | |
| | | Z | 6.41 | 71.27 | 20.75 | | 130.0 | |
| 10629-AAA | IEEE 802.11ac WiFi (80MHz, MCS3, 90pc duty cycle) | X | 5.63 | 66.40 | 16.02 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.65 | 66.69 | 16.33 | | 130.0 | |
| | | Z | 6.76 | 72.18 | 21.15 | | 130.0 | |
| 10630-AAA | IEEE 802.11ac WiFi (80MHz, MCS4, 90pc duty cycle) | X | 6.00 | 67.72 | 16.68 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 6.01 | 67.95 | 16.97 | | 130.0 | |
| | | Z | 7.85 | 75.44 | 22.62 | | 130.0 | |
| 10631-AAA | IEEE 802.11ac WiFi (80MHz, MCS5, 90pc duty cycle) | X | 5.94 | 67.66 | 16.86 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.94 | 67.86 | 17.11 | | 130.0 | |
| | | Z | 7.19 | 73.89 | 22.19 | | 130.0 | |
| 10632-AAA | IEEE 802.11ac WiFi (80MHz, MCS6, 90pc duty cycle) | X | 5.74 | 66.94 | 16.51 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.77 | 67.23 | 16.81 | | 130.0 | |
| | | Z | 7.32 | 74.18 | 22.33 | | 130.0 | |
| 10633-AAA | IEEE 802.11ac WiFi (80MHz, MCS7, 90pc duty cycle) | X | 5.62 | 66.54 | 16.13 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.64 | 66.81 | 16.43 | | 130.0 | |
| | | Z | 6.38 | 71.18 | 20.75 | | 130.0 | |
| 10634-AAA | IEEE 802.11ac WiFi (80MHz, MCS8, 90pc duty cycle) | X | 5.61 | 66.58 | 16.22 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.63 | 66.83 | 16.50 | | 130.0 | |
| | | Z | 6.47 | 71.62 | 21.03 | | 130.0 | |
| 10635-AAA | IEEE 802.11ac WiFi (80MHz, MCS9, 90pc duty cycle) | X | 5.48 | 65.86 | 15.57 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.50 | 66.13 | 15.88 | | 130.0 | |
| | | Z | 6.15 | 70.13 | 19.96 | | 130.0 | |
| 10636-AAA | IEEE 1602.11ac WiFi (160MHz, MCS0, 90pc duty cycle) | X | 5.94 | 66.67 | 16.18 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 5.98 | 66.93 | 16.46 | | 130.0 | |
| | | Z | 6.81 | 71.08 | 20.54 | | 130.0 | |
| 10637-AAA | IEEE 1602.11ac WiFi (160MHz, MCS1, 90pc duty cycle) | X | 6.09 | 67.03 | 16.34 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 6.13 | 67.30 | 16.63 | | 130.0 | |
| | | Z | 7.16 | 72.05 | 20.98 | | 130.0 | |
| 10638-AAA | IEEE 1602.11ac WiFi (160MHz, MCS2, 90pc duty cycle) | X | 6.09 | 67.00 | 16.31 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 6.13 | 67.27 | 16.59 | | 130.0 | |
| | | Z | 7.23 | 72.23 | 21.03 | | 130.0 | |

| | | | | | | | | |
|-----------|--|---|--------|---------|--------|------|-------|---------|
| 10639-AAA | IEEE 1602.11ac WiFi (160MHz, MCS3, 90pc duty cycle) | X | 6.07 | 66.96 | 16.33 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 6.10 | 67.20 | 16.60 | | 130.0 | |
| | | Z | 6.96 | 71.45 | 20.71 | | 130.0 | |
| 10640-AAA | IEEE 1602.11ac WiFi (160MHz, MCS4, 90pc duty cycle) | X | 6.07 | 66.94 | 16.26 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 6.10 | 67.20 | 16.55 | | 130.0 | |
| | | Z | 6.88 | 71.22 | 20.54 | | 130.0 | |
| 10641-AAA | IEEE 1602.11ac WiFi (160MHz, MCS5, 90pc duty cycle) | X | 6.12 | 66.87 | 16.24 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 6.16 | 67.16 | 16.54 | | 130.0 | |
| | | Z | 7.16 | 71.77 | 20.80 | | 130.0 | |
| 10642-AAA | IEEE 1602.11ac WiFi (160MHz, MCS6, 90pc duty cycle) | X | 6.16 | 67.15 | 16.56 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 6.19 | 67.38 | 16.82 | | 130.0 | |
| | | Z | 7.02 | 71.56 | 20.90 | | 130.0 | |
| 10643-AAA | IEEE 1602.11ac WiFi (160MHz, MCS7, 90pc duty cycle) | X | 6.00 | 66.80 | 16.27 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 6.03 | 67.08 | 16.57 | | 130.0 | |
| | | Z | 6.86 | 71.25 | 20.65 | | 130.0 | |
| 10644-AAA | IEEE 1602.11ac WiFi (160MHz, MCS8, 90pc duty cycle) | X | 6.14 | 67.24 | 16.51 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 6.15 | 67.44 | 16.77 | | 130.0 | |
| | | Z | 6.91 | 71.41 | 20.74 | | 130.0 | |
| 10645-AAA | IEEE 1602.11ac WiFi (160MHz, MCS9, 90pc duty cycle) | X | 6.37 | 67.56 | 16.63 | 0.46 | 130.0 | ± 9.6 % |
| | | Y | 6.28 | 67.48 | 16.75 | | 130.0 | |
| | | Z | 8.45 | 75.21 | 22.41 | | 130.0 | |
| 10646-AAC | LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,7) | X | 11.23 | 92.80 | 29.87 | 9.30 | 60.0 | ± 9.6 % |
| | | Y | 21.09 | 110.97 | 37.33 | | 60.0 | |
| | | Z | 100.00 | 173.73 | 61.54 | | 60.0 | |
| 10647-AAB | LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,7) | X | 10.46 | 91.94 | 29.69 | 9.30 | 60.0 | ± 9.6 % |
| | | Y | 18.57 | 108.91 | 36.87 | | 60.0 | |
| | | Z | 100.00 | 176.11 | 62.63 | | 60.0 | |
| 10648-AAA | CDMA2000 (1x Advanced) | X | 0.66 | 62.92 | 10.34 | 0.00 | 150.0 | ± 9.6 % |
| | | Y | 0.73 | 64.84 | 11.47 | | 150.0 | |
| | | Z | 99.99 | 1398.36 | 541.58 | | 150.0 | |

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Auden**

Certificate No: **D750V3-1078_Jun17**

CALIBRATION CERTIFICATE

Object **D750V3 - SN:1078**

Calibration procedure(s) **QA CAL-05.v9**
Calibration procedure for dipole validation kits above 700 MHz

Calibration date: **June 20, 2017**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|-----------------------------|--------------------|---------------------------------|-----------------------|
| Power meter NRP | SN: 104778 | 04-Apr-17 (No. 217-02521/02522) | Apr-18 |
| Power sensor NRP-Z91 | SN: 103244 | 04-Apr-17 (No. 217-02521) | Apr-18 |
| Power sensor NRP-Z91 | SN: 103245 | 04-Apr-17 (No. 217-02522) | Apr-18 |
| Reference 20 dB Attenuator | SN: 5058 (20k) | 07-Apr-17 (No. 217-02528) | Apr-18 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 07-Apr-17 (No. 217-02529) | Apr-18 |
| Reference Probe EX3DV4 | SN: 7349 | 31-May-17 (No. EX3-7349_May17) | May-18 |
| DAE4 | SN: 601 | 28-Mar-17 (No. DAE4-601_Mar17) | Mar-18 |

| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
|---------------------------|----------------|-----------------------------------|------------------------|
| Power meter EPM-442A | SN: GB37480704 | 07-Oct-15 (in house check Oct-16) | In house check: Oct-18 |
| Power sensor HP 8481A | SN: US37292783 | 07-Oct-15 (in house check Oct-16) | In house check: Oct-18 |
| Power sensor HP 8481A | SN: MY41092317 | 07-Oct-15 (in house check Oct-16) | In house check: Oct-18 |
| RF generator R&S SMT-06 | SN: 100972 | 15-Jun-15 (in house check Oct-16) | In house check: Oct-18 |
| Network Analyzer HP 8753E | SN: US37390585 | 18-Oct-01 (in house check Oct-16) | In house check: Oct-17 |

Calibrated by: **Leif Klysner** **Leif Klysner** **Leif Klysner**
Name Function Signature
Laboratory Technician

Approved by: **Katja Pokovic** **Katja Pokovic** **Katja Pokovic**
Technical Manager

Issued: June 27, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

| | |
|-------|---------------------------------|
| TSL | tissue simulating liquid |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|------------------------|-------------|
| DASY Version | DASY5 | V52.10.0 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Modular Flat Phantom | |
| Distance Dipole Center - TSL | 15 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 750 MHz \pm 1 MHz | |

Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Head TSL parameters | 22.0 °C | 41.9 | 0.89 mho/m |
| Measured Head TSL parameters | (22.0 \pm 0.2) °C | 41.2 \pm 6 % | 0.91 mho/m \pm 6 % |
| Head TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Head TSL

| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 2.14 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 8.39 W/kg \pm 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Head TSL | condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 1.39 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 5.47 W/kg \pm 16.5 % (k=2) |

Body TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Body TSL parameters | 22.0 °C | 55.5 | 0.96 mho/m |
| Measured Body TSL parameters | (22.0 \pm 0.2) °C | 54.8 \pm 6 % | 0.97 mho/m \pm 6 % |
| Body TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Body TSL

| SAR averaged over 1 cm ³ (1 g) of Body TSL | Condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 2.19 W/kg |
| SAR for nominal Body TSL parameters | normalized to 1W | 8.67 W/kg \pm 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Body TSL | condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 1.44 W/kg |
| SAR for nominal Body TSL parameters | normalized to 1W | 5.71 W/kg \pm 16.5 % (k=2) |

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

| | |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 55.5 Ω + 0.0 j Ω |
| Return Loss | - 25.6 dB |

Antenna Parameters with Body TSL

| | |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 51.0 Ω - 2.5 j Ω |
| Return Loss | - 31.5 dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.034 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

| | |
|-----------------|-------------------|
| Manufactured by | SPEAG |
| Manufactured on | November 15, 2012 |

DASY5 Validation Report for Head TSL

Date: 20.06.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1078

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: $f = 750$ MHz; $\sigma = 0.91$ S/m; $\epsilon_r = 41.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.49, 10.49, 10.49); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.03.2017
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 59.13 V/m; Power Drift = -0.00 dB


Peak SAR (extrapolated) = 3.27 W/kg

SAR(1 g) = 2.14 W/kg; SAR(10 g) = 1.39 W/kg

Maximum value of SAR (measured) = 2.89 W/kg

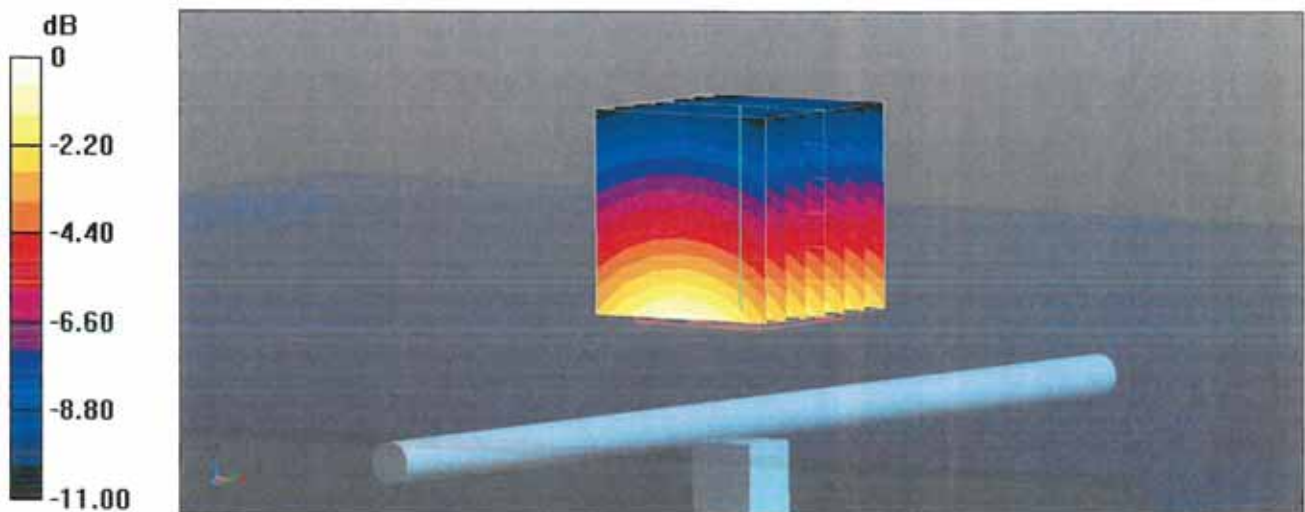

Impedance Measurement Plot for Head TSL

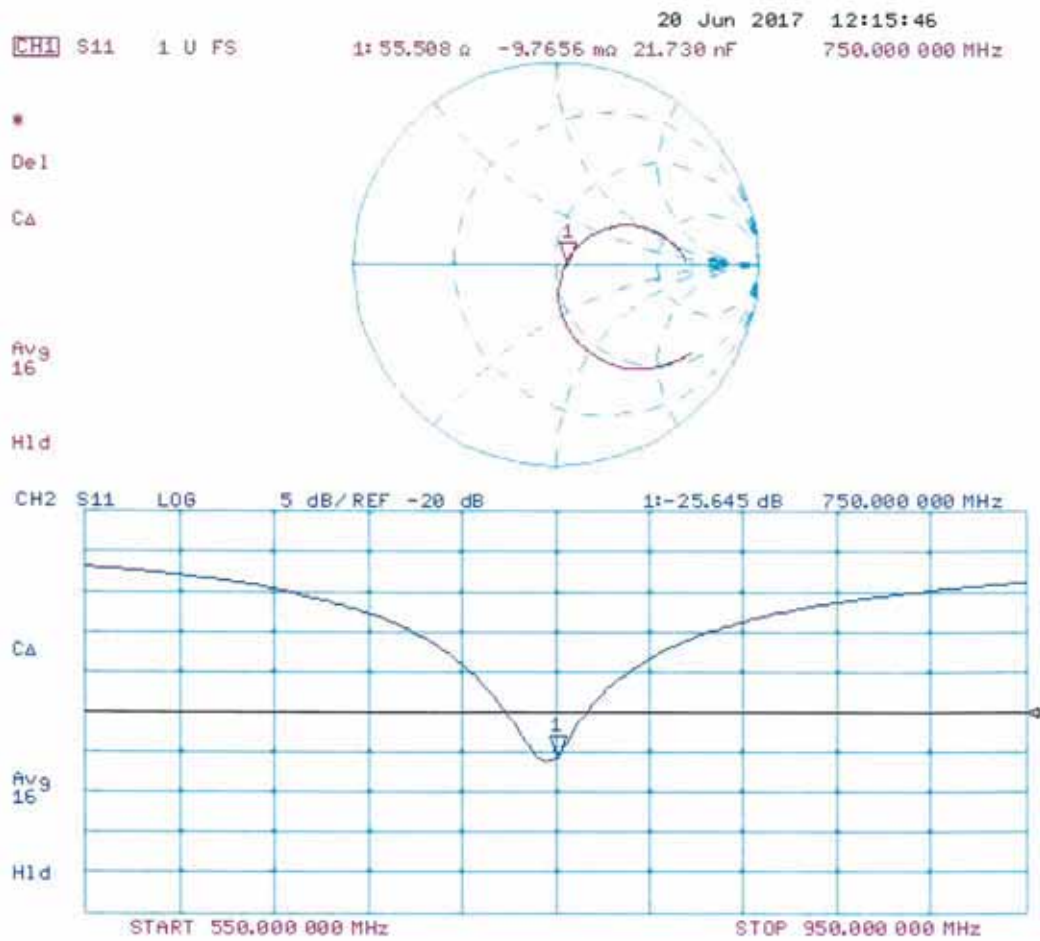

DASY5 Validation Report for Body TSL

Date: 20.06.2017

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1078

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: $f = 750$ MHz; $\sigma = 0.97$ S/m; $\epsilon_r = 54.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.35, 10.35, 10.35); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.03.2017
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.36 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.29 W/kg

SAR(1 g) = 2.19 W/kg; SAR(10 g) = 1.44 W/kg

Maximum value of SAR (measured) = 2.88 W/kg

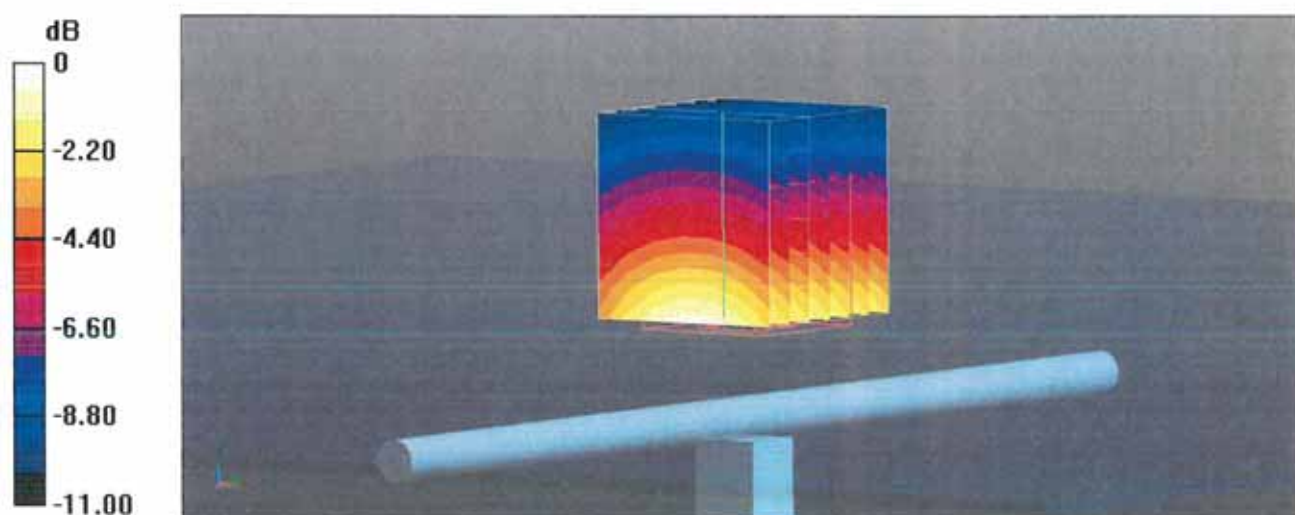

Impedance Measurement Plot for Body TSL


20 Jun 2017 12:15:01
[CH1] S11 1 U FS 1: 51.041 Ω -2.4844 Ω 85.417 pF 750.000 000 MHz

*
De1

Ca

Avg
16

H1 d

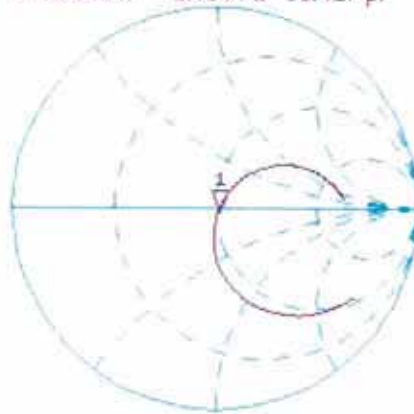


CH2 S11 LOG 5 dB/REF -20 dB 1:-31.483 dB 750.000 000 MHz

Ca

Avg
16

H1 d

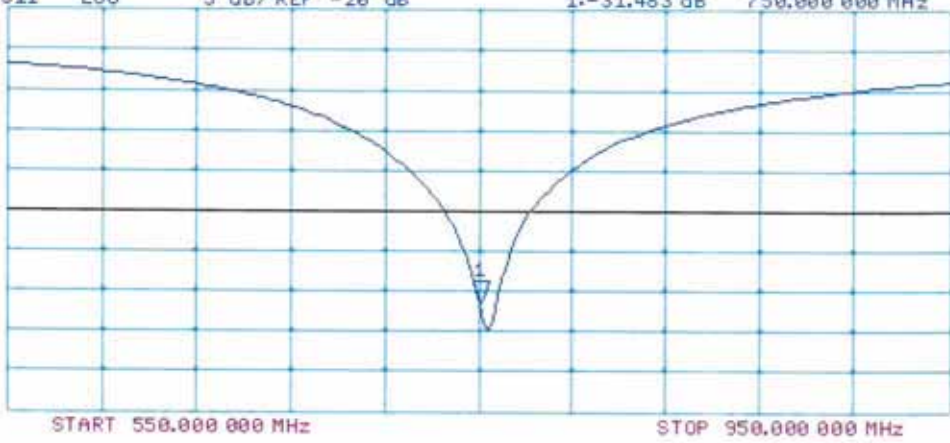



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client **Huawei-SZ (Auden)**

Certificate No: D835V2-4d126_Jul15

CALIBRATION CERTIFICATE

Object **D835V2 - SN: 4d126**

Calibration procedure(s) **QA CAL-05.v9
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **July 23, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^\circ\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A | GB37480704 | 07-Oct-14 (No. 217-02020) | Oct-15 |
| Power sensor HP 8481A | US37292783 | 07-Oct-14 (No. 217-02020) | Oct-15 |
| Power sensor HP 8481A | MY41092317 | 07-Oct-14 (No. 217-02021) | Oct-15 |
| Reference 20 dB Attenuator | SN: 5058 (20k) | 01-Apr-15 (No. 217-02131) | Mar-16 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 01-Apr-15 (No. 217-02134) | Mar-16 |
| Reference Probe ES3DV3 | SN: 3205 | 30-Dec-14 (No. ES3-3205_Dec14) | Dec-15 |
| DAE4 | SN: 601 | 18-Aug-14 (No. DAE4-601_Aug14) | Aug-15 |
| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
| RF generator R&S SMT-06 | 100005 | 04-Aug-99 (in house check Oct-13) | In house check: Oct-16 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-14) | In house check: Oct-15 |

| | | | |
|----------------|------------------------------|-----------------------------------|---------------|
| Calibrated by: | Name Michael Weber | Function Laboratory Technician | Signature |
| Approved by: | Name Katja Pokovic | Function Technical Manager | |

Issued: July 23, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Glossary:

| | |
|-------|---------------------------------|
| TSL | tissue simulating liquid |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|------------------------|-------------|
| DASY Version | DASY5 | V52.8.8 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Modular Flat Phantom | |
| Distance Dipole Center - TSL | 15 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 835 MHz \pm 1 MHz | |

Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Head TSL parameters | 22.0 °C | 41.5 | 0.90 mho/m |
| Measured Head TSL parameters | (22.0 \pm 0.2) °C | 42.4 \pm 6 % | 0.92 mho/m \pm 6 % |
| Head TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Head TSL

| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 2.33 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 9.21 W/kg \pm 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Head TSL | condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 1.51 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 5.98 W/kg \pm 16.5 % (k=2) |

Body TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Body TSL parameters | 22.0 °C | 55.2 | 0.97 mho/m |
| Measured Body TSL parameters | (22.0 \pm 0.2) °C | 54.9 \pm 6 % | 1.00 mho/m \pm 6 % |
| Body TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Body TSL

| SAR averaged over 1 cm ³ (1 g) of Body TSL | Condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 2.41 W/kg |
| SAR for nominal Body TSL parameters | normalized to 1W | 9.41 W/kg \pm 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Body TSL | condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 1.57 W/kg |
| SAR for nominal Body TSL parameters | normalized to 1W | 6.16 W/kg \pm 16.5 % (k=2) |

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

| | |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 51.5 Ω - 0.7 j Ω |
| Return Loss | - 35.8 dB |

Antenna Parameters with Body TSL

| | |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 48.0 Ω - 2.5 j Ω |
| Return Loss | - 29.6 dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.396 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

| | |
|-----------------|---------------|
| Manufactured by | SPEAG |
| Manufactured on | June 29, 2010 |

DASY5 Validation Report for Head TSL

Date: 22.07.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d126

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835$ MHz; $\sigma = 0.92$ S/m; $\epsilon_r = 42.4$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.2, 6.2, 6.2); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 56.43 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.48 W/kg

SAR(1 g) = 2.33 W/kg; SAR(10 g) = 1.51 W/kg

Maximum value of SAR (measured) = 2.73 W/kg

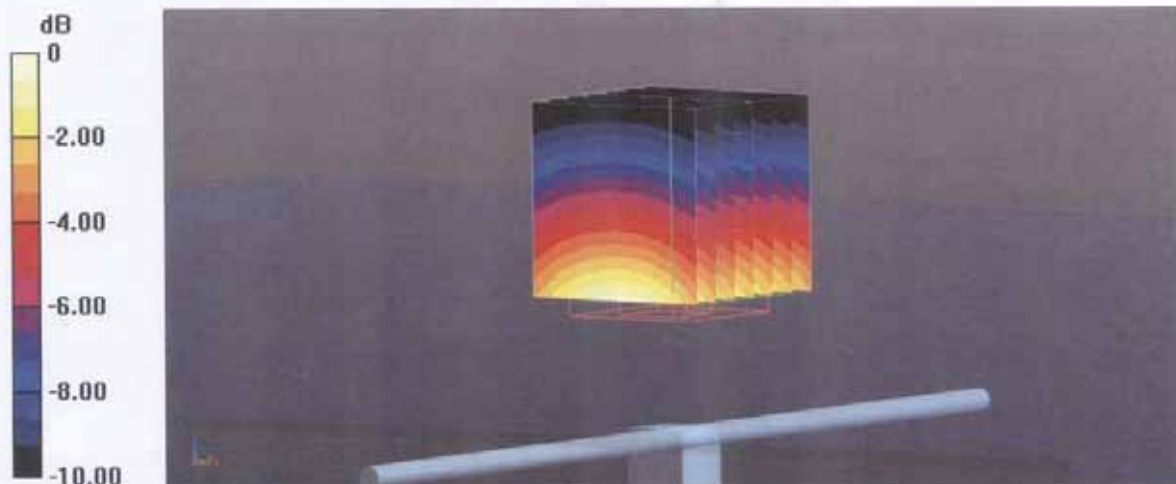



Impedance Measurement Plot for Head TSL

22 Jul 2015 09:18:59
835.000 000 MHz
CH1 S11 1 U FS 1: 51.502 Ω -662.11 m Ω 287.87 pF

De1
Cor

avg
16

H1d

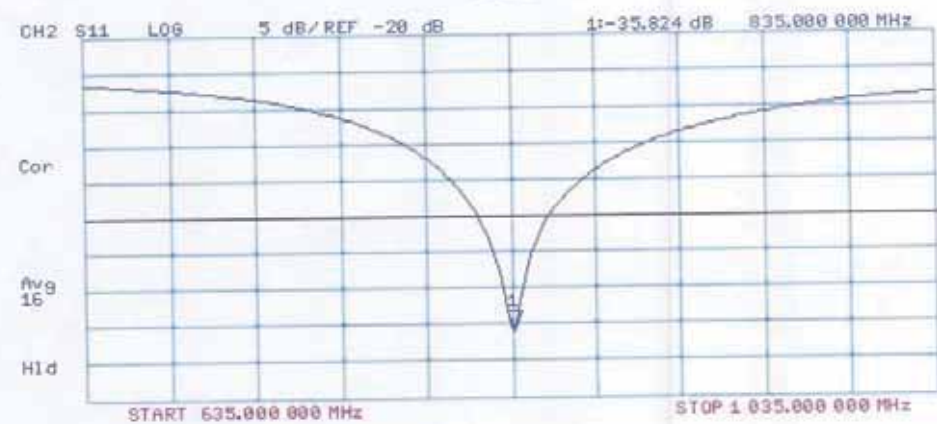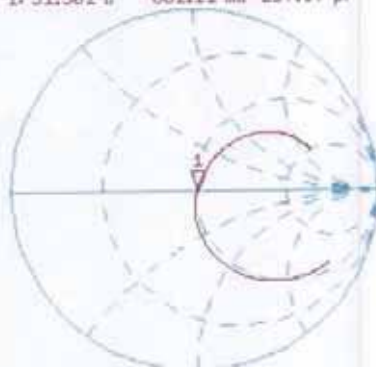

DASY5 Validation Report for Body TSL

Date: 23.07.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d126

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835$ MHz; $\sigma = 1$ S/m; $\epsilon_r = 54.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.17, 6.17, 6.17); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 55.03 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 3.56 W/kg

SAR(1 g) = 2.41 W/kg; SAR(10 g) = 1.57 W/kg

Maximum value of SAR (measured) = 2.82 W/kg

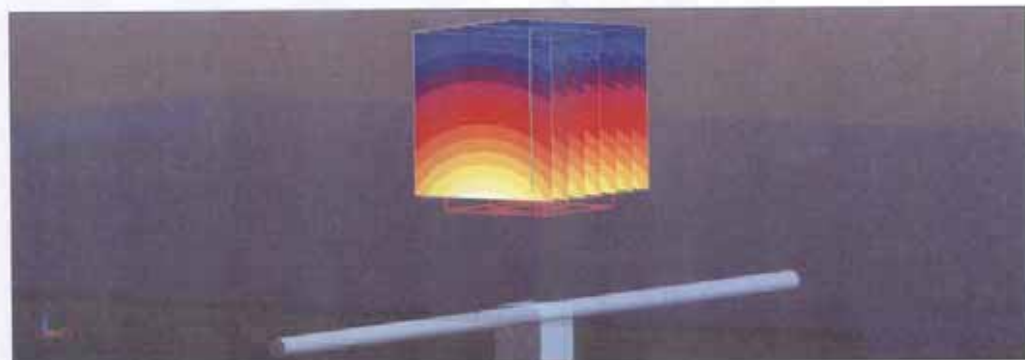


0 dB = 2.82 W/kg = 4.50 dBW/kg

Impedance Measurement Plot for Body TSL

23 Jul 2015 12:07:42
[CH1] S11 1 U FS 1: 47.975 Ω -2.5469 Ω 74.839 pF 835.000 000 MHz

De1
Ca

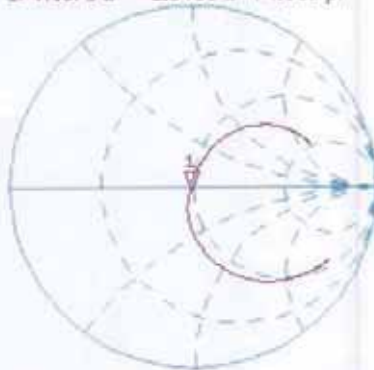

avg
16

H1d


CH2 S11 LOG 5 dB/REF -20 dB 1: -29.577 dB 835.000 000 MHz

De1

Ca

avg
16

H1d

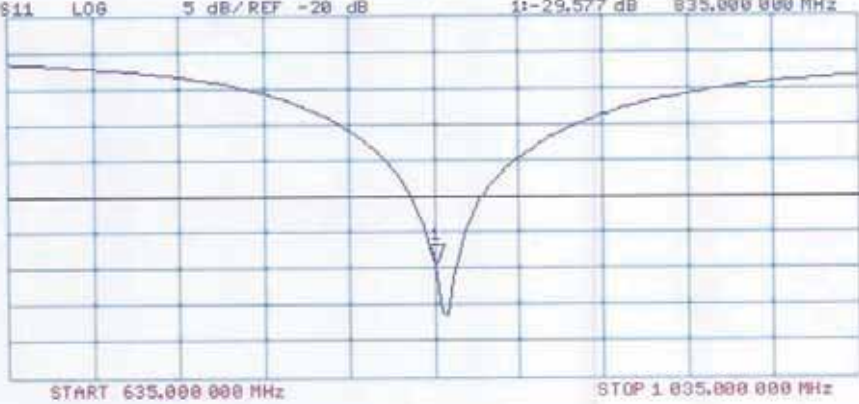

START 635.000 000 MHz

STOP 1 835.000 000 MHz



Accreditation No.: **SCS 0108**

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **Huawei-SZ (Auden)**

Certificate No: **D1900V2-5d091_Sep15**

CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d091**

Calibration procedure(s) **QA CAL-05.v9
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **September 21, 2015**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A | GB37480704 | 07-Oct-14 (No. 217-02020) | Oct-15 |
| Power sensor HP 8481A | US37292783 | 07-Oct-14 (No. 217-02020) | Oct-15 |
| Power sensor HP 8481A | MY41092317 | 07-Oct-14 (No. 217-02021) | Oct-15 |
| Reference 20 dB Attenuator | SN: 5058 (20k) | 01-Apr-15 (No. 217-02131) | Mar-16 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 01-Apr-15 (No. 217-02134) | Mar-16 |
| Reference Probe EX3DV4 | SN: 7349 | 30-Dec-14 (No. EX3-7349_Dec14) | Dec-15 |
| DAE4 | SN: 601 | 17-Aug-15 (No. DAE4-601_Aug15) | Aug-16 |
| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
| RF generator R&S SMT-06 | 100972 | 15-Jun-15 (in house check Jun-15) | In house check: Jun-18 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-14) | In house check: Oct-15 |

Calibrated by: **Name** Michael Weber **Function** Laboratory Technician

Signature

Approved by: **Name** Katja Pokovic **Function** Technical Manager

Issued: September 23, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

| | |
|-------|---------------------------------|
| TSL | tissue simulating liquid |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|------------------------|-------------|
| DASY Version | DASY5 | V52.8.8 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Modular Flat Phantom | |
| Distance Dipole Center - TSL | 10 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 1900 MHz \pm 1 MHz | |

Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Head TSL parameters | 22.0 °C | 40.0 | 1.40 mho/m |
| Measured Head TSL parameters | (22.0 \pm 0.2) °C | 39.3 \pm 6 % | 1.38 mho/m \pm 6 % |
| Head TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Head TSL

| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 10.0 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 40.2 W/kg \pm 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Head TSL | condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 5.25 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 21.1 W/kg \pm 16.5 % (k=2) |

Body TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Body TSL parameters | 22.0 °C | 53.3 | 1.52 mho/m |
| Measured Body TSL parameters | (22.0 \pm 0.2) °C | 52.6 \pm 6 % | 1.52 mho/m \pm 6 % |
| Body TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Body TSL

| SAR averaged over 1 cm ³ (1 g) of Body TSL | Condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 10.0 W/kg |
| SAR for nominal Body TSL parameters | normalized to 1W | 39.9 W/kg \pm 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Body TSL | condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 5.27 W/kg |
| SAR for nominal Body TSL parameters | normalized to 1W | 21.0 W/kg \pm 16.5 % (k=2) |

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

| | |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $52.0 \Omega + 5.5 j\Omega$ |
| Return Loss | - 24.8 dB |

Antenna Parameters with Body TSL

| | |
|--------------------------------------|-----------------------------|
| Impedance, transformed to feed point | $48.2 \Omega + 6.0 j\Omega$ |
| Return Loss | - 24.0 dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.198 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

| | |
|-----------------|--------------------|
| Manufactured by | SPEAG |
| Manufactured on | September 26, 2007 |

DASY5 Validation Report for Head TSL

Date: 21.09.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d091

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.38$ S/m; $\epsilon_r = 39.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(8.14, 8.14, 8.14); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 109.0 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 18.7 W/kg

SAR(1 g) = 10 W/kg; SAR(10 g) = 5.25 W/kg

Maximum value of SAR (measured) = 15.3 W/kg

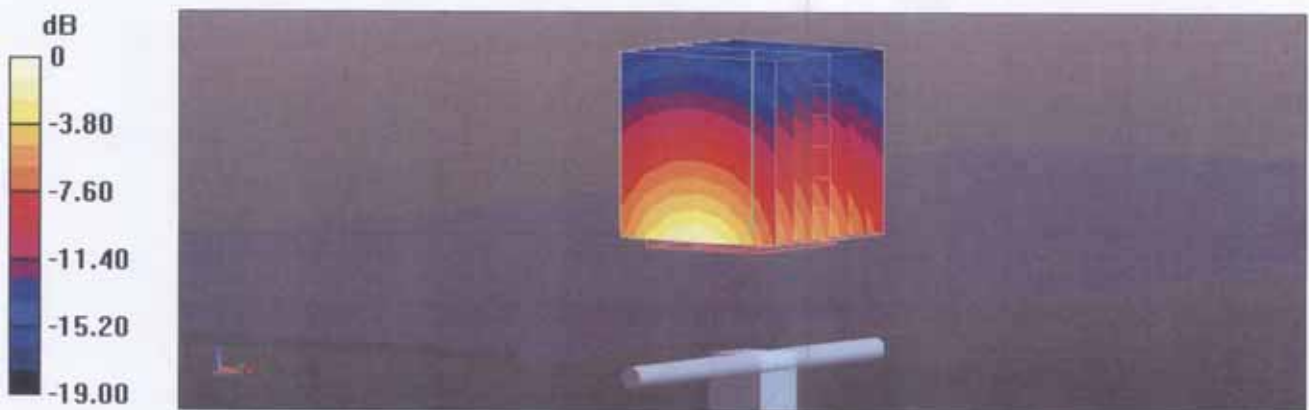

Impedance Measurement Plot for Head TSL


21 Sep 2015 12:00:21
CH1 S11 1 U FS 1: 51.953 μ 5.5293 μ 463.17 pF 1 900.000 000 MHz

De1

CA

Avg
16

H1d

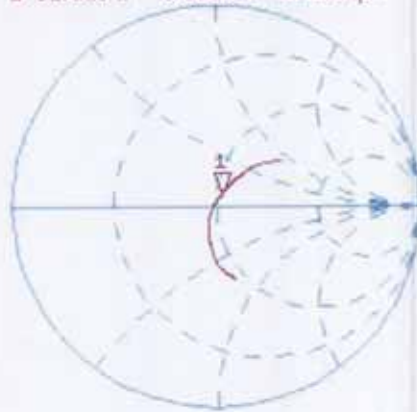


CH2 S11 LOG 5 dB/REF -20 dB 1: -24.809 dB 1 900.000 000 MHz

De1

CA

Avg
16

H1d

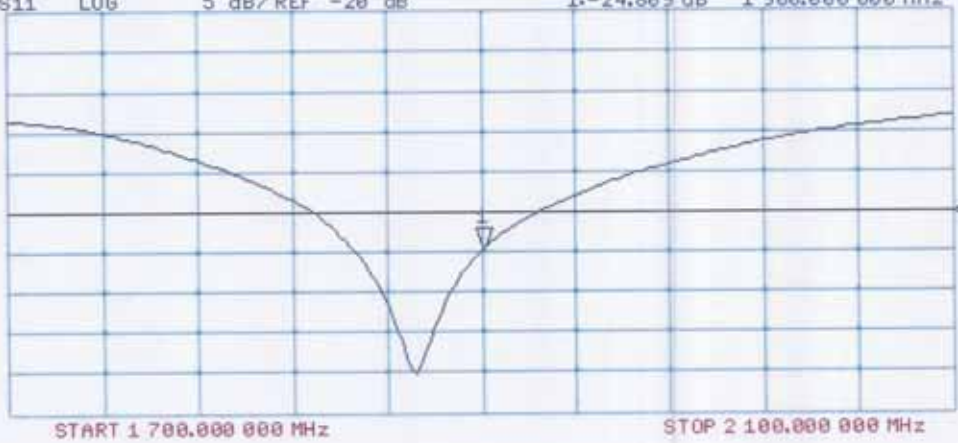

DASY5 Validation Report for Body TSL

Date: 21.09.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d091

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.52$ S/m; $\epsilon_r = 52.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.9, 7.9, 7.9); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 104.6 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 18.1 W/kg

SAR(1 g) = 10 W/kg; SAR(10 g) = 5.27 W/kg

Maximum value of SAR (measured) = 15.4 W/kg

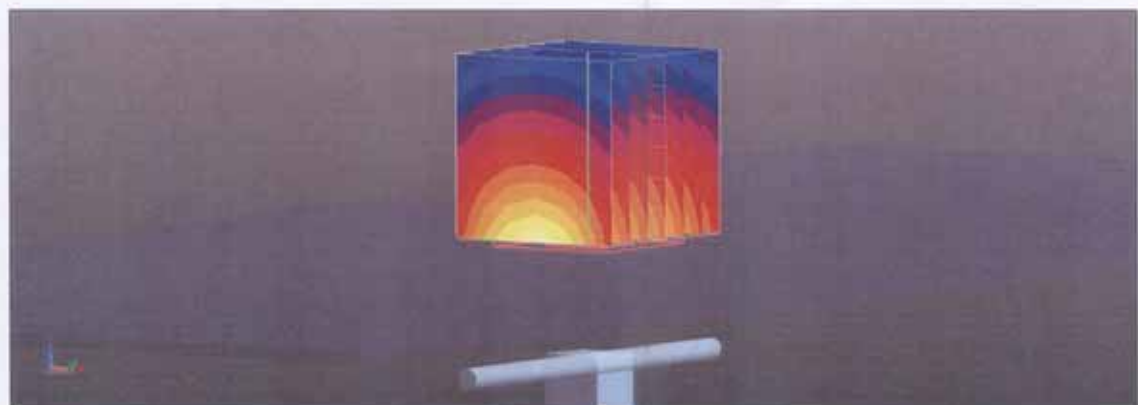

0 dB = 15.4 W/kg = 11.88 dBW/kg

Impedance Measurement Plot for Body TSL

21 Sep 2015 11:59:57

CH1 S11 1 U FS

1: 48.289 Ω 5.9512 Ω 498.58 μ H


1 900.000 000 MHz

*
De1

CA

Avg
16

H1d

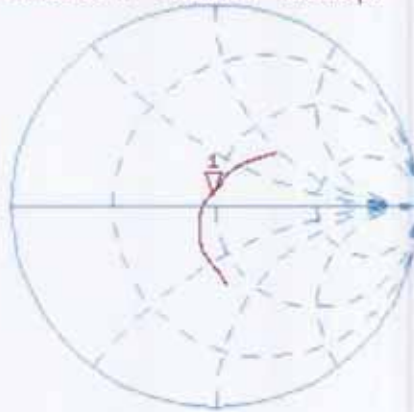

CH2 S11 LOG

5 dB/REF -20 dB

1: -23.992 dB


1 900.000 000 MHz

De1

CA

Avg
16

H1d

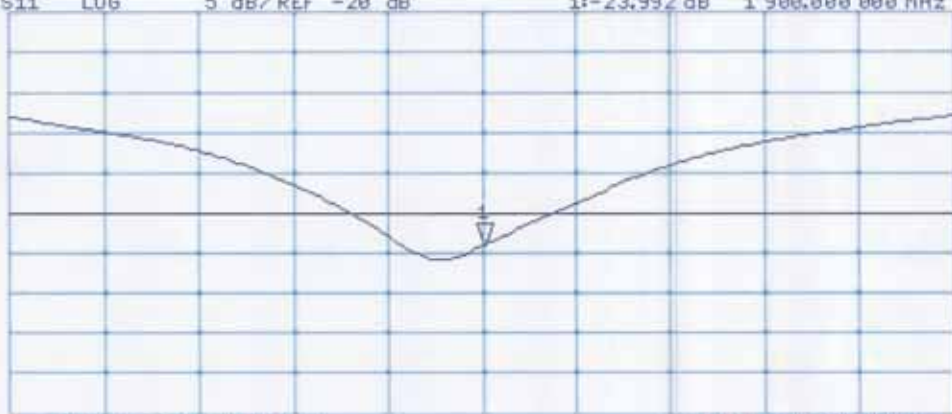

START 1 700.000 000 MHz

STOP 2 100.000 000 MHz



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Huawei (Auden)**

Certificate No: **D2450V2-978_Feb16**

CALIBRATION CERTIFICATE

Object **D2450V2 - SN: 978**

Calibration procedure(s) **QA CAL-05.v9
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **February 08, 2016**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards | ID # | Cal Date (Certificate No.) | Scheduled Calibration |
|-----------------------------|--------------------|-----------------------------------|------------------------|
| Power meter EPM-442A | GB37480704 | 07-Oct-15 (No. 217-02222) | Oct-16 |
| Power sensor HP 8481A | US37292783 | 07-Oct-15 (No. 217-02222) | Oct-16 |
| Power sensor HP 8481A | MY41092317 | 07-Oct-15 (No. 217-02223) | Oct-16 |
| Reference 20 dB Attenuator | SN: 5058 (20k) | 01-Apr-15 (No. 217-02131) | Mar-16 |
| Type-N mismatch combination | SN: 5047.2 / 06327 | 01-Apr-15 (No. 217-02134) | Mar-16 |
| Reference Probe EX3DV4 | SN: 7349 | 31-Dec-15 (No. EX3-7349_Dec15) | Dec-16 |
| DAE4 | SN: 601 | 30-Dec-15 (No. DAE4-601_Dec15) | Dec-16 |
| Secondary Standards | ID # | Check Date (in house) | Scheduled Check |
| RF generator R&S SMT-06 | 100972 | 15-Jun-15 (in house check Jun-15) | In house check: Jun-18 |
| Network Analyzer HP 8753E | US37390585 S4206 | 18-Oct-01 (in house check Oct-15) | In house check: Oct-16 |

| | | | |
|----------------|----------------|-----------------------|-----------|
| | Name | Function | Signature |
| Calibrated by: | Jeton Kastrati | Laboratory Technician | |
| Approved by: | Katja Pokovic | Technical Manager | |

Issued: February 8, 2016

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Glossary:

| | |
|-------|---------------------------------|
| TSL | tissue simulating liquid |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A | not applicable or not measured |

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

| | | |
|------------------------------|------------------------|-------------|
| DASY Version | DASY5 | V52.8.8 |
| Extrapolation | Advanced Extrapolation | |
| Phantom | Modular Flat Phantom | |
| Distance Dipole Center - TSL | 10 mm | with Spacer |
| Zoom Scan Resolution | dx, dy, dz = 5 mm | |
| Frequency | 2450 MHz \pm 1 MHz | |

Head TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Head TSL parameters | 22.0 °C | 39.2 | 1.80 mho/m |
| Measured Head TSL parameters | (22.0 \pm 0.2) °C | 37.9 \pm 6 % | 1.88 mho/m \pm 6 % |
| Head TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Head TSL

| SAR averaged over 1 cm ³ (1 g) of Head TSL | Condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 13.7 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 53.3 W/kg \pm 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Head TSL | condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 6.34 W/kg |
| SAR for nominal Head TSL parameters | normalized to 1W | 24.9 W/kg \pm 16.5 % (k=2) |

Body TSL parameters

The following parameters and calculations were applied.

| | Temperature | Permittivity | Conductivity |
|---|---------------------|----------------|----------------------|
| Nominal Body TSL parameters | 22.0 °C | 52.7 | 1.95 mho/m |
| Measured Body TSL parameters | (22.0 \pm 0.2) °C | 52.2 \pm 6 % | 2.03 mho/m \pm 6 % |
| Body TSL temperature change during test | < 0.5 °C | ---- | ---- |

SAR result with Body TSL

| SAR averaged over 1 cm ³ (1 g) of Body TSL | Condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 13.3 W/kg |
| SAR for nominal Body TSL parameters | normalized to 1W | 52.1 W/kg \pm 17.0 % (k=2) |

| SAR averaged over 10 cm ³ (10 g) of Body TSL | condition | |
|---|--------------------|--|
| SAR measured | 250 mW input power | 6.26 W/kg |
| SAR for nominal Body TSL parameters | normalized to 1W | 24.7 W/kg \pm 16.5 % (k=2) |

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

| | |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 53.0 Ω + 3.6 j Ω |
| Return Loss | - 26.8 dB |

Antenna Parameters with Body TSL

| | |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 49.8 Ω + 5.8 j Ω |
| Return Loss | - 24.7 dB |

General Antenna Parameters and Design

| | |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.154 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

| | |
|-----------------|-------------------|
| Manufactured by | SPEAG |
| Manufactured on | December 30, 2014 |

DASY5 Validation Report for Head TSL

Date: 08.02.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz ; Type: D2450V2; Serial: D2450V2 - SN: 978

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.88$ S/m; $\epsilon_r = 37.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.67, 7.67, 7.67); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7372)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 115.7 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 28.4 W/kg


SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.34 W/kg

Maximum value of SAR (measured) = 23.1 W/kg

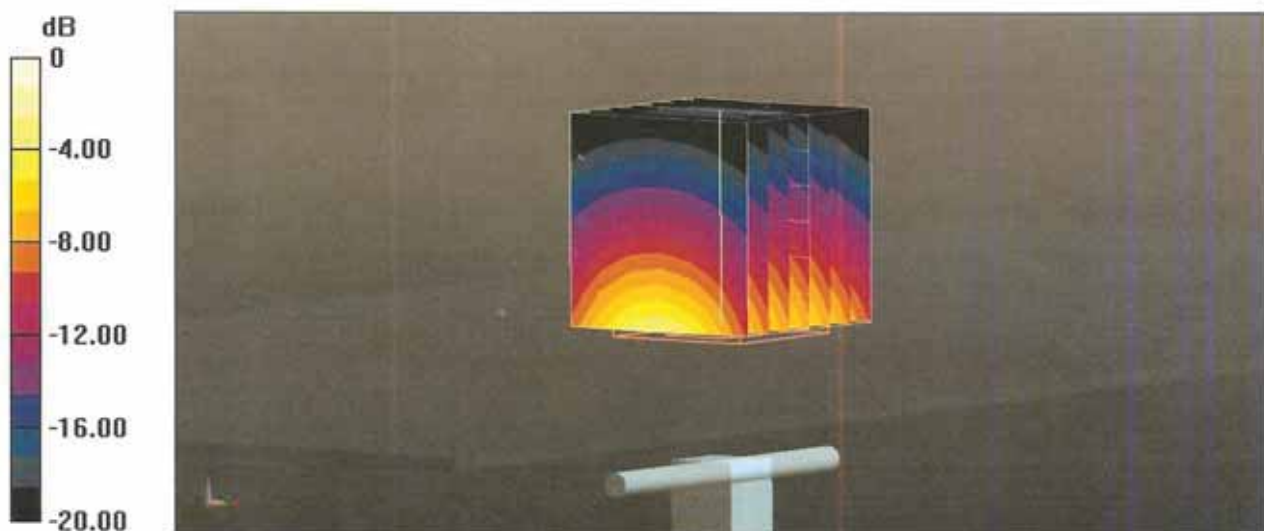

0 dB = 23.1 W/kg = 13.64 dBW/kg

Impedance Measurement Plot for Head TSL

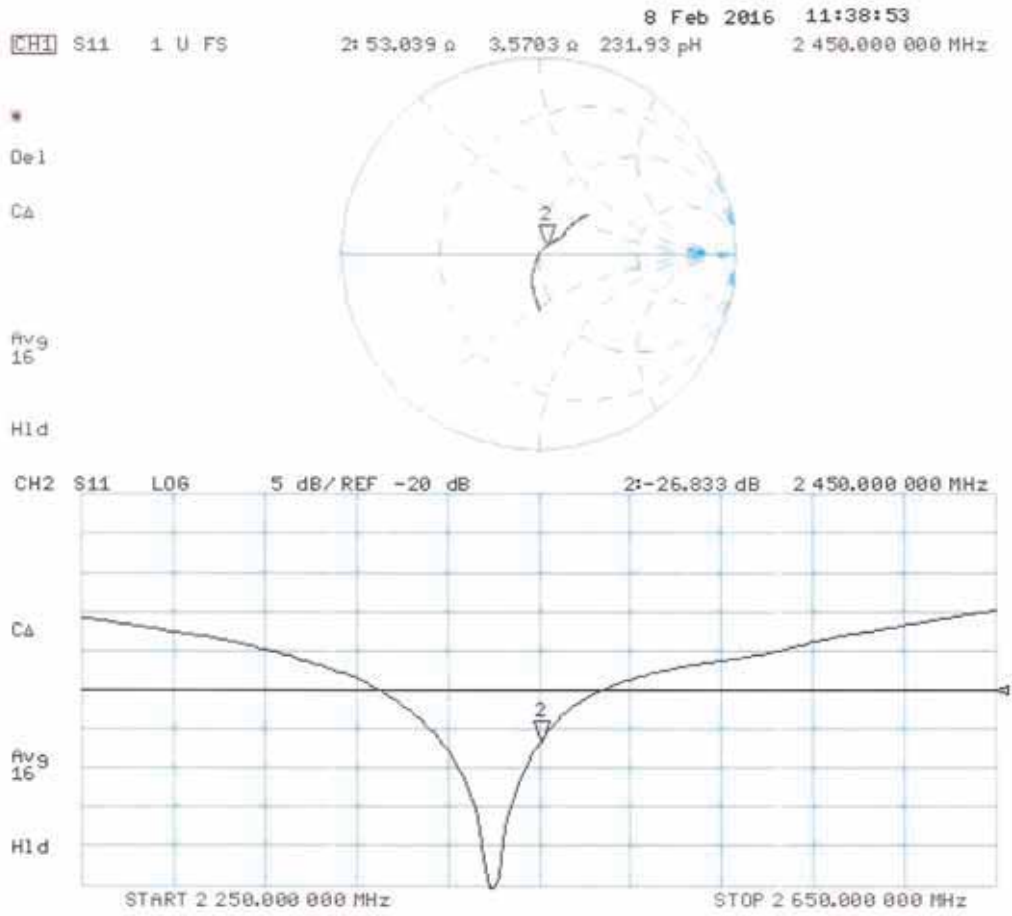

DASY5 Validation Report for Body TSL

Date: 08.02.2016

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz ; Type: D2450V2; Serial: D2450V2 - SN: 978

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 2.03$ S/m; $\epsilon_r = 52.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(7.53, 7.53, 7.53); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7372)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 108.7 V/m; Power Drift = -0.00 dB

Peak SAR (extrapolated) = 26.4 W/kg


SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.26 W/kg

Maximum value of SAR (measured) = 21.7 W/kg

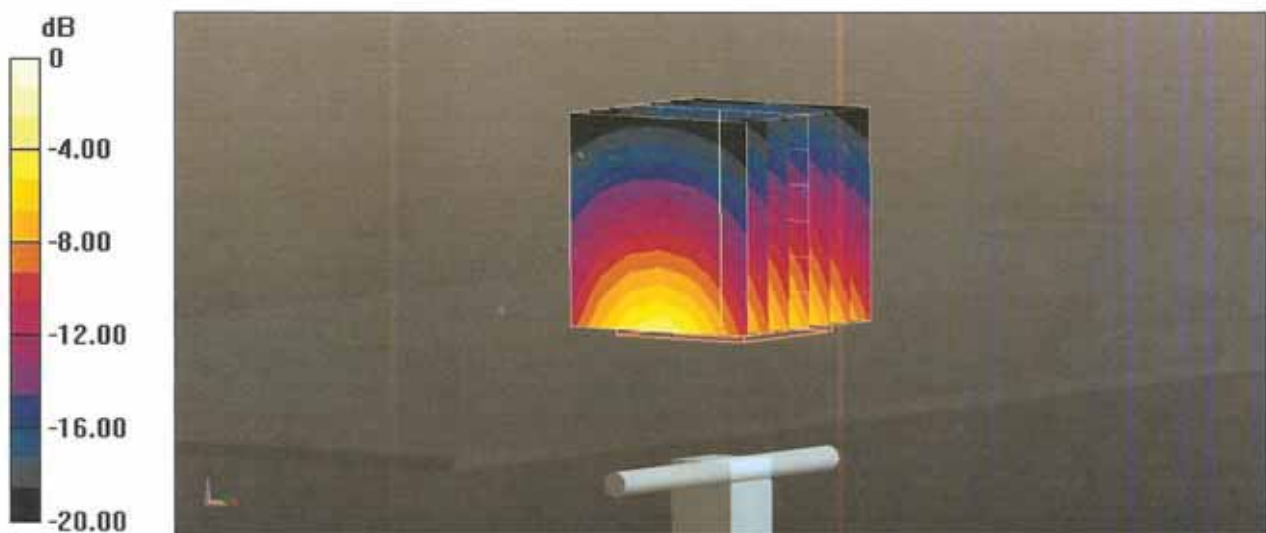

0 dB = 21.7 W/kg = 13.36 dBW/kg

Impedance Measurement Plot for Body TSL

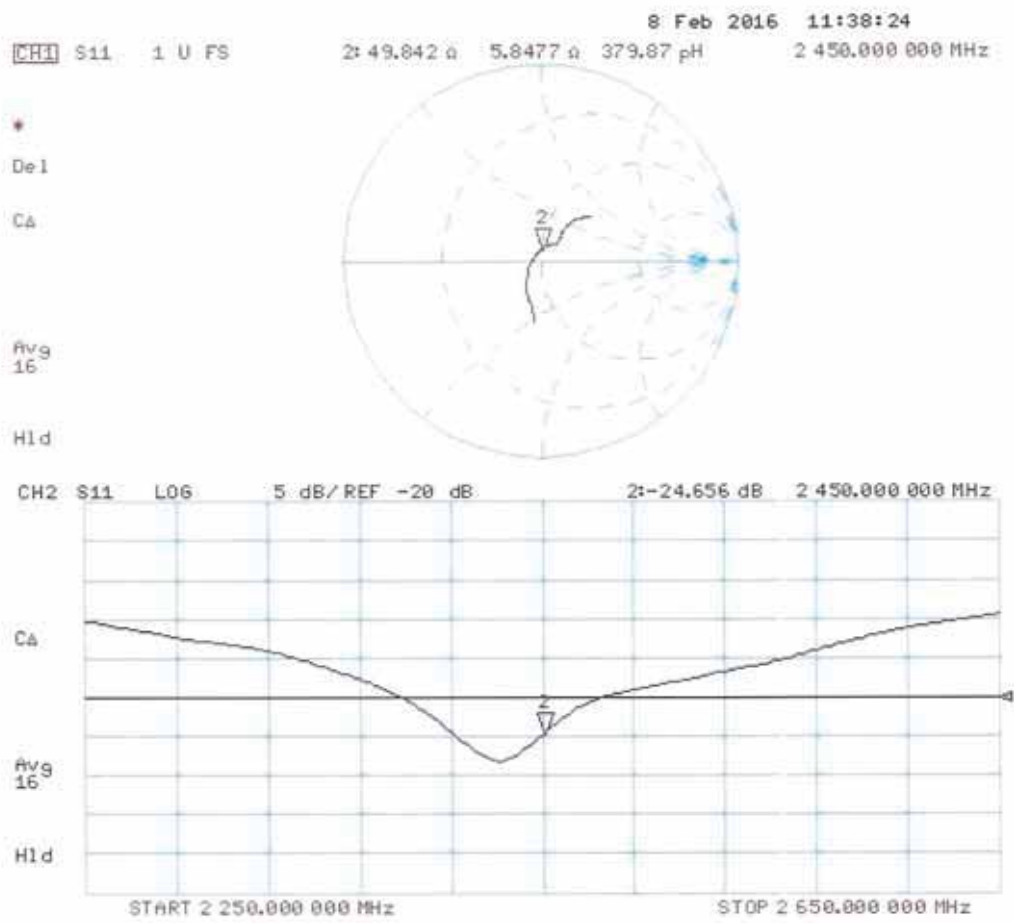



Justification of the extended calibration of Dipole D835V2 SN: 4d126

Per KDB 865664, we have measured the impedance and return loss as below.



- 1) The most recent return-loss result, measured at least annually, deviates by no more than 20% from the previous measurement.
- 2) The most recent measurement of the real or imaginary parts of the impedance, measured at least annually is within 5ohm from the previous measurement.

| Dipole 835 Head TST | Target Value | Measured Value | Difference |
|-------------------------------------|--------------|----------------|---------------------|
| Impedance transformed to feed point | 51.50Ω-0.7jΩ | 47.62Ω-0.67jΩ | R= -3.88Ω, X= 0.03Ω |
| Return Loss | -35.8dB | -32.16dB | 10.17% |
| Dipole 835 Body TST | Target Value | Measured Value | Difference |
| Impedance transformed to feed point | 48Ω-2.5jΩ | 44.09Ω-0.94jΩ | R= -3.91Ω, X= 1.56Ω |
| Return Loss | -29.6dB | -25.2dB | 14.86% |
| Measured Date | 2015-07-23 | 2017-07-19 | ----- |

| | |
|----------------------------|------------------------------|
| Impedance Test-Head | Return Loss Test-Head |
|----------------------------|------------------------------|

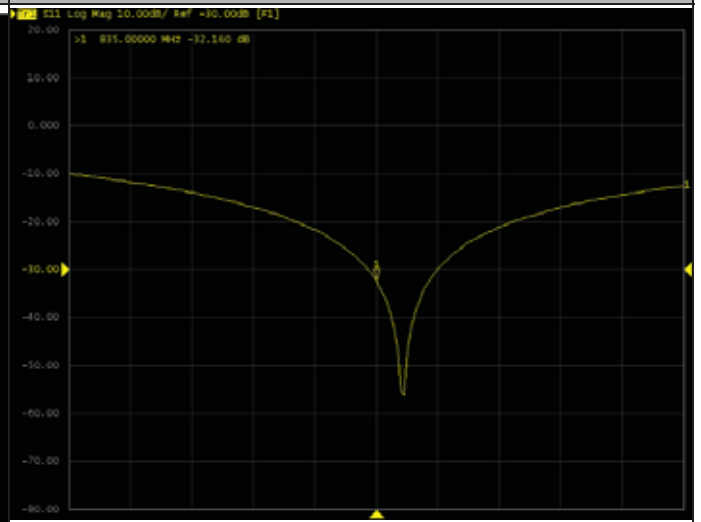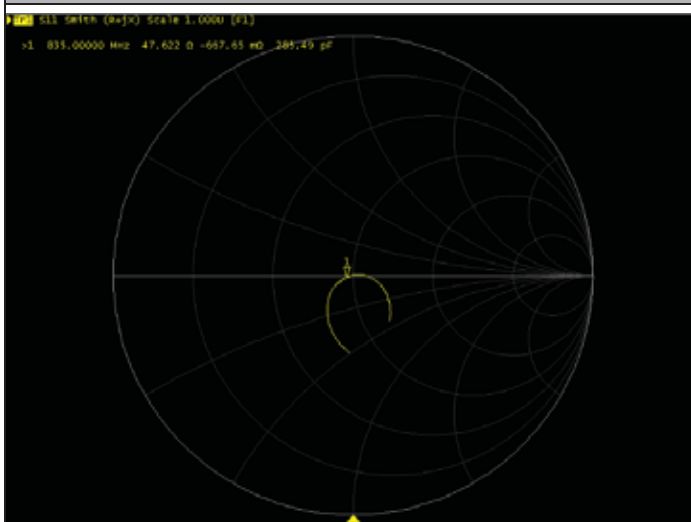

| | |
|----------------------------|-------------------------------|
| Impedance Test-Body | Return Loss Test- Body |
|----------------------------|-------------------------------|

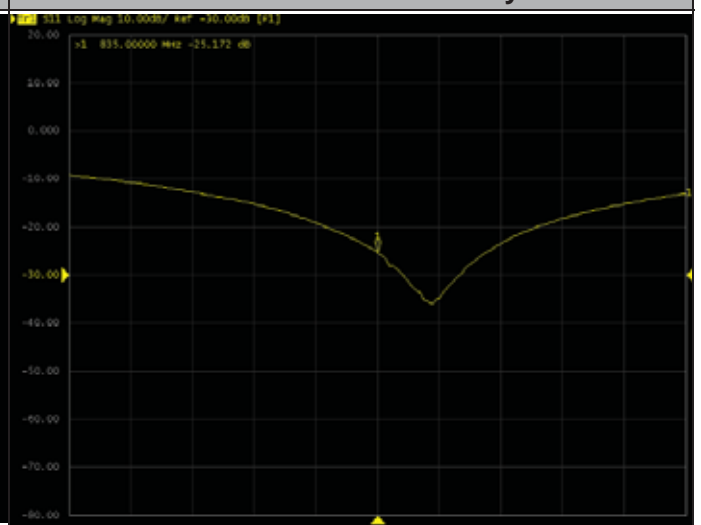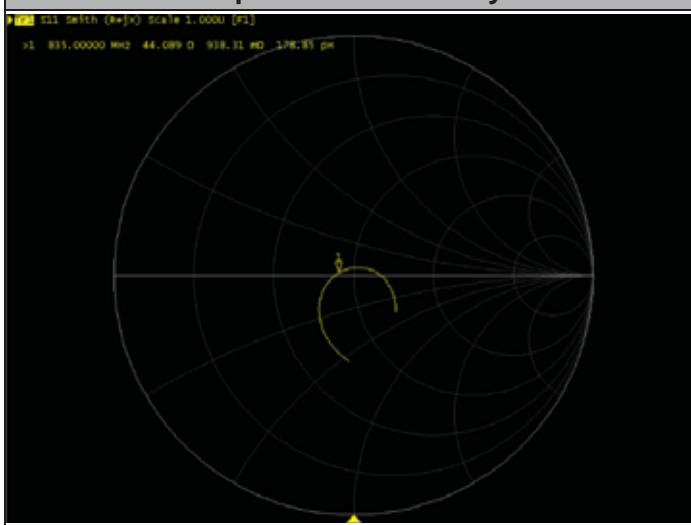


Justification of the extended calibration of Dipole D1900V2 SN: 5d091


Per KDB 865664, we have Measured the Impedance and Return Loss as below, and the return loss is <-20dB, with 20% of prior calibration; the real or imaginary parts of the impedance is with 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

| Dipole1900 Head TST | Target Value | Measured Value | Difference |
|-------------------------------------|--------------|----------------|--------------------|
| Impedance transformed to feed point | 52.0Ω+5.5jΩ | 50.03Ω+3.15jΩ | R=-1.97Ω, X=-2.35Ω |
| Return Loss | -24.8dB | -29.05dB | -17.14% |
| Dipole1900 Body TST | Target Value | Measured Value | Difference |
| Impedance transformed to feed point | 48.2Ω+6.0jΩ | 47.44Ω+5.92jΩ | R=-0.76Ω, X=-0.08Ω |
| Return Loss | -24.0dB | -23.57dB | 1.80% |
| Measured Date | 2015-09-21 | 2017-09-19 | ----- |


Impedance Test-Head

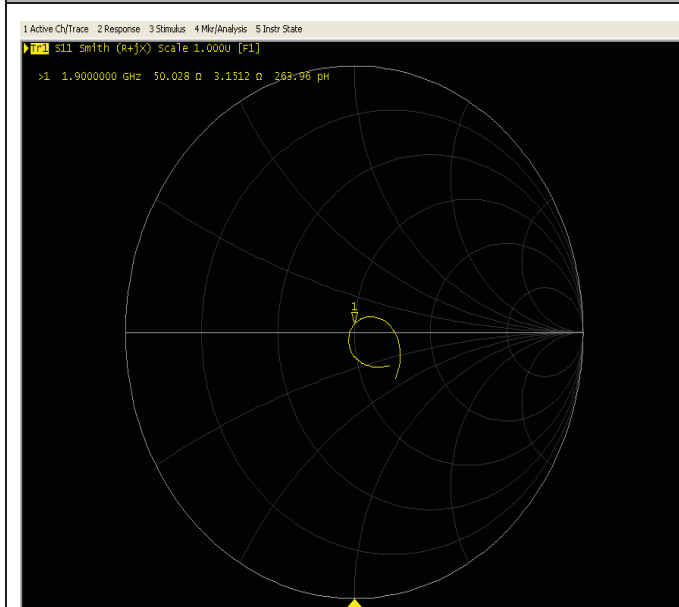


Return Loss Test-Head

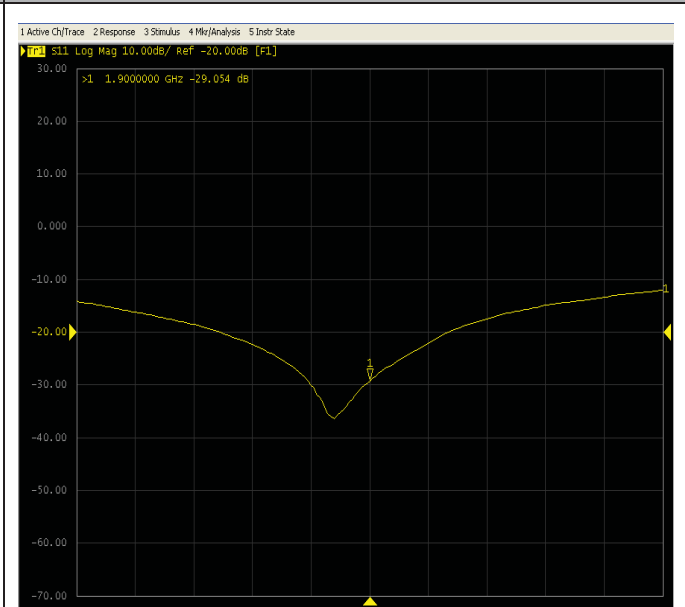

Impedance Test-Body

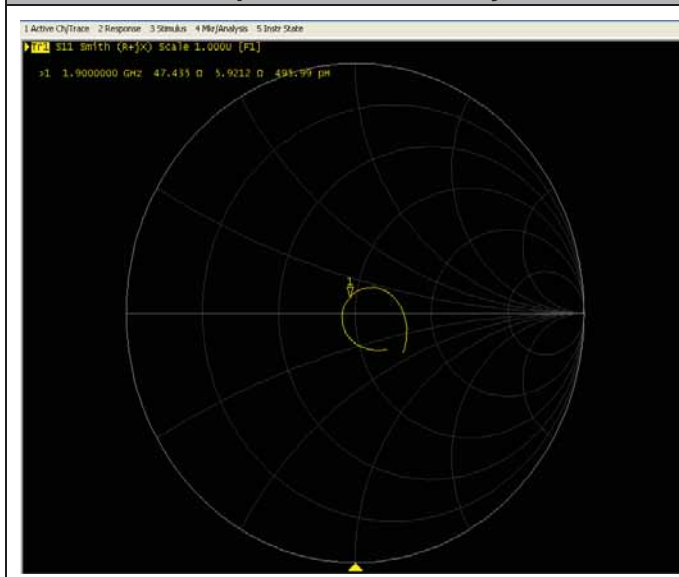

Return Loss Test-Body

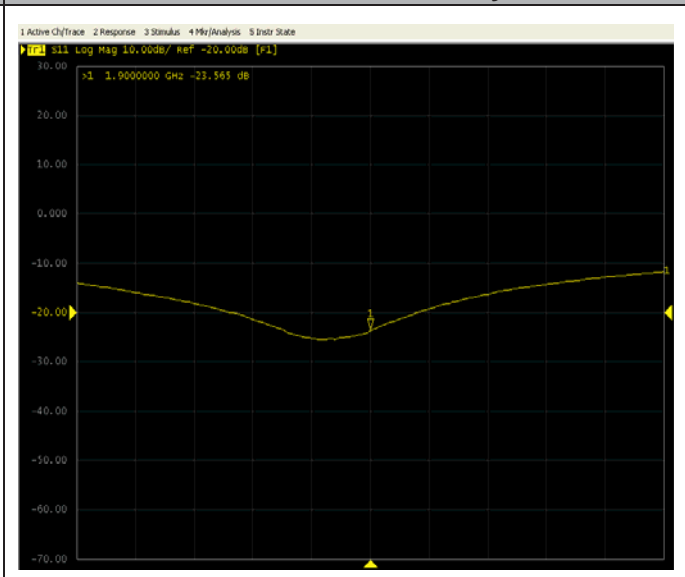


Justification of the extended calibration of Dipole D2450V2 SN:978

Per KDB 865664, we have measured the impedance and return loss as below.


- 1) The most recent return-loss result, measured at least annually, deviates by no more than 20% from the previous measurement.
- 2) The most recent measurement of the real or imaginary parts of the impedance, measured at least annually is within 5ohm from the previous measurement.

| Dipole 2450 Head TST | Target Value | Measured Value | Difference |
|-------------------------------------|--------------|----------------|--------------------|
| Impedance transformed to feed point | 53Ω+3.6jΩ | 49.89Ω+0.34jΩ | R=-3.11Ω, X=-3.26Ω |
| Return Loss | -26.8dB | -29.17dB | 8.84% |
| Dipole 2450 Body TST | Target Value | Measured Value | Difference |
| Impedance transformed to feed point | 49.8Ω+5.8jΩ | 50.68Ω+2.02jΩ | R=0.88Ω, X=-3.78Ω |
| Return Loss | -24.7dB | -23.91dB | -3.20% |
| Measured Date | 2016-02-08 | 2017-01-26 | ----- |


Impedance Test-Head

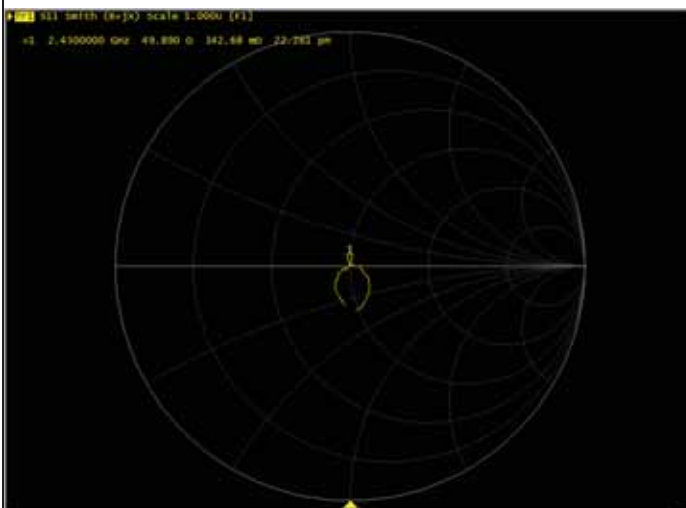

Return Loss Test-Head

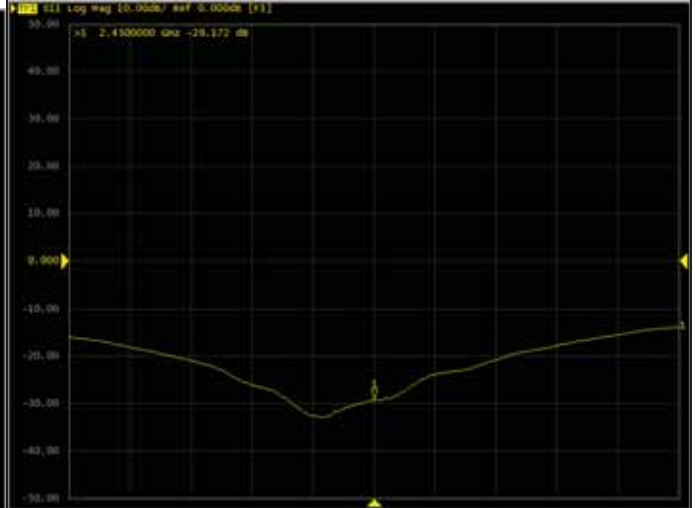

Impedance Test-Body

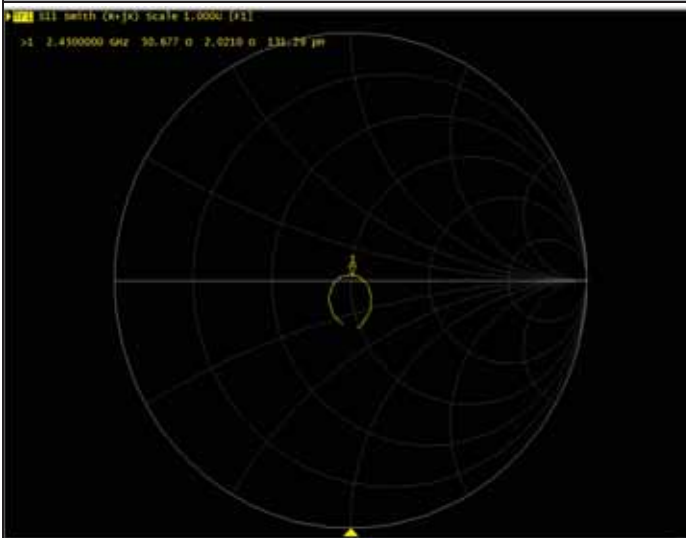

Return Loss Test- Body

