October 24, 2017

10523- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 99pc duty cycle)	X	4.46	66.67	16.14	0.00	150.0	± 9.6 %
		Y	4.37	66.35	15.78		150.0	
		Z	4.52	66.42	15.99		150.0	
10524- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 99pc duty cycle)	X	4.53	66.74	16.27	0.00	150.0	± 9.6 %
		Y	4.43	66.41	15.91		150.0	-
		Z	4.59	66.50	16.13	-	150.0	
10525- AAA	IEEE 802.11ac WiFi (20MHz, MCS0, 99pc duty cycle)	X	4.51	65.77	15.85	0.00	150.0	± 9.6 %
		Y	4.42	65.46	15.50		150.0	
		Z	4.56	65.52	15.71		150.0	
10526- AAA	IEEE 802.11ac WiFi (20MHz, MCS1, 99pc duty cycle)	X	4.68	66.14	16.00	0.00	150.0	± 9.6 %
		Y	4.58	65.81	15.64	-	150.0	
		Z	4.74	65.91	15.86		150.0	
10527- AAA	IEEE 802.11ac WiFi (20MHz, MCS2, 99pc duty cycle)	X	4.60	66.09	15.94	0.00	150.0	± 9.6 %
		Y	4.50	65.75	15.57		150.0	
		Z	4.66	65.87	15.80		150.0	
10528- AAA	IEEE 802.11ac WiFi (20MHz, MCS3, 99pc duty cycle)	×	4.62	66.11	15.97	0.00	150.0	± 9.6 %
		Y.	4.51	65.77	15.60		150.0	
		Z	4.68	65.89	15.83		150.0	
10529- AAA	IEEE 802.11ac WiFi (20MHz, MCS4, 99pc duty cycle)	×	4.62	66.11	15.97	0.00	150.0	± 9.6 %
		Y	4.51	65.77	15.60		150.0	
		Z	4.68	65.89	15.83		150.0	
10531- I AAA S	IEEE 802.11ac WiFi (20MHz, MCS6, 99pc duty cycle)	X	4.61	66.22	15.99	0.00	150.0	± 9.6 %
		Y	4.50	65.85	15.60		150.0	
		Z	4.68	66.01	15.85	-	150.0	
10532- AAA	IEEE 802.11ac WiFi (20MHz, MCS7, 99pc duty cycle)	X	4.47	66.07	15.91	0.00	150.0	±9.6 %
		Y	4.36	65.69	15.52		150.0	
		Z	4.53	65.85	15.77		150.0	
10533- AAA	IEEE 802.11ac WiFi (20MHz, MCS8, 99pc duty cycle)	X	4.63	66.16	15.96	0.00	150.0	±9.6 %
		Y	4.52	65.82	15.59		150.0	
		Z	4.69	65.92	15.81		150.0	
10534- AAA	IEEE 802.11ac WiFi (40MHz, MCS0, 99pc duty cycle)	X	5.16	66.26	16.06	0.00	150.0	±9.6 %
		Y	5.07	65.96	15.74	1	150.0	
		Z	5.22	66.10	15.94		150.0	-
10535- AAA	IEEE 802.11ac WiFi (40MHz, MCS1, 99pc duty cycle)	X	5.23	66.45	16.14	0.00	150.0	± 9.6 %
		Y	5.13	66.15	15.82		150.0	
		Z	5.28	66.25	16.01		150.0	
10536- AAA	IEEE 802.11ac WIFi (40MHz, MCS2, 99pc duty cycle)	×	5.10	66.38	16.09	0.00	150.0	± 9.6 %
		Y	5.00	66.07	15.76		150.0	
1000-		Z	5.15	66.20	15.96		150.0	
10537- AAA	IEEE 802.11ac WiFi (40MHz, MCS3, 99pc duty cycle)	x	5,16	66.35	16.08	0.00	150.0	± 9.6 %
_		Y	5.06	66.05	15.75		150.0	
10500		Z	5.21	66.19	15.96		150.0	
10538- AAA	IEEE 802.11ac WiFi (40MHz, MCS4, 99pc duty cycle)	x	5.25	66.38	16.14	0.00	150.0	±9.6 %
		Y	5.15	66.08	15.81		150.0	
10515	100 00.00 0.00	Z	5.32	66.26	16.04		150.0	
10540- AAA	IEEE 802.11ac WiFi (40MHz, MCS6, 99pc duty cycle)	x	5.18	66.40	16.16	0.00	150.0	±9.6 %
		Y	5.09	66.10	15.84		150.0	
			0.00	00.10			120111	

Certificate No: EX3-7381\_Oct17

October 24, 2017

10541- AAA	IEEE 802.11ac WiFi (40MHz, MCS7, 99pc duty cycle)	X	5.15	66.26	16.08	0.00	150.0	± 9.6 %
	sopo duly cycle)	Y	5.06	65.96	15.76		150.0	
		Z	5.20	66.10	15.96	1	150.0	
10542- AAA	IEEE 802.11ac WiFi (40MHz, MCS8, 99pc duty cycle)	X	5.31	66.34	16.14	0.00	150.0	±9.6 %
		Y	5.21	66.05	15.82		150.0	
		Z	5.37	66.19	16.03		150.0	
10543- AAA	IEEE 802.11ac WiFi (40MHz, MCS9, 99pc duty cycle)	X	5.39	66.39	16.19	0.00	150.0	± 9.6 %
		Y	5.29	66.10	15.87		150.0	
		Z	5.45	66.23	16.07		150.0	
10544- AAA	IEEE 802.11ac WiFi (80MHz, MCS0, 99pc duty cycle)	X	5.47	66.37	16.05	0.00	150.0	± 9.6 %
		Y	5.39	66.11	15.76		150.0	
		Z	5.51	66.22	15.94		150.0	
10545- AAA	IEEE 802.11ac WiFi (80MHz, MCS1, 99pc duty cycle)	x	5.68	66.83	16.24	0.00	150.0	±9.6 %
1917 - S. P		Y	5.58	66.54	15.93		150.0	
		Z	5.73	66.68	16.12		150.0	
10546- AAA	IEEE 802.11ac WiFi (80MHz, MCS2, 99pc duty cycle)	×	5.54	66.59	16.13	0.00	150.0	±9.6 %
		Y	5.44	66.30	15.82		150.0	
		Z	5.60	66.49	16.04		150.0	
10547- AAA	IEEE 802.11ac WiFi (80MHz, MCS3, 99pc duty cycle)	X	5.61	66.63	16.14	0.00	150.0	±9.6 %
		Y	5.52	66.35	15.84		150.0	
		Z	5.69	66.58	16.08		150.0	
10548- AAA	IEEE 802.11ac WiFi (80MHz, MCS4, 99pc duty cycle)	x	5.92	67.76	16.69	0.00	150.0	±9.6 %
		Y	5.76	67.26	16.27		150.0	
		Z	6.05	67.82	16.67		150.0	
10550- AAA	IEEE 802.11ac WiFi (80MHz, MCS6, 99pc duty cycle)	X	5.57	66.62	16.15	0.00	150.0	±9.6 %
		Y	5.48	66.34	15.85		150.0	
2.2222 A.13		Z	5.62	66.46	16.03		150.0	
10551- AAA	IEEE 802.11ac WiFi (80MHz, MCS7, 99pc duty cycle)	X	5.57	66.64	16.12	0.00	150.0	±9.6 %
		Y	5.48	66.36	15.83		150.0	
		Z	5.62	66.51	16.02		150.0	
10552- AAA	IEEE 802.11ac WiFi (80MHz, MCS8, 99pc duty cycle)	X	5.48	66.42	16.02	0.00	150.0	± 9.6 %
		Y	5.40	66.17	15.73		150.0	
		Z	5.53	66.28	15.92		150.0	
10553- AAA	IEEE 802.11ac WiFi (80MHz, MCS9, 99pc duty cycle)	X	5.57	66.47	16.08	0.00	150.0	± 9.6 %
		Y	5.48	66.20	15.78		150.0	
		Z	5.62	66.34	15.98		150.0	
10554- AAB	IEEE 802.11ac WiFi (160MHz, MCS0, 99pc duty cycle)	×	5.88	66.74	16.15	0.00	150.0	±9.6 %
		Y	5.80	66.50	15.87		150.0	
		Z	5.92	66.62	16.06		150.0	
10555- AAB	IEEE 802.11ac WiFi (160MHz, MCS1, 99pc duty cycle)	X	6.02	67.07	16.29	0.00	150.0	±9.6 %
		Y	5.93	66.80	16.00		150.0	
		Z	6.07	66.95	16.20		150.0	
10556- AAB	IEEE 802.11ac WiFi (160MHz, MCS2, 99pc duty cycle)	×	6.04	67.11	16.31	0.00	150.0	± 9.6 %
		Y	5.95	66.84	16.02		150.0	1
		Z	6.08	66.98	16.21	(i	150.0	
10557- AAB	IEEE 802.11ac WiFi (160MHz, MCS3, 99pc duty cycle)	×	6.00	67.01	16.28	0.00	150.0	± 9.6 %
	1	Y	5.91	66.73	15.98		150.0	
		Z	6.06	66.91	16.19		150.0	

Certificate No: EX3-7381\_Oct17

Page 32 of 38

October 24, 2017

10558- AAB	IEEE 802.11ac WiFi (160MHz, MCS4, 99pc duty cycle)	×	6.05	67.18	16.38	0.00	150.0	± 9.6 %
		Y	5.95	66.89	16.07		150.0	
		Z	6.11	67.10	16.30		150.0	
10560- AAB	IEEE 802.11ac WiFi (160MHz, MCS6, 99pc duty cycle)	×	6.04	67.01	16.33	0.00	150.0	± 9.6 %
		Y	5.95	66.75	16.04		150.0	
		Z	6.10	66.92	16.25		150.0	
10561- AAB	IEEE 802.11ac WiFi (160MHz, MCS7, 99pc duty cycle)	X	5.97	67.00	16.36	0.00	150.0	± 9.6 %
		Y	5.88	66.72	16.06	-	150.0	
		Z	6.02	66.89	16.27		150.0	
10562- AAB	IEEE 802.11ac WiFi (160MHz, MCS8, 99pc duty cycle)	X	6.10	67.42	16.57	0.00	150.0	± 9.6 %
		Y	5.99	67.06	16.24		150.0	
		Z	6.18	67.38	16.52		150.0	
10563- AAB	IEEE 802.11ac WiFi (160MHz, MCS9, 99pc duty cycle)	X	6.37	67.83	16.74	0.00	150.0	± 9.6 %
		Y	6.15	67.19	16.27		150.0	
		Z	6.58	68.12	16.84		150.0	
10564- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 9 Mbps, 99pc duty cycle)	X	4.88	66.63	16.36	0.46	150.0	± 9.6 %
		Y	4.80	66.36	16.03		150.0	
		Z	4.94	66.44	16.26		150.0	
10565- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 12 Mbps, 99pc duty cycle)	×	5.11	67.07	16.68	0.46	150.0	± 9.6 %
		Y	5.02	66.80	16.36		150.0	
		Z	5.19	66.91	16.59		150.0	
10566- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 18 Mbps, 99pc duty cycle)	X	4.94	66.91	16.49	0.46	150.0	± 9.6 %
	<ul> <li>A 1 community of a series of a latence or a test conduct and a series of a se</li></ul>	Y	4.85	66.62	16.16		150.0	
		Z	5.02	66.76	16.40		150.0	
10567- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 24 Mbps, 99pc duty cycle)	X	4.96	67.24	16.80	0.46	150.0	± 9.6 %
		Y	4.87	66.98	16.49		150.0	
		Z	5.04	67.10	16.72		150.0	
10568- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 36 Mbps, 99pc duty cycle)	X	4.86	66.71	16.28	0.46	150.0	± 9.6 %
	41 AA 48	Y	4.76	66.40	15.93		150.0	
		Z	4.93	66.51	16.16		150.0	
10569- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 48 Mbps, 99pc duty cycle)	X	4.90	67.28	16.82	0.46	150.0	± 9.6 %
		Y	4.83	67.06	16.55		150.0	
		Z	4.97	67.11	16.74		150.0	
10570- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 54 Mbps, 99pc duty cycle)	x	4.95	67.19	16.80	0.46	150.0	± 9.6 %
		Y	4.87	66.94	16.50		150.0	
		Z	5.03	67.01	16.70		150.0	
10571- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 90pc duty cycle)	X	1.08	63.20	14.80	0.46	130.0	±9.6 %
		Y	1.04	62.15	13.83		130.0	
10.000		Z	1.09	62.67	14.50		130.0	
10572- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 2 Mbps, 90pc duty cycle)	X	1.09	63.63	15.08	0.46	130.0	±9.6 %
		Y	1.04	62.50	14.07		130.0	
		Z	1.09	63.07	14.76		130.0	
10573- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 5.5 Mbps, 90pc duty cycle)	X	1.06	75.27	18.99	0.46	130.0	± 9.6 %
		Y	0.66	67.16	14.93		130.0	
		Z	0.83	70.70	17.11		130.0	
10000	IEEE 802.11b WiFi 2.4 GHz (DSSS, 11	X	1.09	67.76	17.22	0.46	130.0	±9.6 %
10574- AAA	Mbps, 90pc duty cycle)						1.120.00	
	Mbps, 90pc duty cycle)	Y	0.98	65.29	15.54		130.0	

Certificate No: EX3-7381\_Oct17

October 24, 2017

10575- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 6 Mbps, 90pc duty cycle)	X	4.63	66.30	16.32	0.46	130.0	± 9.6 %
		Y	4.56	66.08	16.03		130.0	
		Z	4.71	66.17	16.27		130.0	
10576- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 9 Mbps, 90pc duty cycle)	X	4.65	66.45	16.37	0.46	130.0	± 9.6 %
		Y	4.59	66.24	16.09		130.0	
		Z	4.73	66.31	16.33		130.0	
10577- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 12 Mbps, 90pc duty cycle)	×	4.86	66.76	16.55	0.46	130.0	±9.6 %
		Y	4.78	66.53	16.27		130.0	
_		Z	4.96	66.65	16.52		130.0	
10578- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 18 Mbps, 90pc duty cycle)	X	4.75	66.87	16.62	0.46	130.0	±9.6 %
_		Y	4.68	66.65	16.35		130.0	
12-22-22		Z	4.84	66,77	16.60		130.0	
10579- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 24 Mbps, 90pc duty cycle)	X	4.53	66.23	15.98	0.46	130.0	± 9.6 %
		Y	4.44	65.94	15.66		130.0	
		Z	4.62	66.12	15.95		130.0	
10580- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 36 Mbps, 90pc duty cycle)	X	4.58	66.29	16.02	0.46	130.0	±9.6 %
		Y	4.49	66.00	15.69		130.0	
alla successore		Z	4.66	66.14	15.97		130.0	
10581- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 48 Mbps, 90pc duty cycle)	X	4.64	66.87	16.54	0.46	130.0	±9.6 %
		Y	4.56	66.64	16.26		130.0	
		Z	4.73	66.79	16.52		130.0	
10582- AAA	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 54 Mbps, 90pc duty cycle)	X	4.48	66.04	15.81	0.46	130.0	± 9.6 %
		Y	4.39	65.72	15.46		130.0	
		Z	4.57	65.91	15.76		130.0	
10583- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 6 Mbps, 90pc duty cycle)	X	4.63	66.30	16.32	0.46	130.0	±9.6 %
		Y	4.56	66.08	16.03		130.0	
		Z	4.71	66.17	16.27		130.0	
10584- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 9 Mbps, 90pc duty cycle)	X	4.65	66.45	16.37	0.46	130.0	± 9.6 %
		Y	4.59	66.24	16.09		130.0	
		Z	4.73	66.31	16.33		130.0	
10585- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 12 Mbps, 90pc duty cycle)	X	4.86	66.76	16.55	0.46	130.0	± 9.6 %
		Y	4.78	66.53	16.27		130.0	
		Z	4.96	66.65	16.52		130.0	
10586- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 18 Mbps, 90pc duty cycle)	X	4.75	66.87	16.62	0.46	130.0	±9.6 %
		Y	4.68	66.65	16.35		130.0	
		Z	4.84	66.77	16.60		130.0	
10587- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 24 Mbps, 90pc duty cycle)	X	4.53	66.23	15.98	0.46	130.0	± 9.6 %
		Y	4.44	65.94	15.66		130.0	
1.500.00		Z	4.62	66.12	15.95		130.0	
10588- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 36 Mbps, 90pc duty cycle)	X	4.58	66.29	16.02	0.46	130.0	±9.6 %
		Y	4.49	66.00	15.69		130.0	
		Z	4.66	66.14	15.97		130.0	
10589- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 48 Mbps, 90pc duty cycle)	X	4.64	66.87	16.54	0.46	130.0	± 9.6 %
		Y	4.56	66.64	16.26		130.0	
		Z	4.73	66.79	16.52		130.0	
10590- AAA	IEEE 802.11a/h WiFi 5 GHz (OFDM, 54 Mbps, 90pc duty cycle)	X	4.48	66.04	15.81	0.46	130.0	± 9.6 %
		Y	4.39	65.72	15.46		130.0	
					and the second se			

Certificate No: EX3-7381\_Oct17

Page 34 of 38

October 24, 2017

10591- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS0, 90pc duty cycle)	×	4.79	66.37	16.42	0.46	130.0	± 9.6 %
		Y	4.72	66.18	16.16		130.0	
		Z	4.87	66.25	16.39		130.0	
10592- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS1, 90pc duty cycle)	X	4.94	66.70	16.55	0.46	130.0	± 9.6 %
		Y	4.87	66.50	16.29		130.0	
		Z	5.03	66.59	16.52		130.0	
10593- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS2, 90pc duty cycle)	x	4.86	66.62	16.44	0.46	130.0	± 9.6 %
		Y	4.78	66.39	16.16		130.0	
		Z	4.95	66.52	16.41		130.0	
10594- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS3, 90pc duty cycle)	×	4.91	66.77	16.58	0.46	130.0	± 9.6 %
		Y	4.84	66.56	16.31		130.0	
		Z	5.00	66.66	16.55	-	130.0	
10595- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS4, 90pc duty cycle)	×	4.88	66.72	16.48	0.46	130.0	± 9.6 %
		Y	4.80	66.50	16.20		130.0	
10500		Z	4.97	66.62	16.45		130.0	
10596- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS5, 90pc duty cycle)	X	4.82	66.72	16.48	0.46	130.0	± 9.6 %
		Y	4.74	66.49	16.20		130.0	
		Z	4.91	66.61	16.44		130.0	
10597- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS6, 90pc duty cycle)	×	4.77	66.63	16.37	0.46	130.0	± 9.6 %
		Y	4.69	66.38	16.07		130.0	
		Z	4.86	66.53	16.34		130.0	
10598- AAA	IEEE 802.11n (HT Mixed, 20MHz, MCS7, 90pc duty cycle)	X	4.74	66.81	16.59	0.46	130.0	± 9.6 %
		Y	4.66	66.58	16.32		130.0	
		Z	4.83	66.74	16.58		130.0	
10599- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS0, 90pc duty cycle)	X	5.47	66.99	16.68	0.46	130.0	± 9.6 %
		Y	5.41	66.81	16.44		130.0	
		Z	5.56	66.92	16.65		130.0	
10600- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS1, 90pc duty cycle)	×	5.64	67.53	16.93	0.46	130.0	±9.6 %
		Y	5.55	67.25	16.64		130.0	
		Z	5.77	67.57	16.95		130.0	
10601- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS2, 90pc duty cycle)	X	5.51	67.21	16.78	0.46	130.0	± 9.6 %
		Y	5.43	66.96	16.51		130.0	
		Z	5.61	67.18	16.77		130.0	
10602- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS3, 90pc duty cycle)	×	5.61	67.26	16.73	0.46	130.0	±9.6 %
		Y	5.53	67.04	16.47		130.0	
10000	IPPER AND IN THE OWNER	Z	5.70	67.17	16.69		130.0	
10603- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS4, 90pc duty cycle)	×	5.68	67.51	16.98	0.46	130.0	±9.6 %
		Y	5.60	67.30	16.73		130.0	
1000+	LIPPER DOG 11 HORE	Z	5.77	67.44	16.94		130.0	
10604- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS5, 90pc duty cycle)	×	5.48	66.95	16.69	0.46	130.0	± 9.6 %
		Y	5.43	66.84	16.48		130.0	
10005		Z	5.56	66.89	16.66		130.0	
10605- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS6, 90pc duty cycle)	x	5.61	67.38	16.91	0.46	130.0	±9.6 %
		Y	5.53	67.14	16.63		130.0	
10000		Z	5.69	67.26	16.85		130.0	
10606- AAA	IEEE 802.11n (HT Mixed, 40MHz, MCS7, 90pc duty cycle)	x	5.35	66.69	16.42	0.46	130.0	±9.6 %
		Y	5.26	66.41	16.13		130.0	
		Z	5.44	and the second se				

Certificate No: EX3-7381\_Oct17

Page 35 of 38

October 24, 2017

10607- AAA	IEEE 802.11ac WiFi (20MHz, MCS0, 90pc duty cycle)	X	4.62	65.66	16.02	0.46	130.0	±9.6 %
		Y	4.55	65.44	15.75		130.0	
		Z	4.69	65.52	15.97		130.0	
10608- AAA	IEEE 802.11ac WiFi (20MHz, MCS1, 90pc duty cycle)	X	4.81	66.06	16.19	0.46	130.0	± 9.6 %
	2	Y	4.72	65.83	15.91		130.0	
		Z	4.89	65.94	16.14		130.0	
10609- AAA	IEEE 802.11ac WiFi (20MHz, MCS2, 90pc duty cycle)	×	4.70	65.91	16.03	0.46	130.0	± 9.6 %
		Y	4.61	65.66	15.74		130.0	
		Z	4.78	65.79	15.99		130.0	
10610- AAA	IEEE 802.11ac WiFi (20MHz, MCS3, 90pc duty cycle)	×	4.74	66.05	16.18	0.46	130.0	± 9.6 %
		Y	4.66	65.81	15.90		130.0	
		Z	4.83	65.94	16.14		130.0	
10611- AAA	IEEE 802.11ac WiFi (20MHz, MCS4, 90pc duty cycle)	x	4.66	65.87	16.03	0.46	130.0	± 9.6 %
		Y	4.58	65.62	15.74		130.0	
		Z	4.75	65.77	16.00		130.0	
10612- AAA	IEEE 802.11ac WiFi (20MHz, MCS5, 90pc duty cycle)	×	4.67	66.03	16.08	0.46	130.0	±9.6 %
		Y	4.58	65.76	15.78		130.0	
1153 Sec. 65-		Z	4.76	65.91	16.04		130.0	
10613- AAA	IEEE 802.11ac WiFi (20MHz, MCS6, 90pc duty cycle)	x	4.68	65.94	15.98	0.46	130.0	± 9.6 %
		Y	4.58	65.64	15.66		130.0	
		Z	4.77	65.83	15.94		130.0	
10614- AAA	IEEE 802.11ac WiFi (20MHz, MCS7, 90pc duty cycle)	x	4.61	66.06	16.17	0.46	130.0	±9.6 %
		Y	4.53	65.80	15.88		130.0	
		Z	4.70	65.97	16.14		130.0	
10615- AAA	IEEE 802.11ac WiFi (20MHz, MCS8, 90pc duty cycle)	x	4.67	65.74	15.84	0.46	130.0	± 9.6 %
		Y	4.58	65.47	15.53		130.0	
		Z	4.75	65.61	15.79		130.0	
10616- AAA	IEEE 802.11ac WiFi (40MHz, MCS0, 90pc duty cycle)	X	5.28	66.20	16.26	0.46	130.0	± 9.6 %
		Y	5.21	65.99	16.01		130.0	
		Z	5.37	66.14	16.23		130.0	
10617- AAA	IEEE 802.11ac WiFi (40MHz, MCS1, 90pc duty cycle)	×	5.36	66.41	16.34	0.46	130.0	±9.6 %
		Y	5.28	66.19	16.08		130.0	
		Z	5.43	66.27	16.27		130.0	
10618- AAA	IEEE 802.11ac WiFi (40MHz, MCS2, 90pc duty cycle)	×	5.23	66.37	16.33	0.46	130.0	±9.6 %
		Y	5.16	66.15	16.08		130.0	
		Z	5.32	66.30	16.30		130.0	
10619- AAA	IEEE 802.11ac WiFi (40MHz, MCS3, 90pc duty cycle)	×	5.27	66.24	16.20	0.46	130.0	±9.6 %
		Y	5.18	65.98	15.93		130.0	
		Z	5.35	66.15	16.16		130.0	
10620- AAA	IEEE 802.11ac WiFi (40MHz, MCS4, 90pc duty cycle)	X	5.35	66.27	16.27	0.46	130.0	± 9.6 %
		Y	5.27	66.03	16.00		130.0	
		Z	5.45	66.25	16.26		130.0	
10621- AAA	IEEE 802.11ac WiFi (40MHz, MCS5, 90pc duty cycle)	X	5.34	66.34	16.41	0.46	130.0	±9.6 %
		Y	5.27	66.15	16.18		130.0	
		Z	5.42	66.28	16.39		130.0	
10622- AAA	IEEE 802.11ac WiFi (40MHz, MCS6, 90pc duty cycle)	X	5.36	66.54	16.51	0.46	130.0	± 9.6 %
		Y	5.28	66.31	16.25		130.0	

Certificate No: EX3-7381\_Oct17

Page 36 of 38

October 24, 2017

10623- AAA	IEEE 802.11ac WiFi (40MHz, MCS7, 90pc duty cycle)	×	5.24	66.08	16.16	0.46	130.0	± 9.6 %
_		Y	5.17	65.85	15.90		130.0	
		Z	5.32	65.99	16.12		130.0	
10624- AAA	IEEE 802.11ac WiFi (40MHz, MCS8, 90pc duty cycle)	x	5.44	66.29	16.33	0.46	130.0	± 9.6 %
		Y	5.36	66.07	16.07		130.0	
		Z	5.52	66.22	16.30		130.0	
10625- AAA	IEEE 802.11ac WiFi (40MHz, MCS9, 90pc duty cycle)	X	5.84	67.39	16.94	0.46	130.0	±9.6 %
		Y	5.70	66.97	16.58		130.0	-
		Z	5.98	67.45	16.96		130.0	1
10626- AAA	IEEE 802.11ac WiFi (80MHz, MCS0, 90pc duty cycle)	x	5.58	66.27	16.22	0.46	130.0	±9.6 %
		Y	5.52	66.09	16.00		130.0	
		Z	5.64	66.20	16.19		130.0	
10627- AAA	IEEE 802.11ac WiFi (80MHz, MCS1, 90pc duty cycle)	x	5.84	66.91	16.51	0.46	130.0	± 9.6 %
		Y	5.76	66.68	16.26		130.0	
		Z	5.92	66.85	16.47		130.0	
10628- AAA 90pc duty cycle)	IEEE 802.11ac WiFi (80MHz, MCS2, 90pc duty cycle)	×	5.63	66.41	16.20	0.46	130.0	± 9.6 %
		Y	5.55	66.17	15.93		130.0	
		Z	5.71	66.37	16.17		130.0	
10629- AAA	IEEE 802.11ac WiFi (80MHz, MCS3, 90pc duty cycle)	x	5.72	66.52	16.25	0.46	130.0	±9.6 %
	Environment of the second of t	Y	5.62	66.23	15.96		130.0	
		Z	5.79	66.43	16.20		130.0	
10630- AAA	IEEE 802.11ac WiFi (80MHz, MCS4, 90pc duty cycle)	×	6.25	68.29	17.14	0.46	130.0	±9.6 %
		Y	6.05	67.71	16.70		130.0	
		Z	6.42	68.49	17.22		130.0	
10631- AAA	IEEE 802.11ac WiFi (80MHz, MCS5, 90pc duty cycle)	x	6.05	67.77	17.05	0.46	130.0	±9.6 %
		Y	5.93	67.44	16.76		130.0	
	All the second sec	Z	6.20	67.92	17.12		130.0	
10632- AAA	IEEE 802.11ac WiFi (80MHz, MCS6, 90pc duty cycle)	x	5.80	66.91	16.63	0.46	130.0	± 9.6 %
		Y	5.73	66.73	16.42		130.0	
		Z	5.87	66.85	16.61		130.0	
10633- AAA	IEEE 802.11ac WiFi (80MHz, MCS7, 90pc duty cycle)	X	5.68	66.52	16.28	0.46	130.0	± 9.6 %
		Y	5.60	66.31	16.04		130.0	
		Z	5.77	66.53	16.28		130.0	
10634- AAA	IEEE 802.11ac WiFi (80MHz, MCS8, 90pc duty cycle)	X	5.66	66.54	16.34	0.46	130.0	±9.6 %
		Y	5.59	66.34	16.11		130.0	
		Z	5.75	66.52	16.33		130.0	
10635- AAA	IEEE 802.11ac WiFi (80MHz, MCS9, 90pc duty cycle)	x	5.56	65.97	15.81	0.46	130.0	±9.6 %
		Y	5.48	65.72	15.54		130.0	-
		Z	5.65	65.94	15.79		130.0	
10636- AAB	IEEE 802.11ac WiFi (160MHz, MCS0, 90pc duty cycle)	x	6.01	66.68	16.34	0.46	130.0	± 9.6 %
		Y	5.94	66.49	16.11		130.0	
10007		Z	6.07	66.64	16.32		130.0	
10637- AAB	IEEE 802.11ac WiFi (160MHz, MCS1, 90pc duty cycle)	×	6.17	67.09	16.53	0.46	130.0	±9.6 %
		Y	6.10	66.88	16.29		130.0	
		Z	6.24	67.05	16.51		130.0	
	IEEE 802.11ac WiFi (160MHz, MCS2,	X	6.17	67.06	16.49	0.46	130.0	±9.6 %
10638- AAB	90pc duty cycle)							
	90pc duty cycle)	Y	6.09	66.84	16.25		130.0	

Certificate No: EX3-7381\_Oct17

October 24, 2017

10639- AAB	IEEE 802.11ac WiFi (160MHz, MCS3, 90pc duty cycle)	X	6.14	66.99	16.50	0.46	130.0	± 9.6 %
		Y	6.07	66.78	16.26		130.0	
		Z	6.23	66.98	16.50		130.0	
10640- AAB	IEEE 802.11ac WiFi (160MHz, MCS4, 90pc duty cycle)	X	6.16	67.04	16.47	0.46	130.0	± 9.6 %
		Y	6.07	66.79	16.21		130.0	
		Z	6.25	67.07	16.48		130.0	
10641- AAB	IEEE 802.11ac WiFi (160MHz, MCS5, 90pc duty cycle)	X	6.20	66.93	16.44	0.46	130.0	±9.6 %
	and the second	Y	6.13	66.74	16.21		130.0	
		Z	6.26	66.85	16.39		130.0	
10642- AAB	IEEE 802.11ac WiFi (160MHz, MCS6, 90pc duty cycle)	X	6.23	67.13	16.69	0.46	130.0	± 9.6 %
		Y	6.16	66.95	16.48		130.0	
		Z	6.31	67.12	16.69		130.0	
10643- AAB	IEEE 802.11ac WiFi (160MHz, MCS7, 90pc duty cycle)	X	6.08	66.88	16.48	0.46	130.0	± 9.6 %
		Y	6.00	66.65	16.23		130.0	
		Z	6.15	66.83	16.45		130.0	
10644- AAB	IEEE 802.11ac WiFi (160MHz, MCS8, 90pc duty cycle)	x	6.25	67.41	16.77	0.46	130.0	± 9.6 %
		Y	6.14	67.08	16.46		130.0	
		Z	6.37	67.51	16.81		130.0	
10645- AAB	IEEE 802.11ac WiFi (160MHz, MCS9, 90pc duty cycle)	x	6.68	68.28	17.17	0.46	130.0	±9.6 %
		Y	6.39	67.46	16.61		130.0	
		Z	6.88	68.53	17.27		130.0	
10646- AAD	LTE-TDD (SC-FDMA, 1 RB, 5 MHz, QPSK, UL Subframe=2,7)	X	13.69	105.49	36,33	9.30	60.0	± 9.6 %
10004-0		Y	7.79	92.76	32.47		60.0	
		Z	10.29	98.14	34.43		60.0	
10647- AAC	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK, UL Subframe=2,7)	×	11.78	102.54	35.51	9.30	60.0	± 9.6 %
		Y	6.96	90.51	31.76		60.0	
		Z	9.19	95.89	33.75		60.0	
10648- AAA	CDMA2000 (1x Advanced)	x	0.67	62.83	10.37	0.00	150.0	± 9.6 %
		Y	0.60	61.40	9.04		150.0	
		Z	0.70	62.44	10.40		150.0	
10652- AAB	LTE-TDD (OFDMA, 5 MHz, E-TM 3.1, Clipping 44%)	X	3.26	65.18	15.69	2.23	80.0	±9.6 %
		Y	3.15	64.71	15.36		80.0	
		Z	3.35	65.17	15.95		80.0	
10653- AAB	LTE-TDD (OFDMA, 10 MHz, E-TM 3.1, Clipping 44%)	X	3.85	64.98	16.08	2.23	80.0	±9.6 %
		Y	3.74	64.58	15.78		80.0	10000
		Z	3.91	64.91	16.22		80.0	
10654- AAB	LTE-TDD (OFDMA, 15 MHz, E-TM 3.1, Clipping 44%)	X	3.84	64.69	16.11	2.23	80.0	±9.6 %
		Y	3.75	64.30	15.82		80.0	
	E.	Z	3.89	64.61	16.22		80.0	
10655- AAB	LTE-TDD (OFDMA, 20 MHz, E-TM 3.1, Clipping 44%)	X	3.90	64.72	16.17	2.23	80.0	± 9.6 %
	and the second se	Y	3.82	64.32	15.88		80.0	
		Z	3.95	64.65	16.28		80.0	

<sup>E</sup> Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

# Calibration Laboratory of Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Huawei (Auden) Client

Object	D2450V2 - SN: 9	78	
Calibration procedure(s)	QA CAL-05.v9 Calibration proce	dure for dipole validation kits abo	ove 700 MHz
Calibration date:	February 08, 201	6	
The measurements and the unce	rtainties with confidence p	ional standards, which realize the physical un robability are given on the following pages an ry facility: environment temperature $(22 \pm 3)^{\circ}$	d are part of the certificate.
Calibration Equipment used (M&T	E critical for calibration)		
	E critical for calibration)	Cal Date (Certificate No.)	Scheduled Calibration
rimary Standards	THE R. L.	Cal Date (Certificate No.) 07-Oct-15 (No. 217-02222)	Scheduled Calibration Oct-16
rimary Standards ower meter EPM-442A	ID #		
rimary Standards ower meter EPM-442A ower sensor HP 8481A	ID # GB37480704	07-Oct-15 (No. 217-02222)	Oct-16
rimary Standards ower meter EPM-442A ower sensor HP 8481A ower sensor HP 8481A	ID # GB37480704 US37292783	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222)	Oct-16 Oct-16
rimary Standards ower meter EPM-442A ower sensor HP 8481A ower sensor HP 8481A eference 20 dB Attenuator	ID # GB37480704 US37292783 MY41092317	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223)	Oct-16 Oct-16 Oct-16
rimary Standards ower meter EPM-442A ower sensor HP 8481A ower sensor HP 8481A reference 20 dB Attenuator ype-N mismatch combination	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k)	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131)	Oct-16 Oct-16 Oct-16 Mar-16
Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator ype-N mismatch combination Reference Probe EX3DV4	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) 01-Apr-15 (No. 217-02134)	Oct-16 Oct-16 Oct-16 Mar-16 Mar-16
Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 7349	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. EX3-7349_Dec15)	Oct-16 Oct-16 Oct-16 Mar-16 Mar-16 Dec-16
Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 7349 SN: 601	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. EX3-7349_Dec15) 30-Dec-15 (No. DAE4-601_Dec15)	Oct-16 Oct-16 Oct-16 Mar-16 Mar-16 Dec-16 Dec-16
Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 7349 SN: 601 ID #	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. EX3-7349_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) Check Date (in house)	Oct-16 Oct-16 Oct-16 Mar-16 Mar-16 Dec-16 Dec-16 Scheduled Check
Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Recondary Standards RF generator R&S SMT-06	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 7349 SN: 601 ID # 100972 US37390585 S4206	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 31-Dec-15 (No. EX3-7349_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) Check Date (in house) 15-Jun-15 (in house check Jun-15) 18-Oct-01 (in house check Oct-15)	Oct-16 Oct-16 Oct-16 Mar-16 Mar-16 Dec-16 Dec-16 Scheduled Check In house check: Jun-18
rimary Standards ower meter EPM-442A ower sensor HP 8481A ower sensor HP 8481A deference 20 dB Attenuator ype-N mismatch combination deference Probe EX3DV4 VAE4 econdary Standards E generator R&S SMT-06 letwork Analyzer HP 8753E	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 7349 SN: 601 ID # 100972	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 31-Dec-15 (No. EX3-7349_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) Check Date (in house) 15-Jun-15 (in house check Jun-15)	Oct-16 Oct-16 Oct-16 Mar-16 Mar-16 Dec-16 Dec-16 Scheduled Check In house check: Jun-18
Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Recondary Standards RF generator R&S SMT-06 Retwork Analyzer HP 8753E	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 7349 SN: 601 ID # 100972 US37390585 S4206	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 31-Dec-15 (No. EX3-7349_Dec15) 30-Dec-15 (No. DAE4-601_Dec15) Check Date (in house) 15-Jun-15 (in house check Jun-15) 18-Oct-01 (in house check Oct-15)	Oct-16 Oct-16 Oct-16 Mar-16 Dec-16 Dec-16 Scheduled Check In house check: Jun-18 In house check: Oct-16
Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Recondary Standards RF generator R&S SMT-06 Retwork Analyzer HP 8753E	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 7349 SN: 601 ID # 100972 US37390585 S4206 Name Jeton Kastrati	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 30-Dec-15 (No. 217-02134) 30-Dec-15 (No. 217-02134) 31-Dec-15 (No. 217	Oct-16 Oct-16 Oct-16 Mar-16 Dec-16 Dec-16 Scheduled Check In house check: Jun-18 In house check: Oct-16
Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 7349 SN: 601 ID # 100972 US37390585 S4206 Name	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 30-Dec-15 (No. 217-02134) 30-Dec-15 (No. 217-02134) 30-Dec-15 (No. 217-02134) 30-Dec-15 (No. 217-02134) 31-Dec-15 (No. 217	Oct-16 Oct-16 Oct-16 Mar-16 Dec-16 Dec-16 Scheduled Check In house check: Jun-18 In house check: Oct-16
Calibration Equipment used (M&T Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by: Approved by:	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 7349 SN: 601 ID # 100972 US37390585 S4206 Name Jeton Kastrati	07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02222) 07-Oct-15 (No. 217-02223) 01-Apr-15 (No. 217-02131) 01-Apr-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 31-Dec-15 (No. 217-02134) 30-Dec-15 (No. 217-02134) 30-Dec-15 (No. 217-02134) 31-Dec-15 (No. 217	Oct-16 Oct-16 Oct-16 Mar-16 Dec-16 Dec-16 Scheduled Check In house check: Jun-18 In house check: Oct-16

Accreditation No.: SCS 0108

Schweizerischer Kalibrierdienst S

Service suisse d'étalonnage C

Servizio svizzero di taratura

S Swiss Calibration Service

Certificate No: D2450V2-978\_Feb16

This c

Certificate No: D2450V2-978\_Feb16



# AC-MR

# Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst

- C Service suisse d'étalonnage
- Servizio svizzero di taratura
- S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

# Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

# Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

# Additional Documentation:

e) DASY4/5 System Handbook

## Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY5	V52.8.8
Advanced Extrapolation	
Modular Flat Phantom	
10 mm	with Spacer
dx, dy, dz = 5 mm	
2450 MHz ± 1 MHz	
	Advanced Extrapolation Modular Flat Phantom 10 mm dx, dy, dz = 5 mm

# **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.9 ± 6 %	1.88 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

# SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.7 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	53.3 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.34 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.9 W/kg ± 16.5 % (k=2)

## Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.2 ± 6 %	2.03 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	7 <u>9599</u>	1

# SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition		
SAR measured	250 mW input power	13.3 W/kg	
SAR for nominal Body TSL parameters	normalized to 1W	52.1 W/kg ± 17.0 % (k=2)	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition		
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL SAR measured	condition 250 mW input power	6.26 W/kg	

# Appendix (Additional assessments outside the scope of SCS 0108)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.0 Ω + 3.6 jΩ	
Return Loss	- 26.8 dB	

## Antenna Parameters with Body TSL

Impedance, transformed to feed point	49.8 Ω + 5.8 jΩ
Return Loss	- 24.7 dB

## **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.154 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

## Additional EUT Data

Manufactured by	SPEAG	
Manufactured on	December 30, 2014	

# **DASY5 Validation Report for Head TSL**

Date: 08.02.2016

Test Laboratory: SPEAG, Zurich, Switzerland

## DUT: Dipole 2450 MHz ; Type: D2450V2; Serial: D2450V2 - SN: 978

Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz;  $\sigma$  = 1.88 S/m;  $\epsilon_r$  = 37.9;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

#### DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(7.67, 7.67, 7.67); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7372)


## Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 115.7 V/m; Power Drift = 0.00 dB Peak SAR (extrapolated) = 28.4 W/kg SAR(1 g) = 13.7 W/kg; SAR(10 g) = 6.34 W/kg Maximum value of SAR (measured) = 23.1 W/kg



0 dB = 23.1 W/kg = 13.64 dBW/kg

# Impedance Measurement Plot for Head TSL

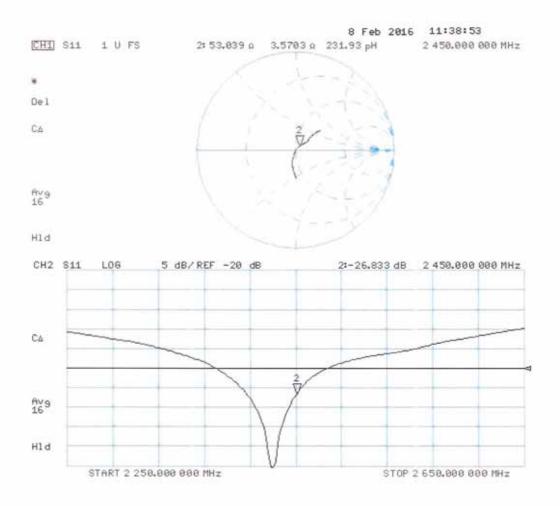

# DASY5 Validation Report for Body TSL

Date: 08.02.2016

Test Laboratory: SPEAG, Zurich, Switzerland

#### DUT: Dipole 2450 MHz ; Type: D2450V2; Serial: D2450V2 - SN: 978


Communication System: UID 0 - CW; Frequency: 2450 MHz Medium parameters used: f = 2450 MHz;  $\sigma$  = 2.03 S/m;  $\epsilon_r$  = 52.2;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

#### DASY52 Configuration:

- Probe: EX3DV4 SN7349; ConvF(7.53, 7.53, 7.53); Calibrated: 30.12.2014;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 17.08.2015
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7372)


#### Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 108.7 V/m; Power Drift = -0.00 dB Peak SAR (extrapolated) = 26.4 W/kg SAR(1 g) = 13.3 W/kg; SAR(10 g) = 6.26 W/kg Maximum value of SAR (measured) = 21.7 W/kg

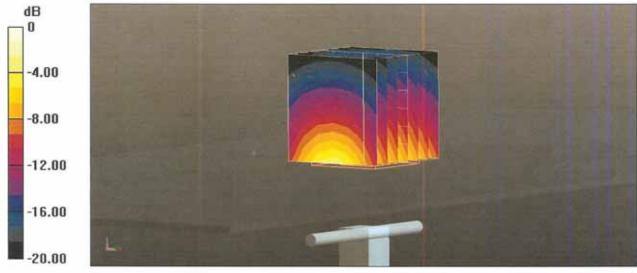

0 dB = 21.7 W/kg = 13.36 dBW/kg

# Impedance Measurement Plot for Body TSL

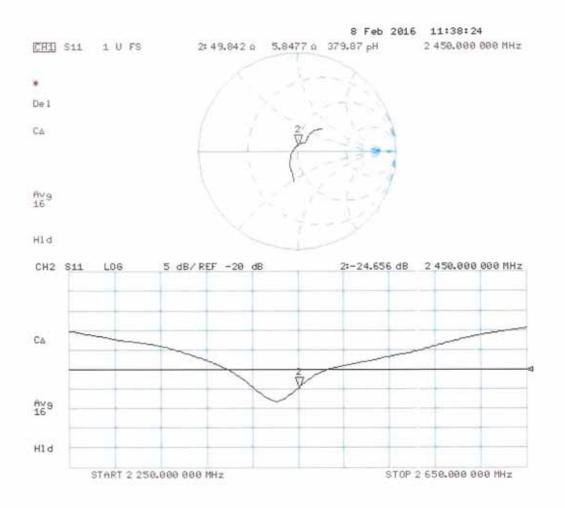

# Justification of the extended calibration of Dipole D2450V2 SN:978

Per KDB 865664, we have Measured the Impedance and Return Loss as below, and the return loss is <-20dB, with 20% of prior calibration; the real or imaginary parts of the impedance is with 5 ohm of prior calibration. Therefore the verification result should support extended calibration.

Dipole2450 Head TST	Target Value	Measured Value	Difference
Impedance transformed to feed point	53Ω+3.6jΩ	50.89Ω+0.18jΩ	R=-2.11Ω, X=-3.42Ω
Return Loss	-26.8dB	-29.84dB	-11.34%
Dipole2450 Body TST	Target Value	Measured Value	Difference
Impedance transformed to feed point	49.8Ω+5.8jΩ	50.63Ω+3.66jΩ	R=0.83Ω, X=-2.14Ω
Return Loss	-24.7dB	-28.74dB	-16.36%
Measured Date	2016-02-08	2018-01-26	
Impedance Tes	st-Head	Return Loss T	est-Head
Find       S11 Swith (k+jk) Scale 1.0000 [F]         >1 2,4500000 GHZ       50.885 n         175.66 mg       JL <tll pit<="" td="">         (1)       (1)</tll>		>10:00       >1 2.4500000 GHZ -29.839 db         10:00       >1 2.4500000 GHZ -29.839 db         -10:00       -10:00         -20:00       -10:00         -30:00       -10:00         -30:00       -10:00         -30:00       -10:00         -30:00       -10:00         -30:00       -10:00         -30:00       -10:00         -30:00       -10:00         -30:00       -10:00         -30:00       -10:00         -30:00       -10:00         -30:00       -10:00         -40:00       -10:00         -50:00       -10:00         -60:00       -10:00         -70:00       -10:00	
Impedance Tes	st-Body	Return Loss T	est-Body
>1       2.4500000 cmz       50.622 n       3.6550 n       237.44 pm		• End         511         Log         Mag         10.000h/ Mef         -20.000h (F1)           30.00         >1         2.500000         Gitz         -28.742         Git           20.00	