

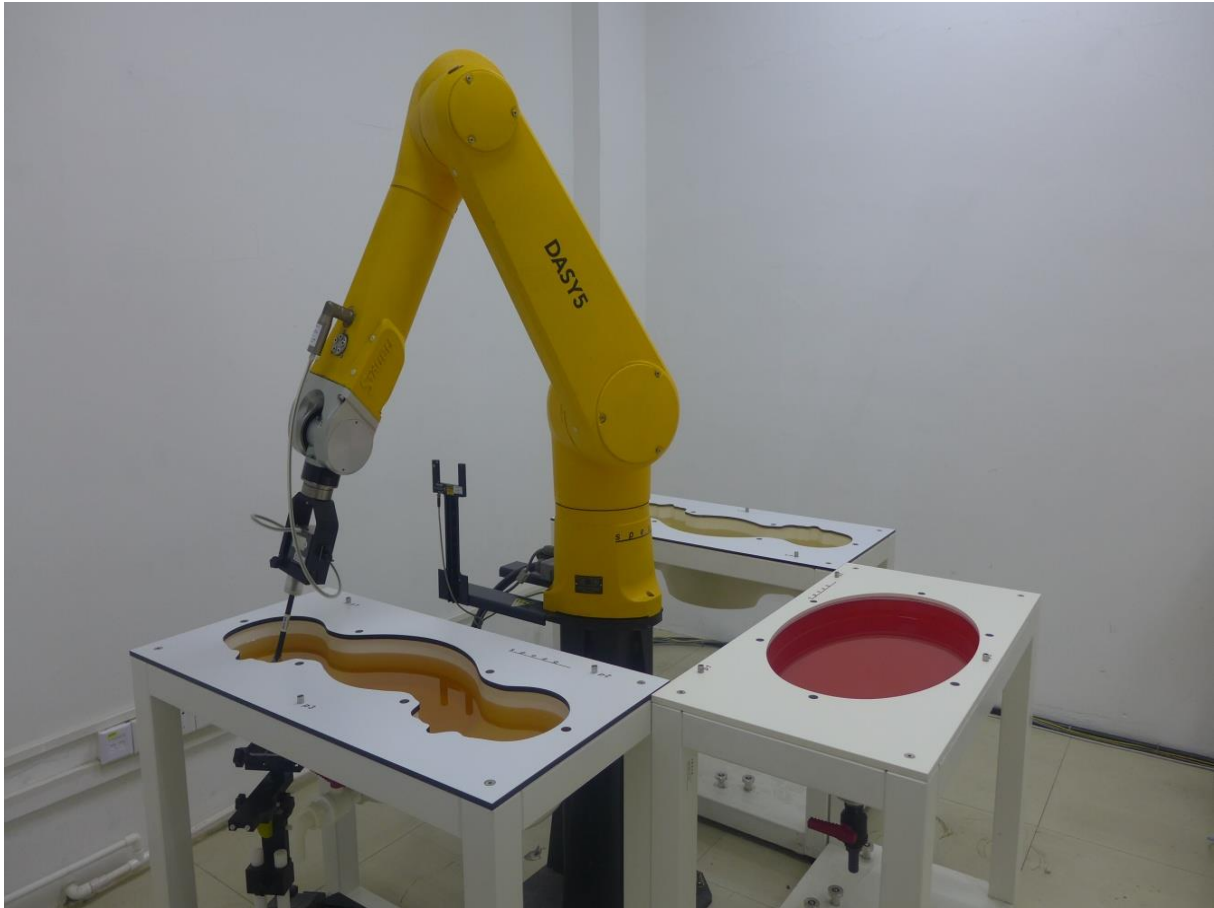


Appendix D

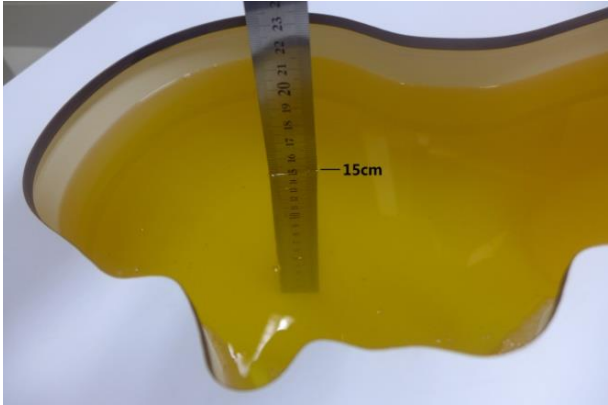
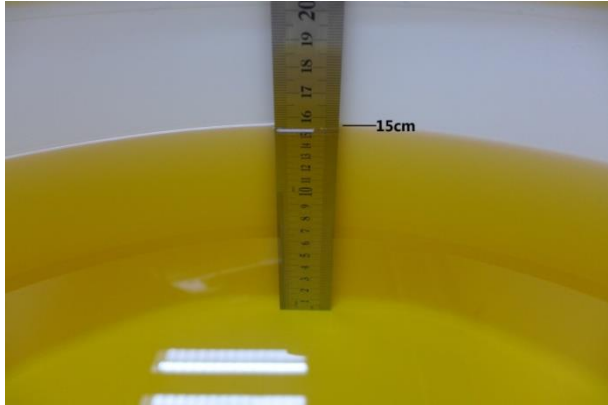
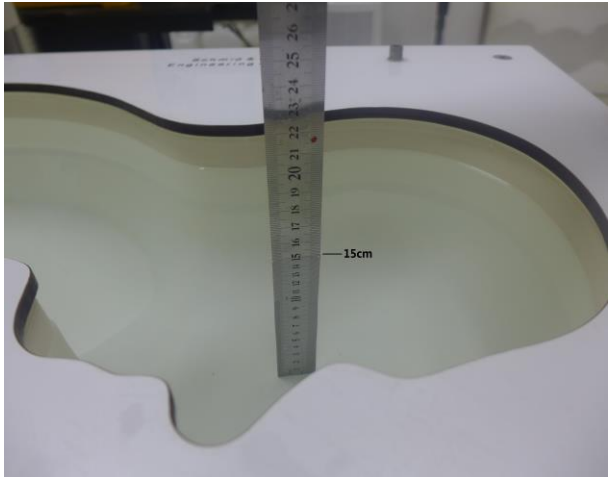
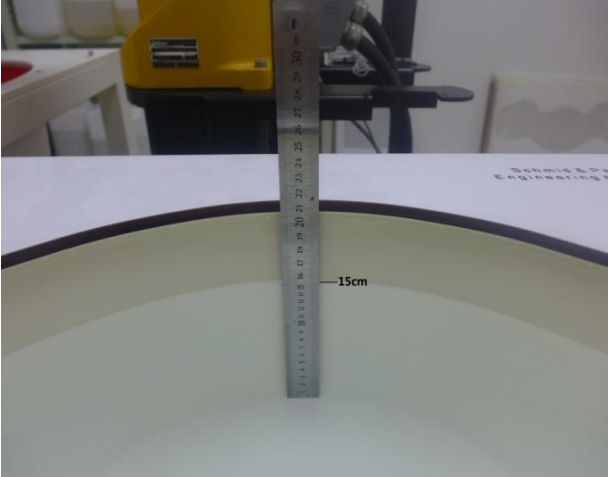
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

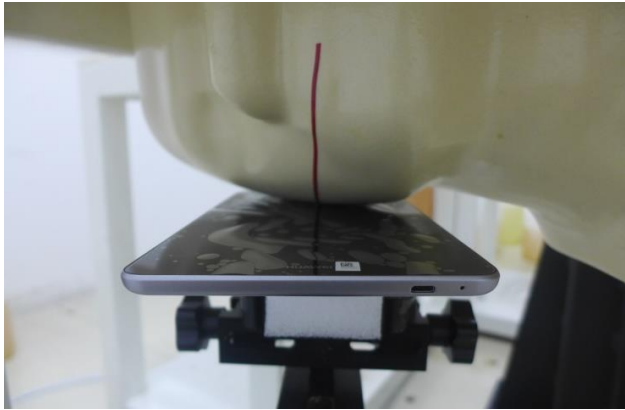
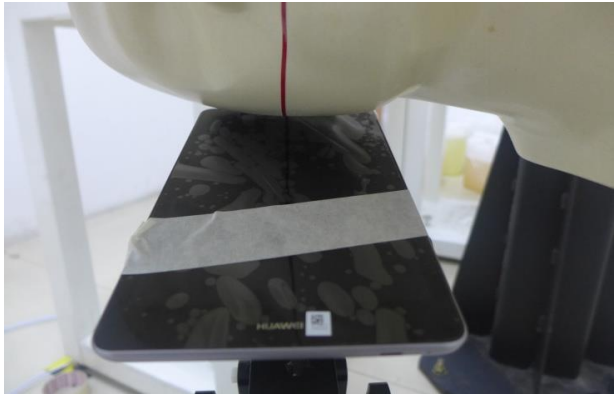

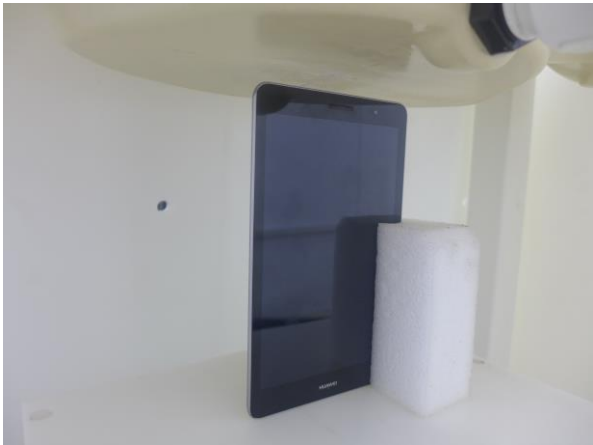
1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

<p>Photo 1: Tissue Simulant Liquid for Head 2450</p>	<p>Photo 2: Tissue Simulant Liquid for Body 2450</p>
	
<p>Photo 3: Tissue Simulant Liquid for Head 5G</p>	<p>Photo 4: Tissue Simulant Liquid for Body 5G</p>
	

3. Photographs of EUT test position

<p>Photo 5: Left touch cheek</p>	<p>Photo 6: Left tilted 15 degree</p>
 A photograph showing a tablet device mounted on a test rig. A red vertical line is drawn on the tablet's surface, indicating the 'left touch cheek' position.	 A photograph showing the tablet device tilted at a 15-degree angle to the left. A red vertical line is drawn on the tablet's surface, indicating the 'left tilted 15 degree' position.
<p>Photo 7: Back side 0mm</p>	<p>Photo 8: Top side 12mm</p>
 A photograph showing the back side of the tablet device mounted on the test rig, with the camera lens and other components visible.	 A photograph showing the top side of the tablet device mounted on the test rig, with a white foam block used for support.

4. EUT Constructional Details

