

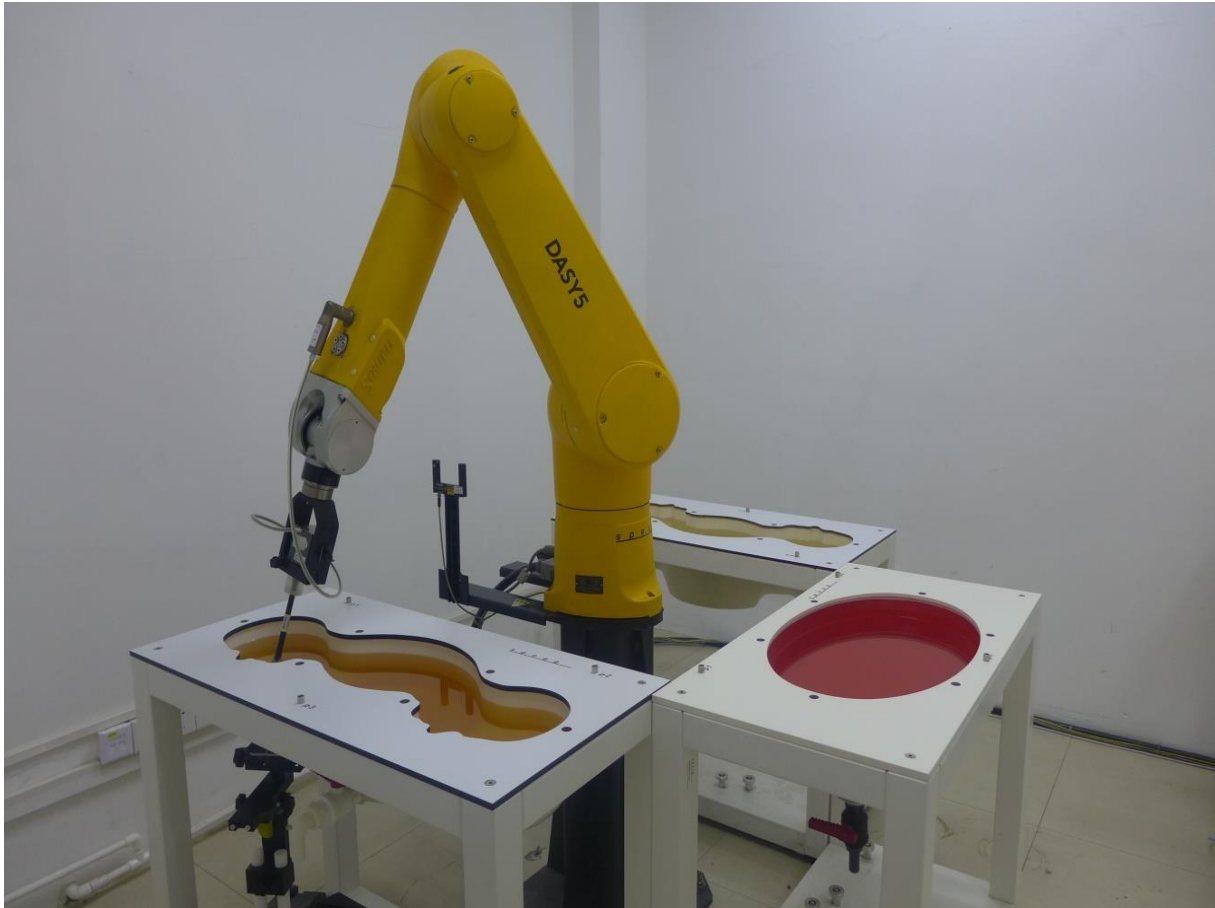


Appendix D

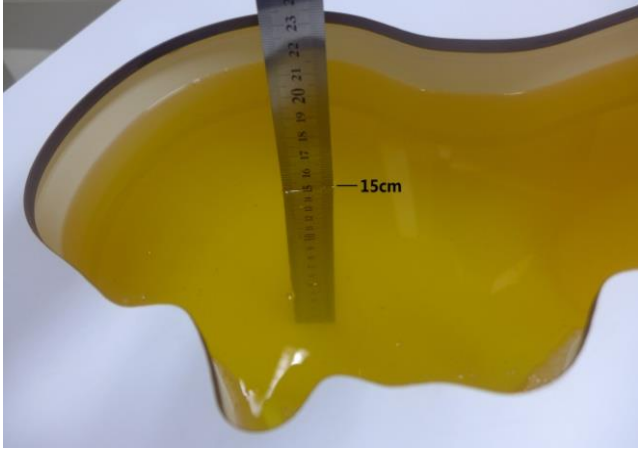
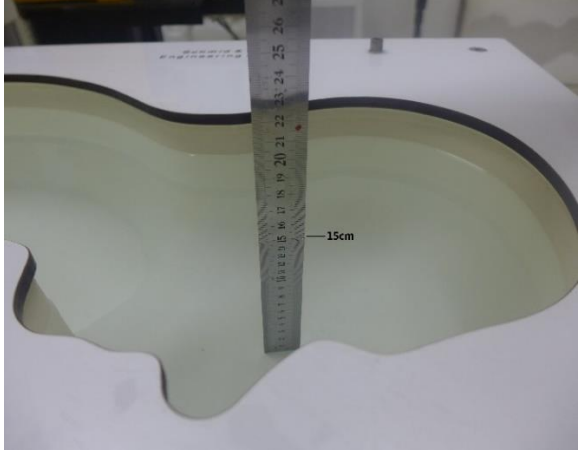
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

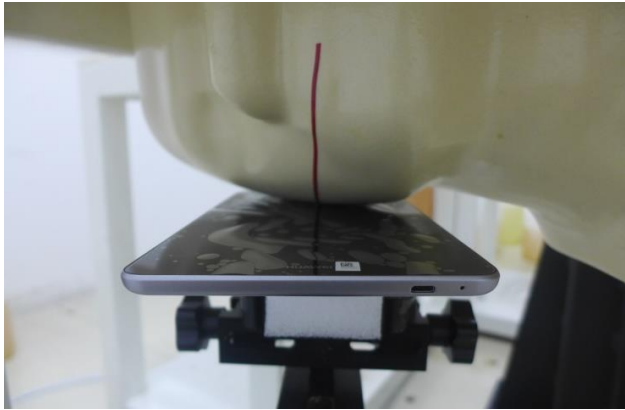
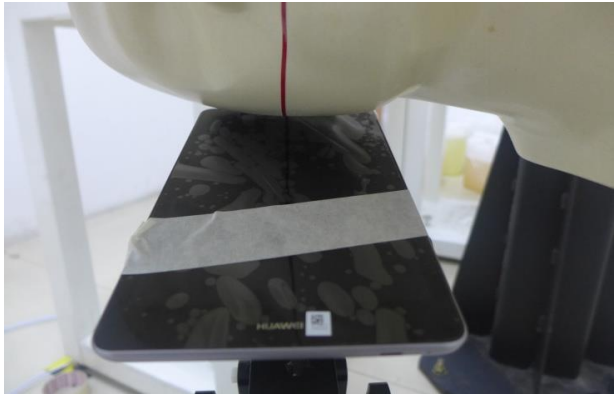

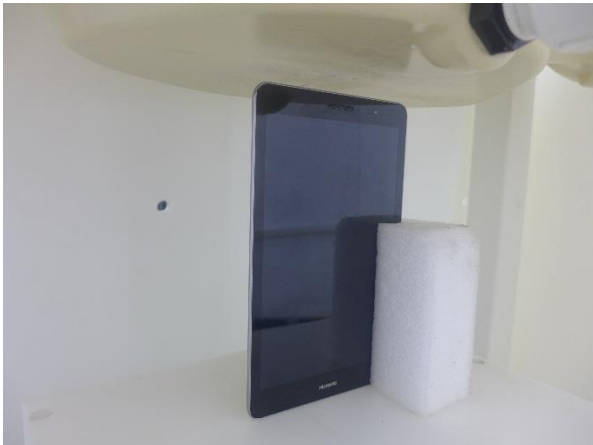
1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2450	Photo 2: Tissue Simulant Liquid for Head 5G
	

3. Photographs of EUT test position

<p>Photo 3: Left touch cheek</p>	<p>Photo 4: Left tilted 15 degree</p>
 <p>A photograph showing a tablet device mounted on a test rig. A red vertical line is drawn on the tablet's screen, indicating the 'left touch cheek' position. The device is held horizontally by a black mechanical fixture.</p>	 <p>A photograph showing the same tablet device on the test rig, but tilted at an angle of 15 degrees to the left. A red vertical line is also present on the screen.</p>
<p>Photo 5: Back side 0mm</p>	<p>Photo 6: Top side 12mm</p>
 <p>A photograph showing the back side of the tablet device. The device is held by a black mechanical fixture, and the camera lens and other components are visible.</p>	 <p>A photograph showing the top side of the tablet device. The device is held vertically by a black mechanical fixture, and a white foam block is visible next to it for support.</p>

4. EUT Constructional Details

