



#### Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.7Ω+ 7.33jΩ	
Return Loss	- 22.4dB	

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.9Ω+ 5.36jΩ
Return Loss	- 25.4dB

#### **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.303 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z15-97179

Page 4 of 8



## No.B18N00005-SAR Page 111 of 132



 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2079
 Fax: +86-10-62304633-2504

 E-mail: cttl@chinattl.com
 Http://www.chinattl.cn

**DASY5 Validation Report for Head TSL** 


#### Date: 11.04.2015

Test Laboratory: CTTL, Beijing, China **DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d088** Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1 Medium parameters used: f = 1900 MHz; σ = 1.385 S/m; εr = 40.56; ρ = 1000 kg/m3 Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:

- Probe: EX3DV4 SN3617; ConvF(8.07, 8.07, 8.07); Calibrated: 8/26/2015;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 8/26/2015
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

System Performance Check/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 100.6 V/m; Power Drift = -0.04 dB Peak SAR (extrapolated) = 18.9W/kg SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.22 W/kg Maximum value of SAR (measured) = 14.5 W/kg

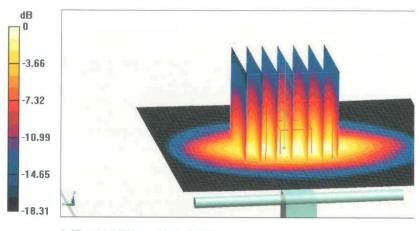

0 dB = 14.5 W/kg = 11.61 dBW/kg


Certificate No: Z15-97179

Page 5 of 8





#### Impedance Measurement Plot for Head TSL

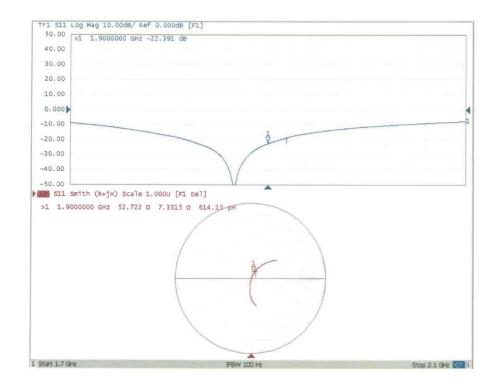

Certificate No: Z15-97179

Page 6 of 8





**DASY5 Validation Report for Body TSL** Test Laboratory: CTTL, Beijing, China Date: 11.04.2015


DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d088

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1 Medium parameters used: f = 1900 MHz;  $\sigma$  = 1.536 S/m;  $\epsilon_r$  = 54.05;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Center Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:

- Probe: EX3DV4 SN3617; ConvF(7.74, 7.74, 7.74); Calibrated: 8/26/2015;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 8/26/2015
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

System Performance Check/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 96.09 V/m; Power Drift = -0.01 dB Peak SAR (extrapolated) = 18.9 W/kg SAR(1 g) = 10.3 W/kg; SAR(10 g) = 5.33 W/kg Maximum value of SAR (measured) = 14.9 W/kg

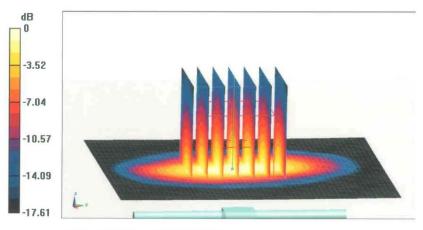

0 dB = 14.9 W/kg = 11.73 dBW/kg


Certificate No: Z15-97179

Page 7 of 8





Impedance Measurement Plot for Body TSL

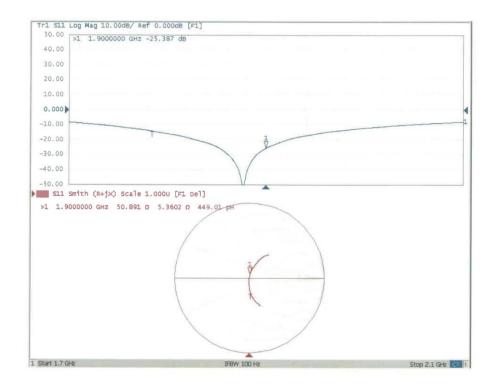

Certificate No: Z15-97179

Page 8 of 8



### 2450 MHz Dipole Calibration Certificate

Tel: +86-10-62304	633-2079 Fax:	strict, Beijing, 100191, China 44, 44, 44, 44, 44, 44, 44, 44, 44, 44	No. L0570
E-mail: cttl@china	attl.com Http: TL(South Brai	nch) Certificate No: Z1	6 07400
And the second se	-		15-97180
CALIBRATION C	ERTIFICA	TE	ALL FALLER
Object	D2450	V2 - SN: 873	
Calibration Procedure(s)			
		1-2-003-01	
	Calibra	ation Procedures for dipole validation kits	
Calibration date:	Octobe	er 30, 2015	
measurements(SI). The me	easurements and	traceability to national standards, which real the uncertainties with confidence probability	
measurements(SI). The me pages and are part of the c All calibrations have beer humidity<70%.	easurements and ertificate. n conducted in	the uncertainties with confidence probability the closed laboratory facility: environment	are given on the following
measurements(SI). The me pages and are part of the c All calibrations have beer humidity<70%. Calibration Equipment used	easurements and ertificate. n conducted in	the uncertainties with confidence probability the closed laboratory facility: environment	are given on the following
measurements(SI). The me pages and are part of the c All calibrations have beer humidity<70%. Calibration Equipment used	easurements and ertificate. n conducted in d (M&TE critical f	I the uncertainties with confidence probability the closed laboratory facility: environment for calibration)	are given on the following temperature(22±3)℃ and
measurements(SI). The me pages and are part of the cr All calibrations have beer humidity<70%. Calibration Equipment used Primary Standards	easurements and ertificate. n conducted in d (M&TE critical f	the uncertainties with confidence probability the closed laboratory facility: environment for calibration) Cal Date(Calibrated by, Certificate No.)	are given on the following temperature(22±3)℃ and Scheduled Calibration
measurements(SI). The me pages and are part of the cr All calibrations have beer humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4	easurements and ertificate. n conducted in d (M&TE critical f ID # 101919 101547	the uncertainties with confidence probability the closed laboratory facility: environment for calibration) Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256)	are given on the following temperature(22±3)℃ and Scheduled Calibration Jun-16
measurements(SI). The me pages and are part of the cr All calibrations have beer humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91	easurements and ertificate. n conducted in d (M&TE critical f ID # 101919 101547	the uncertainties with confidence probability the closed laboratory facility: environment for calibration) Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256)	are given on the following temperature(22±3)℃ and Scheduled Calibration Jun-16 Jun-16
measurements(SI). The me pages and are part of the cr All calibrations have beer humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4	easurements and ertificate. n conducted in d (M&TE critical f ID # 101919 101547 SN 3617	I the uncertainties with confidence probability the closed laboratory facility: environment for calibration) Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 26-Aug-15(SPEAG,No.EX3-3617_Aug15) 26-Aug-15(SPEAG,No.DAE4-777_Aug15)	are given on the following temperature(22±3)℃ and Scheduled Calibration Jun-16 Jun-16 Aug-16 Aug-16
measurements(SI). The me pages and are part of the cr All calibrations have beer humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4	easurements and ertificate. n conducted in d (M&TE critical f ID # 101919 101547 SN 3617 SN 777	I the uncertainties with confidence probability the closed laboratory facility: environment for calibration) Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 26-Aug-15(SPEAG,No.EX3-3617_Aug15) 26-Aug-15(SPEAG,No.DAE4-777_Aug15) Cal Date(Calibrated by, Certificate No.)	are given on the following temperature(22±3)℃ and Scheduled Calibration Jun-16 Jun-16 Aug-16 Aug-16 Scheduled Calibration
measurements(SI). The me pages and are part of the cr All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards	easurements and ertificate. n conducted in d (M&TE critical f ID # 101919 101547 SN 3617 SN 3617 SN 777 ID # ID # MY49071430	I the uncertainties with confidence probability the closed laboratory facility: environment for calibration) Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 26-Aug-15(SPEAG,No.EX3-3617_Aug15) 26-Aug-15(SPEAG,No.DAE4-777_Aug15) Cal Date(Calibrated by, Certificate No.) 02-Feb-15 (CTTL, No.J15X00729)	are given on the following temperature(22±3)℃ and Scheduled Calibration Jun-16 Jun-16 Aug-16 Aug-16
measurements(SI). The me pages and are part of the cr All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	easurements and ertificate. n conducted in d (M&TE critical f ID # 101919 101547 SN 3617 SN 3617 SN 777 ID # ID # MY49071430	I the uncertainties with confidence probability the closed laboratory facility: environment for calibration) Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 26-Aug-15(SPEAG,No.EX3-3617_Aug15) 26-Aug-15(SPEAG,No.DAE4-777_Aug15) Cal Date(Calibrated by, Certificate No.) 02-Feb-15 (CTTL, No.J15X00729)	are given on the following temperature(22±3)°C and Scheduled Calibration Jun-16 Jun-16 Aug-16 Aug-16 Scheduled Calibration Feb-16 Feb-16
measurements(SI). The me pages and are part of the cr All calibrations have beer humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C Network Analyzer E5071C	easurements and ertificate. n conducted in d (M&TE critical f ID # 101919 101547 SN 3617 SN 3617 SN 777 ID # MY49071430 MY46110673	I the uncertainties with confidence probability the closed laboratory facility: environment for calibration) Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 26-Aug-15(SPEAG,No.EX3-3617_Aug15) 26-Aug-15(SPEAG,No.DAE4-777_Aug15) 26-Aug-15(SPEAG,No.DAE4-777_Aug15) Cal Date(Calibrated by, Certificate No.) 02-Feb-15 (CTTL, No.J15X00729) 03-Feb-15 (CTTL, No.J15X00728)	are given on the following temperature(22±3)℃ and Scheduled Calibration Jun-16 Jun-16 Aug-16 Aug-16 Scheduled Calibration Feb-16
measurements(SI). The me pages and are part of the cr All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	easurements and ertificate. n conducted in d (M&TE critical f ID # 101919 101547 SN 3617 SN 3617 SN 777 ID # MY49071430 MY46110673 Name	the uncertainties with confidence probability the closed laboratory facility: environment for calibration) Cal Date(Calibrated by, Certificate No.) 01-Jul-15 (CTTL, No.J15X04256) 01-Jul-15 (CTTL, No.J15X04256) 26-Aug-15(SPEAG,No.DAE4-777_Aug15) 26-Aug-15(SPEAG,No.DAE4-777_Aug15) Cal Date(Calibrated by, Certificate No.) 02-Feb-15 (CTTL, No.J15X00729) 03-Feb-15 (CTTL, No.J15X00728) Function	are given on the following temperature(22±3)°C and Scheduled Calibration Jun-16 Jun-16 Aug-16 Aug-16 Scheduled Calibration Feb-16 Feb-16 Signature

Certificate No: Z15-97180

Page 1 of 8



## No.B18N00005-SAR Page 116 of 132



 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2079
 Fax: +86-10-62304633-2504

 E-mail: cttl@chinattl.com
 Http://www.chinattl.cn

#### **Glossary:**

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) For hand-held devices used in close proximity to the ear (frequency range of 300MHz to 3GHz)", February 2005
- c) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

#### **Additional Documentation:**

d) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
  of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z15-97180

Page 2 of 8



## No.B18N00005-SAR Page 117 of 132



CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com

Http://www.chinattl.cn

a

g

#### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.8.8.1222
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

#### **Head TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.1 ± 6 %	1.82 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.1 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	52.5 mW /g ± 20.8 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	6.01 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.1 mW /g ± 20.4 % (k=2)

#### **Body TSL parameters**

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	53.1 ± 6 %	1.94 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

#### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.0 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	52.3 mW /g ± 20.8 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	6.07 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	24.4 mW /g ± 20.4 % (k=2)

Certificate No: Z15-97180

Page 3 of 8





#### Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.4Ω+ 3.42jΩ	
Return Loss	- 26.6dB	

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.5Ω+ 6.53jΩ	
Return Loss	- 23.7dB	

#### **General Antenna Parameters and Design**

Electrical Delay (one direction)	1.265 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### Additional EUT Data

Manufactured by	SPEAG

Certificate No: Z15-97180

Page 4 of 8



### No.B18N00005-SAR Page 119 of 132



 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2079
 Fax: +86-10-62304633-2504

 E-mail: cttl@chinattl.com
 Http://www.chinattl.cn

Date: 10.30.2015


#### DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 873

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz;  $\sigma = 1.816$  S/m;  $\epsilon r = 40.14$ ;  $\rho = 1000$  kg/m3 Phantom section: Left Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:

- Probe: EX3DV4 SN3617; ConvF(7.24, 7.24, 7.24); Calibrated: 8/26/2015;
- Sensor-Surface: 2mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 8/26/2015
- Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/1
- Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 106.1 V/m; Power Drift = 0.05 dB Peak SAR (extrapolated) = 27.3 W/kg SAR(1 g) = 13.1 W/kg; SAR(10 g) = 6.01 W/kg Maximum value of SAR (measured) = 20.1 W/kg

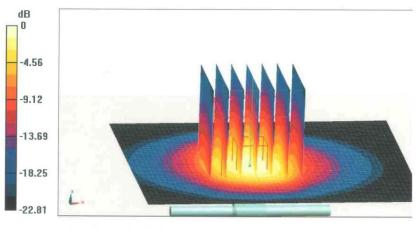

0 dB = 20.1 W/kg = 13.03 dBW/kg


Certificate No: Z15-97180

Page 5 of 8





#### Impedance Measurement Plot for Head TSL

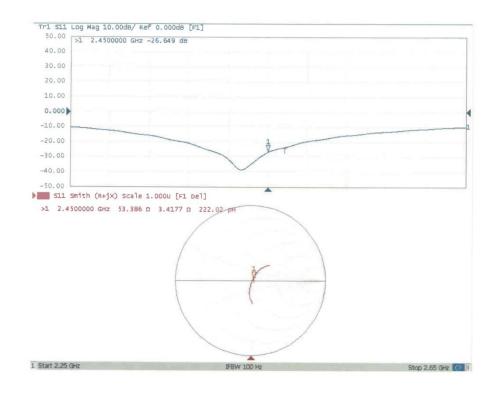


Certificate No: Z15-97180

Page 6 of 8



## No.B18N00005-SAR Page 121 of 132

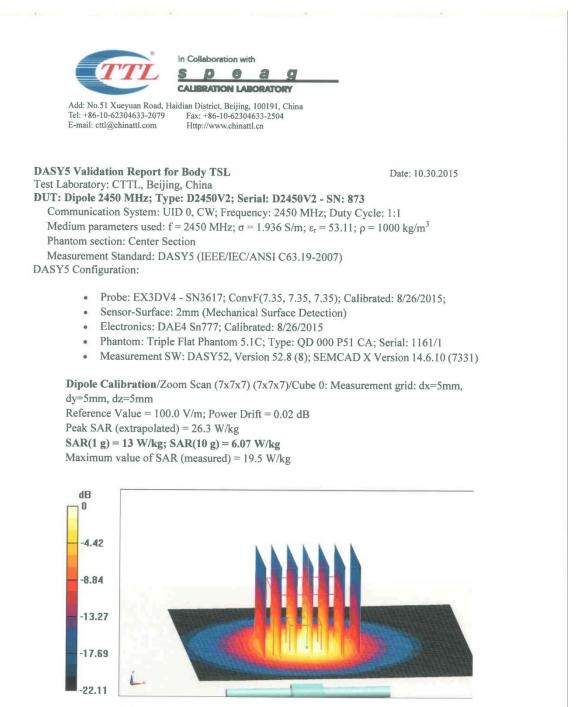

0 dB = 19.5 W/kg = 12.90 dBW/kg

Certificate No: Z15-97180

Page 7 of 8



## No.B18N00005-SAR Page 122 of 132




 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2079
 Fax: +86-10-62304633-2504

 E-mail: cttl@chinattl.com
 Http://www.chinattl.cn

Impedance Measurement Plot for Body TSL

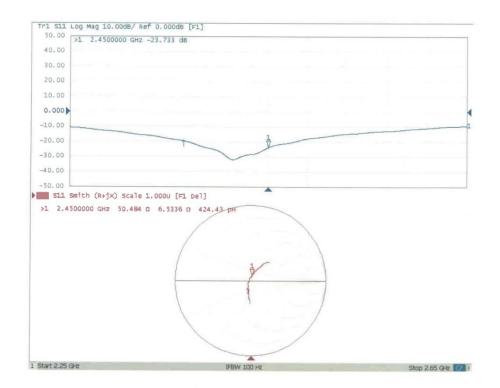

Certificate No: Z15-97180

Page 8 of 8



### 2550 MHz Dipole Calibration Certificate

		Standard S	Swiss Calibration Service
ccredited by the Swiss Accredita he Swiss Accreditation Service	Superior and the second s		ccreditation No.: SCS 0108
ultilateral Agreement for the re			lo: D2550V2-1010 Jul15
ient TMC-SZ (Aude	n)	Certificate N	10: D2550V2-1010_00115
CALIBRATION C	CERTIFICATE		
Dbject	D2550V2 - SN: 10	010	
	04.041.05.0		
Calibration procedure(s)	QA CAL-05.v9 Calibration proces	dure for dipole validation kits ab	ove 700 MHz
Calibration date:	July 24, 2015		
	, ,		
The measurements and the unce All calibrations have been condu	ertainties with confidence proceed in the closed laborator	conal standards, which realize the physical u robability are given on the following pages a y facility: environment temperature $(22 \pm 3)$	and are part of the certificate.
The measurements and the unce All calibrations have been condu Calibration Equipment used (M&	ertainties with confidence protected in the closed laborator	robability are given on the following pages a y facility: environment temperature $(22 \pm 3)$	and are part of the certificate. )°C and humidity < 70%.
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards	ertainties with confidence protected in the closed laborator TE critical for calibration)	robability are given on the following pages a y facility: environment temperature (22 ± 3) Cal Date (Certificate No.)	and are part of the certificate. <sup>19</sup> C and humidity < 70%. Scheduled Calibration
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A	ertainties with confidence provide the closed laborator TE critical for calibration)	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020)	and are part of the certificate. 9°C and humidity < 70%. Scheduled Calibration Oct-15
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A	ertainties with confidence provide the closed laborator TE critical for calibration)           ID #           GB37480704           US37292783	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020) 07-Oct-14 (No. 217-02020)	and are part of the certificate. <sup>19</sup> C and humidity < 70%. Scheduled Calibration
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A	ertainties with confidence provide the closed laborator TE critical for calibration)	Cal Date (Certificate No.) 07-Oct-14 (No. 217-02020)	and are part of the certificate. )°C and humidity < 70%. Scheduled Calibration Oct-15 Oct-15
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator	TE critical for calibration) ID # GB37480704 US37292783 MY41092317	Cal Date (Certificate No.)           07-Oct-14 (No. 217-02020)	and are part of the certificate. y°C and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Oct-15 Oct-15
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination	ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k)	Cal Date (Certificate No.)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02020)           07-Oct-15 (No. 217-02021)           01-Apr-15 (No. 217-02131)	and are part of the certificate. P <sup>c</sup> and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Oct-15 Mar-16
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	ted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327	Cal Date (Certificate No.)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02020)           07-Oct-15 (No. 217-02021)           01-Apr-15 (No. 217-02131)           01-Apr-15 (No. 217-02134)	and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Oct-15 Mar-16 Mar-16
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	ID # GB37480704 US37292783 MY41092317 SN: 5047.2 / 06327 SN: 3205	Cal Date (Certificate No.)           07-Oct-14 (No. 217-02020)           07-Oct-15 (No. 217-02131)           01-Apr-15 (No. 217-02131)           01-Apr-15 (No. 217-02134)           30-Dec-14 (No. ES3-3205_Dec14)	and are part of the certificate. 9°C and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Mar-16 Mar-16 Dec-15
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4	intel swith confidence proceed in the closed laborator           TE critical for calibration)           ID #           GB37480704           US37292783           MY41092317           SN: 5058 (20k)           SN: 5047.2 / 06327           SN: 601           ID #           100005	Cal Date (Certificate No.)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02020)           07-Oct-15 (No. 217-02021)           01-Apr-15 (No. 217-02131)           01-Apr-15 (No. 217-02134)           30-Dec-14 (No. ES3-3205_Dec14)           18-Aug-14 (No. DAE4-601_Aug14)           Check Date (in house)           04-Aug-99 (in house check Oct-13)	and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Oct-15 Mar-16 Mar-16 Dec-15 Aug-15 Scheduled Check In house check: Oct-16
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards	ertainties with confidence proceed in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 50547.2 / 06327 SN: 3205 SN: 601 ID #	Cal Date (Certificate No.)         07-Oct-14 (No. 217-02020)         07-Oct-14 (No. 217-02020)         07-Oct-14 (No. 217-02020)         07-Oct-14 (No. 217-02021)         01-Apr-15 (No. 217-02131)         01-Apr-15 (No. 217-02134)         30-Dec-14 (No. ES3-3205_Dec14)         18-Aug-14 (No. DAE4-601_Aug14)         Check Date (in house)	and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Oct-15 Mar-16 Mar-16 Dec-15 Aug-15 Scheduled Check
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06	ertainties with confidence pro- cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 601 ID # 100005 US37390585 S4206	Cal Date (Certificate No.)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02021)           01-Apr-15 (No. 217-02131)           01-Apr-15 (No. 217-02134)           30-Dec-14 (No. ES3-3205_Dec14)           18-Aug-14 (No. DAE4-601_Aug14)           Check Date (in house)           04-Aug-99 (in house check Oct-13)           18-Oct-01 (in house check Oct-14)	and are part of the certificate. I°C and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Oct-15 Oct-15 Mar-16 Dec-15 Aug-15 Scheduled Check In house check: Oct-16 In house check: Oct-15
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E	in the closed laborator           TE critical for calibration)           ID #           GB37480704           US37292783           MY41092317           SN: 5058 (20k)           SN: 5058 (20k)           SN: 6047.2 / 06327           SN: 601           ID #           100005           US37390585 S4206           Name	Cal Date (Certificate No.)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02021)           01-Apr-15 (No. 217-02131)           01-Apr-15 (No. 217-02131)           01-Apr-15 (No. 217-02134)           30-Dec-14 (No. ES3-3205_Dec14)           18-Aug-14 (No. DAE4-601_Aug14)           Check Date (in house)           04-Aug-99 (in house check Oct-13)           18-Oct-01 (in house check Oct-14)	and are part of the certificate. PC and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Oct-15 Mar-16 Mar-16 Dec-15 Aug-15 Scheduled Check In house check: Oct-16
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06	ertainties with confidence pro- cted in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 601 ID # 100005 US37390585 S4206	Cal Date (Certificate No.)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02021)           01-Apr-15 (No. 217-02131)           01-Apr-15 (No. 217-02134)           30-Dec-14 (No. ES3-3205_Dec14)           18-Aug-14 (No. DAE4-601_Aug14)           Check Date (in house)           04-Aug-99 (in house check Oct-13)           18-Oct-01 (in house check Oct-14)	and are part of the certificate. I°C and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Oct-15 Oct-15 Mar-16 Dec-15 Aug-15 Scheduled Check In house check: Oct-16 In house check: Oct-15
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E	ertainties with confidence proceed in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 5047.2 / 06327 SN: 3205 SN: 601 ID # 100005 US37390585 S4206 Name Jeton Kastrati	Cal Date (Certificate No.)           07-Oct-14 (No. 217-02020)           01-Apr-15 (No. 217-02131)           01-Apr-15 (No. 217-02134)           30-Dec-14 (No. ES3-3205_Dec14)           18-Aug-14 (No. DAE4-601_Aug14)           Check Date (in house)           04-Aug-99 (in house check Oct-13)           18-Oct-01 (in house check Oct-14)           Function           Laboratory Technician	and are part of the certificate. I°C and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Oct-15 Oct-15 Mar-16 Dec-15 Aug-15 Scheduled Check In house check: Oct-16 In house check: Oct-15
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E	in the closed laborator           TE critical for calibration)           ID #           GB37480704           US37292783           MY41092317           SN: 5058 (20k)           SN: 5058 (20k)           SN: 6047.2 / 06327           SN: 601           ID #           100005           US37390585 S4206           Name	Cal Date (Certificate No.)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02020)           07-Oct-14 (No. 217-02021)           01-Apr-15 (No. 217-02131)           01-Apr-15 (No. 217-02131)           01-Apr-15 (No. 217-02134)           30-Dec-14 (No. ES3-3205_Dec14)           18-Aug-14 (No. DAE4-601_Aug14)           Check Date (in house)           04-Aug-99 (in house check Oct-13)           18-Oct-01 (in house check Oct-14)	and are part of the certificate. I°C and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Oct-15 Oct-15 Mar-16 Dec-15 Aug-15 Scheduled Check In house check: Oct-16 In house check: Oct-15
The measurements and the unce All calibrations have been condu Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 DAE4 Secondary Standards RF generator R&S SMT-06 Network Analyzer HP 8753E Calibrated by:	ertainties with confidence proceed in the closed laborator TE critical for calibration) ID # GB37480704 US37292783 MY41092317 SN: 5058 (20k) SN: 5047.2 / 06327 SN: 5047.2 / 06327 SN: 3205 SN: 601 ID # 100005 US37390585 S4206 Name Jeton Kastrati	Cal Date (Certificate No.)           07-Oct-14 (No. 217-02020)           01-Apr-15 (No. 217-02131)           01-Apr-15 (No. 217-02134)           30-Dec-14 (No. ES3-3205_Dec14)           18-Aug-14 (No. DAE4-601_Aug14)           Check Date (in house)           04-Aug-99 (in house check Oct-13)           18-Oct-01 (in house check Oct-14)           Function           Laboratory Technician	and are part of the certificate. I°C and humidity < 70%. Scheduled Calibration Oct-15 Oct-15 Oct-15 Oct-15 Mar-16 Dec-15 Aug-15 Scheduled Check In house check: Oct-16 In house check: Oct-15



## No.B18N00005-SAR Page 124 of 132

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland



Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

S

С

S

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

GI	0	S	S	a	ſ
TC	15				

TSLtissue simulating liquidConvFsensitivity in TSL / NORM x,y,zN/Anot applicable or not measured

#### Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

#### Additional Documentation:

e) DASY4/5 System Handbook

#### Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
  point exactly below the center marking of the flat phantom section, with the arms oriented
  parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
  positioned under the liquid filled phantom. The impedance stated is transformed from the
  measurement at the SMA connector to the feed point. The Return Loss ensures low
  reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2550V2-1010\_Jul15

Page 2 of 8



#### **Measurement Conditions**

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2550 MHz ± 1 MHz	

#### Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.1	1.91 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.5 ± 6 %	1.99 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

#### SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	14.7 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	57.2 W/kg ± 17.0 % (k=2)
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition 250 mW input power	6.67 W/kg

#### Body TSL parameters

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.6	2.09 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.1 ± 6 %	2.15 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

#### SAR result with Body TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.9 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	54.8 W/kg ± 17.0 % (k=2)
	condition	
SAR averaged over 10 cm <sup>3</sup> (10 g) of Body TSL	condition	
	condition 250 mW input power	6.32 W/kg

Certificate No: D2550V2-1010\_Jul15

Page 3 of 8



#### Appendix (Additional assessments outside the scope of SCS 0108)

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.8 Ω - 2.0 jΩ
Return Loss	- 29.5 dB

#### Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.0 Ω - 1.5 jΩ	
Return Loss	- 36.6 dB	

#### **General Antenna Parameters and Design**

1	Electrical Delay (one direction)	1.152 ns
	Electrical Delay (one direction)	1.102.110

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

#### **Additional EUT Data**

Manufactured by	SPEAG
Manufactured on	August 03, 2012

Certificate No: D2550V2-1010\_Jul15

Page 4 of 8



## No.B18N00005-SAR Page 127 of 132

#### **DASY5 Validation Report for Head TSL**

Date: 24.07.2015

Test Laboratory: SPEAG, Zurich, Switzerland

### DUT: Dipole 2550 MHz; Type: D2550V2; Serial: D2550V2 - SN: 1010


Communication System: UID 0 - CW; Frequency: 2550 MHz Medium parameters used: f = 2550 MHz;  $\sigma$  = 1.99 S/m;  $\varepsilon_r$  = 37.5;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.45, 4.45, 4.45); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

## Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 103.6 V/m; Power Drift = 0.01 dB Peak SAR (extrapolated) = 30.5 W/kg SAR(1 g) = 14.7 W/kg; SAR(10 g) = 6.67 W/kg Maximum value of SAR (measured) = 19.5 W/kg

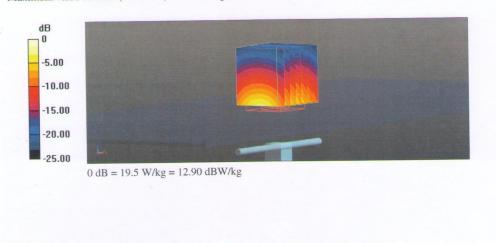

Certificate No: D2550V2-1010\_Jul15

Page 5 of 8



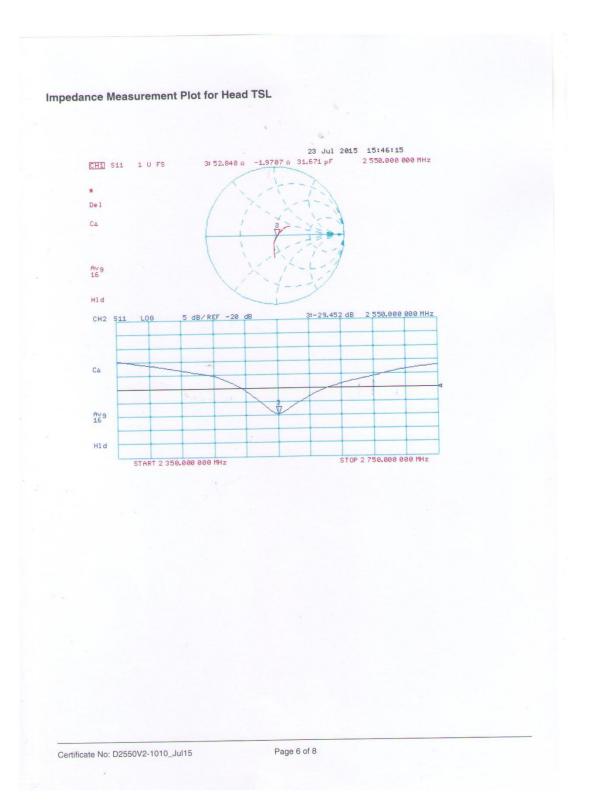



## No.B18N00005-SAR Page 129 of 132

#### DASY5 Validation Report for Body TSL

Date: 24.07.2015

Test Laboratory: SPEAG, Zurich, Switzerland

### DUT: Dipole 2550 MHz; Type: D2550V2; Serial: D2550V2 - SN: 1010


Communication System: UID 0 - CW; Frequency: 2550 MHz Medium parameters used: f = 2550 MHz;  $\sigma$  = 2.15 S/m;  $\epsilon_r$  = 52.1;  $\rho$  = 1000 kg/m<sup>3</sup> Phantom section: Flat Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 SN3205; ConvF(4.2, 4.2, 4.2); Calibrated: 30.12.2014;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 18.08.2014
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

## Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 96.75 V/m; Power Drift = 0.00 dB Peak SAR (extrapolated) = 28.7 W/kg SAR(1 g) = 13.9 W/kg; SAR(10 g) = 6.32 W/kg Maximum value of SAR (measured) = 18.5 W/kg

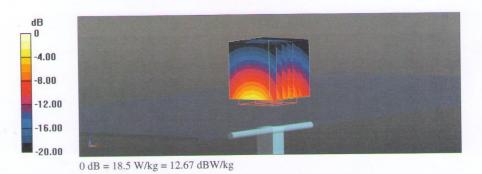

Certificate No: D2550V2-1010\_Jul15

Page 7 of 8



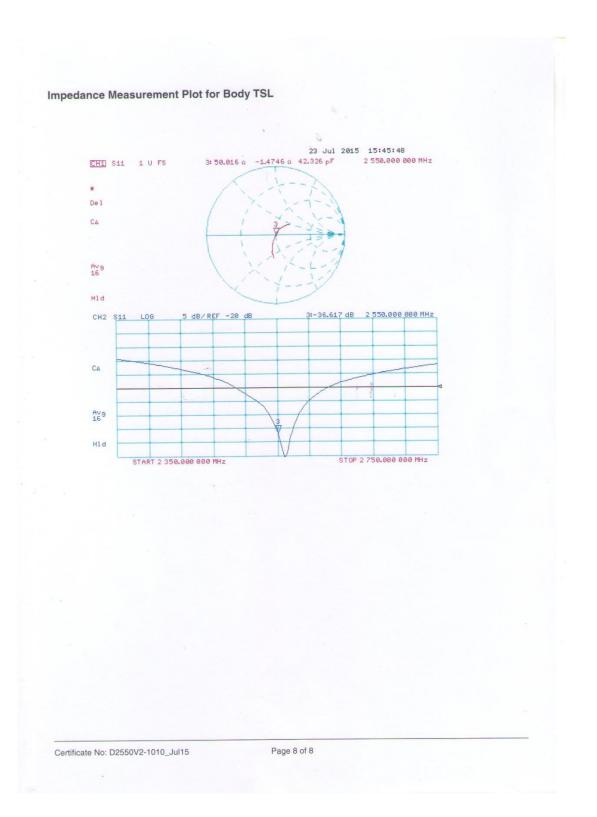



# ANNEX J SENSOR TRIGGERING DATA SUMMARY

Per FCC KDB Publication 616217 D04, this device was tested by the manufacturer to determine the proximity sensor triggering distances for all applicable sides and edges of the device. The measured output power at distances within  $\pm 5$  mm of the triggering points (or until touching the phantom) is included for back side and each applicable edge per Step i) in Section 6.2 of the KDB. The technical descriptions in the filing contain the complete set of triggering data required by Section 6 of FCC KDB Publication 616217 D04.

To ensure all production units are compliant, it is necessary to test SAR at a distance 1 mm less than the smallest distance between the device and SAR phantom (determined from the sensor triggering tests according to FCC KDB 616217 D04) with the device at the maximum output power (without power reduction). These SAR tests are included in addition to the SAR tests for the device touching the SAR phantom (at the reduced output power level).

The operational description contains information explaining how this device remains compliant in the event of a sensor malfunction.

-											
Distance(mm)	19	18	17	26	15	14	13	12	11	10	9
GSM1900	32.22	32.21	32.20	32.21	32.22	23.36	23.36	23.35	23.36	23.34	23.36
WCDMA Band2	22.81	22.79	22.81	22.80	22.81	19.70	19.70	19.69	19.70	19.68	19.70
LTE Band 7	22.84	22.84	22.83	22.84	22.85	19.02	19.02	19.01	19.02	19.00	19.02

### Rear Side (Main Antenna)

Moving device toward the phantom:

### Moving device away from the phantom:

Distance(mm)	19	18	17	26	15	14	13	12	11	10	9
GSM1900	32.21	32.22	32.20	32.22	32.22	23.35	23.36	23.34	23.35	23.34	23.36
WCDMA Band2	22.80	22.79	22.80	22.80	22.80	19.70	19.70	19.69	19.70	19.68	19.70
LTE Band 7	22.85	22.84	22.83	22.85	22.85	19.01	19.02	19.02	19.01	19.00	19.01

Based on the most conservative measured triggering distance of 14 mm, additional SAR measurements were required at 13 mm from the Rear side for the above modes.

### **Bottom Side (Main Antenna)**

Moving device toward the phantom:

Distance(mm)	17	16	15	14	13	12	11	10	9	8	7
GSM1900	32.22	32.21	32.20	32.22	32.22	23.36	23.35	23.36	23.36	23.35	23.36
WCDMA Band2	22.80	22.78	22.79	22.80	22.81	19.70	19.70	19.69	19.70	19.70	19.69
LTE Band 7	22.84	22.85	22.83	22.84	22.85	19.02	19.02	19.01	19.00	19.02	19.02



### Moving device away from the phantom:

Distance(mm)	17	16	15	14	13	12	11	10	9	8	7
GSM1900	32.20	32.21	32.21	32.22	32.22	23.35	23.34	23.36	23.36	23.35	23.36
WCDMA Band2	22.80	22.79	22.79	22.80	22.80	19.71	19.72	19.69	19.71	19.70	19.69
LTE Band 7	22.84	22.84	22.82	22.85	22.85	19.01	19.00	19.02	19.00	19.02	19.01

Based on the most conservative measured triggering distance of 12 mm, additional SAR measurements were required at 11 mm from the Bottom side for the above modes.