

Company Confidential

WR-1017.001



Number: 1819-01

1 (40)

08 June 2006 Accredited Laboratory Certificate

Ver 2.0

**FCC HAC Test Report** 

Test Report Number: WR-1017.001

Terminal device:

Type: Nokia RH-90, HW: 7000, SW: V R220\_03w24\_45\_34.nep (Detailed information is listed in section 5).

Originator: Anu Balijepalli Function: TCC – Dallas Version/Status: 2.0 Approved Location: TCC Directories Date: 08 June 2006

# **Change History:**

Version	Date	Status	Handled By	Comments
0.1	24 February 2006	Draft	Anu Balijepalli	Initial Draft
0.2	24 February 2006	Review	Anu Balijepalli	Submit for Approval
1.0	24 February 2006	Approved	Nerina Walton	Approved
1.1	08 June 2006	New version	Anu Balijepalli	Submit for Approval
2.0	08 June 2006	Approved	Nerina Walton	Approved

**Testing laboratory:** Test & Certification Center (TCC)

Dallas Nokia Inc

6021 Connection Drive Irving, Texas 75039

U.S.A.

Tel. 972-894-5000 Fax. 972-894-4988 Client: Nokia, Inc.

12278 Scripps Summit Dr. San Diego, CA 92131 Tel. +1 858 831 5000 Fax +1 858 831 6500

Date and signatures:

For the Contents:

08 June 2006

Anu Balijepalli, Technical Review

Ameadha

Nerina Walton, Manager Review

FCC HAC Test Report

© 2006 Nokia Mobile Phones

ACCREDITED

2 (40)

Test & Certification Center (TCC) - Dallas

WR-1017.001

08 June 2006

Accredited Laboratory Certificate Number: 1819-01 Ver 2.0

# **TABLE OF CONTENTS**

1.	GENERAL	3
1.1		
1.2		
2.	LIST OF ABBREVIATIONS, ACRONYMS AND TERMS	4
2.1		
2.2 2.3		
3.	STANDARDS BASIS	5
4.	TEST EQUIPMENT LIST	5
5.	EQUIPMENT-UNDER-TEST (EUT)	6
5.1		
5.2	2 PHOTOGRAPH OF TESTED DEVICE(S):	6
6.	TEST METHOD(S) AND SETUP(S)	7
6.1	1 PROBE DESCRIPTION	7
6.2		
6.3		
7.	PASS/FAIL CRITERIA	15
8.	TEST PROCEDURE	16
9.	SYSTEM VALIDATION	17
10.	DETAILED TEST RESULTS	27
10	0.1 NEAR FIELD E AND H RF EMISSIONS MEASUREMENTS	27
	10.1.1 Test Results	
11.	MEASUREMENT UNCERTAINTY	29
APPI	PENDIX A: VALIDATIONS SCANS	30
APPI	PENDIX B: MEASUREMENT SCANS	33
APPI	PENDIX C: PROBE CALIBRATION REPORTS AND DIPOLE CALIBRATION REPOR	TS 40

© No part of this report shall be reproduced out of the context of the report without the written approval of Nokia Mobile Phones, Inc., Dallas Product Creation, TCC – Dallas.



Company Confidential

WR-1017.001

08 June 2006



3 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

# 1. GENERAL

# 1.1 Objective

This test is performed to ensure that the EUT meets the requirements required by the FCC Method of Measurement for near field E and H emissions. Please note that this report is only for near field emissions, not for the T-coil HAC testing.

# 1.2 Test Summary

**Test Results:** The test result relates only to those tested devices mentioned in Section 5 of this test report.

Sample #	Test Performed	Reference	Category
1	Near Field Emissions- E field Near Field Emissions- H field	ANSI C63.19	МЗ



**Company Confidential** 

WR-1017.001

08 June 2006



4 (40)

Ver 2.0 Accredited Laboratory Certificate

Accredited Laboratory Certifica Number: 1819-01

# 2. LIST OF ABBREVIATIONS, ACRONYMS AND TERMS

#### 2.1 Abbreviations

dB - decibel

dBm - decibels per milliwatt (absolute measurement)

MHz - megahertz or 1000000 Hertz

V/m – Volts per meter

A/m – Amps per meter

# 2.2 Acronyms

AMPS - Advanced Mobile Phone System

BSS - Base Station Simulator

CDMA - Code Division Multiple Access

ESN - Electronic Serial Number

**EUT - Equipment under Test** 

GSM - Global System for Mobile communications

IMEI - International Mobile Equipment Identity

PCS - Personal Communication System

RF- Radio Frequency

TDMA - Time Division Multiple Access

#### 2.3 Terms

Base Station Simulator (BSS) - simulates all the necessary signals that a phone would experience while on a live network. There are many types of base station simulators catering for all current protocols, i.e., GSM, AMPS, TDMA, and CDMA.

Cellular - refers to a frequency in the 800MHz band.

PCS - refers to a frequency in the 1900MHz band.

Crest Factor - is the relation between the peak power and the average power in a signal.



WR

Company Confidential



5 (40)

WR-1017.001

08 June 2006

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

# 3. STANDARDS BASIS

Test & Certification Center (TCC) - Dallas

#### Testing has been carried out in accordance with:

REF.	Code of the standard	Name of the standard	
1	-	ANSI C63.19	

Note: Unless otherwise stated, (by reference to a version number and a publication date), the latest version of the above documents applies.

Deviations:

Not Applicable.

#### 4. TEST EQUIPMENT LIST

The listing below indicates the test equipment utilized for the test (s). Calibration interval on all items listed can be obtained from the Engineering Services Group within NMP, Product Creation - Dallas. Where relevant, measuring equipment is subjected to in-service checks between testing. TCC - Dallas shall notify clients promptly, in writing, of identification of defective measuring equipment that casts doubt on the validity of results given in this report.

Test Equipment	NMP#	Calibration Interval	Calibratrion Expiry
SPEAG DASY4 Robot System	2056	NA	NA
SPEAG Data Acquisition Electronics (DAE)	2108	12 months	May - 2006
SPEAG E-field Probe ER3DV6	4036	12 months	Feb- 2006
SPEAG H-field Probe H3DV6	4037	12 months	Feb-2006
SPEAG 1880MHz Dipole CD1880V3	4049	12 months	Jun-2006
Signal Generator HP8648C	0796	12 months	Aug-2006
Boonton Powermeter 4232A	2996	12 months	Sep-2006
AR Power Amplifier 5S1G4	0188	NA	NA
R&S CMU 200	4064	12 months	Feb-2007
R&S FSP	3462	12 months	Jul-2006



**Company Confidential** 

WR-1017.001

08 June 2006



6 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

# 5. EQUIPMENT-UNDER-TEST (EUT)

The results in this report relate only to the items listed below:

# 5.1 Description of Tested Device(s):

Sample #	Mode of Operation	Date of Receipt	Condition of Sample	ltem	Identifying Information
					Type: RH-90
					Model: 2127i
1	CDMA 1900	2/20/06	Good	Phone	ESN: 02604483371
					HW: 7000
					SW: V R220_03w24_45_34.nep
					Code: 0532694AN23BR

# 5.2 Photograph of Tested Device(s):



Company Confidential

WR-1017.001

08 June 2006



7 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

# 6. TEST METHOD(S) AND SETUP(S)

Test & Certification Center (TCC) - Dallas

Testing was performed in accordance with ANSI C63.19.

#### 6.1 Probe Description

#### **E field Probe Description**

#### Construction

One dipole parallel, two dipoles normal to probe axis

Built-in shielding against static charges

#### Calibration

In air from 100 MHz to 3.0 GHz (absolute accuracy ±6.0%, k=2)

#### Frequency

100 MHz to > 6 GHz; Linearity: ± 0.2 dB (100 MHz to 3 GHz)

#### Directivity

± 0.2 dB in air (rotation around probe axis) ± 0.4 dB in air (rotation normal to probe axis)

#### **Dynamic Range**

2 V/m to > 1000 V/m; Linearity:  $\pm$  0.2 dB

#### **Dimensions**

Overall length: 330 mm (Tip: 16 mm) Tip diameter: 8 mm (Body: 12 mm)

Distance from probe tip to dipole centers: 2.5 mm

#### **Application**

General near-field measurements up to 6 GHz

Field component measurements Fast automatic scanning in phantoms

### **H field Probe Description**

#### Construction

Three concentric loop sensors with 3.8 mm loop diameters Resistively loaded detector diodes for linear response Built-in shielding against static charges

#### Frequency

200 MHz to 3 GHz (absolute accuracy ± 6.0%, k=2); Output linearized

#### **Directivity**

± 0.25 dB (spherical isotropy error)

# **Dynamic Range**

10 mA/m to 2 A/m at 1 GHz

#### E-Field Interference

< 10% at 3 GHz (for plane wave)

# **Dimensions**

Overall length: 330 mm (Tip: 40 mm) Tip diameter: 6 mm (Body: 12 mm)

Distance from probe tip to dipole centers: 3 mm

# Application

General magnetic near-field measurements up to 3 GHz





Company Confidential

WR-1017.001

08 June 2006



8 (40)

Ver 2.0


Accredited Laboratory Certificate Number: 1819-01

Field component measurements
Surface current measurements
Measurements in air or liquids
Low interaction with the measured field

#### **Probe Tip Description**

HAC field measurements take place in the close near field with high gradients. Increasing the measuring distance from the source will generally decrease the measured field values. Magnetic field sensors are measuring the integral of the H-field across their sensor area surrounded by the loop. They are calibrated in precise, homogenous field. When measuring a gradient field, the result will be very close to the field in the center of the loop, which is equivalent to the center value. But it will be different from the field at the border of the loop.

Consequently, two sensors with different loop diameters – both calibrated ideally – would give different results when measuring from the edge of the probe sensor elements. The behaviour for electrically small E-field sensors is equivalent. See below for distance plots from a WD, which show the conservative nature of field readings at the probe element center vs. measurements at the sensor end.

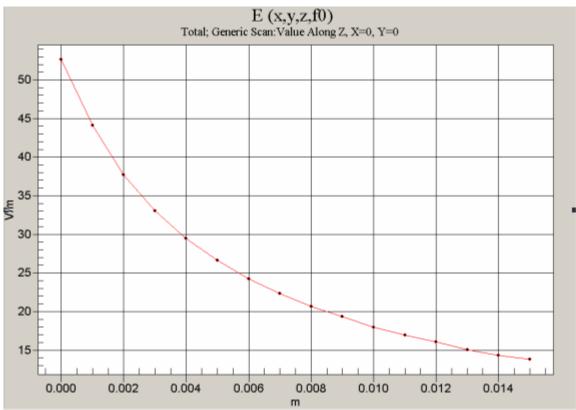

The magnetic field loops of the H3D probes are concentric, with the center 3mm from the tip for H3DV6. Their radius is 1.9mm.

The electric field probes have a more irregular intenal geometry because it is physically not possible to have the 3 orthogonal sensors situated with the same center. The effect of the different sensor centers is accounted for in the HAC uncertainty budget. Their geometric center is at 2.5mm from the tip, and the element ends are 1.1mm closer to the tip.



Company Confidential

WR-1017.001

08 June 2006





9 (40)


Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

#### Connector Plan







The antistatic shielding inside the probe is connected to the probe connector case. It is recommended to connect the probes with the amplifier using a short and well-shielded cable and to connect the cable shielding with the connector case.

Instrumentation Chain:

Conversion of Connector Voltage to E field

$$E_{i} = \sqrt{\frac{u_{i} + (u_{i}^{2}.CF)/(DCP)}{Norm_{i}.ConvF}}$$

whereby

 $E_i$  = Electric field in V/m

 $u_i$  = Voltage of channel i at the connector in  $\mu$  V

*Norm*<sub>i</sub> = Sensitivity of channel in  $\mu V/(V/m)^2$ 

ConvF = enhancement factor in liquid (ConvF = 1 for Air)

DCP = Diode compression point in  $\mu$  V

CF = Signal Crest Factor (peak power/average power)

#### **Probe Response to Frequency**

The E-field sensors have inherently a very flat frequency response. They are calibrated with a number of frequencies resulting in a common calibration factor, with the frequency behaviour documented in the calibration certificate.

WR-1017.001

08 June 2006




10 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

# Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide R22)

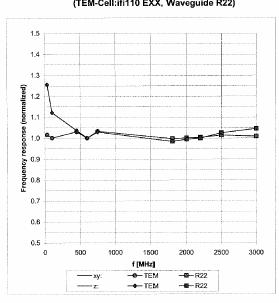


Uncertainty of Frequency Response of E-field:  $\pm$  6.3% (k=2)

H-fileld sensors have frequency dependant sensitivity, which is evaluated for a series of frequencies also visible in the probe calibration certificate. The calibration factors result from a fiiting algorithm. The proper conversion is calculated by the DASY4 software depending on the frequency setting in the procedure.

### Frequency Response of H-Field

(TEM-Cell:ifi110, Waveguide R22)



Uncertainty of Frequency Response of E-field:  $\pm$  6.3% (k=2)



Company Confidential

WR-1017.001

08 June 2006



11 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

#### **Conversion to Peak**

Peak is defined as Peak Envelope Power. All raw measurements from the HAC measurement system are RMS values. The DASY4 system incorporates the crest factor of the signal in the computation of the RMS values. Although the software also has capability to estimate the peak field by applying a square root of crest factor value to the readings, the probe modulation factor was applied manually instead per PC63.19 in the measurement tables in this report. The equation to convert the raw measurements in the data tables are:

Peak Field = 20 log (Raw x PMF)

Where:

Peak Field = Peak field (in dBV/m or dBA/m)

Raw = Raw field measurement from the measurement system (in V/m or A/m).

PMF = Probe Modualtion Factor (in linear units).

Company Confidential

WR-1017.001

08 June 2006



12 (40)


Ver 2.0

Accredited Laboratory Certificate
Number: 1819-01

### 6.2 Speag Robotic System

E-field and H-field measurements are performed using the DASY4 automated dosimetric assessment system. The DASY4 is made by Schmid & Partner Engineering AG (SPEAG) and consists of high precision robotics system (Staubli), robot controller, Pentium 4 computer, near-field probe, probe alignment sensor, and the HAC phantom. The robot is a six- axis industrial robot performing precise movements to the position the probe to the location of maximum EMF.

#### **System Hardware**

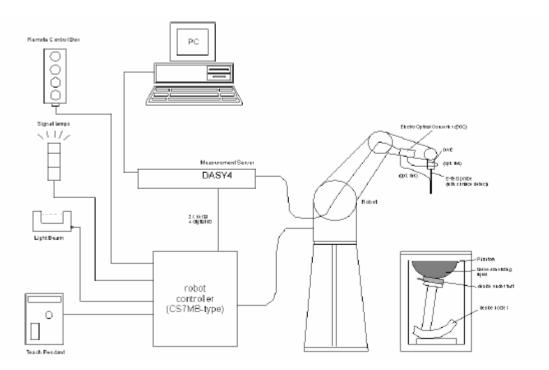

A cell controller system contains the power supply, robot controller; teach pendant, and a remote control used to drive the robot motors. The PC consists of RF meaurement system DASY4 V4.5 with HAC extension, A/D interface card, monitor, mouse and keyboard. The Staubli Robot is connected to the cell controller to allow software manipulation of the robot. A data acquisition electronic (DAE) circuit that performs the signal amplification, signal multiplexing, AD conversion, offset measurements, mechanical surface detection, collision detection, etc is connected to the Electro – optical coupler (EOC). The EOC performs the conversion from the optical into digital electric signal of the DAE and transfers data to the PC plug-in card.

The DAE consists of a highly sensitive electrometer – grade preamplifier with auto-zeroing, a channel and gain switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the PC-card is accomplished through an optical downlink for data and status information and an optical uplink for commands and clock lines. The mechanical probe-mounting device includes two different sensor systems for frontal and sidewise probe contacts. They are also used for mechanical surface detection and probe collision detection. The robot uses its own controller with a built- in VME-bus computer.

Company Confidential

WR-1017.001

08 June 2006



13 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

#### **Data Evaluation**

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power. The formula for each channel can be given as:

$$V_i = U_i + U_2 * (cf/dcpi)$$

with  $V_i$  = compensated signal of channel i (i = x, y, z)

 $U_i$  = input signal of channel i (i = x, y, z)

cf = crest factor of exciting field (DASY parameter)

dcpi = diode compression point (DASY parameter)

From the compensated input signals the primary field data for each channel can be evaluated:

E-field probes: 
$$E_i = \sqrt{\frac{V_i}{Norm_i x ConvF}}$$

H-field probes: 
$$H_i = \sqrt{V_i} x \frac{a_{io} + a_{i1} f + a_{i2} f^2}{f}$$

with  $V_i$  = compensated signal of channel i (i = x, y, z) Norm<sub>i</sub> = sensor sensitivity of channel i (i = x, y, z)  $\mu V/(V/m)_2$  for E-field Probes ConvF = sensitivity enhancement in solution  $a_{ij}$  = sensor sensitivity factors for H-field probes f = carrier frequency [GHz]

E<sub>i</sub> = electric field strength of channel i in V/m H<sub>i</sub> = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The signal response time is evaluated as the time required by the system to reach 90% of the expected final value after an on/off switch of the power source with an integration time of 500 ms and a probe response time of <5ms. In the current implementation, DASY4 waits longer than 100 ms after having reached the grid point before starting a measurement, i.e., the response time uncertainty is negligible.

If the device under test does not emit a CW signal, the integration time applied to measure the electric field at a specific point may introduce additional uncertainties due to the discretization. The tolerances for the different systems had the worst-case of 2.6%.

**Company Confidential** 

WR-1017.001

08 June 2006




14 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

# 6.3 Test Setup

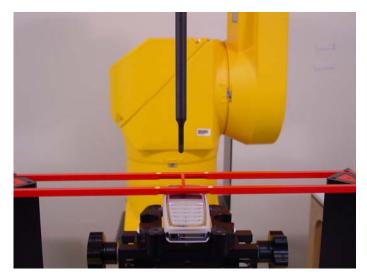





**Company Confidential** 

WR-1017.001

08 June 2006



15 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

# 7. PASS/FAIL CRITERIA

The EUT must meet the following M3 category standards –

Category	Wireless Device Parameters				
Near field	AWF E-field Emissions		H-field Emissions		
		Peak – V/m	Peak – A/m		
Category M3	AWF =0 (TDMA, CDMA)	63.1 to 112.2	0.19 to 0.34		
	AWF = -5 (GSM)	47.3 to 84.1	0.15 to 0.25		
Category M4	AWF =0 (TDMA, CDMA)	< 63.1	< 0.19		
3.7	AWF = -5 (GSM)	< 47.3	< 0.15		



Company Confidential

WR-1017.001

08 June 2006



16 (40)


Ver 2.0

Accredited Laboratory Certificate
Number: 1819-01

### 8. TEST PROCEDURE

The following illustrates a typical RF emissions test scan over a wireless communication device:

- Proper operation of the field probe, probe measurement system, other instrumentation, and the positioning system was confirmed.
- WD is positioned in its intended test position, acoustic output point of the device perpendicular to the field probe.
- The WD operation for maximum rated RF output power was configured and confirmed with the base station simulator, at the test channel and other normal operating parameters as intended for the test. The battery was ensured to be fully charged before each test.
- The center sub-grid was centered over the center of the acoustic output (also audio band magnetic output, if applicable). The WD audio outout was positioned tangent (as physically possible) to the measurement plane.
- A surface calibration was performed before each setup change to ensure repeatable spacing and proper maintenance of the measurement plane using the HAC Phantom.
- The measurement system measured the field strength at the reference location.
- Measurements at 2mm increments in the 5x5 cm region were performed and recorded. A 360 deg rotation about the azimuth axis at the maximum interpolated position was measured. For the worst case condition, the peak reading from this rotation was used in re-evaluating the HAC category.
- The system performed a drift evaluation by measuring the field at the reference location.
- Same steps were done for both the E and H field measurements.

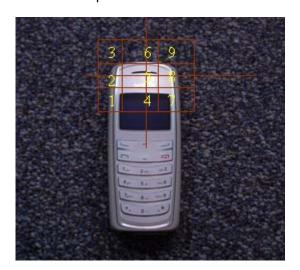

Company Confidential

WR-1017.001

08 June 2006



17 (40)

Ver 2.0

Accredited Laboratory Certificate
Number: 1819-01


#### 9. SYSTEM VALIDATION

The input signal was an unmodulated continous wave. The following points were taken into consideration in performing the system validation:

Average Input Power = 100mW (20dBm RMS) after adjustment for return loss.

The test fixture must meet the 2-wavelength separation criterion.

The proper measurement of the 1cm probe to dipole separation, which is measured from the top surface of the dipole to the calibration reference point of the sensor, defined by the probe manufacturer is shown in the following picture:

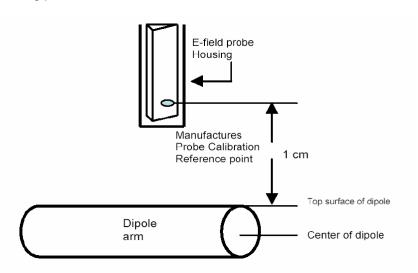

To assure proper operation of the near-field measurement probe the input power to the dipole shall be commensurate to with the full rated output power of the wireless device (eg. – for a cellular phone wireless device the average peak antenna input power will be on the order of 100mW (ie, 20dBm) RMS after adjustment for any mismatch.

A dipole antenna meeting the requirements in PC63.19 was placed in the position normally occupied by the WD. The length of the dipole was scanned with both E-field and H-field probes and the maximum values for each were recoreded.

Using the near-field measurement system, scan the antenna over the radiating dipole and record the greatest field reading observed. Due to the nature of E-fields about freespace dipoles, the two E-field peaks measured over the dipole are averaged to compensate for non-paralellity of the setup, See manufacturer method on dipole calibration certificates, page 2. Field strength measurements shall be made only when the probe is stationary.

Company Confidential

WR-1017.001


08 June 2006



18 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

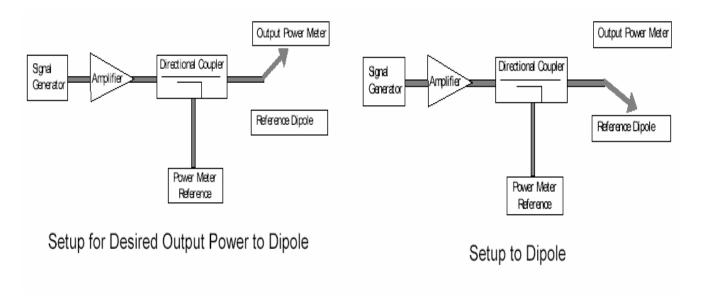


Using this setup configuration, the signal generator was adjusted for the desired output power (100mW) at a specified frequency. The reference power from the coupled port of the directional coupler is recorded. Next, the output cable is connected to the reference dipole, as shown in the figure above.

The input signal was adjusted until the reference power from the coupled port of the directional coupler was the same as previously recorded, to compensate for the impendance mismatch between the output cable and the reference dipole.

To assure proper operation of the near-field measurement probe the input power to the reference dipole was verified to the full rated output power of the wireless device. The dipole was secured in a holder in a manner to meet the 20dB reflection. The near-field measurement probe was postioned over the dipole.

The antenna was scanned over the appropriate sized area to cover the dipole from end to end. SPEAG uses 2D interpolation algorithms between the measured points. Please see below two-dimensional plots showing that the interpolated values interpolate smoothly between 5mm steps for a free space RF dipole:

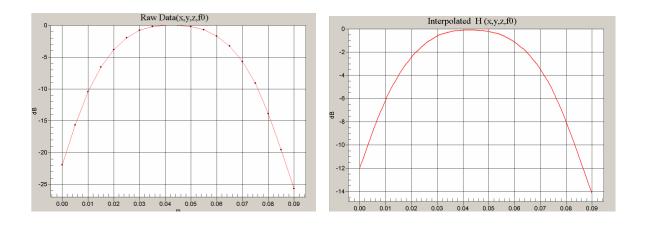



**Company Confidential** 

ACCREDITED

19 (40)

Test & Certification Center (TCC) - Dallas

WR-1017.001

08 June 2006

Accredited Laboratory Certificate Number: 1819-01 Ver 2.0

Validations were performed for CW at 20dBm peak power.

		Recorded	Target Value	% deviation
	E field	126.1	137.6	8.36%
1880 MHz	H field	0.486	0.452	7.52%

Note: Please see Appendix A for the Validation Scans



Company Confidential

WR-1017.001

08 June 2006



20 (40)

Ver 2.0

Accredited Laboratory Certificate
Number: 1819-01

#### **MODULATION FACTOR**

A calibration was made of the modulation response of the probe and its instrumentation chain. This calibration was performed with the field probe, attached to its instrumentation. The response of the probe system to a CW field at the frequency of interest is compared to its response to a modulated signal with equal peak amplitude to that of a CW signal. The field level of the test signals are ensured to be more than 10dB above the ambient level and the noise floor of the instrumentation being used. The ratio of the CW reading to that taken with a modulated reading was applied to the DUT measurements.

This was done using the following procedure:

- The probe was illuminated with a CW signal at the intended measurement frequency.
- The probe was positioned at the field maxima over the dipole antenna (determined afer an area scan over the dipole).
- The reading of the probe measurement system of the CW signal at the maximum point was recorded.
- Using a Spectrum Analyzer, the modulated signal adjusted with the same peak level of the CW signal was determined.
- The probe measurement system reading was recorded with the modulated signal.
- The ratio of the CW reading to the modulated signal reading is the probe modulation factor (PMF) for the modulation and field probe combination.
- Same steps are repeated at all frequency bands and for both E and H field probes.

The modulation factors obtained were applied to readings taken of the actual wireless device, in order to obtain an accurate peak field reading using the formula:

 $Peak = 20log(Raw \times PMF)$ 

This method correlates well with the modulation using the DUT in the alternative substitution method. See below for correlation of signal:



Company Confidential

ACCREDITED

Ver 2.0

21 (40)

08 June 2006


WR-1017.001

Accredited Laboratory Certificate Number: 1819-01

# Signal Generator Modulated Signal:



# Wireless Device Modulated Signal:

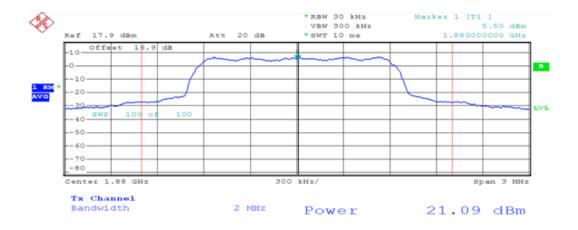

WR-1017.001

08 June 2006




22 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

Modulation Factors were performed for CW, 80%AM and the modulated signal at 20dBm peak power, See below for the picture as well as the Spectrum Analyzer Plots.

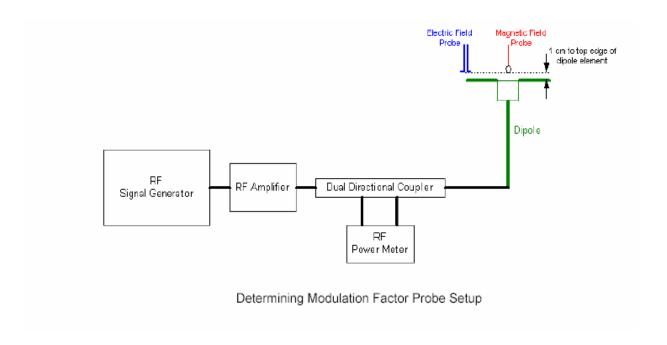



**Company Confidential** 

ACCREDITED

23 (40)


Test & Certification Center (TCC) - Dallas

WR-1017.001

08 June 2006

Accredited Laboratory Certificate Number: 1819-01 Ver 2.0

# CDMA Signal at 1880MHz:

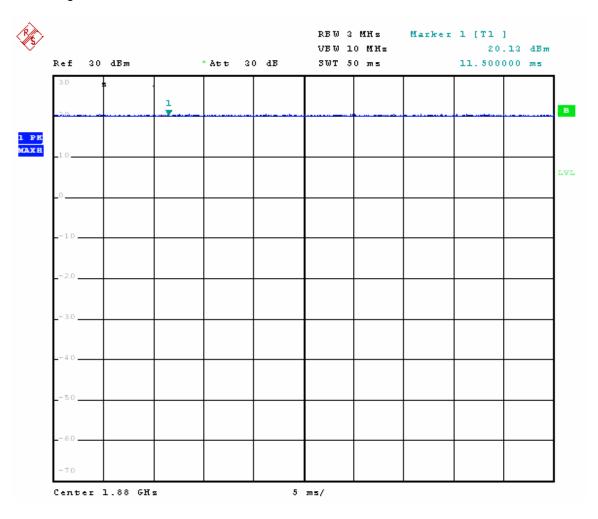





24 (40)

Test & Certification Center (TCC) - Dallas


WR-1017.001

**Company Confidential** 

08 June 2006

Accredited Laboratory Certificate Number: 1819-01 Ver 2.0

# CW Signal at 1880MHz:

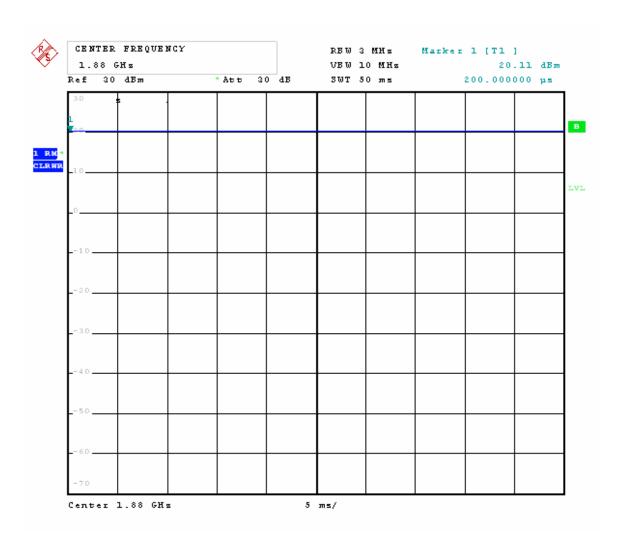



**Company Confidential** 

ACCREDITED

25 (40)


Test & Certification Center (TCC) - Dallas

WR-1017.001

08 June 2006

Accredited Laboratory Certificate Number: 1819-01 Ver 2.0

# 80%AM Signal at 1880MHz:

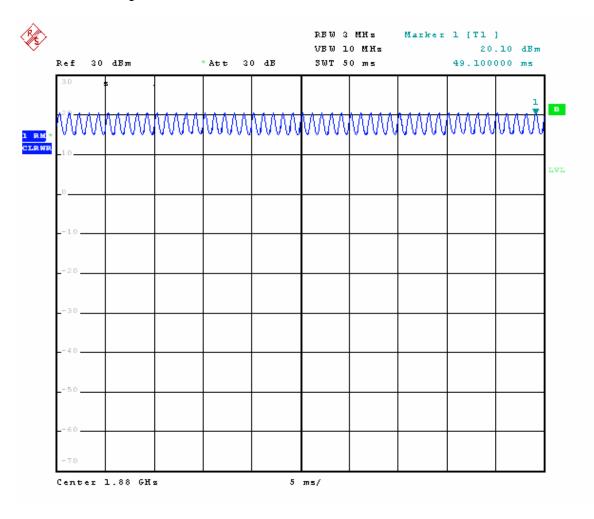



**Company Confidential** 

WR-1017.001

08 June 2006



26 (40)

Accredited Laboratory Certificate
Number: 1819-01

Ver 2.0

1880 MHz	E-Field	H-Field	Modulation Factor (MF) for	Modulation Factor (MF) for
	(V/m)	(A/m)	E-field	H-field
CDMA	118.3	0.57	1.0	0.7
CW	115.0	0.38		
80%AM	71.5	0.24		



**Company Confidential** 

ACCREDITED

27 (40)

Test & Certification Center (TCC) - Dallas

WR-1017.001

08 June 2006

Accredited Laboratory Certificate Number: 1819-01 Ver 2.0

# 10. DETAILED TEST RESULTS

Test Technician / Engineer	Bob Alexander, Michael Sundstrom		
Date of Measurement	February 21-22, 2006		
Temperature / Humidity / Pressure	ure / Humidity / Pressure 20-22°C 36-44%R		
Test Result Complies			

# 10.1 Near Field E and H RF emissions measurements

# 10.1.1 Test Results

#### **CDMA PCS E - FIELD**

CDMA PCS	Conducted Power (dBm)	Power Drift (dB)	E (V/m)	Modulation Factor	Excluded Blocks
Ch 25	23.6	-0.025	74.0	1.0	4,7,8
Ch 600	23.4	0.199	67.9	1.0	4,7,8
Ch 1175	23.2	-0.192	58.8	1.0	1,4,7

# **CDMA PCS H - FIELD**

CDMA PCS	Conducted Power (dBm)	Power Drift (dB)	H (A/m)	Modulation Factor	Excluded Blocks
Ch 25	23.6	-0.096	0.141	0.7	6,8,9
Ch 600	23.4	0.229	0.136	0.7	6,8,9
Ch 1175	23.2	-0.056	0.128	0.7	6,8,9



**Company Confidential** 

ACCREDITED

28 (40)

Ver 2.0

Test & Certification Center (TCC) - Dallas

WR-1017.001


08 June 2006

Accredited Laboratory Certificate Number: 1819-01

#### **WORST CASE CONFIGURATION**

CDMA PCS	E (V/m)	Modulation Factor	FCC M3 Limits (V/m)	Category
Ch 25	75.2	1.0	63.1 to 112.2	M3

The probe rotation was done at the sub grid 5 for Channel 25, E field.

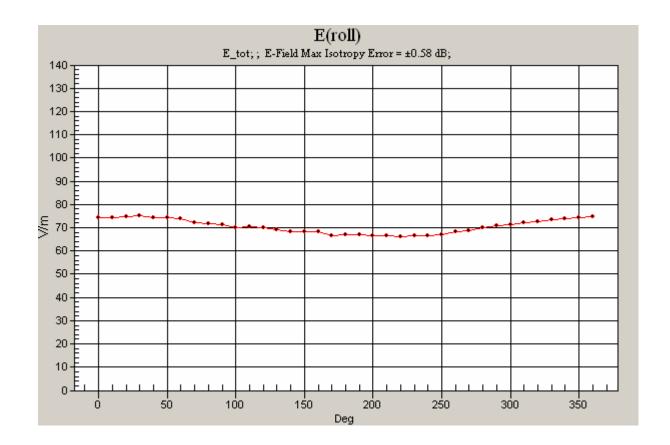

ACCREDITED

29 (40)

Test & Certification Center (TCC) - Dallas

WR-1017.001

08 June 2006

Accredited Laboratory Certificate Number: 1819-01 Ver 2.0

# 11. MEASUREMENT UNCERTAINTY

HAC Uncertainty	Budget	1							
Error Description	Uncertainty value	Prob. Dist.	Div.	(ci) E	(ci) H	Std. Unc. E	Std. Unc. H	Squared E	Squared H
Measurement System									
Probe Calibration	5.1	N	1	1	1	5.1	5.1	26.0	26.0
Axial Isotropy	4.7	R	1.7321	1	1	2.7	2.7	7.4	7.4
Sensor Displacement	16.5	R	1.7321	1	0.145	9.5	1.4	90.7	1.9
Boundary Effects	2.4	R	1.7321	1	1	1.4	1.4	1.9	1.9
Linearity	4.7	R	1.7321	1	1	2.7	2.7	7.4	7.4
Scaling to Peak Envelope Power	2	R	1.7321	1	1	1.2	1.2	1.3	1.3
System Detection Limit	1	R	1.7321	1	1	0.6	0.6	0.3	0.3
Readout Electronics	0.3	N	1	1	1	0.3	0.3	0.1	0.1
Response Time	0.8	R	1.7321	1	1	0.5	0.5	0.2	0.2
Integration Time	2.6	R	1.7321	1	1	1.5	1.5	2.3	2.3
RF Ambient Conditions	3	R	1.7321	1	1	1.7	1.7	3.0	3.0
RF Reflections	12	R	1.7321	1	1	6.9	6.9	48.0	48.0
Probe Positioner	1.2	R	1.7321	1	0.67	0.7	0.5	0.5	0.2
Probe Positioning	4.7	R	1.7321	1	0.67	2.7	1.8	7.4	3.3
Extrap. And Interpolation	1	R	1.7321	1	1	0.6	0.6	0.3	0.3
Test Sample Related								0.0	0.0
Device Positioning Vertical	10	R	1.7321	1	0.67	2.7	1.8	7.4	3.3
Device Positioning Lateral	10	R	1.7321	1	1	0.6	0.6	0.3	0.3
Device Holder	2.4	R	1.7321	1	1	1.4	1.4	1.9	1.9
Power Drift	5	R	1.7321	1	1	2.9	2.9	8.3	8.3
Phantom and Setup Related								0.0	0.0
Phantom Thickness	2.4	R	1.7321	1	0.67	1.4	0.9	1.9	0.9
Combined Std. Ur	ncertainty							16.6	12.8
Expanded Std. Uncerta (k=2)	ainty on Field							33.2%	21.8%

**TCC** 

Test & Certification Center (TCC) - Dallas

**APPENDIX A: VALIDATIONS SCANS** 

**Company Confidential** 

WR-1017.001

08 June 2006



30 (40)

Ver 2.0

Accredited Laboratory Certificate

Number: 1819-01



Company Confidential

WR-1017.001

08 June 2006



31 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

Accredited Laboratory Number: 1819-

Date/Time: 2/20/2006 12:34:31 PM Test Laboratory: TCC Dallas

# 1880MHz, E field, CW Validation

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1

DASY4 Configuration:

- Probe: ER3DV6 - SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005

- Sensor-Surface: (Fix Surface)

- Electronics: DAE3 Sn377; Calibrated: 5/12/2005

- Phantom: HAC Test Arch 4.6; Phantom section: E Dipole Section

- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 160

# E Scan - ER probe center 10mm above CD1880 Dipole/Hearing Aid Compatibility Test

(41x181x1): Measurement grid: dx=5mm, dy=5mm

Maximum value of peak Total field = 122.5 V/m


Probe Modulation Factor = 1.00

Reference Value = 131.8 V/m; Power Drift = -0.013 dB

Hearing Aid Near-Field Category: M2 (AWF 0 dB)

#### Peak E-field in V/m

Grid 1	Grid 2	Grid 3
120.4	122.5	118.3
Grid 4	Grid 5	Grid 6
84.1	86.3	83.9
	<b>86.3</b> Grid 8	

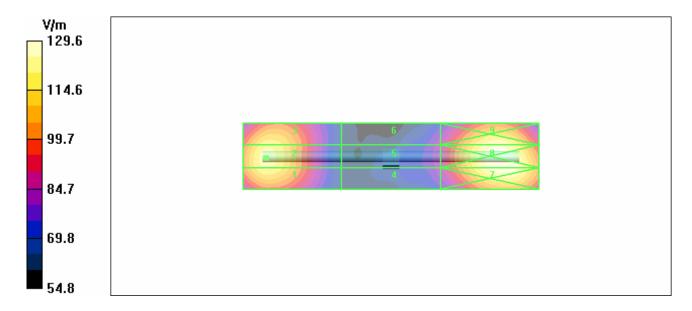



Company Confidential

WR-1017.001

08 June 2006



32 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 2/20/2006 10:13:16 AM Test Laboratory: TCC Dallas

# 1880MHz, H field, CW Validation

Communication System: CW; Frequency: 1800 MHz; Duty Cycle: 1:1

DASY4 Configuration:

- Probe: H3DV6 - SN6155; ; Calibrated: 2/16/2005

- Sensor-Surface: (Fix Surface)

- Electronics: DAE3 Sn377; Calibrated: 5/12/2005

- Phantom: HAC Test Arch 4.6; Phantom section: H Device Section

- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 160

# H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility

**Test (251x251x1):** Measurement grid: dx=2mm, dy=2mm

Maximum value of peak Total field = 0.486 A/m


Probe Modulation Factor = 1.00

Reference Value = 0.475 A/m; Power Drift = -0.044 dB

Hearing Aid Near-Field Category: M2 (AWF 0 dB)

#### Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.372	0.478	0.399
Grid 4	Grid 5	Grid 6
0.384	0.486	0.408
Grid 7	Grid 8	Grid 9
0.376	0.477	0.400

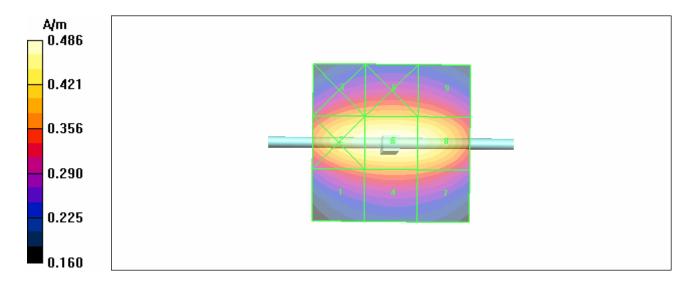

**TCC** 

Test & Certification Center (TCC) - Dallas

**Company Confidential** 

WR-1017.001

08 June 2006



33 (40)

Accredited Laboratory Certificate Number: 1819-01 Ver 2.0

# **APPENDIX B: MEASUREMENT SCANS**



Company Confidential

WR-1017.001

08 June 2006



34 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 2/22/2006 10:06:32 AM Test Laboratory: TCC Dallas

RH-90, CDMA1900, Ch25, E field

Communication System: CDMA1900; Frequency: 1851.25 MHz; Duty Cycle: 1:1

DASY4 Configuration:

- Probe: ER3DV6 - SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005

- Sensor-Surface: (Fix Surface)

- Electronics: DAE3 Sn377; Calibrated: 5/12/2005

- Phantom: HAC Test Arch 4.6; Phantom section: E Device Section

- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 160

# E Scan - ER probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(251x251x1): Measurement grid: dx=2mm, dy=2mm

Maximum value of peak Total field = 74.0 V/m


Probe Modulation Factor = 1.00

Reference Value = 73.7 V/m; Power Drift = -0.025 dB

Hearing Aid Near-Field Category: M3 (AWF 0 dB)

#### Peak E-field in V/m

Grid 1		
65.5	64.9	58.9
Grid 4	Grid 5	Grid 6
72.1	74.0	66.0
		• • •
	Grid 8	

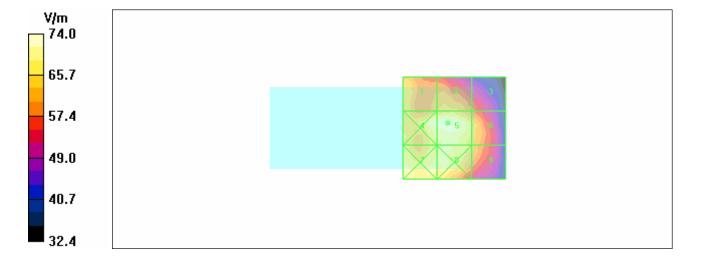



Company Confidential

WR-1017.001

08 June 2006



35 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 2/22/2006 12:21:08 PM Test Laboratory: TCC Dallas

#### RH-90, CDMA1900, Ch600, E field

Communication System: CDMA1900; Frequency: 1880 MHz; Duty Cycle: 1:1

DASY4 Configuration:

- Probe: ER3DV6 - SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005

- Sensor-Surface: (Fix Surface)

- Electronics: DAE3 Sn377; Calibrated: 5/12/2005

- Phantom: HAC Test Arch 4.6; Phantom section: E Device Section

- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 160

# E Scan - ER probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(251x251x1): Measurement grid: dx=2mm, dy=2mm

Maximum value of peak Total field = 67.9 V/m


Probe Modulation Factor = 1.00

Reference Value = 64.5 V/m; Power Drift = 0.199 dB

Hearing Aid Near-Field Category: M3 (AWF 0 dB)

#### Peak E-field in V/m

Grid 1	Grid 2	Grid 3
64.6	59.4	54.0
Grid 4	Grid 5	Grid 6
67.2	67.9	60.2
	•	• • •
	Grid 8	

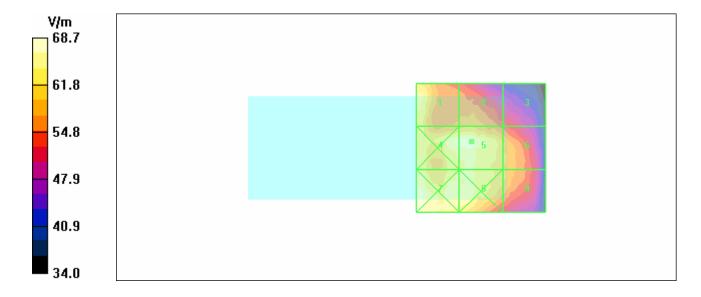



Company Confidential

WR-1017.001

08 June 2006



36 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 2/22/2006 12:43:24 PM Test Laboratory: TCC Dallas

# RH-90, CDMA1900, Ch1175, E field

Communication System: CDMA1900; Frequency: 1908.75 MHz; Duty Cycle: 1:1

DASY4 Configuration:

- Probe: ER3DV6 - SN2337; ConvF(1, 1, 1); Calibrated: 1/31/2005

- Sensor-Surface: (Fix Surface)

- Electronics: DAE3 Sn377; Calibrated: 5/12/2005

- Phantom: HAC Test Arch 4.6; Phantom section: E Device Section

- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 160

# E Scan - ER probe center 10mm above Device Reference/Hearing Aid Compatibility Test

(251x251x1): Measurement grid: dx=2mm, dy=2mm

Maximum value of peak Total field = 58.8 V/m


Probe Modulation Factor = 1.00

Reference Value = 58.0 V/m; Power Drift = -0.192 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

#### Peak E-field in V/m

Grid 1	Grid 2	Grid 3
58.4	51.3	47.9
Grid 4	Grid 5	Grid 6
58.1	58.8	54.4
Grid 7	Grid 8	Grid 9

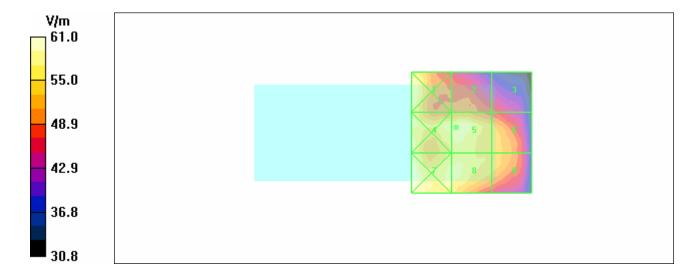



Company Confidential

WR-1017.001

08 June 2006



37 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

Number:

Date/Time: 2/22/2006 9:21:26 AM Test Laboratory: TCC Dallas

RH-90, CDMA1900, Ch25, H field

Communication System: CDMA1900; Frequency: 1851.25 MHz; Duty Cycle: 1:1

DASY4 Configuration:

- Probe: H3DV6 - SN6155; ; Calibrated: 2/16/2005

- Sensor-Surface: (Fix Surface)

- Electronics: DAE3 Sn377; Calibrated: 5/12/2005

- Phantom: HAC Test Arch 4.6; Phantom section: H Device Section

- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 160

## H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility

**Test (251x251x1):** Measurement grid: dx=2mm, dy=2mm

Maximum value of peak Total field = 0.141 A/m


Probe Modulation Factor = 0.700

Reference Value = 0.172 A/m; Power Drift = -0.096 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

#### Peak H-field in A/m

Grid 1		
0.092	0.115	0.115
Grid 4		
0.108	0.141	0.140
Grid 7	Grid 8	Grid 9
0.114	0.140	0.139

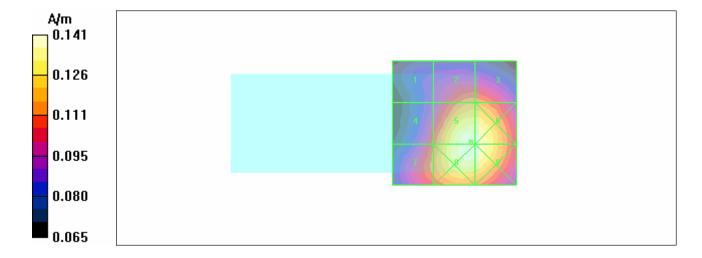



Company Confidential

WR-1017.001

08 June 2006



38 (40)

Ver 2.0

Accredited Laboratory Certificate Number: 1819-01

Date/Time: 2/22/2006 1:15:57 PM Test Laboratory: TCC Dallas

#### RH-90, CDMA1900, Ch600, H field

Communication System: CDMA1900; Frequency: 1880 MHz; Duty Cycle: 1:1

DASY4 Configuration:

- Probe: H3DV6 - SN6155; ; Calibrated: 2/16/2005

- Sensor-Surface: (Fix Surface)

- Electronics: DAE3 Sn377; Calibrated: 5/12/2005

- Phantom: HAC Test Arch 4.6; Phantom section: H Device Section

- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 160

## H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility

**Test (251x251x1):** Measurement grid: dx=2mm, dy=2mm

Maximum value of peak Total field = 0.136 A/m


Probe Modulation Factor = 0.700

Reference Value = 0.166 A/m; Power Drift = 0.229 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

#### Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.093	0.115	0.115
Grid 4		
0.105	0.136	0.134
Grid 7	Grid 8	Grid 9
0.112	0.136	0.134

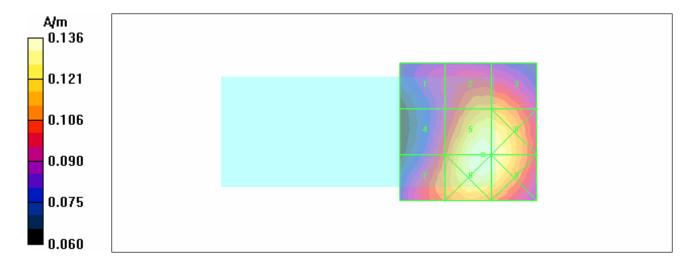



Company Confidential

WR-1017.001

08 June 2006



39 (40)

Ver 2.0

Accredited Laboratory Certificate
Number: 1819-01

Date/Time: 2/21/2006 2:54:23 PM Test Laboratory: TCC Dallas

## RH-90, CDMA1900, Ch1175, H field

Communication System: CDMA1900; Frequency: 1908.75 MHz; Duty Cycle: 1:1

DASY4 Configuration:

- Probe: H3DV6 - SN6155; ; Calibrated: 2/16/2005

- Sensor-Surface: (Fix Surface)

- Electronics: DAE3 Sn377; Calibrated: 5/12/2005

- Phantom: HAC Test Arch 4.6; Phantom section: H Device Section

- Measurement SW: DASY4, V4.6 Build 23; Postprocessing SW: SEMCAD, V1.8 Build 160

## H Scan - H3DV6 probe center 10mm above Device Reference/Hearing Aid Compatibility

**Test (251x251x1):** Measurement grid: dx=2mm, dy=2mm

Maximum value of peak Total field = 0.127 A/m


Probe Modulation Factor = 0.700

Reference Value = 0.157 A/m; Power Drift = -0.056 dB

Hearing Aid Near-Field Category: M4 (AWF 0 dB)

#### Peak H-field in A/m

Grid 1	Grid 2	Grid 3
0.088	0.105	0.105
Grid 4		
0.101	0.127	0.126
Grid 7	Grid 8	Grid 9
0.113	0.128	0.127

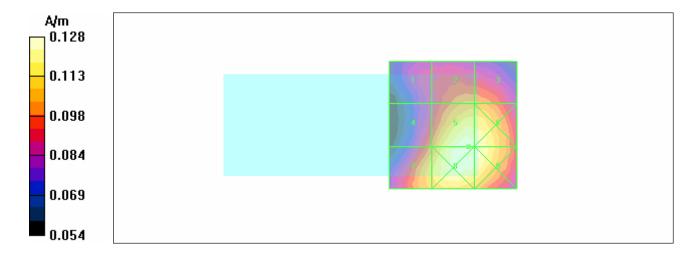



**Company Confidential** 

WR-1017.001

08 June 2006



40 (40)

Accredited Laboratory Certificate Number: 1819-01 Ver 2.0

## APPENDIX C: PROBE CALIBRATION REPORTS AND DIPOLE CALIBRATION REPORTS

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 108

Client

Nokia TX

Certificate No: ER3-2337\_Jan05

## **CALIBRATION CERTIFICATE**

Object ER3DV6 - SN:2337

Calibration procedure(s) QA CAL-02.v4

Calibration procedure for E-field probes optimized for close near field

evaluations in air

Calibration date: January 31, 2005

Condition of the calibrated item In Tolerance

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	5-May-04 (METAS, No. 251-00388)	May-05
Power sensor E4412A	MY41495277	5-May-04 (METAS, No. 251-00388)	May-05
Reference 3 dB Attenuator	SN: S5054 (3c)	10-Aug-04 (METAS, No. 251-00403)	Aug-05
Reference 20 dB Attenuator	SN: S5086 (20b)	3-May-04 (METAS, No. 251-00389)	May-05
Reference 30 dB Attenuator	SN: S5129 (30b)	10-Aug-04 (METAS, No. 251-00404)	Aug-05
Reference Probe ER3DV6	SN: 2328	6-Oct-04 (SPEAG, No. ER3-2328_Oct04)	Oct-05
DAE4	SN: 617	19-Jan-05 (SPEAG, No. DAE4-617_Jan05)	Jan-06
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092180	18-Sep-02 (SPEAG, in house check Oct-03)	In house check: Oct 05
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Dec-03)	In house check: Dec-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-04)	In house check: Nov 05
	Name	Function	Signature
Calibrated by:	Katja Pokovic	Technical Manager	-27 127
			Dai: Rat-
		and the second s	111-
Approved by:	Niels Kuster	Quality Manager 🙎	1 /4
	والمستروب	erannar van de zarenne dimentergene system groeppelije in geropeen ty de groeppelije geroep groep groep de groep	

Issued: February 19, 2005

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ER3-2337\_Jan05

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S wiss Calibration Service

Accreditatio

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

NORMx,y,z sensitivity in free space

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at

measurement center), i.e., 9 = 0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot

coordinate system

## Calibration is Performed According to the Following Standards:

a) IEEE Std 1309-1996, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", 1996.

### **Methods Applied and Interpretation of Parameters:**

- NORMx,y,z: Assessed for E-field polarization 9 = 0 for XY sensors and 9 = 90 for Z sensor (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- NORM(f)x,y,z = NORMx,y,z \* frequency response (see Frequency Response Chart).
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: ER3-2337 Jan05

Page 2 of 9

January 31, 2005

#### ER3DV6 SN:2337

# Probe ER3DV6

SN:2337

Manufactured: Calibrated:

September 9, 2003 January 31, 2005

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

## DASY - Parameters of Probe: ER3DV6 SN:2337

Sensitivity in Free Space  $[\mu V/(V/m)^2]$ 

Diode Compression<sup>A</sup>

NormX **1.51** ± 10.

**1.51** ± 10.1 % (k=2)

DCP X

**95** mV

NormY

**1.43** ± 10.1 % (k=2)

DCP Y

**95** mV

NormZ

**1.58** ± 10.1 % (k=2)

DCP Z

**97** mV

## **Frequency Correction**

Х

0.0

Υ

0.0

Z

0.0

Sensor Offset

(Probe Tip to Sensor Center)

Χ

2.5 mm

Υ

2.5 mm

Ζ

2.5 mm

**Connector Angle** 

-25 °


The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: ER3-2337-Jan05

<sup>&</sup>lt;sup>A</sup> numerical linearization parameter: uncertainty not required


# Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide R22)

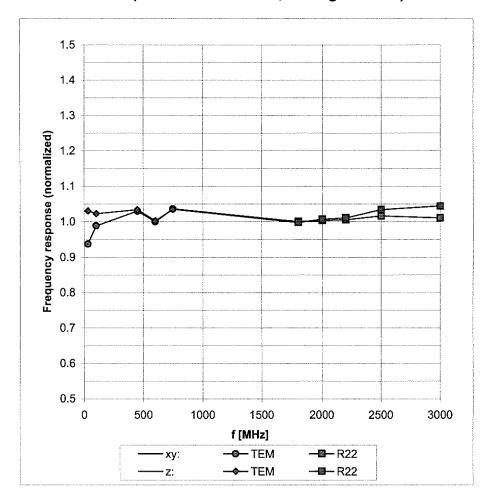


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Receiving Pattern ( $\phi$ ),  $\theta$  = 0°

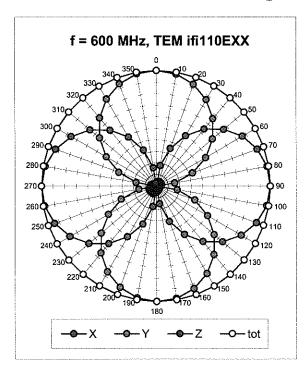

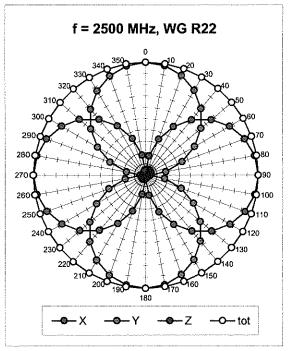


Receiving Pattern ( $\phi$ ),  $\vartheta$  = 90°

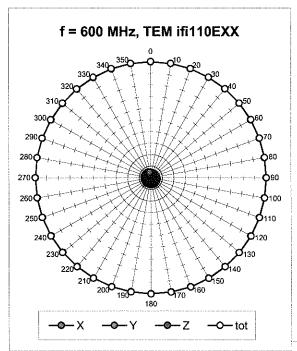

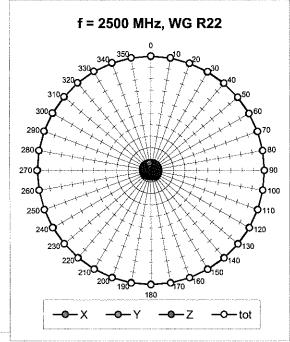


Receiving Pattern ( $\phi$ ),  $\vartheta = 0^{\circ}$ 

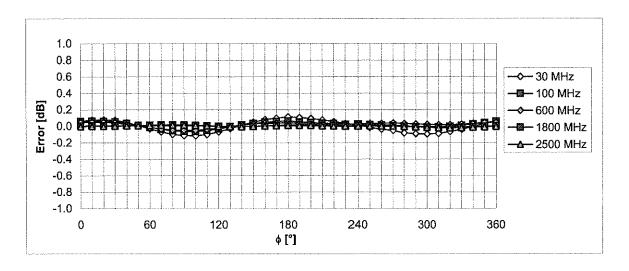

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Receiving Pattern ( $\phi$ ),  $\vartheta$  = 90°

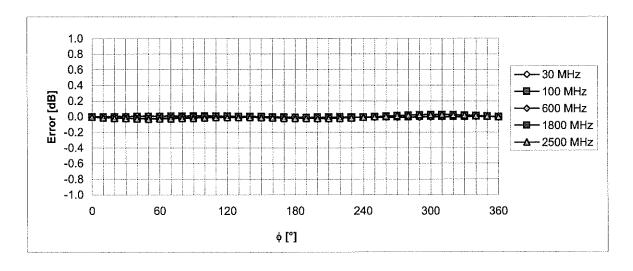


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

# **Dynamic Range f(E-field)**


(Waveguide R22, f = 1800 MHz)

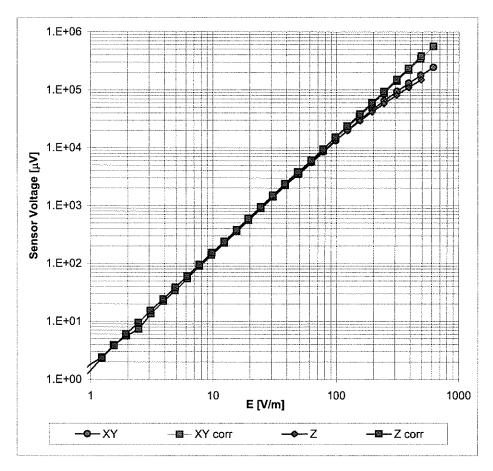

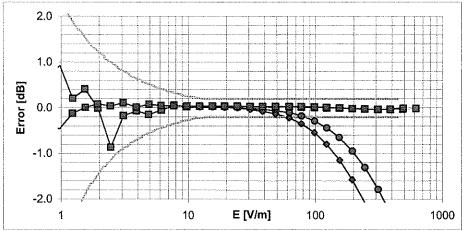

Uncertainty of Linearity Assessment: ± 0.6% (k=2)

# Deviation from Isotropy in Air Error $(\phi, \vartheta)$ , f = 900 MHz

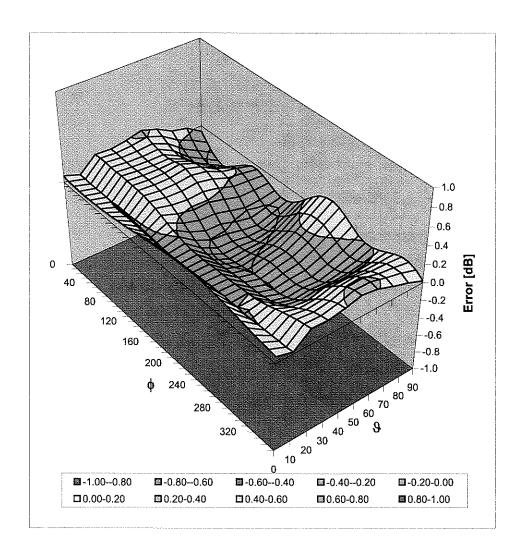

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client

Nokia TX

Certificate No: H3-6155\_Feb05

## **CALIBRATION CERTIFICATE**

Object H3DV6 - SN:6155

Calibration procedure(s) QA CAL-03.v4

Calibration procedure for H-field probes optimized for close near field

evaluations in air

Calibration date: February 16, 2005

Condition of the calibrated item In Tolerance

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	5-May-04 (METAS, No. 251-00388)	May-05
Power sensor E4412A	MY41495277	5-May-04 (METAS, No. 251-00388)	May-05
Reference 3 dB Attenuator	SN: S5054 (3c)	10-Aug-04 (METAS, No. 251-00403)	Aug-05
Reference 20 dB Attenuator	SN: S5086 (20b)	3-May-04 (METAS, No. 251-00389)	May-05
Reference 30 dB Attenuator	SN: S5129 (30b)	10-Aug-04 (METAS, No. 251-00404)	Aug-05
Reference Probe H3DV6	SN: 6182	6-Oct-04 (SPEAG, No. H3-6182_Oct04)	Oct-05
DAE4	SN: 617	19-Jan-05 (SPEAG, No. DAE4-617_Jan05)	Jan-06
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092180	18-Sep-02 (SPEAG, in house check Oct-03)	In house check: Oct 05
RF generator HP 8648C	US3642U01700	4-Aug-99 (SPEAG, in house check Dec-03)	In house check: Dec-05
Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-04)	In house check: Nov 05
	Name	Function	Signature
Calibrated by:	Katja Pokovic	Technical Manager	Ŵ. 11L
			Man's Vert
		V	
Approved by:	Niels Kuster	Quality Manager /	1 Laster
		1991 T. (1991 T. (199	<i>J. J. QVD</i> \
			. 1000

Issued: February 19, 2005

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: H3-6155\_Feb05

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Federal Office of Metrology and Accreditation
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

Polarization 9

NORMx,y,z sensitivity in free space

DCP diode Polarization φ φ rot

diode compression point φ rotation around probe axis

9 rotation around an axis that is in the plane normal to probe axis (at

measurement center), i.e., 9 = 0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot

coordinate system

## Calibration is Performed According to the Following Standards:

a) IEEE Std 1309-1996, "IEEE Standard for calibration of electromagnetic field sensors and probes, excluding antennas, from 9 kHz to 40 GHz", 1996.

## **Methods Applied and Interpretation of Parameters:**

- X, Y,Z\_a0a1a2: Assessed for E-field polarization θ = 90 for XY sensors and θ = 0 for Z sensor (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
- X,Y,Z(f)\_a0a1a2= X,Y,Z\_a0a1a2\* frequency\_response (see Frequency Response Chart).
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency.
- Spherical isotropy (3D deviation from isotropy): in a locally homogeneous field realized using an open waveguide setup.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the  $X_{a0a1a2}$  (no uncertainty required).

Certificate No: H3-6155\_Feb05

Page 2 of 8

# Probe H3DV6

SN:6155

Manufactured:

Calibrated:

June 22, 2004

February 16, 2005

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

## DASY - Parameters of Probe: H3DV6 SN:6155

Sensitivity in Free Space [A/m /  $\sqrt{(\mu V)}$ ]

a0 a1 a2 X 2.719E-03 -7.681E-5 3.643E-5 ± 5.1 % (k=2) Y 2.743E-03 1.819E-5 -1.877E-5 ± 5.1 % (k=2) Z 2.974E-03 -4.287E-5 -1.156E-5 ± 5.1 % (k=2)

Diode Compression<sup>1</sup>

DCP X **86** mV DCP Y **86** mV DCP Z **85** mV

Sensor Offset (Probe Tip to Sensor Center)

X 3.0 mm Y 3.0 mm Z 3.0 mm


Connector Angle 319 °

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

<sup>1</sup> numerical linearization parameter: uncertainty not required


# Frequency Response of H-Field


(TEM-Cell:ifi110, Waveguide R22)

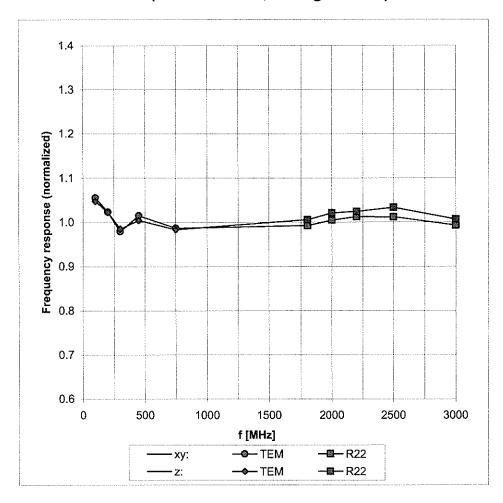


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Receiving Pattern ( $\phi$ ),  $\theta$  = 90°

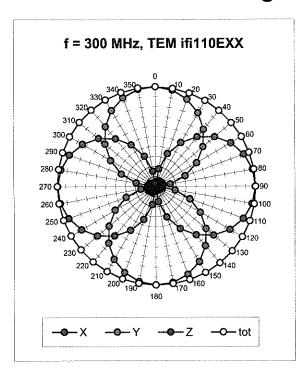

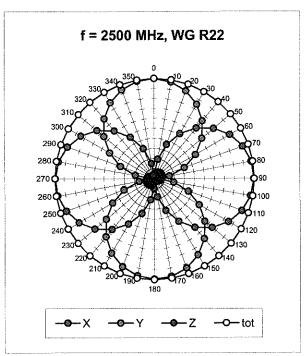


Receiving Pattern ( $\phi$ ),  $\vartheta = 0^{\circ}$ 

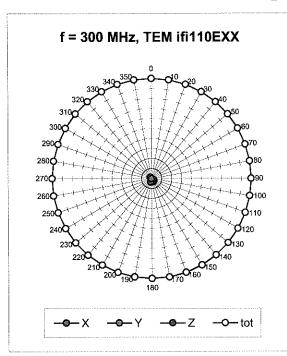

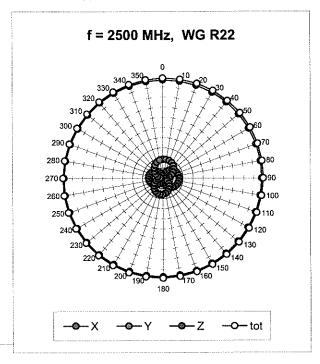


Receiving Pattern ( $\phi$ ),  $\theta$  = 90°

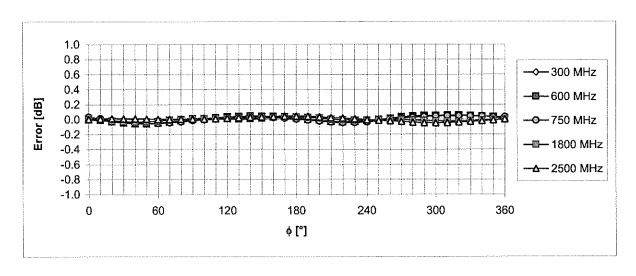

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Receiving Pattern ( $\phi$ ),  $\vartheta = 0^{\circ}$ 

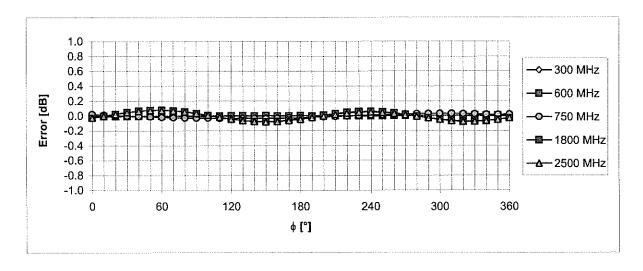


Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)

## Dynamic Range f(H-field)

(Waveguide R22, f = 1800 MHz)

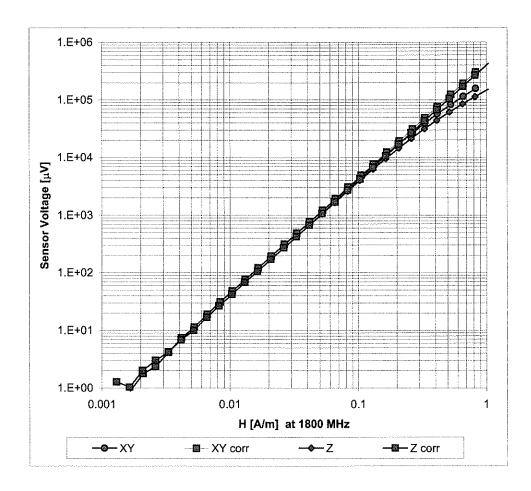

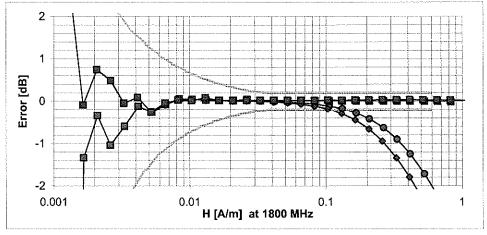

Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

Client

**Nokia TX** 

Certificate No: CD1880V3-1025\_Jun05

## CALIBRATION CERTIFICATE

Object

CD1880V3 - SN: 1025

Calibration procedure(s)

QA CAL-20.v3

Calibration procedure for dipoles in air

Calibration date:

June 2, 2005

Condition of the calibrated item

In Tolerance

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). All calibrations have been conducted at an environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

	Primary Standards	ID#	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
20 dB Attenuator       SN: 5086 (20g)       10-Aug-04 (METAS, No 251-00402)       Aug-05         10 dB Attenuator       SN: 5047.2 (10r)       10-Aug-04 (METAS, No 251-00402)       Aug-05         Secondary Standards       ID #       Check Date (in house)       Scheduled Check         Network Analyzer HP 8753E       US37390585       18-Oct-01 (SPEAG, in house check Nov-04)       In house check: Nov-05         RF generator R&S SML-03       100698       27-Mar-02 (SPEAG, in house check Dec-03)       In house check: Dec-05         DAE4       SN: 901       29-Jun-04 (SPEAG, No. DAE4-901_Jun04)       Calibration, Jun-05	Power meter EPM-442A	GB37480704	12-Oct-04 (METAS, No. 251-00412)	Oct-05
10 dB Attenuator         SN: 5047.2 (10r)         10-Aug-04 (METAS, No 251-00402)         Aug-05           Secondary Standards         ID #         Check Date (in house)         Scheduled Check           Network Analyzer HP 8753E         US37390585         18-Oct-01 (SPEAG, in house check Nov-04)         In house check: Nov-05           RF generator R&S SML-03         100698         27-Mar-02 (SPEAG, in house check Dec-03)         In house check: Dec-05           DAE4         SN: 901         29-Jun-04 (SPEAG, No. DAE4-901_Jun04)         Calibration, Jun-05	Power sensor HP 8481A	US37292783	12-Oct-04 (METAS, No. 251-00412)	Oct-05
Secondary Standards ID # Check Date (in house) Scheduled Check  Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov-05  RF generator R&S SML-03 100698 27-Mar-02 (SPEAG, in house check Dec-03) In house check: Dec-05  DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05	20 dB Attenuator	SN: 5086 (20g)	10-Aug-04 (METAS, No 251-00402)	Aug-05
Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov-05 RF generator R&S SML-03 100698 27-Mar-02 (SPEAG, in house check Dec-03) In house check: Dec-05 DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05	10 dB Attenuator	SN: 5047.2 (10r)	10-Aug-04 (METAS, No 251-00402)	Aug-05
Network Analyzer HP 8753E US37390585 18-Oct-01 (SPEAG, in house check Nov-04) In house check: Nov-05 RF generator R&S SML-03 100698 27-Mar-02 (SPEAG, in house check Dec-03) In house check: Dec-05 DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05				
RF generator R&S SML-03 100698 27-Mar-02 (SPEAG, in house check Dec-03) In house check: Dec-05 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05	Secondary Standards	ID#	Check Date (in house)	Scheduled Check
DAE4 SN: 901 29-Jun-04 (SPEAG, No. DAE4-901_Jun04) Calibration, Jun-05	Network Analyzer HP 8753E	US37390585	18-Oct-01 (SPEAG, in house check Nov-04)	In house check: Nov-05
	RF generator R&S SML-03	100698	27-Mar-02 (SPEAG, in house check Dec-03)	In house check: Dec-05
Probe ER3DV6 SN: 2336 20-Jan-05 (SPEAG, No. ER3-2336_Jan05) Calibration, Jan-06	DAE4	SN: 901	29-Jun-04 (SPEAG, No. DAE4-901_Jun04)	Calibration, Jun-05
	Probe ER3DV6	SN: 2336	20-Jan-05 (SPEAG, No. ER3-2336_Jan05)	Calibration, Jan-06
Probe H3DV6 SN: 6065 10-Dec-04 (SPEAG, No. H3-6065-Dec04) Calibration, Dec-05	Probe H3DV6	SN: 6065	10-Dec-04 (SPEAG, No. H3-6065-Dec04)	Calibration, Dec-05

Calibrated by:

Name

Function

Signature

Mike Meili

Laboratory Technician

M. Peih

Approved by:

Fin Bomholt

**Technical Director** 

Issued: June 13, 2005

F. Bondelf

This calibration certificate is issued as an intermediate solution until the specific calibration procedure is submitted and accepted in the frame of the accreditation of the Calibration Laboratory of Schmid & Partner Engineering AG (based on ISO/IEC 17025 International Standard)

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland

#### References

[1] ANSI-PC63.19-2001 (Draft 3.x, 2005)
American National Standard for Methods of Measurement of Compatibility between Wireless Communications
Devices and Hearing Aids.

#### Methods Applied and Interpretation of Parameters:

- Coordinate System: y-axis is in the direction of the dipole arms. z-axis is from the basis of the antenna (mounted on the table) towards its feed point between the two dipole arms. x-axis is normal to the other axes. In coincidence with standard [1], the measurement planes (probe sensor center) are selected to be at a distance of 10 mm above the the top edge of the dipole arms.
- Measurement Conditions: Further details are available from the hardcopies at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. The forward power to the dipole connector is set with a calibrated power meter connected and monitored with an auxiliary power meter connected to a directional coupler. While the dipole under test is connected, the forward power is adjusted to the same level.
- Antenna Positioning: The dipole is mounted on a HAC Test Arch phantom using the matching dipole positioner with the arms horizontal and the feeding cable coming from the floor. The measurements are performed in a shielded room with absorbers around the setup to reduce the reflections.
  It is verified before the mounting of the dipole under the Test Arch phantom, that its arms are perfectly in a line. It is installed on the HAC dipole positioner with its arms parallel below the dielectric reference wire and able to move elastically in vertical direction without changing its relative position to the top center of the Test Arch phantom. The vertical distance to the probe is adjusted after dipole mounting with a DASY4 Surface Check job. Before the measurement, the distance between phantom surface and probe tip is verified. The proper measurement distance is selected by choosing the matching section of the HAC Test Arch phantom with the proper device reference point (upper surface of the dipole) and the matching grid reference point (tip of the probe) considering the probe sensor offset. The vertical distance to the probe is essential for the accuracy.
- Feed Point Impedance and Return Loss: These parameters are measured using a HP 8753E Vector Network
  Analyzer. The impedance is specified at the SMA connector of the dipole. The influence of reflections was
  eliminating by applying the averaging function while moving the dipole in the air, at least 70cm away from any
  obstacles.
- E- field distribution: E field is measured in the x-y-plane with an isotropic ER3D-field probe with 100 mW forward power to the antenna feed point. In accordance with [1], the scan area is 20mm wide, its length exceeds the dipole arm length (180 or 90mm). The sensor center is 10 mm (in z) above the top of the dipole arms. Two 3D maxima are available near the end of the dipole arms. Assuming the dipole arms are perfectly in one line, the average of these two maxima (in subgrid 2 and subgrid 8) is determined to compensate for any non-parallelity to the measurement plane as well as the sensor displacement. The E-field value stated as calibration value represents the maximum of the interpolated 3D-E-field, 10mm above the dipole surface.
- H-field distribution: H-field is measured with an isotropic H-field probe with 100mW forward power to the
  antenna feed point, in the x-y-plane. The scan area and sensor distance is equivalent to the E-field scan. The
  maximum of the field is available at the center (subgrid 5) above the feed point. The H-field value stated as
  calibration value represents the maximum of the interpolated H-field, 10mm above the dipole surface at the
  feed point.

#### 1 Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY4	V4.5 B31
SEMCAD	V1.8 B149
HAC Test Arch	SD HAC P01 BA, #1002
10 mm	
dx, dy = 5 mm	area = 20 x 90 mm
1880 MHz ± 1 MHz	
20.0 dBm = 100mW	
< 0.05 dB	
	SEMCAD  HAC Test Arch  10 mm  dx, dy = 5 mm  1880 MHz ± 1 MHz  20.0 dBm = 100mW

#### 2 Maximum Field values

H-field 10 mm above dipole surface	condition	interpolated maximum
Maximum measured	100 mW forward power	0.452 A/m

Uncertainty for H-field measurement: 8.2% (k=2)

E-field 10 mm above dipole surface	condition	interpolated maximum
Maximum measured above high end	100 mW forward power	139.4 V/m
Maximum measured above low end	100 mW forward power	135.8 V/m
Averaged maximum above arm	100 mW forward power	137.6 V/m

Uncertainty for E-field measurement: 12.8% (k=2)

### 3 Appendix

#### 3.1 Antenna Parameters

Frequency	Return Loss	Impedance
1710 MHz	19.9 dB	( 61.2 – j0.7 ) Ohm
1880 MHz	20.9 dB	( 58.6 – j4.7 ) Ohm
1900 MHz	21.7 dB	( 55.5 – j6.7 ) Ohm
1950 MHz	30.4 dB	( 49.0 – j2.8 ) Ohm
2000 MHz	21.0 dB	( 54.0 + j8.4 ) Ohm

## 3.2 Antenna Design and Handling

The calibration dipole has a symmetric geometry with a built-in two stub matching network, which leads to the enhanced bandwidth.


The dipole is built of standard semirigid coaxial cable. The internal matching line is open ended. The antenna is therefore open for DC signals.

Do not apply force to dipole arms, as they are liable to bend. The soldered connections near the feedpoint may be damaged. After excessive mechanical stress or overheating, check the impedance characteristics to ensure that the internal matching network is not affected.

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

#### 3.3 Measurement Sheets

#### 3.3.1 Return Loss and Smith Chart

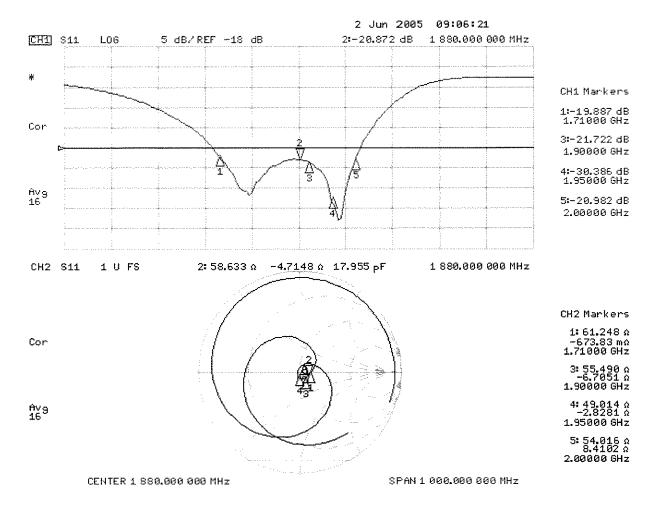

#### 3.3.2 DASY4 H-field result

Date/Time: 6/2/2005 6:15:52 PM

Test Laboratory: SPEAG, Zurich, Switzerland

## DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: 1025

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air

Medium parameters used:  $\sigma = 0$  mho/m,  $\varepsilon_r = 1$ ;  $\rho = 1$  kg/m<sup>3</sup>

Phantom section: H Dipole Section

## DASY4 Configuration:

• Probe: H3DV6 - SN6065; Calibrated: 12/10/2004

• Sensor-Surface: (Fix Surface)

Electronics: DAE4 Sn901; Calibrated: 6/29/2004

• Phantom: HAC Test Arch; Type: SD HAC P01 BA; Serial: 1002

• Measurement SW: DASY4, V4.5 Build 31; Postprocessing SW: SEMCAD, V1.8 Build 149

## H Scan 10mm above CD1880V3/Hearing Aid Compatibility Test (41x181x1):

Measurement grid: dx=5mm, dy=5mm

Maximum value of Total field (slot averaged) = 0.452 A/m


Reference Value = 0.478 A/m; Power Drift = -0.034 dB

## Hearing Aid Near-Field Category: M2 (AWF 0 dB)

H in A/m (Time averaged) H in A/m (Slot averaged)

Grid 1 <b>0.391</b>	Grid 2 <b>0.425</b>	
	Grid 5 <b>0.452</b>	Grid 6 <b>0.437</b>
	Grid 8 <b>0.401</b>	Grid 9 <b>0.389</b>

Grid 1	Grid 2	Grid 3
<b>0.391</b>	<b>0.425</b>	<b>0.408</b>
Grid 4	Grid 5	Grid 6
<b>0.419</b>	<b>0.452</b>	<b>0.437</b>
Grid 7	Grid 8	Grid 9
<b>0.372</b>	<b>0.401</b>	<b>0.389</b>

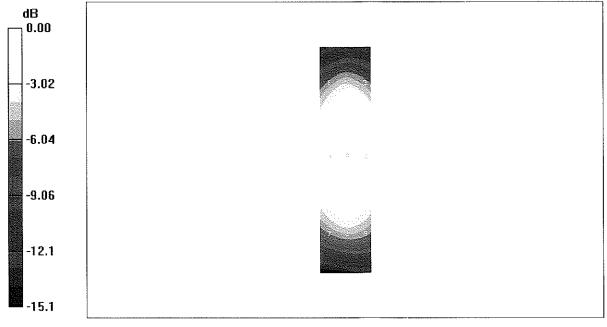

0 dB = 0.452 A/m

Date/Time: 6/2/2005 2:45:27 PM

Test Laboratory: SPEAG, Zurich, Switzerland

## DUT: HAC Dipole 1880 MHz; Type: CD1880V3; Serial: 1025

Communication System: CW; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: Air

Medium parameters used:  $\sigma = 0$  mho/m,  $\varepsilon_r = 1$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: E Dipole Section

## DASY4 Configuration:

Probe: ER3DV6 - SN2336; ConvF(1, 1, 1); Calibrated: 1/20/2005

Sensor-Surface: (Fix Surface)

Electronics: DAE4 Sn901; Calibrated: 6/29/2004

Phantom: HAC Test Arch; Type: SD HAC P01 BA; Serial: 1002

Measurement SW: DASY4, V4.5 Build 31; Postprocessing SW: SEMCAD, V1.8 Build 149

## E Scan 10mm above CD1880V3/Hearing Aid Compatibility Test (41x181x1):

Measurement grid: dx=5mm, dy=5mm

Maximum value of Total field (slot averaged) = 139.4 V/m


Reference Value = 157.2 V/m; Power Drift = 0.013 dB

## Hearing Aid Near-Field Category: M2 (AWF 0 dB)

E in V/m (Time averaged) E in V/m (Slot averaged)

Grid 1 131.9	Grid 2 135.8		
Grid 4 <b>90.0</b>	Grid 5 <b>91.6</b>		
Grid 7	Grid 8 139.4	Grid 9	

Grid 1	Grid 2	Grid 3
<b>131.9</b>	135.8	<b>130.9</b>
Grid 4	Grid 5	Grid 6
<b>90.0</b>	<b>91.6</b>	<b>87.1</b>
70.0		07.11

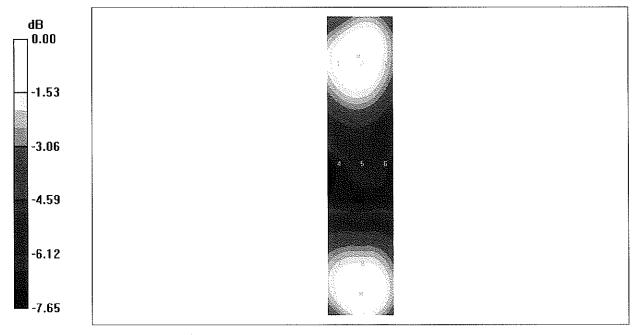

0 dB = 139.4 V/m