
APPENDIX E: RELEVANT PAGES FROM PROBE CALIBRATION REPORT(S)

6044

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **Nokia SD**

Certificate No: **ET3-1399_Feb12**

CALIBRATION CERTIFICATE

Object

ET3DV6R - SN:1399

Calibration procedure(s)

QA CAL-01.v8, QA CAL-23.v4, QA CAL-25.v4
Calibration procedure for dosimetric E-field probes

Calibration date:

February 10, 2012

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	31-Mar-11 (No. 217-01372)	Apr-12
Power sensor E4412A	MY41498087	31-Mar-11 (No. 217-01372)	Apr-12
Reference 3 dB Attenuator	SN: S5054 (3c)	29-Mar-11 (No. 217-01369)	Apr-12
Reference 20 dB Attenuator	SN: S5086 (20b)	29-Mar-11 (No. 217-01367)	Apr-12
Reference 30 dB Attenuator	SN: S5129 (30b)	29-Mar-11 (No. 217-01370)	Apr-12
Reference Probe ES3DV2	SN: 3013	29-Dec-11 (No. ES3-3013_Dec11)	Dec-12
DAE4	SN: 654	3-May-11 (No. DAE4-654_May11)	May-12
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-11)	In house check: Apr-13
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-11)	In house check: Oct-12

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
Issued: February 14, 2012			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

DASY/EASY - Parameters of Probe: ET3DV6R - SN:1399

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
750	41.9	0.89	6.05	6.05	6.05	0.31	3.00	± 12.0 %
835	41.5	0.90	5.82	5.82	5.82	0.42	2.34	± 12.0 %
1810	40.0	1.40	4.92	4.92	4.92	0.80	2.24	± 12.0 %
1950	40.0	1.40	4.69	4.69	4.69	0.80	2.14	± 12.0 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

DASY/EASY - Parameters of Probe: ET3DV6R - SN:1399

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
750	55.5	0.96	5.93	5.93	5.93	0.31	3.00	± 12.0 %
835	55.2	0.97	5.83	5.83	5.83	0.50	2.27	± 12.0 %
1810	53.3	1.52	4.47	4.47	4.47	0.80	2.45	± 12.0 %
1950	53.3	1.52	4.49	4.49	4.49	0.80	2.24	± 12.0 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.



Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Nokia SD**

Certificate No: **EX3-3852_Mar12**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3852**

Calibration procedure(s) **QA CAL-01.v8, QA CAL-14.v3, QA CAL-23.v4, QA CAL-25.v4**
Calibration procedure for dosimetric E-field probes

Calibration date: **March 27, 2012**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	31-Mar-11 (No. 217-01372)	Apr-12
Power sensor E4412A	MY41498087	31-Mar-11 (No. 217-01372)	Apr-12
Reference 3 dB Attenuator	SN: S5054 (3c)	29-Mar-11 (No. 217-01369)	Apr-12
Reference 20 dB Attenuator	SN: S5086 (20b)	29-Mar-11 (No. 217-01367)	Apr-12
Reference 30 dB Attenuator	SN: S5129 (30b)	29-Mar-11 (No. 217-01370)	Apr-12
Reference Probe ES3DV2	SN: 3013	29-Dec-11 (No. ES3-3013_Dec11)	Dec-12
DAE4	SN: 654	3-May-11 (No. DAE4-654_May11)	May-12
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-11)	in house check: Apr-13
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-11)	in house check: Oct-12

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
Issued: March 29, 2012			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3852

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
750	41.9	0.89	9.58	9.58	9.58	0.22	1.35	± 12.0 %
835	41.5	0.90	9.36	9.36	9.36	0.24	1.10	± 12.0 %
1750	40.1	1.37	7.95	7.95	7.95	0.60	0.66	± 12.0 %
1900	40.0	1.40	7.80	7.80	7.80	0.50	0.72	± 12.0 %
2450	39.2	1.80	7.06	7.06	7.06	0.20	1.23	± 12.0 %
2600	39.0	1.96	6.82	6.82	6.82	0.39	0.89	± 12.0 %
5200	36.0	4.66	4.86	4.86	4.86	0.40	1.80	± 13.1 %
5300	35.9	4.76	4.65	4.65	4.65	0.40	1.80	± 13.1 %
5500	35.6	4.96	4.56	4.56	4.56	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.21	4.21	4.21	0.50	1.80	± 13.1 %
5800	35.3	5.27	4.20	4.20	4.20	0.50	1.80	± 13.1 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3852

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha	Depth (mm)	Unct. (k=2)
750	55.5	0.96	9.31	9.31	9.31	0.31	1.01	± 12.0 %
835	55.2	0.97	9.14	9.14	9.14	0.46	0.83	± 12.0 %
1750	53.4	1.49	7.75	7.75	7.75	0.43	0.97	± 12.0 %
1900	53.3	1.52	7.24	7.24	7.24	0.40	0.95	± 12.0 %
2450	52.7	1.95	6.83	6.83	6.83	0.80	0.60	± 12.0 %
2600	52.5	2.16	6.66	6.66	6.66	0.80	0.58	± 12.0 %
5200	49.0	5.30	4.10	4.10	4.10	0.55	1.90	± 13.1 %
5300	48.9	5.42	4.22	4.22	4.22	0.50	1.90	± 13.1 %
5500	48.6	5.65	3.83	3.83	3.83	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.47	3.47	3.47	0.60	1.90	± 13.1 %
5800	48.2	6.00	3.86	3.86	3.86	0.60	1.90	± 13.1 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

APPENDIX F: RELEVANT PAGES FROM DIPOLE VALIDATION KIT REPORT(S)

ASSET 6987

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
 The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Nokia SD**

Certificate No: **D835V2-487_Feb12**

CALIBRATION CERTIFICATE

Object **D835V2 - SN: 487**

Calibration procedure(s) **QA CAL-05.v8**
Calibration procedure for dipole validation kits above 700 MHz

Calibration date: **February 17, 2012**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	05-Oct-11 (No. 217-01451)	Oct-12
Power sensor HP 8481A	US37292783	05-Oct-11 (No. 217-01451)	Oct-12
Reference 20 dB Attenuator	SN: 5086 (20g)	29-Mar-11 (No. 217-01368)	Apr-12
Type-N mismatch combination	SN: 5047.2 / 06327	29-Mar-11 (No. 217-01371)	Apr-12
Reference Probe ES3DV3	SN: 3205	30-Dec-11 (No. ES3-3205_Dec11)	Dec-12
DAE4	SN: 601	04-Jul-11 (No. DAE4-601_Jul11)	Jul-12

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-11)	In house check: Oct-12

	Name	Function	Signature
Calibrated by:	Israe El-Naouq	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: February 17, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

DASY5 Validation Report for Head TSL

Date: 17.02.2012

Test Laboratory: The name of your organization

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 487

Communication System: CW; Frequency: 835 MHz

Medium parameters used: $f = 835$ MHz; $\sigma = 0.89$ mho/m; $\epsilon_r = 41$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.07, 6.07, 6.07); Calibrated: 30.12.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.0(692); SEMCAD X 14.6.4(4989)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 56.945 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 3.4020

SAR(1 g) = 2.31 mW/g; SAR(10 g) = 1.51 mW/g

Maximum value of SAR (measured) = 2.691 mW/g

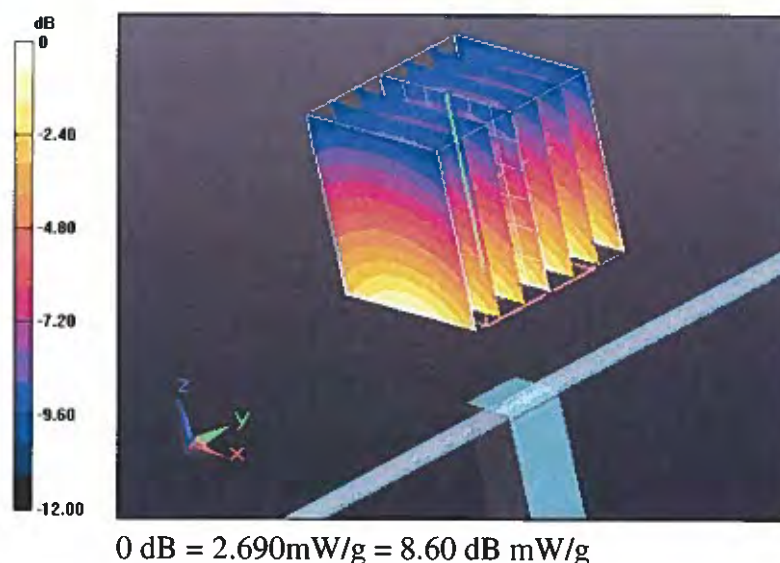

DASY5 Validation Report for Body TSL

Date: 17.02.2012

Test Laboratory: The name of your organization

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 487

Communication System: CW; Frequency: 835 MHz

Medium parameters used: $f = 835$ MHz; $\sigma = 1.01$ mho/m; $\epsilon_r = 55.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.02, 6.02, 6.02); Calibrated: 30.12.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.0(692); SEMCAD X 14.6.4(4989)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 54.922 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 3.5200

SAR(1 g) = 2.44 mW/g; SAR(10 g) = 1.6 mW/g

Maximum value of SAR (measured) = 2.833 mW/g

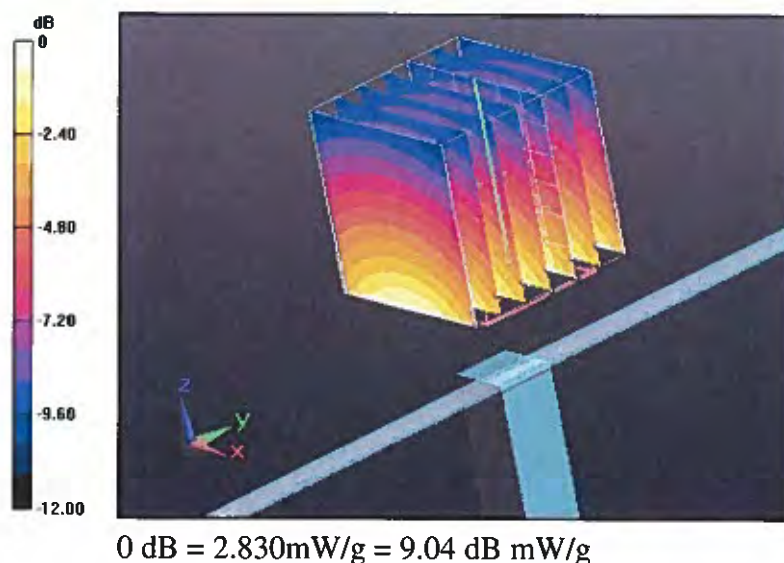



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Nokia SD**

Certificate No: **D1800V2-2d063_Jul11**

CALIBRATION CERTIFICATE

Object **D1800V2 - SN: 2d063**

Calibration procedure(s) **QA CAL-05.v8
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **July 22, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37292783	06-Oct-10 (No. 217-01266)	Oct-11
Reference 20 dB Attenuator	SN: S5086 (20b)	29-Mar-11 (No. 217-01367)	Apr-12
Type-N mismatch combination	SN: 5047.2 / 06327	29-Mar-11 (No. 217-01371)	Apr-12
Reference Probe ES3DV3	SN: 3205	29-Apr-11 (No. ES3-3205_Apr11)	Apr-12
DAE4	SN: 601	04-Jul-11 (No. DAE4-601_Jul11)	Jul-12
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

Calibrated by: **Dimce Iliev** **Laboratory Technician** *D. Iliev*

Approved by: **Katja Pokovic** **Technical Manager** *K. Pokovic*

Issued: July 22, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1800 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	39.2 $\pm$ 6 %	1.37 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.52 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	38.4 mW / g $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.03 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	20.2 mW / g $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	52.2 $\pm$ 6 %	1.50 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.69 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	38.9 mW / g $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.15 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	20.6 mW / g $\pm$ 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.3 Ω - 3.5 j Ω
Return Loss	- 28.0 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	43.9 Ω - 3.6 j Ω
Return Loss	- 22.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.209 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	January 28, 2003

DASY5 Validation Report for Head TSL

Date: 20.07.2011

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d063

Communication System: CW; Frequency: 1800 MHz

Medium parameters used: $f = 1800$ MHz; $\sigma = 1.37$ mho/m; $\epsilon_r = 39.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.07, 5.07, 5.07); Calibrated: 29.04.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 97.327 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 16.968 W/kg


SAR(1 g) = 9.52 mW/g; SAR(10 g) = 5.03 mW/g

Maximum value of SAR (measured) = 11.923 mW/g

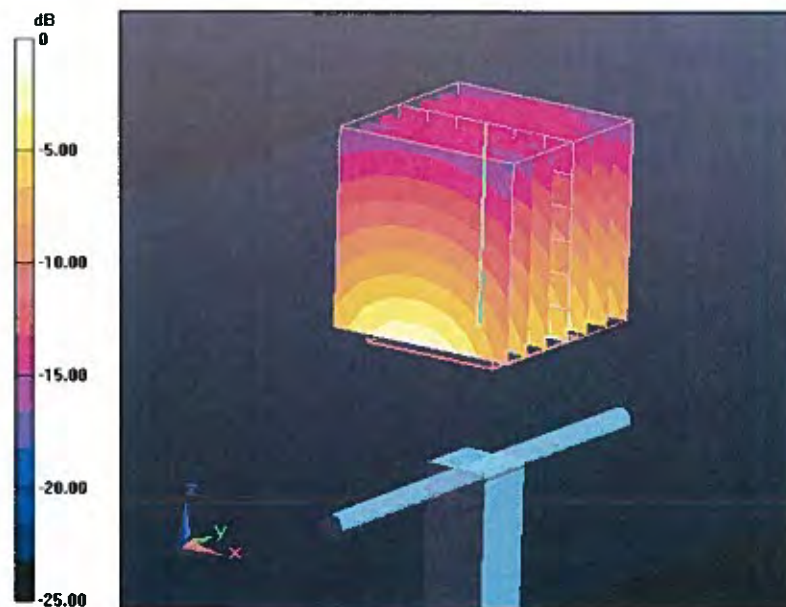

0 dB = 11.920mW/g

Impedance Measurement Plot for Head TSL

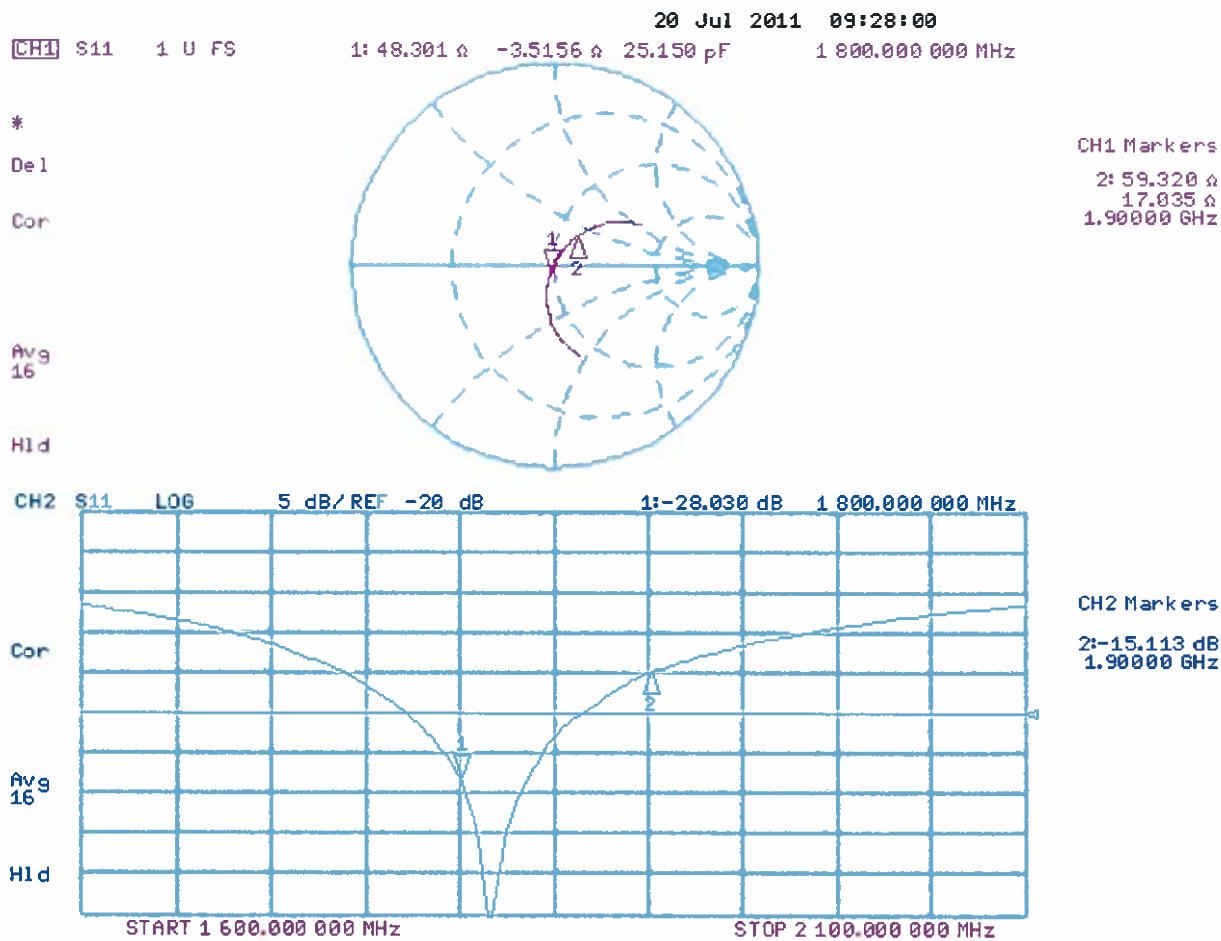

DASY5 Validation Report for Body TSL

Date: 22.07.2011

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d063

Communication System: CW; Frequency: 1800 MHz

Medium parameters used: $f = 1800$ MHz; $\sigma = 1.5$ mho/m; $\epsilon_r = 52.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.74, 4.74, 4.74); Calibrated: 29.04.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.068 V/m; Power Drift = -0.0055 dB

Peak SAR (extrapolated) = 16.989 W/kg

SAR(1 g) = 9.69 mW/g; SAR(10 g) = 5.15 mW/g

Maximum value of SAR (measured) = 12.263 mW/g

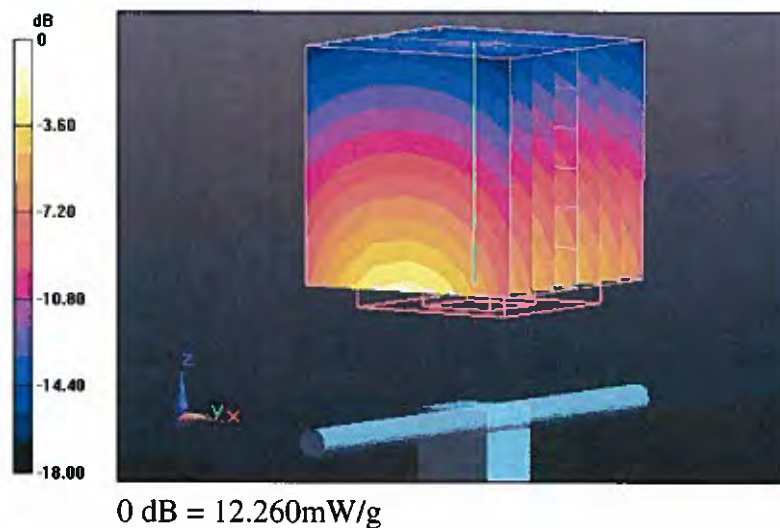


Impedance Measurement Plot for Body TSL

22 Jul 2011 09:24:57
[CH1] S11 1 UFS 1: 43.941 Ω -3.5547 Ω 24.874 pF 1 800.000 000 MHz

*
Del
Cor

Avg
16

H1d

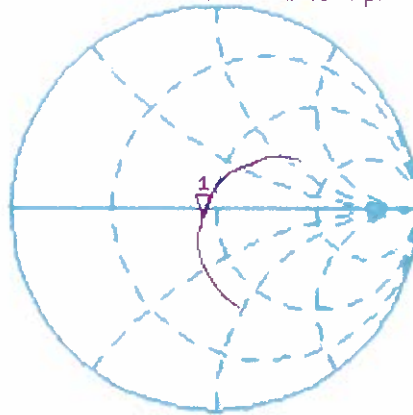


CH2 S11 LOG 5 dB/REF -20 dB 1:-22.534 dB 1 800.000 000 MHz

Cor

Avg
16

H1d

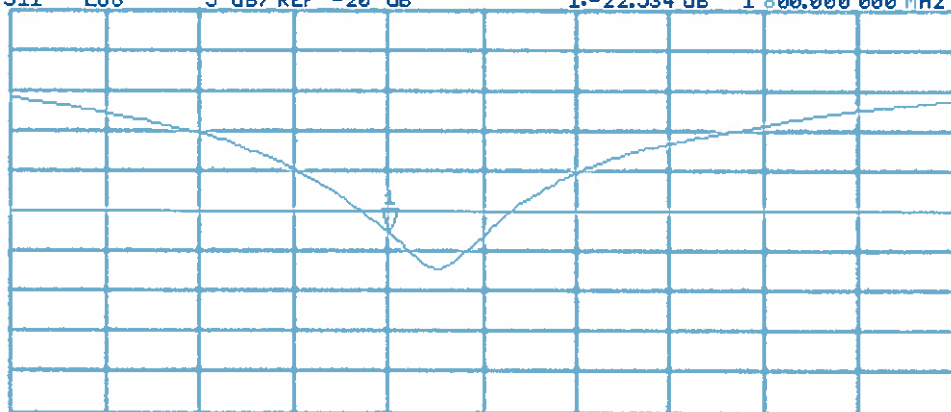

START 1 600.000 000 MHz

STOP 2 100.000 000 MHz

Dipole D1800V2 – SN: 2d063 Antenna Parameters measured: 2012-09-25.


Antenna Parameters with Head TSL

	Calibration certificate	Annual measurement
Impedance, transformed to feed point	48.3 Ω - 3.5 j Ω	47.24 Ω - 6.3 j Ω
Return loss	-28. dB	-23.0 dB


Antenna Parameters with Body TSL

	Calibration certificate	Annual measurement
Impedance, transformed to feed point	43.9 Ω - 3.6 j Ω	43.8 Ω - 5.4 j Ω
Return loss	-22.5 dB	-21.3 dB

Head TSL

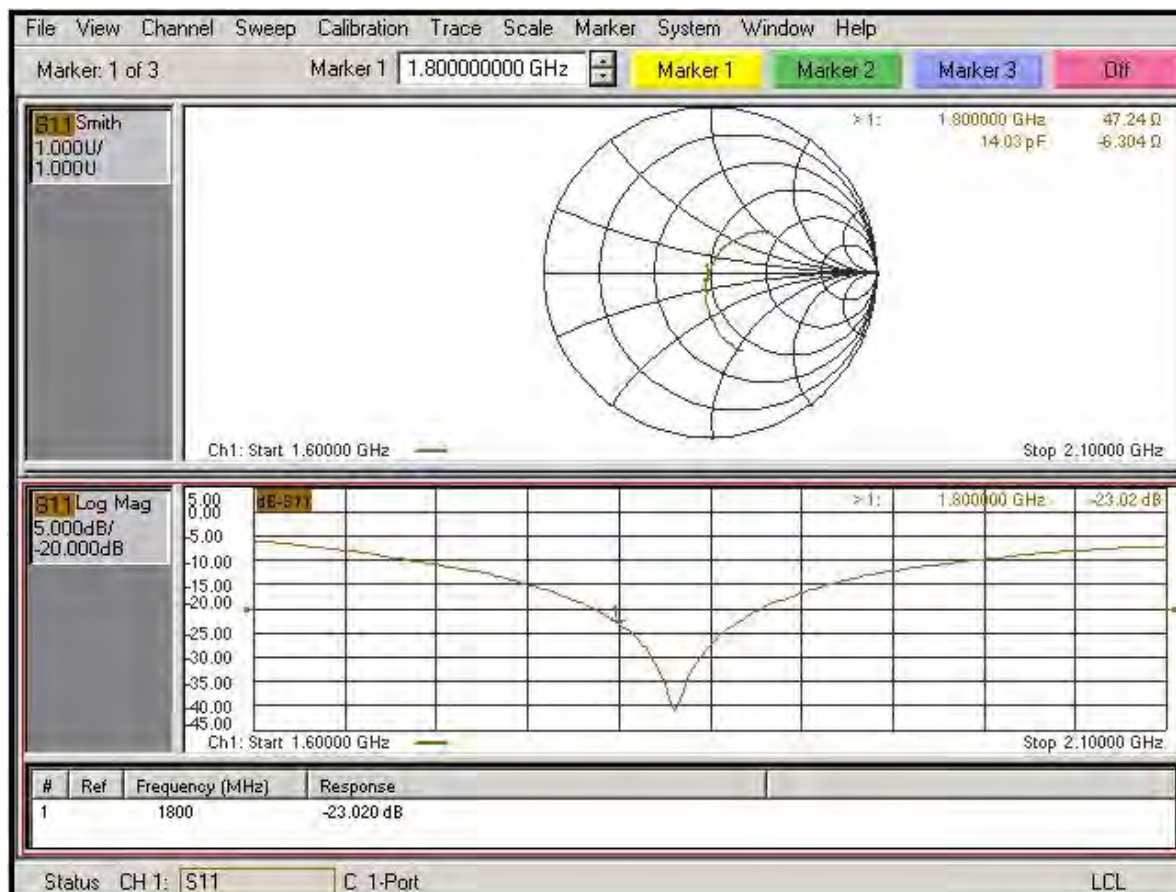

Body TSL

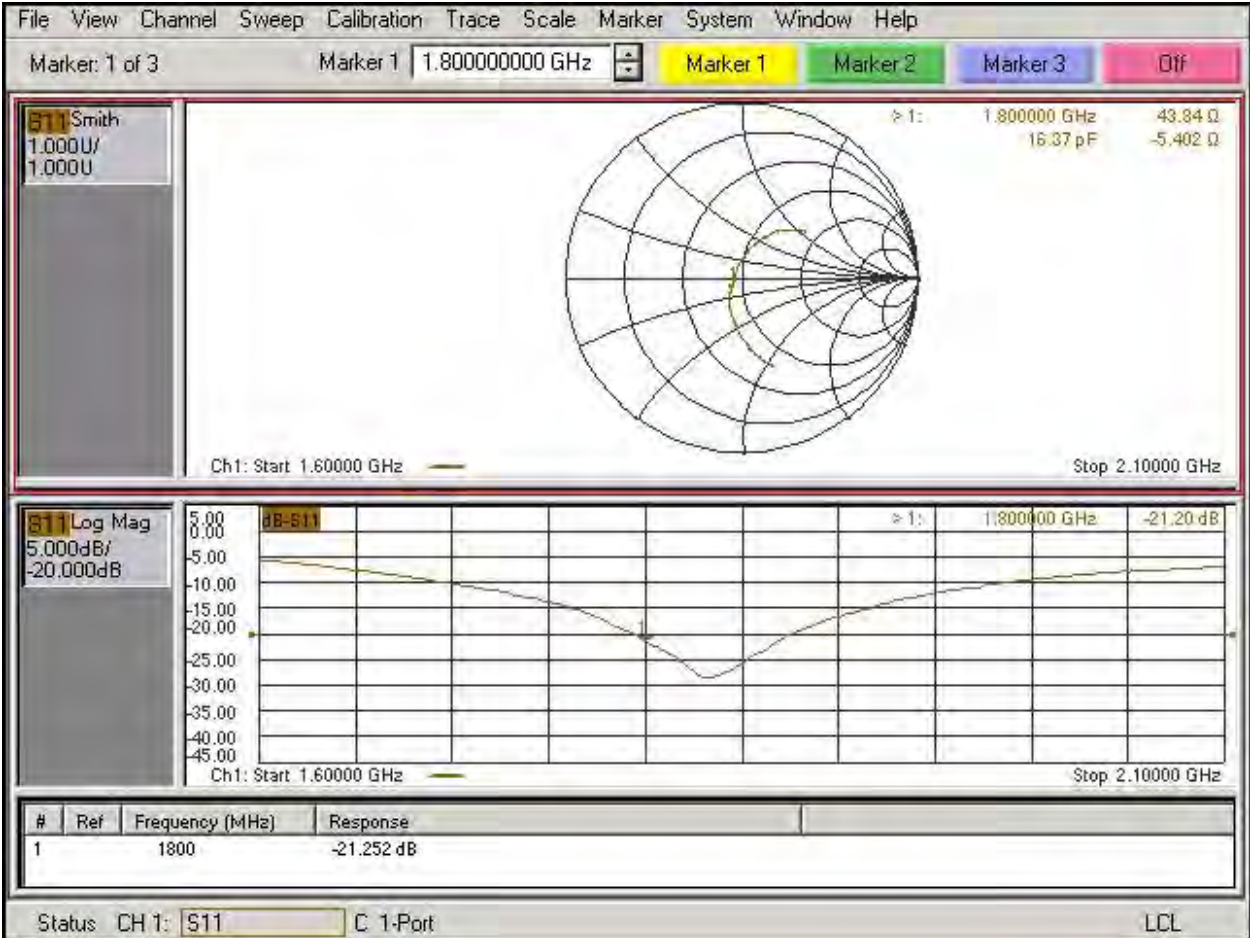



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **Nokia SD**

Certificate No: **D1800V2-215_Aug12**

CALIBRATION CERTIFICATE

Object **D1800V2 - SN: 215**

Calibration procedure(s) **QA CAL-05.v8**
Calibration procedure for dipole validation kits above 700 MHz

Calibration date: **August 09, 2012**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	05-Oct-11 (No. 217-01451)	Oct-12
Power sensor HP 8481A	US37292783	05-Oct-11 (No. 217-01451)	Oct-12
Reference 20 dB Attenuator	SN: 5058 (20k)	27-Mar-12 (No. 217-01530)	Apr-13
Type-N mismatch combination	SN: 5047.2 / 06327	27-Mar-12 (No. 217-01533)	Apr-13
Reference Probe ES3DV3	SN: 3205	30-Dec-11 (No. ES3-3205_Dec11)	Dec-12
DAE4	SN: 601	27-Jun-12 (No. DAE4-601_Jun12)	Jun-13
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-11)	In house check: Oct-12

Calibrated by: **Israe El-Naouq** **Function**
Laboratory Technician

Signature

Approved by: **Katja Pokovic** **Technical Manager**

Issued: August 10, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1800 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	39.8 $\pm$ 6 %	1.38 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.31 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	37.5 mW / g $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	4.94 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	19.9 mW / g $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	52.0 $\pm$ 6 %	1.52 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.62 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	38.3 mW / g $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.11 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	20.4 mW / g $\pm$ 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.1 Ω - 4.2 j Ω
Return Loss	- 26.4 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	44.6 Ω - 3.8 j Ω
Return Loss	- 23.1 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.210 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	November 12, 1997

DASY5 Validation Report for Head TSL

Date: 09.08.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 215

Communication System: CW; Frequency: 1800 MHz

Medium parameters used: $f = 1800$ MHz; $\sigma = 1.38$ mho/m; $\epsilon_r = 39.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.07, 5.07, 5.07); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.2(969); SEMCAD X 14.6.6(6824)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.817 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 16.462 mW/g

SAR(1 g) = 9.31 mW/g; SAR(10 g) = 4.94 mW/g

Maximum value of SAR (measured) = 11.4 W/kg

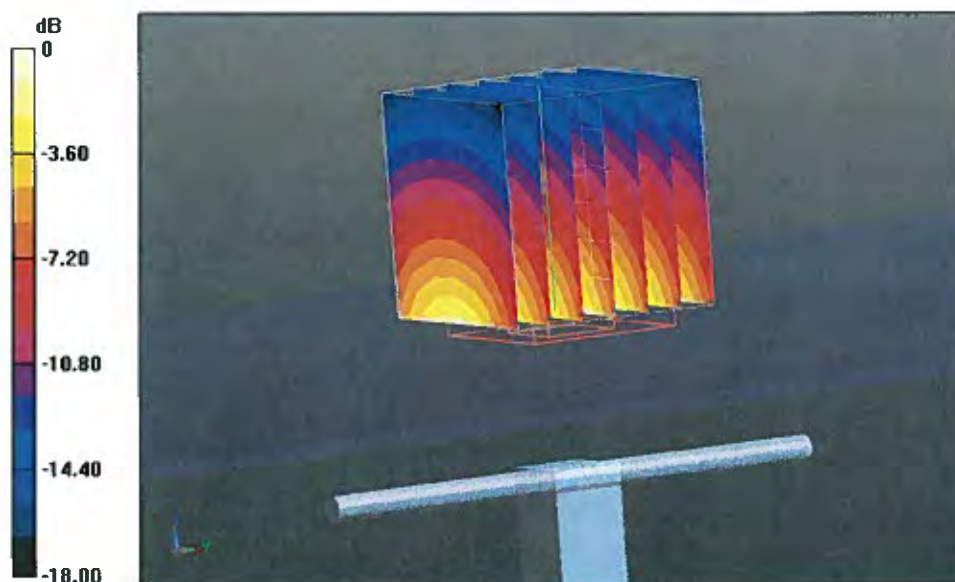

0 dB = 11.4 W/kg = 21.14 dB W/kg


Impedance Measurement Plot for Head TSL

9 Aug 2012 13:29:11
 [CH1] S11 1 U FS 2: 48.061 Ω -4.2480 Ω 20.814 pF 1 800.000 000 MHz

*
 De1
 Ca

Avg
 16

H1d

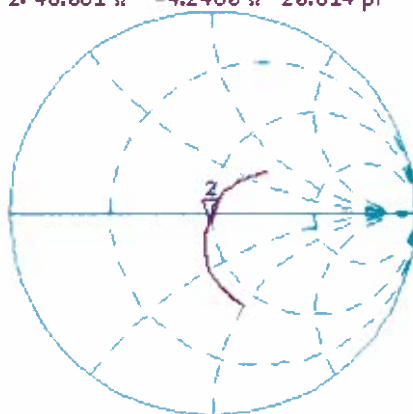


CH2 S11 LOG 5 dB/REF -20 dB 2:-26.448 dB 1 800.000 000 MHz

Ca

Avg
 16

H1d

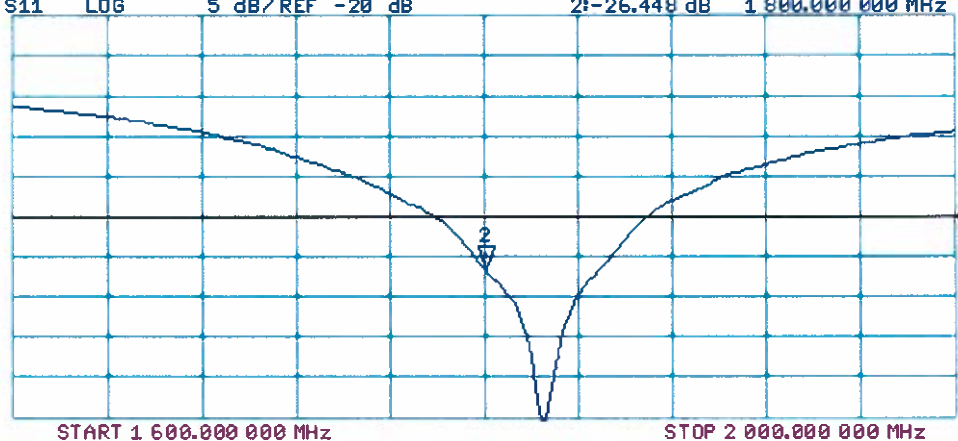

DASY5 Validation Report for Body TSL

Date: 09.08.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 215

Communication System: CW; Frequency: 1800 MHz

Medium parameters used: $f = 1800$ MHz; $\sigma = 1.52$ mho/m; $\epsilon_r = 52$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.74, 4.74, 4.74); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.2(969); SEMCAD X 14.6.6(6824)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 92.802 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 16.905 mW/g

SAR(1 g) = 9.62 mW/g; SAR(10 g) = 5.11 mW/g

Maximum value of SAR (measured) = 12.1 W/kg

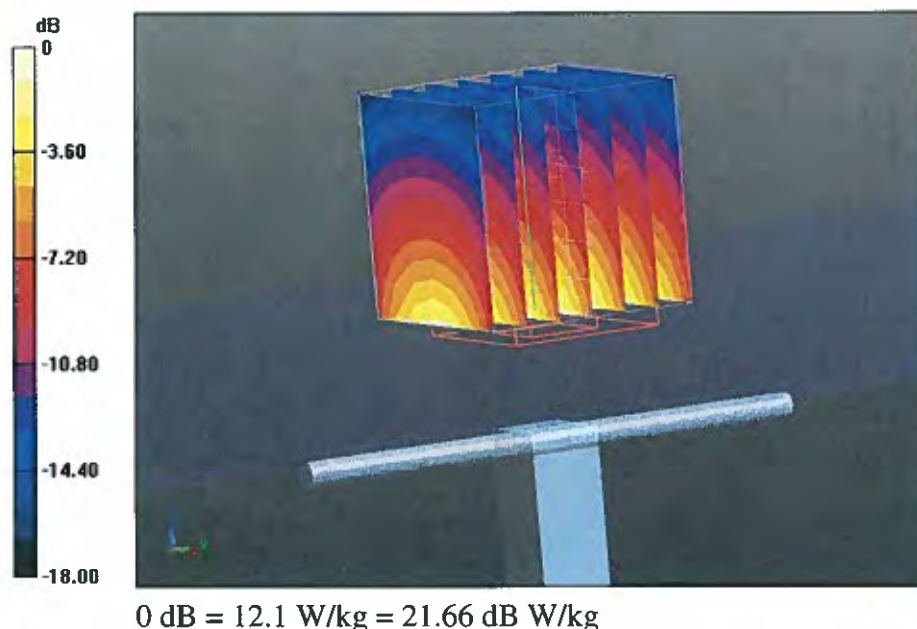

Impedance Measurement Plot for Body TSL

9 Aug 2012 13:28:39
[CH1] S11 1 U FS 2: 44.590 Ω -3.7773 Ω 23.408 pF 1 800.000 000 MHz


*

De1

CA

Avg
16

H1d

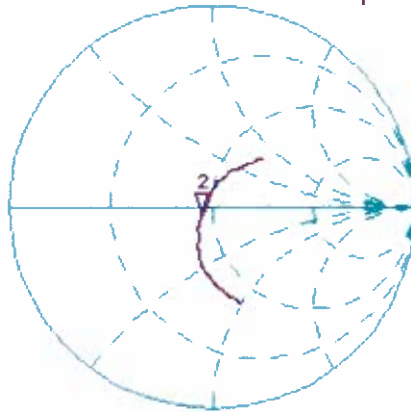


CH2 S11 LOG 5 dB/REF -20 dB 2: -23.136 dB 1 800.000 000 MHz

CA

Avg
15

H1d

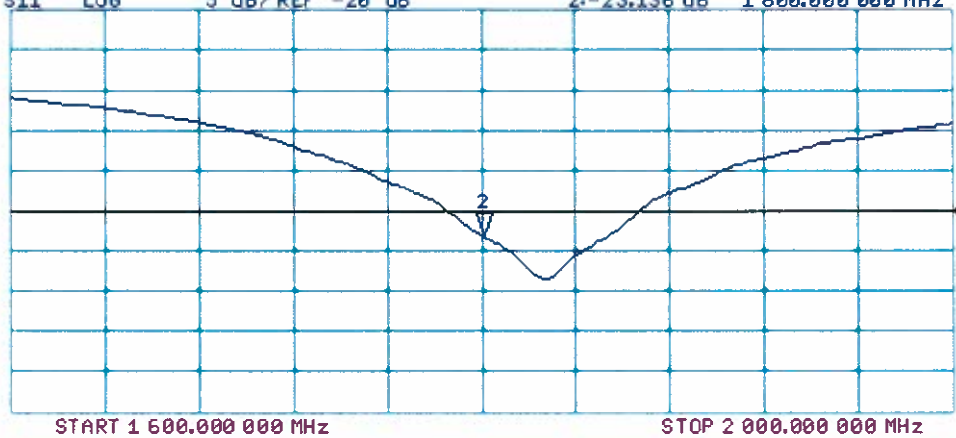

7324

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Client **Nokia SD**

Certificate No: **D1900V2-5d099_Sep11**

CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d099**

Calibration procedure(s) **QA CAL-05.v8**
Calibration procedure for dipole validation kits above 700 MHz

Calibration date: **September 15, 2011**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37292783	06-Oct-10 (No. 217-01266)	Oct-11
Reference 20 dB Attenuator	SN: S5086 (20b)	29-Mar-11 (No. 217-01367)	Apr-12
Type-N mismatch combination	SN: 5047.2 / 06327	29-Mar-11 (No. 217-01371)	Apr-12
Reference Probe ES3DV3	SN: 3205	29-Apr-11 (No. ES3-3205_Apr11)	Apr-12
DAE4	SN: 601	04-Jul-11 (No. DAE4-601_Jul11)	Jul-12
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

Calibrated by: **Dimce Iliev** **Function** **Laboratory Technician** **Signature** *D. Iliev*

Approved by: **Katja Pokovic** **Technical Manager** *K. Pokovic*

Issued: September 15, 2011

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.6.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	39.6 $\pm$ 6 %	1.43 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.1 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	39.8 mW / g $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.26 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	20.9 mW / g $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	54.2 $\pm$ 6 %	1.59 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.6 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	41.4 mW / g $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.56 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	22.0 mW / g $\pm$ 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$50.9 \Omega + 6.4 j\Omega$
Return Loss	- 23.9 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$46.3 \Omega + 6.8 j\Omega$
Return Loss	- 22.0 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.203 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	September 26, 2007

DASY5 Validation Report for Head TSL

Date: 15.09.2011

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d099

Communication System: CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.43$ mho/m; $\epsilon_r = 39.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.01, 5.01, 5.01); Calibrated: 29.04.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 98.201 V/m; Power Drift = 0.03 dB


Peak SAR (extrapolated) = 18.370 W/kg

SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.26 mW/g

Maximum value of SAR (measured) = 12.759 mW/g



Impedance Measurement Plot for Head TSL

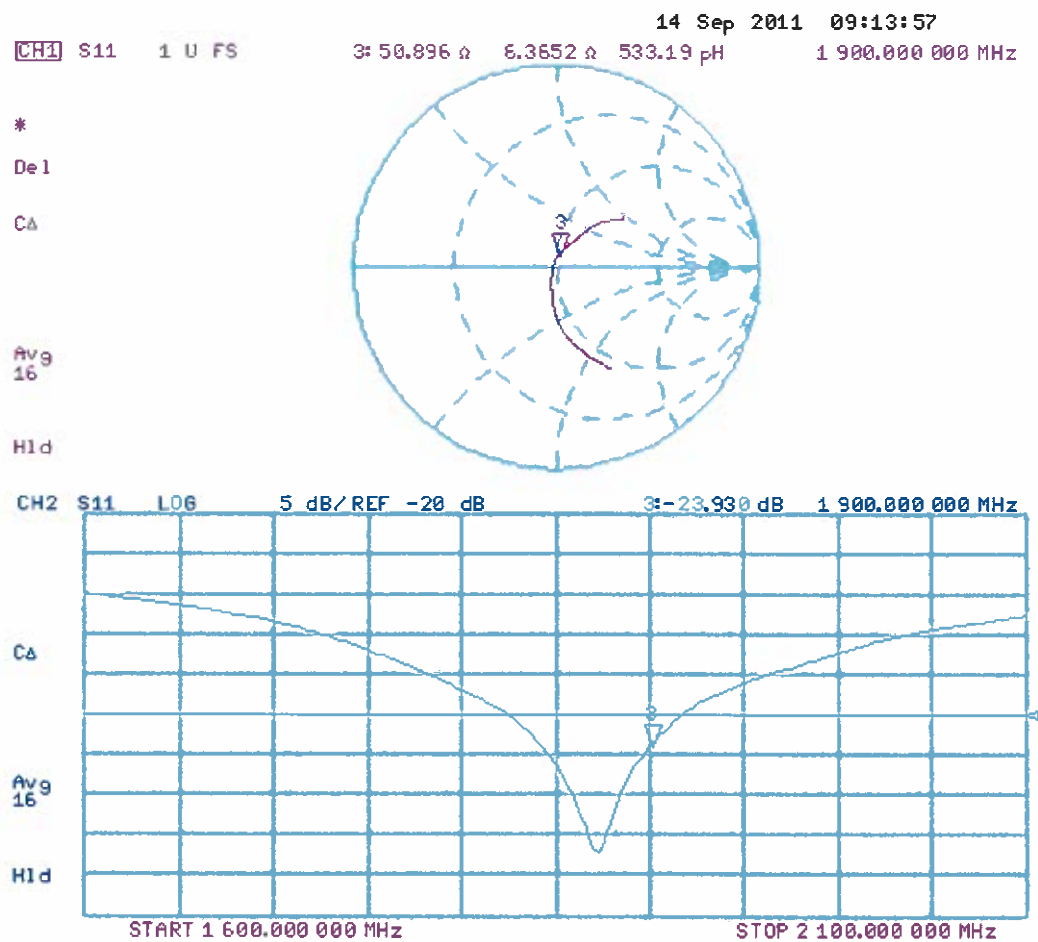

DASY5 Validation Report for Body TSL

Date: 14.09.2011

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d099

Communication System: CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.59$ mho/m; $\epsilon_r = 54.2$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.62, 4.62, 4.62); Calibrated: 29.04.2011
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.6.2(482); SEMCAD X 14.4.5(3634)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.840 V/m; Power Drift = 0.00072 dB

Peak SAR (extrapolated) = 18.707 W/kg


SAR(1 g) = 10.6 mW/g; SAR(10 g) = 5.56 mW/g

Maximum value of SAR (measured) = 13.461 mW/g

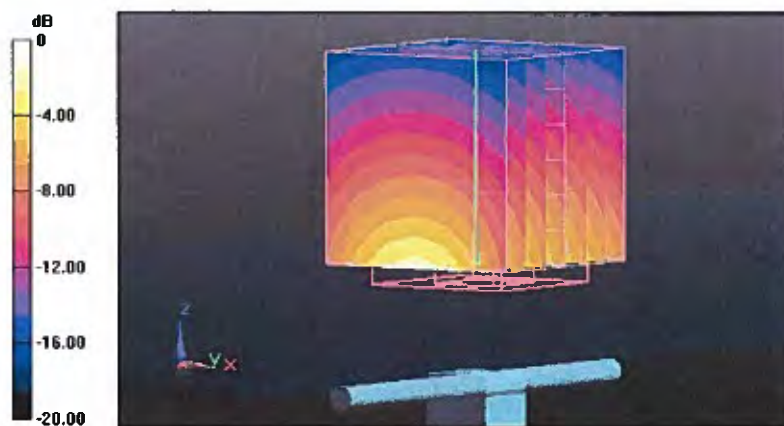

0 dB = 13.460mW/g

Impedance Measurement Plot for Body TSL

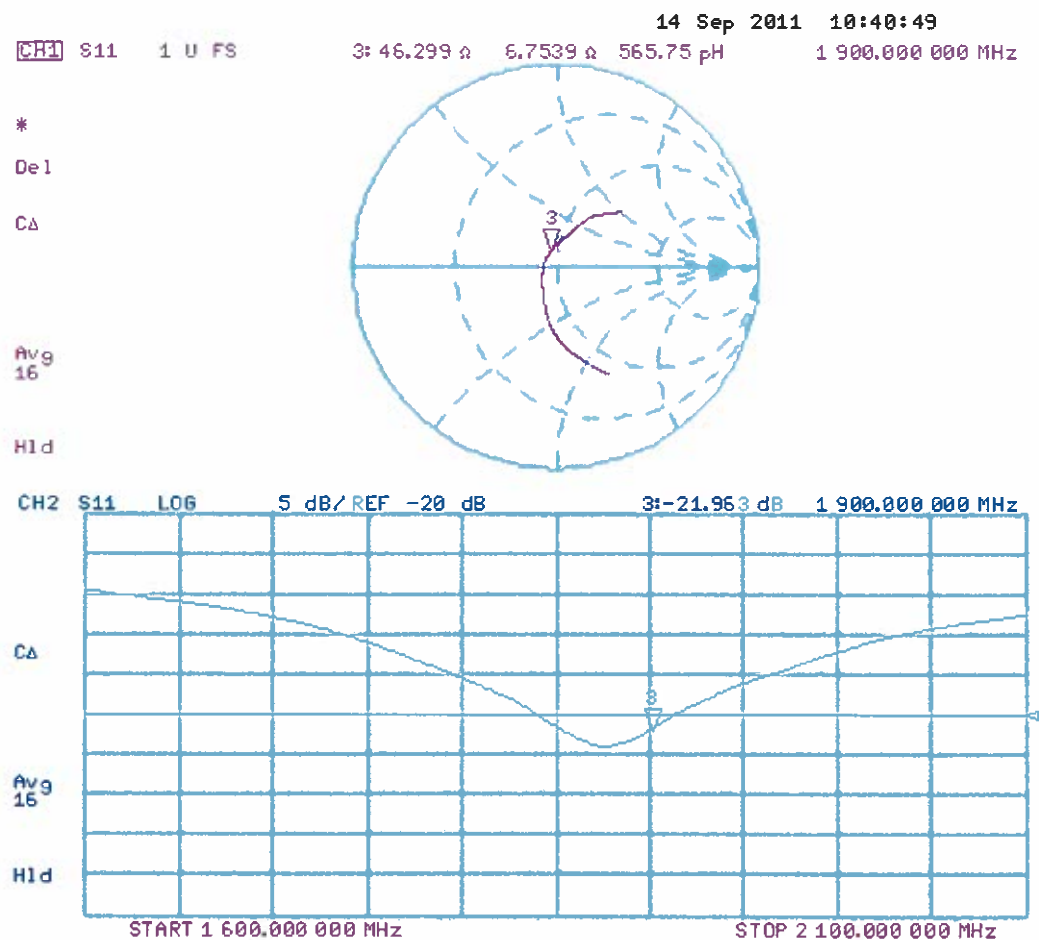

Dipole D1900V2 – SN: 5d099 Antenna Parameters measured: 2012-09-25.


Antenna Parameters with Head TSL

	Calibration certificate	Annual measurement
Impedance, transformed to feed point	50.9 Ω + 6.4 j Ω	48.5 Ω + 3.8 j Ω
Return loss	-23.9 dB	-27.6 dB


Antenna Parameters with Body TSL

	Calibration certificate	Annual measurement
Impedance, transformed to feed point	46.3 Ω + 6.8 j Ω	45.0 Ω + 4.3 j Ω
Return loss	-22.0 dB	-23.1 dB

Head TSL

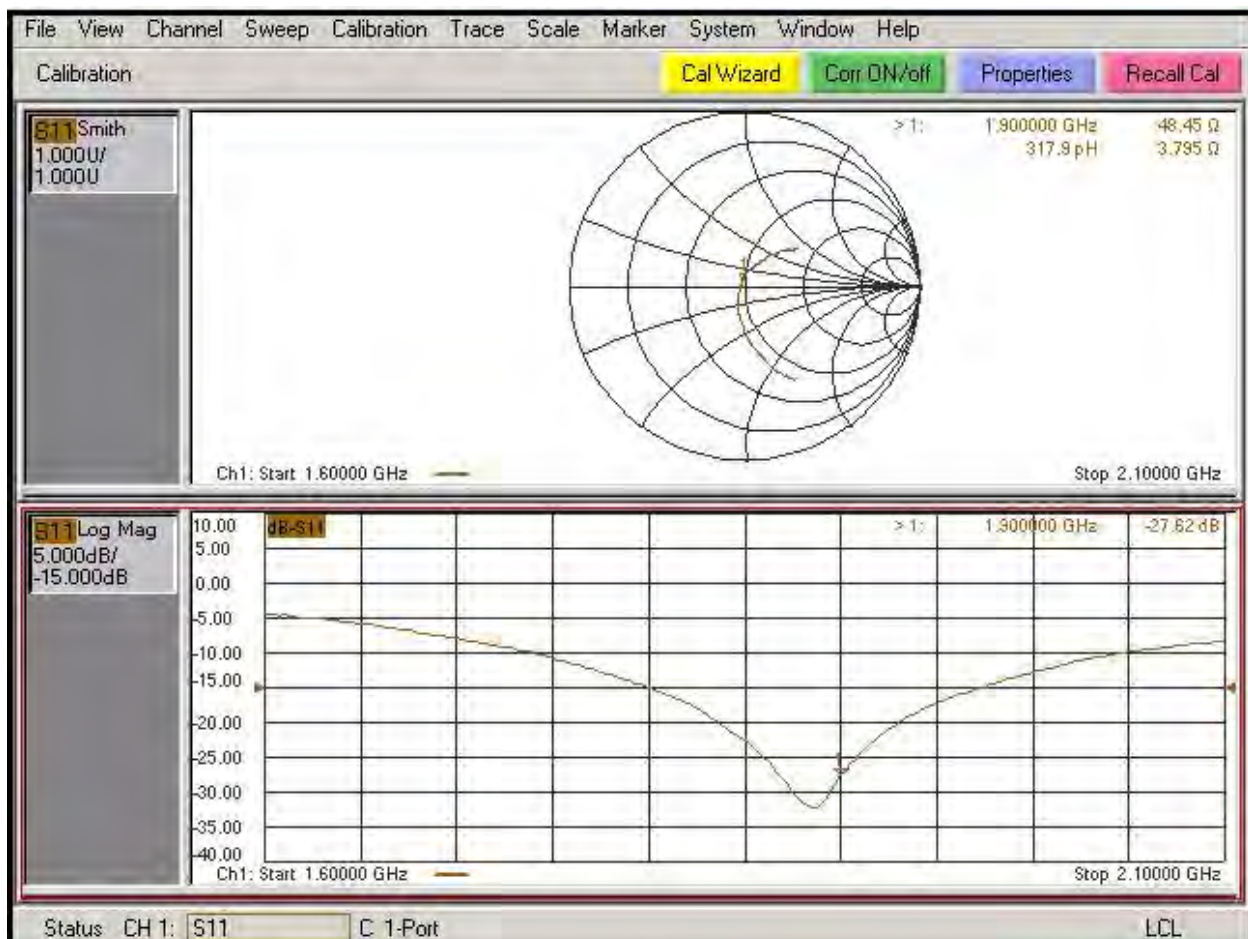

Body TSL

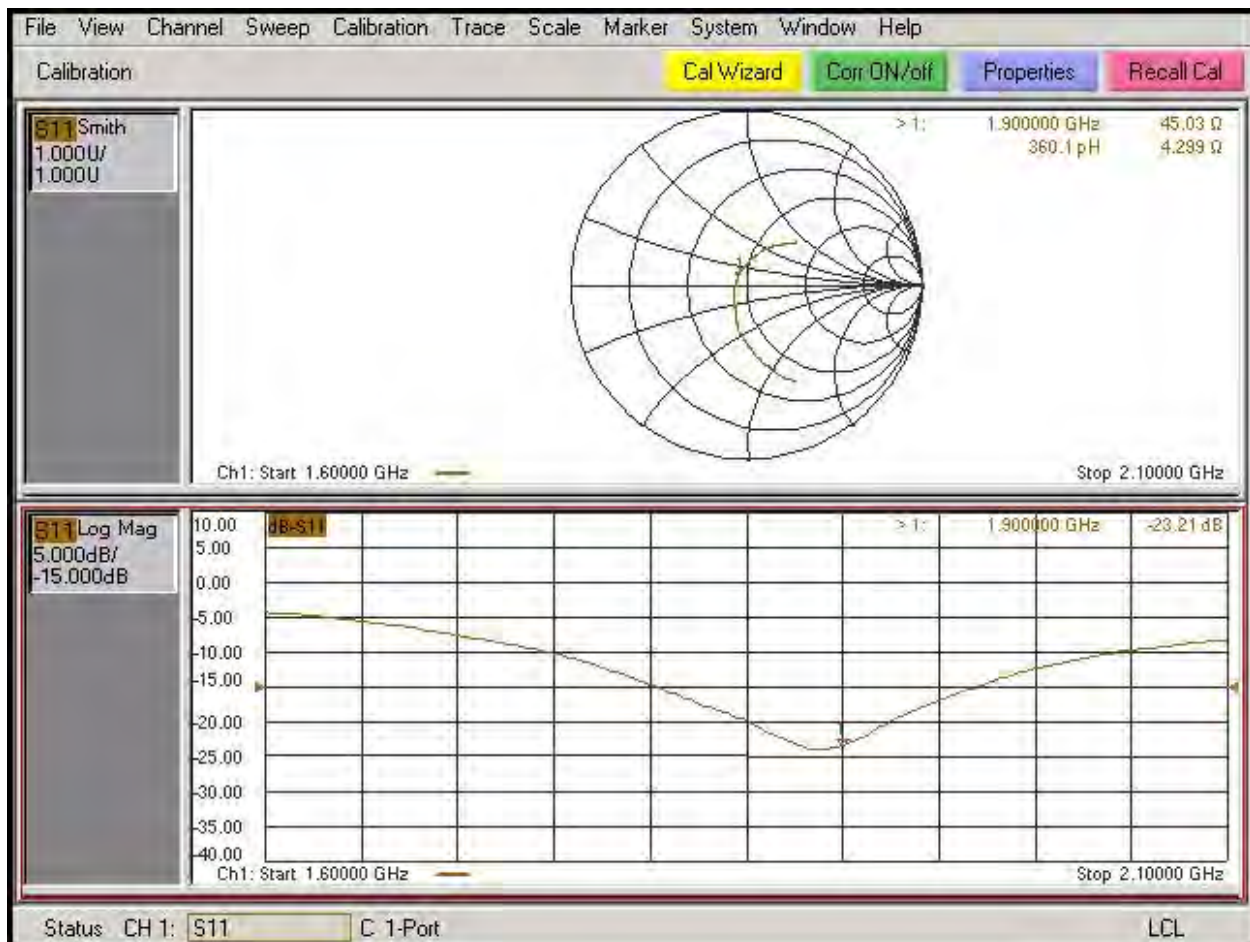

6048

Calibration Laboratory of
Schmid & Partner
Engineering AG
 Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Nokia SD**

Certificate No: **D1900V2-534_Sep12**

CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 534**

Calibration procedure(s) **QA CAL-05.v8**
 Calibration procedure for dipole validation kits above 700 MHz

Calibration date: **September 14, 2012**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	05-Oct-11 (No. 217-01451)	Oct-12
Power sensor HP 8481A	US37292783	05-Oct-11 (No. 217-01451)	Oct-12
Reference 20 dB Attenuator	SN: 5058 (20k)	27-Mar-12 (No. 217-01530)	Apr-13
Type-N mismatch combination	SN: 5047.2 / 06327	27-Mar-12 (No. 217-01533)	Apr-13
Reference Probe ES3DV3	SN: 3205	30-Dec-11 (No. ES3-3205_Dec11)	Dec-12
DAE4	SN: 601	27-Jun-12 (No. DAE4-601_Jun12)	Jun-13
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-11)	In house check: Oct-12

Calibrated by: **Jeton Kastrati** Name: **Jeton Kastrati** Function: **Laboratory Technician**

Approved by: **Katja Pokovic** Technical Manager

Signature

Issued: September 14, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	40.6 $\pm$ 6 %	1.37 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	9.64 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	39.2 mW / g $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.11 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	20.6 mW / g $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 $\pm$ 0.2) °C	52.5 $\pm$ 6 %	1.54 mho/m $\pm$ 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.1 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	40.0 mW / g $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.34 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	21.2 mW / g $\pm$ 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$52.0\ \Omega + 4.5\ j\Omega$
Return Loss	- 26.3 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$47.6\ \Omega + 4.5\ j\Omega$
Return Loss	- 25.6 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.204 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	January 31, 2001

DASY5 Validation Report for Head TSL

Date: 14.09.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 534

Communication System: CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.37$ mho/m; $\epsilon_r = 40.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(5.01, 5.01, 5.01); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.2(969); SEMCAD X 14.6.6(6824)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.550 V/m; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 17.069 mW/g

SAR(1 g) = 9.64 mW/g; SAR(10 g) = 5.11 mW/g

Maximum value of SAR (measured) = 11.8 W/kg

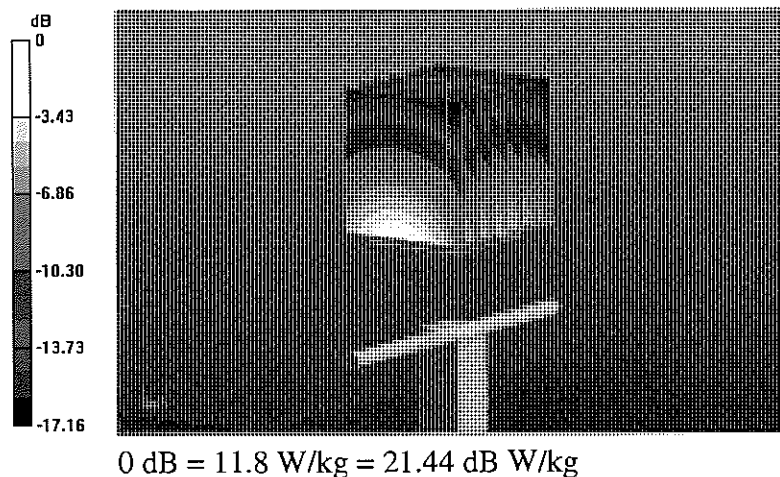

Impedance Measurement Plot for Head TSL

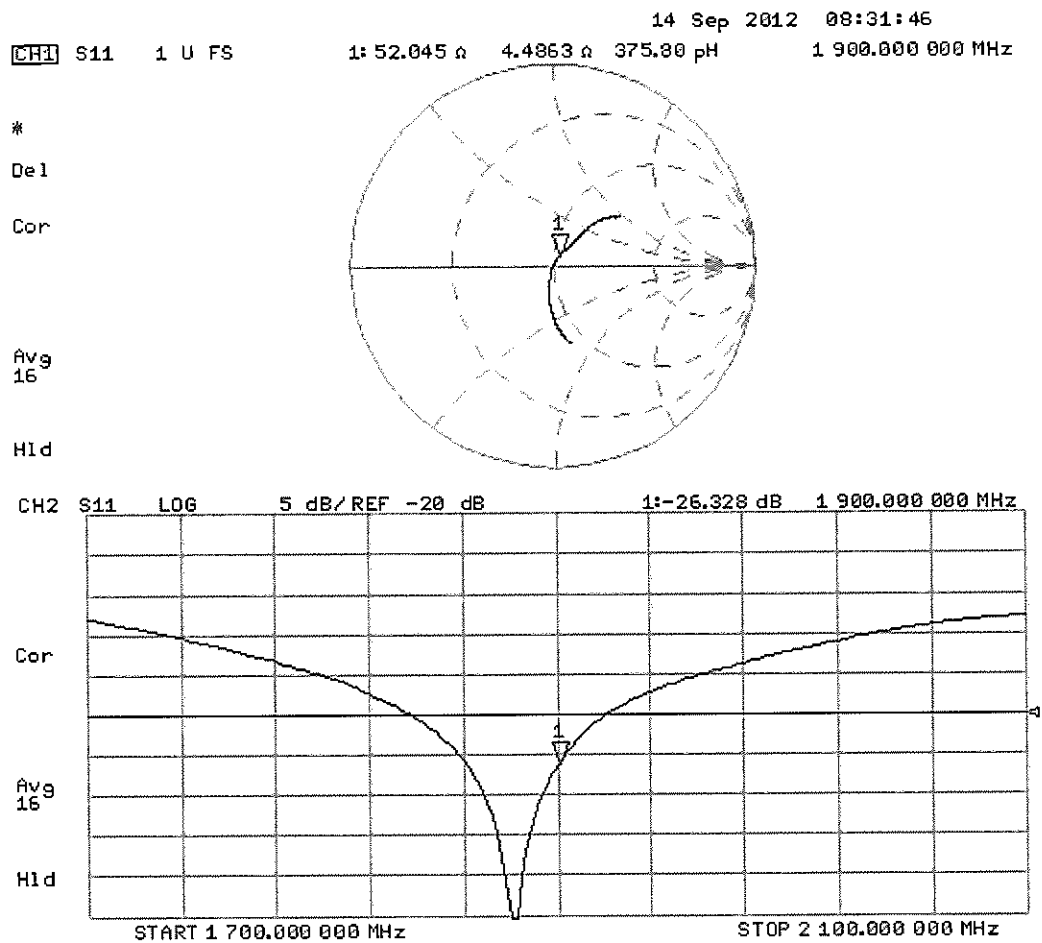

DASY5 Validation Report for Body TSL

Date: 14.09.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 534

Communication System: CW; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.54$ mho/m; $\epsilon_r = 52.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.62, 4.62, 4.62); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 27.06.2012
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.2(969); SEMCAD X 14.6.6(6824)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.550 V/m; Power Drift = 0.02 dB


Peak SAR (extrapolated) = 17.586 mW/g

SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.34 mW/g

Maximum value of SAR (measured) = 12.7 W/kg

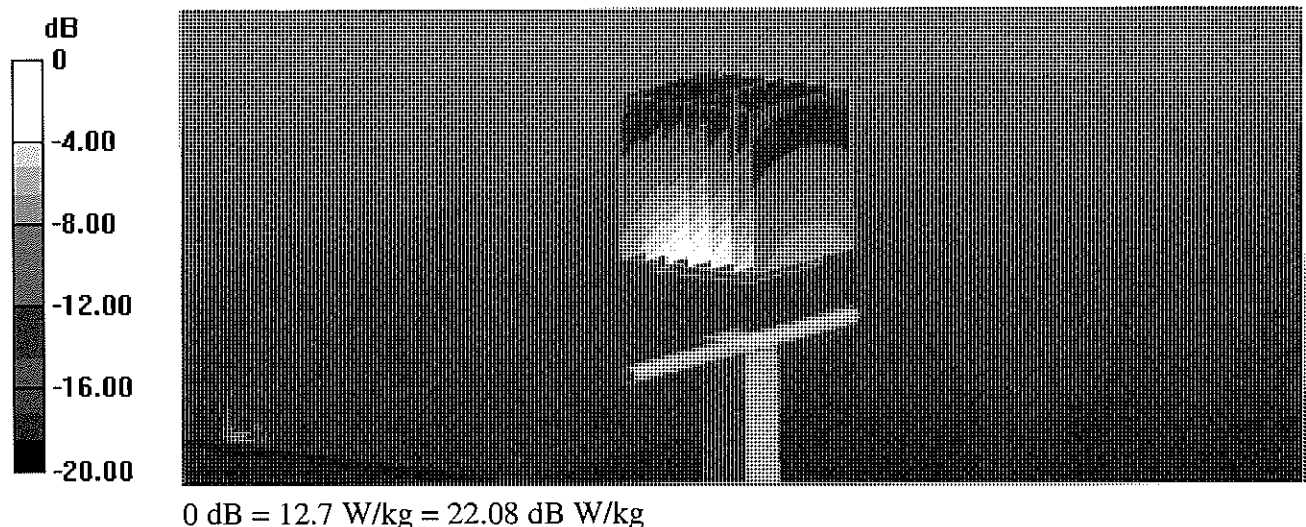

Impedance Measurement Plot for Body TSL

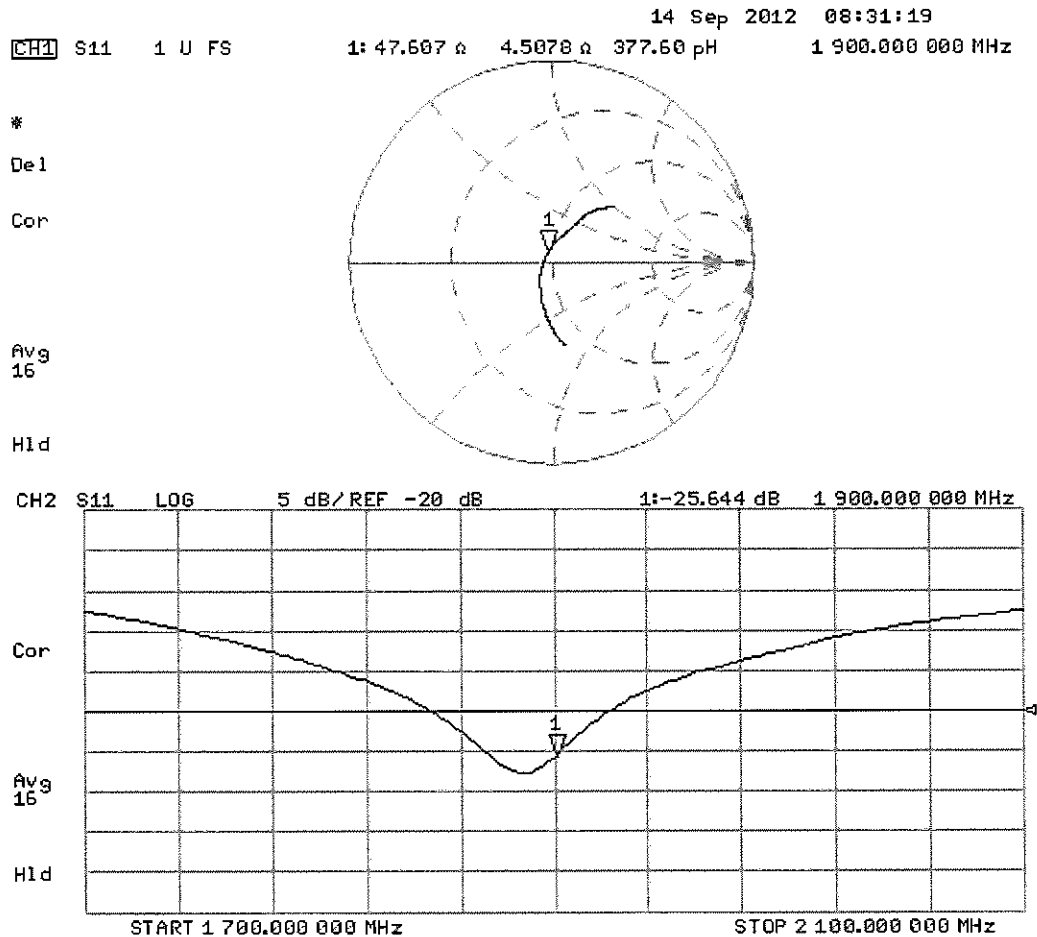



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
 Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **Nokia Oulu TCC**

Certificate No: **D2450V2-758_Nov10**

CALIBRATION CERTIFICATE

Object **D2450V2 - SN: 758**

Calibration procedure(s) **QA CAL-05.v7**
Calibration procedure for dipole validation kits

Calibration date: **November 11, 2010**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
 The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	06-Oct-10 (No. 217-01266)	Oct-11
Power sensor HP 8481A	US37292783	06-Oct-10 (No. 217-01266)	Oct-11
Reference 20 dB Attenuator	SN: 5086 (20g)	30-Mar-10 (No. 217-01158)	Mar-11
Type-N mismatch combination	SN: 5047.2 / 06327	30-Mar-10 (No. 217-01162)	Mar-11
Reference Probe ES3DV3	SN: 3205	30-Apr-10 (No. ES3-3205_Apr10)	Apr-11
DAE4	SN: 601	10-Jun-10 (No. DAE4-601_Jun10)	Jun-11
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-09)	In house check: Oct-11
RF generator R&S SMT-06	100005	4-Aug-99 (in house check Oct-09)	In house check: Oct-11
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-10)	In house check: Oct-11

Calibrated by:	Name Jeton Kastrati	Function Laboratory Technician
Approved by:	Katja Pokovic	Technical Manager

Signature



Issued: November 12, 2010

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz $\pm$ 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	38.8 $\pm$ 6 %	1.72 mho/m $\pm$ 6 %
Head TSL temperature during test	(22.5 $\pm$ 0.2) °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.0 mW / g
SAR normalized	normalized to 1W	52.0 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	53.0 mW /g $\pm$ 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.10 mW / g
SAR normalized	normalized to 1W	24.4 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.5 mW /g $\pm$ 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.3 ± 6 %	1.92 mho/m ± 6 %
Body TSL temperature during test	(22.0 ± 0.2) °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.6 mW / g
SAR normalized	normalized to 1W	50.4 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	50.7 mW / g ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.83 mW / g
SAR normalized	normalized to 1W	23.3 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	23.3 mW / g ± 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	$55.4 \Omega + 5.0 j\Omega$
Return Loss	- 23.1 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	$50.9 \Omega + 7.6 j\Omega$
Return Loss	- 22.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.157 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	April 22, 2004

DASY5 Validation Report for Head TSL

Date/Time: 11.11.2010 11:06:34

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:758

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: HSL U12 BB

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.72$ mho/m; $\epsilon_r = 38.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- Measurement SW: DASY52, V52.2 Build 0, Version 52.2.0 (163)
- Postprocessing SW: SEMCAD X, V14.2 Build 2, Version 14.2.2 (1685)


Pin=250 mW/d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7)/Cube 0: Measurement
grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 102.3 V/m; Power Drift = 0.050 dB

Peak SAR (extrapolated) = 26.5 W/kg


SAR(1 g) = 13 mW/g; SAR(10 g) = 6.1 mW/g

Maximum value of SAR (measured) = 16.7 mW/g

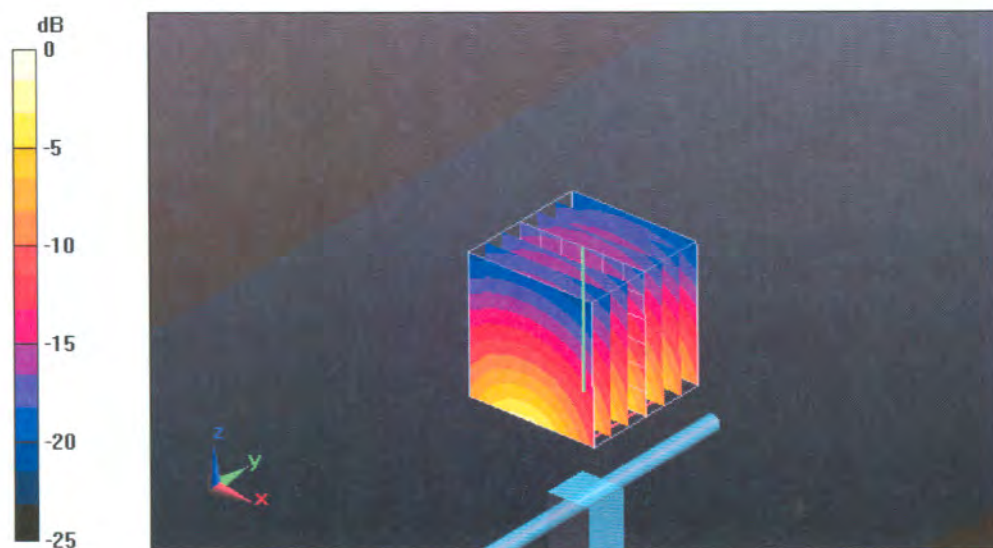

0 dB = 16.7mW/g

Impedance Measurement Plot for Head TSL

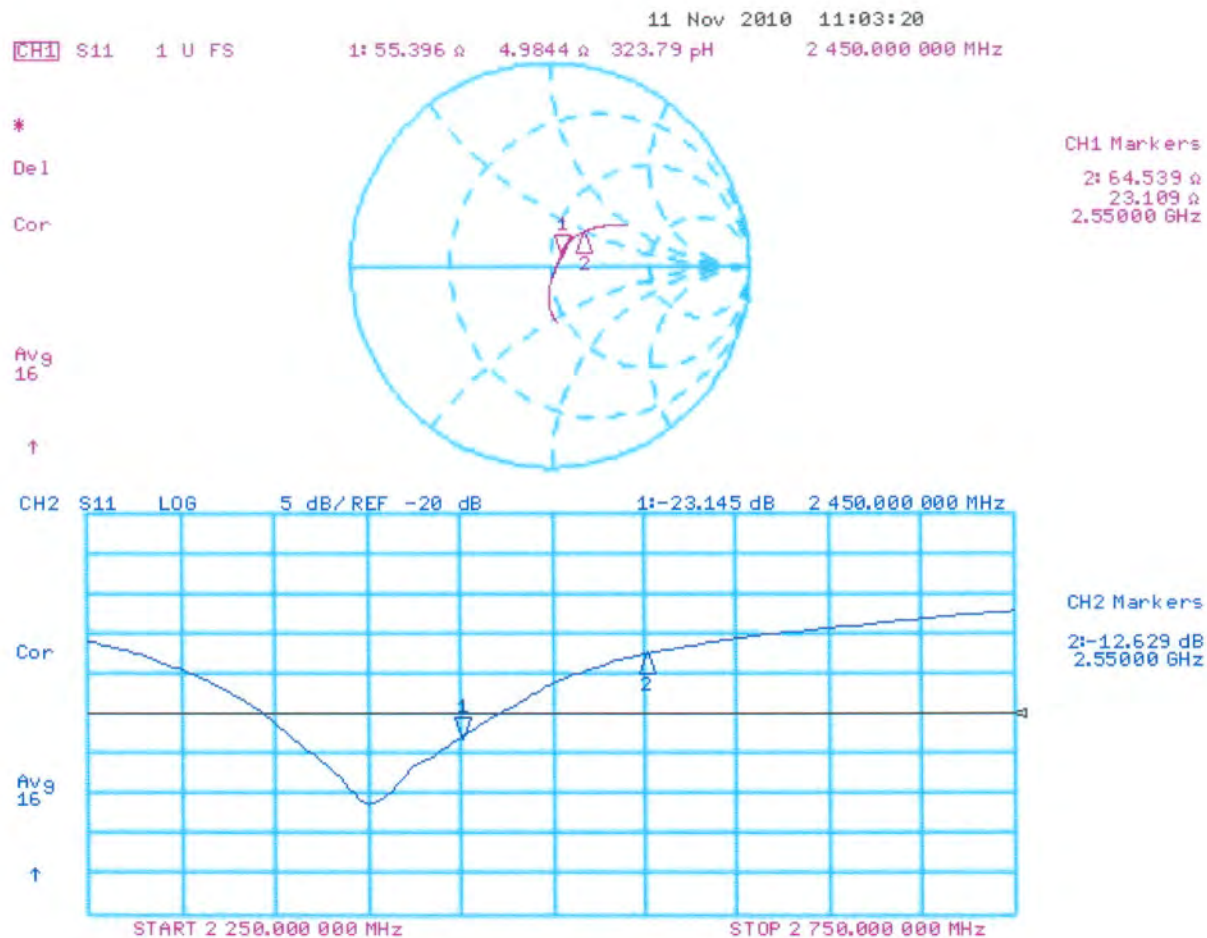

DASY5 Validation Report for Body

Date/Time: 11.11.2010 13:37:58

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:758

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: MSL U12 BB

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.92$ mho/m; $\epsilon_r = 52.3$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.31, 4.31, 4.31); Calibrated: 30.04.2010
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 10.06.2010
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- Measurement SW: DASY52, V52.2 Build 0, Version 52.2.0 (163)
- Postprocessing SW: SEMCAD X, V14.2 Build 2, Version 14.2.2 (1685)

Pin=250 mW /d=10mm, dist=3.0mm (ES-Probe)/Zoom Scan (7x7x7)/Cube 0: Measurement
grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.5 V/m; Power Drift = 0.00833 dB

Peak SAR (extrapolated) = 26.3 W/kg


SAR(1 g) = 12.6 mW/g; SAR(10 g) = 5.83 mW/g

Maximum value of SAR (measured) = 16.4 mW/g



0 dB = 16.4mW/g

Impedance Measurement Plot for Body TSL

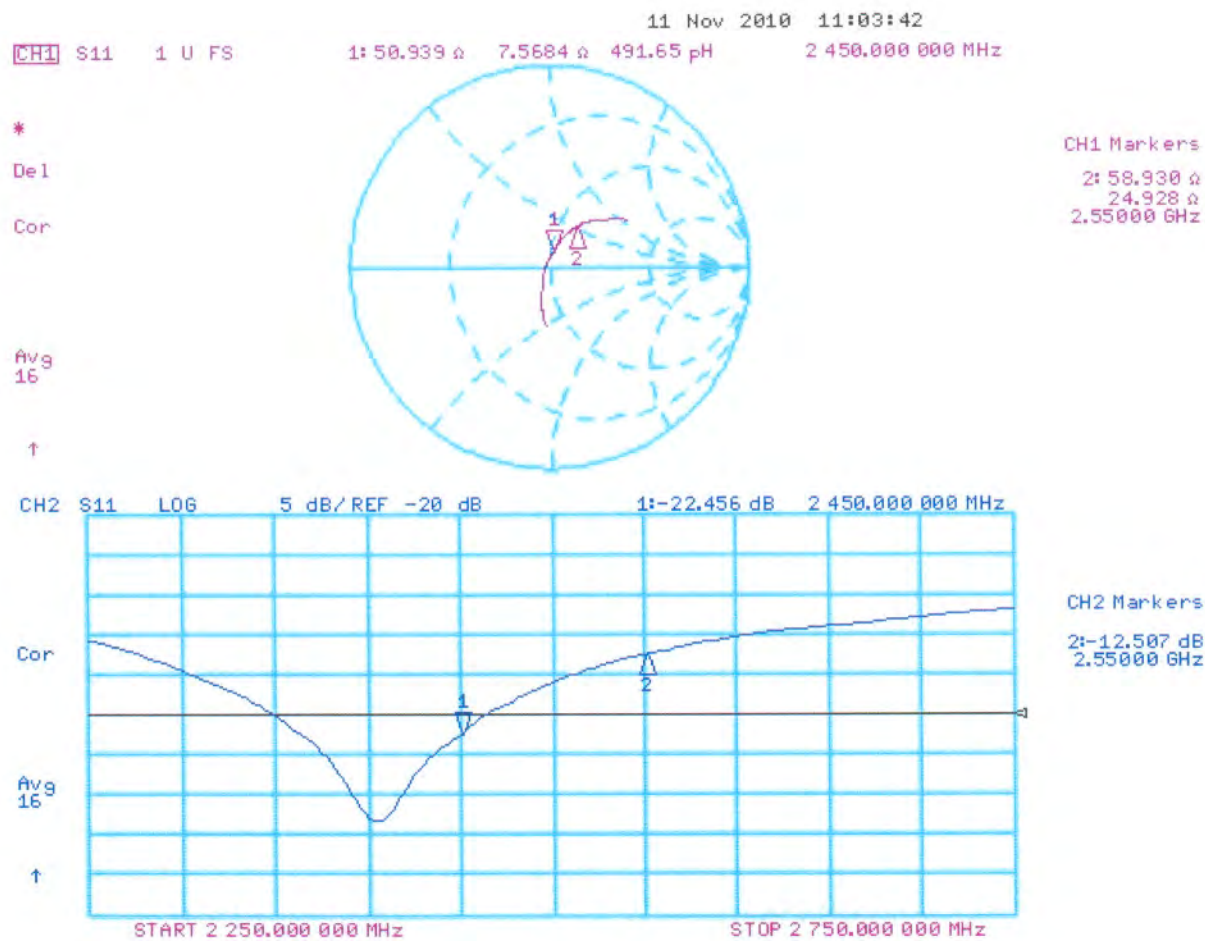

Dipole D2450V2 – SN: 758 Antenna Parameters measured: 2012-09-25.


Antenna Parameters with Head TSL

	Calibration certificate	2-year measurement
Impedance, transformed to feed point	55.4 Ω + 5.0 j Ω	54.4 Ω - 5.3 j Ω
Return loss	-23.1 dB	-23.6 dB


Antenna Parameters with Body TSL

	Calibration certificate	2-year measurement
Impedance, transformed to feed point	50.9 Ω + 7.6 j Ω	51.6 Ω - 8.6 j Ω
Return loss	-22.5 dB	-21.3 dB

Head TSL

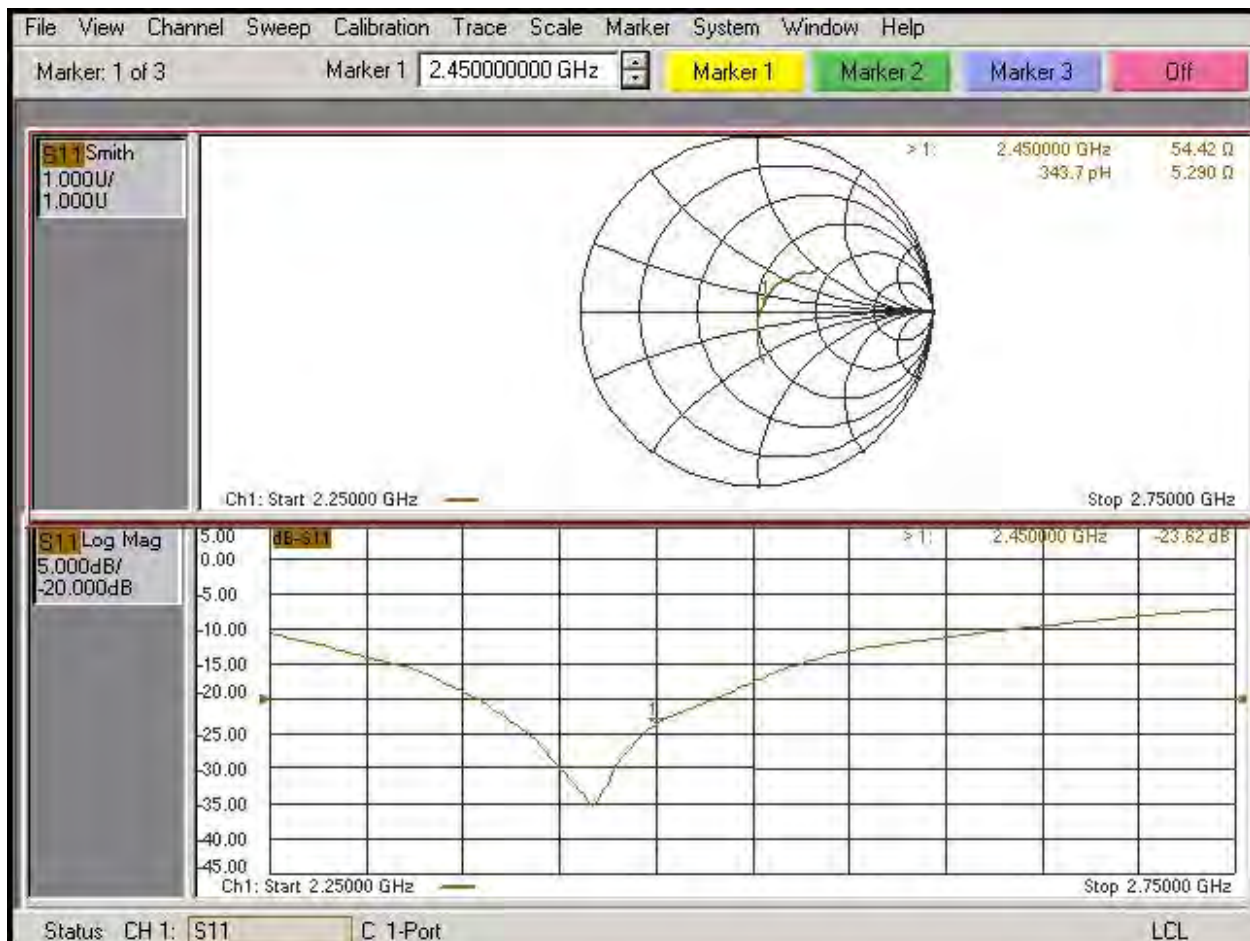

Body TSL

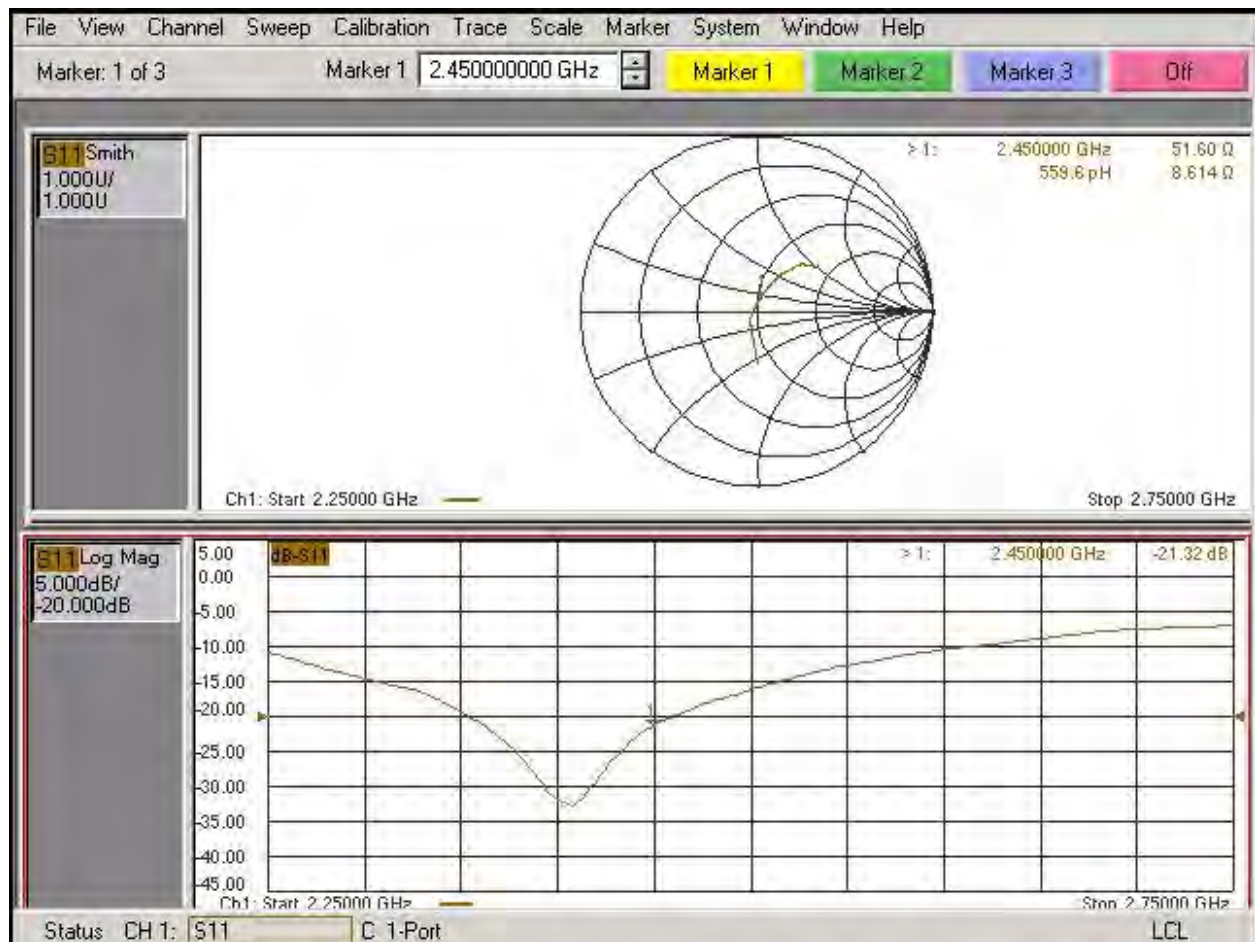



**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client **Nokia SD**

Certificate No: **D5GHzV2-1123_May12**

CALIBRATION CERTIFICATE

Object **D5GHzV2 - SN: 1123**

Calibration procedure(s) **QA CAL-22.v1
Calibration procedure for dipole validation kits between 3-6 GHz**

Calibration date: **May 04, 2012**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}\text{C}$ and humidity $< 70\%$.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	05-Oct-11 (No. 217-01451)	Oct-12
Power sensor HP 8481A	US37292783	05-Oct-11 (No. 217-01451)	Oct-12
Reference 20 dB Attenuator	SN: 5058 (20k)	27-Mar-12 (No. 217-01530)	Apr-13
Type-N mismatch combination	SN: 5047.2 / 06327	27-Mar-12 (No. 217-01533)	Apr-13
Reference Probe EX3DV4	SN: 3503	30-Dec-11 (No. EX3-3503_Dec11)	Dec-12
DAE4	SN: 601	04-Jul-11 (No. DAE4-601_Jul11)	Jul-12
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power sensor HP 8481A	MY41092317	18-Oct-02 (in house check Oct-11)	In house check: Oct-13
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-11)	In house check: Oct-13
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-11)	In house check: Oct-12

Calibrated by:	Name Israe El-Naouq	Function Laboratory Technician	Signature
Approved by:	Katja Pokovic	Technical Manager	

Issued: May 7, 2012

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEC 62209-2, "Evaluation of Human Exposure to Radio Frequency Fields from Handheld and Body-Mounted Wireless Communication Devices in the Frequency Range of 30 MHz to 6 GHz: Human models, Instrumentation, and Procedures"; Part 2: "Procedure to determine the Specific Absorption Rate (SAR) for including accessories and multiple transmitters", March 2010
- b) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

- c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.1
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom V5.0	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5200 MHz $\pm$ 1 MHz 5500 MHz $\pm$ 1 MHz 5800 MHz $\pm$ 1 MHz	

Head TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	35.7 $\pm$ 6 %	4.59 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5200 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.07 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	80.5 mW / g $\pm$ 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.31 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	23.0 mW / g $\pm$ 19.5 % (k=2)

Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	35.2 $\pm$ 6 %	4.89 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5500 MHz

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.59 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	85.6 mW / g $\pm$ 19.9 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.45 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	24.4 mW / g $\pm$ 19.5 % (k=2)

Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	5.19 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL at 5800 MHz

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	8.04 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	80.1 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	100 mW input power	2.29 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	22.8 mW / g ± 19.5 % (k=2)

Body TSL parameters at 5200 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	49.0	5.30 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.7 ± 6 %	5.44 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL at 5200 MHz

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.32 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	73.2 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.05 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	20.5 mW / g ± 19.5 % (k=2)

Body TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.6	5.65 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.1 ± 6 %	5.83 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL at 5500 MHz

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.93 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	79.2 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.20 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	22.0 mW / g ± 19.5 % (k=2)

Body TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.2	6.00 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.6 ± 6 %	6.25 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL at 5800 MHz

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.25 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	72.4 mW / g ± 19.9 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	100 mW input power	2.01 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	20.1 mW / g ± 19.5 % (k=2)

Appendix

Antenna Parameters with Head TSL at 5200 MHz

Impedance, transformed to feed point	51.5 Ω - 7.5 j Ω
Return Loss	- 22.5 dB

Antenna Parameters with Head TSL at 5500 MHz

Impedance, transformed to feed point	52.9 Ω - 1.6 j Ω
Return Loss	- 29.8 dB

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	57.0 Ω - 1.4 j Ω
Return Loss	- 23.6 dB

Antenna Parameters with Body TSL at 5200 MHz

Impedance, transformed to feed point	51.9 Ω - 6.2 j Ω
Return Loss	- 24.0 dB

Antenna Parameters with Body TSL at 5500 MHz

Impedance, transformed to feed point	54.8 Ω - 0.3 j Ω
Return Loss	- 26.7 dB

Antenna Parameters with Body TSL at 5800 MHz

Impedance, transformed to feed point	57.7 Ω + 1.0 j Ω
Return Loss	- 22.8 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.199 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	September 08, 2011

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1123

Communication System: CW; Frequency: 5200 MHz, Frequency: 5500 MHz, Frequency: 5800 MHz
Medium parameters used: $f = 5200$ MHz; $\sigma = 4.59$ mho/m; $\epsilon_r = 35.7$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5500$ MHz; $\sigma = 4.89$ mho/m; $\epsilon_r = 35.2$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5800$ MHz; $\sigma = 5.19$ mho/m; $\epsilon_r = 34.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(5.41, 5.41, 5.41), ConvF(4.91, 4.91, 4.91), ConvF(4.81, 4.81, 4.81); Calibrated: 30.12.2011
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.1(838); SEMCAD X 14.6.5(6469)

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 64.566 V/m; Power Drift = 0.07 dB

Peak SAR (extrapolated) = 30.0150 mW/g

SAR(1 g) = 8.07 mW/g; SAR(10 g) = 2.31 mW/g

Maximum value of SAR (measured) = 18.509 mW/g

Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 65.375 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 33.9990 mW/g

SAR(1 g) = 8.59 mW/g; SAR(10 g) = 2.45 mW/g

Maximum value of SAR (measured) = 20.086 mW/g


Dipole Calibration for Head Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 61.857 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 33.4580 mW/g


SAR(1 g) = 8.04 mW/g; SAR(10 g) = 2.29 mW/g

Maximum value of SAR (measured) = 19.185 mW/g

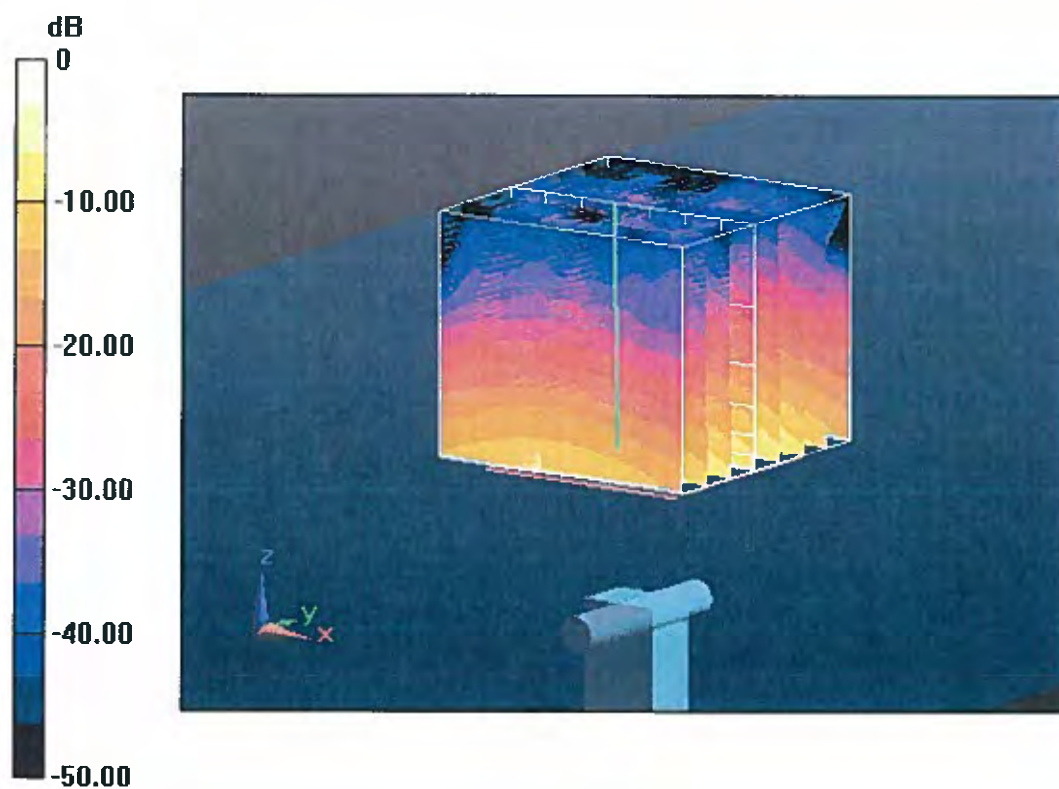

0 dB = 19.180mW/g = 25.66 dB mW/g

Impedance Measurement Plot for Head TSL

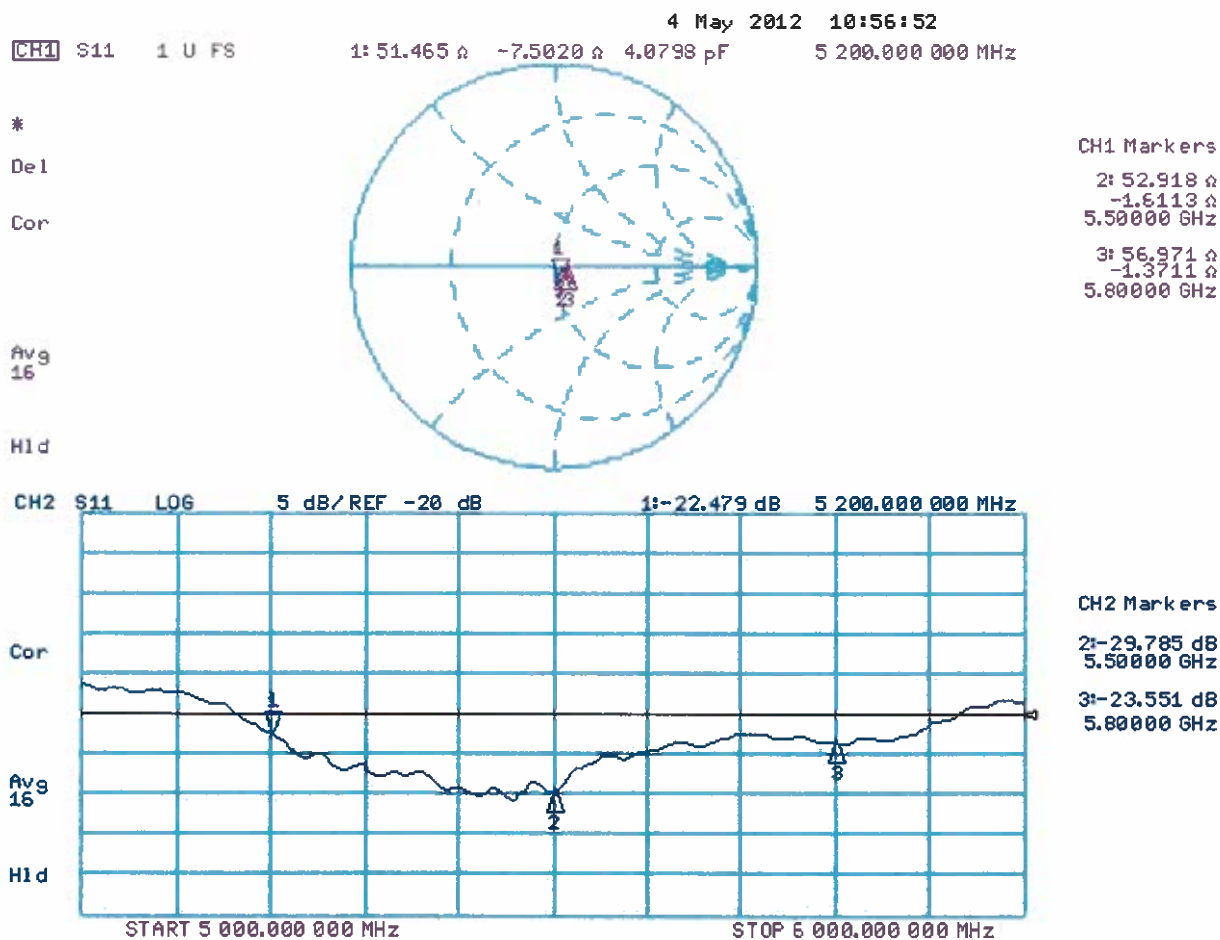

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1123

Communication System: CW; Frequency: 5200 MHz, Frequency: 5500 MHz, Frequency: 5800 MHz
Medium parameters used: $f = 5200$ MHz; $\sigma = 5.44$ mho/m; $\epsilon_r = 48.7$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5500$ MHz; $\sigma = 5.83$ mho/m; $\epsilon_r = 48.1$; $\rho = 1000$ kg/m³, Medium parameters used: $f = 5800$ MHz; $\sigma = 6.25$ mho/m; $\epsilon_r = 47.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: EX3DV4 - SN3503; ConvF(4.91, 4.91, 4.91); Calibrated: 30.12.2011, ConvF(4.43, 4.43, 4.43); Calibrated: 30.12.2011, ConvF(4.38, 4.38, 4.38); Calibrated: 30.12.2011;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.1(838); SEMCAD X 14.6.5(6469)

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 57.889 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 28.896 mW/g

SAR(1 g) = 7.32 mW/g; SAR(10 g) = 2.05 mW/g

Maximum value of SAR (measured) = 17.2 mW/g

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 58.366 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 34.150 mW/g

SAR(1 g) = 7.93 mW/g; SAR(10 g) = 2.2 mW/g

Maximum value of SAR (measured) = 19.2 mW/g


Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 54.272 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 33.782 mW/g


SAR(1 g) = 7.25 mW/g; SAR(10 g) = 2.01 mW/g

Maximum value of SAR (measured) = 18.0 mW/g

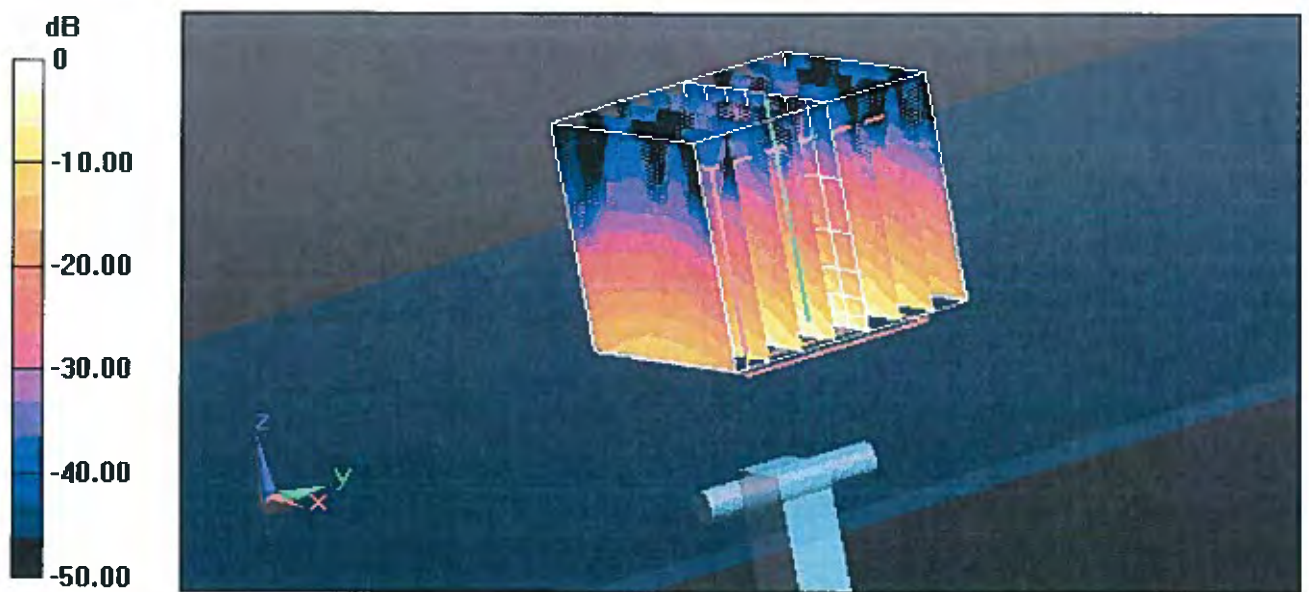

0 dB = 18.410mW/g = 25.30 dB mW/g

Impedance Measurement Plot for Body TSL

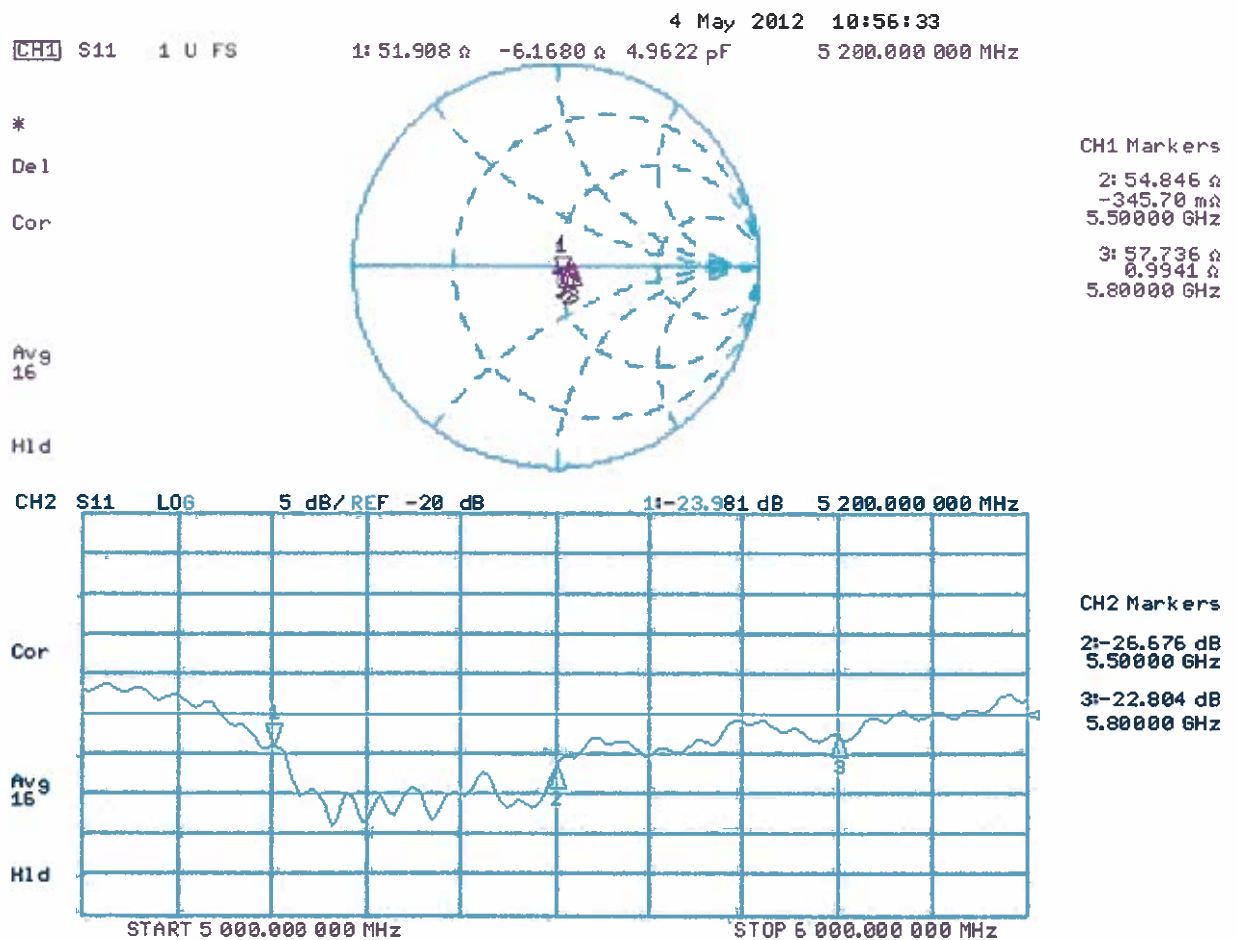

APPENDIX G: CONDUCTED POWER MEASUREMENTS FOR SUPPORTED LTE TRANSMISSION MODES

G.1 Power Tuning Targets

Tuning targets LTE			
Band	Low channel	Mid channel	High channel
LTE1700/2100 (Band 4)	23.0	23.0	23.0

G.2 Conducted Power from the Samples used in the Testing

Type: RM-878; Serial number: 004402/47/109933/7 used for LTE1700/2100 (Band 4) for SAR Head, Body-worn and Wireless Router measurements.

“Max Average Power (dBm)” column lists measured powers with MPR active. The “Reduced Power” column lists measured powers with MPR and A-MPR active (as defined by 3GPP TS 36.101). A-MPR is not supported in this device.

Frequency (MHz)	Channel Number	Bandwidth (MHz)	RB Number	RB Offset	Modulation	Max Average Power (dBm)	Reduced Power(dBm)
1720.0	20050	1.4	1	0	QPSK	23.12	-
1720.0	20050	1.4	1	5	QPSK	23.06	-
1720.0	20050	1.4	1	2	QPSK	23.07	-
1720.0	20050	1.4	3	2	QPSK	23.13	-
1720.0	20050	1.4	6	0	QPSK	22.18	-
1720.0	20050	1.4	1	0	16QAM	22.09	-
1720.0	20050	1.4	1	5	16QAM	21.99	-
1720.0	20050	1.4	1	2	16QAM	22.10	-
1720.0	20050	1.4	3	2	16QAM	22.00	-
1720.0	20050	1.4	6	0	16QAM	21.11	-
1732.5	20175	1.4	1	0	QPSK	23.06	-
1732.5	20175	1.4	1	5	QPSK	23.05	-
1732.5	20175	1.4	1	2	QPSK	23.08	-
1732.5	20175	1.4	3	2	QPSK	22.98	-
1732.5	20175	1.4	6	0	QPSK	22.03	-
1732.5	20175	1.4	1	0	16QAM	22.03	-
1732.5	20175	1.4	1	5	16QAM	22.00	-
1732.5	20175	1.4	1	2	16QAM	21.98	-
1732.5	20175	1.4	3	2	16QAM	21.97	-
1732.5	20175	1.4	6	0	16QAM	21.03	-
1745.0	20300	1.4	1	0	QPSK	23.05	-
1745.0	20300	1.4	1	5	QPSK	23.04	-
1745.0	20300	1.4	1	2	QPSK	23.06	-
1745.0	20300	1.4	3	2	QPSK	22.98	-
1745.0	20300	1.4	6	0	QPSK	22.08	-
1745.0	20300	1.4	1	0	16QAM	21.97	-
1745.0	20300	1.4	1	5	16QAM	22.04	-
1745.0	20300	1.4	1	2	16QAM	22.05	-
1745.0	20300	1.4	3	2	16QAM	21.79	-
1745.0	20300	1.4	6	0	16QAM	21.01	-

Frequency (MHz)	Channel Number	Bandwidth (MHz)	RB Number	RB Offset	Modulation	Max Average Power (dBm)	Reduced Power(dBm)
1720.0	20050	3	1	0	QPSK	23.09	-
1720.0	20050	3	1	14	QPSK	22.98	-
1720.0	20050	3	1	7	QPSK	23.06	-
1720.0	20050	3	8	3	QPSK	22.12	-
1720.0	20050	3	15	0	QPSK	22.04	-
1720.0	20050	3	1	0	16QAM	22.37	-
1720.0	20050	3	1	14	16QAM	22.16	-
1720.0	20050	3	1	7	16QAM	22.16	-
1720.0	20050	3	8	3	16QAM	21.02	-
1720.0	20050	3	15	0	16QAM	21.02	-
1732.5	20175	3	1	0	QPSK	23.00	-
1732.5	20175	3	1	14	QPSK	23.09	-
1732.5	20175	3	1	7	QPSK	23.11	-
1732.5	20175	3	8	3	QPSK	22.02	-
1732.5	20175	3	15	0	QPSK	21.91	-
1732.5	20175	3	1	0	16QAM	22.23	-
1732.5	20175	3	1	14	16QAM	21.97	-
1732.5	20175	3	1	7	16QAM	22.14	-
1732.5	20175	3	8	3	16QAM	20.83	-
1732.5	20175	3	15	0	16QAM	20.93	-
1745.0	20300	3	1	0	QPSK	23.13	-
1745.0	20300	3	1	14	QPSK	23.11	-
1745.0	20300	3	1	7	QPSK	23.02	-
1745.0	20300	3	8	3	QPSK	22.07	-
1745.0	20300	3	15	0	QPSK	22.09	-
1745.0	20300	3	1	0	16QAM	21.97	-
1745.0	20300	3	1	14	16QAM	22.03	-
1745.0	20300	3	1	7	16QAM	21.90	-
1745.0	20300	3	8	3	16QAM	20.77	-
1745.0	20300	3	15	0	16QAM	20.99	-

Frequency (MHz)	Channel Number	Bandwidth (MHz)	RB Number	RB Offset	Modulation	Max Average Power (dBm)	Reduced Power(dBm)
1720.0	20050	5	1	0	QPSK	23.13	-
1720.0	20050	5	1	24	QPSK	23.00	-
1720.0	20050	5	1	12	QPSK	22.98	-
1720.0	20050	5	12	6	QPSK	22.02	-
1720.0	20050	5	25	0	QPSK	21.98	-
1720.0	20050	5	1	0	16QAM	22.25	-
1720.0	20050	5	1	24	16QAM	22.08	-
1720.0	20050	5	1	12	16QAM	22.02	-
1720.0	20050	5	12	6	16QAM	21.01	-
1720.0	20050	5	25	0	16QAM	20.93	-
1732.5	20175	5	1	0	QPSK	23.03	-
1732.5	20175	5	1	24	QPSK	23.01	-
1732.5	20175	5	1	12	QPSK	23.12	-
1732.5	20175	5	12	6	QPSK	22.03	-
1732.5	20175	5	25	0	QPSK	21.95	-
1732.5	20175	5	1	0	16QAM	22.10	-
1732.5	20175	5	1	24	16QAM	22.10	-
1732.5	20175	5	1	12	16QAM	22.12	-
1732.5	20175	5	12	6	16QAM	20.95	-
1732.5	20175	5	25	0	16QAM	20.90	-
1745.0	20300	5	1	0	QPSK	23.08	-
1745.0	20300	5	1	24	QPSK	23.08	-
1745.0	20300	5	1	12	QPSK	23.12	-
1745.0	20300	5	12	6	QPSK	22.04	-
1745.0	20300	5	25	0	QPSK	22.08	-
1745.0	20300	5	1	0	16QAM	22.08	-
1745.0	20300	5	1	24	16QAM	22.25	-
1745.0	20300	5	1	12	16QAM	22.28	-
1745.0	20300	5	12	6	16QAM	20.98	-
1745.0	20300	5	25	0	16QAM	21.04	-

Frequency (MHz)	Channel Number	Bandwidth (MHz)	RB Number	RB Offset	Modulation	Max Average Power (dBm)	Reduced Power(dBm)
1720.0	20050	10	1	0	QPSK	23.12	-
1720.0	20050	10	1	49	QPSK	23.01	-
1720.0	20050	10	1	24	QPSK	23.04	-
1720.0	20050	10	25	12	QPSK	22.09	-
1720.0	20050	10	50	0	QPSK	22.02	-
1720.0	20050	10	1	0	16QAM	22.20	-
1720.0	20050	10	1	49	16QAM	22.05	-
1720.0	20050	10	1	24	16QAM	22.01	-
1720.0	20050	10	25	12	16QAM	21.01	-
1720.0	20050	10	50	0	16QAM	21.00	-
1732.5	20175	10	1	0	QPSK	22.99	-
1732.5	20175	10	1	49	QPSK	22.96	-
1732.5	20175	10	1	24	QPSK	23.16	-
1732.5	20175	10	25	12	QPSK	22.03	-
1732.5	20175	10	50	0	QPSK	21.94	-
1732.5	20175	10	1	0	16QAM	21.45	-
1732.5	20175	10	1	49	16QAM	22.20	-
1732.5	20175	10	1	24	16QAM	22.05	-
1732.5	20175	10	25	12	16QAM	20.97	-
1732.5	20175	10	50	0	16QAM	20.83	-
1745.0	20300	10	1	0	QPSK	23.11	-
1745.0	20300	10	1	49	QPSK	23.02	-
1745.0	20300	10	1	24	QPSK	23.13	-
1745.0	20300	10	25	12	QPSK	22.00	-
1745.0	20300	10	50	0	QPSK	22.03	-
1745.0	20300	10	1	0	16QAM	21.99	-
1745.0	20300	10	1	49	16QAM	21.97	-
1745.0	20300	10	1	24	16QAM	21.97	-
1745.0	20300	10	25	12	16QAM	20.91	-
1745.0	20300	10	50	0	16QAM	20.99	-

Frequency (MHz)	Channel Number	Bandwidth (MHz)	RB Number	RB Offset	Modulation	Max Average Power (dBm)	Reduced Power(dBm)
1720.0	20050	15	1	0	QPSK	23.02	-
1720.0	20050	15	1	74	QPSK	22.99	-
1720.0	20050	15	1	36	QPSK	23.04	-
1720.0	20050	15	37	18	QPSK	22.12	-
1720.0	20050	15	75	0	QPSK	22.08	-
1720.0	20050	15	1	0	16QAM	21.92	-
1720.0	20050	15	1	74	16QAM	22.07	-
1720.0	20050	15	1	36	16QAM	22.28	-
1720.0	20050	15	37	18	16QAM	21.06	-
1720.0	20050	15	75	0	16QAM	21.00	-
1732.5	20175	15	1	0	QPSK	23.05	-
1732.5	20175	15	1	74	QPSK	23.05	-
1732.5	20175	15	1	36	QPSK	23.04	-
1732.5	20175	15	37	18	QPSK	21.94	-
1732.5	20175	15	75	0	QPSK	21.92	-
1732.5	20175	15	1	0	16QAM	22.00	-
1732.5	20175	15	1	74	16QAM	21.98	-
1732.5	20175	15	1	36	16QAM	21.99	-
1732.5	20175	15	37	18	16QAM	20.95	-
1732.5	20175	15	75	0	16QAM	20.93	-
1745.0	20300	15	1	0	QPSK	23.00	-
1745.0	20300	15	1	74	QPSK	22.91	-
1745.0	20300	15	1	36	QPSK	23.03	-
1745.0	20300	15	37	18	QPSK	22.03	-
1745.0	20300	15	75	0	QPSK	21.98	-
1745.0	20300	15	1	0	16QAM	22.02	-
1745.0	20300	15	1	74	16QAM	22.16	-
1745.0	20300	15	1	36	16QAM	22.21	-
1745.0	20300	15	37	18	16QAM	20.92	-
1745.0	20300	15	75	0	16QAM	20.99	-

Frequency (MHz)	Channel Number	Bandwidth (MHz)	RB Number	RB Offset	Modulation	Max Average Power (dBm)	Reduced Power(dBm)
1720.0	20050	20	1	0	QPSK	23.09	-
1720.0	20050	20	1	99	QPSK	22.97	-
1720.0	20050	20	1	49	QPSK	23.09	-
1720.0	20050	20	50	24	QPSK	22.00	-
1720.0	20050	20	100	0	QPSK	22.08	-
1720.0	20050	20	1	0	16QAM	21.98	-
1720.0	20050	20	1	99	16QAM	21.91	-
1720.0	20050	20	1	49	16QAM	22.13	-
1720.0	20050	20	50	24	16QAM	21.00	-
1720.0	20050	20	100	0	16QAM	20.97	-
1732.5	20175	20	1	0	QPSK	23.02	-
1732.5	20175	20	1	99	QPSK	23.10	-
1732.5	20175	20	1	49	QPSK	23.07	-
1732.5	20175	20	50	24	QPSK	21.94	-
1732.5	20175	20	100	0	QPSK	21.94	-
1732.5	20175	20	1	0	16QAM	22.24	-
1732.5	20175	20	1	99	16QAM	21.87	-
1732.5	20175	20	1	49	16QAM	22.31	-
1732.5	20175	20	50	24	16QAM	20.84	-
1732.5	20175	20	100	0	16QAM	20.87	-
1745.0	20300	20	1	0	QPSK	22.99	-
1745.0	20300	20	1	99	QPSK	23.01	-
1745.0	20300	20	1	49	QPSK	23.08	-
1745.0	20300	20	50	24	QPSK	22.00	-
1745.0	20300	20	100	0	QPSK	21.94	-
1745.0	20300	20	1	0	16QAM	22.01	-
1745.0	20300	20	1	99	16QAM	21.99	-
1745.0	20300	20	1	49	16QAM	22.01	-
1745.0	20300	20	50	24	16QAM	20.88	-
1745.0	20300	20	100	0	16QAM	20.87	-

APPENDIX H: CONDUCTED POWER MEASUREMENTS FOR SUPPORTED GSM/GPRS/EGPRS TRANSMISSION MODES

H.1 Power Tuning Targets for Head, Body-worn and Wireless Router measurements

GSM 850			
Slot configuration	Low channel	Mid channel	High channel
GSM 1-slot	32.5	32.5	32.5
GPRS 2-slot	31.0	31.0	31.0
GPRS 3-slot	29.0	29.0	29.0
GPRS 4-slot	28.0	28.0	28.0
EGRPS 1-slot	26.2	26.2	26.2
EGPRS 2-slot	26.2	26.2	26.2
EGPRS 3-slot	25.0	25.0	25.0
EGPRS 4-slot	24.0	24.0	24.0

GSM 1900			
Slot configuration	Low channel	Mid channel	High channel
GSM 1-slot	29.5	29.5	29.5
GPRS 2-slot	29.0	29.0	29.0
GPRS 3-slot	27.0	27.0	27.0
GPRS 4-slot	26.0	26.0	26.0
EGRPS 1-slot	25.5	25.5	25.5
EGPRS 2-slot	25.5	25.5	25.5
EGPRS 3-slot	24.0	24.0	24.0
EGPRS 4-slot	23.0	23.0	23.0

H.2 Conducted Power from the Samples used in the Testing

Type: RM-878; Serial number: 004402/47/109944/4 used for GSM/GPRS/EGPRS850 SAR Head, Body-worn and Wireless router measurements.

GSM 850			
Slot configuration	Low channel	Mid channel	High channel
GSM 1-slot	32.5	32.6	32.6
GPRS 2-slot	30.8	31.2	30.9
GPRS 3-slot	28.5	28.8	28.9
GPRS 4-slot	27.8	28.0	28.2
EGPRS 1-slot	27.2	27.3	27.5
EGPRS 2-slot	26.6	26.7	26.8
EGPRS 3-slot	25.6	26.7	25.6
EGPRS 4-slot	24.5	24.5	24.5

Type: RM-878; Serial number: 004402/47/109947/7 used for GSM/GPRS/EGPRS1900 SAR Head and Body-worn measurements.

GSM 1900			
Slot configuration	Low channel	Mid channel	High channel
GSM 1-slot	29.7	29.7	29.7
GPRS 2-slot	29.2	29.1	29.3
GPRS 3-slot	27.2	27.2	27.3
GPRS 4-slot	26.3	26.4	26.3
EGPRS 1-slot	26.3	26.4	26.4
EGPRS 2-slot	26.3	26.4	26.3
EGPRS 3-slot	25.0	25.0	25.0
EGPRS 4-slot	23.8	23.8	24.0

Type: RM-878; Serial number: 004402/47/109925/3 used for GSM/GPRS/EGPRS1900 SAR Wireless Router measurements.

GSM 1900			
Slot configuration	Low channel	Mid channel	High channel
GSM 1-slot	29.3	29.3	29.4
GPRS 2-slot	28.8	28.7	28.8
GPRS 3-slot	26.7	26.8	26.9
GPRS 4-slot	25.9	25.9	25.8
EGPRS 1-slot	25.8	26.0	26.1
EGPRS 2-slot	26.0	25.9	26.0
EGPRS 3-slot	24.5	24.5	24.6
EGPRS 4-slot	23.5	23.4	23.5

APPENDIX I: CONDUCTED POWER MEASUREMENTS FOR SUPPORTED WCDMA TRANSMISSION MODES

1. I.1 Power Tuning Targets

WCDMA 5 For Head, Body-worn and WR measurements			
Mode	Low channel	Mid channel	High channel
WCDMA	23.5	23.5	23.5

WCDMA1700/2100 For Head and body-worn measurements			
Mode	Low channel	Mid channel	High channel
WCDMA	23.5	23.5	23.5

WCDMA1900 For Head and body-worn measurements			
Mode	Low channel	Mid channel	High channel
WCDMA	23.0	23.0	23.0

WCDMA1700/2100 For WR measurements			
Mode	Low channel	Mid channel	High channel
WCDMA	22.5	22.5	22.5

WCDMA1900 For WR measurements			
Mode	Low channel	Mid channel	High channel
WCDMA	22.0	22.0	22.0

I.2 Conducted Power from the Samples used in the Testing

Type: RM-878; Serial number: 004402/47/109944/4 used for WCDMA850 SAR Head and Body-worn measurements.

WCDMA 5			
Mode	Low channel	Mid channel	High channel
WCDMA	23.5	23.2	23.4

Type: RM-878; Serial number: 004402/47/109947/7 used for WCDMA1700/2100 and WCDMA1900 SAR Head and Body-worn measurements.

WCDMA 4			
Mode	Low channel	Mid channel	High channel
WCDMA	23.2	23.1	23.2

WCDMA 2			
Mode	Low channel	Mid channel	High channel
WCDMA	22.5	22.5	22.3

Type: RM-878; Serial number: 004402/47/109925/3 used for WCDMA850, WCDMA1700/2100 and WCDMA1900 SAR Wireless Router measurements.

WCDMA850			
Mode	Low channel	Mid channel	High channel
WCDMA	23.5	23.1	23.3

WCDMA1700/2100			
Mode	Low channel	Mid channel	High channel
WCDMA	22.7	22.5	22.7

WCDMA1900			
Mode	Low channel	Mid channel	High channel
WCDMA	22.2	22.5	22.0

WCDMA and HSUPA Subtest mode conducted powers, measured from a separate, fully representative sample are presented in Appendix D.

APPENDIX J: CONDUCTED POWER MEASUREMENTS FOR SUPPORTED WLAN TRANSMISSION MODES

J.1 Power Tuning Targets for Head, Body-worn and Wireless Router measurements

WLAN 2.4 GHz, tuning targets					
Modulation mode	Ch 1	Ch 2	Ch 6	Ch 10	Ch 11
b-mode WLAN DSSS 1 Mbps	17	17	17	17	17
b-mode WLAN DSSS 2 Mbps	17	17	17	17	17
b-mode WLAN DSSS 5.5 Mbps	17	17	17	17	17
b-mode WLAN DSSS 11 Mbps	17	17	17	17	17
g-mode WLAN OFDM 6 Mbps	16	16	16	16	16
g-mode WLAN OFDM 9 Mbps	16	16	16	16	16
g-mode WLAN OFDM 12 Mbps	15	15	15	15	15
g-mode WLAN OFDM 18 Mbps	15	15	15	15	15
g-mode WLAN OFDM 24 Mbps	14	14	14	14	14
g-mode WLAN OFDM 36 Mbps	14	14	14	14	14
g-mode WLAN OFDM 48 Mbps	13	13	13	13	13
g-mode WLAN OFDM 54 Mbps	13	13	13	13	13
n-mode MCS 0: OFDM 6.5 / 7.25 Mbps	15	15	15	15	15
n-mode MCS 1: OFDM 13.0 / 14.4 Mbps	15	15	15	15	15
n-mode MCS 2: OFDM 19.5 / 21.7 Mbps	15	15	15	15	15
n-mode MCS 3: OFDM 26.0 / 28.9 Mbps	15	15	15	15	15
n-mode MCS 4: OFDM 39.0 / 43.3 Mbps	13	13	13	13	13
n-mode MCS 5: OFDM 52.0 / 57.8 Mbps	13	13	13	13	13
n-mode MCS 6: OFDM 58.5 / 65.0 Mbps	13	13	13	13	13
n-mode MCS 7: OFDM 65.0 / 72.2 Mbps	13	13	13	13	13

WLAN 5GHz, tuning targets	
Mode	All channels
WLAN OFDM 6 Mbps	12
WLAN OFDM 9 Mbps	12
WLAN OFDM 12 Mbps	12
WLAN OFDM 18 Mbps	12
WLAN OFDM 24 Mbps	12
WLAN OFDM 36 Mbps	12
WLAN OFDM 48 Mbps	12
WLAN OFDM 54 Mbps	12
MCS 0: OFDM 6.5 / 7.25 Mbps	12
MCS 1: OFDM 13.0 / 14.4 Mbps	12
MCS 2: OFDM 19.5 / 21.7 Mbps	12
MCS 3: OFDM 26.0 / 28.9 Mbps	12
MCS 4: OFDM 39.0 / 43.3 Mbps	12
MCS 5: OFDM 52.0 / 57.8 Mbps	12
MCS 6: OFDM 58.5 / 65.0 Mbps	12
MCS 7: OFDM 65.0 / 72.2 Mbps	12
MCS 0: OFDM 13.5 / 15.0 Mbps	10
MCS 1: OFDM 27.0 / 30.0 Mbps	10
MCS 2: OFDM 40.5 / 45.0 Mbps	10
MCS 3: OFDM 54.0 / 60.0 Mbps	10
MCS 4: OFDM 81.0 / 90.0 Mbps	10
MCS 5: OFDM 108.0 / 120.0 Mbps	10
MCS 6: OFDM 121.5 / 135.0 Mbps	10
MCS 7: OFDM 135.0 / 150.0 Mbps	10

J.2 Conducted Power from the Samples used in the Testing

Type: RM-878; Serial number: 004402/47/109927/9 used for WLAN2450 SAR Head, Body-worn and Wireless Router measurements.

WLAN 2.4 GHz					
Modulation mode	Ch 1	Ch 2	Ch 6	Ch 10	Ch 11
b-mode WLAN DSSS 1 Mbps	17.49	17.93	17.66	17.70	17.55
b-mode WLAN DSSS 2 Mbps	17.08	17.93	17.67	17.24	17.55
b-mode WLAN DSSS 5.5 Mbps	18.09	18.02	17.72	17.35	17.70
b-mode WLAN DSSS 11 Mbps	18.04	17.98	17.70	17.81	17.65
g-mode WLAN OFDM 6 Mbps	16.45	16.81	16.86	16.12	16.03
g-mode WLAN OFDM 9 Mbps	16.41	16.39	16.82	16.76	16.64
g-mode WLAN OFDM 12 Mbps	15.97	15.91	15.90	15.18	15.68
g-mode WLAN OFDM 18 Mbps	15.96	15.89	15.88	15.23	15.69
g-mode WLAN OFDM 24 Mbps	15.45	15.83	15.93	15.96	15.62
g-mode WLAN OFDM 36 Mbps	15.95	16.44	15.98	15.88	15.76
g-mode WLAN OFDM 48 Mbps	14.00	14.22	14.23	13.74	13.66
g-mode WLAN OFDM 54 Mbps	14.20	14.28	14.22	13.60	14.36
n-mode MCS 0: OFDM 6.5 / 7.25 Mbps	15.08	15.42	14.97	15.60	15.44
n-mode MCS 1: OFDM 13.0 / 14.4 Mbps	15.05	15.42	14.93	14.91	14.76
n-mode MCS 2: OFDM 19.5 / 21.7 Mbps	15.01	14.95	14.95	14.95	14.83
n-mode MCS 3: OFDM 26.0 / 28.9 Mbps	15.05	14.82	14.94	14.90	14.77
n-mode MCS 4: OFDM 39.0 / 43.3 Mbps	13.94	14.36	13.80	13.83	14.46
n-mode MCS 5: OFDM 52.0 / 57.8 Mbps	14.37	14.29	13.82	13.87	14.36
n-mode MCS 6: OFDM 58.5 / 65.0 Mbps	13.95	14.30	13.87	14.54	14.30
n-mode MCS 7: OFDM 65.0 / 72.2 Mbps	14.02	13.84	13.80	14.53	13.69

J.2 Conducted Power from the Samples used in the Testing

Type: RM-878; Serial number: 004402/47/109927/9 used for WLAN5000 SAR Head and Body-worn measurements.

Mode	36	40	44	48	52	56
WLAN OFDM 6 Mbps	10.78	10.96	11.28	11.36	11.62	11.58
WLAN OFDM 9 Mbps	10.85	11.21	11.36	11.18	11.21	11.48
WLAN OFDM 12 Mbps	11.16	11.09	11.03	11.21	11.23	11.08
WLAN OFDM 18 Mbps	10.87	11.07	10.94	11.08	11.35	11.07
WLAN OFDM 24 Mbps	11.14	11.16	11.00	11.17	11.34	11.50
WLAN OFDM 36 Mbps	10.80	10.76	10.96	11.14	11.32	10.94
WLAN OFDM 48 Mbps	11.33	11.05	11.49	10.98	11.32	11.14
WLAN OFDM 54 Mbps	10.72	10.82	11.43	11.15	11.35	11.32
MCS 0: OFDM 6.5 / 7.25 Mbps	11.00	11.28	11.18	11.30	11.32	11.44
MCS 1: OFDM 13.0 / 14.4 Mbps	11.39	11.35	11.14	11.34	11.36	11.58
MCS 2: OFDM 19.5 / 21.7 Mbps	11.26	11.20	11.42	11.20	11.34	11.54
MCS 3: OFDM 26.0 / 28.9 Mbps	11.20	10.88	11.14	11.50	11.00	11.16
MCS 4: OFDM 39.0 / 43.3 Mbps	11.17	11.18	11.02	11.18	11.36	11.45
MCS 5: OFDM 52.0 / 57.8 Mbps	11.23	11.28	11.05	11.38	11.36	11.54
MCS 6: OFDM 58.5 / 65.0 Mbps	11.29	10.96	11.41	11.20	11.39	11.16
MCS 7: OFDM 65.0 / 72.2 Mbps	10.78	10.96	11.28	11.36	11.62	11.58
MCS 0: OFDM 13.5 / 15.0 Mbps	7.10	7.45	7.65	7.26	7.85	7.60
MCS 1: OFDM 27.0 / 30.0 Mbps	7.25	7.44	7.40	7.76	7.38	7.79
MCS 2: OFDM 40.5 / 45.0 Mbps	7.55	7.49	7.69	7.78	7.32	8.06
MCS 3: OFDM 54.0 / 60.0 Mbps	7.41	7.24	7.62	7.20	7.37	7.55
MCS 4: OFDM 81.0 / 90.0 Mbps	7.30	7.33	7.63	7.16	7.51	7.57
MCS 5: OFDM 108.0 / 120.0 Mbps	7.49	7.18	7.18	7.38	7.46	7.56
MCS 6: OFDM 121.5 / 135.0 Mbps	7.16	7.07	6.88	7.25	7.37	7.21
MCS 7: OFDM 135.0 / 150.0 Mbps	7.56	7.02	7.66	7.73	7.38	7.58

Mode	60	64	100	104	108	112
WLAN OFDM 6 Mbps	11.26	11.31	11.45	11.24	11.21	11.35
WLAN OFDM 9 Mbps	11.26	11.22	11.42	11.10	11.21	11.29
WLAN OFDM 12 Mbps	11.19	11.58	11.47	11.33	11.20	11.38
WLAN OFDM 18 Mbps	11.33	11.61	11.47	11.52	11.18	11.63
WLAN OFDM 24 Mbps	11.28	11.51	11.83	11.50	11.38	11.28
WLAN OFDM 36 Mbps	11.30	11.51	11.51	11.44	11.14	11.25
WLAN OFDM 48 Mbps	11.30	11.27	11.57	11.37	11.15	11.40
WLAN OFDM 54 Mbps	11.31	11.19	11.71	11.36	11.12	11.41
MCS 0: OFDM 6.5 / 7.25 Mbps	11.35	11.60	11.56	11.66	11.69	11.76
MCS 1: OFDM 13.0 / 14.4 Mbps	11.41	11.76	11.58	11.56	11.67	11.48
MCS 2: OFDM 19.5 / 21.7 Mbps	11.36	11.35	11.70	11.48	11.35	11.39
MCS 3: OFDM 26.0 / 28.9 Mbps	11.43	11.12	11.70	11.60	11.42	11.49
MCS 4: OFDM 39.0 / 43.3 Mbps	11.02	11.17	11.72	11.49	11.33	11.34
MCS 5: OFDM 52.0 / 57.8 Mbps	11.28	11.57	11.68	11.44	11.60	11.36
MCS 6: OFDM 58.5 / 65.0 Mbps	10.95	11.26	11.52	11.56	11.51	11.54
MCS 7: OFDM 65.0 / 72.2 Mbps	11.26	11.31	11.45	11.24	11.21	11.35
MCS 0: OFDM 13.5 / 15.0 Mbps	7.51	8.21	7.98	8.26	7.71	8.27
MCS 1: OFDM 27.0 / 30.0 Mbps	7.49	8.23	8.00	7.83	8.19	8.30
MCS 2: OFDM 40.5 / 45.0 Mbps	7.41	8.22	8.01	7.87	7.79	8.31
MCS 3: OFDM 54.0 / 60.0 Mbps	7.30	8.20	7.97	7.84	7.70	7.85
MCS 4: OFDM 81.0 / 90.0 Mbps	7.23	8.16	8.42	8.22	8.18	7.92
MCS 5: OFDM 108.0 / 120.0 Mbps	7.50	8.13	7.98	7.77	7.73	7.86
MCS 6: OFDM 121.5 / 135.0 Mbps	7.16	8.13	7.92	8.26	7.75	7.83
MCS 7: OFDM 135.0 / 150.0 Mbps	7.52	8.13	7.96	7.84	8.15	8.28

Mode	116	120	124	128	132	136
WLAN OFDM 6 Mbps	11.30	11.21	11.32	11.65	11.37	11.48
WLAN OFDM 9 Mbps	11.20	11.52	11.47	11.38	11.70	11.38
WLAN OFDM 12 Mbps	11.30	11.24	11.41	11.43	11.36	11.52
WLAN OFDM 18 Mbps	11.17	11.13	11.35	11.54	11.48	11.46
WLAN OFDM 24 Mbps	11.59	11.17	11.38	11.43	11.37	11.52
WLAN OFDM 36 Mbps	11.29	11.29	11.52	11.28	11.36	11.34
WLAN OFDM 48 Mbps	11.25	11.32	11.47	11.15	11.42	11.42
WLAN OFDM 54 Mbps	11.28	11.09	11.25	11.42	11.39	11.40
MCS 0: OFDM 6.5 / 7.25 Mbps	11.37	11.32	11.59	11.43	11.61	11.48
MCS 1: OFDM 13.0 / 14.4 Mbps	11.36	11.61	11.41	11.43	11.47	11.51
MCS 2: OFDM 19.5 / 21.7 Mbps	11.37	11.30	11.64	11.62	11.59	11.51
MCS 3: OFDM 26.0 / 28.9 Mbps	11.33	11.31	11.45	11.52	11.46	11.44
MCS 4: OFDM 39.0 / 43.3 Mbps	11.35	11.31	11.56	11.52	11.43	11.38
MCS 5: OFDM 52.0 / 57.8 Mbps	11.30	11.34	11.40	11.40	11.40	11.41
MCS 6: OFDM 58.5 / 65.0 Mbps	11.35	11.28	11.62	11.37	11.43	11.41
MCS 7: OFDM 65.0 / 72.2 Mbps	11.30	11.21	11.32	11.65	11.37	11.48
MCS 0: OFDM 13.5 / 15.0 Mbps	8.27	7.71	8.19	7.94	7.96	7.91
MCS 1: OFDM 27.0 / 30.0 Mbps	7.83	8.18	7.76	7.95	7.97	7.92
MCS 2: OFDM 40.5 / 45.0 Mbps	7.83	7.78	7.79	7.98	7.96	7.51
MCS 3: OFDM 54.0 / 60.0 Mbps	7.84	7.63	8.14	7.89	7.87	7.83
MCS 4: OFDM 81.0 / 90.0 Mbps	7.77	7.71	8.22	7.92	7.82	7.95
MCS 5: OFDM 108.0 / 120.0 Mbps	7.69	7.60	8.21	7.89	7.91	7.79
MCS 6: OFDM 121.5 / 135.0 Mbps	8.29	7.72	7.74	7.89	7.92	7.86
MCS 7: OFDM 135.0 / 150.0 Mbps	7.83	7.73	7.77	7.92	7.93	7.89

Mode	140	149	153	157	161	165
WLAN OFDM 6 Mbps	11.53	11.47	11.43	11.47	11.43	11.50
WLAN OFDM 9 Mbps	11.34	11.46	11.54	11.46	11.28	11.36
WLAN OFDM 12 Mbps	11.35	11.48	11.38	11.50	11.33	11.39
WLAN OFDM 18 Mbps	11.43	11.13	11.37	11.53	11.52	11.38
WLAN OFDM 24 Mbps	11.39	11.21	11.45	11.57	11.22	11.50
WLAN OFDM 36 Mbps	11.45	11.06	11.36	11.64	11.35	11.38
WLAN OFDM 48 Mbps	11.29	11.54	11.52	11.47	11.38	11.24
WLAN OFDM 54 Mbps	11.28	10.98	11.32	11.49	11.31	11.40
MCS 0: OFDM 6.5 / 7.25 Mbps	11.45	11.49	11.50	11.73	11.49	11.53
MCS 1: OFDM 13.0 / 14.4 Mbps	11.43	11.37	11.59	11.45	11.42	11.50
MCS 2: OFDM 19.5 / 21.7 Mbps	11.72	11.56	11.53	11.65	11.47	11.68
MCS 3: OFDM 26.0 / 28.9 Mbps	11.79	11.54	11.52	11.61	11.50	11.55
MCS 4: OFDM 39.0 / 43.3 Mbps	11.45	11.45	11.34	11.56	11.46	11.39
MCS 5: OFDM 52.0 / 57.8 Mbps	11.52	11.09	11.56	11.58	11.46	11.49
MCS 6: OFDM 58.5 / 65.0 Mbps	11.45	11.42	11.46	11.53	11.51	11.39
MCS 7: OFDM 65.0 / 72.2 Mbps	11.53	11.47	11.43	11.47	11.43	11.50
MCS 0: OFDM 13.5 / 15.0 Mbps	8.08	7.84	7.90	7.85	7.70	7.92
MCS 1: OFDM 27.0 / 30.0 Mbps	8.15	7.84	7.89	7.87	7.69	7.93
MCS 2: OFDM 40.5 / 45.0 Mbps	8.10	7.90	7.96	7.89	7.74	7.96
MCS 3: OFDM 54.0 / 60.0 Mbps	8.05	7.79	7.84	7.82	7.68	7.93
MCS 4: OFDM 81.0 / 90.0 Mbps	8.11	7.78	7.84	7.88	7.74	7.97
MCS 5: OFDM 108.0 / 120.0 Mbps	8.01	7.80	7.87	7.88	7.68	7.86
MCS 6: OFDM 121.5 / 135.0 Mbps	8.10	7.88	7.80	7.82	7.75	7.90
MCS 7: OFDM 135.0 / 150.0 Mbps	8.08	7.81	7.88	7.85	7.71	7.91