

ECIT	

Add: No.51 Xuey	uan Road, Haidian D	ATION LABORATORY	CNAS 校准 CALIBRATION
Tel: +86-10-62304 E-mail: cttl@china		:+86-10-62304633-2504	CNAS L0570
Client EC	IT	Certificate No:	Z18-60042
CALIBRATION C	ERTIFICA	TE	
Object	D5GH	IzV2 - SN: 1172	
Calibration Procedure(s)			
Calibration Procedure(s)		1-003-01	
	Calibr	ation Procedures for dipole validation kits	
Calibration date:	March	30, 2018	
pages and are part of the c All calibrations have been	ertificate.	d the uncertainties with confidence probabili the closed laboratory facility: environme	
humidity<70%.			
Calibration Equipment used			
1.4	d (M&TE critical	for calibration)	
Primary Standards	ID#	for calibration) Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
Primary Standards Power Meter NRP2	ID # 102083	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756)	Oct-18
Primary Standards Power Meter NRP2 Power sensor NRP-Z91	ID # 102083 100542	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756)	Oct-18 Oct-18
Primary Standards	ID # 102083	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 12-Sep-17(SPEAG,No.EX3-7464_Sep17)	Oct-18 Oct-18) Sep-18
Primary Standards Power Meter NRP2 Power sensor NRP-Z91 ReferenceProbe EX3DV4	ID # 102083 100542 SN 7464	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756)	Oct-18 Oct-18) Sep-18
Primary Standards Power Meter NRP2 Power sensor NRP-Z91 ReferenceProbe EX3DV4 DAE4 Secondary Standards	ID # 102083 100542 SN 7464 SN 1525 ID #	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 12-Sep-17(SPEAG,No.EX3-7464_Sep17)	Oct-18 Oct-18) Sep-18
Primary Standards Power Meter NRP2 Power sensor NRP-Z91 ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	ID # 102083 100542 SN 7464 SN 1525 ID # MY49071430	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 12-Sep-17(SPEAG,No.EX3-7464_Sep17 02-Oct-17(SPEAG,No.DAE4-1525_Oct17 Cal Date(Calibrated by, Certificate No.) 23-Jan-18 (CTTL, No.J18X00560)	Oct-18 Oct-18) Sep-18 7) Oct-18 Scheduled Calibration Jan-19
Primary Standards Power Meter NRP2 Power sensor NRP-Z91 ReferenceProbe EX3DV4 DAE4 Secondary Standards	ID # 102083 100542 SN 7464 SN 1525 ID #	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 12-Sep-17(SPEAG,No.EX3-7464_Sep17 02-Oct-17(SPEAG,No.DAE4-1525_Oct17 Cal Date(Calibrated by, Certificate No.)	Oct-18 Oct-18) Sep-18 7) Oct-18 Scheduled Calibration
Primary Standards Power Meter NRP2 Power sensor NRP-Z91 ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	ID # 102083 100542 SN 7464 SN 1525 ID # MY49071430	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 12-Sep-17(SPEAG,No.EX3-7464_Sep17 02-Oct-17(SPEAG,No.DAE4-1525_Oct17 Cal Date(Calibrated by, Certificate No.) 23-Jan-18 (CTTL, No.J18X00560)	Oct-18 Oct-18) Sep-18 7) Oct-18 Scheduled Calibration Jan-19 Jan-19
Primary Standards Power Meter NRP2 Power sensor NRP-Z91 ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzerE5071C	ID # 102083 100542 SN 7464 SN 1525 ID # MY49071430 MY46110673	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 12-Sep-17(SPEAG,No.EX3-7464_Sep17 02-Oct-17(SPEAG,No.DAE4-1525_Oct17 Cal Date(Calibrated by, Certificate No.) 23-Jan-18 (CTTL, No.J18X00560) 24-Jan-18 (CTTL, No.J18X00561)	Oct-18 Oct-18) Sep-18 7) Oct-18 Scheduled Calibration Jan-19
Primary Standards Power Meter NRP2 Power sensor NRP-Z91 ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzerE5071C	ID # 102083 100542 SN 7464 SN 1525 ID # MY49071430 MY46110673 Name Zhao Jing	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 12-Sep-17(SPEAG,No.EX3-7464_Sep17, 02-Oct-17(SPEAG,No.DAE4-1525_Oct17 Cal Date(Calibrated by, Certificate No.) 23-Jan-18 (CTTL, No.J18X00560) 24-Jan-18 (CTTL, No.J18X00561) Function	Oct-18 Oct-18) Sep-18 7) Oct-18 Scheduled Calibration Jan-19 Jan-19
Primary Standards Power Meter NRP2 Power sensor NRP-Z91 ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzerE5071C	ID # 102083 100542 SN 7464 SN 1525 ID # MY49071430 MY46110673 Name	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 12-Sep-17(SPEAG,No.EX3-7464_Sep17, 02-Oct-17(SPEAG,No.DAE4-1525_Oct17 Cal Date(Calibrated by, Certificate No.) 23-Jan-18 (CTTL, No.J18X00560) 24-Jan-18 (CTTL, No.J18X00561) Function	Oct-18 Oct-18) Sep-18 7) Oct-18 Scheduled Calibration Jan-19 Jan-19
Primary Standards Power Meter NRP2 Power sensor NRP-Z91 ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzerE5071C Calibrated by: Reviewed by:	ID # 102083 100542 SN 7464 SN 1525 ID # MY49071430 MY46110673 Name Zhao Jing	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 12-Sep-17(SPEAG,No.EX3-7464_Sep17, 02-Oct-17(SPEAG,No.DAE4-1525_Oct17 Cal Date(Calibrated by, Certificate No.) 23-Jan-18 (CTTL, No.J18X00560) 24-Jan-18 (CTTL, No.J18X00561) Function SAR Test Engineer	Oct-18 Oct-18) Sep-18 7) Oct-18 Scheduled Calibration Jan-19 Jan-19
Primary Standards Power Meter NRP2 Power sensor NRP-Z91 ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzerE5071C Calibrated by: Reviewed by:	ID # 102083 100542 SN 7464 SN 1525 ID # MY49071430 MY46110673 Name Zhao Jing Lin Hao	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 12-Sep-17(SPEAG,No.EX3-7464_Sep17, 02-Oct-17(SPEAG,No.DAE4-1525_Oct17 Cal Date(Calibrated by, Certificate No.) 23-Jan-18 (CTTL, No.J18X00560) 24-Jan-18 (CTTL, No.J18X00561) Function SAR Test Engineer SAR Test Engineer	Oct-18 Oct-18 Oct-18 Sep-18 Oct-18 Scheduled Calibration Jan-19 Jan-19 Signature
Primary Standards Power Meter NRP2 Power sensor NRP-Z91 ReferenceProbe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzerE5071C Calibrated by: Reviewed by:	ID # 102083 100542 SN 7464 SN 1525 ID # MY49071430 MY46110673 Name Zhao Jing Lin Hao Qi Dianyuan	Cal Date(Calibrated by, Certificate No.) 01-Nov-17 (CTTL, No.J17X08756) 01-Nov-17 (CTTL, No.J17X08756) 12-Sep-17(SPEAG,No.EX3-7464_Sep17) 02-Oct-17(SPEAG,No.DAE4-1525_Oct17) Cal Date(Calibrated by, Certificate No.) 23-Jan-18 (CTTL, No.J18X00560) 24-Jan-18 (CTTL, No.J18X00561) Function SAR Test Engineer SAR Test Engineer SAR Test Engineer	Oct-18 Oct-18 Oct-18 Sep-18 Oct-18 Scheduled Calibration Jan-19 Jan-19 Signature





Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 E-mail: cttl@chinattl.com

Fax: +86-10-62304633-2504 http://www.chinattl.cn

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed . point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z18-60042

Page 2 of 16





E-mail: cttl@chinattl.com

 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2512
 Fax: +86-10-62304633-2504

 E-mail: cttl@chinattl.com
 http://www.chinattl.cn

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.0.1446
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5200 MHz ± 1 MHz 5300 MHz ± 1 MHz 5500 MHz ± 1 MHz 5600 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5200 MHz

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.2 ± 6 %	4.70 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

SAR result with Head TSL at 5200 MHz

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.48 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	74.9 mW /g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.14 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	21.4 mW /g ± 24.2 % (k=2)

Certificate No: Z18-60042

Page 3 of 16





Head TSL parameters at 5300 MHz The following parameters and calculations we

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.7 ± 6 %	4.77 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

SAR result with Head TSL at 5300 MHz

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.54 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	75.8 mW /g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.11 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	21.2 mW /g ± 24.2 % (k=2)

Head TSL parameters at 5500 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.8 ± 6 %	4.97 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

SAR result with Head TSL at 5500 MHz

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.99 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	80.0 mW /g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.26 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	22.6 mW /g ± 24.2 % (k=2)

Certificate No: Z18-60042

Page 4 of 16





Head TSL parameters at 5600 MHz

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.8 ± 6 %	5.10 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

and the st

SAR result with Head TSL at 5600 MHz

SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.91 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	79.3 mW /g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.21 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	22.2 mW /g ± 24.2 % (k=2)

Head TSL parameters at 5800 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.6 ± 6 %	5.28 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

SAR result with Head TSL at 5800 MHz

SAR averaged over 1 Cm^3 (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	7.36 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	73.7 mW /g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.06 mW / g
SAR for nominal Head TSL parameters	normalized to 1W	20.7 mW /g ± 24.2 % (k=2)

Certificate No: Z18-60042

Page 5 of 16





Body TSL parameters at 5200 MHz

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	49.0	5.30 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.9 ± 6 %	5.29 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

SAR result with Body TSL at 5200 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.09 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	70.9 mW /g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	1.98 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	19.8 mW /g ± 24.2 % (k=2)

Body TSL parameters at 5300 MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.9	5.42 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.7 ± 6 %	5.40 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

SAR result with Body TSL at 5300 MHz

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition		
SAR measured	100 mW input power	7.12 mW / g	
SAR for nominal Body TSL parameters	normalized to 1W	71.1 mW /g ± 24.4 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition		
SAR measured	100 mW input power	1.98 mW / g	
SAR for nominal Body TSL parameters	normalized to 1W	19.8 mW /g ± 24.2 % (k=2)	

Certificate No: Z18-60042

Page 6 of 16





Body TSL parameters at 5500 MHz

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.6	5.65 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.2 ± 6 %	5.67 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

SAR result with Body TSL at 5500 MHz

SAR averaged over 1 cm^3 (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.72 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	77.1 mW /g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.14 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	21.4 mW /g ± 24.2 % (k=2)

Body TSL parameters at 5600 MHz The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.5	5.77 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	48.1 ± 6 %	5.81 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

SAR result with Body TSL at 5600 MHz

SAR averaged over 1 cm^3 (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.52 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	75.1 mW /g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.10 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	21.0 mW /g ± 24.2 % (k=2)

Certificate No: Z18-60042

Page 7 of 16





Body TSL parameters at 5800 MHz The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	48.2	6.00 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	47.7 ± 6 %	6.09 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		

SAR result with Body TSL at 5800 MHz

SAR averaged over 1 cm^3 (1 g) of Body TSL	Condition	
SAR measured	100 mW input power	7.27 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	72.6 mW /g ± 24.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	100 mW input power	2.02 mW / g
SAR for nominal Body TSL parameters	normalized to 1W	20.2 mW /g ± 24.2 % (k=2)

Certificate No: Z18-60042

Page 8 of 16



	8 In Co	llabora	tion wit	h	
TT	, S	p	е	а	g
	CALI	BRATIC	ON LAP	ORAT	DRY

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL at 5200 MHz

E-mail: cttl@chinattl.com

Impedance, transformed to feed point	53.1Ω - 8.16jΩ
Return Loss	- 21.5dB

Antenna Parameters with Head TSL at 5300 MHz

Impedance, transformed to feed point	49.8Ω - 5.65jΩ	
Return Loss	- 25.0dB	

Antenna Parameters with Head TSL at 5500 MHz

Impedance, transformed to feed point	53.2Ω - 6.65jΩ	
Return Loss	- 22.9dB	

Antenna Parameters with Head TSL at 5600 MHz

Impedance, transformed to feed point	58.6Ω - 2.98jΩ
Return Loss	- 21.6dB

Antenna Parameters with Head TSL at 5800 MHz

Impedance, transformed to feed point	55.0Ω - 3.20jΩ	
Return Loss	- 24.9dB	

Antenna Parameters with Body TSL at 5200 MHz

Impedance, transformed to feed point	50.5Ω - 9.39jΩ
Return Loss	- 20.6dB

Antenna Parameters with Body TSL at 5300 MHz

Impedance, transformed to feed point	51.0Ω - 4.11jΩ	
Return Loss	- 27.6dB	

Certificate No: Z18-60042

Page 9 of 16



*	In Co	ollabora	tion wit	th	
TTT	S	p	е	а	g
	CAL	BRATIC	ON LAP	ORATO	DRY

Antenna Parameters with Body TSL at 5500 MHz

Impedance, transformed to feed point	50.3Ω - 4.72jΩ	
Return Loss	- 26.5dB	

Antenna Parameters with Body TSL at 5600 MHz

Impedance, transformed to feed point	57.0Ω - 5.31jΩ	
Return Loss	- 21.7dB	

Antenna Parameters with Body TSL at 5800 MHz

Impedance, transformed to feed point	58.8Ω - 0.73jΩ	
Return Loss	- 21.9dB	

General Antenna Parameters and Design

Electrical Delay (one direction)	1.071 ns	

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

SPEAG

Additional EUT Data

Manufactured by	

Certificate No: Z18-60042

Page 10 of 16



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 E-mail: ettl@chinattl.com http://www.chinattl.cn	
DASY5 Validation Report for Head TSL. Test Laboratory: CTTL, Beijing, China DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1172 Communication System: CW; Frequency: 5200 MHz, Frequency: 5300 MHz, Frequency: 5500 MHz, Frequency: 5600 MHz, Frequency: 5800 MHz, Medium parameters used: f = 5200 MHz; σ = 4.704 mho/m; ϵ r = 36.22; ρ = 1000 kg/m3, Medium parameters used: f = 5500 MHz; σ = 4.77 mho/m; ϵ r = 36.74; ρ = 1000 kg/m3, Medium parameters used: f = 5500 MHz; σ = 5.104 mho/m; ϵ r = 35.76; ρ = 1000 kg/m3, Medium parameters used: f = 5600 MHz; σ = 5.104 mho/m; ϵ r = 35.78; ρ = 1000 kg/m3, Medium parameters used: f = 5800 MHz; σ = 5.281 mho/m; ϵ r = 35.78; ρ = 1000 kg/m3, Medium parameters used: f = 5800 MHz; σ = 5.281 mho/m; ϵ r = 35.78; ρ = 1000 kg/m3, Medium parameters used: f = 5800 MHz; σ = 5.281 mho/m; ϵ r = 35.78; ρ = 1000 kg/m3, Medium parameters used: f = 5800 MHz; σ = 5.281 mho/m; ϵ r = 35.78; ρ = 1000 kg/m3, Medium parameters used: f = 5800 MHz; σ = 5.281 mho/m; ϵ r = 35.78; ρ = 1000 kg/m3, Medium parameters used: f = 5800 MHz; σ = 5.281 mho/m; ϵ r = 35.78; ρ = 1000 kg/m3, Medium parameters used: f = 5800 MHz; σ = 5.281 mho/m; ϵ r = 35.62; ρ = 1000 kg/m3, Phantom section: Left Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: • Probe: EX3DV4 - SN7464; ConvF(5.82, 5.82, 5.82); Calibrated: 9/12/2017, ConvF(5.51,5.53,5.53); Calibrated: 9/12/2017, ConvF(5.21,5.21,5.21); Calibrated: 9/12/2017, ConvF(4.98,4.98,4.98); Calibrated: 9/12/2017, ConvF(5.11,5.11,5.11); Calibrated: 9/12/2017, • Sensor-Surface: 1.4mm (Mechanical Surface Detection) • Electronics: DAE4 Sn1525; Calibrated: 2017-10-02 • Phantom: Triple Flat Phantom 5.1C; Type: QD 000 P51 CA; Serial: 1161/3 • Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)	
Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 60.30 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 32.5 W/kg SAR(1 g) = 7.48 W/kg; SAR(10 g) = 2.14 W/kg Maximum value of SAR (measured) = 18.7 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 66.18 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 34.1 W/kg SAR(1 g) = 7.54 W/kg; SAR(10 g) = 2.11 W/kg	
Maximum value of SAR (measured) = 18.7 W/kg	

Certificate No: Z18-60042

Page 11 of 16




In Collaboration with S pea g CALIBRATION LABORATORY Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com http://www.chinattl.cn Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 62.80 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 35.7 W/kg SAR(1 g) = 7.99 W/kg; SAR(10 g) = 2.26 W/kg Maximum value of SAR (measured) = 19.3 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.90 V/m; Power Drift = 0.06 dB Peak SAR (extrapolated) = 37.2 W/kg SAR(1 g) = 7.91 W/kg; SAR(10 g) = 2.21 W/kg Maximum value of SAR (measured) = 19.7 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 60.37 V/m; Power Drift = 0.02 dB Peak SAR (extrapolated) = 37.1 W/kg SAR(1 g) = 7.36 W/kg; SAR(10 g) = 2.06 W/kg Maximum value of SAR (measured) = 19.0 W/kg dB 0 -8.83 17.67 -26.50 35.34 -44.17 0 dB = 19.0 W/kg = 12.79 dBW/kg Certificate No: Z18-60042 Page 12 of 16





Impedance Measurement Plot for Head TSL

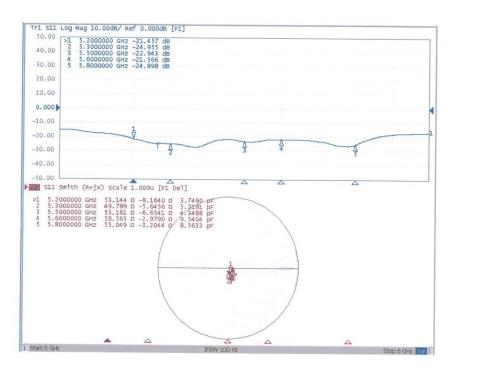

Certificate No: Z18-60042

Page 13 of 16



Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 E-mail: cttl@chinattl.com	-		
DASY5 Validation Report for Body TSL. Test Laboratory: CTTL, Beijing, China DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - Communication System: CW; Frequency: 5200 H Frequency: 5500 MHz, Frequency: 5600 MHz, Freq Medium parameters used: f = 5200 MHz; σ = 5.288 kg/m3, Medium parameters used: f = 5300 MHz; σ = 1000 kg/m3, Medium parameters used: f = 5500 MH ρ = 1000 kg/m3, Medium parameters used: f = 560 48.05; ρ = 1000 kg/m3, Medium parameters used: f = 560 48.05; ρ = 1000 kg/m3, Medium parameters used: f ϵr = 47.65; ρ = 1000 kg/m3, Phantom section: Center Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C6 DASY5 Configuration: • Probe: EX3DV4 - SN7464; ConvF(5.39, 5.39, 5. ConvF(5.19, 5.19, 5.19); Calibrated: 9/12/2017, Calibrated: 9/12/2017, ConvF(4.5,4.5,4.5); Calib ConvF(4.67,4.67,4.67); Calibrated: 9/12/2017, • Sensor-Surface: 1.4mm (Mechanical Surface De Electronics: DAE4 Sn1525; Calibrated: 2017-10 • Phantom: Triple Flat Phantom 5.1C; Type: QD 00 • Measurement SW: DASY52, Version 52.10 (0); (7417)	MHz, Frequency: 5300 MHz, uency: 5800 MHz, 5 mho/m; $\epsilon r = 48.89$; $\rho = 1000$ = 5.398 mho/m; $\epsilon r = 48.67$; $\rho =$ z; $\sigma = 5.674$ mho/m; $\epsilon r = 48.24$; 0 MHz; $\sigma = 5.813$ mho/m; $\epsilon r =$ = 5800 MHz; $\sigma = 6.093$ mho/m; 33.19-2007) 39); Calibrated: 9/12/2017, ConvF(4.61,4.61,4.61); rated: 9/12/2017, etection) -02 00 P51 CA; Serial: 1161/3 5 SEMCAD X Version 14.6.10		
Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.11 V/m; Power Drift = -0.01 dB Peak SAR (extrapolated) = 32.2 W/kg SAR(1 g) = 7.09 W/kg; SAR(10 g) = 1.98 W/kg Maximum value of SAR (measured) = 17.3 W/kg			
Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 62.15 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 33.3 W/kg SAR(1 g) = 7.12 W/kg; SAR(10 g) = 1.98 W/kg Maximum value of SAR (measured) = 17.5 W/kg			
Certificate No: Z18-60042 Page 14 of 16			






Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.49 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 37.5 W/kg SAR(1 g) = 7.72 W/kg; SAR(10 g) = 2.14 W/kg Maximum value of SAR (measured) = 19.5 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 64.69 V/m; Power Drift = 0.00 dB Peak SAR (extrapolated) = 36.4 W/kg SAR(1 g) = 7.52 W/kg; SAR(10 g) = 2.1 W/kg Maximum value of SAR (measured) = 18.5 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 62.28 V/m; Power Drift = 0.00 dB Peak SAR (extrapolated) = 37.9 W/kg SAR(1 g) = 7.27 W/kg; SAR(10 g) = 2.02 W/kg Maximum value of SAR (measured) = 18.5 W/kg

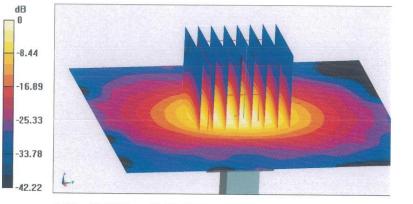


0 dB = 18.5 W/kg = 12.67 dBW/kg

Certificate No: Z18-60042


Page 15 of 16



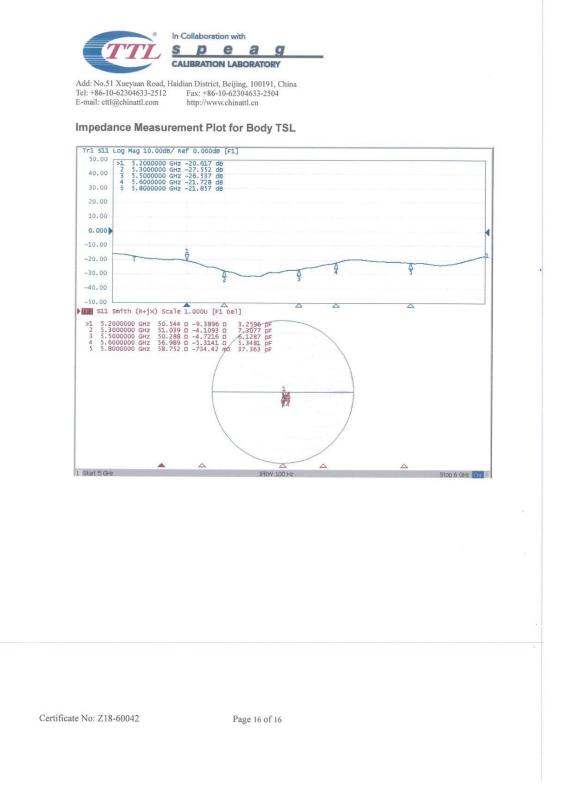



ANNEX D. Accreditation Certification

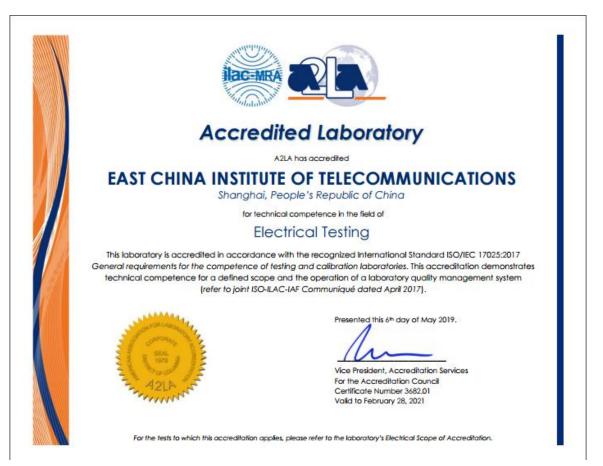

***********End of the Report*********