

ELECTRONIC TECHNOLOGY SYSTEMS DR. GENZ GMBH

TEST - REPORT

SAR Compliance Test Report

Test report no.:

G6M204040005-S-8

SAR



TABLE OF CONTENTS

1	General information
1.1	Notes
1.2	Testing laboratory
1.3	Details of approval holder
1.4	Manufacturer
1.5	Application details
1.6	Test item
1.7	Test results
1.8	Test standards
2	Technical test
2.1	Summary of test results
2.2	Test environment
2.3	Test equipment utilized
2.4	Definitions
2.5	Measurement system description
2.6	Test system specification
2.7	Measurement procedure
2.8	Reference points
2.9	Test positions
2.10	Measurement uncertainty
3	Tissue and system verification
3.1	Tissue verification
3.2	System verification
4	Test Results
5	References
6	Appendix



1 General Information

1.1 Notes

The purpose of conformity testing is to increase the probability of adherence to the essential requirements or conformity specifications, as appropriate.

The complexity of the technical specifications, however, means that full and thorough testing is impractical for both technical and economic reasons.

Furthermore, there is no guarantee that a test sample which has passed all the relevant tests conforms to a specification.

The existence of the tests nevertheless provides the confidence that the test sample possesses the qualities as maintained and that is performance generally conforms to representative cases of communications equipment.

The test results of this test report relate exclusively to the item tested as specified in 1.5.

The test report may only be reproduced or published in full.

Reproduction or publication of extracts from the report requires the prior written approval of the ELECTRONIC TECHNOLOGY SYSTEMS DR. GENZ GMBH.

I attest to the accuracy of data. All measurements reported herein were performed by me or were made under my supervision and are correct to the best of my knowledge and belief. I assume full responsibility for the completeness of these measurements and vouch for the qualification of all persons taking them.

Tester:

12.07.2004		N. Kaspar	Unbert Waspar	
Date	ETS-Lab.	Name	Signature	

Technical responsibility for area of testing:

12.07.2004		Dr. Genz	i.H. lea
Date	ETS	Name	Signature



1.2 **Testing laboratory**

1.2.1 Location

ELECTRONIC TECHNOLOGY SYSTEM DR. GENZ GMBH (ETS)

Storkower Straße 38c

D-15526 Reichenwalde b. Berlin

Germany

Telephone: +49 33631 888 00 : +49 33631 888 660 Fax

1.2.2 **Details of accreditation status**

ACCREDITED TESTING LABORATORY

DAR-REGISTRATION NUMBER: TTI-P-G 126/96

FCC FILED TEST LABORATORY REG. No. 96970

BLUETOOTH QUALIFICATION TEST FACILITY (BQTF)

ACCREDITED BY BLUETOOTH QUALIFICATION REVIEW BOARD

INDUSTRY CANADA FILED TEST LABORATORY REG. No. IC 3470

A2LA ACCREDITED Certificate Number 1983-01

1.3 **Details of approval holder**

Name : Compal Communications Inc. Street : 7F, 319, Sec. 4, Pa-Teh Road

Town : Taipei (105) Country : Taiwan, R.O.C. Telephone : +886-2-2528-8198 Fax : +886-2-2748-7547 Contact : Mr. Jacky Wu

E-Mail : Jacky Wu@compal.com

1.4 Manufacturer: (if applicable)

Name Street Town Country

ETS Dr. Genz GmbH, Germany



1.5 Application details

Date of receipt of application : 29.04.2004 Date of receipt of test item : 29.04.2004

Date of test : 11.06.2004 - 24.06.2004

1.6 Test item

FCC ID : QQXEB-X500U

Description of test item : GPRS Dual-Band (GSM850/PCS1900) Handset Phase II+

Type identification : EB-X500U

Serial number : without; Identical prototype

Device category : PCE (Licensed Portable Transmitter held to ear)

Technical data

GSM850 PCS 1900

TX Frequency range : 824,2 - 848,8 MHz 1850,2 - 1909,8 MHz
RX Frequency range : 869,2 - 893,8 MHz 1930,2 - 1989,8 MHz

Max. Radiated RF output power : 30,7 dBm / (1174,9 mW) 30,4 dBm / (1096,48 mW)

Power supply : 3,8 V DC rechargeable battery

Antenna Tx : integral
Antenna RX : integral

Additional information : Tx and Rx. antenna are the same.

1.7 Test Results

Max. SAR Measurement : 0,223 W/kg (averaged over 1 gram)

This EUT has been shown to be capable of compliance for localized specific absorption rate (SAR) for uncontrolled environment/general population exposure limits specified in ANSI/IEEE Std. C95.1-1992 and had been tested in accordance with the measurement procedures specified in FCC/OET Bulletin 65 Supplement C (2001) and IEEE Std. 1528-2003, December 2003.

ETS Dr. Genz GmbH, Germany



1.8 Test standards

Standards : - IEEE Std. 1528-2003, December 2003

FCC Rule Part(s) : - FCC OET Bulletin 65, Supplement C, Edition 01-01

2 Technical test

2.1 Summary of test results

Applicable Configuration

Handset (Head)	X
Handset (Body)	X
Headset (Head)	
Body Worn Equipment	

EUT complies with the RF radiation exposure limits of the FCC as shown by the SAR measurement results. These measurements are taken to simulate the RF effects exposure under worst-case conditions. The EUT complies with the requirements in respect to all parameters subject to the test. The test results and statements relate only to the item(s) tested.

Please note that the absorption and distribution of electromagnetic energy in the body are very complex phenomena that depend on the mass, shape, and size of the body, the orientation of the body with respect to the field vectors, and the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because innumerable factors may interact to determine the specific biological outcome of an exposure to electromagnetic fields, any protection guide shall consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables. [1]

In case of multiple hotspots the hotspot with the highest value is displayed only. All other hotspots are measured and stored by the measurement system too. Only the highest value is displayed as cube in the measurement plot and the results table. All other hotspots are at least 2 dB lower than maximum hotspot.

2.2 Test environment

Room temperature : 22,1 -22,5 °C

Liquid temperature : 22,0 -22,3 °C

Relative humidity content : 20 ... 75 %

Air pressure : 86 ... 103 k P a

Details of power supply : 3,8 V DC

ETS Dr. Genz GmbH, Germany



2.3 Test equipment utilized

No.	Measurement device:	Type:	Manufacturer:
ETS 0449	Stäubli Robot	RX90B L	Stäubli
ETS 0450	Stäubli Robot Controller	CS/MBs&p	Stäubli
ETS 0451	DASY 4 Measurement Server		Schmid & Partner
ETS 0452	Control Pendant		Stäubli
ETS 0453	Compaq Computer	Pentium IV, 2 GHz,	Schmid & Partner
ETS 0454	Dabu Acquisition Electronics	DAE3V1	Schmid & Partner
ETS 0455	Dummy Probe		Schmid & Partner
ETS 0456	Dosimetric E-Field Probe	ET3DV6	Schmid & Partner
ETS 0457	Dosimetric E-Field Probe	ET3DV6	Schmid & Partner
ETS 0458	Dosimetric H-Field Probe	H3DV6	Schmid & Partner
ETS 0459	System Validation Kit	D900V2	Schmid & Partner
ETS 0460	System Validation Kit	D1800V2	Schmid & Partner
ETS 0461	System Validation Kit	D1900V2	Schmid & Partner
ETS 0462	System Validation Kit	D2450V2	Schmid & Partner
ETS 0463	Probe Alignment Unit	LBV2	Schmid & Partner
ETS 0464	SAM Twin phantom	V 4.0	Schmid & Partner
ETS 0465	Mounting Device	V 3.1	Schmid & Partner
ETS 0224a	Millivoltmeter	URV 5	Rohde & Schwarz
ETS 0219	Power sensor	NRV-Z2	Rohde & Schwarz
ETS 0268	RF signal generator	SMP 02	Rohde & Schwarz
ETS 0322	Insertion unit	URV5-Z4	Rohde & Schwarz
ETS 0466	Directional Coupler	HP 87300B	HP
ETS0231	Radio Communication Tester	CMD65	Rohde & Schwarz
ETS 0467	Universal Radio Communication Tester	CMU 200	Rohde & Schwarz
ETS 0468	Network Analyzer 300 kHz to 3 GHz	8753C	Agilent
ETS 0469	Dielectric Probe Kit	85070C	Agilent



2.4 Definitions

2.4.1 SAR

The specific absorption rate (SAR) is defined as the time derivative of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dV) of a given density (ρ_t) , expressed in watts per kilogram (W/kg)

SAR =
$$\frac{d}{dt} \left(\frac{dW}{dm} \right) = \frac{d}{dt} \left(\frac{dW}{\rho_t dV} \right) = \frac{\sigma}{\rho_t} |E_t|^2$$

where:

$$\frac{dW}{dt} = \int_{V} E \cdot J \, dV = \int_{V} \sigma E^2 dV$$

2.4.2 Uncontrolled Exposure

The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity. Warning labels placed on low-power consumer devices such as cellular telephones are not considered sufficient to allow the device to be considered under the occupational/controlled category, and the general population/uncontrolled exposure limits apply to these devices. [2]

2.4.3 Controlled Exposure

In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means. Awareness of the potential for RF exposure in a workplace or similar environment can be provided through specific training as part of a RF safety program. If appropriate, warning signs and labels can also be used to establish such awareness by providing prominent information on the risk of potential exposure and instructions on the risk of potential exposure risks. [2]

ETS Dr. Genz GmbH, Germany



2.5 Measurement System Description

2.5.1 System Setup

Measurements are performed using the DASY4 automated dosimetric assessment system (figure 1) made by Schmid & Partner Engineering AG (SPEAG)in Zurich, Switzerland.

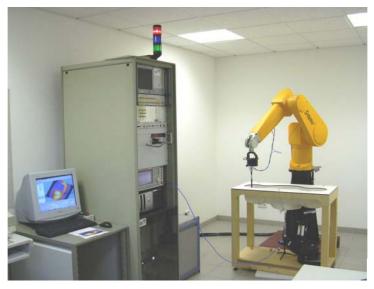


Figure 1

The DASY4 system for performing compliance tests consists of the following items:

- A standard high precision 6-axis robot (Stäubli RX family) with controller, teach pendant and software. An arm extension for accommodating the data acquisition electronics (DAE).
- A dosimetric probe, i.e., an isotropic E-field probe optimized and calibrated for usage in tissue simulating liquid. The probe is equipped with an optical surface detector system.
- A data acquisition electronics (DAE) which performs the signal amplification, signal multiplexing, AD-conversion, offset measurements, mechanical surface detection, collision detection, etc. The unit is battery powered with standard or rechargeable batteries. The signal is optically transmitted to the EOC.
- An unit to operate the optical surface detector which is connected to the EOC.
- The Electro-optical converter (EOC) performs the conversion from the optical into a digital electric signal of the DAE. The EOC is connected to the measurement server.
- The functions of the measurement server is to perform the time critical task such as signal filtering, surveillance of the robot operation, fast movement interrupts.
- A probe alignment unit which improves the (absolute) accuracy of the probe positioning.
- A computer operating Windows 2000 or Windows NT.
- DASY4 software.
- Remote control with teach pendant and additional circuitry for robot safety such as warning lamps, etc.
- The SAM twin phantom enabling testing left-hand and right-hand usage.
- The device holder for handheld mobile phones.
- Tissue simulating liquid mixed according to the given recipes (see Application Notes).
- System validation dipoles allowing to validate the proper functioning of the system.



2.5.2 Phantom Description



Figure 2

The SAM twin phantom V4.0 (figure 2) is a fiberglass shell phantom with 2 mm shell thickness. It has three measurement areas:

- Left hand
- Right hand
- Flat phantom

The phantom is integrated in a wooden table.

The bottom plate of the table contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. Only one device holder is necessary if two phantoms are used (e.g., for different liquids).

A cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. Free space scans of devices on the cover are possible.

On the phantom top, three reference markers are provided to identify the phantom positions with respect to the robot.

2.5.3 Tissue Simulating Liquids

The parameters of the tissue simulating liquid strongly influence the SAR. The parameters for the different frequencies are defined in the corresponding compliance standards (e.g., EN 50361, IEEE P1528-200X).

Tissue dielectric properties

	Не	ad	В	ody
Frequency (MHz)	Relative Dielectric Constant (ε _r)	Conductivity (σ) (S/m)	Relative Dielectric Constant (ε _r)	Conductivity (σ) (S/m)
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
900	41.5	0.97	55.0	1.05
1450	40.5	1.20	54.0	1.30
1800	40.0	1.40	53.3	1.52
1900	40.0	1.40	53.3	1.52
2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73

ETS Dr. Genz GmbH, Germany



2.5.4 Device Holder

The DASY device holder (figure 3.1 and 3.2) is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear openings). The rotation centers for both scales is the ear opening. Thus the device needs no repositioning when changing the angles.



Figure 3.1

The DASY device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity $\varepsilon = 3$ and loss tangent $\delta = 0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.

Figure 3.2

2.5.5 Probes

The SAR measurements were conducted with the dosimetric probe ET3DV6 (figure 4), designed in the classical triangular configuration and optimized for dosimetric evaluation. [3] The probe is constructed using the thick film technique; with printed resistive lines on ceramic substrates. The probe is equipped with an optical multifiber line ending at the front of the probe tip. It is connected to the EOC box on the robot arm and provides an automatic detection of the phantom surface. Half of the fibers are connected to a pulsed infrared transmitter, the other half to a synchronized receiver. As the probe approaches the surface, the reflection from the surface produces a coupling from the transmitting to the receiving fibers. This reflection increases first during the approach, reaches maximum and then decreases. If the probe is flatly touching the surface, the coupling is zero. The distance of the coupling maximum to the surface is independent of the surface reflectivity and largely independent of the surface to probe angle. The DASY4 software reads the reflection during a software approach and looks for the maximum using a 2nd order fitting. The approach is stopped at reaching the maximum.



Figure 4



Probe Specifications

Calibration: In air from 10 MHz to 2.5 GHz

In brain and muscle simulating tissue at Frequencies of 835 MHz, 900

MHz, 1800 MHz, 1900 MHz and 2450 MHz Calibration certificates please find attached.

Frequency: 10 MHz to > 3 GHz; Linearity: $\pm 0.2 \text{ dB}$ (30 MHz to 3 GHz)

Directivity: $\pm 0.2 \text{ dB}$ in HSL (rotation around probe axis)

± 0.4 dB in HSL (rotation normal probe axis)

Dynamic Range: $5 \mu \text{W/g to} > 100 \text{ mW/g}$;

Linearity: $\pm 0.2 \text{ dB}$

Dimensions: Overall length: 330 m

Tip length: 16 mm Body diameter: 12 mm Tip diameter: 6.8 mm

Distance from probe tip to dipole centers: 2.7 mm

Application: General dosimetry up to 3 GHz

Compliance tests of mobile phones

Fast automatic scanning in arbitrary phantoms

2.6 Test System Specification

Positioner

Robot: Stäubli Animation Corp. Robot Model: RX90B L

Repeatability: 0.02 mm

No. of axis:

Data Acquisition Electronic (DAE) System

Cell Controller

Processor: Pentium IV Clock Speed: 2.0 GHz

Operating System: Windows 2000
Data Card: DASY4 PC-Board

Data Converter

Features: Signal Amplifier, multiplexer, A/D converter, & control logic

Software: DASY4 software

Connecting Lines: Optical downlink for data and status info.

Optical uplink for commands and clock

PC Interface Card

Function: 24 bit (64 MHz) DSP for real time processing

Link to DAE3

16 bit A/D converter for surface detection system

serial link to robot

direct emergency stop output for robot

ETS Dr. Genz GmbH, Germany Registration number: G6M204040005-S-8 Page 11 of 27



E-Field Probes

Model: ET3DV6 SN1711

Construction: Triangular core fiber optic detection system

Frequency: 10 MHz to 6 GHz

Linearity: $\pm 0.2 \text{ dB } (30 \text{MHz to 3 GHz})$

Phantom

Phantom: SAM Twin Phantom (V4.0)

Shell Material: Fiberglass Thickness: $2.0 \pm 0.2 \text{ mm}$

2.7 Measurement Procedure

The evaluation was performed using the following procedure:

- 1. The SAR measurement was taken at a selected spatial reference point to monitor power variations during testing. This fixed location point was measured and used as a reference value.
- 2. The SAR distribution at the exposed side of the head was measured at a distance of 3.9mm from the inner surface of the shell. The area covered the entire dimension of the head and the horizontal grid spacing was 10mm x 10mm.
- 3. Based on the area scan data, the area of the maximum absorption was determined by spline interpolation. Around this point, a volume of 30mm x 30mm x 30mm (fine resolution volume scan, zoom scan) was assessed by measuring 5 x 5 x 5 points. On this basis of this data set, the spatial peak SAR value was evaluated with the following procedure:
 - a. The data at the surface was extrapolated, since the center of the dipoles is 2.7mm away from the tip of the probe and the distance between the surface and the lowest measuring point is 1.2mm. The extrapolation was based on a least square algorithm [4]. A polynomial of the fourth order was calculated through the points in z-axes. This polynomial was then used to evaluate the points between the surface and the probe tip.
 - b. The maximum interpolated value was searched with a straight-forward algorithm. Around this maximum the SAR values averaged over the spatial volumes (1g or 10g) were computed using the 3D-Spline interpolation algorithm. The 3D-spline is composed of three one-dimensional splines with the "Not a knot" condition (in x, y, and z directions) [4] [5]. The volume was integrated with the trapezoidal algorithm. One thousand points (10 x 10 x 10) were interpolated to calculate the average.
 - c. All neighboring volumes were evaluated until no neighboring volume with a higher average value was found.
- 4. The SAR reference value, at the same location as procedure #1, was remeasured. If the value changed by more than 5%, the evaluation is repeated.


ETS Dr. Genz GmbH, Germany Registration number: G6M204040005-S-8 Page 12 of 27



2.8 Reference Points

2.8.1 Ear Reference Points

Figure 5.1 shows the front, back and side vies of SAM. The point "M" is the reference point for the center of mouth, "LE" is the left ear reference point (ERP), and "RE" is the right ERP. The ERPs are 15 mm posterior to the entrance to ear canal (EEC) along the B-M line (Back-Mouth), as shown in Figure 5.2. The plane passing through the two ear reference points and M is defined as the Reference Plane. The line N-F (Neck-Front) perpendicular to the reference plane and passing through the RE (or LE) is called the Reference Pivoting Line (see Figure 5.3). Line B-M is perpendicular to the N-F line. Both N-F and B-M lines should be marked on the external phantom shell to facilitate handset positioning. Posterior to the N-F line, the thickness of the N-F line, the ear is truncated as illustrated in Figure 5.2. The ear truncation is introduced to avoid the handset from touching the ear lobe, which can cause unstable handset positioning at the cheek. [6]

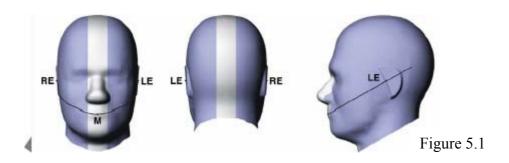






Figure 5.2





2.8.2 Handset Reference Points

Two imaginary lines on the handset were defined: the vertical centerline and the horizontal line. The vertical centerline passes through two points on the front side of the handset: the midpoint of the width w_t of the handset at the level of the acoustic output (point A on Figures 6.1 and 6.2), and the midpoint of the width wb of the bottom of the handset (point B). The horizontal line is perpendicular to the vertical centerline and passes through the center of the acoustic output (see Figure 6.1). The two lines intersect at point A. For many handsets, point A coincides with the center of the acoustic output. However, the acoustic output may be located elsewhere on the horizontal line. The vertical centerline is not necessarily parallel to the front face of the handset (see Figure 6.2), especially for clamshell handsets, handsets with flip pieces, and other irregularly-shaped handsets.

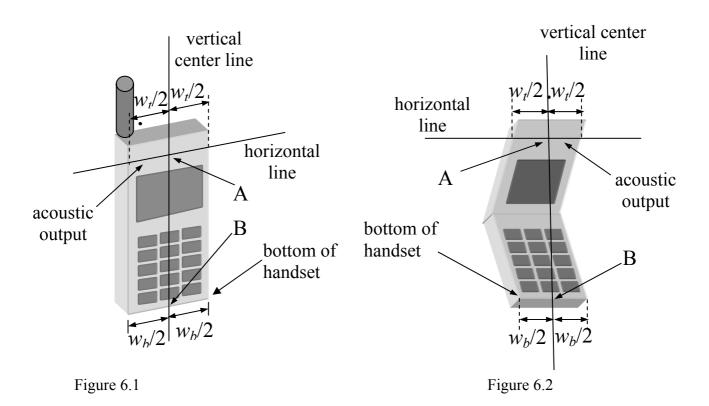



2.9 Test Positions

2.9.1 "Cheek" / "Touch" Position

The EUT was positioned close to the surface of the phantom such that point A is on the (virtual) extension of the line passing through points RE and LE on the phantom (see Figure 7), such that the plane defined by the vertical center line and the horizontal line of the handset is approximately parallel to the sagittal plane of the phantom.

The EUT was translated towards the phantom along the line passing through RE and LE until the handset touches the pinna.

While maintaining the handset in this plane, the EUT was rotated it around the LE-RE line until the vertical centerline was in the plane normal to MB-NF including the line MB (called the reference plane).

The EUT was rotated around the vertical centerline until the handset (horizontal line) was symmetrical with respect to the line NF.

While maintaining the vertical centerline in the reference plane, keeping point A on the line passing through RE and LE and maintaining the handset contact with the pinna, the EUT was rotated about the line NF until any point on the handset was in contact with a phantom point below the pinna (cheek). [6] See Figure 7.



Figure 7



2.9.2 "Tilted" Position

The EUT was in "cheek position".

While maintaining the orientation of the handset move the handset away from the pinna along the line passing through RE and LE in order to enable a rotation of the handset by 15 degrees.

The EUT was rotated around the horizontal line by 15 degrees.

While maintaining the orientation of the handset, the EUT was moved towards the phantom on a line passing through RE and LE until any part of the handset touched the ear. The tilted position is obtained when the contact is on the pinna. If the contact was at any location other than the pinna (e.g., the antenna with the back of the phantom head), the angle of the handset would be reduced. In this case, the tilted position is obtained if any part of the handset was in contact with the pinna as well as a second part of the handset was in contact with the phantom (e.g., the antenna with the back of the head). [6] See Figure 8.



Figure 8



2.9.3 Belt Clip/Holster Configuration

Test configurations for body-worn operated EUTs are carried out while the belt-clip and/or holster is attached to the EUT and placed against a flat phantom in a regular configuration (see Figure 9). An EUT with a headset output is tested with a headset connected to the device.

Body dielectric parameters are used.

There are two categories for accessories for body-worn operation configurations:

- 1. accessories not containing metallic components
- 2. accessories containing metallic components.

When the EUT is equipped with accessories not containing metallic components the tests are done with the accessory that dictates the closest spacing to the body. For accessories containing metallic parts a test with each one is implemented. If the multiple accessories share an identical metallic component (e.g. the same metallic belt-clip used with different holsters with no other metallic components) only the accessory that has the closest spacing to the body is tested.

In case that a EUT authorized to be body-worn is not supplied or has no options to be operated with any accessories, a test configuration where a separation distance between the back of the device and the flat phantom is used. All test position spacings are documented.

Transmitters operating in front of a person's face (e.g. push-to-talk configurations) are tested for SAR compliance with the front of the device positioned to face the flat platform. SAR Compliance tests for shoulder, waist or chest-worn transmitters are carried out with the accessories including headsets and microphones attached to the device and placed against a flat phantom in a regular configuration.

The SAR measurements are performed to investigate the worst-case positioning. This is documented and used to perform Body SAR testing. [2].



Figure 9

ETS Dr. Genz GmbH, Germany



2.9.4 Headset Configuration

Headsets which have their radiating structure in close proximity to the head are measured according to the following conditions.

- Head tissue liquid is used.
- The EUT is positioned on the surface of the head of phantom according the picture below. Right and left position is tested according to the normal use (see figure 10).
- Additional metallic parts like clips or others are subject of testing, too.



Figure 10

Headsets which have their radiating structure in close proximity to the body are tested as body worn equipment.



2.10 Measurement uncertainty

The uncertainty budget has been determined for the DASY4 system performance check according to IEEE Std. 1528-2003, December 2003.

	Tol.	Prob.	Div.	$(^{c}i^{)1}$	Std. unc.	$(v_i)^{2}$
Error Description	(± %)	dist.		(1g)	(1g) (± %)	
Measurement System						
Probe Calibration	4.8	N	1	1	4.8	8
Axial Isotropy	4.7	R	√3	0.7	1.9	8
Hemispherical Isotropy	9.6	R	√3	0.7	3.9	8
Boundary Effects	1.0	R	√3	1	0.6	8
Linearity	4.7	R	√3	1	2.7	8
System Detection Limit	1.0	R	√3	1	0.6	∞
Readout Electronics	1.0	N	1	1	1.0	∞
Response Time	0.8	R	√3	1	0.5	∞
Integration Time	2.6	R	√3	1	1.5	∞
RF Ambient Conditions	3.0	R	√3	1	1.7	∞
Probe Positioner	0.4	R	√3	1	0.2	∞
Probe Positioning	2.9	R	√3	1	1.7	∞
Algorithms for Max. SAR Eval.	1.0	R	$\sqrt{3}$	1	0.6	∞
Test Sample Related						
Device Positioning	2.9	N	1	1	2.9	145
Device Holder	3.6	N	1	1	3.6	5
Power Drift	5.0	R	$\sqrt{3}$	1	2.9	∞
Phantom and Setup			,			
Phantom Uncertainty	4.0	R	√3	1	2.3	∞
Liquid Conductivity (target)	5.0	R.	√3	0.64	1.8	∞
Liquid Conductivity (meas.)	2.6	N	1	0.64	1.7	∞
Liquid Permittivity (target)	5.0	R	$\sqrt{3}$	0.6	1.7	∞
Liquid Permittivity (meas.)	3.8	N	1	0.6	2.3	∞
Combined Standard Uncertainty					10.4	330
Expanded Uncertainty kp=2						
Coverage Factor for 95%					20.8	

The budget is valid for the frequency range 300 MHz - 3 GHz and represent a worst case analysis. For specific tests and configurations, the uncertainty could be considerable smaller.



3. Tissue and System Verification

3.1 Tissue Verification

Dielectric parameters of the simulating liquids were verified using a Dielectric Probe Kit Agilent 85070D to a tolerance of \pm 5 %.

Room Temperature: 22,1 -22,5 °C

		Measured Tissue Parameters					
	900 MI	Hz Brain	1900 MHz Brain				
	Target Measured Target 22.06.2004		Measured 15.06.2004				
Room Temperature:		22,1 ° C		22,0 ° C			
Liquid Temperature:		22,0 ° C		22,3 ° C			
Dielectric Constant: ε	41,5	41,3	40,0	39,8			
Conductivity: σ	0,97	0,96	1,40	1,42			

Room Temperature: 22,1 -22,5 °C

		Measured Tissue Parameters					
	900 MHz Muscle 1900 MHz Muscle						
	Target	Measured 11.06.2004					
Room Temperature:		22,0 ° C		22,0 ° C			
Liquid Temperature:		22,0 ° C		22,1 ° C			
Dielectric Constant: ε	55,0	54,4	53,3	51,9			
Conductivity: σ	1,05	1,04	1,52	1,58			



3.2 System Verification

Prior to the assessment, the system was verified by using a 900 MHz /1900 MHz validation dipole. Power level of 250mW was supplied to the dipole antenna placed under the flat section of SAM Phantom. This system validation is valid for a frequency range of 900 ± 100 MHz.

The system was verified to a tolerance of \pm 10 %.

Liquid Temperature: 22,0 -22,3 ° C Room Temperature: 22,1 -22,5 ° C Liquid Depth: >15.5 cm

System Dipole Validation Target & Measurement								
Date	System Validation Kit:	Liquid	Targeted SAR 1g (mW/g)	Measured SAR 1g (mW/g)	Deviation (%)			
22.06.2004	D900V2 SN164	900 MHz Head	10,2	10,32	1,17			
23.06.2004	D900V2 SN164	900 MHz Head	10,2	10,12	-0,78			
15.06.2004	D1900V2 SN5d025	1900 MHz Head	40,4	39,80	-1,48			
16.06.2004	D1900V2 SN5d025	1900 MHz Head	40,4	40,80	0,99			

Liquid Temperature: 22,0 -22,3 ° C Room Temperature: 22,1 -22,5 ° C Liquid Depth: >15.5 cm

System Dipole Validation Target & Measurement							
Date System Validation Liquid Kit:			Targeted SAR 1g (mW/g)	Measured SAR 1g (mW/g)	Deviation (%)		
24.06.2004	D900V2 SN164	900 MHz Muscle	11,2	11,0	-1,79		
11.06.2004	D1900V2 SN5d025	1900 MHz Muscle	45,6	42,20	-7,45		
14.06.2004	D1900V2 SN5d025	1900 MHz Muscle	45,6	42,60	-6,57		

Comment: Please find attached the measurement plots.

ETS Dr. Genz GmbH, Germany Registration number: G6M204040005-S-8 Page 21 of 27



4. Test Results

Procedures Used To Establish Test Signal

The EUT was placed into simulated call mode (e.g. AMPS, Cellular CDMA & PCS CDMA modes) using manufacturers test codes. Such test signals offer a consistent means for testing SAR and are recommended for evaluating SAR [2]. The actual transmission is activated through a base station simulator or similar when test modes are not available or inappropriate for testing the EUT.

The EUT is rechargeable battery operated. The battery used for the SAR measurements was completely charged. The device was tested at full power verified by implementing conducted output power measurements. For confirming of the output power it was tested before and after each SAR measurement. The test was repeated if a conducted power deviation of more than 5 % occurred.

Mixture Type: 900 MHz Head

Date: 22.06.2004 - 23.06.2004

Liquid Temperature: 22,0 -22,3 °C Room Temperature: 22,1 -22,5 °C

Sample under slide closed condition.

Frequency		Power Drift	Antenna Pos.	Phantom	Test	SAR	
MHz	Channel	Modulation	dBm		Section	Position	(W/kg)
824,2	128	GSM	0,0	Integral ant1	Right Ear	Cheek	0,072
836,4	189	GSM	-0,0	Integral ant1	Right Ear	Cheek	0,095
836,4	189	GSM	0,0	Integral ant1	Right Ear	Tilt	0,049
836,4	189	GSM	0,0	Integral ant1	Left Ear	Cheek	0,082
836,4	189	GSM	-0,0	Integral ant1	Left Ear	Tilt	0,054
848,8	251	GSM	-0,0	Integral ant1	Right Ear	Tilt	0,051

Sample under slide open condition.

	Frequency	7	Power Drift	Antenna Pos.	Phantom	Test	SAR
MHz	Channel	Modulation	dBm		Section	Position	(W/kg)
824,2	128	GSM	0,1	Integral ant1	Right Ear	Cheek	0,036
836,4	189	GSM	0,0	Integral ant1	Right Ear	Cheek	0,068
836,4	189	GSM	-0,1	Integral ant1	Right Ear	Tilt	0,029
836,4	189	GSM	0,0	Integral ant1	Left Ear	Cheek	0,046
836,4	189	GSM	0,1	Integral ant1	Left Ear	Tilt	0,027
848,8	251	GSM	0,1	Integral ant1	Right Ear	Tilt	0,026

ETS Dr. Genz GmbH, Germany Registration number: G6M204040005-S-8 Page 22 of 27



Page 23 of 27

Mixture Type: 900 MHz Muscle
Date: 24.06.2004
Liquid Temperature: 22.0 -22.3 °C

Liquid Temperature: 22,0 -22,3 °C Room Temperature: 22,1 -22,5 °C

Sample under slide close condition.

	Frequency	7	Power Drift	Antenna Pos.	Phantom	Test	SAR
MHz	Channel	Modulation	dBm		Section	Position -15 mm	(W/kg)
824,2	128	GSM	-0,1	Integral	Flat	Back	0,103
836,4	189	GSM	-0,1	Integral	Flat	Front	0,019
836,4	189	GSM	0,0	Integral	Flat	Back	0,087
848,8	251	GSM	0,0	Integral	Flat	Back	0,078

Note: Device positioning: spacing from flat phantom was adjusted at 1.5 cm.

Sample under slide open condition.

	Frequency	,	Power Drift	Antenna Pos.	Phantom	Test	SAR
MHz	Channel	Modulation	dBm		Section	Position -15 mm	(W/kg)
824,2	128	GSM	-0,0	Integral	Flat	Back	0,064
836,4	189	GSM	-0,0	Integral	Flat	Front	0,009
836,4	189	GSM	0,1	Integral	Flat	Back	0,063
848,8	251	GSM	0,0	Integral	Flat	Back	0,062

Note: Device positioning: spacing from flat phantom was adjusted at 1.5 cm.

Limits:

T	SAR (W/kg)				
Exposure Limits	Uncontrolled Exposure/General Population Environment	Controlled Exposure/Occupational Environment			
Spatial Average SAR (averaged over the whole body)	0.08	0.40			
Spatial Peak SAR (averaged over any 1g of tissue)	1.60	8.00			
Spatial Peak SAR (Hands, Feet, Ankles, Wrist) (averaged over any 10g of tissue)	4.00	20.00			

Notes:

- 1. Test data represent the worst case SAR value and test procedure used are according to OET Bulletin 65, Supplement C (01-01).
- 2. All modes of operation were investigated.

ETS Dr. Genz GmbH, Germany Registration number: G6M204040005-S-8



Mixture Type: 1900 MHz Head Date: 15.06.2004 - 16.04.2004

Liquid Temperature: 22,0 -22,3 °C Room Temperature: 22,1 -22,5 °C

Sample under slide close condition.

	Frequency	7	Power Drift	Antenna Pos.	Phantom	Test	SAR
MHz	Channel	Modulation	dBm		Section	Position	(W/kg)
1850,2	512	GSM	-0,1	Integral ant1	Right Ear	Cheek	0,084
1880,0	661	GSM	-0,1	Integral ant1	Right Ear	Cheek	0,102
1880,0	661	GSM	-0,0	Integral ant1	Right Ear	Tilt	0,098
1909,8	810	GSM	-0,1	Integral ant1	Right Ear	Cheek	0,149
1880,0	661	GSM	-0,1	Integral ant1	Left Ear	Cheek	0,102
1880,0	661	GSM	0,0	Integral ant1	Left Ear	Tilt	0,066

Sample under slide open condition.

	Frequency	7	Power Drift	Antenna Pos.	Phantom	Test	SAR
MHz	Channel	Modulation	dBm		Section	Position	(W/kg)
1850,2	512	GSM	-0,0	Integral ant1	Right Ear	Cheek	0,049
1880,0	661	GSM	-0,1	Integral ant1	Right Ear	Cheek	0,068
1880,0	661	GSM	-0,1	Integral ant1	Right Ear	Tilt	0,037
1909,8	810	GSM	-0,0	Integral ant1	Right Ear	Cheek	0,079
1880,0	661	GSM	-0,1	Integral ant1	Left Ear	Cheek	0,060
1880,0	661	GSM	-0,0	Integral ant1	Left Ear	Tilt	0,033



Mixture Type: 1900 MHz Muscle
Date: 24.04.2002
Liquid Temperature: 22,0 -22,3 °C

erature: 22,0 -22,3 °C Room Temperature: 22,1 -22,5 °C

Sample under slide close condition.

	Frequency	7		Antenna Pos.	Phantom	Test	SAR
MHz	Channel	Modulation	dBm		Section	Position -15 mm	(W/kg)
1850,2	512	GSM	0,0	Integral	Flat	Back	0,119
1880,0	661	GSM	-0,1	Integral	Flat	Front	0,009
1880,0	661	GSM	-0,002	Integral	Flat	Back	0,148
1909,8	810	GSM	-0,0	Integral	Flat	Back	0,223

Sample under slide open condition.

	Frequency		Power Drift	Antenna Pos.	Phantom	Test	SAR
MHz	Channel	Modulation	dBm		Section	Position -15 mm	(W/kg)
1850,2	512	GSM	0,009	Integral	Flat	Back	0,078
1880,0	661	GSM	-0,1	Integral	Flat	Front	0,011
1880,0	661	GSM	-0,0	Integral	Flat	Back	0,101
1909,8	810	GSM	-0,0	Integral	Flat	Back	0,153

Limits:

T	SAR (W/kg)				
Exposure Limits	Uncontrolled Exposure/General Population Environment	Controlled Exposure/Occupational Environment			
Spatial Average SAR (averaged over the whole body)	0.08	0.40			
Spatial Peak SAR (averaged over any 1g of tissue)	1.60	8.00			
Spatial Peak SAR (Hands, Feet, Ankles, Wrist) (averaged over any 10g of tissue)	4.00	20.00			

Notes:

- 3. Test data represent the worst case SAR value and test procedure used are according to OET Bulletin 65, Supplement C (01-01).
- 4. All modes of operation were investigated.

ETS Dr. Genz GmbH, Germany Registration number: G6M204040005-S-8 Page 25 of 27



5. References

- [1] ANSI/IEEE C95.3 1991, IEEE Recommended Practice for the Measurement of Potentially Hazardous Electromagnetic fields, 300 kHz to 100 GHz, New York: IEEE, Aug. 1992
- [2] Federal Communications Commission, OET Bulletin 65 (Edition 97-01), Supplement C (Edition 01-01), Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields, July 2001.
- [3] T. Schmid, O. Egger, N. Kuster, *Automated E-field scanning system for dosimetric assessments*, IEEE Transaction on Microwave Theory and Techniques, vol. 44, Jan. 1996, pp. 105-113.
- [4] W. Gander, *Computermathematics*, Birkhaeuser, Basel, 1992.
- [5] W.H. Press, S.A. Teukolsky, W.T. Vetterling, and B.P. Flannery, *Numerical Recipes in C*, The Art of Scientific Computing, Second edition, Cambridge University Press, 1992.
- [6] IEEE Standards Coordinating Committee 34 IEEE Std. 1528-2003, December 2003 Recommended Practice for Determining the Peak Spatial-Average Absorption Rate (SAR in the Human Body Due to Wireless Communications Devices: Experimental Techniques.
- [7] DASY4 Dosimetric Assessment System Manual; Draft; September 6, 2002; Schmid & Partner Engineering AG



6. Appendix

1. Appendix A Calibration Certificate D900V2 SN164

D1900V2 SN5d025 ET3DV6 SN1711 DAE3V1-522

2. Appendix B Measurement Plots

3. Appendix C Pictures



Appendix A

Calibration Certificate

Schmid & Partner **Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

900 MHz System Validation Dipole

Type:	D900V2
Serial Number:	164
Place of Calibration:	Zurich
Date of Calibration:	September 5, 2002
Calibration Interval:	24 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

> N. Veller Calibrated by:

> Approved by:

Schmid & Partner **Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

DASY

Dipole Validation Kit

Type: D900V2

Serial: 164

Manufactured: April 30, 2002

Calibrated:

September 5, 2002

1. Measurement Conditions

The measurements were performed in the flat section of the new SAM twin phantom filled with head simulating solution of the following electrical parameters at 900 MHz:

Relative Dielectricity 40.6 $\pm 5\%$ Conductivity 0.95 mho/m $\pm 5\%$

The DASY System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 6.5 at 900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 15mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 20mm was aligned with the dipole. The 5x5x7 fine cube was chosen for cube integration. Probe isotropy errors were cancelled by measuring the SAR with normal and 90° turned probe orientations and averaging.

The dipole input power (forward power) was $250 \text{mW} \pm 3 \%$. The results are normalized to 1W input power.

2 SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the <u>advanced extrapolation</u> are:

averaged over 1 cm³ (1 g) of tissue: 10.2 mW/g

averaged over 10 cm³ (10 g) of tissue: 6.56 mW/g

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay:

1.408 ns

(one direction)

Transmission factor:

0.990

(voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 900 MHz:

 $Re{Z} = 50.7 \Omega$

Im $\{Z\} = -5.2 \Omega$

Return Loss at 900 MHz

-25.7 dB

4. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

5. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

6. Power Test

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.


Validation Dipole D900V2 SN:164, d=15 mm


Frequency: 900 MHz, Antenna Input Power: 250 [mW] SAM Phantom; Flat Section; Grid Spacing: Dx = 20.0, Dy = 20.0, Dz = 10.0

Probe: ET3DV6 - SN1507, ConvF(6.50,6.50,6.50) at 900 MHz, IEEE 1528 900 MHz. $\sigma = 0.95$ mho/m $\epsilon_{\rm r} = 40.6$ $\rho = 1.00$ g/cm³

Cubes (2): Peak: 3.80 mW/g \pm 0.03 dB, SAR (1g): 2.54 mW/g \pm 0.03 dB, SAR (10g): 1.64 mW/g \pm 0.02 dB, (Advanced extrapolation) Penetration depth: 12.5 (12.3, 13.0) [mm]

Powerdrift: -0.01 dB

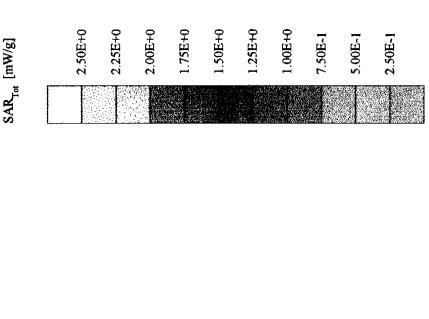

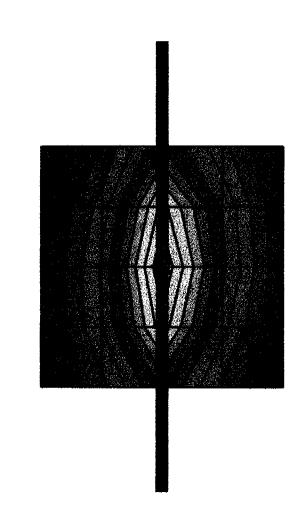


Validation Dipole D900V2 SN:164, d=15 mm

Frequency: 900 MHz, Antenna Input Power: 250 [mW] SAM Phantom; Flat Section; Grid Spacing: Dx = 20.0, Dy = 20.0, Dz = 10.0

Probe: ET3DV6 - SN1507; ConvF(6.50,6.50, 6.50) at 900 MHz; IEEE 1528 900 MHz; $\sigma = 0.95$ mho/m $\epsilon_r = 40.6$ $\rho = 1.00$ g/cm³

Cubes (2): Peak: 4.29 mW/g ± 0.03 dB, SAR (1g): 2.71 mW/g ± 0.03 dB, SAR (10g): 1.72 mW/g ± 0.02 dB, (Worst-case extrapolation)
Penetration depth: 11.6 (10.7, 12.8) [mm]
Powerdrift: -0.01 dB

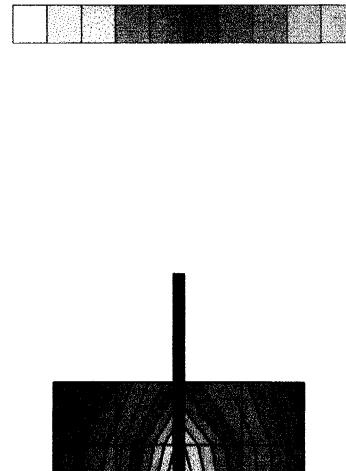

1.25E+0

1.50E+0

1.00E+0

7.50E-1

5.00E-1

2.50E-1

Schmid & Partner Engineering AG, Zurich, Switzerland


2.50E+0

SAR_{Tot} [mW/g]


2.25E+0

2.00E+0

1.75E+0

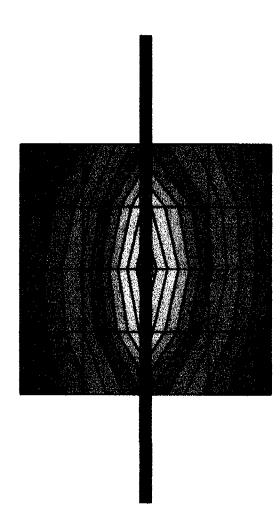

STOP 1 100.000 000 MHz

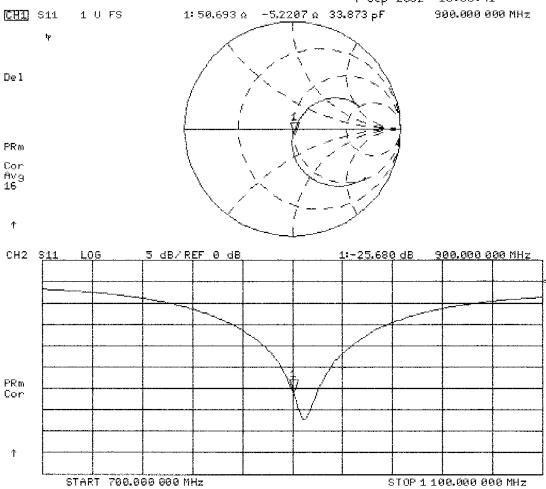



ELECTRONIC TECHNOLOGY SYSTEMS DR. GENZ GMBH - ETS - STORKOWER STRASSE 38c, D-15526 REICHENWALDE B. BERLIN

Tel: 033631 888 00 FAX: 033631 888 660

D2: 900MHz SYSTEM VALIDATION DIPOLE

CALIBRATION CERTIFICATE

900 MHz System Validation Dipole (Muscle)

Туре:	D900V2
Serial Number:	164
Place of Calibration:	Reichenwalde
Date of Calibration:	September 05, 2003
Calibration Interval:	24 month

ETS Dr. Genz GmbH hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of ETS Dr. Genz GmbH.

Wherever applicable, the standards used in the calibration process are traceable to International standards.

Calibrated by: W. Treffke

Approved by: K. Damm



ELECTRONIC TECHNOLOGY SYSTEMS DR. GENZ GMBH - ETS - STORKOWER STRASSE 38c, D-15526 REICHENWALDE B. BERLIN

Tel: 033631 888 00 FAX: 033631 888 660

DASY

DIPOLE VALIDATION KIT

Type: D900V2

Serial: 164

Manufactured: April 30, 2002

Calibrated : September 05, 2003



Measurement Conditions

The measurements were performed in the flat section of the new SAM twin phantom filled with body simulating solution of the following electrical parameters at 900 MHz:

Relative permittivity 54.41 +/- 5 % Conductivity 1.038 mho/m +/- 10 %

The DASY System with a dosimetric E-field probe ET3DV6 (SN: 1711, conversion factor 6.2 at 900 MHz body) was used for the measurements.

The dipole feed-point was positioned below the center marking and oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10 mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 5 mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was 250 mW +/- 3 %. The results are normalized to 1 W input power.



SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 4. The results (see figure supplied) have been normalized to a dipole input power of 1 W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1711 and applying the advanced extrapolation are:

Averaged over 1 cm3 (1 g) of tissue: 11.2 mW/g

Averaged over 10 cm3 (10 g) of tissue: 7.16 mW/g

Dipole impedance and return loss

The dipole was positioned at the flat phantom sections according to section 4 (Measurement conditions) (with body tissue inside the phantom) and the distance holder was in place during impedance measurements.

Feed-point impedance at 900 MHz: Re $\{Z\}$ = 54.3 Ω

Im $\{Z\} = -3.2 \Omega$

Return Loss at 900 MHz: - 23.6 dB

Date/Time: 09/05/03 13:33:02

Test Laboratory: ELECTRONIC TECHNOLOGY SYSTEMS DR. GENZ GMBH

File Name: Dipol Calibr.900 (m) 250mW.da4

Dipol Calibr.900 (m) 250mW

DUT: Dipole 900 MHz; Type: D900V2; Serial: SN: 164

Program: Dipol Calibration 900 Muscle

Communication System: CW; Frequency: 900 MHz; Duty Cycle: 1:1

Medium: Muscle 900 MHz ($\sigma = 1.03749 \text{ mho/m}, \epsilon_r = 54.4094, \rho = 1000 \text{ kg/m}^3$)

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 SN1711; ConvF(6.2, 6.2, 6.2); Calibrated: 11/29/2002
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn522; Calibrated: 9/11/2002
- Phantom: SAM 12; Type: TP-1217; Serial: QD000P40CA
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

(250 mW)/Area Scan (101x161x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 55.5 V/m

Power Drift = 0.009 dB

Maximum value of SAR = 3.03 mW/g

(250 mW)/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 4.05 W/kg

SAR(1 g) = 2.8 mW/g; SAR(10 g) = 1.79 mW/g

Reference Value = 55.5 V/m

Power Drift = 0.009 dB

Maximum value of SAR = 3.02 mW/g

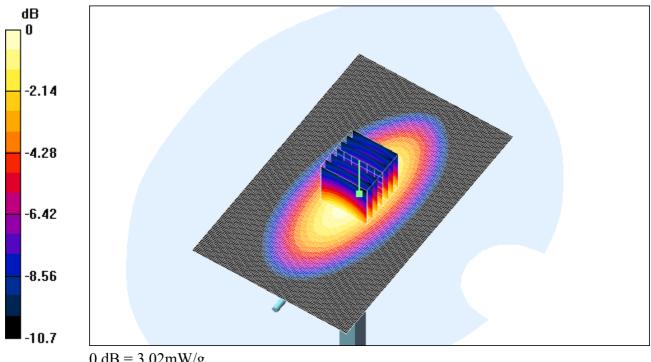

0 dB = 3.02 mW/g

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

1900 MHz System Validation Dipole

Type:	D1900V2
Serial Number:	50025
Place of Calibration:	Zurich:
Date of Calibration:	October 14, 2002
Calibration Interval:	24 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

Approved by:

Approved by:

Approved by:

Schmid & Partner **Engineering AG**

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

DASY

Dipole Validation Kit

Type: D1900V2

Serial: 5d025

Manufactured:

July 29, 2002

Calibrated: October 14, 2002

1. Measurement Conditions

The measurements were performed in the flat section of the new SAM twin phantom filled with head simulating glycol solution of the following electrical parameters at 1900 MHz:

Relative Dielectricity 38.7 $\pm 5\%$ Conductivity 1.45 mho/m $\pm 5\%$

The DASY4 System with a dosimetric E-field probe ET3DV6 (SN:1507, Conversion factor 5.2 at 1900 MHz) was used for the measurements.

The dipole was mounted on the small tripod so that the dipole feedpoint was positioned below the center marking of the flat phantom section and the dipole was oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 15mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was $250 \text{mW} \pm 3 \%$. The results are normalized to 1W input power.

2 SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 1. The results (see figure supplied) have been normalized to a dipole input power of 1W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1507 and applying the <u>advanced extrapolation</u> are:

averaged over 1 cm³ (1 g) of tissue: 40.4 mW/g

averaged over 10 cm³ (10 g) of tissue: 20.6 mW/g

3. Dipole Impedance and Return Loss

The impedance was measured at the SMA-connector with a network analyzer and numerically transformed to the dipole feedpoint. The transformation parameters from the SMA-connector to the dipole feedpoint are:

Electrical delay: 1.196 ns (one direction)

Transmission factor: 0.997 (voltage transmission, one direction)

The dipole was positioned at the flat phantom sections according to section 1 and the distance holder was in place during impedance measurements.

Feedpoint impedance at 1900 MHz: $Re\{Z\} = 51.6 \Omega$

 $Im \{Z\} = 4.7 \Omega$

Return Loss at 1900 MHz -26.3 dB

4. Handling

Do not apply excessive force to the dipole arms, because they might bend. Bending of the dipole arms stresses the soldered connections near the feedpoint leading to a damage of the dipole.

5. Design

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

6. Power Test

After long term use with 40W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

Date/Time: 10/14/02 17:57:28

Test Laboratory: SPEAG, Zurich, Switzerland

File Name: SN5d025 SN1507 HSL1900 141002.da4

DUT: Dipole 1900 MHz Type & Serial Number: D1900V2 - SN5d025 Program: Dipole Calibration; Pin = 250 mW; d = 10 mm

Communication System: CW-1900; Frequency: 1900 MHz; Duty Cycle: 1:1 Medium: HSL 1900 MHz ($\sigma = 1.45$ mho/m, $\epsilon = 38.7$, $\rho = 1000$ kg/m³)

Phantom section: FlatSection


DASY4 Configuration:


- Probe: ET3DV6 SN1507; ConvF(5.2, 5.2, 5.2); Calibrated: 1/24/2002
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 SN410; Calibrated: 7/18/2002
- Phantom: SAM 4.0 TP:1006
- Software: DASY4, V4.0 Build 35

Area Scan (81x81x1): Measurement grid: dx=15mm, dy=15mm Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm Reference Value = 93 V/m Peak SAR = 18.3 mW/g


SAR(1 g) = 10.1 mW/g; SAR(10 g) = 5.16 mW/g

Power Drift = -0.0005 dB



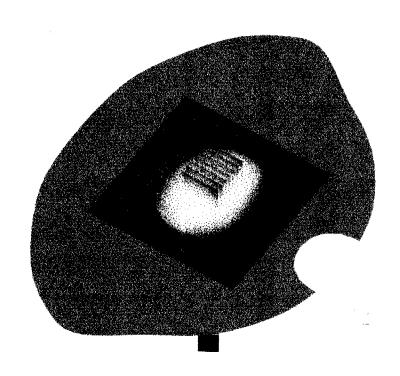

STOP 2 100.000 000 MHz

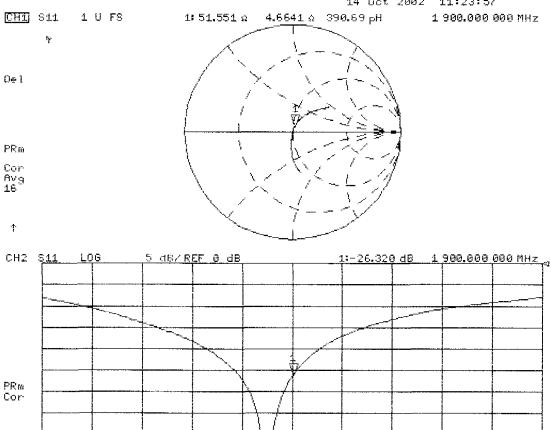

†

START 1 700.000 000 MHz



ELECTRONIC TECHNOLOGY SYSTEMS DR. GENZ GMBH - ETS - STORKOWER STRASSE 38c, D-15526 REICHENWALDE B. BERLIN

Tel: 033631 888 00 FAX: 033631 888 660

D2: 1900MHz SYSTEM VALIDATION DIPOLE

CALIBRATION CERTIFICATE

1900 MHz System Validation Dipole (Muscle)

Туре:	D1900V2
Serial Number:	5d025
Place of Calibration:	Reichenwalde
Date of Calibration:	July 24, 2003
Calibration Interval:	24 month

ETS Dr. Genz GmbH hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of ETS Dr. Genz GmbH.

Wherever applicable, the standards used in the calibration process are traceable to International standards.

Calibrated by: W. Treffke

Approved by: K. Damm



ELECTRONIC TECHNOLOGY SYSTEMS DR. GENZ GMBH - ETS - STORKOWER STRASSE 38c, D-15526 REICHENWALDE B. BERLIN

Tel: 033631 888 00 FAX: 033631 888 660

DASY

DIPOLE VALIDATION KIT

Type: D1900V2

Serial: 5d025

Manufactured : Juli 29, 2002 Calibrated : Juli 24, 2003



Measurement Conditions

The measurements were performed in the flat section of the new SAM twin phantom filled with body simulating solution of the following electrical parameters at 1900 MHz:

Relative permittivity 51.41 +/- 5 % Conductivity 1.565 mho/m +/- 10 %

The DASY System with a dosimetric E-field probe ET3DV6 (SN: 1711, conversion factor 5,0 at 1900 MHz body) was used for the measurements.

The dipole feed-point was positioned below the center marking and oriented parallel to the body axis (the long side of the phantom). The standard measuring distance was 10 mm from dipole center to the solution surface. The included distance holder was used during measurements for accurate distance positioning.

The coarse grid with a grid spacing of 10 mm was aligned with the dipole. The 7x7x7 fine cube was chosen for cube integration.

The dipole input power (forward power) was 250 mW +/- 3%. The results are normalized to 1 W input power.



SAR Measurement with DASY4 System

Standard SAR-measurements were performed according to the measurement conditions described in section 4. The results (see figure supplied) have been normalized to a dipole input power of 1 W (forward power). The resulting averaged SAR-values measured with the dosimetric probe ET3DV6 SN:1711 and applying the advanced extrapolation are:

Averaged over 1 cm3 (1 g) of tissue: 45.6 mW/g

Averaged over 10 cm3 (10 g) of tissue: 23.7 mW/g

Dipole impedance and return loss

The dipole was positioned at the flat phantom sections according to section 4 (Measurement conditions) (with body tissue inside the phantom) and the distance holder was in place during impedance measurements.

Feed-point impedance at 1900 MHz: Re $\{Z\}$ = 54.9 Ω

Im $\{Z\} = -3.8 \Omega$

Return Loss at 1900 MHz: - 24.2 dB

Date/Time: 07/24/03 09:06:17

Test Laboratory: ELECTRONIC TECHNOLOGY SYSTEMS DR. GENZ GMBH

File Name: Dipol Calibr.1900 (m) 250mW.da4

Dipol Calibr.1900 (m) 250mW

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d025

Program: Dipol Calibration 1900 Muscle

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: Muscle 1800 MHz ($\sigma = 1.56554 \text{ mho/m}, \epsilon_r = 51.4058, \rho = 1000 \text{ kg/m}^3$)

Phantom section: Flat Section

DASY4 Configuration:

- Probe: ET3DV6 SN1711; ConvF(5, 5, 5); Calibrated: 11/29/2002
- Sensor-Surface: 4mm (Mechanical And Optical Surface Detection)
- Electronics: DAE3 Sn522; Calibrated: 9/11/2002
- Phantom: SAM 12; Type: TP-1217; Serial: QD000P40CA
- Measurement SW: DASY4, V4.1 Build 47; Postprocessing SW: SEMCAD, V1.6 Build 115

(24dBm)/Area Scan (81x81x1): Measurement grid: dx=10mm, dy=10mm

Reference Value = 92.1 V/m

Power Drift = 0.001 dB

Maximum value of SAR = 12.9 mW/g

(24dBm)/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Peak SAR (extrapolated) = 20.4 W/kg

SAR(1 g) = 11.4 mW/g; SAR(10 g) = 5.93 mW/g

Reference Value = 92.1 V/m

Power Drift = 0.001 dB

Maximum value of SAR = 12.8 mW/g

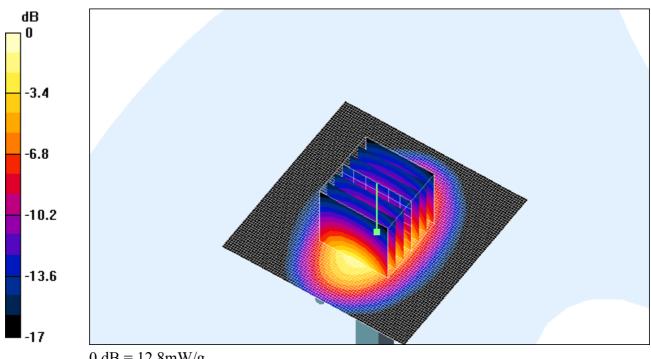

0 dB = 12.8 mW/g

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

Dosimetric E-Field Probe

Type:	1911310176
Serial Number:	1710
Place of Calibration:	Zurich
Date of Calibration:	September 3, 2002
Calibration Interval:	12 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

Approved by:

D.Vellen

Description

**Description

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Telephone +41 1 245 97 00, Fax +41 1 245 97 79

Probe ET3DV6

SN:1711

Manufactured:

August 7, 2002

Last calibration:

September 3, 2002

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

DASY - Parameters of Probe: ET3DV6 SN:1711

Sensitivity in	Free Space	Diode Compres	ssion	
Norm)	1.38 μV/(V/m) ²	DCP X	97	mV
Norm'	1.60 μV/(V/m) ²	DCP Y	97	mV
Norma	Z 1.53 μV/(V/m) ²	DCP Z	97	mV

Sensitivity in Tissue Simulating Liquid

Head Head	900 MHz 835 MHz		$\varepsilon_r = 41.5 \pm 5\%$ $\varepsilon_r = 41.5 \pm 5\%$	0.97 ± 5% r 0.90 ± 5% r	
	ConvF X	6.4	± 9.5% (k=2)	Boundary e	effect:
	ConvF Y	6.4	± 9.5% (k=2)	Alpha	0.47
	ConvF Z	6.4	± 9.5% (k=2)	Depth	2.17
Head Head	1800 MHz 1900 MHz		$\varepsilon_r = 40.0 \pm 5\%$ $\varepsilon_r = 40.0 \pm 5\%$	1.40 ± 5% r 1.40 ± 5% r	
	ConvF X	5.3	± 9.5% (k=2)	Boundary e	ffect:
	ConvF Y	5.3	± 9.5% (k=2)	Alpha	0.49
	ConvF Z	5.3	± 9.5% (k=2)	Depth	2.52


Boundary Effect


Head	900	MHz	Typical SAR gradient: 5	5 % per mm	
	Probe Tip to	Boundar	у	1 mm	2 mm
	SAR _{be} [%]	Without	Correction Algorithm	9.6	5.3
	SAR _{be} [%]	With Cor	rection Algorithm	0.2	0.4
Head	1800	MHz	Typical SAR gradient: 1	0 % per mm	
	Probe Tip to	Boundar	у	1 mm	2 mm
	SAR _{be} [%]	Without	Correction Algorithm	12.5	8.4
	SAR _{be} [%]	With Cor	rection Algorithm	0.2	0.2


Sensor Offset

Probe Tip to Sensor Center	2.7	mm
Optical Surface Detection	1.3 ± 0.2	mm


Receiving Pattern (ϕ), θ = 0°

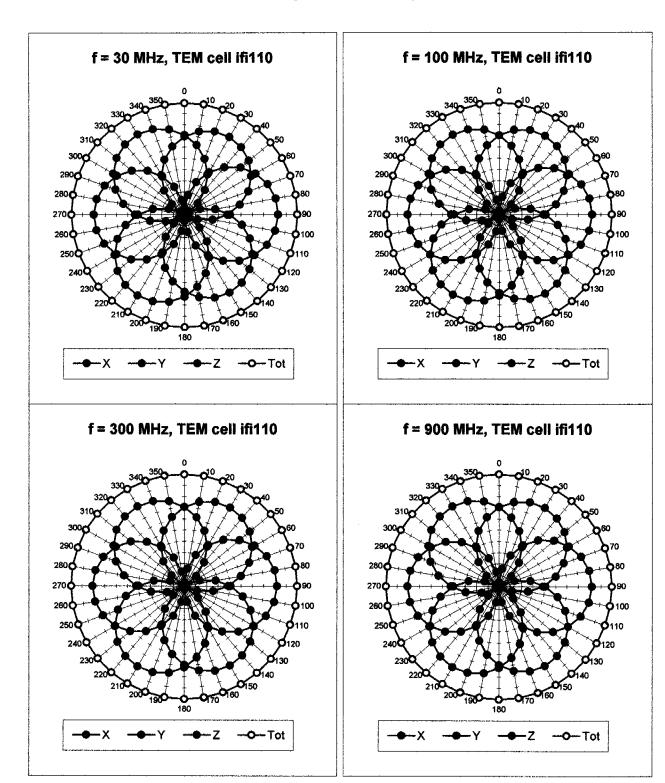

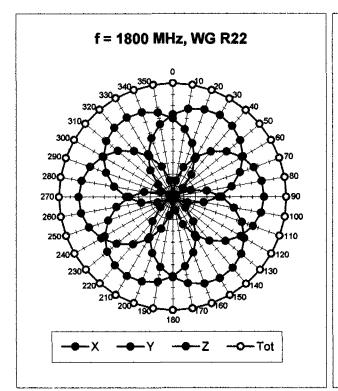

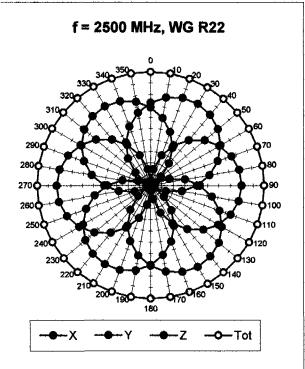


Isotropy Error (ϕ), θ = 0°

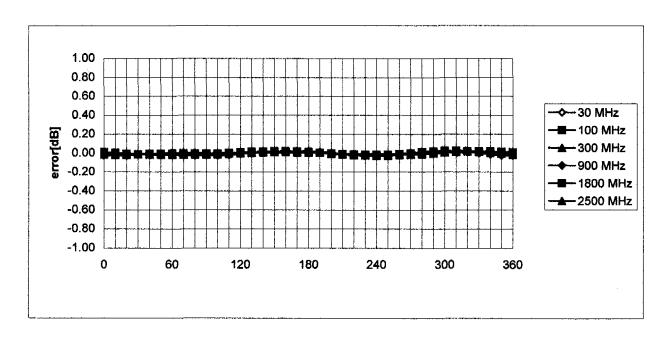


Frequency Response of E-Field


(TEM-Cell:ifi110, Waveguide R22)

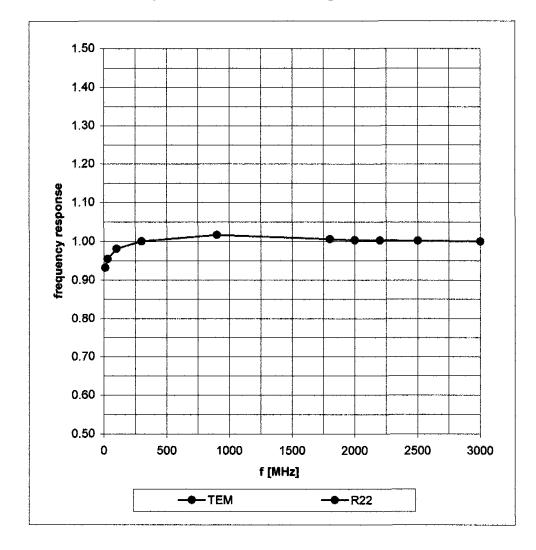


Dynamic Range f(SAR_{brain})


(Waveguide R22)

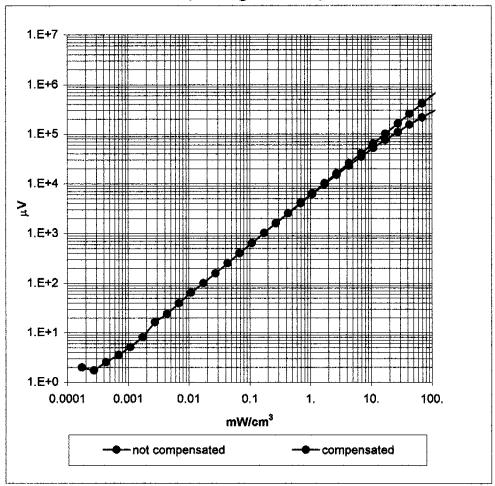

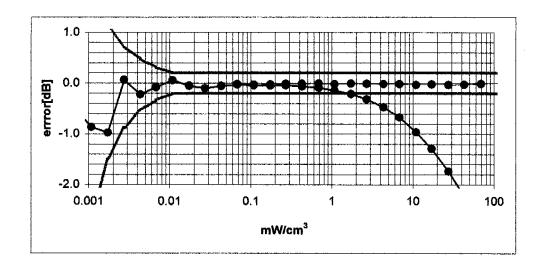

Conversion Factor Assessment

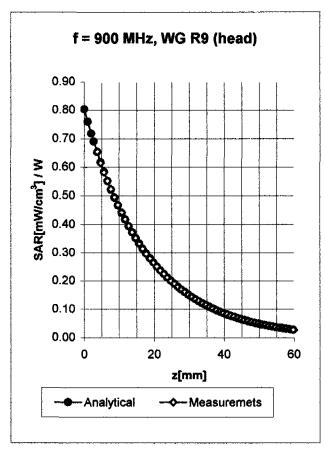

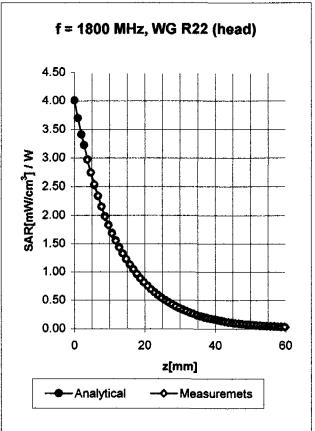


Head	900 MHz	$\varepsilon_{\rm r}$ = 41.5 ± 5%	σ = 0.97 ± 5% mho/m	
Head	835 MHz	$\varepsilon_{\rm r}$ = 41.5 ± 5%	σ = 0.90 ± 5% mho/m	
	ConvF X	6.4 ± 9.5% (k=2)	Boundary effect:	
	ConvF Y	6.4 ± 9.5% (k=2)	Alpha 0.47	
	ConvF Z	6.4 ± 9.5% (k=2)	Depth 2.17	

Head	1800 MHz	$\varepsilon_{\rm r}$ = 40.0 ± 5%	σ = 1.40 ± 5% mho/m	
Head	1900 MHz	$\varepsilon_{\rm r}$ = 40.0 ± 5%	$\sigma = 1.40 \pm 5\% \text{ mho/m}$	
	ConvF X	5.3 ± 9.5% (k=2)	Boundary effect:	
	ConvF Y	5.3 ± 9.5% (k=2)	Alpha 0.	.49
	ConvF Z	5.3 ± 9.5% (k=2)	Depth 2.	.52

Deviation from Isotropy in HSL

Error (θ,ϕ) , f = 900 MHz

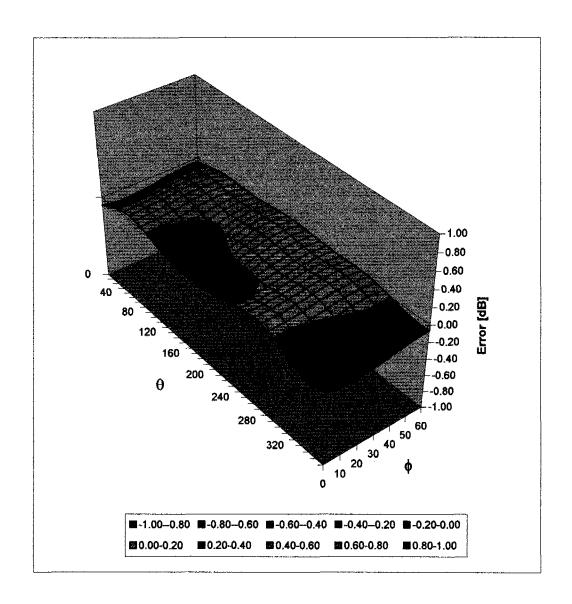

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Phone +41 1 245 97 00, Fax +41 1 245 97 79

Calibration Certificate

Dosimetric E-Field Probe

Type:	ET3DV6
Serial Number:	
Place of Calibration:	Zurich
Date of Calibration:	November 26, 2002
Calibration Interval:	12 months

Schmid & Partner Engineering AG hereby certifies, that this device has been calibrated on the date indicated above. The calibration was performed in accordance with specifications and procedures of Schmid & Partner Engineering AG.

Wherever applicable, the standards used in the calibration process are traceable to international standards. In all other cases the standards of the Laboratory for EMF and Microwave Electronics at the Swiss Federal Institute of Technology (ETH) in Zurich, Switzerland have been applied.

Calibrated by:

Approved by:

Total Control of Cont

Schmid & Partner Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland, Telephone +41 1 245 97 00, Fax +41 1 245 97 79

Probe ET3DV6

SN:1711

Additional Conversion Factors


Calibrated:


November 26, 2002

Calibrated for DASY Systems

(Note: non-compatible with DASY2 system!)

Conversion Factor Assessment

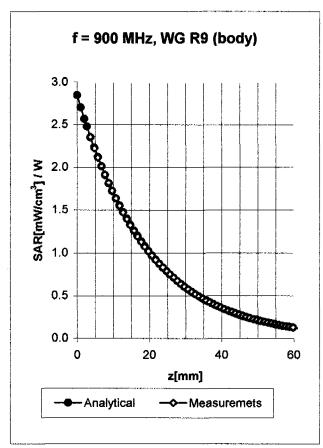


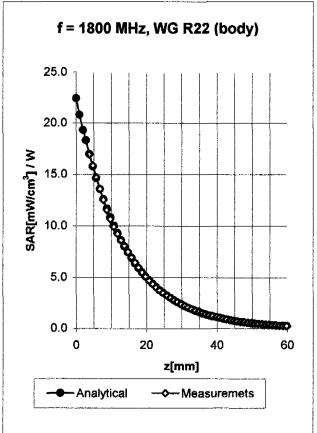


Body	900 MHz	ε _r = 55.0 ± 5%	$\sigma = 1.05 \pm 5\% \text{ mho/m}$
Body	835 MHz	$\varepsilon_{\rm r}$ = 55.2 ± 5%	σ = 0.97 ± 5% mho/m
	ConvF X	6.2 ± 9.5% (k=2)	Boundary effect:
	ConvF Y	6.2 ± 9.5% (k=2)	Alpha 0.41
	ConvF Z	6.2 ± 9.5% (k=2)	Depth 2.49

Body	1800 MHz	$\varepsilon_r = 53.3 \pm 5\%$	σ = 1.52 ± 5% mho/m
Body	1900 MHz	$\varepsilon_{\rm r}$ = 53.3 ± 5%	σ = 1.52 ± 5% mho/m
	ConvF X	5.0 ± 9.5% (k=2)	Boundary effect:
	ConvF Y	5.0 ± 9.5% (k=2)	Alpha 0.63
	ConvF Z	5.0 ± 9.5% (k=2)	Depth 2.26

Conversion Factor Assessment

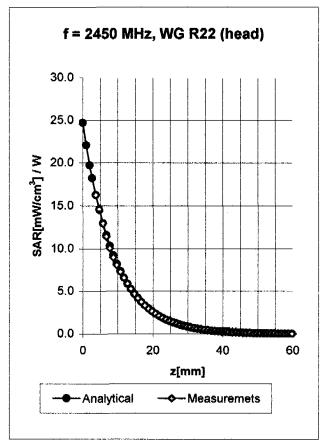

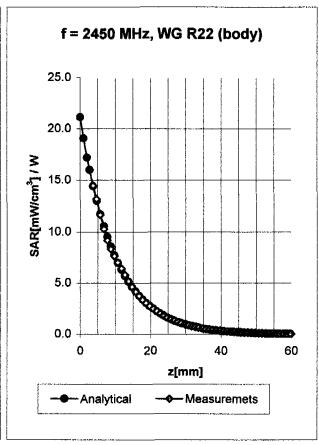

2450	Head	MHz	$\varepsilon_r = 39.2 \pm 5\%$	$\sigma = 1.80 \pm 5\% \text{ m}$	iho/m
	ConvF X	4.9	± 8.9% (k=2)	Boundary ef	fect:
	ConvF Y	4.9	± 8.9% (k=2)	Alpha	1.00
	ConvF Z	4.9	± 8.9% (k=2)	Depth	1.72
2450	Body	MHz	ε_r = 52.7 ± 5%	o = 1.95 ± 5% m	iho/m
	ConvF X	4.4	± 8.9% (k=2)	Boundary ef	fect:
	ConvF Y	4.4	± 8.9% (k=2)	Alpha	1.00
	ConvF Z	4.4	± 8.9% (k=2)	Depth	1.85

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

Additional Conversion Factors

for Dosimetric E-Field Probe

Type:	ET3DV6
Serial Number:	1711
Place of Assessment:	Zurich
Date of Assessment:	September 30, 2003
Probe Calibration Date:	September 3, 2002

Schmid & Partner Engineering AG hereby certifies that conversion factor(s) of this probe have been evaluated on the date indicated above. The assessment was performed using the FDTD numerical code SEMCAD of Schmid & Partner Engineering AG. Since the evaluation is coupled with measured conversion factors, it has to be recalculated yearly, i.e., following the re-calibration schedule of the probe. The uncertainty of the numerical assessment is based on the extrapolation from measured value at 900 MHz or at 1800 MHz.

Men = Katja

Assessed by:

Zeughausstrasse 43, 8004 Zurich, Switzerland Phone +41 1 245 9700, Fax +41 1 245 9779 info@speag.com, http://www.speag.com

Dosimetric E-Field Probe ET3DV6 SN:1771

Conversion factor (± standard deviation)

150 MHz (100-200 MHz)	ConvF	8.9 ± 8%	$\epsilon_r = 52.3 \pm 5\%$ $\sigma = 0.76 \pm 5\% \text{ mho/m}$ (head tissue)
150 MHz (100-200 MHz)	ConvF	$8.5 \pm 8\%$	$\epsilon_r = 61.9 \pm 5\%$ $\sigma = 0.80 \pm 5\% \text{ mho/m}$ (body tissue)
300 MHz (250-350 MHz)	ConvF	7.7 ± 8%	$\varepsilon_r = 45.3 \pm 5\%$ $\sigma = 0.87 \pm 5\% \text{ mho/m}$ (head tissue)
450 MHz (400-500 MHz)	ConvF	$7.3 \pm 8\%$	$\epsilon_r = 43.5 \pm 5\%$ $\sigma = 0.87 \pm 5\%$ mho/m (head tissue)
450 MHz (400-500 MHz)	ConvF	$7.5 \pm 8\%$	$\varepsilon_r = 56.7 \pm 5\%$ $\sigma = 0.94 \pm 5\% \text{ mho/m}$ (body tissue)

Schmid & Partner Engineering AG

DASY - DOSIMETRIC ASSESSMENT SYSTEM

CALIBRATION REPORT

DATA ACQUISITION ELECTRONICS

MODEL:

DAE3 V1

SERIAL NUMBER:

522

This Data Acquisition Unit was calibrated and tested using a FLUKE 702 Process Calibrator. Calibration and verification were performed at an ambient temperature of 23 ± 5 °C and a relative humidity of < 70%.

Measurements were performed using the standard DASY software for converting binary values, offset compensation and noise filtering. Software settings are indicated in the reports.

Results from this calibration relate only to the unit calibrated.

Calibrated by:

Storchenegger

Calibration Date:

11.09.2002

DASY Software Version:

DASY3 V3.1c

1. DC Voltage Measurement

DA - Converter Values from DAE

High Range: 1LSB =

6.1μV ,

full range =

400 mV

Low Range:

1LSB = 61nV, full range =

4 mV

Software Set-up: Calibration time: 3 sec

Measuring time: 3 sec

Setup	Х	Υ	Z
High Range	403.7567398	403.5333268	403.8600523
Low Range	3.90623	3.92439	3.92633
Connector Position			

High Range	Input	Reading in μV	% Error
Channel X + Input	200mV	200000.4	0.00
	20mV	19994.9	-0.03
Channel X - Input	20mV	-19994.4	-0.03
Channel Y + Input	200mV	199999.9	0.00
	20mV	19996.04	-0.02
Channel Y - Input	20mV	-19995.35	-0.02
Channel Z + Input	200mV	200000	0.00
	20mV	19993.57	-0.03
Channel Z - Input	20mV	-19994.59	-0.03

Low Range	Input	Reading in μV	% Error
Channel X + Input	2mV	2000.07	0.00
	0.2mV	200.266	0.13
Channel X - Input	0.2mV	-200.669	0.33
Channel Y + Input	2mV	2000.005	0.00
	0.2mV	199.4087	-0.30
Channel Y - Input	0.2mV	-200.5428	0.27
Channel Z + Input	2mV	2000.05	0.00
	0.2mV	199.285	-0.36
Channel Z - Input	0.2mV	-201.008	0.50

2. Common mode sensitivity

Software Set-up

Calibration time:

3 sec, Measuring time:

3 sec

High/Low Range

in μV	Common mode Input Voltage	High Range Reading	Low Range Reading
Channel X	200mV	1.89173	1.5706
	- 200mV	-0.957298	-1.63568
Channel Y	200mV	1.06159	0.55289
1 1111	- 200mV	-1.07262	-1.60898
Channel Z	200mV	-7.02304	-7.75271
	- 200mV	6.48984	6.11901

3. Channel separation

Software Set-up

Calibration time:

3 sec, Measuring time:

3 sec

High Range

in μV	Input Voltage	Channel X	Channel Y	Channel Z
Channel X	200mV	-	0.967802	-0.38491
Channel Y	200mV	0.985686	-	-0.851851
Channel Z	200mV	0.469187	-0.713242	-

4. AD-Converter Values with inputs shorted

in LSB	Low Range	High Range	
Channel X	14950.9	15343	
Channel Y	14931.4	15456.6	
Channel Z	15332.2	15470.3	

5. Input Offset Measurement

Measured after 15 min warm-up time of the Data Acquisition Electronic. Every Measurement is preceded by a calibration cycle.

Software set-up:

Calibration time:

3 sec

Measuring time:

3 sec

Number of measurements:

100, Low Range

Input $10M\Omega$

in μV	Average	min. Offset	max. Offset	Std. Deviation
Channel X	-1.11	-3.70	0.56	0.65
Channel Y	0.79	-0.47	2.26	0.38
Channel Z	-1.60	-3.56	-0.55	0.34

Input shorted

in μV	Average	min. Offset	max. Offset	Std. Deviation
Channel X	-1.36	-2.30	0.49	0.39
Channel Y	0.05	-0.63	1.82	0.33
Channel Z	-0.53	-1.37	0.58	0.21

6. Input Offset Current

in fA	Input Offset Current
Channel X	< 25
Channel Y	< 25
Channel Z	< 25

7. Input Resistance

	Calibrating	Measuring
Channel X	200 kΩ	200 ΜΩ
Channel Y	200 kΩ	200 MΩ
Channel Z	200 kΩ	200 MΩ

8. Low Battery Alarm Voltage

in V	Alarm Level
Supply (+ Vcc)	7.83 V
Supply (- Vcc)	-7.62 V

9. Power Consumption

in mA	Switched off	Stand by	Transmitting
Supply (+ Vcc)	0.000	5.79	13.9
Supply (- Vcc)	-0.011	-8.07	-9.24

10. Functional test

Touch async pulse 1	ok
Touch async pulse 2	ok
Touch status bit 1	ok
Touch status bit 2	ok
Remote power off	ok
Remote analog Power control	ok
Modification Status	B – C

Date: 11.09.02 Signature: 1. Manual Control of the Control of the