

Test Laboratory: Eurofins Product Service GmbH

## LTE-FDD4 Cat-M1 CH20050 QPSK BW 20 RB 3 ROffset 3 NBI 15 - Flat Right 0 mm

DUT: CardioMessenger Smart 4G; Type: Handset; Serial: 80216063

Communication System: UID 0, LTE FDD 4 Cat-M1 (0); Frequency: 1720 MHz; Duty Cycle: 1:3.33043  
Medium parameters used:  $f = 1720$  MHz;  $\sigma = 1.472$  S/m;  $\epsilon_r = 53.287$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:


- Probe: EX3DV4 - SN3893; ConvF(8.61, 8.61, 8.61) @ 1720 MHz; Calibrated: 20.09.2019
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn522; Calibrated: 11.09.2019
- Phantom: ELI v4.0; Type: QDOVA001BB;
- Measurement SW: DASY52, Version 52.10 (2);

### Configuration 2/CardioMessenger Smart 4G/Area Scan (7x17x1):

Measurement grid: dx=10mm, dy=10mm  
Maximum value of SAR (measured) = 1.13 W/kg

### Configuration 2/CardioMessenger Smart 4G/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 27.02 V/m; Power Drift = 0.06 dB  
Peak SAR (extrapolated) = 1.74 W/kg  
**SAR(1 g) = 1.03 W/kg; SAR(10 g) = 0.579 W/kg**  
Maximum value of SAR (measured) = 1.15 W/kg

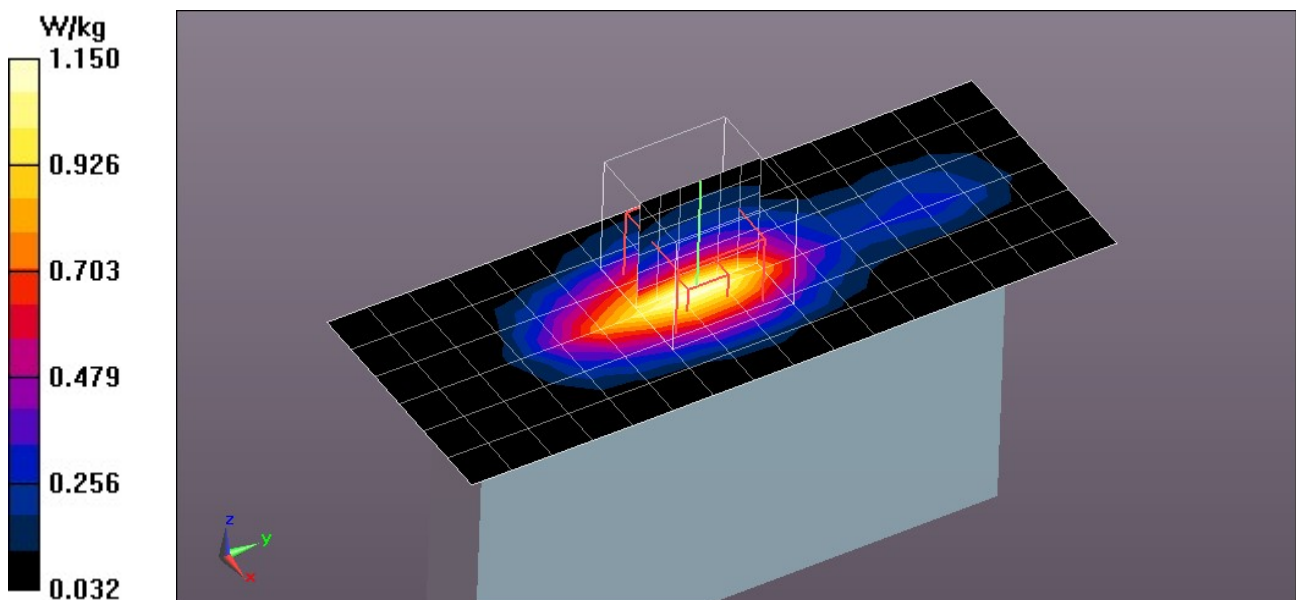

Test Laboratory: Eurofins Product Service GmbH

## LTE-FDD12 Cat-M1 CH23130 QPSK BW 10 RB 3 RBoffset 3 NBI 7 - Flat Right 0 mm

DUT: CardioMessenger Smart 4G; Type: Handset; Serial: 80216063

Communication System: UID 0, LTE FDD 12 Cat-M1 (0); Frequency: 711 MHz; Duty Cycle: 1:3.33043

Medium parameters used:  $f = 711$  MHz;  $\sigma = 0.925$  S/m;  $\epsilon_r = 54.955$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3893; ConvF(10.28, 10.28, 10.28) @ 711 MHz; Calibrated: 20.09.2019
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn522; Calibrated: 11.09.2019
- Phantom: ELI v4.0; Type: QDOVA001BB;
- Measurement SW: DASY52, Version 52.10 (2);

### Configuration 2/CardioMessenger Smart 4G/Area Scan (7x17x1):

Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 0.471 W/kg

### Configuration 2/CardioMessenger Smart 4G/Zoom Scan (7x8x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 18.75 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 0.649 W/kg

**SAR(1 g) = 0.432 W/kg; SAR(10 g) = 0.288 W/kg**

Maximum value of SAR (measured) = 0.468 W/kg

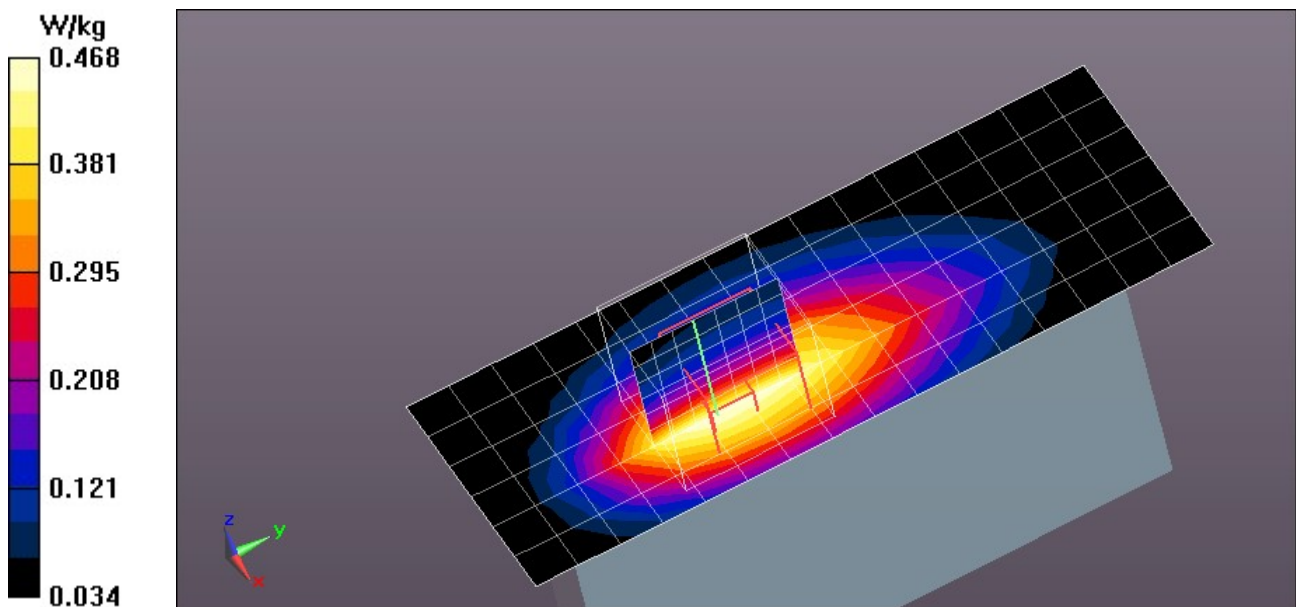

Test Laboratory: Eurofins Product Service GmbH

## LTE-FDD26 Cat-M1 CH26965 QPSK BW 15 RB 3 RBoffset 3 NBI 11 - Flat Right 0 mm

**DUT: CardioMessenger Smart 4G; Type: Handset; Serial: 80216063**

Communication System: UID 0, LTE FDD 26 Cat-M1 (0); Frequency: 841.5 MHz; Duty Cycle: 1:3.33043  
Medium parameters used (interpolated):  $f = 841.5$  MHz;  $\sigma = 0.979$  S/m;  $\epsilon_r = 53.62$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:


- Probe: EX3DV4 - SN3893; ConvF(9.92, 9.92, 9.92) @ 841.5 MHz; Calibrated: 20.09.2019
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn522; Calibrated: 11.09.2019
- Phantom: ELI v4.0; Type: QDOVA001BB;
- Measurement SW: DASY52, Version 52.10 (2);

### Configuration 2/CardioMessenger Smart 4G/Area Scan (7x17x1):

Measurement grid: dx=10mm, dy=10mm  
Maximum value of SAR (measured) = 0.407 W/kg

### Configuration 2/CardioMessenger Smart 4G/Zoom Scan (7x11x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 19.92 V/m; Power Drift = -0.02 dB  
Peak SAR (extrapolated) = 0.748 W/kg  
**SAR(1 g) = 0.390 W/kg; SAR(10 g) = 0.251 W/kg**  
Maximum value of SAR (measured) = 0.440 W/kg

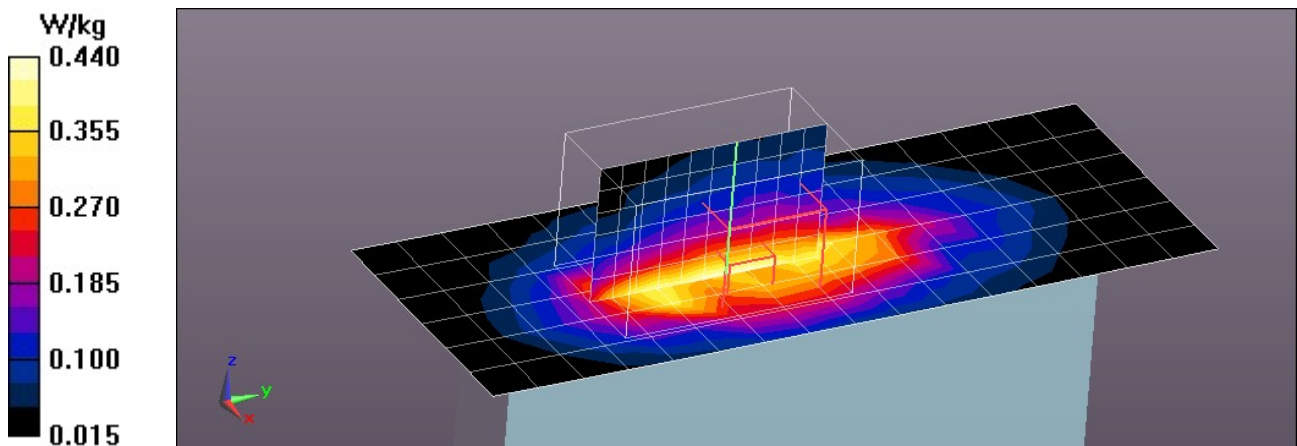

Test Laboratory: Eurofins Product Service GmbH

## LTE-FDD4 Cat-M1 CH20050 QPSK BW 20 RB 3 ROffset 3 NBI 15 - Flat Right 0 mm - 1st Repeated

DUT: CardioMessenger Smart 4G; Type: Handset; Serial: 80216063

Communication System: UID 0, LTE FDD 4 Cat-M1 (0); Frequency: 1720 MHz; Duty Cycle: 1:3.33043  
Medium parameters used:  $f = 1720$  MHz;  $\sigma = 1.505$  S/m;  $\epsilon_r = 52.931$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:


- Probe: EX3DV4 - SN3893; ConvF(8.61, 8.61, 8.61) @ 1720 MHz; Calibrated: 20.09.2019
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn522; Calibrated: 11.09.2019
- Phantom: ELI v4.0; Type: QDOVA001BB;
- Measurement SW: DASY52, Version 52.10 (2);

### Configuration 2/CardioMessenger Smart 4G/Area Scan (7x17x1):

Measurement grid:  $dx=10$ mm,  $dy=10$ mm  
Maximum value of SAR (measured) = 1.09 W/kg

### Configuration 2/CardioMessenger Smart 4G/Zoom Scan (7x7x7)/Cube 0:

Measurement grid:  $dx=5$ mm,  $dy=5$ mm,  $dz=5$ mm  
Reference Value = 26.36 V/m; Power Drift = -0.07 dB  
Peak SAR (extrapolated) = 1.71 W/kg  
**SAR(1 g) = 1.01 W/kg; SAR(10 g) = 0.569 W/kg**  
Maximum value of SAR (measured) = 1.12 W/kg

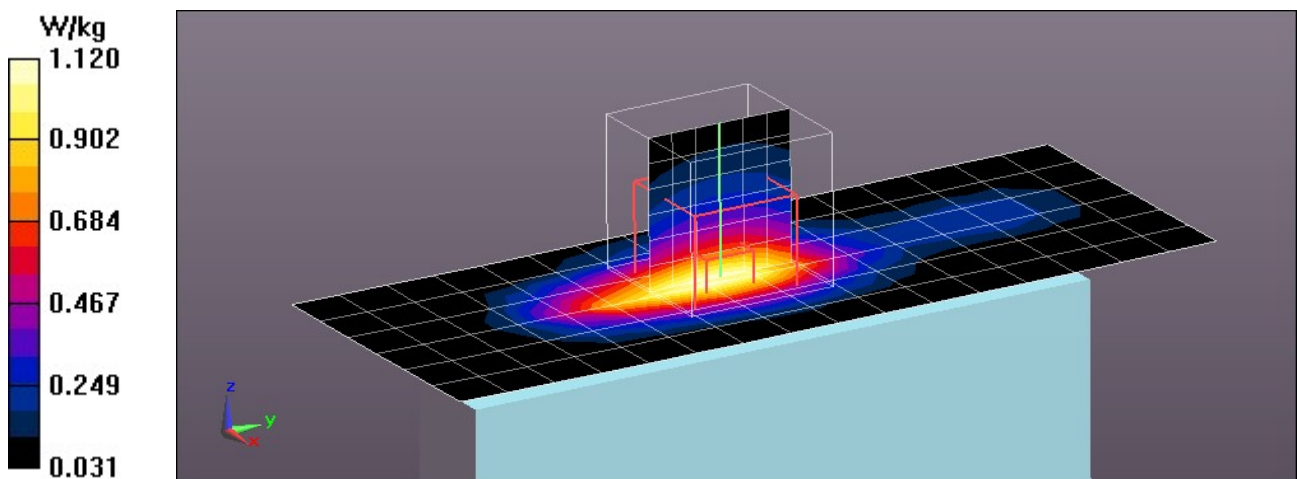

Test Laboratory: Eurofins Product Service GmbH

## LTE-FDD4 Cat-M1 CH20050 QPSK BW 20 RB 3 ROffset 3 NBI 15 - Flat Right 0 mm - DUT Holder Perturbations (without Holder)

DUT: CardioMessenger Smart 4G; Type: Handset; Serial: 80216063

Communication System: UID 0, LTE FDD 4 Cat-M1 (0); Frequency: 1720 MHz; Duty Cycle: 1:3.33043  
Medium parameters used:  $f = 1720$  MHz;  $\sigma = 1.505$  S/m;  $\epsilon_r = 52.931$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:


- Probe: EX3DV4 - SN3893; ConvF(8.61, 8.61, 8.61) @ 1720 MHz; Calibrated: 20.09.2019
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn522; Calibrated: 11.09.2019
- Phantom: ELI v4.0; Type: QDOVA001BB;
- Measurement SW: DASY52, Version 52.10 (2);

### Configuration 2/CardioMessenger Smart 4G/Area Scan (9x19x1):

Measurement grid: dx=10mm, dy=10mm  
Maximum value of SAR (measured) = 1.18 W/kg

### Configuration 2/CardioMessenger Smart 4G/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 20.80 V/m; Power Drift = 0.17 dB  
Peak SAR (extrapolated) = 1.80 W/kg  
**SAR(1 g) = 1.07 W/kg; SAR(10 g) = 0.601 W/kg**  
Maximum value of SAR (measured) = 1.19 W/kg

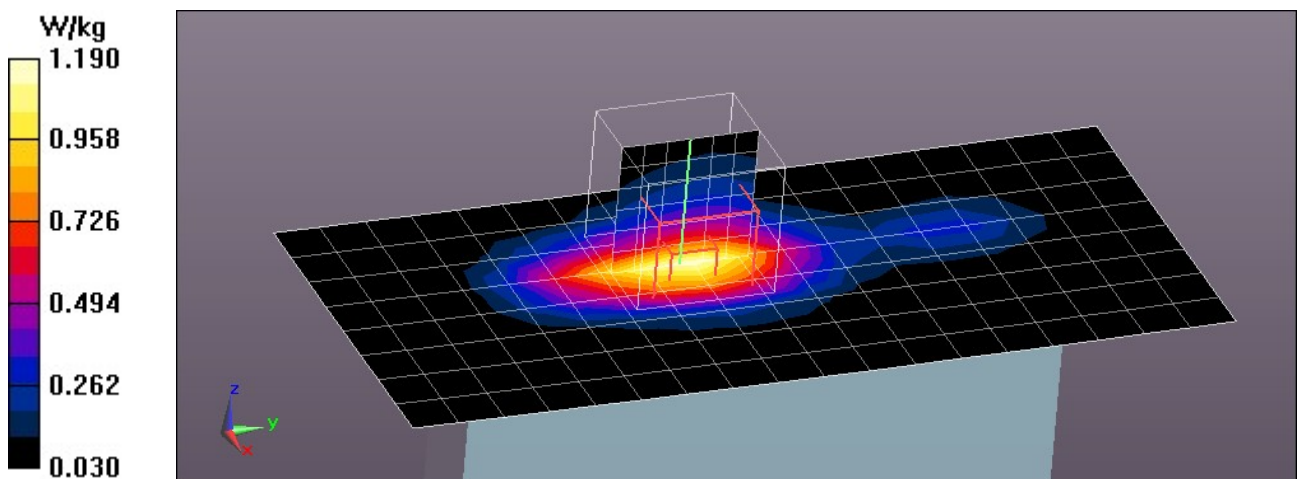

Test Laboratory: Eurofins Product Service GmbH

### Dipol Valid.1900 (m)\_250mW ELI4

**DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d025**

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium parameters used:  $f = 1900$  MHz;  $\sigma = 1.579$  S/m;  $\epsilon_r = 53.583$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

DASY5 Configuration:

- Probe: EX3DV4 - SN3893; ConvF(8.32, 8.32, 8.32) @ 1900 MHz; Calibrated: 20.09.2019
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn522; Calibrated: 11.09.2019
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP: 1013
- Measurement SW: DASY52, Version 52.10 (2); SEMCAD X Version 14.6.12 (7470)

### System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=4.0mm (EX-Probe)/Area Scan (11x10x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 11.9 W/kg


### System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=4.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 87.01 V/m; Power Drift = 0.08 dB

Peak SAR (extrapolated) = 19.3 W/kg

**SAR(1 g) = 10.8 W/kg; SAR(10 g) = 5.72 W/kg**

Maximum value of SAR (measured) = 12.2 W/kg

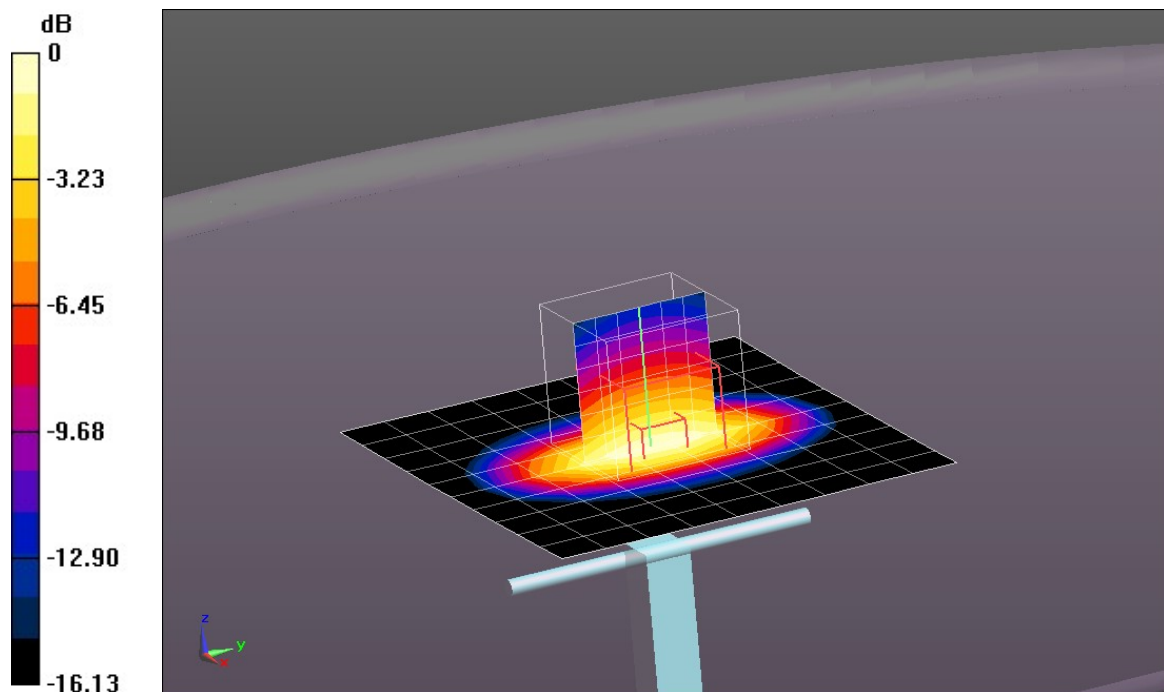

0 dB = 12.2 W/kg = 10.86 dBW/kg

Test Laboratory: Eurofins Product Service GmbH

## Dipol Valid.1750 (m) 250mW ELI4 - 2020-01-13

DUT: Dipole 1750 MHz D1750V2; Type: D1750V2; Serial: D1750V2 - SN:1126

Communication System: UID 0, CW (0); Frequency: 1750 MHz;Duty Cycle: 1:1  
Medium parameters used:  $f = 1750$  MHz;  $\sigma = 1.488$  S/m;  $\epsilon_r = 53.06$ ;  $\rho = 1000$  kg/m<sup>3</sup>  
Phantom section: Flat Section

DASY5 Configuration:


- Probe: EX3DV4 - SN3893; ConvF(8.61, 8.61, 8.61) @ 1750 MHz; Calibrated: 20.09.2019
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn522; Calibrated: 11.09.2019
- Phantom: ELI v4.0; Type: QDOVA001BB;
- Measurement SW: DASY52, Version 52.10 (2);

### System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=4.0mm (EX-Probe)/Area Scan (11x11x1):

Measurement grid: dx=10mm, dy=10mm  
Maximum value of SAR (measured) = 12.1 W/kg

### System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=4.0mm (EX-Probe)/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 89.99 V/m; Power Drift = -0.55 dB  
Peak SAR (extrapolated) = 17.1 W/kg  
**SAR(1 g) = 9.53 W/kg; SAR(10 g) = 5.11 W/kg**  
Maximum value of SAR (measured) = 10.8 W/kg

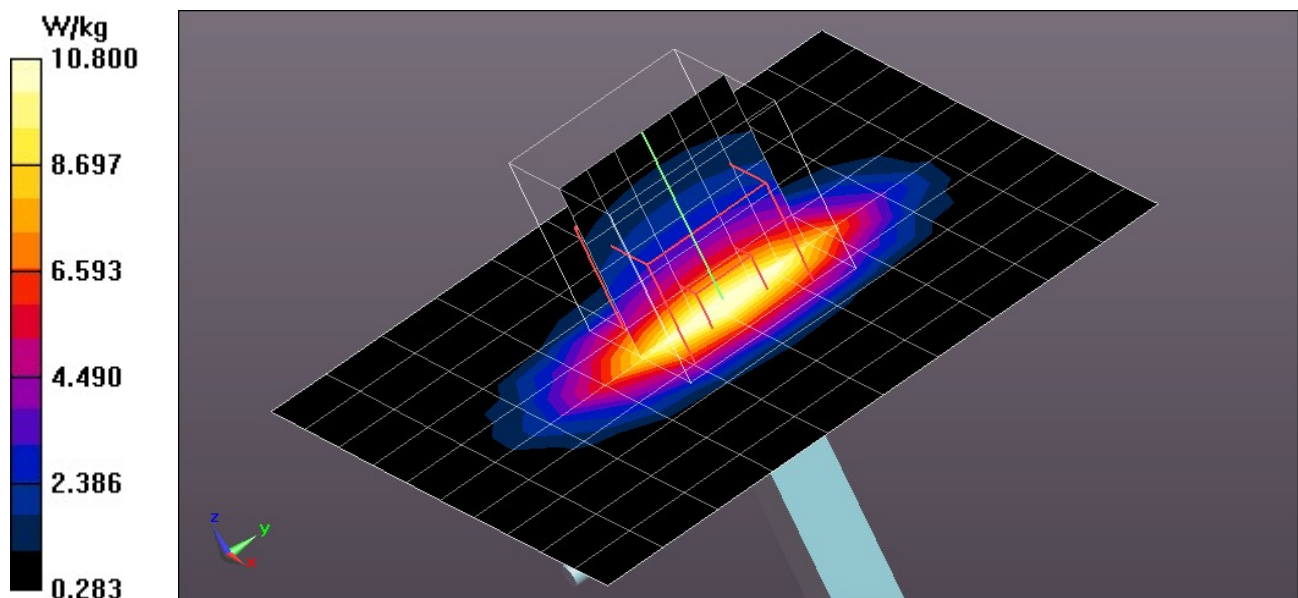

Test Laboratory: Eurofins Product Service GmbH

## Dipol Valid.900 (h)\_250mW ELI4\_2020-05-11

**DUT: Dipole 900 MHz D900V2; Type: D900V2; Serial: D900V2 - SN:164**

Communication System: UID 0, CW (0); Frequency: 900 MHz; Duty Cycle: 1:1  
Medium parameters used:  $f = 900 \text{ MHz}$ ;  $\sigma = 1.01 \text{ S/m}$ ;  $\epsilon_r = 53.262$ ;  $\rho = 1000 \text{ kg/m}^3$   
Phantom section: Flat Section

DASY5 Configuration:


- Probe: EX3DV4 - SN3893; ConvF(9.92, 9.92, 9.92) @ 900 MHz; Calibrated: 20.09.2019
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn522; Calibrated: 11.09.2019
- Phantom: ELI v4.0; Type: QDOVA001BB;
- Measurement SW: DASY52, Version 52.10 (2);

### System Performance Check at Frequencies below 1 GHz/d=15mm, Pin=250 mW, dist=4.0mm (EX-Probe)/Area Scan (9x17x1):

Measurement grid: dx=10mm, dy=10mm  
Maximum value of SAR (measured) = 2.77 W/kg

### System Performance Check at Frequencies below 1 GHz/d=15mm, Pin=250 mW, dist=4.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm  
Reference Value = 52.29 V/m; Power Drift = 0.04 dB  
Peak SAR (extrapolated) = 3.95 W/kg  
**SAR(1 g) = 2.62 W/kg; SAR(10 g) = 1.7 W/kg**  
Maximum value of SAR (measured) = 2.83 W/kg

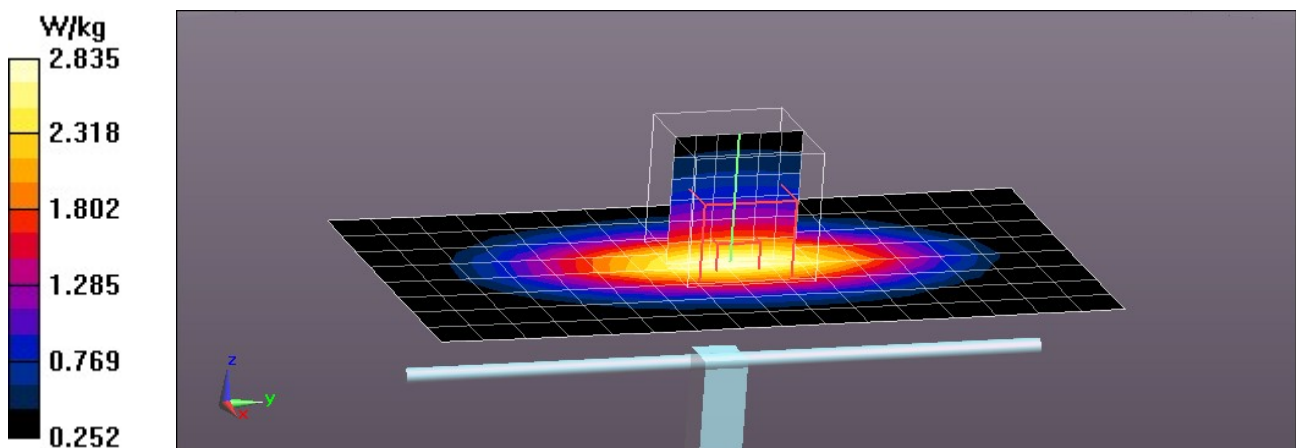



Test Laboratory: Eurofins Product Service GmbH

## Dipol Valid.750 (m)\_250mW ELI4 - 2020-05-04

**DUT: Dipole 750 MHz D750V3; Type: D750V3; Serial: D750V3 - SN:1125**

Communication System: UID 0, CW (0); Frequency: 750 MHz; Duty Cycle: 1:1  
 Medium parameters used:  $f = 750 \text{ MHz}$ ;  $\sigma = 0.961 \text{ S/m}$ ;  $\epsilon_r = 54.546$ ;  $\rho = 1000 \text{ kg/m}^3$   
 Phantom section: Flat Section

DASY5 Configuration:


- Probe: EX3DV4 - SN3893; ConvF(10.28, 10.28, 10.28) @ 750 MHz; Calibrated: 20.09.2019
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn522; Calibrated: 11.09.2019
- Phantom: ELI v4.0; Type: QDOVA001BB;
- Measurement SW: DASY52, Version 52.10 (2);

### System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=4.0mm (EX-Probe)/Area Scan (11x11x1):

Measurement grid:  $dx=10\text{mm}$ ,  $dy=10\text{mm}$   
 Maximum value of SAR (measured) = 2.35 W/kg

### System Performance Check at Frequencies above 1 GHz/d=10mm, Pin=250 mW, dist=4.0mm (EX-Probe)/Zoom Scan (7x7x7)/Cube 0:

Measurement grid:  $dx=5\text{mm}$ ,  $dy=5\text{mm}$ ,  $dz=5\text{mm}$   
 Reference Value = 49.50 V/m; Power Drift = 0.02 dB  
 Peak SAR (extrapolated) = 3.21 W/kg  
**SAR(1 g) = 2.19 W/kg; SAR(10 g) = 1.47 W/kg**  
 Maximum value of SAR (measured) = 2.36 W/kg

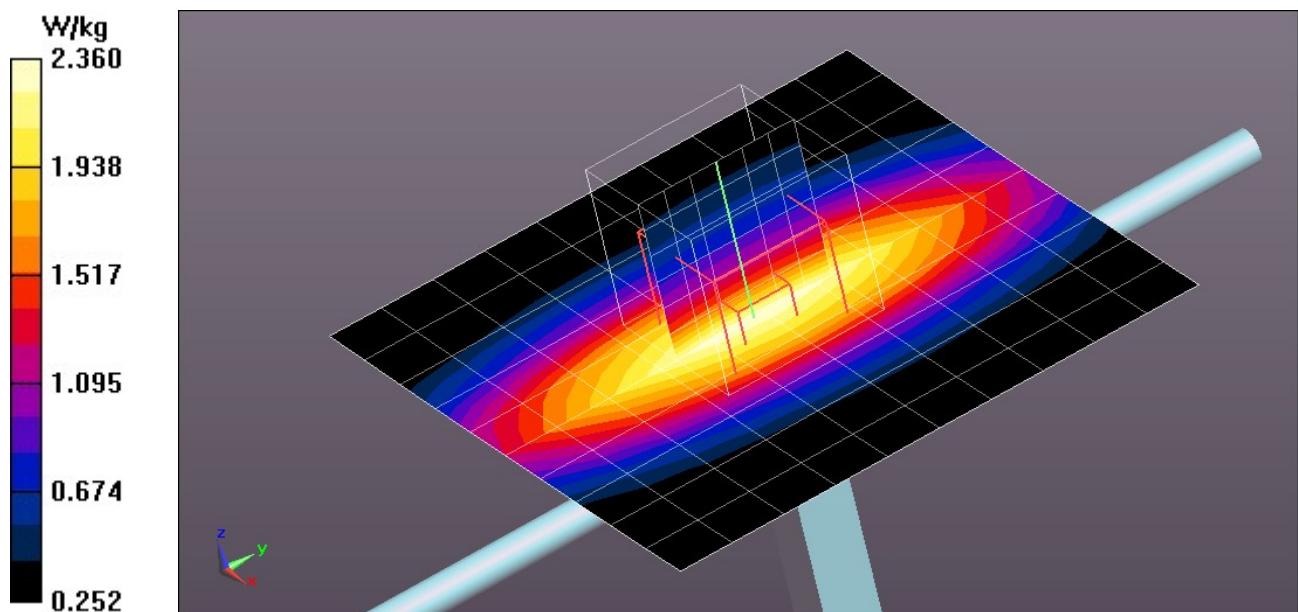

**ANNEX F Calibration Document**



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **Eurofins**

Certificate No: **D750V3-1125\_Sep17**

## CALIBRATION CERTIFICATE

Object **D750V3 - SN:1125**

Calibration procedure(s) **QA CAL-05.v9**  
**Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **September 21, 2017**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature ( $22 \pm 3$ )°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-17 (No. 217-02521/02522)	Apr-18
Power sensor NRP-Z91	SN: 103244	04-Apr-17 (No. 217-02521)	Apr-18
Power sensor NRP-Z91	SN: 103245	04-Apr-17 (No. 217-02522)	Apr-18
Reference 20 dB Attenuator	SN: 5058 (20k)	07-Apr-17 (No. 217-02528)	Apr-18
Type-N mismatch combination	SN: 5047.2 / 06327	07-Apr-17 (No. 217-02529)	Apr-18
Reference Probe EX3DV4	SN: 7349	31-May-17 (No. EX3-7349_May17)	May-18
DAE4	SN: 601	28-Mar-17 (No. DAE4-601_Mar17)	Mar-18

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-16)	In house check: Oct-17

Calibrated by: **Michael Weber**      Name: **Michael Weber**      Function: **Laboratory Technician**

Signature

Approved by: **Katja Pokovic**      Name: **Katja Pokovic**      Function: **Technical Manager**

Issued: September 21, 2017

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

**Glossary:**

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

**Additional Documentation:**

- e) DASY4/5 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of approximately 95%.

## Measurement Conditions

DASY system configuration, as far as not given on page 1.

<b>DASY Version</b>	DASY5	V52.10.0
<b>Extrapolation</b>	Advanced Extrapolation	
<b>Phantom</b>	Modular Flat Phantom	
<b>Distance Dipole Center - TSL</b>	15 mm	with Spacer
<b>Zoom Scan Resolution</b>	dx, dy, dz = 5 mm	
<b>Frequency</b>	750 MHz $\pm$ 1 MHz	

## Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Head TSL parameters</b>	22.0 °C	41.9	0.89 mho/m
<b>Measured Head TSL parameters</b>	(22.0 $\pm$ 0.2) °C	41.2 $\pm$ 6 %	0.90 mho/m $\pm$ 6 %
<b>Head TSL temperature change during test</b>	< 0.5 °C	----	----

## SAR result with Head TSL

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Head TSL</b>	Condition	
SAR measured	250 mW input power	2.08 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>8.22 W/kg <math>\pm</math> 17.0 % (k=2)</b>

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Head TSL</b>	condition	
SAR measured	250 mW input power	1.35 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	<b>5.35 W/kg <math>\pm</math> 16.5 % (k=2)</b>

## Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
<b>Nominal Body TSL parameters</b>	22.0 °C	55.5	0.96 mho/m
<b>Measured Body TSL parameters</b>	(22.0 $\pm$ 0.2) °C	55.5 $\pm$ 6 %	0.96 mho/m $\pm$ 6 %
<b>Body TSL temperature change during test</b>	< 0.5 °C	----	----

## SAR result with Body TSL

<b>SAR averaged over 1 cm<sup>3</sup> (1 g) of Body TSL</b>	Condition	
SAR measured	250 mW input power	2.13 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>8.52 W/kg <math>\pm</math> 17.0 % (k=2)</b>

<b>SAR averaged over 10 cm<sup>3</sup> (10 g) of Body TSL</b>	condition	
SAR measured	250 mW input power	1.41 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	<b>5.64 W/kg <math>\pm</math> 16.5 % (k=2)</b>

## Appendix (Additional assessments outside the scope of SCS 0108)

### Antenna Parameters with Head TSL

Impedance, transformed to feed point	55.6 $\Omega$ - 0.7 j $\Omega$
Return Loss	- 25.5 dB

### Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.0 $\Omega$ - 5.0 j $\Omega$
Return Loss	- 26.1 dB

### General Antenna Parameters and Design

Electrical Delay (one direction)	1.033 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

### Additional EUT Data

Manufactured by	SPEAG
Manufactured on	June 23, 2014

## DASY5 Validation Report for Head TSL

Date: 21.09.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1125**

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used:  $f = 750$  MHz;  $\sigma = 0.9$  S/m;  $\epsilon_r = 41.2$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.49, 10.49, 10.49); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.03.2017
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

**Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:**


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 58.66 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 3.22 W/kg

**SAR(1 g) = 2.08 W/kg; SAR(10 g) = 1.35 W/kg**

Maximum value of SAR (measured) = 2.82 W/kg

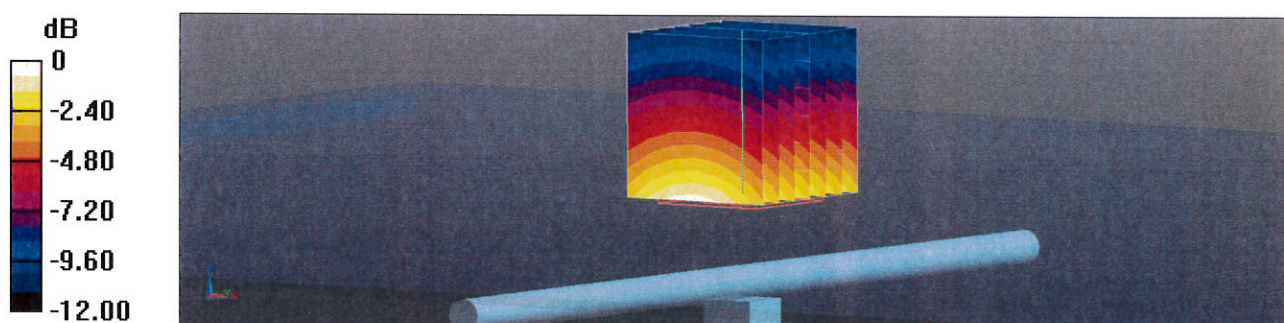


0 dB = 2.82 W/kg = 4.50 dBW/kg

# Impedance Measurement Plot for Head TSL

21 Sep 2017 12:00:11  
 [CH1] S11 1 U FS 1: 55.570  $\Omega$  -689.45 m $\Omega$  307.79 pF 750.000 000 MHz

\*  
 De1  
 CA

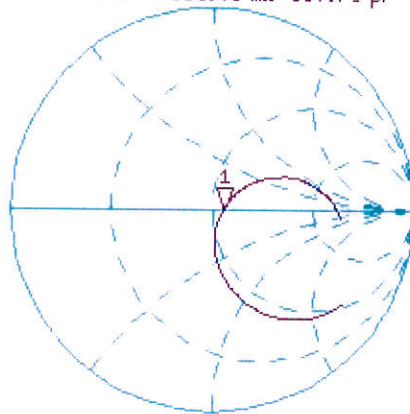

Avg  
 16


H1d

CH2 S11 LOG 5 dB/REF -20 dB 1:-25.481 dB 750.000 000 MHz

CA

Avg  
 16

H1d

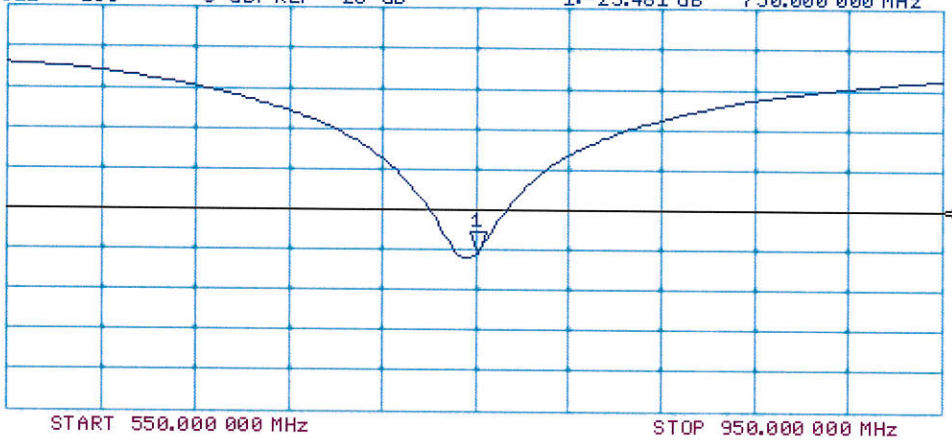



## DASY5 Validation Report for Body TSL

Date: 21.09.2017

Test Laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1125**

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used:  $f = 750$  MHz;  $\sigma = 0.96$  S/m;  $\epsilon_r = 55.5$ ;  $\rho = 1000$  kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.35, 10.35, 10.35); Calibrated: 31.05.2017;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.03.2017
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.0(1446); SEMCAD X 14.6.10(7417)

### Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.01 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 3.17 W/kg

**SAR(1 g) = 2.13 W/kg; SAR(10 g) = 1.41 W/kg**

Maximum value of SAR (measured) = 2.81 W/kg

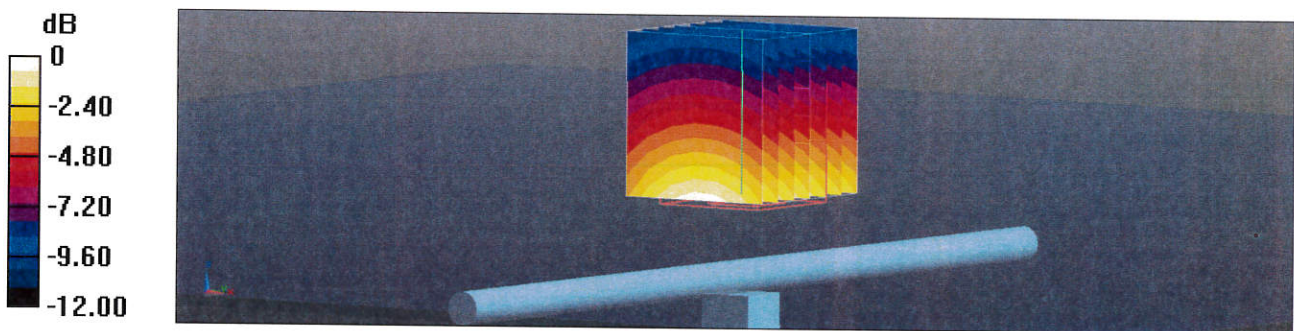

0 dB = 2.81 W/kg = 4.49 dBW/kg