

BIOTRONIK GmbH & Co. KG · Postfach 470255 · 12311 Berlin

Federal Communications
Commission
Equipment Authorization
Branch
7435 Oakland Mills Road
Columbia, MD 21046
USA

Tel +49 (0) 30 68905-1213
Fax +49 (0) 30 68905-1921
gunnar.boersch@biotronik.com
www.biotronik.com


Berlin, March 27, 2008

Re: Label Sample FCC ID: QRILUMAXT

Lumax 500 HF-T



IS-1
IS-1
IS-1
DF-1
DF-1



REF 360342
Cat. No.

SN 12345678
Serial No.

2009-03
Use Before

41-113 °F
Stor. Temp.






Implantable Cardioverter Defibrillator

(01)04035479103330(17)090320(21)12345678


Lumax 500 HF-T

PID 89
Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physician (or properly licenced practitioner)

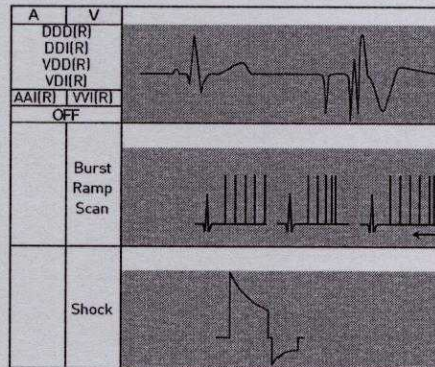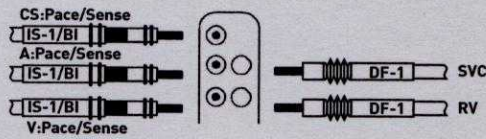

FCC ID: QRI LUMAXT



For single use only, do not resterilize. Refer to technical manual for instructions. ICD is shipped with all therapy disabled.

BIOTRONIK GmbH & Co. KG
Woermannkehre 1
12359 Berlin - Germany
Tel +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com



C/803 30009

Lumax 540 HF-T



IS-1
IS-1
IS-1
DF-1
DF-1



REF 360347
Cat. No.

SN 12345678
Serial No.

2009-03
Use Before

41-113 °F
Stor. Temp.





(01)04035479103385(17)090320(21)12345678

Implantable Cardioverter Defibrillator


Lumax 540 HF-T

PID 89
Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physician (or properly licenced practitioner)

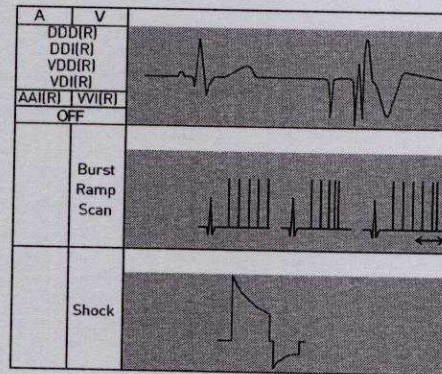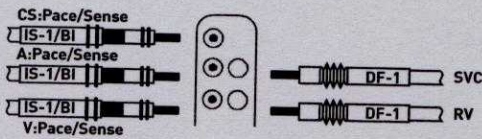

FCC ID: QRI LUMAXT



For single use only, do not resterilize. Refer to technical manual for instructions. ICD is shipped with all therapy disabled.

BIOTRONIK GmbH & Co. KG
Woermannkehe 1
12359 Berlin - Germany
Tel +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com



C 9803 30009

Lumax 500 VR-T



IS-1
DF-1
DF-1



REF 360345
Cat. No.

SN 12345678
Serial No.

2009-03
Use Before

41-113 °F
Stor. Temp.





(01)04035479103361(17)090320(21)12345678

Implantable Cardioverter Defibrillator


Lumax 500 VR-T

PID 89
Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physician (or properly licenced practitioner)

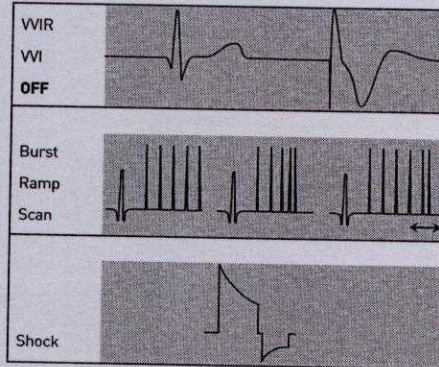

FCC ID: QRI LUMAXT



For single use only, do not resterilize. Refer to technical manual for instructions. ICD is shipped with all therapy disabled.

BIOTRONIK GmbH & Co. KG
Woermannkehre 1
12359 Berlin - Germany
Tel +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com



B/803 30009

Lumax 500 VR-T



IS-1
DF-1
DF-1



REF 360344
Cat. No.

SN 12345678
Serial No.

2009-03
Use Before

41-113 °F
Stor. Temp.





(01)04035479103354(17)090320(21)12345678

Implantable Cardioverter Defibrillator


Lumax 500 VR-T

PID 89
Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physician (or properly licenced practitioner)

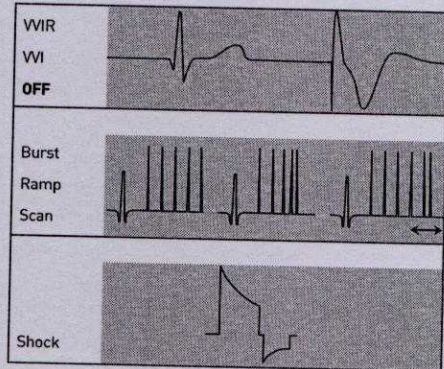

FCC ID: QRI LUMAXT



For single use only, do not resterilize. Refer to technical manual for instructions. ICD is shipped with all therapy disabled.

BIOTRONIK GmbH & Co. KG
Woermannkehrle 1
12359 Berlin · Germany
Tel +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com




C/03 30009

Lumax 500 DR-T



IS-1
IS-1
DF-1
DF-1



REF 360341
Cat. No.

SN 12345678
Serial No.

2009-03
Use Before

41-113 °F
Stor. Temp.






(01)04035479103323(17)090320(21)12345678

Implantable Cardioverter Defibrillator


Lumax 500 DR-T

PID 89
Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physician (or properly licenced practitioner)

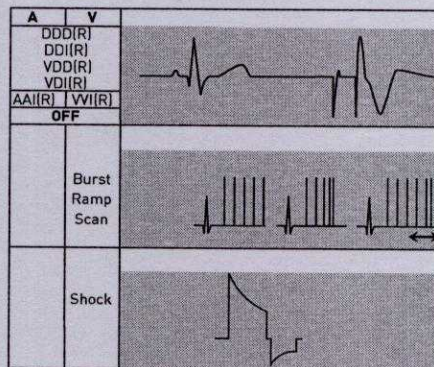

FCC ID: QRI LUMAXT



BIOTRONIK GmbH & Co. KG
Woermannkehre 1
12359 Berlin - Germany
Tel +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com


For single use only, do not resterilize. Refer to technical manual for instructions.
ICD is shipped with all therapy disabled.



C/803 3009

Lumax 500 DR-T

IS-1
IS-1
DF-1
DF-1



Implantable Cardioverter Defibrillator

REF 360340
Cat. No.

SN 12345678
Serial No.

8 2009-03
Use Before

41-113 °F
Stor. Temp.





(01)04035479103316(17)090320(21)12345678



Lumax 500 DR-T

PID 89
Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physician (or properly licenced practitioner)



FCC ID: QRI LUMAXT

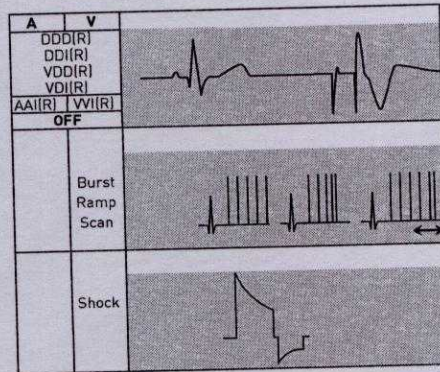

For single use only, do not resterilize. Refer to technical manual for instructions. ICD is shipped with all therapy disabled.


BIOTRONIK GmbH & Co. KG
Woermannkehe 1
12359 Berlin - Germany
Tel +49 (0) 30 68905-0
Fax +49 (0) 30 6852804
sales@biotronik.com

C/8/03 30009

Lumax 540 DR-T



IS-1
IS-1
DF-1
DF-1



REF 360346

Cat. No.

SN 12345678

Serial No.

Use Before 2009-03

Use Before

Stor. Temp. 41-113 °F

Stor. Temp.



(01)04035479103378(17)090320(21)12345678




Implantable Cardioverter Defibrillator

Lumax 540 DR-T


PID 89

Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physician (or properly licenced practitioner)

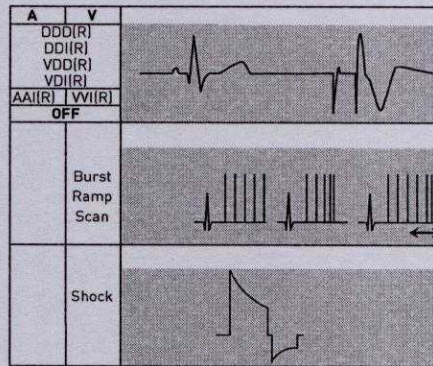

FCC ID: QRI LUMAXT



For single use only, do not resterilize. Refer to technical manual for instructions. ICD is shipped with all therapy disabled.

BIOTRONIK GmbH & Co. KG
 Woermannkehe 1
 12359 Berlin - Germany
 Tel +49 (0) 30 68905-0
 Fax +49 (0) 30 6852804
 sales@biotronik.com



C/003 30009

Lumax 540 VR-T



IS-1
DF-1
DF-1



REF 360348
Cat. No.

SN 12345678
Serial No.

2009-03
Use Before

41-113 °F
Stor. Temp.






(01)04035479103392(17)090320(21)12345678

Implantable Cardioverter Defibrillator

Lumax 540 VR-T


PID 89
Prod. ID

Caution: Federal law (U.S.A.) restricts this device to sale by, or on the order of, a physician (or properly licenced practitioner)

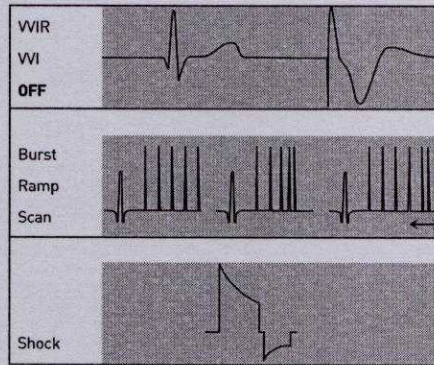

C/603 30009

FCC ID: QRI LUMAXT



For single use only, do not reesterilize. Refer to technical manual for instructions. ICD is shipped with all therapy disabled.

BIOTRONIK GmbH & Co. KG
Woermannkehe 1
12359 Berlin · Germany
Tel: +49 (0) 30 68905-0
Fax: +49 (0) 30 6852804
sales@biotronik.com

