

FCC TEST REPORT FCC 47 CFR Part 95I Medical Device Radio communication Service (MedRadio) Industry Canada RSS-243 Medical Devices Operating in the 401 – 406 MHz Frequency Band	
Report Reference No.	G0M-1507-4972-TFC95IMR2-V01
Testing Laboratory	Eurofins Product Service GmbH
Address	Storkower Str. 38c 15526 Reichenwalde Germany
Accreditation	<div style="display: flex; align-items: center; justify-content: center;">   </div> <p>A2LA Accredited Testing Laboratory, Certificate No.: 1983.01 FCC Filed Test Laboratory, Reg.-No.: 96970 IC OATS Filing assigned code: 3470A</p>
Applicant's name	Biotronik SE & Co. KG
Address	Woermannkehre 1 12359 Berlin GERMANY
Test specification:	
Standard.....	47 CFR Part 95E 47 CFR Part 95I 47 CFR Part 15C RSS-243, Issue 3, 2010-02 RSS-Gen, Issue 4, 2014-11 ANSI C63.4:2014 EN 301 839-1 V1.3.1:2009-10
Test scope.....	complete Radio compliance test
Equipment under test (EUT):	
Product description	Primus Nano Plus Pacemaker Family
Model No.	Edora 8 HF-T ProMRI
Additional Model(s)	see page4: List of Models to be included in the family
Brand Name(s)	Biotronik
Hardware version	ASM-0474_0A (See model matrix on page 4 to 6)
Firmware / Software version	7801RomRev_02.02 / 7801RamRev_02.03
	FCC-ID: QRIPNP IC: 4708A-PNP
Test result	Passed

Possible test case verdicts:

- neither assessed nor tested : N/N
- required by standard but not appl. to test object : N/A
- required by standard but not tested : N/T
- not required by standard for the test object : N/R
- test object does meet the requirement : P (Pass)
- test object does not meet the requirement : F (Fail)

Testing:


Test Lab Temperature : 22 – 26 °C


Test Lab Humidity : 30 – 50 %

Date of receipt of test item : 2015-09-28

Date (s) of performance of tests : 2015-09-28 – 2015-09-29

Compiled by : Christian Weber

Tested by (+ signature) : Wilfried Treffke 
 (Responsible for Test)

Approved by (+ signature) : Toralf Jahn 
 (Deputy Head of Lab)

Date of issue : 2016-03-11

Total number of pages : 31

General remarks:

The test results presented in this report relate only to the object tested.

The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report.

This report shall not be reproduced, except in full, without the written approval of the Issuing testing laboratory.

Additional comments:

Family Explanation

All devices feature the two RF-Telemetry functions Home Monitoring and wireless Wand. RF-Telemetry functions are using the MICS-Band (402MHz – 405MHz).

A „-T“ inside the name of the device represents a device containing RF-Telemetry.

HF-T are triple-chamber devices. (Master for all tests)

HF-T QP are triple chamber quadro polar

DR-T are dual-chamber devices.

SR-T are single-chamber devices with additional atrial detection.

DR are dual-chamber without home monitoring software.

SR are single-chamber without home monitoring software.

D are dual-chamber with no radio, only coil communication.

S are single-chamber with no radio, only coil communication.

All of these differences are only relevant in terms of medical aspects. They do not interfere with the RF-performance.

Evaluation measurements were performed for worst case antenna selection and the Edora 8 HF-T ProMRI was selected. The model Edora 8 HF-T ProMRI, as the most complex model, was selected for the measurements.

Family Certification
List of Models to be included in the family

(1) Applicant:	<u>BIOTRONIK SE & CO. KG</u>
(2) Certification Number:	_____

No.	Model Number	Description of Differences
1	Edora 8 HF-T ProMRI (Master)	(Master configuration) , 3 chamber, 3x IS-1 Connector, BOM-0296, SCH-0185, ASM-0474 Software Features (Brand 1) With Home Monitoring and MRI Software
2	Edora 8 HF-T QP ProMRI	3 chamber, 2x IS-1, 1x IS-4 Connector, BOM-0296, SCH-0185, ASM-0474 Software Features (Brand 1) With Home Monitoring and MRI Software
3	Evity 8 HF-T ProMRI	3 chamber, 3x IS-1 Connector, BOM-0296, SCH-0185, ASM-0474 Software Features (Brand 2) With Home Monitoring and MRI Software
4	Evity 8 HF-T QP ProMRI	3 chamber, 2x IS-1, 1x IS-4 Connector, BOM-0296, SCH-0185, ASM-0474 Software Features (Brand 2) With Home Monitoring and MRI Software
5	Enitra 8 HF-T ProMRI	3 chamber, 3x IS-1 Connector, BOM-0296, SCH-0185, ASM-0474 Software Features (Brand 3) With Home Monitoring and MRI Software
6	Enitra 8 HF-T QP ProMRI	3 chamber, 2x IS-1, 1x IS-4 Connector, BOM-0296, SCH-0185, ASM-0474 Software Features (Brand 3) With Home Monitoring and MRI Software
7	Enticos 8 HF-T	3 chamber, 3x IS-1 Connector, BOM-0296, SCH-0185, ASM-0474 Software Features (Brand 4) With Home Monitoring
8	Enticos 8 HF-T QP	3 chamber, 2x IS-1, 1x IS-4 Connector, BOM-0296, SCH-0185, ASM-0474 Premium-Tier Software Features (Brand 4) With Home Monitoring
9	Edora 8 DR-T ProMRI	2 chamber, 2x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 1) With Home Monitoring and MRI Software
10	Edora 8 SR-T ProMRI	1 chamber, 1x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 1) With Home Monitoring and MRI Software
11	Edora 8 DR ProMRI	2 chamber, 2x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 1) Without Home Monitoring, With MRI Software

 Test Report No.: G0M-1507-4972-TFC95IMR2-V01

12	Edora 8 SR ProMRI	1 chamber, 1x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 1) Without Home Monitoring, With MRI Software
13	Evity 8 DR-T ProMRI	2 chamber, 2x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 2) With Home Monitoring and MRI Software
14	Evity 8 SR-T ProMRI	1 chamber, 1x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 2) With Home Monitoring and MRI Software
15	Enitra 8 DR-T ProMRI	2 chamber, 2x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Premium-Tier Software Features (Brand 3) With Home Monitoring and MRI Software
16	Enitra 8 SR-T ProMRI	1 chamber, 1x IS-1 Connector, , BOM-0294, BOM-0295_0B, SCH-0186, ASM-0476 Software Features (Brand 3) With Home Monitoring and MRI Software
17	Enticos 8 DR-T	2 chamber, 2x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 4) With Home Monitoring
18	Enticos 8 SR-T	1 chamber, 1x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 4) With Home Monitoring
19	Evity 6 DR-T ProMRI	2 chamber, 2x IS-1 Connector, BOM-0294_0A, BOM-0295_0B, SCH-0186_0B, ASM-0476_0B Mid-Tier Software Features (Brand 2) With Home Monitoring and MRI Software
20	Evity 6 SR-T ProMRI	1 chamber, 1x IS-1 Connector BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 2) With Home Monitoring and MRI Software
21	Enitra 6 DR-T ProMRI	2 chamber, 2x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 3) With Home Monitoring and MRI Software
22	Enitra 6 SR-T ProMRI	1 chamber, 1x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 3) With Home Monitoring and MRI Software
23	Enitra 6 DR ProMRI	2 chamber, 2x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 3) Without Home Monitoring, With MRI Software
24	Enitra 6 SR ProMRI	1 chamber, 1x IS-1 Connector, BOM-0294, BOM-0295, SCH-0186, ASM-0476 Software Features (Brand 3) Without Home Monitoring, With MRI Software

25	Enticos 4 DR	2 chamber, 2x IS-1 Connector, BOM-0297, BOM-0298, SCH-0186, ASM-0476 Software Features (Brand 4) No Radio Circuit or Antenna, Coil Only
26	Enticos 4 SR	1 chamber, 1x IS-1 Connector, BOM-0297, BOM-0298, SCH-0186, ASM-0476 Software Features (Brand 4) No Radio Circuit or Antenna, Coil Only
27	Enticos 4 D	2 chamber, 2x IS-1 Connector, BOM-0297, BOM-0298, SCH-0186, ASM-0476 Software Features (Brand 4) No Radio Circuit or Antenna, Coil Only
28	Enticos 4 S	1 chamber, 1x IS-1 Connector, BOM-0297, BOM-0298, SCH-0186, ASM-0476 Software Features (Brand 4) No Radio Circuit or Antenna, Coil Only

Version History

Version	Issue Date	Remarks	Revised by
01	2016-03-11	Initial Release	

REPORT INDEX

1	EQUIPMENT (TEST ITEM) DESCRIPTION	9
1.1	Photos - Equipment external	11
1.2	Photos - Equipment internal	16
1.3	Photos – Test setup	19
1.4	Photos – Auxiliary/Associated Equipment	20
1.5	Supporting Equipment Used During Testing	21
1.6	Test Modes	22
1.7	Test Equipment Used During Testing	23
1.8	Sample emission level calculation	24
1.9	Simulated human body	25
2	RESULT SUMMARY	26
3	TEST CONDITIONS AND RESULTS	27
3.1	Test Conditions and Results – Occupied Bandwidth	27
3.2	Test Conditions and Results – Emission Bandwidth	31
3.3	Test Conditions and Results – Frequency stability	35
3.4	Test Conditions and Results – Transmitter output power	37
3.5	Test Conditions and Results – Band-edge and In-band Emissions	39
3.6	Test Conditions and Results – Transmitter unwanted emissions	41
3.7	Test Conditions and Results – Receiver spurious emissions	43

1 Equipment (Test item) Description

Description	Primus Nano Plus Pacemaker Family	
Model	Edora 8 HF-T ProMRI	
Additional Model(s)	see page4: List of Models to be included in the family	
Brand Name(s)	Biotronik	
Serial number	66454950 (for master) additional see model matrix on page 4 to 6	
Hardware version	ASM-0474_0A (for master) additional see model matrix on page 4 to 6	
Software / Firmware version	7801RomRev_02.02 / 7801RamRev_02.03	
FCC-ID	QRIPNP	
IC	4708A-PNP	
Equipment type	End product	
Radio type	Transceiver	
Number of Radios	1	
Radio technology	MedRadio (MICS) active medical implant	
Operating frequency range	402 - 405 MHz	
Assigned frequency band	402 - 405 MHz	
Main test frequencies	F _{LOW}	402.45 MHz
	F _{MID}	403.65 MHz
	F _{HIGH}	404.85 MHz
Modulations	FSK	
Emission designator	F1D	
Number of channels	9	
Channel spacing	300 kHz	
Spectrum access	LBT/AFA (channel access controlled by ULP-AMI-P device outside the human body)	
Number of antennas	1	
Antenna	Type	integrated
	Model	PNP Mini Rings
	Manufacturer	Biotronik SE & Co. KG
	Gain	-31.8 dBi (Determined by measurements)
Manufacturer	Biotronik SE & Co. KG Woermannkehre 1 12359 Berlin GERMANY	

Power supply	V _{NOM}	3.0 VDC
	V _{MIN}	2.0 VDC
	V _{MAX}	3.5 VDC
Temperature	T _{NOM}	37 °C
	T _{MIN}	25 °C
	T _{MAX}	45 °C
AC/DC-Adaptor	Model	N/A
	Vendor	N/A
	Input	N/A
	Output	N/A

1.5 Supporting Equipment Used During Testing

Product Type*	Device	Manufacturer	Model No.	Comments
AE	Programer	Biotronik	USB TelBox	64kHz system
AE	Programer	Biotronik	405 TELBOX II	400MHz system
<p>*Note: Use the following abbreviations:</p> <p>AE : Auxiliary/Associated Equipment, or</p> <p>SIM : Simulator (Not Subjected to Test)</p> <p>CABL : Connecting cables</p>				

1.6 Test Modes

Mode #	Description	
Unmodulated	General conditions:	EUT powered by fully charged battery
	Radio conditions:	Mode = standalone transmit Spreading = None Modulation = None Duty cycle = 100 % Power level = Maximum
Modulated	General conditions:	EUT powered by fully charged battery
	Radio conditions:	Mode = standalone transmit Modulation = FSK Duty cycle = 100 % Power level = Maximum
Receive	General conditions:	EUT powered by fully charged battery
	Radio conditions:	Mode = standalone receive Modulation = FSK

1.7 Test Equipment Used During Testing

Measurement Software			
Description	Manufacturer	Name	Version
EMC Test Software	Dare Instruments	Radimation	2015.2.4

Occupied Bandwidth					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSIQ26	EF00242	2015-04	2016-04

Emission Bandwidth					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSIQ26	EF00242	2015-04	2016-04

Frequency Stability					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSIQ26	EF00242	2015-04	2016-04

Effective radiated power					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic chamber	Frankonia	AC 2	EF00197	-	-
Spectrum Analyzer	R&S	FSIQ26	EF00242	2015-04	2016-04
LPD Antenna	R&S	HL 223	EF00212	2013-02	2016-02

Radiated spurious emissions					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic chamber	Frankonia	AC 2	EF00197	-	-
Spectrum Analyzer	R&S	FSIQ26	EF00242	2015-04	2016-04
Biconical Antenna	R&S	HK 116	EF00012	2013-02	2016-02
LPD Antenna	R&S	HL 223	EF00187	2014-03	2017-03
LPD Antenna	R&S	HL 025	EF00327	2015-10	2018-10

1.8 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyzer in dB μ V. Any external preamplifiers used are taken into account through internal analyzer settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyzer. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

$$\text{Reading on Analyzer (dB}\mu\text{V)} + \text{A.F. (dB)} = \text{Net field strength (dB}\mu\text{V/m)}$$

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dB μ V/m). The FCC limits are given in units of μ V/m. The following formula is used to convert the units of μ V/m to dB μ V/m:

$$\text{Limit (dB}\mu\text{V/m)} = 20 * \log (\mu\text{V/m})$$

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:

$$\begin{array}{rclcl} \text{Reading} & + & \text{AF} & = & \text{Net Reading} & : & \text{Net reading - FCC limit} & = & \text{Margin} \\ 21.5 \text{ dB}\mu\text{V} & + & 26 \text{ dB} & = & 47.5 \text{ dB}\mu\text{V/m} & : & 47.5 \text{ dB}\mu\text{V/m} - 57.0 \text{ dB}\mu\text{V/m} & = & -9.5 \text{ dB} \end{array}$$

1.9 Simulated human body

For radiated tests the implant was placed in a simulated human body.

Liquid components	
Component	percentage per weight
Deionized water	52.4
Bactericide	0.08
Hydroxy ethyl cellulose (HCE)	1.0
Sodium chloride	1.4
Sucrose	45.0

Measured tissue parameters:


Tissue parameters – 403.5MHz			
Component	Target	Measured	Tolerance [%]
Dielectric constant ϵ	62.5	63.08	0.93
Conductivity σ [ms/cm]	9.0	8.8	-2.22

2 Result Summary

FCC 47 CFR Part 95E, 95I, 15C, IC RSS-243, IC RSS-Gen				
Product Specific Standard Section	Requirement – Test	Reference Method	Result	Remarks
IC RSS-243 3.2 IC RSS-Gen 6.6	Occupied bandwidth	RSS-Gen 6.6	N/A	Informational only
FCC 95.628(d) FCC § 95.633(e) IC RSS-243 3.6, 5.1	Emission bandwidth	FCC § 95.628(a)(6)(i) FCC § 95.633(e)(3)	PASS	
FCC 95.628(e) IC RSS-243 3.3, 5.3 RSS-Gen 8.11	Frequency stability	EN 301 839-1 8.1	PASS	
FCC § 95.6369(f) IC RSS-243 § 5.4	Transmitter output power	EN 301 839-1 8.3	PASS	
FCC § 95.635(d) IC RSS-243 § 3.4, 5.5	Band edge compliance	FCC § 95.635(d) ANSI C63.4	PASS	
FCC § 95.635(d) IC RSS-243 § 3.4, 5.5 RSS-Gen 6.13	Transmitter unwanted emissions	FCC § 95.635(d) ANSI C63.4	PASS	
IC RSS-243 3.5, 5.6 IC RSS-Gen 7.1	Receiver spurious emissions	ANSI C63.4	PASS	
FCC § 15.207 IC RSS-Gen 8.8	AC power line conducted emissions	ANSI C63.4	N/A	EUT battery powered
FCC § 95.628(a)(3) IC RSS-243 3.6, 5.7.1	System threshold power levels	EN 301 839-1 10.1	N/A	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(1) IC RSS-243 3.6, 5.7.2	Monitoring system bandwidth	EN 301 839-1 10.2	N/A	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(2) IC RSS-243 3.6, 5.7.3	Scan cycle time	EN 301 839-1 10.3	N/A	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(2) IC RSS-243 3.6, 5.7.4	Minimum channel monitoring period	EN 301 839-1 10.3	N/A	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(4) IC RSS-243 3.6, 5.7.5	Channel Access	EN 301 839-1 10.4	N/A	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(4) IC RSS-243 3.6, 5.7.6	Discontinuation of MICS or MEDS session	EN 301 839-1 10.5	N/A	Applies only to equipment by which LBT is performed
FCC § 95.628(a)(5) IC RSS-243 3.6, 5.7.7	Use of the pre-scanned alternate channel	EN 301 839-1 10.6	N/A	Not used
Remarks:				

3 Test Conditions and Results


3.1 Test Conditions and Results – Occupied Bandwidth

Occupied Bandwidth acc. to IC RSS-243		Verdict: PASS
Test according to measurement reference	Reference Method	
	RSS-Gen 6.6	
Test frequency range	Tested frequencies	
	F _{LOW} / F _{MID} / F _{HIGH}	
EUT test mode	Modulated	
Limits		
None (Informational only)		
Test setup		
 <pre> graph LR SA[Spectrum Analyzer] --- EUT[EUT] </pre>		
Test procedure		
<ol style="list-style-type: none"> 1. EUT set to test mode (Communication tester is used if needed) 2. Span set to at least twice the emission spectrum 3. Resolution bandwidth set to 1 % of span 4. Occupied Bandwidth (99 %) measurement with spectrum analyzer built in measurement function 		
Test results		
Channel	Frequency [MHz]	Occupied Bandwidth [kHz]
F _{LOW}	402.45	229.3
F _{MID}	403.65	229.3
F _{HIGH}	404.85	229.3
Comments:		

Occupied Bandwidth – F_{Low}
Occupied Bandwidth acc. to RSS-Gen

Project Number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Wilfried Treffke
 Test Conditions: Tnom / Vnom
 Mode: Tx 402.45 MHz, 2FSK
 Test Date: 2015-09-30
 Verdict: NONE (INFORMATION ONLY)
 Note 1: A spectrum analyzer with an integrated 99% power bandwidth function is used

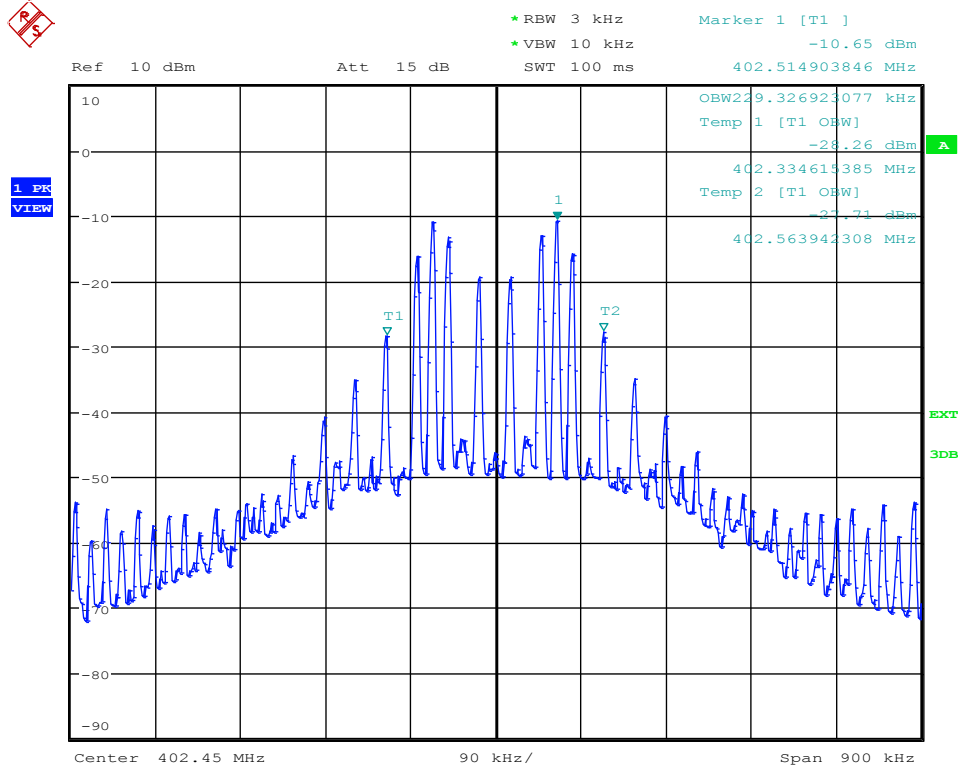


Date: 30.SEP.2015 11:48:21

Occupied Bandwidth - F_{MID}
Occupied Bandwidth acc. to RSS-Gen

Project Number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Wilfried Treffke
 Test Conditions: Tnom / Vnom
 Mode: Tx 403.65 MHz, 2FSK
 Test Date: 2015-09-30
 Verdict: NONE (INFORMATION ONLY)
 Note 1: A spectrum analyzer with an integrated 99% power bandwidth function is used

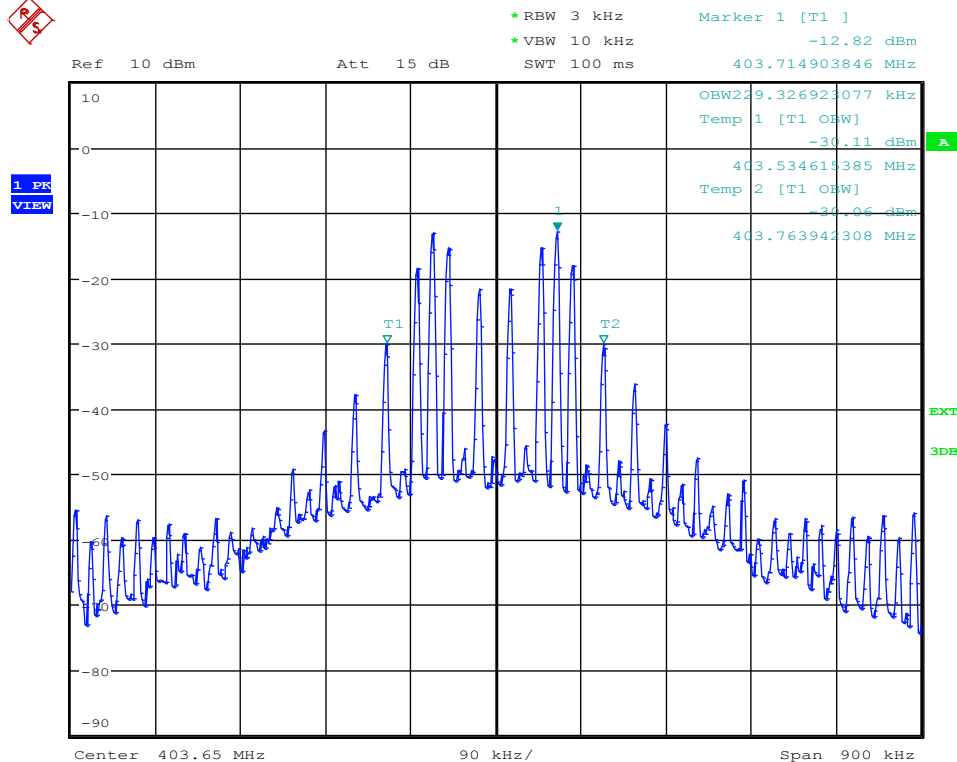


Date: 30.SEP.2015 11:42:07

Occupied Bandwidth - F_{HIGH}
Occupied Bandwidth acc. to RSS-Gen


Project Number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Wilfried Treffke
 Test Conditions: Tnom / Vnom
 Mode: Tx 404.85 MHz, 2FSK
 Test Date: 2015-09-30
 Verdict: NONE (INFORMATION ONLY)
 Note 1: A spectrum analyzer with an integrated 99% power bandwidth function is used

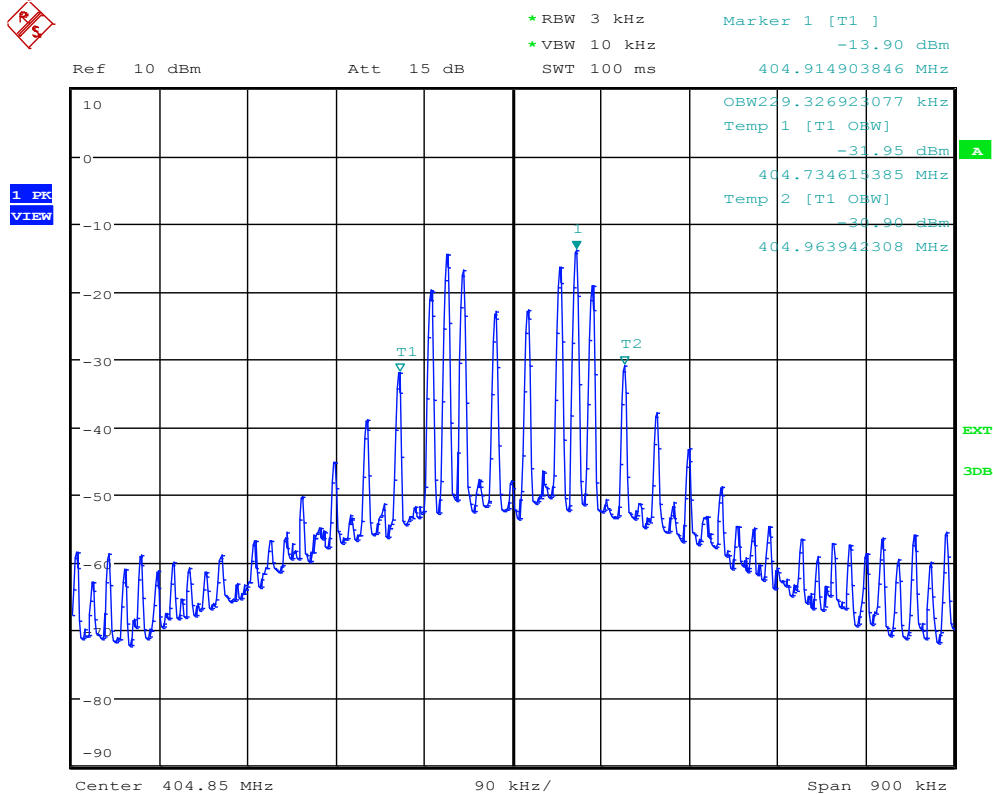

Date: 30.SEP.2015 12:46:39


3.2 Test Conditions and Results – Emission Bandwidth

Emission Bandwidth acc. to FCC Part 95 / IC RSS-243		Verdict: PASS		
EUT requirement rule parts and clause	Reference			
	FCC 95.628(d) / FCC 95.633(e) / IC RSS-243 3.3 5.1			
Test according to measurement reference	Reference Method			
	FCC 95.628(a)(6)(i) / FCC 95.633(e)(3)			
Test frequency range	Tested frequencies			
	$F_{\text{LOW}} / F_{\text{MID}} / F_{\text{HIGH}}$			
EUT test mode	Modulated			
Limits				
≤ 300 kHz				
Test setup				
 <pre> graph LR SA[Spectrum Analyzer] --- EUT[EUT] </pre>				
Test procedure				
<ol style="list-style-type: none"> 1. EUT set to test mode 2. Span set to at least twice the emission spectrum 3. Detector set to peak and max hold 4. Envelope peak value of emission spectrum is selected 5. Marker on envelope of spectrum is set to level of -20 dB to the left of the peak 6. Marker on envelope of spectrum is set to level of -20 dB to the right of the peak 7. 20 dB Emission Bandwidth is determined by marker frequency separation 				
Test results				
Channel	Frequency [MHz]	Emission Bandwidth [kHz]	Limit [kHz]	Result
F_{LOW}	402.45	234.5	≤ 300	PASS
F_{MID}	403.65	234.5	≤ 300	PASS
F_{HIGH}	404.85	234.5	≤ 300	PASS
Comments:				

Emission Bandwidth – F_{LOW}
Emission Bandwidth acc. to FCC Part 95.633

Project Number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Wilfried Treffke
 Test Conditions: Tnom / Vnom
 Mode: Tx 402.45 MHz, 2FSK
 Test Date: 2015-09-30
 Verdict: PASS
 Note 1: 20 dB bandwidth

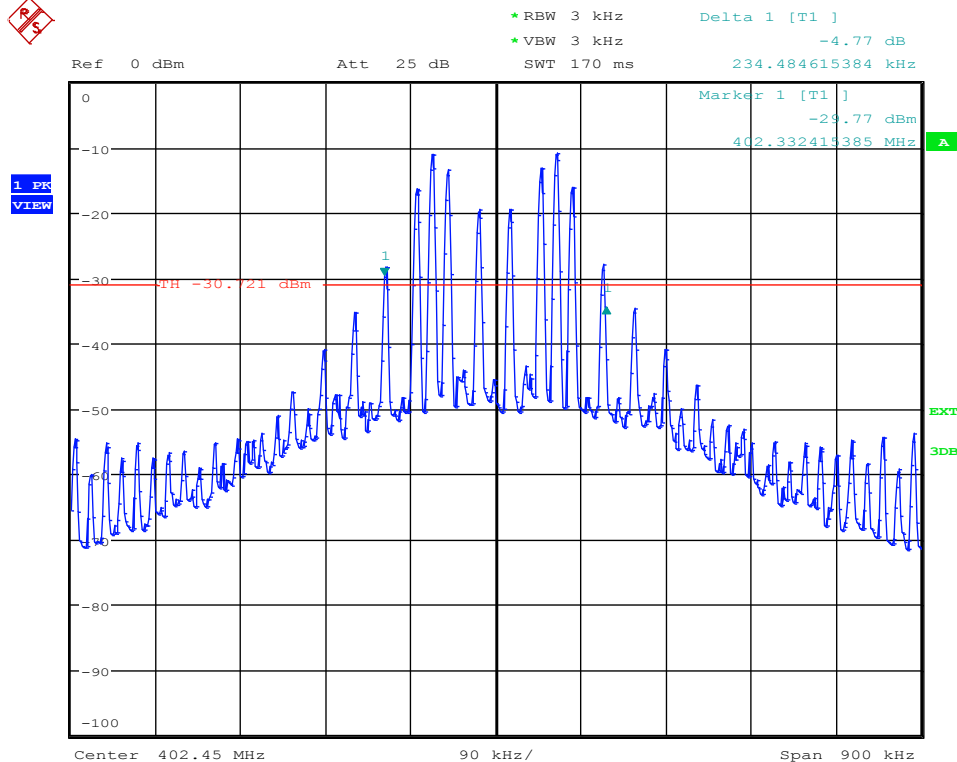


Date: 30.SEP.2015 13:12:00

Emission Bandwidth – F_{MD}
Emission Bandwidth acc. to FCC Part 95.633

Project Number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Wilfried Treffke
 Test Conditions: Tnom / Vnom
 Mode: Tx 403.65 MHz, 2FSK
 Test Date: 2015-09-30
 Verdict: PASS
 Note 1: 20 dB bandwidth

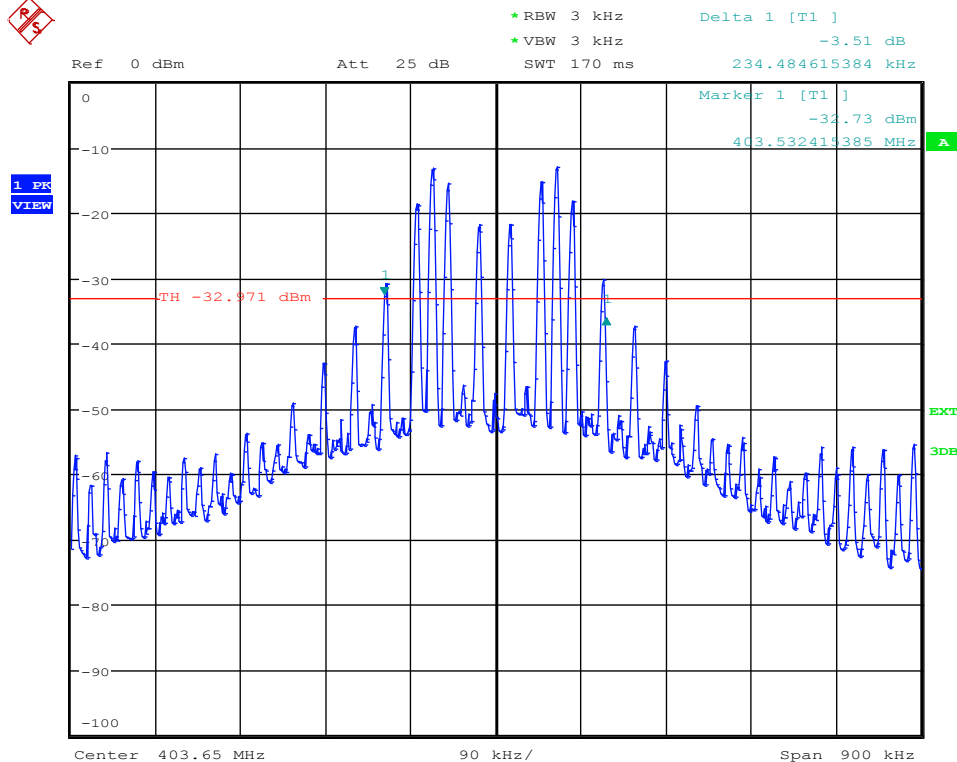


Date: 30.SEP.2015 13:05:32

Emission Bandwidth – 1 F_{HIGH}

Emission Bandwidth acc. to FCC Part 95.633


Project Number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Wilfried Treffke
 Test Conditions: Tnom / Vnom
 Mode: Tx 404.85 MHz, 2FSK
 Test Date: 2015-09-30
 Verdict: PASS
 Note 1: 20 dB bandwidth

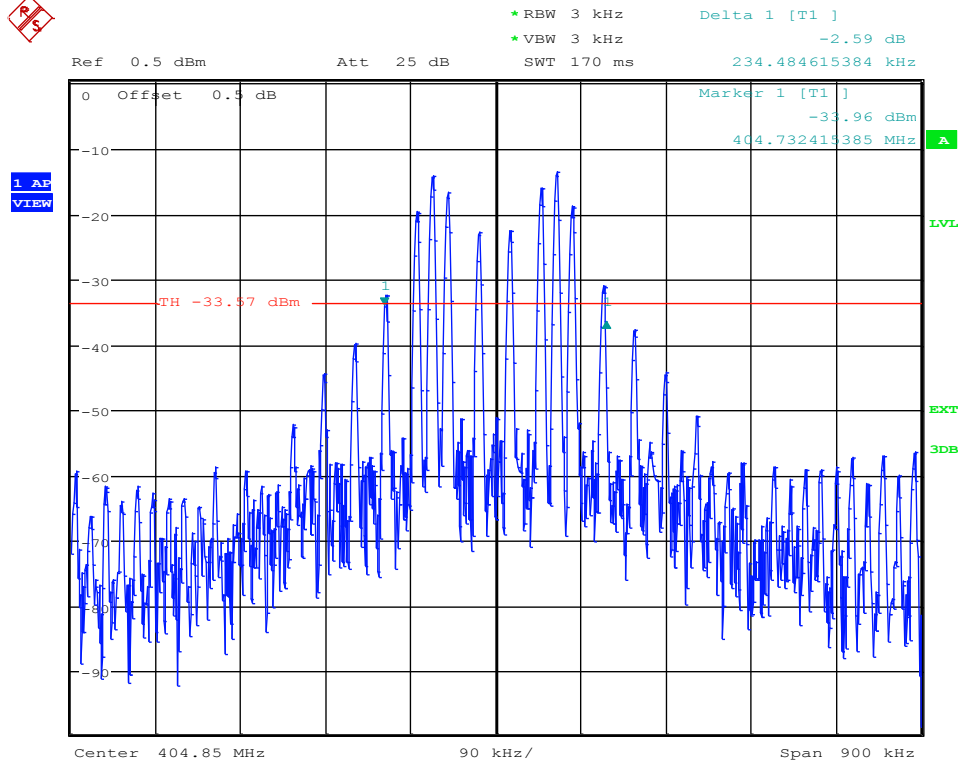


Date: 30.SEP.2015 12:57:01

3.3 Test Conditions and Results – Frequency stability

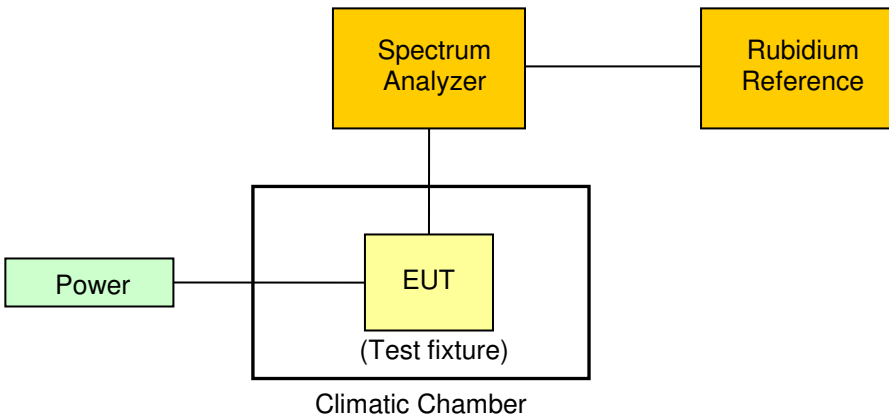Frequency stability acc. to FCC Part 95 / IC RSS-243		Verdict: PASS
EUT requirement rule parts and clause	Reference	
	FCC 95.628(e) / IC RSS-243 3.3 5.3 / RSS-Gen 4.7	
Test according to measurement reference	Reference Method	
	EN 301 839-1 8.1	
Test frequency range	Tested frequencies	
	$F_{\text{LOW}} / F_{\text{MID}} / F_{\text{HIGH}}$	
EUT test mode	Unmodulated	
Limits		
$\leq \pm 100$ ppm		
Test setup		
 <pre> graph LR Power[Power] --- EUT[EUT (Test fixture)] subgraph Climatic Chamber EUT end EUT --- SA[Spectrum Analyzer] SA --- RR[Rubidium Reference] </pre>		
Test procedure		
<ol style="list-style-type: none"> 1. EUT set to test mode with supply voltage and temperature set to nominal conditions 2. EUT transmits without modulation 3. Detector set to peak and max hold 4. Peak of emission is measured using a frequency counter 5. The frequency error is determined as the deviation of the emission frequency from the nominal frequency stated by the customer. 		


Test results					
Channel	Nominal Frequency [MHz]	Temperature	Supply voltage	Frequency [MHz]	Drift [ppm]
F _{LOW}	402.45	T _{NOM} = 37 °C	V _{NOM} = 3.0 VDC	402.448021	-04.92
F _{LOW}	402.45	T _{MIN} = 25 °C	V _{NOM} = 3.0 VDC	402.448492	-03.75
F _{LOW}	402.45	T _{MAX} = 45 °C	V _{NOM} = 3.0 VDC	402.447624	-05.90
F _{MID}	403.65	T _{NOM} = 37 °C	V _{NOM} = 3.0 VDC	403.648088	-04.74
F _{MID}	403.65	T _{MIN} = 25 °C	V _{NOM} = 3.0 VDC	403.648584	-03.51
F _{MID}	403.65	T _{MAX} = 45 °C	V _{NOM} = 3.0 VDC	403.647718	-05.65
F _{HIGH}	404.85	T _{NOM} = 37 °C	V _{NOM} = 3.0 VDC	404.848193	-04.46
F _{HIGH}	404.85	T _{MIN} = 25 °C	V _{NOM} = 3.0 VDC	404.848649	-03.34
F _{HIGH}	404.85	T _{MAX} = 45 °C	V _{NOM} = 3.0 VDC	404.847771	-05.51
Comments:					

3.4 Test Conditions and Results – Transmitter output power

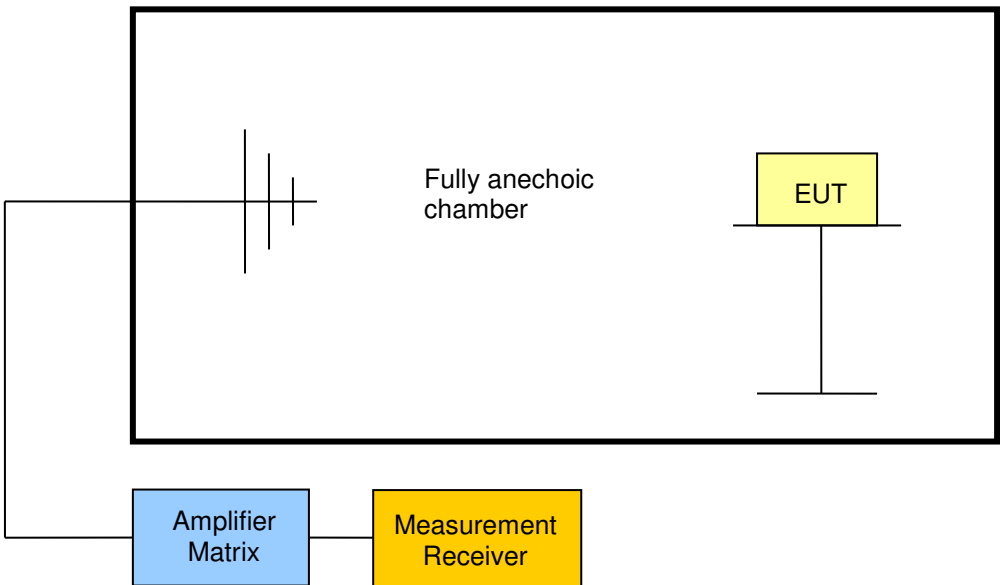Transmitter output power acc. to FCC Part 95 / IC RSS-243		Verdict: PASS
EUT requirement rule parts and clause	Reference	
	FCC 95.639(f) / IC RSS-243 5.4	
Test according to measurement reference	Reference Method	
	EN 301 839-1 8.3	
Test frequency range	Tested frequencies	
	$F_{LOW} / F_{MID} / F_{HIGH}$	
EUT test mode	Modulated	
Limits		
$\leq 25 \mu W (-16 \text{ dBm}) \text{ e.i.r.p.}$		
Test setup		
 <p>The diagram illustrates the test setup. An Amplifier Matrix (blue box) is connected to a Fully anechoic chamber (large rectangle). Inside the chamber, an EUT (yellow box) is mounted on a stand. The chamber is represented by a rectangle with a cross-hatch pattern on its left side. A Measurement Receiver (yellow box) is connected to the EUT. The Amplifier Matrix is connected to the chamber via a line that enters from the left and connects to the chamber's boundary.</p>		
Test procedure		
<ol style="list-style-type: none"> 1. EUT set to test frequency with modulation 2. Measurement polarization is set to vertical 3. Span is set according to measurement range and detector is set to peak and max hold 4. Resolution bandwidth is set to be at least twice the emission bandwidth 5. During the sweep the EUT is rotated to obtain maximum emission level 6. Measurement is repeated with horizontal measurement polarization 		


Test results					
Channel	Frequency [MHz]	Emission Level [dbm e.i.r.p.]	Detector	Limit [dbm e.i.r.p.]	Margin [dB]
F _{LOW}	402.45	-36.0	pk	-16	-20.00
F _{MID}	403.65	-35.2	pk	-16	-19.20
F _{HIGH}	404.85	-37.3	pk	-16	-21.30
Comments:					

3.5 Test Conditions and Results – Band-edge and In-band Emissions

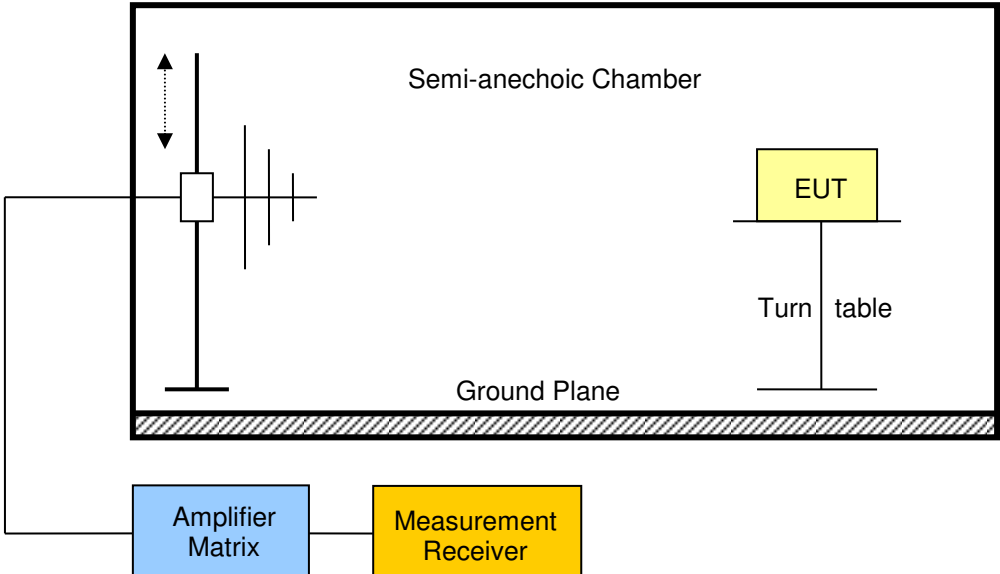Band-edge and in-band emission compliance acc. to FCC Part 95 / IC RSS-243		Verdict: PASS
EUT requirement rule parts and clause	Reference FCC 95.635(d) / IC RSS-243 3.5 5.5 / RSS-Gen 4.9	
Test according to measurement reference	Reference Method FCC 95.635(d) / ANSI C 63.4	
Test frequency range	Tested frequencies $F_{LOW} / F_{MID} / F_{HIGH}$	
EUT test mode	Modulated	
Limits - FCC		
Frequency range	Limit	
$402 \text{ MHz} - 250 \text{ kHz} \leq f \leq 402 \text{ MHz}$	20 dB below maximum permitted output power	
$402 \text{ MHz} < f < 150 \text{ kHz} - f_C$	20 dB below transmitter output power	
$150 \text{ kHz} + f_C < f < 405 \text{ MHz}$	20 dB below transmitter output power	
$405 \text{ MHz} \leq f \leq 405 \text{ MHz} + 250 \text{ kHz}$	20 dB below maximum permitted output power	
Limits - IC		
Frequency range	Limit	
$402 \text{ MHz} - 250 \text{ kHz} < f < 150 \text{ kHz} - f_C$	20 dB below maximum permitted output power	
$150 \text{ kHz} + f_C < f < 405 \text{ MHz} + 250 \text{ kHz}$	20 dB below maximum permitted output power	
Because the FCC limits are more stringent than the Industry Canada limits, the FCC limits are used to show compliance with the band-edge emission requirements.		
Test setup		
 <p>The diagram illustrates the test setup. A Semi-anechoic Chamber is shown with a Ground Plane at the bottom. Inside the chamber, an Amplifier Matrix is connected to a Measurement Receiver. The EUT (Equipment Under Test) is placed on a Turn table. The chamber is designed to minimize reflections, ensuring accurate measurements of the EUT's emissions.</p>		


Test procedure					
1. EUT set to test frequency with modulation 2. Measurement polarization is set to vertical 3. Span it set according to measurement range 4. Resolution bandwidth is set to 1% of the emission bandwidth and detector is set to peak 5. During the sweep the EUT is rotated to obtain maximum emission level 6. Measurement is repeated with horizontal measurement polarization					
Test results					
Channel	Frequency [MHz]	Max. Emission Level [dB μ V/m]	Max. Carrier Level [dB μ V/m]	In-band Limit [dB μ V/m]	Result
F _{LOW}	402.45	24.95	70.82	50.82	PASS
F _{LOW}	402.45	24.47	70.82	50.82	PASS
F _{HIGH}	404.85	21.14	67.80	47.80	PASS
F _{HIGH}	404.85	14.45	67.80	47.80	PASS
Comments: see attached diagrams					

3.6 Test Conditions and Results – Transmitter unwanted emissions

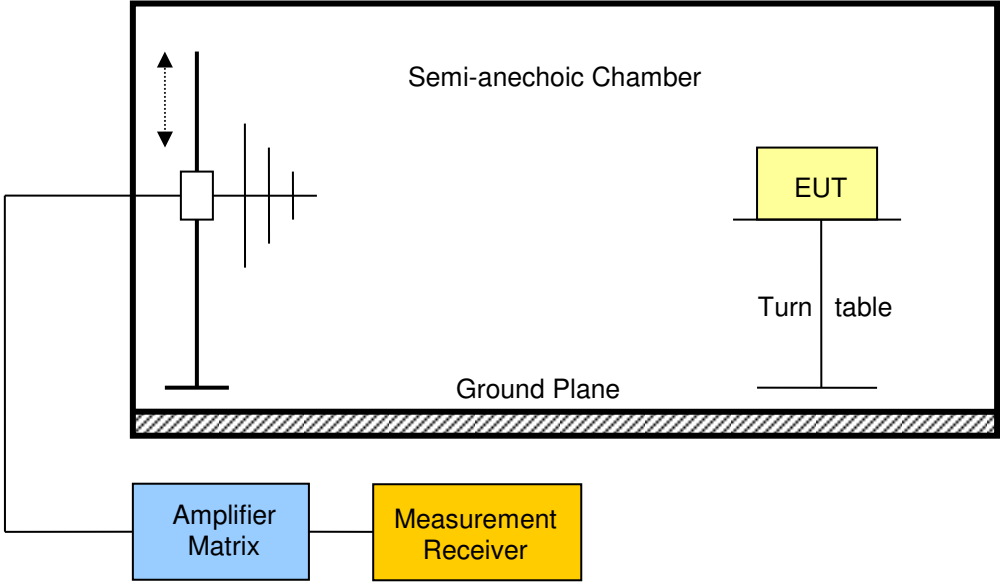Transmitter unwanted emissions acc. to FCC Part 95 / IC RSS-243				Verdict: PASS
Test according referenced standards	Reference Method			
	FCC 95.635(d) / IC RSS-243 3.4 5.5 / IC RSS-Gen 4.9			
Test according to measurement reference	Reference Method			
	FCC 95.635(d) / ANSI C 63.4			
Test frequency range	Tested frequencies			
	30 MHz – 10 th Harmonic			
Limits				
Frequency range [MHz]	Detector	Limit [μ V/m]	Limit [dB μ V/m]	Limit Distance [m]
30 – 88	Quasi-Peak	100	40	3
88 – 216	Quasi-Peak	150	43.5	3
216 – 960	Quasi-Peak	200	46	3
960 – 1000	Quasi-Peak	500	54	3
> 1000	Average	500	54	3
Test setup				
 <p>The diagram illustrates the test setup. A Semi-anechoic Chamber is shown with a Ground Plane at the bottom. Inside the chamber, an Amplifier Matrix is connected to a Measurement Receiver. The EUT (Equipment Under Test) is placed on a Turn table. The chamber is labeled 'Semi-anechoic Chamber' and 'Ground Plane'. The Amplifier Matrix and Measurement Receiver are shown as separate components connected to the chamber.</p>				

Test procedure									
1. EUT set to test mode 2. Span it set according to measurement range 3. Resolution bandwidth below 1 GHz is set according to CISPR 16 with peak/quasi-peak detector and RBW of 1 MHz with peak/average detector is used above 1 GHz 4. Markers are set to peak emission levels within restricted bands									
Test results									
Channel	Frequency [MHz]	Mode	Emission [MHz]	Level [db μ V/m]	Det.	Pol.	Limit [db μ V/m]	Limit dist. [m]*	Margin [dB]
F _{LOW}	402.45	Modulated	83.38	27.87	pk	ver	40.00	3m	-12.13
F _{LOW}	402.45	Modulated	400.54	14.02	pk	hor	46.00	3m	-31.98
F _{LOW}	402.45	Modulated	401.939	01.24	pk	ver	59.40	3m	-58.16
F _{LOW}	402.45	Modulated	407.629	16.66	pk	hor	46.00	3m	-29.34
F _{LOW}	402.45	Modulated	407.629	14.30	pk	ver	46.00	3m	-31.70
F _{HIGH}	404.85	Modulated	398.522	24.67	pk	hor	46.00	3m	-21.33
F _{HIGH}	404.85	Modulated	398.522	23.30	pk	ver	46.00	3m	-22.70
F _{HIGH}	404.85	Modulated	405.029	17.51	pk	hor	59.40	3m	-41.89
F _{HIGH}	404.85	Modulated	405.029	17.41	pk	ver	59.40	3m	-41.99
F _{HIGH}	404.85	Modulated	406.44	20.04	pk	hor	46.00	3m	-25.96
F _{HIGH}	404.85	Modulated	406.44	17.44	pk	ver	46.00	3m	-28.56
Comments: * Physical distance between EUT and measurement antenna.									

3.7 Test Conditions and Results – Receiver spurious emissions

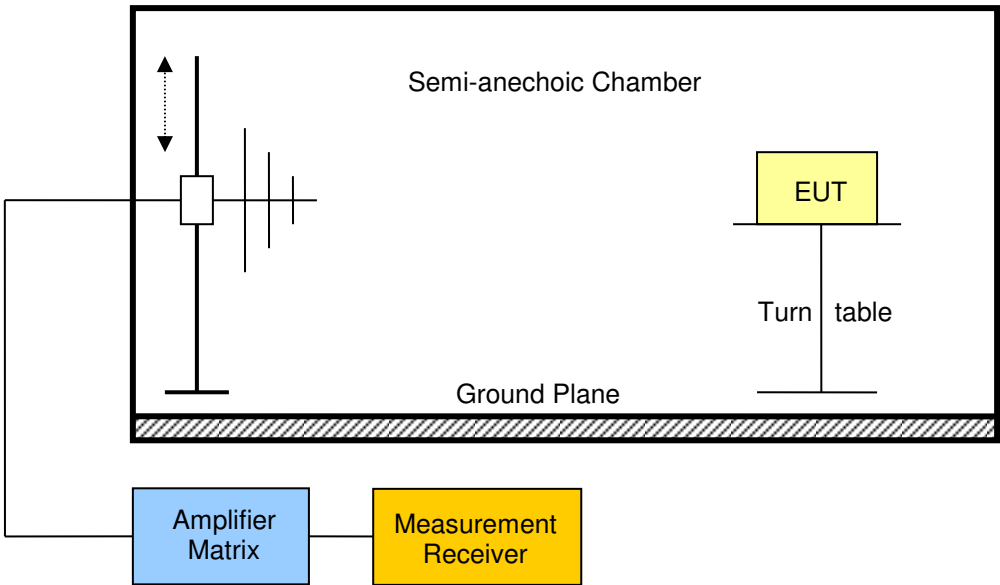Receiver spurious emissions acc. to IC RSS-243				Verdict: PASS
Test according referenced standards	Reference Method			
	IC RSS-243 3.5 5.6 / IC RSS-Gen 4.10 6.1			
Test according to measurement reference	Reference Method			
	ANSI C 63.4			
Test frequency range	Tested frequencies			
	30 MHz – 5 th Harmonic			
EUT test mode	Receive			
Limits				
Frequency range [MHz]	Detector	Limit [μ V/m]	Limit [dB μ V/m]	Limit Distance [m]
30 – 88	Quasi-Peak	100	40	3
88 – 216	Quasi-Peak	150	43.5	3
216 – 960	Quasi-Peak	200	46	3
960 – 1000	Quasi-Peak	500	54	3
> 1000	Average	500	54	3
Test setup				
 <p>The diagram illustrates the test setup within a Semi-anechoic Chamber. A Ground Plane is located at the bottom. An EUT (Equipment Under Test) is placed on a Turn table. An Amplifier Matrix is connected to the chamber, and its output is fed into a Measurement Receiver. A vertical antenna is positioned to receive signals from the EUT.</p>				

Test procedure							
1. EUT set to receive mode (Communication tester is used if needed) 2. Span it set according to measurement range 3. Resolution bandwidth below 1 GHz is set according to CISPR 16 with peak/quasi-peak detector and RBW of 1 MHz with peak/average detector is used above 1 GHz 4. Markers are set to peak emission levels							
Test results							
Channel	Frequency [MHz]	Emission [MHz]	Emission Level [dB μ V/m]	Det.	Pol.	Limit [dB μ V/m]	Margin [dB]
F _{MID}	403.65	30.68	29.32	pk	ver	40.00	-10.68
F _{MID}	403.65	187.08	32.76	pk	hor	43.50	-10.74
F _{MID}	403.65	873.6	19.18	pk	ver	46.00	-26.82
F _{MID}	403.65	1702	34.45	pk	hor	53.98	-19.53
F _{MID}	403.65	3940	40.29	pk	hor	53.98	-13.69
Comments:							


ANNEX A Transmitter radiated power

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: Tx; 402.45 MHz
 Test Date: 2016-02-22
 Note: Tx Power EIRP

Index 53

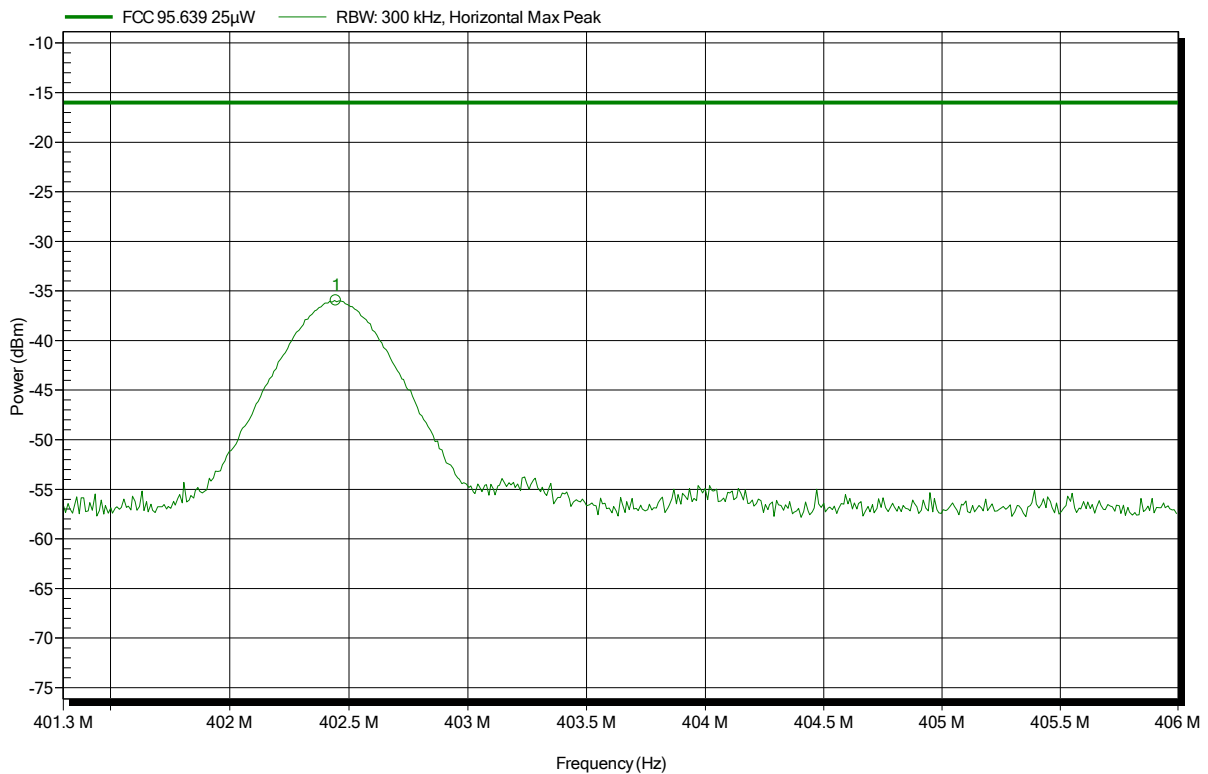


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
402.445 MHz	-36 dBm	-16 dBm	-19.97 dB	Pass

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Vertical
Measurement distance:	3 m
Mode:	Tx; 402.45 MHz
Test Date:	2016-02-22
Note:	Tx Power EIRP

Index 54

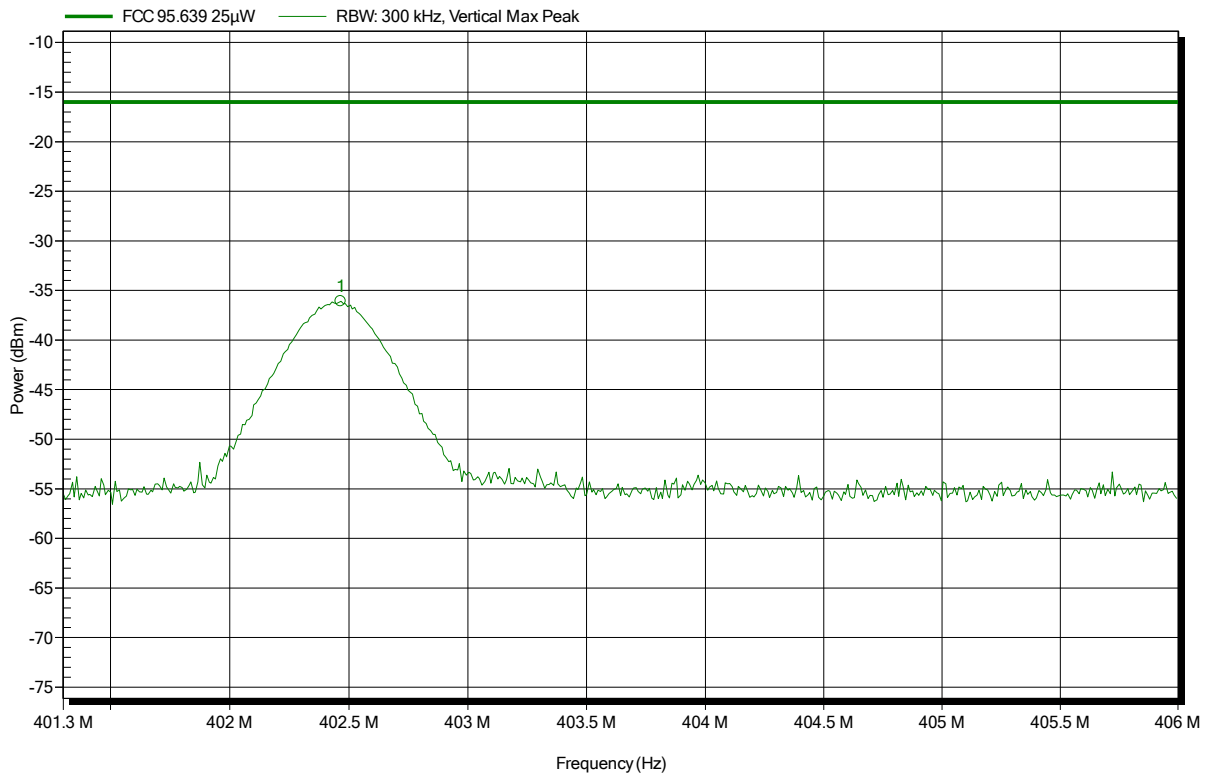


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
402.466 MHz	-36.1 dBm	-16 dBm	-20.08 dB	Pass

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Horizontal
Measurement distance:	3 m
Mode:	Tx; 402.45 MHz
Test Date:	2016-02-22
Note:	Power dB μ V/m ERP

Index 56

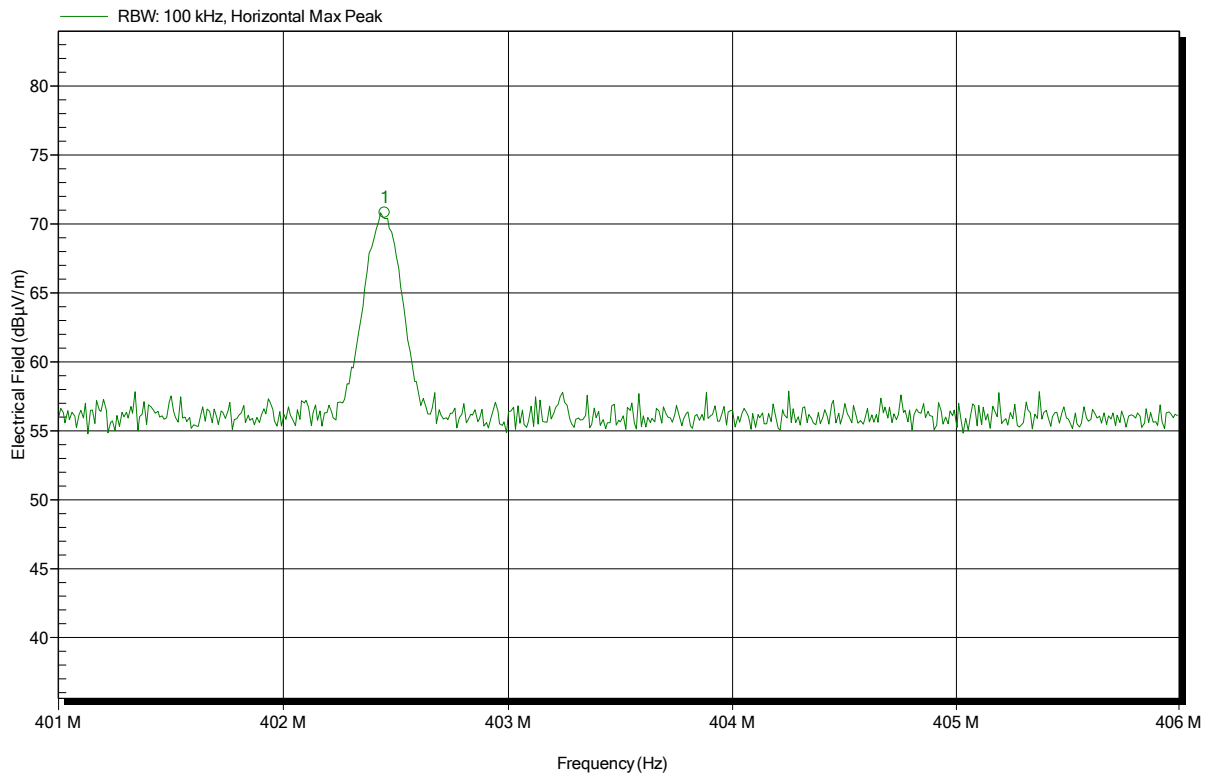
 Frequency
402.45 MHz


 Peak
70.82 dB μ V/m

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Vertical
Measurement distance:	3 m
Mode:	Tx; 402.45 MHz
Test Date:	2016-02-22
Note:	Power dB μ V/m ERP

Index 55

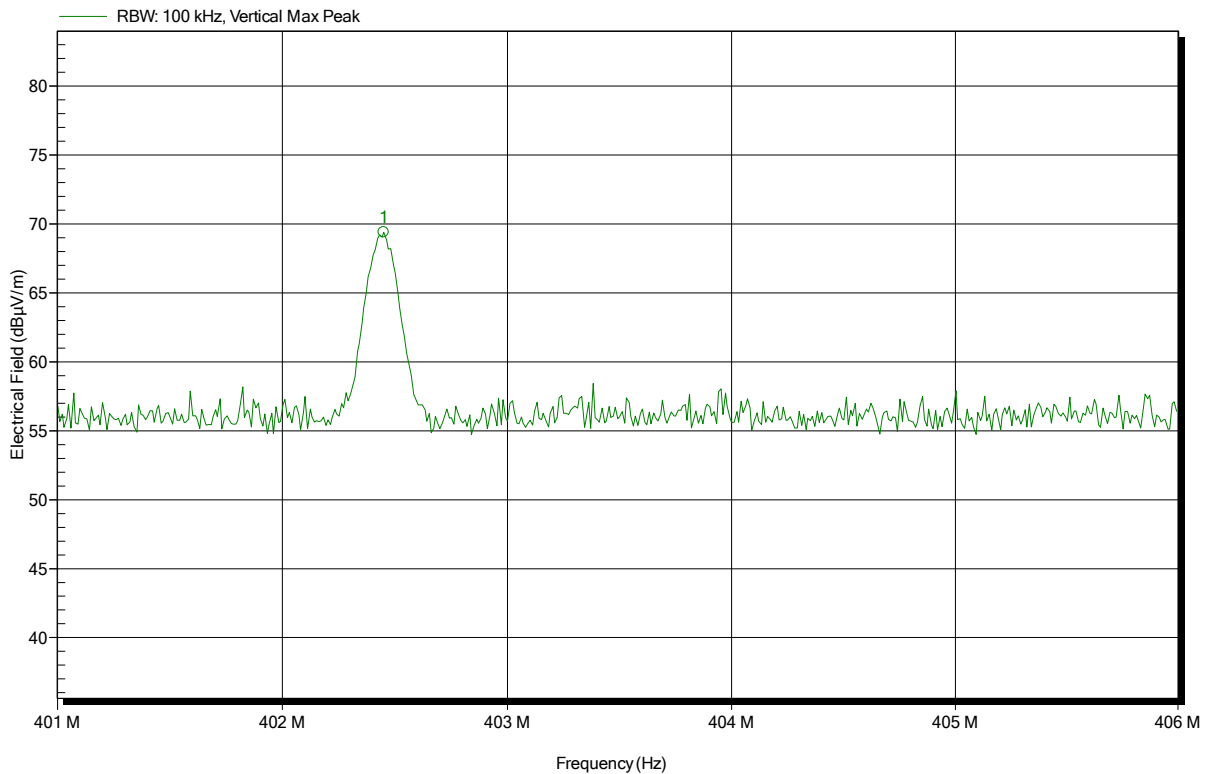
 Frequency
402.45 MHz


 Peak
69.39 dB μ V/m

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Horizontal
Measurement distance:	3 m
Mode:	Tx; 403.65 MHz
Test Date:	2016-02-22
Note:	Tx Power EIRP

Index 51

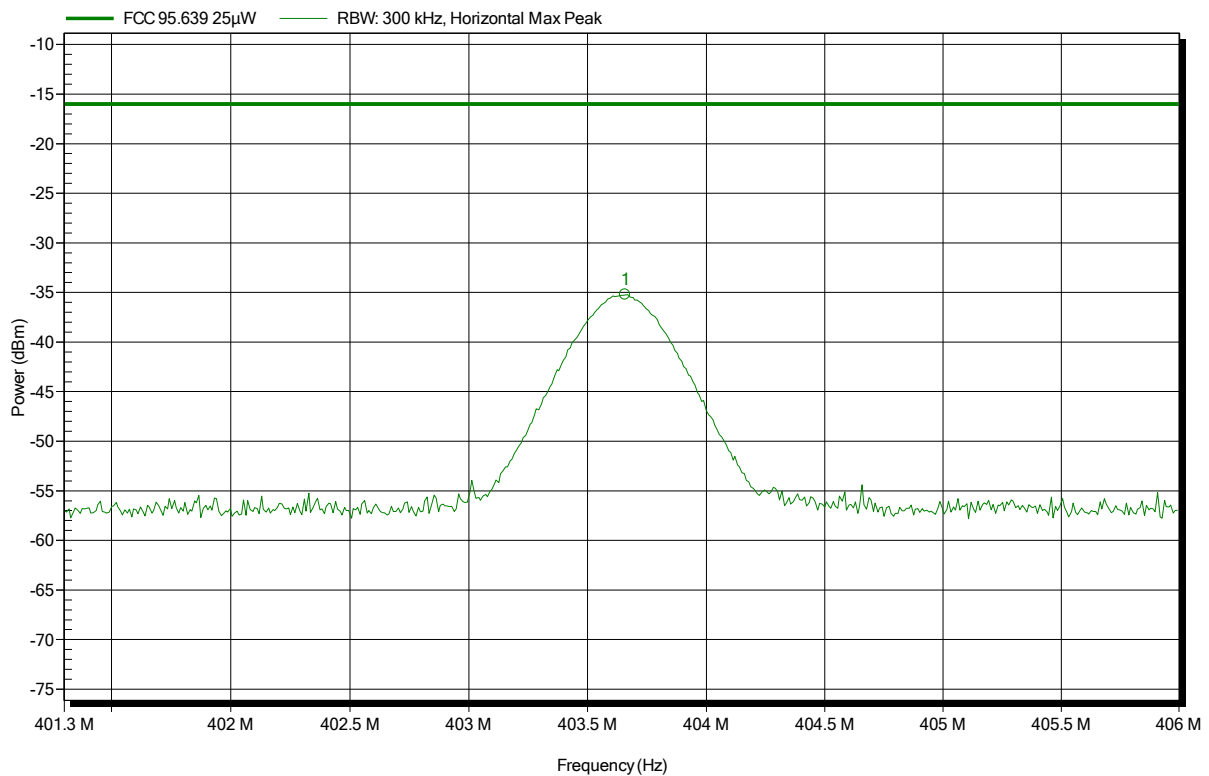


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
403.658 MHz	-35.2 dBm	-16 dBm	-19.22 dB	Pass

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Vertical
Measurement distance:	3 m
Mode:	Tx; 403.65 MHz
Test Date:	2016-02-22
Note:	Tx Power EIRP

Index 50

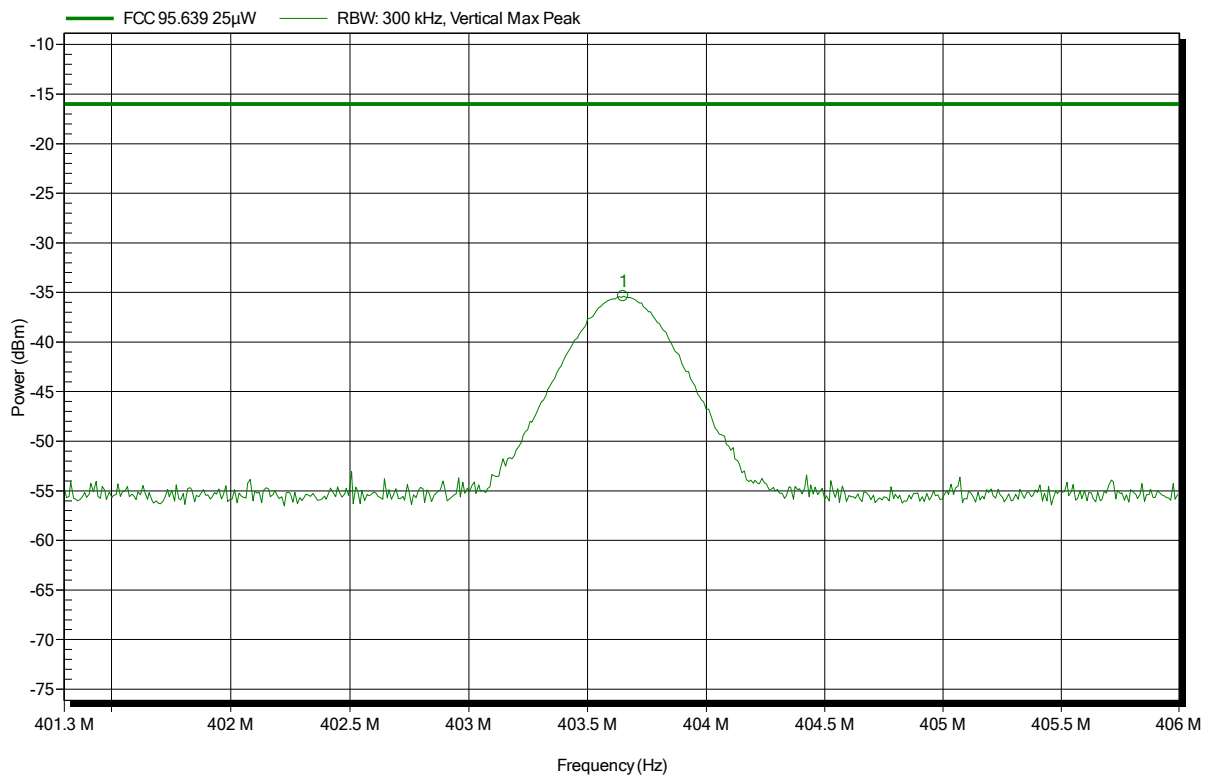

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
403.65 MHz	-35.4 dBm	-16 dBm	-19.38 dB	Pass

 Test Report No.: G0M-1507-4972-TFC95IMR2-V01


 Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Horizontal
Measurement distance:	3 m
Mode:	Tx; 404.85 MHz
Test Date:	2016-02-22
Note:	Tx Power EIRP

Index 57

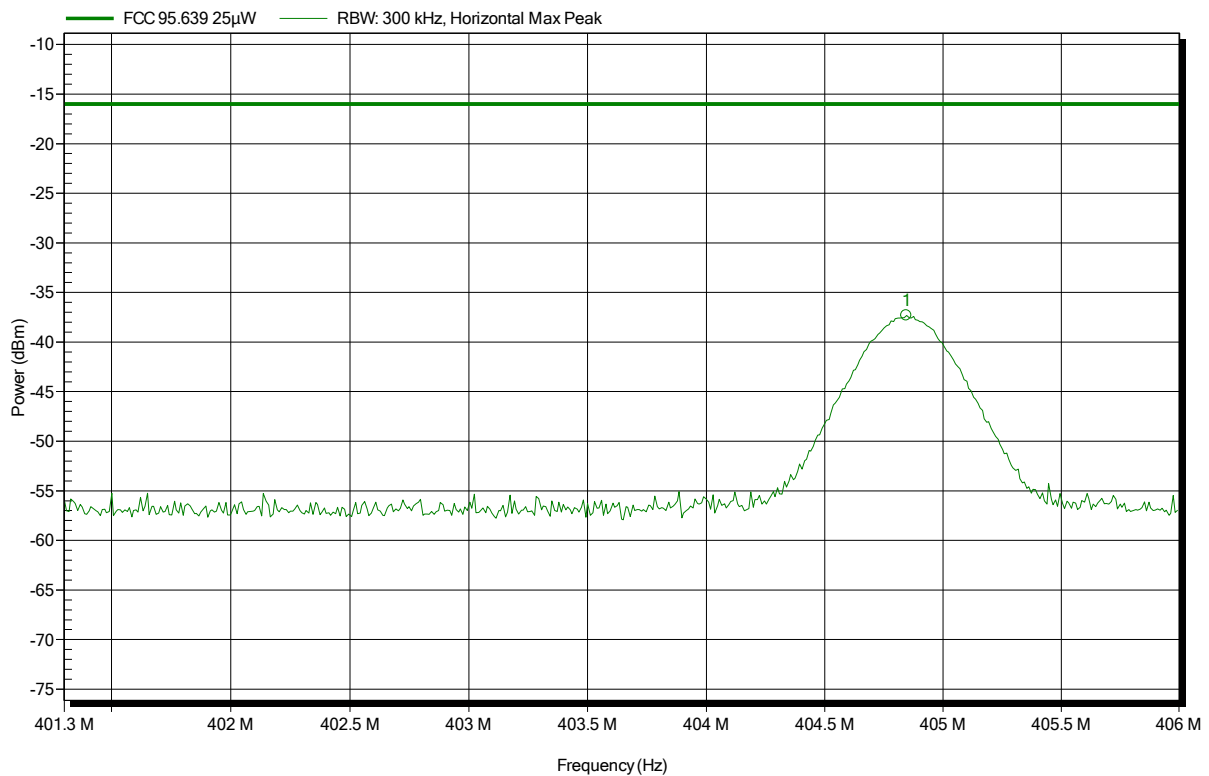


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
404.845 MHz	-37.3 dBm	-16 dBm	-21.33 dB	Pass

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Vertical
Measurement distance:	3 m
Mode:	Tx; 404.85 MHz
Test Date:	2016-02-22
Note:	Tx Power EIRP

Index 58

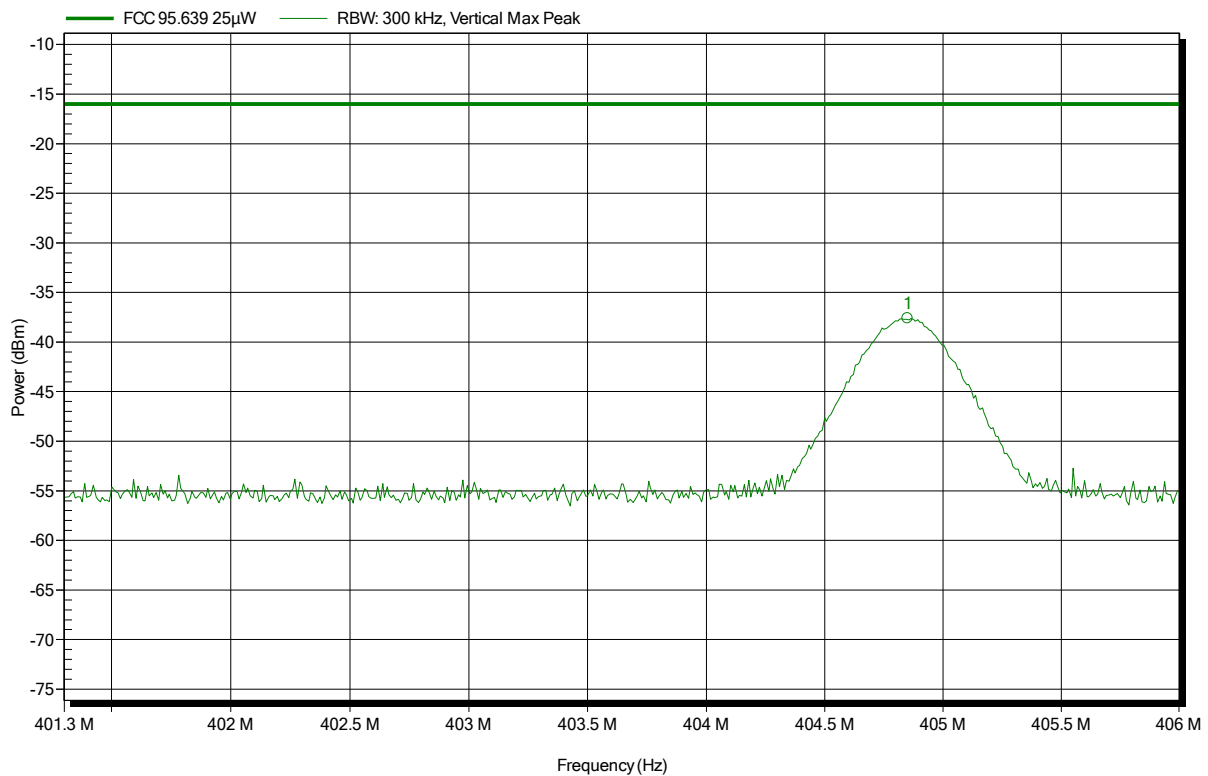

Frequency	Peak	Peak Limit	Peak Difference	Peak Status
404.85 MHz	-37.6 dBm	-16 dBm	-21.6 dB	Pass

 Test Report No.: G0M-1507-4972-TFC95IMR2-V01


 Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Horizontal
Measurement distance:	3 m
Mode:	Tx; 404.85 MHz
Test Date:	2016-02-22
Note:	Power dB μ V/m ERP

Index 60

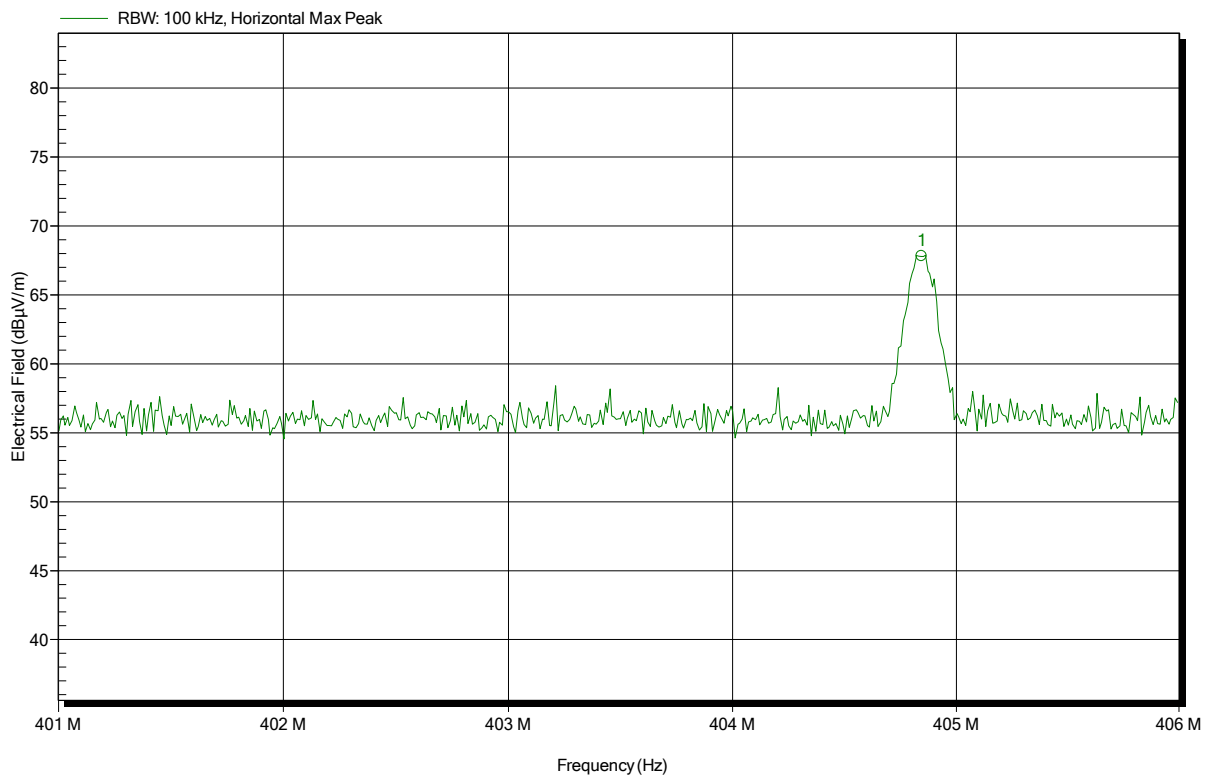
 Frequency
404.845 MHz


 Peak
67.81 dB μ V/m

Radiated power according to FCC Part 95; Subpart E

Order number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Vertical
Measurement distance:	3 m
Mode:	Tx; 404.85 MHz
Test Date:	2016-02-22
Note:	Power dB μ V/m ERP

Index 59

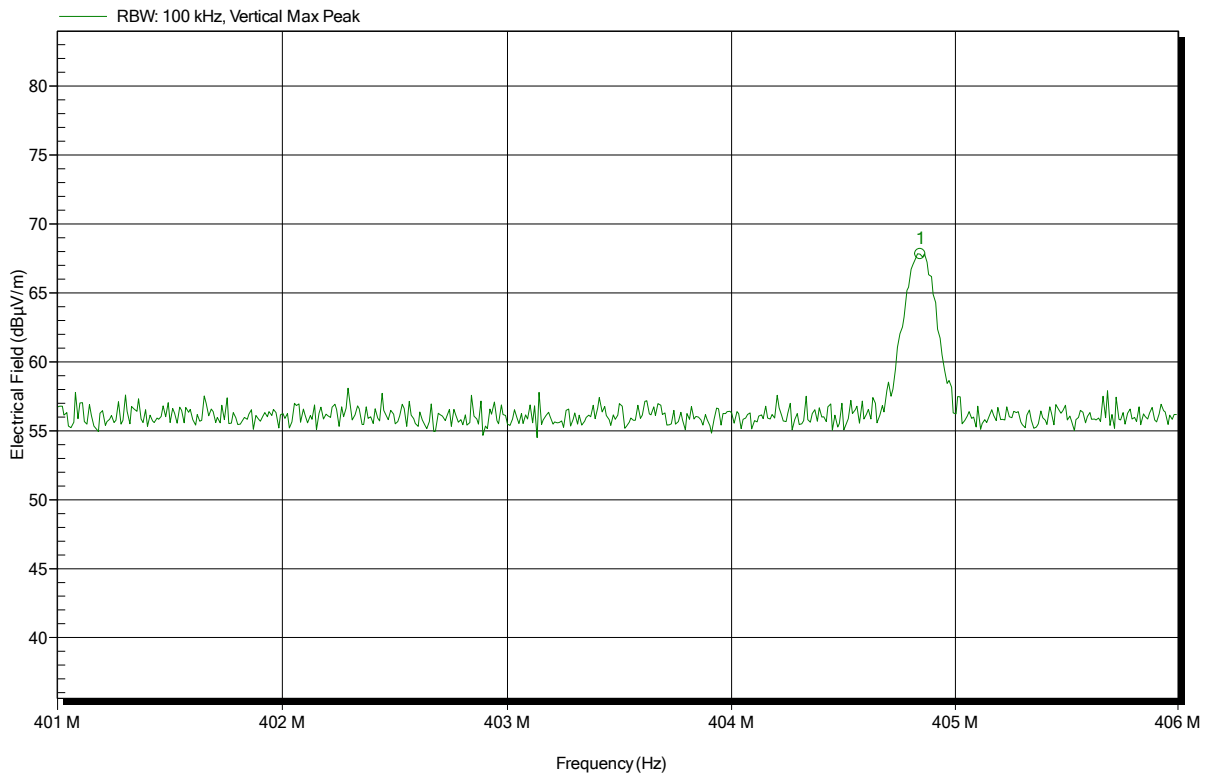
 Frequency
404.844 MHz

 Peak
67.81 dB μ V/m


ANNEX B Transmitter radiated spurious emissions

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HK116, Horizontal
Measurement distance:	3 m
Mode:	TX; 402.45 MHz
Test Date:	2016-02-23
Note:	

Index 64

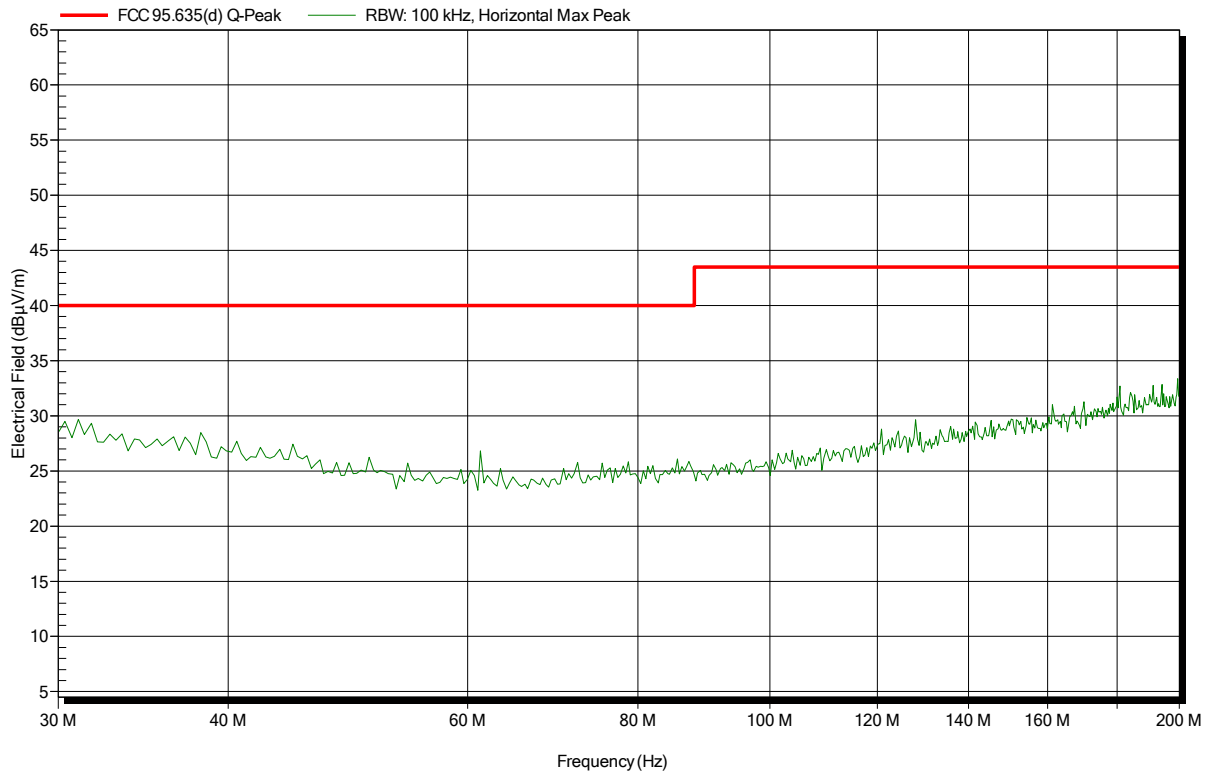


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HK116, Vertical
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz
 Test Date: 2016-02-23
 Note:

Index 65

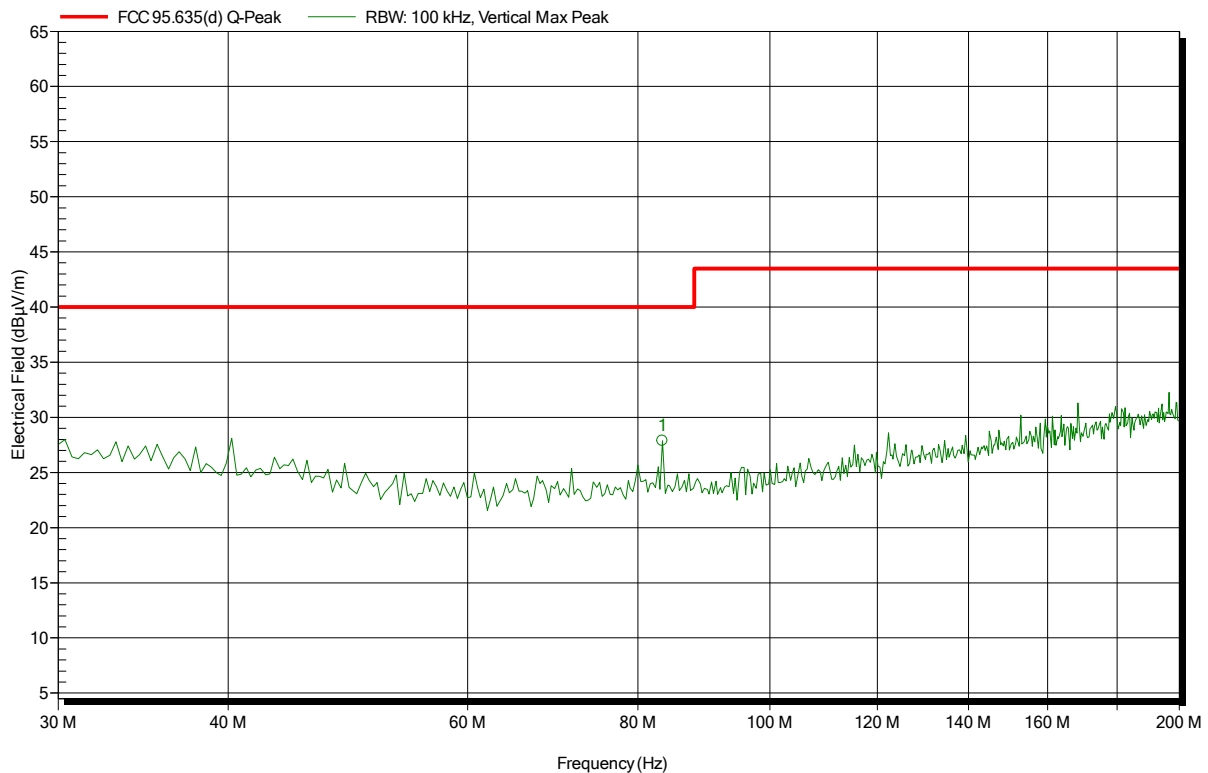


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
83.38 MHz	27.87 dBµV/m	40 dBµV/m	-12.13 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz
 Test Date: 2016-02-23
 Note:

Index 66

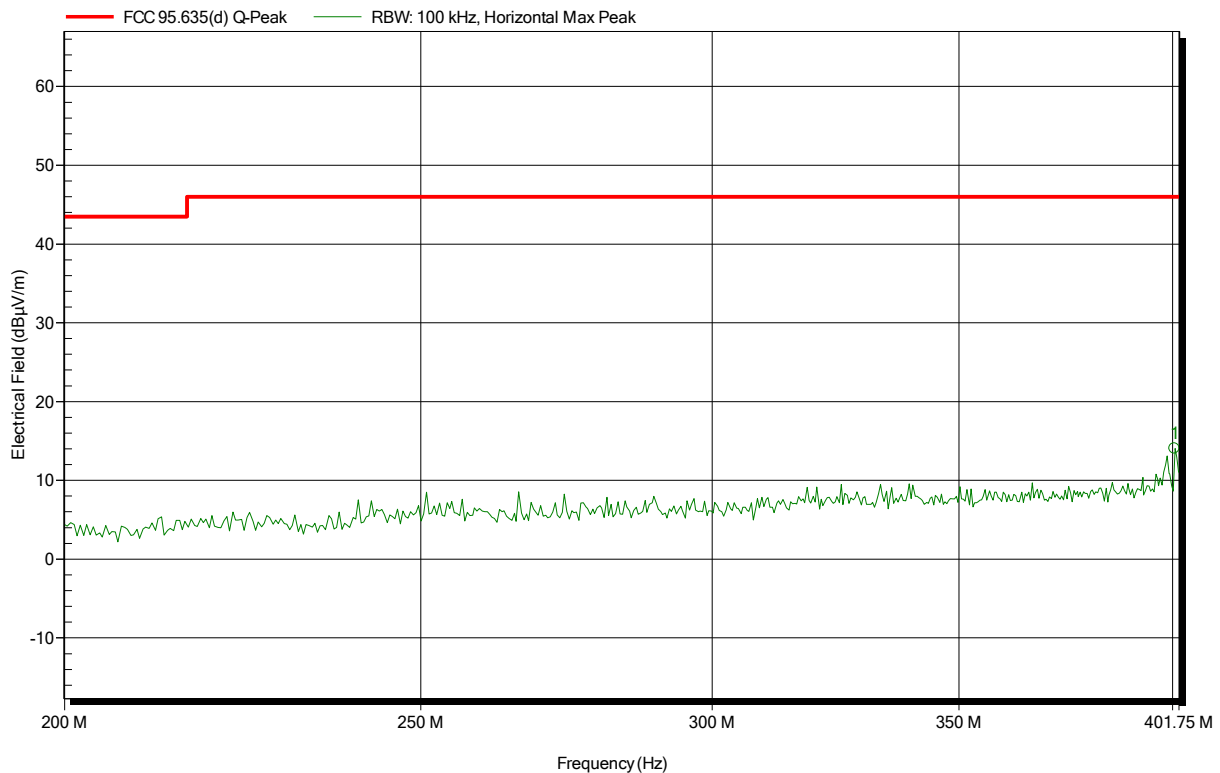


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
400.54 MHz	14.02 dBµV/m	46 dBµV/m	-31.98 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Horizontal
Measurement distance:	3 m
Mode:	TX; 402.45 MHz
Test Date:	2016-02-23
Note:	

Index 67

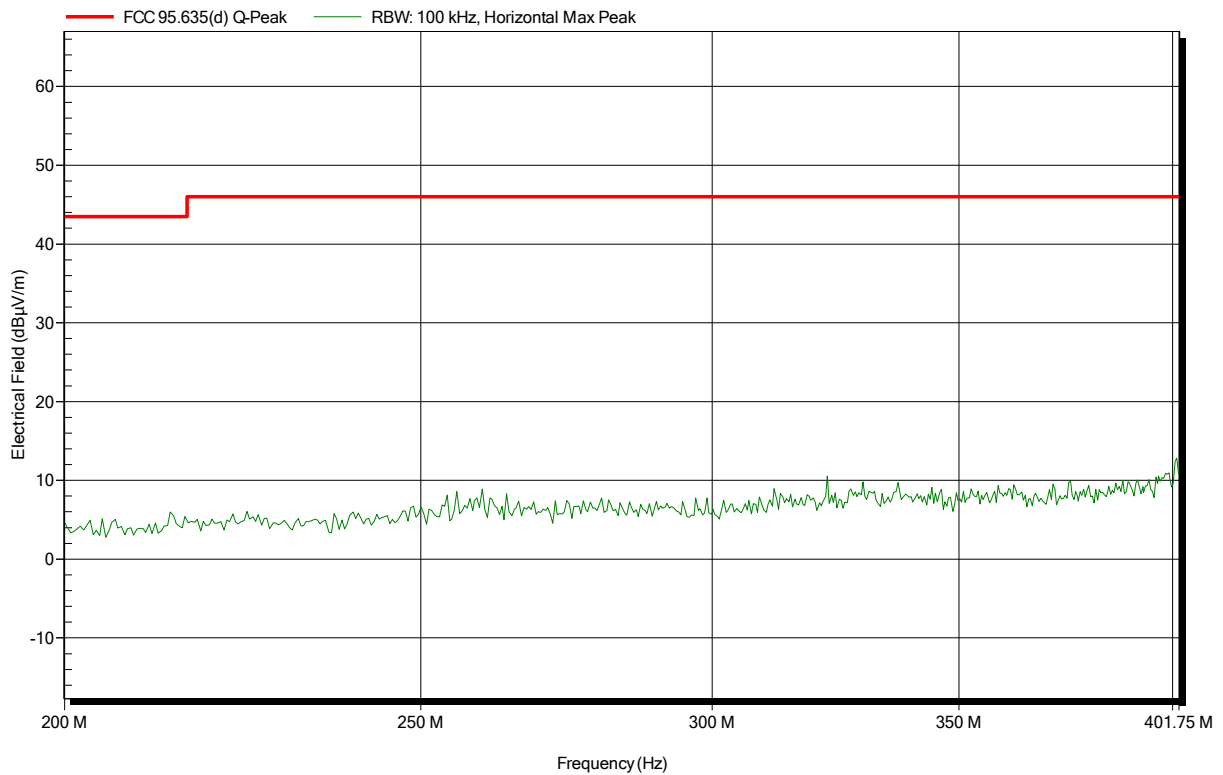


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Horizontal
Measurement distance:	3 m
Mode:	TX; 402.45 MHz
Test Date:	2016-02-23
Note:	Band-edge

Index 69

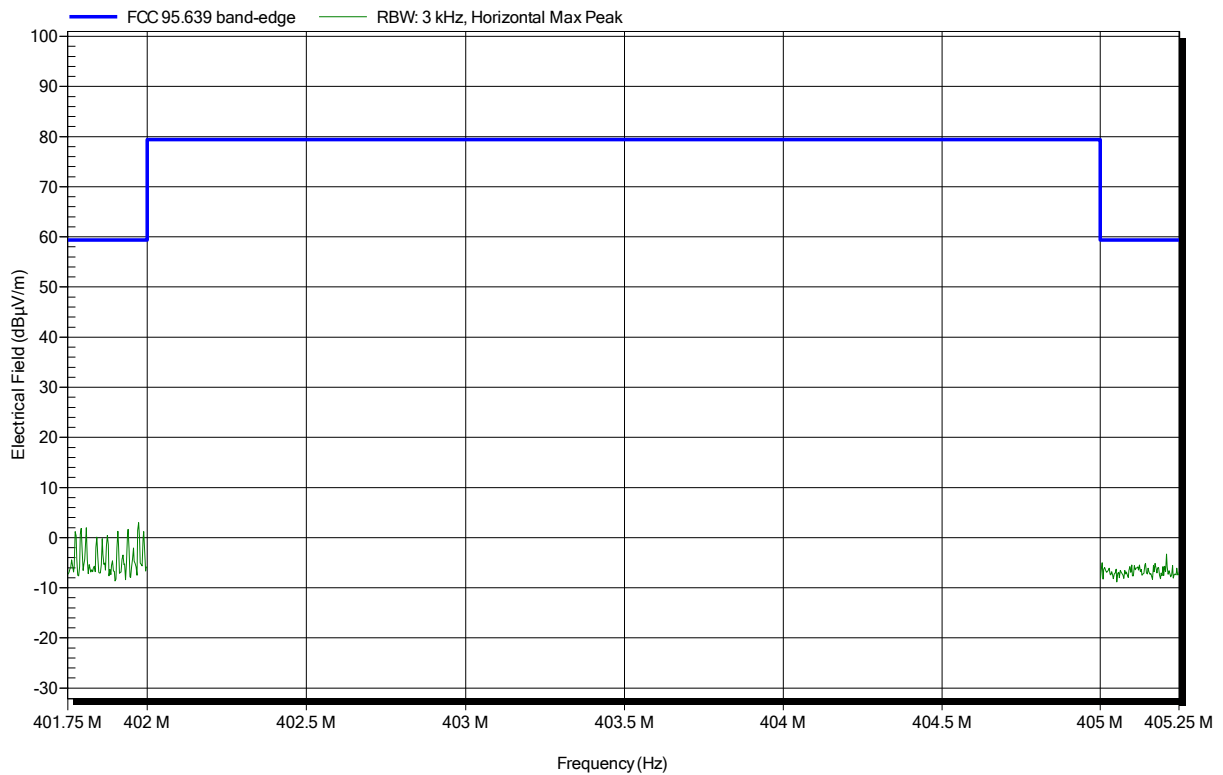


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz
 Test Date: 2016-02-23
 Note: Band-edge

Index 68

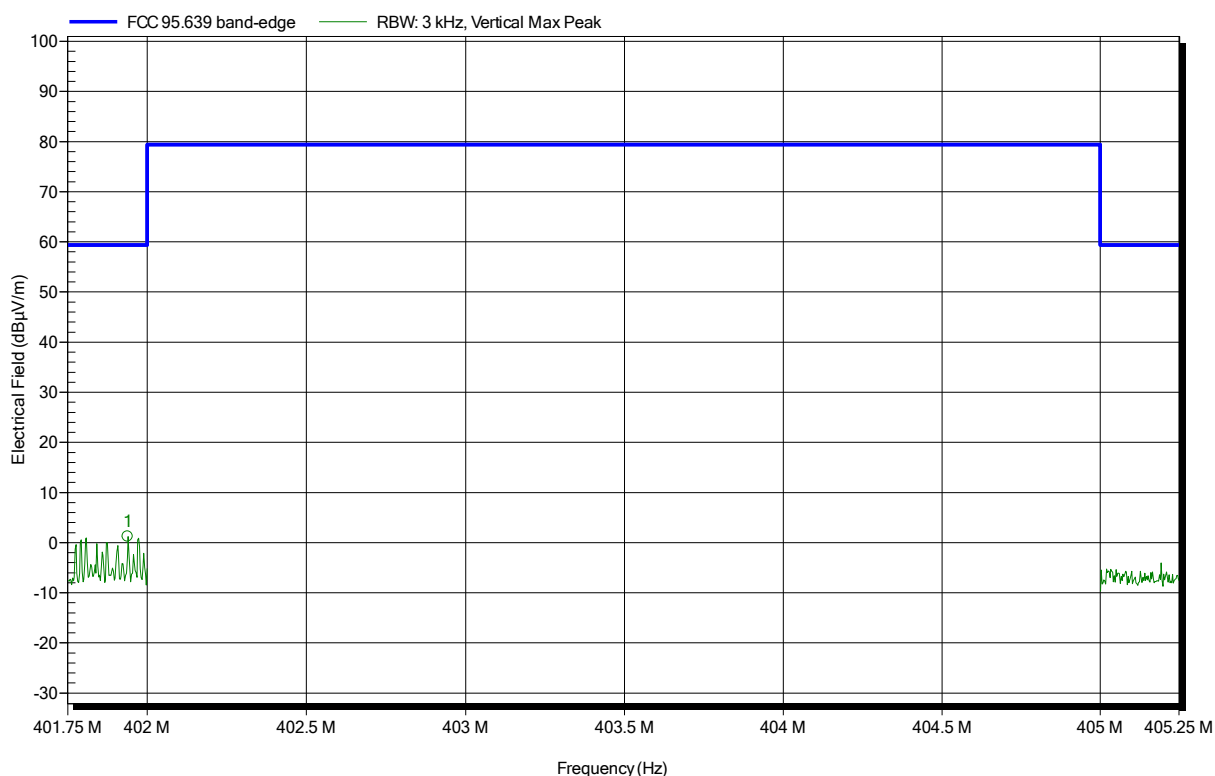


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
401.939 MHz	1.24 dBµV/m	59.4 dBµV/m	-58.16 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz
 Test Date: 2016-02-23
 Note: In-band emissions

Index 70

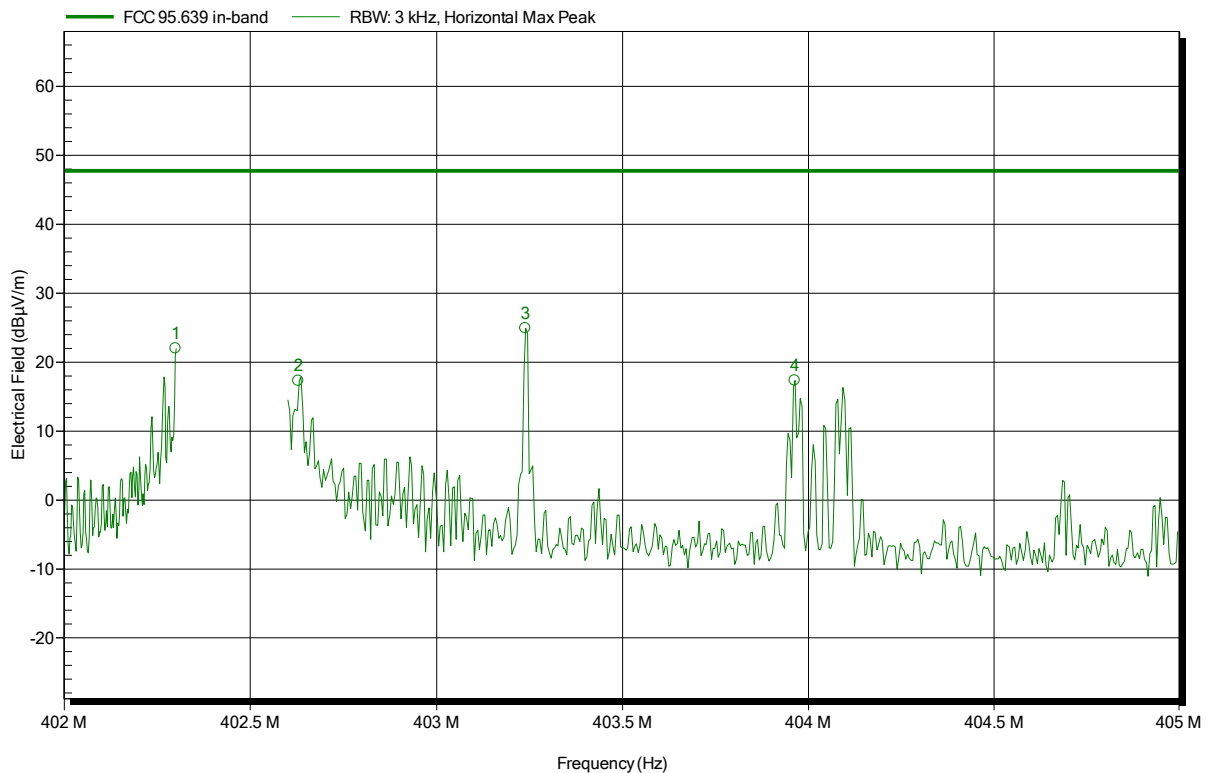


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
402.299 MHz	21.98 dBµV/m	47.8 dBµV/m	-25.82 dB	Pass
402.629 MHz	17.27 dBµV/m	47.8 dBµV/m	-30.53 dB	Pass
403.238 MHz	24.95 dBµV/m	47.8 dBµV/m	-22.85 dB	Pass
403.963 MHz	17.35 dBµV/m	47.8 dBµV/m	-30.45 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz
 Test Date: 2016-02-23
 Note: In-band emissions

Index 71

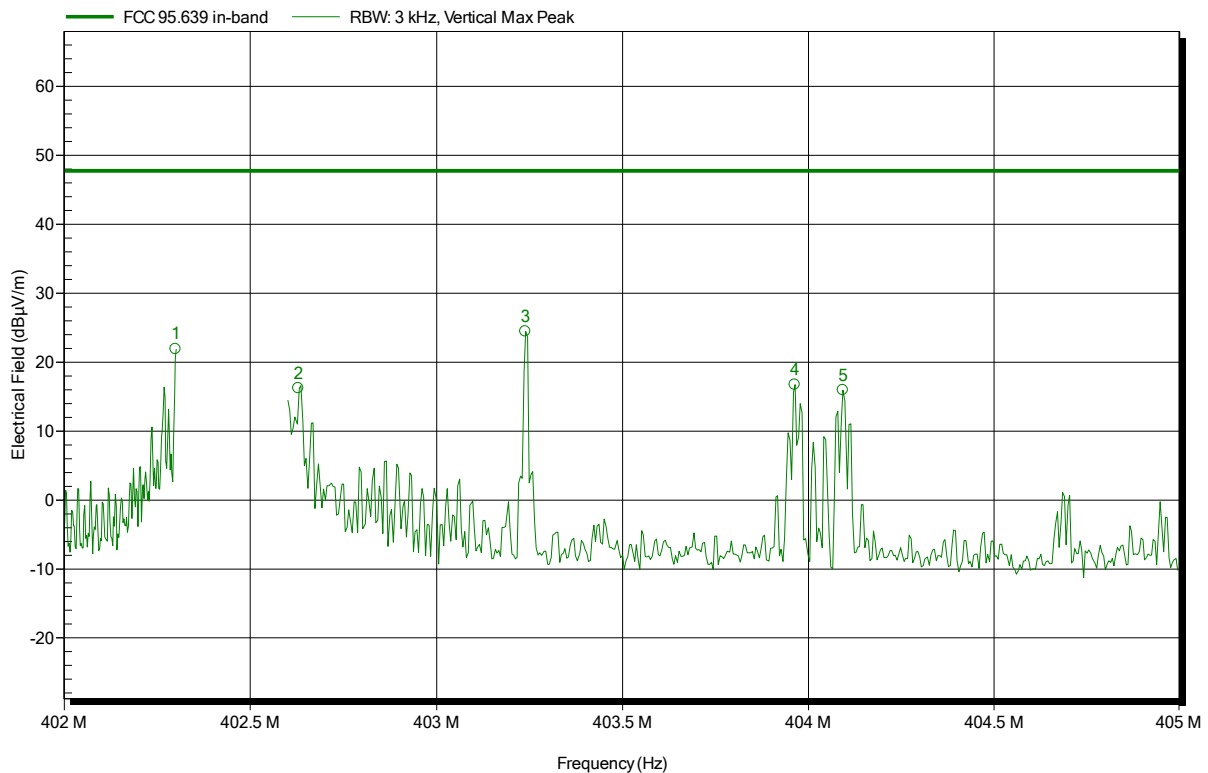


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
402.299 MHz	21.9 dBµV/m	47.8 dBµV/m	-25.9 dB	Pass
402.629 MHz	16.21 dBµV/m	47.8 dBµV/m	-31.59 dB	Pass
403.238 MHz	24.47 dBµV/m	47.8 dBµV/m	-23.33 dB	Pass
403.963 MHz	16.73 dBµV/m	47.8 dBµV/m	-31.07 dB	Pass
404.093 MHz	15.93 dBµV/m	47.8 dBµV/m	-31.87 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz
 Test Date: 2016-02-23
 Note:

Index 73

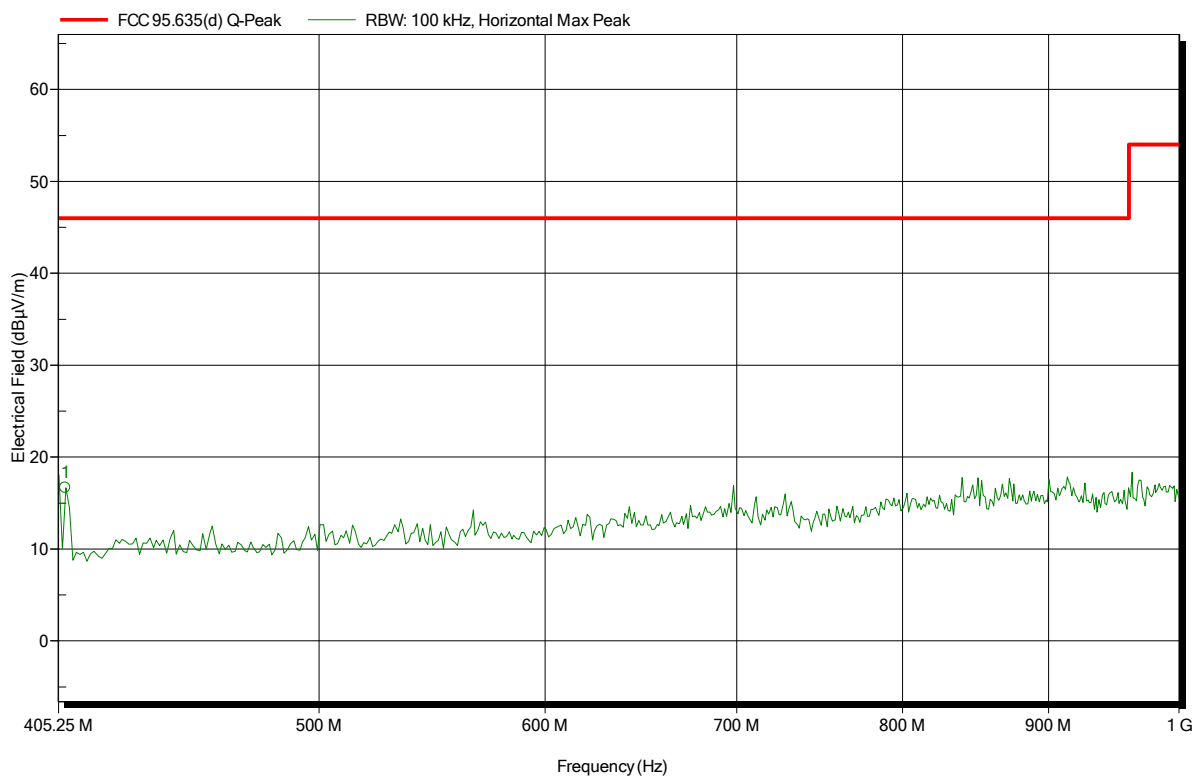


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
407.629 MHz	16.66 dBµV/m	46 dBµV/m	-29.34 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 402.45 MHz
 Test Date: 2016-02-23
 Note:

Index 72

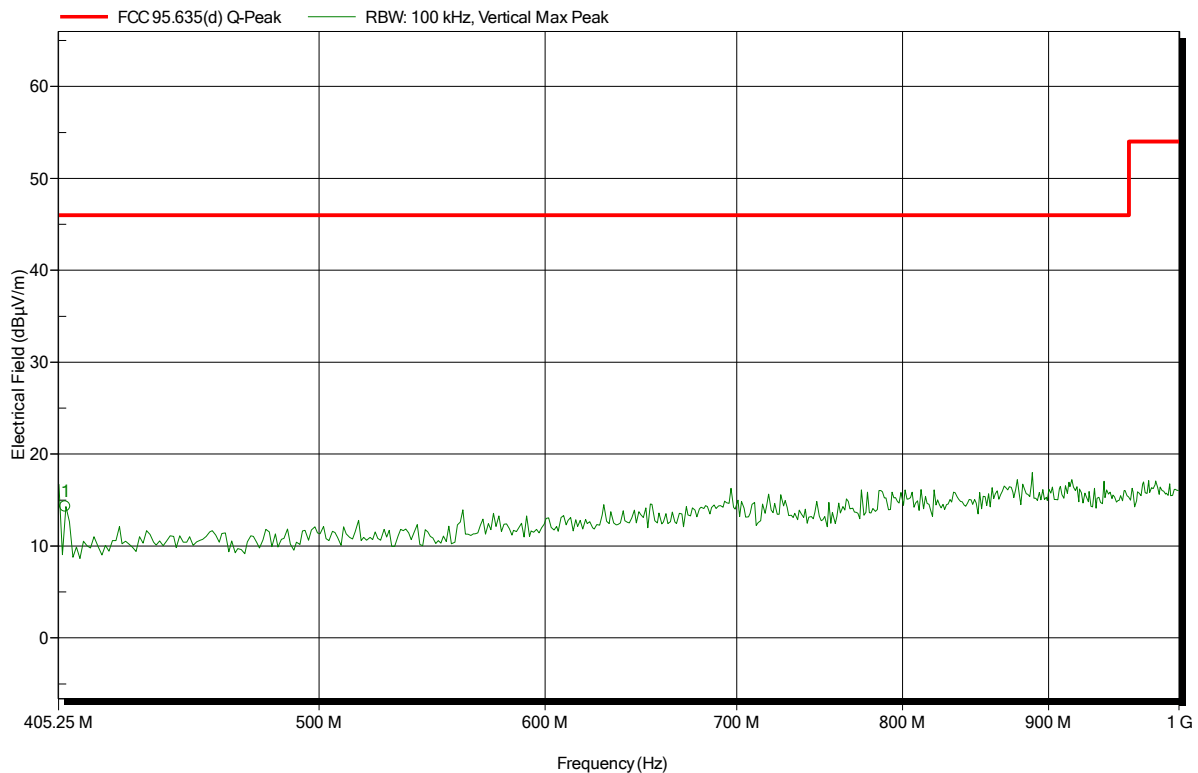


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
407.629 MHz	14.3 dBµV/m	46 dBµV/m	-31.7 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL025, Horizontal
Measurement distance:	3 m
Mode:	TX; 402.45 MHz
Test Date:	2016-02-23
Note:	

Index 61

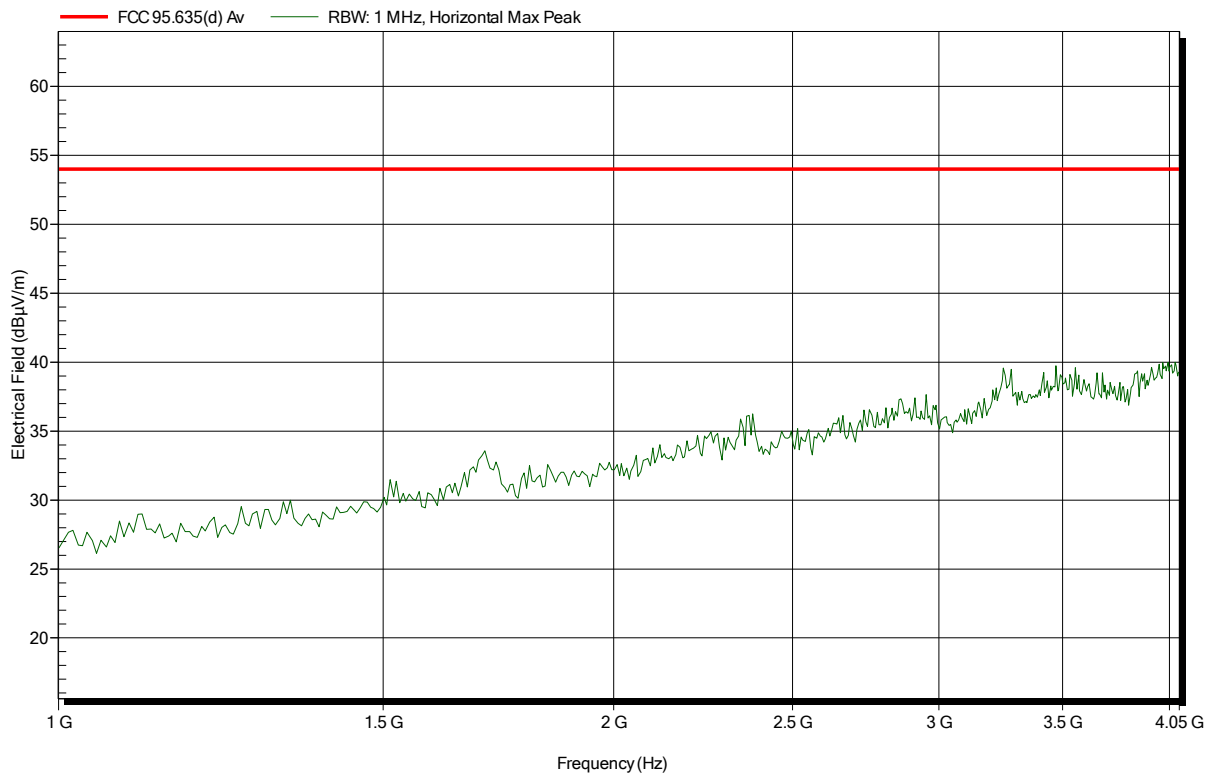


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL025, Vertical
Measurement distance:	3 m
Mode:	TX; 402.45 MHz
Test Date:	2016-02-23
Note:	

Index 62

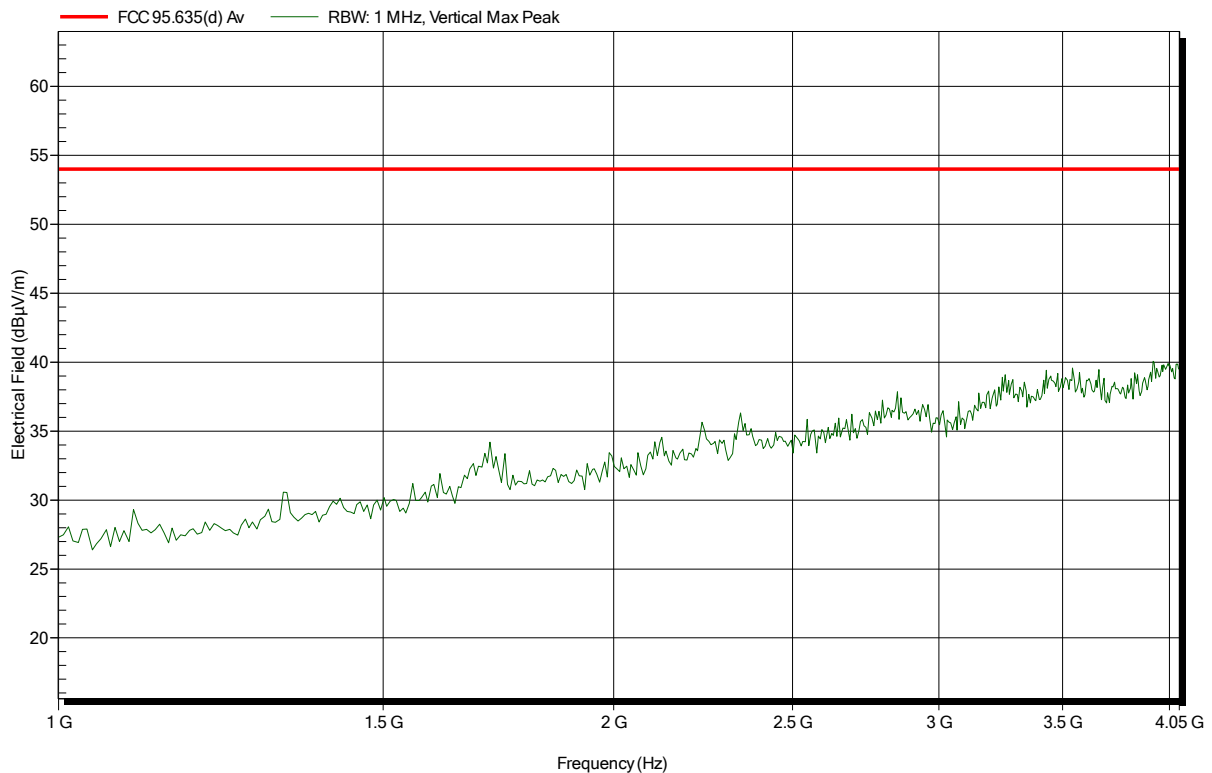


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HK116, Horizontal
Measurement distance:	3 m
Mode:	TX; 404.85 MHz
Test Date:	2016-02-24
Note:	

Index 84

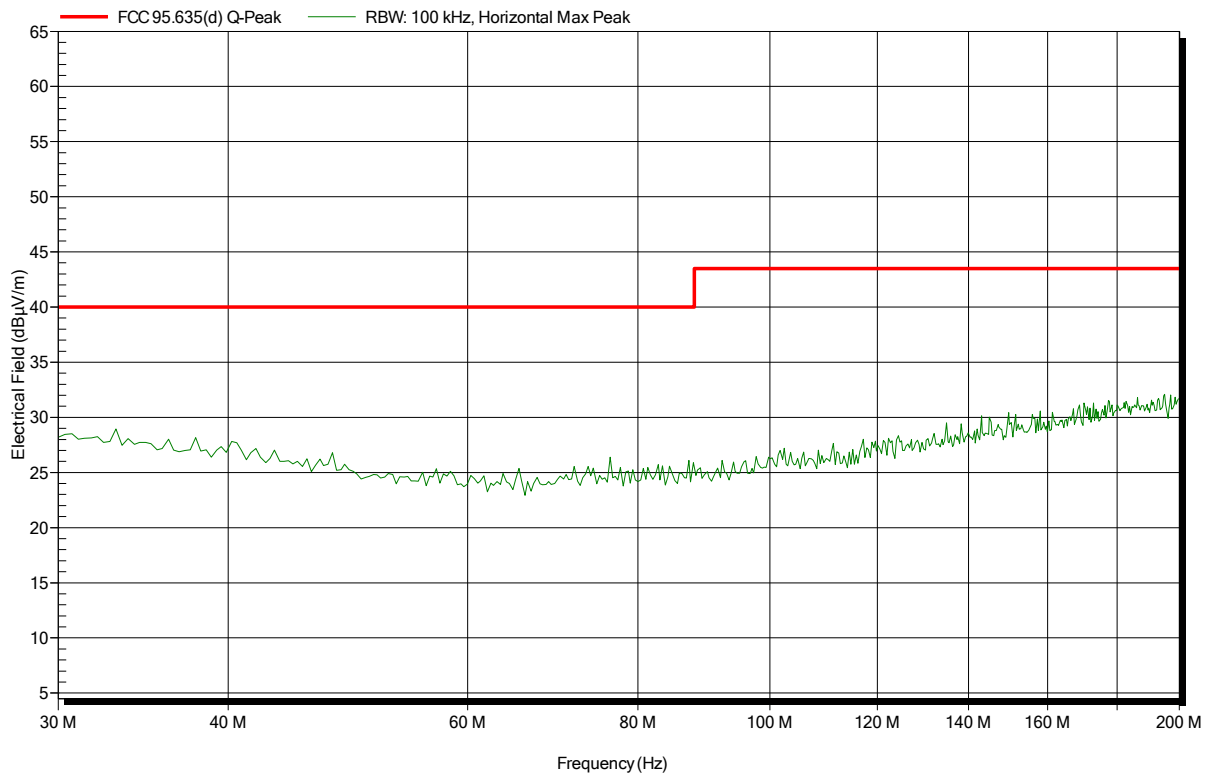


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HK116, Vertical
Measurement distance:	3 m
Mode:	TX; 404.85 MHz
Test Date:	2016-02-24
Note:	

Index 85

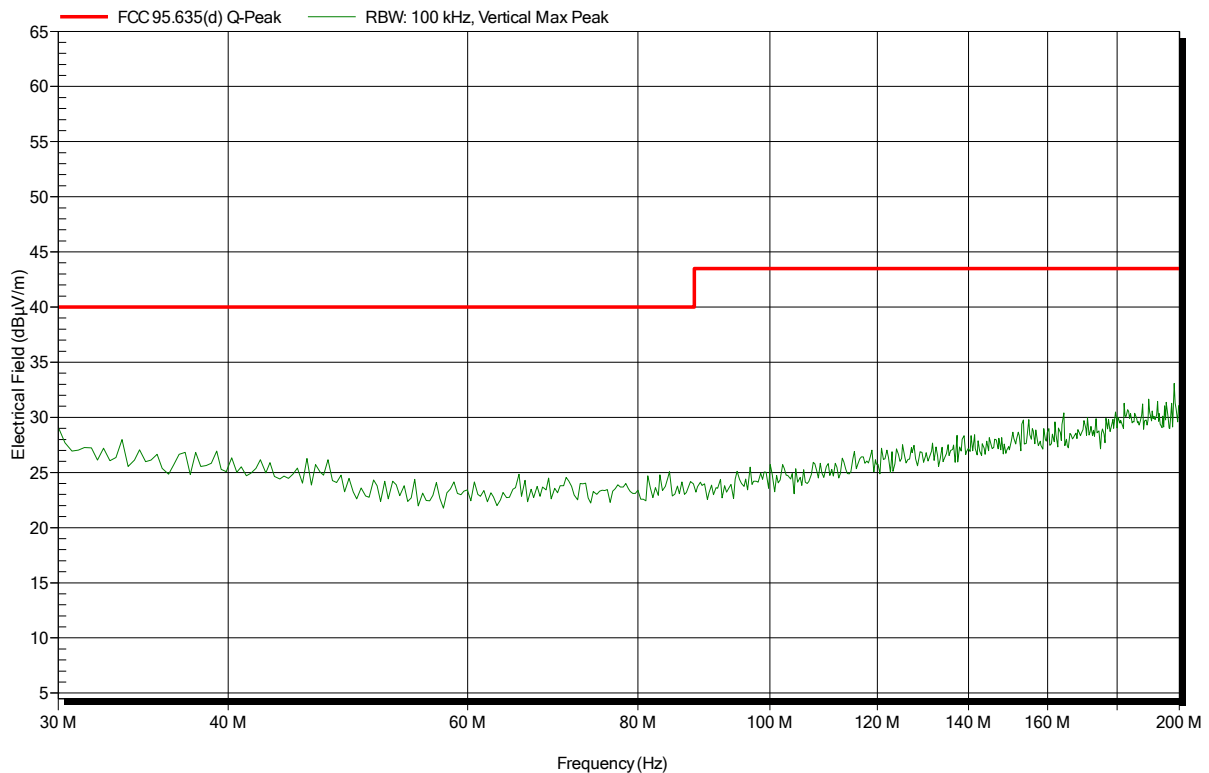


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz
 Test Date: 2016-02-23
 Note:

Index 74

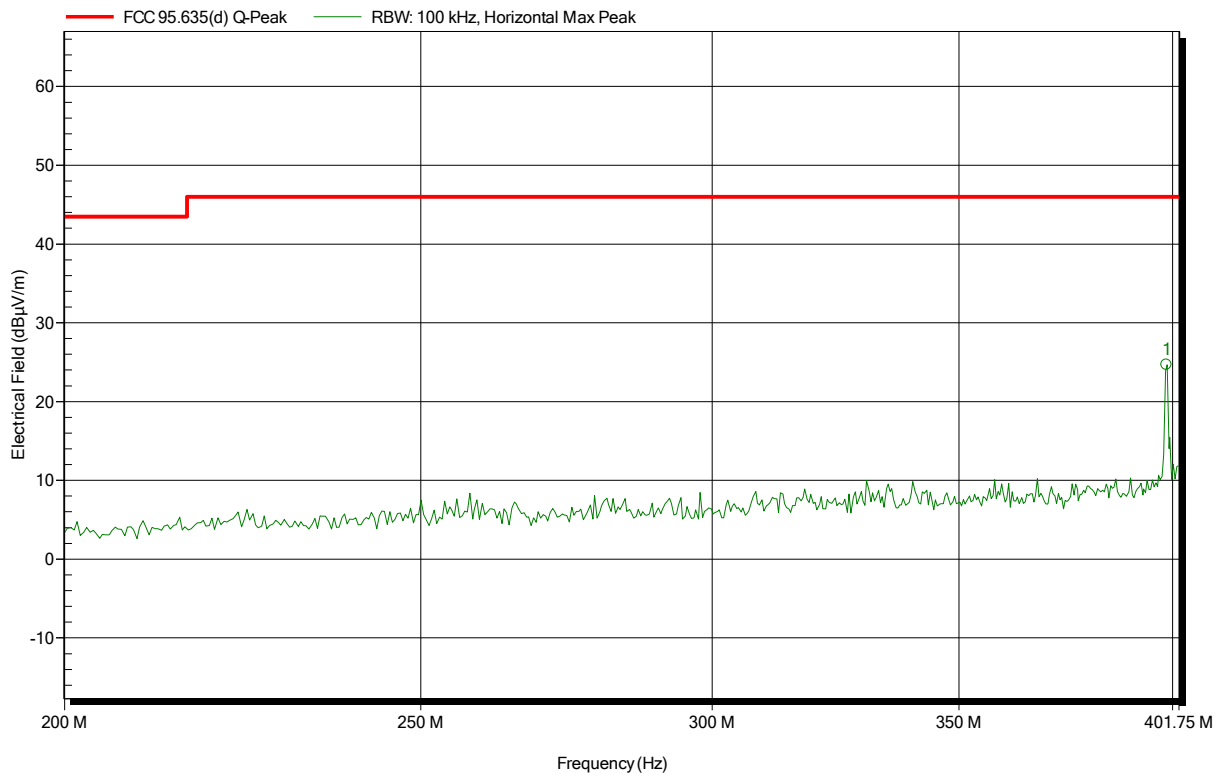


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
398.522 MHz	24.67 dBµV/m	46 dBµV/m	-21.33 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Vertical
Measurement distance:	3 m
Mode:	TX; 404.85 MHz
Test Date:	2016-02-23
Note:	

Index 75

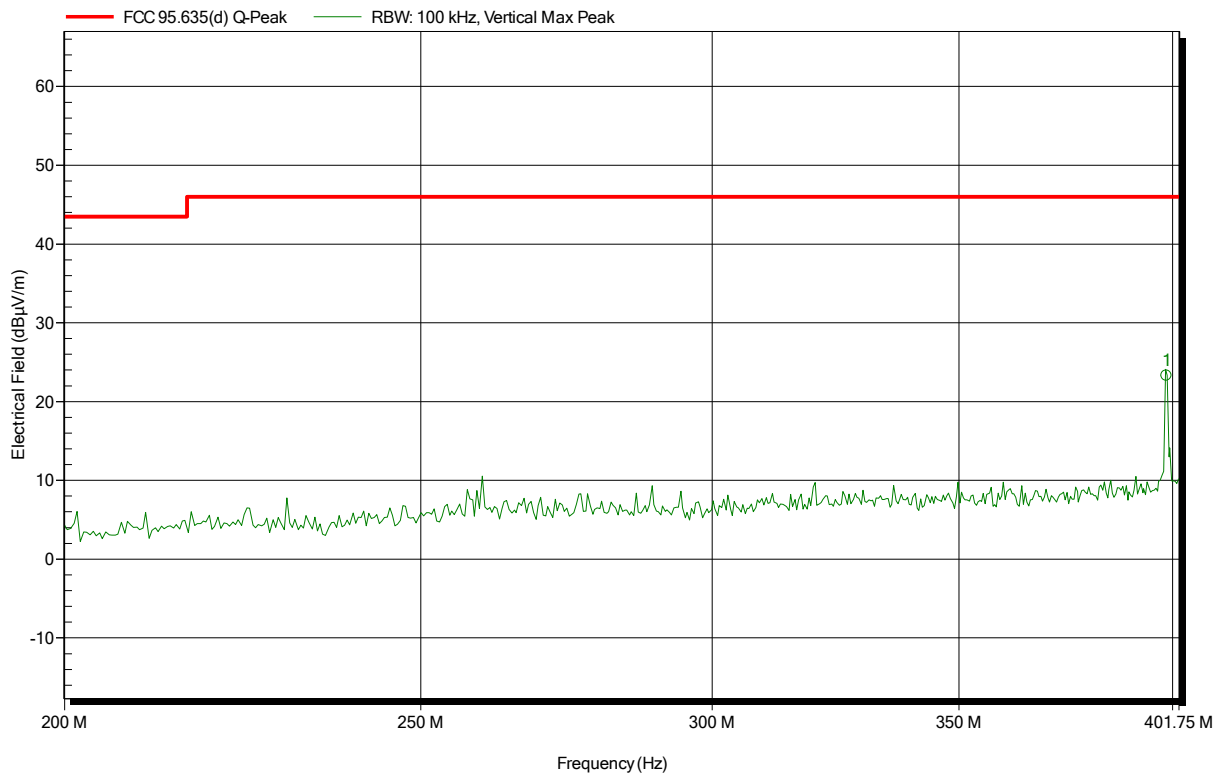


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
398.522 MHz	23.3 dBµV/m	46 dBµV/m	-22.7 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz
 Test Date: 2016-02-23
 Note: Band-edge

Index 77

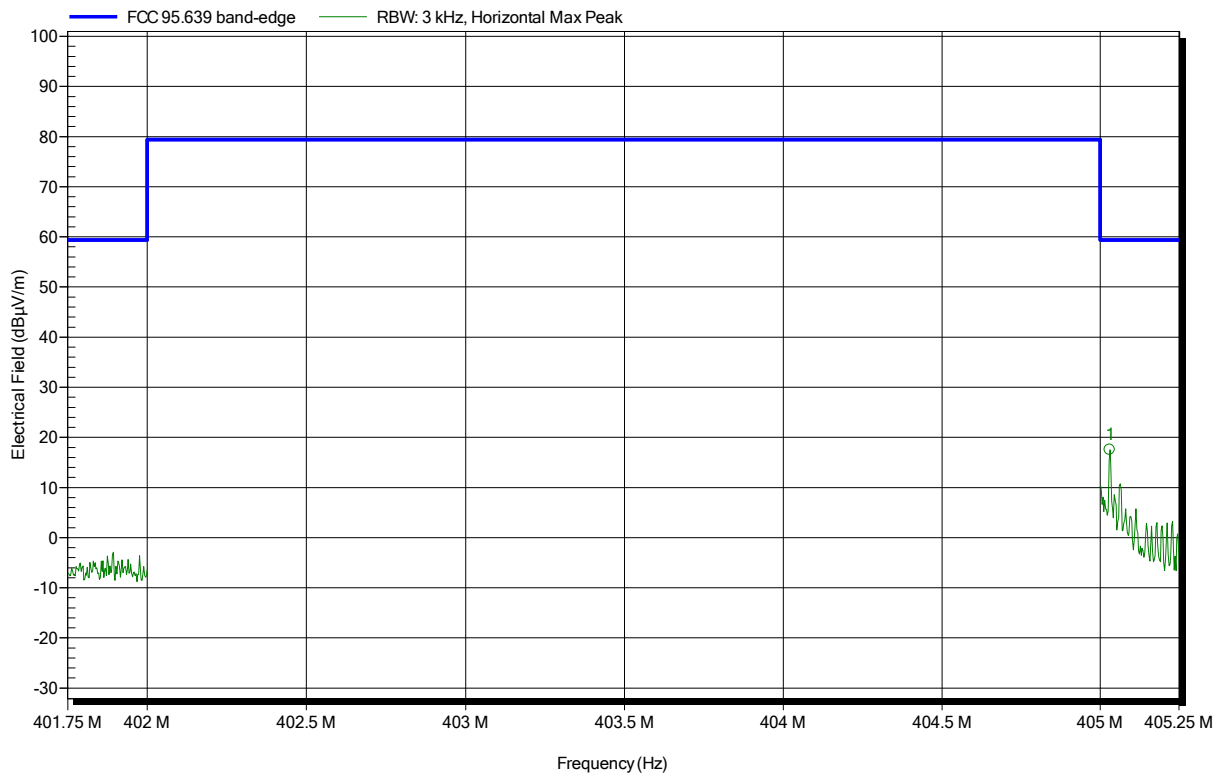


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
405.029 MHz	17.51 dBµV/m	59.4 dBµV/m	-41.89 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz
 Test Date: 2016-02-23
 Note: Band-edge

Index 76

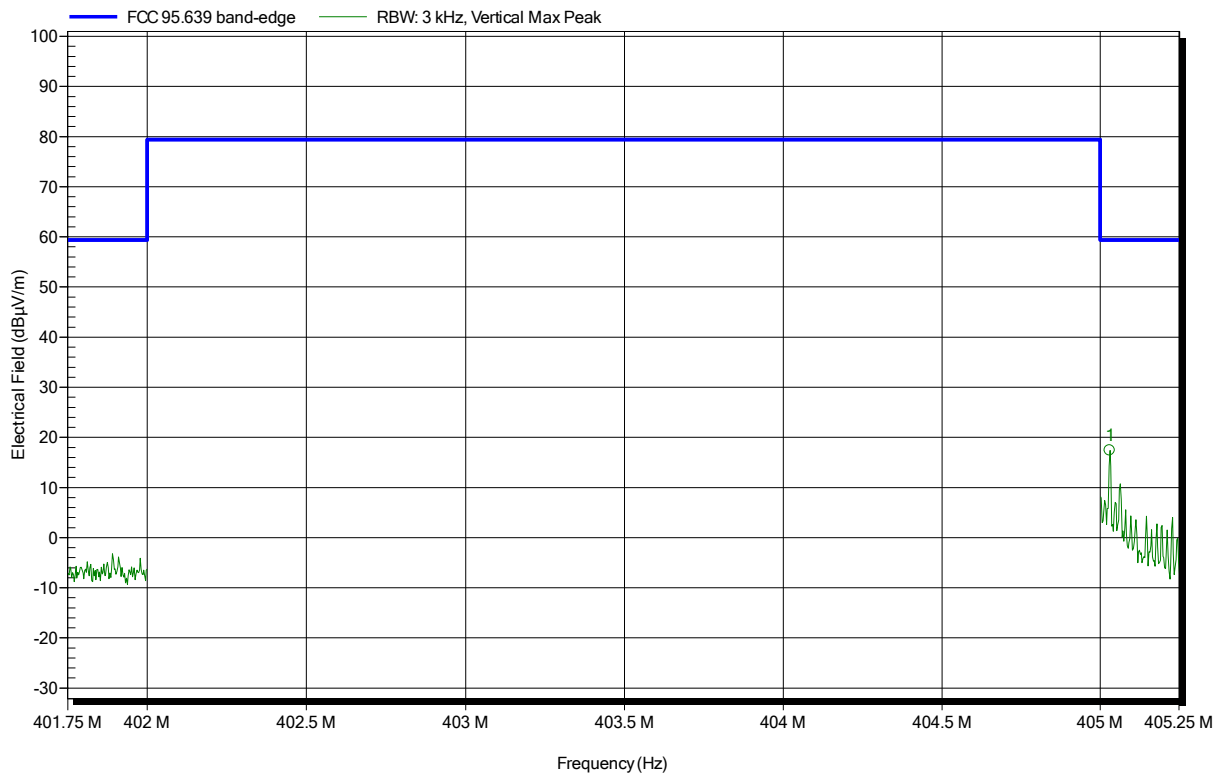


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
405.029 MHz	17.41 dBµV/m	59.4 dBµV/m	-41.99 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz
 Test Date: 2016-02-23
 Note: In-band emissions

Index 78

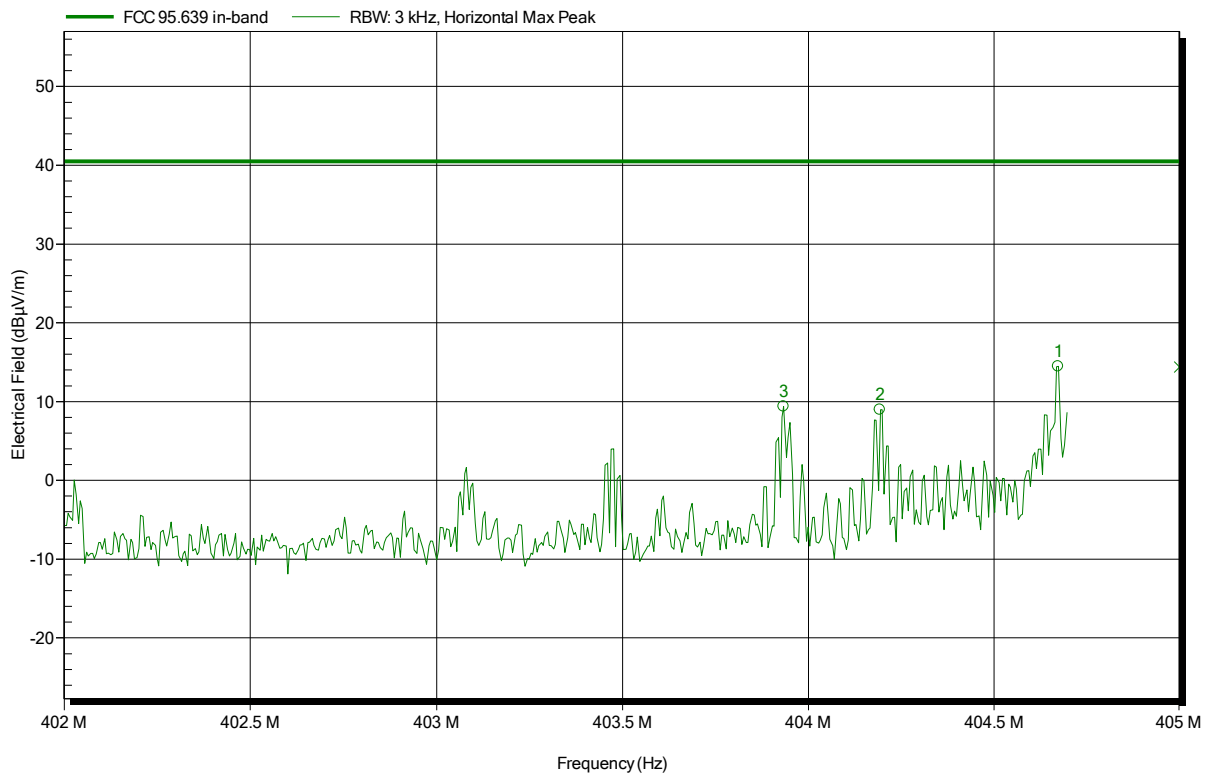


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
403.933 MHz	9.36 dBµV/m	40.5 dBµV/m	-31.14 dB	Pass
404.192 MHz	8.97 dBµV/m	40.5 dBµV/m	-31.53 dB	Pass
404.673 MHz	14.45 dBµV/m	40.5 dBµV/m	-26.05 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz
 Test Date: 2016-02-23
 Note: In-band emissions

Index 79

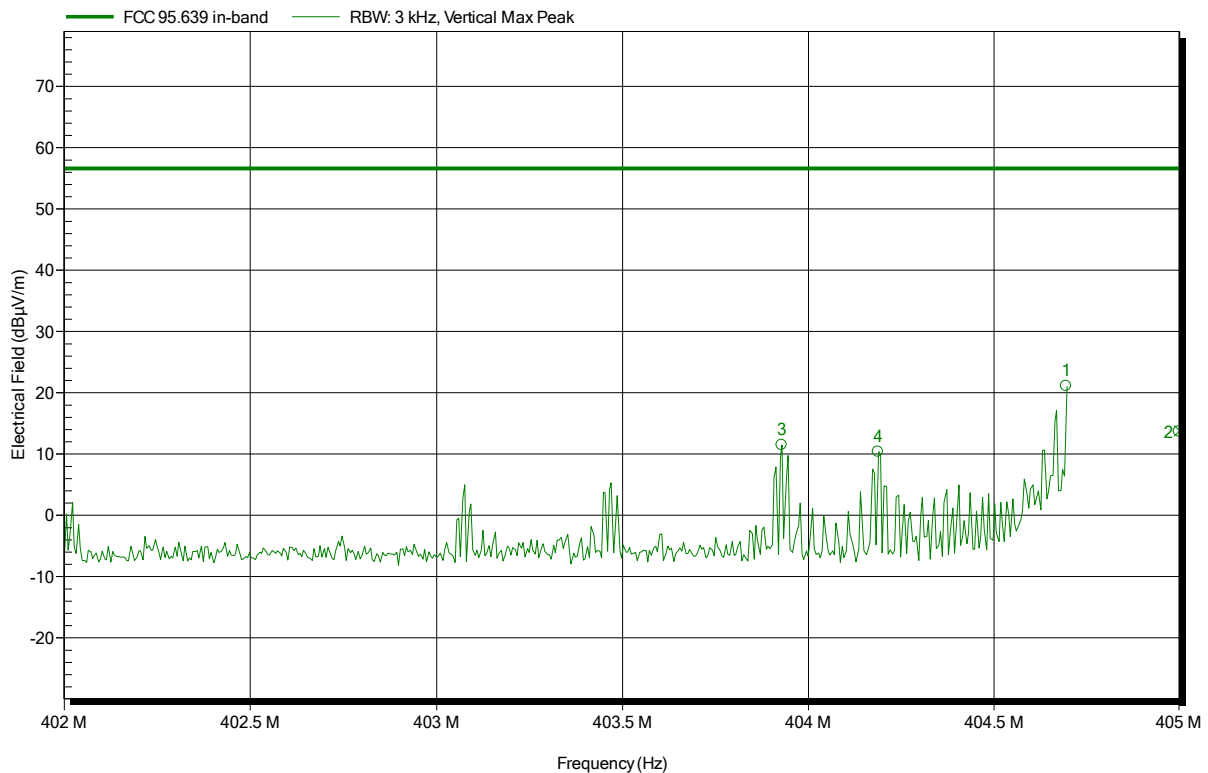


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
403.928 MHz	11.5 dBµV/m	56.6 dBµV/m	-45.1 dB	Pass
404.187 MHz	10.4 dBµV/m	56.6 dBµV/m	-46.2 dB	Pass
404.695 MHz	21.14 dBµV/m	56.6 dBµV/m	-35.46 dB	Pass
404.999 MHz	13.69 dBµV/m	56.6 dBµV/m	-42.91 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Horizontal
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz
 Test Date: 2016-02-23
 Note:

Index 81

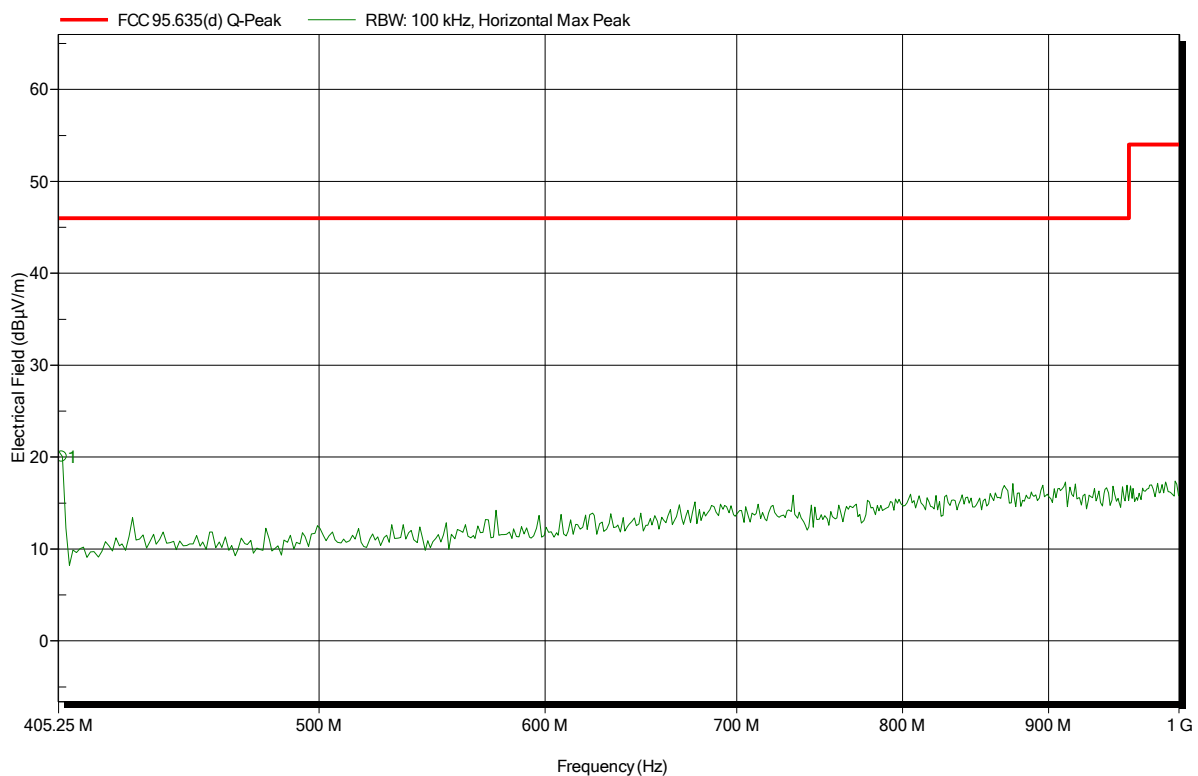


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
406.44 MHz	20.04 dBµV/m	46 dBµV/m	-25.96 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: TX; 404.85 MHz
 Test Date: 2016-02-23
 Note:

Index 80

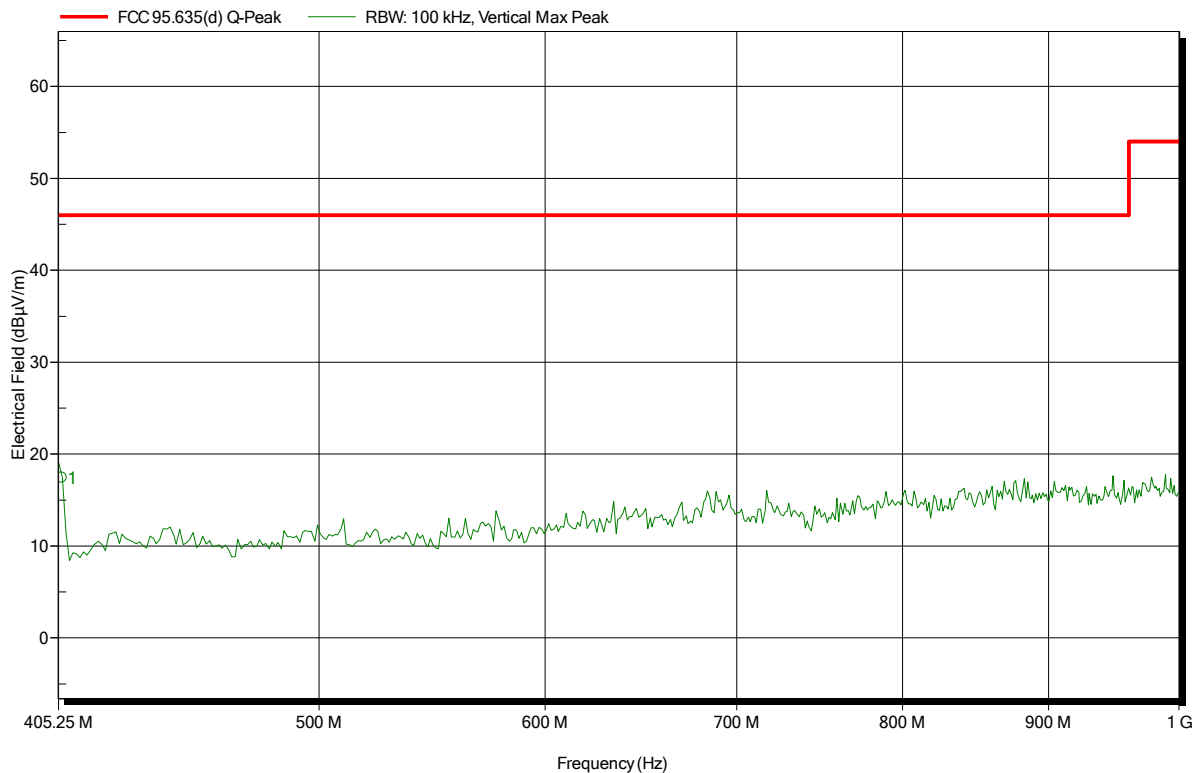


Frequency	Peak	Peak Limit	Peak Difference	Peak Status
406.44 MHz	17.44 dBµV/m	46 dBµV/m	-28.56 dB	Pass

Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL025, Horizontal
Measurement distance:	3 m
Mode:	TX; 404.85 MHz
Test Date:	2016-02-24
Note:	

Index 87

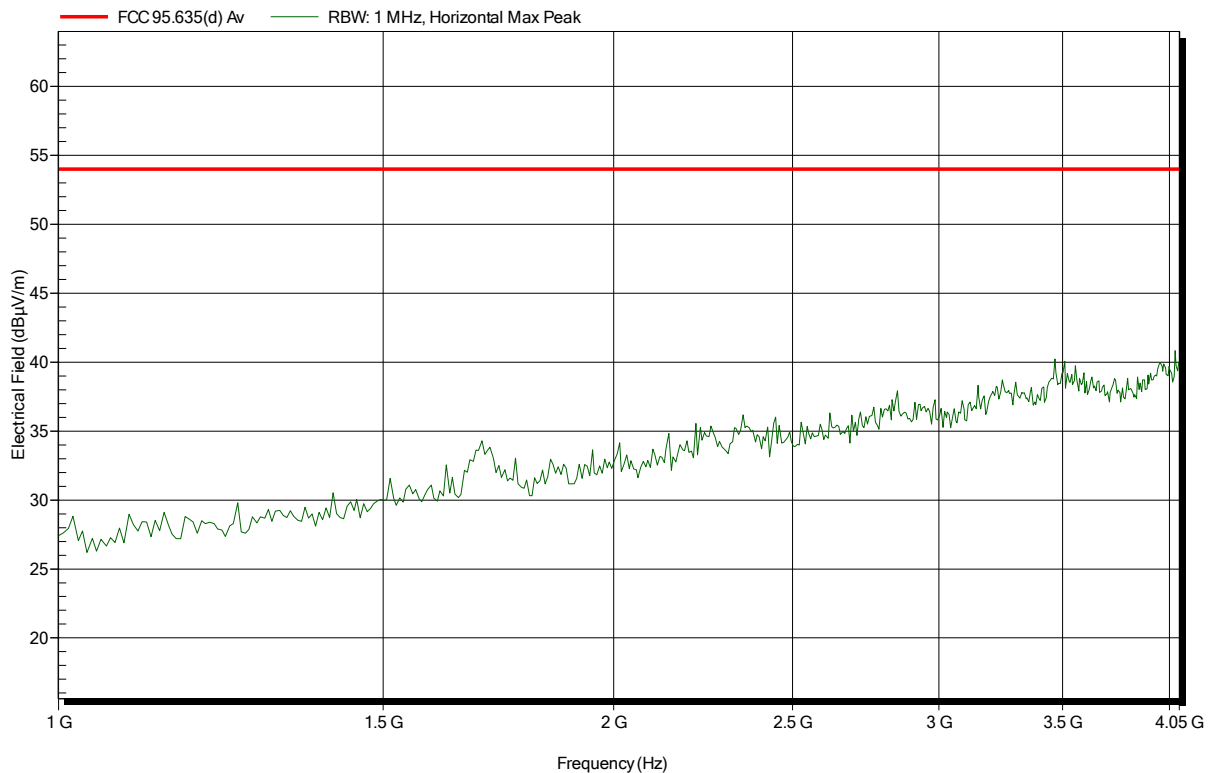


Spurious emissions according to FCC Part 95; Subpart E

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL025, Vertical
Measurement distance:	3 m
Mode:	TX; 404.85 MHz
Test Date:	2016-02-24
Note:	

Index 86

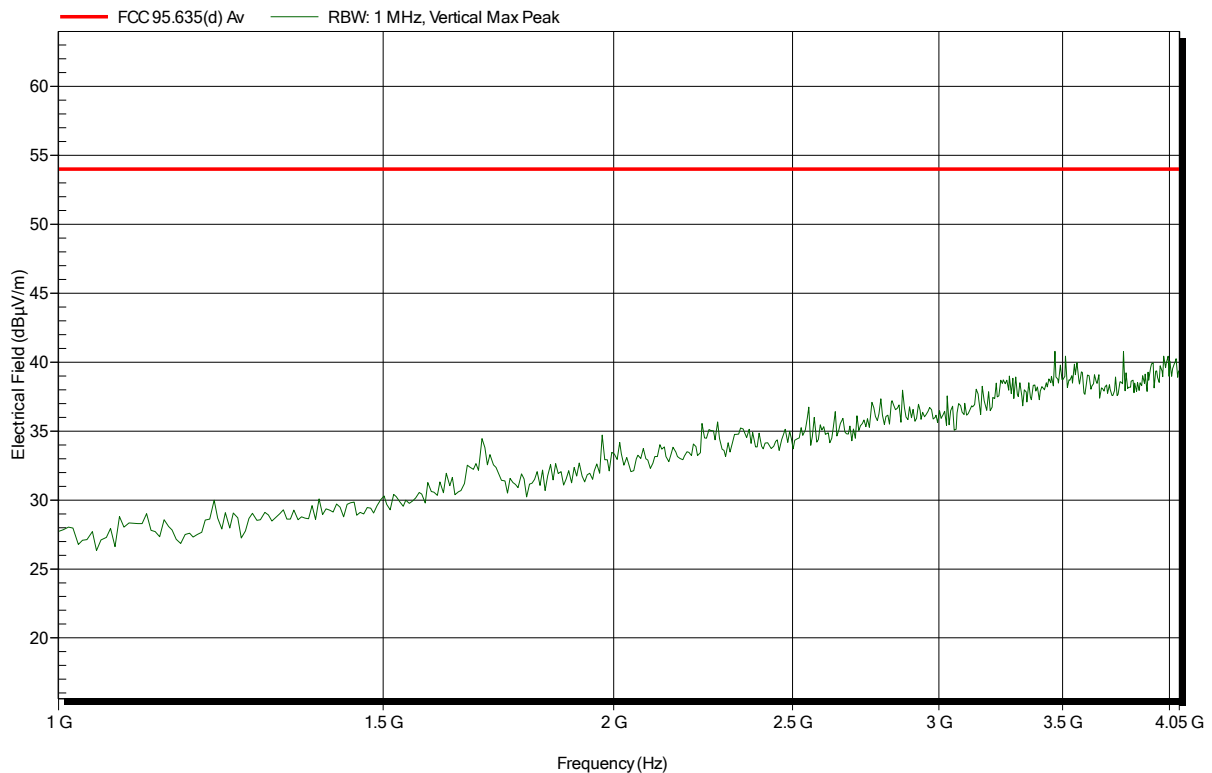


ANNEX C Receiver radiated spurious emissions

Spurious emissions according to RSS-Gen

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HK116, Horizontal
 Measurement distance: 3 m
 Mode: RX; 403.65 MHz
 Test Date: 2016-02-22
 Note:

Index 52

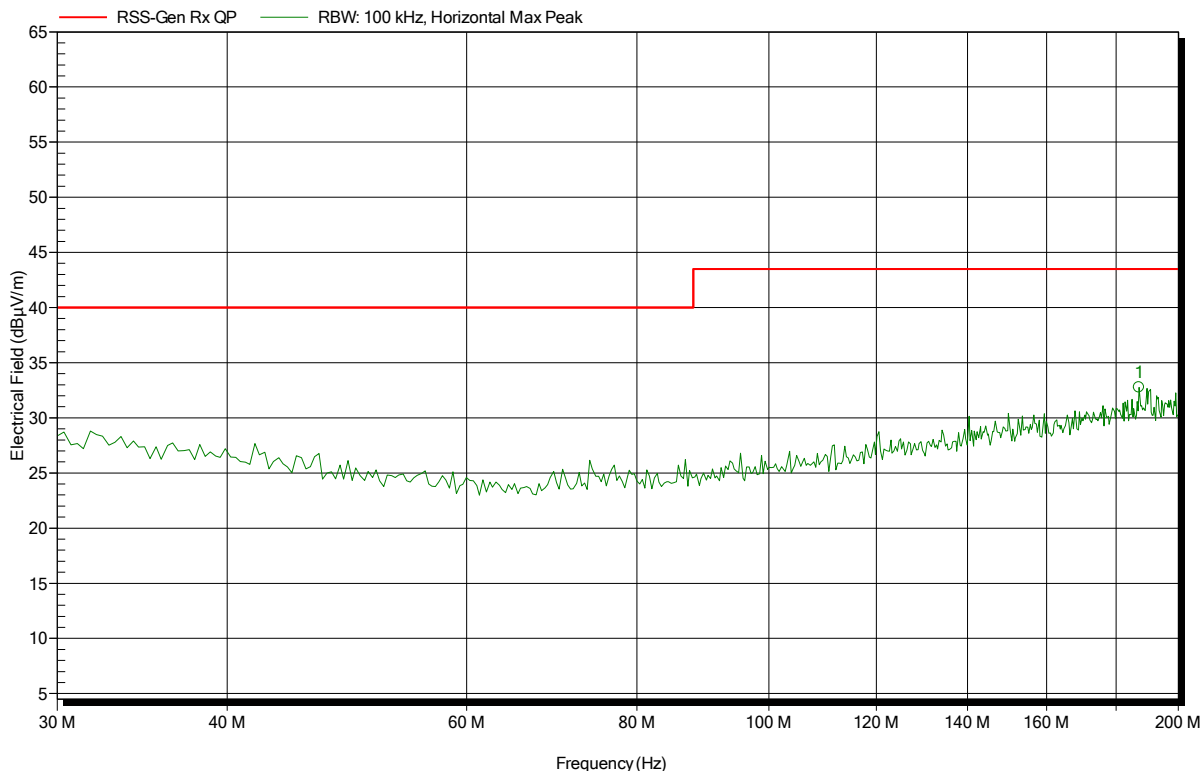


Frequency	Peak	Peak Limit	Peak Difference	Status
187.08 MHz	32.76 dBµV/m	43.5 dBµV/m	-10.74 dB	Pass

Spurious emissions according to RSS-Gen

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HK116, Vertical
 Measurement distance: 3 m
 Mode: RX; 403.65 MHz
 Test Date: 2016-02-22
 Note:

Index 51

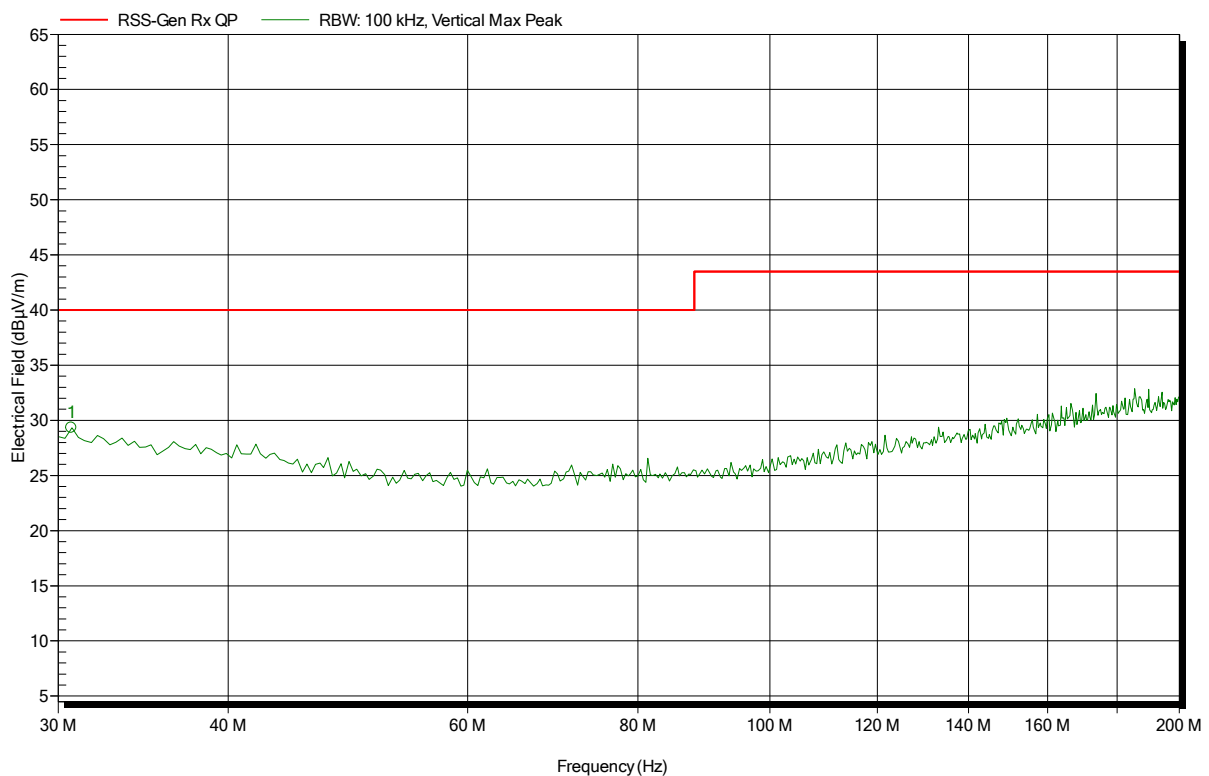


Frequency	Peak	Peak Limit	Peak Difference	Status
30.68 MHz	29.32 dBµV/m	40 dBµV/m	-10.68 dB	Pass

Spurious emissions according to RSS-Gen

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL223, Horizontal
Measurement distance:	3 m
Mode:	RX; 403.65 MHz
Test Date:	2016-02-22
Note:	

Index 53

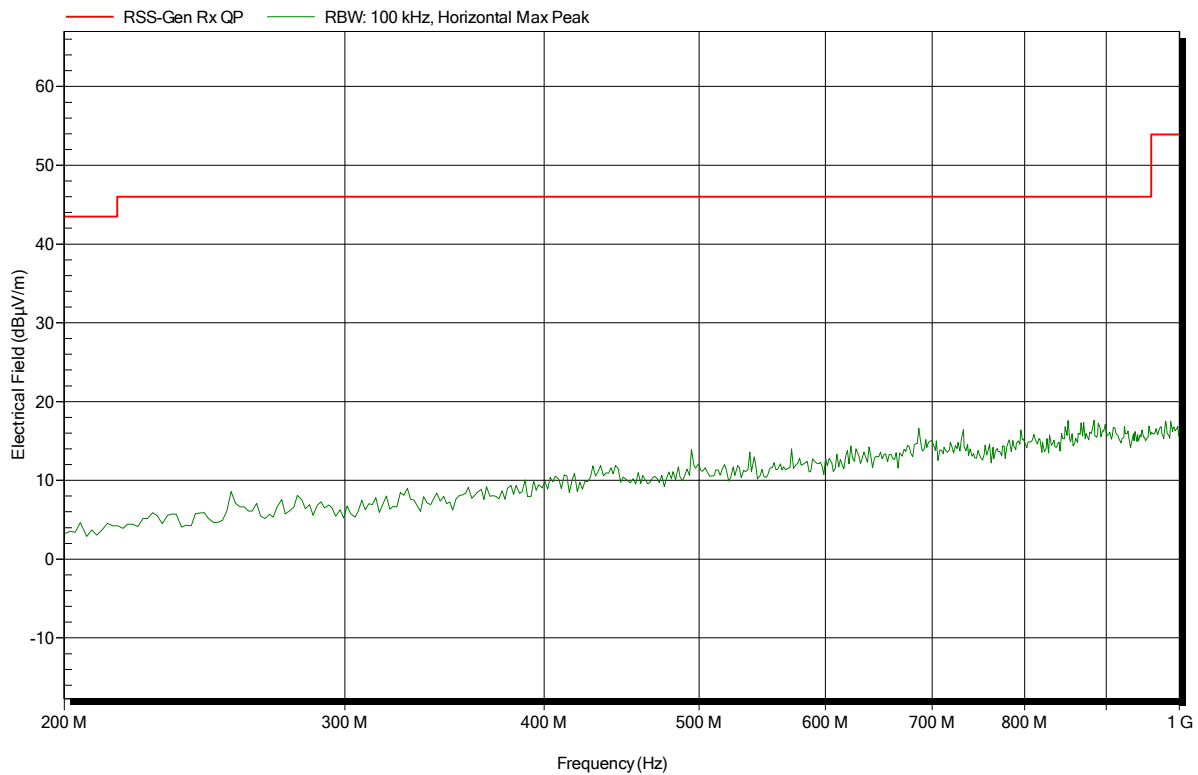


Spurious emissions according to RSS-Gen

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL223, Vertical
 Measurement distance: 3 m
 Mode: RX; 403.65 MHz
 Test Date: 2016-02-22
 Note:

Index 54

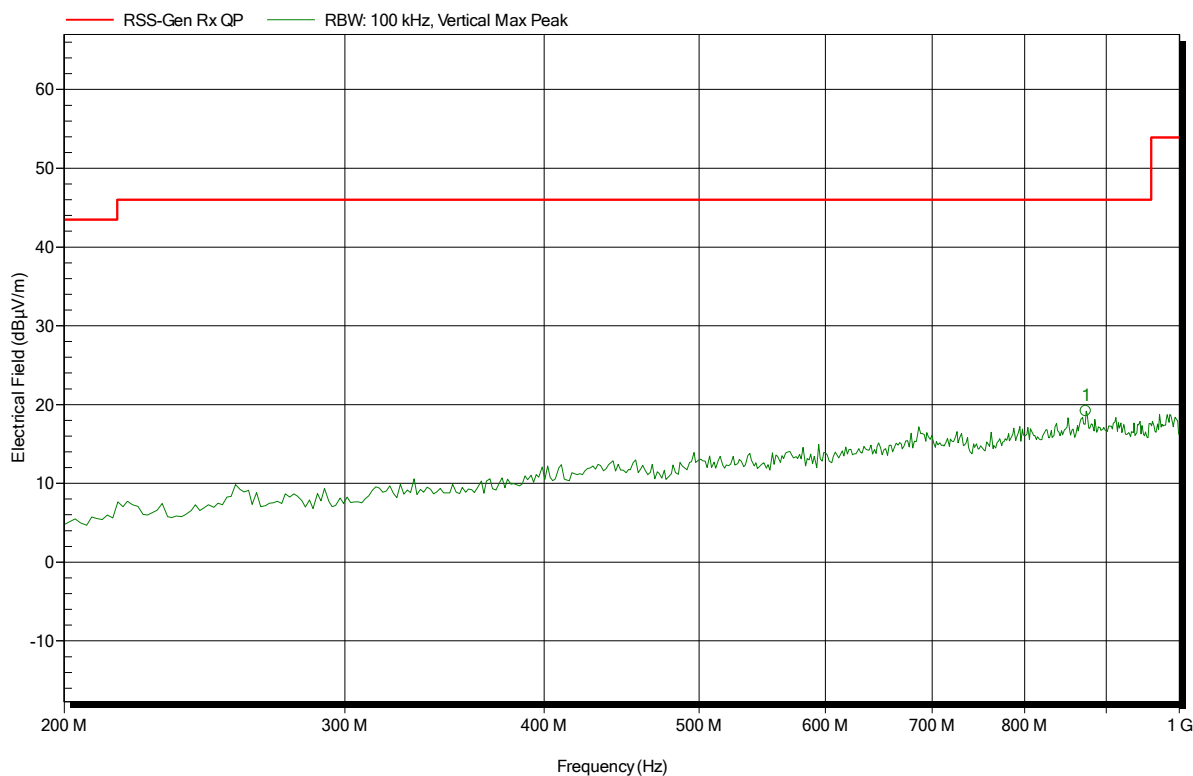


Frequency	Peak	Peak Limit	Peak Difference	Status
873.6 MHz	19.18 dBµV/m	46 dBµV/m	-26.82 dB	Pass

Spurious emissions according to RSS-Gen

Project number: G0M-1507-4972

Applicant: Biotronik SE & Co. KG
 EUT Name: Primus Nano Plus Pacemaker Family
 Model: Edora 8 HF-T ProMRI
 Test Site: Eurofins Product Service GmbH
 Operator: Treffke
 Test Conditions: Tnom: 23°C, Vnom: 3.0 V DC battery
 Antenna: HL025, Horizontal
 Measurement distance: 3 m
 Mode: RX; 403.65 MHz
 Test Date: 2016-02-22
 Note:

Index 55

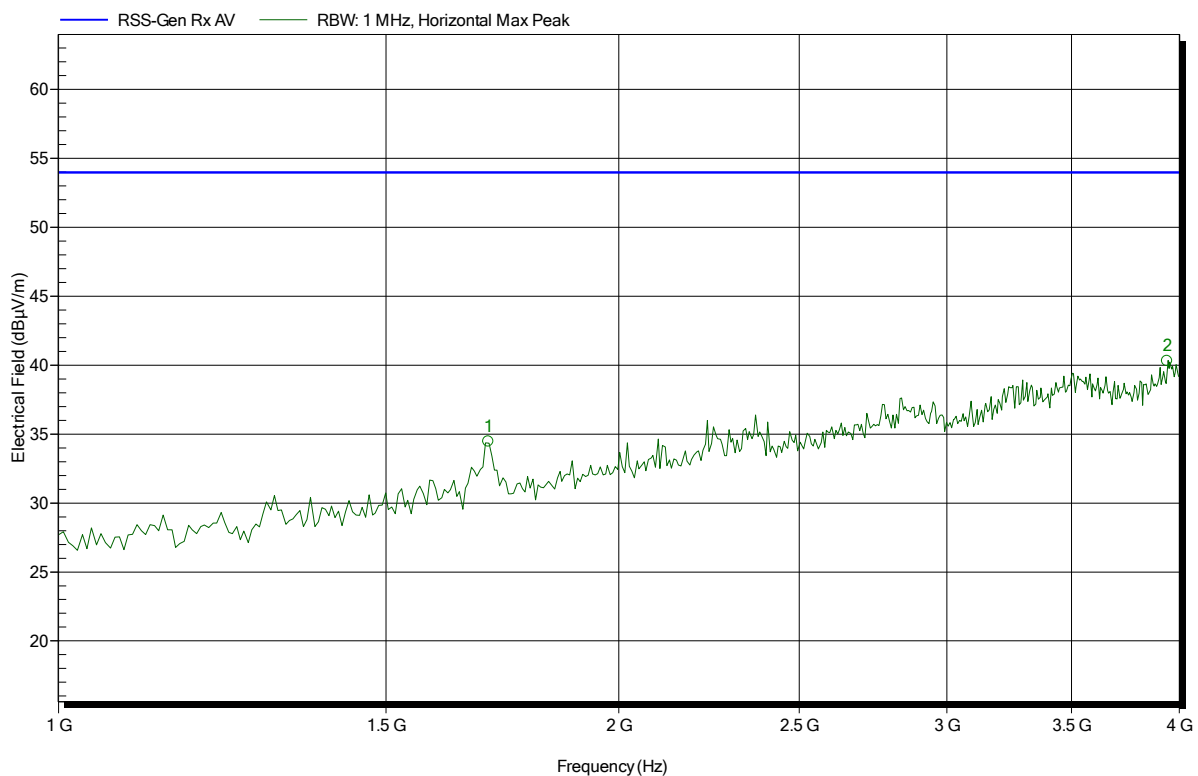


Frequency	Peak	Peak Limit	Peak Difference	Status
1.702 GHz	34.45 dBµV/m	53.98 dBµV/m	-19.53 dB	Pass
3.94 GHz	40.29 dBµV/m	53.98 dBµV/m	-13.69 dB	Pass

Spurious emissions according to RSS-Gen

Project number: G0M-1507-4972

Applicant:	Biotronik SE & Co. KG
EUT Name:	Primus Nano Plus Pacemaker Family
Model:	Edora 8 HF-T ProMRI
Test Site:	Eurofins Product Service GmbH
Operator:	Treffke
Test Conditions:	Tnom: 23°C, Vnom: 3.0 V DC battery
Antenna:	HL025, Vertical
Measurement distance:	3 m
Mode:	RX; 403.65 MHz
Test Date:	2016-02-22
Note:	

Index 56

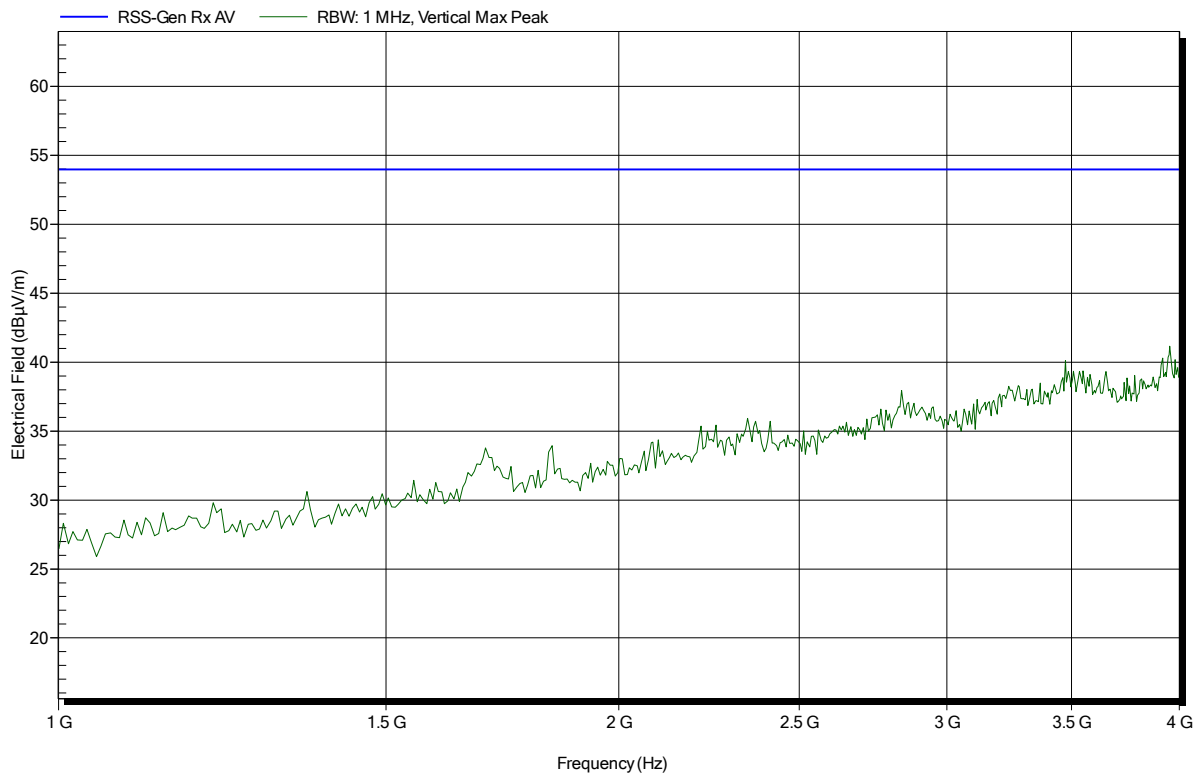



ANNEX D Evaluation measurements for sample selection
Antenna Pattern

Project Number: G0M-1507-4972
 Product: Primus Nano Plus Pacemaker Family
 Model: DR-T
 EUT Position: vertical, without leads
 EUT Antenna: integral
 Operating Conditions: Tnom / Vnom
 Operating Frequency: 403.65 MHz
 Detector: Peak
 RBW: 1 MHz
 VBW: 3 MHz
 Sweep Time: 100 ms
 Conducted Power: -6.5 dBm
 Operator: Mr. Treffke
 Date: 2016-02-22

Result Summary

Antenna Polarization	Turn table Angle [°]	Max. rad. power [dBm e.i.r.p.]	Max. antenna gain [dBi]
Vertical	148	-35.83	-29.33
Horizontal	160	-40.03	-33.53

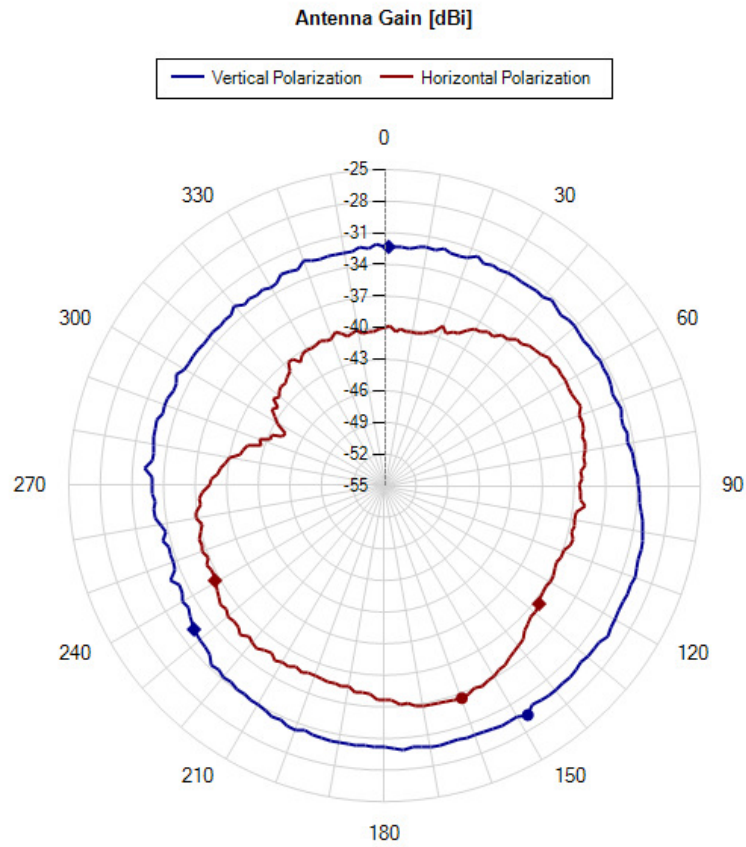

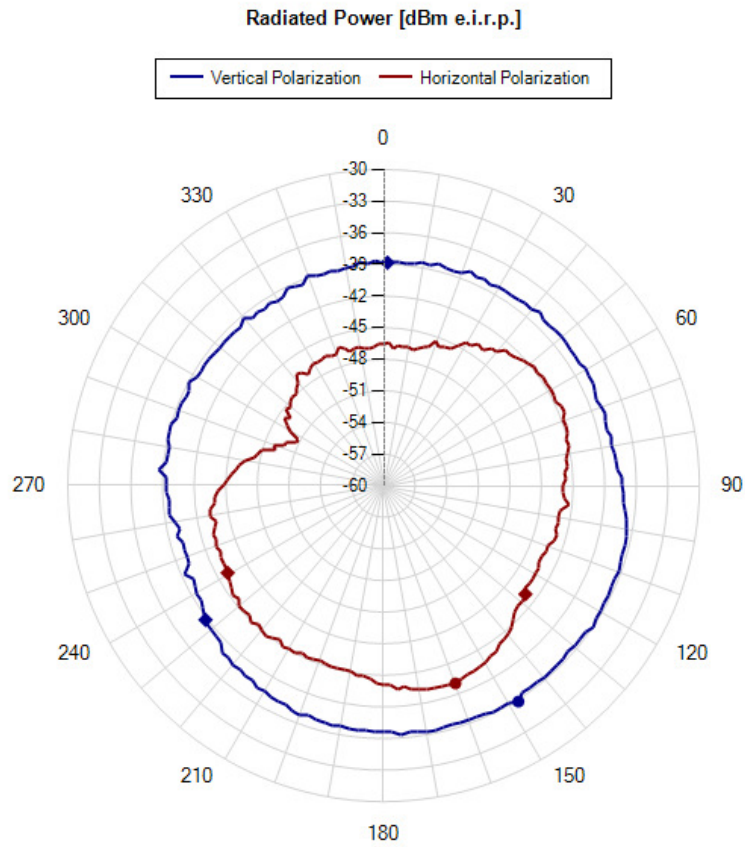



Antenna Pattern

Project Number: G0M-1507-4972
 Product: Primus Nano Plus Pacemaker Family
 Model: HF-T QP
 EUT Position: vertical, without leads
 EUT Antenna: integral
 Operating Conditions: Tnom / Vnom
 Operating Frequency: 403.65 MHz
 Detector: Peak
 RBW: 1 MHz
 VBW: 3 MHz
 Sweep Time: 100 ms
 Conducted Power: -6.5 dBm
 Operator: Mr. Treffke
 Date: 2016-02-22

Result Summary

Antenna Polarization	Turn table Angle [°]	Max. rad. power [dBm e.i.r.p.]	Max. antenna gain [dBi]
Vertical	112	-32.98	-26.48
Horizontal	160	-36.24	-29.74

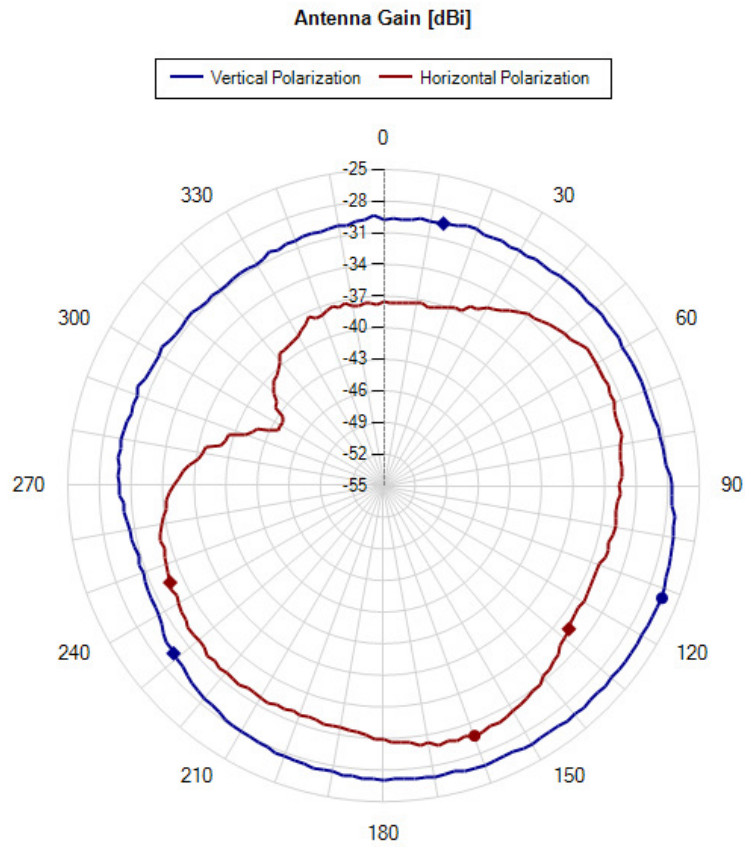

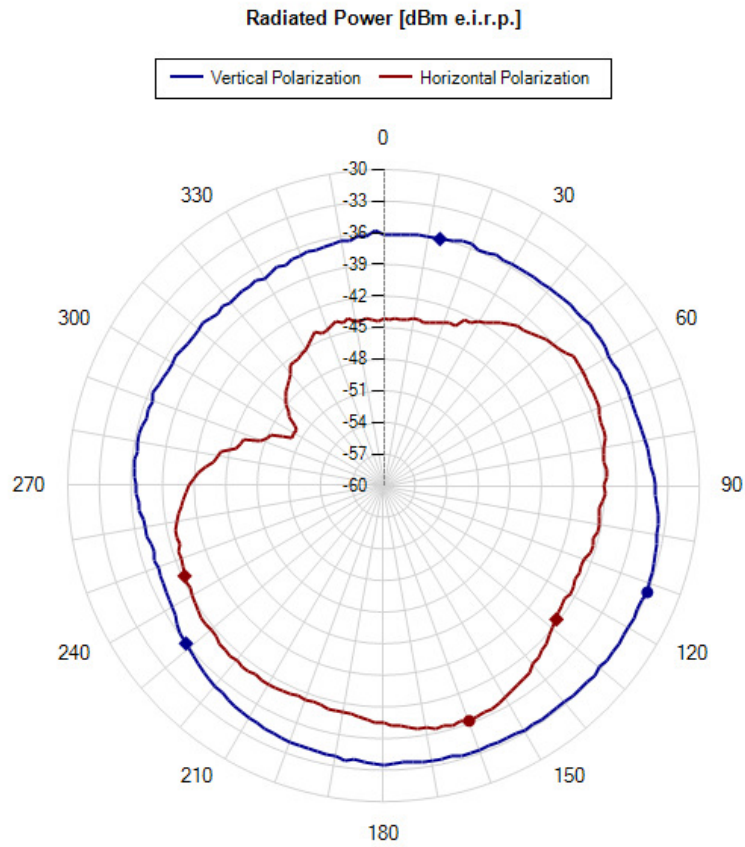



Antenna Pattern

Project Number: G0M-1507-4972
 Product: Primus Nano Plus Pacemaker Family
 Model: HF-T
 EUT Position: vertical, without leads
 EUT Antenna: integral
 Operating Conditions: Tnom / Vnom
 Operating Frequency: 403.65 MHz
 Detector: Peak
 RBW: 1 MHz
 VBW: 3 MHz
 Sweep Time: 100 ms
 Conducted Power: -6.5 dBm
 Operator: Mr. Treffke
 Date: 2016-02-22

Result Summary

Antenna Polarization	Turn table Angle [°]	Max. rad. power [dBm e.i.r.p.]	Max. antenna gain [dBi]
Vertical	118	-32.34	-25.84
Horizontal	160	-36.33	-29.83

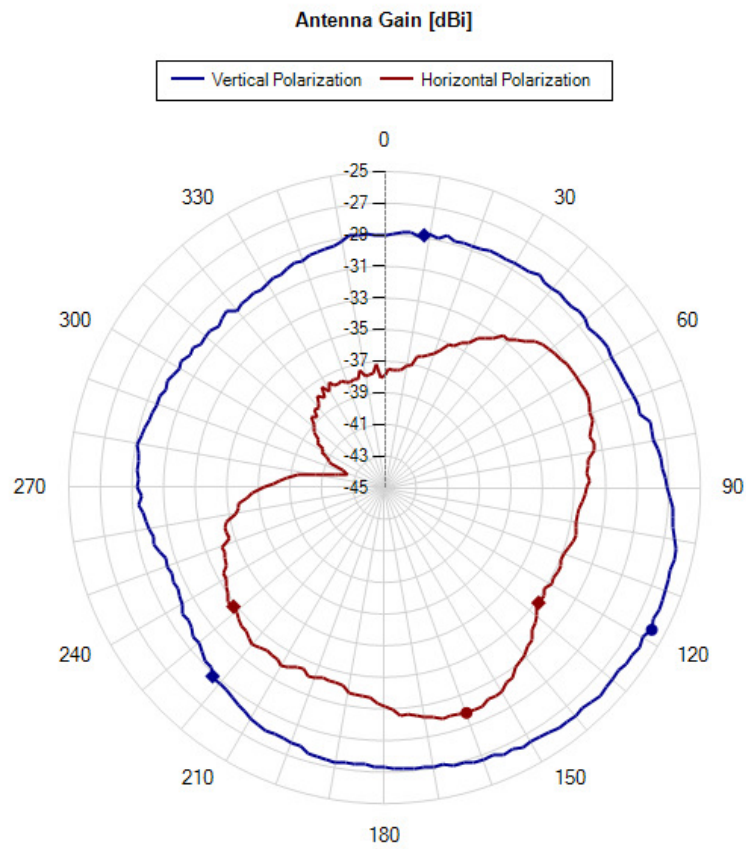

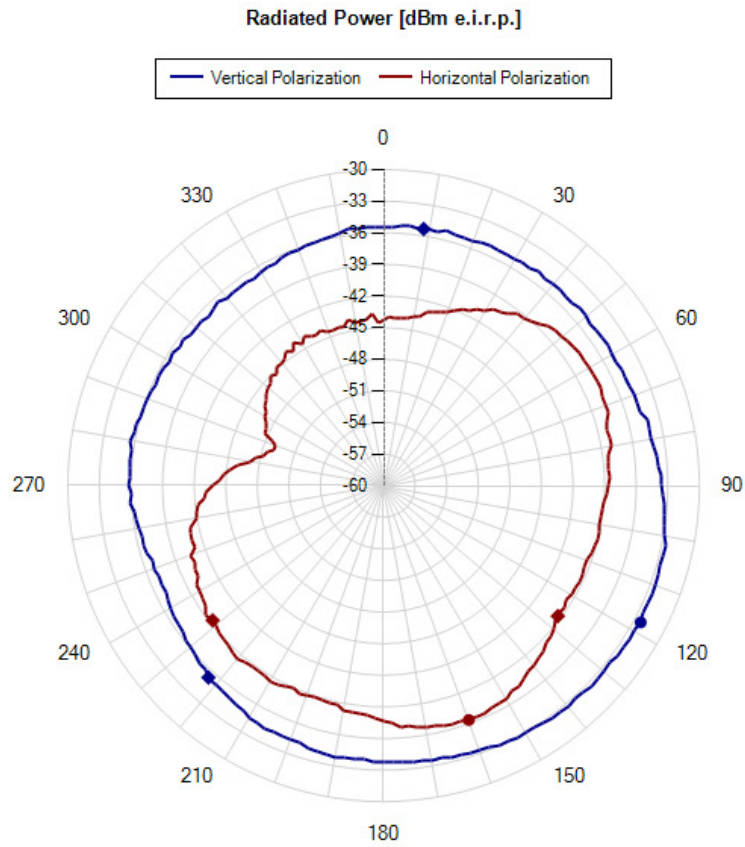

Antenna Pattern

Project Number: G0M-1507-4972
 Product: Primus Nano Plus Pacemaker Family
 Model: SR-T
 EUT Position: vertical, without leads
 EUT Antenna: integral
 Operating Conditions: Tnom / Vnom
 Operating Frequency: 403.65 MHz
 Detector: Peak
 RBW: 1 MHz
 VBW: 3 MHz
 Sweep Time: 100 ms
 Conducted Power: -6.5 dBm
 Operator: Mr. Treffke
 Date: 2016-02-22

Result Summary

Antenna Polarization	Turn table Angle [°]	Max. rad. power [dBm e.i.r.p.]	Max. antenna gain [dBi]
Vertical	152	-35.96	-29.46
Horizontal	158	-40.12	-33.62

