

Appendix 2 Photodocumentation

Description: Open view

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/104

Page: 2 of 21

Date: 13.01.2005

checked by: 

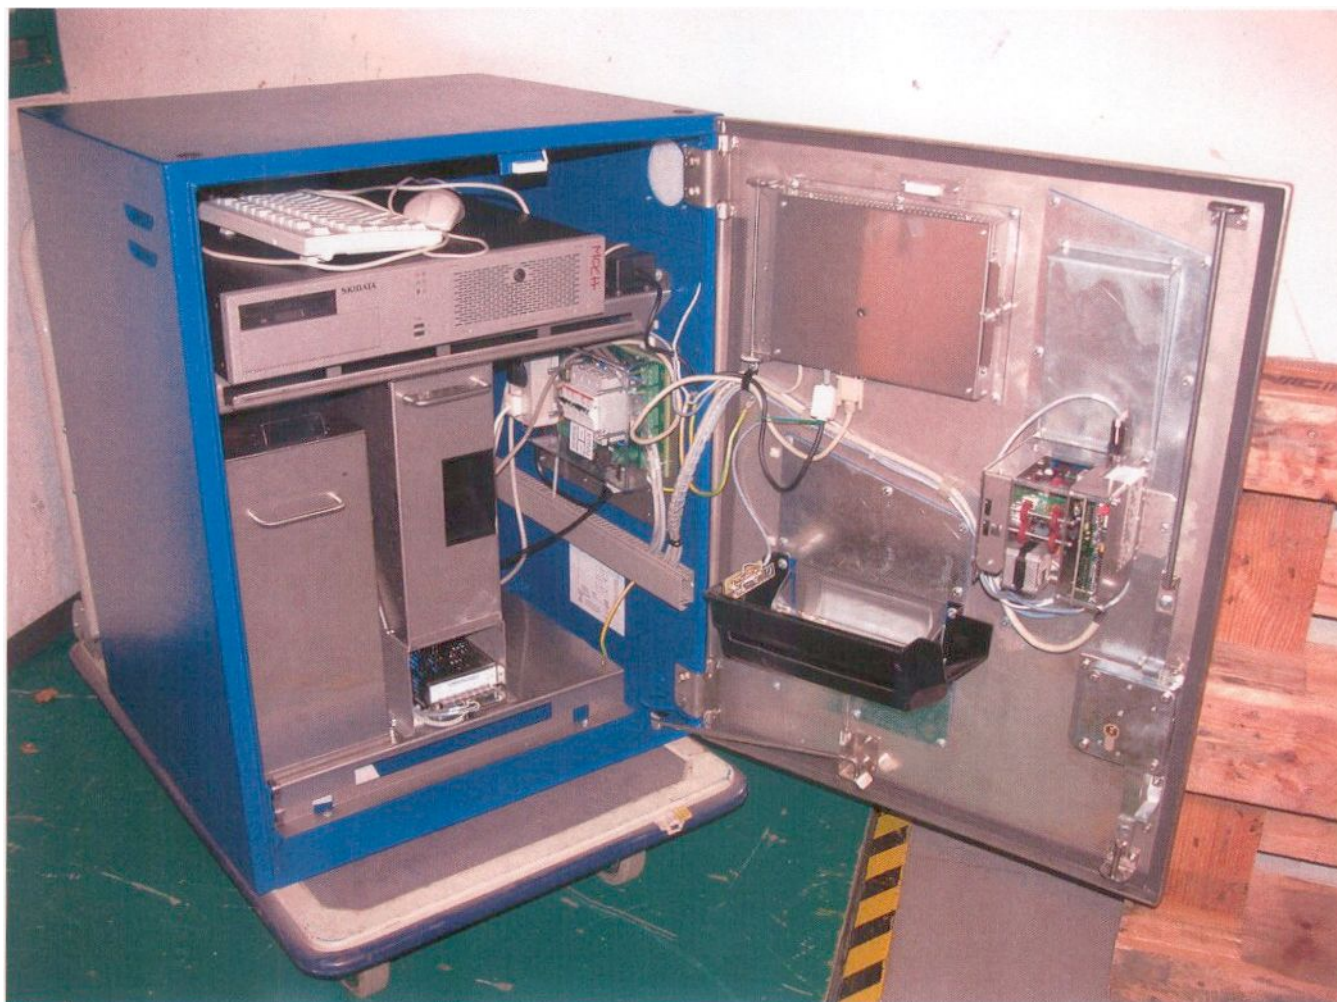

Appendix 2 Photodocumentation

Description: Collection tray


Medizintechnik/Nachrichtentechnik/EMV

Department: EMC

Test report reference:
M/EMV-05/104

Page: 3 of 21

Date: 13.01.2005

checked by: 



Appendix 2
Photodocumentation

Description: Display general

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/104

Page: 4 of 21

Date: 13.01.2005

checked by: 

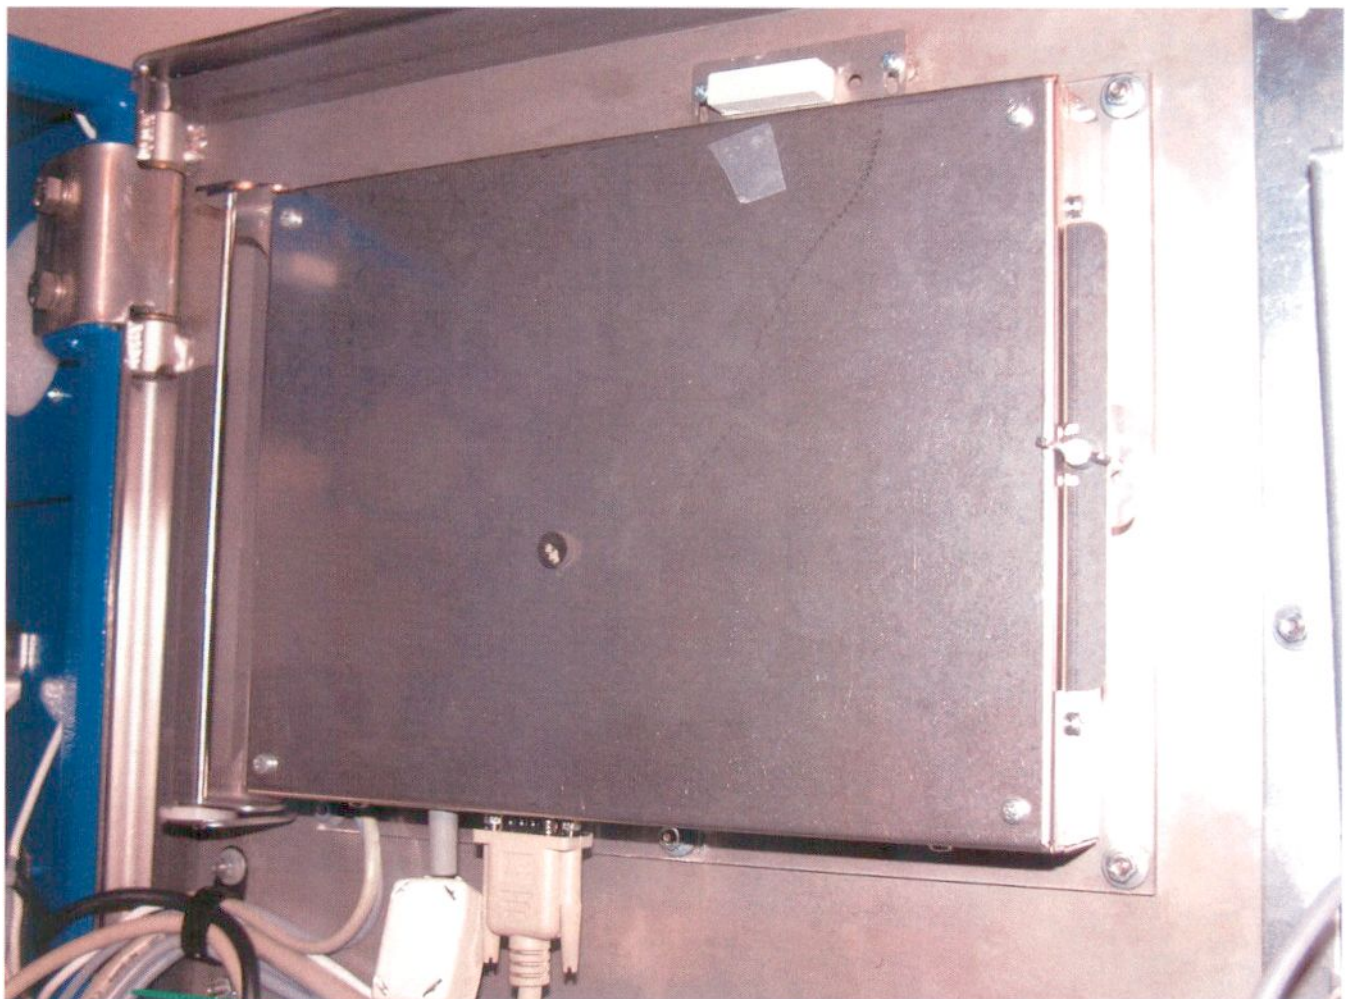

Appendix 2 Photodocumentation

Description: Display open

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/104

Page: 5 of 21

Date: 13.01.2005

checked by: 

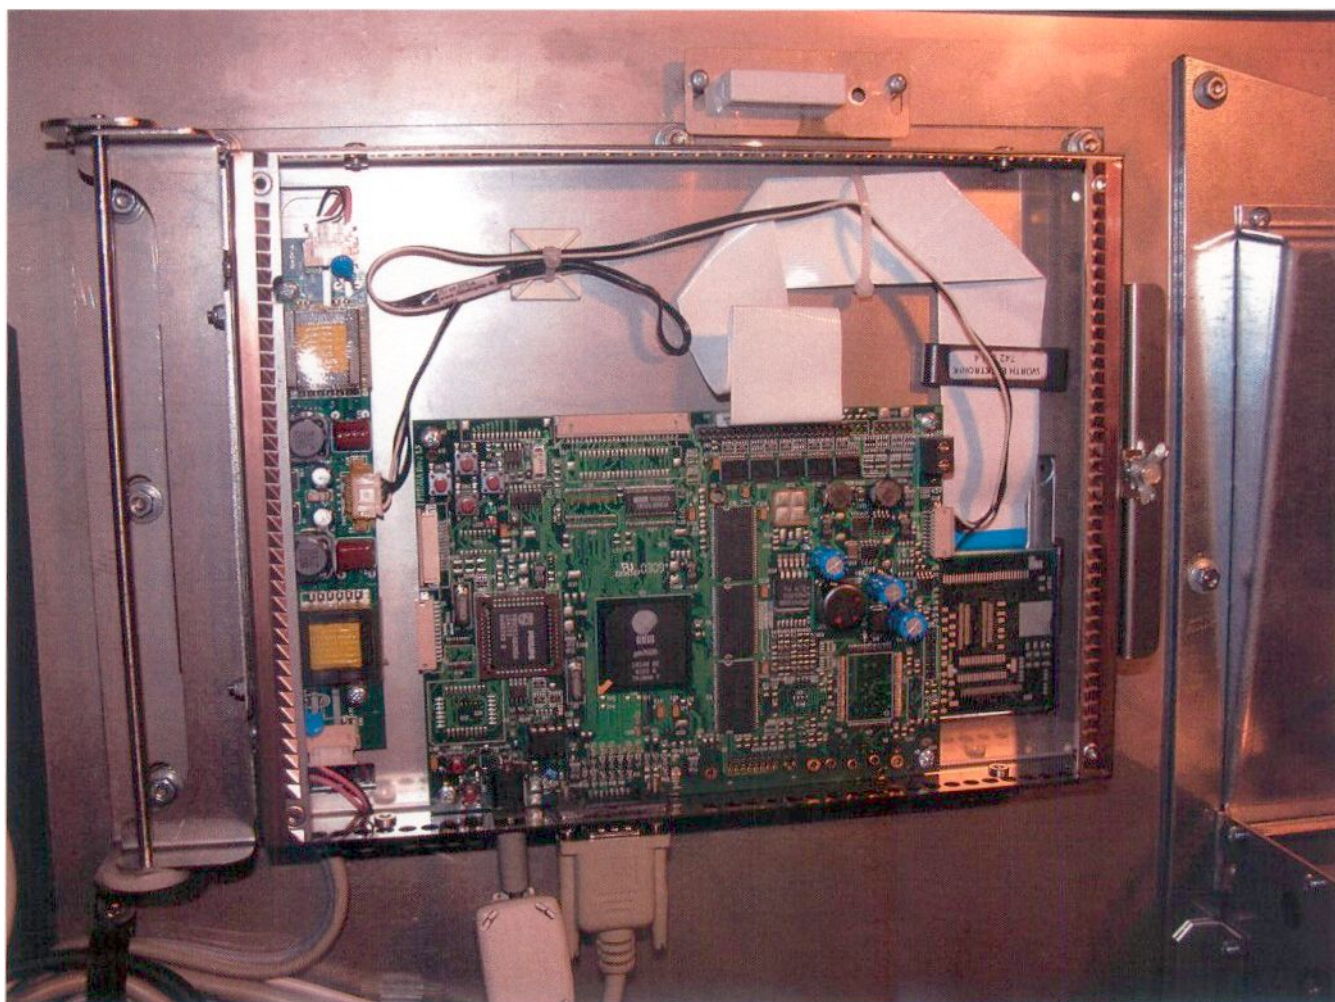

Appendix 2 Photodocumentation

Description: Display PCB #1

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/104

Page: 6 of 21

Date: 13.01.2005

checked by: 

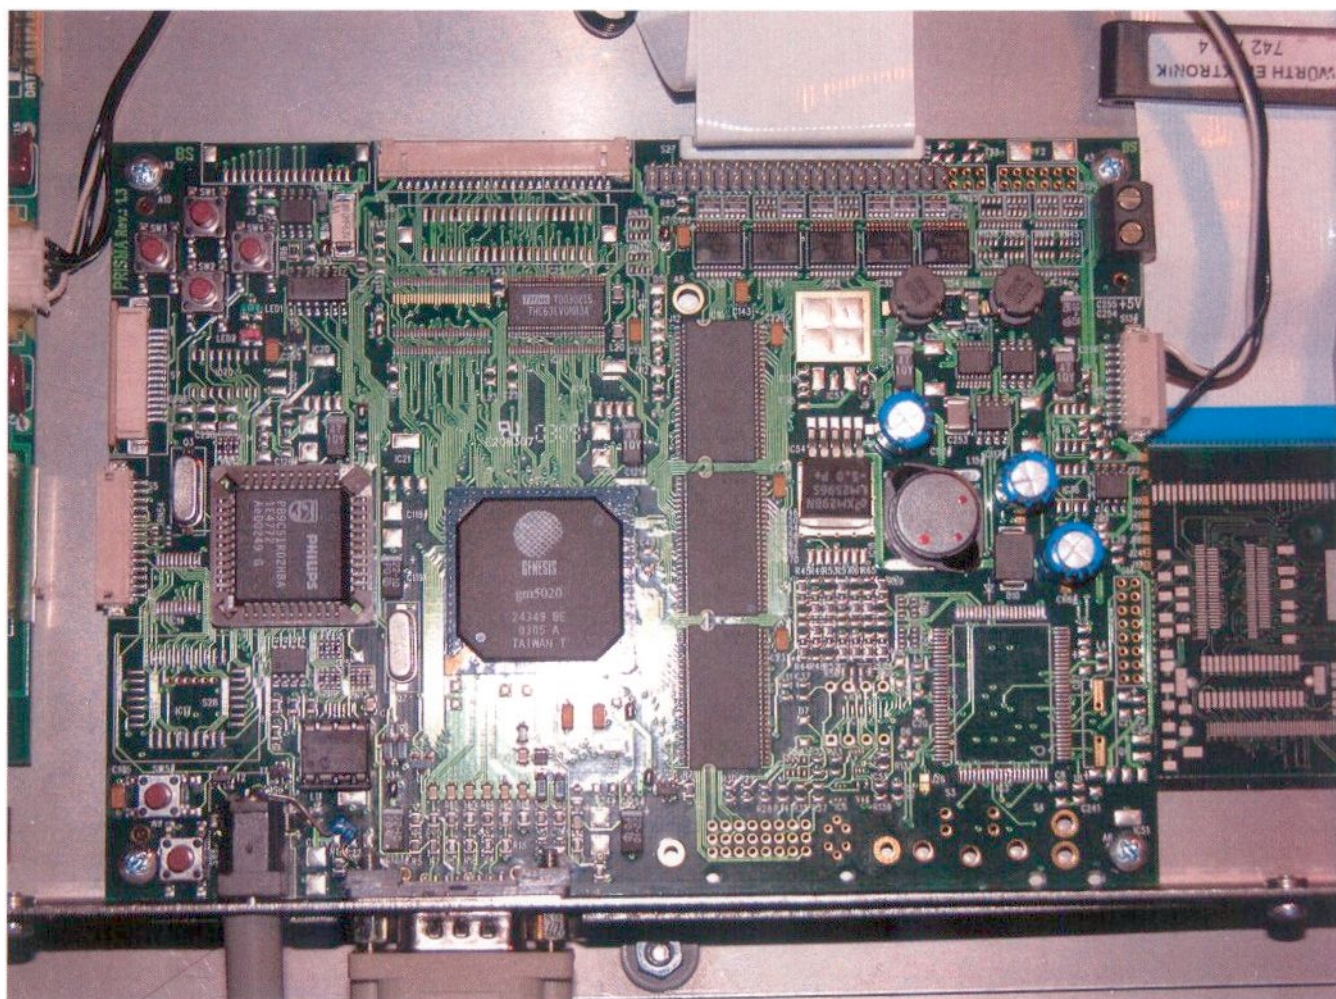

Appendix 2 Photodocumentation

Description: Display PCB #2

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/104

Page: 7 of 21

Date: 13.01.2005

checked by: 

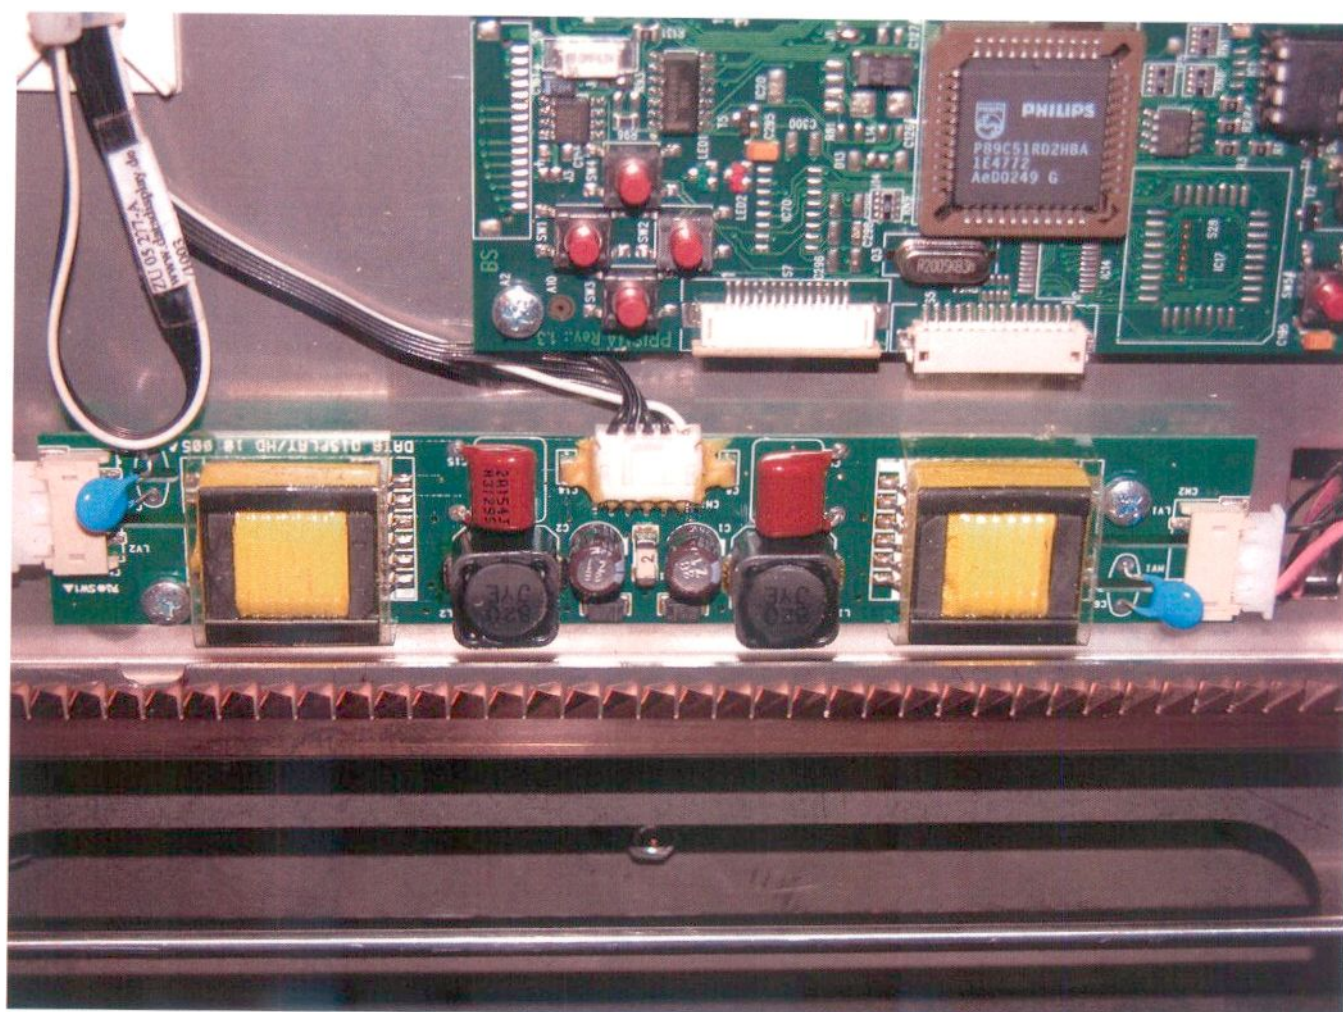

Appendix 2
Photodocumentation

Description: Display power supply model plate

Medizintechnik/Nach-
richtentechnik/EMV

Department: EMC

Test report reference:
M/EMV-05/104

Page: 8 of 21

Date: 13.01.2005

checked by: 



Appendix 2 Photodocumentation

Description: Power supply general view

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/104

Page: 9 of 21

Date: 13.01.2005

checked by: *[Signature]*

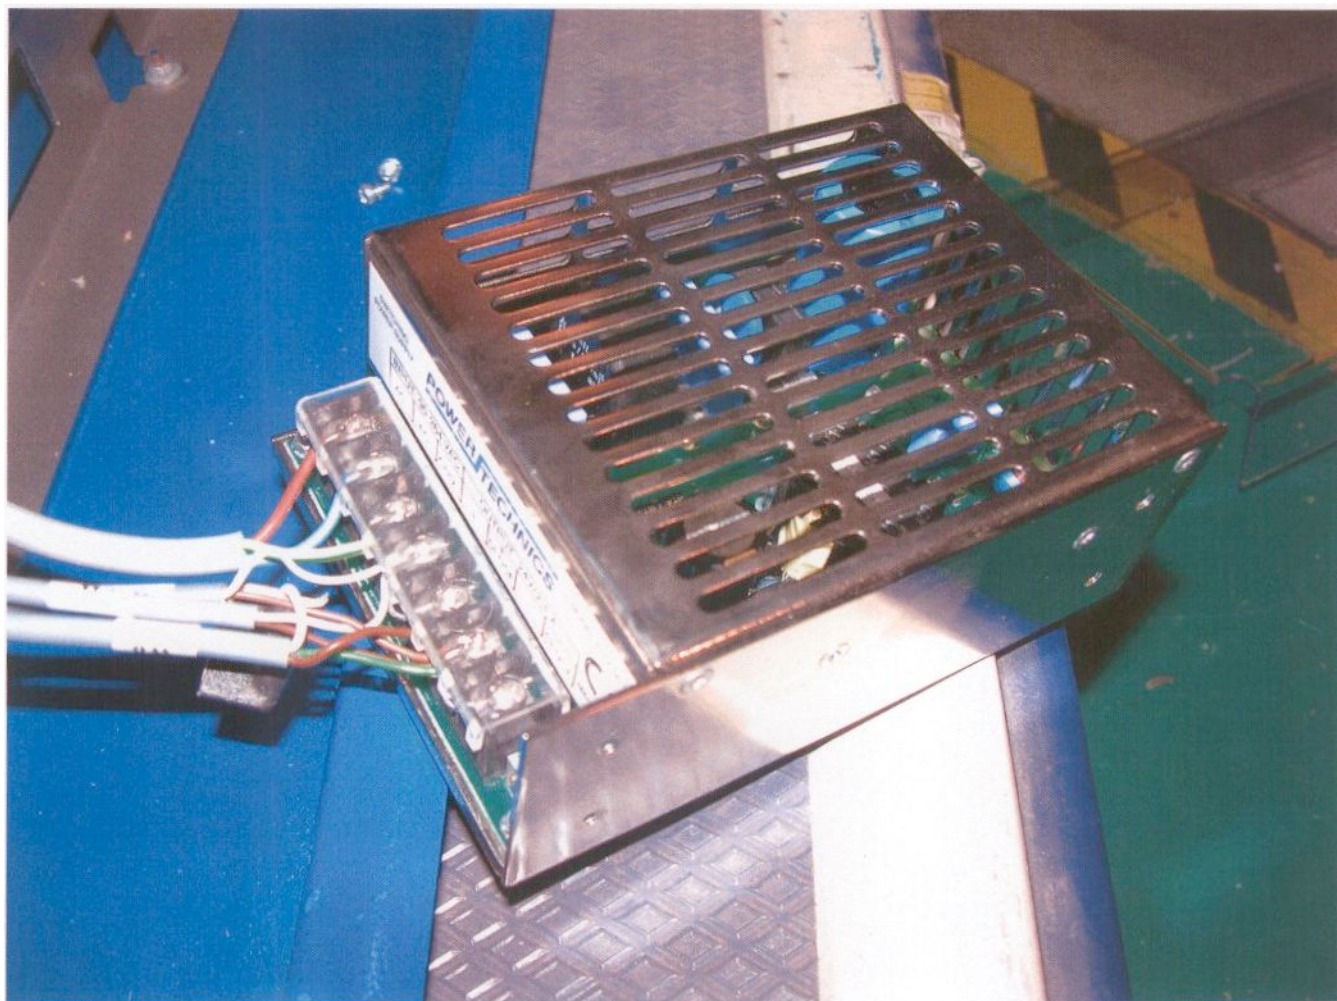

Appendix 2 Photodocumentation

Description: Power supply model plate

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/104

Page: 10 of 21

Date: 13.01.2005

checked by: 

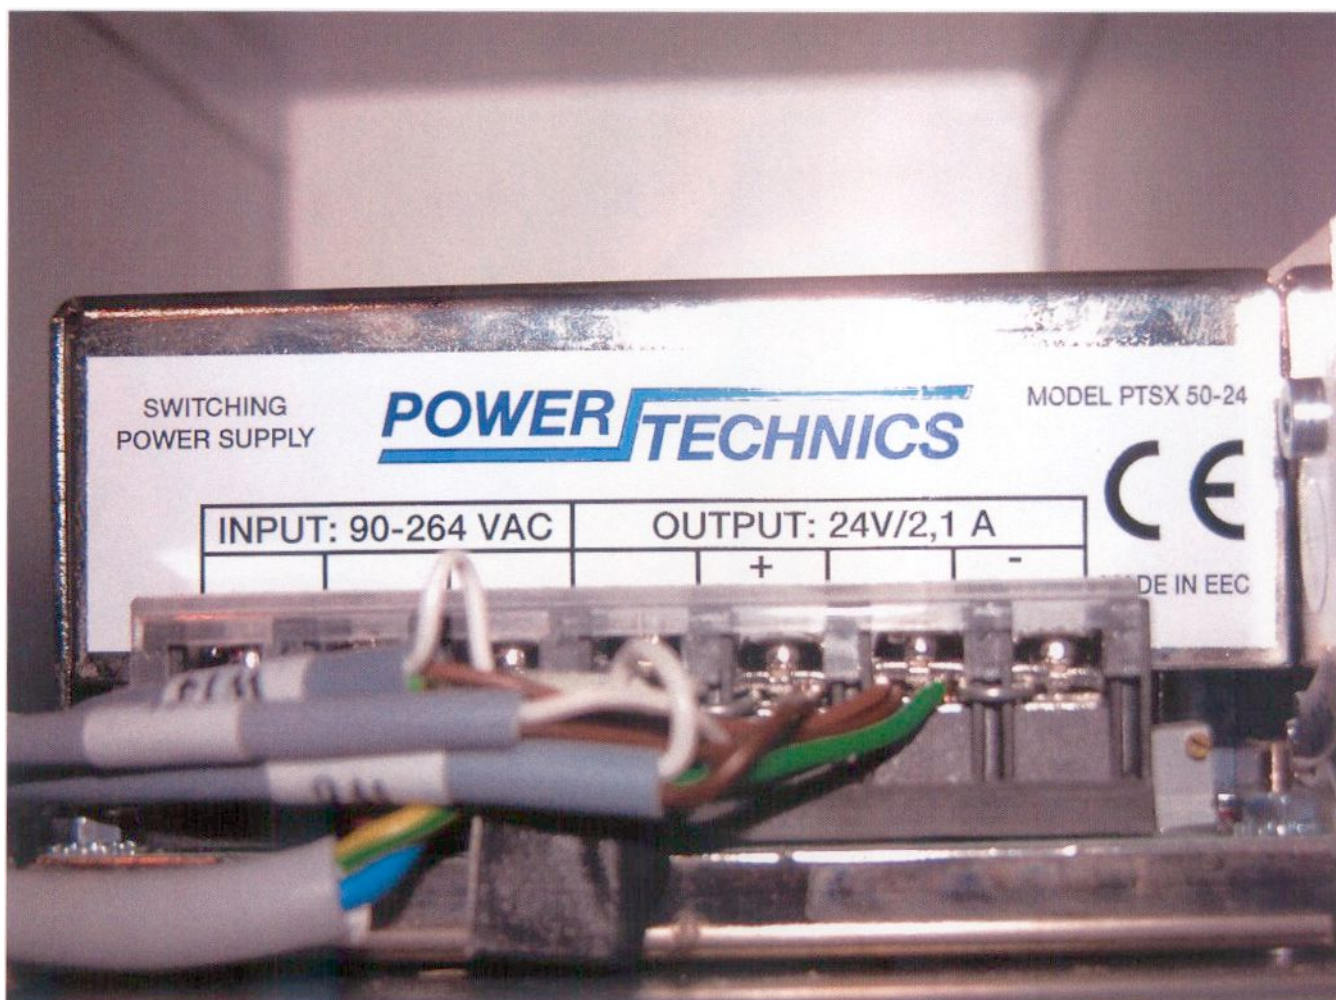

Appendix 2 Photodocumentation

Description: sd412 general view

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/104

Page: 11 of 21

Date: 13.01.2005

checked by:

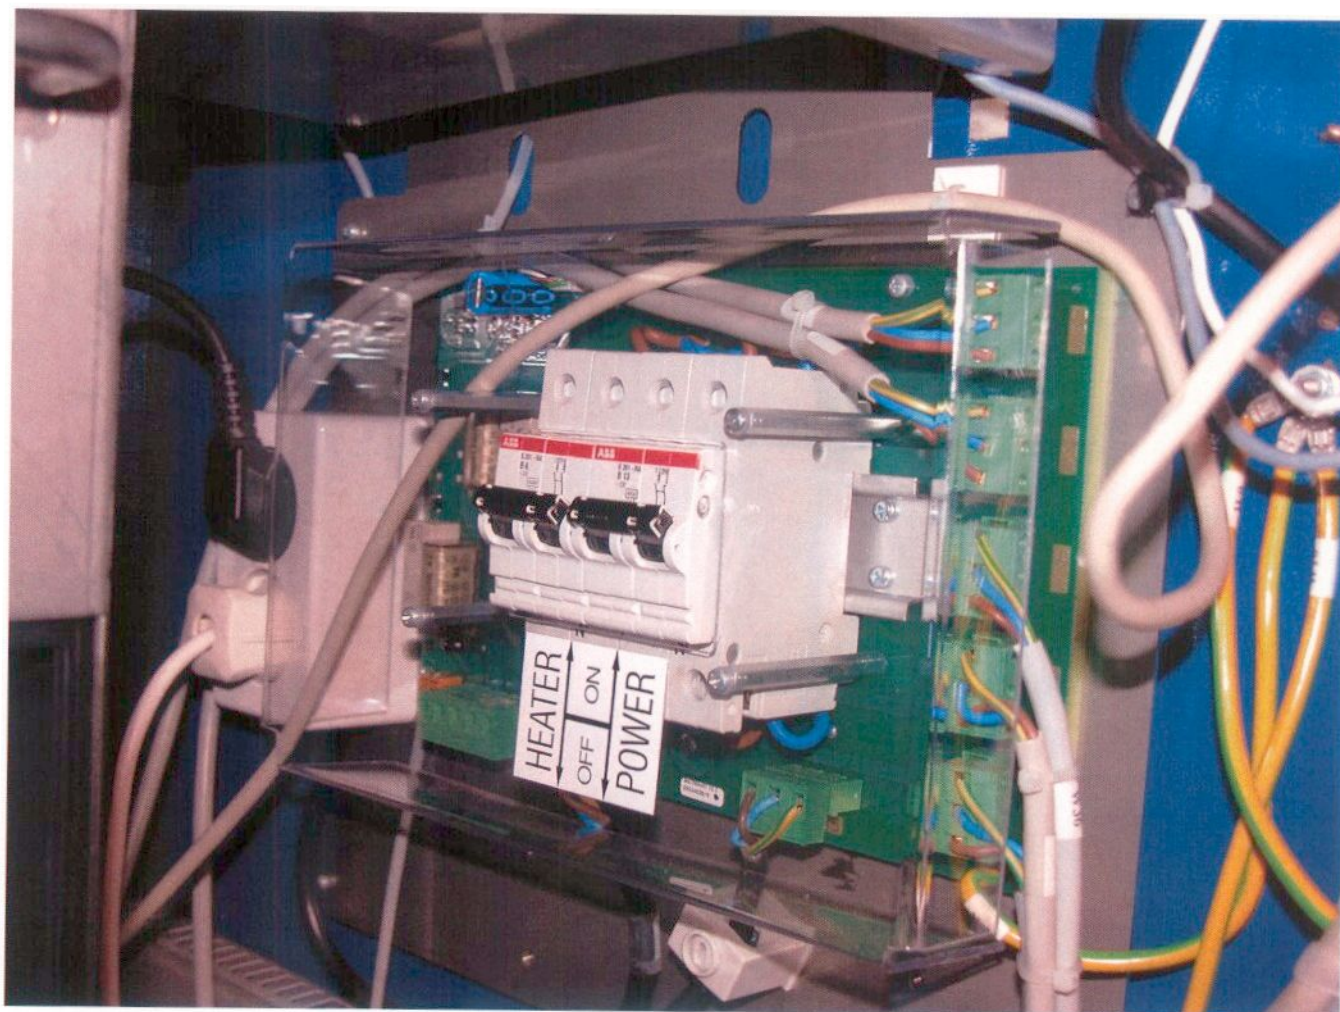

Appendix 2 Photodocumentation

Description: sd412 component side

Medizintechnik/Nachrichtentechnik/EMV



Department: EMC

Test report reference:
M/EMV-05/104

Page: 12 of 21

Date: 13.01.2005

checked by:

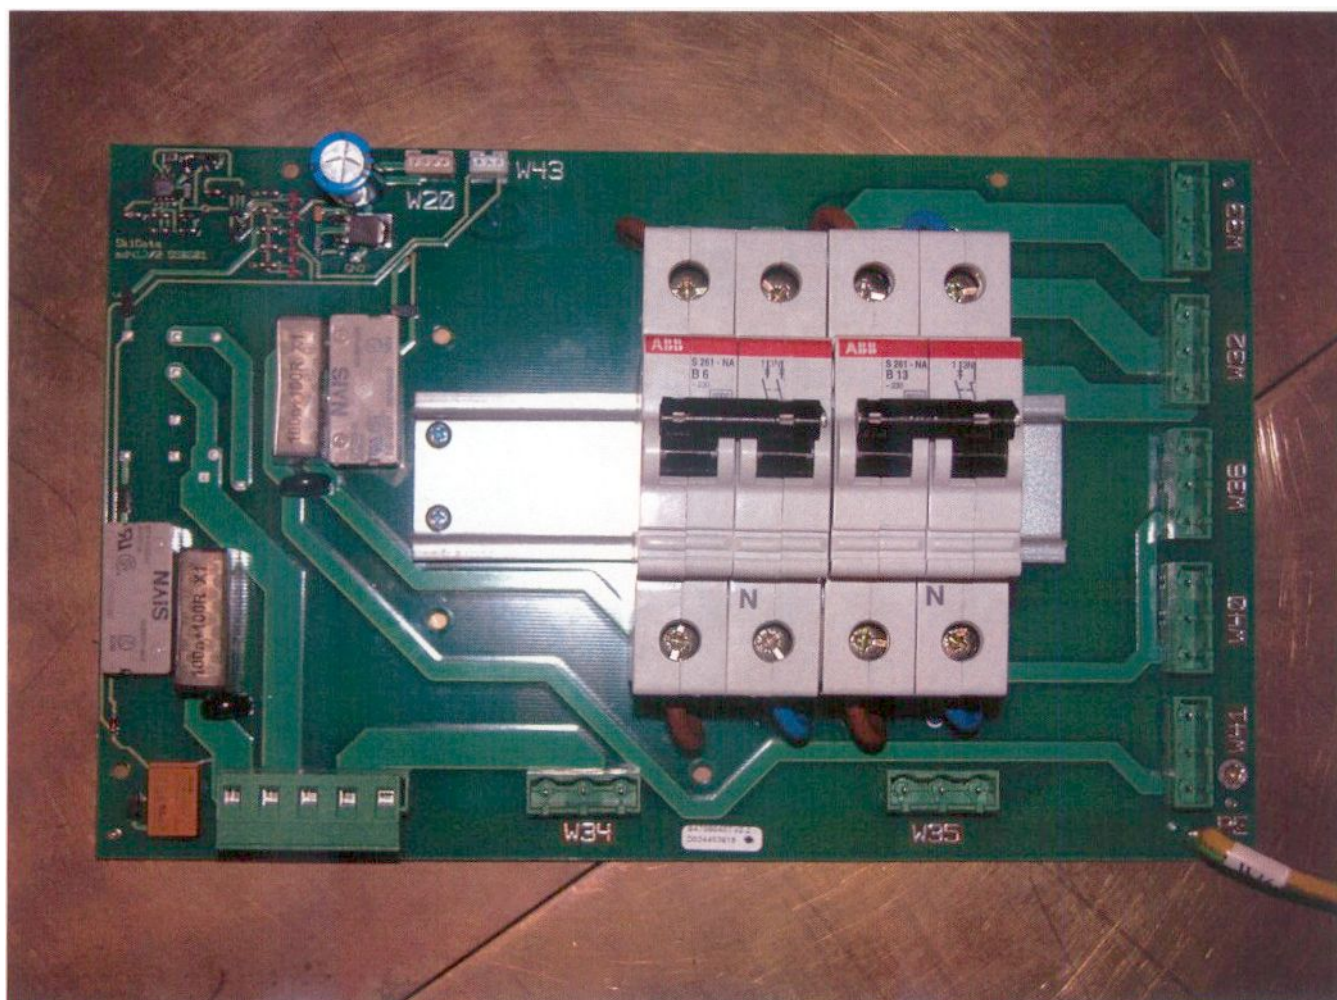

Appendix 2 Photodocumentation

Description: sd412 solder side

Medizintechnik/Nach-
richtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/104

Page: 13 of 21

Date: 13.01.2005

checked by: 

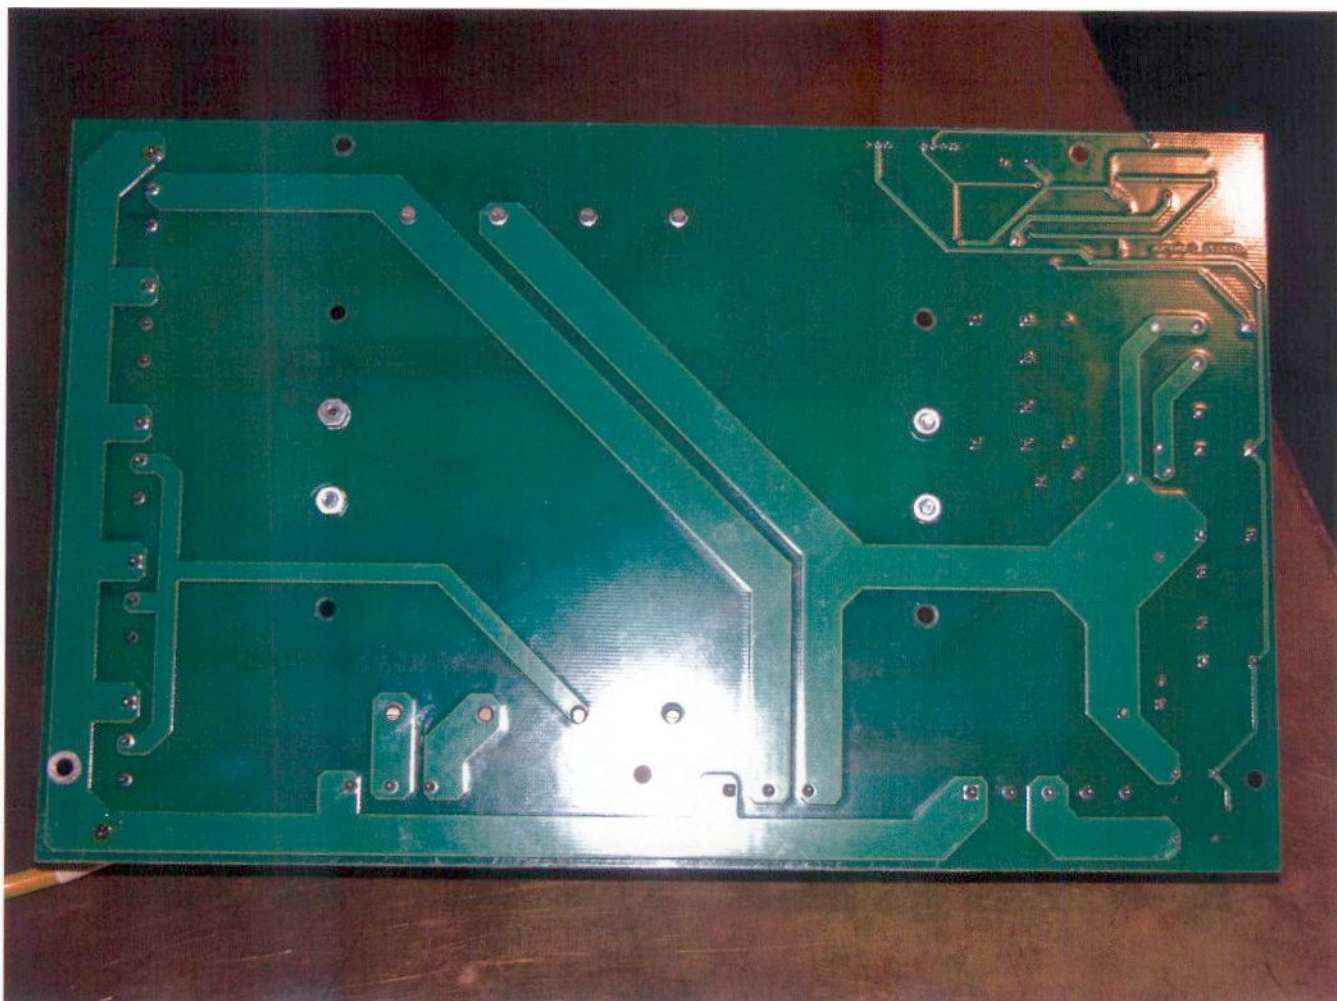

Appendix 2 Photodocumentation

Description: PC


Medizintechnik/Nachrichtentechnik/EMV

Department: EMC

Test report reference:
M/EMV-05/104

Page: 14 of 21

Date: 13.01.2005

checked by: 



Appendix 2 Photodocumentation

Description: PC connections

Medizintechnik/Nachrichtentechnik/EMV

Department: EMC

Test report reference:
M/EMV-05/104

Page: 15 of 21

Date: 13.01.2005

checked by: 



Appendix 2 Photodocumentation

Description: PC open view

Medizintechnik/Nachrichtentechnik/EMV

Department: EMC

Test report reference:
M/EMV-05/104

Page: 16 of 21

Date: 13.01.2005

checked by:



Appendix 2 Photodocumentation

Description: PC power supply

Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/104

Page: 17 of 21

Date: 13.01.2005

checked by: 

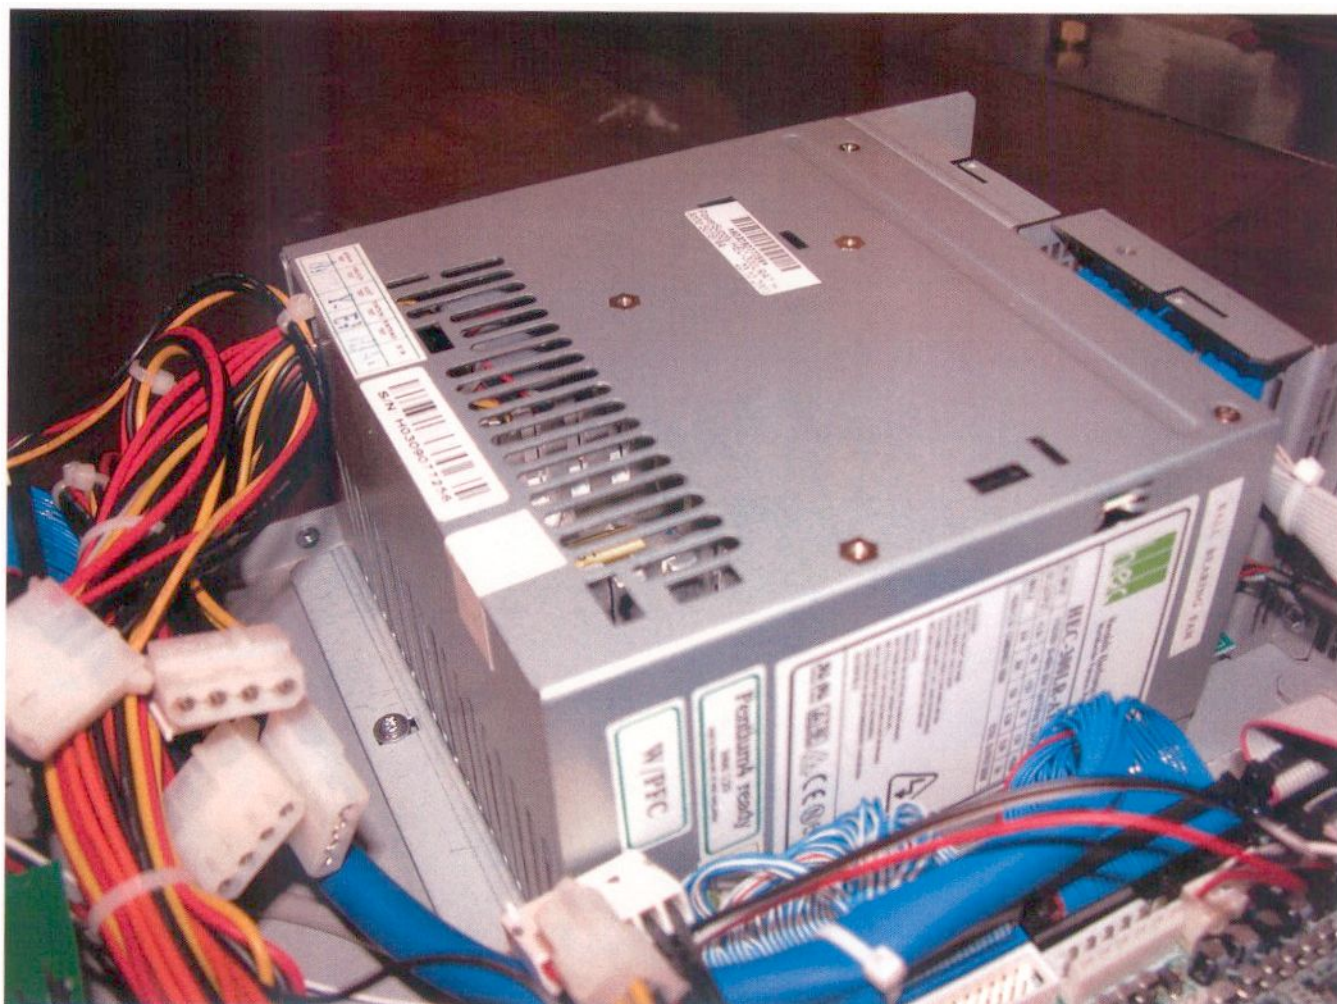

Appendix 2
Photodocumentation

Description: PC model plate

Medizintechnik/Nachrichtentechnik/EMV

Department: EMC

Test report reference:
M/EMV-05/104

Page: 18 of 21

Date: 13.01.2005

checked by: 



Appendix 2 Photodocumentation

Description: Mechanic ME 360 general view


Medizintechnik/Nachrichtentechnik/EMV


Department: EMC

Test report reference:
M/EMV-05/104

Page: 19 of 21

Date: 13.01.2009

checked by: 

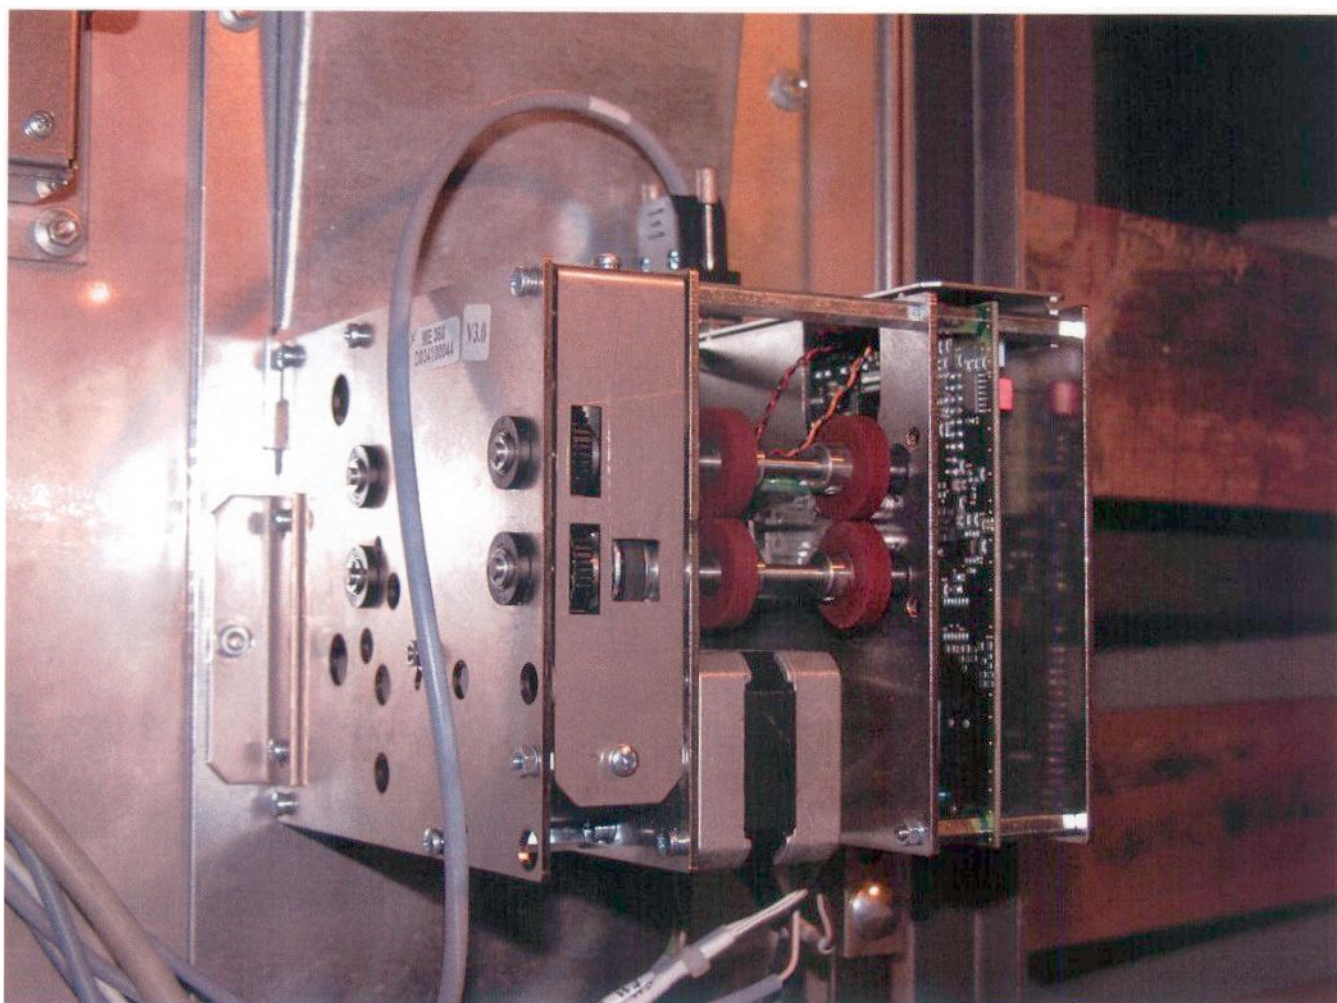

Appendix 2 Photodocumentation

Description: detail

Medizintechnik/Nachrichtentechnik/EMV

Department: EMC

Test report reference:
M/EMV-05/104

Page: 20 of 21

Date: 13.01.2005

checked by: 