

Report No: JYTSZB-R14-2100055

FCC SAR REPORT

Applicant:	Power7 Technology (Dong Guan) Co., Ltd.		
Address of Applicant:	No.28 Binjiang Street. Shishuikou Village, Qiaotou Town, Dongguan City, GuangDong Province P.R.China		
Equipment Under Test (E	EUT)		
Product Name:	Intelligent visible pore cleaner		
Model No.:	wisdom		
Trade mark	GOODtime		
FCC ID:	QT7-WISDOM		
Applicable standards:	FCC 47 CFR Part 2.1093		
Date of Test:	16 Apr., 2021 ~ 16 Apr., 2021		
Test Result:	Maximum Reported 1-g SAR (W/kg) Body: 0.108		

Authorized Signature:



Laboratory Manager

This report details the results of the testing carried out on one sample. The results contained in this test report do not relate to other samples of the same product and does not permit the use of the JYT product certification mark. The manufacturer should ensure that all products in series production are in conformity with the product sample detailed in this report.

This report may only be reproduced and distributed in full. If the product in this report is used in any configuration other than that detailed in the report, the manufacturer must ensure the new system complies with all relevant standards.

This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 90 days only.



2 Version

Version No.	Date	Description
00	20 Apr., 2021	Original

Tested by:

Date:

20 Apr., 2021

20 Apr., 2021

Test Engineer

Kin Li

Reviewed by:

Janet Wei Date:

Project Engineer



3	(Contents	
1	C	OVER PAGE	1
2	V	ERSION	2
3	C	ONTENTS	
4	S	AR RESULTS SUMMARY	4
5		ENERAL INFORMATION	
	5.1	CLIENT INFORMATION	5
	5.2	GENERAL DESCRIPTION OF EUT	-
	5.3 5.4	MAXIMUM RF OUTPUT POWER Environment of Test Site	-
	5.4 5.5	Test Sample Plan	
	5.6	TEST LOCATION	
6	IN	NTRODUCTION	7
	6.1		
_	6.2		
7		F EXPOSURE LIMITS	
	7.1 7.2	ONCONTROLLED ENVIRONMENT	
	7.3	RF Exposure Limits	
8	S	AR MEASUREMENT SYSTEM	9
	8.1	E-Field Probe	
	8.2	DATA ACQUISITION ELECTRONICS (DAE)	
	8.3 8.4	Robot Measurement Server	
	8.5	LIGHT BEAM UNIT	
	8.6	Рналтом	
	8.7 8.8	DEVICE HOLDER DATA STORAGE AND EVALUATION	
	8.9	TEST EQUIPMENT LIST	
9	ті	ISSUE SIMULATING LIQUIDS	
10	S	AR SYSTEM VERIFICATION	
11	E	UT TESTING POSITION	
12	М	IEASUREMENT PROCEDURES	21
	12.1	SPATIAL PEAK SAR EVALUATION	21
	12.2		
	12.3 12.4		
	12.4		
	12.6		
13	C	ONDUCTED RF OUTPUT POWER	24
	13.1	WLAN 2.4 GHz BAND CONDUCTED POWER	24
14	E	XPOSURE POSITIONS CONSIDERATION	25
	14.1		-
	14.2		
15		AR TEST RESULTS SUMMARY	
	15.1 15.2		
	15.2		
16	R	EFERENCE	
-		NDIX A: PLOTS OF SAR SYSTEM CHECK	
		NDIX B: PLOTS OF SAR TEST DATA	
AF	PEN	NDIX C: SYSTEM CALIBRATION CERTIFICATE	



4 SAR Results Summary

The maximum results of Specific Absorption Rate (SAR) found during test as bellows:

<Highest Reported standalone SAR Summary>

Exposure Position	Frequency Band	Reported 1-g SAR (W/kg)	Equipment Class	Highest Reported 1-g SAR (W/kg)
Body (0 mm Gap)	WLAN 2.4GHz	0.108	DTS	0.108



5 General Information

5.1 Client Information

Applicant:	Power7 Technology (Dong Guan) Co., Ltd.	
Address of Applicant: No.28 Binjiang Street.Shishuikou Village,Qiaotou Town, Dongguan City,GuangDong Province P.R.China		
Manufacturer:	Power7 Technology (Dong Guan) Co., Ltd.	
Address of Manufacturer:	No.28 Binjiang Street.Shishuikou Village,Qiaotou Town, Dongguan City,GuangDong Province P.R.China	

5.2 General Description of EUT

Product Name:	Intelligent visible pore cleaner			
Model No.:	wisdom	wisdom		
Category of device	Portable	Portable device		
Operation Frequency:	Wi-Fi:	Wi-Fi: 2412MHz~2472MHz		
Modulation technology:	Wi-Fi:	Wi-Fi: 🛛 802.11b(DSSS) 🖾 802.11g/n (OFDM)		
Antenna Type:	Internal Antenna			
Antenna Gain:	Wi-Fi: 0.5 dBi			
Dimensions (L*W*H):	125 mm (L)× 13 mm (W)× 13 mm (H)			
Accessories information:	Battery: Rechargeable Li-ion Battery 3.7V/200mAh			

5.3 Maximum RF Output Power

WLAN 2.4 GHz Band Average Power (dBm)				
Mode/Band b g n (HT-20) n (HT-40)				
WLAN 2.4GHz	9.51	10.59	10.33	10.05



5.4 Environment of Test Site

Temperature:	18°C ~25 °C
Humidity:	35%~75% RH
Atmospheric Pressure:	1010 mbar

5.5 Test Sample Plan

Sample Number	Used for Test Items
1#	SAR
Domorky lienVan Teating	Crown Shanzhan Ca. Itd. is any reananaible for the test project date of the

Remark: JianYan Testing Group Shenzhen Co., Ltd. is only responsible for the test project data of the above samples, and will keep the above samples for a month.

5.6 Test Location

Jian Yan Testing Group Shenzhen Co., Ltd.

No.101, Building 8, Innovation Wisdom Port, No.155 Hongtian Road, Huangpu Community, Xinqiao Street, Bao'an District, Shenzhen, Guangdong, People's Republic of China. Tel: +86-755-23118282, Fax: +86-755-23116366 Email: info@ccis-cb.com, Website: http://www.ccis-cb.com



6 Introduction

6.1 Introduction

SAR is related to the rate at which energy is absorbed per unit mass in an object exposed to a radio field. The SAR distribution in a biological body is complicated and is usually carried out by experimental techniques or numerical modeling. The standard recommends limits for two tiers of groups, occupational/controlled and general population/uncontrolled, based on a person's awareness and ability to exercise control over his or her exposure. In general, occupational/controlled exposure limits are higher than the limits for general population/uncontrolled.

6.2 SAR Definition

The SAR definition is the time derivative (rate) of the incremental energy (dW) absorbed by (dissipated in) an incremental mass (dm) contained in a volume element (dv) of a given density (ρ). The equation description is as below:

$$SAR = \frac{d}{dt} \left(\frac{dU}{dm} \right) = \frac{d}{dt} \left(\frac{dU}{\rho dv} \right)$$

SAR is expressed in units of Watts per kilogram (W/kg)

SAR measurement can be either related to the temperature elevation in tissue by

$$SAR = C \left(\frac{\delta T}{\delta t}\right)$$

Where: C is the specific heat capacity, δT is the temperature rise and δt is the exposure duration, or related to the electrical field in the tissue by

$$SAR = \frac{\sigma \cdot E^2}{\rho}$$

Where: σ is the conductivity of the tissue, ρ is the mass density of the tissue and E is the RMS electrical field strength. However for evaluating SAR of low power transmitter, electrical field measurement is typically applied.





7 **RF Exposure Limits**

7.1 Uncontrolled Environment

Uncontrolled Environments are defined as locations where there is the exposure of individuals who have no knowledge or control of their exposure. The general population/uncontrolled exposure limits are applicable to situations in which the general public may be exposed or in which persons who are exposed as a consequence of their employment may not be made fully aware of the potential for exposure or cannot exercise control over their exposure. Members of the general public would come under this category when exposure is not employment-related; for example, in the case of a wireless transmitter that exposes persons in its vicinity.

7.2 Controlled Environment

Controlled Environments are defined as locations where there is exposure that may be incurred by persons who are aware of the potential for exposure, (i.e. as a result of employment or occupation). In general, occupational/controlled exposure limits are applicable to situations in which persons are exposed as a consequence of their employment, who have been made fully aware of the potential for exposure and can exercise control over their exposure. This exposure category is also applicable when the exposure is of a transient nature due to incidental passage through a location where the exposure levels may be higher than the general population/uncontrolled limits, but the exposed person is fully aware of the potential for exposure and can exercise control over his or her exposure by leaving the area or by some other appropriate means.

7.3 RF Exposure Limits

SAR Human Exposure Specified in ANSI/IEEE C95.1-1992 and Health Canada Safety Code 6

HUMAN EXPOSURE LIMITS			
	UNCONTROLLED ENVIRONMENT	CONTROLLED ENVIRONMENT	
	General Population (W/kg) or (mW/g)	Occupational (W/kg) or (mW/g)	
SPATIAL PEAK SAR Brain	1.6	8.0	
SPATIAL AVERAGE SAR Whole Body	0.08	0.4	
SPATIAL PEAK SAR Hands, Feet, Ankles, Wrists	4.0	20	

Note:

- 1. The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.
- 2. The Spatial Average value of the SAR averaged over the whole body.
- 3. The Spatial Peak value of the SAR averaged over any 10 grams of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.



8 SAR Measurement System

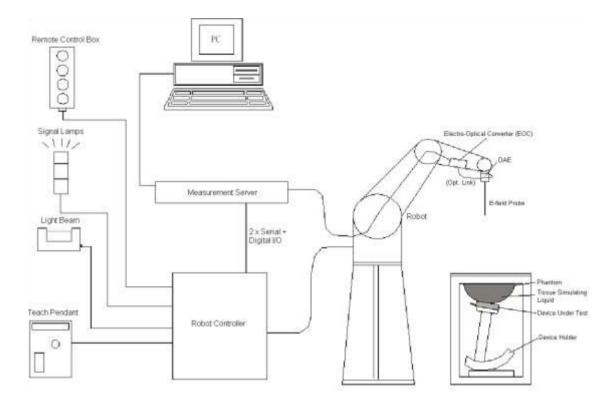


Fig. 8.1 SPEAG DASY System Configurations

The DASY system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- > A standard high precision 6-axis robot with controller, a teach pendant and software
- > A data acquisition electronic (DAE) attached to the robot arm extension
- > A dosimetric probe equipped with an optical surface detector system
- > The electro-optical converter (EOC) performs the conversion between optical and electrical signals
- A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- > A probe alignment unit which improves the accuracy of the probe positioning
- A computer operating Windows XP
- DASY software
- Remove control with teach pendant and additional circuitry for robot safety such as warming lamps, etc.
- The SAM twin phantom
- A device holder
- Tissue simulating liquid
- Dipole for evaluating the proper functioning of the system

Component details are described in the following sub-sections.



8.1 E-Field Probe

The SAR measurement is conducted with the dosimetric probe (manufactured by SPEAG). The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency. This probe has a built in optical surface detection system to prevent from collision with phantom.

> E-Field Probe Specification

<EX3DV4 Probe>

Construction	Ourses state of state interview suith the surface state. Durit in	
Construction	Symmetrical design with triangular core Built-in	
	shielding against static charges PEEK	
	enclosure material (resistant to organic	
	solvents, e.g., DGBE)	
F	o ,	
Frequency	10 MHz to 6 GHz; Linearity: ± 0.2 dB	
Directivity	± 0.3 dB in HSL (rotation around probe axis)	
-	± 0.5 dB in tissue material (rotation normal to	E
	probe axis)	
Dynamic Range	10 µW/g to 100 mW/g; Linearity: ± 0.2 dB	RESEATLY .
,	(noise: typically < $1 \mu W/g$)	
Dimensions	Overall length: 330 mm (Tip: 20mm)	
	Tip diameter: 2.5 mm (Body: 12mm)	
	Typical distance from probe tip to dipole	
	centers: 1 mm	
		Fig. 8.2 Photo of E-Field Probe

> E-Field Probe Calibration

Each probe needs to be calibrated according to a dosimetric assessment procedure with accuracy better than \pm 10%. The spherical isotropy shall be evaluated and within \pm 0.25 dB. The sensitivity parameters (Norm X, Norm Y and Norm Z), the diode compression parameter (DCP) and the conversion factor (ConvF) of the probe are tested. The calibration data can be referred to appendix E of this report.

8.2 Data Acquisition Electronics (DAE)

The Data acquisition electronics (DAE) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit. Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock. The input impedance of the DAE is 200 MOhm; the inputs are symmetrical and floating. Common mode rejection is above 80 dB.




Fig. 8.3 Photo of DAE



Fig. 8.4 Photo of Robot


8.3 Robot

The SPEAG DASY system uses the high precision robots (DASY5: TX60L) type from Stäubli SA (France). For the 6-axis controller system, the robot controller version (DASY5: CS8c) from Stäubli is used. The Stäubli robot series have many features that are important for our application:

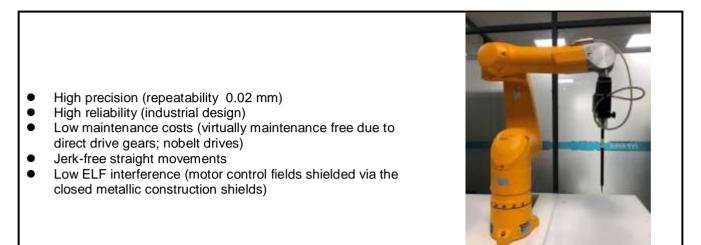

8.4 Measurement Server


The measurement server is based on a PC/104 CPU board with CPU (DASY 5: 400MHz, Intel Celeron), chipdisk (DASY5: 128 MB), RAM (DASY5: 128 MB). The necessary circuits for communication with the DAE electronic box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY I/O board, which is directly connected to the PC/104 bus of the CPU board. The measurement server performs all the real-time data evaluation for field measurements and surface detection, controls robot movements and handles safety operations.

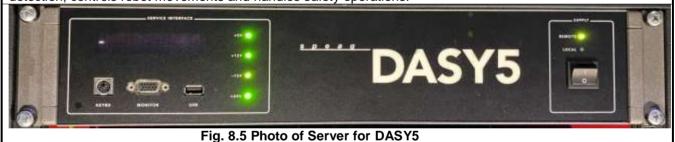

8.5 Light Beam Unit

The light beam switch allows automatic "tooling" of the probe. During the process, the actual position of the probe tip with respect to the robot arm is measured, as well as the probe length and the horizontal probe offset. The software then corrects all movements, such that the robot coordinates are valid for the probe tip.

The repeatability of this process is better than0.1 mm. If a position has been taught with an aligned probe, the same position will be reached with another aligned probe within 0.1 mm, even if the other probe has different dimensions. During probe rotations, the probe tip will keep its actual position.





8.6 Phantom

<SAM Twin Phantom>

Shell Thickness	2 ± 0.2 mm; Center ear point: 6 ± 0.2 mm	
Filling Volume Dimensions	Approx. 25 liters Length: 1000mm; Width: 500mm;	
Measurement Areas	Height: adjustable feet Left Head, Right Head, Flat phantom	
		Fig. 8.7 Photo of SAM Twin Phantom

The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

<ELI4 Phantom >

The ELI4 phantom is intended for compliance testing of handheld and body-mounted wireless devices in the frequency range of 30MHz to 6 GHz. ELI4 is fully compatible with the latest draft of the standard IEC 62209-2 and all known tissue simulating liquids.

ELI4 has been optimized regarding its performance and can be integrated into a SPEAG standard phantom table. A cover prevents evaporation of the liquid. Reference markings on the phantom allow installation of the complete setup, including all predefined phantom positions and measurement grids, by teaching three points The phantom can be used with the following tissue simulating liquids:

- Water-sugar based liquids can be left permanently in the phantom. Always cover the liquid if the system is not in use; otherwise the parameters will change due to water evaporation.
- DGBE based liquids should be used with care. As DGBE is a softener for most plastics, the liquid should be taken out of the phantom and the phantom should be dried when the system is not in use (desirable at least once a week).
- Do not use other organic solvents without previously testing the phantom resistiveness



Fig.8.8 Photo of ELI4 Phantom



8.7 Device Holder

<Device Holder for SAM Twin Phantom>

The SAR in the phantom is approximately inversely proportional to the square of the distance between the source and the liquid surface. For a source at 5 mm distance, a positioning uncertainty of \pm 0.5 mm would produce a SAR uncertainty of \pm 20 %. Accurate device positioning is therefore crucial for accurate and repeatable measurements. The positions in which the devices must be measured are defined by the standards. The DASY device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation center for both scales is the ear reference point (ERP). Thus the device needs no repositioning when changing the angles.

The DASY device holder is constructed of low-low POM material having the following dielectric parameters: relative permittivity $\varepsilon = 3$ and loss tangent $\delta = 0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



JianYan Testing Group Shenzhen Co., Ltd.Project No.: JYTSZE2104015No.101, Building 8, Innovation Wisdom Port, No.155 Hongtian Road, Huangpu Community, Xinqiao Street,
Bao'an District, Shenzhen, Guangdong, People's Republic of China.People's Republic of China.Telephone: +86 (0) 755 23118282 Fax: +86 (0) 755 23116366, E-mail: info@ccis-cb.comPage 13 of 58



8.8 Data storage and Evaluation

Data Storage

The DASY software stores the assessed data from the data acquisition electronics as raw data (in microvolt readings from the probe sensors), together with all the necessary software parameters for the data evaluation (probe calibration data, liquid parameters and device frequency and modulation data) in measurement files. The post-processing software evaluates the desired unit and format for output each time the data is visualized or exported. This allows verifications of the complete software setup even after the measurement and allows correction of erroneous parameter settings. For example, if a measurement has been performed with an incorrect crest factor parameter in the device setup, the parameter can be corrected afterwards and the data can be reevaluated.

The measured data can be visualized or exported in different units or formats, depending on the selected probe type (e.g., [V/m], [mW/g]). Some of these units are not available in certain situations or give meaningless results, e.g., a SAR-output in a non-lose media, will always be zero. Raw data can also be exported to perform the evaluation with other software packages.

Data Evaluation

The DASY post-processing software (SEMCAD) automatically executes the following procedures to calculate the field units from the microvolt readings at the probe connector. The parameters used in the evaluation are stored in the configuration modules of the software:

Probe Parameters:	- Sensitivity - Conversion - Diode compression point	Norm _i , a _{i0} , a _{i1} , a _{i2} ConvF _i dcp _i
Device Parameters:	- Frequency - Crest	f cf
Media Parameters:	- Conductivity - Density	σ ρ

These parameters must be set correctly in the software. They can be found in the component documents or they can be imported into the software from the configuration files issued for the DASY components. In the direct measuring mode of the multi-meter option, the parameters of the actual system setup are used. In the scan visualization and export modes, the parameters stored in the corresponding document files are used.

The first step of the evaluation is a linearization of the filtered input signal to account for the compression characteristics of the detector diode. The compensation depends on the input signal, the diode type and the DC-transmission factor from the diode to the evaluation electronics. If the exciting field is pulsed, the crest factor of the signal must be known to correctly compensate for peak power.



The formula for each channel can be given as:

$$V_i = U_i + U_i^2 \cdot \frac{cf}{dcp_i}$$

With

 V_i = compensated signal of channel i, (i = x, y, z)

 U_i = input signal of channel i, (i = x, y, z)

cf = crest factor of exciting field (DASY parameter)

dcpⁱ = diode compression point (DASY parameter)

From the compensated input signals, the primary field data for each channel can be evaluated:

E- Field Probes: $E_i = \sqrt{\frac{v_i}{Norm_i \cdot ConvF}}$

H-Field Probes:
$$H_i = \sqrt{V_i} \cdot \frac{a_{i0} + a_{i1}f + a_{i2}f^2}{f}$$

With

 V_i = compensated signal of channel i, (i = x, y, z) Norm_i = senor sensitivity of channel i, (i = x, y, z), $\mu V/(V/m)^2$ ConvF = sensitivity enhancement in solution a_{ii} = sensor sensitivity factors for H-field probes f = carrier frequency (GHz) E_i = electric field strength of channel i in V/m

Hi = magnetic field strength of channel i in A/m

The RSS value of the field components gives the total field strength (Hermitian magnitude):

$$E_{tot} = \sqrt{E_x^2 + E_y^2 + E_z^2}$$

The primary field data are used to calculate the derived field units.

$$\mathsf{SAR} = E_{tot}^2 \cdot \frac{\sigma}{\rho \cdot 1000}$$

With

SAR = local specific absorption rate in mW/g

 E_{tot} = total field strength in V/m

 σ = conductivity in (mho/m) or (Siemens/m)

 ρ = equipment tissue density in g/cm³

Note that the density is set to 1, to account for actual head tissue density rather than the density of the tissue simulating liquid.



8.9 Test Equipment List

Manufacturer		Madal	C/N	Cal. Info	ormation
Manufacturer	Equipment Description	Model S/N		Last Cal.	Due Date
SPEAG	2450MHz System Validation Kit	D2450V2	910	06.10.2019	06.09.2022
SPEAG	Data Acquisition Electronics	DAE4	1373	07.27.2020	07.26.2021
SPEAG	Dosimetric E-Field Probe	EX3DV4	3924	09.23.2020	09.22.2021
SPEAG	DASY 52 Measurement Software	DASY 52	Version: 52.8.8.1222	N.C.R	N.C.R
SPEAG	DASY 52 File Conversion Software	SEMCAD X	Version: 14.6.10 (7331)	N.C.R	N.C.R
SPEAG	Phantom	Twin Phantom	1765	N.C.R	N.C.R
SPEAG	Phantom	ELI V5.0	1208	N.C.R	N.C.R
SPEAG	Phone Positioner	N/A	N/A	N.C.R	N.C.R
Stäubli	Robot TX60L		F13/5P6VB1/A/01	N.C.R	N.C.R
R&S	Universal Radio Communication Tester	CMU200	113097	06.18.2020	06.17.2021
HP	Network Analyzer	8753D	3410A06291	06.18.2020	06.17.2021
KEYSIGHT	EPM Series Power Meter	N1914A	MY60400002	12.12.2020	12.11.2021
KEYSIGHT	E-Series Power Sensor	E9300H	MY60310002	07.31.2020	07.30.2021
KEYSIGHT	E-Series Power Sensor	E9300H	MY60340003	08.21.2020	08.20.2021
R&S	Signal Generator	N5182A	MY49060014	11.16.2020	11.15.2021
Huber Suhner	RF Cable	SUCOFLEX	12341	See N	Note 3
Huber Suhner	RF Cable	SUCOFLEX	17268	See N	Note 3
Huber Suhner	RF Cable	SUCOFLEX	2080	See N	Note 3
Weinschel	Attenuator	23-3-34	BL5513	See N	Note 3
Anritsu	Directional Coupler	MP654A	100217491	See Note 3	
SPEAG	Dielectric Assessment Kit	3.5 Probe	1119	See N	Note 4
SPEAG	DAK Measurement Software	DAK	Version: DAK 3.5	N.(C.R
Mini-circuits	Low Noise Amplifier	Power amplifier	LNA-00500200- 2515	See N	Note 5

Note:

1. The calibration certificate of DASY can be referred to appendix C of this report.

2. Referring to KDB 865664 D01v01r04, the dipole calibration interval can be extended to 3 years with justification. The dipoles are also not physically damaged, or repaired during the interval.

3. The Insertion Loss calibration of Dual Directional Coupler and Attenuator were characterized via the network analyzer and compensated during system check.

4. The dielectric probe kit was calibrated via the network analyzer, with the specified procedure (calibrated in pure water) and calibration kit (standard) short circuit, before the dielectric measurement. The specific procedure and calibration kit are provided by Speag.

5. In system check we need to monitor the level on the power meter, and adjust the power amplifier level to have precise power level to the dipole; the measured SAR will be normalized to 1 W input power according to the ratio of 1 W to the input power to the dipole. For system check, the calibration of the power amplifier is deemed not critically required for correct measurement; the power meter is critical and we do have calibration for it

6. Attenuator insertion loss is calibrated by the network Analyzer, which the calibration is valid, before system check.

7. N.C.R means No Calibration Requirement.



9 Tissue Simulating Liquids

For the measurement of the field distribution inside the SAM phantom with DASY, the phantom must be filled with around 25 liters of homogeneous body tissue simulating liquid. For body SAR testing, the liquid height from the center of the flat phantom to liquid top surface is larger than 15 cm, which is shown in Fig. 9.1.

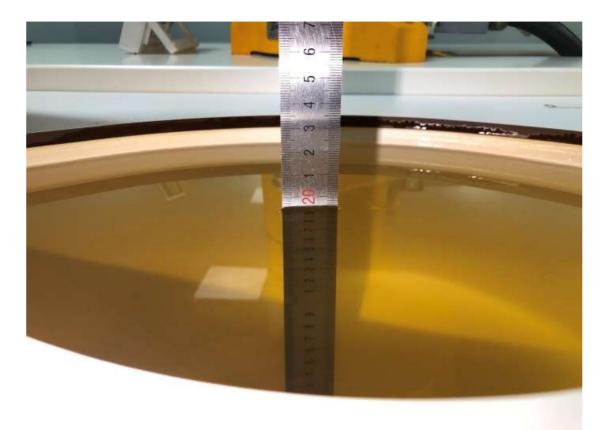


Fig. 9.3 Photo of Liquid Height for Body SAR (2000MHz~2600MHz) (depth>15cm)

The relative permittivity and conductivity of the tissue material should be within $\pm 5\%$ of the values given in the table below recommended by the FCC OET 65 supplement C and RSS 102 Issue 5.

Target Frequency (MHz)	٤r	σ(S/m)
150	52.3	0.76
300	45.3	0.87
450	43.5	0.87
835	41.5	0.90
900	41.5	0.97
915	41.5	0.98
1450	40.5	1.20
1610	40.3	1.29
1800-2000	40.0	1.40
2450	39.2	1.80
3000	38.5	2.40
5800	35.3	5.27

(ϵr = relative permittivity, σ = conductivity and ρ = 1000 kg/m³)

JianYan Testing Group Shenzhen Co., Ltd.Project No.: JYTSZE2104015No.101, Building 8, Innovation Wisdom Port, No.155 Hongtian Road, Huangpu Community, Xinqiao Street,
Bao'an District, Shenzhen, Guangdong, People's Republic of China.Project No.: JYTSZE2104015Telephone: +86 (0) 755 23118282 Fax: +86 (0) 755 23116366, E-mail: info@ccis-cb.comPage 17 of 58



The dielectric parameters of liquids were verified prior to the SAR evaluation using a Speag Dielectric Probe Kit and an Agilent Network Analyzer.

The following table shows the measuring results for simulating liquid.

Frequency (MHz)	Liquid Temp. (°C)	Conductivity (σ)	Permittivity (εr)	Conductivity Target(σ)	Permittivity Target(εr)	Delta (σ)%	Delta (ɛr)%	Limit (%)	Date (mm/dd/yy)
2450	23.3	1.85	38.82	1.80	39.2	2.78	-0.97	±5	04.16.2021



10 SAR System Verification

Each DASY system is equipped with one or more system validation kits. These units, together with the predefined measurement procedures within the DASY software, enable the user to conduct the system performance check and system validation. System validation kit includes a dipole, tripod holder to fix it underneath the flat phantom and a corresponding distance holder.

> Purpose of System Performance check

The system performance check verifies that the system operates within its specifications. System and operator errors can be detected and corrected. It is recommended that the system performance check be performed prior to any usage of the system in order to guarantee reproducible results. The system performance check uses normal SAR measurements in a simplified setup with a well characterized source. This setup was selected to give a high sensitivity to all parameters that might fail or vary over time. The system check does not intend to replace the calibration of the components, but indicates situations where the system uncertainty is exceeded due to drift or failure.

> System Setup

In the simplified setup for system evaluation, the EUT is replaced by a calibrated dipole and the power source is replaced by a continuous wave that comes from a signal generator. The calibrated dipole must be placed beneath the flat phantom section of the SAM twin phantom with the correct distance holder. The distance holder should touch the phantom surface with a light pressure at the reference marking and be oriented parallel to the long side of the phantom. The equipment setup is shown below:

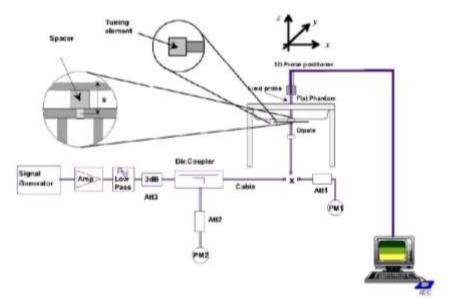


Fig.10.1 System Verification Setup Diagram



Fig.10.2 Photo of Dipole setup



> System Verification Results

Comparing to the original SAR value provided by SPEAG, the verification data should be within its specification of 10%. The table as below indicates the system performance check can meet the variation criterion and the plots can be referred to Appendix C of this report.

_	Date h/dd/yy)	Frequency (MHz)	Power fed onto dipole (mW)	Measured 10g SAR (W/kg)	Normalized to 1W 10g SAR (W/kg)	1W Target 1g SAR (W/kg)	Deviation (%)
04.1	6.2021	2450	40	2.19	54.75	52.6	4.09



11 **EUT Testing Position**

This EUT was tested in six different positions. They are Surface 1/ Surface 2/ Surface 3/ Surface 4/ Surface 5/ Surface 6 of the EUT with phantom 0 mm gap, as illustrated below, please refer to Appendix B for the test setup photos.

12 **Measurement Procedures**

The measurement procedures are as bellows:

<Conducted power measurement>

- For WWAN power measurement, use base station simulator to configure EUT WWAN transition in \geq conducted connection with RF cable, at maximum power in each supported wireless interface and frequency band.
- Read the WWAN RF power level from the base station simulator.
- For WLAN/BT power measurement, use engineering software to configure EUT WLAN/BT continuously \triangleright transmission, at maximum RF power in each supported wireless interface and frequency band.
- Connect EUT RF port through RF cable to the power meter or spectrum analyzer, and measure WLAN/BT \triangleright output power.

<Conducted power measurement>

- Use base station simulator to configure EUT WWAN transmission in radiated connection, and engineering ⊳ software to configure EUT WLAN/BT continuously transmission, at maximum RF power, in the highest power channel.
- \triangleright Place the EUT in positions as Appendix B demonstrates.
- Set scan area, grid size and other setting on the DASY software. \triangleright
- Measure SAR results for the highest power channel on each testing position. \triangleright
- ⊳ Find out the largest SAR result on these testing positions of each band.
- \triangleright Measure SAR results for other channels in worst SAR testing position if the Reported SAR or highest power channel is larger than 0.8 W/kg.

According to the test standard, the recommended procedure for assessing the peak spatial-average SAR value consists of the following steps:

- Power reference measurement
- Area scan
- Zoom scan
- Power drift measurement \triangleright

12.1 Spatial Peak SAR Evaluation

The procedure for spatial peak SAR evaluation has been implemented according to the test standard. It can be conducted for 1g and 10g, as well as for user-specific masses. The DASY software includes all numerical procedures necessary to evaluate the spatial peak SAR value.

The base for the evaluation is a "cube" measurement. The measured volume must include the 1g and 10 g cubes with the highest averaged SAR values. For that purpose, the center of the measured volume is aligned to the interpolated peak SAR value of a previously performed area scan.

The entire evaluation of the spatial peak values is performed within the post-processing engine (SEMCAD). The system always gives the maximum values for 1g and 10g cubes. The algorithm to find the cube with highest averaged SAR is divided into the following stages:

- Extraction of the measured data (grid and values) from the Zoom Scan. \triangleright
- Calculation of the SAR value at every measurement point based on all stored data (A/D values and \triangleright measurement parameters).
- Generation of a high-resolution mesh within the measured volume.
- Interpolation of all measured values form the measurement grid to the high-resolution grid \triangleright
- ≻ Extrapolation of the entire 3-D field distribution to the phantom surface over the distance from sensor to surface
- \triangleright Calculation of the averaged SAR within masses of 1g and 10g.

JianYan Testing Group Shenzhen Co., Ltd.



12.2 Power Reference Measurement

The Power Reference Measurement and Power Drift Measurement are for monitoring the power drift of the device under test in the batch process. The minimum distance of probe sensors to surface determines the closest measurement point to phantom surface. This distance cannot be smaller than the distance of sensor calibration points to probe tip as defined in the probe properties.

12.3 Area & Zoom Scan Procedures

First Area Scan is used to locate the approximate location(s) of the local peak SAR value(s). The measurement grid within an Area Scan is defined by the grid extent, grid step size and grid offset. Next, in order to determine the EM field distribution in a three-dimensional spatial extension, Zoom Scan is required. The Zoom Scan is performed around the highest E-field value to determine the averaged SAR-distribution over 10g. Area scan and zoom scan resolution setting follows KDB 865664 D01v01r04 quoted below.

		≤3 GHz	> 3 GHz
		$5 \pm 1 \mathrm{mm}$	$\frac{1}{2} \cdot \delta \cdot \ln(2) \pm 0.5 \text{ mm}$
		30° ± 1°	20°±1°
		≤ 2 GHz: ≤ 15 mm 2 - 3 GHz: ≤ 12 mm	3 – 4 GHz: ≤ 12 mm 4 – 6 GHz: ≤ 10 mm
atial resolt	ation: Δx _{Area} , Δy _{Area}	measurement plane orientation the measurement resolution in x or y dimension of the test of	on, is smaller than the above must be≤the corresponding levice with at least one
apatial reso	lution: Δx_{Zoon} , Δy_{Zoon}	≤ 2 GHz: ≤ 8 mm 2 - 3 GHz: ≤ 5 mm	3 – 4 GHz: ≤ 5 mm 4 – 6 GHz: ≤ 4 mm
uniform	grid: Az _{Zoon} (n)	≤5 mm	$\begin{array}{l} 3-4 \ \mathrm{GHz:} \leq 4 \ \mathrm{mm} \\ 4-5 \ \mathrm{GHz:} \leq 3 \ \mathrm{mm} \\ 5-6 \ \mathrm{GHz:} \leq 2 \ \mathrm{mm} \end{array}$
m 1 st two points cl		≤4 mm	$\begin{array}{l} 3-4 \text{ GHz:} \leq 3 \text{ mm} \\ 4-5 \text{ GHz:} \leq 2.5 \text{ mm} \\ 5-6 \text{ GHz:} \leq 2 \text{ mm} \end{array}$
grid	Δz _{2.com} (n>1); between subsequent points	<u>≤</u> 1.5·Δz	200m(n-1)
x, y, z		≥ 30 mm	3 – 4 GHz: ≥ 28 mm 4 – 5 GHz: ≥ 25 mm 5 – 6 GHz: ≥ 22 mm
	obe sensor from prob leasureme atial resolu- spatial resolu- uniform graded grid	grid Δz _{2.com} (n>1); between subsequent points	$\frac{1}{10000000000000000000000000000000000$



12.4 Volume Scan Procedures

The volume scan is used for assess overlapping SAR distributions for antennas transmitting in different frequency bands. It is equivalent to an oversized zoom scan used in standalone measurements. The measurement volume will be used to enclose all the simultaneous transmitting antennas. For antennas transmitting simultaneously in different frequency bands, the volume scan is measured separately in each frequency band. In order to sum correctly to compute the 1g aggregate SAR, the EUT remain in the same test position for all measurements and all volume scan use the same spatial resolution and grid spacing. When all volume scan were completed, the software, SEMCAD post-processor scan combine and subsequently superpose these measurement data to calculating the multiband SAR.

12.5 SAR Averaged Methods

In DASY, the interpolation and extrapolation are both based on the modified Quadratic Shepard's method. The interpolation scheme combines a least-square fitted function method and a weighted average method which are the two basic types of computational interpolation and approximation.

Extrapolation routines are used to obtain SAR values between the lowest measurement points and the inner phantom surface. The extrapolation distance is determined by the surface detection distance and the probe sensor offset. The uncertainty increases with the extrapolation distance. To keep the uncertainty within 1% for the 1g and 10g cubes, the extrapolation distance should not be larger than 5 mm.

12.6 Power Drift Monitoring

All SAR testing is under the EUT install full charged battery and transmit maximum output power. In DASY measurement software, the power reference measurement and power drift measurement procedures are used for monitoring the power drift of EUT during SAR test. Both these procedures measure the field at a specified reference position before and after the SAR testing. The software will calculate the field difference in dB. If the power drifts more than 5%, the SAR will be retested.



13 Conducted RF Output Power

13.1 WLAN 2.4 GHz Band Conducted Power

Average Power (dBm)									
Channel	Frequency (MHz)	802.11 b	802.11 g	802.11n (HT20)					
CH 01	2412	7.70	7.36	7.19					
CH 06	2437	8.46	8.91	8.68					
CH 11	2462	9.51	10.59	10.33					

Average Power (dBm)							
Channel	Frequency (MHz)	802.11n (HT40)					
CH 03	2422	8.14					
CH 06	2437	9.08					
CH 09	2452	10.05					

Note:

1. Per KDB 248227 D01v02r02, choose the highest output power channel to test SAR and determine further SAR exclusion.

Per KDB 248227 D01v02r02, In the 2.4 GHz band, separate SAR procedures are applied to DSSS and OFDM configurations to simplify DSSS test requirements. SAR is not required for the following 2.4 GHz OFDM conditions:
 1) When KDB Publication 447498 SAR test exclusion applies to the OFDM configuration.
 2) When the highest reported SAR for DSSS is adjusted by the ratio of OFDM to DSSS specified maximum output power and the adjusted SAR is ≤ 1.2 W/kg.

- 3. The output power of all data rate were pre-scan, just the worst case (the lowest data rate) of all mode were shown in report.
- 4. Per KDB 248227 D01V02r02 section 2.2, when the EUT in continuously transmitting mode, the actual duty cycle is 99.76%, so the duty cycle factor is 1.01.



14 Exposure Positions Consideration

14.1 EUT Antenna Locations

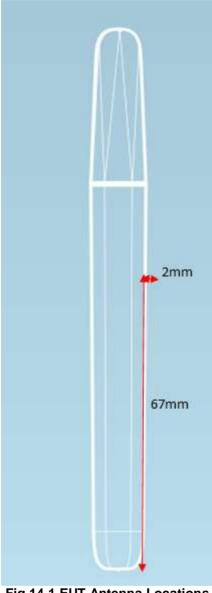


Fig.14.1 EUT Antenna Locations

Note: This antenna diagram is only used as a reference for the distance from the antenna to each edge. For the specific shape of the antenna, please refer to the physical photo.



14.2 Test Positions Consideration

	Distance of Antennas to EUT edge/surface Test distance: 0mm									
Antennas – Surtace 1 – Surtace 2 – Surtace 3 – Surtace 4 – Surtace 5 – Surtace 6 – Lon Side								Bottom Side		
WLAN <25mm <25mm <25mm <25mm <25mm 67mm										

	Test Positions Test distance: 0mm									
Antennas Surface 1 Surface 2 Surface 3 Surface 4 Surface 5 Surface 6 Top Side Bottom Side								Bottom Side		
WLAN Yes Yes Yes Yes Yes No No										



15 SAR Test Results Summary

15.1 Standalone Body SAR

WLAN 2.4GHz Body SAR

Plot No.	Band/Mode	Test Position	CH.	Freq. (MHz)	Ave. Power (dBm)	Power Drift (dB)	Tune-Up Limit (dBm)	Meas. SAR _{1g} (W/kg)	Scaling Factor	D.C Factor	Reported SAR _{1g} (W/kg)
1	2.4GHz/802.11b	Surface 1	11	2462	9.51	-0.01	10.0	0.096	1.119	1.01	0.108
	2.4GHz/802.11b	Surface 2	11	2462	9.51	0.11	10.0	0.009	1.119	1.01	0.010
	2.4GHz/802.11b	Surface 3	11	2462	9.51	-0.09	10.0	0.013	1.119	1.01	0.015
	2.4GHz/802.11b	Surface 4	11	2462	9.51	0.16	10.0	0.007	1.119	1.01	0.008
	2.4GHz/802.11b	Surface 5	11	2462	9.51	0.02	10.0	0.011	1.119	1.01	0.012
	2.4GHz/802.11b	Surface 6	11	2462	9.51	0.17	10.0	0.062	1.119	1.01	0.070
ANSI / IEEE C95.1 – SAFETY LIMIT Spatial Peak Uncontrolled Exposure/General Population							N/kg (mV aged ove				

Note:

1. Per KDB 447498 D01v06, for each exposure position, if the highest output channel Reported SAR ≤0.8W/kg, other channels SAR testing is not necessary.

2. Per KDB 865664 D01v01r04, for each frequency band, repeated SAR measurement is required when the measured SAR is ≥0.8W/kg.

3. According to KDB 865664 D02v01r02, SAR plot is required for the highest measured SAR in each exposure configuration, wireless mode and frequency band combination.



15.2 Measurement Uncertainty

The component of uncertainly may generally be categorized according to the methods used to evaluate them. The evaluation of uncertainly by the statistical analysis of a series of observations is termed a Type A evaluation of uncertainty. The evaluation of uncertainty by means other than the statistical analysis of a series of observation is termed a Type B evaluation of uncertainty. Each component of uncertainty, however evaluated, is represented by an estimated standard deviation, termed standard uncertainty, which is determined by the positive square root of the estimated variance.

A Type A evaluation of standard uncertainty may be based on any valid statistical method for treating data. This includes calculating the standard deviation of the mean of a series of independent observations; using the method of least squares to fit a curve to the data in order to estimate the parameter of the curve and their standard deviations; or carrying out an analysis of variance in order to identify and quantify random effects in certain kinds of measurement.

A Type B evaluation of standard uncertainty is typically based on scientific judgment using all of the relevant information available. These may include previous measurement data, experience, and knowledge of the behavior and properties of relevant materials and instruments, manufacture's specification, data provided in calibration reports and uncertainties assigned to reference data taken from handbooks. Broadly speaking, the uncertainty is either obtained from an outdoor source or obtained from an assumed distribution, such as the normal distribution, rectangular or triangular distributions indicated in below Table.

Uncertainty Distributions	Normal	Rectangular	Triangular	U-Shape
Multi-plying Factor	1/k(b)	1/√3	1/√6	1/√2

Standard Uncertainty for Assumed Distribution

The combined standard uncertainty of the measurement result represents the estimated standard deviation of the result. It is obtained by combining the individual standard uncertainties of both Type A and Type B evaluation using the usual "root-sum-squares" (RSS) methods of combining standard deviations by taking the positive square root of the estimated variances.

Expanded uncertainty is a measure of uncertainty that defines an interval about the measurement result within which the measured value is confidently believed to lie. It is obtained by multiplying the combined standard uncertainty by a coverage factor. Typically, the coverage factor ranges from 2 to 3. Using a coverage factor allows the true value of a measured quantity to be specified with a defined probability within the specified uncertainty range. For purpose of this document, a coverage factor two is used, which corresponds to confidence interval of about 95 %. The DASY uncertainty Budget is shown in the following tables.



Report No: JYTSZB-R14-2100055

Uncertainty Component	Section	Uncert. Value	Prob. Dist.	Div.	(C _i) (1 g)	(C _i) (10 g)	Std. Unc. (1 g)	Std. Unc. (10 g)	Vi
Measurement System									
Probe Calibration	E.2.1	±7.4%	N	1	1	1	±7.4%	±7.4%	∞
Axial Isotropy	E.2.2	±1.2%	R	√3	0.7	0.7	±0.49%	±0.49%	8
Hemispherical Isotropy	E.2.2	±3.2%	R	√3	0.7	0.7	±1.29%	±1.29%	∞
Boundary Effects	E.2.3	±1.0%	R	√3	1	1	±0.58%	±0.58%	∞
Linearity	E.2.4	±0.9%	R	√3	1	1	±0.52%	±0.52%	∞
System Detection Limits	E.2.5	±0.25%	R	√3	1	1	±0.14%	±0.14%	∞
Readout Electronics	E.2.6	±0.3%	Ν	1	1	1	±0.3%	±0.3%	8
Response Time	E.2.7	±0.8%	R	√3	1	1	±0.46%	±0.46%	∞
Integration Time	E.2.8	±2.6%	R	√3	1	1	±1.5%	±1.5%	∞
RF Ambient Noise	E.6.1	±3.0%	R	√3	1	1	±1.73%	±1.73%	∞
RF Ambient Reflections	E.6.1	±3.0%	R	√3	1	1	±1.73%	±1.73%	∞
Probe positioner mechanical tolerances	E.6.2	±0.4%	R	√3	1	1	±0.23%	±0.23%	∞
Probe positioning tolerance with respect to the phantom shell surface	E.6.3	±2.9%	R	$\sqrt{3}$	1	1	±1.68%	±1.68%	ø
Interpolation, extrapolation, and integration algorithm For max. SAR Evaluation.	E.5	±1.0%	R	√3	1	1	±0.58%	±0.58%	œ
Test Sample Related									r
Device Positioning	E.4.2	±4.6%	N	1	1	1	±4.6%	±4.6%	M-1
Device Holder	E.4.1	±5.2%	N	1	1	1	±5.2%	±5.2%	M-1
Power Drift	6.6.2	±5.0%	R	√3	1	1	±2.89%	±2.89%	∞
Phantom and Setup								L	
Phantom Uncertainty	E.3.1	±4.0%	R	$\sqrt{3}$	1	1	±2.31%	±2.31%	∞
Liquid conductivity (measured value)	E.3.3	±2.97%	Ν	1	0.78	0.71	±2.32%	±2.11%	М
Liquid dielectric constant (measured value)	E.3.3	±3.08%	Ν	1	0.23	0.26	±0.71%	±0.8%	М
Liquid Conductivity - Temperature Uncertainty	E.3.4	±1.3%	R	√3	0.78	0.71	±0.59%	±0.53%	∞
Liquid Dielectric Constant - Temperature Uncertainty	E.3.4	±1.1%	R	√3	0.23	0.26	±0.15%	±0.17%	∞
Combined Standard Uncertainty (RSS)							±11.55%	±11.51%	
Expanded Uncertainty (95% Confidence Level, k = 2)							±23.11%	±23.01%	

Uncertainty Budget for frequency range 300 MHz to 3 GHz according to IEEE1528-2003



15.3 Measurement Conclusion

The SAR evaluation indicates that the EUT complies with the RF radiation exposure limits of the FCC and Industry Canada, with respect to all parameters subject to this test. These measurements were taken to simulate the RF effects of RF exposure under worst-case conditions. Precise laboratory measures were taken to assure repeatability of the tests. The results and statements relate only to the item(s) tested. Please note that the absorption and distribution of electromagnetic energy in the body are very complex phenomena that depend on the mass, shape, and size of the body, the orientation of the body with respect to the field vectors, and the electrical properties of both the body and the environment. Other variables that may play a substantial role in possible biological effects are those that characterize the environment (e.g. ambient temperature, air velocity, relative humidity, and body insulation) and those that characterize the individual (e.g. age, gender, activity level, debilitation, or disease). Because various factors may interact with one another to vary the specific biological outcome of an exposure to electromagnetic fields, any protection guide should consider maximal amplification of biological effects as a result of field-body interactions, environmental conditions, and physiological variables.



16 Reference

- [1]. FCC 47 CFR Part 2 "Frequency Allocations and Radio Treaty Matters; General Rules and Regulations"
- [2]. ANSI/IEEE Std. C95.1-1992, "IEEE Standard for Safety Levels with Respect to Human Exposure to Radio Frequency Electromagnetic Fields, 3 kHz to 300 GHz", September 1992
- [3]. IEEE Std. 1528-2003, "Recommended Practice for Determining the Peak Spatial-Average Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- [4]. SPEAG DASY52 System Handbook
- [5]. FCC KDB 248227 D01 v02r02, "SAR GUIDANCE FOR IEEE 802.11 (Wi-Fi) TRANSMITTERS", October 2015
- [6]. FCC KDB 447498 D01 v06, "RF EXPOSURE PROCEDURES AND EQUIPMENT AUTHORIZATION POLICIES FOR MOBILE AND PORTABLE DEVICES", October 2015
- [7]. FCC KDB 616217 D04 v01r02, "SAR EVALUATION CONSIDERATIONS FOR LAPTOP, NOTEBOOK, NETBOOK AND TABLET COMPUTERS", October 2015
- [8]. FCC KDB 648474 D04 v01r03, "SAR EVALUATION CONSIDERATIONS FOR WIRELESS HANDSETS", October 2015
- [9]. FCC KDB 941225 D01 v03r01, "3G SAR MEAUREMENT PROCEDURES", October 2015
- [10]. FCC KDB 941225 D03 v01, "Recommended SAR Test Reduction Procedures for GSM / GPRS / EDGE", December 2008
- [11]. FCC KDB 941225 D06 v02r01, " SAR EVALUATION PROCEDURES FOR PORTABLE DEVICES WITH WIRELESS ROUTER CAPABILITIES", October 2015
- [12]. FCC KDB 865664 D01 v01r04, "SAR MEASUREMENT REQUIREMENTS FOR 100 MHz TO 6 GHz", August 2015



Appendix A: Plots of SAR System Check



Test Laboratory: JYTSZ

Date/Time: 04.16.2021 08:18:42

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: SN:910

Communication System: UID 0, CW (0); Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz; $\sigma = 1.845$ S/m; $\epsilon_r = 38.823$; $\rho = 1000$ kg/m³ Phantom section: Flat Section


DASY5 Configuration:

- Probe: EX3DV4 SN3924; ConvF(7.58, 7.58, 7.58) @ 2450 MHz; Calibrated: 09.23.2020;
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1373; Calibrated: 07.27.2020
- Phantom: SAM 5.0; Type: QD000P40CD; Serial: TP:1765
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

System Performance Check at Frequency 2450MHz Head Tissue/d=10mm, Pin=40 mW, dist=2.0mm (EX-Probe)/Area Scan (51x61x1): Interpolated grid: dx=1.200 mm, dy=1.200 mm Maximum value of SAR (interpolated) = 3.91 W/kg

System Performance Check at Frequency 2450MHz Head Tissue/d=10mm, Pin=40 mW, dist=2.0mm (EX-Probe)/Zoom Scan (7x7x7) (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mmReference Value = 43.46 V/m; Power Drift = 0.09 dB Peak SAR (extrapolated) = 4.93 W/kg SAR(1 g) = 2.19 W/kg; SAR(10 g) = 0.987 W/kg Smallest distance from peaks to all points 3 dB below = 8 mm Ratio of SAR at M2 to SAR at M1 = 42.8% Maximum value of SAR (measured) = 3.44 W/kg

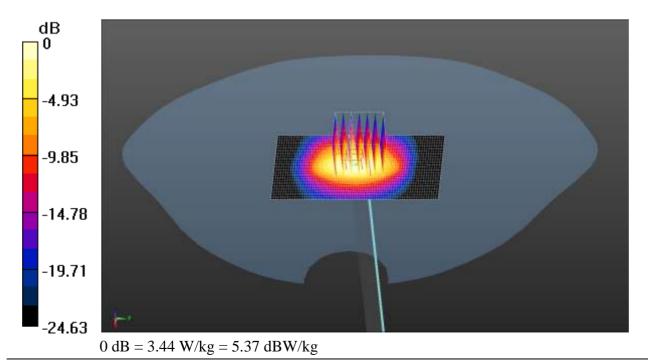



Appendix B: Plots of SAR Test Data



Test Laboratory: JYTSZ

Date/Time: 04.16.2021 21:59:18

DUT: Intelligent visible pore cleaner; Type: wisdom; Serial: 1#

Communication System: UID 0, IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps) (0); Frequency: 2462 MHz; Duty Cycle: 1:1 Medium parameters used (interpolated): f = 2462 MHz; $\sigma = 1.853$ S/m; $\varepsilon_r = 38.674$; $\rho = 1000$ kg/m³ Phantom section: Flat Section

DASY5 Configuration:


- Probe: EX3DV4 SN3924; ConvF(7.58, 7.58, 7.58) @ 2462 MHz; Calibrated: 09.23.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection) •
- Electronics: DAE4 Sn1373; Calibrated: 07.27.2020
- Phantom: SAM 5.0; Type: QD000P40CD; Serial: TP:1765 •
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

WIFI Body Surface 1/High Channel/Area Scan (31x61x1): Interpolated grid:

dx=1.200 mm, dy=1.200 mm Maximum value of SAR (interpolated) = 0.192 W/kg

WIFI Body Surface 1/High Channel/Zoom Scan (5x5x7)/Cube 0: Measurement

grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 8.623 V/m; Power Drift = -0.01 dB Peak SAR (extrapolated) = 0.209 W/kgSAR(1 g) = 0.096 W/kg; SAR(10 g) = 0.041 W/kgSmallest distance from peaks to all points 3 dB below = 5.8 mm Ratio of SAR at M2 to SAR at M1 = 53.3%Maximum value of SAR (measured) = 0.164 W/kg

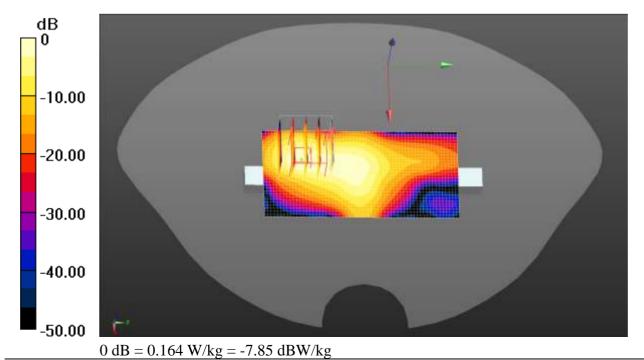

JianYan Testing Group Shenzhen Co., Ltd. Project No.: JYTSZE2104015 No.101, Building 8, Innovation Wisdom Port, No.155 Hongtian Road, Huangpu Community, Xingiao Street, Bao'an District, Shenzhen, Guangdong, People's Republic of China. Telephone: +86 (0) 755 23118282 Fax: +86 (0) 755 23116366, E-mail: info@ccis-cb.com



Appendix C: System Calibration Certificate



Calibration information for E-field probes

	CALIBRATION LI toad, Haidian District, B		CALIBRAT CNAS LOS
Tel: +86-10-62304633- E-mail: cttl@chinattl.co		62304633-2504 hinattl.cn	
Client CCIS		Certificate No:	Z20-60314
CALIBRATION CEP	RTIFICATE		ine stagen
Dbject	EX3DV4 - S	N : 3924	
Calibration Procedure(s)	FF-Z11-004-	02	
	Calibration F	Procedures for Dosimetric E-field Probes	
Calibration date:	September 2	23, 2020	
Il calibrations have been o umidity<70%. Calibration Equipment used (N		closed laboratory facility: environment t	emperature(22±3)℃ and
umidity<70%.			emperature(22±3)°C and Scheduled Calibration
umidity<70%. Calibration Equipment used (N	M&TE critical for ca	libration)	
umidity<70%. alibration Equipment used (M rimary Standards Power Meter NRP2	M&TE critical for ca	libration) Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration
umidity<70%. Calibration Equipment used (M Primary Standards Power Meter NRP2 Power sensor NRP-Z91	M&TE critical for ca ID # 101919	libration) Cal Date(Calibrated by, Certificate No.) 16-Jun-20(CTTL, No.J20X04344)	Scheduled Calibration Jun-21
umidity<70%. Calibration Equipment used (N Primary Standards	M&TE critical for ca ID # 101919 101547 101548	libration) Cal Date(Calibrated by, Certificate No.) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344)	Scheduled Calibration Jun-21 Jun-21
umidity<70%. Calibration Equipment used (M Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91	M&TE critical for ca ID # 101919 101547 101548 18N50W-10dB	libration) Cal Date(Calibrated by, Certificate No.) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344)	Scheduled Calibration Jun-21 Jun-21 Jun-21
umidity<70%. Calibration Equipment used (M Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 10dBAttenuator	M&TE critical for ca ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB	libration) Cal Date(Calibrated by, Certificate No.) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 10-Feb-20(CTTL, No.J20X00525)	Scheduled Calibration Jun-21 Jun-21 Jun-21 Feb-22 Feb-22
umidity<70%. Calibration Equipment used (M Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 10dBAttenuator Reference 20dBAttenuator	M&TE critical for ca ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB	libration) Cal Date(Calibrated by, Certificate No.) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 10-Feb-20(CTTL, No.J20X00525) 10-Feb-20(CTTL, No.J20X00526)	Scheduled Calibration Jun-21 Jun-21 Jun-21 Feb-22 Feb-22 20) May-21
umidity<70%. Calibration Equipment used (M Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 10dBAttenuator Reference 20dBAttenuator Reference Probe EX3DV4	M&TE critical for ca ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7307	libration) Cal Date(Calibrated by, Certificate No.) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 10-Feb-20(CTTL, No.J20X00525) 10-Feb-20(CTTL, No.J20X00526) 29-May-20(SPEAG, No.EX3-7307_May	Scheduled Calibration Jun-21 Jun-21 Jun-21 Feb-22 Feb-22 20) May-21
umidity<70%. alibration Equipment used (M rimary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 10dBAttenuator Reference 20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards	M&TE critical for ca ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7307 SN 1556 ID #	libration) Cal Date(Calibrated by, Certificate No.) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 10-Feb-20(CTTL, No.J20X04344) 10-Feb-20(CTTL, No.J20X00525) 10-Feb-20(CTTL, No.J20X00526) 29-May-20(SPEAG, No.EX3-7307_May 4-Feb-20(SPEAG, No.DAE4-1556_Feb2	Scheduled Calibration Jun-21 Jun-21 Jun-21 Feb-22 Feb-22 20) May-21 20) Feb-21
umidity<70%. alibration Equipment used (M rimary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 10dBAttenuator Reference 20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGenerator MG3700A	M&TE critical for ca ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7307 SN 1556 ID #	libration) Cal Date(Calibrated by, Certificate No.) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 10-Feb-20(CTTL, No.J20X00525) 10-Feb-20(CTTL, No.J20X00526) 29-May-20(SPEAG, No.EX3-7307_May 4-Feb-20(SPEAG, No.DAE4-1556_Feb2 Cal Date(Calibrated by, Certificate No.)	Scheduled Calibration Jun-21 Jun-21 Jun-21 Feb-22 Feb-22 20) May-21 20) Feb-21 Scheduled Calibration
umidity<70%. Calibration Equipment used (M Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 10dBAttenuator Reference 20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGenerator MG3700A Network Analyzer E5071C	M&TE critical for ca ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7307 SN 1556 ID # A 6201052605	libration) Cal Date(Calibrated by, Certificate No.) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 10-Feb-20(CTTL, No.J20X00525) 10-Feb-20(CTTL, No.J20X00526) 29-May-20(SPEAG, No.EX3-7307_May: 4-Feb-20(SPEAG, No.DAE4-1556_Feb2 Cal Date(Calibrated by, Certificate No.) 23-Jun-20(CTTL, No.J20X04343)	Scheduled Calibration Jun-21 Jun-21 Jun-21 Feb-22 Feb-22 20) May-21 20) Feb-21 Scheduled Calibration Jun-21
aumidity<70%. Calibration Equipment used (N Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 10dBAttenuator Reference 20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGenerator MG3700A Network Analyzer E5071C	M&TE critical for cal ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7307 SN 1556 ID # 4 6201052605 MY46110673	libration) Cal Date(Calibrated by, Certificate No.) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 10-Feb-20(CTTL, No.J20X00525) 10-Feb-20(CTTL, No.J20X00526) 29-May-20(SPEAG, No.EX3-7307_May 4-Feb-20(SPEAG, No.DAE4-1556_Feb2 Cal Date(Calibrated by, Certificate No.) 23-Jun-20(CTTL, No.J20X04343) 10-Feb-20(CTTL, No.J20X00515)	Scheduled Calibration Jun-21 Jun-21 Jun-21 Feb-22 Feb-22 20) May-21 20) Feb-21 Scheduled Calibration Jun-21 Feb-21
Aumidity<70%. Calibration Equipment used (M Primary Standards Power Meter NRP2 Power sensor NRP-Z91 Power sensor NRP-Z91 Reference 10dBAttenuator Reference 20dBAttenuator Reference Probe EX3DV4 DAE4 Secondary Standards SignalGenerator MG3700A Network Analyzer E5071C N Calibrated by:	M&TE critical for ca ID # 101919 101547 101548 18N50W-10dB 18N50W-20dB SN 7307 SN 1556 ID # Colored for the second sec	libration) Cal Date(Calibrated by, Certificate No.) 16-Jun-20(CTTL, No.J20X04344) 16-Jun-20(CTTL, No.J20X04344) 10-Feb-20(CTTL, No.J20X00525) 10-Feb-20(CTTL, No.J20X00526) 29-May-20(SPEAG, No.EX3-7307_May 4-Feb-20(SPEAG, No.DAE4-1556_Feb2 Cal Date(Calibrated by, Certificate No.) 23-Jun-20(CTTL, No.J20X04343) 10-Feb-20(CTTL, No.J20X00515) Function	Scheduled Calibration Jun-21 Jun-21 Jun-21 Feb-22 Feb-22 20) May-21 20) Feb-21 Scheduled Calibration Jun-21 Feb-21

Certificate No: Z20-60314

Page 1 of 10





Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com Http://www.chinattl.cn

Glossary:

tissue simulating liquid
sensitivity in free space
sensitivity in TSL / NORMx,y,z
diode compression point
crest factor (1/duty_cycle) of the RF signal
modulation dependent linearization parameters
Φ rotation around probe axis
θ rotation around an axis that is in the plane non

normal to probe axis (at measurement center), i θ=0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques®, June 2013
- b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010

d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORMX, y, z: Assessed for E-field polarization 0=0 (f≤900MHz in TEM-cell; f>1800MHz; waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not effect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z* frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx, y,z: DCP are numerical linearization parameters assessed based on the data of power sweep (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- Ax,y,z; Bx,y,z; Cx,y,z; VRx,y,z:A,B,C are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f≤800MHz) and inside waveguide using analytical field distributions based on power measurements for f >800MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty valued are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z* ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from±50MHz to±100MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No:Z20-60314

Page 2 of 10





Tel: +86-10-62304633-2512 E-mail: cttl@chinattl.com Http://www.chinattl.cn

DASY/EASY – Parameters of Probe: EX3DV4 – SN:3924

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm(µV/(V/m) ²) ^A	0.50	0.42	0.67	±10.0%
DCP(mV) ⁸	101.3	100.1	99.8	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dBõV	C	D dB	VR mV	Unc ^E (k=2)
0	CW	x	0.0	0.0	1.0	0.00	172.6	±1.9%
		Y	0.0	0.0	1.0		149.2	
		Z	0.0	0.0	1.0		200.0	

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X, Y, Z do not affect the E²-field uncertainty inside TSL (see Page 4 and Page 5). ⁸ Numerical linearization parameter: uncertainty not required.

E Uncertainly is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

Certificate No:Z20-60314

Page 3 of 10





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2512
 Fax: +86-10-62304633-2504

 E-mail: ettl@chinattl.com
 Http://www.chinattl.cn

DASY/EASY – Parameters of Probe: EX3DV4 – SN:3924

f [MHz] ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	41.9	0.89	10.11	10.11	10.11	0.40	0.75	±12.1%
835	41.5	0.90	9.71	9.71	9.71	0.18	1.20	±12.1%
900	41.5	0.97	9.67	9.67	9.67	0.21	1.15	±12.1%
1750	40.1	1.37	8.43	8.43	8.43	0.20	1.11	±12.1%
1900	40.0	1.40	8.14	8.14	8.14	0.22	1.14	±12.1%
2300	39.5	1.67	7.83	7.83	7.83	0.48	0.72	±12.1%
2450	39.2	1.80	7.58	7.58	7.58	0.50	0.75	±12.1%
2600	39.0	1.96	7.35	7.35	7.35	0.60	0.69	±12.1%
5250	35.9	4.71	5.42	5.42	5.42	0.45	1.32	±13.3%
5600	35.5	5.07	4.85	4.85	4.85	0.50	1.20	±13.3%
5750	35.4	5.22	4.96	4.96	4.96	0.55	1.20	±13.3%

Calibration Parameter Determined in Head Tissue Simulating Media

^c Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

^F At frequency below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters. ^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No:Z20-60314

Page 4 of 10





E-mail: cttl@chinattl.com

Fax: +86-10-62304633-25 Http://www.chinattl.cn

DASY/EASY – Parameters of Probe: EX3DV4 – SN:3924

f [MHz] ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (<i>k</i> =2)
750	55.5	0.96	10.06	10.06	10.06	0.40	0.82	±12.1%
835	55.2	0.97	9.70	9.70	9.70	0.18	1.36	±12.1%
900	55.0	1.05	9.72	9.72	9.72	0.28	1.04	±12.1%
1750	53.4	1.49	8.16	8.16	8.16	0.20	1.28	±12.1%
1900	53.3	1.52	7.78	7.78	7.78	0.21	1.34	±12.1%
2300	52.9	1.81	7.65	7.65	7.65	0.47	0.85	±12.1%
2450	52.7	1.95	7.50	7.50	7.50	0.55	0.78	±12.1%
2600	52.5	2.16	7.29	7.29	7.29	0.66	0.69	±12.1%
5250	48.9	5.36	4.86	4.86	4.86	0.50	1.40	±13.3%
5600	48.5	5.77	4.24	4.24	4.24	0.60	1.30	±13.3%
5750	48.3	5.94	4.35	4.35	4.35	0.55	1.45	±13.3%

Calibration Parameter Determined in Body Tissue Simulating Media


^c Frequency validity above 300 MHz of ±100MHz only applies for DASY v4.4 and higher (Page 2), else it is restricted to ±50MHz. The uncertainty is the RSS of ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

F At frequency below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ±10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ±5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.
^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for the frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No:Z20-60314

Page 5 of 10



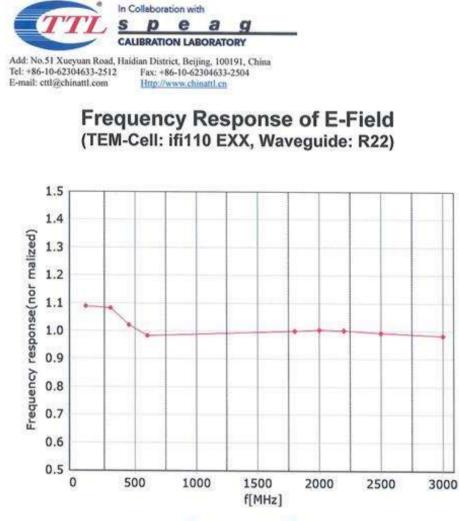




Uncertainty of Frequency Response of E-field: ±7.4% (k=2)

Certificate No:Z20-60314

Page 6 of 10



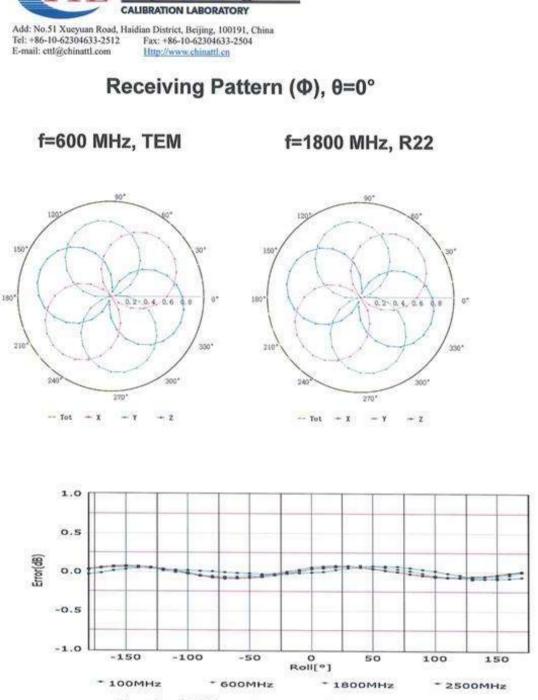

In Collaboration with

p

e

a


S

Uncertainty of Axial Isotropy Assessment: ±1.2% (k=2)


Certificate No:Z20-60314

Page 7 of 10




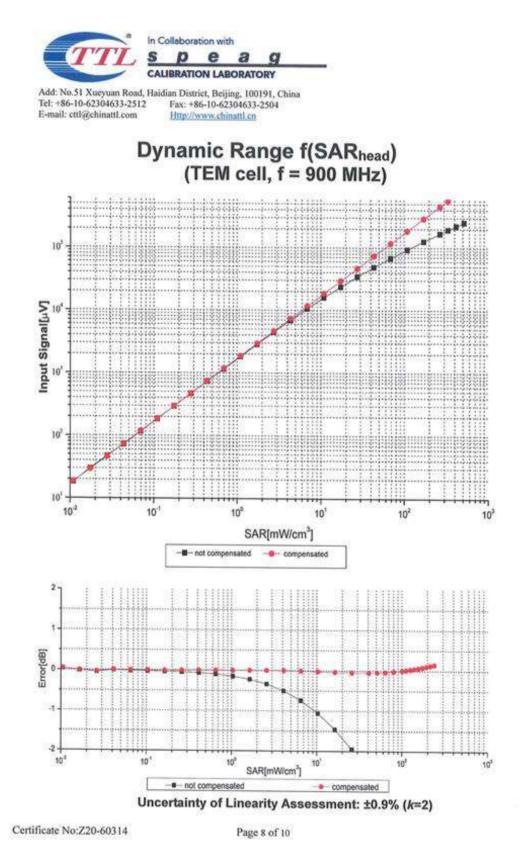



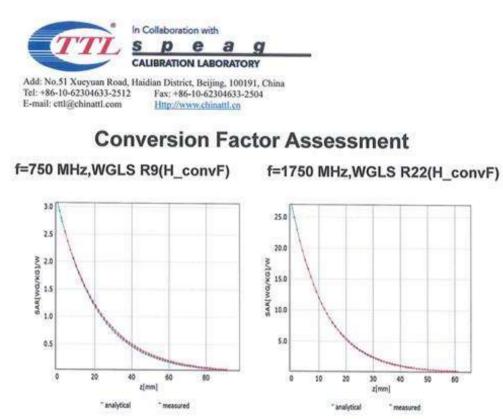

Deviation from Isotropy in Liquid



Uncertainty of Spherical Isotropy Assessment: ±3.2% (k=2)

Certificate No:Z20-60314

Page 9 of 10





DASY/EASY – Parameters of Probe: EX3DV4 – SN:3924

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	159
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disable
Probe Overall Length	337mm
Probe Body Diameter	10mm
Tip Length	10mm
Tip Diameter	2.5mm
Probe Tip to Sensor X Calibration Point	1mm
Probe Tip to Sensor Y Calibration Point	1mm
Probe Tip to Sensor Z Calibration Point	1mm
Recommended Measurement Distance from Surface	1.4mm

Certificate No:Z20-60314

Page 10 of 10




Calibration information for Dipole

E-mail: cttl@chinatt Client CCIS	ALCONTROL OF	www.chinattl.cn	
Client Colo		Certificate No: Z19	-60177
		2.2	5-00177
CALIBRATION CE	ERTIFICAT		
Object	D2450	/2 - SN: 910	
Calibration Procedure(s)	FF-Z11	-003-01	
		tion Procedures for dipole validation kits	
Calibration date:	June 10), 2019	
pages and are part of the ce	ertificate.		are given on the following
	conducted in	the closed laboratory facility: environment	
All calibrations have been humidity<70%. Calibration Equipment used	conducted in	the closed laboratory facility: environment	
All calibrations have been numidity<70%. Calibration Equipment used	conducted in	the closed laboratory facility: environment or calibration)	temperature(22±3)で and
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards	(M&TE critical for	the closed laboratory facility: environment or calibration) Cal Date(Calibrated by, Certificate No.)	temperature(22±3)℃ and Scheduled Calibration
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2	Conducted in (M&TE critical fe ID # 106277 104291	the closed laboratory facility: environment or calibration) Cal Date(Calibrated by, Certificate No.) 20-Aug-18 (CTTL, No.J18X06862)	temperature(22±3)℃ and Scheduled Calibration Aug-19
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S	Conducted in (M&TE critical fe ID # 106277 104291	the closed laboratory facility: environment or calibration) Cal Date(Calibrated by, Certificate No.) 20-Aug-18 (CTTL, No.J18X06862) 20-Aug-18 (CTTL, No.J18X06862)	temperature(22±3)℃ and Scheduled Calibration Aug-19 Aug-19
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4	Conducted in (M&TE critical fe ID # 106277 104291 SN 7514	the closed laboratory facility: environment or calibration) Cal Date(Calibrated by, Certificate No.) 20-Aug-18 (CTTL, No.J18X06862) 20-Aug-18 (CTTL, No.J18X06862) 27-Aug-18 (SPEAG,No.EX3-7514_Aug18) 20-Aug-18 (SPEAG,No.DAE4-1556_Aug18)	temperature(22±3)℃ and Scheduled Calibration Aug-19 Aug-19 Aug-19
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4	Conducted in (M&TE critical for ID # 106277 104291 SN 7514 SN 1556	the closed laboratory facility: environment or calibration) Cal Date(Calibrated by, Certificate No.) 20-Aug-18 (CTTL, No.J18X06862) 20-Aug-18 (CTTL, No.J18X06862) 27-Aug-18(SPEAG,No.EX3-7514_Aug18)	temperature(22±3)℃ and Scheduled Calibration Aug-19 Aug-19 Aug-19 Aug-19
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards	Conducted in (M&TE critical fe 106277 104291 SN 7514 SN 1556 ID #	the closed laboratory facility: environment or calibration) Cal Date(Calibrated by, Certificate No.) 20-Aug-18 (CTTL, No.J18X06862) 20-Aug-18 (CTTL, No.J18X06862) 27-Aug-18 (SPEAG,No.EX3-7514_Aug18) 20-Aug-18 (SPEAG,No.DAE4-1556_Aug18) Cal Date(Calibrated by, Certificate No.)	temperature(22±3)℃ and Scheduled Calibration Aug-19 Aug-19 Aug-19 Aug-19 Aug-19 Scheduled Calibration
All calibrations have been humidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	conducted in (M&TE critical fe 106277 104291 SN 7514 SN 1556 ID # MY49071430 MY46110673	the closed laboratory facility: environment or calibration) Cal Date(Calibrated by, Certificate No.) 20-Aug-18 (CTTL, No.J18X06862) 20-Aug-18 (CTTL, No.J18X06862) 27-Aug-18 (SPEAG,No.EX3-7514_Aug18) 20-Aug-18 (SPEAG,No.DAE4-1556_Aug18) Cal Date(Calibrated by, Certificate No.) 23-Jan-19 (CTTL, No.J19X00336) 24-Jan-19 (CTTL, No.J19X00547)	temperature(22±3)℃ and Scheduled Calibration Aug-19 Aug-19 Aug-19 Aug-19 Scheduled Calibration Jan-20 Jan-20
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	Conducted in (M&TE critical for 106277 104291 SN 7514 SN 1556 ID # MY49071430 MY46110673 Name	the closed laboratory facility: environment or calibration) Cal Date(Calibrated by, Certificate No.) 20-Aug-18 (CTTL, No.J18X06862) 20-Aug-18 (CTTL, No.J18X06862) 27-Aug-18 (SPEAG,No.EX3-7514_Aug18) 20-Aug-18 (SPEAG,No.DAE4-1556_Aug18) 20-Aug-18 (SPEAG,No.DAE4-1556_Aug18) Cal Date(Calibrated by, Certificate No.) 23-Jan-19 (CTTL, No.J19X00336) 24-Jan-19 (CTTL, No.J19X00547) Function	temperature(22±3)℃ and Scheduled Calibration Aug-19 Aug-19 Aug-19 Aug-19 Scheduled Calibration Jan-20
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C	conducted in (M&TE critical fe 106277 104291 SN 7514 SN 1556 ID # MY49071430 MY46110673	the closed laboratory facility: environment or calibration) Cal Date(Calibrated by, Certificate No.) 20-Aug-18 (CTTL, No.J18X06862) 20-Aug-18 (CTTL, No.J18X06862) 27-Aug-18 (SPEAG,No.EX3-7514_Aug18) 20-Aug-18 (SPEAG,No.DAE4-1556_Aug18) Cal Date(Calibrated by, Certificate No.) 23-Jan-19 (CTTL, No.J19X00336) 24-Jan-19 (CTTL, No.J19X00547)	temperature(22±3)℃ and Scheduled Calibration Aug-19 Aug-19 Aug-19 Aug-19 Scheduled Calibration Jan-20 Jan-20
All calibrations have been numidity<70%. Calibration Equipment used Primary Standards Power Meter NRP2 Power sensor NRP8S Reference Probe EX3DV4 DAE4 Secondary Standards Signal Generator E4438C NetworkAnalyzer E5071C	Conducted in (M&TE critical for 106277 104291 SN 7514 SN 1556 ID # MY49071430 MY46110673 Name	the closed laboratory facility: environment or calibration) Cal Date(Calibrated by, Certificate No.) 20-Aug-18 (CTTL, No.J18X06862) 20-Aug-18 (CTTL, No.J18X06862) 27-Aug-18 (SPEAG,No.EX3-7514_Aug18) 20-Aug-18 (SPEAG,No.DAE4-1556_Aug18) 20-Aug-18 (SPEAG,No.DAE4-1556_Aug18) Cal Date(Calibrated by, Certificate No.) 23-Jan-19 (CTTL, No.J19X00336) 24-Jan-19 (CTTL, No.J19X00547) Function	temperature(22±3)℃ and Scheduled Calibration Aug-19 Aug-19 Aug-19 Aug-19 Scheduled Calibration Jan-20 Jan-20

Certificate No: Z19-60177

Page 1 of 8





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2079
 Fax: +86-10-62304633-2504

 E-mail: cttl@chinattl.com
 http://www.chinattl.cn

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORMx,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Measurement procedure for assessment of specific absorption rate of human exposure to radio frequency fields from hand-held and body-mounted wireless communication devices- Part 1: Device used next to the ear (Frequency range of 300MHz to 6GHz)", July 2016
- c) IEC 62209-2, "Procedure to measure the Specific Absorption Rate (SAR) For wireless communication devices used in close proximity to the human body (frequency range of 30MHz to 6GHz)", March 2010
- d) KDB865664, SAR Measurement Requirements for 100 MHz to 6 GHz

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z19-60177

Page 2 of 8





In Collaboration with s pea q CALIBRATION LABORATORY

Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: cttl@chinattl.com http://www.chinattl.cn

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.2.1495
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8±6%	1.83 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.2 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.6 W/kg ± 18.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	6.11 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.4 W/kg ± 18.7 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.1 ± 6 %	1.96 mho/m ± 6 %
Body TSL temperature change during test	<1.0 °C		22.02

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.8 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	50.9 W/kg ± 18.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Body TSL	Condition	
SAR measured	250 mW input power	5.94 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.7 W/kg ± 18.7 % (k=2)

Certificate No: Z19-60177

Page 3 of 8



	S	p	e	a	g
-	CAL	BRATIO	ON LAP	ORATO	DRY

Tel: +86-10-62304633-2079 Fax: E-mail: cttl@chinattl.com http:

an District, Beijing, 100191, China Fax: +86-10-62304633-2504 http://www.chinattl.en

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	54.1Ω+ 2.51 JΩ	
Return Loss	- 26.8dB	

Antenna Parameters with Body TSL

Impedance, transformed to feed point	52.3Ω+ 3.40 jΩ	
Return Loss	- 27.9dB	_

General Antenna Parameters and Design

Electrical Delay (one direction)	1.020 ns	
----------------------------------	----------	--

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG

Certificate No: Z19-60177

Page 4 of 8

Date: 06.10.2019




In Collaboration with s pe a CALIBRATION LABORATORY Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ettl@chinattl.com http://www.chinattl.cn DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 910 Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz; $\sigma = 1.825 \text{ S/m}$; $\epsilon_r = 39.75$; $\rho = 1000 \text{ kg/m3}$ Phantom section: Right Section DASY5 Configuration:

- Probe: EX3DV4 SN7514; ConvF(6.95, 6.95, 6.95) @ 2450 MHz; Calibrated: 8/27/2018
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 8/20/2018
- Phantom: MFP_V5.1C; Type: QD 000 P51CA; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (2); SEMCAD X Version 14.6.12 (7450)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

```
Reference Value = 97.66 V/m; Power Drift = 0.02 dB
Peak SAR (extrapolated) = 27.4 W/kg
SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.11 W/kg
```

Maximum value of SAR (measured) = 22.3 W/kg

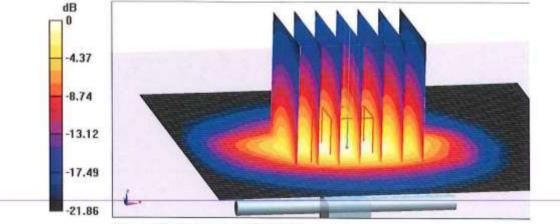

0 dB = 22.3 W/kg = 13.48 dBW/kg

Certificate No: Z19-60177

Page 5 of 8






http://www.chinattl.cn

Impedance Measurement Plot for Head TSL

E-mail: cttl@chinattl.com

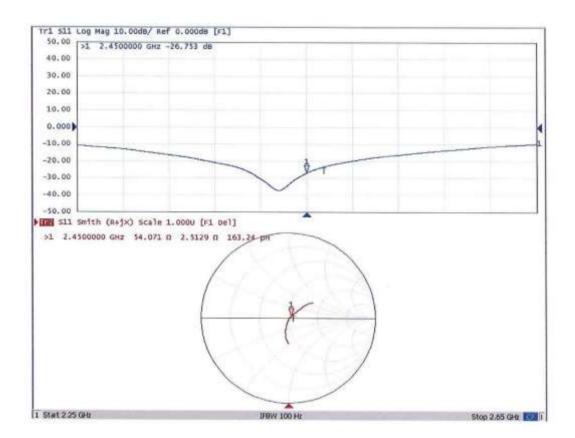

Certificate No: Z19-60177

Page 6 of 8





Date: 06.10.2019

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 910

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2450 MHz; $\sigma = 1.962$ S/m; $\varepsilon_r = 52.06$; $\rho = 1000$ kg/m3 Phantom section: Center Section


DASY5 Configuration:

- Probe: EX3DV4 SN7514; ConvF(7.13, 7.13, 7.13) @ 2450 MHz; Calibrated: 8/27/2018
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1556; Calibrated: 8/20/2018
- Phantom: MFP_V5.1C ; Type: QD 000 P51CA; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (2); SEMCAD X Version 14.6.12 (7450)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

```
Reference Value = 89.63 V/m; Power Drift = -0.02 dB
Peak SAR (extrapolated) = 26.4 W/kg
```

SAR(1 g) = 12.8 W/kg; SAR(10 g) = 5.94 W/kg Maximum value of SAR (measured) = 21.3 W/kg

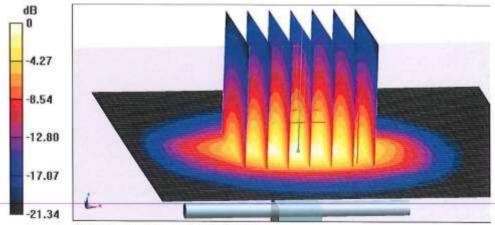

0 dB = 21.3 W/kg = 13.28 dBW/kg

Certificate No: Z19-60177


Page 7 of 8





Tel: +86-10-62304633-2079 Fax: +86-10-62304633-2504 E-mail: ettl@chinattLcom http://www.chinattLen

Impedance Measurement Plot for Body TSL

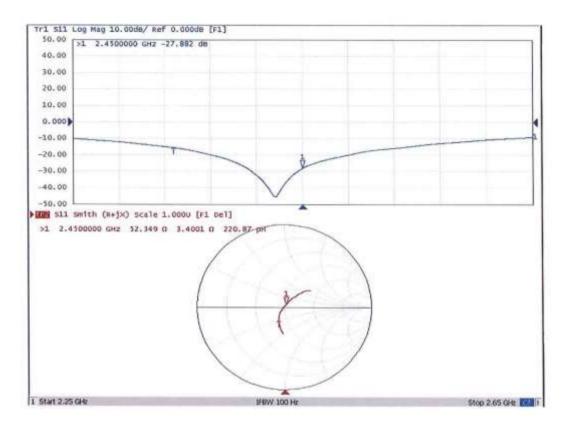

Certificate No: Z19-60177

Page 8 of 8



Dipole Impedance and Return Loss calibration Report

Object:	D2450V2 - SN: 910					
Calibration Date:	June 11, 2020					
Calibration reference:	IEEE Std 1528:2013, IEC 62209-1:2006, FCC KDB 865664 D01					
Calibrated By:	Janet Wei (Janet Wei, SAR project engineer)					

Reviewed By:

Winner Mang


(Winner Zhang, Technical manager)

Environment of Test Site


Temperature:	18 ~ 25°C
Humidity:	50~60% RH
Atmospheric Pressure:	1011 mbar


Test Data

Measurement Plot for Head TSL In 2020

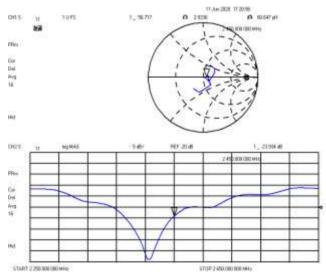

Comparison with Original report



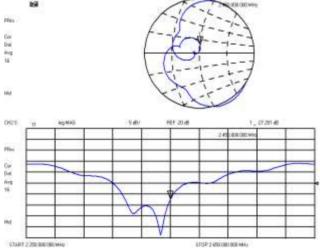

Items	Calibrated By CTTL	Calibrated By JYT In 2020	Deviation	Limit
Impendence for Head TSL	54.1Ω+2.51jΩ	56.72Ω+2.93jΩ	2.62Ω+0.42 jΩ	±5Ω
Return Loss for Head TSL	-26.8dB	-23.93dB	-10.71%	±20%(No less than 20 dB)
Impendence for Body TSL	52.3Ω+3.4jΩ	51.17Ω+4.37jΩ	-1.13Ω-0.97 jΩ	±5Ω
Return Loss for Body TSL	-27.9dB	-27.2dB	-2.51%	±20%(No less than 20 dB)

Result

Compliance



Calibration information for DAE

Add: No.51 Xu Tel: +86-10-623 E-mail: ettl@eh	04633-2512 Fa	c: +86-10-62304633-2504	CNAS L05
Client : CC			icate No: Z20-60270
CALIBRATION	CERTIFIC	ATE	
Object	DAE	4 - SN: 1373	
Calibration Procedure(s)	EE 7	11-002-01	
		pration Procedure for the Data /	Acquisition Electronics
Calibration date:	July	27, 2020	
measurements(SI). The pages and are part of the All calibrations have be humidity<70%.	measurements a a certificate. aen conducted i	nd the uncertainties with confidence	s, which realize the physical units o a probability are given on the following environment temperature(22±3)°C and
measurements(SI). The pages and are part of the All calibrations have be	measurements and certificate.	nd the uncertainties with confidence	e probability are given on the following environment temperature(22±3)°C and
measurements(SI). The in pages and are part of the All calibrations have be humidity<70%. Calibration Equipment us	measurements and certificate.	nd the uncertainties with confidence n the closed laboratory facility: e al for calibration)	e probability are given on the following environment temperature(22±3)°C and No.) Scheduled Calibration
measurements(SI). The pages and are part of the pages and are part of the All calibrations have be humidity<70%. Calibration Equipment us Primary Standards	measurements and certificate. een conducted in sed (M&TE critica	nd the uncertainties with confidence n the closed laboratory facility: e al for calibration) Cal Date(Calibrated by, Certificate I	e probability are given on the following environment temperature(22±3)°C and No.) Scheduled Calibration
measurements(SI). The pages and are part of the pages and are part of the humidity<70%. Calibration Equipment us Primary Standards	measurements and e certificate. een conducted in sed (M&TE critica ID # (1971018	nd the uncertainties with confidence n the closed laboratory facility: e al for calibration) Cal Date(Calibrated by, Certificate 1 16-Jun-20 (CTTL, No.J20X0434 Function	e probability are given on the following environment temperature(22±3)°C and No.) Scheduled Calibration
measurements(SI). The p pages and are part of the All calibrations have be numidity<70%. Calibration Equipment us Primary Standards	measurements and e certificate. een conducted in sed (M&TE critica ID # (1971018	nd the uncertainties with confidence n the closed laboratory facility: e al for calibration) Cal Date(Calibrated by, Certificate 1 16-Jun-20 (CTTL, No.J20X0434 Function	e probability are given on the following environment temperature(22±3)°C and No.) Scheduled Calibration I2) Jun-21 Signature

Certificate No: Z20-60270

Page 1 of 3





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2512
 Fax: +86-10-62304633-2504

 E-mail: cttl@chinattl.com
 Http://www.chinattl.cn

Glossary: DAE Connector angle

data acquisition electronics information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters:

- DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The report provide only calibration results for DAE, it does not contain other performance test results.

Certificate No: Z20-60270

Page 2 of 3





 Add: No.51 Xueyuan Road, Haidian District, Beijing, 100191, China

 Tel: +86-10-62304633-2512
 Fax: +86-10-62304633-2504

 E-mail: ettl@chinattl.com
 Http://www.chinattl.cn

DC Voltage Measurement

A/D - Converter Re				
High Range:	1LSB =	6.1µV.	full range =	-100+300 mV
Low Range:	1LSB =	61nV ,	full range =	-1+3mV
DASY measuremen	t parameters	Auto Zero	Time: 3 sec; Meas	uring time: 3 sec

Calibration Factors	x	Y	z
High Range	403.934 ± 0.15% (k=2)	403.899 ± 0.15% (k=2)	404.192 ± 0.15% (k=2)
Low Range	3.98735 ± 0.7% (k=2)	$4.00822 \pm 0.7\%$ (k=2)	4.01196 ± 0.7% (k=2)

Connector Angle

Connector Angle to be used in DASY system	346.5°±1 °

Certificate No: Z20-60270

Page 3 of 3

-----End of Report-----