



# **Appendix D**


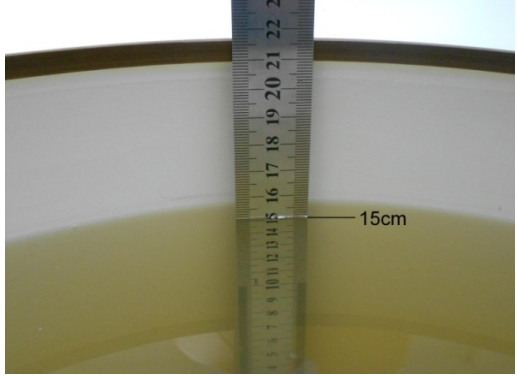




## **Photographs**


1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

## 1. SAR measurement System





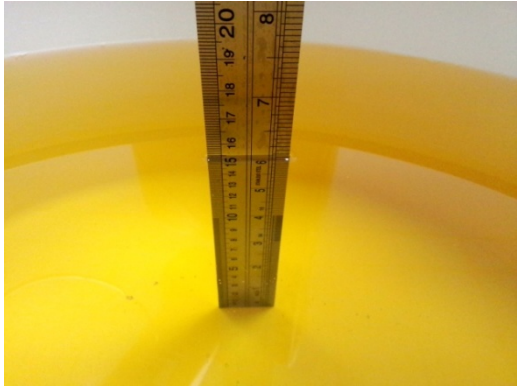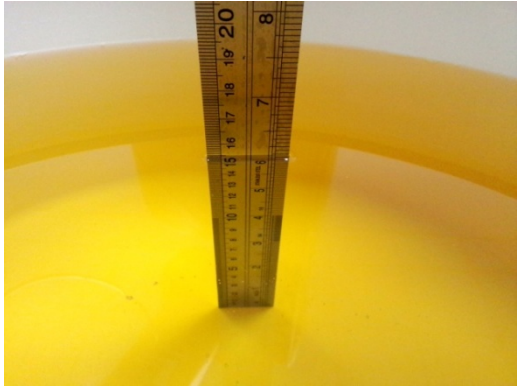

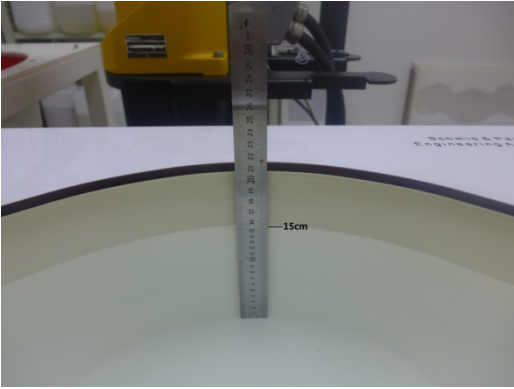

## 2. Photographs of Tissue Simulate Liquid

<p><b>Photo 1: Tissue Simulant Liquid for Head 750</b></p>	<p><b>Photo 2: Tissue Simulant Liquid for Head 835</b></p>
	
<p><b>Photo 3: Tissue Simulant Liquid for Head 1750</b></p>	<p><b>Photo 4: Tissue Simulant Liquid for Head 1900</b></p>
	
<p><b>Photo 5: Tissue Simulant Liquid for Head 2450</b></p>	<p><b>Photo 6: Tissue Simulant Liquid for Head 2600</b></p>
	

<b>Photo 7: Tissue Simulant Liquid for Head 5G</b>	<b>NA</b>
	<p><b>NA</b></p>

### 3. Photographs of EUT test position

<p>Photo 8: Front side 10mm</p>	<p>Photo 9: Back side 10mm</p>
	
<p>Photo 10: Left side 10mm</p>	<p>Photo 11: Right side 10mm</p>
	
<p>Photo 12: Top side 10mm</p>	<p>Photo 13: Bottom side 10mm</p>
	

#### 4. EUT Constructional Details

