

5

4

3

2

1

D

C

B


A

A

D

B 0034-0966-00235-0X1

ABIOMED Inc. PROPRIETARY AND PRIVATE
 The information contained in this document is the property of ABIOMED Inc. and shall be kept in strict confidence. Except with the express written permission of ABIOMED Inc., such information shall not be published or disclosed to others, or used for manufacture, sale or any other purpose, and this document shall not be reproduced, in whole or in part. If written permission is granted for reproduction, this legend shall be included in any such reproduction. This document and all copies of this document, in whole or in part, and with or without modifications, shall be returned to ABIOMED Inc. upon request, upon completion of the use for which it was made available to recipient, or termination of relationship with recipient, whichever first occurs. Any recipient so agrees by acceptance of this document.

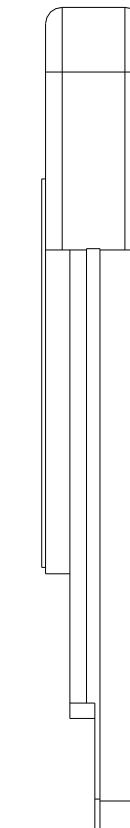

REVISIONS

ZONE	LTR	DESCRIPTION	DATE	APPROVED
	X X		X	X

ITEM NO.	QTY REQ	PART OR IDENTIFYING NO.	NOMENCLATURE OR DESCRIPTION	MATERIAL
LIST OF PARTS				

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES. TOLERANCES ARE: DECIMALS .X ± .1 .XX ± .010 .XXX ± .005 .XXXX ± .0005	DO NOT SCALE DRAWING		ABIOMED, INC. CHERRY HILL DR. DANVERS, MA 01923 (978) 777-5410
	APPROVALS	DATE	
	DRAWN B. Soares	23-Jun-04	
	CHECKED	—	
	ENGR	—	
	APPROV	—	SIZE DRAWING NO. B 0034-0966-00235-0X1 REV
	QA	—	
	DOC CTRL	—	SCALE NTS 1 of 1

NEXT ASSY	USED ON	FINISHED SURFACES $\sqrt{.63}$ BREAK SHARP CORNERS $\sqrt{.005}$
APPLICATION	DO NOT SCALE DRAWING	

5


4

3

2

1

REVISIONS			
LTR	DESCRIPTION	DATE	APPROVED

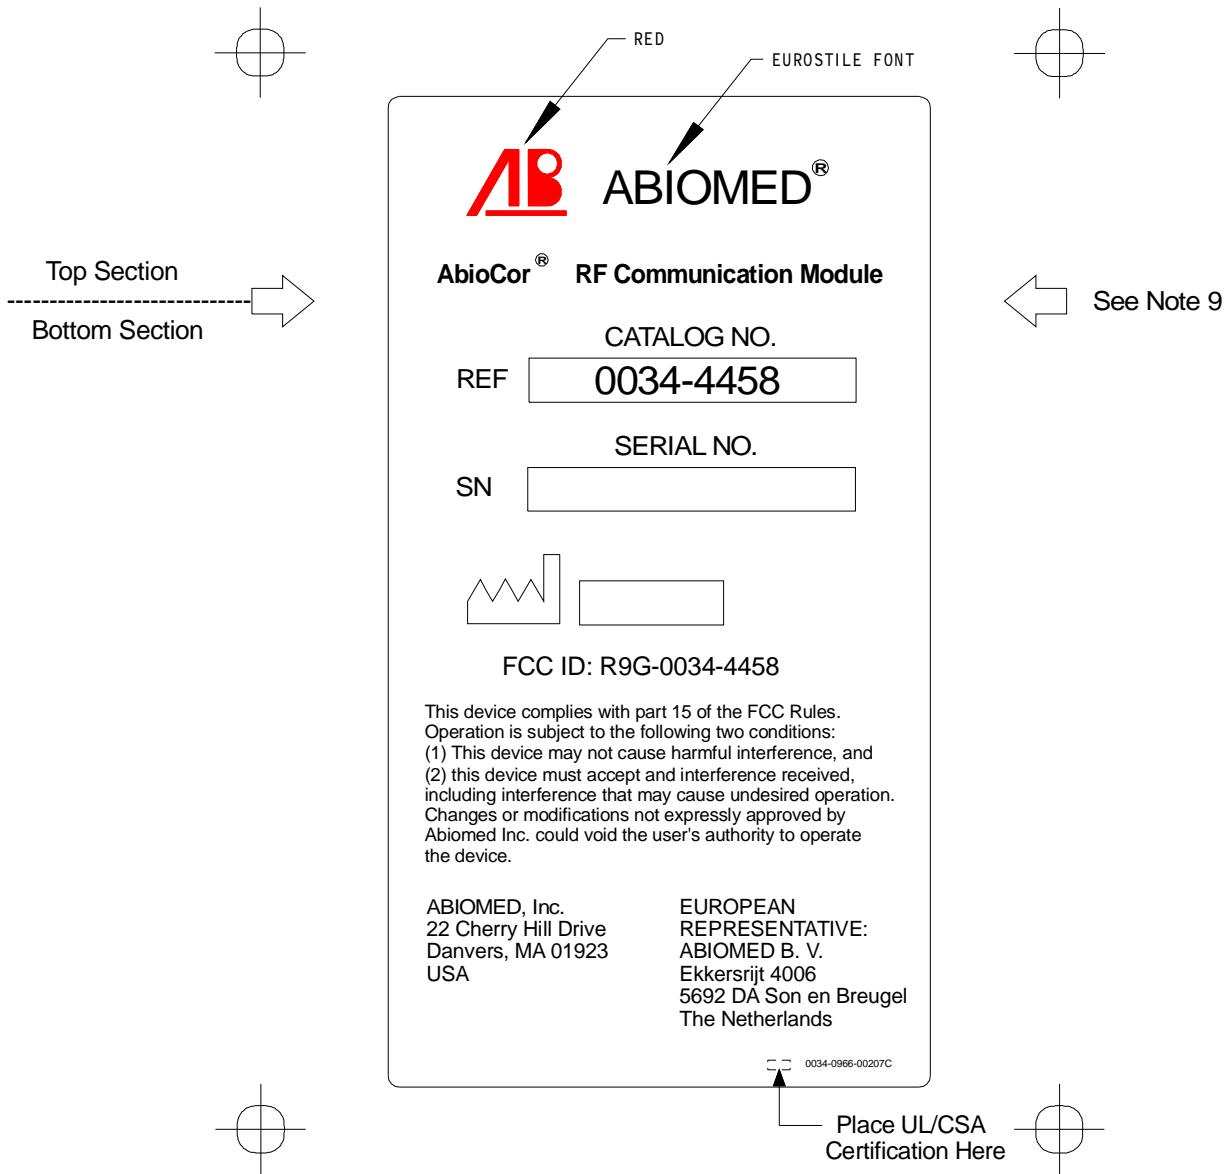

Notes

1. Material: MM-200 Mylar with OM-100 Compucal Laminate; 2 Mil Matte Clear Mylar Overlay Laminate.
2. Adhesive: L23
3. Ink Color(s): All content Black on White background unless otherwise specified. Red: Pantone PMS 185M
4. Finished Size: 5.25" x 2.88" with 0.06" Radius Corners
5. Font: Arial, unless otherwise specified.
6. Certification to UL and CSA Standards: LI 1003E or Equivalent, Date of Manufacturer, P. O. Number, and Quantity.
7. Storage: Dry, 50 - 85 °F.
8. Attach overlay laminate to top section of label with peel off on bottom section. Overlay laminate boundary shall not interfere with any content.

		APPROVALS		DATE	
DRAWN	BS			6/23/04	
CHECKED					
RESP ENG					
MFG ENG					
DO NOT SCALE DRAWING		SIZE	DWG. NO.		REV.
		A	0034-0966-00207-BX1		
		SCALE NONE	CAD FILE: 0034-0966-00207-BX1.dwg	SHEET 1	OF 1