
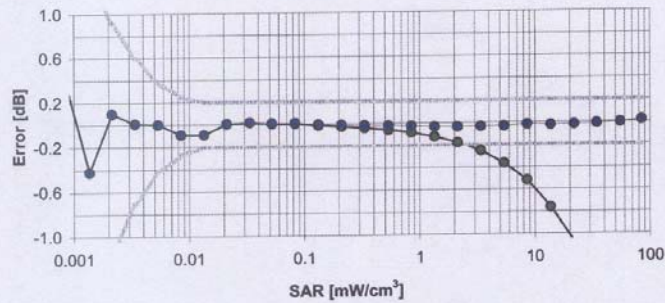


ES3DV3 SN: 3149

October 1, 2008

### Dynamic Range $f(\text{SAR}_{\text{head}})$ (Waveguide: WG8, $f = 1800 \text{ MHz}$ )

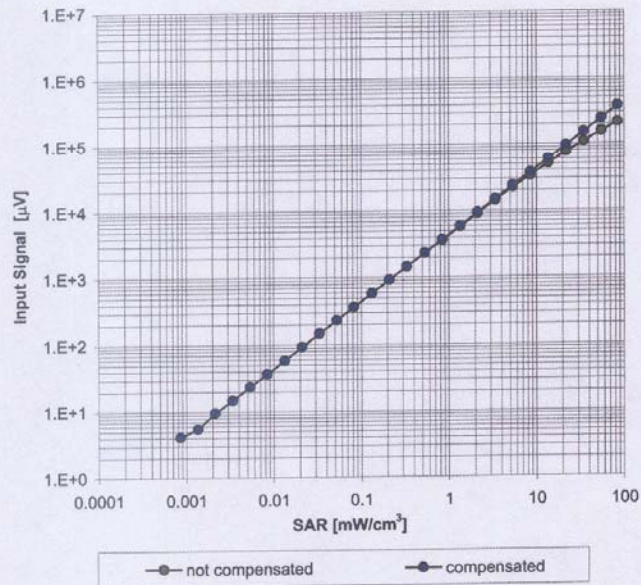


Uncertainty of Linearity Assessment:  $\pm 0.5\%$  ( $k=2$ )

ES3DV3 SN: 3149

October 1, 2008

### Conversion Factor Assessment

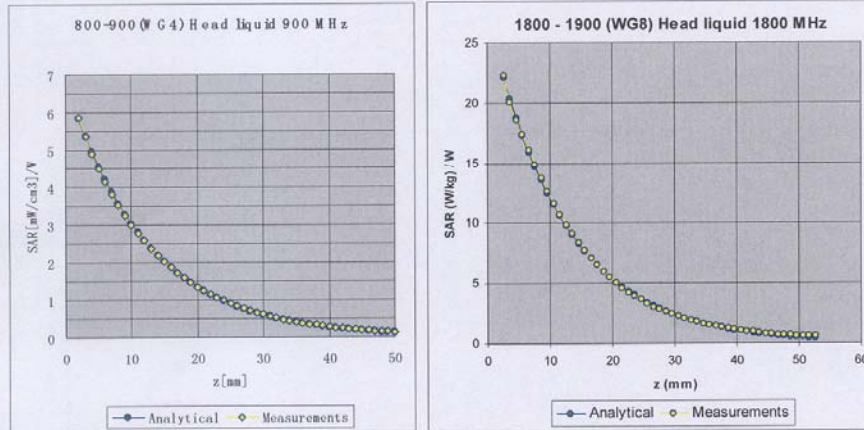


| f[MHz] | Validity[MHz] <sup>C</sup> | TSL  | Permittivity | Conductivity | Alpha | Depth | ConvF | Uncertainty  |
|--------|----------------------------|------|--------------|--------------|-------|-------|-------|--------------|
| 850    | ±50 /±100                  | Head | 41.5±5%      | 0.90±5%      | 0.91  | 1.13  | 6.56  | ±11.0% (k=2) |
| 900    | ±50 /±100                  | Head | 41.5±5%      | 0.97±5%      | 0.83  | 1.26  | 6.34  | ±11.0% (k=2) |
| 1800   | ±50 /±100                  | Head | 40.0±5%      | 1.40±5%      | 0.69  | 1.47  | 5.18  | ±11.0% (k=2) |
| 1900   | ±50 /±100                  | Head | 40.0±5%      | 1.40±5%      | 0.72  | 1.38  | 5.03  | ±11.0% (k=2) |
| 850    | ±50 /±100                  | Body | 55.2±5%      | 0.97±5%      | 0.76  | 1.26  | 6.22  | ±11.0% (k=2) |
| 900    | ±50 /±100                  | Body | 55.0±5%      | 1.05±5%      | 0.99  | 1.06  | 6.02  | ±11.0% (k=2) |
| 1800   | ±50 /±100                  | Body | 53.3±5%      | 1.52±5%      | 0.75  | 1.34  | 4.97  | ±11.0% (k=2) |
| 1900   | ±50 /±100                  | Body | 53.3±5%      | 1.52±5%      | 0.62  | 1.33  | 4.68  | ±11.0% (k=2) |

<sup>C</sup> The validity of ±100 MHz only applies for DASY v4.4 and higher (see Page 2). The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

ES3DV3 SN: 3149

October 1, 2008

**Deviation from Isotropy**  
Error ( $\phi, \theta$ ),  $f = 900$  MHz

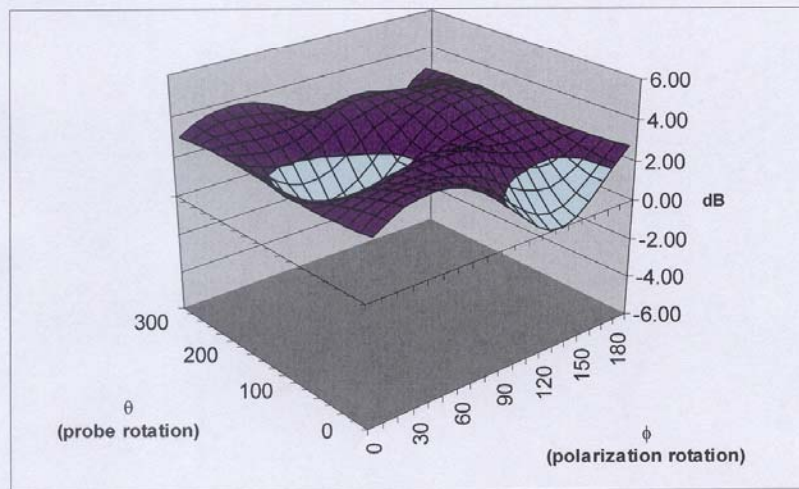

**Uncertainty of Spherical Isotropy Assessment:  $\pm 2.5\%$  ( $k=2$ )**

## ANNEX F DIPOLE CALIBRATION CERTIFICATE

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Federal Office of metrology and Accreditation  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client TMC China

Certificate No: D835V2-443\_Feb09

### CALIBRATION CERTIFICATE



|                                  |  |
|----------------------------------|--|
| Object                           | D835V2-SN: 443   |
| Calibration procedure(s)         | QA CAL-05.v6<br>Calibration procedure for dipole validation kits |
| Calibration date:                | February 18, 2009  |
| Condition of the calibrated item | In Tolerance   |

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements(SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted at an environment temperature (22±3)<sup>0</sup>C and humidity<70%

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID#             | Cal Data (Calibrated by, Certification NO.) | Scheduled Calibration   |
|-----------------------------|-----------------|---|-------------------------|
| Power meter EPM-442A        | GB37480704      | 01-Oct-08 (METAS, NO. 217-00608)            | Oct-09                  |
| Power sensor 8481A          | US37292783      | 01-Oct-08 (METAS, NO. 217-00608)            | Oct-09                  |
| Reference 20 dB Attenuator  | SN:5086 (20g )  | 08-Aug-08 (METAS, NO. 217-00591)            | Aug-09                  |
| Reference 10 dB Attenuator  | SN:5047_2 (10r) | 08-Aug-08 (METAS, NO. 217-00591)            | Aug-09                  |
| DAE4                        | SN:601          | 28-Jan-09 (SPEAG, NO.DAE4-601_Jan09)        | Jan-10                  |
| Reference Probe ET3DV6 (HF) | SN: 1507        | 17-Oct-08 (SPEAG, NO. ET3-1507_Oct08)       | Oct-09                  |
| Secondary Standards         | ID#             | Check Data (in house)                       | Scheduled Calibration   |
| Power sensor HP 8481A       | MY41092317      | 18-Oct-02(SPEAG, in house check Oct-07)     | In house check: Oct-09  |
| RF generator Aglient E4421B | MY41000676      | 11-May-05(SPEAG, in house check Nov-07)     | In house check: Nov -09 |
| Network Analyzer HP 8753E   | US37390585S4206 | 18-Oct-01(SPEAG, in house check Oct-08)     | In house check: Oct -09 |

|                | Name          | Function              | Signature   |
|----------------|---------------|-----------------------|---|
| Calibrated by: | Marcel Fehr   | Laboratory Technician |  |
| Approved by:   | Katja Pokovic | Technical Director    |  |

Issued: February 19, 2009

This calibration certificate shall not be reported except in full without written approval of the laboratory.

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zaughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- d) DASY4 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                           |             |
|------------------------------|---------------------------|-------------|
| DASY Version                 | DASY4                     | V4.7        |
| Extrapolation                | Advanced Extrapolation    |             |
| Phantom                      | Modular Flat Phantom V4.9 |             |
| Distance Dipole Center - TSL | 15 mm                     | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm         |             |
| Frequency                    | 835 MHz $\pm$ 1 MHz       |             |

### Head TSL parameters

The following parameters and calculations were applied.

|                                  | Temperature         | Permittivity   | Conductivity         |
|----------------------------------|---------------------|----------------|----------------------|
| Nominal Head TSL parameters      | 22.0 °C             | 41.5           | 0.90 mho/m           |
| Measured Head TSL parameters     | (22.0 $\pm$ 0.2) °C | 39.9 $\pm$ 6 % | 0.88 mho/m $\pm$ 6 % |
| Head TSL temperature during test | (21.2 $\pm$ 0.2) °C | ---            | ---                  |

### SAR result with Head TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | Condition          |                                |
|---|--------------------|--------------------------------|
| SAR measured  | 250 mW input power | 2.48 mW / g                    |
| SAR normalized  | normalized to 1W   | 9.90 mW / g                    |
| SAR for nominal Head TSL parameters <sup>1</sup>      | normalized to 1W   | 9.70 mW / g $\pm$ 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                                |
|---|--------------------|--------------------------------|
| SAR measured  | 250 mW input power | 1.60 mW / g                    |
| SAR normalized  | normalized to 1W   | 6.40 mW / g                    |
| SAR for nominal Head TSL parameters <sup>1</sup>        | normalized to 1W   | 6.31 mW / g $\pm$ 16.5 % (k=2) |

**Appendix**

**Antenna Parameters with Head TSL**

|                                      |                |
|--------------------------------------|----------------|
| Impedance, transformed to feed point | 50.5Ω - 6.8 jΩ |
| Return Loss                          | - 25.8 dB      |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.402 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |                   |
|-----------------|-------------------|
| Manufactured by | SPEAG             |
| Manufactured on | September 3, 2001 |

**DASY4 Validation Report for Head TSL**

Date/Time: 18.02.2009 10:13:45

Test laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 835 MHz; Type: D835V2; serial: D835V2-SN: 443**

Communication System: CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: HSL 835 MHz;

Medium parameters used:  $f=835$  MHz;  $\sigma=0.88$  mho/m;  $\epsilon_r=39.9$ ;  $\rho= 1000\text{kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6-SN1507(HF); ConvF(6.01,6.01,6.01); Calibrated: 17.10.2008
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.1\_2009
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA;
- Measurement SW: DASY, V4.7 Build 53; Post processing SW: SEMCAD, V1.8 Build 172


**Pin = 250 mW; d = 15 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm**

Reference Value = 56.6 V/m; Power Drift = 0.010 dB

Peak SAR (extrapolated) = 3.72 W/kg

**SAR(1 g) = 2.48 mW/g; SAR(10 g) = 1.60 mW/g**


Maximum value of SAR (measured) = 2.70 mW/g

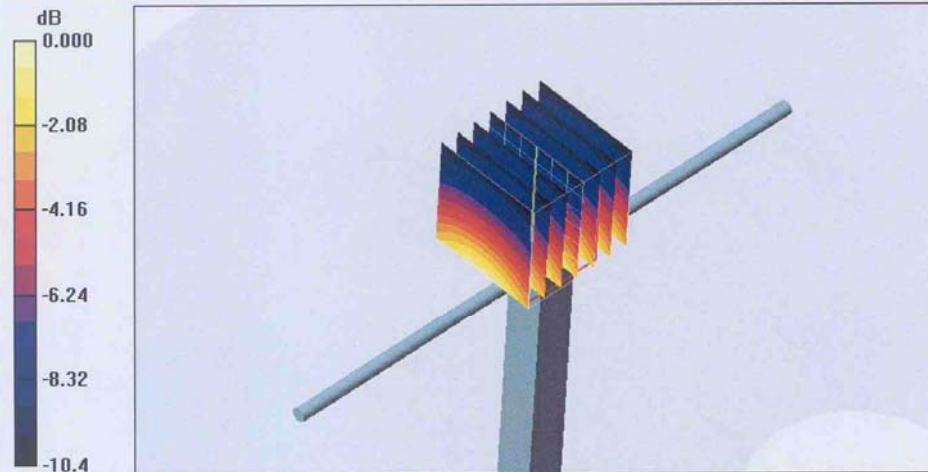

0 dB = 2.70mW/g



### Impedance measurement Plot for Head TSL

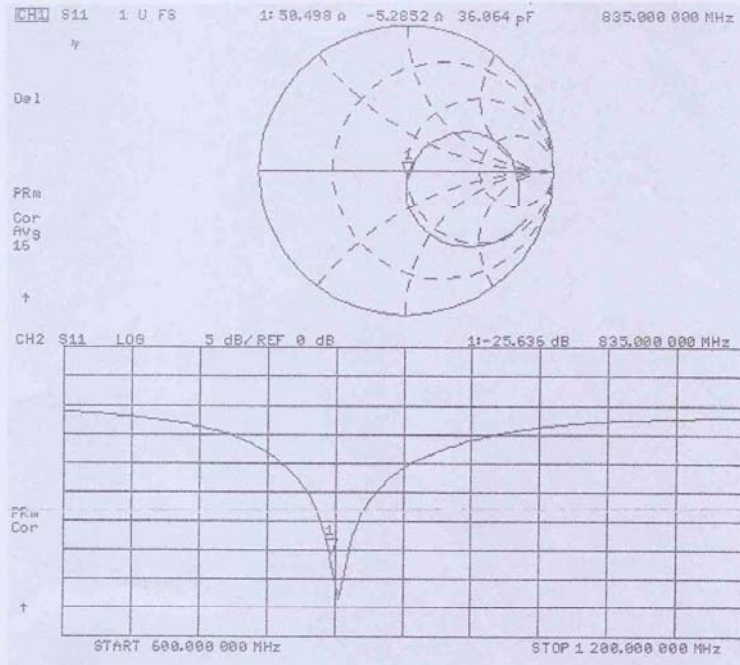

**Calibration Laboratory of  
Schmid & Partner  
Engineering AG**  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Federal Office of metrology and Accreditation  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates  
Client TMC China

Accreditation No.: SCS 108

Certificate No: D1900V2-541\_Feb09

**CALIBRATION CERTIFICATE**

|                                  |  |
|----------------------------------|--|
| Object                           | D1900V2-SN: 541  |
| Calibration procedure(s)         | QA CAL-05.v6<br>Calibration procedure for dipole validation kits |
| Calibration date:                | February 19, 2009  |
| Condition of the calibrated item | In Tolerance   |

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements(SI).  
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted at an environment temperature (22±3)°C and humidity<70%

Calibration Equipment used (M&TE critical for calibration)

| Primary Standards           | ID#             | Cal Data (Calibrated by, Certification NO.) | Scheduled Calibration   |
|-----------------------------|-----------------|---|-------------------------|
| Power meter EPM-442A        | GB37480704      | 01-Oct-08 (METAS, NO. 217-00608)            | Oct-09                  |
| Power sensor 8481A          | US37292783      | 01-Oct-08 (METAS, NO. 217-00608)            | Oct-09                  |
| Reference 20 dB Attenuator  | SN:5086 (20g )  | 08-Aug-08 (METAS, NO. 217-00591)            | Aug-09                  |
| Reference 10 dB Attenuator  | SN:5047_2 (10r) | 08-Aug-08 (METAS, NO. 217-00591)            | Aug-09                  |
| DAE4                        | SN:601          | 28-Jan-09 (SPEAG, NO.DAE4-601_Jan09)        | Jan-10                  |
| Reference Probe ET3DV6 (HF) | SN: 1507        | 17-Oct-08 (SPEAG, NO. ET3-1507_Oct08)       | Oct-09                  |
| Secondary Standards         | ID#             | Check Data (in house)                       | Scheduled Calibration   |
| Power sensor HP 8481A       | MY41092317      | 18-Oct-02(SPEAG, in house check Oct-07)     | In house check: Oct-09  |
| RF generator Agilent E4421B | MY41000676      | 11-May-05(SPEAG, in house check Nov-07)     | In house check: Nov -09 |
| Network Analyzer HP 8753E   | US37390585S4206 | 18-Oct-01(SPEAG, in house check Oct-08)     | In house check: Oct -10 |

|                | Name          | Function              | Signature |
|----------------|---------------|-----------------------|-----------|
| Calibrated by: | Marcel Fehr   | Laboratory Technician |           |
| Approved by:   | Katja Pokovic | Technical Director    |           |

Issued: February 20, 2009

This calibration certificate shall not be reported except in full without written approval of the laboratory.

Calibration Laboratory of  
Schmid & Partner  
Engineering AG  
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst  
C Service suisse d'étalonnage  
S Servizio svizzero di taratura  
S Swiss Calibration Service

Accredited by the Swiss Federal Office of Metrology and Accreditation  
The Swiss Accreditation Service is one of the signatories to the EA  
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

**Glossary:**

|       |                                 |
|-------|---------------------------------|
| TSL   | tissue simulating liquid        |
| ConvF | sensitivity in TSL / NORM x,y,z |
| N/A   | not applicable or not measured  |

**Calibration is Performed According to the Following Standards:**

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) CENELEC EN 50361, "Basic standard for the measurement of Specific Absorption Rate related to human exposure to electromagnetic fields from mobile phones (300 MHz - 3 GHz), July 2001
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

**Additional Documentation:**

- d) DASY4 System Handbook

**Methods Applied and Interpretation of Parameters:**

- *Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- *Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- *Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- *Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- *SAR measured:* SAR measured at the stated antenna input power.
- *SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- *SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

### Measurement Conditions

DASY system configuration, as far as not given on page 1.

|                              |                           |             |
|------------------------------|---------------------------|-------------|
| DASY Version                 | DASY4                     | V4.7        |
| Extrapolation                | Advanced Extrapolation    |             |
| Phantom                      | Modular Flat Phantom V5.0 |             |
| Distance Dipole Center - TSL | 10 mm                     | with Spacer |
| Zoom Scan Resolution         | dx, dy, dz = 5 mm         |             |
| Frequency                    | 1900 MHz ± 1 MHz          |             |

### Head TSL parameters

The following parameters and calculations were applied.

|                                  | Temperature     | Permittivity | Conductivity     |
|----------------------------------|-----------------|--------------|------------------|
| Nominal Head TSL parameters      | 22.0 °C         | 40.0         | 1.40 mho/m       |
| Measured Head TSL parameters     | (22.0 ± 0.2) °C | 38.9 ± 6 %   | 1.38 mho/m ± 6 % |
| Head TSL temperature during test | (22.1 ± 0.2) °C | ---          | ---              |

### SAR result with Head TSL

| SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL | condition          |                            |
|---|--------------------|----------------------------|
| SAR measured  | 250 mW input power | 9.73 mW /g                 |
| SAR normalized  | normalized to 1W   | 38.9 mW /g                 |
| SAR for nominal Head TSL parameters <sup>1</sup>      | normalized to 1W   | 38.6 mW / g ± 17.0 % (k=2) |

| SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL | condition          |                            |
|---|--------------------|----------------------------|
| SAR measured  | 250 mW input power | 5.09 mW /g                 |
| SAR normalized  | normalized to 1W   | 20.4 mW /g                 |
| SAR for nominal Head TSL parameters <sup>1</sup>        | normalized to 1W   | 20.2 mW / g ± 16.5 % (k=2) |

<sup>1</sup> Correction to nominal TSL parameters according to d), chapter "SAR Sensitivities"

**Appendix**

**Antenna Parameters with Head TSL**

|                                      |                                |
|--------------------------------------|--------------------------------|
| Impedance, transformed to feed point | 48.4 $\Omega$ - 8.9 j $\Omega$ |
| Return Loss                          | - 26.4 dB                      |

**General Antenna Parameters and Design**

|                                  |          |
|----------------------------------|----------|
| Electrical Delay (one direction) | 1.214 ns |
|----------------------------------|----------|

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals.  
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

**Additional EUT Data**

|                 |                  |
|-----------------|------------------|
| Manufactured by | SPEAG            |
| Manufactured on | October 4 , 2001 |

**DASY4 Validation Report for Head TSL**

Date/Time: 19.02.2009 09:37:10

Test laboratory: SPEAG, Zurich, Switzerland

**DUT: Dipole 1900 MHz; Type: D1900V2; serial: D1900V2-SN: 541**

Communication System: CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: HSL 1900 MHz;

Medium parameters used:  $f=1900$  MHz;  $\sigma=1.38$  mho/m;  $\epsilon_r=38.9$ ;  $\rho= 1000$ kg/m<sup>3</sup>

Phantom section: Flat Section

Measurement Standard: DASY4 (High Precision Assessment)

DASY4 Configuration:

- Probe: ET3DV6-SN1507(HF); ConvF(5.03, 5.03, 5.03); Calibrated: 17.10.2008
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 28.1\_2009
- Phantom: Flat Phantom 4.9L; Type: QD00P49AA;
- Measurement SW: DASY, V4.7 Build 53; Post processing SW: SEMCAD, V1.8 Build 172


**Pin = 250 mW; d = 15 mm/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm**

Reference Value = 92.1 V/m; Power Drift = 0.059 dB

Peak SAR (extrapolated) = 16.9 W/kg

**SAR(1 g) = 9.73 mW/g; SAR(10 g) = 5.09 mW/g**

Maximum value of SAR (measured) = 11.3 mW/g

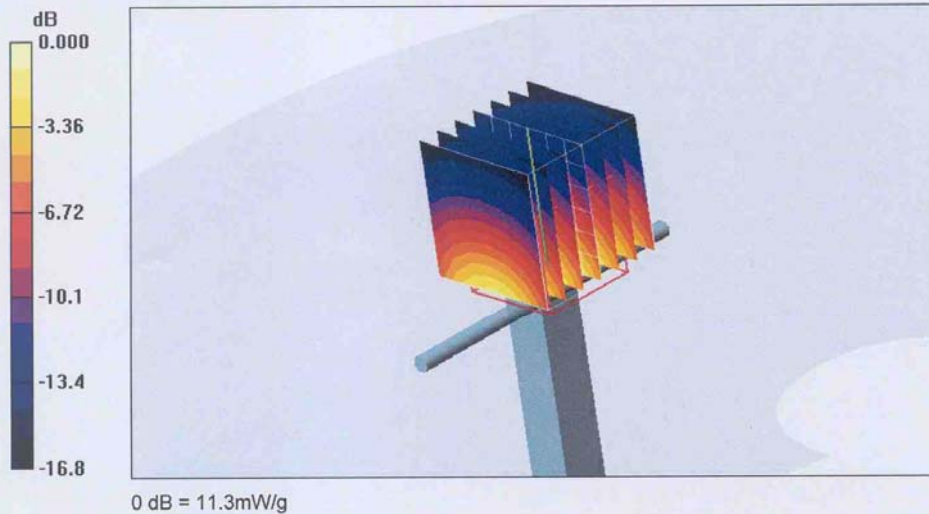

### Impedance measurement Plot for Head TSL

