


Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
 Reference Value = 58.162 V/m; Power Drift = -0.01 dB
 Peak SAR (extrapolated) = 34.7 W/kg
SAR(1 g) = 7.97 W/kg; SAR(10 g) = 2.21 W/kg
 Maximum value of SAR (measured) = 19.3 W/kg

Dipole Calibration for Body Tissue/Pin=100mW, dist=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm
 Reference Value = 55.100 V/m; Power Drift = 0.01 dB
 Peak SAR (extrapolated) = 34.1 W/kg
SAR(1 g) = 7.43 W/kg; SAR(10 g) = 2.05 W/kg
 Maximum value of SAR (measured) = 18.1 W/kg

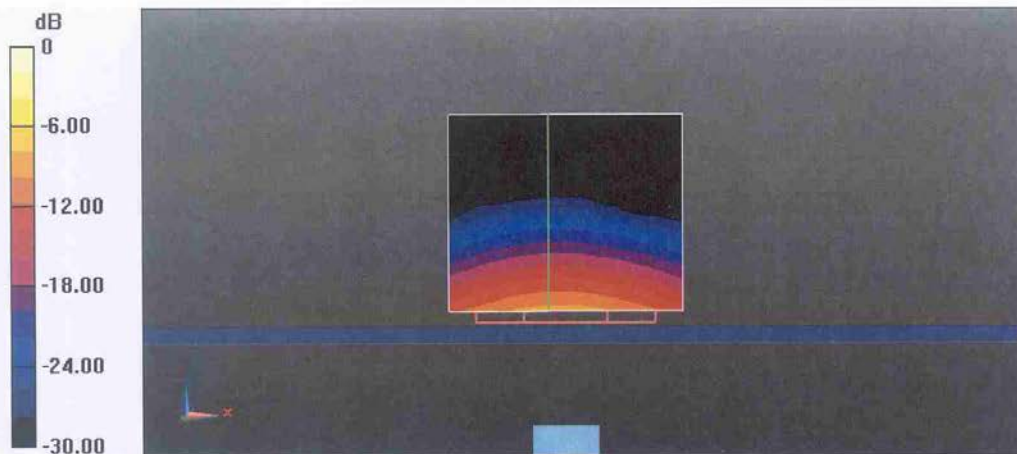

0 dB = 18.1 W/kg = 12.58 dBW/kg

Impedance Measurement Plot for Body TSL

