

DASY5 Validation Report for Head TSL

Date: 02.05.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1012

Communication System: CW; Frequency: 2600 MHz

Medium parameters used: $f = 2600$ MHz; $\sigma = 1.98$ mho/m; $\epsilon_r = 39.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.39, 4.39, 4.39); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.1(838); SEMCAD X 14.6.5(6469)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.7 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 30.026 mW/g

SAR(1 g) = 14.3 mW/g; SAR(10 g) = 6.39 mW/g

Maximum value of SAR (measured) = 18.7 mW/g

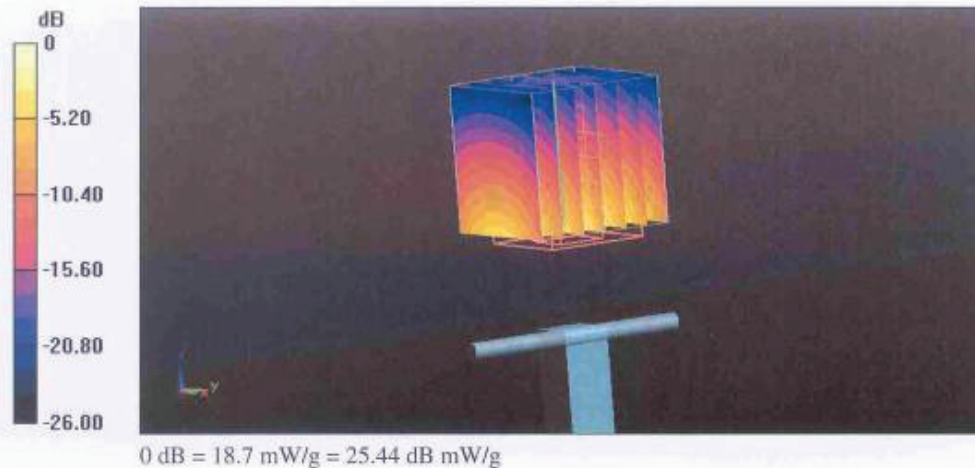


TA Technology (Shanghai) Co., Ltd.
Test Report

Report No.: RXA1412-0289SAR01R3

Page 175 of 189

Impedance Measurement Plot for Head TSL

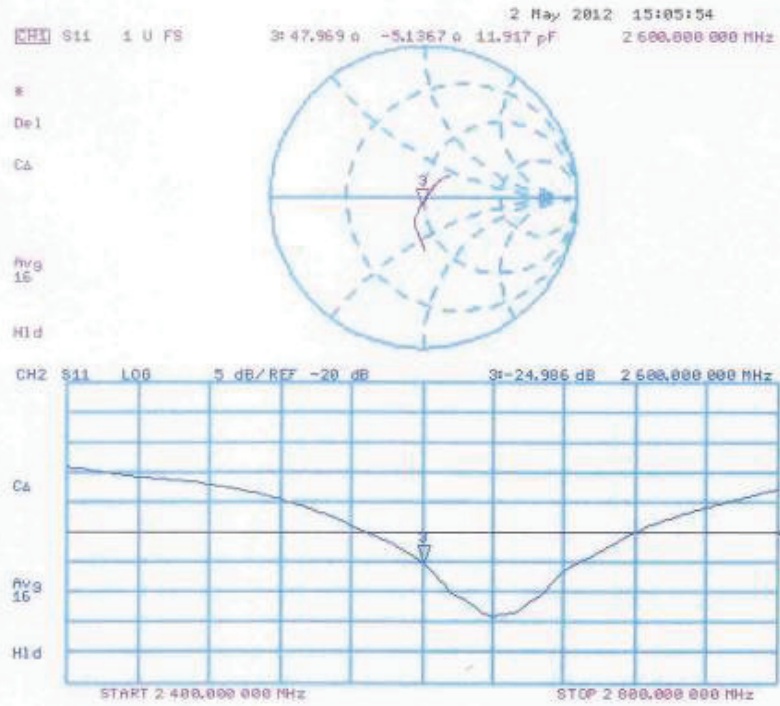

DASY5 Validation Report for Body TSL

Date: 02.05.2012

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: D2600V2 - SN: 1012

Communication System: CW; Frequency: 2600 MHz

Medium parameters used: $f = 2600$ MHz; $\sigma = 2.16$ mho/m; $\epsilon_r = 52.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.16, 4.16, 4.16); Calibrated: 30.12.2011;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 04.07.2011
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.1(838); SEMCAD X 14.6.5(6469)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.978 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 28.165 mW/g

SAR(1 g) = 13.6 mW/g; SAR(10 g) = 6.09 mW/g

Maximum value of SAR (measured) = 18.1 mW/g

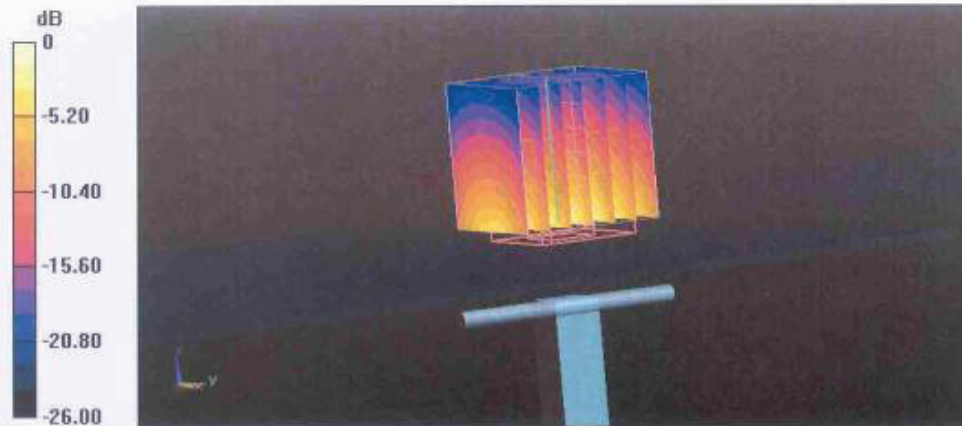


0 dB = 18.1 mW/g = 25.15 dB mW/g

TA Technology (Shanghai) Co., Ltd.
Test Report

Report No.: RXA1412-0289SAR01R3

Page 177 of 189

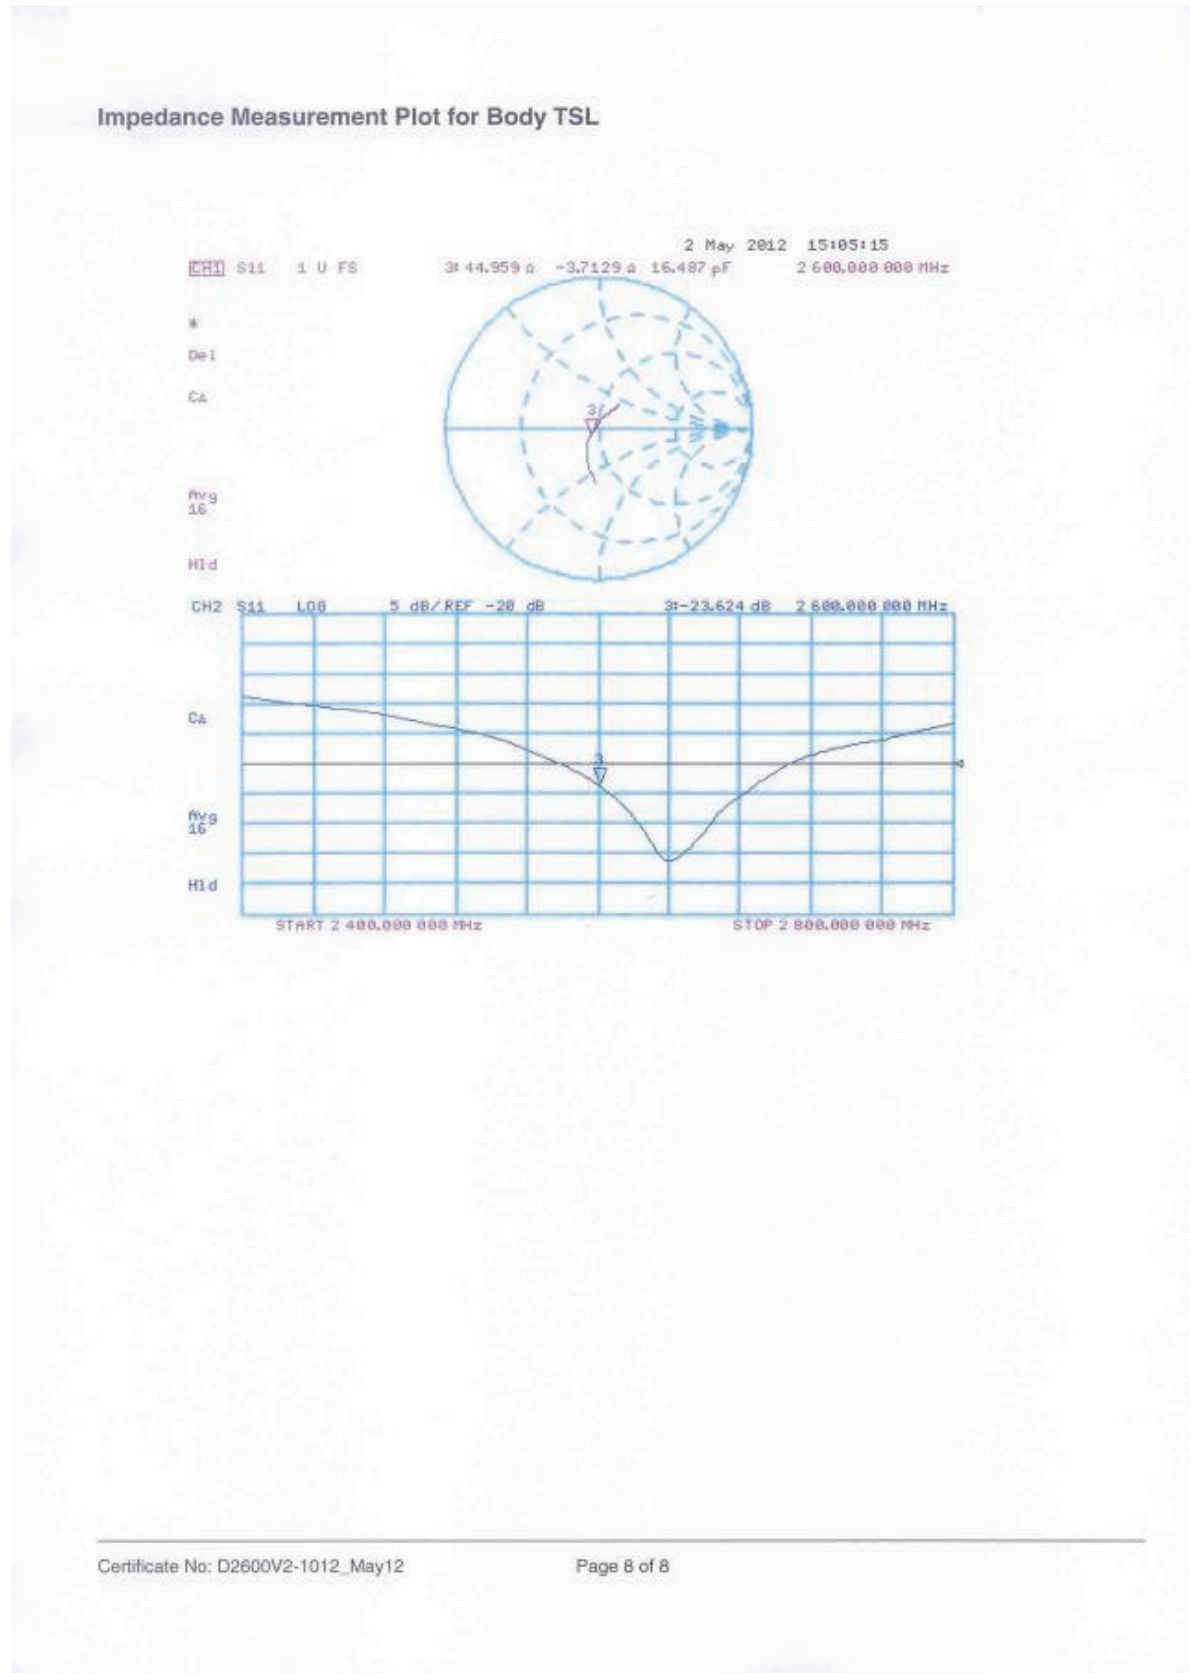

TA Technology (Shanghai) Co., Ltd.
Test Report

Report No.: RXA1412-0289SAR01R3

Page 178 of 189

ANNEX K: DAE4 Calibration Certificate

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client TA-Shanghai (Auden)

Certificate No: DAE4-1291_Nov14

CALIBRATION CERTIFICATE

Object DAE4 - SD 000 D04 BM - SN: 1291

Calibration procedure(s) QA CAL-06.v28
Calibration procedure for the data acquisition electronics (DAE)

Calibration date: November 14, 2014

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	03-Oct-14 (No:15573)	Oct-15
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	07-Jan-14 (in house check)	In house check: Jan-15
Calibrator Box V2.1	SE UMS 006 AA 1002	07-Jan-14 (in house check)	In house check: Jan-15

Calibrated by: Name Dominique Steffen Function Technician Signature

Approved by: Fin Bornholt Deputy Technical Manager

Issued: November 14, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

TA Technology (Shanghai) Co., Ltd.

Test Report

Report No.: RXA1412-0289SAR01R3

Page 179 of 189

**Calibration Laboratory of
Schmid & Partner
Engineering AG**
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary

DAE data acquisition electronics
Connector angle information used in DASY system to align probe sensor X to the robot coordinate system.

Methods Applied and Interpretation of Parameters

- **DC Voltage Measurement:** Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.
- **Connector angle:** The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - **DC Voltage Measurement Linearity:** Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement.
 - **Common mode sensitivity:** Influence of a positive or negative common mode voltage on the differential measurement.
 - **Channel separation:** Influence of a voltage on the neighbor channels not subject to an input voltage.
 - **AD Converter Values with inputs shorted:** Values on the internal AD converter corresponding to zero input voltage
 - **Input Offset Measurement:** Output voltage and statistical results over a large number of zero voltage measurements.
 - **Input Offset Current:** Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - **Input resistance:** Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - **Low Battery Alarm Voltage:** Typical value for information. Below this voltage, a battery alarm signal is generated.
 - **Power consumption:** Typical value for information. Supply currents in various operating modes.

TA Technology (Shanghai) Co., Ltd.
Test Report

Report No.: RXA1412-0289SAR01R3

Page 180 of 189

DC Voltage Measurement

A/D - Converter Resolution nominal

High Range: 1LSB = 6.1 μ V , full range = -100...+300 mV

Low Range: 1LSB = 61nV , full range = -1.....+3mV

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	X	Y	Z
High Range	402.613 $\pm$ 0.02% (k=2)	403.293 $\pm$ 0.02% (k=2)	403.205 $\pm$ 0.02% (k=2)
Low Range	3.97544 $\pm$ 1.50% (k=2)	3.93356 $\pm$ 1.50% (k=2)	3.99377 $\pm$ 1.50% (k=2)

Connector Angle

Connector Angle to be used in DASY system	308.5 ° $\pm$ 1 °
---	-------------------

TA Technology (Shanghai) Co., Ltd.

Test Report

Report No.: RXA1412-0289SAR01R3

Page 181 of 189

Appendix (Additional assessments outside the scope of SCS108)

1. DC Voltage Linearity

High Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	200033.82	-3.10	-0.00
Channel X + Input	20004.15	-0.02	-0.00
Channel X - Input	-20004.31	1.85	-0.01
Channel Y + Input	200033.24	-3.41	-0.00
Channel Y + Input	20003.47	-0.54	-0.00
Channel Y - Input	-20006.08	0.19	-0.00
Channel Z + Input	200036.05	-0.73	-0.00
Channel Z + Input	20001.26	-2.68	-0.01
Channel Z - Input	-20007.69	-1.47	0.01

Low Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	2000.57	-0.08	-0.00
Channel X + Input	200.57	-0.14	-0.07
Channel X - Input	-199.31	-0.00	0.00
Channel Y + Input	1999.81	-0.79	-0.04
Channel Y + Input	200.05	-0.62	-0.31
Channel Y - Input	-199.06	0.30	-0.15
Channel Z + Input	2001.14	0.56	0.03
Channel Z + Input	199.16	-1.42	-0.71
Channel Z - Input	-200.73	-1.23	0.62

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	9.64	7.77
	- 200	-6.77	-8.44
Channel Y	200	13.71	13.30
	- 200	-14.01	-14.19
Channel Z	200	-16.88	-16.56
	- 200	13.70	13.86

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	-	3.91	-4.26
Channel Y	200	8.88	-	3.64
Channel Z	200	10.51	7.45	-

TA Technology (Shanghai) Co., Ltd.

Test Report

Report No.: RXA1412-0289SAR01R3

Page 182 of 189

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16003	13374
Channel Y	15805	15470
Channel Z	16035	14317

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input 10M Ω

	Average (μ V)	min. Offset (μ V)	max. Offset (μ V)	Std. Deviation (μ V)
Channel X	0.37	-1.17	1.61	0.49
Channel Y	0.25	-0.91	1.56	0.48
Channel Z	-0.62	-1.83	0.60	0.47

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9