

Date: 05.18.2021



Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 http://www.chinattl.cn

#### **DASY5 Validation Report for Head TSL**

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1200

Communication System: CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz,

Medium parameters used: f = 5250 MHz;  $\sigma$  = 4.668 S/m;  $\epsilon_r$  = 35.48;  $\rho$  = 1000 kg/m³, Medium parameters used: f = 5600 MHz;  $\sigma$  = 5.045 S/m;  $\epsilon_r$  = 34.88;  $\rho$  = 1000 kg/m³, Medium parameters used: f = 5750 MHz;  $\sigma$  = 5.208 S/m;  $\epsilon_r$  = 34.67;  $\rho$  = 1000 kg/m³,

Phantom section: Center Section

#### DASY5 Configuration:

- Probe: EX3DV4 SN3846; ConvF(5.43, 5.43, 5.43) @ 5250 MHz; ConvF(4.69, 4.69, 4.69) @ 5600 MHz; ConvF(4.9, 4.9, 4.9) @ 5750 MHz; Calibrated: 2021-04-26
- · Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 2021-01-08
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

Dipole Calibration /Pin=100mW, d=10mm, f=5250 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 69.22 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 32.9 W/kg

SAR(1 g) = 7.8 W/kg; SAR(10 g) = 2.22 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.3%

Maximum value of SAR (measured) = 18.9 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 70.18 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 35.5 W/kg

SAR(1 g) = 8.15 W/kg; SAR(10 g) = 2.32 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 62.9%

Maximum value of SAR (measured) = 19.8 W/kg

Certificate No: Z21-60173

Page 9 of 14





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel; +86-10-62304633-2512 Fax: +86-10-62304633-2504 http://www.chinattl.cn

# Dipole Calibration /Pin=100mW, d=10mm, f=5750 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 68.06 V/m; Power Drift = -0.09 dB


Peak SAR (extrapolated) = 34.6 W/kg

SAR(1 g) = 7.75 W/kg; SAR(10 g) = 2.18 W/kg

Smallest distance from peaks to all points 3 dB below = 7.4 mm

Ratio of SAR at M2 to SAR at M1 = 62.1%

Maximum value of SAR (measured) = 19.0 W/kg

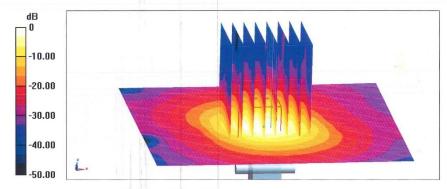

0 dB = 19.0 W/kg = 12.79 dBW/kg


Page 10 of 14





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 http://www.chinattl.cn

### Impedance Measurement Plot for Head TSL

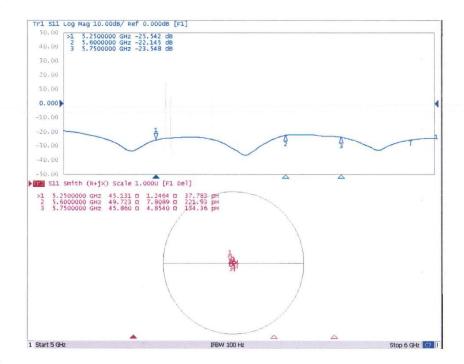

Report No.: BL-SZ23B0215-AC-2





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 Fax: +86-10-6230463-10-62304 Fax: +86-10-62304 Fa

**DASY5 Validation Report for Body TSL** 

Date: 05.18.2021

Test Laboratory: CTTL, Beijing, China

DUT: Dipole 5GHz; Type: D5GHzV2; Serial: D5GHzV2 - SN: 1200

Communication System: CW; Frequency: 5250 MHz, Frequency: 5600 MHz, Frequency: 5750 MHz,

Medium parameters used: f = 5250 MHz;  $\sigma$  = 5.34 S/m;  $\epsilon_r$  = 49.12;  $\rho$  = 1000 kg/m³, Medium parameters used: f = 5600 MHz;  $\sigma$  = 5.815 S/m;  $\epsilon_r$  = 48.44;  $\rho$  = 1000 kg/m³, Medium parameters used: f = 5750 MHz;  $\sigma$  = 6.045 S/m;  $\epsilon_r$  = 48.11;  $\rho$  = 1000 kg/m³,

Phantom section: Right Section

#### DASY5 Configuration:

- Probe: EX3DV4 SN3846; ConvF(4.95, 4.95, 4.95) @ 5250 MHz; ConvF(4.32, 4.32, 4.32) @ 5600 MHz; ConvF(4.38, 4.38, 4.38) @ 5750 MHz; Calibrated: 2021-04-26.
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn777; Calibrated: 2021-01-08
- Phantom: MFP\_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- Measurement SW: DASY52, Version 52.10 (4); SEMCAD X Version 14.6.14 (7483)

Dipole Calibration /Pin=100mW, d=10mm, f=5250 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.86 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 29.6 W/kg

SAR(1 g) = 7.33 W/kg; SAR(10 g) = 2.05 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 65.3%

Maximum value of SAR (measured) = 17.2 W/kg

Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 66.06 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 33.1 W/kg

SAR(1 g) = 7.72 W/kg; SAR(10 g) = 2.16 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 63.1%

Maximum value of SAR (measured) = 18.8 W/kg

Certificate No: Z21-60173

Page 12 of 14





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 http://www.chinattl.cn

### Dipole Calibration /Pin=100mW, d=10mm, f=5750 MHz/Zoom Scan,

dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 64.58 V/m; Power Drift = -0.04 dB


Peak SAR (extrapolated) = 32.8 W/kg

SAR(1 g) = 7.34 W/kg; SAR(10 g) = 2.03 W/kg

Smallest distance from peaks to all points 3 dB below = 7.2 mm

Ratio of SAR at M2 to SAR at M1 = 62%

Maximum value of SAR (measured) = 18.1 W/kg

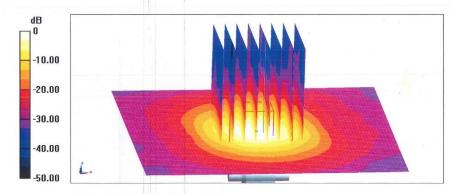

0 dB = 18.1 W/kg = 12.58 dBW/kg


Page 13 of 14





Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304633-2512 Fax: +86-10-62304633-2504 http://www.chinattl.cn

# Impedance Measurement Plot for Body TSL

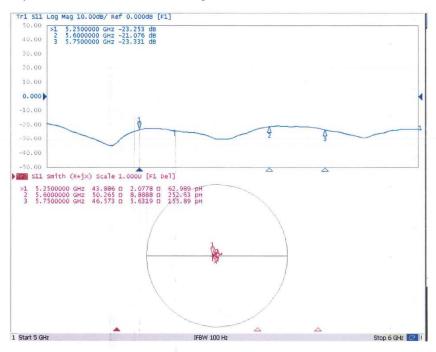


Page 14 of 14




D5GHzV2 Dipole impedance and return loss Validation

Meas. Results	Current Meas.	Previous Meas.	Max. Deviation
Meas. Data	2023.05.16	2022.05.17	/
5.25GHz	-27.820	-29.961	-7.15%
Return Loss(dB)	-27.020	-29.901	-7.15%
5.25GHz	49.06 Ω -0.322 jΩ	48.925 Ω +1.802	-2.124Ω
Impedance	49.00 12 -0.322 112	jΩ	(Imaginary part)
5.6GHz	-21.574	-25.244	-14.54%
Return Loss(dB)	-21.574	-25.244	-14.54%
5.6GHz	52.121Ω +3.482	47.163Ω +3.417	4.958Ω
Impedance	jΩ	jΩ	(Real part)
5.75GHz	-27.547	-27.284	0.96%
Return Loss(dB)	-27.547	-21.204	0.96%
5.75GHz	46.944Ω +4.023	50.693Ω +8.724	-4.701Ω
Impedance	jΩ	jΩ	(Imaginary part)

# Return Loss for Head TSL

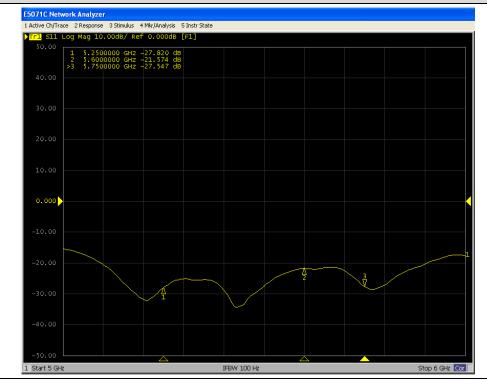



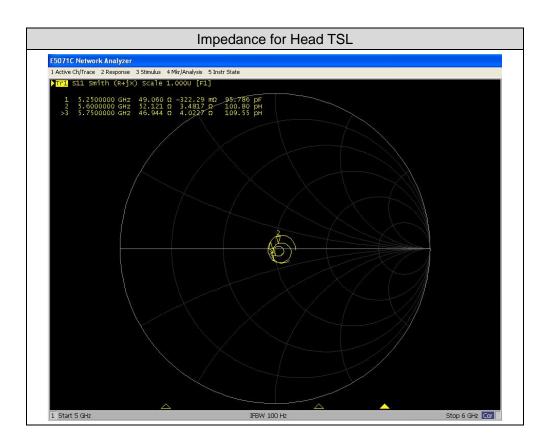



F.5 6.5GHz Dipole

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

D6.5GHzV2-1037 Jul21

ALIBITATION OF	ERTIFICATE			
Dbject	D6.5GHzV2 - SN:1037			
Calibration procedure(s)	QA CAL-22.v6 Calibration Procedure for SAR Validation Sources between 3-10 GHz			
Calibration date:	July 01, 2021			
The measurements and the uncerta	ainties with confidence p	onal standards, which realize the physical unitrobability are given on the following pages and y facility: environment temperature $(22 \pm 3)^{\circ}$ C	d are part of the certificate.	
Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration	
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03291/03292)	Apr-22	
Power sensor NRP-Z91	SN: 103244	09-Apr-21 (No. 217-03291)	Apr-22	
Power sensor NRP-Z91	SN: 103245	09-Apr-21 (No. 217-03292)	Apr-22	
Power sensor R&S NRP33T	SN: 100967	08-Apr-21 (No. 217-03293)	Apr-22	
D /	SN: BH9394 (20k)	09-Apr-21 (No. 217-03343)	Apr-22	
Reference 20 dB Attenuator		09-Apr-21 (No. 217-03344)	Apr-22	
Reference 20 dB Attenuator Type-N mismatch combination	SN: 310982 / 06327	09-Apr-21 (No. 217-03344)	Apr-ac	
	SN: 310982 / 06327 SN: 7405	30-Dec-20 (No. EX3-7405_Dec20)	Dec-21	
Type-N mismatch combination Reference Probe EX3DV4			Co. Lancoure	
Type-N mismatch combination Reference Probe EX3DV4 DAE4	SN: 7405	30-Dec-20 (No. EX3-7405_Dec20)	Dec-21	
Type-N mismatch combination	SN: 7405 SN: 908	30-Dec-20 (No. EX3-7405_Dec20) 24-Jun-21 (No. DAE4-908_Jun21)	Dec-21 Jun-22	
Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator Anapico APSIN20G	SN: 7405 SN: 908	30-Dec-20 (No. EX3-7405_Dec20) 24-Jun-21 (No. DAE4-908_Jun21) Check Date (in house)	Dec-21 Jun-22 Scheduled Check	
Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards	SN: 7405 SN: 908 ID # SN: 669	30-Dec-20 (No. EX3-7405_Dec20) 24-Jun-21 (No. DAE4-908_Jun21)  Check Date (in house) 28-Mar-17 (in house check Dec-18)	Dec-21 Jun-22 Scheduled Check In house check: Dec-21	
Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator Anapico APSIN20G	SN: 7405 SN: 908 ID # SN: 669 SN: 101093	30-Dec-20 (No. EX3-7405_Dec20) 24-Jun-21 (No. DAE4-908_Jun21)  Check Date (in house) 28-Mar-17 (in house check Dec-18) 10-May-12 (in house check Dec-18)	Dec-21 Jun-22 Scheduled Check In house check: Dec-21 In house check: Dec-21	
Type-N mismatch combination Reference Probe EX3DV4 DAE4 Secondary Standards RF generator Anapico APSIN20G Network Analyzer R&S ZVL13	SN: 7405 SN: 908 ID # SN: 669 SN: 101093	30-Dec-20 (No. EX3-7405_Dec20) 24-Jun-21 (No. DAE4-908_Jun21)  Check Date (in house) 28-Mar-17 (in house check Dec-18) 10-May-12 (in house check Dec-18)	Dec-21 Jun-22 Scheduled Check In house check: Dec-21 In house check: Dec-21	

Certificate No: D6.5GHzV2-1037\_Jul21

Page 1 of 6



Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL ConvF N/A tissue simulating liquid

sensitivity in TSL / NORM x,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.

#### **Additional Documentation:**

b) DASY System Handbook

#### Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point
  exactly below the center marking of the flat phantom section, with the arms oriented parallel to the
  body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned
  under the liquid filled phantom. The impedance stated is transformed from the measurement at the
  SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty
  required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.
- The absorbed power density (APD): The absorbed power density is evaluated according to Samaras T, Christ A, Kuster N, "Compliance assessment of the epithelial or absorbed power density above 6 GHz using SAR measurement systems", Bioelectromagnetics, 2021 (submitted). The additional evaluation uncertainty of 0.55 dB (rectangular distribution) is considered.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D6.5GHzV2-1037\_Jul21

Page 2 of 6



### **Measurement Conditions**

DASY system configuration, as far as not given on page 1.

DASY Version	DASY6	V16.0	
Extrapolation	Advanced Extrapolation		
Phantom	Modular Flat Phantom		
Distance Dipole Center - TSL	5 mm	with Spacer	
Zoom Scan Resolution	dx, dy = 3.4  mm, dz = 1.4  mm	Graded Ratio = 1.4 (Z direction)	
Frequency	6500 MHz ± 1 MHz		

Head TSL parameters
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	34.5	6.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	33.6 ± 6 %	6.12 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

# SAR result with Head TSL

SAR averaged over 1 cm <sup>3</sup> (1 g) of Head TSL	Condition	
SAR measured	100 mW input power	28.8 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	286 W/kg ± 24.7 % (k=2)

SAR averaged over 10 cm <sup>3</sup> (10 g) of Head TSL	condition	
SAR measured	100 mW input power	5.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	52.6 W/kg ± 24.4 % (k=2)

Certificate No: D6.5GHzV2-1037\_Jul21

Page 3 of 6



# Appendix

#### Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.5 Ω - 2.4 jΩ	
Return Loss	- 30.9 dB	

# APD (Absorbed Power Density)

APD averaged over 1 cm <sup>2</sup>	Condition	
APD measured	100 mW input power	286 W/m <sup>2</sup>
APD measured	normalized to 1W	2860 W/m <sup>2</sup> ± 29.2 % (k=2)

APD averaged over 4 cm <sup>2</sup>	condition	
APD measured	100 mW input power	128 W/m <sup>2</sup>
APD measured	normalized to 1W	1280 W/m <sup>2</sup> ± 28.9 % (k=2)

# General Antenna Parameters and Design

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

# **Additional EUT Data**

Manufactured by	SPEAG

Certificate No: D6.5GHzV2-1037\_Jul21

Page 4 of 6



# **DASY6 Validation Report for Head TSL**

Measurement Report for D6.5GHz-1037, UID 0 -, Channel 6500 (6500.0MHz)

**Device under Test Properties** 

Name, Manufacturer D6.5GHz

Dimensions [mm] 16.0 x 6.0 x 300.0

IMEI SN: 1037 DUT Type

**Exposure Conditions** 

Phantom Section, TSL

Position, Test Band Distance [mm] 5.00 Band Group, UID CW,

Frequency Conversion [MHz] Factor 6500 5.75

Measurement Results

6.12

TSL Cond. [S/m] Permittivity

33.6

Hardware Setup Phantom

Flat, HSL

MFP V8.0 Center - 1182

HBBL600-10000V6

Probe, Calibration Date EX3DV4 - SN7405, 2020-12-30 DAE, Calibration Date DAE4 Sn908, 2021-06-24

Scan Setup


Grid Extents [mm] Grid Steps [mm] Sensor Surface [mm] Graded Grid **Grading Ratio** MAIA Surface Detection Scan Method

Zoom Scan 22.0 x 22.0 x 22.0 3.4 x 3.4 x 1.4

Date psSAR1g [W/Kg] psSAR10g [W/Kg] Power Drift [dB] 1.4 Yes Power Scaling N/A Scaling Factor [dB] VMS + 6p TSL Correction Measured M2/M1 [%] Dist 3dB Peak [mm]

Zoom Scan 2021-07-10, 10:54 28.8 5.30 0.00 Disabled

No correction 50.2 4.8




Certificate No: D6.5GHzV2-1037\_Jul21

Page 5 of 6



# Impedance Measurement Plot for Head TSL

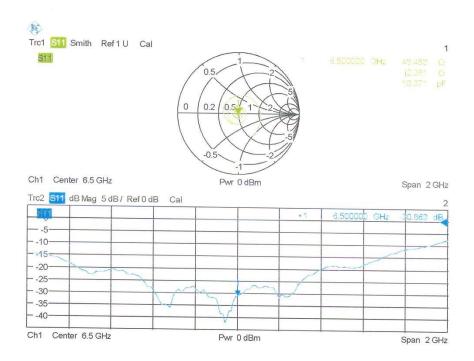

Certificate No: D6.5GHzV2-1037\_Jul21

Page 6 of 6



D6.5GHzV2 Dipole impedance and return loss Validation

2 Dipole impedance a	ind return loss valida	alion	
Meas. Results	Current Meas.	Previous Meas.	Max. Deviation
Meas. Data	2023.05.31	2022.05.31	/
Return Loss(dB)	-29.911 -25.126 19.04%		
Impedance	49.329 Ω -0.432	52.111 Ω -0.153	-2.782Ω
Impodanoo	jΩ	jΩ	(Real part)
	Retur	n Loss	
>Tr1 S11 Log Mag 10.00dB 50.00			
>1 6.5000000	GHZ -29.911 dB		
40.00			
30.00			
20.00			
10.00			
0.000			
d. 650			
-10.00			
-20.00			
		1	
-30.00			
-40.00		VI	
		V	
-50.00 L	IFBW 10	10 Hz	Stop 7.5 GHz Cor
	Impe	dance	
>1 6.5000000 GHz 49.	ale 1.000U [F1] 329 Ω =432.02 mΩ 567677 pF		
1 Start 5.5 GHz	IFBW 10	0 Hz	Stop 7.5 GHz Cor

--END OF REPORT--