

SAR Evaluation Report for

Report No.: SESF1410101

IEEE Std1528-2013 / FCC 47 CFR Part 2 (2.1093) / KDB 248227 D01 v01r02 / KDB 447498 D01 v05r01 / KDB 865664 D01 v01r03

Report No.:1410101

Client	:	DXG Technology Corp.
Product	:	HD Action Camcorder

Model DVS5M9

FCC ID RD2DS5M9001

Manufacturer/ supplier : DXG Technology Corp. Test Date November 13,2014 Date of issue November 14.2014

Test Result Compliance ■Not Compliance

Statement of Compliance:

The SAR values measured for the test sample are below the maximum recommended level of 1.6 W/kg averaged over any 1g tissue according to FCC KDBs and IEEE Std.1528-2013.

The test result only corresponds to the tested sample. It is not permitted to copy this report, in part or in full, without the permission of the test laboratory.

Total number of pages of this test report: 86 pages

The testing described in this report has been carried out to the best of our knowledge and ability, and our responsibility is limited to the exercise of reasonable care. This certification is not intended to believe the sellers from their legal and/or contractual obligations.

Test Engineer: Approved by:

Leo Chen Miro Chueh

Issued Date: November 13th, 2014 Cerpass Technology Corp. Page No. : 1 of 56



Applicant Information

Client : DXG Technology Corp.

15Fl., No. 4, Sec. 3, Ming-Chuan East Road, **Address**

Taipei, Taiwan, R.O.C.

: DXG Technology Corp. Manufacturer

: 15Fl., No. 4, Sec. 3, Ming-Chuan East Road, **Address**

Taipei, Taiwan, R.O.C.

HD Action Camcorder **EUT**

: DVS5M9 Model No.

Standard Applied : IEEE Std1528-2013 and FCC 47 CFR Part 2 (2.1093)

> KDB 248227 D01 v01r02 KDB 447498 D01 v05r01 KDB 865664 D01 v01r03

: CERPASS TECHNOLOGY CORP. Laboratory

No.66, Tangzhuang Road, Suzhou Industrial Park, Jiangsu

Report No.: SESF1410101

215006, China.

Max. Average Power WLAN: 17.03dBm

: 802.11b: 0.915W/kg(1g) Max. Reported SAR Value

Issued Date : November 13th, 2014 Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 2 of 56



Contents

Report No.: SESF1410101

Issued Date : November 13th, 2014

: 3 of 56

Page No.

1.	Gene	ral Information	4
	1.1.	Executive Summary	4
	1.2.	Description of Equipment under Test	4
	1.3.	Antenna Location	5
	1.4.	Test Configuration	5
	1.5.	Simultaneous Transmission Configurations	5
	1.6.	Environment Condition	5
	1.7.	Test Standards	6
	1.8.	RF Exposure Limits	6
2.	The S	SAR Measurement Procedure	7
	2.1.	System Performance Check	7
	2.2.	Test Requirements	10
3.	DASY	'5 Measurement System	
	3.1.	Uncertainty of Inter-/Extrapolation and Averaging	14
	3.2.	DASY5 E-Field Probe	14
	3.3.	Data Acquisition Electronics (DAE)	15
	3.4.	Robot	15
	3.5.	Light Beam Unit	15
	3.6.	Measurement Server	16
	3.7.	SAM Phantom	16
	3.8.	Device Holder	17
	3.9.	Test Equipment List	18
	3.10.	Annul Internal Check of Impedance and Return Loss	19
4.	Resu	lts	20
	4.1.	Summary of Test Results	
	4.2.	Description for EUT test position	20
	4.3.	Conducted power (Average)	20
	4.4.	SAR Test Results Summary	21
		urement Uncertainty	
6.	APPE	NDIX A. SAR System Verification Data	23
9.	APPE	NDIX B. SAR measurement Data	24
7.	APPE	NDIX C Antenna Location, EUT and Test Setup Photographs	32
		NDIX D. Probe Calibration Data	
9.	Appe	ndix E. Dipole Calibration Data	44



1. General Information

1.1. Executive Summary

The EUT is a HD Action camera with operations in 2.4GHz frequency ranges. It contains 802.11b/g/n and BT functions for SAR testing. Camera communicates with the watch accessories by wifi. The measurement was conducted by CERPASS, carried out with the dosimetric assessment system under DASY5. And it conducts according to the IEEE Std.1528-2013 and FCC KDBs for SAR evaluating compliance.

Report No.: SESF1410101

1.2. Description of Equipment under Test

1.2. Description of Equipment under rest				
Product Name	HD Action Camcorder			
Model No.	DVS5M9			
Device Category	Portable			
RF Exposure Environment	Uncontrolled			
Antenna Type	Internal			
Wi-Fi				
Wi-Fi Frequency	802.11b/g/n: 2412 ~ 2462 MHz			
Type of modulation	802.11b:			
	CCK, DQPSK, DBPSK			
	802.11g:			
	64 QAM, 16 QAM, QPSK, BPSK			
	802.11n:			
	BPSK, QPSK, 16-QAM, 64-QAM			
Data Rate	8802.11b:			
	11, 5.5, 2, 1 Mbps;			
	802.11g:			
	54, 48, 36, 24, 18, 12, 9, 6 Mbps			
	802.11n:			
	MCS 0 to 7 for HT20MHz;			
	MCS 0 to 7 for HT40MHz			
Antenna Gain	0.44dBi			

Issued Date : November 13th, 2014 Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 4 of 56

1.3. Antenna Location

Rear of the Camera edge_1

Report No.: SESF1410101



1.4. Test Configuration

Mode	Back	Front	Edge_1	Edge_2	Edge_3	Edge_4
2.4GHz	Yes	No	Yes	Yes	Yes	No

1.5. Simultaneous Transmission Configurations

Note: No simultaneous transmission configuration

1.6. Environment Condition

Item	Target	Measured
Ambient Temperature()	18~25	21.5±2
Temperature of Simulant()	20~22	21±2
Relative Humidity(%RH)	30~70	52

Issued Date: November 13th, 2014 Cerpass Technology Corp.

> Page No. : 5 of 56



CERPASS TECHNOLOGY CORP.

Report No.: SESF1410101

1.7. Test Standards

- 1. IEEE Std.1528-2013
- 2. FCC KDB Publication 447498 D01 General RF Exposure Guidance v05r01
- 3. FCC KDB Publication 865664 D01 SAR Measurement 100 MHz to 6 GHz v01r01
- 4. FCC KDB Publication 248227 D01 SAR measurement for 802 11 a b g v01r02

1.8. RF Exposure Limits

Human Exposure	Basic restrictions for electric, magnetic and electromagnetic fields. (Unin mW/ or W/kg)	
Spatial Peak SAR ¹ (Head and Body)	1.60	
Spatial Average SAR ² (Whole Body)	0.08	
Spatial Peak SAR ³ (Arms and Legs)	4.00	

Notes:

- 1. The Spatial Peak value of the SAR averaged over any 1 gram of tissue (defined as a tissue volume in the shape of a cube) and over the appropriate averaging time.
- 2. The Spatial Average value of the SAR averaged over the whole body.
- 3. The Spatial Peak value of the SAR averaged over any 1 grams of tissue (defined as a tissue volume in the shape of a cube) and over appropriate averaging time.

Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 6 of 56



2. The SAR Measurement Procedure

2.1. System Performance Check

2.1.1 Purpose

- 1. To verify the simulating liquids are valid for testing.
- 2. To verify the performance of testing system is valid for testing.

2.1.2 Tissue Dielectric Parameters for Head and Body Phantoms

Target Frequency	Hea	ad	Во	ody
(MHz)	$\epsilon_{\rm r}$	σ (S/m)	$\epsilon_{\rm r}$	σ (S/m)
150	52.3	0.76	61.9	0.80
300	45.3	0.87	58.2	0.92
450	43.5	0.87	56.7	0.94
835	41.5	0.90	55.2	0.97
850	41.5	0.92	55.2	0.99
900	41.5	0.97	55.0	1.05
915	41.5	0.98	55.0	1.06
1450	40.5	1.20	54.0	1.30
1610	40.3	1.29	53.8	1.40
1800 – 2000	40.0	1.40	53.3	1.52
2450	39.2	1.80	52.7	1.95
3000	38.5	2.40	52.0	2.73
5800	35.3	5.27	48.2	6.00

Report No.: SESF1410101

(ε_r = relative permittivity, σ = conductivity and ρ = 1000 kg/m³)

Cerpass Technology Corp. Issued Date : November 13th, 2014

Page No. : 7 of 56

CERPASS TECHNOLOGY CORP. Report No.: SESF1410101

2.1.3 Tissue Calibration Result

♣ The dielectric parameters of the liquids were verified prior to the SAR evaluation using DASY5 Dielectric Assessment Kit and Agilent Vector Network Analyzer E5071C.

Body Tissue Simulant Measurement						
Frequency	Description	Dielectric P	Tissue Temp.			
[MHz] Description		٤ _٢	σ [s/m]	[°C]		
	Reference result	52.7	1.95	N/A		
2450MHz	± 5% window	50.07 to 55.34	1.85 to 2.05	IN/A		
	10-11-2014	50.62	1.94	21.0		

Refer to KDB 865664 D01 v01r01, The depth of body tissue-equivalent liquid in a phantom must be \geq 15.0 cm with \leq ± 0.5 cm variation for SAR measurements \leq 3 GHz and \geq 10.0 cm with \leq ± 0.5 cm variation for measurements > 3 GHz.

2.1.4 System Performance Check Procedure

The DASY5 installation includes predefined files with recommended procedures for measurements and the system performance check. They are read-only document files and destined as fully defined but unmeasured masks, so the finished system performance check must be saved under a different name. The system performance check document requires the SAM Twin Phantom or ELI4 Phantom, so the phantom must be properly installed in your system. (User defined measurement procedures can be created by opening a new document or editing an existing document file). Before you start the system performance check, you need only to tell the system with which components (probe, medium, and device) you are performing the system performance check; the system will take care of all parameters.

- The Power Reference Measurement and Power Drift Measurement jobs are located at the beginning and end of the batch process. They measure the field drift at one single point in the liquid over the complete procedure. The indicated drift is mainly the variation of the Dipole output power. If it is too high (above ±0.2 dB), the system performance check should be repeated;
- The Surface Check job tests the optical surface detection system of the DASY5 system by repeatedly detecting the surface with the optical and mechanical surface detector and comparing the results. The output gives the detecting heights of both systems, the difference between the two systems and the standard deviation of the detection repeatability. Air bubbles or refraction in the liquid due to separation of the sugar-water mixture gives poor repeatability (above ±0.1mm). In that case it is better to abort the system performance check and stir the liquid;
- The Area Scan job measures the SAR above the dipole on a plane parallel to the surface. It is used to locate the approximate location of the peak SAR. The proposed scan uses large grid spacing for faster measurement; due to the symmetric field, the peak detection is reliable;
- The Zoom Scan job measures the field in a volume around the peak SAR value assessed in the previous Area Scan job (for more information see the application note on SAR evaluation). If the system performance check gives reasonable results. The dipole input power(forward power) was 250mW, 1 g and 10 g spatial average SAR values normalized to 1W dipole input power give reference data for comparisons and it's equal to 10x(dipole forward power). The next sections analyze the expected uncertainties of these values, as well as additional checks for further information or troubleshooting.


Cerpass Technology Corp. Issued Date : November 13th, 2014

Page No.

: 8 of 56




2.1.5 System Performance Check Setup

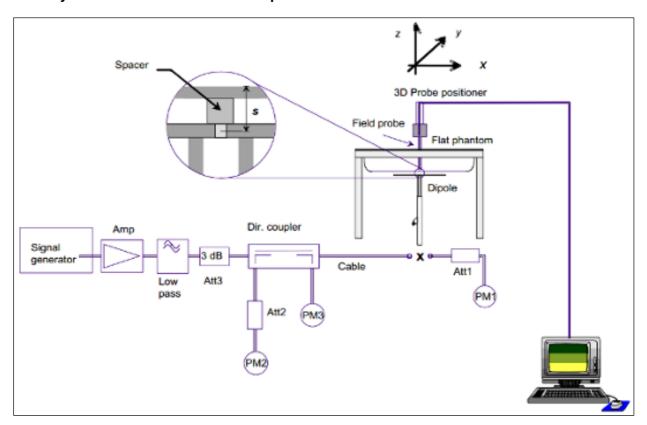

2.1.6 Validation Dipoles

The dipoles use is based on the IEEE Std.1528-2013 and FCC KDB 865664 D01 SAR Measurement 100 MHz to 6 GHz v01r01standard, and is complied with mechanical and electrical specifications in line with the requirements of both EN62209-1 and EN62209-2. The table below provides details for the mechanical and electrical specifications for the dipoles.

Frequency	L (mm)	h (mm)	d (mm)
2450MHz	53.5	30.4	3.6



Report No.: SESF1410101

Cerpass Technology Corp. Issued Date : November 1

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 9 of 56



CERPASS TECHNOLOGY CORP.

Report No.: SESF1410101

2.1.7 Result of System Performance Check: Valid Result

System Performance Check at 2450MHz for Body.

Validation Kit: D2450V2-SN: 914

Frequency [MHz]	Description	SAR [w/kg] 1g	SAR [w/kg] 10g	Tissue Temp. [°C]
2450 MHz	Reference result ± 10% window	51.5 46.35 to 56.65	23.9 21.51 to 26.29	N/A
	10-11-2014	51.2	23.4	21.0

Note: All SAR values are normalized to 1W forward power.

2.2. Test Requirements

2.2.1 Test Procedures

Step 1 Setup a Connection

First, engineer should record the conducted power before the test. Then establish a call in handset at the maximum power level with a base station simulator via air interface, or make the EUT estimate by itself in testing band. Place the EUT to the specific test location. After the testing, must export SAR test data by SEMCAD. Then writing down the conducted power of the EUT into the report, also the SAR values tested.

Step 2 Power Reference Measurements

To measure the local E-field value at a fixed location which value will be taken as a reference value for calculating a possible power drift.

Step 3 Area Scan

The Area Scan is used as a fast scan in two dimensions to find the area of high field values, before doing a fine measurement around the hot spot. The sophisticated interpolation routines implemented in DASY software can find the maximum locations even in relatively coarse grids. When an Area Scan has measured all reachable points, it computes the field maximal found in the scanned area, within a range of the global maximum. The range (in dB) is specified in the standards for compliance testing. For example, a 2 dB range is required in IEEE Standard 1528 and IEC 62209 standards, whereby 3 dB is a requirement when compliance is assessed in accordance with the ARIB standard (Japan). If only one Zoom Scan follows the Area Scan, then only the absolute maximum will be taken as reference. For cases where multiple maximums are detected, the number of Zoom Scans has to be increased accordingly.

Issued Date : November 13th, 2014 Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 10 of 56

Area Scan Parameters extracted from KDB 865664 D01v01r01

	≤3 GHz	> 3 GHz
Maximum distance from closest measurement point (geometric center of probe sensors) to phantom surface	5 ± 1 mm	$\frac{1}{2} \cdot \delta \cdot \ln(2) \pm 0.5 \text{ mm}$
Maximum probe angle from probe axis to phantom surface normal at the measurement location	30° ± 1°	20° ± 1°
	\leq 2 GHz: \leq 15 mm 2 – 3 GHz: \leq 12 mm	3 – 4 GHz: ≤ 12 mm 4 – 6 GHz: ≤ 10 mm
Maximum area scan spatial resolution: Δx_{Area} , Δy_{Area}	When the x or y dimension of the test device, in the measurement plane orientation, is smaller than the about the measurement resolution must be \leq the corresponding x or y dimension of the test device with at least one measurement point on the test device.	

Step 4 Zoom Scan

Zoom Scans are used to assess the peak spatial SAR values within a cubic averaging volume containing 1 g and 10 g of simulated tissue. The Zoom Scan measures points (refer to table below) within a cube whose base faces are centered on the maxima found in a preceding area scan job within the same procedure. When the measurement is done, the Zoom Scan evaluates the averaged SAR for 1 g and 10 g and displays these values next to the job's label.

Zoom Scan Parameters extracted from KDB 865664 D01 v01r01

			≤ 3 GHz	> 3 GHz
Maximum zoom scan s	spatial reso	olution: Δx_{Zoom} , Δy_{Zoom}	\leq 2 GHz: \leq 8 mm 2 – 3 GHz: \leq 5 mm [*]	3 – 4 GHz: ≤ 5 mm* 4 – 6 GHz: ≤ 4 mm*
	uniform grid: Δz _{Zoom} (n)		≤ 5 mm	$3-4 \text{ GHz}: \le 4 \text{ mm}$ $4-5 \text{ GHz}: \le 3 \text{ mm}$ $5-6 \text{ GHz}: \le 2 \text{ mm}$
Maximum zoom scan spatial resolution, normal to phantom surface	n graded	Δz _{Zoom} (1): between 1 st two points closest to phantom surface	≤ 4 mm	$3-4 \text{ GHz: } \le 3 \text{ mm}$ $4-5 \text{ GHz: } \le 2.5 \text{ mm}$ $5-6 \text{ GHz: } \le 2 \text{ mm}$
	grid $\Delta z_{Zoom}(n>1)$: between subsequent points		≤ 1.5 ⋅ 1	Δz _{Zoom} (n-1)
Minimum zoom scan volume	x, y, z		≥ 30 mm	3 – 4 GHz: ≥ 28 mm 4 – 5 GHz: ≥ 25 mm 5 – 6 GHz: ≥ 22 mm

Note: δ is the penetration depth of a plane-wave at normal incidence to the tissue medium; see draft standard IEEE P1528-2011 for details.

Step 5 Power Drift Measurements

Repetition of the E-field measurement at the fixed location mentioned in Step 1 to make sure the two results differ by less than ± 0.2 dB.

Issued Date: November 13th, 2014 Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 11 of 56

When zoom scan is required and the reported SAR from the area scan based 1-g SAR estimation procedures of KDB 447498 is $\leq 1.4 \text{ W/kg}, \leq 8 \text{ mm}, \leq 7 \text{ mm}$ and $\leq 5 \text{ mm}$ zoom scan resolution may be applied, respectively, for 2 GHz to 3 GHz, 3 GHz to 4 GHz and 4 GHz to 6 GHz.



CERPASS TECHNOLOGY CORP. Report No.: SESF1410101

2.2.2 Test Channel Choosing

- 1. 1) Per KDB 248227 D01v01r02, SAR is not required for 802.11g/HT20 channels when the maximum average output power is less than 1/4 dB higher than that measured on the corresponding 802.11b channels.
 - 2) SAR is not required for Channels 12 and 13, if the tune-up limit and the measured output power for these two channels are no greater than those for the default test channels.

Mode			Tunks	"De	fault Test	Channels"	
	GHz	Channel	Turbo Channel	§15	.247	UNII	
			Channel	802.11b	802.11g	UNII	
802.11 b/g	2.412	1#		√	∇		
	2.437	6	6	√ √	∇		
	2.462	11#		√ √	∇		

- √ = "default test channels"
- * = possible 802.11a channels with maximum average output > the "default test channels"
- ∇ = possible 802.11g channels with maximum average output ¼ dB ≥ the "default test channels"
- # = when output power is reduced for channel 1 and/or 11 to meet restricted band requirements the highest output channels closest to each of these channels should be tested

Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 12 of 56



3. DASY5 Measurement System

DASY5 Measurement System

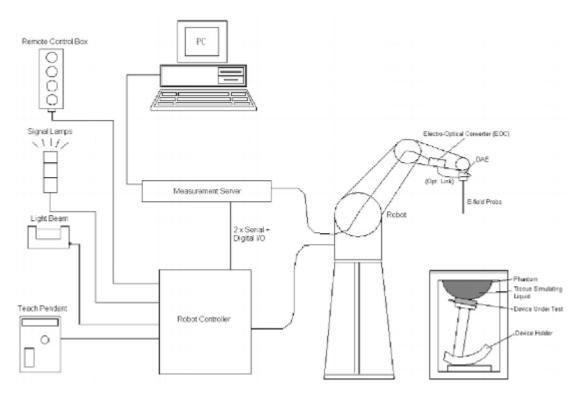


Figure 2.1 SPEAG DASY5 System Configurations

Report No.: SESF1410101

The DASY5 system for performance compliance tests is illustrated above graphically. This system consists of the following items:

- A standard high precision 6-axis robot with controller, a teach pendant and software
- ♦ A data acquisition electronic(DAE)attached to the robot arm extension
- ♦ A dosimetric probe equipped with an optical surface detector system
- The electro-optical converter(ECO)performs the conversion between optical and electrical signals
- ♦ A measurement server performs the time critical tasks such as signal filtering, control of the robot operation and fast movement interrupts.
- ♦ A probe alignment unit which improves the accuracy of the probe positioning
- ♦ A computer operating Windows 7
- ♦ DASY5 software
- Remove control with teach pendant additional circuitry for robot safety such as warming lamps, etc.
- ♦ The SAM twin phantom
- ♦ A device holder
- ♦ Tissue simulating liquid
- Dipole for evaluating the proper functioning of the system

Cerpass Technology Corp. Issued Date : November 13th, 2014

Page No.

: 13 of 56



3.1. Uncertainty of Inter-/Extrapolation and Averaging

In order to evaluate the uncertainty of the interpolation, extrapolation and averaged SAR calculation algorithms of the Postprocessor, DASY5 allows the generation of measurement grids which are artificially predefined by analytically based test functions. Therefore, the grids of area scans and zoom scans can be filled with uncertainty test data, according to the SAR benchmark functions of IEEE 1528. The three analytical functions shown in equations as below are used to describe the possible range of the expected SAR distributions for the tested handsets. The field gradients are covered by the spatially flat distribution f1, the spatially steep distribution f3 and f2 accounts for H-field cancellation on the phantom/tissue surface.

Report No.:

SESF1410101

$$\begin{split} f_1(x,y,z) &= A e^{-\frac{z}{2a}} \cos^2 \left(\frac{\pi}{2} \frac{\sqrt{x'^2 + y'^2}}{5a} \right) \\ f_2(x,y,z) &= A e^{-\frac{z}{a}} \frac{a^2}{a^2 + x'^2} \left(3 - e^{-\frac{2z}{a}} \right) \cos^2 \left(\frac{\pi}{2} \frac{y'}{3a} \right) \\ f_3(x,y,z) &= A \frac{a^2}{\frac{a^2}{4} + x'^2 + y'^2} \left(e^{-\frac{2z}{a}} + \frac{a^2}{2(a+2z)^2} \right) \end{split}$$

3.2. DASY5 E-Field Probe

The SAR measurement is conducted with the dosimetric probe manufactured by SPEAG. The probe is specially designed and calibrated for use in liquid with high permittivity. The dosimetric probe has special calibration in liquid at different frequency.

SPEAG conducts the probe calibration in compliance with international and national standards (e.g. IEEE 1528, EN 62209-1, IEC 62209, etc.) under ISO 17025. The calibration data are in Appendix D.

Model	EX3DV4	
Construction	Symmetrical design with triangular core Built-in shieldin	g against static charges
	PEEK enclosure material (resistant to organic solvents,	e.g., DGBE)
Frequency	10 MHz to 6 GHz	
	Linearity: ± 0.2 dB (30 MHz to 6 GHz)	
Directivity	± 0.3 dB in HSL (rotation around probe axis)	
	± 0.5 dB in tissue material (rotation normal to probe	
	axis)	
Dynamic Range	10 μW/g to 100 mW/g	
	Linearity: ± 0.2 dB (noise: typically < 1 μW/g)	
Dimensions	Overall length: 330 mm (Tip: 20 mm)	
	Tip diameter: 2.5 mm (Body: 12 mm)	
	Typical distance from probe tip to dipole centers: 1 mm	
Application	High precision dosimetric measurements in any expos	sure scenario (e.g., very
	strong gradient fields). Only probe which enables	compliance testing for
	frequencies up to 6 GHz with precision of better 30%.	

Cerpass Technology Corp.

Issued Date: November 13th, 2014




3.3. Data Acquisition Electronics (DAE)

The data acquisition electronics (DAE) consists of a highly sensitive electrometer-grade preamplifier with auto-zeroing, a channel and gain-switching multiplexer, a fast 16 bit AD-converter and a command decoder and control logic unit.

Transmission to the measurement server is accomplished through an optical downlink for data and status information as well as an optical uplink for commands and the clock.

The input impedance of the DAE4 is 200M Ohm; the inputs are symmetrical and floating. Common mode rejection is above 80dB.



Report No.: SESF1410101

3.4. Robot

The DASY5 system uses the high precision robots TX90 XL type out of the newer series from Stäubli SA (France). For the 6-axis controller DASY5 system, the CS8C robot controller version from Stäubli is used.

The XL robot series have many features that are important for our application:

- High precision (repeatability 0.02 mm)
- → High reliability (industrial design)
- ♦ Jerk-free straight movements
- Low ELF interference (the closed metallic construction shields against motor control fields)
- ♦ 6-axis controller

3.5. Light Beam Unit

The light beam switch allows automatic "tooling" of the probe. During the process, the actual position of the probe tip with respect to the robot arm is measured, as well as the probe length and the horizontal probe offset. The software then corrects all movements, such that the robot coordinates are valid for the probe tip.

The repeatability of this process is better than 0.1 mm. If a position has been taught with an aligned probe, the same position will be reached with another aligned probe within 0.1 mm, even if the other probe has different dimensions. During probe rotations, the probe tip will keep its actual position.





Cerpass Technology Corp. Issued Date: November 13th, 2014

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 15 of 56

CERPASS TECHNOLOGY CORP. Report No.: SESF1410101

3.6. Measurement Server

The DASY5 measurement server is based on a PC/104 CPU board with a 400MHz intel ULV Celeron, 128MB chipdisk and 128MB RAM. The necessary circuits for communication with the DAE electronics box, as well as the 16 bit AD converter system for optical detection and digital I/O interface are contained on the DASY5 I/O board, which is directly connected to the PC/104 bus of the CPU board.



3.7. SAM Phantom

The SAM twin phantom is a fiberglass shell phantom with 2mm shell thickness (except the ear region where shell thickness increases to 6mm). It has three measurement areas:

- ♦ Left head
- ♦ Right head
- ♦ Flat phantom

The ELI4 Phantom also is a fiberglass shell phantom with 2mm shell thickness. It has 30 liters filling volume, and with a dimension of 600mm for major ellipse axis, 400mm for minor axis. It is intended for compliance testing of handheld and body-mounted wireless devices in frequency range of 30 MHz to 6GHz. ELI4 is fully compatible with standard and all known tissue simulating liquids.





The bottom plate contains three pair of bolts for locking the device holder. The device holder positions are adjusted to the standard measurement positions in the three sections. A white cover is provided to tap the phantom during off-periods to prevent water evaporation and changes in the liquid parameters. On the phantom top, three reference markers are provided to identify the phantom position with respect to the robot.

Issued Date: November 13th, 2014

Page No. : 16 of 56


CERPASS TECHNOLOGY CORP. Report No.: SESF1410101

3.8. Device Holder

♦ The DASY5 device holder is designed to cope with different positions given in the standard. It has two scales for the device rotation (with respect to the body axis) and the device inclination (with respect to the line between the ear reference points). The rotation center for both scales is the ear reference point (EPR). Thus the device needs no repositioning when changing the angles. The DASY5 device holder has been made out of low-loss POM material having the following dielectric parameters: relative permittivity $\varepsilon r = 3$ and loss tangent $\delta = 0.02$. The amount of dielectric material has been reduced in the closest vicinity of the device, since measurements have suggested that the influence of the clamp on the test results could thus be lowered.



♦ The laptop extension is lightweight and made of POM, acrylic glass and foam. It fits easily on upper part of the mounting device in place of the phone positioned. The extension is fully compatible with the SAM Twin and ELI phantoms.



Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No.

Issued Date: November 13th, 2014

: 17 of 56



3.9. Test Equipment List

Instrument	Manufacturer	Model No.	Serial No.	Cali. Due Date
Stäubli Robot TX60L	Stäubli	TX60L	5P6VA1/A/01	only once
Controller	Stäubli	SP1	1371	only once
Dipole Validation Kits	Speag	D850V2	1008	2015.06.12
Dipole Validation Kits	Speag	D1750V2	1097	2015.06.10
Dipole Validation Kits	Speag	D1900V2	5d174	2015.06.09
Dipole Validation Kits	Speag	D2450V2	914	2015.06.06
SAM Twin Phantom	Speag	SAM	1767	N/A
Device Holder	Speag	SD 000 H01 KA	N/A	N/A
Laptop Holder	Speag	SM LH1 001CD	N/A	N/A
Data Acquisition Electronic	Speag	DAE4	1739	2015.05.23
E-Field Probe	Speag	EX3DV4	3927	2015.05.19
SAR Software	Speag	DASY5	V5.2 Build 162	N/A
Power Amplifier	Mini-Circuit	ZVA-183W-S+	MN136701248	N/A
Directional Coupler	Agilent	772D	MY52180104	N/A
Universal Radio Communication Tester	R&S	CMU 200	108823	2015.01.08
Vector Network	Agilent	E5071C	MY4631693	2015.01.15
Signal Generator	R&S	SML	103287	2015.03.09
Power Meter	BONN	BLWA0830-160/100/40D	76659	2015.11.10
AUG Power Sensor	R&S	NRP-Z91	100384	2015.03.09

Report No.: SESF1410101


Cerpass Technology Corp. Issued Date: November 13th, 2014

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 18 of 56




3.10. Annul Internal Check of Impedance and Return Loss

2450MHz Body calibrated impedance 52.051 Ω ; measured impedance: 50.948 Ω (within 5 Ω)

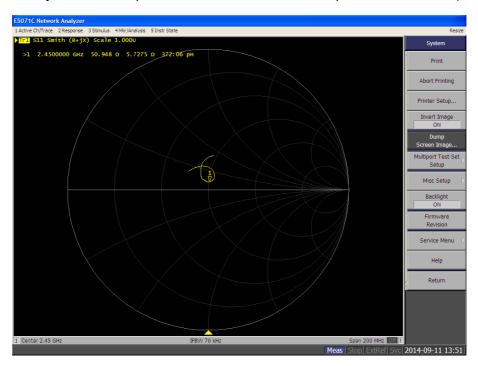

2450MHz Body calibrated return loss: -28.024 dB; Measured return loss: -26.968dB (within 20%)

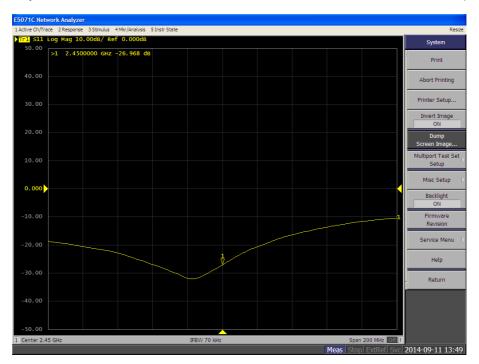

Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 19 of 56

4. Results

4.1. Summary of Test Results

No deviations form the technical specification(s) were ascertained in the course of the tests performed	
The deviations as specified in this chapter were ascertained in the course of the tests Performed.	

Report No.: SESF1410101

4.2. Description for EUT test position

The following procedure had been used to prepare the EUT for the SAR test.

- ♦ The client supplied a special driver to program the EUT, allowing it to continually transmit the specified maximum power and change the channel frequency.
- ♦ The output power(dBm) we measured before SAR test in different channel
- ♦ Performing the highest output power channel first
- ♦ SAR test Tip edge and Bottom Flat mode.

4.3. Conducted power (Average)

WLAN

Test Mode	Channel No.	Frequency (MHz)	Average Power (dBm)	Max. Power (dBm)	Scaling Factor
	01	2412	14.32	14.5	1.04
802.11b	06	2437	16.34	16.5	1.04
	11	2462	17.03	17.5	1.11
	01	2412	10.20	10.5	1.07
802.11g	06	2437	11.86	12.5	1.16
	11	2462	12.62	13.0	1.09
	01	2412	11.03	11.5	1.11
802.11n (20MHz)	06	2437	12.26	12.5	1.06
	11	2462	13.22	13.5	1.07

Note 1: Justification for reduced test configurations for Wi-Fi channels Per KDB Publication 248227 D01v01r02 and KDB 447498 D01v05r01.

- 2: For 2.4 GHz, highest average RF output power channels for 5.5Mbps rate for IEEE 802.11b were selected for SAR evaluation. Other IEEE 802.11 modes (including 802.11g/n) were not investigated since the average output powers over all channels and data rates were not more than 0.25 dB higher than the tested channel in the lowest data rate of IEEE 802.11b mode.
- 3: When the maximum extrapolated peak SAR of the zoom scan for the maximum output channel is <1.6 W/kg and the reported 1g averaged SAR is <0.8 W/kg, SAR testing on other channels is not required. Otherwise, the other default (or corresponding required) test channels were additionally tested using the lowest data rate.
- 4: The bolded channel above was firstly tested for SAR.

Issued Date: November 13th, 2014 Cerpass Technology Corp. Page No. : 20 of 56

4.4. SAR Test Results Summary

SAR MEASUREMENT	
Ambient Temperature (°C): 21.5 ± 2	Relative Humidity (%): 52
Liquid Temperature (°C): 21.0 ± 2	Depth of Liquid (cm):>15

Product: Mobile Phone

Camera Body Worn Configuration

Test Mode: 802.11b (Max. Tune-up power: 17.5dBm)

Test Position Flat	Antenna	Freq	uency	Avg. Power	Power Drift	SAR 1g	Scaling	Scaled SAR 1g	Limit	
(0mm gap)	Position	Ch.	MHz	(dBm)	(<±0.2) (W/kg)		Factor	(W/kg)	(W/kg)	
Back	Fixed	1	2412	14.32	-0.05	0.66	1.04	0.686	1.6	
Back	Fixed	6	2437	16.34	-0.05	0.692	1.04	0.720	1.6	
Back	Fixed	11	2462	17.03	-0.13	0.824	1.11	0.915	1.6	
Back*	Fixed	11	2462	17.03	0.11	0.810	1.11	0.899	1.6	
Edge1	Fixed	11	2462	17.03	-0.12	0.092	1.11	0.102	1.6	
Edge2	Fixed	11	2462	17.03	0.18	0.564	1.11	0.626	1.6	
Edge3	Fixed	11	2462	17.03	-0.12	0.272	1.11	0.302	1.6	

Note: * - repeated at the highest SAR measurement according to the FCC KDB 865664

Issued Date: November 13th, 2014 Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 21 of 56



5. Measurement Uncertainty

	D	ASY5 Und	ertainty	/ Budge	et			
	according	to IEEE 15	28/2011	(0.3-3G	Hz range	e)		
Error Description	Uncert.	Prob.	Div.	(ci)	(ci)	Std.Unc.	Std. nc.	(vi)
	value	Dist.		1g	10g	(1g)	(10g)	veff
Measurement System					•		•	
Probe Calibration	±6.0%	N	1	1	1	±6.0%	±6.0%	∞
Axial Isotropy	±4.7%	R	√3	0.7	0.7	±1.9%	±1.9%	∞
Hemispherical Isotropy	±9.6%	R	√3	0.7	0.7	±3.9%	±3.9%	∞
Boundary Effects	±1.0%	R	√3	1	1	±0.6%	±0.6%	∞
Linearity	±4.7%	R	√3	1	1	±2.7%	±2.7%	∞
System Detection Limits	±1.0%	R	√3	1	1	±0.6%	±0.6%	∞
Modulation Response	±2.4%	R	√3	1	1	±1.4%	±1.4%	∞
Readout Electronics	±0.3%	N	1	1	1	±0.3%	±0.3%	∞
Response Time	±0.8%	R	√3	1	1	±0.5%	±0.5%	∞
Integration Time	±2.6%	R	√3	1	1	±1.5%	±1.5%	∞
RF Ambient Noise	±3.0%	R	√3	1	1	±1.7%	±1.7%	∞
RF Ambient Reflections	±3.0%	R	√3	1	1	±1.7%	±1.7%	∞
Probe Positioner	±0.4%	R	√3	1	1	±0.2%	±0.2%	∞
Probe Positioning	±2.9%	R	√3	1	1	±1.7%	±1.7%	∞
Max.SAR Eval.	±2.0%	R	√3	1	1	±1.2%	±1.2%	∞
Test Sample Related		•	•		•	•	•	•
Device Positioning	±2.9%	N	1	1	1	±2.9%	±2.9%	145
Device Holder	±3.6%	N	1	1	1	±3.6%	±3.6%	5
Power Drift	±5.0%	R	√3	1	1	±2.9%	±2.9%	∞
Power Scaling ^p	±0%	R	√3	0	0	±0%	±0%	∞
Phantom and Setup		•	•		•	•	•	•
Phantom Uncertainty	±6.1%	R	√3	1	1	±3.5%	±3.5%	∞
SAR correction	±1.9%	R	√3	1	0.84	±1.1%	±0.9%	∞
Liquid Conductivity (mea.) ^{DAK}	±2.5%	R	√3	0.78	0.71	±1.1%	±1.0%	∞
Liquid Permittivity (mea.) ^{DAK}	±2.5%	R	√3	0.26	0.26	±0.3%	±0.4%	∞
Temp. unc. –Conductivity ^{BB}	±3.4%	R	√3	0.78	0.71	±1.5%	±1.4%	∞
Temp. unc. – Permittivity ^{BB}	±0.4%	R	√3	0.23	0.26	±0.1%	±0.1%	∞
Combined Std. Uncertainty						±11.2%	±11.1%	361
Expanded STD Uncertainty(Co	verage factor=	:2)				±22.3%	±22.2%	

Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666

Issued Date: November 13th, 2014

Page No. : 22 of 56

6. APPENDIX A. SAR System Verification Data

Date/Time: 10/11/2014

Report No.: SESF1410101

Test Laboratory: Cerpass Lab

SystemPerformanceCheck-D2450 Body

DUT: Dipole 2450 MHz D2450V2; Type: D2450V2

Communication System: CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz; $\sigma = 1.94$ S/m; $\epsilon r = 50.62$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Meas. Ambient Temp (celsius) -22°C; Input power-250mW

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY Configuration:

- Probe: EX3DV4 SN3927; ConvF(7.63, 7.63, 7.63); Calibrated: 2014/5/23;
- Sensor-Surface: 4mm (Mechanical Surface Detection), z = 1.0, 31.0
- Electronics: DAE4 Sn1379; Calibrated: 2014/5/19
- Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)


Configuration/SystemPerformanceCheck-D2450 Body/Area Scan (4x6x1): Measurement grid:

dx=15mm, dy=15mm, Maximum value of SAR (measured) = 10.4 W/kg

Configuration/SystemPerformanceCheck-D2450 Body/Zoom Scan

(7x7x7)/Cube0: Measurement grid: dx=5mm, dy=5mm, dz=5mm, Reference Value = 89.29 V/m; Power Drift = 0.04 dB, Peak SAR (extrapolated) = 27.5 W/kg

SAR(1 g) = 12.8 W/kg; SAR(10 g) = 5.85 W/kg Maximum value of SAR (measured) = 14.7 W/kg

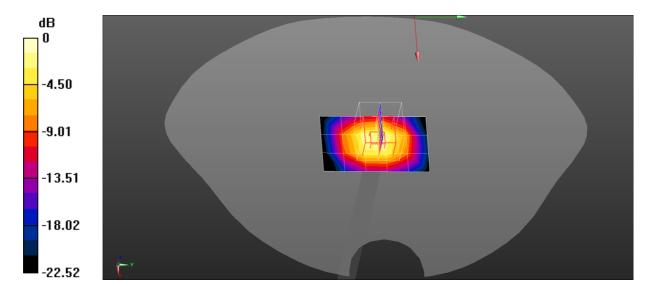

0 dB = 14.7 W/kg = 11.67 dBW/kg

Issued Date: November 13th, 2014 Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666

Page No.

9. APPENDIX B. SAR measurement Data

Date/Time: 10/11/2014

Report No.: SESF1410101

Test Laboratory: Cerpass Lab

DUT: HD Action camera; Type: DVS5M9

Procedure Name: 802.11b 2412MHz Low Camera Body Worn-Back Position

Communication System Band: 802.11b; Frequency: 2412 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2412 MHz; $\sigma = 1.89$ S/m; $\epsilon r = 50.91$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Tissue Temp (celsius) - 21 °C Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY5 Configuration:

Probe: EX3DV4 - SN3927; ConvF(7.63, 7.63, 7.63); Calibrated: 2014/5/23;

• Sensor-Surface: 4mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn1379; Calibrated: 2014/5/19

Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD

Measurement SW: DASY52, Version 52.8 (8);

Configuration/802.11b 2412MHz Low Camera Body Worn-Back Position/Area Scan (7x11x1):


Measurement grid: dx=12mm, dy=12mm, Maximum value of SAR (measured) = 0.790 W/kg

Configuration/802.11b 2412MHz Low Camera Body Worn-Back Position/Zoom Scan

(5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 2.852 V/m;

Power Drift = -0.05 dB, Peak SAR (extrapolated) = 1.23 W/kg

SAR(1 g) = 0.660 W/kg; SAR(10 g) = 0.300 W/kg Maximum value of SAR (measured) = 0.752 W/kg

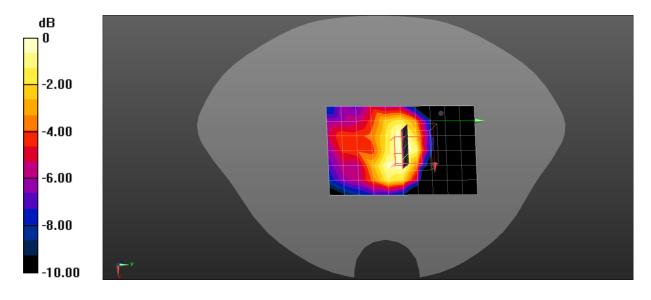

0 dB = 0.752 W/kg = -1.24 dBW/kg

Cerpass Technology Corp. Issued Date : November 13th, 2014

Page No.

: 24 of 56

Date/Time: 10/11/2014

Report No.: SESF1410101

Test Laboratory: Cerpass Lab

DUT: HD Action camera; Type: DVS5M9

Procedure Name: 802.11b 2437MHz Mid Camera Body Worn-Back Position

Communication System Band: 802.11b; Frequency: 2437 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2437 MHz; σ = 1.93 S/m; ϵ r = 50.72; ρ = 1000 kg/m3

Phantom section: Flat Section; Tissue Temp (celsius) - 21 °C Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY5 Configuration:

- Probe: EX3DV4 SN3927; ConvF(7.63, 7.63, 7.63); Calibrated: 2014/5/23;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1379; Calibrated: 2014/5/19
- Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD
- Measurement SW: DASY52, Version 52.8 (8);


Configuration/802.11b 2437MHz Mid Camera Body Worn-Back Position/Area Scan (7x11x1):

Measurement grid: dx=12mm, dy=12mm, Maximum value of SAR (measured) = 0.829 W/kg

Configuration/802.11b 2437MHz Mid Camera Body Worn-Back Position/Zoom Scan

(5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 2.863 V/m; Power Drift = -0.05 dB, Peak SAR (extrapolated) = 1.29 W/kg

SAR(1 g) = 0.692 W/kg; SAR(10 g) = 0.314 W/kg Maximum value of SAR (measured) = 0.789 W/kg

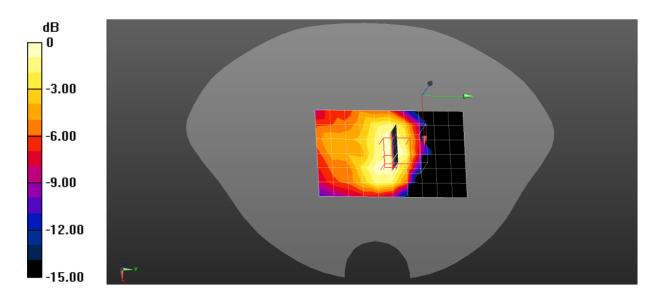

0 dB = 0.789 W/kg = -1.03 dBW/kg

Issued Date: November 13th, 2014 Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666

Page No.

Date/Time: 10/11/2014

Report No.: SESF1410101

Test Laboratory: Cerpass Lab

DUT: HD Action camera; Type: DVS5M9

Procedure Name: 802.11b 2462MHz High Camera Body Worn-Back Position

Communication System Band: 802.11b; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz; $\sigma = 1.96$ S/m; $\epsilon r = 50.53$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Tissue Temp (celsius) - 21 °C Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY5 Configuration:

- Probe: EX3DV4 SN3927; ConvF(7.63, 7.63, 7.63); Calibrated: 2014/5/23;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1379; Calibrated: 2014/5/19
- Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD
- Measurement SW: DASY52, Version 52.8 (8);

Configuration/802.11b 2462MHz High Camera Body Worn-Back Position/Area Scan (6x9x1):


Measurement grid: dx=15mm, dy=15mm, Maximum value of SAR (measured) = 0.931 W/kg

Configuration/802.11b 2462MHz High Camera Body Worn-Back Position/Zoom Scan

(5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 3.289 V/m;

Power Drift = -0.13 dB, Peak SAR (extrapolated) = 1.65 W/kg

SAR(1 g) = 0.824 W/kg; SAR(10 g) = 0.385 W/kg Maximum value of SAR (measured) = 0.899 W/kg

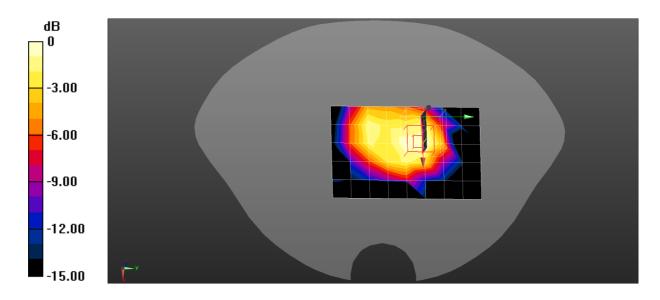

0 dB = 0.899 W/kg = -0.46 dBW/kg


Cerpass Technology Corp. Issued Date : November 13th, 2014

Page No.

: 26 of 56



Z-Axis Plot

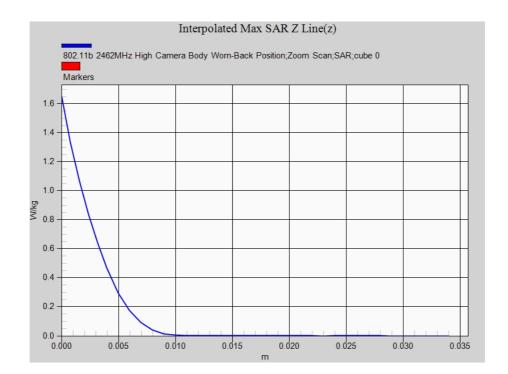

Report No.: SESF1410101

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No.

Date/Time: 10/11/2014

Test Laboratory: Cerpass Lab

DUT: HD Action camera; Type: DVS5M9

Procedure Name: 802.11b 2462MHz High Camera Body Worn-Back Position*

Communication System Band: 802.11b; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz; σ = 7.63 S/m; ϵ r = 50.53; ρ = 1000 kg/m3

Phantom section: Flat Section; Tissue Temp (celsius) - 21 °C Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY5 Configuration:

- Probe: EX3DV4 SN3927; ConvF(7.63, 7.63, 7.63); Calibrated: 2014/5/23;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1379; Calibrated: 2014/5/19
- Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD
- Measurement SW: DASY52, Version 52.8 (8);

Configuration/802.11b 2462MHz High Camera Body Worn-Back Position/Area Scan

(6x9x1): Measurement grid: dx=15mm, dy=15mm, Maximum value of SAR (measured) = 0.916 W/kg


Configuration/802.11b 2462MHz High Camera Body Worn-Back Position/Zoom Scan

(5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 3.289 V/m; Power Drift = 0.11 dB

Peak SAR (extrapolated) = 1.62 W/kg

SAR(1 g) = 0.810 W/kg; SAR(10 g) = 0.379 W/kg Maximum value of SAR (measured) = 0.884 W/kg

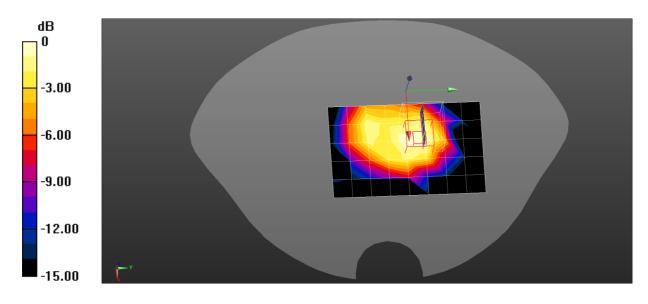

0 dB = 0.884 W/kg = -0.54 dBW/kg

Issued Date: November 13th, 2014

Page No.

: 28 of 56

Date/Time: 10/11/2014

Test Laboratory: Cerpass Lab

DUT: HD Action camera; Type: DVS5M9

Procedure Name: 802.11b 2462MHz High Camera Body Worn-Edge_1 Position

Communication System Band: 802.11b; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz; σ = 1.96 S/m; ϵ r = 50.53; ρ = 1000 kg/m3

Phantom section: Flat Section; Tissue Temp (celsius) - 21 °C Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY5 Configuration:

- Probe: EX3DV4 SN3927; ConvF(7.63, 7.63, 7.63); Calibrated: 2014/5/23;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1379; Calibrated: 2014/5/19
- Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD
- Measurement SW: DASY52, Version 52.8 (8);

Configuration/802.11b 2462MHz High Camera Body Worn-Edge_1 Position/Area Scan (7x11x1):


Measurement grid: dx=12mm, dy=12mm, Maximum value of SAR (measured) = 0.0946 W/kg

Configuration/802.11b 2462MHz High Camera Body Worn-Edge_1 Position/Zoom Scan

(5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 6.271 V/m;

Power Drift = -0.12 dB, Peak SAR (extrapolated) = 0.185 W/kg

SAR(1 g) = 0.092 W/kg; SAR(10 g) = 0.046 W/kg Maximum value of SAR (measured) = 0.102 W/kg

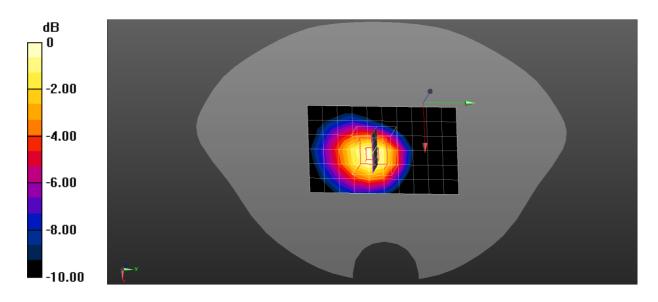

0 dB = 0.102 W/kg = -9.91 dBW/kg

Issued Date: November 13th, 2014 Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666

: 29 of 56

Page No.

Date/Time: 10/11/2014

Test Laboratory: Cerpass Lab

DUT: HD Action camera; Type: DVS5M9

Procedure Name: 802.11b 2462MHz High Camera Body Worn-Edge_2 Position

Communication System Band: 802.11b; Frequency: 2462 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2462 MHz; $\sigma = 1.96$ S/m; $\epsilon r = 50.53$; $\rho = 1000$ kg/m3

Phantom section: Flat Section; Tissue Temp (celsius) - 21° C Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY5 Configuration:

- Probe: EX3DV4 SN3927; ConvF(7.63, 7.63, 7.63); Calibrated: 2014/5/23;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1379; Calibrated: 2014/5/19
- Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD
- Measurement SW: DASY52, Version 52.8 (8);


Configuration/802.11b 2462MHz High Camera Body Worn-Edge_2 Position/Area Scan (6x9x1):

Measurement grid: dx=15mm, dy=15mm, Maximum value of SAR (measured) = 0.726 W/kg

Configuration/802.11b 2462MHz High Camera Body Worn-Edge_2 Position/Zoom Scan

(5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 1.471 V/m; Power Drift = 0.18 dB, Peak SAR (extrapolated) = 2.69 W/kg

SAR(1 g) = 0.564 W/kg; SAR(10 g) = 0.156 W/kg Maximum value of SAR (measured) = 0.642 W/kg

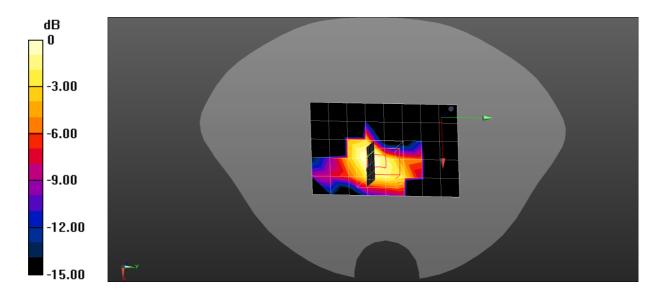

0 dB = 0.642 W/kg = -1.92 dBW/kg

Cerpass Technology Corp. Issued Date : November 13th, 2014

Page No.

: 30 of 56

Date/Time: 10/11/2014

Report No.: SESF1410101

Test Laboratory: Cerpass Lab

DUT: HD Action camera; Type: DVS5M9

Procedure Name: 802.11b 2462MHz High Camera Body Worn-Edge_3 Position

Communication System Band: 802.11b; Frequency: 2462 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2462 MHz; σ = 1.96 S/m; ϵ r = 50.53; ρ = 1000 kg/m3

Phantom section: Flat Section; Tissue Temp (celsius) - 21 °C Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY5 Configuration:

- Probe: EX3DV4 SN3927; ConvF(7.63, 7.63, 7.63); Calibrated: 2014/5/23;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn1379; Calibrated: 2014/5/19
- Phantom: SAM (30deg probe tilt) with CRP v5.0; Type: QD000P40CD
- Measurement SW: DASY52, Version 52.8 (8);

Configuration/802.11b 2462MHz High Camera Body Worn-Edge_3 Position/Area Scan (7x11x1):


Measurement grid: dx=12mm, dy=12mm, Maximum value of SAR (measured) = 0.281 W/kg

Configuration/802.11b 2462MHz High Camera Body Worn-Edge_3 Position/Zoom Scan

(5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm, Reference Value = 6.271 V/m;

Power Drift = -0.12 dB, Peak SAR (extrapolated) = 0.549 W/kg

SAR(1 g) = 0.272 W/kg; SAR(10 g) = 0.137 W/kg Maximum value of SAR (measured) = 0.304 W/kg

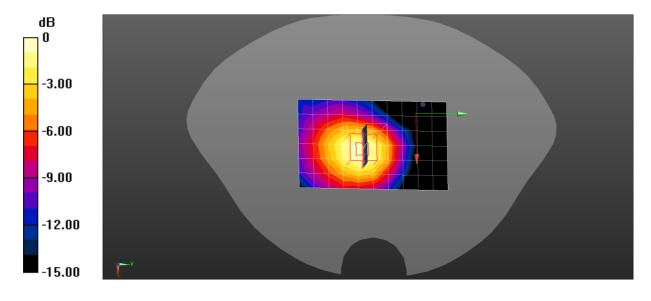

0 dB = 0.304 W/kg = -5.17 dBW/kg

Issued Date: November 13th, 2014 Cerpass Technology Corp.

Tel:86-512-6917-5888 Fax:86-512-6917-5666

Page No.



7. APPENDIX C Antenna Location, EUT and Test Setup Photographs

Report No.: SESF1410101

Note: Antenna Location, EUT and test setup photograph, see separate documents in PDF, named FCC SAR-Appendix C-Antenna internal/outside view Photographs and FCC SAR-Appendix C-Test Setup Photographs.

Cerpass Technology Corp. Issued Date: November 13th, 2014

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 32 of 56



CERPASS TECHNOLOGY CORP.

8. APPENDIX D. Probe Calibration Data

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Cerpass (Auden)

Certificate No: EX3-3927 May14

Accreditation No.: SCS 108

C

Report No.: SESF1410101

CALIBRATION CERTIFICATE

Object

EX3DV4 - SN:3927

Calibration procedure(s)

QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,

QA CAL-25.v6

Calibration procedure for dosimetric E-field probes

Calibration date:

May 23, 2014

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).

The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	03-Apr-14 (No. 217-01911)	Apr-15
Power sensor E4412A	MY41498087	03-Apr-14 (No. 217-01911)	Apr-15
Reference 3 dB Attenuator	SN: S5054 (3c)	03-Apr-14 (No. 217-01915)	Apr-15
Reference 20 dB Attenuator	SN: S5277 (20x)	03-Apr-14 (No. 217-01919)	Apr-15
Reference 30 dB Attenuator	SN: S5129 (30b)	03-Apr-14 (No. 217-01920)	Apr-15
Reference Probe ES3DV2	SN: 3013	30-Dec-13 (No. ES3-3013_Dec13)	Dec-14
DAE4	SN: 660	13-Dec-13 (No. DAE4-660_Dec13)	Dec-14
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

Name Function
Calibrated by: Claudio Leubler Laboratory Technician

Approved by: Katja Pokovic Technical Manager

Issued: May 23, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Certificate No: EX3-3927_May14

Cerpass Technology Corp.

Page 1 of 11

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 33 of 56

Issued Date : November 13th, 2014



CERPASS TECHNOLOGY CORP.

Report No.: SESF1410101

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid NORMx,y,z sensitivity in free space sensitivity in TSL / NORMx,y,z ConvF DCP diode compression point

CF crest factor (1/duty_cycle) of the RF signal A, B, C, D modulation dependent linearization parameters

Polarization o φ rotation around probe axis

9 rotation around an axis that is in the plane normal to probe axis (at measurement center), Polarization 9

i.e., 9 = 0 is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement
- Techniques", June 2013
 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E2-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: EX3-3927 May14

Page 2 of 11

Issued Date: November 13th, 2014 Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 34 of 56



EX3DV4 - SN:3927

May 23, 2014

Probe EX3DV4

SN:3927

Manufactured:

March 8, 2013

Calibrated:

May 23, 2014

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

Certificate No: EX3-3927_May14

Page 3 of 11

Cerpass Technology Corp. Issued Date : November 13th, 2014

Page No.

: 35 of 56



EX3DV4-SN:3927

May 23, 2014

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3927

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m) ²) ^A	0.57	0.33	0.61	± 10.1 %
DCP (mV) ⁸	96.7	96.5	92.4	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc [±] (k=2)
0	CW	X	0.0	0.0	1.0	0.00		±3.3 %
	7.000	Y	0.0	0.0	1.0		148.7	
		Z	0.0	0.0	1.0		135.9	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: EX3-3927_May14

Page 4 of 11

Issued Date: November 13th, 2014

Page No. : 36 of 56

A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 5 and 6).

Numerical linearization parameter: uncertainty not required.

Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

EX3DV4-SN:3927 May 23, 2014

Report No.: SESF1410101

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3927

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
450	43.5	0.87	11.02	11.02	11.02	0.15	1.30	± 13.3 %
850	41.5	0.92	10.23	10.23	10.23	0.43	0.81	± 12.0 %
1750	40.1	1.37	8.55	8.55	8.55	0.40	0.90	± 12.0 %
1900	40.0	1.40	8.31	8.31	8.31	0.60	0.66	± 12.0 %
2100	39.8	1.49	8.47	8.47	8.47	0.56	0.65	± 12.0 %
2450	39.2	1.80	7.48	7.48	7.48	0.68	0.59	± 12.0 %
5200	36.0	4.66	5.35	5.35	5.35	0.30	1.80	± 13.1 %
5500	35.6	4.96	4.97	4.97	4.97	0.35	1.80	± 13.1 %
5600	35.5	5.07	4.78	4.78	4.78	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.65	4.65	4.65	0.40	1.80	± 13.1 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Above 5 GHz frequency validity can be extended to ± 110 MHz. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 84, 128, 150 and 220 MHz respectively.

^C At frequencies below 3 GHz, the validity of tissue parameters (s and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (s and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Certificate No: EX3-3927_May14

Page 5 of 11

Issued Date: November 13th, 2014 Tel:86-512-6917-5888 Fax:86-512-6917-5666

Page No. : 37 of 56

measured SAR values. At requencies above 3 GHz, the valuiny of issue parameters (c and d) is restricted to £ 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

EX3DV4-SN:3927

May 23, 2014

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3927

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ⁶	Depth ^G (mm)	Unct. (k=2)
450	56.7	0.94	11.67	11.67	11.67	0.10	1.20	± 13.3 %
850	55.2	0.99	9.91	9.91	9.91	0.28	1.18	± 12.0 %
1750	53.4	1.49	8.45	8.45	8.45	0.71	0.64	± 12.0 %
1900	53.3	1.52	8.10	8.10	8.10	0.38	0.91	± 12.0 %
2100	53.2	1.62	8.40	8.40	8.40	0.40	0.87	± 12.0 %
2450	52.7	1.95	7.63	7.63	7.63	0.80	0.50	± 12.0 %
5200	49.0	5.30	4.61	4.61	4.61	0.40	1.90	± 13.1 %
5500	48.6	5.65	4.30	4.30	4.30	0.40	1.90	± 13,1 %
5600	48.5	5.77	4.23	4.23	4.23	0.40	1.90	± 13.1 %
5800	48.2	6.00	4.25	4.25	4.25	0.45	1.90	± 13.1 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Above 5 GHz frequency validity can be extended to ± 110 MHz. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively.

**A frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target fissue parameters.

**AlphaDeghth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX3-3927_May14

Page 6 of 11

Issued Date: November 13th, 2014 Cerpass Technology Corp.


Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 38 of 56

EX3DV4-SN:3927

May 23, 2014

Frequency Response of E-Field

(TEM-Cell:ifi110 EXX, Waveguide: R22)

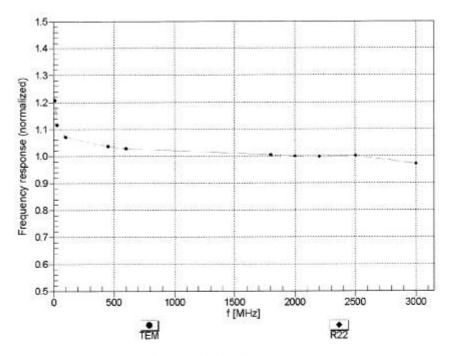

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)

Certificate No: EX3-3927_May14

Page 7 of 11


Cerpass Technology Corp. Issued Date : November 13th, 2014


Page No.

: 39 of 56

EX3DV4- SN:3927 May 23, 2014

Receiving Pattern (ϕ), $\theta = 0^{\circ}$

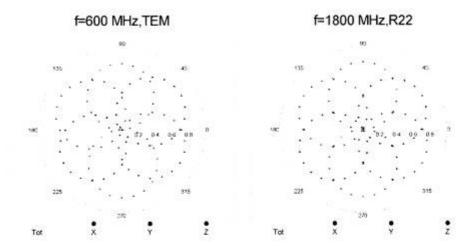

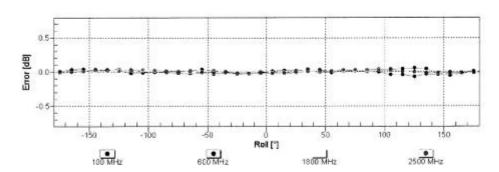

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Certificate No: EX3-3927_May14 Page 8 of 11


Issued Date: November 13th, 2014

Cerpass Technology Corp.

EX3DV4-SN:3927 May 23, 2014

Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

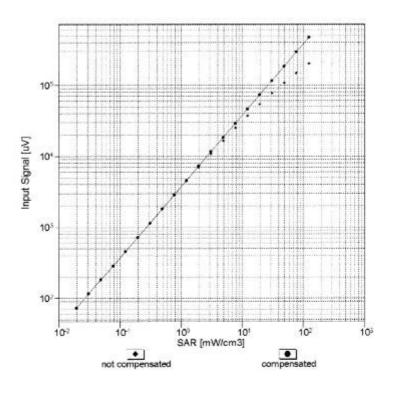

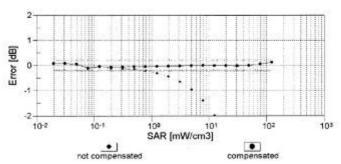

Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Certificate No: EX3-3927_May14

Page 9 of 11


Issued Date: November 13th, 2014 Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 41 of 56

EX3DV4- SN:3927 May 23, 2014

Conversion Factor Assessment

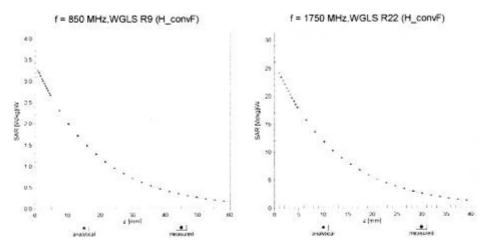

Deviation from Isotropy in Liquid

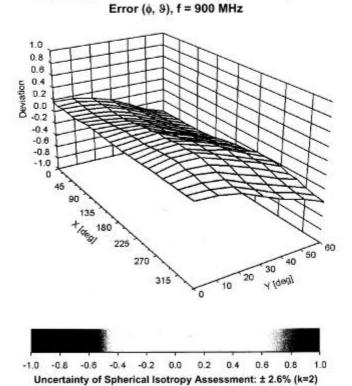

Certificate No: EX3-3927_May14

Page 10 of 11

Cerpass Technology Corp. Issued Date : November 13th, 2014

: 42 of 56

EX3DV4- SN:3927

May 23, 2014

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3927

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	25.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	.9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm

Certificate No: EX3-3927_May14

Page 11 of 11

Cerpass Technology Corp. Issued Date : November 13th, 2014

Page No.

: 43 of 56



CERPASS TECHNOLOGY CORP.

9. Appendix E. Dipole Calibration Data

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdlenst
C Service sulsse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 108

Client Cerpass (Auden)

Certificate No: D2450V2-914 Jun13

Report No.: SESF1410101

CALIDDATION			
CALIBRATION	CERTIFICATE	2.7	
Object	D2450V2 - SN: 9	914	
Calibration procedure(s)	QA CAL-05.v9 Calibration proce	edure for dipole validation kits ab	ove 700 MHz
Calibration date;	June 07, 2013		
The measurements and the unce	rtainties with confidence p	ional standards, which realize the physical un probability are given on the following pages ar ry facility: environment temperature (22 ± 3)°	nd are part of the certificate.
ai calbiations have been condu	cled in the closed labbrator	ry facility: environment temperature (22 ± 3)*	C and humidity < 70%,
Calibration Equipment used (M&	TE critical for calibration)		
Calibration Equipment used (M&	,		
Calibration Equipment used (M&	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Calibration Equipment used (M& Primary Standards Power meter EPM-442A	ID # GB37480704	Cal Date (Certificate No.) 01-Nov-12 (No. 217-01640)	Scheduled Calibration Oct-13
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 5481A	ID # GB37480704 US37292783		
Calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator	ID # GB37480704 US37292783 SN: 5058 (20k)	01-Nov-12 (No. 217-01640)	Oct-13
rimary Standards rower meter EPM-442A rower sensor HP 5481A reference 20 dB Attenuator rope-N mismatch combination	ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327	01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739)	Oct-13 Oct-13
calibration Equipment used (M& Primary Standards Power meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3	ID # GB37480704 US37292783 SN: 5058 (20k)	01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736)	Oct-13 Oct-13 Apr-14
rimary Standards rower meter EPM-442A rower sensor HP 8481A leference 20 dB Attenuator rype-N mismatch combination leference Probe ES3DV3	ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327	01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739)	Oct-13 Oct-13 Apr-14 Apr-14
rimary Standards rimary Standards ower meter EPM-442A ower sensor HP 8481A leference 20 dB Attenuator ype-N mismatch combination leference Probe ES3DV3 AE4	ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205	01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13)	Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14
calibration Equipment used (M&Calibration Equipment used (M&Calibration Equipment used (M&Calibration Education Educ	ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601	01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13)	Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check
Calibration Equipment used (M&Calibration Equipment used (M&Calibr	ID # GB37480704 US37292763 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601	01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11)	Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13
Calibration Equipment used (M&	ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317	01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13)	Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check
Primary Standards Primary Standards Prover meter EPM-442A Power sensor HP 8481A Reference 20 dB Attenuator Type-N mismatch combination Reference Probe ES3DV3 RAE4 Recondary Standards Rower sensor HP 8481A RE generator R&S SMT-06 Retwork Analyzer HP 8753E	ID # GB37480704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005	01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-11)	Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13
	ID # GB374B0704 US37292783 SN: 5058 (20k) SN: 5047.3 / 06327 SN: 3205 SN: 601 ID # MY41092317 100005 US37390585 S4206 Name	01-Nov-12 (No. 217-01640) 01-Nov-12 (No. 217-01640) 04-Apr-13 (No. 217-01736) 04-Apr-13 (No. 217-01739) 28-Dec-12 (No. ES3-3205_Dec12) 25-Apr-13 (No. DAE4-601_Apr13) Check Date (in house) 18-Oct-02 (in house check Oct-11) 04-Aug-99 (in house check Oct-12) Function	Oct-13 Oct-13 Apr-14 Apr-14 Dec-13 Apr-14 Scheduled Check In house check: Oct-13 In house check: Oct-13

Certificate No: D2450V2-914_Jun13

Cerpass Technology Corp.

Page 1 of 8

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 44 of 56



CERPASS TECHNOLOGY CORP. Report No.: SESF1410101

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage

C Service suisse d'etaionnage Servizio svizzero di taratura

Accreditation No.: SCS 108

Issued Date: November 13th, 2014

S Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilisteral Agreement for the recognition of calibration certificates

Glossary:

TSL

tissue simulating liquid

ConvF

sensitivity in TSL / NORM x,y,z

N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2003, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", December 2003
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) Federal Communications Commission Office of Engineering & Technology (FCC OET), "Evaluating Compliance with FCC Guidelines for Human Exposure to Radiofrequency Electromagnetic Fields; Additional Information for Evaluating Compliance of Mobile and Portable Devices with FCC Limits for Human Exposure to Radiofrequency Emissions", Supplement C (Edition 01-01) to Bulletin 65

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end
 of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D2450V2-914_Jun13

Page 2 of 8

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 45 of 56



Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Report No.: SESF1410101

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	37.8 ± 6 %	1.81 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.5 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	53.4 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.24 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.8 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	50.9 ± 6 %	2.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		****

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	13.2 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	51.5 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	6.07 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.9 W/kg ± 16.5 % (k=2)

Certificate No: D2450V2-914_Jun13

Page 3 of 8

Issued Date: November 13th, 2014

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 46 of 56



Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	57.0 Ω + 1.9 jΩ
Return Loss	- 23.3 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	52.1 Ω + 3.5 jΩ
Return Loss	- 28.0 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.160 ns

After long term use with 100W radiated power, only a slight warming of the dpole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	December 19, 2012

Certificate No: D2450V2-914_Jun13

Cerpass Technology Corp.

Page 4 of 8

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 47 of 56

DASY5 Validation Report for Head TSL

Date: 07.06.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 914

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 37.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.52, 4.52, 4.52); Calibrated: 28.12.2012;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 25.04.2013

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.695 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 28.3 W/kg

SAR(1 g) = 13.5 W/kg; SAR(10 g) = 6.24 W/kg

Maximum value of SAR (measured) = 17.6 W/kg



0 dB = 17.6 W/kg = 12.46 dBW/kg

Certificate No: D2450V2-914_Jun13

Cerpass Technology Corp.


Page 5 of 8

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 48 of 56

Issued Date : November 13th, 2014



Impedance Measurement Plot for Head TSL

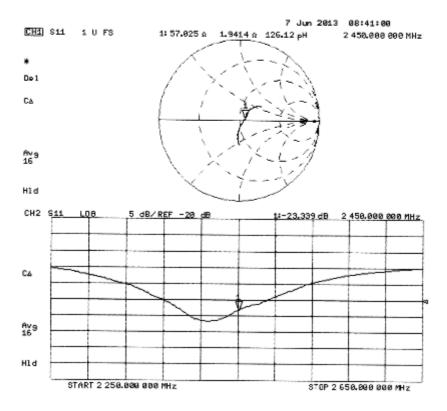

Report No.: SESF1410101

Certificate No: D2450V2-914_Jun13

Page 6 of 8

Cerpass Technology Corp.Tel:86-512-6917-5888 Fax:86-512-6917-5666

Issued Date: November 13th, 2014

Page No. : 49 of 56

DASY5 Validation Report for Body TSL

Date: 07.06.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 914

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: f = 2450 MHz; $\sigma = 2.02$ S/m; $\varepsilon_r = 50.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.42, 4.42, 4.42); Calibrated: 28.12.2012;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 25.04.2013

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 95.695 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 27.6 W/kg

SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.07 W/kg

Maximum value of SAR (measured) = 17.5 W/kg



0 dB = 17.5 W/kg = 12.43 dBW/kg

Certificate No: D2450V2-914_Jun13


Cerpass Technology Corp.

Page 7 of 8

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 50 of 56



Impedance Measurement Plot for Body TSL

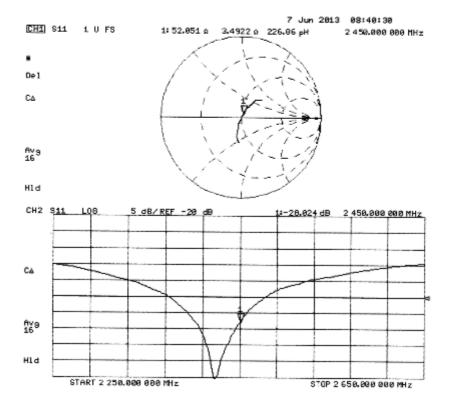

Report No.: SESF1410101

Certificate No: D2450V2-914_Jun13

Page 8 of 8

Cerpass Technology Corp.Tel:86-512-6917-5888 Fax:86-512-6917-5666

Issued Date: November 13th, 2014

Page No. : 51 of 56



CERPASS TECHNOLOGY CORP.

Report No.: SESF1410101

Appendix F. DAE Calibration Data

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

Cerpass (Auden)

Certificate No: DAE4-1379_May14

Accreditation No.: SCS 108

CALIBRATION CERTIFICATE

DAE4 - SD 000 D04 BJ - SN: 1379

Calibration procedure(s)

QA CAL-06.v26

Calibration procedure for the data acquisition electronics (DAE)

Calibration date:

May 19, 2014

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (St). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Keithley Multimeter Type 2001	SN: 0810278	01-Oct-13 (No:13976)	Oct-14
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Auto DAE Calibration Unit	SE UWS 053 AA 1001	07-Jan-14 (in house check)	In house check: Jan-15
Calibrator Box V2.1	SE UMS 006 AA 1002	07-Jan-14 (in house check)	In house check: Jan-15

Calibrated by:

Name

Function

Dominique Steffen

This calibration certificate shall not be reproduced except in full without written approval of the laboratory

Technician

Approved by:

Cerpass Technology Corp.

Fin Bomholt

Deputy Technical Manager

Issued: May 19, 2014

Certificate No: DAE4-1379_May14

Page 1 of 5

Tel:86-512-6917-5888 Fax:86-512-6917-5666

Issued Date: November 13th, 2014

Page No.

: 52 of 56



CERPASS TECHNOLOGY CORP.

SESF1410101 Report No.:

Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary

DAE data acquisition electronics

Connector angle information used in DASY system to align probe sensor X to the robot

coordinate system.

Methods Applied and Interpretation of Parameters

DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range.

- Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required.
- The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty.
 - DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this
 - Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement.
 - Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage.
 - AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage
 - Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements.
 - Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance.
 - Input resistance: Typical value for information: DAE input resistance at the connector, during internal auto-zeroing and during measurement.
 - Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated.
 - Power consumption: Typical value for information. Supply currents in various operating modes.

Certificate No: DAE4-1379_May14	Page 2 of 5	

Issued Date: November 13th, 2014 Cerpass Technology Corp.

Page No.

: 53 of 56

Tel:86-512-6917-5888 Fax:86-512-6917-5666



DC Voltage Measurement

A/D - Converter Resolution nominal

6.1μV , 61nV , full range = -100...+300 mV full range = -1......+3mV High Range: 1LSB = Low Range: 1LSB = DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Calibration Factors	x	Υ	Z
High Range	403.805 ± 0.02% (k=2)	404.075 ± 0.02% (k=2)	404.011 ± 0.02% (k=2)
Low Range	3.99838 ± 1.50% (k=2)	3.99504 ± 1.50% (k=2)	4.00152 ± 1.50% (k=2)

Connector Angle

Connector Angle to be used in DASY system	149.5°±1°
---	-----------

Certificate No: DAE4-1379_May14

Page 3 of 5

Issued Date: November 13th, 2014

Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 54 of 56

Cerpass Technology Corp.

Appendix

1. DC Voltage Linearity

High Range	Reading (µV)	Difference (μV)	Error (%)
Channel X + Input	199994.29	-1.98	-0.00
Channel X + Input	19999.30	-1.30	-0.01
Channel X - Input	-19998.41	2.90	-0.01
Channel Y + Input	199996.73	0.29	0.00
Channel Y + Input	19996.72	-3.84	-0.02
Channel Y - Input	-20001.24	-0.12	0.00
Channel Z + Input	199995.04	-1.34	-0.00
Channel Z + Input	19998.92	-1,47	-0.01
Channel Z - Input	-20002.08	-0.85	0.00

Low Range	Reading (μV)	Difference (μV)	Error (%)
Channel X + Input	2001.97	1.11	0.06
Channel X + Input	201.61	0.19	0.10
Channel X - Input	-198.88	-0.22	0.11
Channel Y + Input	2001.25	0.31	0.02
Channel Y + Input	201.42	0.07	0.03
Channel Y - Input	-199.14	-0.59	0.30
Channel Z + Input	2001.40	0.60	0.03
Channel Z + Input	199.50	-1.64	-0.82
Channel Z - Input	-199.24	-0.49	0.25

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)
Channel X	200	-17.61	-19.05
	- 200	20.93	18.82
Channel Y	200	-4.43	-4.39
	- 200	4.21	4.00
Channel Z	200	-10.49	-10.31
	- 200	8.62	8.36

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)
Channel X	200	- S	-0.60	-5.10
Channel Y	200	8.15		0.34
Channel Z	200	10.42	5.32	

Certificate No: DAE4-1379_May14

Page 4 of 5

Issued Date: November 13th, 2014 Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 55 of 56



4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16034	13894
Channel Y	16256	12489
Channel Z	15825	15529

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec Input 10MΩ

	Average (μV)	min. Offset (μV)	max. Offset (μV)	Std. Deviation (µV)
Channel X	-1.79	-3.29	-0.79	0.47
Channel Y	-0.21	-2.44	1.81	0.71
Channel Z	-0.03	-1.33	2.40	0.79

6. Input Offset Current

Nominal Input circuitry offset current on all channels: <25fA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (MOhm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)	
Supply (+ Vcc)	+7.9	
Supply (- Vcc)	-7.6	

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-1379_May14

Page 5 of 5

Issued Date: November 13th, 2014 Tel:86-512-6917-5888 Fax:86-512-6917-5666 Page No. : 56 of 56