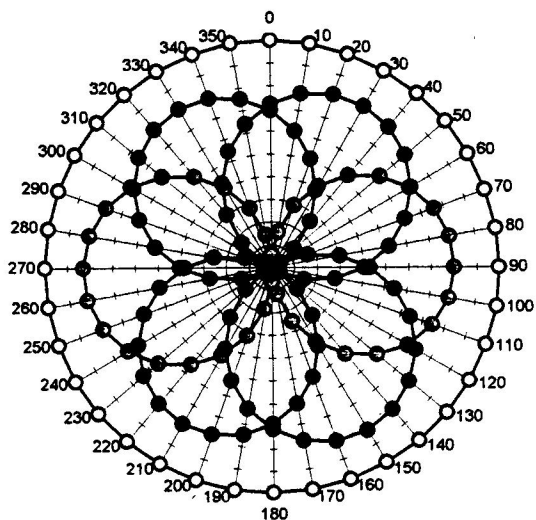


Probe ET3DV6


SN:1687

Manufactured:	May 28, 2002
Last calibration:	June 5, 2002


Calibrated for System DASY3

Receiving Pattern (ϕ), $\theta = 0^\circ$ **f = 30 MHz, TEM cell if110**


—●— X —●— Y —●— Z —○— Tot

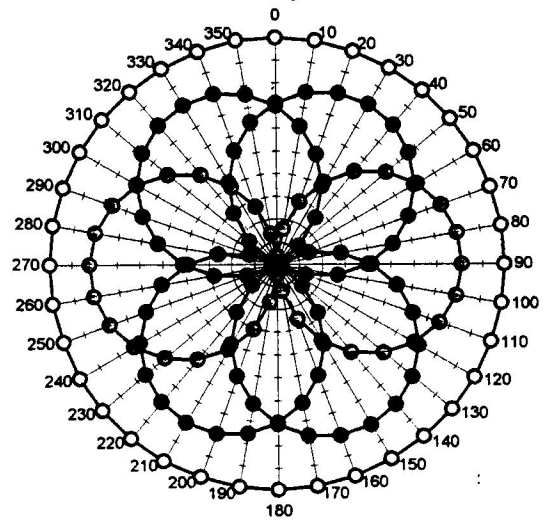f = 100 MHz, TEM cell if110



—●— X —●— Y —●— Z —○— Tot

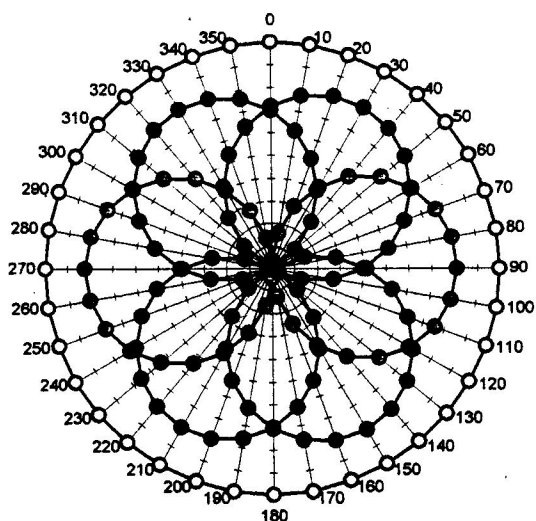f = 300 MHz, TEM cell if110

—●— X —●— Y —●— Z —○— Tot

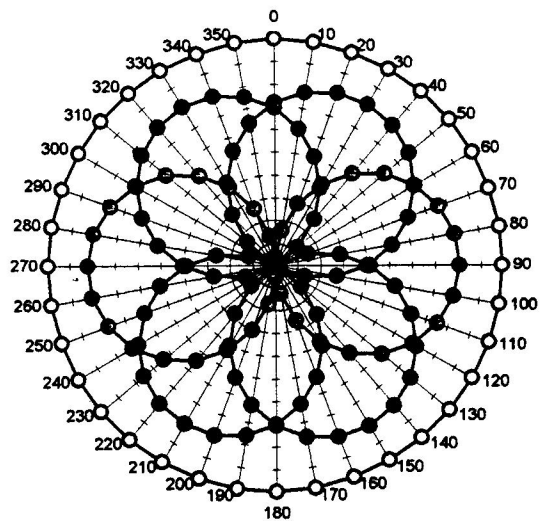f = 900 MHz, TEM cell if110

—●— X —●— Y —●— Z —○— Tot

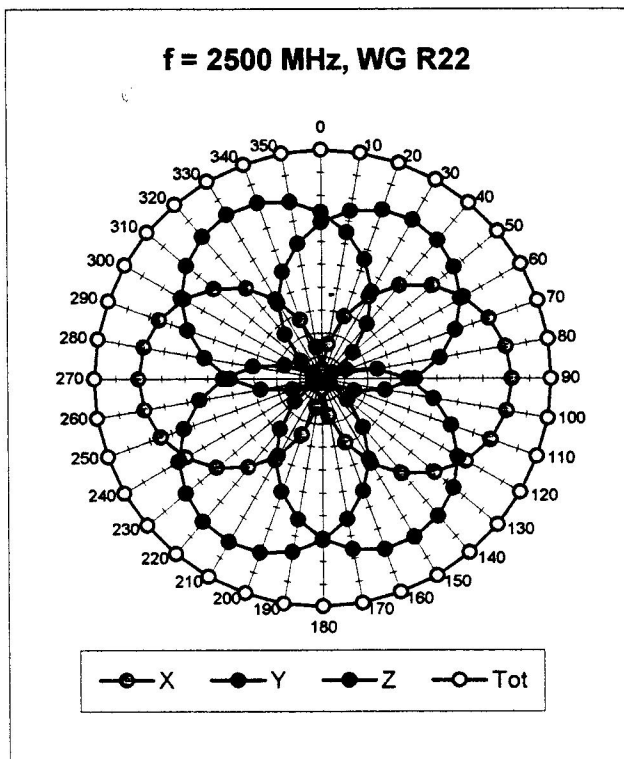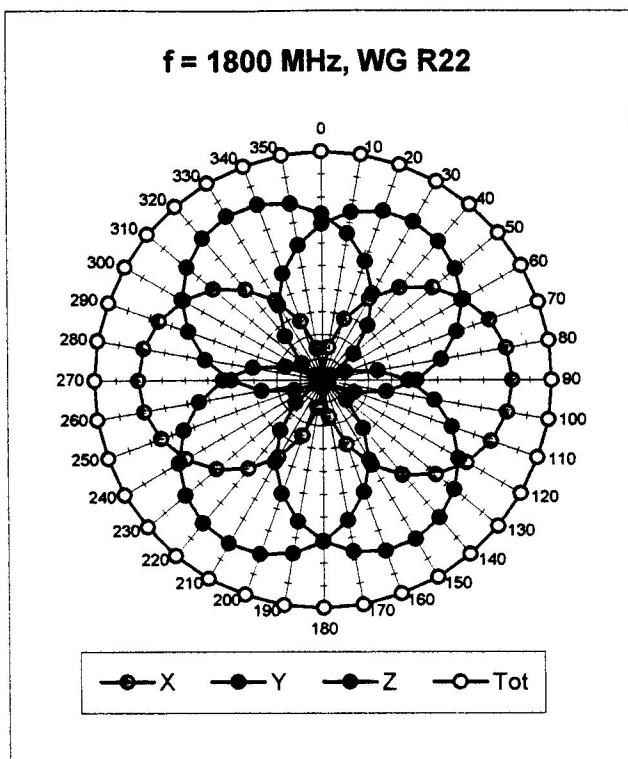

Isotropy Error (ϕ), $\theta = 0^\circ$

