

Appendix
Photographs of Test Setup



Fig.1 Photograph of the SAR measurement System

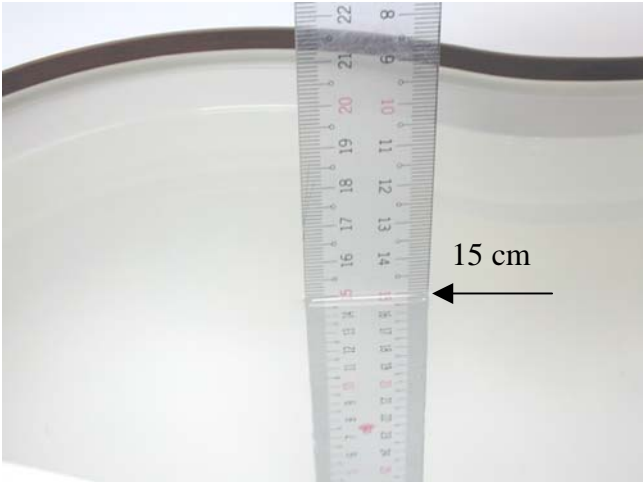


Fig.2 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Right-head Side

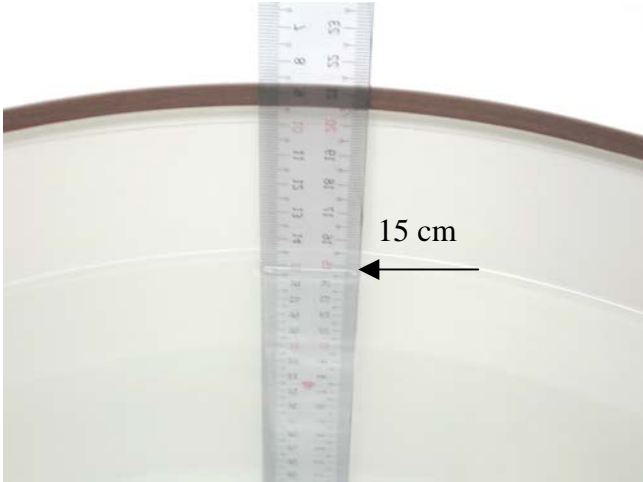


Fig.3 Photograph of the Tissue Simulant Fluid liquid depth 15cm for Flat (Body)

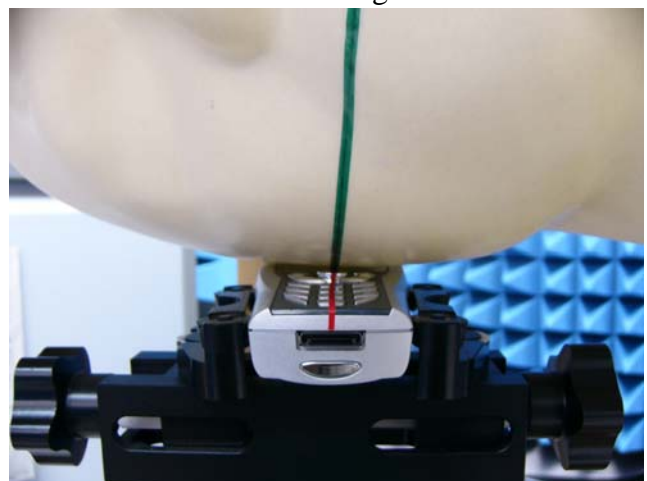
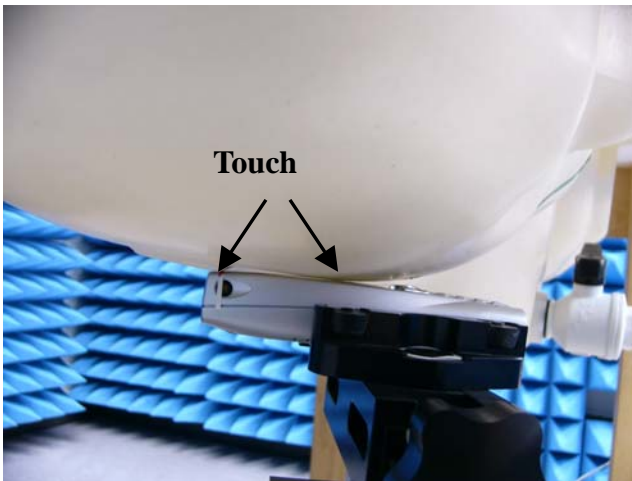


Fig.4 Right Head Section / Cheek-Touch Position



Fig.5 Right Head Section / Ear-Tilt Position(15°)

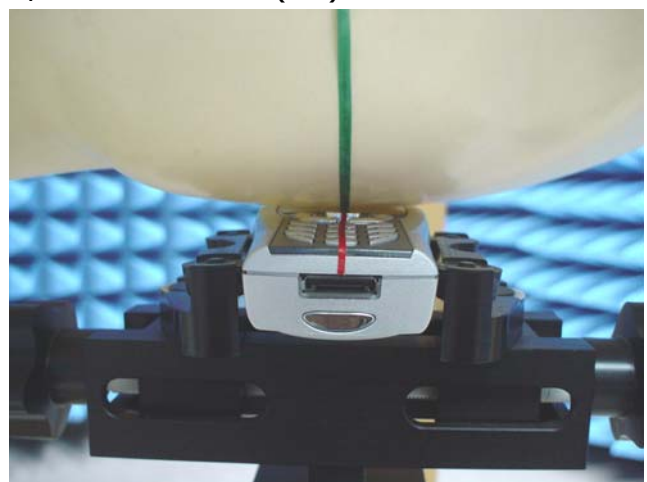
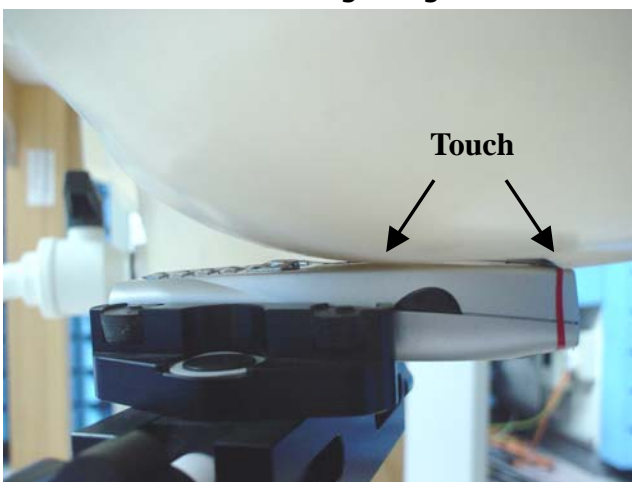


Fig.6 Left Head Section / Cheek-Touch Position

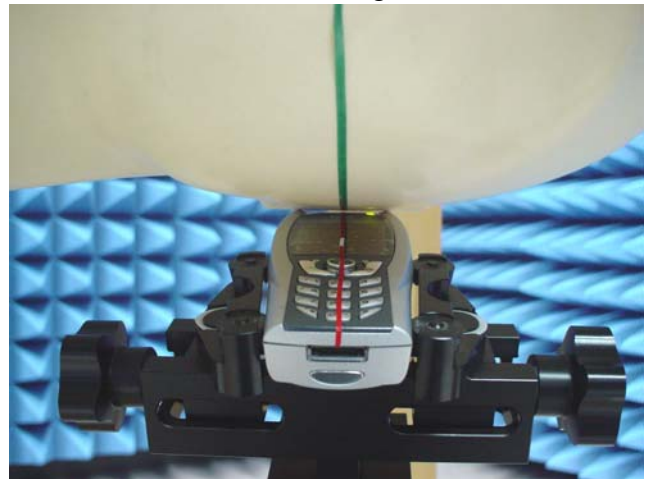
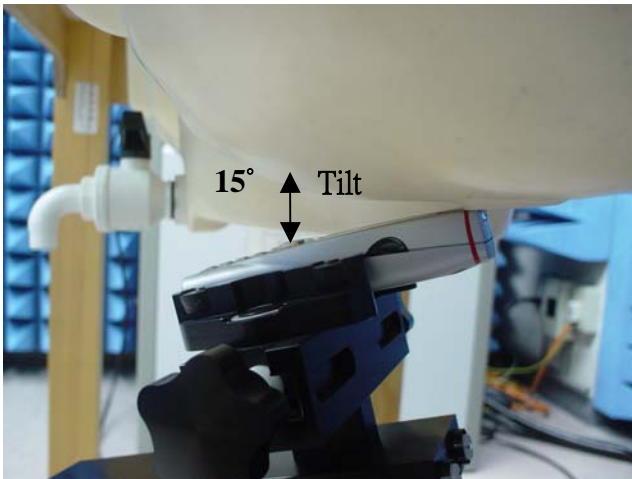


Fig.7 Left Head Section / Ear-Tilt Position(15°)

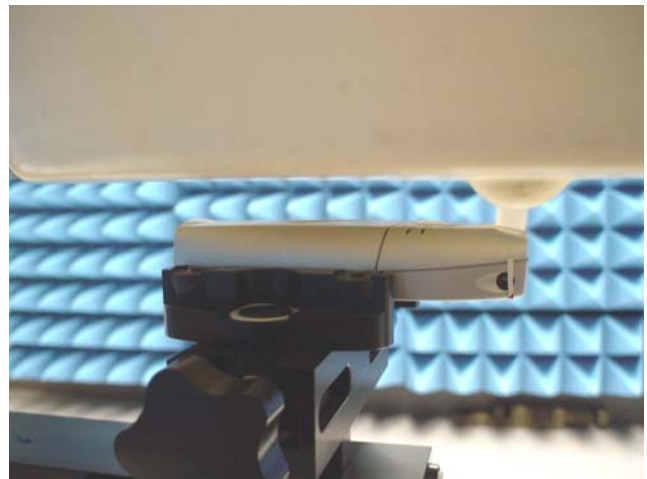
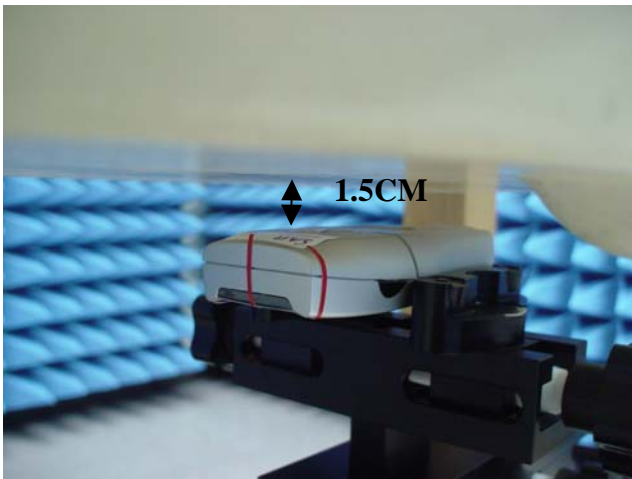


Fig.8 Body Worn with Headset Position