

Contents

10. Photographs of Test Setup	54
11. Photographs of the EUT	56

10. Photographs of Test Setup



Fig.1 Photograph of the SAR measurement System

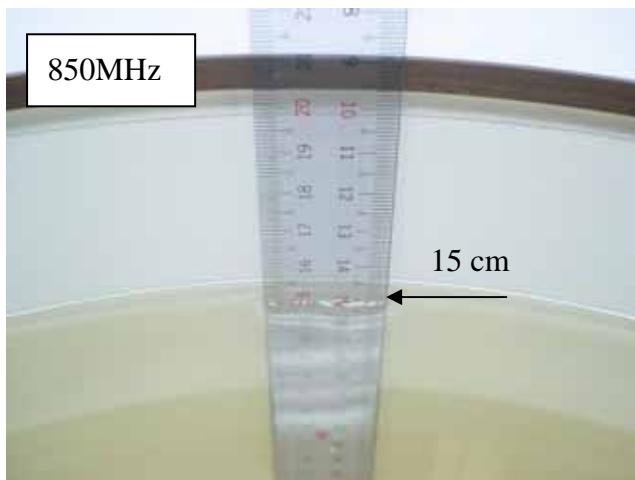


Fig.2.1 Photograph of the Tissue Simulant
Fluid liquid depth 15cm for Flat (Body)

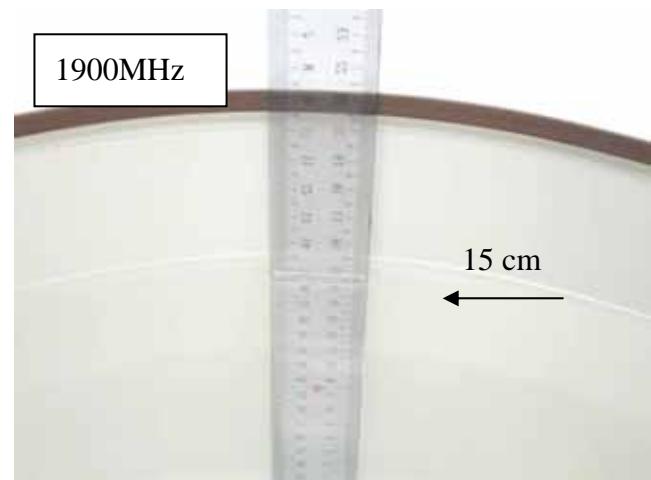


Fig.2.2 Photograph of the Tissue Simulant
Fluid liquid depth 15cm for Flat (Body)

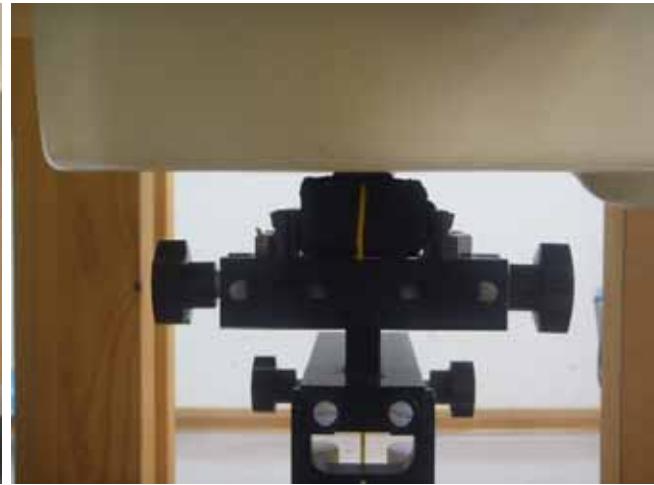


Fig.3 Put the EUT into holster and front side of EUT is paralleled with flat phantom, holster is paralleled and contacted with flat phantom.



Fig.4 Put the EUT into holster and back side of EUT is paralleled with flat phantom, holster is paralleled and contacted with flat phantom.

11. Photographs of the EUT



Fig.5 Front view of EUT



Fig.6 Back view of EUT



Fig.7 Left Side of EUT



Fig.8 Right Side of EUT



Fig.9 AC charger



Fig.10 Serial Model: TR-2031



Fig.11 Front view of Holster



Fig.12 Back view of Holster

End of Report