

SAR Plots

- Verification Plots
- SAR Test Plots

DT&C Co., Ltd.

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:920

Communication System: CW (0); Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.753$ S/m; $\epsilon_r = 40.56$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(7.17, 7.17, 7.17); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-25; Ambient Temp: 20.8; Tissue Temp: 21.2

2450 MHz System Verification


Area Scan (7x9x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.04 dB

Peak SAR (extrapolated) = 30.0 W/kg

SAR(1 g) = 13.5 W/kg; SAR(10 g) = 6.05 W/kg

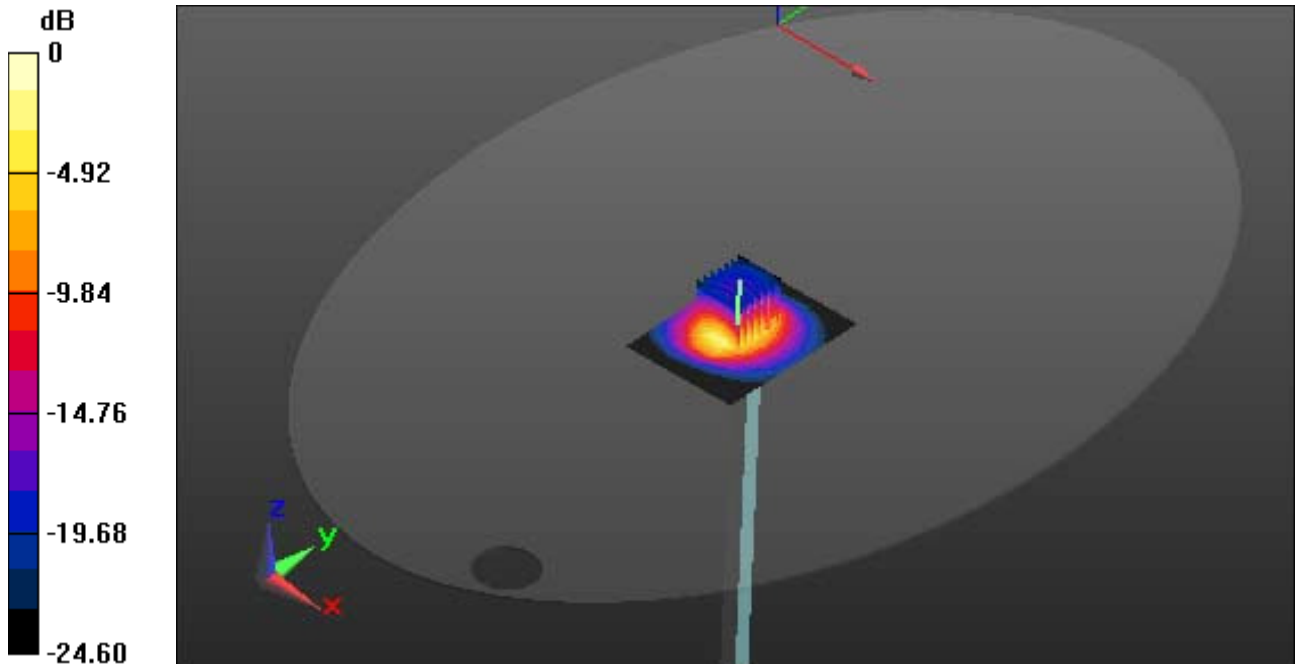

0 dB = 19.5 W/kg

DT&C Co., Ltd.

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:920

Communication System: CW (0); Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.753$ S/m; $\epsilon_r = 40.56$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(7.17, 7.17, 7.17); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-25; Ambient Temp: 20.8; Tissue Temp: 21.2

2450 MHz System Verification


Area Scan (7x9x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.04 dB

Peak SAR (extrapolated) = 30.0 W/kg

SAR(1 g) = 13.5 W/kg; SAR(10 g) = 6.05 W/kg

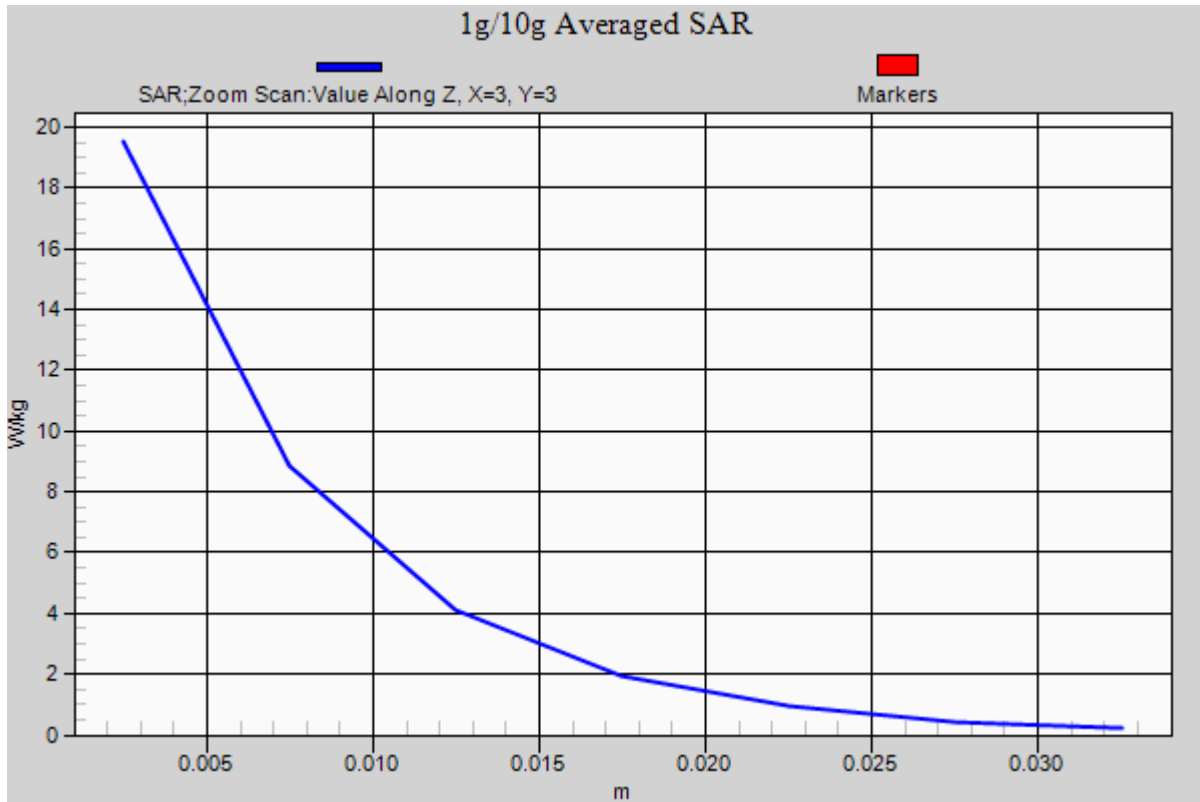

DT&C Co., Ltd.

DUT: Dipole 5000 MHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1212

Communication System: CW; Frequency: 5200 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5200$ MHz; $\sigma = 4.796$ S/m; $\epsilon_r = 36.318$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(5.34, 5.34, 5.34); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-31; Ambient Temp: 20.7; Tissue Temp: 21.0

5200 MHz System Verification


Area Scan (7x8x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x11)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = 0.10 dB

Peak SAR (extrapolated) = 34.7 W/kg

SAR(1 g) = 7.7 W/kg; SAR(10 g) = 2.16 W/kg

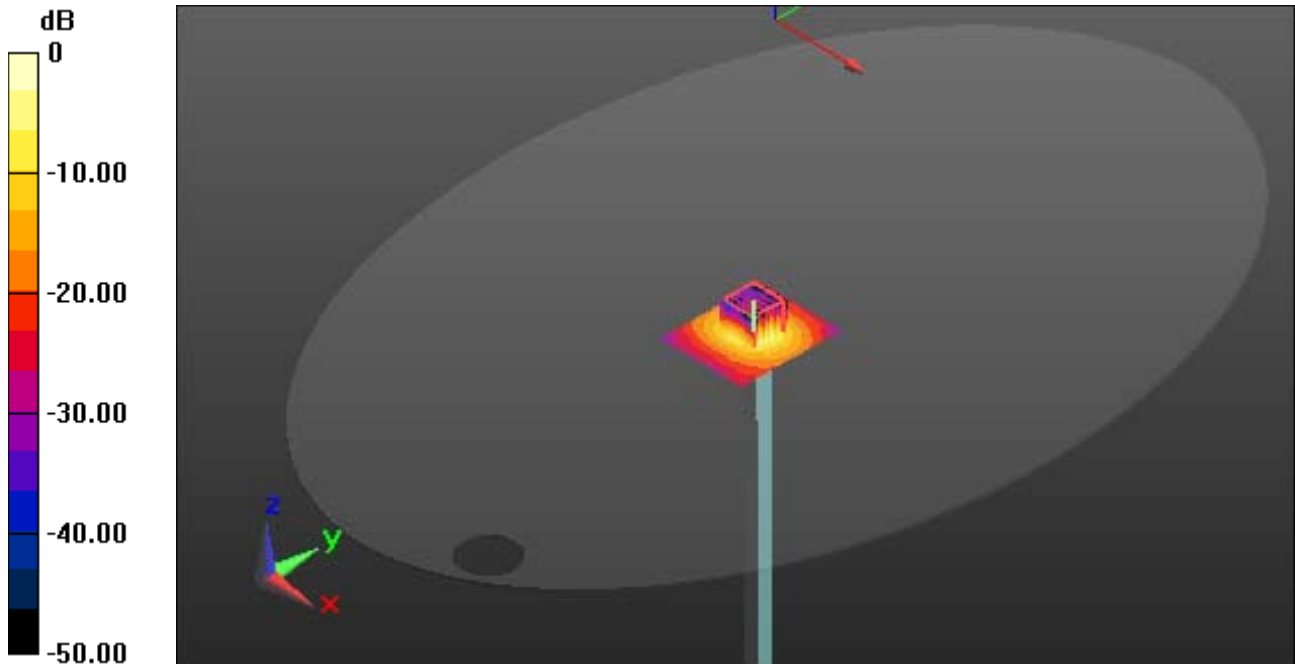

0 dB = 16.1 W/kg

DT&C Co., Ltd.

DUT: Dipole 5000 MHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1212

Communication System: CW; Frequency: 5200 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5200$ MHz; $\sigma = 4.796$ S/m; $\epsilon_r = 36.318$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(5.34, 5.34, 5.34); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-31; Ambient Temp: 20.7; Tissue Temp: 21.0

5200 MHz System Verification


Area Scan (7x8x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x11)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = 0.10 dB

Peak SAR (extrapolated) = 34.7 W/kg

SAR(1 g) = 7.7 W/kg; SAR(10 g) = 2.16 W/kg

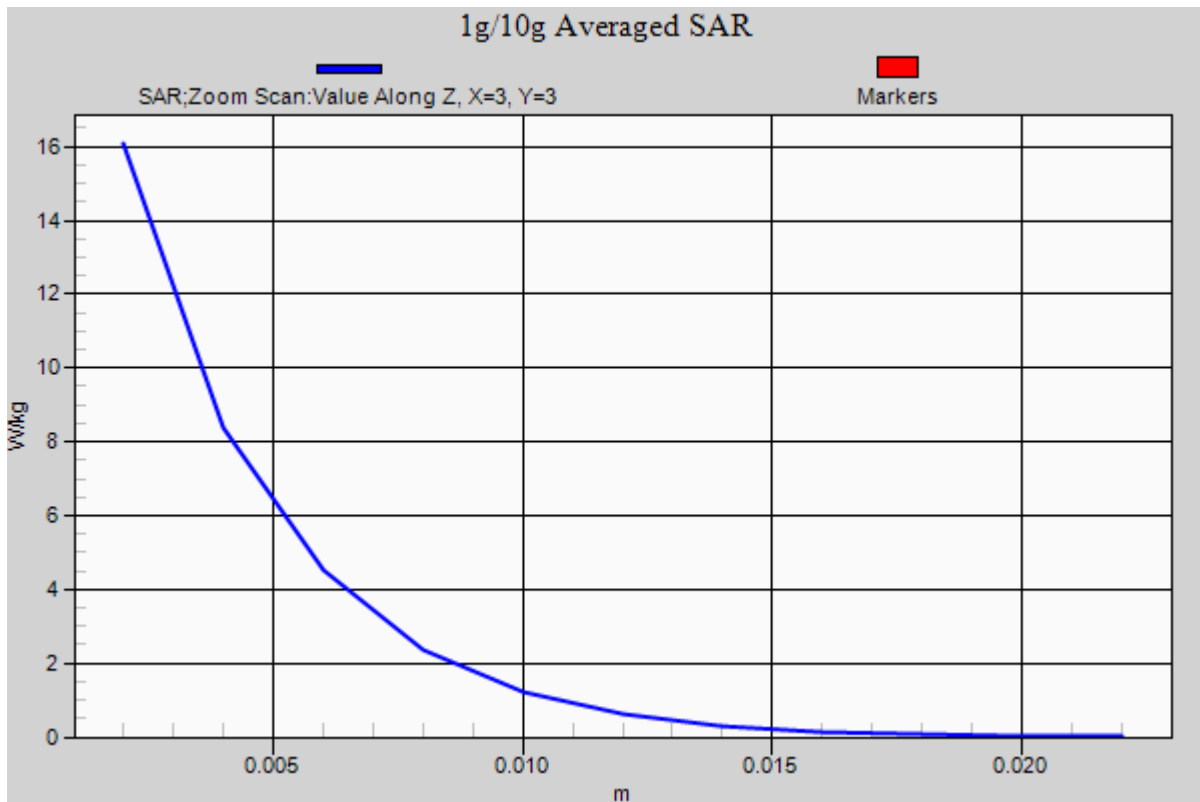

DT&C Co., Ltd.

DUT: Dipole 5000 MHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1212

Communication System: CW; Frequency: 5800 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5800$ MHz; $\sigma = 5.214$ S/m; $\epsilon_r = 34.835$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.58, 4.58, 4.58); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-02-03; Ambient Temp: 21.3; Tissue Temp: 21.7

5800 MHz System Verification


Area Scan (7x8x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x11)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = 0.05 dB

Peak SAR (extrapolated) = 33.0 W/kg

SAR(1 g) = 7.75 W/kg; SAR(10 g) = 2.17 W/kg

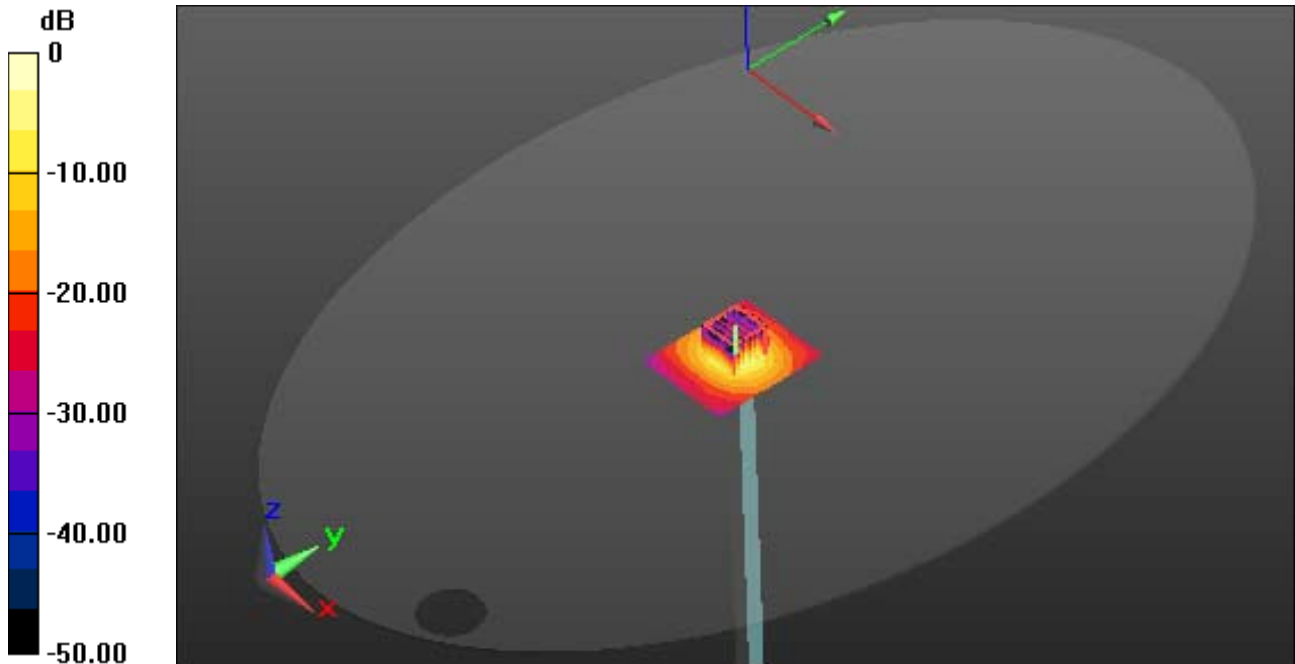

0 dB = 16.3 W/kg

DT&C Co., Ltd.

DUT: Dipole 5000 MHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1212

Communication System: CW; Frequency: 5800 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5800$ MHz; $\sigma = 5.214$ S/m; $\epsilon_r = 34.835$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.58, 4.58, 4.58); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-02-03; Ambient Temp: 21.3; Tissue Temp: 21.7

5800 MHz System Verification


Area Scan (7x8x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x11)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = 0.05 dB

Peak SAR (extrapolated) = 33.0 W/kg

SAR(1 g) = 7.75 W/kg; SAR(10 g) = 2.17 W/kg

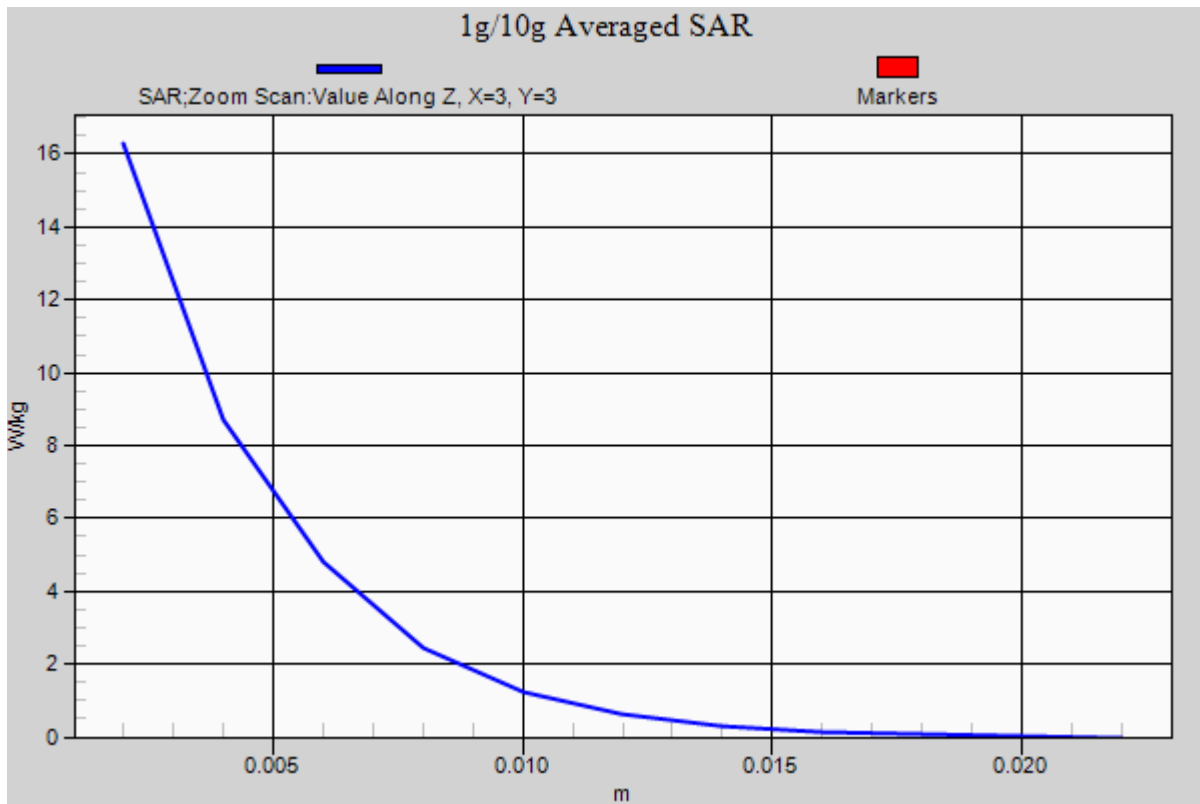

DT&C Co., Ltd.

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:920

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.913$ S/m; $\epsilon_r = 52.573$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(7.2, 7.2, 7.2); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-25; Ambient Temp: 20.8; Tissue Temp: 21.4

2450 MHz System Verification


Area Scan (6x8x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.11 dB

Peak SAR (extrapolated) = 27.2 W/kg

SAR(1 g) = 12.9 W/kg; SAR(10 g) = 5.94 W/kg

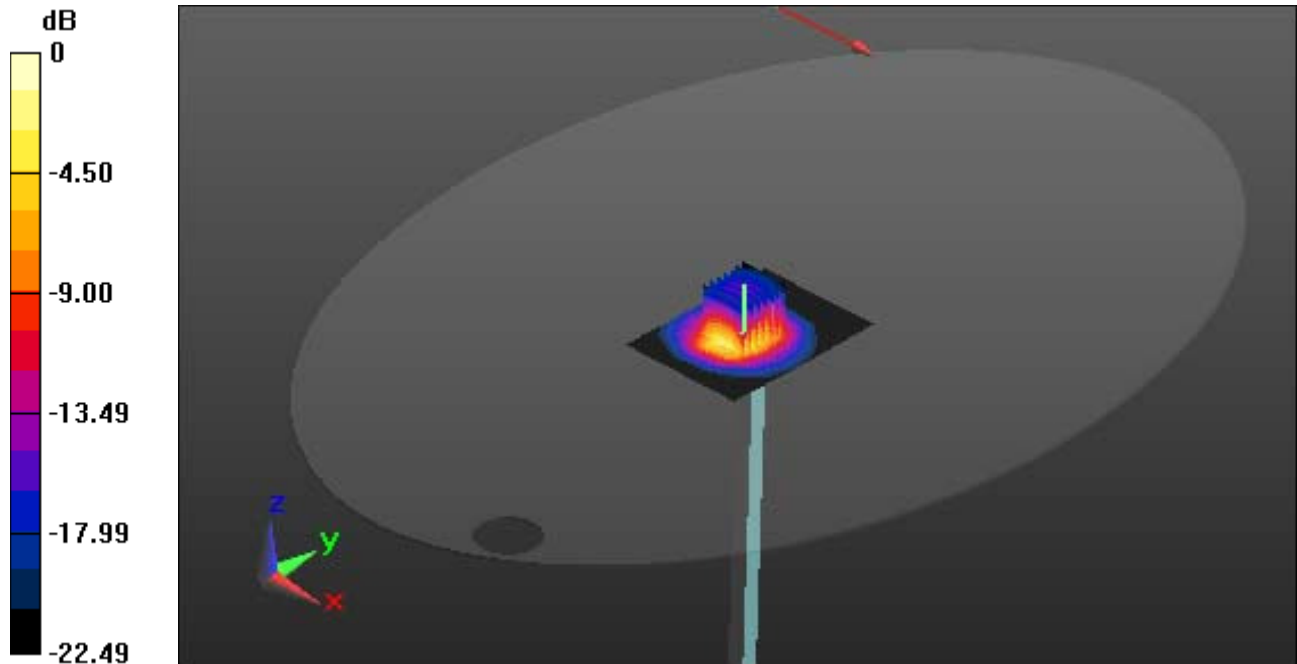

0 dB = 18.2 W/kg

DT&C Co., Ltd.

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:920

Communication System: CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.913$ S/m; $\epsilon_r = 52.573$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(7.2, 7.2, 7.2); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-25; Ambient Temp: 20.8; Tissue Temp: 21.4

2450 MHz System Verification


Area Scan (6x8x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.11 dB

Peak SAR (extrapolated) = 27.2 W/kg

SAR(1 g) = 12.9 W/kg; SAR(10 g) = 5.94 W/kg

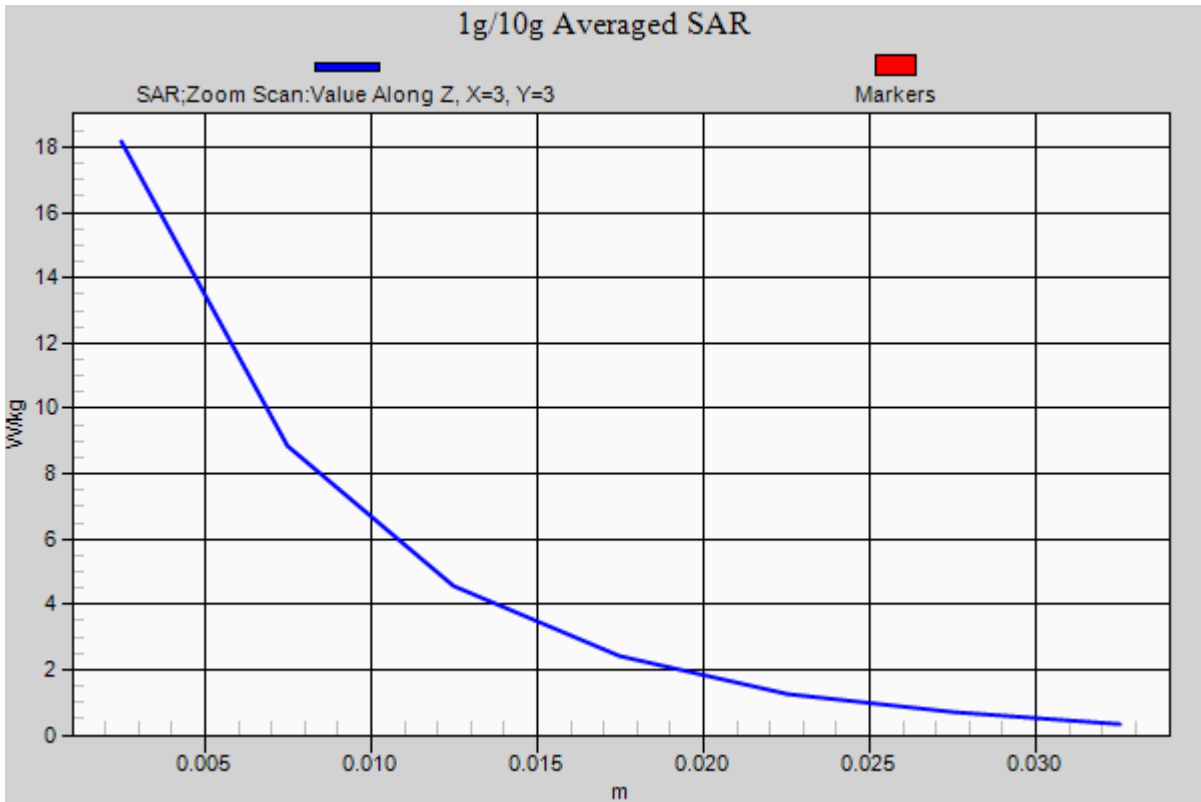

DT&C Co., Ltd.

DUT: Dipole 5000 MHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1212

Communication System: CW (0); Frequency: 5200 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5200$ MHz; $\sigma = 5.375$ S/m; $\epsilon_r = 47.433$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.65, 4.65, 4.65); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-31; Ambient Temp: 20.7; Tissue Temp: 20.9

5200 MHz System Verification


Area Scan (7x8x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x11)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = 0.11 dB

Peak SAR (extrapolated) = 31.7 W/kg

SAR(1 g) = 7.48 W/kg; SAR(10 g) = 2.08 W/kg

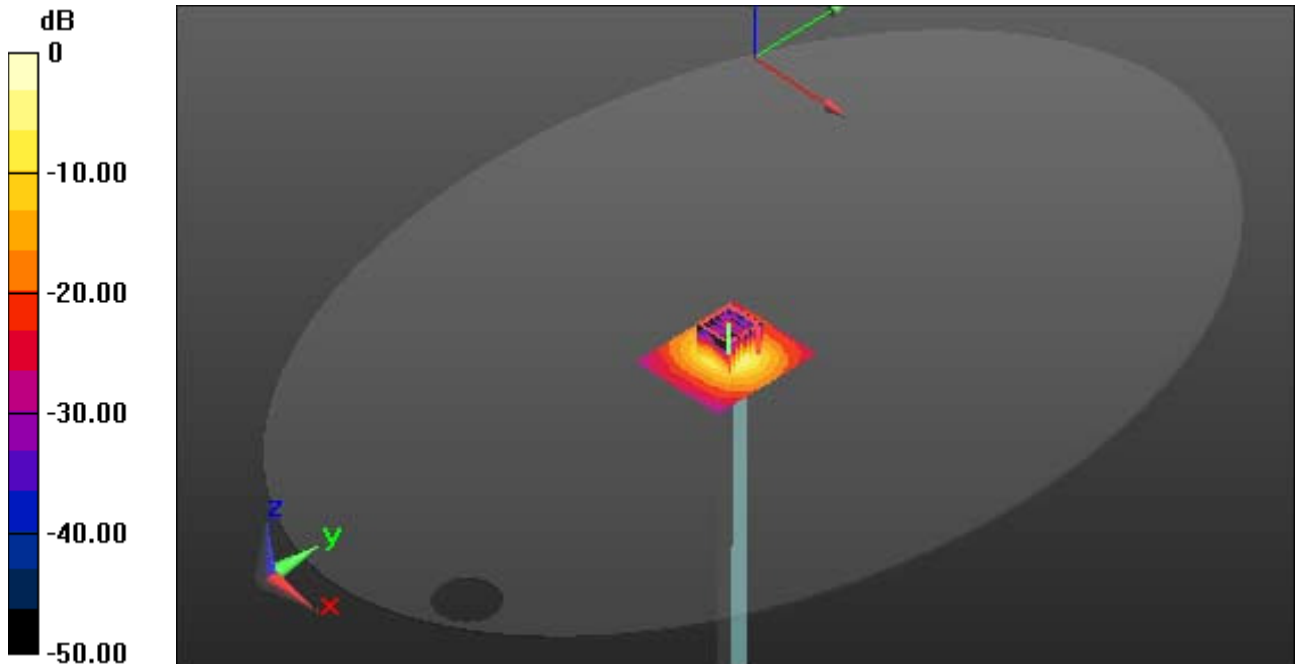

0 dB = 15.8 W/kg

DT&C Co., Ltd.

DUT: Dipole 5000 MHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1212

Communication System: CW (0); Frequency: 5200 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5200$ MHz; $\sigma = 5.375$ S/m; $\epsilon_r = 47.433$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.65, 4.65, 4.65); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-31; Ambient Temp: 20.7; Tissue Temp: 20.9

5200 MHz System Verification


Area Scan (7x8x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x11)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = 0.11 dB

Peak SAR (extrapolated) = 31.7 W/kg

SAR(1 g) = 7.48 W/kg; SAR(10 g) = 2.08 W/kg

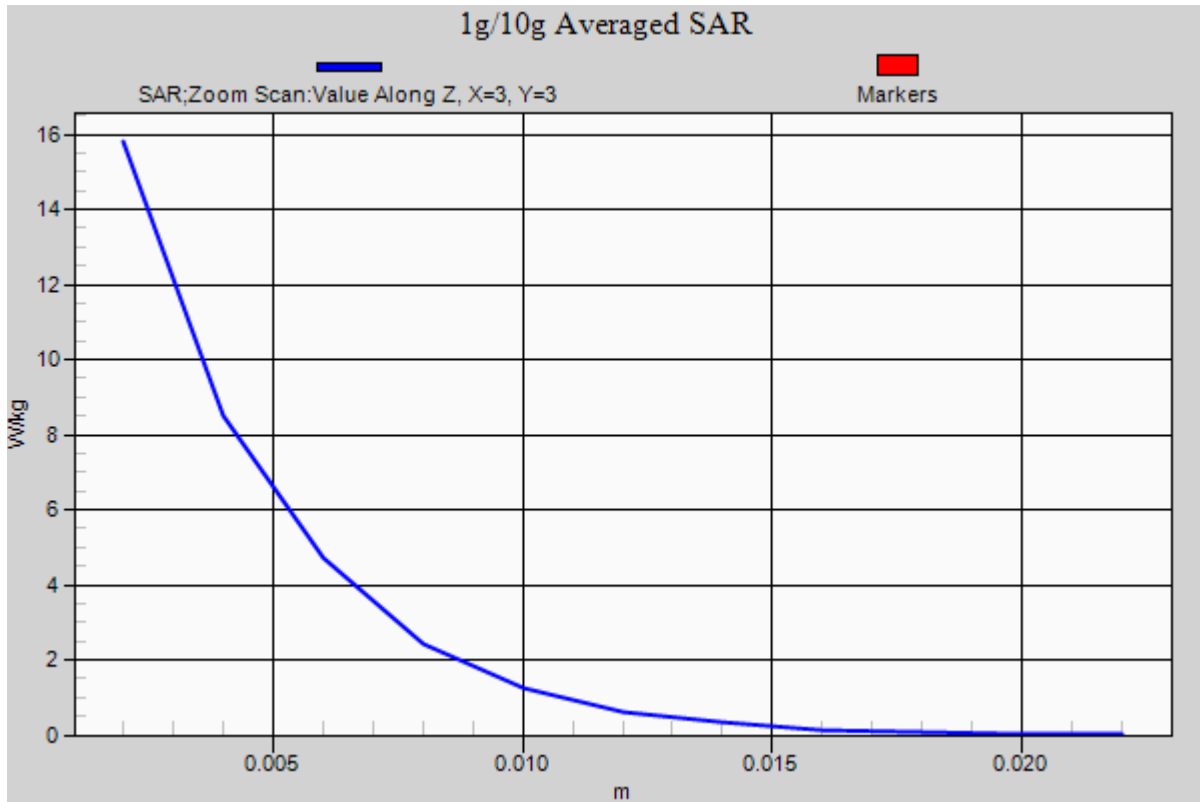

DT&C Co., Ltd.

DUT: Dipole 5000 MHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1212

Communication System: CW; Frequency: 5800 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5800$ MHz; $\sigma = 6.144$ S/m; $\epsilon_r = 46.324$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.05, 4.05, 4.05); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-02-03; Ambient Temp: 21.3; Tissue Temp: 21.0

5800 MHz System Verification


Area Scan (7x8x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x11)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = 0.08 dB

Peak SAR (extrapolated) = 28.7 W/kg

SAR(1 g) = 7.23 W/kg; SAR(10 g) = 2.03 W/kg

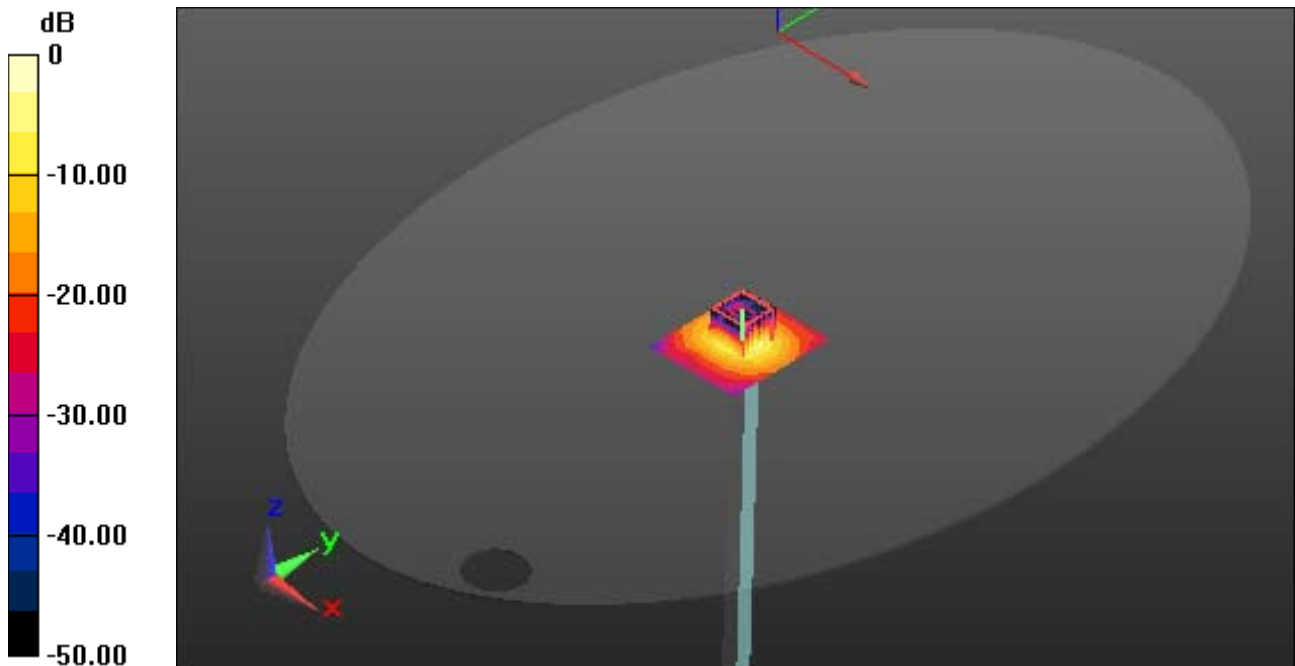

0 dB = 15.2 W/kg

DT&C Co., Ltd.

DUT: Dipole 5000 MHz; Type: D5GHzV2; Serial: D5GHzV2 - SN:1212

Communication System: CW; Frequency: 5800 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5800$ MHz; $\sigma = 6.144$ S/m; $\epsilon_r = 46.324$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.05, 4.05, 4.05); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-02-03; Ambient Temp: 21.3; Tissue Temp: 21.0

5800 MHz System Verification


Area Scan (7x8x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x11)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = 0.08 dB

Peak SAR (extrapolated) = 28.7 W/kg

SAR(1 g) = 7.23 W/kg; SAR(10 g) = 2.03 W/kg

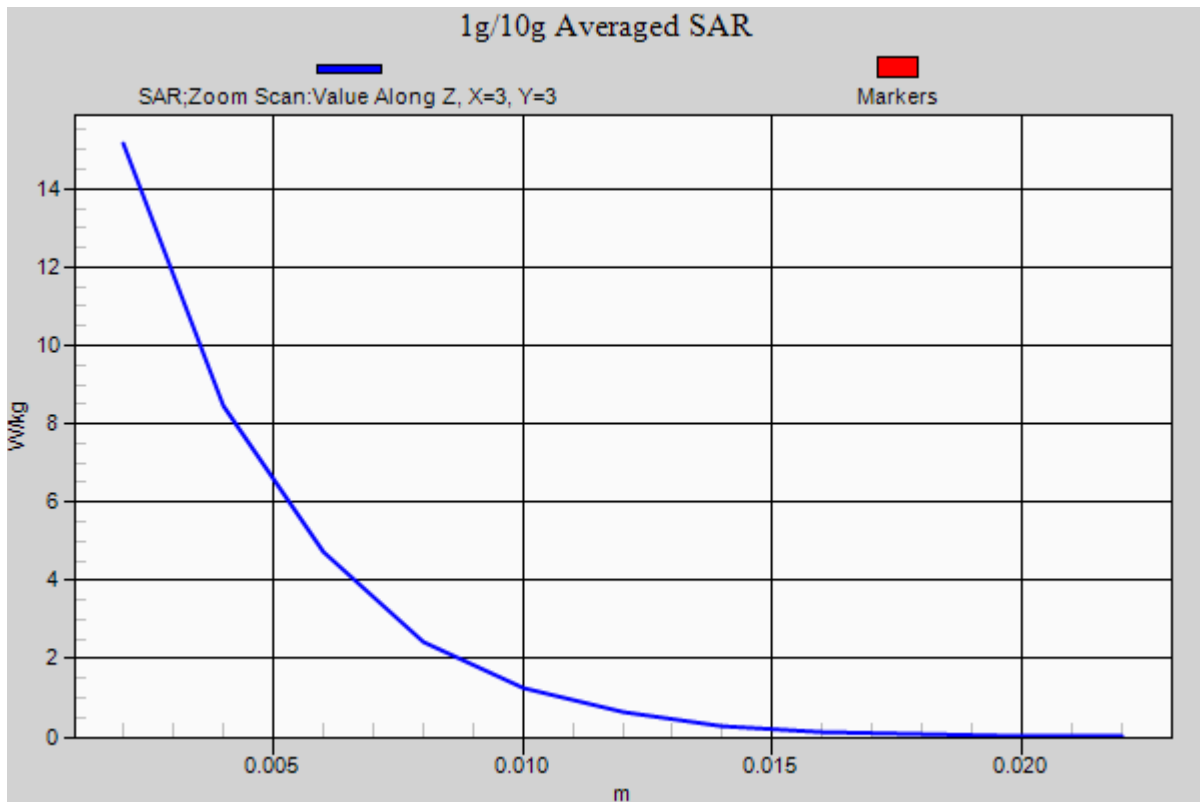

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 2.4G(802.11b/g/n20, 40) (0); Frequency: 2462 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 2462$ MHz; $\sigma = 1.761$ S/m; $\epsilon_r = 40.519$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(7.17, 7.17, 7.17); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-25; Ambient Temp: 20.8; Tissue Temp:21.2

Touch from Body, Front, W-LAN(802.11b - 2.4G) Ch. 11, Ant Internal

Ant. 1


Area Scan (17x17x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = 0.06 dB

Peak SAR (extrapolated) = 0.287 W/kg

SAR(1 g) = 0.098 W/kg; SAR(10 g) = 0.037 W/kg

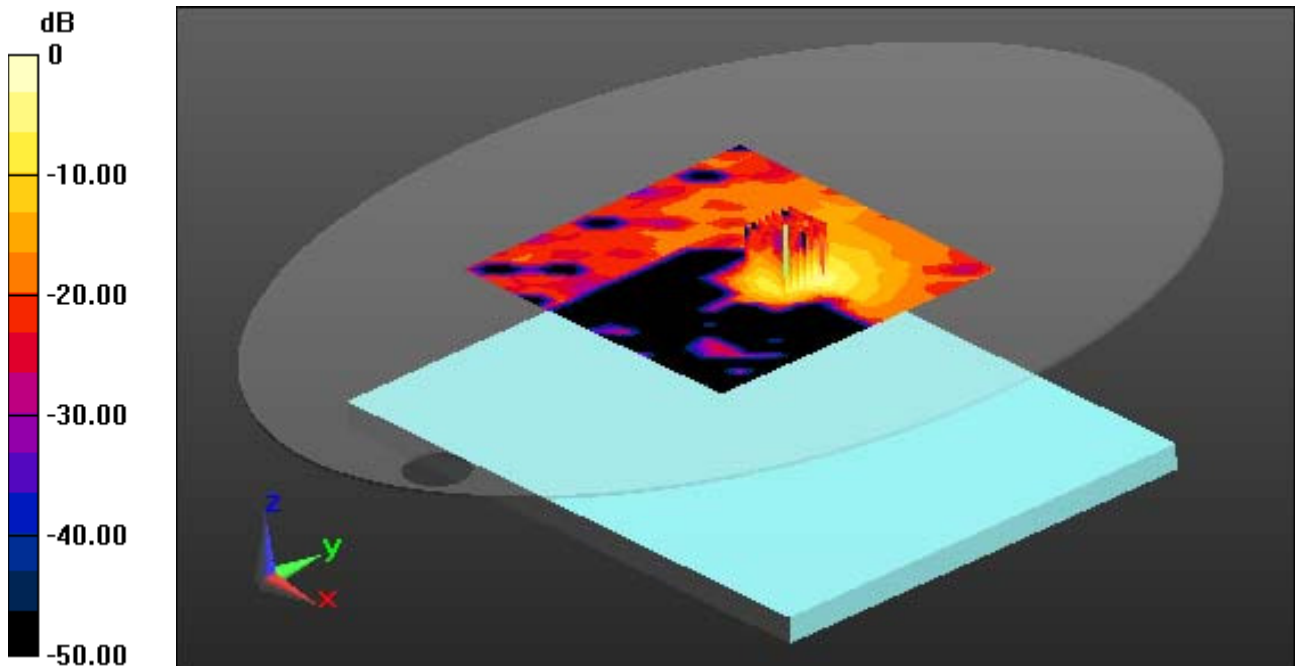

0 dB = 0.176 W/kg

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 2.4G(802.11b/g/n20, 40) (0); Frequency: 2462 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 2462$ MHz; $\sigma = 1.761$ S/m; $\epsilon_r = 40.519$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(7.17, 7.17, 7.17); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-25; Ambient Temp: 20.8; Tissue Temp:21.2

Touch from Body, Front, W-LAN(802.11b - 2.4G) Ch. 11, Ant Internal

Ant. 1

With Enlarge plot image


Area Scan (17x17x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = 0.06 dB

Peak SAR (extrapolated) = 0.287 W/kg

SAR(1 g) = 0.098 W/kg; SAR(10 g) = 0.037 W/kg

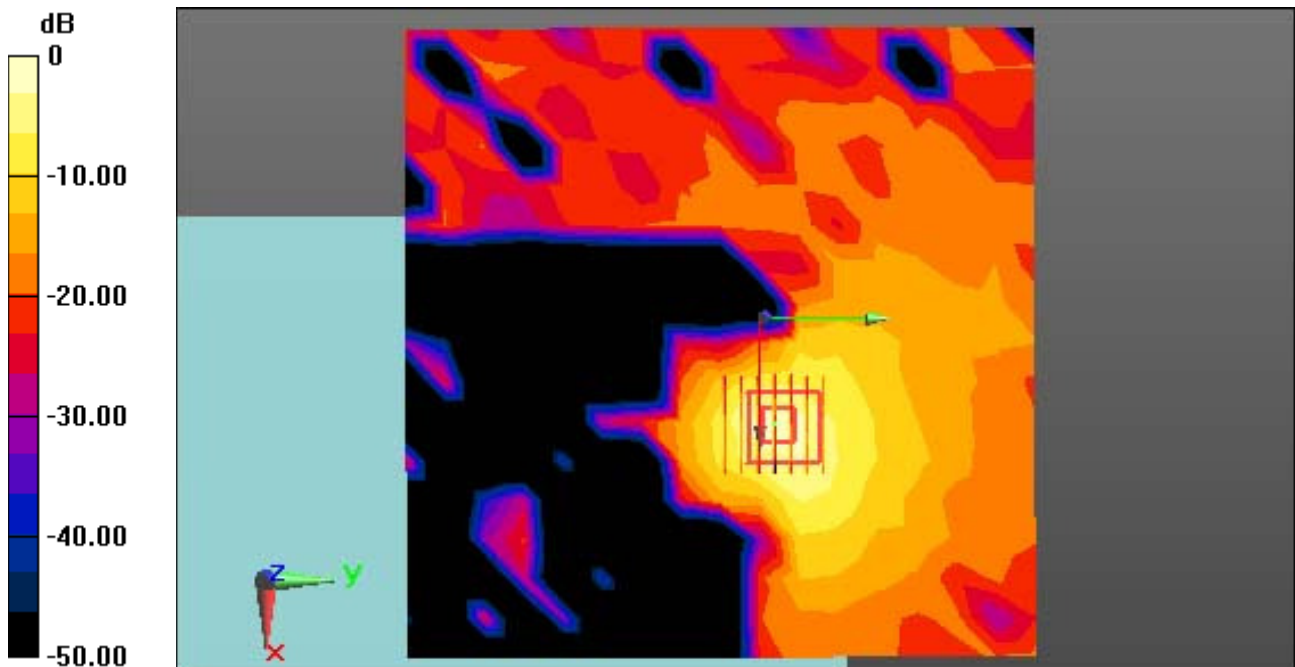

0 dB = 0.176 W/kg

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 2.4G(802.11b/g/n20, 40) (0); Frequency: 2462 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 2462$ MHz; $\sigma = 1.761$ S/m; $\epsilon_r = 40.519$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(7.17, 7.17, 7.17); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-25; Ambient Temp: 20.8; Tissue Temp:21.2

Touch from Body, Front, W-LAN(802.11b - 2.4G) Ch. 11, Ant Internal

Ant. 1


Area Scan (17x17x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = 0.06 dB

Peak SAR (extrapolated) = 0.287 W/kg

SAR(1 g) = 0.098 W/kg; SAR(10 g) = 0.037 W/kg

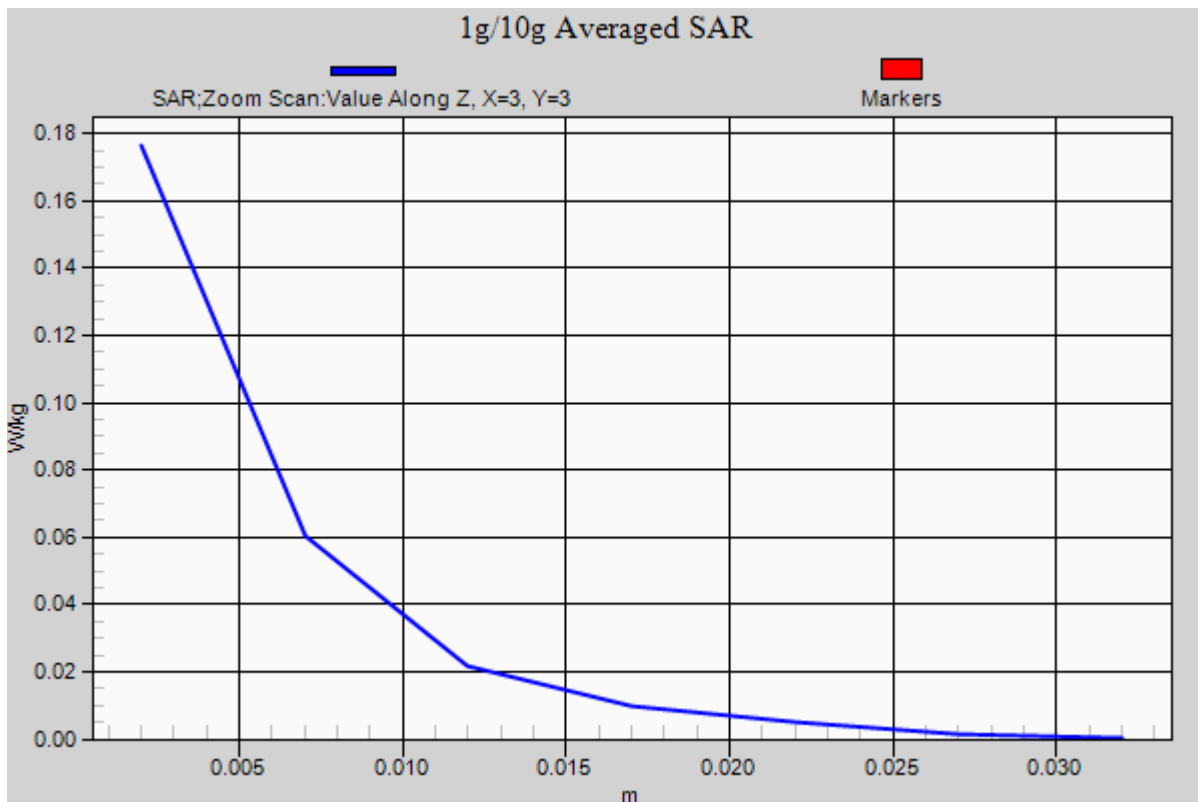

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.2G(802.11a/n/ac) (0); Frequency: 5190 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 5190$ MHz; $\sigma = 4.795$ S/m; $\epsilon_r = 36.314$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(5.34, 5.34, 5.34); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-31; Ambient Temp: 20.7; Tissue Temp:21.0

Touch from Body, Front, W-LAN(802.11n HT40 - 5.2G) Ch. 38, Ant Internal

Ant. 2


Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = 0.01 dB

Peak SAR (extrapolated) = 1.90 W/kg

SAR(1 g) = 0.482 W/kg; SAR(10 g) = 0.172 W/kg

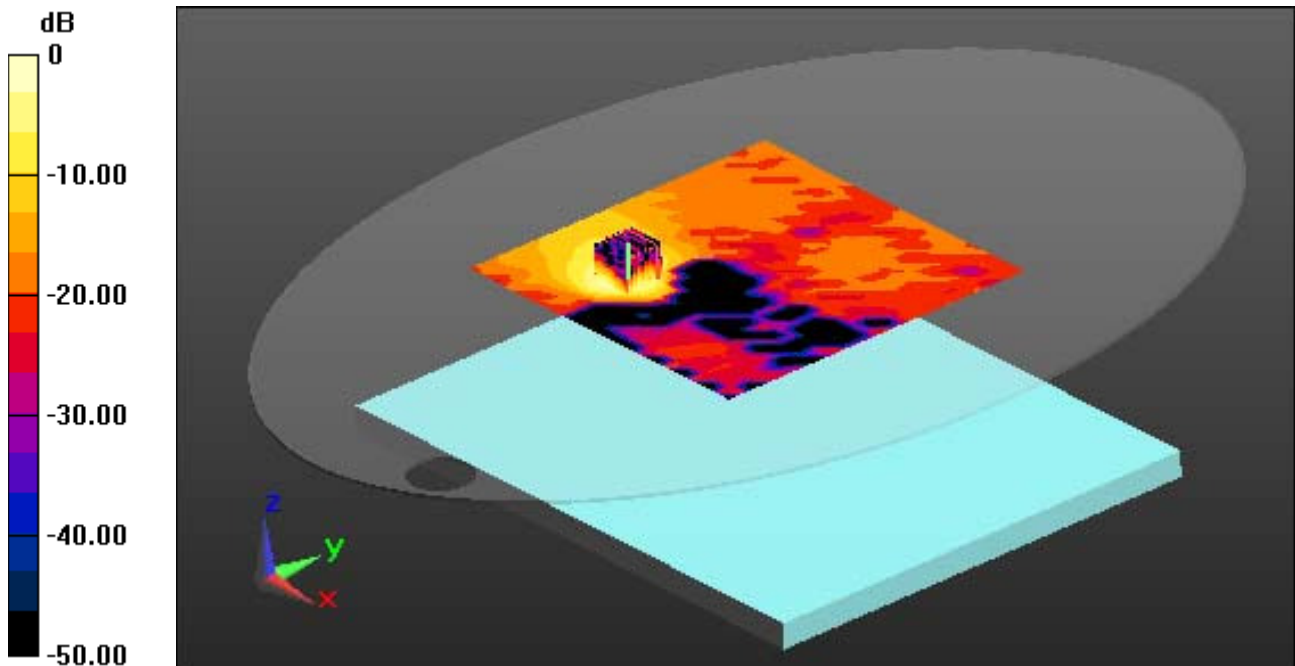

0 dB = 0.913 W/kg

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.2G(802.11a/n/ac) (0); Frequency: 5190 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 5190$ MHz; $\sigma = 4.795$ S/m; $\epsilon_r = 36.314$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(5.34, 5.34, 5.34); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-31; Ambient Temp: 20.7; Tissue Temp:21.0

Touch from Body, Front, W-LAN(802.11n HT40 - 5.2G) Ch. 38, Ant Internal

Ant. 2

With Enlarge plot image


Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = 0.01 dB

Peak SAR (extrapolated) = 1.90 W/kg

SAR(1 g) = 0.482 W/kg; SAR(10 g) = 0.172 W/kg

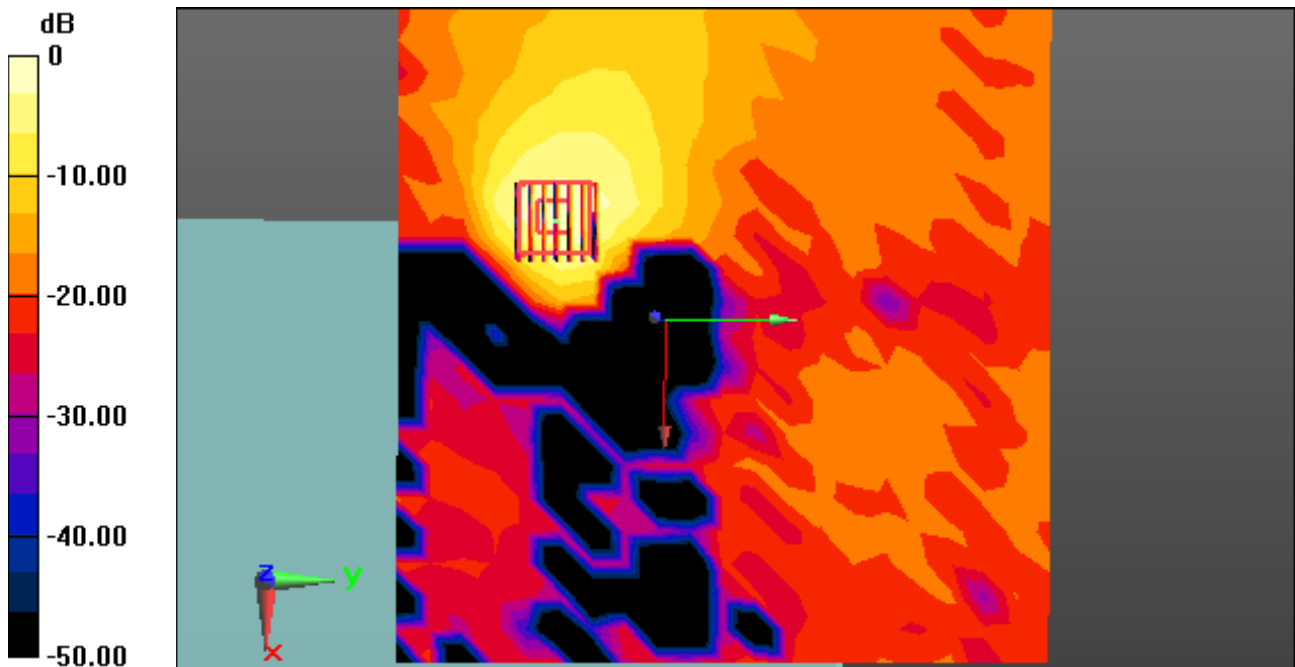

0 dB = 0.913 W/kg

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.2G(802.11a/n/ac) (0); Frequency: 5190 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5190$ MHz; $\sigma = 4.795$ S/m; $\epsilon_r = 36.314$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(5.34, 5.34, 5.34); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-31; Ambient Temp: 20.7; Tissue Temp: 21.0

Touch from Body, Front, W-LAN(802.11n HT40 - 5.2G) Ch. 38, Ant Internal

Ant. 2


Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = 0.01 dB

Peak SAR (extrapolated) = 1.90 W/kg

SAR(1 g) = 0.482 W/kg; SAR(10 g) = 0.172 W/kg

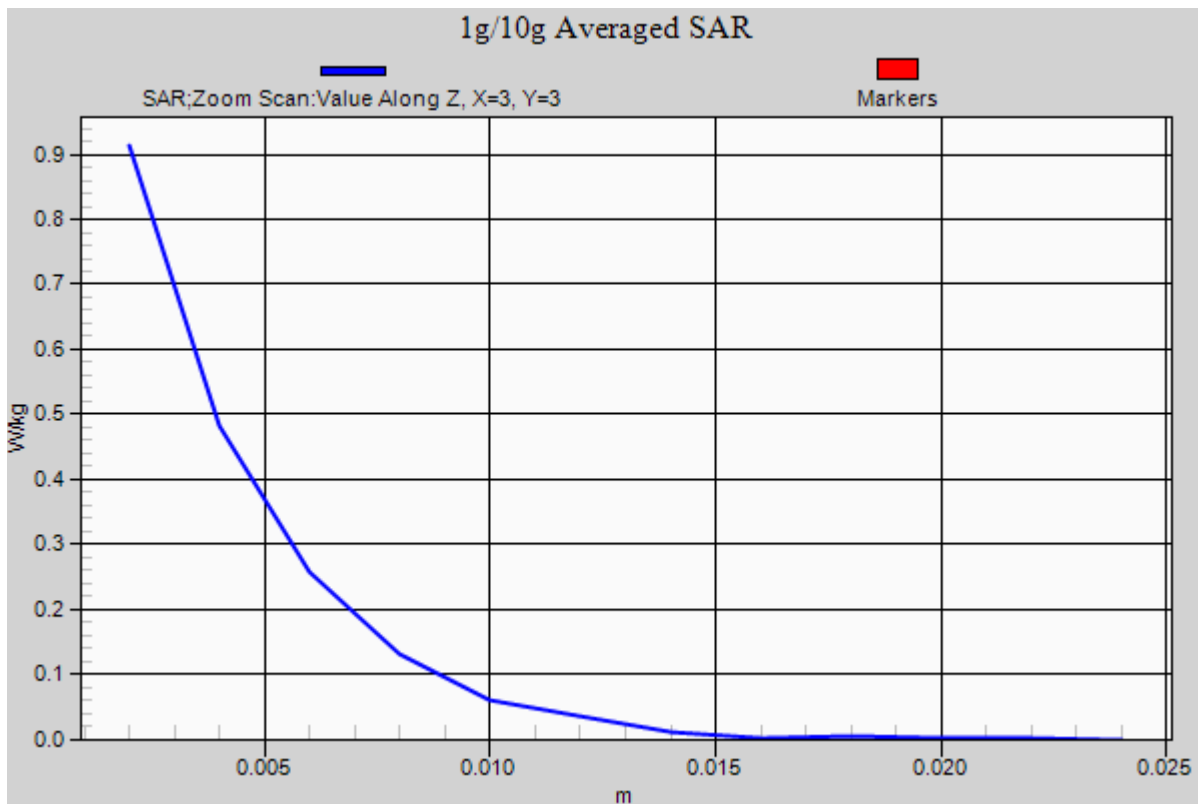

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.8G(802.11a/n/ac) (0); Frequency: 5745 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5745$ MHz; $\sigma = 5.152$ S/m; $\epsilon_r = 34.93$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.58, 4.58, 4.58); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-02-03; Ambient Temp: 21.3; Tissue Temp: 21.7

Touch from Body, Front, W-LAN(802.11n HT20 - 5.8G) Ch. 149, Ant Internal

Ant. 2


Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = -0.10 dB

Peak SAR (extrapolated) = 2.81 W/kg

SAR(1 g) = 0.661 W/kg; SAR(10 g) = 0.227 W/kg

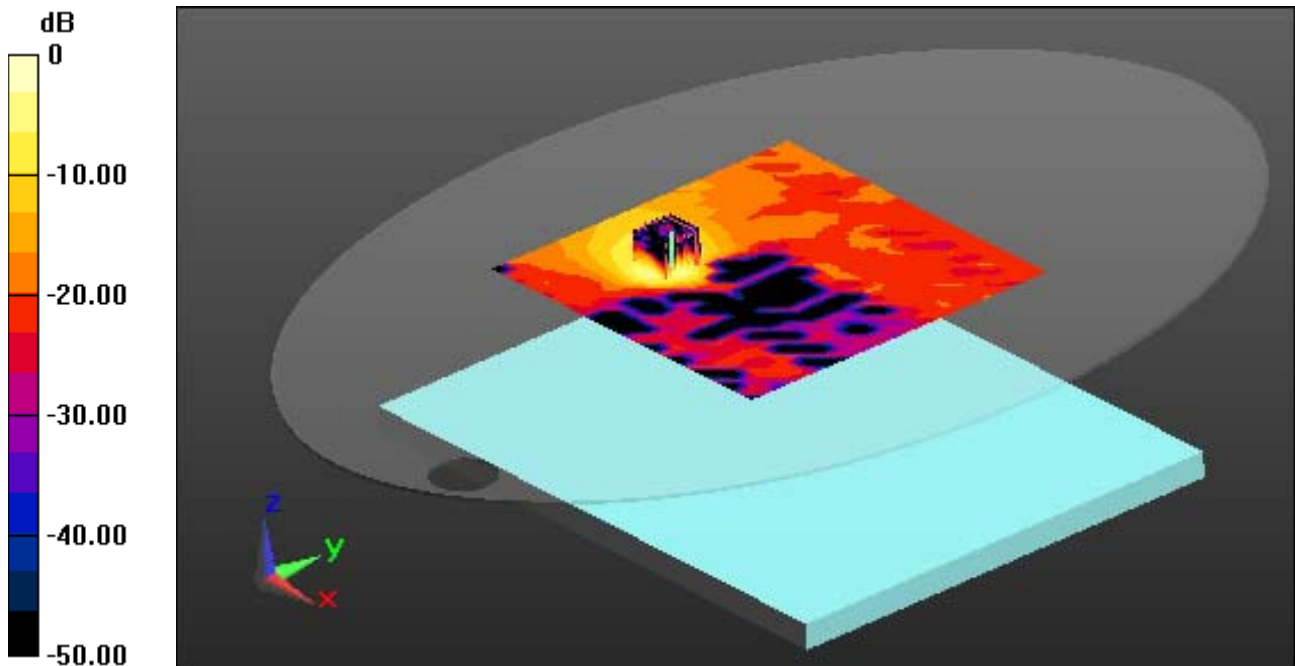

0 dB = 1.32 W/kg

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.8G(802.11a/n/ac) (0); Frequency: 5745 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 5745$ MHz; $\sigma = 5.152$ S/m; $\epsilon_r = 34.93$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.58, 4.58, 4.58); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-02-03; Ambient Temp: 21.3; Tissue Temp:21.7

Touch from Body, Front, W-LAN(802.11n HT20 - 5.8G) Ch. 149, Ant Internal

Ant. 2

With Enlarge plot image

Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = -0.10 dB

Peak SAR (extrapolated) = 2.81 W/kg

SAR(1 g) = 0.661 W/kg; SAR(10 g) = 0.227 W/kg

The figure is a 2D color plot representing the SAR field distribution. The vertical axis on the left is labeled 'dB' and ranges from 0 at the top to -50.00 at the bottom, with major ticks at 0, -10.00, -20.00, -30.00, -40.00, and -50.00. The plot area shows a complex, irregular pattern of colors, with a bright yellow/orange region at the top center, transitioning through red, orange, and purple to dark blue/black at the bottom. A red grid is overlaid on the plot, and a small 3D antenna model is visible in the bottom left corner. The plot is surrounded by a grey border.

0 dB = 1.32 W/kg

A3

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.8G(802.11a/n/ac) (0); Frequency: 5745 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 5745$ MHz; $\sigma = 5.152$ S/m; $\epsilon_r = 34.93$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.58, 4.58, 4.58); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-02-03; Ambient Temp: 21.3; Tissue Temp:21.7

Touch from Body, Front, W-LAN(802.11n HT20 - 5.8G) Ch. 149, Ant Internal

Ant. 2


Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = -0.10 dB

Peak SAR (extrapolated) = 2.81 W/kg

SAR(1 g) = 0.661 W/kg; SAR(10 g) = 0.227 W/kg

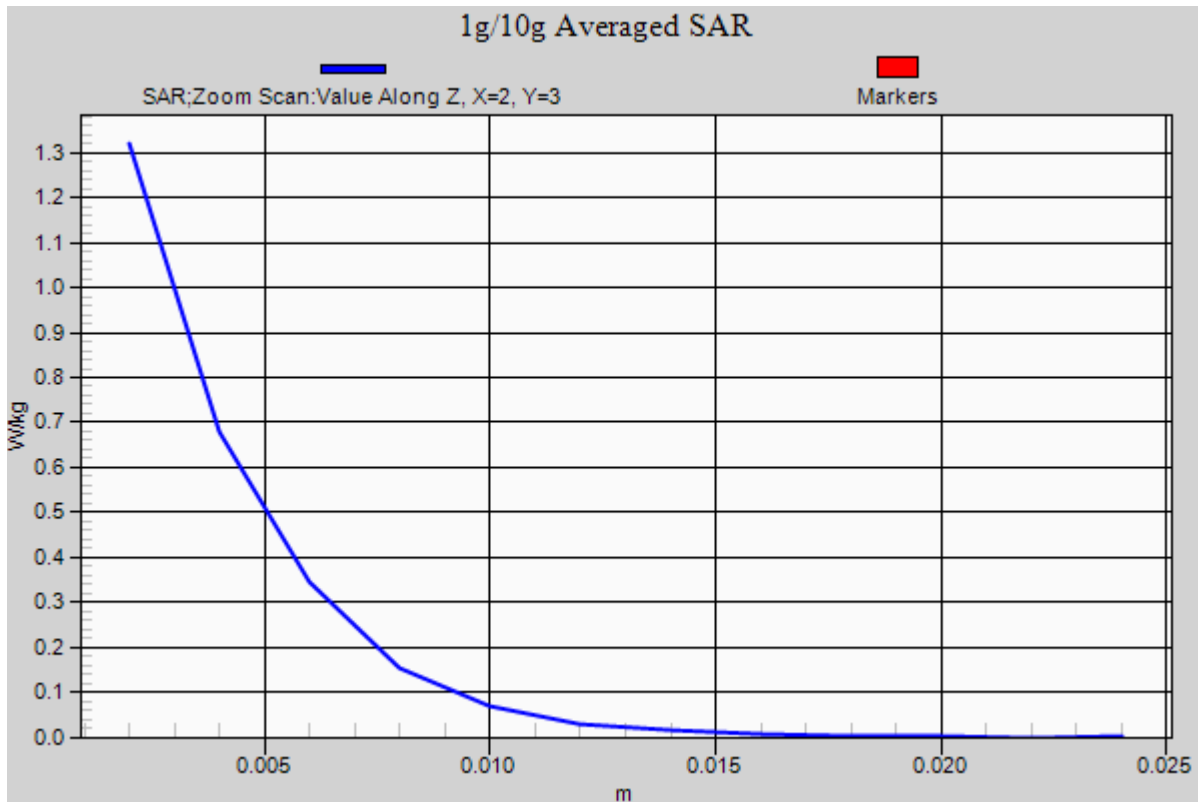

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 2.4G(802.11b/g/n20, 40) (0); Frequency: 2462 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 2462$ MHz; $\sigma = 1.922$ S/m; $\epsilon_r = 52.522$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(7.2, 7.2, 7.2); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-25; Ambient Temp: 20.8; Tissue Temp:21.4

Touch from Body, Front, W-LAN(802.11b - 2.4G) Ch. 11, Ant Internal

Ant. 1


Area Scan (17x17x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.04 dB

Peak SAR (extrapolated) = 0.254 W/kg

SAR(1 g) = 0.089 W/kg; SAR(10 g) = 0.034 W/kg

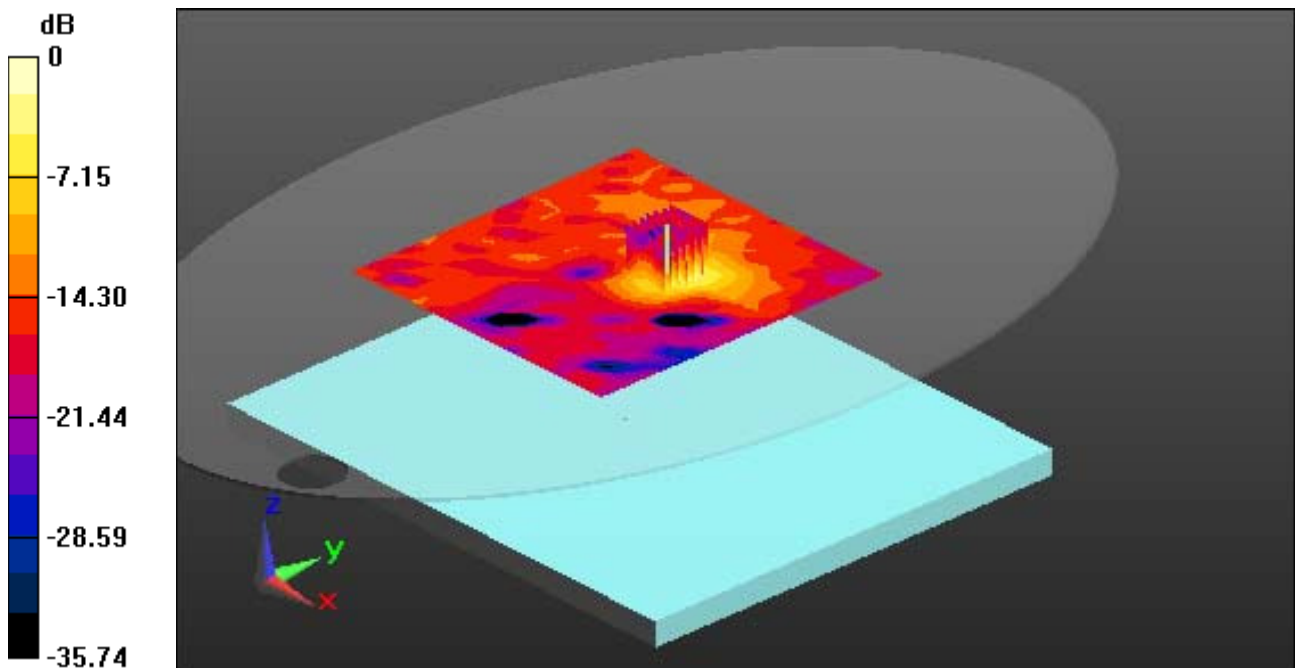

0 dB = 0.159 W/kg

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 2.4G(802.11b/g/n20, 40) (0); Frequency: 2462 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 2462$ MHz; $\sigma = 1.922$ S/m; $\epsilon_r = 52.522$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(7.2, 7.2, 7.2); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-25; Ambient Temp: 20.8; Tissue Temp:21.4

Touch from Body, Front, W-LAN(802.11b - 2.4G) Ch. 11, Ant Internal

Ant. 1

With Enlarge plot image


Area Scan (17x17x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.04 dB

Peak SAR (extrapolated) = 0.254 W/kg

SAR(1 g) = 0.089 W/kg; SAR(10 g) = 0.034 W/kg

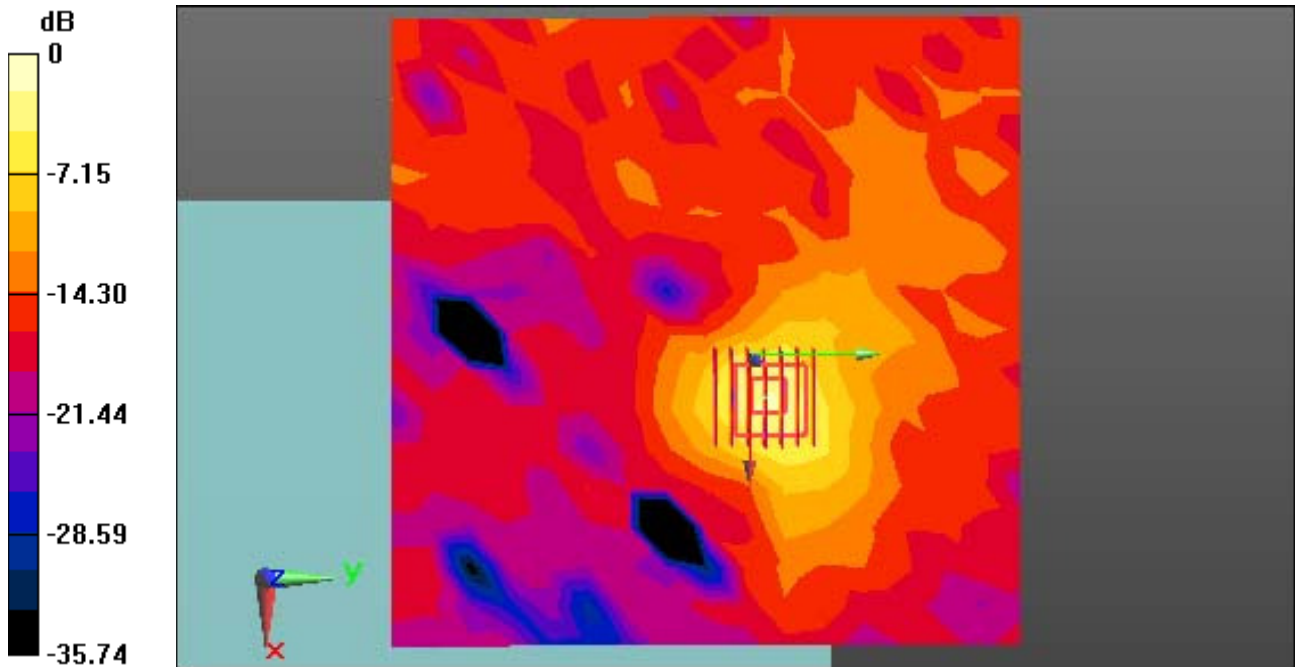

0 dB = 0.159 W/kg

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 2.4G(802.11b/g/n20, 40) (0); Frequency: 2462 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 2462$ MHz; $\sigma = 1.922$ S/m; $\epsilon_r = 52.522$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(7.2, 7.2, 7.2); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-25; Ambient Temp: 20.8; Tissue Temp:21.4

Touch from Body, Front, W-LAN(802.11b - 2.4G) Ch. 11, Ant Internal

Ant. 1


Area Scan (17x17x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.04 dB

Peak SAR (extrapolated) = 0.254 W/kg

SAR(1 g) = 0.089 W/kg; SAR(10 g) = 0.034 W/kg

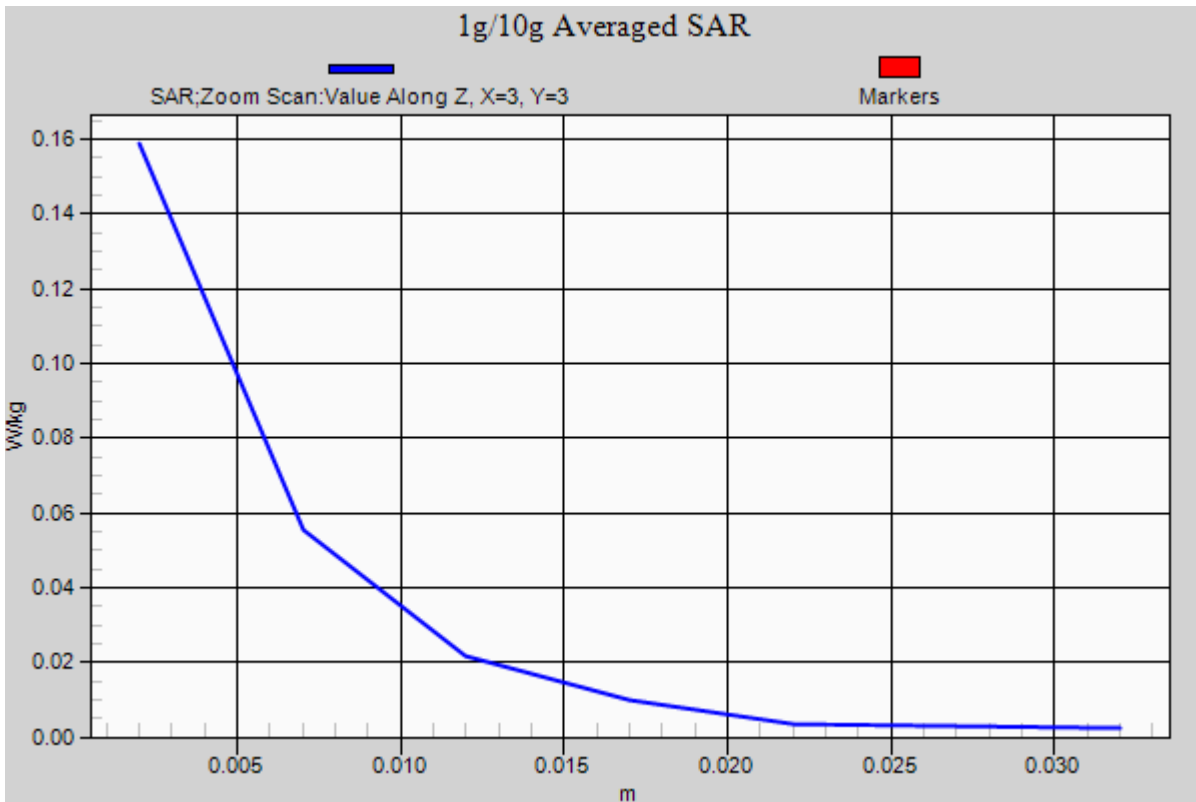

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.2G(802.11a/n/ac) (0); Frequency: 5180 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5180$ MHz; $\sigma = 5.348$ S/m; $\epsilon_r = 47.469$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.65, 4.65, 4.65); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-31; Ambient Temp: 20.7; Tissue Temp: 20.9

Touch from Body, Front, W-LAN(802.11n HT40 - 5.2G) Ch. 38, Ant Internal

Ant. 2


Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = -0.05 dB

Peak SAR (extrapolated) = 0.591 W/kg

SAR(1 g) = 0.156 W/kg; SAR(10 g) = 0.052 W/kg

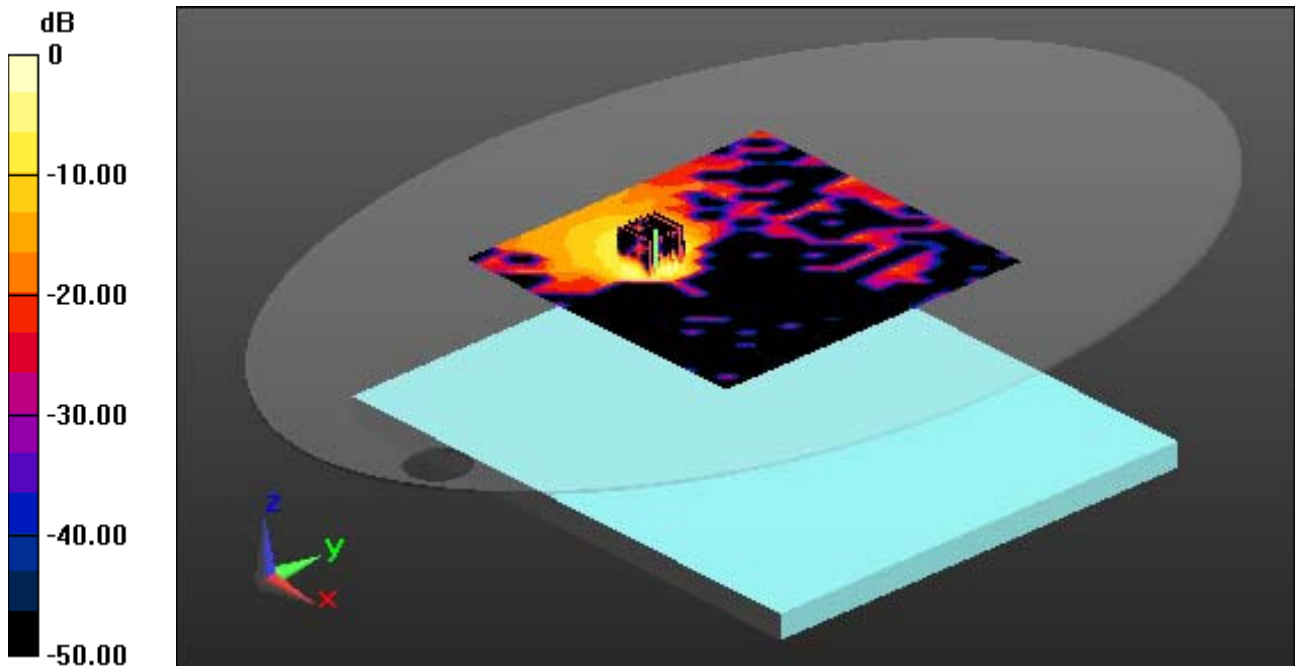

0 dB = 0.329 W/kg

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.2G(802.11a/n/ac) (0); Frequency: 5180 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 5180$ MHz; $\sigma = 5.348$ S/m; $\epsilon_r = 47.469$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.65, 4.65, 4.65); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-31; Ambient Temp: 20.7; Tissue Temp:20.9

Touch from Body, Front, W-LAN(802.11n HT40 - 5.2G) Ch. 38, Ant Internal

Ant. 2

With Enlarge plot image

Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = -0.05 dB

Peak SAR (extrapolated) = 0.591 W/kg

SAR(1 g) = 0.156 W/kg; SAR(10 g) = 0.052 W/kg

The figure is a 2D color plot representing the SAR field distribution. The vertical axis on the left is labeled 'dB' and ranges from 0 to -50.00 in increments of 10.00. The plot shows a central high-intensity region (yellow/orange) with a grid overlay, surrounded by lower intensity regions (red, blue, black). A 3D coordinate system (x, y, z) is visible in the bottom left corner.

0 dB = 0.329 W/kg

A5

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.2G(802.11a/n/ac) (0); Frequency: 5180 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 5180$ MHz; $\sigma = 5.348$ S/m; $\epsilon_r = 47.469$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.65, 4.65, 4.65); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-01-31; Ambient Temp: 20.7; Tissue Temp:20.9

Touch from Body, Front, W-LAN(802.11n HT40 - 5.2G) Ch. 38, Ant Internal


Ant. 2

Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm Power
Drift = -0.05 dB

Peak SAR (extrapolated) = 0.591 W/kg

SAR(1 g) = 0.156 W/kg; SAR(10 g) = 0.052 W/kg

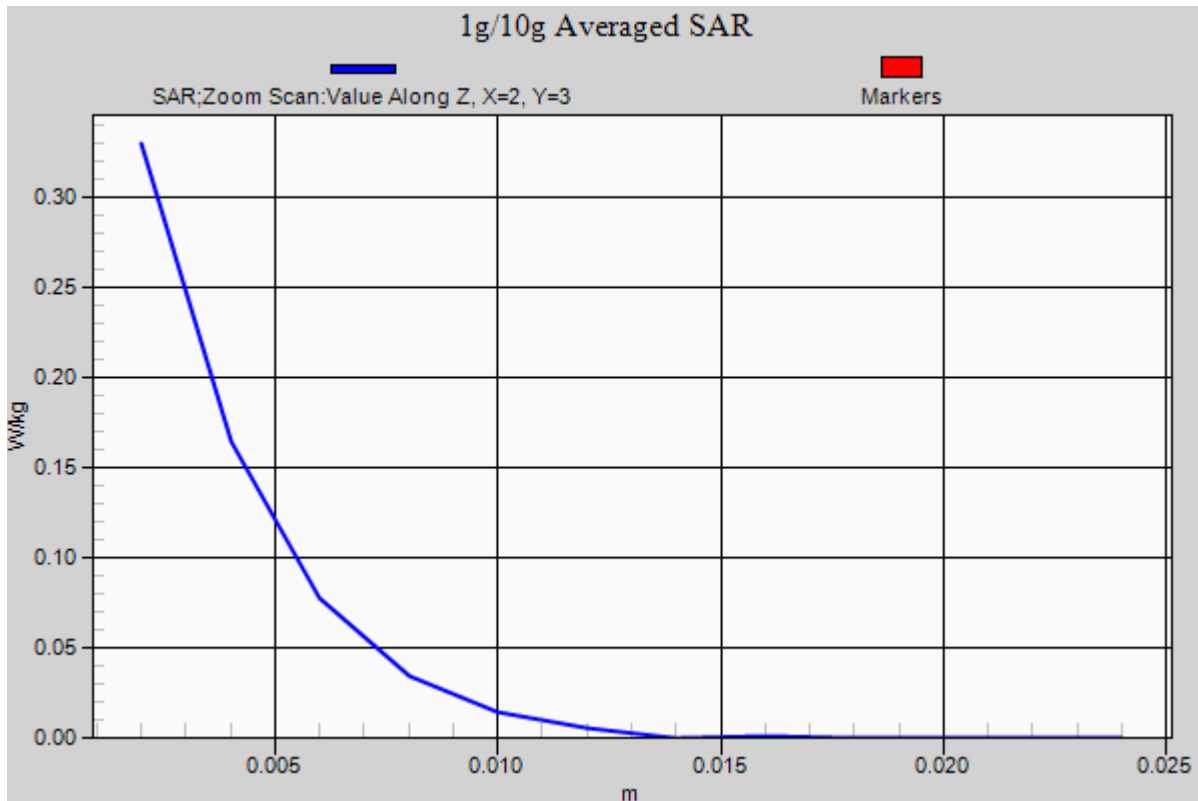

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.8G(802.11a/n/ac) (0); Frequency: 5745 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5745$ MHz; $\sigma = 6.058$ S/m; $\epsilon_r = 46.441$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.05, 4.05, 4.05); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-02-03; Ambient Temp: 21.3; Tissue Temp: 21.0

Touch from Body, Front, W-LAN(802.11n HT20 - 5.8G) Ch. 149, Ant Internal

Ant. 2


Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = -0.07 dB

Peak SAR (extrapolated) = 1.00 W/kg

SAR(1 g) = 0.270 W/kg; SAR(10 g) = 0.090 W/kg

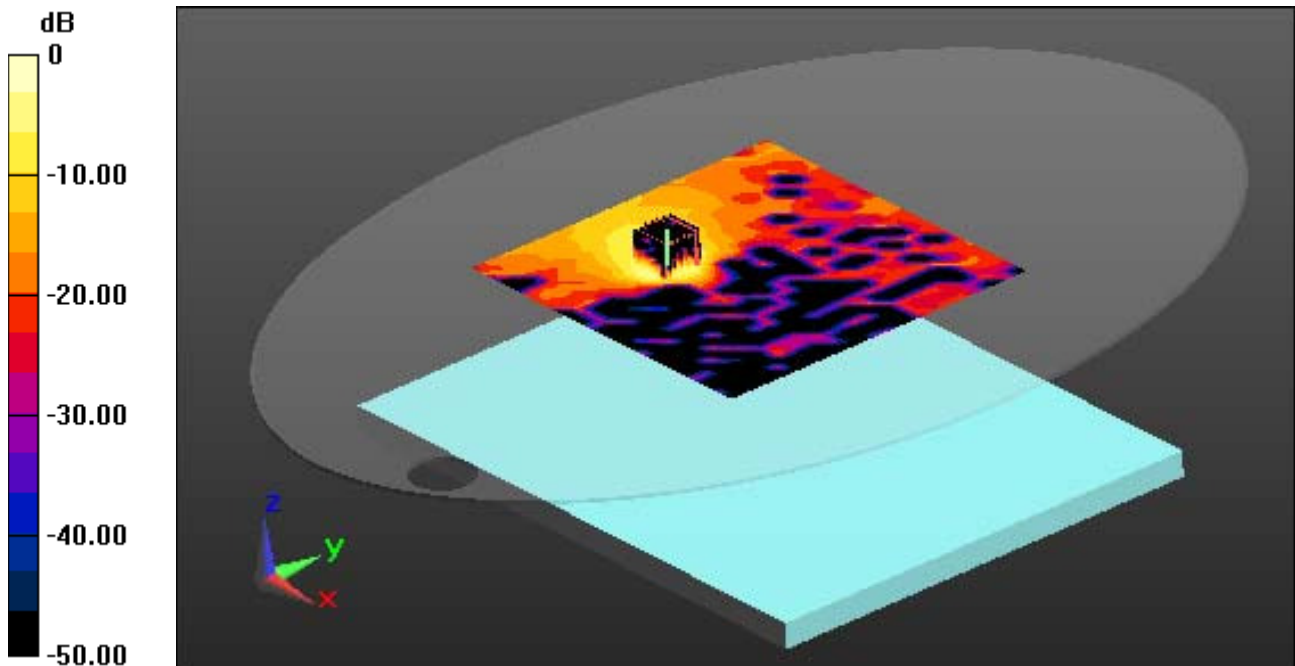

0 dB = 0.541 W/kg

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.8G(802.11a/n/ac) (0); Frequency: 5745 MHz;Duty Cycle: 1:1
Medium parameters used: $f = 5745$ MHz; $\sigma = 6.058$ S/m; $\epsilon_r = 46.441$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.05, 4.05, 4.05); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-02-03; Ambient Temp: 21.3; Tissue Temp:21.0

Touch from Body, Front, W-LAN(802.11n HT20 - 5.8G) Ch. 149, Ant Internal

Ant. 2

With Enlarge plot image

Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = -0.07 dB

Peak SAR (extrapolated) = 1.00 W/kg

SAR(1 g) = 0.270 W/kg; SAR(10 g) = 0.090 W/kg

The figure is a 2D color plot representing the SAR field distribution. The vertical axis on the left is labeled 'dB' and ranges from 0 to -50.00 in increments of 10.00. The plot shows a central high-intensity region (yellow/orange) with a peak value of 0 dB. This region is surrounded by a complex pattern of lower-intensity fields (red, purple, blue). A small inset in the bottom-left corner shows a 3D coordinate system with x, y, and z axes. A red box highlights a specific area of interest within the field distribution.

0 dB = 0.541 W/kg

A6

DT&C Co., Ltd.

DUT: EVS 2430W; Type: X-ray Detector

Communication System: W-LAN 5.8G(802.11a/n/ac) (0); Frequency: 5745 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 5745$ MHz; $\sigma = 6.058$ S/m; $\epsilon_r = 46.441$; $\rho = 1000$ kg/m³
Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN3866; ConvF(4.05, 4.05, 4.05); Calibrated: 6/29/2016; Electronics: DAE4 Sn1392
Phantom: ELI v6.0; Type: QDOVA003AA; Serial: TP:2008
Measurement SW: DASY52, Version 52.8 (8); SEMCAD X Version 14.6.10 (7331)

Test Date: 2017-02-03; Ambient Temp: 21.3; Tissue Temp: 21.0

Touch from Body, Front, W-LAN(802.11n HT20 - 5.8G) Ch. 149, Ant Internal

Ant. 2

Area Scan (21x21x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x12)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=2mm

Power Drift = -0.07 dB

Peak SAR (extrapolated) = 1.00 W/kg

SAR(1 g) = 0.270 W/kg; SAR(10 g) = 0.090 W/kg

