



Label and Location




**Detector Case
(460 x 460 mm)**



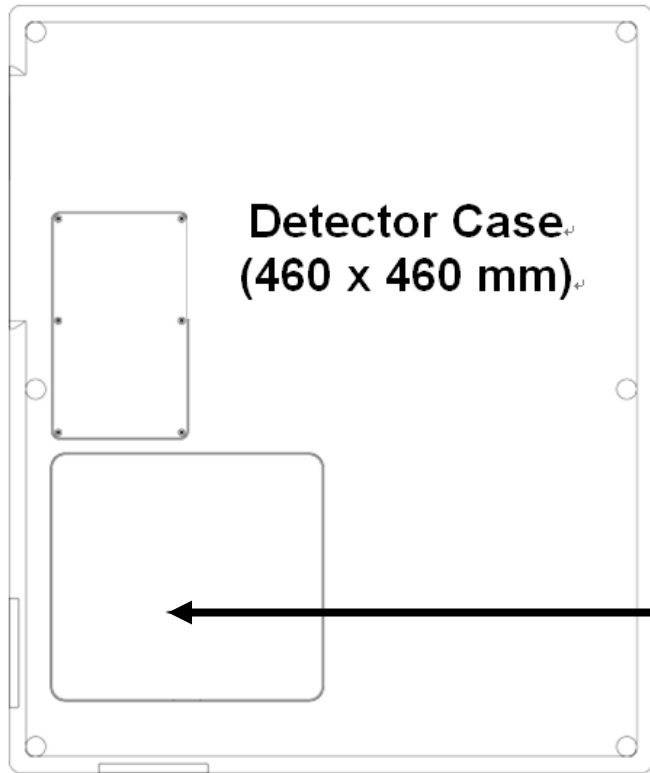


DRTECH  DRTECH Corporation
Suite No.2, 3 Floor, 29, Dunchon-daero 541beon-gil,
Jungwon-gu, Seongnam-si, Gyeonggi-do, Republic of Korea
Tel : 82-31-730-6800 FAX: 82-31-730-6899
<http://www.drtech.co.kr>

Product Name : Flat Panel Digital X-ray Detector
Model : EVS 3643
Weight/Dimension (WxLxH) : 2.98kg / 386 x 460 x 14mm
Power : Use only with adaptor XP Power, AHM85PS12 or Li-ion Polymer Battery DRTECH, EVS-Battery-Pack

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions:
(1) This device may not cause harmful interference, and
(2) this device must accept any interference received, including interference that may cause undesired operation.

EC REP EXAMION GmbH
Erich-Herion Stuttgart, 37 in 70736 Fellbach, Germany

 No field serviceable component inside. – Do not attempt to open the case.

   FCC ID : RNH-EVS3643   MEDICAL EQUIPMENT
ANSI/AAMI ES60601-1(2012)
CAN/CSA-C22.2
NO.60601-1(2014)

1177 35LV