

## #01\_HAC\_E\_GSM850\_GSM Voice\_Ch128

Communication System: GSM-FDD (TDMA, GMSK); Frequency: 824.2 MHz; Duty Cycle: 1:8.6896

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1399; Calibrated: 2017/11/16
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

### E Scan - ER3D: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test

**(101x101x1)**: Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 123.2 V/m; Power Drift = -0.04 dB

Applied MIF = 3.63 dB

RF audio interference level = 40.91 dBV/m

**Emission category: M3**

MIF scaled E-field



|  |  |  |
|--|--|--|
| Grid 1 <b>M4</b><br><b>37.77 dBV/m</b> | Grid 2 <b>M3</b><br><b>40.02 dBV/m</b> | Grid 3 <b>M4</b><br><b>39.4 dBV/m</b>  |
| Grid 4 <b>M4</b><br><b>38.53 dBV/m</b> | Grid 5 <b>M3</b><br><b>40.91 dBV/m</b> | Grid 6 <b>M3</b><br><b>40.12 dBV/m</b> |
| Grid 7 <b>M4</b><br><b>38.5 dBV/m</b>  | Grid 8 <b>M3</b><br><b>40.84 dBV/m</b> | Grid 9 <b>M3</b><br><b>40.03 dBV/m</b> |

**Cursor:**

Total = 40.91 dBV/m

E Category: M3

Location: -2.5, 5, 8.7 mm

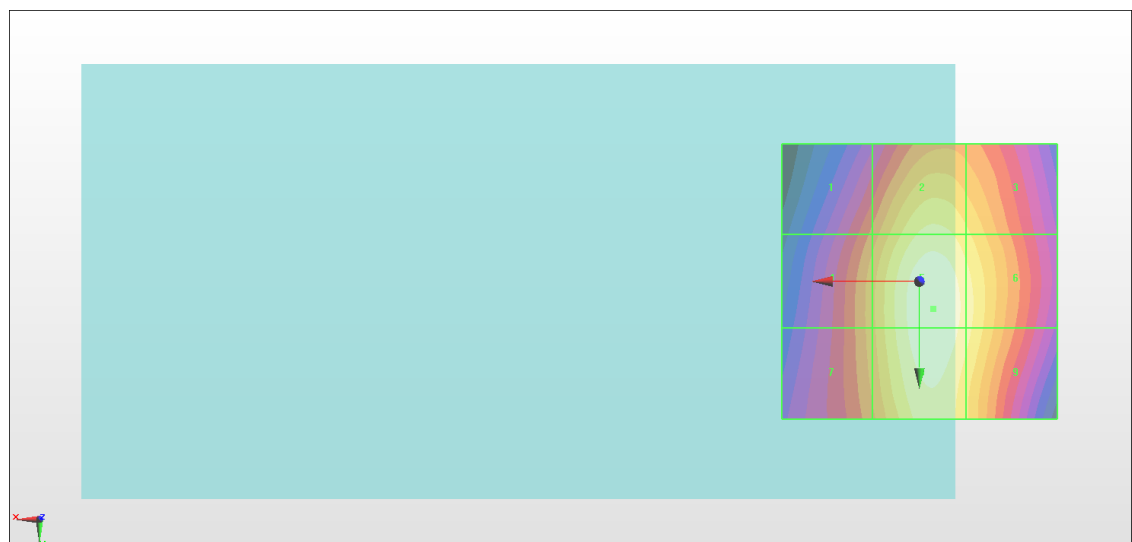

0 dB = 111.1 V/m = 40.91 dBV/m

## #02\_HAC\_E\_GSM850\_GSM Voice\_Ch189

Communication System: GSM-FDD (TDMA, GMSK); Frequency: 836.4 MHz; Duty Cycle: 1:8.6896

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1399; Calibrated: 2017/11/16
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

### E Scan - ER3D: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test

**(101x101x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 129.6 V/m; Power Drift = -0.08 dB

Applied MIF = 3.63 dB

RF audio interference level = 41.39 dBV/m

**Emission category: M3**

MIF scaled E-field


|  |  |  |
|--|--|--|
| Grid 1 <b>M4</b><br><b>38.05 dBV/m</b> | Grid 2 <b>M3</b><br><b>40.4 dBV/m</b>  | Grid 3 <b>M4</b><br><b>39.87 dBV/m</b> |
| Grid 4 <b>M4</b><br><b>38.91 dBV/m</b> | Grid 5 <b>M3</b><br><b>41.39 dBV/m</b> | Grid 6 <b>M3</b><br><b>40.7 dBV/m</b>  |
| Grid 7 <b>M4</b><br><b>38.9 dBV/m</b>  | Grid 8 <b>M3</b><br><b>41.37 dBV/m</b> | Grid 9 <b>M3</b><br><b>40.65 dBV/m</b> |

**Cursor:**

Total = 41.39 dBV/m

E Category: M3

Location: -2.5, 6, 8.7 mm

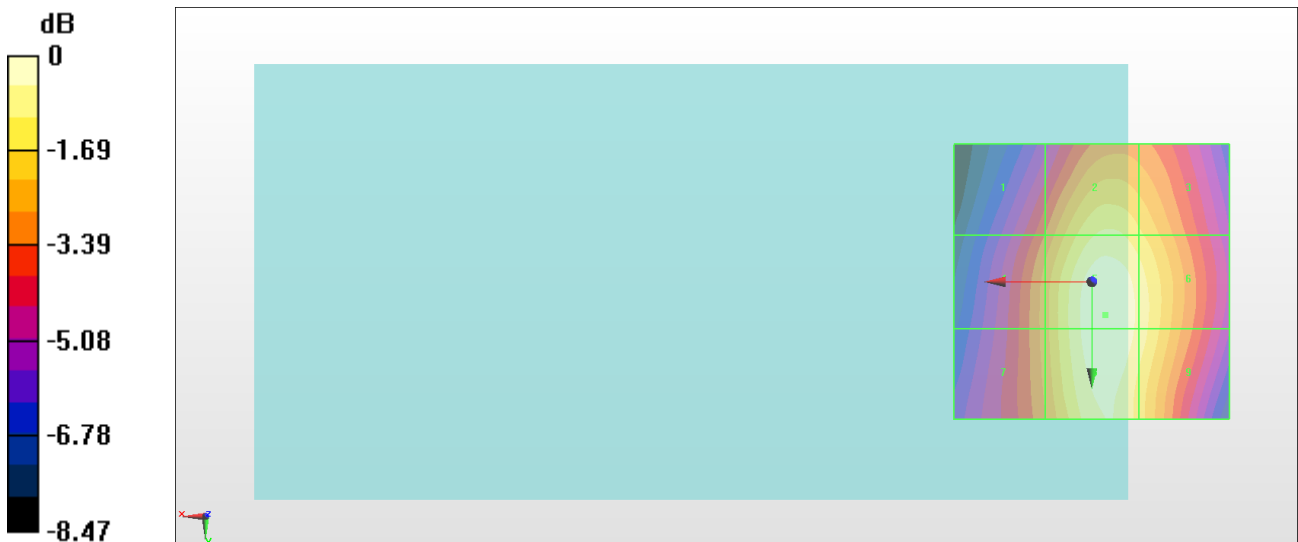

0 dB = 117.4 V/m = 41.39 dBV/m

### #03\_HAC\_E\_GSM850\_GSM Voice\_Ch251

Communication System: GSM-FDD (TDMA, GMSK); Frequency: 848.8 MHz; Duty Cycle: 1:8.6896

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1399; Calibrated: 2017/11/16
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

### E Scan - ER3D: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test

**(101x101x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 136.1 V/m; Power Drift = -0.01 dB

Applied MIF = 3.63 dB

RF audio interference level = 41.95 dBV/m

**Emission category: M3**

MIF scaled E-field


|  |  |  |
|--|--|--|
| Grid 1 <b>M4</b><br><b>38.3 dBV/m</b>  | Grid 2 <b>M3</b><br><b>40.72 dBV/m</b> | Grid 3 <b>M3</b><br><b>40.3 dBV/m</b>  |
| Grid 4 <b>M4</b><br><b>39.42 dBV/m</b> | Grid 5 <b>M3</b><br><b>41.95 dBV/m</b> | Grid 6 <b>M3</b><br><b>41.27 dBV/m</b> |
| Grid 7 <b>M4</b><br><b>39.43 dBV/m</b> | Grid 8 <b>M3</b><br><b>41.94 dBV/m</b> | Grid 9 <b>M3</b><br><b>41.25 dBV/m</b> |

**Cursor:**

Total = 41.95 dBV/m

E Category: M3

Location: -3, 7, 8.7 mm

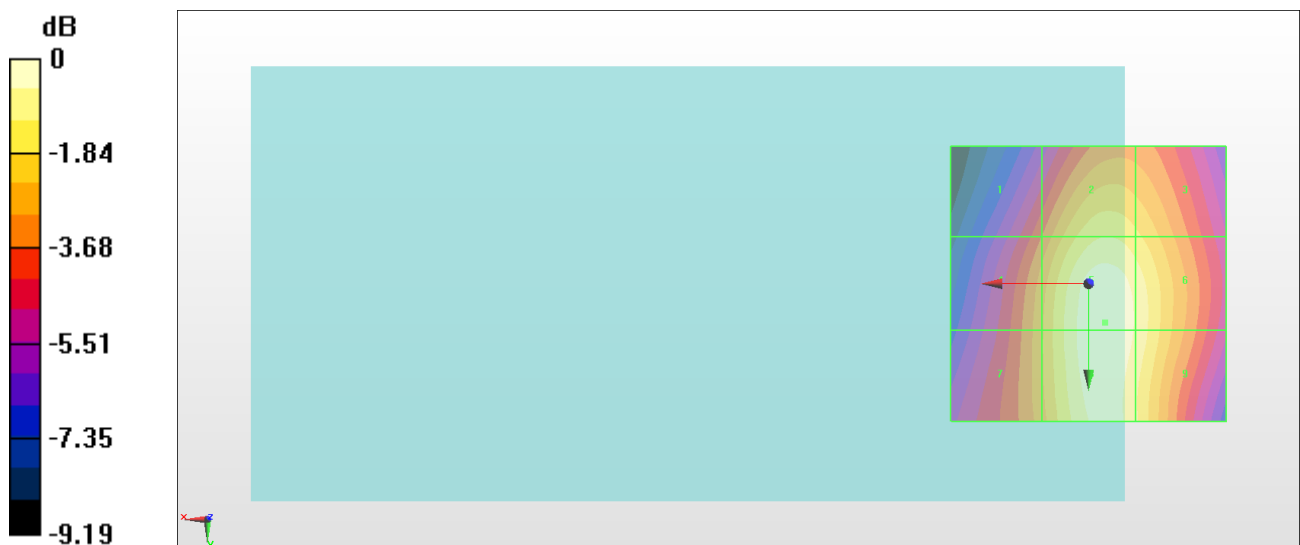

0 dB = 125.1 V/m = 41.95 dBV/m

## #04\_HAC\_E\_GSM1900\_GSM Voice\_Ch512

Communication System: GSM-FDD (TDMA, GMSK); Frequency: 1850.2 MHz; Duty Cycle: 1:8.6896

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1399; Calibrated: 2017/11/16
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

### E Scan - ER3D: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test

**(101x101x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 20.96 V/m; Power Drift = 0.01 dB

Applied MIF = 3.63 dB

RF audio interference level = 24.80 dBV/m

**Emission category: M4**

MIF scaled E-field



|  |  |  |
|--|--|--|
| Grid 1 <b>M4</b><br><b>22.14 dBV/m</b> | Grid 2 <b>M4</b><br><b>22.8 dBV/m</b>  | Grid 3 <b>M4</b><br><b>22.05 dBV/m</b> |
| Grid 4 <b>M4</b><br><b>22.84 dBV/m</b> | Grid 5 <b>M4</b><br><b>24.8 dBV/m</b>  | Grid 6 <b>M4</b><br><b>23.86 dBV/m</b> |
| Grid 7 <b>M4</b><br><b>22.04 dBV/m</b> | Grid 8 <b>M4</b><br><b>24.22 dBV/m</b> | Grid 9 <b>M4</b><br><b>23.65 dBV/m</b> |

**Cursor:**

Total = 24.80 dBV/m

E Category: M4

Location: -1, 3.5, 8.7 mm

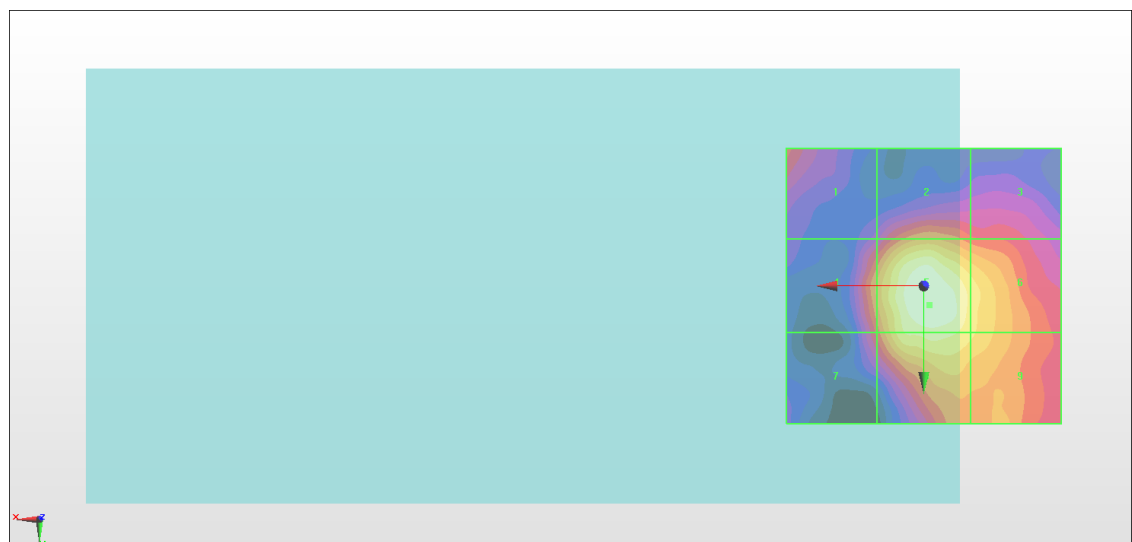

0 dB = 17.37 V/m = 24.80 dBV/m

### #05\_HAC\_E\_GSM1900\_GSM Voice\_Ch661

Communication System: GSM-FDD (TDMA, GMSK); Frequency: 1880 MHz; Duty Cycle: 1:8.6896

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1399; Calibrated: 2017/11/16
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

### E Scan - ER3D: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test

**(101x101x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 21.44 V/m; Power Drift = -0.01 dB

Applied MIF = 3.63 dB

RF audio interference level = 25.22 dBV/m

**Emission category: M4**

MIF scaled E-field



|  |  |  |
|--|--|--|
| Grid 1 <b>M4</b><br><b>23.06 dBV/m</b> | Grid 2 <b>M4</b><br><b>23.21 dBV/m</b> | Grid 3 <b>M4</b><br><b>22.26 dBV/m</b> |
| Grid 4 <b>M4</b><br><b>23.31 dBV/m</b> | Grid 5 <b>M4</b><br><b>25.22 dBV/m</b> | Grid 6 <b>M4</b><br><b>24.08 dBV/m</b> |
| Grid 7 <b>M4</b><br><b>22.43 dBV/m</b> | Grid 8 <b>M4</b><br><b>24.76 dBV/m</b> | Grid 9 <b>M4</b><br><b>23.97 dBV/m</b> |

**Cursor:**

Total = 25.22 dBV/m

E Category: M4

Location: -1, 4, 8.7 mm

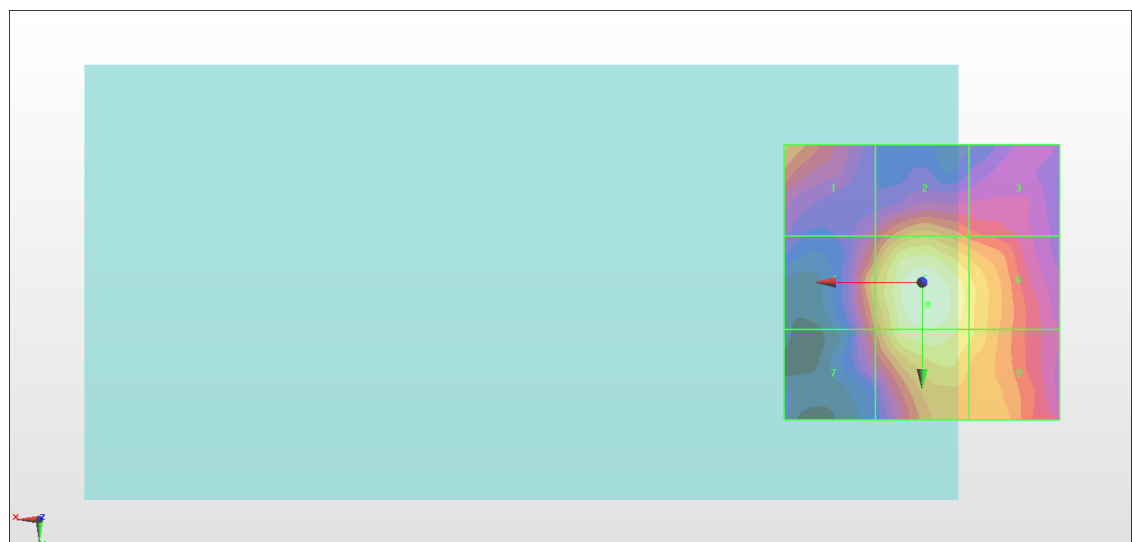

0 dB = 18.25 V/m = 25.23 dBV/m

## #06\_HAC\_E\_GSM1900\_GSM Voice\_Ch810

Communication System: GSM-FDD (TDMA, GMSK); Frequency: 1909.8 MHz; Duty Cycle: 1:8.6896

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1399; Calibrated: 2017/11/16
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

### E Scan - ER3D: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test

**(101x101x1):** Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 21.15 V/m; Power Drift = 0.02 dB

Applied MIF = 3.63 dB

RF audio interference level = 24.97 dBV/m

**Emission category: M4**

MIF scaled E-field



|  |  |  |
|--|--|--|
| Grid 1 <b>M4</b><br><b>22.43 dBV/m</b> | Grid 2 <b>M4</b><br><b>22.93 dBV/m</b> | Grid 3 <b>M4</b><br><b>22.11 dBV/m</b> |
| Grid 4 <b>M4</b><br><b>22.88 dBV/m</b> | Grid 5 <b>M4</b><br><b>24.97 dBV/m</b> | Grid 6 <b>M4</b><br><b>23.9 dBV/m</b>  |
| Grid 7 <b>M4</b><br><b>22.02 dBV/m</b> | Grid 8 <b>M4</b><br><b>24.38 dBV/m</b> | Grid 9 <b>M4</b><br><b>23.68 dBV/m</b> |

**Cursor:**

Total = 24.97 dBV/m

E Category: M4

Location: -1, 3.5, 8.7 mm

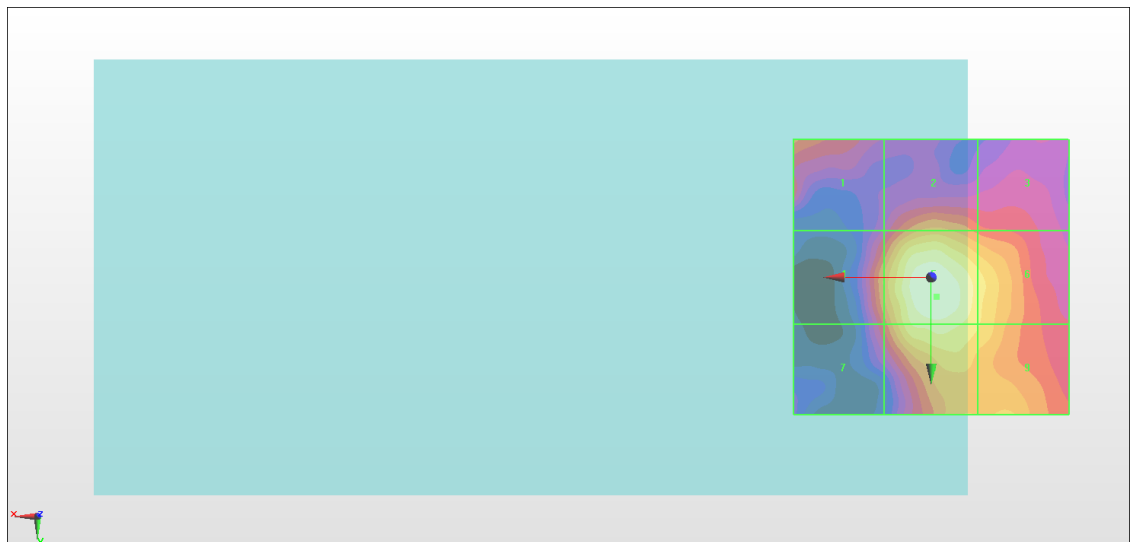

0 dB = 17.72 V/m = 24.97 dBV/m

### #07\_HAC\_E\_LTE Band 41\_20M\_QPSK\_1\_0\_Ch39750

Communication System: LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK); Frequency: 2506 MHz; Duty Cycle: 1:8.33681

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1399; Calibrated: 2017/11/16
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

### E Scan - ER3D: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test (101x101x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 5.292 V/m; Power Drift = 0.19 dB

Applied MIF = -1.62 dB

RF audio interference level = 15.12 dBV/m

**Emission category: M4**

MIF scaled E-field



|  |  |  |
|--|--|--|
| Grid 1 <b>M4</b><br><b>13.13 dBV/m</b> | Grid 2 <b>M4</b><br><b>14.96 dBV/m</b> | Grid 3 <b>M4</b><br><b>14.27 dBV/m</b> |
| Grid 4 <b>M4</b><br><b>13.04 dBV/m</b> | Grid 5 <b>M4</b><br><b>13.02 dBV/m</b> | Grid 6 <b>M4</b><br><b>12.82 dBV/m</b> |
| Grid 7 <b>M4</b><br><b>14.02 dBV/m</b> | Grid 8 <b>M4</b><br><b>14.92 dBV/m</b> | Grid 9 <b>M4</b><br><b>15.12 dBV/m</b> |

**Cursor:**

Total = 15.12 dBV/m

E Category: M4

Location: -14, 25, 8.7 mm

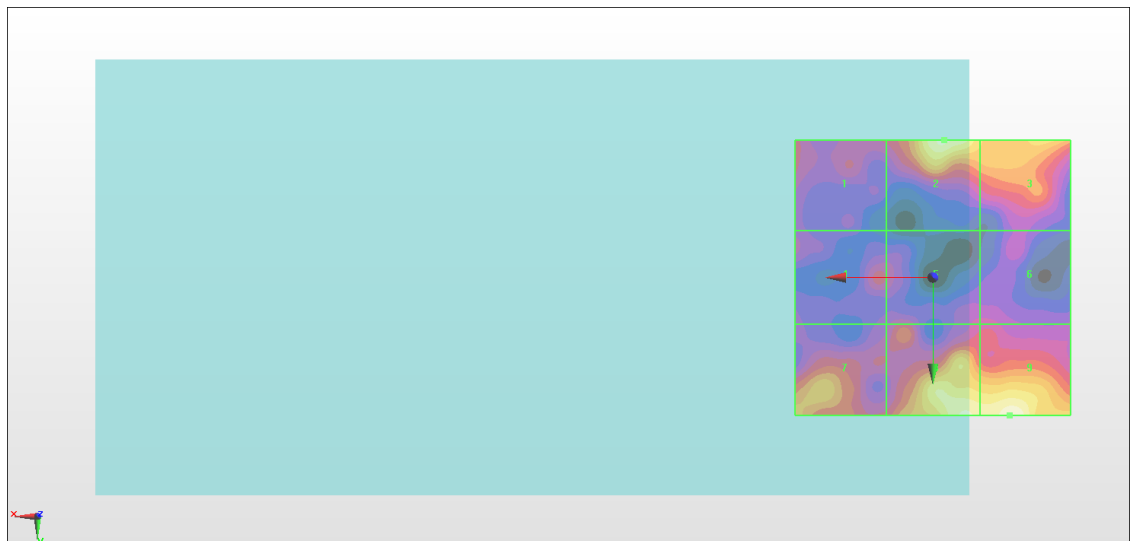

0 dB = 5.699 V/m = 15.12 dBV/m

### #08\_HAC\_E\_LTE Band 41\_20M\_QPSK\_1\_0\_Ch40185

Communication System: LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK); Frequency: 2549.5 MHz; Duty Cycle: 1:8.33681

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1399; Calibrated: 2017/11/16
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

### E Scan - ER3D: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test (101x101x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 7.272 V/m; Power Drift = -0.04 dB

Applied MIF = -1.62 dB

RF audio interference level = 15.84 dBV/m

**Emission category: M4**

MIF scaled E-field


|  |  |  |
|--|--|--|
| Grid 1 <b>M4</b><br><b>14.7 dBV/m</b>  | Grid 2 <b>M4</b><br><b>14.86 dBV/m</b> | Grid 3 <b>M4</b><br><b>14.7 dBV/m</b>  |
| Grid 4 <b>M4</b><br><b>15.05 dBV/m</b> | Grid 5 <b>M4</b><br><b>15.06 dBV/m</b> | Grid 6 <b>M4</b><br><b>15.46 dBV/m</b> |
| Grid 7 <b>M4</b><br><b>15.84 dBV/m</b> | Grid 8 <b>M4</b><br><b>15.24 dBV/m</b> | Grid 9 <b>M4</b><br><b>15.52 dBV/m</b> |

**Cursor:**

Total = 15.84 dBV/m

E Category: M4

Location: 21, 19.5, 8.7 mm



0 dB = 6.194 V/m = 15.84 dBV/m



### #09\_HAC\_E\_LTE Band 41\_20M\_QPSK\_1\_0\_Ch40620

Communication System: LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK); Frequency: 2593 MHz; Duty Cycle: 1:8.33681

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1399; Calibrated: 2017/11/16
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

### E Scan - ER3D: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test (101x101x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 8.026 V/m; Power Drift = -0.06 dB

Applied MIF = -1.62 dB

RF audio interference level = 16.96 dBV/m

**Emission category: M4**

MIF scaled E-field


|  |  |  |
|--|--|--|
| Grid 1 <b>M4</b><br><b>15.55 dBV/m</b> | Grid 2 <b>M4</b><br><b>16.96 dBV/m</b> | Grid 3 <b>M4</b><br><b>16.74 dBV/m</b> |
| Grid 4 <b>M4</b><br><b>15.97 dBV/m</b> | Grid 5 <b>M4</b><br><b>16.08 dBV/m</b> | Grid 6 <b>M4</b><br><b>16.7 dBV/m</b>  |
| Grid 7 <b>M4</b><br><b>16.44 dBV/m</b> | Grid 8 <b>M4</b><br><b>15.09 dBV/m</b> | Grid 9 <b>M4</b><br><b>15.43 dBV/m</b> |

**Cursor:**

Total = 16.96 dBV/m

E Category: M4

Location: -2, -25, 8.7 mm

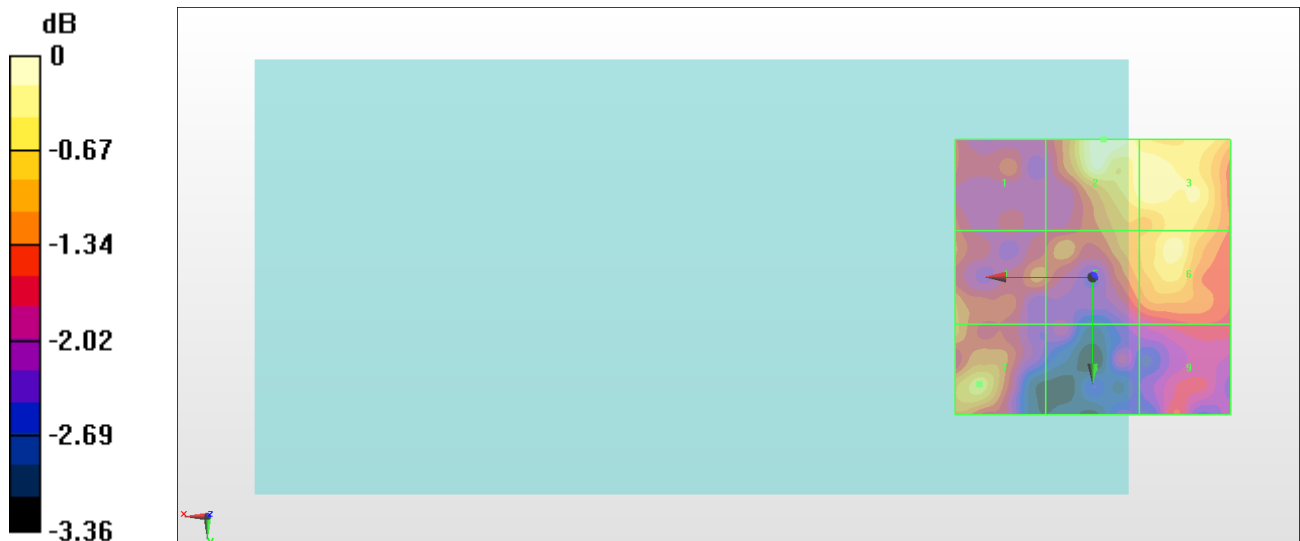

0 dB = 7.047 V/m = 16.96 dBV/m

## #10\_HAC\_E\_LTE Band 41\_20M\_QPSK\_1\_0\_Ch41055

Communication System: LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK); Frequency: 2636.5 MHz; Duty Cycle: 1:8.33681

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1399; Calibrated: 2017/11/16
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

### E Scan - ER3D: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test (101x101x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 7.150 V/m; Power Drift = 0.13 dB

Applied MIF = -1.62 dB

RF audio interference level = 17.76 dBV/m

**Emission category: M4**

MIF scaled E-field


|  |  |  |
|--|--|--|
| Grid 1 <b>M4</b><br><b>16.05 dBV/m</b> | Grid 2 <b>M4</b><br><b>17.76 dBV/m</b> | Grid 3 <b>M4</b><br><b>17.47 dBV/m</b> |
| Grid 4 <b>M4</b><br><b>16.17 dBV/m</b> | Grid 5 <b>M4</b><br><b>16.4 dBV/m</b>  | Grid 6 <b>M4</b><br><b>16.93 dBV/m</b> |
| Grid 7 <b>M4</b><br><b>16.77 dBV/m</b> | Grid 8 <b>M4</b><br><b>14.9 dBV/m</b>  | Grid 9 <b>M4</b><br><b>15.61 dBV/m</b> |

**Cursor:**

Total = 17.76 dBV/m

E Category: M4

Location: -2.5, -25, 8.7 mm

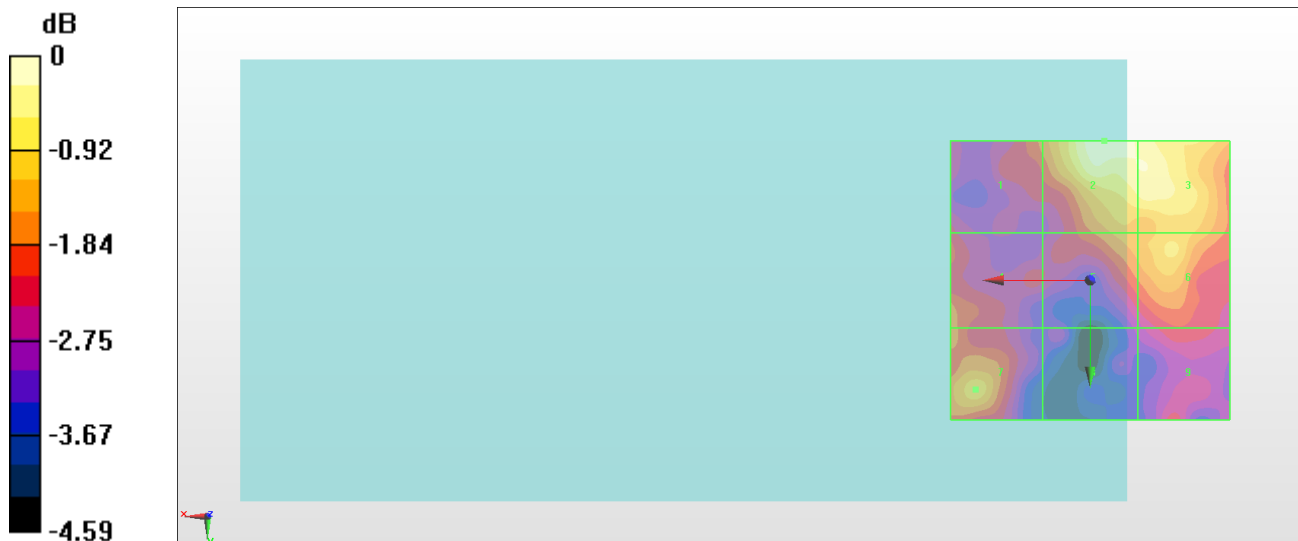

0 dB = 7.723 V/m = 17.76 dBV/m

## #11\_HAC\_E\_LTE Band 41\_20M\_QPSK\_1\_0\_Ch41490

Communication System: LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK); Frequency: 2680 MHz; Duty Cycle: 1:8.33681

Medium: Air Medium parameters used:  $\sigma = 0$  S/m,  $\epsilon_r = 1$ ;  $\rho = 0$  kg/m<sup>3</sup>

Ambient Temperature : 23.5 °C

DASY5 Configuration:

- Probe: ER3DV6 - SN2358; ConvF(1, 1, 1); Calibrated: 2018/1/19;
- Sensor-Surface: (Fix Surface)
- Electronics: DAE4 Sn1399; Calibrated: 2017/11/16
- Phantom: HAC Test Arch with AMCC; Type: SD HAC P01 BA;
- Measurement SW: DASY52, Version 52.10 (0); SEMCAD X Version 14.6.10 (7417)

### E Scan - ER3D: 15 mm from Probe Center to the Device/Hearing Aid Compatibility Test (101x101x1): Interpolated grid: dx=0.5000 mm, dy=0.5000 mm

Device Reference Point: 0, 0, -6.3 mm

Reference Value = 7.368 V/m; Power Drift = 0.03 dB

Applied MIF = -1.62 dB

RF audio interference level = 17.79 dBV/m

**Emission category: M4**

MIF scaled E-field



|  |  |  |
|--|--|--|
| <b>Grid 1 M4</b><br><b>16.04 dBV/m</b> | <b>Grid 2 M4</b><br><b>17.79 dBV/m</b> | <b>Grid 3 M4</b><br><b>17.68 dBV/m</b> |
| <b>Grid 4 M4</b><br><b>15.35 dBV/m</b> | <b>Grid 5 M4</b><br><b>16.46 dBV/m</b> | <b>Grid 6 M4</b><br><b>17 dBV/m</b>    |
| <b>Grid 7 M4</b><br><b>15.31 dBV/m</b> | <b>Grid 8 M4</b><br><b>14.59 dBV/m</b> | <b>Grid 9 M4</b><br><b>14.64 dBV/m</b> |

**Cursor:**

Total = 17.79 dBV/m

E Category: M4

Location: -2.5, -25, 8.7 mm

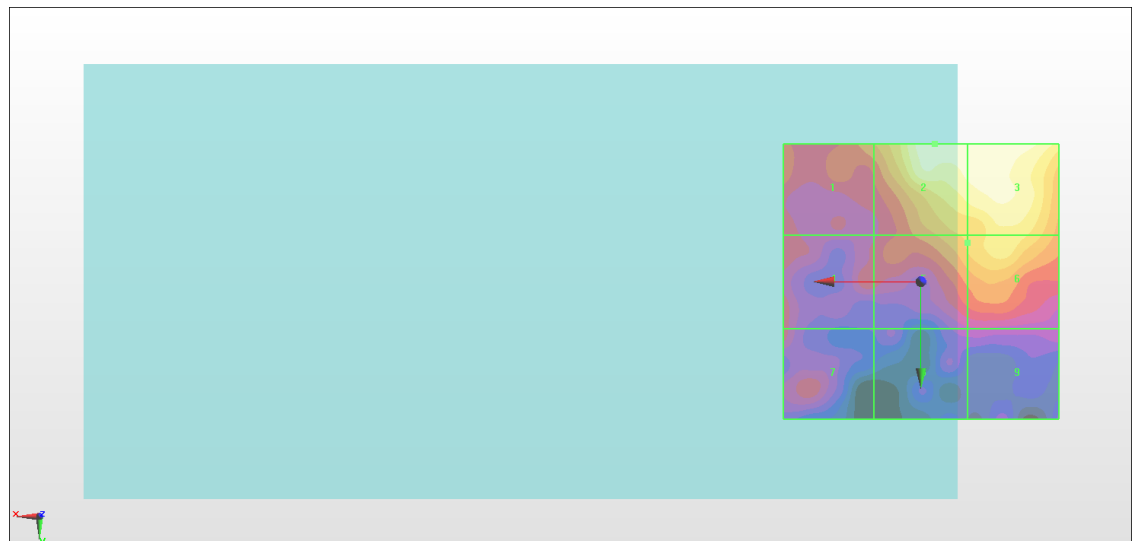

0 dB = 7.749 V/m = 17.79 dBV/m