


<b>ViVIX-S</b>		<b>CE</b> 0434	
Wireless		Digital Imaging System	
<b>Part No.: FXRD-1417WA</b>			
<b>SN:</b>		Follow Instruction for use	
<b>Rating: 24V <math>\equiv</math> Max. 0.5A</b>			
(Use only with FXRS-03A)			
	Date of manufacture:	RN:	
	Medical Equipment UL60601-1/CAN.CSA CSS.2 NO.601.1 FACTORY ID : VWF2	Contain FCC ID : RYK-WPEA121N Contains IC Number : 6158A-WPEA121NW	
		CMIIT ID: 007-AA0193	
KCC- RMM-VJM - FXRD1417W	Electric Shock	5.15-5.35GHz is indoor use only.	
	<b>CAUTION:</b> Federal law restricts this device to sale by or on the order of a physician or a licensed practitioner.		
	<b>Manufacturer: Vieworks Co., Ltd.</b> #107~108,601~610, Suntechcity II, 52 Sagimakgol-ro, Jungwon-gu, Seongnam-si, Gyeonggi-do, 462-736, South Korea		
MADE IN KOREA			

<b>ViVIX-S</b>		<b>CE</b> 0434	
Wireless		Digital Imaging System	
<b>Part No.: FXRD-1417WB</b>			
<b>SN:</b>		Follow Instruction for use	
<b>Rating: 24V <math>\equiv</math> Max. 0.5A</b>			
(Use only with FXRS-03A)			
	Date of manufacture:	RN:	
	Medical Equipment UL60601-1/CAN.CSA CSS.2 NO.601.1 FACTORY ID : VWF2	Contain FCC ID : RYK-WPEA121N Contains IC Number : 6158A-WPEA121NW	
		CMIIT ID: 007-AA0193	
KCC- RMM-VJM - FXRD1417W	Electric Shock	5.15-5.35GHz is indoor use only.	
	<b>CAUTION:</b> Federal law restricts this device to sale by or on the order of a physician or a licensed practitioner.		
	<b>Manufacturer: Vieworks Co., Ltd.</b> #107~108,601~610, Suntechcity II, 52 Sagimakgol-ro, Jungwon-gu, Seongnam-si, Gyeonggi-do, 462-736, South Korea		
MADE IN KOREA			

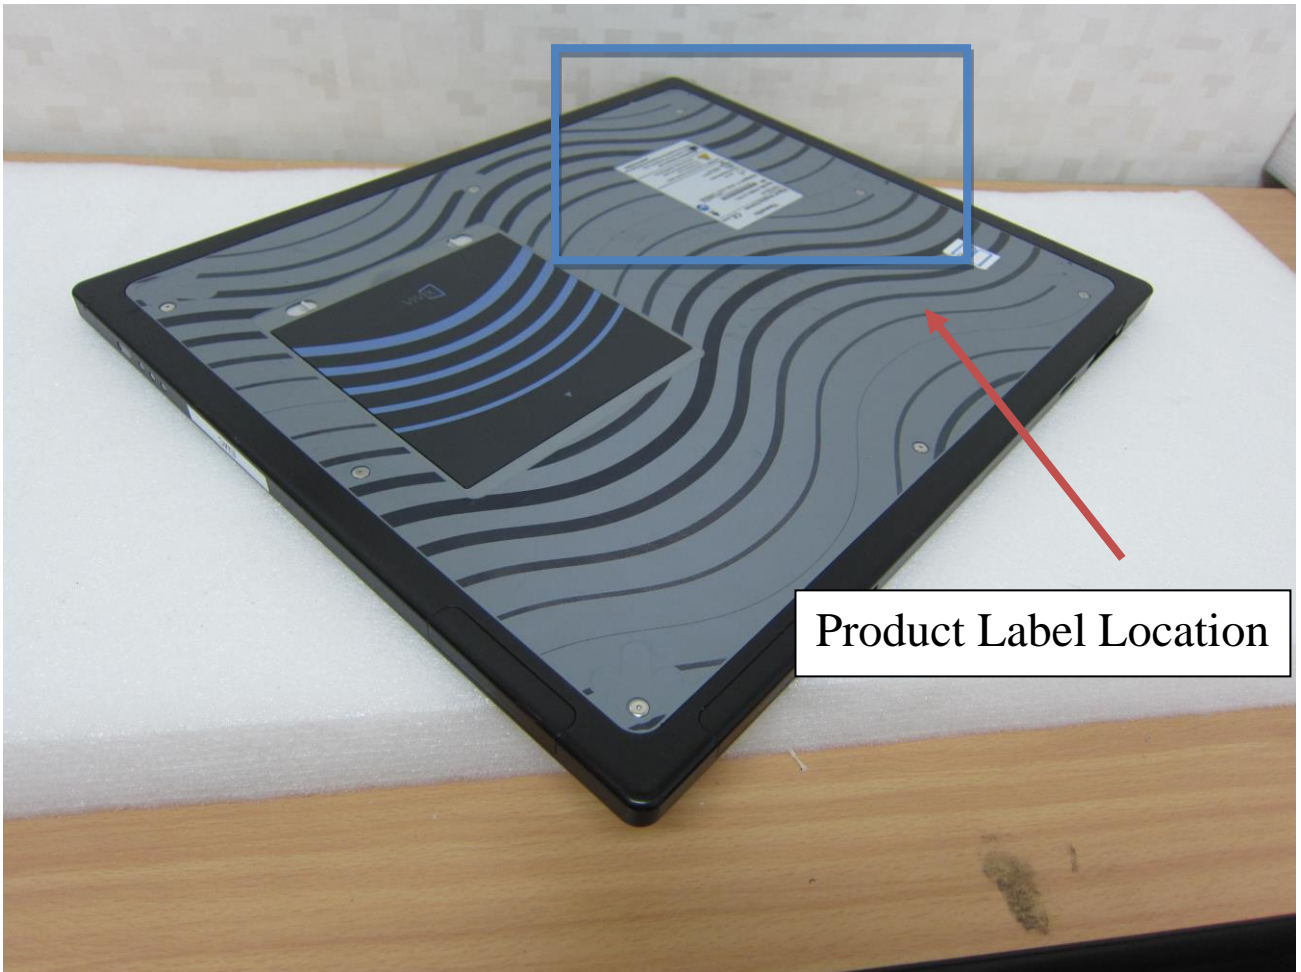

**Product Label Location**