



Appendix D


Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

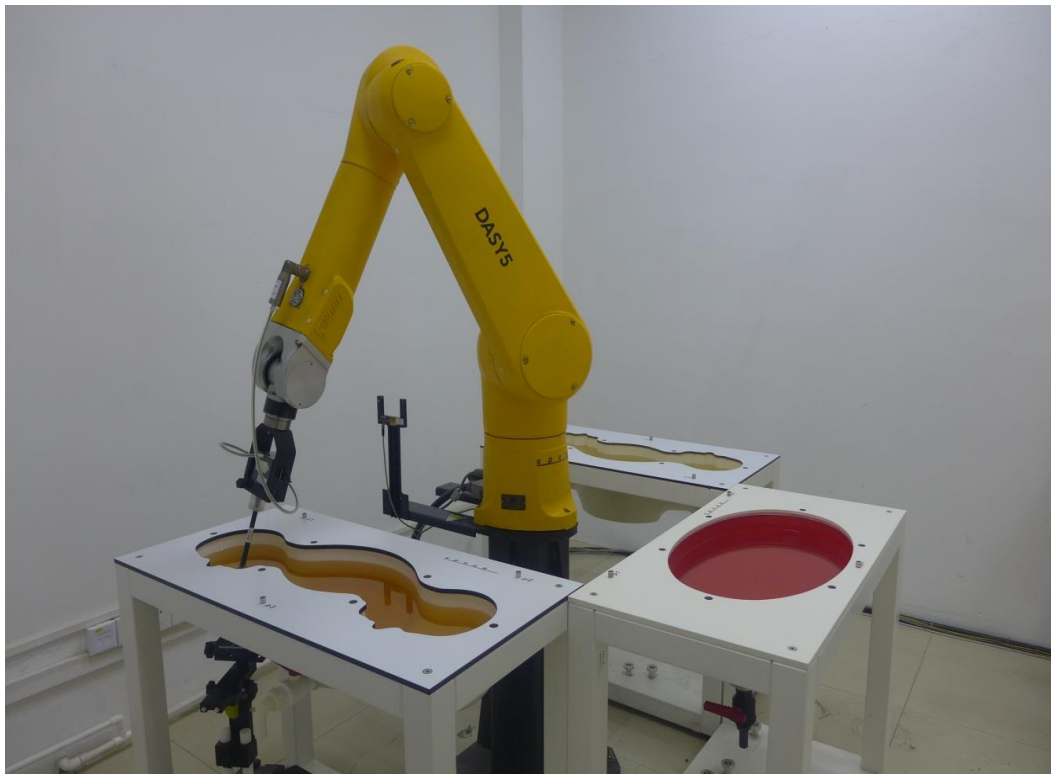


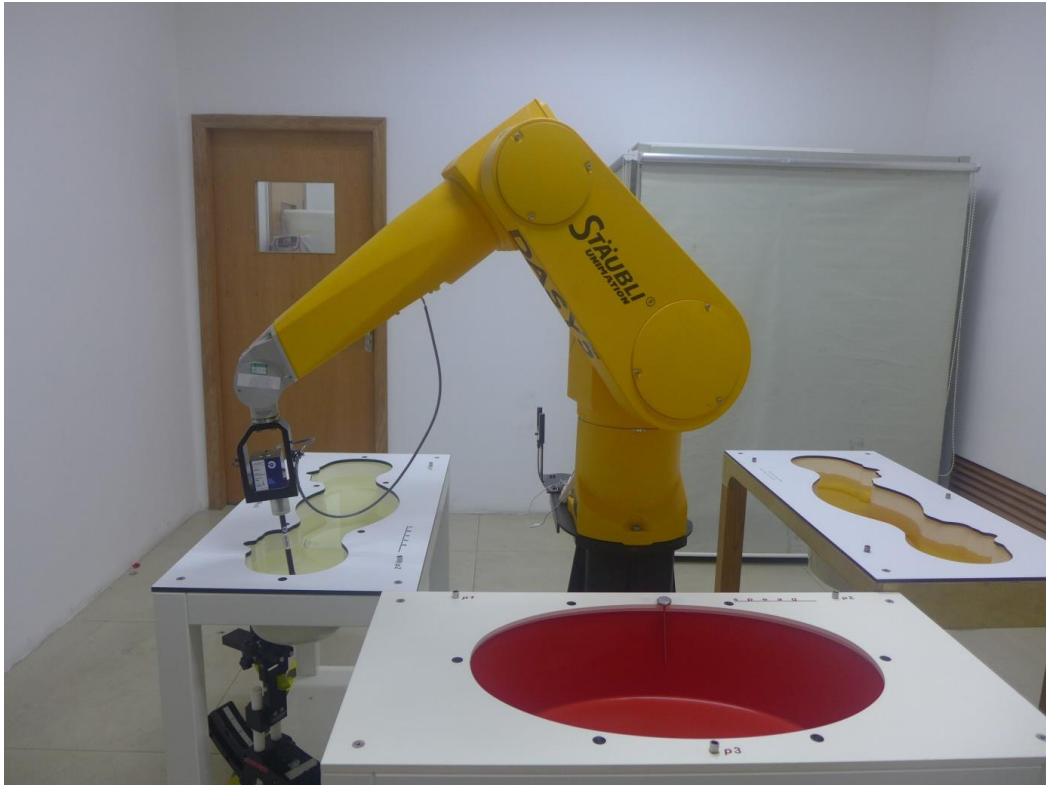


1. SAR measurement System





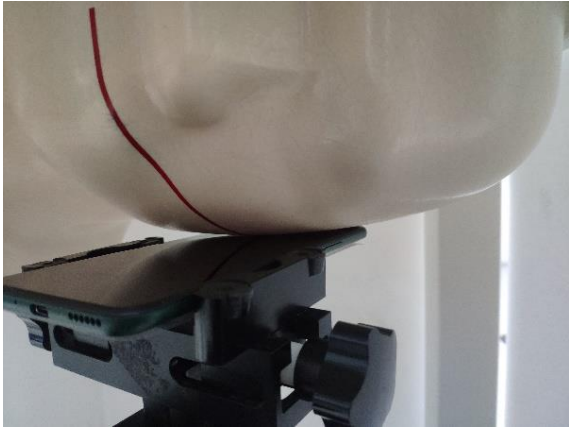



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
	NA

3. Photographs of EUT test position

<p>Photo 2: Left cheek</p>	<p>Photo 3: Left tilted</p>
	
<p>Photo 4: Right cheek</p>	<p>Photo 5: Right tilted</p>
	
<p>Photo 6: Front side 15mm</p>	<p>Photo 7: Back side 15mm</p>
	

<p>Photo 8: Front side 10mm</p>	<p>Photo 9: Back side 10mm</p>
	
<p>Photo 10: Left side 10mm</p>	<p>Photo 11: Right side 10mm</p>
	
<p>Photo 12: Top side 10mm</p>	<p>Photo 13: Bottom side 10mm</p>
	

<p>Photo 14: Front side 0mm</p>	<p>Photo 15: Back side 0mm</p>
	
<p>Photo 16: Left side 0mm</p>	<p>Photo 17: Right side 0mm</p>
	
<p>Photo 18: Top side 0mm</p>	<p>Photo 19: Bottom side 0mm</p>
	

4. EUT Constructional Details

Photo 20: Front View	Photo 21: Back View
