

APPENDIX**10. Photographs of Test Setup**

Fig.1 Photograph of the SAR measurement system

Photograph of the Tissue Simulant Fluid Liquid Depth

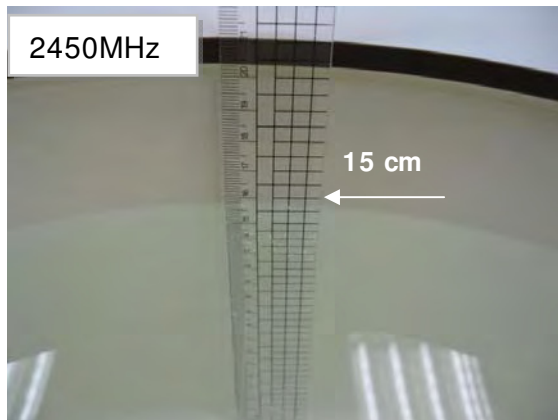


Fig.2.1

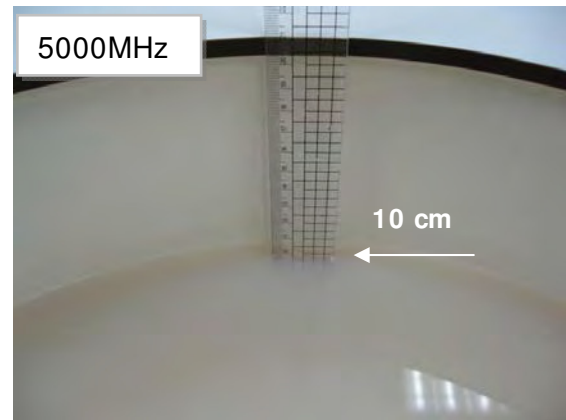


Fig.2.2

Body - distance between flat phantom and EUT is 0 mm



Fig.3 EUT Back side to flat phantom



Fig.4 EUT Top side to flat phantom

11. Photographs of the EUT



Fig.5 Front view of EUT

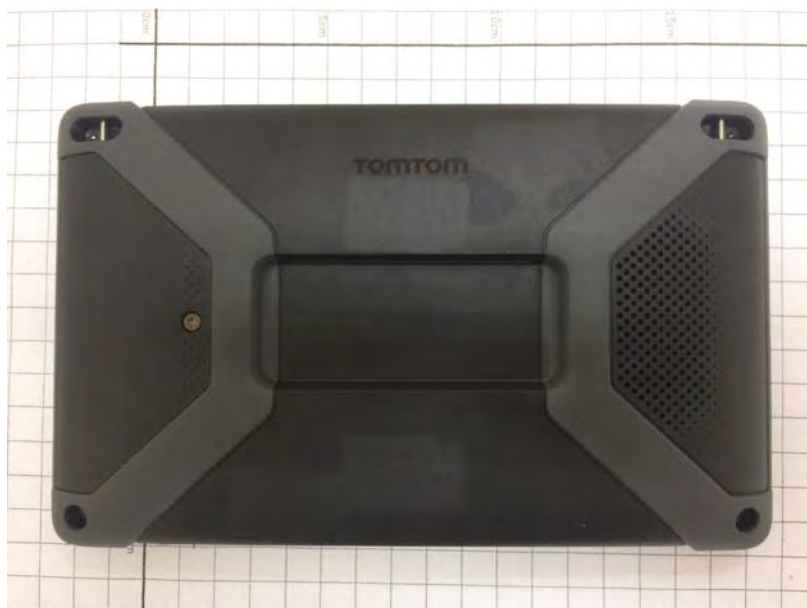


Fig.6 Back view of EUT

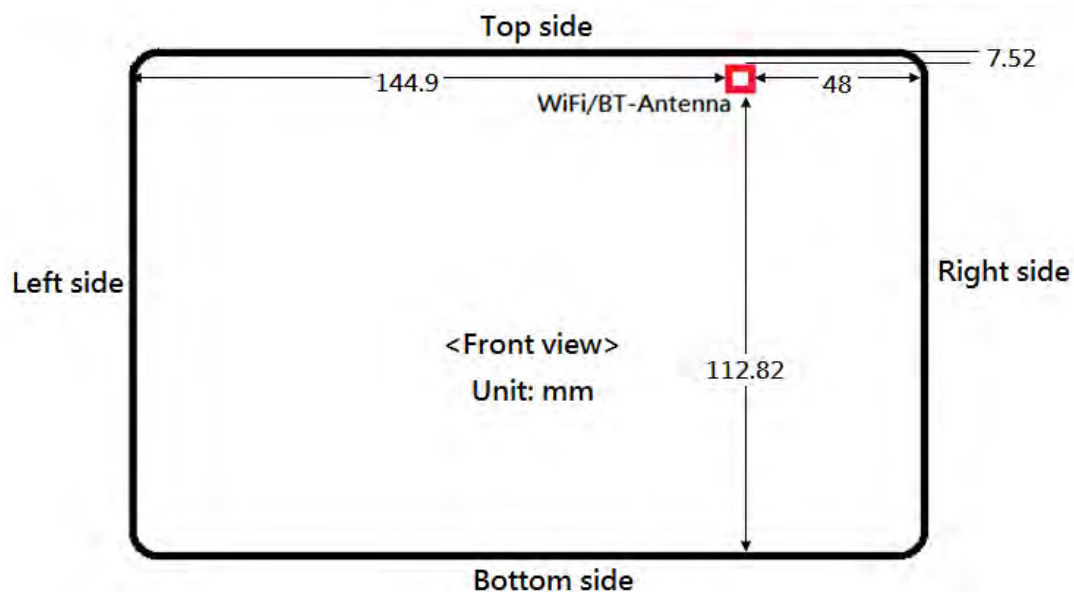


Fig.7 Antenna position of EUT

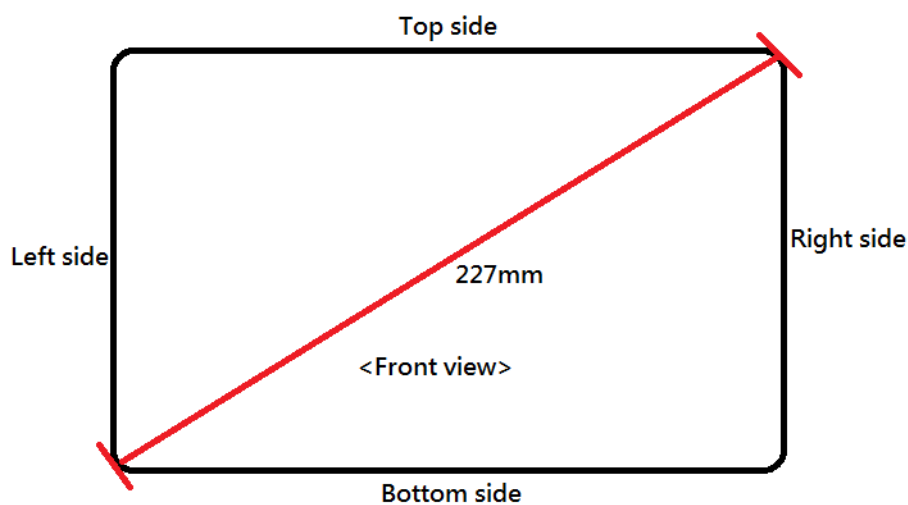


Fig.8 Antenna location - Diagonal Dimension (Front view)

- End of Report -