

SAR Plots

- Verification Plots
- SAR Test Plots

DT&C Co., Ltd.

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN:726

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1
Medium parameters used: $f = 2450$ MHz; $\sigma = 1.818$ S/m; $\epsilon_r = 39.606$; $\rho = 1000$ kg/m³
Phantom section: Flat Section


DASY5 Configuration:

Probe: EX3DV4 - SN7368; ConvF(7.81, 7.81, 7.81) @ 2450 MHz; Calibrated: 1/30/2020 Electronics: DAE4 Sn1391
Sensor-Surface: 2mm (Mechanical Surface Detection)
Phantom: Twin-SAM V5.0 ; Type: QD 000 P40 CD; Serial: 1679
Measurement SW: DASY52, Version 52.10 (3); SEMCAD X Version 14.6.13 (7474)

Test Date: 2020-07-15; Ambient Temp: 22.1; Tissue Temp: 21.9

2450 MHz System Verification(100mW)

Area Scan (7x9x1): Measurement grid: dx=12mm, dy=12mm
Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Power Drift = 0.09 dB
Peak SAR (extrapolated) = 11.5 W/kg
SAR(1 g) = 5.51 W/kg; SAR(10 g) = 2.54 W/kg

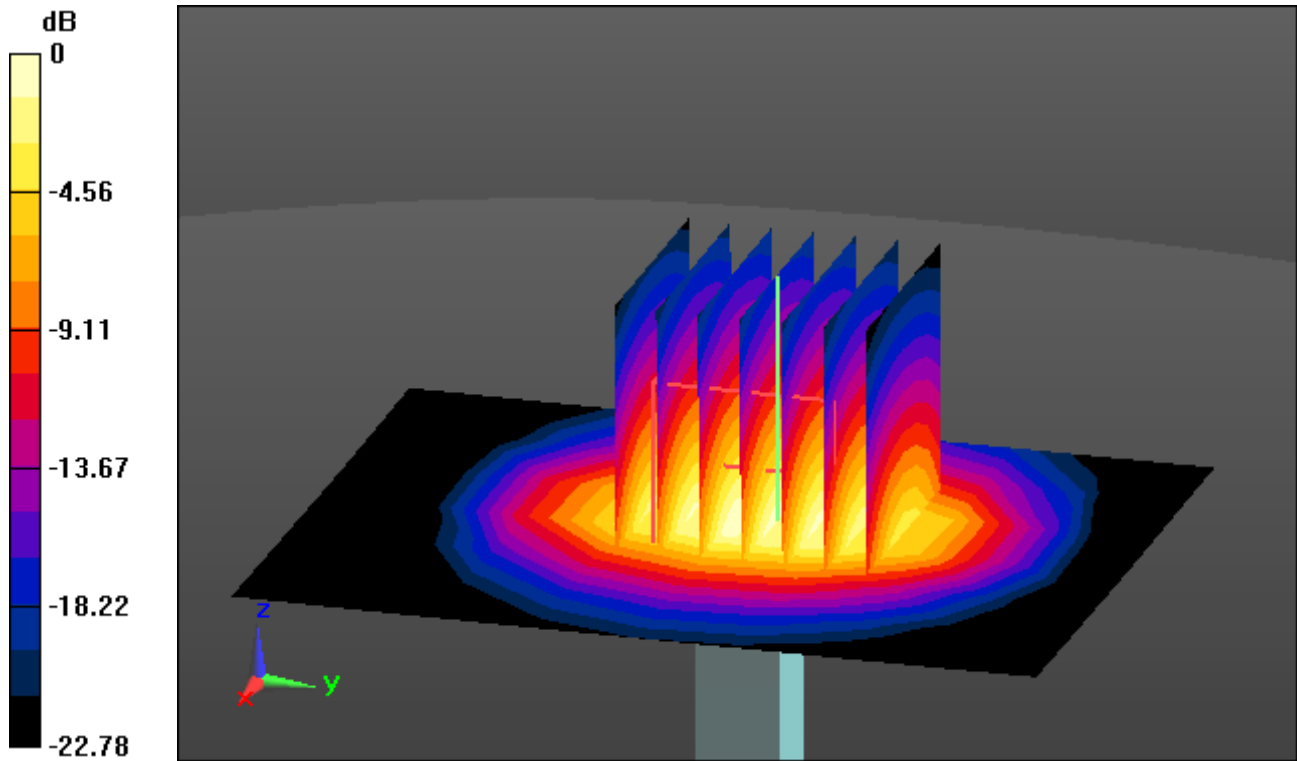

0 dB = 8.46 W/kg

DT&C Co., Ltd.

DUT: SP83; Type: Bluetooth Headset

Communication System: UID 0, Bluetooth (0); Frequency: 2441 MHz; Duty Cycle: 1:1.302

Medium parameters used: $f = 2441$ MHz; $\sigma = 1.807$ S/m; $\epsilon_r = 39.631$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

DASY5 Configuration:

Probe: EX3DV4 - SN7368; ConvF(7.81, 7.81, 7.81) @ 2441 MHz; Calibrated: 1/30/2020 Electronics: DAE4 Sn1391

Sensor-Surface: 2mm (Mechanical Surface Detection)

Phantom: Twin-SAM V5.0 ; Type: QD 000 P40 CD; Serial: 1679

Measurement SW: DASY52, Version 52.10 (3); SEMCAD X Version 14.6.13 (7474)

Test Date: 2020-07-15; Ambient Temp: 22.1; Tissue Temp: 21.9

1 cm space from Body, Rear, Bluetooth 1Mbps Ch. 39, Ant Internal


Area Scan (7x11x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Power Drift = -0.04 dB

Peak SAR (extrapolated) = 0.682 W/kg

SAR(1 g) = 0.390 W/kg; SAR(10 g) = 0.216 W/kg

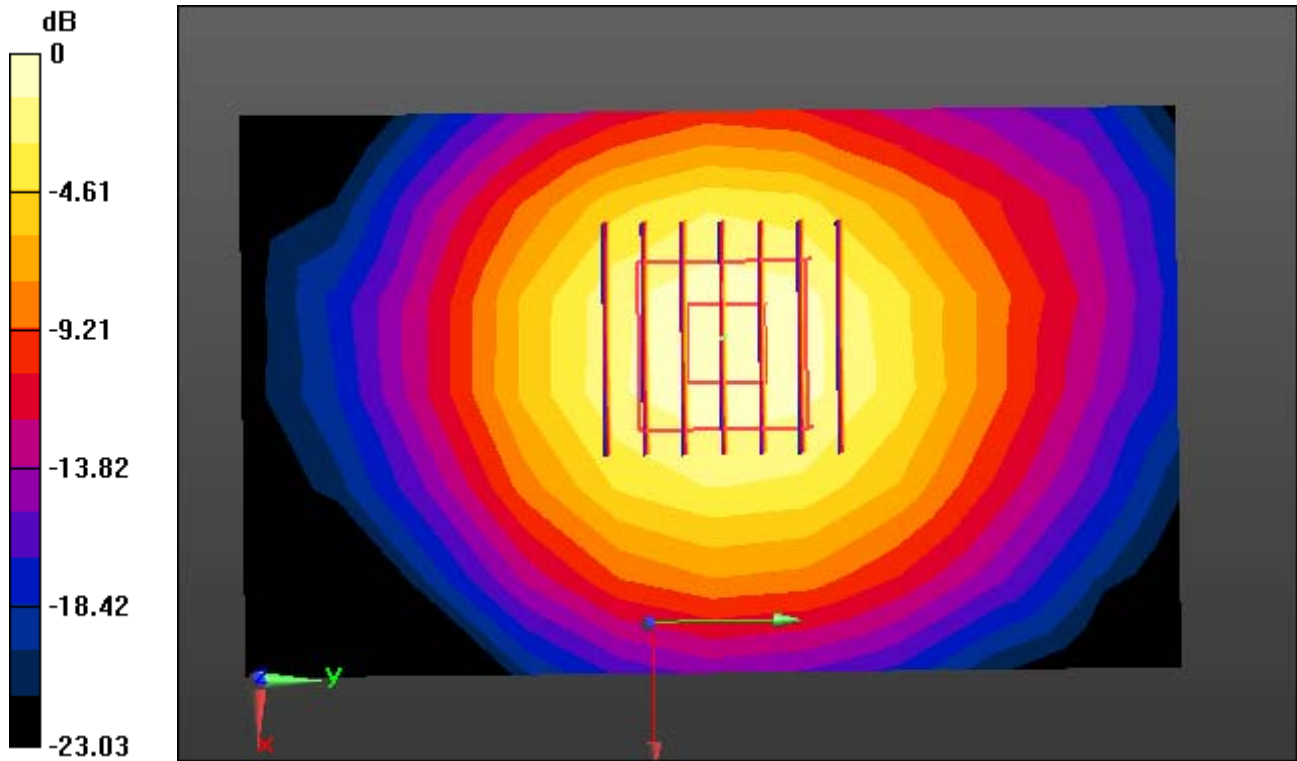

0 dB = 0.539 W/kg